



Appendix D



Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

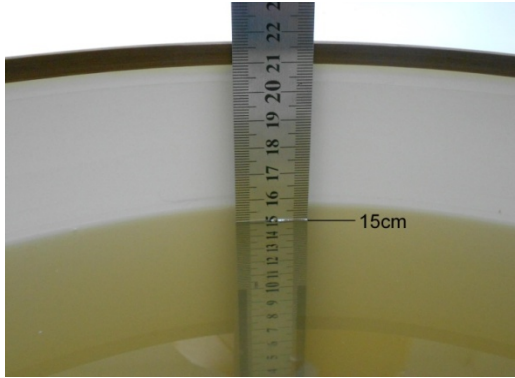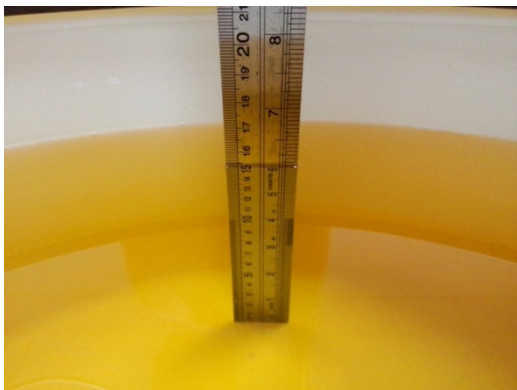Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 2600
	

3. Photographs of EUT test position




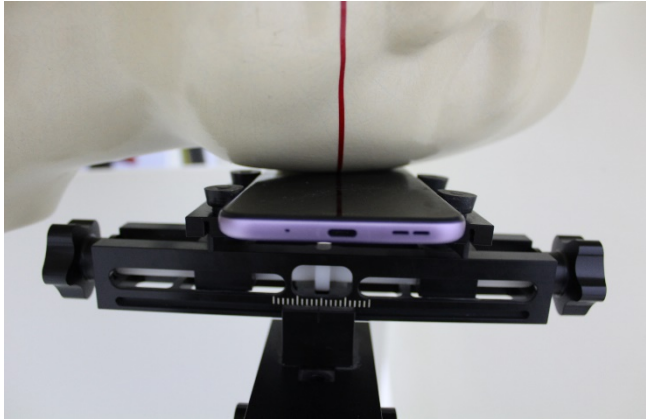
Photo 7: Left touch cheek	Photo 8: Left tilted 15 degree
	
Photo 9: Right touch cheek	Photo 10: Right tilted 15 degree
	
Photo 11: Front side 10mm	Photo 12: Back side 10mm
	

Photo 13: Left side 10mm	Photo 14: Right side 10mm
	
Photo 15: Top side 10mm	Photo 16: Bottom side 10mm
	

4. EUT Constructional Details

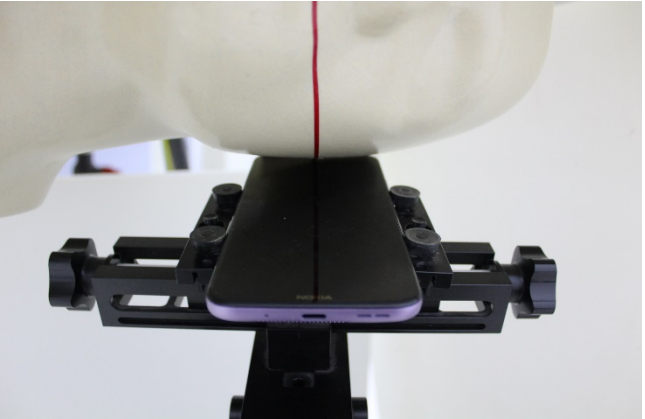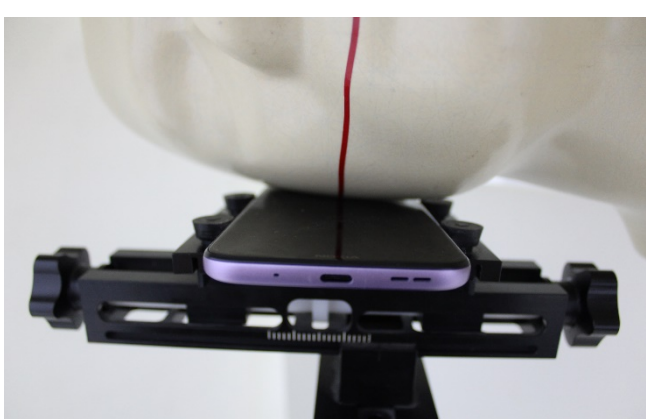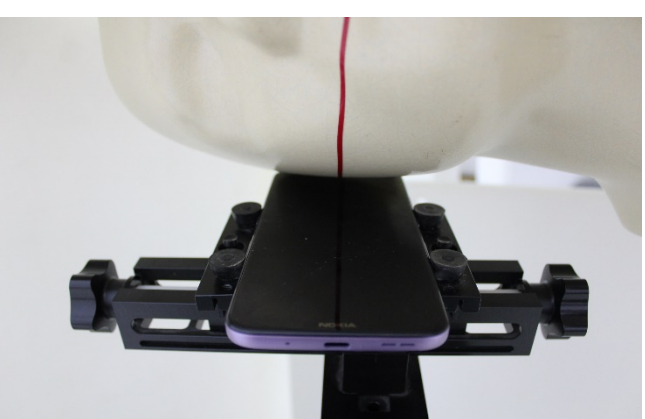