Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 08/26/04 13:45:36

#### Body\_802.11b Ch6\_Keypad Up With Touch\_20040826

#### Mono\_28 Key\_PICO imager\_2x Battery

#### DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 2$  mho/m;  $\varepsilon_r = 51.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature : 22.3 °C; Liquid Temperature : 22.3 °C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

# **CH6/Area Scan (71x151x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.042 mW/g


CH6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.694 V/m; Power Drift = -0.0 dB

Peak SAR (extrapolated) = 0.126 W/kg

SAR(1 g) = 0.034 mW/g; SAR(10 g) = 0.015 mW/g

Maximum value of SAR (measured) = 0.040 mW/g

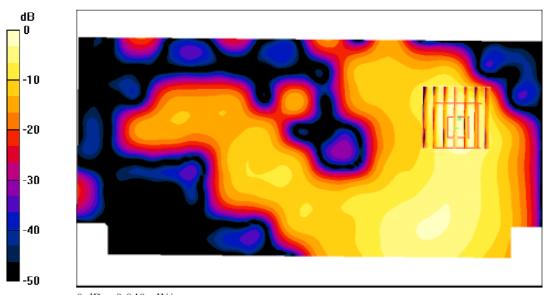

0 dB = 0.040 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 08/26/04 14:26:36

#### Body\_802.11b Ch6\_Keypad Up With Touch\_20040826

#### Mono\_38 Key\_PICO Imager\_2x Battery

#### DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 2$  mho/m;  $\varepsilon_r = 51.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature : 22.3 °C; Liquid Temperature : 22.2 °C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

# **CH6/Area Scan (71x151x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.041 mW/g


CH6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.564 V/m; Power Drift = 0.2 dB

Peak SAR (extrapolated) = 0.084 W/kg

SAR(1 g) = 0.038 mW/g; SAR(10 g) = 0.016 mW/g

Maximum value of SAR (measured) = 0.042 mW/g

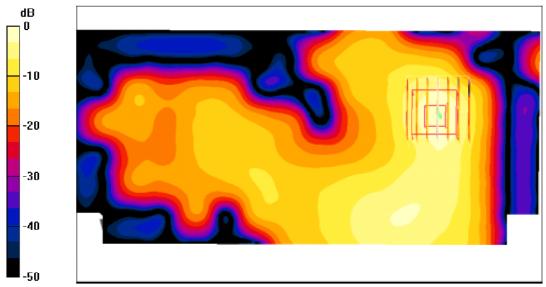

0 dB = 0.042 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 08/26/04 14:59:36

#### Body\_802.11b Ch6\_Keypad Up With Touch\_20040826

Mono\_38 Key\_SE800hP\_2x Battery

DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 2$  mho/m;  $\varepsilon_r = 51.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature ∶ 22.2 °C; Liquid Temperature ∶ 22.3 °C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

# **CH6/Area Scan (71x151x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.081 mW/g

CH6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 1.37 V/m; Power Drift = 0.007 dB

Peak SAR (extrapolated) = 0.153 W/kg

SAR(1 g) = 0.068 mW/g; SAR(10 g) = 0.030 mW/gMaximum value of SAR (measured) = 0.078 mW/g

-10 -20 -30 -40

0 dB = 0.078 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab

Date/Time: 08/26/04 15:33:36

#### Body\_802.11b Ch6\_Keypad Up With Touch\_20040826

Mono\_38 Key\_SE800hP\_1x Battery

#### DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 2$  mho/m;  $\varepsilon_r = 51.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature ∶ 22.3 °C; Liquid Temperature ∶ 22.2 °C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

### CH6/Area Scan (71x151x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.046 mW/g


CH6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.176 V/m; Power Drift = -0.1 dB

Peak SAR (extrapolated) = 0.092 W/kg

SAR(1 g) = 0.042 mW/g; SAR(10 g) = 0.018 mW/g

Maximum value of SAR (measured) = 0.049 mW/g

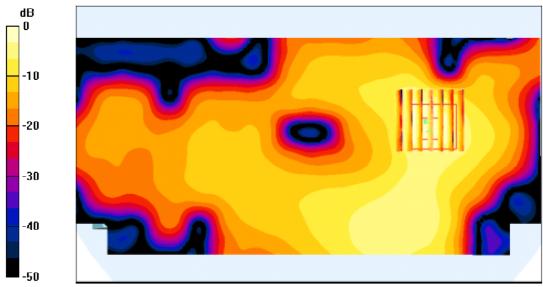

0 dB = 0.049 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 08/26/04 16:05:36

#### Body\_802.11b Ch1\_Keypad Up With Touch\_20040826

Mono\_38 Key\_SE800hP\_2x Battery

DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma = 1.94$  mho/m;  $\varepsilon_r = 51.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature : 22.3 °C; Liquid Temperature : 22.2 °C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

### CH1/Area Scan (71x151x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.079 mW/g


CH1/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.464 V/m; Power Drift = 0.0 dB

Peak SAR (extrapolated) = 0.153 W/kg

SAR(1 g) = 0.067 mW/g; SAR(10 g) = 0.030 mW/g

Maximum value of SAR (measured) = 0.077 mW/g

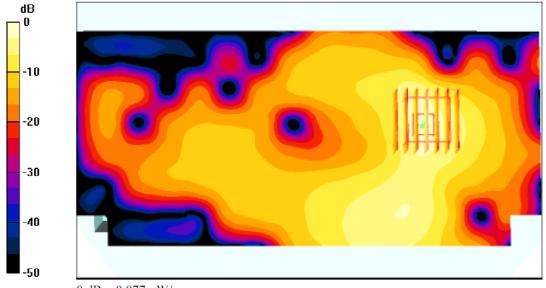

0 dB = 0.077 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 08/26/04 14:59:36

#### Body\_802.11b Ch6\_Keypad Up With Touch\_20040826

Mono\_38 Key\_SE800hP\_2x Battery

DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 2$  mho/m;  $\varepsilon_r = 51.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature  $: 22.2 \, ^{\circ}\mathrm{C} \: ; \: Liquid Temperature \: : \: 22.3 \, ^{\circ}\mathrm{C} \:$ 

#### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

# **CH6/Area Scan (71x151x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.081 mW/g


CH6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 1.37 V/m; Power Drift = 0.007 dB

Peak SAR (extrapolated) = 0.153 W/kg

SAR(1 g) = 0.068 mW/g; SAR(10 g) = 0.030 mW/g

Maximum value of SAR (measured) = 0.078 mW/g

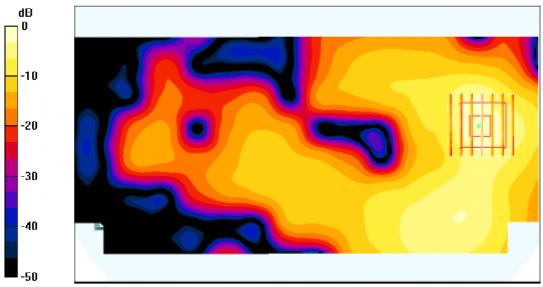

0 dB = 0.078 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 08/26/04 16:42:16

#### Body\_802.11b Ch11\_Keypad Up With Touch\_20040826

Mono\_38 Key\_SE800hP\_2x Battery

DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11b; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2462 MHz;  $\sigma = 2.02$  mho/m;  $\varepsilon_r = 51.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature : 22.1 °C; Liquid Temperature : 22.2 °C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

# **CH11/Area Scan (71x151x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.028 mW/g


CH11/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.204 V/m; Power Drift = -0.2 dB

Peak SAR (extrapolated) = 0.092 W/kg

SAR(1 g) = 0.025 mW/g; SAR(10 g) = 0.00999 mW/g

Maximum value of SAR (measured) = 0.028 mW/g

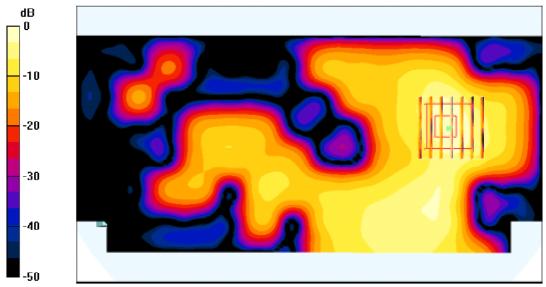

0 dB = 0.028 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 08/27/04 19:41:09

#### Body\_802.11g Ch1\_Keypad Up With Touch\_20040827

Mono\_38 Key\_SE800hP\_2x Battery

DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma = 1.94$  mho/m;  $\varepsilon_r = 51.4$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature : 22.0  $^{\circ}$ C; Liquid Temperature : 22.1  $^{\circ}$ C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

# **CH1/Area Scan (71x151x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.044 mW/g


CH1/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.403 V/m; Power Drift = 0.1 dB

Peak SAR (extrapolated) = 0.122 W/kg

SAR(1 g) = 0.047 mW/g; SAR(10 g) = 0.021 mW/g

Maximum value of SAR (measured) = 0.054 mW/g

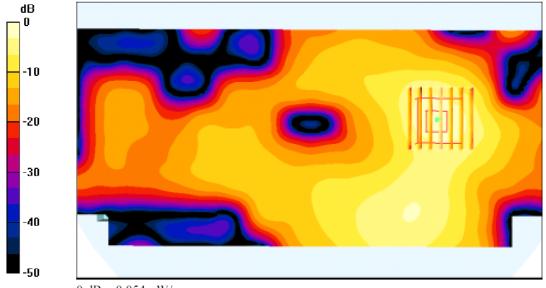

0 dB = 0.054 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 08/27/04 19:41:09

#### Body\_802.11g Ch6\_Keypad Up With Touch\_20040827

Mono\_38 Key\_SE800hP\_2x Battery

DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11g; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 2$  mho/m;  $\varepsilon_r = 51.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature ∶ 22.1 °C; Liquid Temperature ∶ 22.1 °C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

### CH6/Area Scan (71x151x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.033 mW/g


CH6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.716 V/m; Power Drift = -0.2 dB

Peak SAR (extrapolated) = 0.260 W/kg

SAR(1 g) = 0.028 mW/g; SAR(10 g) = 0.012 mW/g

Maximum value of SAR (measured) = 0.033 mW/g

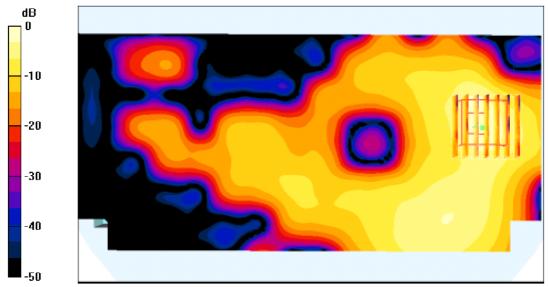

0 dB = 0.033 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 08/27/04 10:53:31

#### Body\_802.11g Ch11\_Keypad Up With Touch\_20040827

Mono\_38 Key\_SE800hP\_2x Battery

#### DUT: SYMBOL MC3090 project; Type: Mobile Computer

Communication System: 802.11g; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2462 MHz;  $\sigma = 2.02$  mho/m;  $\varepsilon_r = 51.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature : 22.2 °C; Liquid Temperature : 22.1 °C

#### DASY4 Configuration:

- Probe: ET3DV6 SN1787; ConvF(4.5, 4.5, 4.5); Calibrated: 2003/8/29
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 2003/11/21
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.3 Build 16; Postprocessing SW: SEMCAD, V1.8 Build 123

### CH11/Area Scan (71x151x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.030 mW/g

CH11/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 1.14 V/m; Power Drift = 0.2 dB

Peak SAR (extrapolated) = 0.063 W/kg

SAR(1 g) = 0.027 mW/g; SAR(10 g) = 0.013 mW/g

Maximum value of SAR (measured) = 0.031 mW/g


CH11/Zoom Scan (7x7x7)/Cube 1: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 1.14 V/m; Power Drift = 0.2 dB

Peak SAR (extrapolated) = 0.048 W/kg

SAR(1 g) = 0.022 mW/g; SAR(10 g) = 0.011 mW/g

Maximum value of SAR (measured) = 0.024 mW/g

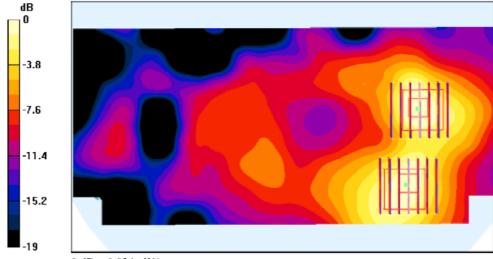

0 dB = 0.024 mW/g



### Appendix C – Calibration Data

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

Auden > Sporton Int. Inc.

| D2450V2 - SN:736  |   |  |  |
|---|---|--|--|
| QA CAL-05.v2 Calibration procedure for dipole validation kits   |   |  |  |
|   |   |  |  |
| August 27, 20   | 003   |  |  |
| In Tolerance (according to the specific calibration document)   |   |  |  |
|   |   |  |  |
| TE critical for calibration)  |   |  |  |
| ID#   | Cal Date (Calibrated by, Certificate No.)   | Scheduled Calibration  |  |
| 100698  | 27-Mar-2002 (R&S, No. 20-92389)   | In house check: Mar-05   |  |
| MY41092317  | 18-Oct-02 (Agilent, No. 20021018)   | Oct-04   |  |
| US37292783  | 30-Oct-02 (METAS, No. 252-0236)   | Oct-03   |  |
| GB37480704  |   | Oct-03   |  |
| US37390585  | 18-Oct-01 (Agilent, No. 24BR1033101)  | In house check: Oct 03   |  |
| Name  | Function  | Signature  |  |
| Judith Mueller  | Technician  | Gradile  |  |
| C 447 THE C 127 C 147 C 147 C 148 C |   |  |  |
|   |   |  |  |
| Katja Pokovic   | Laboratory Cirector   | Mon 16th   |  |
| Katja Pokovic   | Laboratory Offector   | Date issued: August 28, 2003   |  |
|   | QA CAL-05. v Calibration pr August 27, 20 In Tolerance elember traceability of M&Te sted in the closed laborat TE critical for calibration) ID# 100698 MY41092317 US37292783 GB37480704 US37390585 Name | QA CAL-05.v2 Calibration procedure for dipole validation kits  August 27, 2003  In Tolerance (according to the specific calibration ents traceability of M&TE used in the calibration procedures and conformity ented in the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facility: environment temperature 22 +/- 2 degree to the closed laboratory facilit |  |



Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

# DASY

Dipole Validation Kit

Type: D2450V2

Serial: 736

Manufactured: August 26, 2003 Calibrated: August 27, 2003

#### 1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with head simulating solution of the following electrical parameters at 2450 MHz:

Relative Dielectricity 38.2  $\pm$  5% Conductivity 1.89 mho/m  $\pm$  5%

The DASY4 System with a dosimetric E-field probe ES3DV2 (SN:3013, Conversion factor 4.8 at 2450 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was  $250mW \pm 3$  %. The results are normalized to 1W input power.

#### 2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ES3DV2-SN:3013 and applying the <u>advanced extrapolation</u> are:

averaged over 1 cm<sup>3</sup> (1 g) of tissue: 55.6 mW/g  $\pm$  16.8 % (k=2)<sup>1</sup>

averaged over 10 cm<sup>3</sup> (10 g) of tissue: 25.0 mW/g  $\pm$  16.2 % (k=2)

<sup>1</sup> validation uncertainty

#### Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:

1.158 ns (one direction)

Transmission factor:

0.983

(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 2450 MHz:

 $Re{Z} = 52.5 \Omega$ 

Im  $\{Z\} = 3.6 \Omega$ 

Return Loss at 2450 MHz

-27.5 dB

#### Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with body simulating solution of the following electrical parameters at 2450 MHz:

Relative Dielectricity

± 5%

Conductivity

2.03 mho/m ± 5%

The DASY4 System with a dosimetric E-field probe ES3DV2 (SN:3013, Conversion factor 4.2 at 2450 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was 250mW ± 3 %. The results are normalized to 1W input power.

#### 5. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ES3DV2 SN:3013 and applying the advanced extrapolation are:

averaged over 1 cm3 (1 g) of tissue:

56.0 mW/g  $\pm$  16.8 % (k=2)<sup>2</sup>

averaged over 10 cm3 (10 g) of tissue:

25.8 mW/g  $\pm$  16.2 % (k=2)<sup>2</sup>

#### 6. Dipole Impedance and Return Loss

The dipole was positioned at the flat phantom sections according to section 4 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 2450 MHz:

 $Re{Z} = 48.7 \Omega$ 

Im  $\{Z\} = 4.8 \Omega$ 

Return Loss at 2450 MHz

-25.8 dB

#### 7. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

#### 8. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Small end caps have been added to the dipole arms in order to improve matching when loaded according to the position as explained in Sections 1 and 4. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

#### 9. Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

<sup>&</sup>lt;sup>2</sup> validation uncertainty

Page 1 of 1

Date/Time: 08/27/03 15:43:04

Test Laboratory: SPEAG, Zurich, Switzerland File Name: SN736 SN3013 M2450 270803.da4

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Program: Dipole Calibration

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: Muscle 2450 MHz ( $\sigma = 2.03 \text{ mho/m}, \epsilon_p = 50.75, \rho = 1000 \text{ kg/m}^3$ )

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:

- Probe: ES3DV2 SN3013; ConvF(4.2, 4.2, 4.2); Calibrated: 1/19/2003
- · Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 SN411; Calibrated: 1/16/2003
- Phantom: SAM with CRP TP1006; Type: SAM 4.0; Serial: TP:1006
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

#### Pin = 250 mW; d = 10 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 91 V/m

Power Drift = -0.02 dB

Maximum value of SAR = 15.7 mW/g

#### Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm,


dz=5mm


Peak SAR (extrapolated) = 27.8 W/kg

SAR(1 g) = 14 mW/g; SAR(10 g) = 6.46 mW/g Reference Value = 91 V/m

Power Drift = -0.02 dB

Maximum value of SAR = 16 mW/g

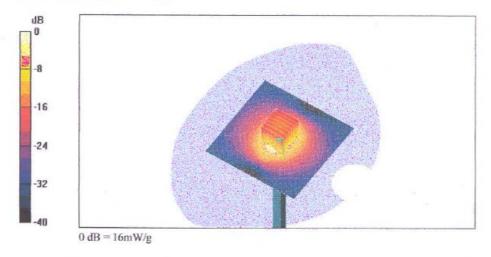

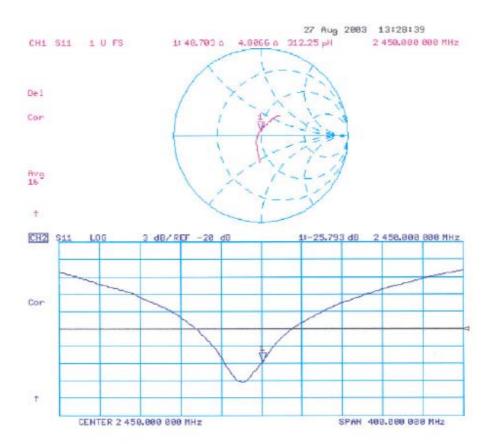

Page 1 of 1

Date/Time: 08/27/03 11:42:12

Test Laboratory: SPEAG, Zurich, Switzerland File Name: SN736\_SN3013\_HSL2450\_270803.da4

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Program: Dipole Calibration

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: HSL 2450 MHz ( $\sigma$  = 1.89 mho/m,  $\epsilon_r$  = 38.19,  $\rho$  = 1000 kg/m³)

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:

- Probe: ES3DV2 SN3013; ConvF(4.8, 4.8, 4.8); Calibrated: 1/19/2003
- · Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 SN411; Calibrated: 1/16/2003
- Phantom: SAM with CRP TP1006; Type: SAM 4.0; Serial: TP:1006
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

#### Pin = 250 mW; d = 10 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 91.5 V/m

Power Drift = -0.04 dB

Maximum value of SAR = 15.3 mW/g


#### Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 30.2 W/kg

SAR(1 g) = 13.9 mW/g; SAR(10 g) = 6.25 mW/gReference Value = 91.5 V/m

Power Drift = -0.04 dB

Maximum value of SAR = 15.5 mW/g

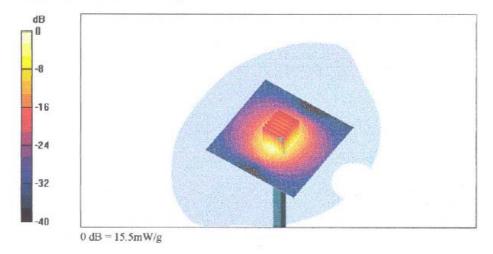

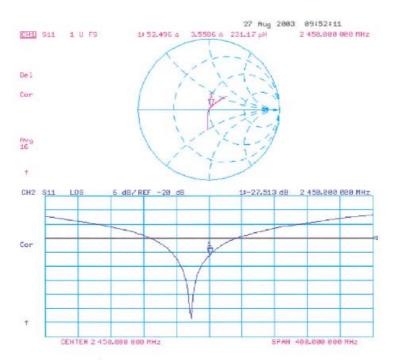



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

Auden > Sporton Int. Inc.

| Object(s)   | ET3DV6 - SN:   | 1788  |  |  |
|---|--|---|--|--|
| Calibration procedure(s)  | QA CAL-01 v2   |   |  |  |
|   | Calibration pro  | ocedure for dosimetric E-field probe  | es ::  |  |
| Calibration date:   | August 29, 2003  |   |  |  |
| Condition of the calibrated item  | In Tolerance (according to the specific calibration document)  |   |  |  |
| This calibration statement document<br>17025 international standard.  | ts traceability of M&TE  | used in the calibration procedures and conformity of  | f the procedures with the ISO/IEC  |  |
| U calibrations have been conducted  | d in the closed laborato   | ory facility: environment temperature 22 +/- 2 degrees  | s Celsius and humidity < 75%.  |  |
| Calibration Equipment used (M&TE  | critical for calibration)  |   |  |  |
|   |  |   |  |  |
| fodel Type  | ID#  | Cal Date (Calibrated by, Certificate No.)   | Scheduled Calibration  |  |
| 1. 1 S x 1 x 1 x 1 x 1 x 1 x 1 x 1 x 1 x 1  | ID#<br>US3642U01700  | Cal Date (Calibrated by, Certificate No.)<br>4-Aug-99 (SPEAG, in house check Aug-02)  | Scheduled Calibration<br>In house check: Aug-05  |  |
| F generator HP 8684C  |  |   |  |  |
| RF generator HP 8684C<br>Power sensor E4412A  | US3642U01700   | 4-Aug-99 (SPEAG, in house check Aug-02)   | In house check: Aug-05   |  |
| RF generator HP 8684C<br>Power sensor E4412A<br>Power sensor HP 8481A   | US3642U01700<br>MY41495277   | 4-Aug-99 (SPEAG, in house check Aug-02)<br>2-Apr-03 (METAS, No 252-0250)  | In house check: Aug-05<br>Apr-04   |  |
| RF generator HP 8684C<br>Power sensor E4412A<br>Power sensor HP 8481A<br>Power meter EPM E4419B   | US3642U01700<br>MY41495277<br>MY41092180<br>GB41293874<br>US37390585   | 4-Aug-99 (SPEAG, in house check Aug-02)<br>2-Apr-03 (METAS, No 252-0250)<br>18-Sep-02 (Agilent, No. 20020918)   | In house check: Aug-05<br>Apr-04<br>Sep-03   |  |
| RF generator HP 8684C<br>Power sensor E4412A<br>Power sensor HP 8481A<br>Power meter EPM E4419B<br>Network Analyzer HP 8753E  | US3642U01700<br>MY41495277<br>MY41092180<br>GB41293874   | 4-Aug-99 (SPEAG, in house check Aug-02)<br>2-Apr-03 (METAS, No 252-0250)<br>18-Sep-02 (Agilent, No. 20020918)<br>2-Apr-03 (METAS, No 252-0250)  | In house check: Aug-05<br>Apr-04<br>Sep-03<br>Apr-04   |  |
| RF generator HP 8684C<br>Power sensor E4412A<br>Power sensor HP 8481A<br>Power meter EPM E4419B<br>Network Analyzer HP 8753E  | US3642U01700<br>MY41495277<br>MY41092180<br>GB41293874<br>US37390585   | 4-Aug-99 (SPEAG, in house check Aug-02)<br>2-Apr-03 (METAS, No 252-0250)<br>18-Sep-02 (Agilent, No. 20020918)<br>2-Apr-03 (METAS, No 252-0250)<br>18-Oct-01 (Agilent, No. 24BR1033101)                                    | In house check: Aug-05<br>Apr-04<br>Sep-03<br>Apr-04<br>In house check: Oct 03   |  |
| RF generator HP 8684C<br>Power sensor E4412A<br>Power sensor HP 8481A<br>Power meter EPM E4419B<br>Network Analyzer HP 8753E<br>Fiske Process Calibrator Type 702                                 | US3642U01700<br>MY41495277<br>MY41092160<br>GB41293874<br>US37390585<br>SN: 6295803                          | 4-Aug-99 (SPEAG, in house check Aug-02)<br>2-Apr-03 (METAS, No 252-0250)<br>18-Sep-02 (Agilent, No. 20020918)<br>2-Apr-03 (METAS, No 252-0250)<br>18-Oct-01 (Agilent, No. 24BR1033101)<br>3-Sep-01 (ELCAL, No.2360)       | In house check: Aug-05<br>Apr-04<br>Sep-03<br>Apr-04<br>In house check: Oct 03<br>Sep-03   |  |
| RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A Power meter EPM E4419B Network Analyzer HP 8753E Fluke Process Celibrator Type 702 Calibrated by:                                 | US3842U01700<br>MY41495277<br>MY41092180<br>GB41293874<br>US37390585<br>SN: 6295803                          | 4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250) 18-Oct-01 (Agilent, No. 24BR1033101) 3-Sep-01 (ELCAL, No.2360)                      | In house check: Aug-05<br>Apr-04<br>Sep-03<br>Apr-04<br>In house check: Oct 03<br>Sep-03   |  |
| Model Type  RF generator HP 8684C  Power sensor E4412A  Power sensor HP 8481A  Power meter EPM E4419B  Network Analyzer HP 8753E  Fluke Process Calibrator Type 702  Calibrated by:  Approved by: | US3842U01700<br>MY41495277<br>MY41092180<br>GB41293874<br>US37390585<br>SN: 6295803<br>Name                  | 4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250) 18-Oct-01 (Agilent, No. 24BR1033101) 3-Sep-01 (ELCAL, No.2360)  Function Tentricism | In house check: Aug-05<br>Apr-04<br>Sep-03<br>Apr-04<br>In house check: Oct 03<br>Sep-03   |  |
| RF generator HP 8684C Power sensor E4412A Power sensor HP 8481A Power meter EPM E4419B Retwork Analyzer HP 8753E Riske Process Calibrator Type 702 Calibrated by:                                 | US3842U01700<br>MY41495277<br>MY41092180<br>GB41293874<br>US37390585<br>SN: 6295803<br>Name<br>Nico Vellerii | 4-Aug-99 (SPEAG, in house check Aug-02) 2-Apr-03 (METAS, No 252-0250) 18-Sep-02 (Agilent, No. 20020918) 2-Apr-03 (METAS, No 252-0250) 18-Oct-01 (Agilent, No. 24BR1033101) 3-Sep-01 (ELCAL, No.2360)  Function Tentricism | In house check: Aug-05 Apr-04 Sep-03 Apr-04 In house check: Oct 03 Sep-03 Signature Discount Control of the con |  |

880-KP0301061-A