


Impedance Plot for SN 29/15 DIP 2G450-393


2450 Head

Calibrated impedance: $52.3\Omega + 3.4j\Omega$; Measurement impedance: $50.0\Omega + 5.0j\Omega$ (within 5Ω)

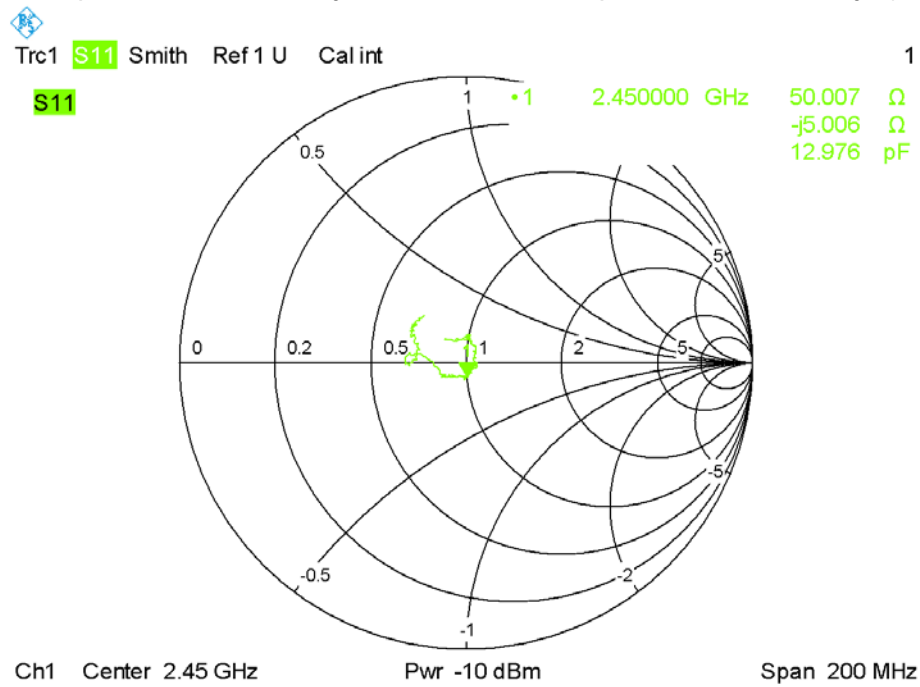

Date: 21.FEB.2024 19:04:50


Calibrated return loss: -27.80dB; Measurement return loss: -26.75dB (within 20%)

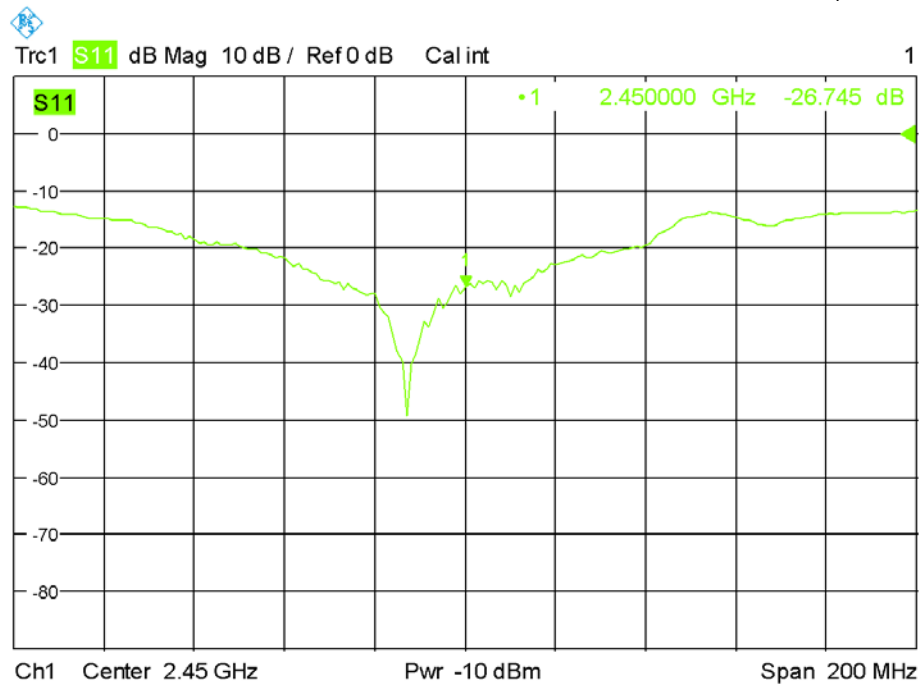

Date: 26.FEB.2024 19:28:46


Impedance Plot for SN17/22 DIP 5G000-671 5200 Head

Calibrated impedance: $54.06\Omega + 8.44j\Omega$; Measurement impedance: $51.58\Omega - 9.03j\Omega$ (within 5Ω)

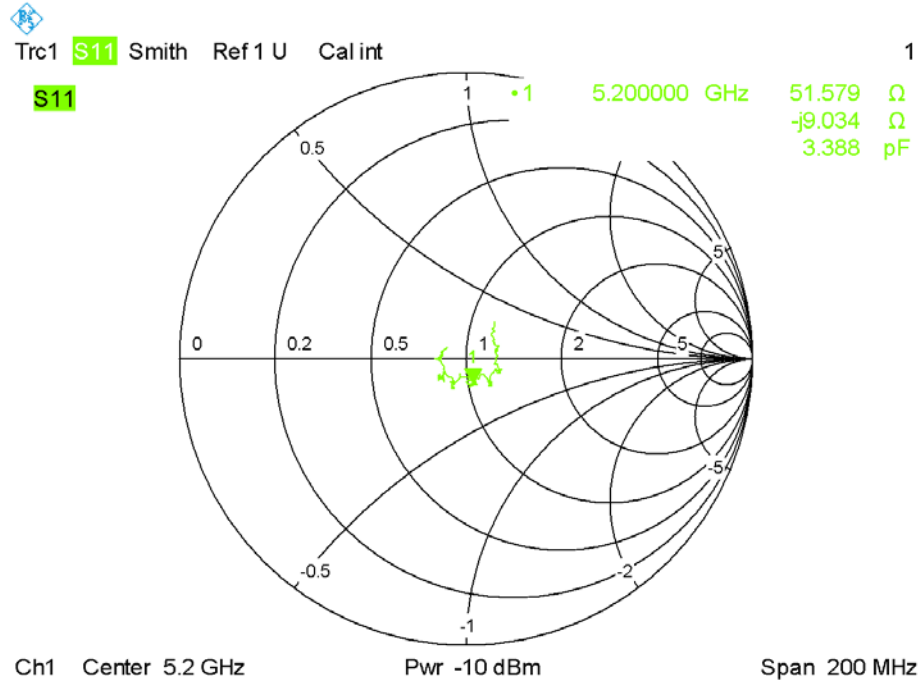

Date: 21.FEB.2024 19:26:34


Calibrated return loss: -20.52dB; Measurement return loss: -21.81dB (within 20%)

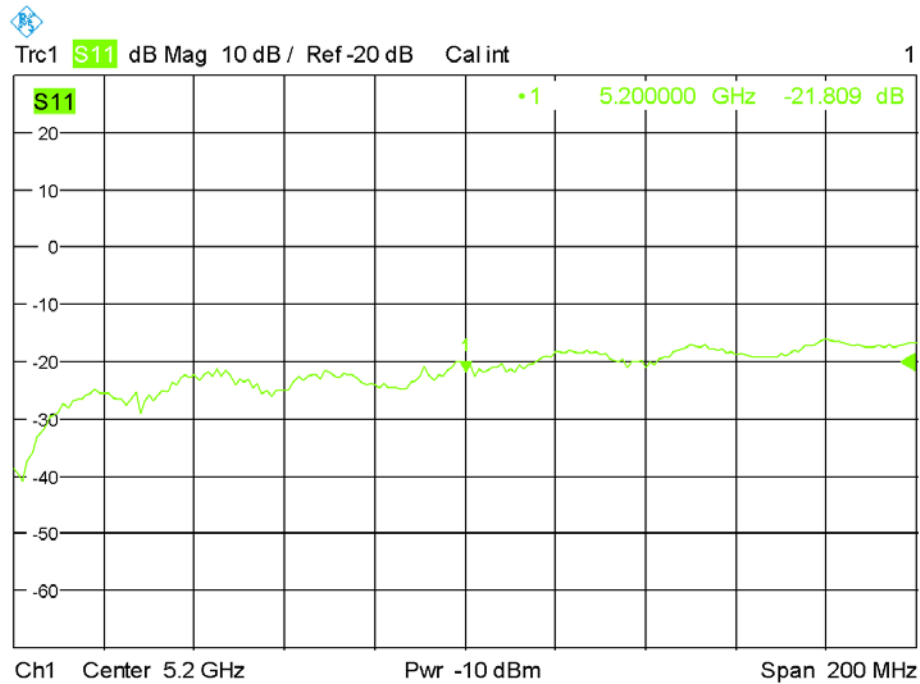

Date: 21.FEB.2024 19:25:47


Impedance Plot for SN17/22 DIP 5G000-671
5400 Head

Calibrated impedance: $47.05\Omega + 1.02j\Omega$; Measurement impedance: $50.84\Omega - 11.27j\Omega$ (within 5Ω)

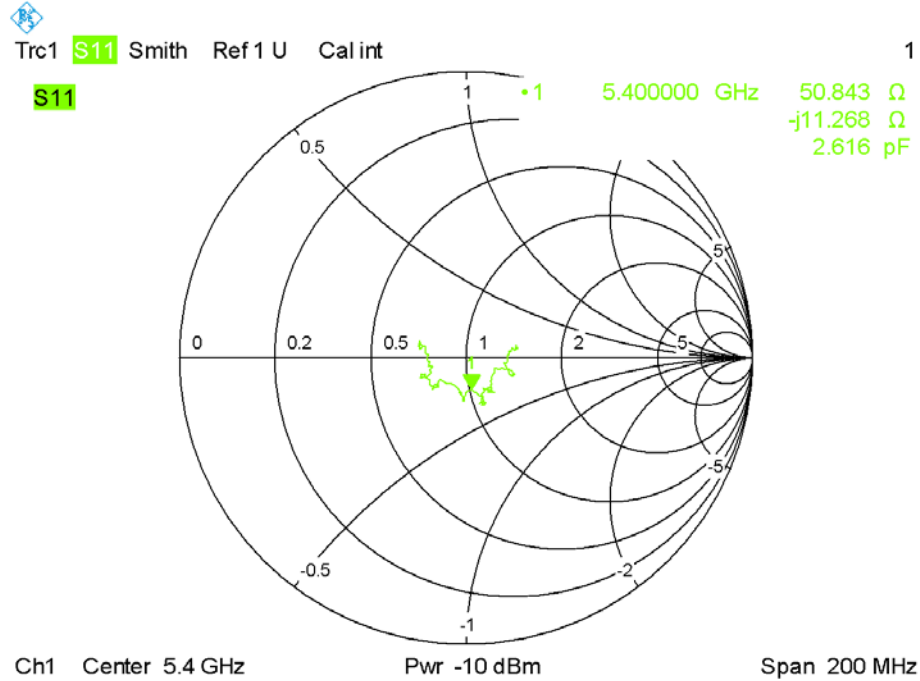

Date: 21.FEB.2024 19:27:08


Calibrated return loss: -30.10dB; Measurement return loss: -31.37dB (within 20%)

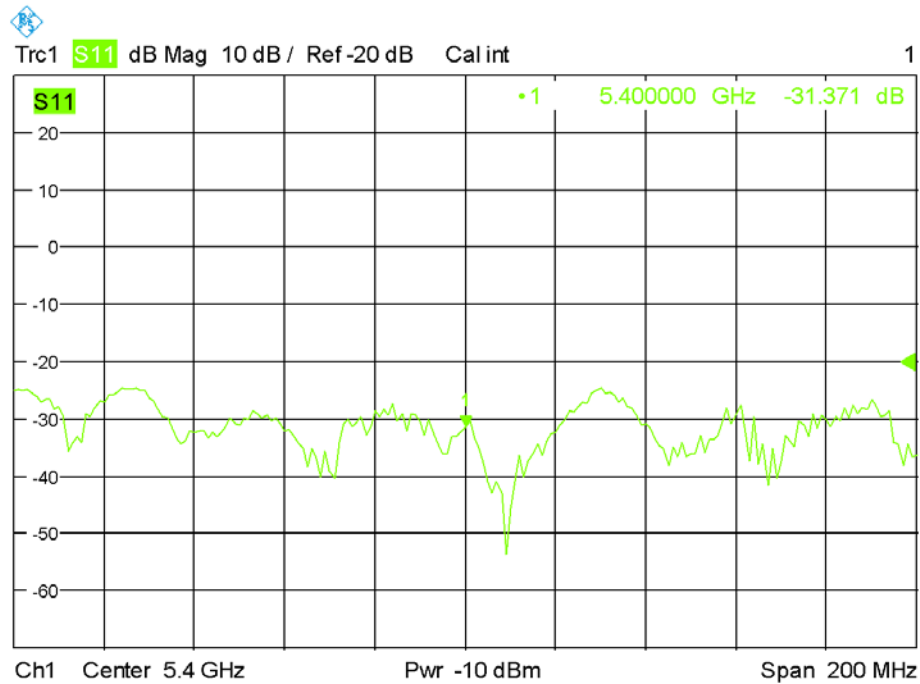

Date: 21.FEB.2024 19:27:43


Impedance Plot for SN17/22 DIP 5G000-671 5600 Head

Calibrated impedance: $49.63\Omega + 8.57j\Omega$; Measurement impedance: $51.44\Omega + 6.00j\Omega$ (within 5Ω)

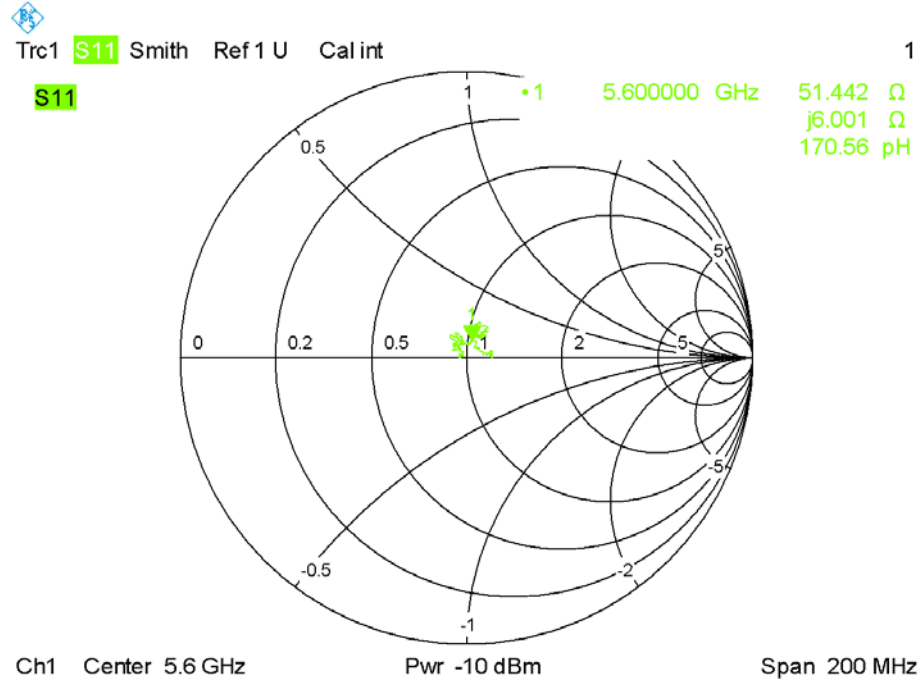

Date: 21.FEB.2024 19:55:35


Calibrated return loss: -21.30dB; Measurement return loss: -20.27dB (within 20%)

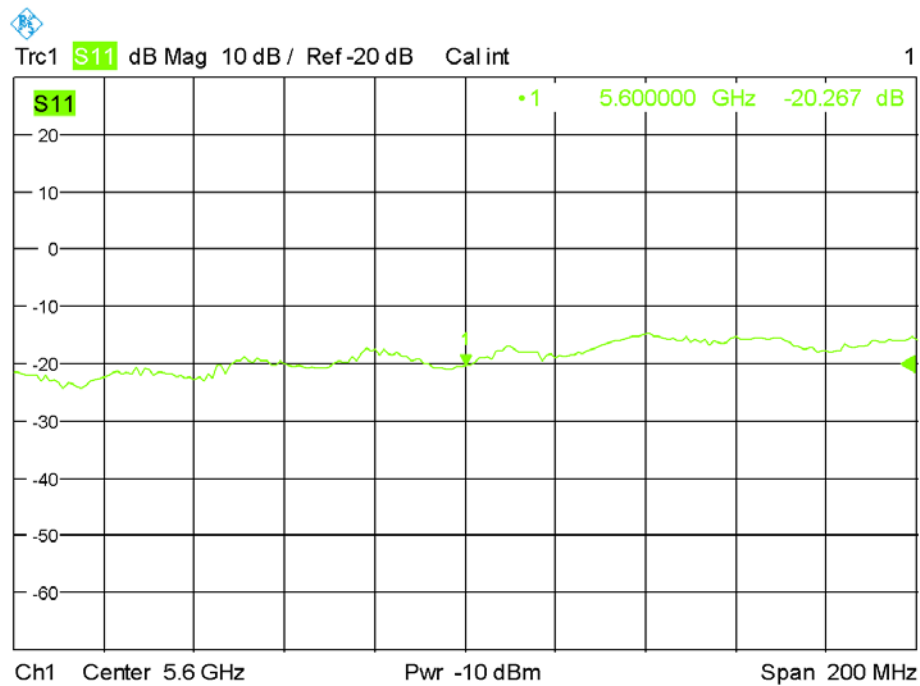

Date: 21.FEB.2024 19:55:08

Impedance Plot for SN17/22 DIP 5G000-671 5800 Head

Calibrated impedance: $47.44\Omega - 4.21j\Omega$; Measurement impedance: $45.59\Omega - 8.43j\Omega$ (within 5Ω)

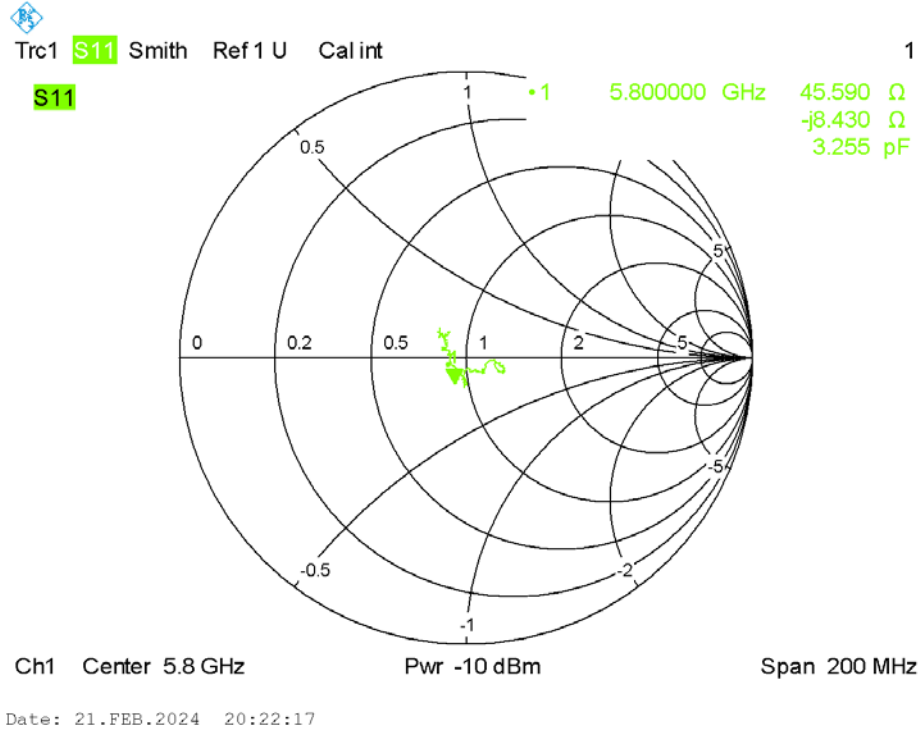

Calibrated return loss: -26.14dB; Measurement return loss: -25.57dB (within 20%)

