

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

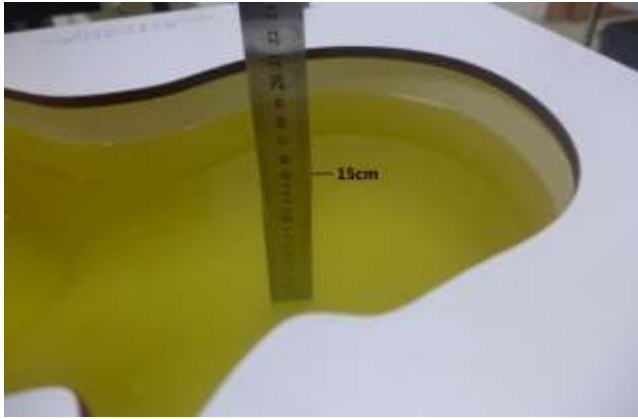
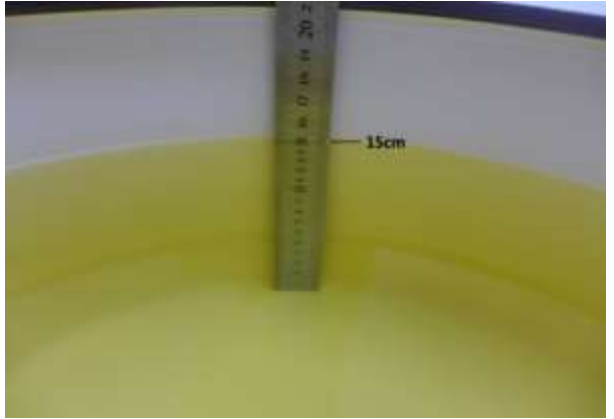
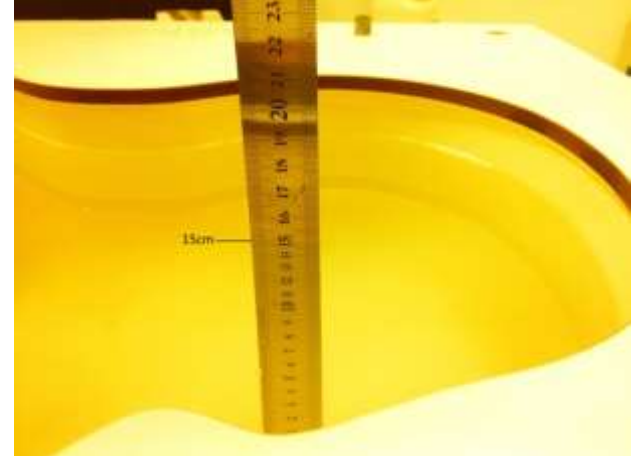
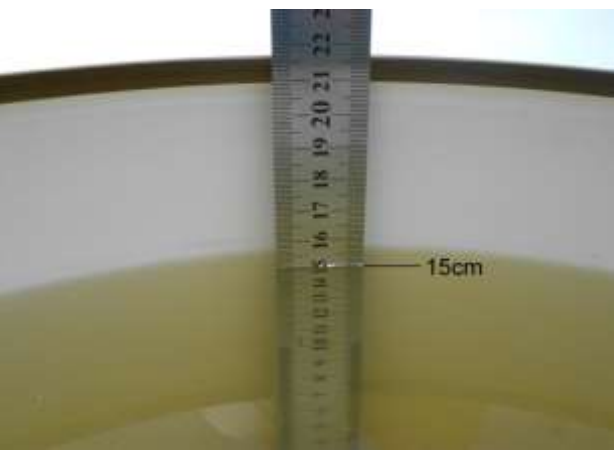
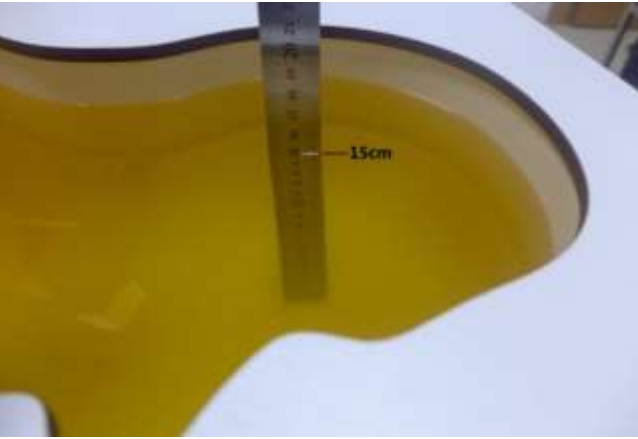
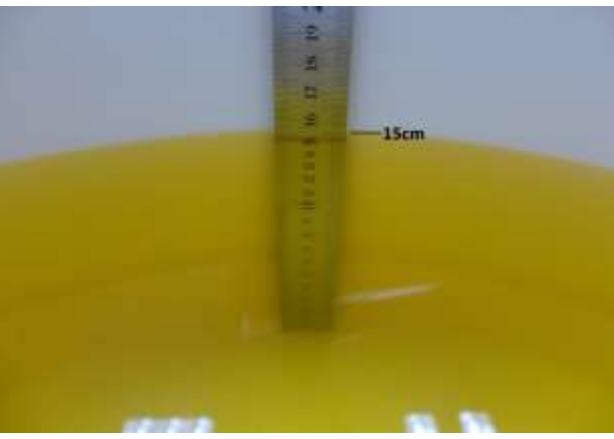
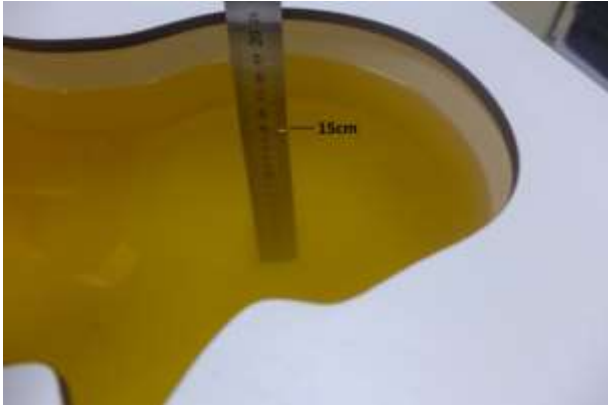
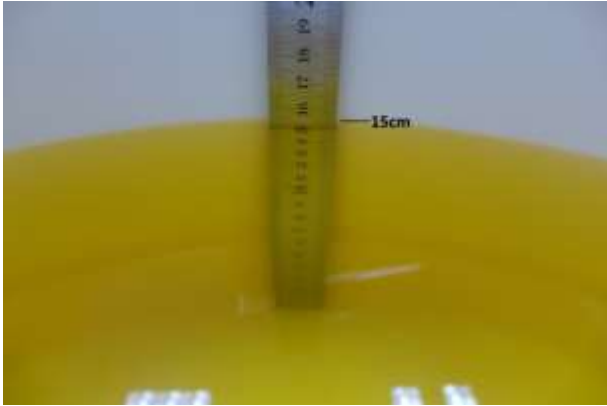
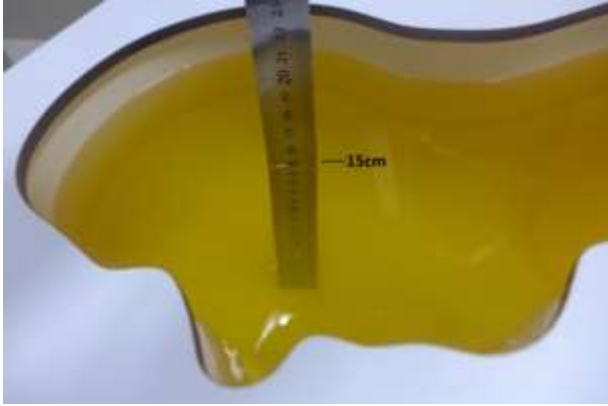
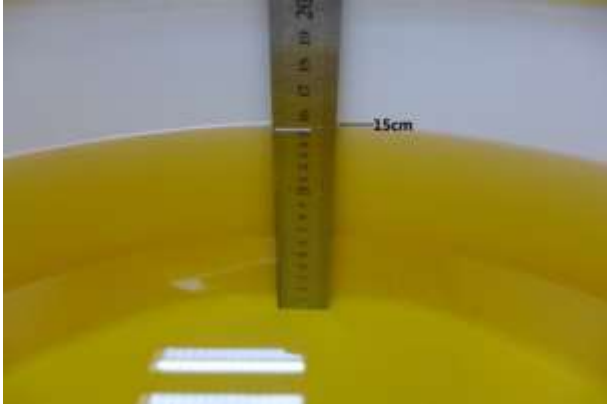
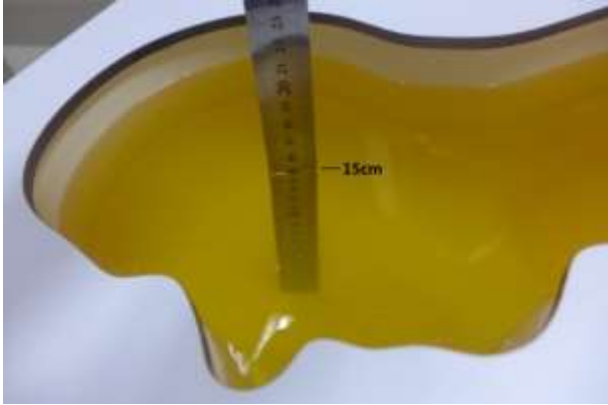
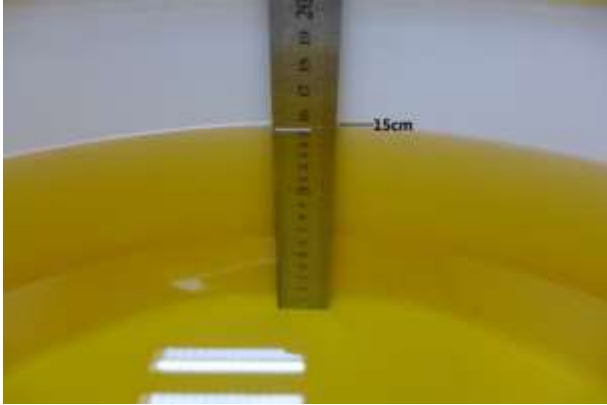
Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Body 750
	
Photo 3: Tissue Simulant Liquid for Head 835	Photo 4: Tissue Simulant Liquid for Body 835
	
Photo 5: Tissue Simulant Liquid for Head 1750	Photo 6: Tissue Simulant Liquid for Body 1750
	

Photo 7: Tissue Simulant Liquid for Head 1900	Photo 8: Tissue Simulant Liquid for Body 1900
	
Photo 9: Tissue Simulant Liquid for Head 2450	Photo 10: Tissue Simulant Liquid for Body 2450
	
Photo 11: Tissue Simulant Liquid for Head 2600	Photo 12: Tissue Simulant Liquid for Body 2600
	

3. Photographs of EUT test position

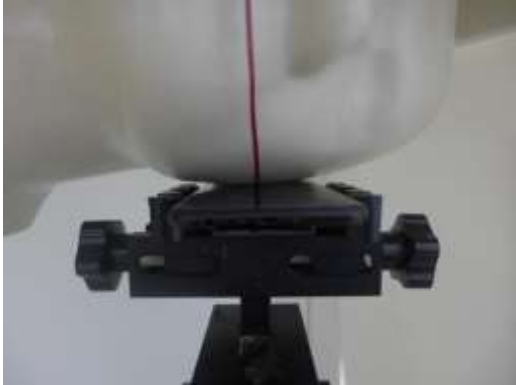
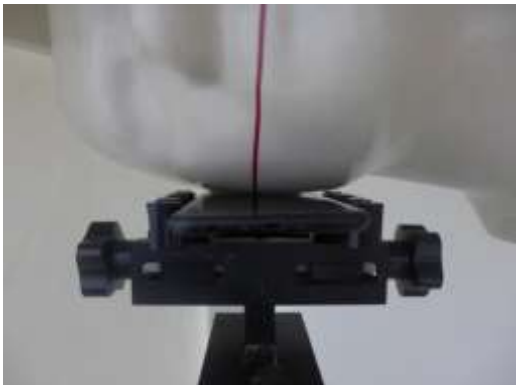
Photo 13: Left touch cheek 	Photo 14: Left tilted 15 degree 
Photo 15: Right touch cheek 	Photo 16: Right tilted 15 degree 
Photo 17: Front side 15mm 	Photo 18: Back side 15mm 

Photo 19: Front side 10mm	Photo 20: Back side 10mm
	
Photo 21: Left side 10mm	Photo 22: Right side 10mm
	
Photo 23: Top side 10mm	Photo 24: Bottom side 10mm
	

Photo 25: Back side 8mm	Photo 26: Back side 0mm
	
Photo 27: Bottom side 7mm	Photo 28: Bottom side 0mm
	

4. EUT Constructional Details

Photo 29: Front View	Photo 30: Back View
	

Photo 31: Accessory	
	