

June 04, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	UncE k =:
10753	AAC	IEEE 802.11ax (160 MHz, MCS10, 90pc duty cycle)	WLAN	9.00	±9.6
0754	AAC	IEEE 802.11ax (160 MHz, MCS11, 90pc duty cycle)	WLAN	8.94	±9.6
0755	AAC	IEEE 802.11ax (160 MHz, MCS0, 99pc duty cycle)	WLAN	8.64	±9.6
0756	AAC	IEEE 802.11ax (160 MHz, MCS1, 99pc duty cycle)	WLAN	8.77	±9.6
0757	AAC	IEEE 802.11ax (160 MHz, MCS2, 99pc duty cycle)	WLAN	8.77	±9.6
0758	AAC	IEEE 802.11ax (160 MHz, MCS3, 99pc duty cycle)	WLAN	8.69	±9.6
0759	AAC	IEEE 802.11ax (160 MHz, MCS4, 99pc duty cycle)	WLAN	8.58	±9.6
10760	AAC	IEEE 802.11ax (160 MHz, MCS5, 99pc duty cycle)	WLAN	8.49	±9.6
10761	AAC	IEEE 802.11ax (160 MHz, MCS6, 99pc duty cycle)	WLAN	8.58	±9.6
10762	AAC	IEEE 802.11ax (160 MHz, MCS7, 99pc duty cycle)	WLAN	8.49	±9.6
10763	AAC	IEEE 802.11ax (160 MHz, MCS8, 99pc duty cycle)	WLAN	8.53	±9.6
10764	AAC	IEEE 802.11ax (160 MHz, MCS9, 99pc duty cycle)	WLAN	8.54	±9.6
10765	AAC	IEEE 802.11ax (160 MHz, MCS10, 99pc duty cycle)	WLAN	8.54	±9.6
10766	AAC	IEEE 802.11ax (160 MHz, MCS11, 99pc duty cycle)	WLAN	8.51	±9.6
10767	AAG	5G NR (CP-OFDM, 1 RB, 5 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	7.99	±9.6
10768	AAE	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.01	±9.6
10769	AAD	5G NR (CP-OFDM, 1 RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.01	±9.6
10770	AAE	5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.02	±9.6
10771	AAD	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.02	±9.6
10772	AAE	5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.23	±9.6
10773	AAF	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.03	±9.6
10774	AAE	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.02	±9.6
10775	AAF	5G NR (CP-OFDM, 50% RB, 5MHz, QPSK, 15kHz)	5G NR FR1 TDD	8.31	±9.6
10776	AAE	5G NR (CP-OFDM, 50% RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.30	±9.6
10777	AAC	5G NR (CP-OFDM, 50% RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.30	±9.6
10778	AAE	5G NR (CP-OFDM, 50% RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.34	±9.6
10779	AAC	5G NR (CP-OFDM, 50% RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.42	±9.6
10780	AAE	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.38	±9.6
10781	AAF	5G NR (CP-OFDM, 50% RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.38	±9.6
0782	AAE	5G NR (CP-OFDM, 50% RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.43	±9.6
10783	AAG	5G NR (CP-OFDM, 100% RB, 5 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.31	±9.6
10784	AAE	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.29	±9.6
10785	AAD	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.40	±9.6
10786	AAE	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.35	±9.6
10787	AAD	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.44	±9.6
10788	AAE	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.39	±9.6
10789	AAF	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.37	±9.6
10790	AAE	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.39	±9.6
10791	AAG	5G NR (CP-OFDM, 1 RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.83	±9.6
10792	AAE	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.92	±9.6
10793	AAD	5G NR (CP-OFDM, 1 RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.95	±9.6
10794	AAE	5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.82	±9.6
10795	AAD	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.84	±9.6
10796	AAE	5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.82	±9.6
10797	AAF	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.01	±9.6
10798	AAE	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.89	±9.6
10799	AAF	5G NR (CP-OFDM, 1 RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.93	±9.6
10801	AAF	5G NR (CP-OFDM, 1 RB, 80 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.89	±9.6
10802	AAE	5G NR (CP-OFDM, 1 RB, 90 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.87	±9.6
10803	AAF	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.93	±9.6
10805	AAE	5G NR (CP-OFDM, 50% RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	±9.6
10806	AAD	5G NR (CP-OFDM, 50% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.37	±9.6
10809	AAE	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	±9.6
10810	AAF	5G NR (CP-OFDM, 50% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	±9.6
10812	AAF	5G NR (CP-OFDM, 50% RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.35	±9.6
10817	AAG	5G NR (CP-OFDM, 100% RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.35	±9.6
10818	AAE	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	±9.6
10819	AAD	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.33	±9.6
10820	AAE	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.30	±9.6
10821	AAD	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.41	±9.6
10822	AAE	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.41	±9.6
10823	AAF	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.36	±9.6
10824	AAE	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.39	±9.6
10825	AAF	5G NR (CP-OFDM, 100% RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	B.41	±9.6
10827	AAF	5G NR (CP-OFDM, 100% RB, 80 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.42	±9.6
10828	AAE	5G NR (CP-OFDM, 100% RB, 90 MHz, QPSK, 30 kHz)			

Certificate No: EX-7689\_Jun24

Page 19 of 22



June 04, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
10829	AAF	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.40	±9.6
10830	AAE	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.63	±9.6
10831	AAD	5G NR (CP-OFDM, 1 RB, 15 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.73	±9.6
10832	AAE	5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.74	±9.6
10833	AAD	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.70	±9.6
10834	AAE	5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.75	±9.6
10835	AAF	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.70	±9.6
10836	AAE	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.66	±9.6
10837	AAF	5G NR (CP-OFDM, 1 RB, 60 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.68	±9.6
10839	AAF	5G NR (CP-OFDM, 1 RB, 80 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.70	±9.6
10840	AAE	5G NR (CP-OFDM, 1 RB, 90 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.67	±9.6
10841	AAF	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.71	±9.6
10843	AAD	5G NR (CP-OFDM, 50% RB, 15 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.49	±9.6
10844	AAE	5G NR (CP-OFDM, 50% RB, 20 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.34	±9.6
10846	AAE	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	±9.6
10854	AAE	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.34	±9.6
10855	AAD	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.36	±9.6
10856	AAE	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.37	±9.6
10857	AAD	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.35	±9.6
10858	AAE	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.36	±9.6
10859	AAF	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.34	±9.6
10860	AAE	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	±9.6
10861	AAF	5G NR (CP-OFDM, 100% RB, 60 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.40	±9.6
10863	AAF	5G NR (CP-OFDM, 100% RB, 80 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	±9.6
10864	AAE	5G NR (CP-OFDM, 100% RB, 90 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.37	±9.6
10865	AAF	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	±9.6
0866	AAF	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
0868	AAF	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.89	±9.6
0869	AAE	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.75	±9.6
0870	AAE	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.86	±9.6
0871	AAE	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	5.75	±9.6
10872	AAE	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.52	±9.6
10873	AAE	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.61	±9.6
10874	AAE	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.65	±9.6
10875	AAE	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	7.78	±9.6
10876	AAE	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	8.39	19.6
10877	AAE	5G NR (CP-OFDM, 1 RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	7.95	±9.6
10878	AAE	5G NR (CP-OFDM, 100% RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	8.41	±9.6
10879	AAE	5G NR (CP-OFDM, 1 RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.12	±9.6
10880	AAE	5G NR (CP-OFDM, 100% RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.38	±9.6
10881	AAE	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.75	±9.6
10882	AAE	5G NR (DFT:s-OFDM, 100% RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.96	±9.6
10883	AAE	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.57	±9.6
0884	AAE	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.53	±9.6
10885	AAE	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.61	±9.6
10886	AAE	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.65	±9.6
10887	AAE	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	7.78	±9.6
10888	AAE	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	8.35	±9.6
0889	AAE	5G NR (CP-OFDM, 1 RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	B.02	±9.6
0890	AAE	5G NR (CP-OFDM, 100% RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	8.40	±9.6
10891	AAE	5G NR (CP-CFDM, 1 RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.13	±9.6
0892	AAE	5G NR (CP-CFDM, 100% RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.41	±9.6
0897	AAE	5G NR (DFT:s-OFDM, 1 RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.66	±9.6
0898	AAC	5G NR (DFT-s-OFDM, 1 RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.67	±9.6
0899	AAB	5G NR (DFT-s-OFDM, 1 RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.67	±9.6
0900	AAC	5G NR (DFT-6-OFDM, 1 RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
0901	AAB	5G NR (DFT-s-OFDM, 1 RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10902	AAC	5G NR (DFT-s-OFDM, 1 RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10903	AAD	5G NR (DFT-8-OFDM, 1 RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10904	AAC	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10905	AAD	5G NR (DFT-s-OFDM, 1 RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10906	AAD	5G NR (DFT-s-OFDM, 1 RB, 80 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	±9.6
10907	AAE	5G NR (DFT-s-OFDM, 50% RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.78	±9.6
10908	AAC	5G NR (DFT-s-OFDM, 50% RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.93	±9.6
10909	AAB	5G NR (DFT-s-OFDM, 50% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.96	±9.6
10910	AAC	5G NR (DFT-s-OFDM, 50% RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.83	±9.6

Certificate No: EX-7689\_Jun24

Page 20 of 22



June 04, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k =
0911	AAB	5G NR (DFT-s-OFDM, 50% RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.93	±9.6
0912	AAC	5G NR (DFT-s-OFDM, 50% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.84	±9.6
0913	AAD	5G NR (DFT-s-OFDM, 50% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.84	±9.6
0913	AAC	5G NR (DFT-s-OFDM, 50% RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.85	±9.6
			5G NR FR1 TDD	5.83	±9.6
0915	AAD	5G NR (DFT-s-OFDM, 50% RB, 60 MHz, OPSK, 30 kHz)	5G NR FRI TDD	5.87	±9.6
0916	AAD	5G NR (DFT-s-OFDM, 50% RB, 80 MHz, OPSK, 30 kHz)			
0917	AAD	5G NR (CFT-s-OFDM, 50% RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.94	±9.6
0918	AAE	5G NR (DFT-s-OFDM, 100% RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.86	±9.6
0919	AAC	5G NR (DFT-s-OFDM, 100% RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.86	±9.6
0920	AAB	5G NR (DFT-s-OFDM, 100% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.87	±9.6
0921	AAC	5G NR (DFT-8-OFDM, 100% RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.84	±9.6
0922	AAB	5G NR (DFT-s-OFDM, 100% RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.82	±9.6
0923	AAC	5G NR (DFT-s-OFDM, 100% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.84	±9.6
0924	AAD	5G NR (DFT-s-OFDM, 100% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.84	±9.6
0925	AAC	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.95	±9.6
0926	AAD	5G NR (DFT-s-OFDM, 100% RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.84	±9.6
0927	AAD	5G NR (DFT-s-OFDM, 100% RB, 80 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.94	±9.6
0928	AAD	5G NR (DFT-s-OFDM, 1 RB, 5 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.52	±9.6
0929	AAD	5G NR (DFT-s-OFDM, 1 RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.52	±9.6
0930	AAC	5G NR (DFT-s-OFDM, 1 RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.52	±9.6
0931	AAC	5G NR (DFTs-OFDM, 1 RB, 20 MHz, QPSK, 15 kHz)	5G NB FB1 FDD	5.51	+9.6
0931	AAC	5G NR (DFT-s-OFDM, 1 RB, 25 MHz, OPSK, 15 KHz)	5G NR FR1 FDD	5.51	±9.6
	AAC		5G NR FR1 FDD	5.51	±9.6
0933	AAC	5G NR (DFT-s-OFDM, 1 RB, 30 MHz, OPSK, 15 kHz)	5G NR FR1 FDD		
0934	100000	5G NR (DFT-s-OFDM, 1 RB, 40 MHz, QPSK, 15 kHz)		5.51	±9.6
0935	AAD	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.51	±9.6
0936	AAD	5G NR (DFT-s-OFDM, 50% RB, 5 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.90	±9.6
0937	AAD	5G NR (DFT-s-OFDM, 50% RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.77	±9.6
0938	AAC	5G NR (DFT-s-OFDM, 50% RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.90	±9.6
0939	AAC	5G NR (DFT-s-OFDM, 50% RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.82	±9.6
0940	AAC	5G NR (DFT-s-OFDM, 50% RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.89	±9.6
0941	AAC	5G NR (DFT-s-OFDM, 50% RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.83	±9.6
0942	AAC	5G NR (DFT-s-OFDM, 50% RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.85	±9.6
0943	AAD	5G NR (DFT-s-OFDM, 50% RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.95	±9.6
0944	AAD	5G NR (DFT-s-OFDM, 100% RB, 5MHz, QPSK, 15kHz)	5G NR FR1 FDD	5.81	±9.6
0945	AAD	5G NR (DFT-s-OFDM, 100% RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.85	±9.6
0946	AAC	5G NR (DFT-s-OFDM, 100% RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.83	±9.6
0947	AAC	5G NR (DFT-s-OFDM, 100% RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.87	±9.6
0948	AAC	5G NR (DFT-s-OFDM, 100% RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.94	±9.6
0949	AAC	5G NR (DFT-s-OFDM, 100% RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.87	+9.6
0950	AAC	5G NR (DFT-s-OFDM, 100% RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.94	+9.6
0951	AAD	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 FDD	5.92	+9.6
10952	AAA	5G NR DL (CP-OFDM, TM 3.1, 5MHz, 64-QAM, 15kHz)	5G NR FR1 FDD	8.25	±9.6
				- ALCONT	
0953	AAA	5G NR DL (CP-OFDM, TM 3.1, 10 MHz, 64-QAM, 15 kHz)	5G NR FR1 FDD	8.15	±9.6
0954	AAA	5G NR DL (CP-OFDM, TM 3.1, 15MHz, 64-QAM, 15kHz)	5G NR FR1 FDD	8.23	±9.6
0955	AAA	5G NR DL (CP-OFDM, TM 3.1, 20 MHz, 64-QAM, 15 kHz)	5G NR FR1 FDD	8.42	±9.6
0956	AAA	5G NR DL (CP-OFDM, TM 3.1, 5 MHz, 64-QAM, 30 kHz)	5G NR FR1 FDD	8.14	±9.6
0957	AAA	5G NR DL (CP-OFDM, TM 3.1, 10 MHz, 64-QAM, 30 kHz)	5G NR FR1 FDD	8.31	±9.6
0958	AAA	5G NR DL (CP-OFDM, TM 3.1, 15 MHz, 64-QAM, 30 kHz)	5G NR FR1 FDD	8.61	±9.
0959	AAA	5G NR DL (CP-OFDM, TM 3.1, 20 MHz, 64-QAM, 30 kHz)	5G NR FR1 FDD	8.33	±9.6
0960	AAE	5G NR DL (CP-OFDM, TM 3.1, 5 MHz, 64-QAM, 15 kHz)	5G NR FR1 TDD	9.32	±9.
0961	AAC	5G NR DL (CP-OFDM, TM 3.1, 10 MHz, 64-QAM, 15 kHz)	5G NR FR1 TDD	9.36	±9.8
0962	AAB	5G NR DL (CP-OFDM, TM 3.1, 15 MHz, 64-QAM, 15 kHz)	5G NR FR1 TDD	9.40	±9.6
0963	AAC	5G NR DL (CP-OFDM, TM 3.1, 20 MHz, 64-QAM, 15 kHz)	5G NR FR1 TDD	9.55	±9.4
0964	AAE	5G NR DL (CP-OFDM, TM 3.1, 5 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.29	±9.4
0965	AAC	5G NR DL (CP-OFDM, TM 3.1, 10 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.37	±9.6
0966	AAB	5G NR DL (CP-OFDM, TM 3.1, 15 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.55	±0.0
0967	AAC	5G NR DL (CP-OFDM, TM 3.1, 20 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.35	±9.0
0968	AAD	5G NR DL (CP-OFDM, TM 3.1, 20 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.42	-
0958	-	5G NR (CP-OFDM, 1M 3.1, 100 MHz, 64-QAM, 30 KHz) 5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 15 kHz)			±9.6
			5G NR FR1 TDD	11.59	±9.6
0973	-	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	9.06	±9.6
10974	- in the second second	5G NR (CP-OFDM, 100% RB, 100 MHz, 256-QAM, 30 kHz)	5G NR FR1 TDD	10.28	±9.6
10978		ULLA BDR	ULLA	1.16	±9.6
10979	AAA	ULLA HDR4	ULLA	8.58	±9.6
10980	AAA	ULLA HDR8	ULLA	10.32	±9.6
10981	AAA	ULLA HDRp4	ULLA	3.19	±9.6
10982	AAA	ULLA HDRp8	ULLA	3.43	19.6

Certificate No: EX-7689\_Jun24

Page 21 of 22



June 04, 2024

UID	Rev	Communication System Name	Group	PAR (dB)	Unc <sup>E</sup> k = 2
10983	AAC	5G NR DL (CP-OFDM, TM 3.1, 40 MHz, 64-QAM, 15 kHz)	5G NR FR1 TDD	9.31	±9.6
10984	AAB	5G NR DL (CP-OFDM, TM 3.1, 50 MHz, 64-QAM, 15 kHz)	5G NR FR1 TDD	9.42	±9.6
10985	AAC	5G NR DL (CP-OFDM, TM 3.1, 40 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.54	±9.6
10986	AAB	5G NR DL (CP-OFDM, TM 3.1, 50 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.50	±9.6
10987	AAC	5G NR DL (CP-OFDM, TM 3.1, 60 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.53	±9.6
10988	AAB	5G NR DL (CP-OFDM, TM 3.1, 70 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.38	±9.6
10989	AAC	5G NR DL (CP-OFDM, TM 3.1, 80 MHz, 84-QAM, 30 kHz)	5G NR FR1 TDD	9.33	±9.6
10990	AAB	5G NR DL (CP-OFDM, TM 3.1, 90 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	9.52	±9.6
11003	AAA	5G NR DL (CP-OFDM, TM 3.1, 30 MHz, 64-QAM, 15 kHz)	5G NR FR1 TDD	10.24	±9.6
11004	AAA	5G NR DL (CP-OFDM, TM 3.1, 30 MHz, 64-QAM, 30 kHz)	5G NR FR1 TDD	10.73	±9.6
11005	AAA	5G NR DL (CP-OFDM, TM 3.1, 25 MHz, 64-QAM, 15 kHz)	5G NR FR1 FDD	8.70	±9.6
11006	AAA	5G NR DL (CP-OFDM, TM 3.1, 30 MHz, 64-QAM, 15 kHz)	5G NR FR1 FDD	8.55	±9.6
11007	AAA	5G NR DL (CP-OFDM, TM 3.1, 40 MHz, 64-QAM, 15 kHz)	5G NR FR1 FDD	8.46	±9.6
11008	AAA	5G NR DL (CP-OFDM, TM 3.1, 50 MHz, 64-QAM, 15 kHz)	5G NR FR1 FDD	8.51	±9.6
11009	AAA	5G NR DL (CP-OFDM, TM 3.1, 25 MHz, 64-QAM, 30 kHz)	5G NR FR1 FDD	8.76	±9.6
11010	AAA	5G NR DL (CP-OFDM, TM 3.1, 30 MHz, 64-QAM, 30 kHz)	5G NR FR1 FDD	8.95	±9.6
11011	AAA	5G NR DL (CP-OFDM, TM 3.1, 40 MHz, 64-QAM, 30 kHz)	5G NR FR1 FDD	8.96	±9.6
11012	AAA	5G NR DL (CP-OFDM, TM 3.1, 50 MHz, 64-QAM, 30 kHz)	5G NR FR1 FDD	8.68	±9.6
11013	AAB	IEEE 802.11be (320 MHz, MCS1, 99pc duty cycle)	WLAN	8.47	±9.6
11014	AAB	IEEE 802.11be (320 MHz, MCS2, 99pc duty cycle)	WLAN	8.45	±9.6
11015	AAB	IEEE 802.11be (320 MHz, MCS3, 99pc duty cycle)	WLAN	8.44	±9.6
11016	AAB	IEEE 802.11be (320 MHz, MCS4, 99pc duty cycle)	WLAN	8.44	±9.6
11017	AAB	IEEE 802.11be (320 MHz, MCS5, 99pc duty cycle)	WLAN	8.41	±9.6
11018	AAB	IEEE 802.11be (320 MHz, MCS6, 99pc duty cycle)	WLAN	8.40	±9.6
11019	AAB	IEEE 802.11be (320 MHz, MCS7, 99pc duty cycle)	WLAN	8.29	±9.6
11020	AAB	IEEE 802.11be (320 MHz, MCS8, 99pc duty cycle)	WLAN	8.27	±9.6
11021	AAB	IEEE 802.11be (320 MHz, MCS9, 99pc duty cycle)	WLAN	8.46	±9.6
11022	AAB	IEEE 802.11be (320 MHz, MCS10, 99pc duty cycle)	WLAN	8.36	±9.6
11023	AAB	IEEE 802.11be (320 MHz, MCS11, 99pc duty cycle)	WLAN	8.09	±9.6
11024	AAB	IEEE 802.11be (320 MHz, MCS12, 99pc duty cycle)	WLAN	8.42	±9.6
11025	AAB	IEEE 802.11be (320 MHz, MCS13, 99pc duty cycle)	WLAN	8.37	±9.6
11026	AAB	IEEE 802.11be (320 MHz, MCS0, 99pc duty cycle)	WLAN	8.39	±9.6

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX-7689\_Jun24

Page 22 of 22



## ANNEX E: D835V2 Dipole Calibration Certificate

Calibration Laborator Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zuric			<ul> <li>S Schweizerischer Kalibrierdienst</li> <li>Service suisse d'étalonnage</li> <li>Servizio svizzero di taratura</li> <li>Swiss Calibration Service</li> </ul>
Accredited by the Swiss Accreditat The Swiss Accreditation Service Multilateral Agreement for the re	is one of the signatorie		Accreditation No.: SCS 0108
Client TA Shanghai City		Certificate No	D835V2-4d020_Sep23
CALIBRATION C	ERTIFICAT	E	
Object	D835V2 - SN:4d	020	
Calibration procedure(s)	QA CAL-05.v12 Calibration Proce	edure for SAR Validation Source	es between 0.7-3 GHz
Calibration date:	September 15, 2	023	
The measurements and the uncert	lainties with confidence p ed in the closed laborato	ional standards, which realize the physical u robability are given on the following pages a ry facility: environment temperature $(22 \pm 3)$	ind are part of the certificate.
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TF Primary Standards	lainties with confidence p ed in the closed laborato	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.)	nd are part of the certificate. °C and humidity < 70%. Scheduled Calibration
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TF Primary Standards Power meter NRP2	ainties with confidence p ed in the closed laborato E critical for calibration)	robability are given on the following pages a ry facility: environment temperature $(22\pm3)$	nd are part of the certificate. °C and humidity < 70%.
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TF Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805)	nd are part of the certificate. °C and humidity < 70%. Scheduled Calibration Mar-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k)	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805)	nd are part of the certificate. °C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&Tt Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: BH9394 (20k) SN: 310982 / 06327	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810)	nd are part of the certificate. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Mar-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k)	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805)	nd are part of the certificate. °C and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24 Mar-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103244 SN: 103245 SN: 8H9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601	robability are given on the following pages a ry facility: environment temperature (22 ± 3) <u>Cal Date (Certificate No.)</u> 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22)	rnd are part of the certificate. °C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Jan-24 Dec-23
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID #	robability are given on the following pages a ry facility: environment temperature (22 ± 3) <u>Cal Date (Certificate No.)</u> 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house)	rnd are part of the certificate. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103244 SN: 103245 SN: 8H9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601	robability are given on the following pages a ry facility: environment temperature (22 ± 3) <u>Cal Date (Certificate No.)</u> 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) <u>Check Date (in house)</u> 30-Oct-14 (in house check Oct-22)	Ind are part of the certificate. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: 6B39512475	robability are given on the following pages a ry facility: environment temperature (22 ± 3) <u>Cal Date (Certificate No.)</u> 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house)	rnd are part of the certificate. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A Reference R&S SMT-06	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 103245 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: WY41093315 SN: 100972	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22)	Ind are part of the certificate. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: WY41093315	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22)	rd are part of the certificate. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer Agilent E8358A	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 310982 / 06327 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: WY41093315 SN: 100972 SN: US41080477 Name	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22)	Ind are part of the certificate. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24 In house check: Oct-24 In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer Agilent E8358A	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: GB39512475 SN: US37292783 SN: MY41093315 SN: 100972 SN: US41080477	robability are given on the following pages a ry facility: environment temperature (22 ± 3) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22)	In are part of the certificate. *C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TF Primary Standards Power meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sen	ainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 310982 / 06327 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: WY41093315 SN: 100972 SN: US41080477 Name	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22) Function	In are part of the certificate. C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Power meter NRP2 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer Agilent E8358A Calibrated by:	ainties with confidence p ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 310982 / 06327 SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: US37292783 SN: US37292783 SN: US41080477 Name Paulo Pina Sven Kühn	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22) Function Laboratory Technician	Ind are part of the certificate. "C and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24 Signature



Calibration Laboratory of Schweizerischer Kalibrierdienst s Schmid & Partner Service suisse d'étalonnage C Engineering AG Servizio svizzero di taratura Zeughausstrasse 43, 8004 Zurich, Switzerland S Swiss Calibration Service Accredited by the Swiss Accreditation Service (SAS) Accreditation No.: SCS 0108 The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Glossary: TSL tissue simulating liquid ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020. b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz" Additional Documentation: c) DASY System Handbook Methods Applied and Interpretation of Parameters: Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The source is mounted in a touch configuration below the . center marking of the flat phantom. Return Loss: This parameter is measured with the source positioned under the liquid filled ٠ phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. . SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna ٠ connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D835V2-4d020\_Sep23

Page 2 of 6

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

## Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.93 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	6222	

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.49 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.75 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 c) of Hood TSI	an dition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL SAR measured SAR for nominal Head TSL parameters	condition 250 mW input power normalized to 1W	1.62 W/kg

Certificate No: D835V2-4d020\_Sep23

Page 3 of 6



## Appendix (Additional assessments outside the scope of SCS 0108)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.6 Ω - 3.8 jΩ	
Return Loss	- 28.3 dB	

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.390 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

## Additional EUT Data

Manufactured by		SPEAG	
cate No: D835V2-4d020_Sep23			_
ale 110. 0000 vz.40020_oep20	Page 4 of 6		

## **DASY5 Validation Report for Head TSL**

Test Laboratory: SPEAG, Zurich, Switzerland

Date: 15.09.2023

## DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d020


Communication System: UID 0 - CW; Frequency: 835 MHz Medium parameters used: f = 835 MHz;  $\sigma = 0.93$  S/m;  $\varepsilon_r = 42.1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(9.69, 9.69, 9.69) @ 835 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19.12.2022
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 66.58 V/m; Power Drift = -0.09 dBPeak SAR (extrapolated) = 3.74 W/kg**SAR(1 g) = 2.49 \text{ W/kg}; SAR(10 g) = 1.62 \text{ W/kg}** Smallest distance from peaks to all points 3 dB below = 16 mmRatio of SAR at M2 to SAR at M1 = 66.4%Maximum value of SAR (measured) = 3.27 W/kg

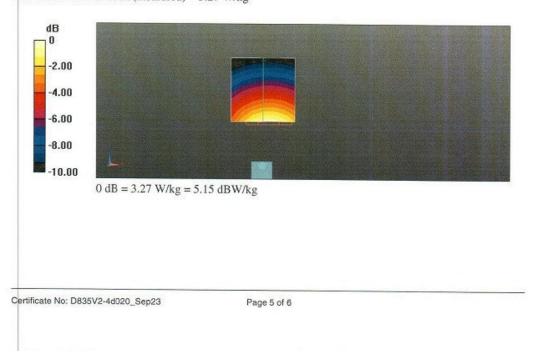



Impedance Measurement Plot for Head TSL View Channel Sweep Calibration Irace Scale Marker System Window Help File 835.000000 MHz 50 555 Ω 49.743 pF -3.8318 Q \$35.000000 MHz 38.476 mU -79.571 ° Ch 1 Avg = 20 Ch1: Start 635.000 MHz Stop 1.03500 GHz 0.00 dB S1 296 dE 5.00 0.00 5.00 10.00 15.00 20.00 -25.00 30.00 -35.00 40.00 Ch 1 Avg = 20 Ch 1: Start 635.000 MHz Stop 1.03500 GHz Status CH 1: 511 C\* 1-Port Avg=20 Delay LCL Certificate No: D835V2-4d020\_Sep23 Page 6 of 6



Report No.: R2407A0983-S1V1

## ANNEX F: D1750V2 Dipole Calibration Certificate

Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com	http://www.cai	ct.ac.cn	
Client AUDE			22-60230
CALIBRATION CE	RTIFICAT	Έ	
Object	D1750\	/2 - SN: 1023	
Calibration Procedure(s)	FF-Z11	-003-01	
	Calibrat	tion Procedures for dipole validation kits	
Calibration date:	June 21	1, 2022	
	a anoarto.		
pages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used	conducted in t	he closed laboratory facility: environment or calibration)	temperature (22±3)°C and
All calibrations have been humidity<70%. Calibration Equipment used	conducted in t	or calibration)	
All calibrations have been numidity<70%. Calibration Equipment used	conducted in the conduc		
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards	conducted in the conduc	or calibration) Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	conducted in the conducted in the conducted in the conducted for t	Cal Date (Calibrated by, Certificate No.) 24-Sep-21 (CTTL, No.J21X08326)	Scheduled Calibration Sep-22
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S	conducted in the conducted in the conducted in the conducted for t	Cal Date (Calibrated by, Certificate No.) 24-Sep-21 (CTTL, No.J21X08326) 24-Sep-21 (CTTL, No.J21X08326)	Scheduled Calibration Sep-22 Sep-22
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4	conducted in t (M&TE critical for ID # 106277 104291 SN 7464	Cal Date (Calibrated by, Certificate No.) 24-Sep-21 (CTTL, No.J21X08326) 24-Sep-21 (CTTL, No.J21X08326) 26-Jan-22(SPEAG,No.EX3-7464_Jan22)	Scheduled Calibration Sep-22 Sep-22 Jan-23 Jan-23
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4	conducted in the critical for the critic	Cal Date (Calibrated by, Certificate No.) 24-Sep-21 (CTTL, No.J21X08326) 24-Sep-21 (CTTL, No.J21X08326) 26-Jan-22(SPEAG,No.EX3-7464_Jan22) 12-Jan-22(CTTL-SPEAG,No.Z22-60007)	Scheduled Calibration Sep-22 Sep-22 Jan-23 Jan-23
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards	conducted in the conduc	Cal Date (Calibrated by, Certificate No.) 24-Sep-21 (CTTL, No.J21X08326) 24-Sep-21 (CTTL, No.J21X08326) 26-Jan-22(SPEAG,No.EX3-7464_Jan22) 12-Jan-22(CTTL-SPEAG,No.Z22-60007) Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration Sep-22 Sep-22 Jan-23 Jan-23 Scheduled Calibration
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	conducted in the conducted in the critical for the critic	Cal Date (Calibrated by, Certificate No.) 24-Sep-21 (CTTL, No.J21X08326) 24-Sep-21 (CTTL, No.J21X08326) 26-Jan-22(SPEAG,No.EX3-7464_Jan22) 12-Jan-22(CTTL-SPEAG,No.Z22-60007) Cal Date (Calibrated by, Certificate No.) 13-Jan-22 (CTTL, No.J22X00409)	Scheduled Calibration Sep-22 Sep-22 Jan-23 Jan-23 Scheduled Calibration Jan-23
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C Network Analyzer E5071C	conducted in t (M&TE critical for 104291 SN 7464 SN 1556 ID # MY49071430 MY46110673	Cal Date (Calibrated by, Certificate No.) 24-Sep-21 (CTTL, No.J21X08326) 24-Sep-21 (CTTL, No.J21X08326) 26-Jan-22(SPEAG,No.EX3-7464_Jan22) 12-Jan-22(CTTL-SPEAG,No.Z22-60007) Cal Date (Calibrated by, Certificate No.) 13-Jan-22 (CTTL, No.J22X00409) 14-Jan-22 (CTTL, No.J22X00406)	Scheduled Calibration Sep-22 Sep-22 Jan-23 Jan-23 Scheduled Calibration Jan-23 Jan-23 Signature
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	conducted in the conduc	Cal Date (Calibrated by, Certificate No.) 24-Sep-21 (CTTL, No.J21X08326) 24-Sep-21 (CTTL, No.J21X08326) 26-Jan-22(SPEAG,No.EX3-7464_Jan22) 12-Jan-22(CTTL-SPEAG,No.Z22-60007) Cal Date (Calibrated by, Certificate No.) 13-Jan-22 (CTTL, No.J22X00409) 14-Jan-22 (CTTL, No.J22X00406) Function	Scheduled Calibration Sep-22 Sep-22 Jan-23 Jan-23 Scheduled Calibration Jan-23 Jan-23

Certificate No: Z22-60230

Page 1 of 6





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

## Glossary:

TSL	tissue simulating liquid			
ConvF	sensitivity in TSL / NORMx,y,z			
N/A	not applicable or not measured			

## Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Additional Documentation:

c) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60230

Page 2 of 6







Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: ettl@chinattl.com http://www.caict.ac.en

## **Measurement Conditions**

 DASY system configuration, as far as not given on page 1.

 DASY Version
 DASY52

 Extrapolation
 Advanced Extrapolation

 Phantom
 Triple Flat Phantom 5.1C

 Distance Dipole Center - TSL
 10 mm
 with Spacer

 Zoom Scan Resolution
 dx, dy, dz = 5 mm
 Frequency

 Frequency
 1750 MHz ± 1 MHz

## **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.1	1.37 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.1 ± 6 %	1.38 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.20 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	36.8 W/kg ± 18.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	4.87 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	19.5 W/kg ± 18.7 % (k=2)

Certificate No: Z22-60230

Page 3 of 6







Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

#### Appendix (Additional assessments outside the scope of CNAS L0570)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.6Ω- 1.40jΩ	
Return Loss	- 34.0dB	

#### **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.118 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

## Additional EUT Data

Manufactured by	SPEAG

Page 4 of 6



S



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

а

## DASY5 Validation Report for Head TSL

In Collaboration with

CALIBRATION LABORATORY

p e

Date: 2022-06-21


Test Laboratory: CTTL, Beijing, China **DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN: 1023** Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1750 MHz;  $\sigma = 1.382$  S/m;  $\epsilon_r = 41.1$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN7464; ConvF(8.52, 8.52, 8.52) @ 1750 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm,

dy=5mm, dz=5mm Reference Value = 92.55 V/m; Power Drift = -0.02 dB Peak SAR (extrapolated) = 16.9 W/kg **SAR(1 g) = 9.2 W/kg; SAR(10 g) = 4.87 W/kg** Smallest distance from peaks to all points 3 dB below = 10 mm Ratio of SAR at M2 to SAR at M1 = 55% Maximum value of SAR (measured) = 14.2 W/kg

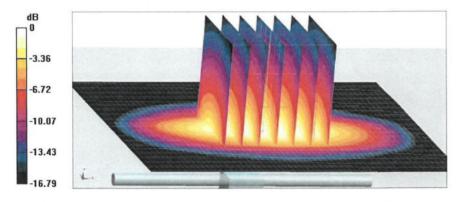

0 dB = 14.2 W/kg = 11.52 dBW/kg

Certificate No: Z22-60230

Page 5 of 6








Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

## Impedance Measurement Plot for Head TSL

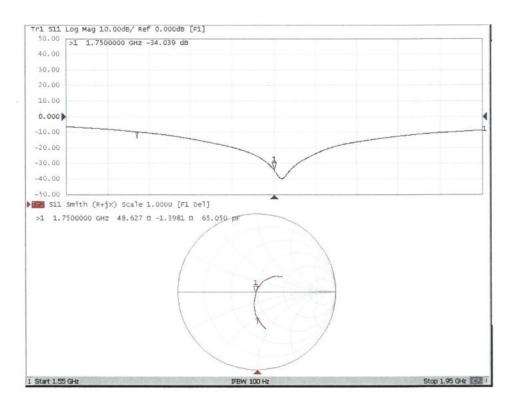

Certificate No: Z22-60230

Page 6 of 6



Report No.: R2407A0983-S1V1

## ANNEX G: D1900V2 Dipole Calibration Certificate

Add: No.52 HuaYuanBei Ro Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn		ordering rootst setting	NAS L0570
Client TA(SI	hanghai)	Certificate No: 2	3J02Z80017
CALIBRATION CI	ERTIFICAT	Έ	
Object	D1900	/2 - SN: 5d060	
Calibration Procedure(s)			
		-003-01 tion Procedures for dipole validation kits	
Calibration date:		•	
Janufation date.	Septer	ber 12, 2023	
pages and are part of the ce	artificate.	the uncertainties with confidence probability	
pages and are part of the ce	artificate.	he closed laboratory facility: environment	temperature (22±3)°C and
pages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used	artificate.	he closed laboratory facility: environment	temperature (22±3)°C and Scheduled Calibration
bages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used	ortificate. conducted in t (M&TE critical for	he closed laboratory facility: environment or calibration)	
ages and are part of the ce M calibrations have been numidity<70%. Calibration Equipment used Primary Standards	ortificate. conducted in t (M&TE critical fo ID #	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
ages and are part of the ce All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	ID # 106277 104291	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561)	Scheduled Calibration Sep-23
ages and are part of the ce All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S	ID # 106277 104291	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561)	Scheduled Calibration Sep-23 Sep-23
ages and are part of the ce All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4	ID # 106277 104291 SN 3617	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034)	Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24
ages and are part of the ce All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4	ertificate. conducted in t (M&TE critical fe ID # 106277 104291 SN 3617 SN 1556	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24 Scheduled Calibration
Pages and are part of the contract of the cont	ertificate. conducted in t (M&TE critical for ID # 106277 104291 SN 3617 SN 1556 ID #	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034)	Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24
Pages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	ertificate. conducted in t (M&TE critical for ID # 106277 104291 SN 3617 SN 1556 ID # ID # MY49071430	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107)	Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24 Scheduled Calibration Jan-24
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power Sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	ertificate. conducted in t (M&TE critical fe ID # 106277 104291 SN 3617 SN 1556 ID # MY49071430 MY46110673	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107) 10-Jan-23 (CTTL, No. J23X00104)	Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24 Scheduled Calibration Jan-24 Jan-24
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	ertificate. conducted in t (M&TE critical fe ID # 106277 104291 SN 3617 SN 1556 ID # MY49071430 MY46110673 Name	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107) 10-Jan-23 (CTTL, No. J23X00104) Function	Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24 Scheduled Calibration Jan-24 Jan-24

Certificate No: 23J02Z80017

Page 1 of 6







Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: ettl@chinattl.com http://www.caiet.ac.en

## Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation:

c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: 23J02Z80017

Page 2 of 6







Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

## **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.42 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	10 <u>0000</u> 04)	

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.4 W/kg ± 18.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.25 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	20.9 W/kg ± 18.7 % (k=2)

Certificate No: 23J02Z80017

Page 3 of 6



·	In C	ollabora	tion wit	'n		
TTL	S	p	e	а	g	
	CAL	IBRATIO	ON LAB	ORATO	ORY	



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: ettl@chinattl.com http://www.caict.ac.en

### Appendix (Additional assessments outside the scope of CNAS L0570)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.5Ω+ 6.32jΩ	
Return Loss	- 24.0dB	

## **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.102 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

## Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: 23J02Z80017

Page 4 of 6





**DASY5 Validation Report for Head TSL** 


Date: 2023-09-12

Test Laboratory: CTTL, Beijing, China **DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d060** Communication System: UID 0, CW; Frequency: 1900 MHz Medium parameters used: f = 1900 MHz;  $\sigma = 1.42$  S/m;  $\epsilon_r = 39.77$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(8.14, 8.14, 8.14) @ 1900 MHz; Calibrated: 2023-03-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration**/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 96.76 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 19.4 W/kg SAR(1 g) = 10.2 W/kg; SAR(10 g) = 5.25 W/kg Smallest distance from peaks to all points 3 dB below = 9.2 mm Ratio of SAR at M2 to SAR at M1 = 53% Maximum value of SAR (measured) = 16.0 W/kg

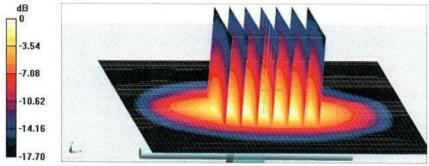

0 dB = 16.0 W/kg = 12.04 dBW/kg

Certificate No: 23J02Z80017

Page 5 of 6








Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.en

## Impedance Measurement Plot for Head TSL

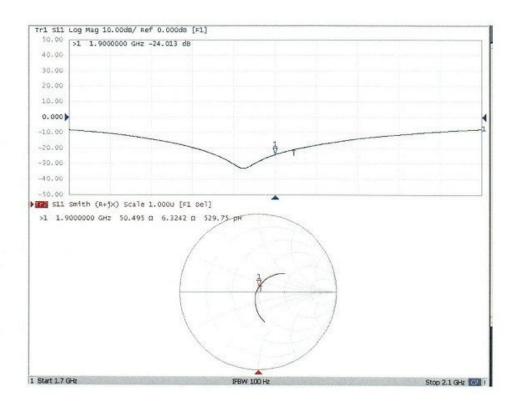

Certificate No: 23J02Z80017

Page 6 of 6



## ANNEX H: D2450V2 Dipole Calibration Certificate

Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com	http://www.caid		J02Z80018
Client TA(Sh	anghal)		002200010
Object	D2450\	/2 - SN: 786	
Calibration Procedure(s)	FF-Z11	-003-01	
	Calibrat	tion Procedures for dipole validation kits	
Calibration date:	Septem	ber 12, 2023	
pages and are part of the ce All calibrations have been	ertificate.	the uncertainties with confidence probability he closed laboratory facility: environment	
pages and are part of the ce All calibrations have been humidity<70%.	conducted in t (M&TE critical for	he closed laboratory facility: environment to	temperature (22±3)℃ and
pages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards	ortificate. conducted in t (M&TE critical for ID #	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.)	temperature (22±3)°C and Scheduled Calibration
bages and are part of the ce All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	Conducted in t (M&TE critical for ID # 106277	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561)	temperature (22±3)°C and Scheduled Calibration Sep-23
ages and are part of the ce All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S	ID # 106277 104291	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561)	temperature (22±3)°C and Scheduled Calibration Sep-23 Sep-23
bages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	ID # 106277 104291	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561)	temperature (22±3)°C and Scheduled Calibration Sep-23
bages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4	ID # 106277 104291 SN 3617	he closed laboratory facility: environment i or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161)	temperature (22±3)°C and Scheduled Calibration Sep-23 Sep-23 Mar-24
bages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4	ID # 106277 104291 SN 3617 SN 1556	he closed laboratory facility: environment or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034)	temperature (22±3)℃ and Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24
pages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards	Conducted in t (M&TE critical for ID # 106277 104291 SN 3617 SN 1556 ID #	he closed laboratory facility: environment i or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.)	temperature (22±3)℃ and Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24 Scheduled Calibration
bages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	Conducted in t conducted in t (M&TE critical for 106277 104291 SN 3617 SN 1556 ID # MY49071430	he closed laboratory facility: environment i or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107)	temperature (22±3)℃ and Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24 Scheduled Calibration Jan-24
pages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	ertificate. conducted in t (M&TE critical fe ID # 106277 104291 SN 3617 SN 1556 ID # MY49071430 MY46110673	he closed laboratory facility: environment i or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107) 10-Jan-23 (CTTL, No. J23X00104)	temperature (22±3)℃ and Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24 Scheduled Calibration Jan-24 Jan-24
pages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	ertificate. conducted in t (M&TE critical for 106277 104291 SN 3617 SN 1556 ID # MY49071430 MY46110673 Name	he closed laboratory facility: environment is or calibration) Cal Date (Calibrated by, Certificate No.) 22-Sep-22 (CTTL, No.J22X09561) 22-Sep-22 (CTTL, No.J22X09561) 31-Mar-23(CTTL-SPEAG,No.Z23-60161) 11-Jan-23(CTTL-SPEAG,No.Z23-60034) Cal Date (Calibrated by, Certificate No.) 05-Jan-23 (CTTL, No. J23X00107) 10-Jan-23 (CTTL, No. J23X00104) Function	temperature (22±3)℃ and Scheduled Calibration Sep-23 Sep-23 Mar-24 Jan-24 Scheduled Calibration Jan-24 Jan-24

Certificate No: 23J02Z80018

Page 1 of 6









Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

## Glossary:

TSL tissue simulating liquid ConvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured

## Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: 23J02Z80018

Page 2 of 6







Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.cn

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

## **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.9 ± 6 %	1.81 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.6 W/kg ± 18.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.13 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 18.7 % (k=2)

Certificate No: 23J02Z80018

Page 3 of 6



TL	In Colla	1.50	1	a	
-	CALIBR			RY	

Add: No.52 Hua ruanber Koad, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: ctt@chinattl.com http://www.caict.ac.cn

#### Appendix (Additional assessments outside the scope of CNAS L0570)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.2Ω+ 3.34jΩ	
Return Loss	- 28.2dB	

## **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.060 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: 23J02Z80018

Page 4 of 6






- Probe: EX3DV4 SN3617; ConvF(7.68, 7.68, 7.68) @ 2450 MHz; Calibrate 2023-03-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2023-01-11
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration**/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 100.7 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 27.6 W/kg SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.13 W/kg Smallest distance from peaks to all points 3 dB below = 8.5 mm Ratio of SAR at M2 to SAR at M1 = 48.5% Maximum value of SAR (measured) = 22.2 W/kg

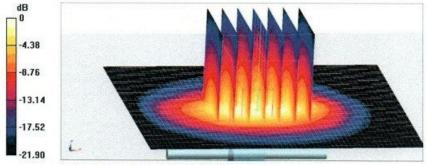

0 dB = 22.2 W/kg = 13.46 dBW/kg

Page 5 of 6








Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: cttl@chinattl.com http://www.caict.ac.en

Impedance Measurement Plot for Head TSL

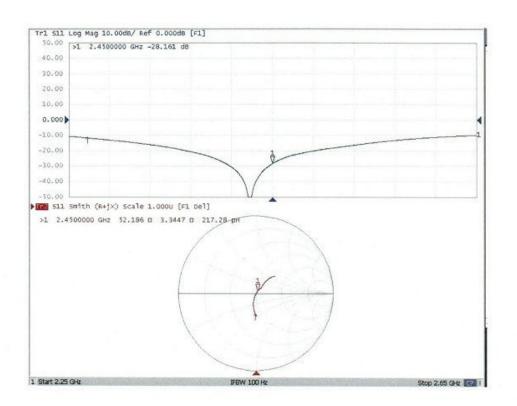

Certificate No: 23J02Z80018

Page 6 of 6



## ANNEX I: D2600V2 Dipole Calibration Certificate

E-mail: cmf@caict.ac.cn Client: TA(Shan CALIBRATION CI	MERCE INTERNATION	Certificate No	o: 24J02Z000225
CALIBRATION C	MERCE INTERNATION	and a second	
Object	D2600	/2 - SN: 1025	
Calibration Procedure(s)	FE-711	-003-01	
		tion Procedures for dipole validation kits	
Calibration date:	May 8,		
All calibrations have been humidity<70%.	conducted in t	he closed laboratory facility: environment te	emperature (22±3)°C and
Calibration Equipment used	(M&TE critical f	or calibration)	
			Scheduled Calibration
	(M&TE critical f	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183)	Scheduled Calibration May-24
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	
Primary Standards Power Meter NRP2	ID # 106276	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183)	May-24
Primary Standards Power Meter NRP2 Power sensor NRP6A	ID # 106276 101369	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183)	May-24 May-24
Primary Standards Power Meter NRP2 Power sensor NRP6A ReferenceProbe EX3DV4	ID # 106276 101369 SN 3846	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-May-23(SPEAG,No.EX-3846_May23)	May-24 May-24 May-24
Primary Standards Power Meter NRP2 Power sensor NRP6A ReferenceProbe EX3DV4 DAE4	ID # 106276 101369 SN 3846 SN 1556	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-May-23 (SPEAG,No.EX-3846_May23) 03-Jan-24 (CTTL-SPEAG,No.24J02Z80002)	May-24 May-24 May-24 Jan-25
Primary Standards Power Meter NRP2 Power sensor NRP6A ReferenceProbe EX3DV4 DAE4 Secondary Standards	ID # 106276 101369 SN 3846 SN 1556 ID #	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-May-23 (SPEAG,No.EX-3846_May23) 03-Jan-24 (CTTL-SPEAG,No.24J02Z80002) Cal Date (Calibrated by, Certificate No.)	May-24 May-24 May-24 Jan-25 Scheduled Calibration
Primary Standards Power Meter NRP2 Power sensor NRP6A ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	ID # 106276 101369 SN 3846 SN 1556 ID # MY49071430	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-May-23 (SPEAG,No.EX-3846_May23) 03-Jan-24 (CTTL-SPEAG,No.24J02Z80002) Cal Date (Calibrated by, Certificate No.) 25-Dec-23 (CTTL, No. J23X13426)	May-24 May-24 May-24 Jan-25 Scheduled Calibration Dec-24
Primary Standards Power Meter NRP2 Power sensor NRP6A ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	ID # 106276 101369 SN 3846 SN 1556 ID # MY49071430 MY46110673	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-May-23 (SPEAG,No.EX-3846_May23) 03-Jan-24 (CTTL-SPEAG,No.24J02Z80002) Cal Date (Calibrated by, Certificate No.) 25-Dec-23 (CTTL, No. J23X13426) 25-Dec-23 (CTTL, No. J23X13425)	May-24 May-24 May-24 Jan-25 Scheduled Calibration Dec-24 Dec-24 Jan-25 Signature
Primary Standards Power Meter NRP2 Power sensor NRP6A ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C OCP DAK-3.5(weighted)	ID # 106276 101369 SN 3846 SN 1556 ID # MY49071430 MY46110673 1040	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-May-23(SPEAG,No.EX-3846_May23) 03-Jan-24(CTTL-SPEAG,No.24J02Z80002) Cal Date (Calibrated by, Certificate No.) 25-Dec-23 (CTTL, No. J23X13426) 25-Dec-23 (CTTL, No. J23X13425) 22-Jan-24(SPEAG, No.OCP-DAK3.5-1040_Jan24)	May-24 May-24 Jan-25 Scheduled Calibration Dec-24 Dec-24 Jan-25
Primary Standards Power Meter NRP2 Power sensor NRP6A ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C OCP DAK-3.5(weighted) Calibrated by:	ID # 106276 101369 SN 3846 SN 1556 ID # MY49071430 MY46110673 1040 Name	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-May-23 (SPEAG,No.EX-3846_May23) 03-Jan-24 (CTTL-SPEAG,No.24J02Z80002) Cal Date (Calibrated by, Certificate No.) 25-Dec-23 (CTTL, No. J23X13426) 25-Dec-23 (CTTL, No. J23X13425) 22-Jan-24 (SPEAG, No.OCP-DAK3.5-1040_Jan24) Function	May-24 May-24 Jan-25 Scheduled Calibration Dec-24 Dec-24 Jan-25 Signature
Power sensor NRP6A ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	ID # 106276 101369 SN 3846 SN 1556 ID # MY49071430 MY46110673 1040 Name Zhao Jing	Cal Date (Calibrated by, Certificate No.) 15-May-23 (CTTL, No.J23X04183) 15-May-23 (CTTL, No.J23X04183) 31-May-23 (SPEAG,No.EX-3846_May23) 03-Jan-24 (CTTL-SPEAG,No.24J02Z80002) Cal Date (Calibrated by, Certificate No.) 25-Dec-23 (CTTL, No. J23X13426) 25-Dec-23 (CTTL, No. J23X13425) 22-Jan-24 (SPEAG, No.OCP-DAK3.5-1040_Jan24) Function SAR Test Engineer	May-24 May-24 May-24 Jan-25 Scheduled Calibration Dec-24 Dec-24 Jan-25 Signature

Certificate No: 24J02Z000225

Page 1 of 6





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn http://www.caict.ac.cn

## Glossary:

TSL	tissue simulating liquid	
ConvF	sensitivity in TSL / NORMx,y,z	
N/A	not applicable or not measured	

### Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

## Additional Documentation:

c) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Page 2 of 6







Add: No.52 HunYuanBei Rond, Haidian District, Beijing, 100191, China Tel: +86-10-62204633-2117 E-mail: cmf@caict.ac.cn http://www.caict.ac.cn

## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2600 MHz ± 1 MHz	

## **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.5 ± 6 %	1.99 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	—	_

## SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	14.0 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	55.5 W/kg ± 18.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.31 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	25.1 W/kg ± 18.7 % (k=2)

Certificate No: 24J02Z000225

Page 3 of 6







Add: No.52 Hua\uanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: em@csict.ac.en http://www.cnict.ac.en

## Appendix (Additional assessments outside the scope of CNAS L0570)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.0Ω- 6.02jΩ	
Return Loss	- 24.2dB	

#### **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.055 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.


The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

## **Additional EUT Data**

EAG
P

Page 4 of 6



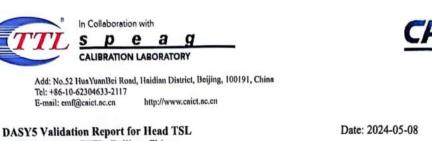


Test Laboratory: CTTL, Beijing, China **DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1025** Communication System: UID 0, CW; Frequency: 2600 MHz Medium parameters used: f = 2600 MHz;  $\sigma = 1.985$  S/m;  $\epsilon_r = 38.52$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:

- Probe: EX3DV4 SN3846; ConvF(6.72, 7.04, 7.5) @ 2600 MHz; Calibrated: 2023-05-31
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2024-01-03
- Phantom: MFP V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

**Dipole Calibration**/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.9 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 28.9 W/kg SAR(1 g) = 14 W/kg; SAR(10 g) = 6.31 W/kg Smallest distance from peaks to all points 3 dB below = 8.5 mm Ratio of SAR at M2 to SAR at M1 = 49.3% Maximum value of SAR (measured) = 23.6 W/kg

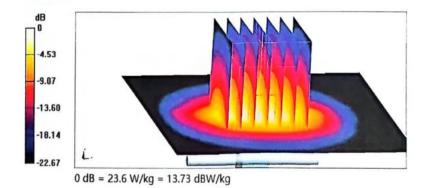


Certificate No: 24J02Z000225

Page 5 of 6





## Impedance Measurement Plot for Head TSL

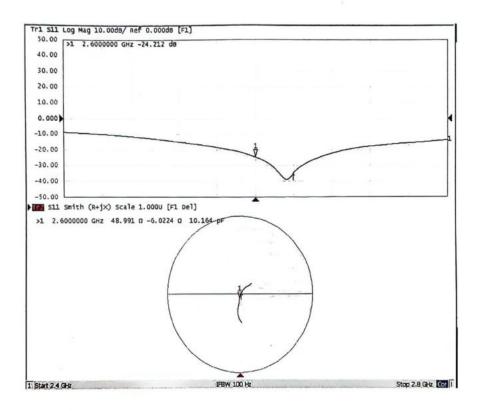

#### Certificate No: 24J02Z000225

Page 6 of 6



Report No.: R2407A0983-S1V1

# ANNEX J: DAE4 Calibration Certificate (SN: 1692)

Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn	http://www.caict.ac		
Oliciti .	Shanghai)		No: 23J02Z80174
CALIBRATION	CERTIFICA	ATE	
Object	DAE	4 - SN: 1692	
Calibration Procedure(s)	EE-7	11_002_01	
	Calib	FF-Z11-002-01 Calibration Procedure for the Data Acquisition Electronics (DAEx)	
Calibration date:	Dece	ember 08, 2023	
pages and are part of the All calibrations have be humidity<70%.	e certificate. een conducted i	nd the uncertainties with confidence prob- n the closed laboratory facility: enviror al for calibration)	
pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us	e certificate. een conducted in sed (M&TE critica	n the closed laboratory facility: enviror	
pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us Primary Standards	e certificate. een conducted in sed (M&TE critica	n the closed laboratory facility: environ	nment temperature(22±3)°C ar
pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us Primary Standards	e certificate. een conducted in sed (M&TE critica ID # (	n the closed laboratory facility: enviror al for calibration) Cal Date(Calibrated by, Certificate No.)	nment temperature(22±3)°C an Scheduled Calibration
pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us Primary Standards Process Calibrator 753	e certificate. een conducted in sed (M&TE critica ID # ( 1971018	n the closed laboratory facility: environ al for calibration) Cal Date(Calibrated by, Certificate No.) 12-Jun-23 (CTTL, No.J23X05436) Function	nment temperature(22±3)°C an Scheduled Calibration Jun-24
pages and are part of the	e certificate. een conducted in sed (M&TE critica ID # ( 1971018 Name	n the closed laboratory facility: environ al for calibration) Cal Date(Calibrated by, Certificate No.) 12-Jun-23 (CTTL, No.J23X05436) Function	nment temperature(22±3)°C an Scheduled Calibration Jun-24

Certificate No: 23J02Z80174

Page 1 of 3



Report No.: R2407A0983-S1V1





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn http://www.caict.ac.cn

## Glossary: DAE

SAR Test Report

Connector angle

data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters:


- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

Certificate No: 23J02Z80174

Page 2 of 3









Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2117 E-mail: emf@caict.ac.cn http://www.caict.ac.cn

## **DC Voltage Measurement**

A/D - Converter Resolution nominal High Range: 1LSB = 6 6.1µV , -100...+300 mV full range = full range = Low Range: 1LSB = 61nV , -1.....+3mV DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Y	z
High Range	404.485 ± 0.15% (k=2)	404.556 ± 0.15% (k=2)	404.407 ± 0.15% (k=2)
Low Range	3.95218 ± 0.7% (k=2)	4.00338 ± 0.7% (k=2)	3.97970 ± 0.7% (k=2)

## **Connector Angle**

Connector Angle to be used in DASY system	336° ± 1 °
Connector Angle to be used in DASY system	336° ± 1 °

Certificate No: 23J02Z80174

Page 3 of 3



## **ANNEX K: The EUT Appearance**

The EUT Appearance are submitted separately.



## **ANNEX L: Test Setup Photos**

The Test Setup Photos are submitted separately.

\*\*\*\*\*\*END OF REPORT \*\*\*\*\*\*