


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

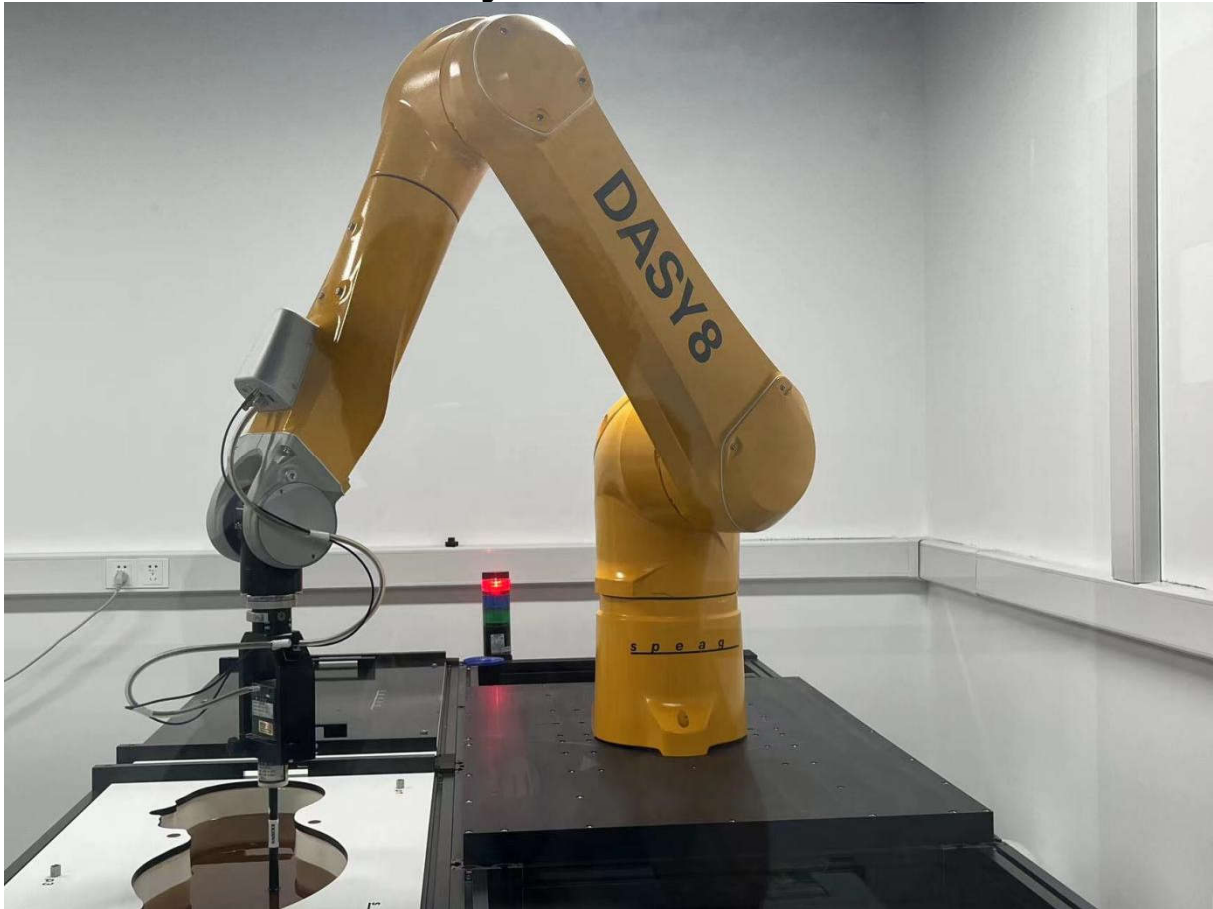

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
	NA

3. Photographs of EUT test position

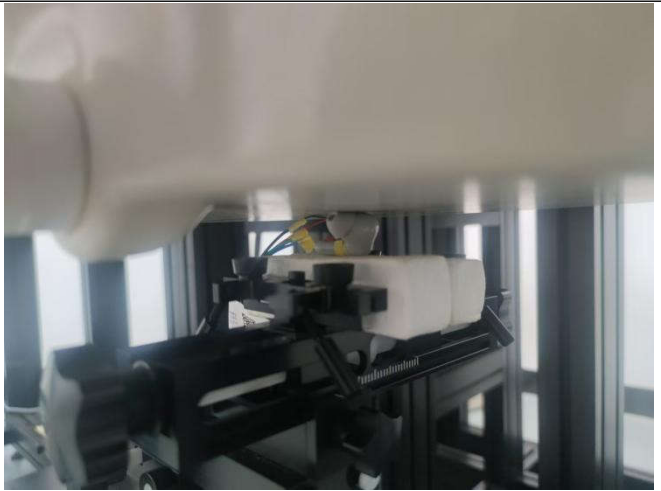
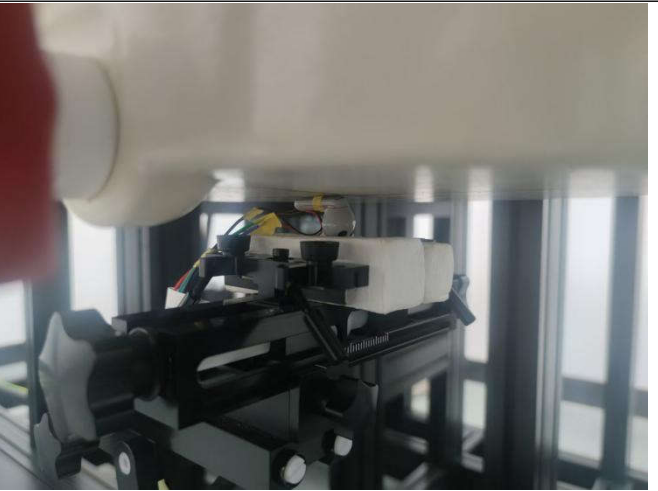
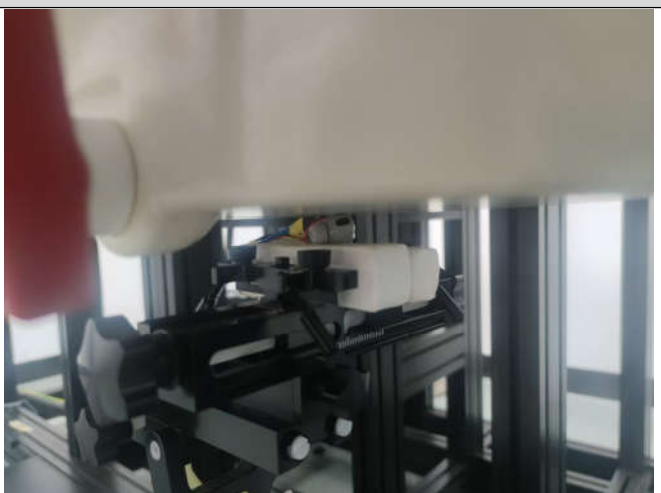
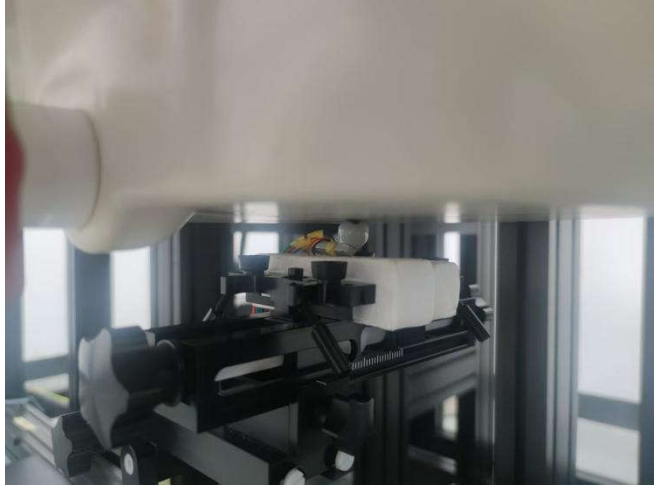
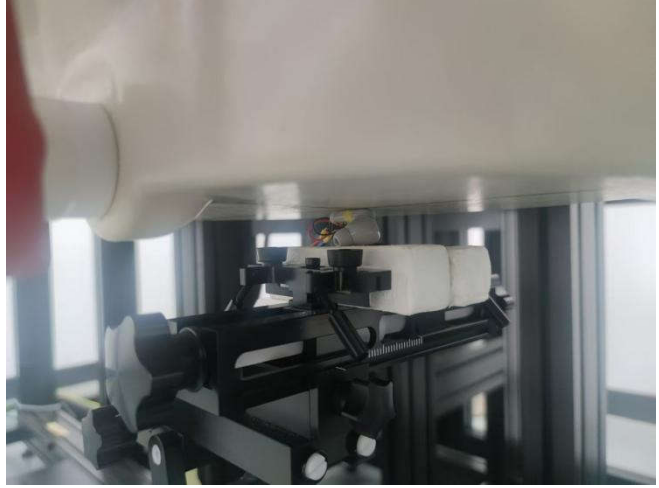
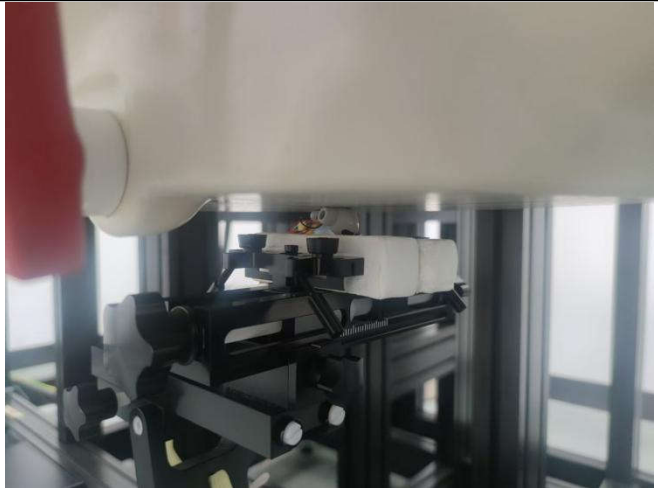
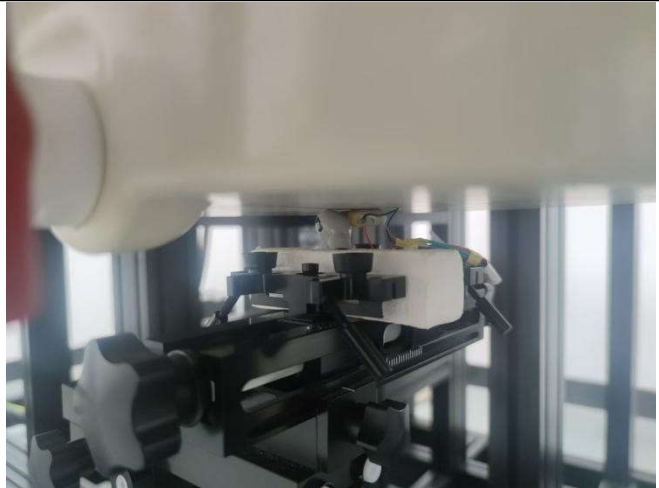
Photo 2: Left ear Front side 0mm	Photo 3: Left ear Back side 0mm
	
Photo 4: Left ear Left side 0mm	Photo 5: Left ear Right side 0mm
	
Photo 6: Left ear Top side 0mm	Photo 7: Left ear Bottom side 0mm
	

Photo 8: Right ear Front side 0mm	Photo 9: Right ear Back side 0mm
	
Photo 10: Right ear Left side 0mm	Photo 11: Right ear Right side 0mm
	
Photo 12: Right ear Top side 0mm	Photo 13: Right ear Bottom side 0mm
	

4. EUT Constructional Details

Photo 14: Left ear Front View

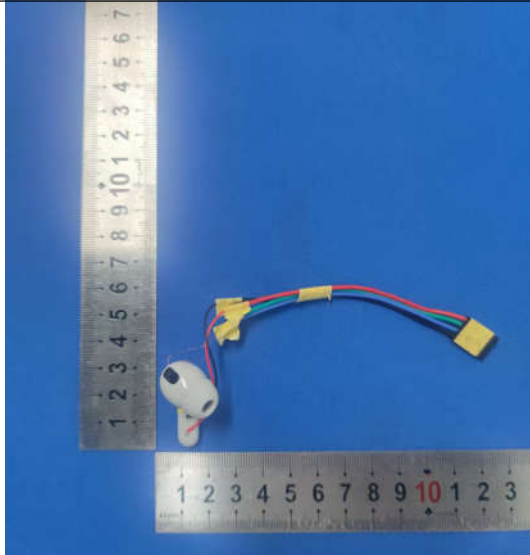


Photo 15: Left ear Back View

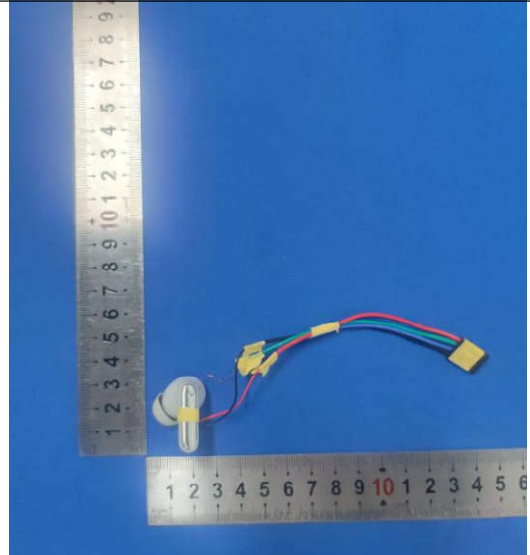


Photo 16: Right ear Front View

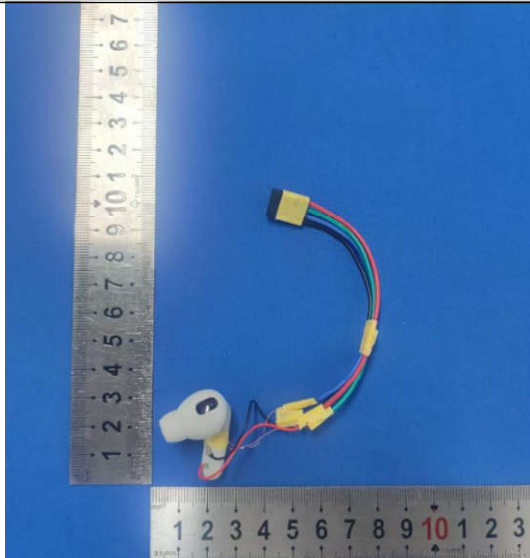


Photo 17: Right ear Back View

