

System Performance Check Report for D750V3 - SN1122

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	750.0	TSL Permittivity	40.9
Group / UID	CW / 0--	TSL Conductivity [S/m]	0.890
Conversion Factor	8.37	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7645 2024-09-23	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2024-07-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.786	0.788
psSAR10g [W/Kg]	0.525	0.545
Power Drift [dB]		0.01
Dist 3dB Peak [mm]		16.8
M2/M1 [%]		88.6

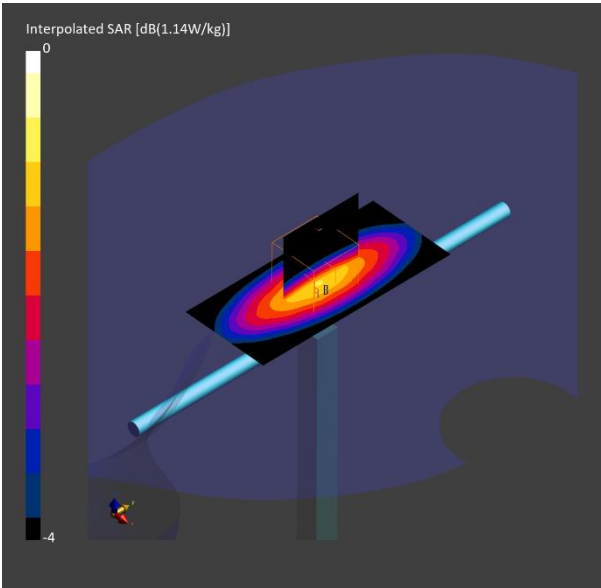

System Performance Check Report for D835V2 - SN4d174

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	835.0	TSL Permittivity	40.6
Group / UID	CW / 0--	TSL Conductivity [S/m]	0.911
Conversion Factor	8.25	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7645 2024-09-23	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2024-07-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.893	0.897
psSAR10g [W/Kg]	0.591	0.615
Power Drift [dB]		-0.01
Dist 3dB Peak [mm]		18.1
M2/M1 [%]		88.7

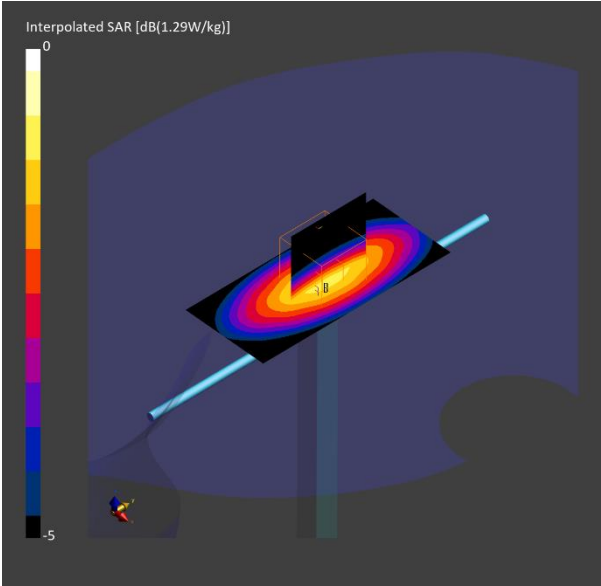

System Performance Check Report for D1750V2 - SN1125

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1750.0	TSL Permittivity	40.1
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.33
Conversion Factor	7.56	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7645 2024-09-23	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2024-07-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.38	3.40
psSAR10g [W/Kg]	1.83	1.92
Power Drift [dB]		0.00
Dist 3dB Peak [mm]		10.8
M2/M1 [%]		84.9

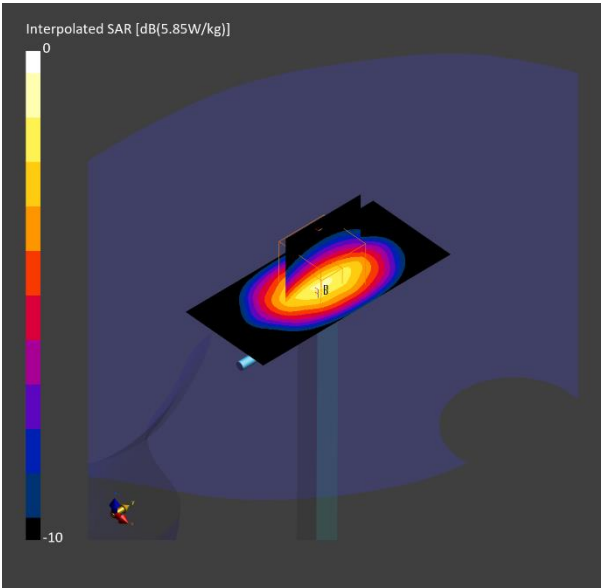

System Performance Check Report for D1900V2 - SN5d199

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1900.0	TSL Permittivity	39.1
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.38
Conversion Factor	7.47	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7645 2024-09-23	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2024-07-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.78	3.78
psSAR10g [W/Kg]	1.99	2.09
Power Drift [dB]		-0.04
Dist 3dB Peak [mm]		10.8
M2/M1 [%]		86.4

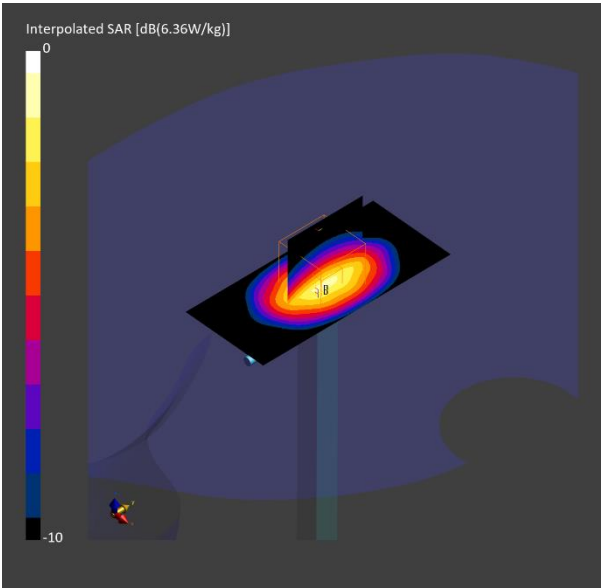

System Performance Check Report for D2600V2 - SN1097

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2600.0	TSL Permittivity	40.3
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.91
Conversion Factor	6.84	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7645 2024-09-23	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2024-07-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	5.33	5.25
psSAR10g [W/Kg]	2.43	2.53
Power Drift [dB]		-0.10
Dist 3dB Peak [mm]		9.0
M2/M1 [%]		83.3

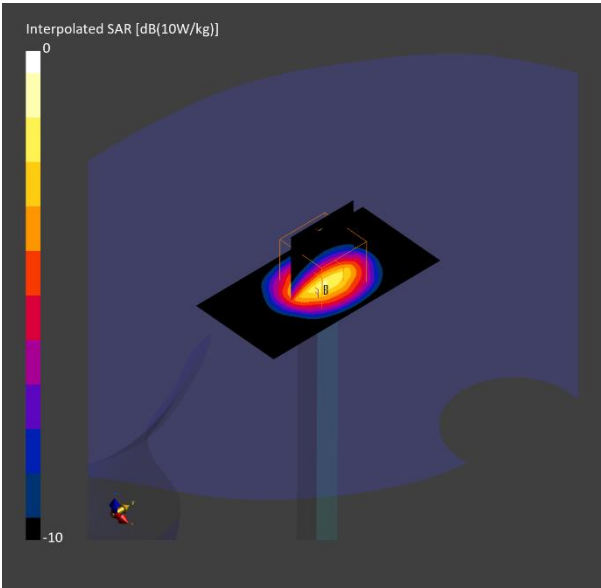

System Performance Check Report for D5GHzV2 - SN1184

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	5250.0	TSL Permittivity	36.2
Group / UID	CW / 0--	TSL Conductivity [S/m]	4.60
Conversion Factor	5.3	Phantom Section / TSL	Flat / HSL

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7645 2024-09-23	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2024-07-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	7.11	7.67
psSAR10g [W/Kg]	2.06	2.26
Power Drift [dB]		0.03
Dist 3dB Peak [mm]		7.4
M2/M1 [%]		65.1

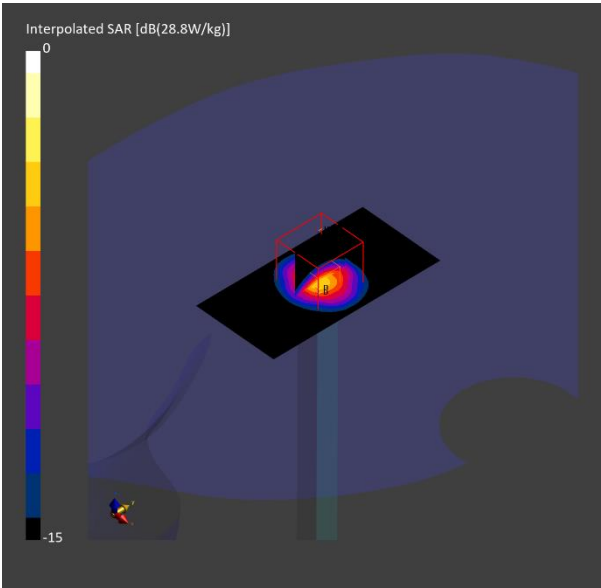

System Performance Check Report for D2450V2 - SN939

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2450.0	TSL Permittivity	39.1
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.73
Conversion Factor	6.91	Phantom Section / TSL	Flat / HSL

DASY Configuration

Probe Calibration Date	EX3DV4 - SN7645 2024-09-23	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1494 2024-07-15	TSL Type	HBBL-600-10000
Software Version	16.2.2.1588		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	4.89	4.82
psSAR10g [W/Kg]	2.27	2.35
Power Drift [dB]		-0.04
Dist 3dB Peak [mm]		9.0
M2/M1 [%]		82.3

