



In Collaboration with

CALIBRATION LABORATORY

E-mail: cttl@chinattl.com

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 http://www.chinattl.cn

### DASY5 Validation Report for Head TSL

Date: 05.19.2021

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 952

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz;  $\sigma = 1.788$  S/m;  $\epsilon_r = 39.43$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Center Section

DASY5 Configuration:

- Probe: EX3DV4 SN3846; ConvF(7.45, 7.45, 7.45) @ 2450 MHz; Calibrated: 2021-04-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 2021-01-08
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14

**Dipole Calibration**/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 107.4 V/m; Power Drift = -0.04 dB


Peak SAR (extrapolated) = 28.2 W/kg

SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 46.4%

Maximum value of SAR (measured) = 22.5 W/kg

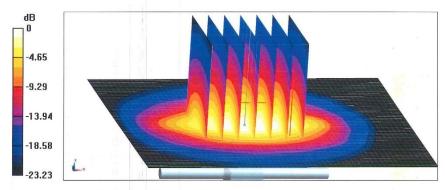

0 dB = 22.5 W/kg = 13.52 dBW/kg


Certificate No: Z21-60171

Page 5 of 8





### Impedance Measurement Plot for Head TSL

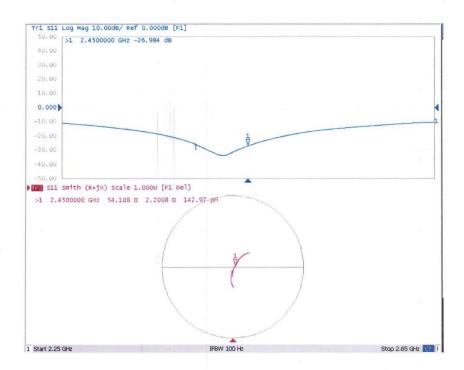

Page 6 of 8





DASY5 Validation Report for Body TSL

Date: 05.19.2021

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 952

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f=2450 MHz;  $\sigma=1.96$  S/m;  $\epsilon_r=52.15$ ;  $\rho=1000$  kg/m<sup>3</sup>

Phantom section: Right Section

DASY5 Configuration:

- Probe: EX3DV4 SN3846; ConvF(7.37, 7.37, 7.37) @ 2450 MHz; Calibrated: 2021-04-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 2021-01-08
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

**Dipole Calibration**/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.3 V/m; Power Drift = 0.04 dB


Peak SAR (extrapolated) = 26.9 W/kg

SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.06 W/kg

Smallest distance from peaks to all points 3 dB below = 8.5 mm

Ratio of SAR at M2 to SAR at M1 = 49.7%

Maximum value of SAR (measured) = 22.1 W/kg

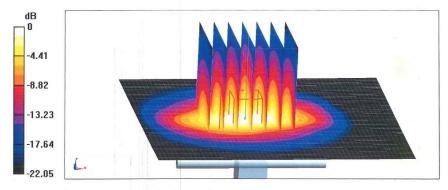


0 dB = 22.1 W/kg = 13.44 dBW/kg

Page 7 of 8





### Impedance Measurement Plot for Body TSL

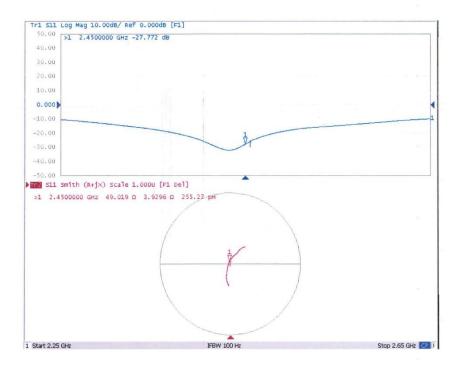





# D2450V2 Dipole impedance and return loss Validation

Meas. Results	Current Meas.	Previous Meas.	Max. Deviation
Meas. Data	2022.05.18	2021.05.19	/
Return Loss(dB)	-26.401	-26.984	-2.16%
lman a dan a a	F4 103 O +3 930 iO	54.108 Ω +2.201	0.629Ω
Impedance	54.102 Ω +2.830 jΩ	jΩ	(Imaginary part)

## Return Loss for Head TSL

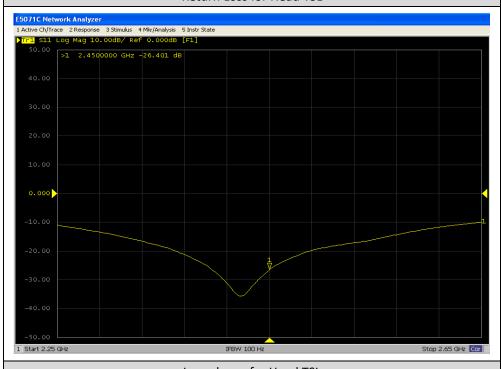

# Impedance for Head TSL

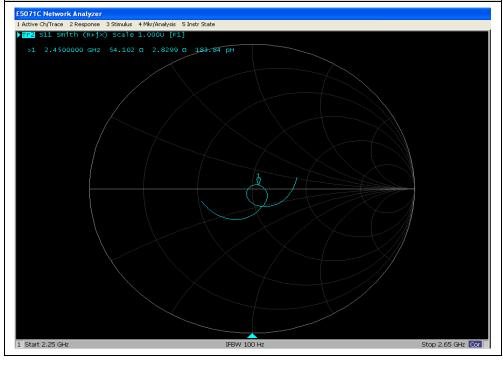



## F.4 5GHz Dipole



Client

baluntek

Certificate No:

Z21-60173

## **CALIBRATION CERTIFICATE**

Object

D5GHzV2 - SN: 1200

Calibration Procedure(s)

FF-Z11-003-01

Calibration Procedures for dipole validation kits

Calibration date:

May 18, 2021

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22\pm3)^{\circ}$ C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date(Calibrated by, Certificate No.)  Scheduled Calibrate  Scheduled Calibrate  Scheduled Calibrate  Scheduled Calibrate  Scheduled Calibrate		
Power Meter NRP2	106277	23-Sep-20 (CTTL, No.J20X08336)	Sep-21	
Power sensor NRP8S	104291	23-Sep-20 (CTTL, No.J20X08336)	Sep-21	
ReferenceProbe EX3DV4	SN 3846	26-Apr-21(CTTL-SPEAG,No.Z21-60084)	Apr-22	
DAE4	SN 777	08-Jan-21(CTTL-SPEAG,No.Z21-60003)	Jan-22	
Secondary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration	
Signal Generator E4438C	MY49071430	25-Feb-20 (CTTL, No.J20X00516)	Feb-21	
NetworkAnalyzerE5071C	MY46110673	10-Feb-20 (CTTL, No.J20X00515)	Feb-21	
	Name	Function	Signature	
Calibrated by:	Zhao Jing	SAR Test Engineer	多色	
Reviewed by:	Lin Hao	SAR Test Engineer	林光	
Approved by:	Qi Dianyuan	SAR Project Leader	26	
		Issued: May		
This calibration certificate s	hall not be repro	duced except in full without written approval	of the laboratory.	

Certificate No: Z21-60173

Page 1 of 14





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com http://www.chinattl.cn

Glossary:

TSL ConvF N/A tissue simulating liquid sensitivity in TSL / NORMx,y,z not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

### **Additional Documentation:**

e) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center
  marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z21-60173

Page 2 of 14





### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5250 MHz ± 1 MHz 5600 MHz ± 1 MHz 5750 MHz ± 1 MHz	т.

## Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.71 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.5 ± 6 %	4.67 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL at 5250 MHz

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.80 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	77.8 W/kg ± 24.4 % (k=2)
SAR averaged over 10 $\ cm^3$ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.22 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)

Certificate No: Z21-60173

Page 3 of 14





## Head TSL parameters at 5600 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.9 ± 6 %	5.05 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL at 5600 MHz

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.15 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	81.2 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.32 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.1 W/kg ± 24.2 % (k=2)

## Head TSL parameters at 5750 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.4	5.22 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.21 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL at 5750 MHz

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	7
SAR measured	100 mW input power	7.75 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	77.2 W/kg ± 24.4 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.18 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.7 W/kg ± 24.2 % (k=2)

Certificate No: Z21-60173

Page 4 of 14





Body TSL parameters at 5250 MHz
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.36 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.1 ± 6 %	5.34 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL at 5250 MHz

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.33 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	73.4 W/kg ± 24.4 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.05 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.5 W/kg ± 24.2 % (k=2)

Body TSL parameters at 5600 MHz
The following parameters and calculations were applied.

Ji	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.4 ± 6 %	5.82 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL at 5600 MHz

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.72 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	77.2 W/kg ± 24.4 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.16 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.6 W/kg ± 24.2 % (k=2)

Certificate No: Z21-60173

Page 5 of 14





# Body TSL parameters at 5750 MHz

he following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.3	5.94 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.1 ± 6 %	6.05 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	//	·

SAR result with Body TSL at 5750 MHz

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.34 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	73.4 W/kg ± 24.4 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.03 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.3 W/kg ± 24.2 % (k=2)

Certificate No: Z21-60173

Page 6 of 14





## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL at 5250 MHz

Impedance, transformed to feed point	$45.1\Omega + 1.25j\Omega$	
Return Loss	- 25.5dB	

### Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	49.7Ω + 7.81jΩ		
Return Loss	- 22.1dB		

## Antenna Parameters with Head TSL at 5750 MHz

Impedance, transformed to feed point	45.9Ω + 4.85jΩ	
Return Loss	- 23.5dB	

### Antenna Parameters with Body TSL at 5250 MHz

Impedance, transformed to feed point	$43.9\Omega + 2.08j\Omega$	
Return Loss	- 23.3dB	

## Antenna Parameters with Body TSL at 5600 MHz

Impedance, transformed to feed point	50.3Ω + 8.89jΩ	
Return Loss	- 21.1dB	

## Antenna Parameters with Body TSL at 5750 MHz

Impedance, transformed to feed point	46.6Ω + 5.63jΩ	
Return Loss	- 23.3dB	

Certificate No: Z21-60173

Page 7 of 14





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel; +86-10-62304633-2512 Fax: +86-10-62304633-2504 http://www.chinattl.cn

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.096 ns	7

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### **Additional EUT Data**

Manufactured by	SPEAG	
manaratar a a y	5	

Certificate No: Z21-60173

Page 8 of 14



Date: 05.18.2021



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 http://www.chinattl.cn

#### **DASY5 Validation Report for Head TSL**

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1200

Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz,

Medium parameters used: f = 5250 MHz;  $\sigma$  = 4.668 S/m;  $\epsilon_r$  = 35.48;  $\rho$  = 1000 kg/m³, Medium parameters used: f = 5600 MHz;  $\sigma$  = 5.045 S/m;  $\epsilon_r$  = 34.88;  $\rho$  = 1000 kg/m³, Medium parameters used: f = 5750 MHz;  $\sigma$  = 5.208 S/m;  $\epsilon_r$  = 34.67;  $\rho$  = 1000 kg/m³,

Phantom section: Center Section

#### DASY5 Configuration:

- Probe: EX3DV4 SN3846; ConvF(5.43, 5.43, 5.43) @ 5250 MHz; ConvF(4.69, 4.69, 4.69) @ 5600 MHz; ConvF(4.9, 4.9, 4.9) @ 5750 MHz; Calibrated: 2021-04-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 2021-01-08
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 69.22 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 32.9 W/kg

SAR(1 g) = 7.8 W/kg; SAR(10 g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.3%

Maximum value of SAR (measured) = 18.9 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 70.18 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 35.5 W/kg

SAR(1 g) = 8.15 W/kg; SAR(10 g) = 2.32 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.9%

Maximum value of SAR (measured) = 19.8 W/kg

Certificate No: Z21-60173

Page 9 of 14






Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 68.06 V/m; Power Drift = -0.09 dB Peak SAR (extrapolated) = 34.6 W/kg

SAR(1 g) = 7.75 W/kg; SAR(10 g) = 2.18 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm Ratio of SAR at M2 to SAR at M1 = 62.1%

Maximum value of SAR (measured) = 19.0 W/kg

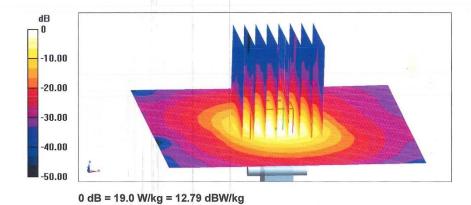


Certificate No: Z21-60173

Page 10 of 14





### Impedance Measurement Plot for Head TSL

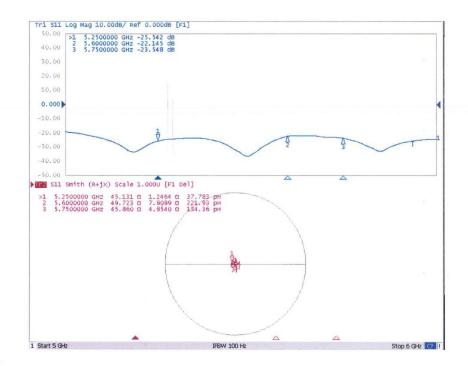

Page 11 of 14





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 http://www.chinattl.cn

**DASY5 Validation Report for Body TSL** 

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1200

Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz,

Date: 05.18.2021

Medium parameters used: f = 5250 MHz;  $\sigma$  = 5.34 S/m;  $\epsilon_r$  = 49.12;  $\rho$  = 1000 kg/m³, Medium parameters used: f = 5600 MHz;  $\sigma$  = 5.815 S/m;  $\epsilon_r$  = 48.44;  $\rho$  = 1000 kg/m³, Medium parameters used: f = 5750 MHz;  $\sigma$  = 6.045 S/m;  $\epsilon_r$  = 48.11;  $\rho$  = 1000 kg/m³,

Phantom section: Right Section

#### DASY5 Configuration:

- Probe: EX3DV4 SN3846; ConvF(4.95, 4.95, 4.95) @ 5250 MHz; ConvF(4.32, 4.32, 4.32) @ 5600 MHz; ConvF(4.38, 4.38, 4.38) @ 5750 MHz; Calibrated: 2021-04-26.
- · Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 2021-01-08
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.86 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 29.6 W/kg

SAR(1 g) = 7.33 W/kg; SAR(10 g) = 2.05 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.3%

Maximum value of SAR (measured) = 17.2 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 66.06 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 33.1 W/kg

SAR(1 g) = 7.72 W/kg; SAR(10 g) = 2.16 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.1%

Maximum value of SAR (measured) = 18.8 W/kg


Certificate No: Z21-60173

Page 12 of 14





Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 64.58 V/m; Power Drift = -0.04 dB
Peak SAR (extrapolated) = 32.8 W/kg
SAR(1 g) = 7.34 W/kg; SAR(10 g) = 2.03 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 62%
Maximum value of SAR (measured) = 18.1 W/kg

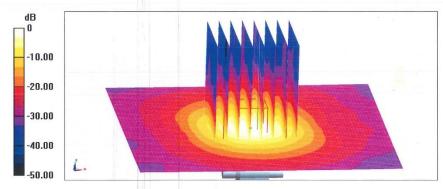


0 dB = 18.1 W/kg = 12.58 dBW/kg

Page 13 of 14





## Impedance Measurement Plot for Body TSL

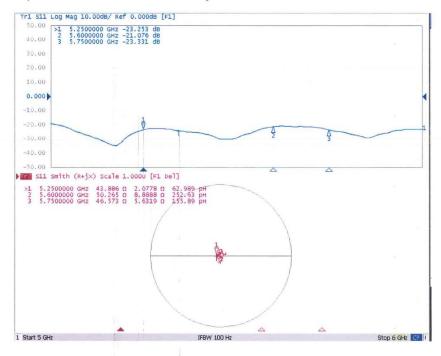


Page 14 of 14




D5GHzV2 Dipole impedance and return loss Validation

Meas. Results	Current Meas.	Previous Meas.	Max. Deviation
Meas. Data	2022.05.17	2021.05.18	/
5.25GHz	-29.961	-25.542	17.30%
Return Loss(dB)	-29.961	-23.542	17.30%
5.25GHz	49 025 0 11 902 (0	45.131 Ω +1.246	3.794Ω
Impedance	48.925 Ω +1.802 jΩ	jΩ	(Real part)
5.6GHz	-25.244	-22.145	13.99%
Return Loss(dB)	-23.244	-22.145	15.99%
5.6GHz	47 1620 +2 417 10	49.723 Ω +7.809	-4.392Ω
Impedance	47.163Ω +3.417 jΩ	jΩ	(Imaginary part)
5.75GHz	-27.284	-23.548	15.87%
Return Loss(dB)	-27.204	-23.546	15.67 //
5.75GHz	50.693Ω +8.724 jΩ	45.860 Ω +4.854	4.833Ω
Impedance	30.09312 +0.724 ][2	jΩ	(Real part)

# Return Loss for Head TSL

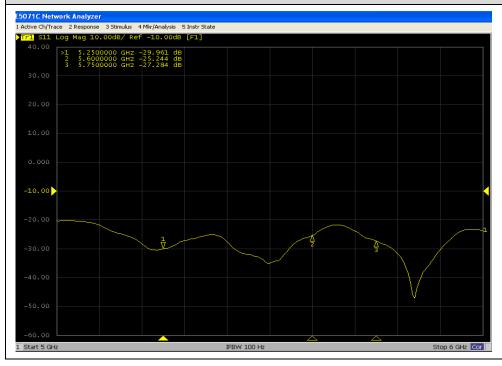



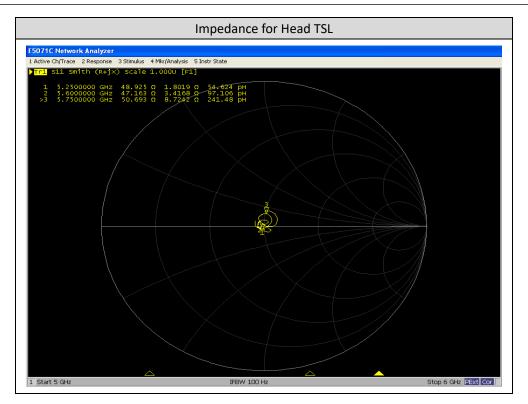



# F.5 6.5GHz Dipole

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

ALIBRATION CE	ERTIFICATE		
Dbject	D6.5GHzV2 - SN	:1037	
Calibration procedure(s)	QA CAL-22.v6 Calibration Proce	dure for SAR Validation Sources	between 3-10 GHz
Calibration date:	July 01, 2021		
The measurements and the uncerta	ainties with confidence po	onal standards, which realize the physical unit robability are given on the following pages and y facility: environment temperature (22 $\pm$ 3)°C	d are part of the certificate.
Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
	The second secon		
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22
	SN: 104778 SN: 103244	09-Apr-21 (No. 217-03291/03292) 09-Apr-21 (No. 217-03291)	Apr-22 Apr-22
Power sensor NRP-Z91			
Power sensor NRP-Z91 Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22
Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T	SN: 103244 SN: 103245	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292)	Apr-22 Apr-22
Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T Reference 20 dB Attenuator	SN: 103244 SN: 103245 SN: 100967	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292) 08-Apr-21 (No. 217-03293)	Apr-22 Apr-22 Apr-22
Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T Reference 20 dB Attenuator Type-N mismatch combination	SN: 103244 SN: 103245 SN: 100967 SN: BH9394 (20k)	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292) 08-Apr-21 (No. 217-03293) 09-Apr-21 (No. 217-03343)	Apr-22 Apr-22 Apr-22 Apr-22
Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4	SN: 103244 SN: 103245 SN: 100967 SN: BH9394 (20k) SN: 310982 / 06327	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292) 08-Apr-21 (No. 217-03293) 09-Apr-21 (No. 217-03343) 09-Apr-21 (No. 217-03344)	Apr-22 Apr-22 Apr-22 Apr-22 Apr-22
Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4	SN: 103244 SN: 103245 SN: 100967 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7405	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292) 08-Apr-21 (No. 217-03293) 09-Apr-21 (No. 217-03343) 09-Apr-21 (No. 217-03344) 30-Dec-20 (No. EX3-7405_Dec20)	Apr-22 Apr-22 Apr-22 Apr-22 Apr-22 Dec-21
Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards	SN: 103244 SN: 103245 SN: 100967 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7405 SN: 908	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292) 08-Apr-21 (No. 217-03293) 09-Apr-21 (No. 217-03343) 09-Apr-21 (No. 217-03344) 30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21)	Apr-22 Apr-22 Apr-22 Apr-22 Apr-22 Dec-21 Jun-22
Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator Anapico APSIN20G	SN: 103244 SN: 103245 SN: 100967 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7405 SN: 908	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292) 08-Apr-21 (No. 217-03293) 09-Apr-21 (No. 217-03343) 09-Apr-21 (No. 217-03344) 30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21) Check Date (in house)	Apr-22 Apr-22 Apr-22 Apr-22 Apr-22 Dec-21 Jun-22 Scheduled Check
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator Anapico APSIN20G Network Analyzer R&S ZVL13	SN: 103244 SN: 103245 SN: 100967 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7405 SN: 908	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292) 08-Apr-21 (No. 217-03293) 09-Apr-21 (No. 217-03343) 09-Apr-21 (No. 217-03344) 30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21) Check Date (in house) 28-Mar-17 (in house check Dec-18)	Apr-22 Apr-22 Apr-22 Apr-22 Apr-22 Dec-21 Jun-22 Scheduled Check In house check: Dec-21
Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator Anapico APSIN20G	SN: 103244 SN: 103245 SN: 100967 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7405 SN: 908 ID # SN: 669 SN: 101093	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292) 08-Apr-21 (No. 217-03293) 09-Apr-21 (No. 217-03293) 09-Apr-21 (No. 217-03344) 30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21) Check Date (in house) 28-Mar-17 (in house check Dec-18) 10-May-12 (in house check Dec-18)	Apr-22 Apr-22 Apr-22 Apr-22 Apr-22 Dec-21 Jun-22 Scheduled Check In house check: Dec-21 In house check: Dec-21
Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor R&S NRP33T Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator Anapico APSIN20G Network Analyzer R&S ZVL13	SN: 103244 SN: 103245 SN: 100967 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7405 SN: 908 ID # SN: 669 SN: 101093	09-Apr-21 (No. 217-03291) 09-Apr-21 (No. 217-03292) 08-Apr-21 (No. 217-03293) 09-Apr-21 (No. 217-03343) 09-Apr-21 (No. 217-03344) 30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21) Check Date (in house) 28-Mar-17 (in house check Dec-18) 10-May-12 (in house check Dec-18)	Apr-22 Apr-22 Apr-22 Apr-22 Apr-22 Dec-21 Jun-22 Scheduled Check In house check: Dec-21 In house check: Dec-21

Certificate No: D6.5GHzV2-1037\_Jul21

Page 1 of 6



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL ConvF N/A tissue simulating liquid sensitivity in TSL / NORM x,y,z

not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.

## **Additional Documentation:**

b) DASY System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point
  exactly below the center marking of the flat phantom section, with the arms oriented parallel to the
  body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned
  under the liquid filled phantom. The impedance stated is transformed from the measurement at the
  SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty
  required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.
- The absorbed power density (APD): The absorbed power density is evaluated according to Samaras T, Christ A, Kuster N, "Compliance assessment of the epithelial or absorbed power density above 6 GHz using SAR measurement systems", Bioelectromagnetics, 2021 (submitted). The additional evaluation uncertainty of 0.55 dB (rectangular distribution) is considered.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D6.5GHzV2-1037\_Jul21

Page 2 of 6



### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY6	V16.0	
Extrapolation	Advanced Extrapolation		
Phantom	Modular Flat Phantom		
Distance Dipole Center - TSL	5 mm	with Spacer	
Zoom Scan Resolution	dx, dy = 3.4  mm, dz = 1.4  mm	Graded Ratio = 1.4 (Z direction)	
Frequency	6500 MHz ± 1 MHz		

Head TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	34.5	6.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	33.6 ± 6 %	6.12 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	28.8 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	286 W/kg ± 24.7 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	5.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.6 W/kg ± 24.4 % (k=2)

Certificate No: D6.5GHzV2-1037\_Jul21

Page 3 of 6



## **Appendix**

## Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.5 Ω - 2.4 jΩ
Return Loss	- 30.9 dB

## APD (Absorbed Power Density)

APD averaged over 1 cm <sup>2</sup>	Condition	
APD measured	100 mW input power	286 W/m <sup>2</sup>
APD measured	normalized to 1W	2860 W/m <sup>2</sup> ± 29.2 % (k=2)

APD averaged over 4 cm <sup>2</sup>	condition		
APD measured	100 mW input power	128 W/m <sup>2</sup>	
APD measured	normalized to 1W	1280 W/m <sup>2</sup> ± 28.9 % (k=2)	

## General Antenna Parameters and Design

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### **Additional EUT Data**

Manufactured by SPEAG
-----------------------

Certificate No: D6.5GHzV2-1037\_Jul21

Page 4 of 6



# **DASY6 Validation Report for Head TSL**

Measurement Report for D6.5GHz-1037, UID 0 -, Channel 6500 (6500.0MHz)

Device	under	Test	Pro	perties
--------	-------	------	-----	---------

Name, Manufacturer D6.5GHz

Dimensions [mm] 16.0 x 6.0 x 300.0 IMEI SN: 1037 **DUT Type** 

**Exposure Conditions** 

Phantom Section, TSL

Position, Test Band Distance [mm] Band

Group, UID CW,

Frequency [MHz] 6500

Conversion Factor 5.75

TSL Cond. [S/m]

6.12

Permittivity

33.6

Flat, HSL Hardware Setup

5.00

HBBL600-10000V6

Probe, Calibration Date EX3DV4 - SN7405, 2020-12-30 DAE, Calibration Date DAE4 Sn908, 2021-06-24

Scan Setup

Phantom

Grid Extents [mm] Grid Steps [mm] Sensor Surface [mm] Graded Grid **Grading Ratio** MAIA Surface Detection Scan Method

MFP V8.0 Center - 1182


Zoom Scan 22.0 x 22.0 x 22.0 3.4 x 3.4 x 1.4 1.4

Yes 1.4 N/A VMS + 6p Measured Measurement Results Date psSAR1g [W/Kg] psSAR10g [W/Kg] Power Drift [dB] Power Scaling Scaling Factor [dB] TSL Correction M2/M1 [%]

Dist 3dB Peak [mm]

Zoom Scan 2021-07-10, 10:54 28.8 5.30 0.00 Disabled

No correction 50.2 4.8




Certificate No: D6.5GHzV2-1037\_Jul21

Page 5 of 6



# Impedance Measurement Plot for Head TSL

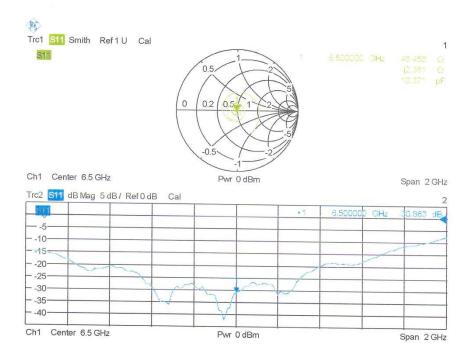


Certificate No: D6.5GHzV2-1037\_Jul21

Page 6 of 6



D6.5GHzV2 Dipole impedance and return loss Validation

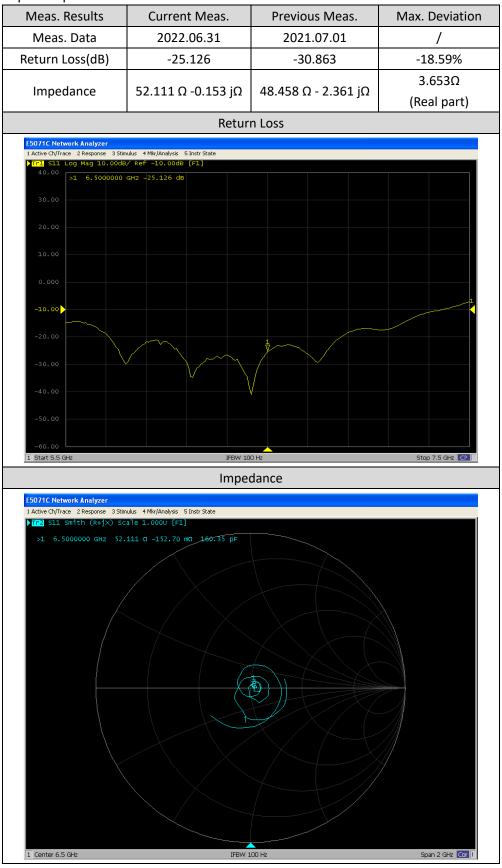

--END OF REPORT--