

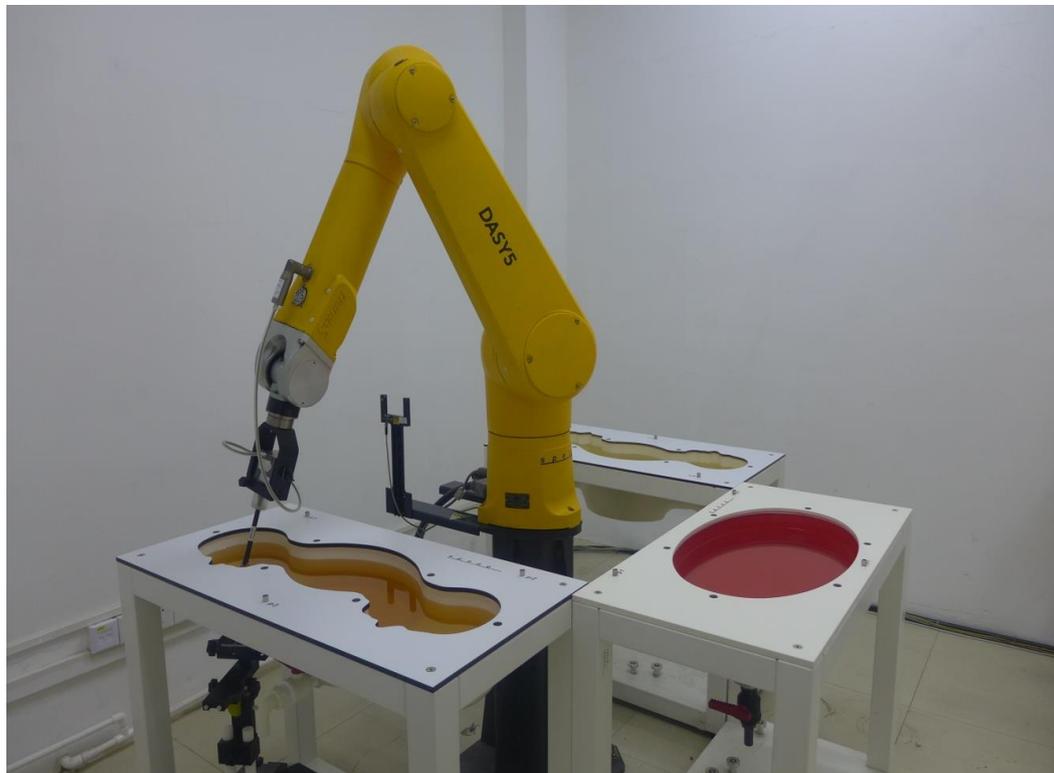


# **Appendix D**

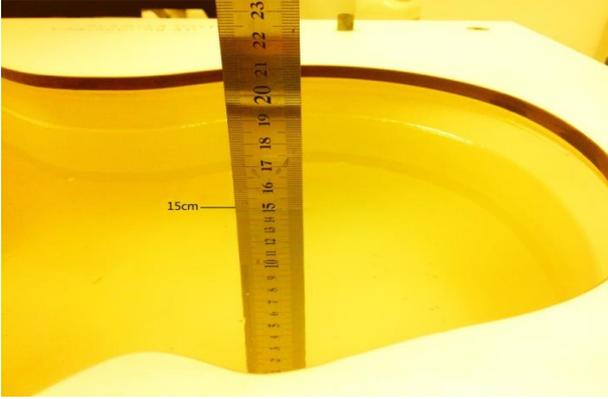
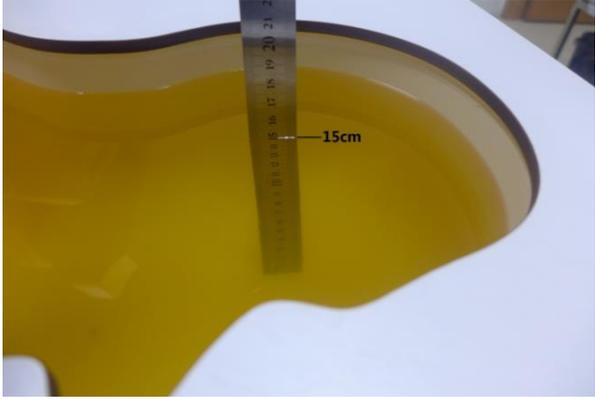
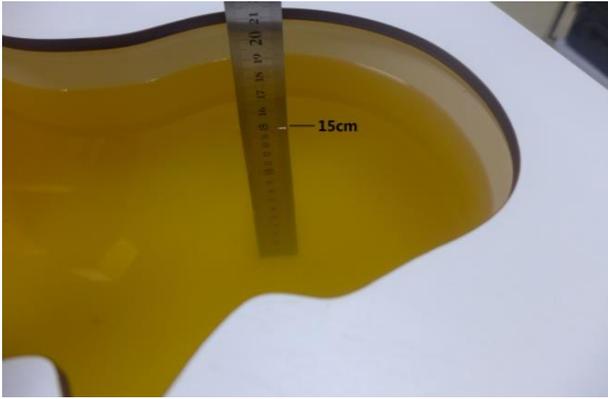
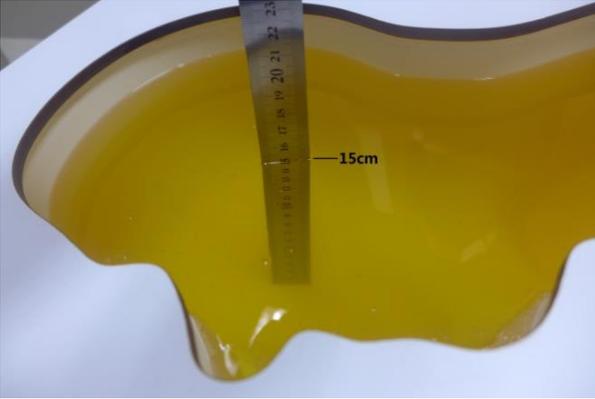
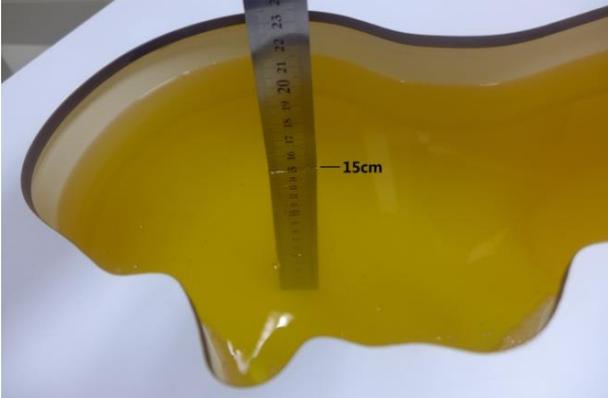
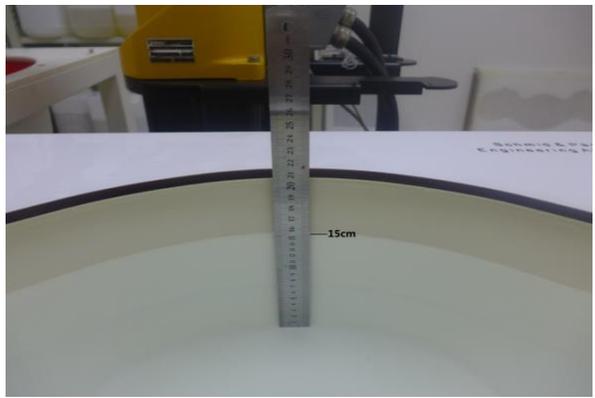
## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

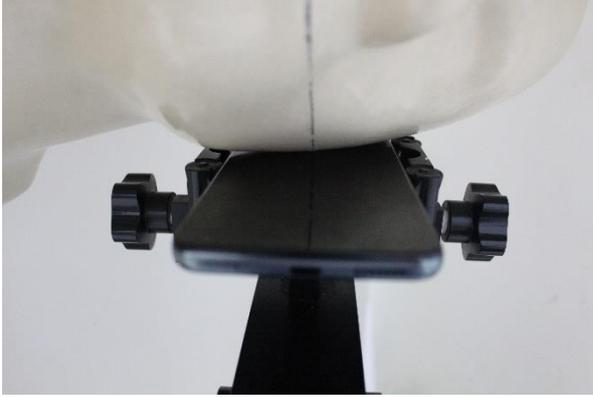
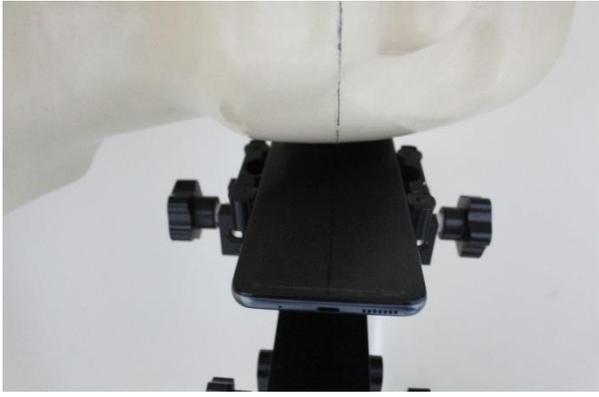
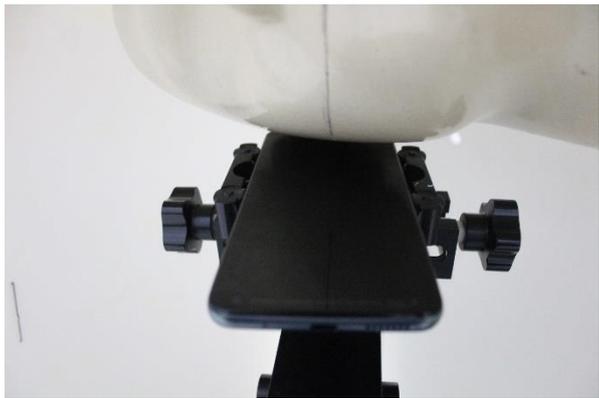
## 1. SAR measurement System



## 2. Photographs of Tissue Simulate Liquid

<p><b>Photo 1: Tissue Simulant Liquid for Head 835</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Head 1750</b></p>
	
<p><b>Photo 3: issue Simulant Liquid for Head 1900</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Head 2450</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Head 2600</b></p>	<p><b>Photo 6: Tissue Simulant Liquid for Head 5G</b></p>
	

### 3. Photographs of EUT test position

<p>Photo 7: Left cheek</p>	<p>Photo 8: Left tilted</p>
	
<p>Photo 9: Right cheek</p>	<p>Photo 10: Right tilted</p>
	
<p>Photo 11: Front side 5mm</p>	<p>Photo 12: Back side 5mm</p>
	

<p><b>Photo 13: Left side 5mm</b></p>	<p><b>Photo 14: Right side 5mm</b></p>
	
<p><b>Photo 15: Top side 5mm</b></p>	<p><b>Photo 16: Bottom side 5mm</b></p>
	
<p><b>Photo 17: Front side 0mm</b></p>	<p><b>Photo 18: Back side 0mm</b></p>
	

Photo 19: Left side 0mm	Photo 20: Right side 0mm
	
Photo 21: Top side 0mm	Photo 22: Bottom side 0mm
	
Photo 23: Front side 4mm	Photo 24: Front side 10mm
	

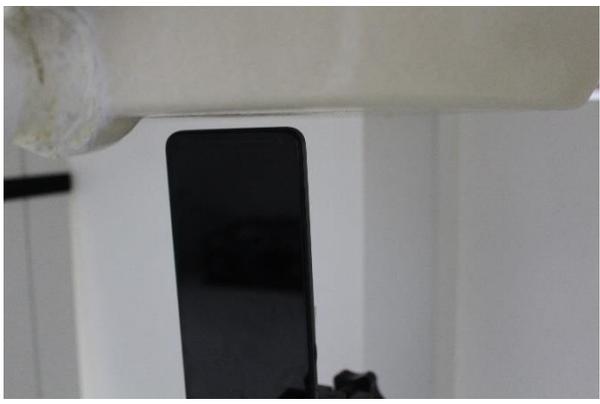
<p><b>Photo 25: Back side 6mm</b></p>	<p><b>Photo 26: Back side 17mm</b></p>
	
<p><b>Photo 27: Left side 4mm</b></p>	<p><b>Photo 28: Left side 7mm</b></p>
	
<p><b>Photo 29: Right side 11mm</b></p>	<p><b>Photo 30: Bottom side 7mm</b></p>
	

Photo 31: Bottom side 13mm	Photo 32: Back side with headset 5mm
	

#### 4. EUT Constructional Details

Photo 33: Front View	Photo 34: Back View
	