

Date/Time: 10/19/04 23:54:38

Test Laboratory: A Test Lab Techno Corp.

04-0517-S_Philips 568_Flat_PCS CH512_20041020_Earphone_**DUT: Philips 568; Type: GSM Three Band Mobile Phone; Serial: 354054000000488**

Communication System: GSM 1900; Frequency: 1850.2 MHz; Duty Cycle: 1:8.3

Medium: Body 1900MHz Medium parameters used (interpolated): $f = 1850.2$ MHz; $s = 1.5$ mho/m; $\epsilon_r = 53.1$;Conductivity= kg/m^3 ; Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530; ConvF(4.43, 4.43, 4.43); Calibrated: 9/1/2004
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

Flat/Area Scan (51x101x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (interpolated) = 0.272 mW/g

Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 28.1 V/m; Power Drift = -0.0 dB

Peak SAR (extrapolated) = 0.354 W/kg

SAR(1 g) = 0.236 mW/g; SAR(10 g) = 0.146 mW/g

Maximum value of SAR (measured) = 0.254 mW/g


Flat/Zoom Scan (5x5x7)/Cube 1: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 28.1 V/m; Power Drift = -0.0 dB

Peak SAR (extrapolated) = 0.327 W/kg

SAR(1 g) = 0.227 mW/g; SAR(10 g) = 0.148 mW/g

Maximum value of SAR (measured) = 0.245 mW/g

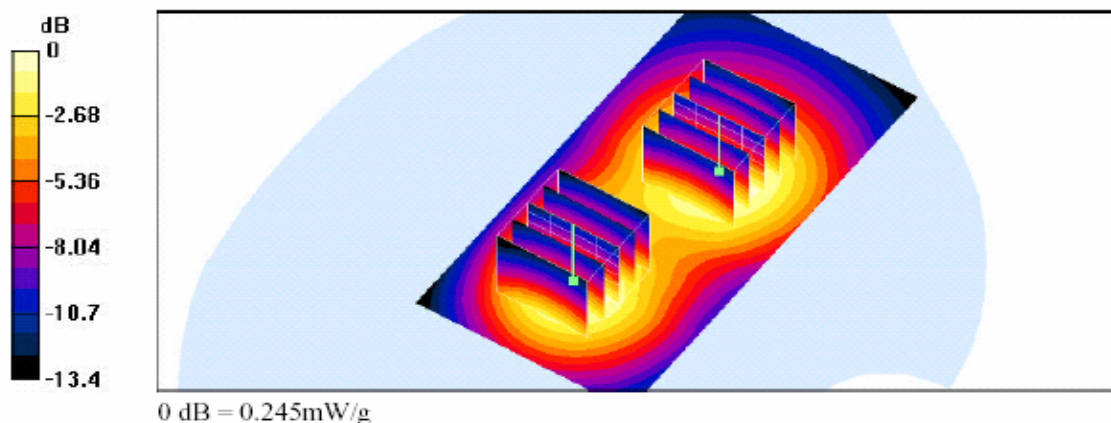**Body-SAR Test Result for Flat Position – Channel 512**

Date/Time: 10/20/04 00:17:51

Test Laboratory: A Test Lab Techno Corp.

04-0517-S_Philips 568_Flat_PCS CH661_20041020_Earphone_**DUT: Philips 568; Type: GSM Three Band Mobile Phone; Serial: 354054000000488**

Communication System: GSM 1900; Frequency: 1880 MHz; Duty Cycle: 1:8.3

Medium: Body 1900MHz Medium parameters used: $f = 1880$ MHz; $s = 1.52$ mho/m; $\epsilon_r = 53$;Conductivity=1000kg/m³; Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530; ConvF(4.43, 4.43, 4.43); Calibrated: 9/1/2004
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn393; Calibrated: 1/8/2004
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

Flat/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.252 mW/g

Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 26.8 V/m; Power Drift = 0.0 dB

Peak SAR (extrapolated) = 0.342 W/kg

SAR(1 g) = 0.220 mW/g; SAR(10 g) = 0.136 mW/g

Maximum value of SAR (measured) = 0.237 mW/g


Flat/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 26.8 V/m; Power Drift = 0.0 dB

Peak SAR (extrapolated) = 0.317 W/kg

SAR(1 g) = 0.215 mW/g; SAR(10 g) = 0.139 mW/g

Maximum value of SAR (measured) = 0.233 mW/g

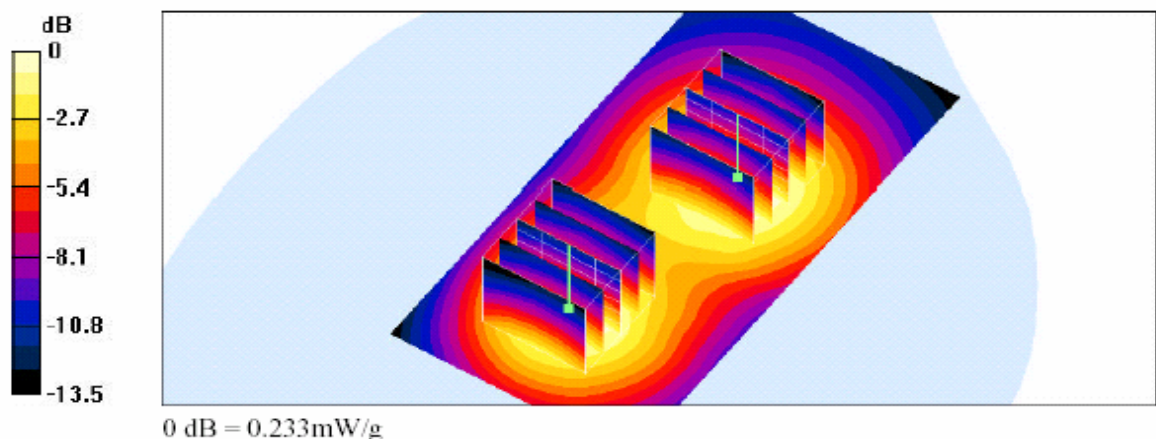**Body-SAR Test Result for Flat Position – Channel 661**

Date/Time: 10/20/04 00:41:16

Test Laboratory: A Test Lab Techno Corp.

04-0517-S_Philips 568_Flat_PCS CH810_20041020_Earphone_

DUT: Philips 568; Type: GSM Three Band Mobile Phone; Serial: 354054000000488

Communication System: GSM 1900; Frequency: 1909.8 MHz; Duty Cycle: 1:8.3

Medium: Body 1900MHz Medium parameters used (interpolated): $f = 1909.8 \text{ MHz}$; $s = 1.56 \text{ mho/m}$; $\epsilon_r = 53.1$;

Conductivity= 1000 kg/m^3 ; Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530; ConvF(4.43, 4.43, 4.43); Calibrated: 9/1/2004

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

Flat/Area Scan (51x101x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (interpolated) = 0.217 mW/g

Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 24 V/m ; Power Drift = -0.0 dB

Peak SAR (extrapolated) = 0.299 W/kg

SAR(1 g) = 0.201 mW/g ; SAR(10 g) = 0.129 mW/g

Maximum value of SAR (measured) = 0.215 mW/g


Flat/Zoom Scan (5x5x7)/Cube 1: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 24 V/m ; Power Drift = -0.0 dB

Peak SAR (extrapolated) = 0.288 W/kg

SAR(1 g) = 0.183 mW/g ; SAR(10 g) = 0.112 mW/g

Maximum value of SAR (measured) = 0.197 mW/g

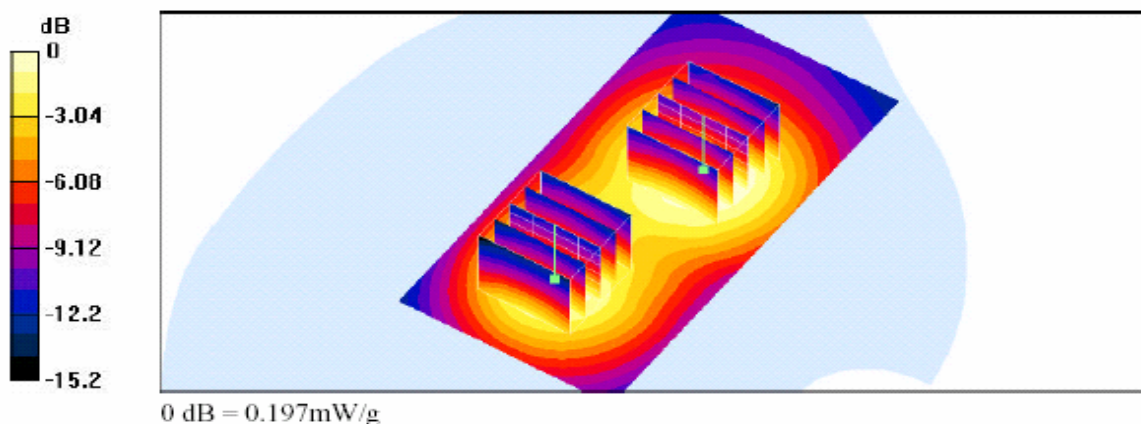

Body-SAR Test Result for Flat Position – Channel 810

Date/Time: 10/20/04 01:07:00

Test Laboratory: A Test Lab Techno Corp.

04-0517-S_Philips 568_Flat_PCS CH512_20041020_Earphone_GPRS_

DUT: Philips 568; Type: GSM Three Band Mobile Phone; Serial: 354054000000488

Communication System: PCS 1900 GPRS(2Down,2Up); Frequency: 1850.2 MHz;Duty Cycle: 1:4.2

Medium: Body 1900MHz Medium parameters used (interpolated): $f = 1850.2$ MHz; $s = 1.5$ mho/m; $\epsilon_r = 53.1$;

Conductivity= 1000kg/m^3 ;Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530; ConvF(4.43, 4.43, 4.43); Calibrated: 9/1/2004

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

Flat/Area Scan (51x101x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Maximum value of SAR (interpolated) = 0.644 mW/g

Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 43.1 V/m ; Power Drift = -0.1 dB

Peak SAR (extrapolated) = 0.907 W/kg

SAR(1 g) = 0.569 mW/g ; SAR(10 g) = 0.340 mW/g

Maximum value of SAR (measured) = 0.618 mW/g


Flat/Zoom Scan (5x5x7)/Cube 1: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 43.1 V/m ; Power Drift = -0.1 dB

Peak SAR (extrapolated) = 0.665 W/kg

SAR(1 g) = 0.455 mW/g ; SAR(10 g) = 0.294 mW/g

Maximum value of SAR (measured) = 0.489 mW/g

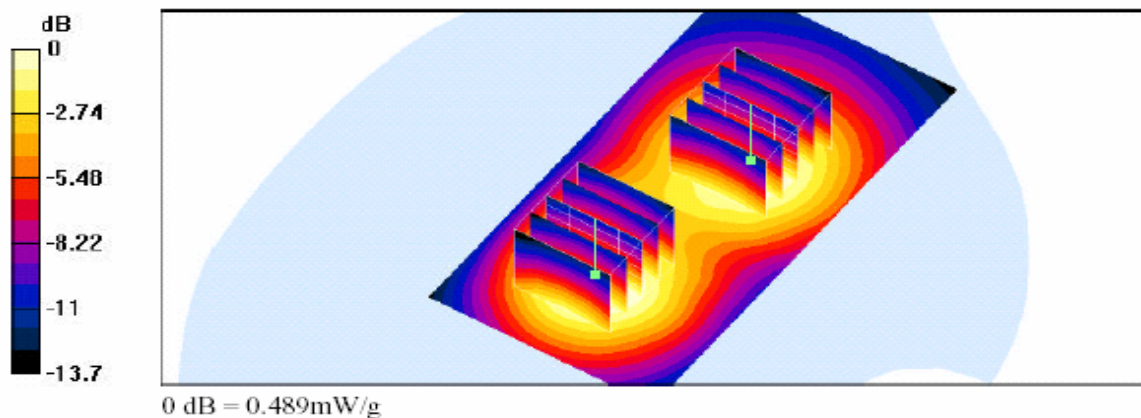

Body-GPRS SAR Test Result for Flat Position – Channel 512

Date/Time: 10/20/04 01:36:29

Test Laboratory: A Test Lab Techno Corp.

04-0517-S_Philips 568_Flat_PCS CH661_20041020_Earphone_GPRS_

DUT: Philips 568; Type: GSM Three Band Mobile Phone; Serial: 354054000000488

Communication System: PCS 1900 GPRS(2Down,2Up); Frequency: 1880 MHz;Duty Cycle: 1:4.2

Medium: Body 1900MHz Medium parameters used: $f = 1880$ MHz; $s = 1.52$ mho/m; $\epsilon_r = 53$;

Conductivity=1000kg/m3;Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1530; ConvF(4.43, 4.43, 4.43); Calibrated: 9/1/2004

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)

- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009

- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

Flat/Area Scan (51x101x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 0.578 mW/g

Flat/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 41 V/m; Power Drift = -0.1 dB

Peak SAR (extrapolated) = 0.802 W/kg

SAR(1 g) = 0.509 mW/g; SAR(10 g) = 0.309 mW/g

Maximum value of SAR (measured) = 0.550 mW/g


Flat/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 41 V/m; Power Drift = -0.1 dB

Peak SAR (extrapolated) = 0.611 W/kg

SAR(1 g) = 0.426 mW/g; SAR(10 g) = 0.278 mW/g

Maximum value of SAR (measured) = 0.443 mW/g

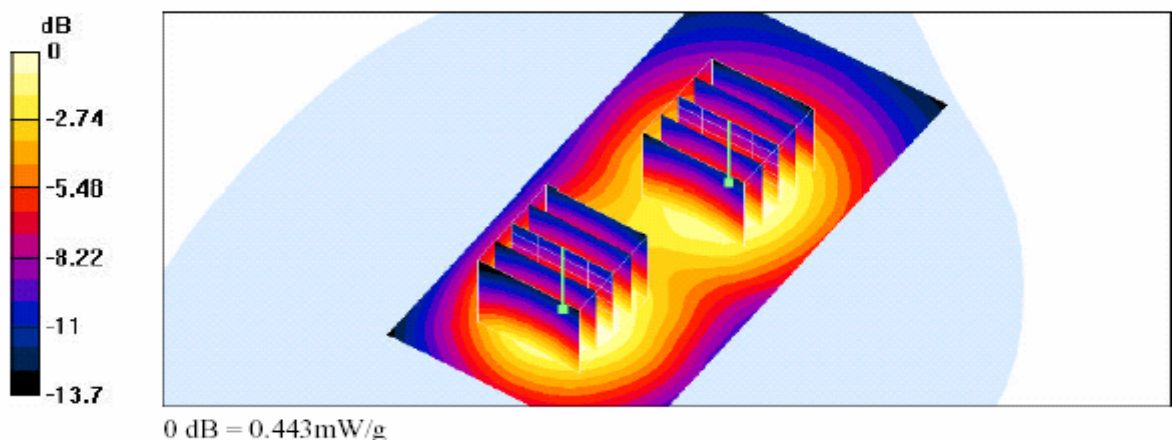

Body-GPRS SAR Test Result for Flat Position – Channel 661

Date/Time: 10/20/04 01:58:21

Test Laboratory: A Test Lab Techno Corp.

04-0517-S_Philips 568_Flat_PCS CH810_20041020_Earphone_GPRS_**DUT: Philips 568; Type: GSM Three Band Mobile Phone; Serial: 354054000000488**

Communication System: PCS 1900 GPRS(2Down,2Up); Frequency: 1909.8 MHz;Duty Cycle: 1:4.2

Medium: Body 1900MHz Medium parameters used (interpolated): $f = 1909.8 \text{ MHz}$; $s = 1.56 \text{ mho/m}$; $\epsilon_r = 53.1$;Conductivity= 1000 kg/m^3 ;Phantom section: Flat Section

DASY4 Configuration:


- Probe: ET3DV6 - SN1530; ConvF(4.43, 4.43, 4.43); Calibrated: 9/1/2004

- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)


- Electronics: DAE3 Sn393; Calibrated: 1/8/2004

- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009


- Measurement SW: DASY4, V4.3 Build 22; Postprocessing SW: SEMCAD, V1.8 Build 127

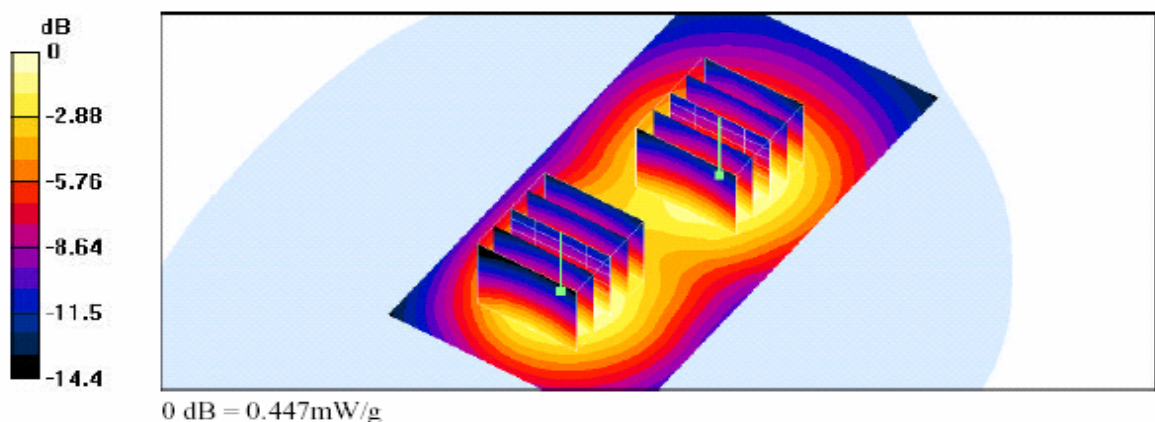Flat/Area Scan (51x101x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$ Maximum value of SAR (interpolated) = 0.507 mW/g **Flat/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$ Reference Value = 37.3 V/m ; Power Drift = -0.0 dB Peak SAR (extrapolated) = 0.726 W/kg **SAR(1 g) = 0.444 mW/g ; SAR(10 g) = 0.268 mW/g** Maximum value of SAR (measured) = 0.480 mW/g **Flat/Zoom Scan (5x5x7)/Cube 1:** Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$ Reference Value = 37.3 V/m ; Power Drift = -0.0 dB Peak SAR (extrapolated) = 0.631 W/kg **SAR(1 g) = 0.420 mW/g ; SAR(10 g) = 0.266 mW/g** Maximum value of SAR (measured) = 0.447 mW/g **Body-GPRS SAR Test Result for Flat Position – Channel 810**

Z-axis Plot for Maximum SAR

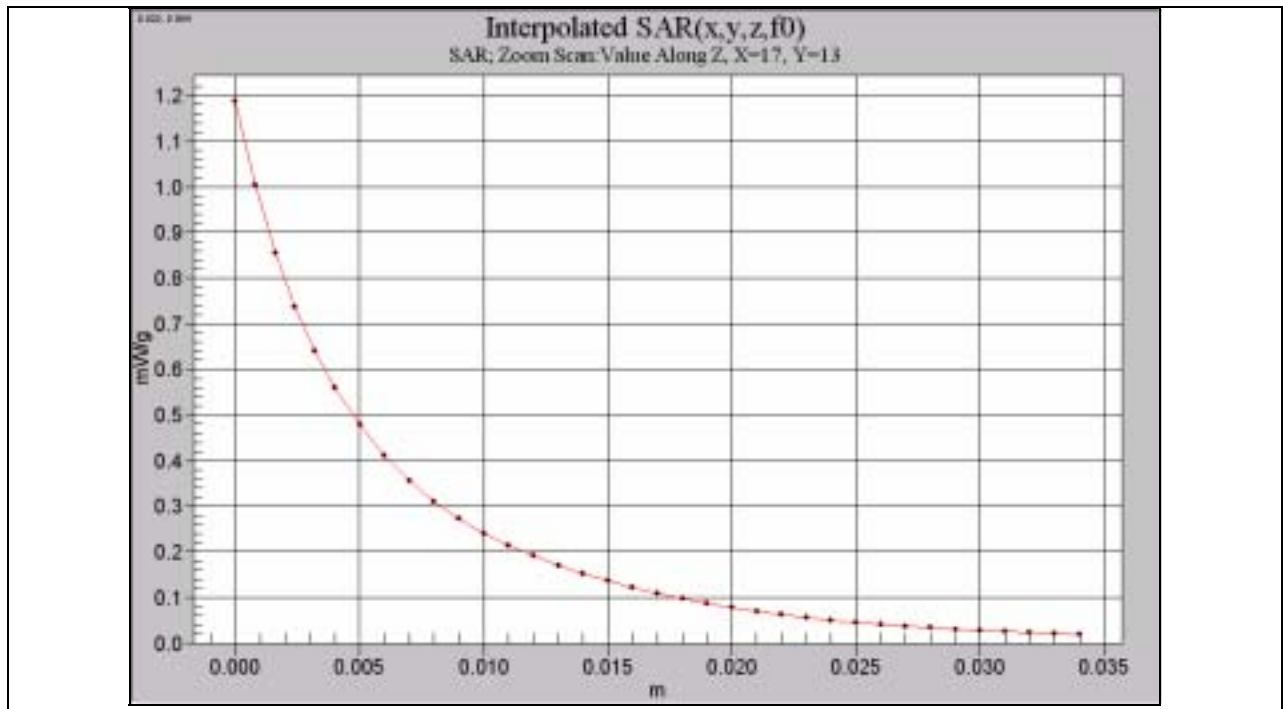

Head-SAR Test Result for Right Cheek Position – Channel 661

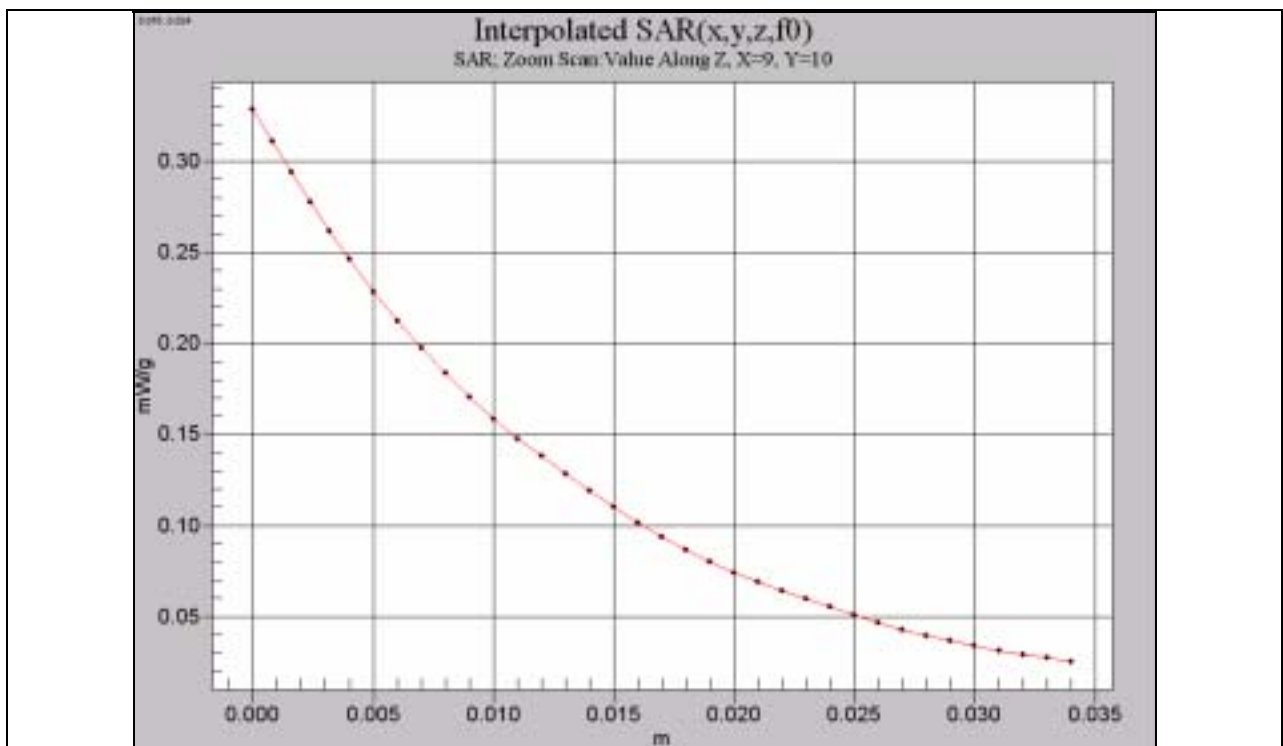

Body-SAR Test Result for Flat Position – Channel 512



Body-GPRS SAR Test Result for Flat Position – Channel 512

Appendix C – Dipole Calibration

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8204 Zurich, Switzerland			
Client		Auden	
CALIBRATION CERTIFICATE			
Object(s)	D900V2 - SN:172		
Calibration procedure(s)	QA CAL-05.v2 Calibration procedure for dipole validation kits		
Calibration date:	January 13, 2004		
Condition of the calibrated item	In Tolerance (according to the specific calibration document)		
This calibration statement documents traceability of M&E used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.			
All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.			
Calibration Equipment used (M&E critical for calibration)			
Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM E442	GB37480704	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Power sensor HP 8401A	UG37292783	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Power sensor HP 8401A	MY41082317	18-Oct-02 (Agilent, No. 20021018)	Oct-04
RF generator R&S SML-03	100656	27-Mar-2002 (R&S, No. 20-82369)	In house check: Mar-05
Network Analyzer HP 8753E	US37190585	18-Oct-01 (SPEAG, in house check Nov-03)	In house check: Oct-05
Calibrated by:	Name Judith Mueller	Function Technician	Signature 
Approved by:	Name Katja Polkevic	Function Laboratory Director	Signature 
Date issued: January 19, 2004			
This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.			



880-KP0301061-A
Page 1 (T)

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland

Phone +41 1 245 9700, Fax +41 1 245 9779

info@speag.com, <http://www.speag.com>

DASY

Dipole Validation Kit

Type: D900V2

Serial: 172

Manufactured: September 23, 2002

Calibrated: January 13, 2004

1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **head simulating solution** of the following electrical parameters at 900 MHz:

Relative Dielectricity	40.3	$\pm 5\%$
Conductivity	0.94 mho/m	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.6 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was $250\text{mW} \pm 3\%$. The results are normalized to 1W input power.

2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm^3 (1 g) of tissue:	10.3 mW/g $\pm 16.8\%$ ($k=2$)¹
averaged over 10 cm^3 (10 g) of tissue:	6.68 mW/g $\pm 16.2\%$ ($k=2$)¹

¹ validation uncertainty

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	1.399 ns	(one direction)
Transmission factor:	0.987	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 900 MHz:	$\text{Re}\{Z\} = 51.0 \Omega$
---------------------------------	--

	$\text{Im}\{Z\} = -4.3 \Omega$
--	--

Return Loss at 900 MHz	-27.1 dB
------------------------	-----------------

4. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **body simulating solution** of the following electrical parameters at 900 MHz:

Relative Dielectricity	54.4	$\pm 5\%$
Conductivity	1.04 mho/m	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.3 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was $250\text{mW} \pm 3\%$. The results are normalized to 1W input power.

5. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm³ (1 g) of tissue: **10.8 mW/g ± 16.8 % (k=2)²**

averaged over 10 cm³ (10 g) of tissue: **7.00 mW/g ± 16.2 % (k=2)²**

6. Dipole Impedance and Return Loss

The dipole was positioned at the flat phantom sections according to section 4 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 900 MHz: **Re {Z} = 46.1 Ω**

Im {Z} = -6.4 Ω

Return Loss at 900 MHz **-22.2 dB**

7. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

8. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

9. Power Test

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

² validation uncertainty

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN172

Communication System: CW-900; Frequency: 900 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 900 \text{ MHz}$; $\sigma = 0.94 \text{ mho/m}$; $\epsilon_r = 40.3$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(6.6, 6.6, 6.6); Calibrated: 1/18/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 - SN411; Calibrated: 1/16/2003
- Phantom: SAM with CRP - TP1006; Type: SAM 4.0; Serial: TP:1006
- Measurement SW: DASY4, V4.2 Build 12; Postprocessing SW: SEMCAD, V1.8 Build 93

Pin = 250 mW; d = 15 mm/Area Scan (81x81x1); Measurement grid: dx=15mm, dy=15mm

Reference Value = 56.5 V/m

Power Drift = 0.002 dB

Maximum value of SAR = 2.8 mW/g

Pin = 250 mW; d = 15 mm/Zoom Scan (7x7x7)/Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 3.86 W/kg

SAR(1 g) = 2.58 mW/g; SAR(10 g) = 1.67 mW/g

Reference Value = 56.5 V/m

Power Drift = 0.002 dB

Maximum value of SAR = 2.79 mW/g

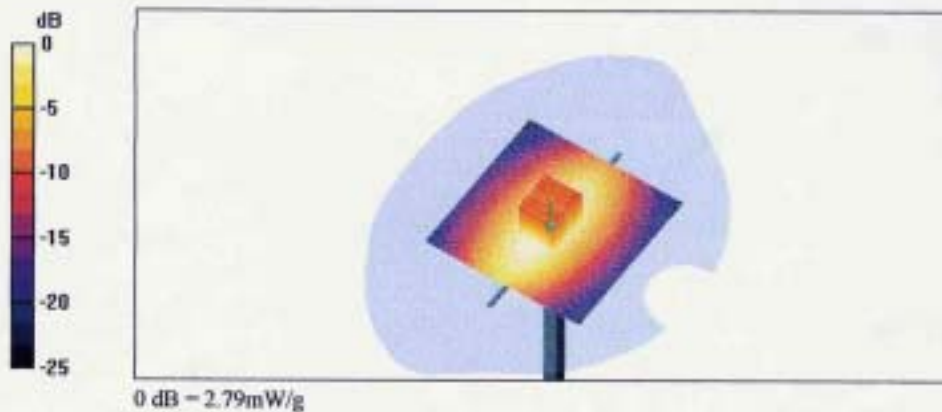


ATL Techno. Corp. RF Testing Lab

Shin-Tien Lab : No. 99, An-Chung Rd., Hsin-Tien City, Taipei Hsien, Taiwan R.O.C.

Tel : 886-(0)2-82122828 / Fax : 886-(0)2-82122829

Tao-Yuan Lab : No. 19, Lane 772, Ho-Ping Rd., Pa-Te City, Taoyuan Hsien, Taiwan R.O.C.

Tel : 886-(0)3-363-1901 / Fax : 886-(0)3-3635002

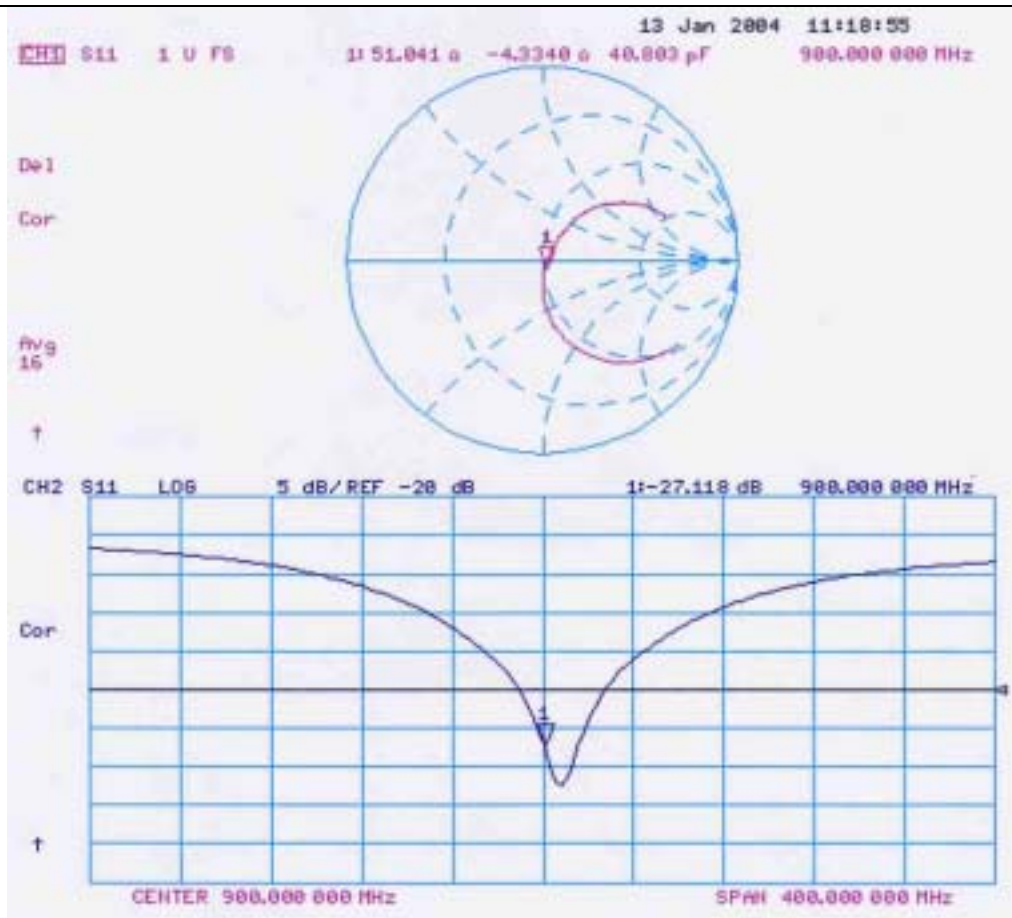Test Report No : 04-0517-S-00-02-01**Test Dates : Sep. 3,6~7, 2004****Oct. 19-20, 2004**

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN172

Communication System: CW-900; Frequency: 900 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 900$ MHz; $\sigma = 1.04$ mho/m; $\epsilon_r = 54.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(6.3, 6.3, 6.3); Calibrated: 1/18/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 - SN411; Calibrated: 1/16/2003
- Phantom: SAM with CRP - TP1006; Type: SAM 4.0; Serial: TP:1006
- Measurement SW: DASY4, V4.2 Build 12; Postprocessing SW: SEMCAD, V1.8 Build 93

Pin = 250 mW; d = 15 mm/Area Scan (81x81x1); Measurement grid: dx=15mm, dy=15mm

Reference Value = 55 V/m

Power Drift = 0.0 dB

Maximum value of SAR = 2.89 mW/g

Pin = 250 mW; d = 15 mm/Zoom Scan (7x7x7)/Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 4.01 W/kg

SAR(1 g) = 2.7 mW/g; SAR(10 g) = 1.75 mW/g

Reference Value = 55 V/m

Power Drift = 0.0 dB

Maximum value of SAR = 2.93 mW/g

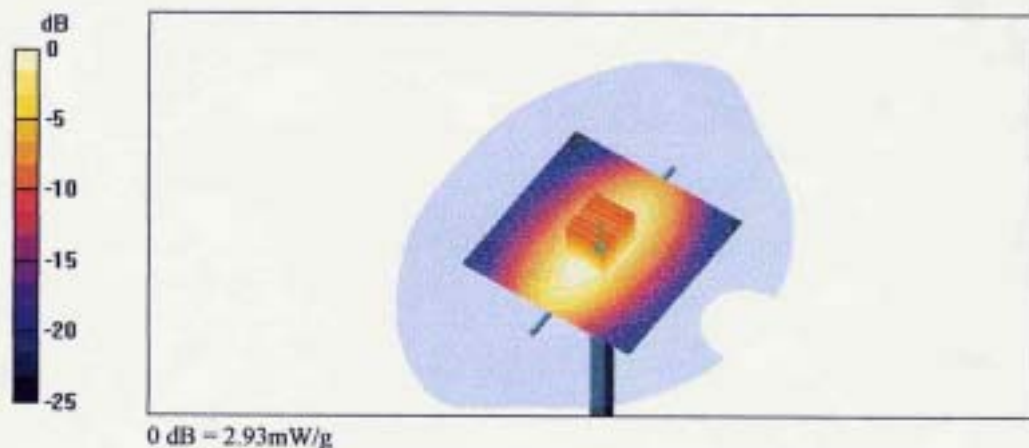


ATL Techno. Corp. RF Testing Lab

Shin-Tien Lab : No. 99, An-Chung Rd., Hsin-Tien City, Taipei Hsien, Taiwan R.O.C.

Tel : 886-(0)2-82122828 / Fax : 886-(0)2-82122829

Tao-Yuan Lab : No. 19, Lane 772, Ho-Ping Rd., Pa-Te City, Taoyuan Hsien, Taiwan R.O.C.

Tel : 886-(0)3-363-1901 / Fax : 886-(0)3-3635002

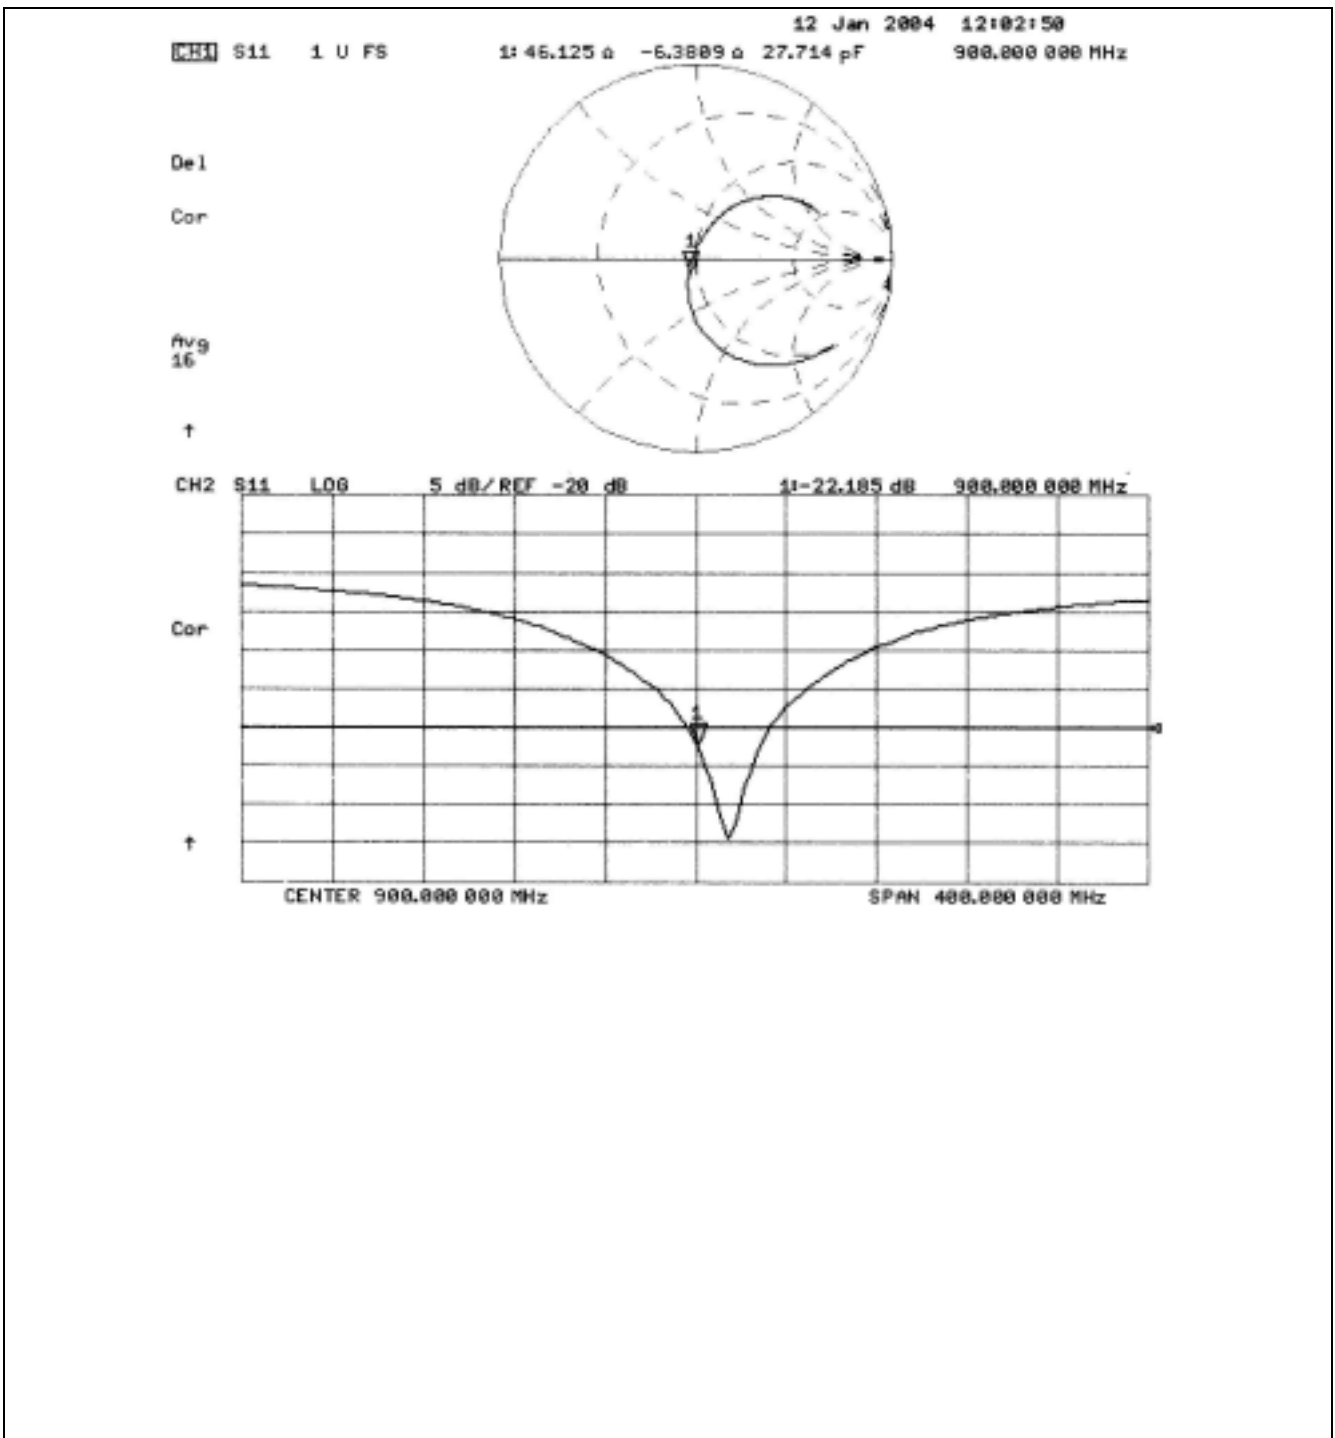Test Report No : 04-0517-S-00-02-01**Test Dates : Sep. 3,6~7, 2004****Oct. 19-20, 2004**

AEL 035

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **Auden**

CALIBRATION CERTIFICATE

Object(s) **D1800V2 - SN:2d057**

Calibration procedure(s) **QA CAL-05.v2
Calibration procedure for dipole validation kits**

Calibration date: **February 9, 2004**

Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM E442	GB37480704	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Power sensor HP 8481A	US37292783	6-Nov-03 (METAS, No. 252-0254)	Nov-04
Power sensor HP 8481A	MY41092317	18-Oct-02 (Agilent, No. 20021018)	Oct-04
RF generator R&S SML-03	100698	27-Mar-2002 (R&S, No. 20-92389)	In house check: Mar-05
Network Analyzer HP 8753E	US37360585	18-Oct-01 (SPEAG, in house check Nov-03)	In house check: Oct 05

Calibrated by: **Judith Mueller** Name: **Judith Mueller** Function: **Technician** Signature: *[Signature]*

Approved by: **Katja Pokovic** Name: **Katja Pokovic** Function: **Laboratory Director** Signature: *[Signature]*

Date issued: February 18, 2004

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 international Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

880-KP0301051-A

合格
93.2.09
羅登科技品質保證
專用章

世安福 吳俊志

Page 1 (1)

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland

Phone +41 1 245 9700, Fax +41 1 245 9779

info@speag.com, <http://www.speag.com>

DASY

Dipole Validation Kit

Type: D1800V2

Serial: 2d057

Manufactured: Octobre 16, 2002

Calibrated: February 9, 2004

1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **head simulating solution** of the following electrical parameters at 1800 MHz:

Relative Dielectricity	39.2	$\pm 5\%$
Conductivity	1.37 mho/m	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 5.08 at 1800 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was 250mW $\pm 3\%$. The results are normalized to 1W input power.

2. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm ³ (1 g) of tissue:	39.6 mW/g $\pm 16.8\%$ (k=2)¹
averaged over 10 cm ³ (10 g) of tissue:	21.1 mW/g $\pm 16.2\%$ (k=2)¹

¹ validation uncertainty

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	1.201 ns	(one direction)
Transmission factor:	0.997	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 1800 MHz:	$\text{Re}\{Z\} = \mathbf{48.9\ \Omega}$
----------------------------------	--

	$\text{Im}\{Z\} = \mathbf{-5.0\ \Omega}$
--	--

Return Loss at 1800 MHz	-25.8 dB
-------------------------	-----------------

4. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **body simulating solution** of the following electrical parameters at 1800 MHz:

Relative Dielectricity	53.0	$\pm 5\%$
Conductivity	1.49 mho/m	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 4.61 at 1800 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was $250\text{ mW} \pm 3\%$. The results are normalized to 1W input power.

5. SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm³ (1 g) of tissue: **39.8 mW/g ± 16.8 % (k=2)²**

averaged over 10 cm³ (10 g) of tissue: **21.6 mW/g ± 16.2 % (k=2)²**

6. Dipole Impedance and Return Loss

The dipole was positioned at the flat phantom sections according to section 4 and the distance spacer was in place during impedance measurements.

Feedpoint impedance at 1800 MHz: **Re {Z} = 44.8 Ω**

Im {Z} = -3.9 Ω

Return Loss at 1800 MHz **-23.2 dB**

7. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

8. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

9. Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

² validation uncertainty

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN2d057

Communication System: CW-1800; Frequency: 1800 MHz; Duty Cycle: 1:1

Medium: HSL 1800 MHz

Medium parameters used: $f = 1800$ MHz; $\sigma = 1.37$ mho/m; $\epsilon_r = 39.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(5.08, 5.08, 5.08); Calibrated: 1/23/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn411; Calibrated: 11/6/2003
- Phantom: SAM with CRP - TP1006; Type: SAM 4.0; Serial: TP:1006
- Measurement SW: DASY4, V4.2 Build 25; Postprocessing SW: SEMCAD, V1.8 Build 93

Pin = 250 mW; d = 10 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 93.5 V/m

Power Drift = 0.0 dB

Maximum value of SAR = 11.2 mW/g

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 17.6 W/kg

SAR(1 g) = 9.9 mW/g; SAR(10 g) = 5.27 mW/g

Reference Value = 93.5 V/m

Power Drift = 0.0 dB

Maximum value of SAR = 11.2 mW/g

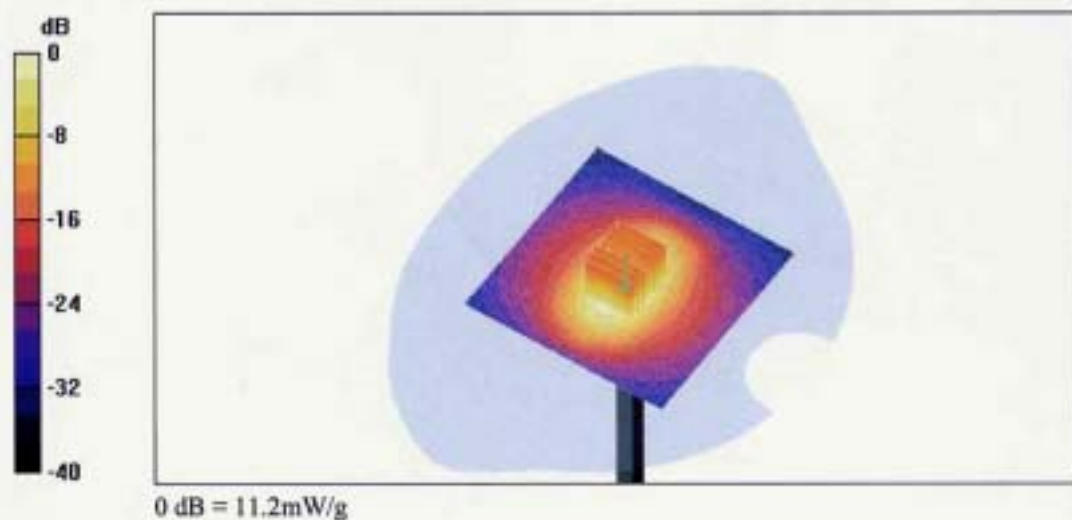


ATL Techno. Corp. RF Testing Lab

Shin-Tien Lab : No. 99, An-Chung Rd., Hsin-Tien City, Taipei Hsien, Taiwan R.O.C.

Tel : 886-(0)2-82122828 / Fax : 886-(0)2-82122829

Tao-Yuan Lab : No. 19, Lane 772, Ho-Ping Rd., Pa-Te City, Taoyuan Hsien, Taiwan R.O.C.

Tel : 886-(0)3-363-1901 / Fax : 886-(0)3-3635002

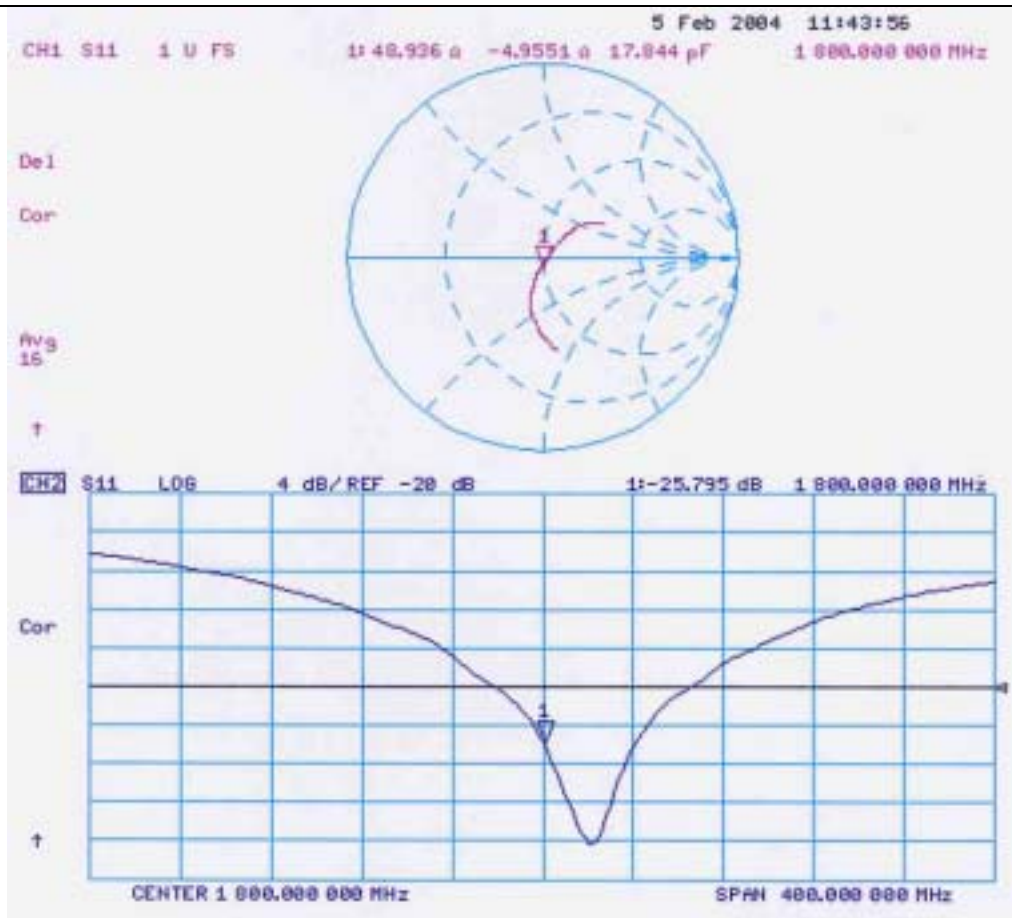Test Report No : 04-0517-S-00-02-01**Test Dates : Sep. 3,6~7, 2004****Oct. 19-20, 2004**

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN2d057

Communication System: CW-1800; Frequency: 1800 MHz; Duty Cycle: 1:1

Medium: Muscle 1800 MHz;

Medium parameters used: $f = 1800$ MHz; $\sigma = 1.49$ mho/m; $\epsilon_r = 53$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 - SN1507; ConvF(4.61, 4.61, 4.61); Calibrated: 1/23/2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 - SN411; Calibrated: 11/6/2003
- Phantom: SAM with CRP - TP1006; Type: SAM 4.0; Serial: TP:1006;
- Measurement SW: DASY4, V4.2 Build 25; Postprocessing SW: SEMCAD, V1.8 Build 101

Pin = 250 mW; d = 10 mm/Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 93.4 V/m; Power Drift = -0.002 dB

Maximum value of SAR (interpolated) = 11.2 mW/g


Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 93.4 V/m; Power Drift = -0.002 dB

Maximum value of SAR (measured) = 11.2 mW/g

Peak SAR (extrapolated) = 16.6 W/kg

SAR(1 g) = 9.95 mW/g; SAR(10 g) = 5.39 mW/g

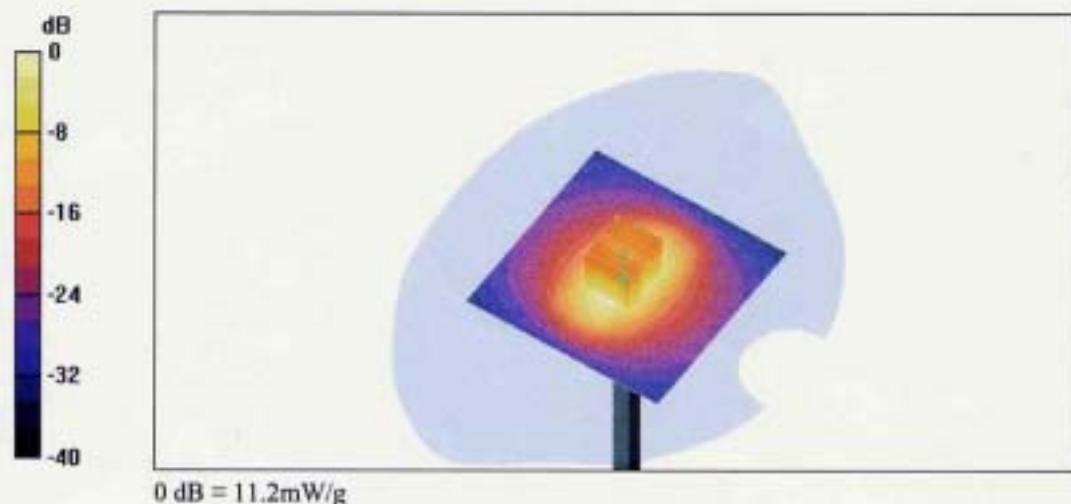


ATL Techno. Corp. RF Testing Lab

Shin-Tien Lab : No. 99, An-Chung Rd., Hsin-Tien City, Taipei Hsien, Taiwan R.O.C.


Tel : 886-(0)2-82122828 / Fax : 886-(0)2-82122829



Tao-Yuan Lab : No. 19, Lane 772, Ho-Ping Rd., Pa-Te City, Taoyuan Hsien, Taiwan R.O.C.

Tel : 886-(0)3-363-1901 / Fax : 886-(0)3-3635002

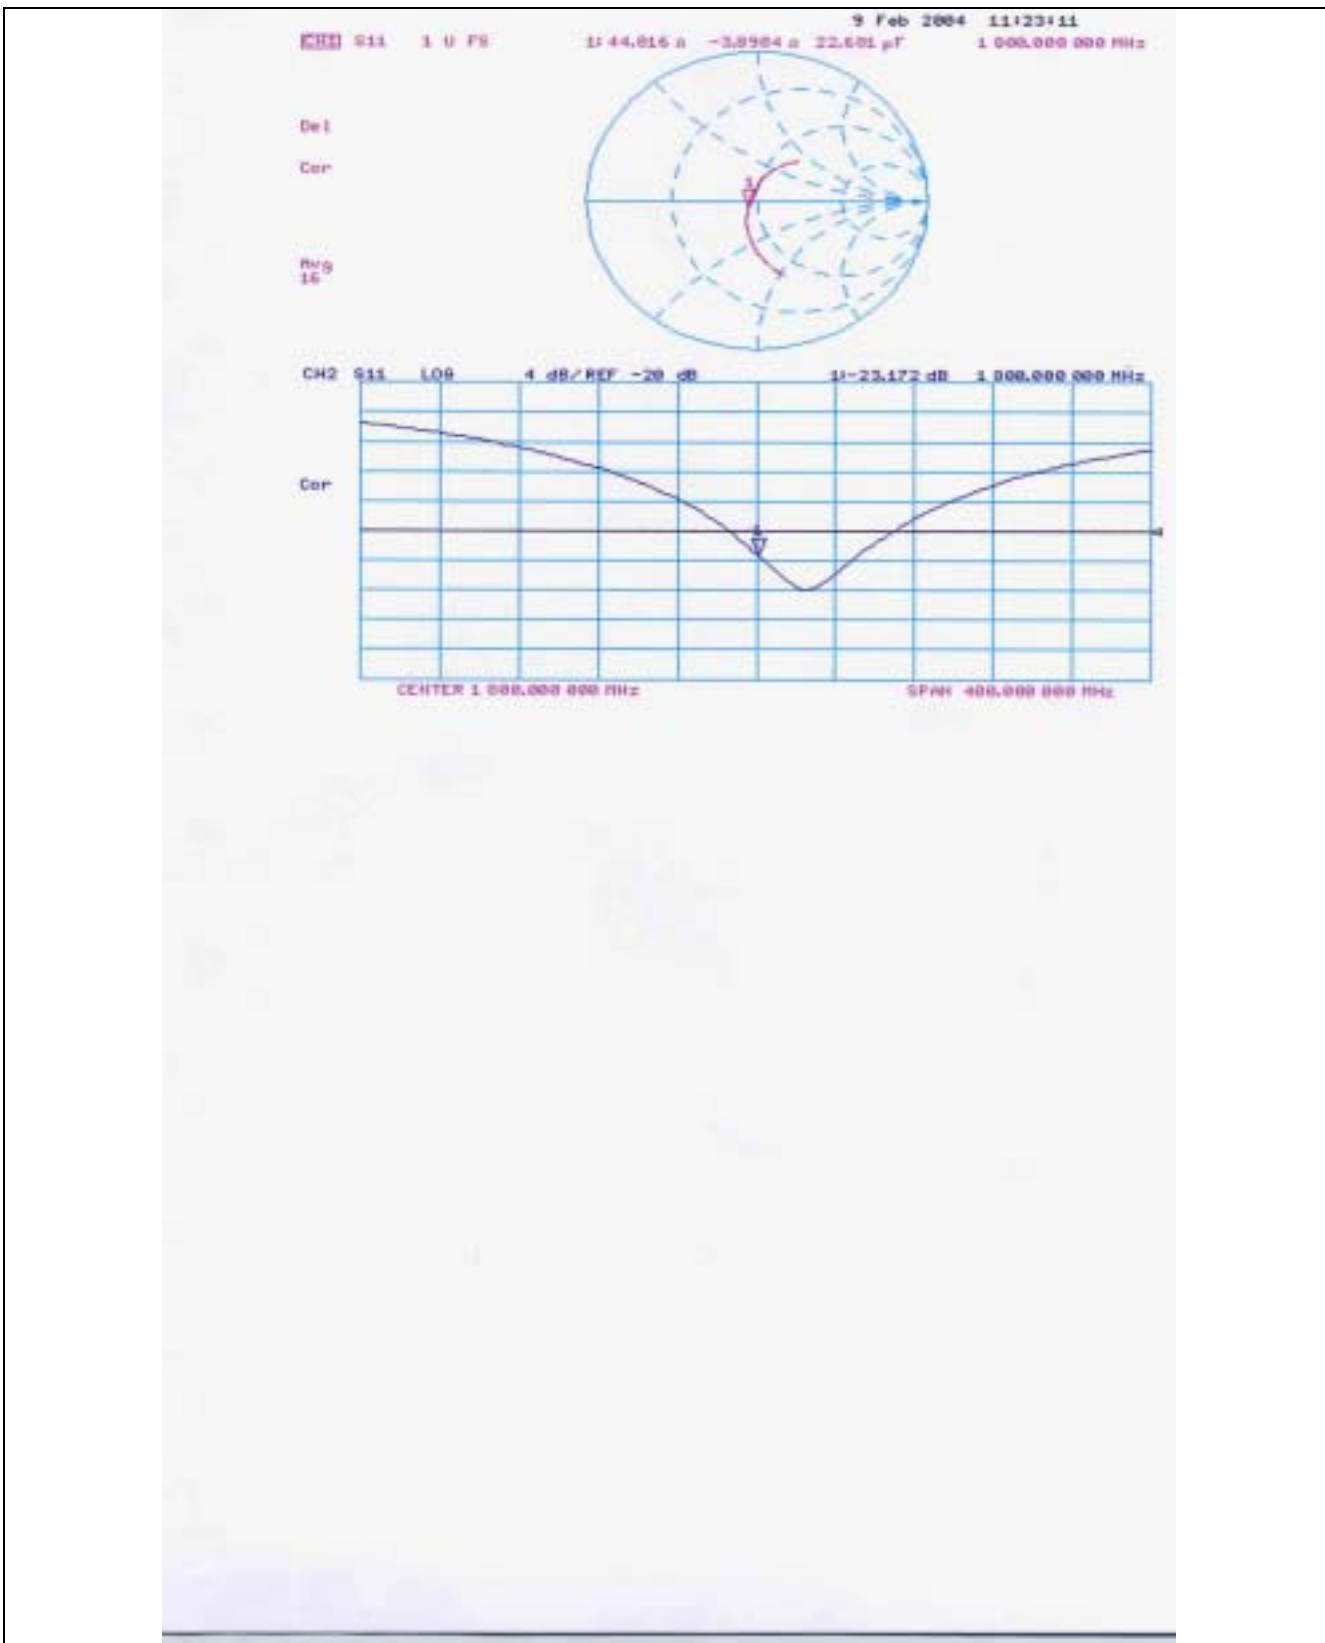Test Report No : 04-0517-S-00-02-01**Test Dates : Sep. 3,6~7, 2004****Oct. 19-20, 2004**

Appendix D – Probe Calibration

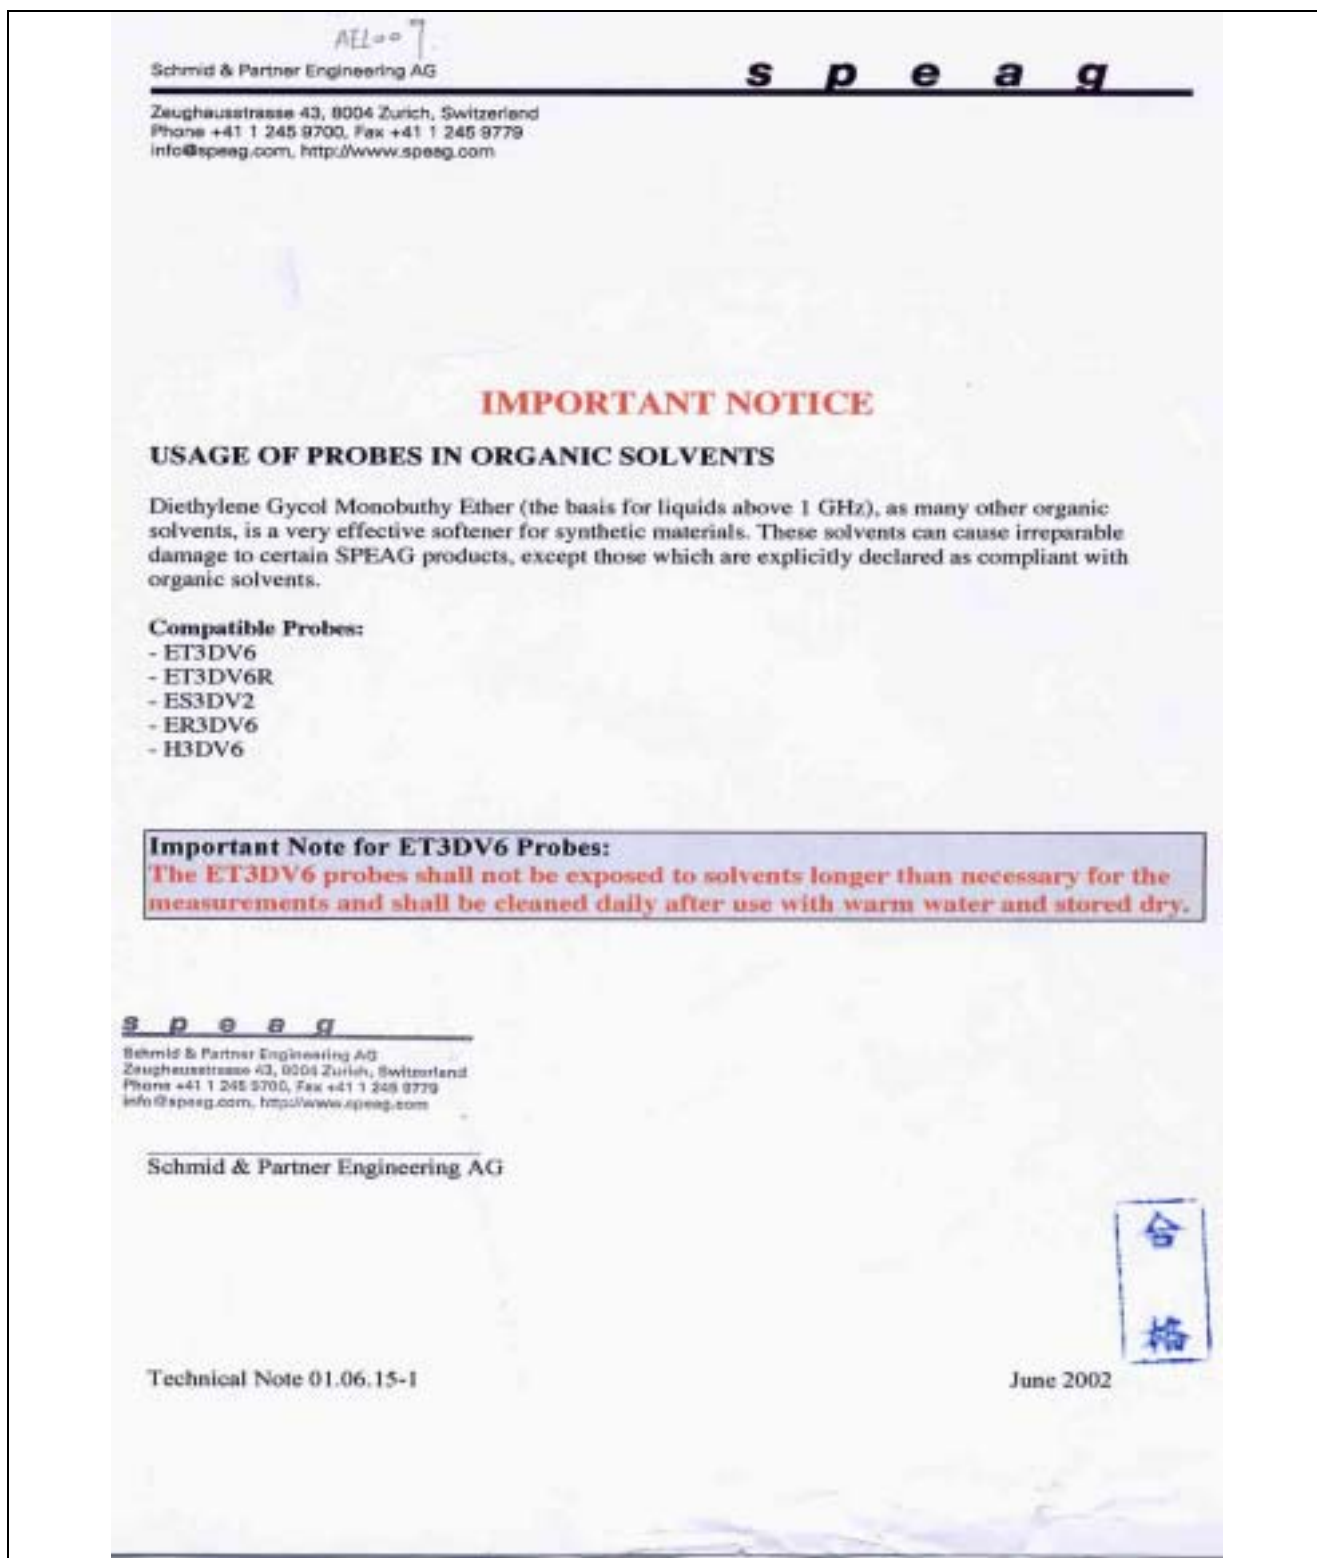

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland			
Client		Auden	
CALIBRATION CERTIFICATE			
Object(s)	ET3DV6 - SN:1531		
Calibration procedure(s)	QA CAL-01 v2 Calibration procedure for dosimetric E-field probes		
Calibration date:	September 19, 2003		
Condition of the calibrated item	In Tolerance (according to the specific calibration document)		
This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 International standard.			
All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.			
Calibration Equipment used (M&TE critical for calibration)			
Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM E4419B	GB41293574	2-Apr-03 (METAS, No 252-0250)	Apr-04
Power sensor E4412A	MY41495277	2-Apr-03 (METAS, No 252-0250)	Apr-04
Reference 20 dB Attenuator	SN: 5086 (20%)	3-Apr-03 (METAS No. 251-0340)	Apr-04
Fluke Process Calibrator Type 762	SN: 6295893	8-Sep-03 (Simbel SCS No. E-003020)	Sep-04
Power sensor HP 8481A	MY41092180	18-Sep-02 (Agilent, No. 20020918)	In house check: Oct 03
RF generator HP 8684C	US3642U01709	4-Aug-99 (SPEAG, in house check Aug-02)	In house check: Aug-05
Network Analyzer HP 8753E	US37395585	18-Oct-01 (Agilent, No. 24BR1033101)	In house check: Oct 03
Calibrated by:	Name Katja Pukovic	Function Laboratory Director	Signature 
Approved by:	Name Fin Borcholt	Function R&D Director	Signature 
Date issued: September 19, 2003			
This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.			
880-KP0301061-A		Page 1 (1) 	

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland

Phone +41 1 245 9700, Fax +41 1 245 9779

info@speag.com, <http://www.speag.com>

Probe ET3DV6

SN:1531

Manufactured:	July 15, 2000
Last calibration:	August 27, 2002
Recalibrated:	September 19, 2003

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1531

September 19, 2003

DASY - Parameters of Probe: ET3DV6 SN:1531**Sensitivity in Free Space****Diode Compression**

NormX	1.45 $\mu\text{V}/(\text{V}/\text{m})^2$	DCP X	95	mV
NormY	1.48 $\mu\text{V}/(\text{V}/\text{m})^2$	DCP Y	95	mV
NormZ	1.51 $\mu\text{V}/(\text{V}/\text{m})^2$	DCP Z	95	mV

Sensitivity in Tissue Simulating LiquidHead 900 MHz $\epsilon_r = 41.5 \pm 5\%$ $\sigma = 0.97 \pm 5\%$ mho/m

Valid for f=855-945 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	6.3 $\pm 9.5\%$ (k=2)	Boundary effect:	
ConvF Y	6.3 $\pm 9.5\%$ (k=2)	Alpha	0.29
ConvF Z	6.3 $\pm 9.5\%$ (k=2)	Depth	3.64

Head 1800 MHz $\epsilon_r = 40.0 \pm 5\%$ $\sigma = 1.40 \pm 5\%$ mho/m

Valid for f=1710-1890 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	5.3 $\pm 9.5\%$ (k=2)	Boundary effect:	
ConvF Y	5.3 $\pm 9.5\%$ (k=2)	Alpha	0.52
ConvF Z	5.3 $\pm 9.5\%$ (k=2)	Depth	2.58

Boundary Effect

Head 900 MHz Typical SAR gradient: 5 % per mm

Probe Tip to Boundary		1 mm	2 mm
SAR _{be} [%] Without Correction Algorithm		12.5	7.8
SAR _{be} [%] With Correction Algorithm		0.8	0.8

Head 1800 MHz Typical SAR gradient: 10 % per mm

Probe Tip to Boundary		1 mm	2 mm
SAR _{be} [%] Without Correction Algorithm		13.9	9.2
SAR _{be} [%] With Correction Algorithm		0.1	0.0


Sensor Offset

Probe Tip to Sensor Center	2.7	mm
Optical Surface Detection	1.4 $\pm$ 0.2	mm

ET3DV6 SN:1531



September 19, 2003

Receiving Pattern (ϕ), $\theta = 0^\circ$

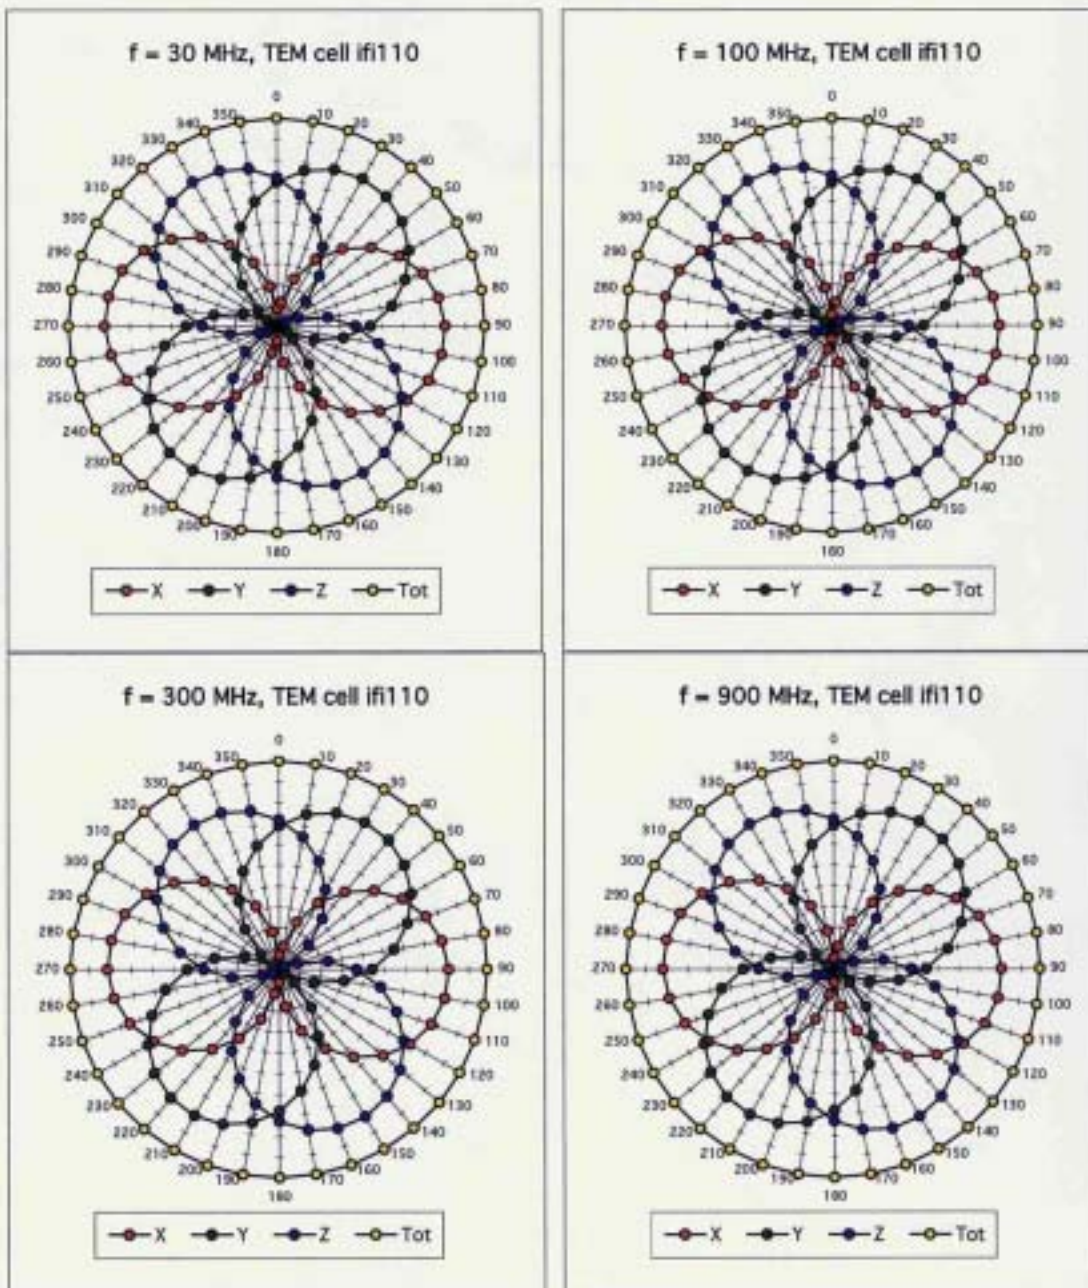


ET3DV6 SN:1531

September 19, 2003

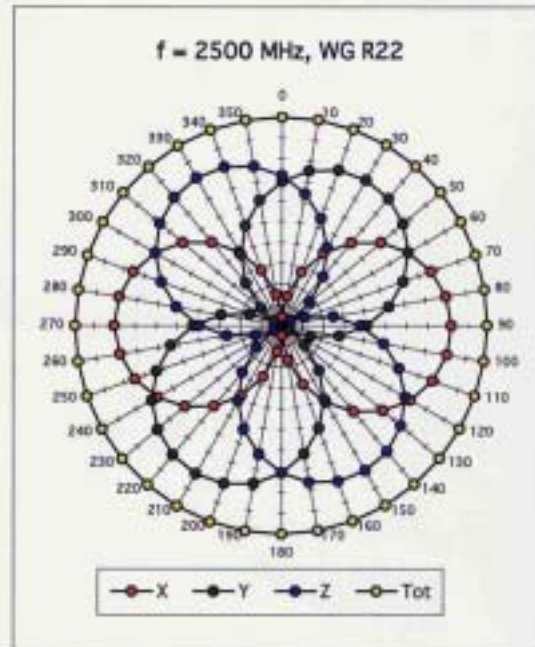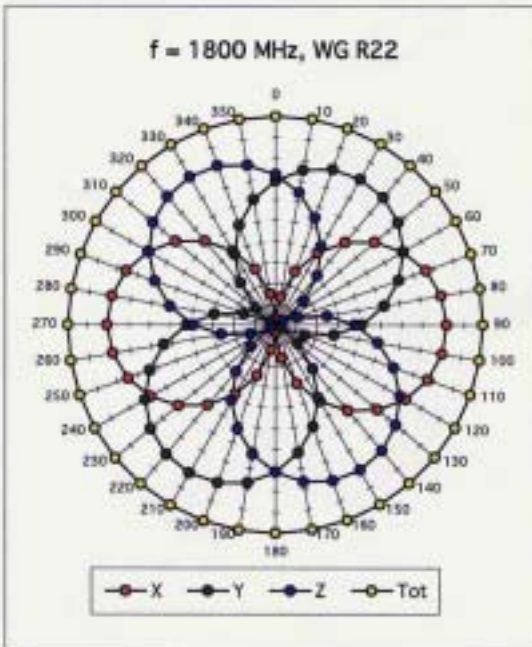

Isotropy Error (ϕ), $\theta = 0^\circ$

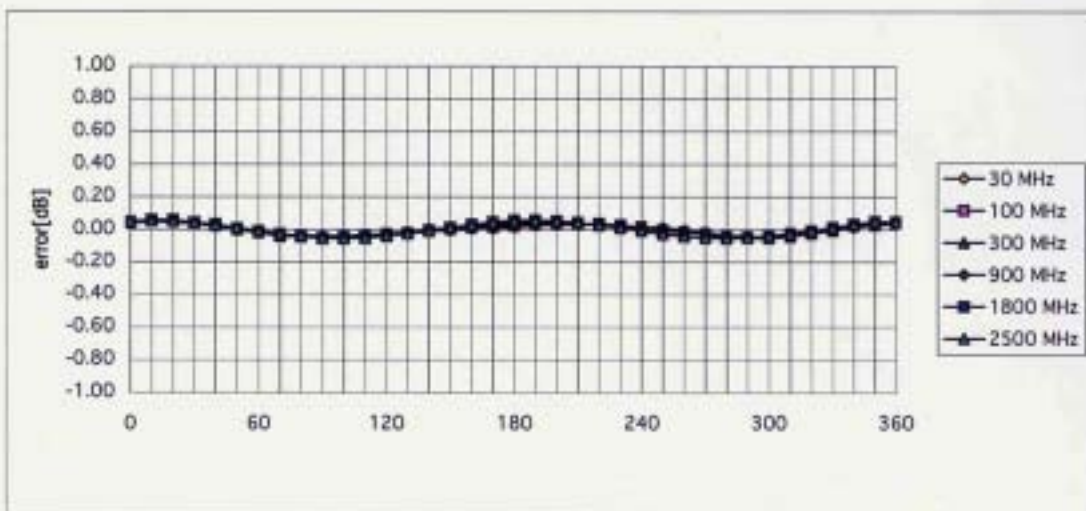


ET3DV6 SN:1531

September 19, 2003

Frequency Response of E-Field

(TEM-Cell:ifi110, Waveguide R22)


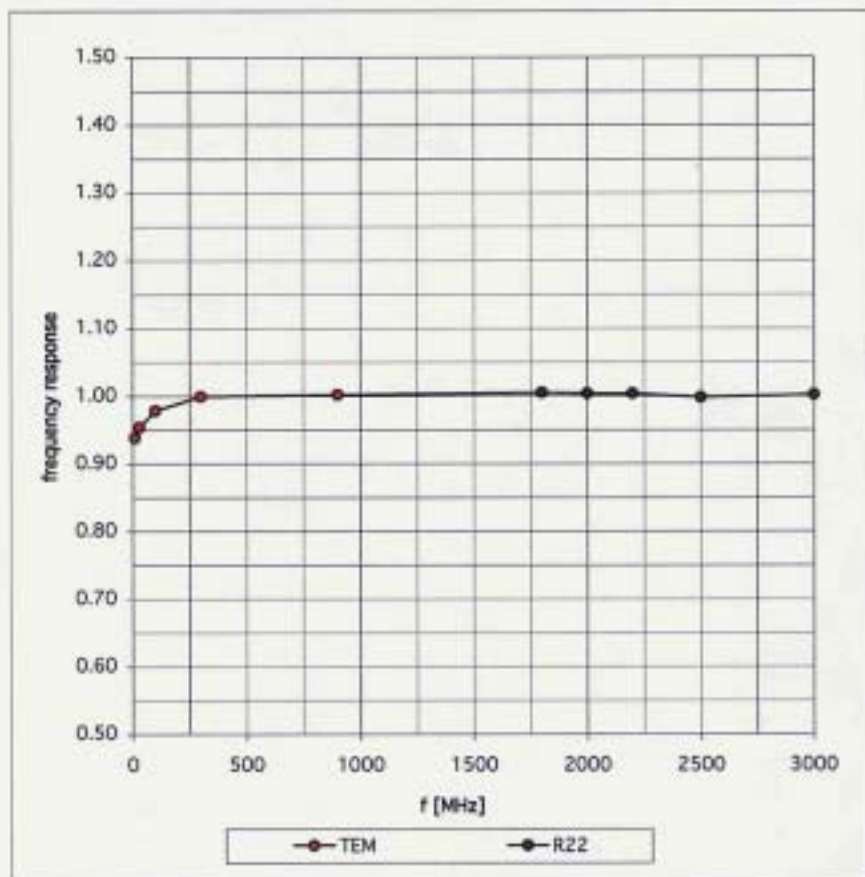



ET3DV6 SN:1531


September 19, 2003


Dynamic Range f(SARhead)


(Waveguide R22)

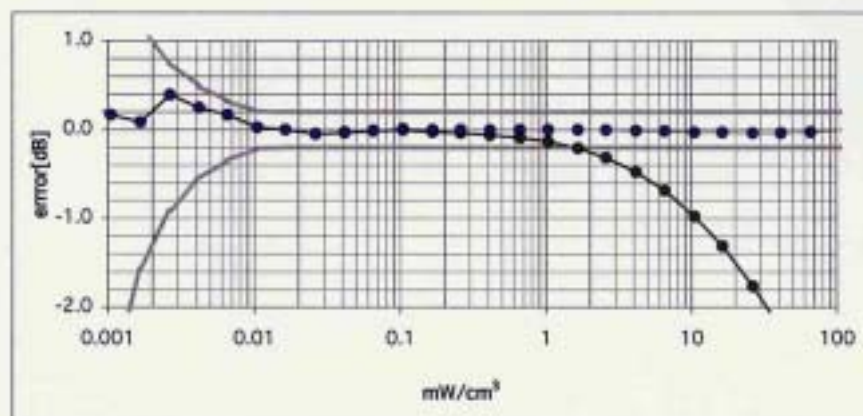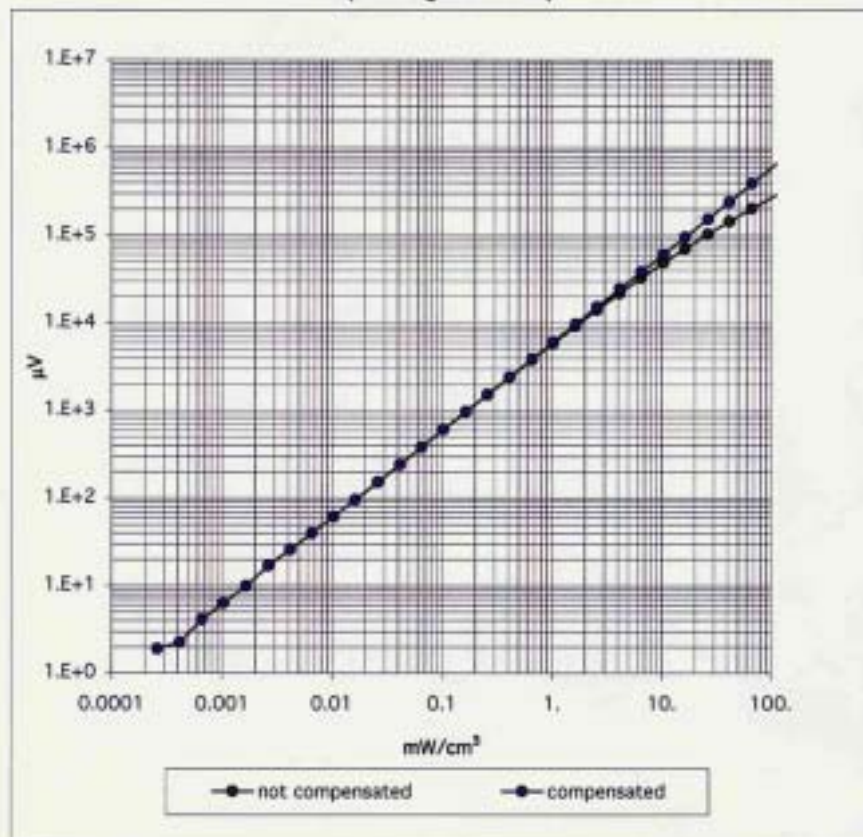


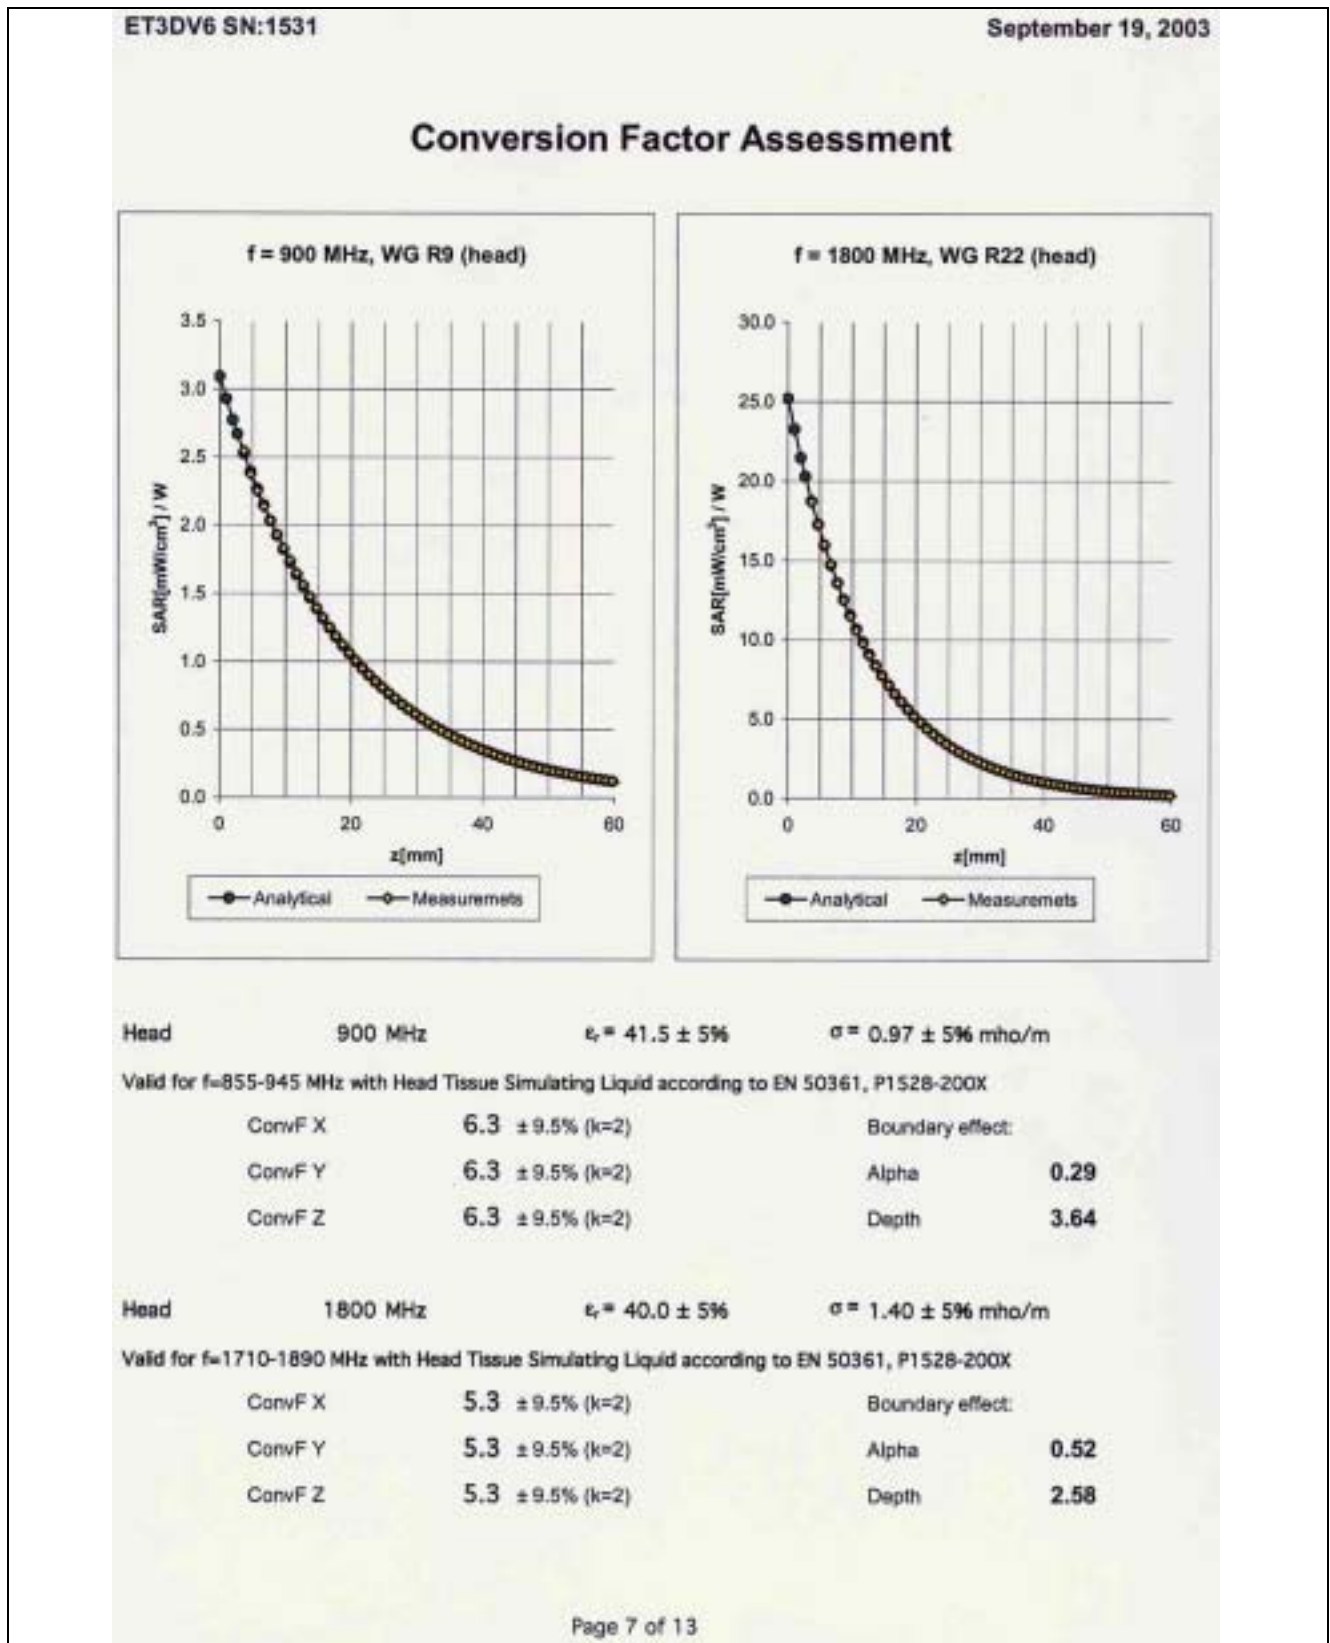


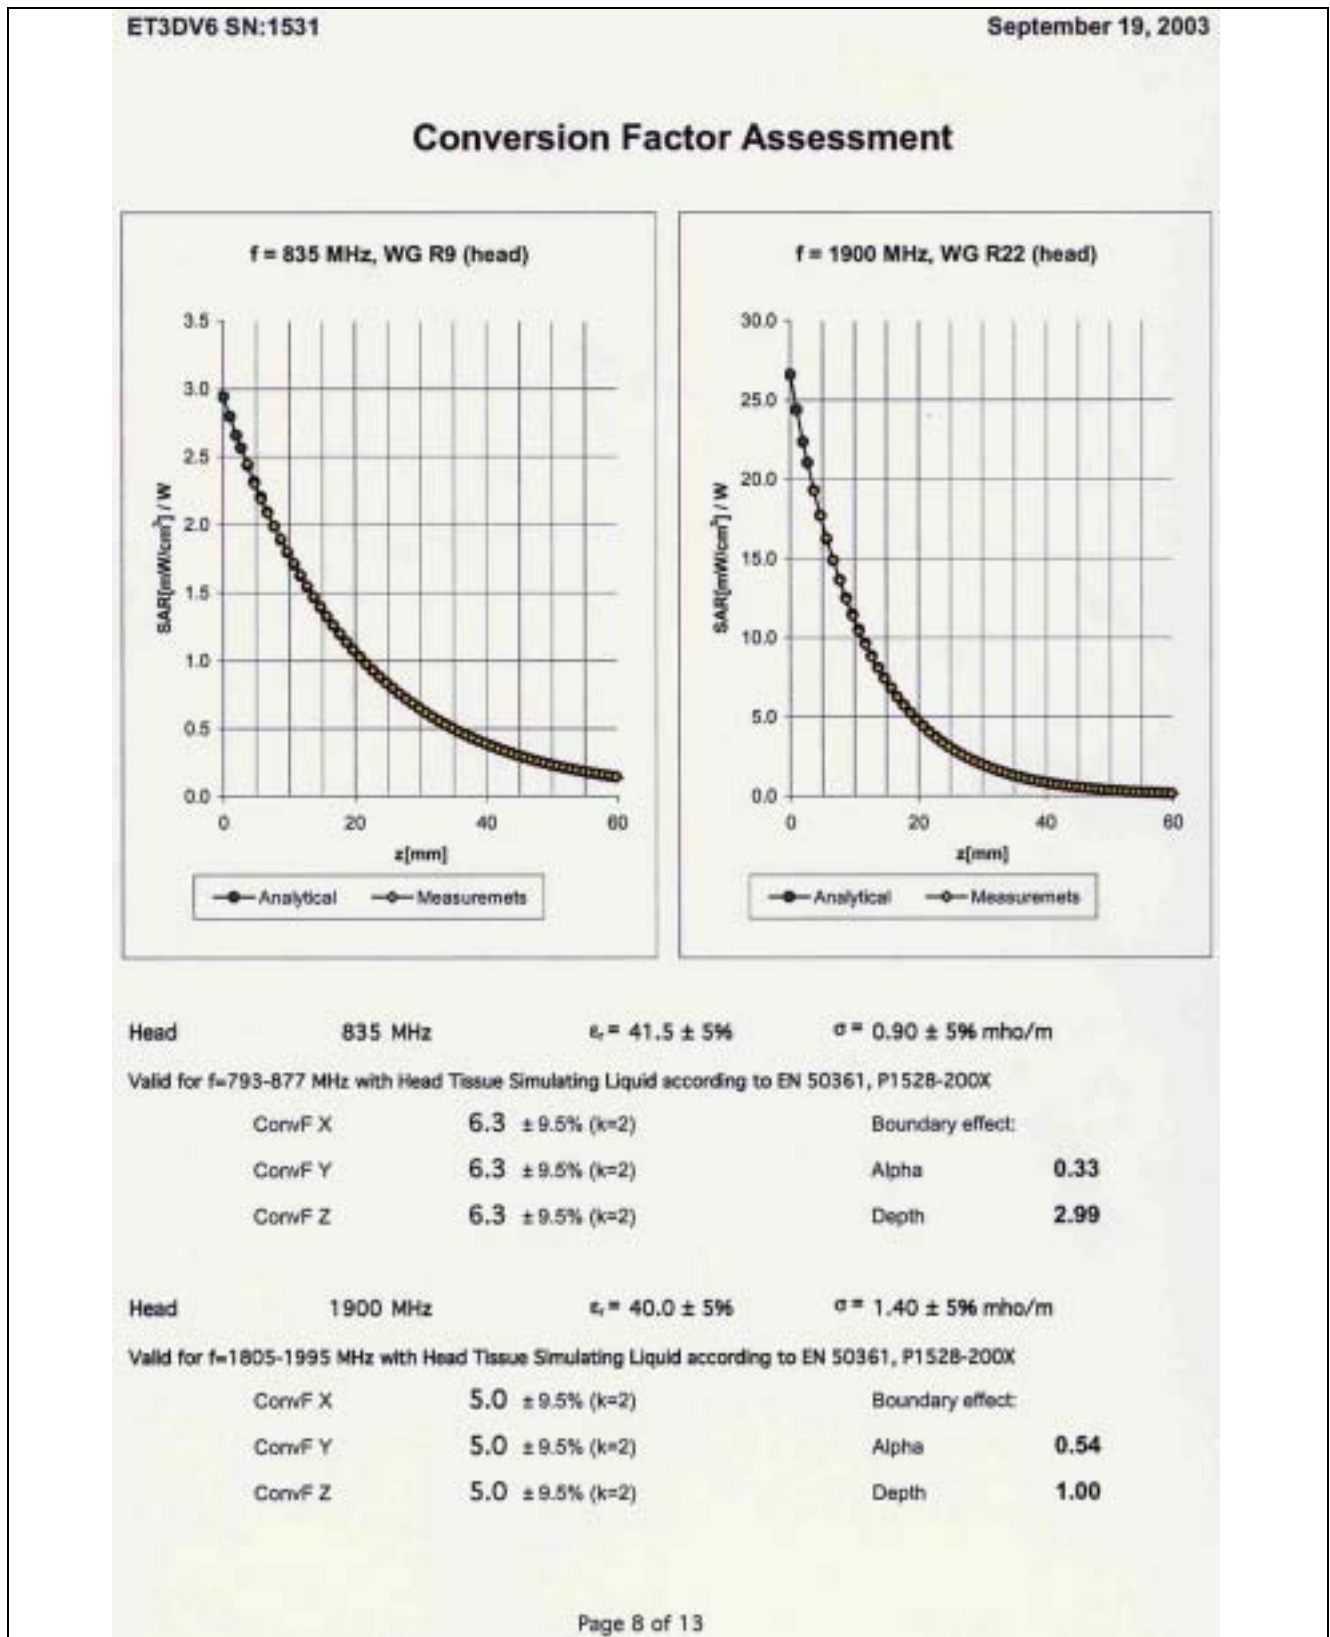


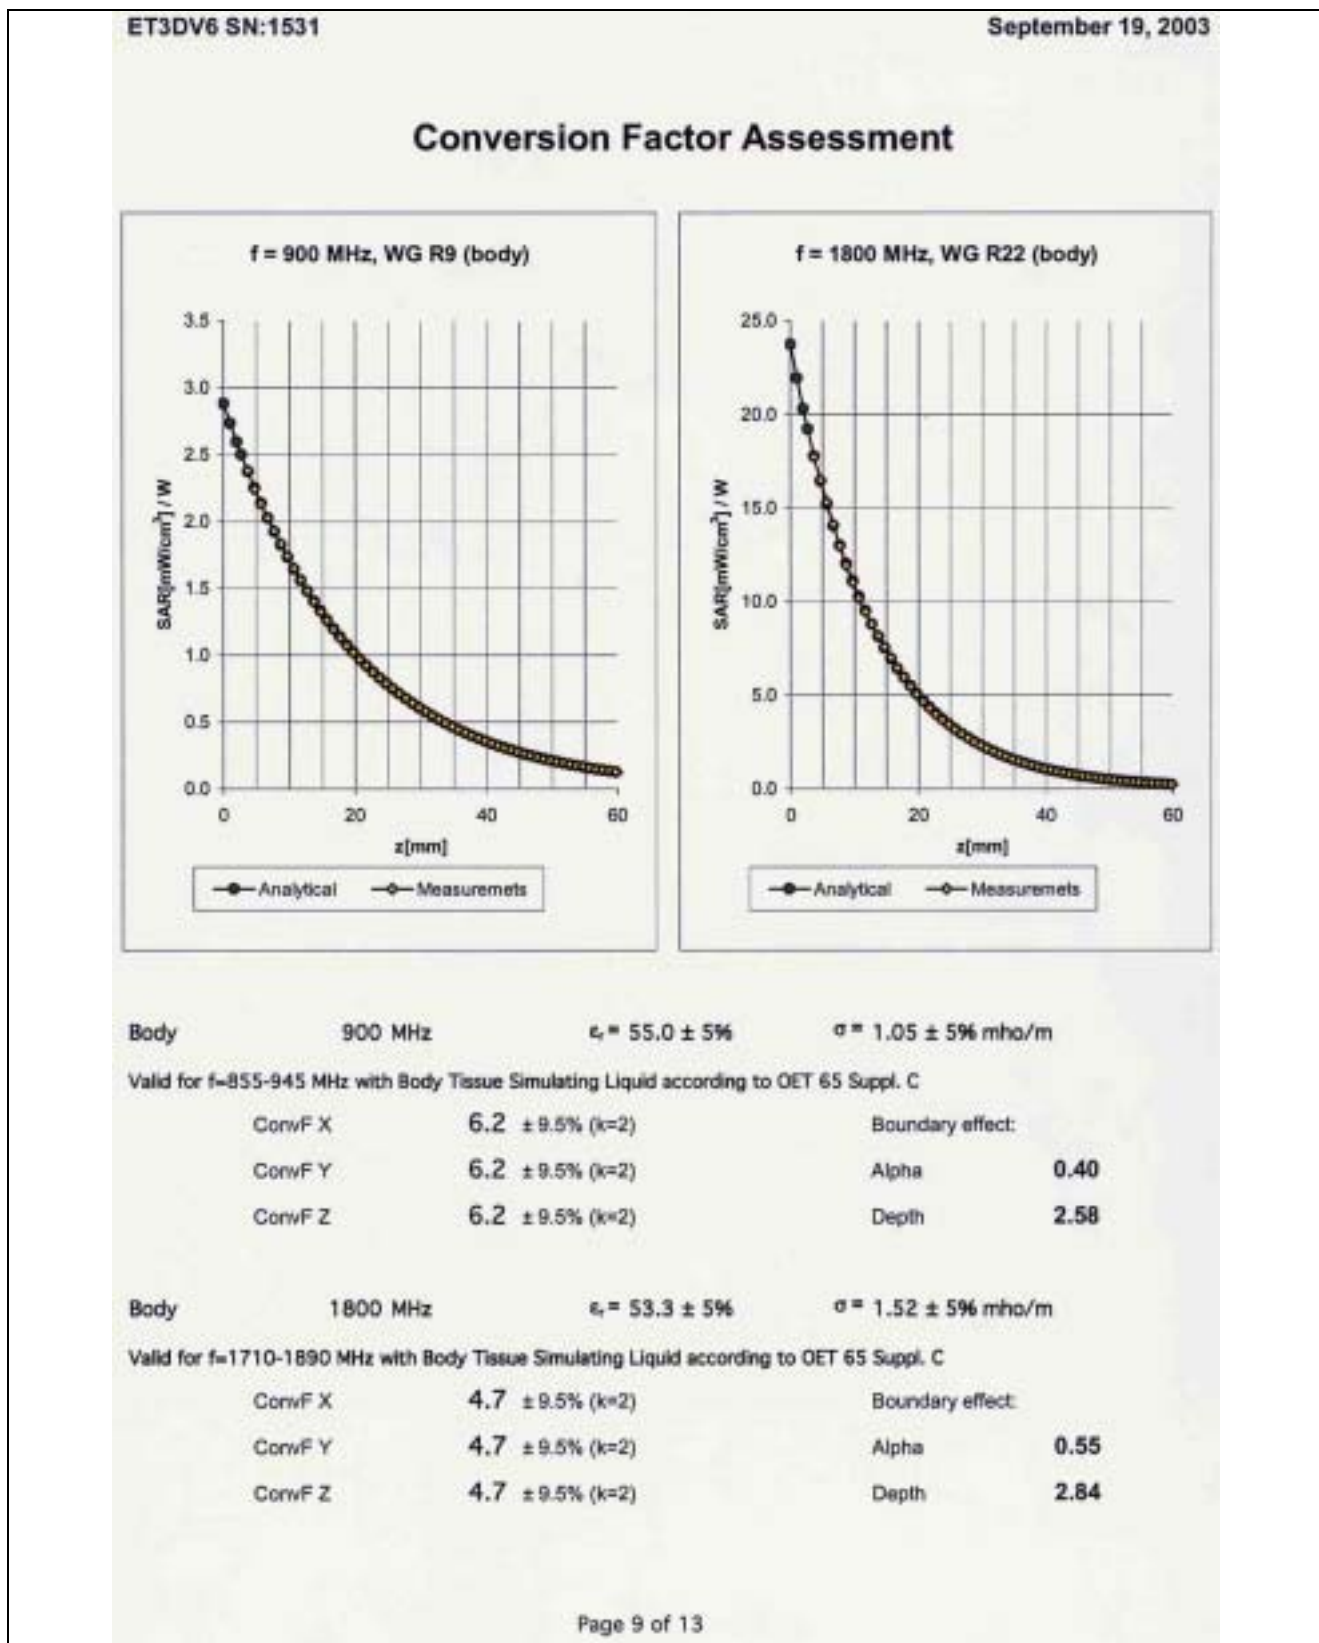

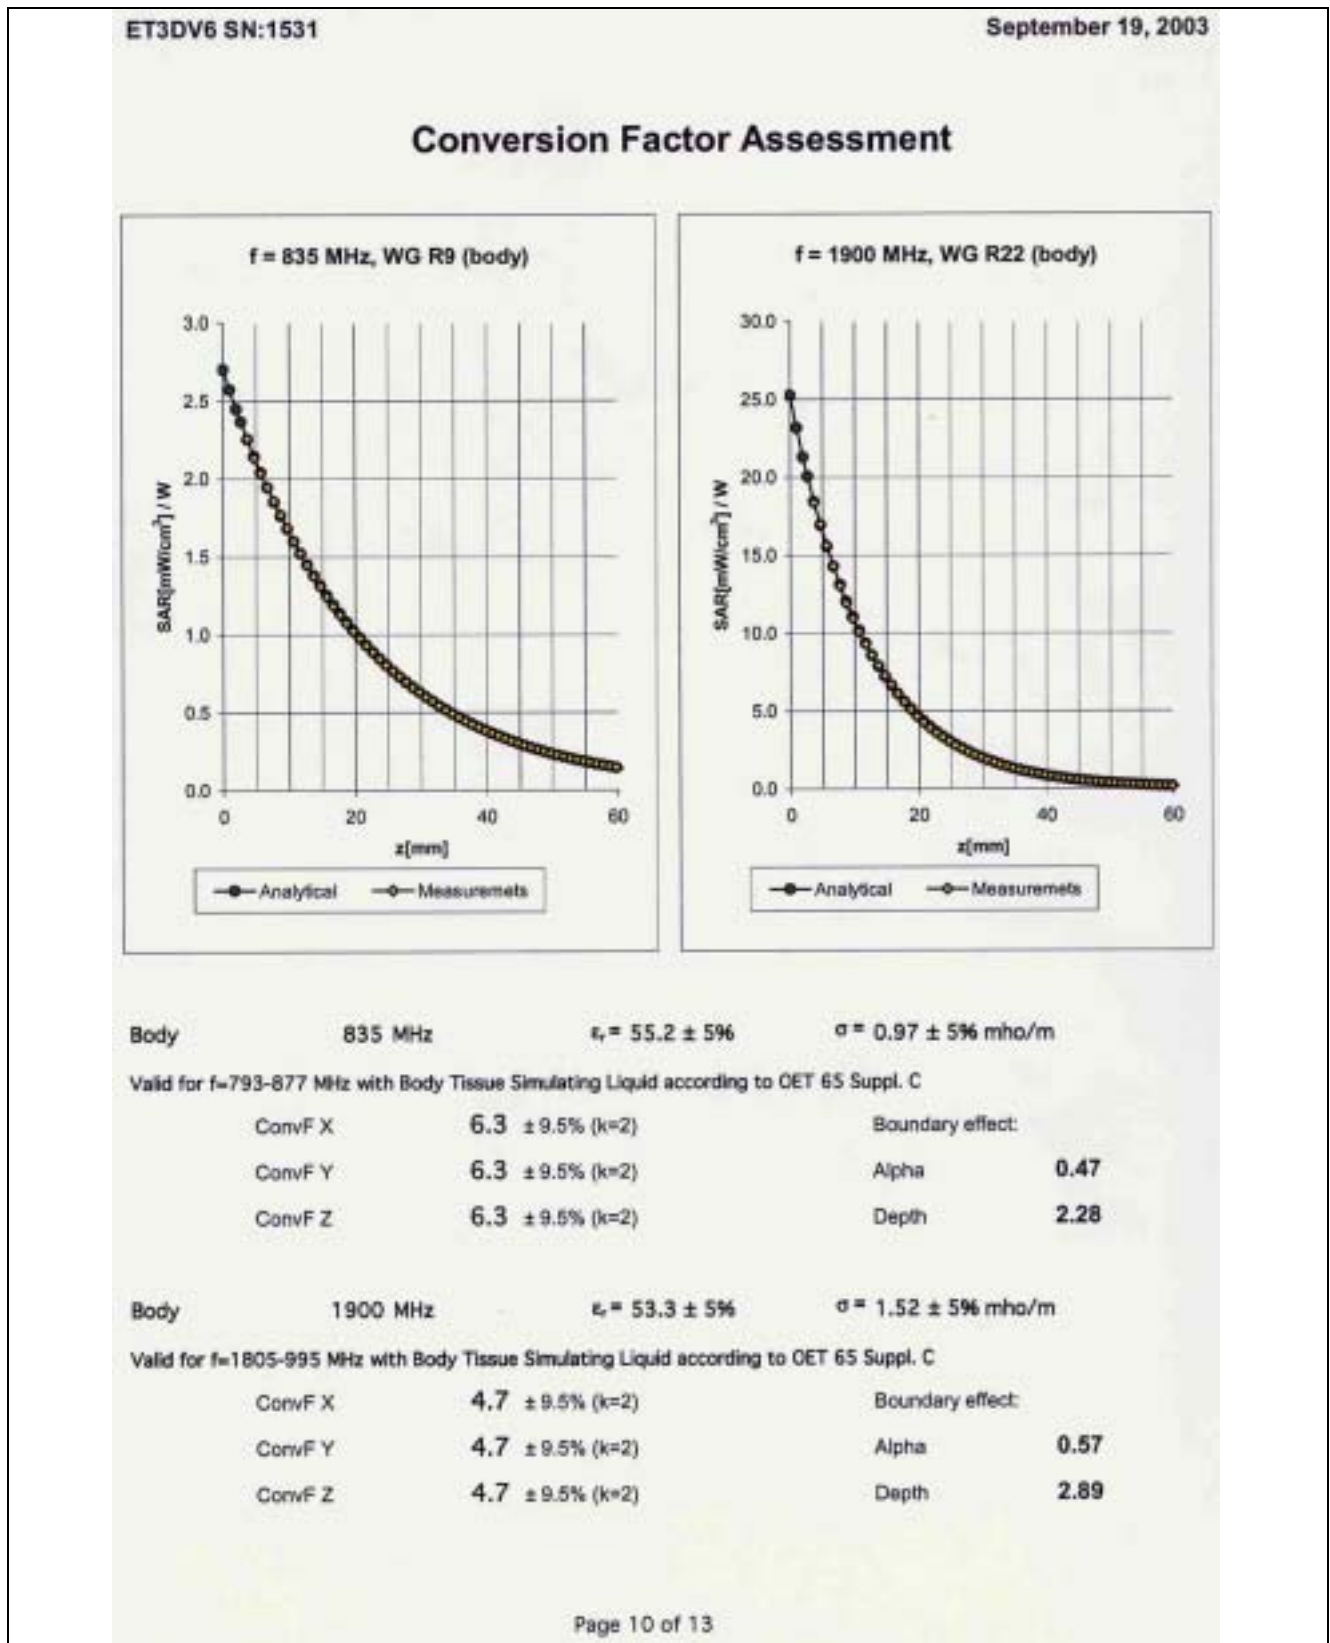

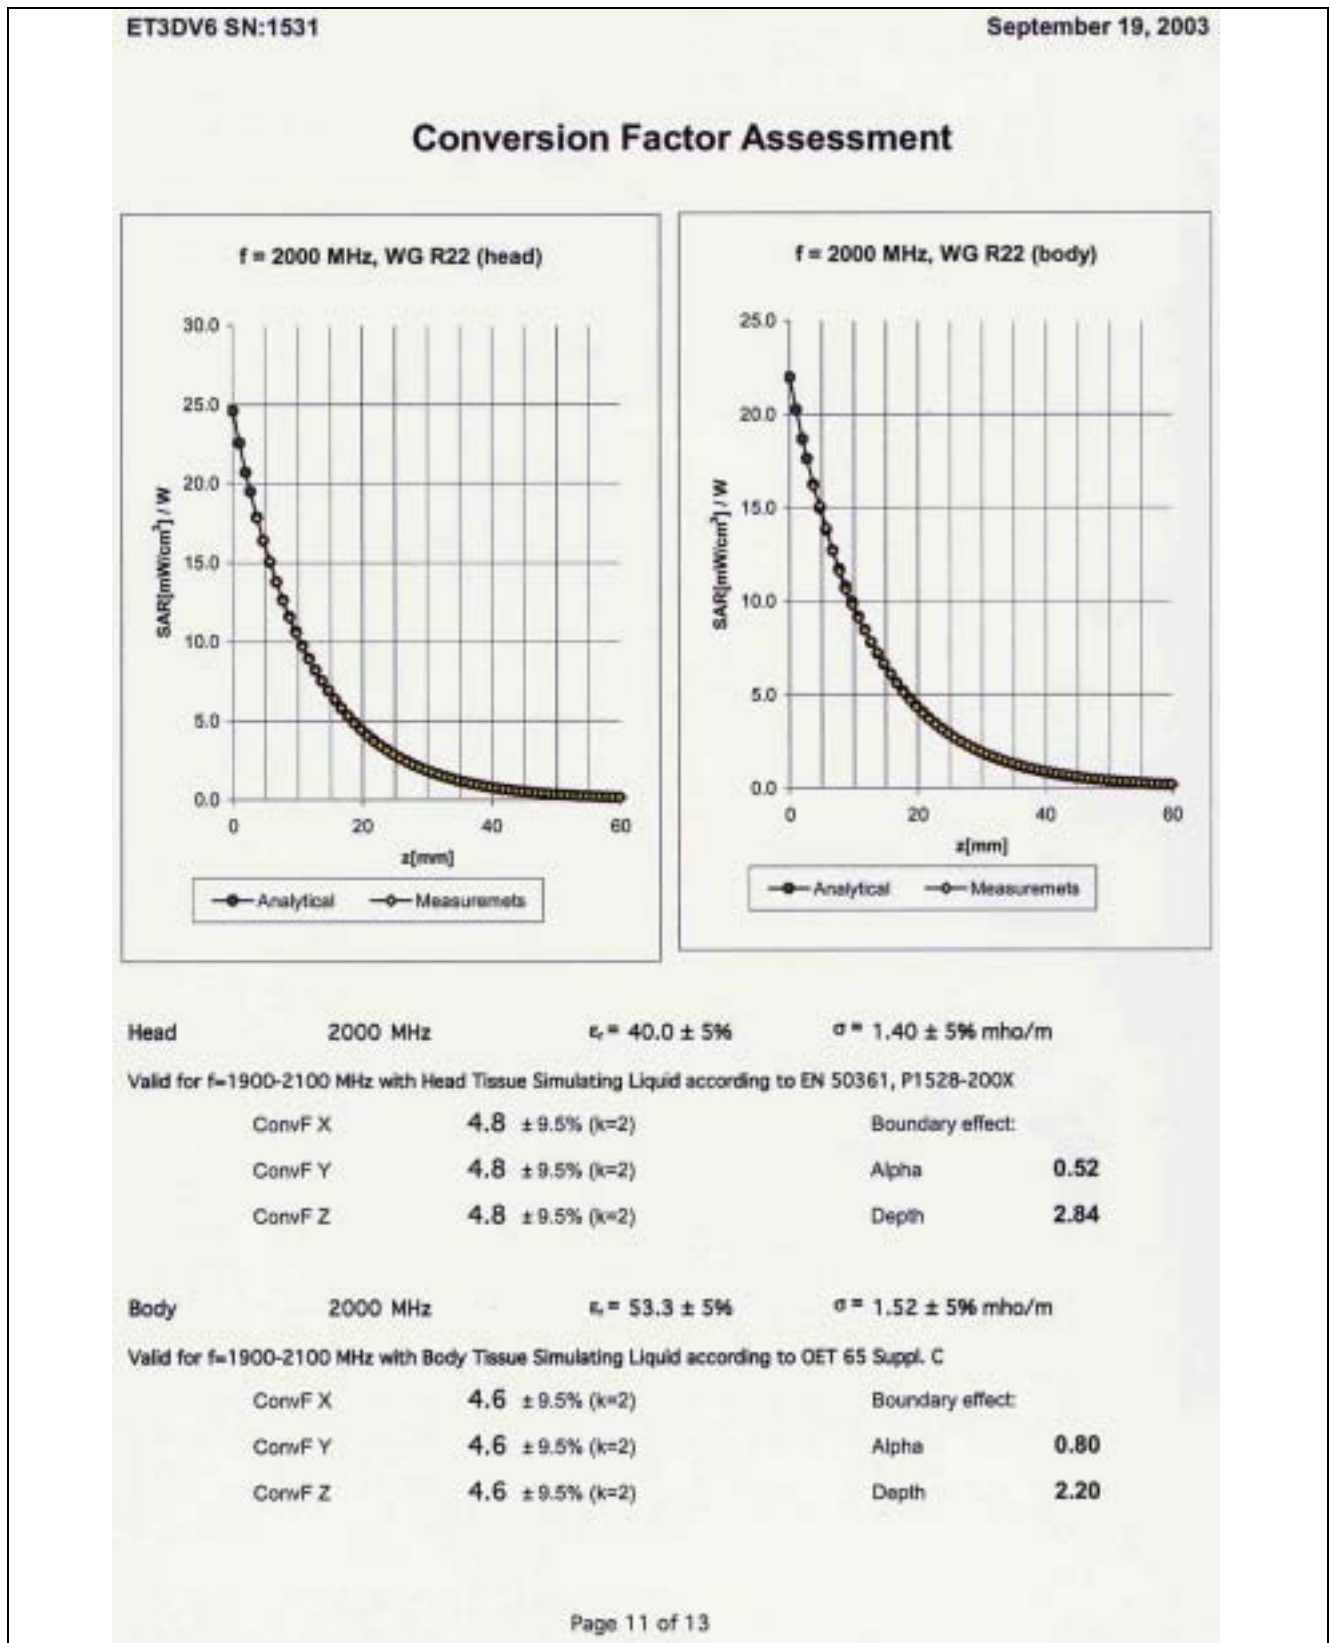

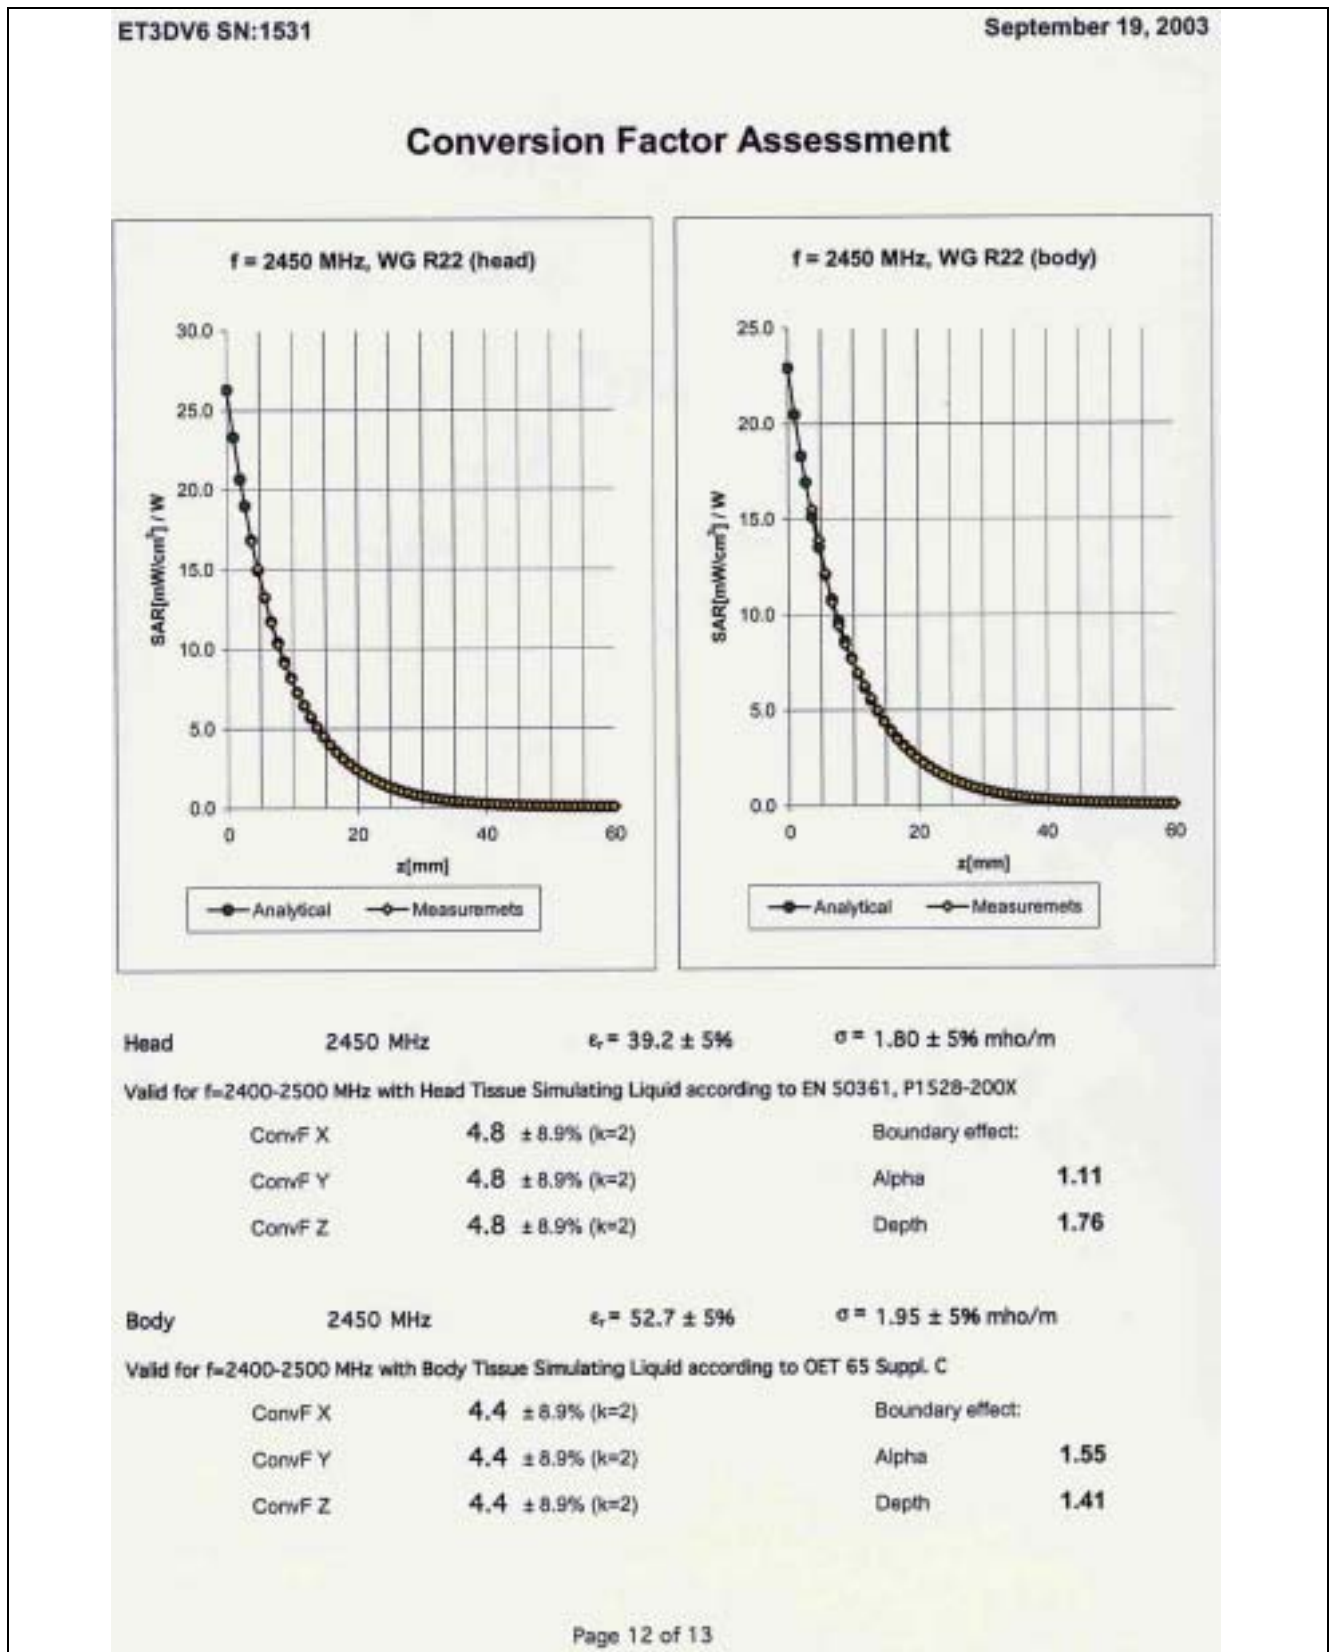

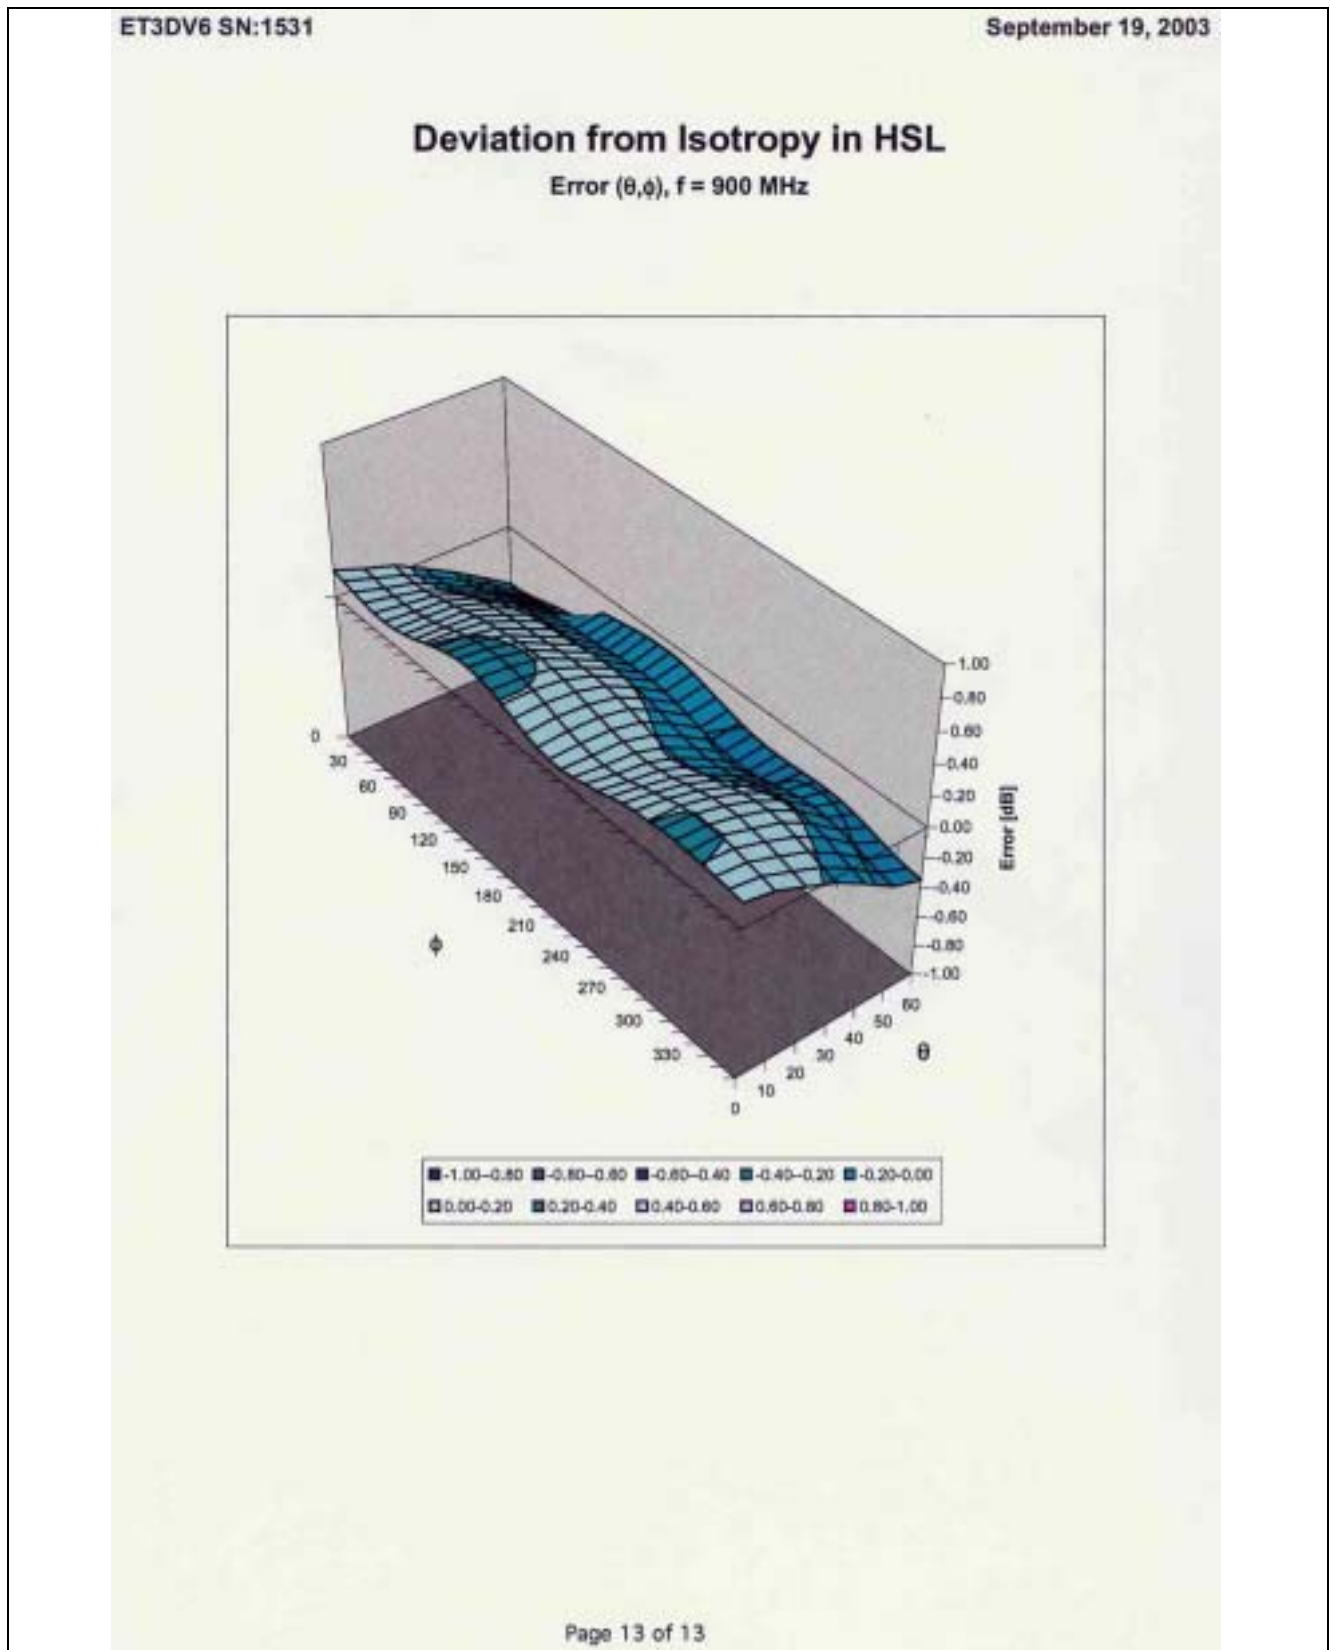

Appendix E – Data Acquisition Electronic (DAE) Calibration

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland			
Client		Auden	
CALIBRATION CERTIFICATE			
Object(s)	DAE3 – SD 000 D03 AA – SN:393		
Calibration procedure(s)	QA CAL-06.v5a Calibration procedure for the data acquisition unit (DAE)		
Calibration date:	08.01.2004		
Condition of the calibrated item	In Tolerance (according to the specific calibration document)		
This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.			
All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.			
Calibration Equipment used (M&TE critical for calibration)			
Model Type	ID #	Cal Date	Scheduled Calibration
Fuke Process Calibrator Type 702	SN: 6295603	8-Sep-03	Sep-04
Calibrated by:		Name	Function
		Philipp Storchenegger	Technician
Approved by:		Name	Function
		F. Bornholt	R&D Director
		Date issued: 08.01.2004	
This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.			





DAE3 SN: 393

DATE: 08.01.2004

1. Cal Lab. Incoming Inspection & Pre Test

Modification Status	Note Status here → → → →	BC
Visual Inspection	Note anomalies.....	None
Pre Test	Indication	Yes/No
Probe Touch	Function	Yes
Probe Collision	Function	Yes
Probe Touch&Collision	Function	Yes

2. DC Voltage Measurement

A/D - Converter Resolution nominal

 High Range: 1LSB = 6.1μV, full range = 400 mV
 Low Range: 1LSB = 61nV, full range = 4 mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.989	404.251	404.118
Low Range	3.96967	3.95088	3.95250
Connector Angle to be used	in DASY System 15°		

High Range	Input	Reading in μV	% Error
Channel X + Input	200mV	199999.5	0.00
	20mV	19999.8	0.00
Channel X - Input	20mV	-19992.4	-0.04
Channel Y + Input	200mV	200000.2	0.00
	20mV	19996.1	-0.02
Channel Y - Input	20mV	-19992.5	-0.04
Channel Z + Input	200mV	200000.0	0.00
	20mV	20001.4	0.01
Channel Z - Input	20mV	-19998.8	-0.01

Low Range	Input	Reading in μV	% Error
Channel X + Input	2mV	1999.91	0.00
	0.2mV	199.98	-0.01
Channel X - Input	0.2mV	-200.39	0.19
Channel Y + Input	2mV	1999.94	0.00
	0.2mV	199.28	-0.36
Channel Y - Input	0.2mV	-200.58	0.29
Channel Z + Input	2mV	2000.03	0.00
	0.2mV	199.19	-0.41
Channel Z - Input	0.2mV	-201.21	0.61

Page 2 of 4

DAE3 SN: 393

DATE: 08.01.2004

6. Input Offset Measurement

DASY measurement parameters:

Auto Zero Time: 3 sec,

Measuring time: 3 sec

Number of measurements:

100, Low Range

 Input 10M Ω

in μ V	Average	min. Offset	max. Offset	Std. Deviation
Channel X	1.27	0.41	1.94	0.27
Channel Y	-1.15	-2.03	-0.01	0.32
Channel Z	-0.17	-2.91	1.44	0.42

Input shorted

in μ V	Average	min. Offset	max. Offset	Std. Deviation
Channel X	0.14	-0.33	0.69	0.18
Channel Y	-0.77	-1.88	-0.17	0.22
Channel Z	-0.87	-2.76	0.98	0.38

7. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

8. Input Resistance

In MOhm	Calibrating	Measuring
Channel X	0.1999	198.3
Channel Y	0.2001	198.4
Channel Z	0.1998	198.6

9. Low Battery Alarm Voltage

in V	Alarm Level
Supply (+ Vcc)	8.01
Supply (- Vcc)	-7.74

10. Power Consumption

in mA	Switched off	Stand by	Transmitting
Supply (+ Vcc)	0.00	5.43	13.8
Supply (- Vcc)	-0.01	-7.60	-8.79

Page 4 of 4