



Appendix D

Photographs

- | |
|--|
| 1. SAR measurement System |
| 2. Photographs of Tissue Simulate Liquid |
| 3. Photographs of EUT test position |
| 4. EUT Constructional Details |






1. SAR measurement System






2. Photographs of Tissue Simulate Liquid

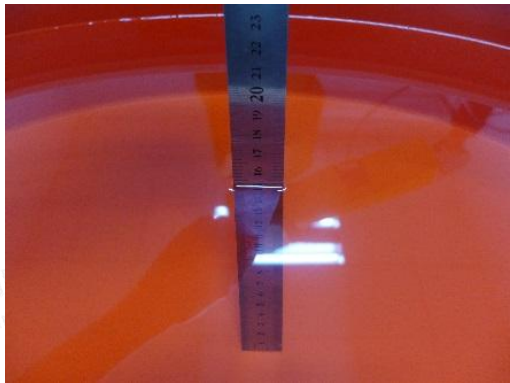Photo 1: Tissue Simulant Liquid for Head 2300-2500	Photo 2: Tissue Simulant Liquid for Head 5000-6000
	





3. Photographs of EUT test position

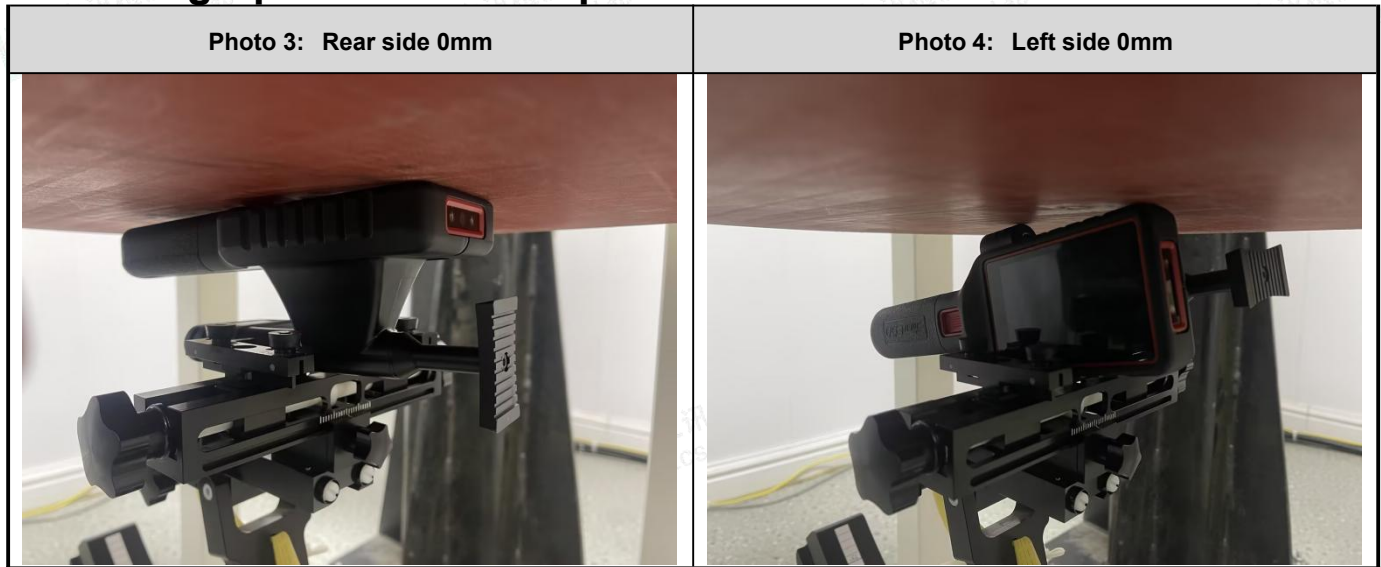

4. EUT Constructional Details

Photo 5: Front View	Photo 6: Back View
	
Photo 7: Front View 2	
	

