

System Check_Head_13MHz

DUT: CLA13-1022

Communication System: CW; Frequency: 13 MHz; Duty Cycle: 1:1

Medium: HSL_13_240328 Medium parameters used : $f = 13$ MHz; $\sigma = 0.728$ S/m; $\epsilon_r = 54.685$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.6 °C; Liquid Temperature : 22.6 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN7306; ConvF(16.9, 16.9, 16.9) @ 13 MHz; Calibrated: 2023/7/18
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2024/1/22
- Phantom: ELI v4.0_Mid; Type: QDOVA001AA; Serial: TP:1026
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

Pin=1000mW/Area Scan (81x81x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm

Maximum value of SAR (interpolated) = 1.12 W/kg

Pin=1000mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 38.63 V/m; Power Drift = -0.07 dB


Peak SAR (extrapolated) = 1.39 W/kg

SAR(1 g) = 0.612 W/kg; SAR(10 g) = 0.367 W/kg

Smallest distance from peaks to all points 3 dB below = 16 mm

Ratio of SAR at M2 to SAR at M1 = 54%

Maximum value of SAR (measured) = 1.10 W/kg

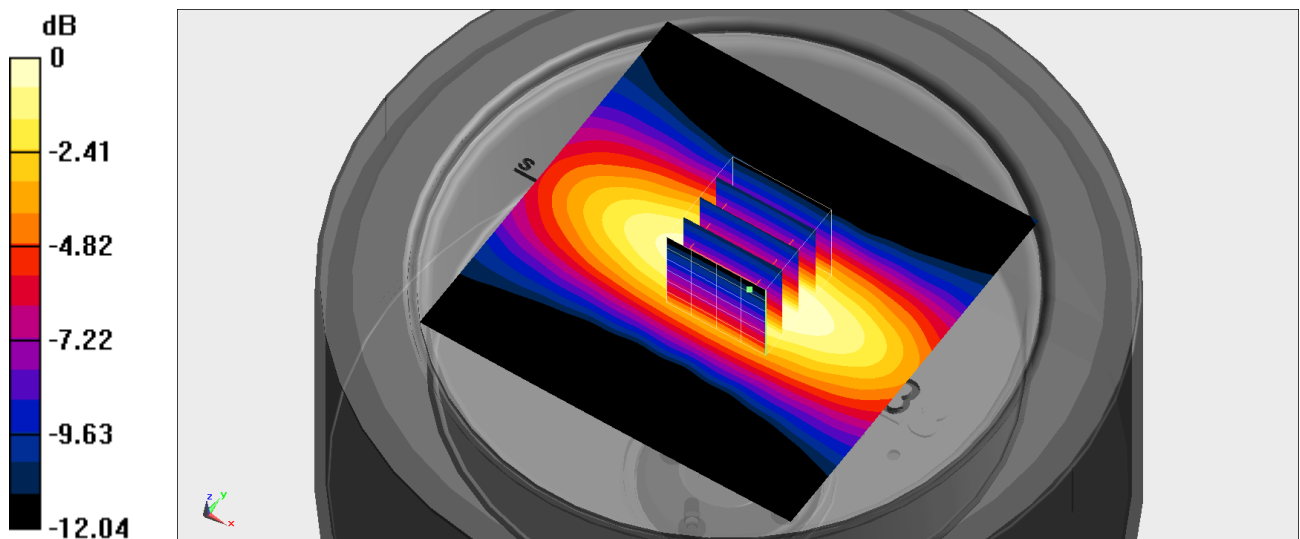

0 dB = 1.10 W/kg = 0.41 dBW/kg

System Check_Head_2450MHz

DUT: D2450V2 - SN736

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL_2450_240306 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 39.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(6.89, 6.89, 7.21); Calibrated: 2023-08-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2023-07-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.44 W/kg; SAR (10g) = 1.12 W/kg;


Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.03 dB

SAR (1g) = 2.46 W/kg; SAR (8g) = 1.27 W/kg; SAR (10g) = 1.15 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.8 %

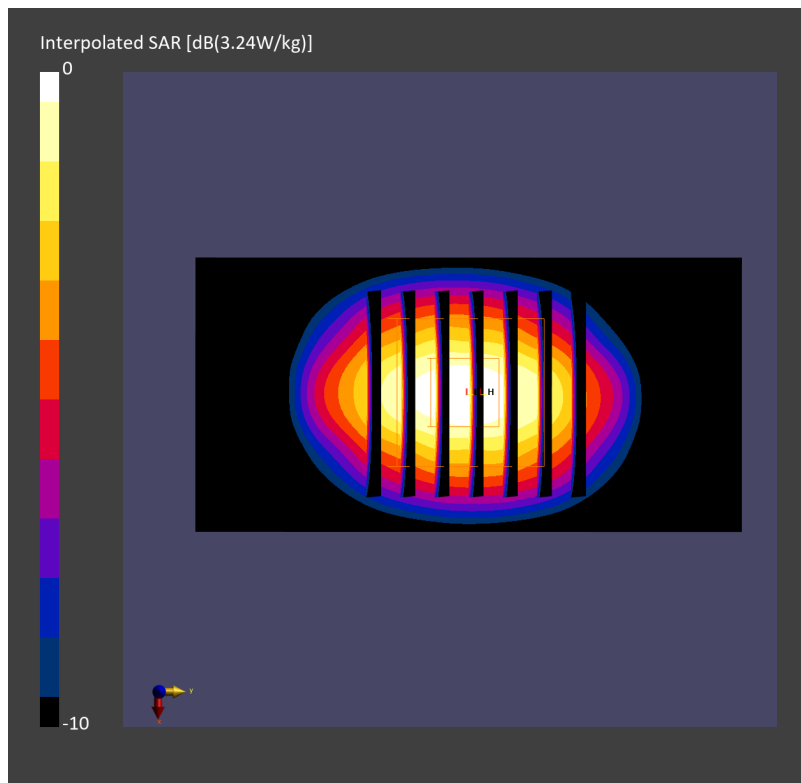

System Check_Head_2450MHz

DUT: D2450V2-736

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL_2450_240315 Medium parameters used: $f = 2450$ MHz; $\sigma = 1.854$ S/m; $\epsilon_r = 39.865$;

$\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(7.92, 7.92, 7.92) @ 2450 MHz; Calibrated: 2023/4/25
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2024/1/22
- Phantom: SAM_Left; Type: QD 000 P40 CD; Serial: TP:1801
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

Pin=50mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 4.42 W/kg

Pin=50mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.79 V/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 5.51 W/kg

SAR(1 g) = 2.67 W/kg; SAR(10 g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 49.1%

Maximum value of SAR (measured) = 4.42 W/kg

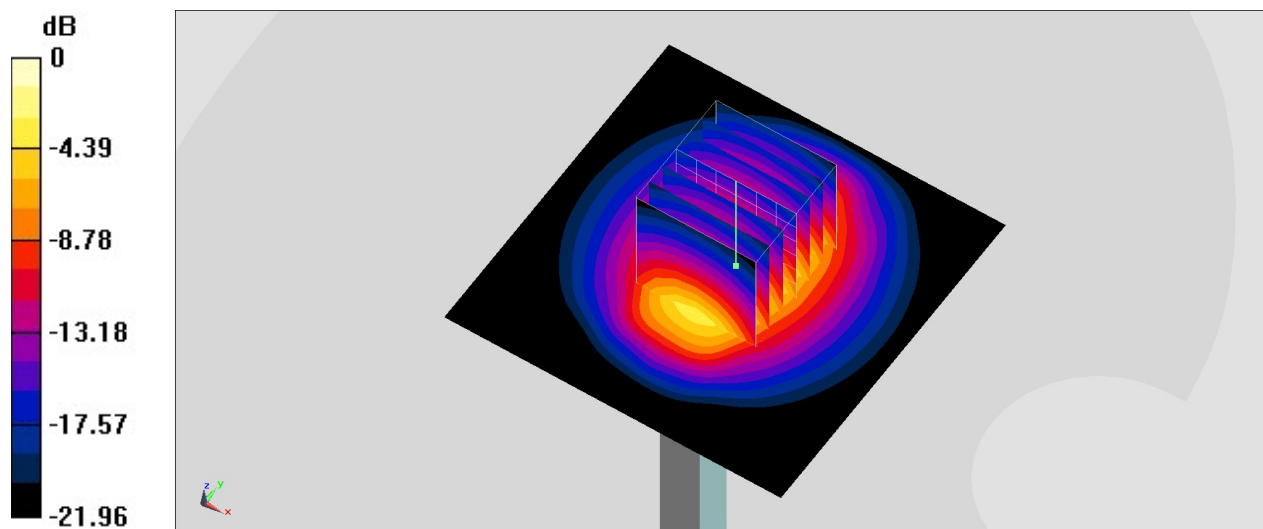

0 dB = 4.42 W/kg = 6.45 dBW/kg

System Check_Head_2450MHz

DUT: D2450V2-929

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL_2450_240319 Medium parameters used: $f = 2450$ MHz; $\sigma = 1.835$ S/m; $\epsilon_r = 39.735$;

$\rho = 1000$ kg/m³

Ambient Temperature : 23.5 °C ; Liquid Temperature : 22.5 °C

DASY5 Configuration:

- Probe: ES3DV3 - SN3169; ConvF(4.56, 4.56, 4.56) @ 2450 MHz; Calibrated: 2023/5/19
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2024/1/22
- Phantom: SAM_Left; Type: QD 000 P40 CD; Serial: TP:1801
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

Pin=250mW/Area Scan (71x71x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm

Maximum value of SAR (interpolated) = 18.1 W/kg

Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 99.71 V/m; Power Drift = 0.07 dB


Peak SAR (extrapolated) = 26.4 W/kg

SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.3 W/kg

Smallest distance from peaks to all points 3 dB below = 9.5 mm

Ratio of SAR at M2 to SAR at M1 = 51.6%

Maximum value of SAR (measured) = 17.5 W/kg

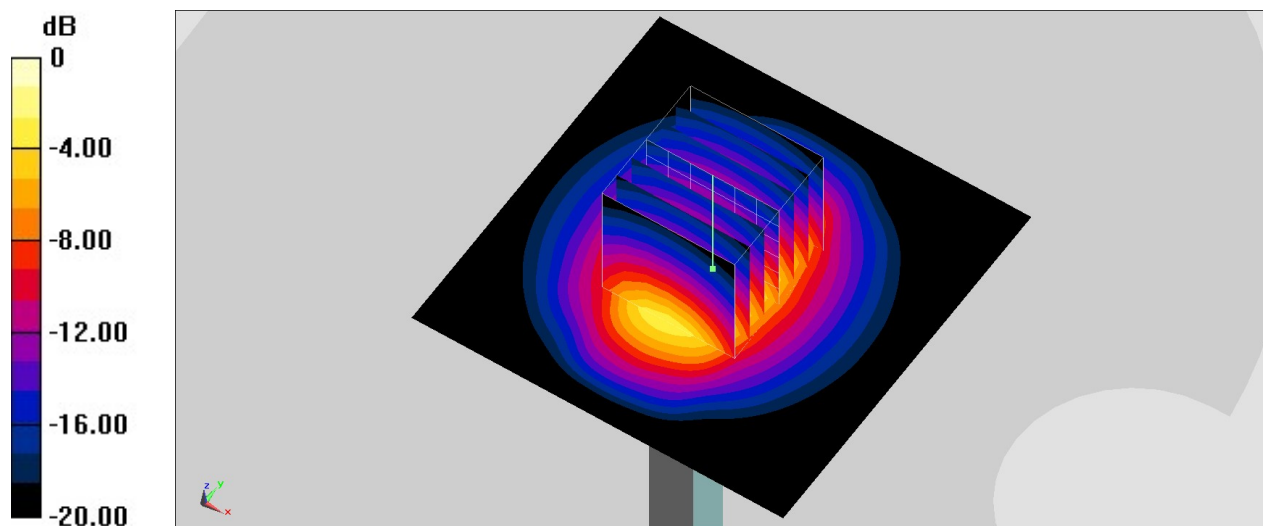

0 dB = 17.5 W/kg = 12.43 dBW/kg

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5250_240307 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.76$ S/m; $\epsilon_r = 36.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(5.38, 5.34, 5.57); Calibrated: 2023-08-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2023-07-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.97 W/kg; SAR (10g) = 1.97 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 7.41 W/kg; SAR (8g) = 2.47 W/kg; SAR (10g) = 2.12 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 64.2 %

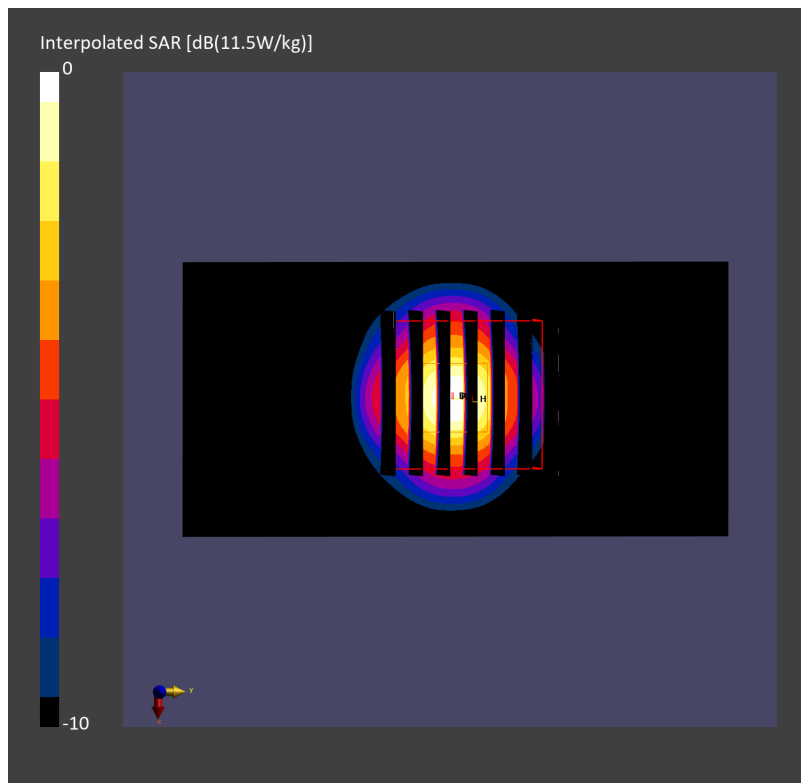

System Check_Head_5250MHz

DUT: D5GHzV2-1006-5250

Communication System: CW; Frequency: 5250 MHz; Duty Cycle: 1:1

Medium: HSL_5G_240313 Medium parameters used: $f = 5250$ MHz; $\sigma = 4.588$ S/m; $\epsilon_r = 35.847$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.2 °C ; Liquid Temperature : 22.2 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(5.64, 5.64, 5.64) @ 5250 MHz; Calibrated: 2023/4/25
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2024/1/22
- Phantom: SAM_Left; Type: QD 000 P40 CD; Serial: TP:1801
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

Pin=100mW/Area Scan (71x71x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm

Maximum value of SAR (interpolated) = 18.7 W/kg

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 71.46 V/m; Power Drift = -0.01 dB


Peak SAR (extrapolated) = 30.3 W/kg

SAR(1 g) = 7.62 W/kg; SAR(10 g) = 2.17 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.3%

Maximum value of SAR (measured) = 19.2 W/kg

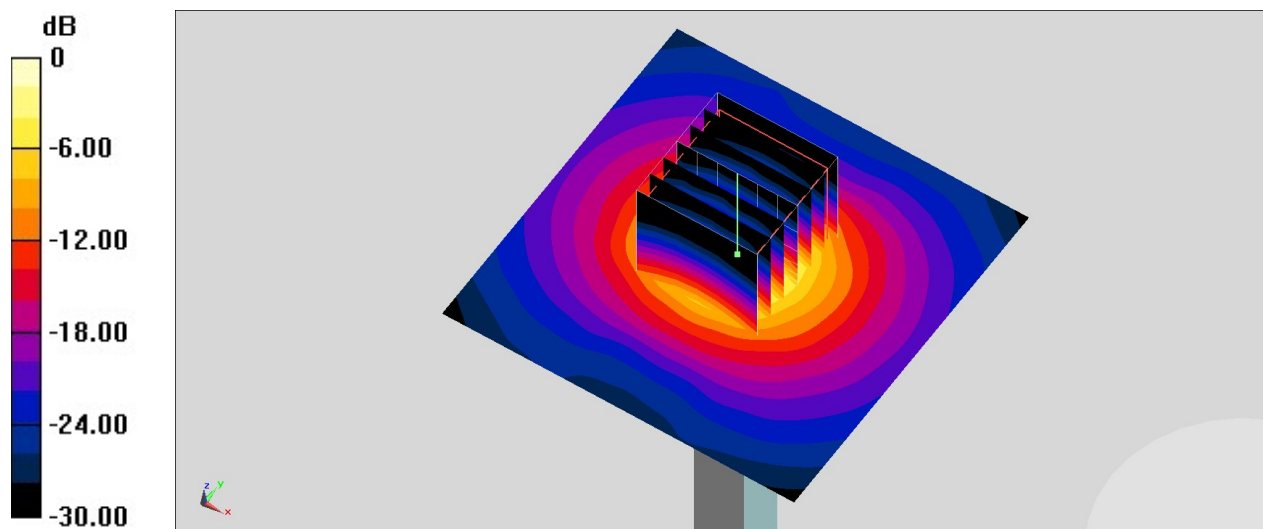

0 dB = 19.2 W/kg = 12.83 dBW/kg

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL_5250_240408 Medium parameters used: $f = 5250.000$ MHz; $\sigma = 4.76$ S/m; $\epsilon_r = 36.6$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(5.38, 5.34, 5.57); Calibrated: 2023-08-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2023-07-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 6.85 W/kg; SAR (10g) = 1.94 W/kg;


Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 7.39 W/kg; SAR (8g) = 2.45 W/kg; SAR (10g) = 2.11 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 64.2 %

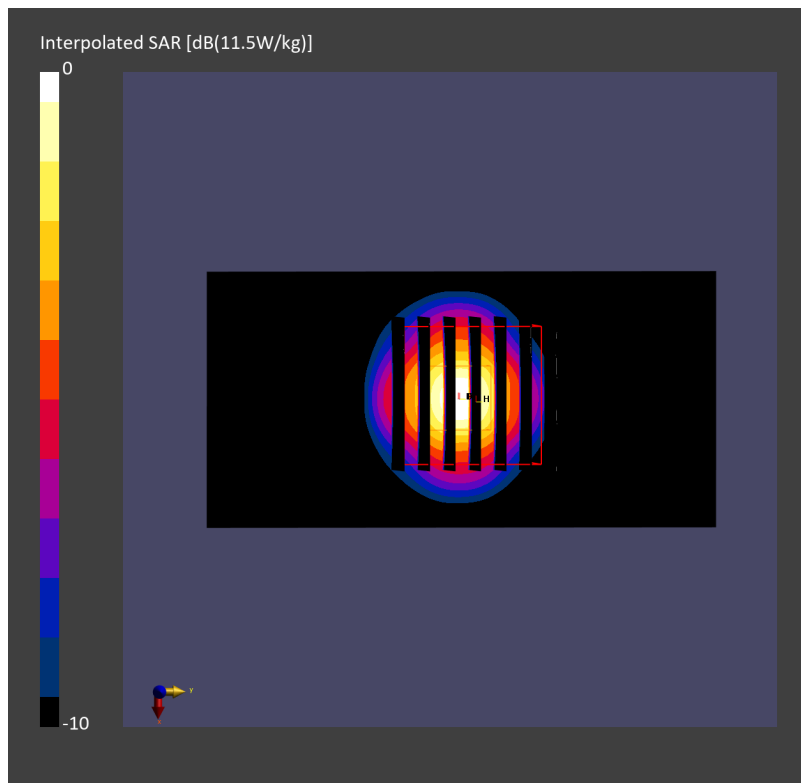

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL_5600_240307 Medium parameters used: $f = 5600.000$ MHz; $\sigma = 5.13$ S/m; $\epsilon_r = 36.1$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(4.59, 4.48, 4.7); Calibrated: 2023-08-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2023-07-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.79 W/kg; SAR (10g) = 1.05 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.93 W/kg; SAR (8g) = 1.29 W/kg; SAR (10g) = 1.10 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62.3 %

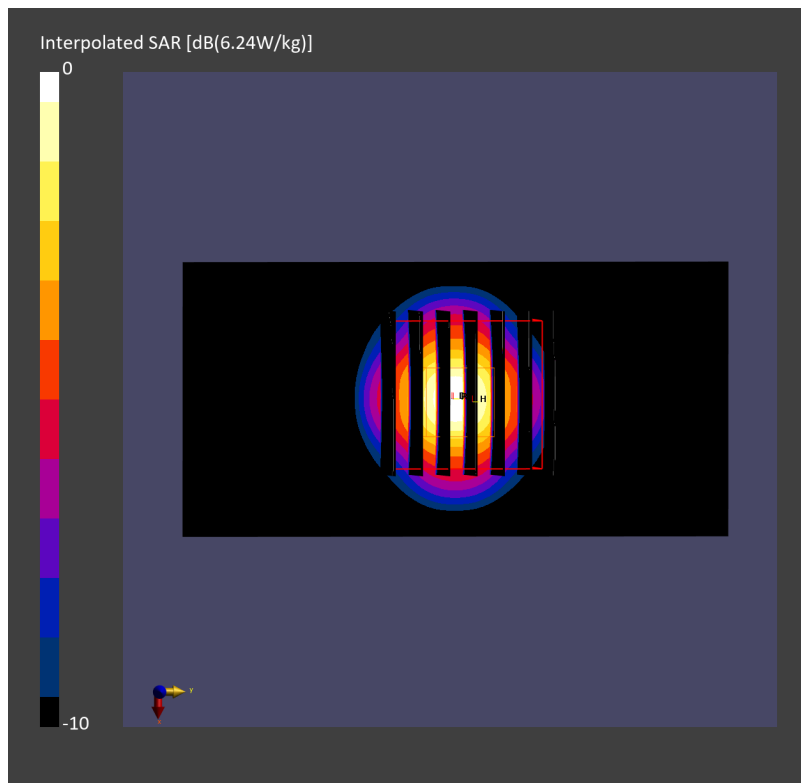

System Check_Head_5600MHz

DUT: D5GHzV2-1006-5600

Communication System: CW; Frequency: 5600 MHz; Duty Cycle: 1:1

Medium: HSL_5G_240313 Medium parameters used: $f = 5600$ MHz; $\sigma = 4.945$ S/m; $\epsilon_r = 35.365$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.2 °C ; Liquid Temperature : 22.2 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(4.95, 4.95, 4.95) @ 5600 MHz; Calibrated: 2023/4/25
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2024/1/22
- Phantom: SAM_Left; Type: QD 000 P40 CD; Serial: TP:1801
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

Pin=100mW/Area Scan (71x71x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm

Maximum value of SAR (interpolated) = 20.7 W/kg

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 73.14 V/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 35.4 W/kg

SAR(1 g) = 8.16 W/kg; SAR(10 g) = 2.33 W/kg

Smallest distance from peaks to all points 3 dB below = 7.5 mm

Ratio of SAR at M2 to SAR at M1 = 62.3%

Maximum value of SAR (measured) = 21.1 W/kg

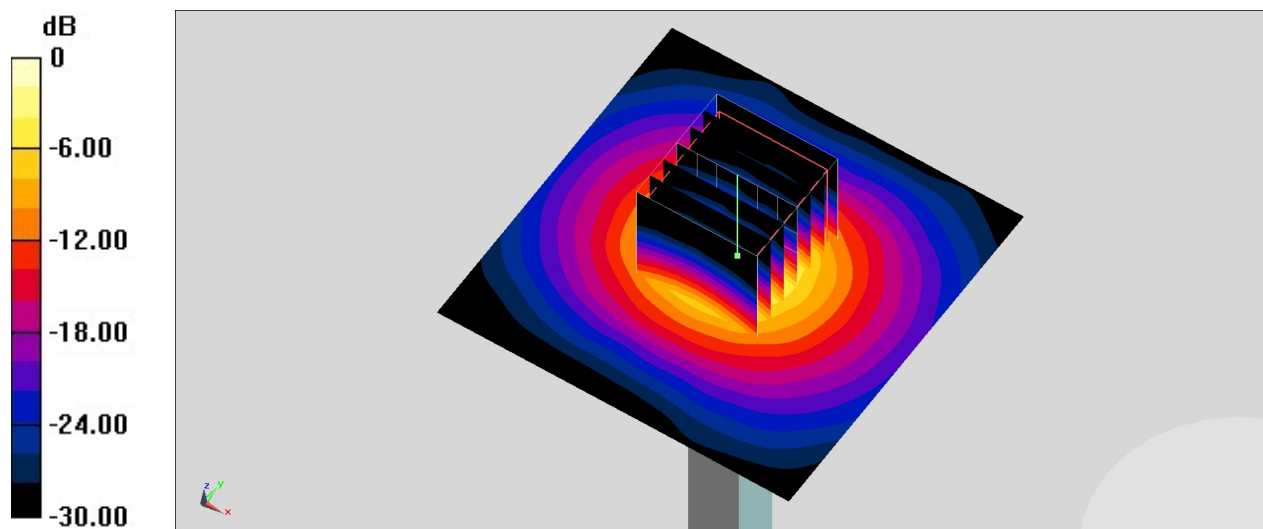

0 dB = 21.1 W/kg = 13.24 dBW/kg

System Check_Head_5750MHz

DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5750.000 MHz

Medium: HSL_5750_240307 Medium parameters used: $f = 5750.000$ MHz; $\sigma = 5.29$ S/m; $\epsilon_r = 35.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(4.68, 4.58, 4.85); Calibrated: 2023-08-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2023-07-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.71 W/kg; SAR (10g) = 1.09 W/kg;


Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.67 W/kg; SAR (8g) = 1.21 W/kg; SAR (10g) = 1.06 W/kg

Smallest distance from peaks to all points 3 dB below = 7.6 mm

Ratio of SAR at M2 to SAR at M1 = 60.4 %

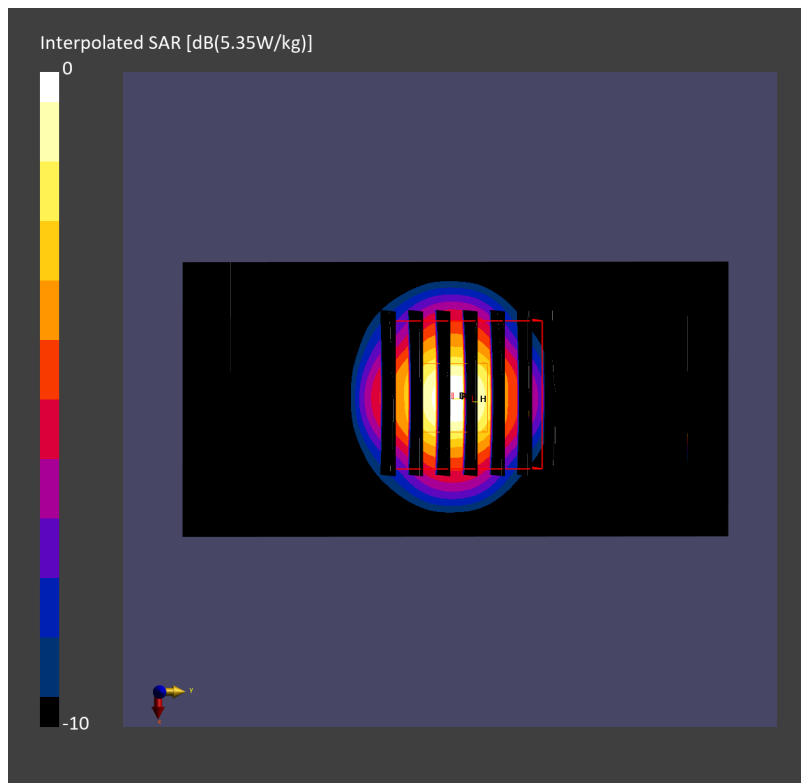

System Check_Head_5750MHz

DUT: D5GHzV2-1006-5750

Communication System: CW; Frequency: 5750 MHz; Duty Cycle: 1:1

Medium: HSL_5G_240313 Medium parameters used: $f = 5750$ MHz; $\sigma = 5.095$ S/m; $\epsilon_r = 35.089$; $\rho = 1000$ kg/m³

Ambient Temperature : 23.2 °C ; Liquid Temperature : 22.2 °C

DASY5 Configuration:

- Probe: EX3DV4 - SN3925; ConvF(5.1, 5.1, 5.1) @ 5750 MHz; Calibrated: 2023/4/25
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2024/1/22
- Phantom: SAM_Left; Type: QD 000 P40 CD; Serial: TP:1801
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7501)

Pin=100mW/Area Scan (71x71x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm

Maximum value of SAR (interpolated) = 19.9 W/kg

Pin=100mW/Zoom Scan (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 69.53 V/m; Power Drift = -0.03 dB


Peak SAR (extrapolated) = 34.9 W/kg

SAR(1 g) = 7.78 W/kg; SAR(10 g) = 2.2 W/kg

Smallest distance from peaks to all points 3 dB below = 7.5 mm

Ratio of SAR at M2 to SAR at M1 = 61.3%

Maximum value of SAR (measured) = 20.3 W/kg

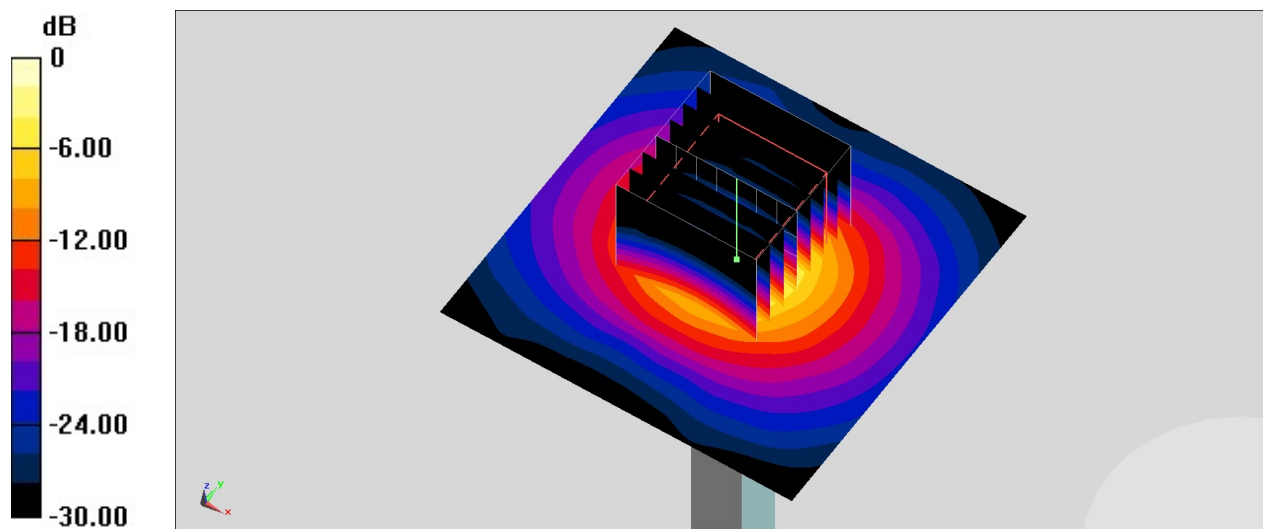

0 dB = 20.3 W/kg = 13.07 dBW/kg

System Check_6500MHz

DUT: D6.5GHzV2 - SN1083

Communication System: CW; Frequency: 6500.000 MHz

Medium: HSL_6500_240308 Medium parameters used: $f = 6500.000$ MHz; $\sigma = 6.18$ S/m; $\epsilon_r = 34.9$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY8 Configuration:

- Probe: EX3DV4 - SN7822; ConvF(5.06, 5.12, 5.2); Calibrated: 2023-08-02
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1823; Calibrated: 2023-07-31
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2149; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 27.9 W/kg; SAR (10g) = 5.45 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm


Power Drift = -0.05 dB

SAR (1g) = 30.6 W/kg; SAR (8g) = 7.01 W/kg; SAR (10g) = 5.73 W/kg

Smallest distance from peaks to all points 3 dB below = 4.9 mm

Ratio of SAR at M2 to SAR at M1 = 51.1 %

psAPD (1.0cm², sq) = 306 [W/m²]; psAPD (4.0cm², sq) = 140 [W/m²]

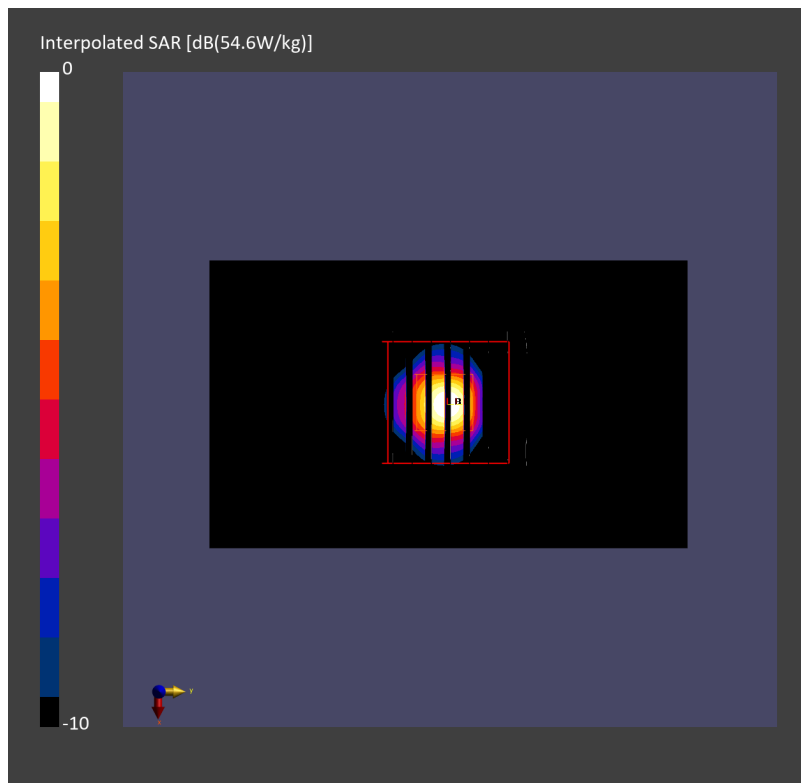

Device Under Test Properties

DUT Type
D2450V2-736

Exposure Conditions

Phantom Section, TSL	Group, UID	Frequency [MHz]	TSL Conductivity [S/m]	TSL Permittivity
Wrist, HSL	CW, 0--	2450.000	1.82	39.0

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
Generic Forearm - 1103	HSL_2450, 2024-03-06	EX3DV4 - SN7822, 2023-08-02	DAE4ip Sn1823, 2023-07-31

Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	x x
Grid Steps [mm]	5.0 x 5.0	x x
Sensor Surface [mm]	2.5	

SAR Pattern

Measurement Results


	FastVolume Scan	Zoom Scan
Date	2024-04-02	
psSAR1g [W/Kg]	14.2	
psSAR10g [W/Kg]	6.19	
Power Drift [dB]	-0.13	

1g IEEE/IEC62704-1 Avg.SAR on surface [dB(14.2W/kg)]

0



-10

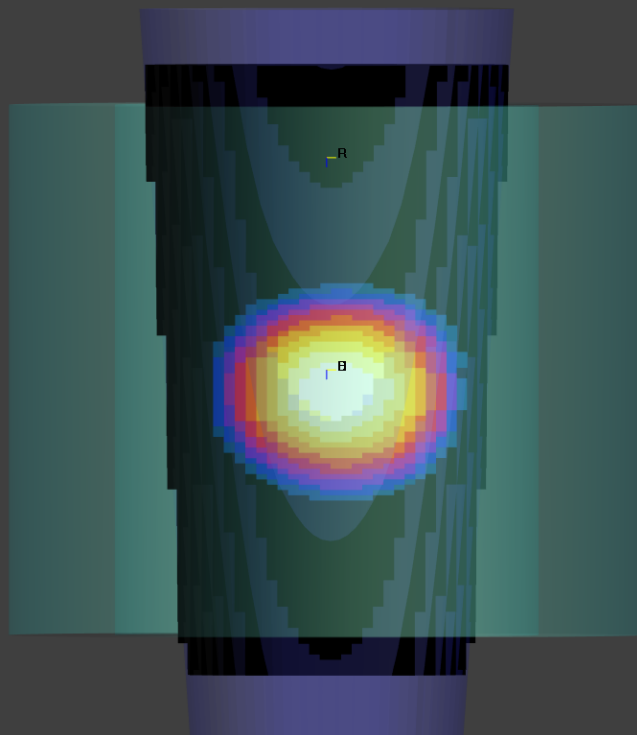

Device Under Test Properties

DUT Type
D2450V2-736

Exposure Conditions

Phantom Section, TSL	Group, UID	Frequency [MHz]	TSL Conductivity [S/m]	TSL Permittivity
Wrist, HSL	CW, 0--	2450.000	1.82	39.0

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
Generic Forearm - 1103	HSL_2450, 2024-03-06	EX3DV4 - SN7822, 2023-08-02	DAE4ip Sn1823, 2023-07-31

Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	x x
Grid Steps [mm]	5.0 x 5.0	x x
Sensor Surface [mm]	2.5	

SAR Pattern

Measurement Results


	FastVolume Scan	Zoom Scan
Date	2024-04-02	
psSAR1g [W/Kg]	16.3	
psSAR10g [W/Kg]	7.60	
Power Drift [dB]	0.03	

1g IEEE/IEC62704-1 Avg.SAR on surface [dB(16.3W/kg)]

0



-10

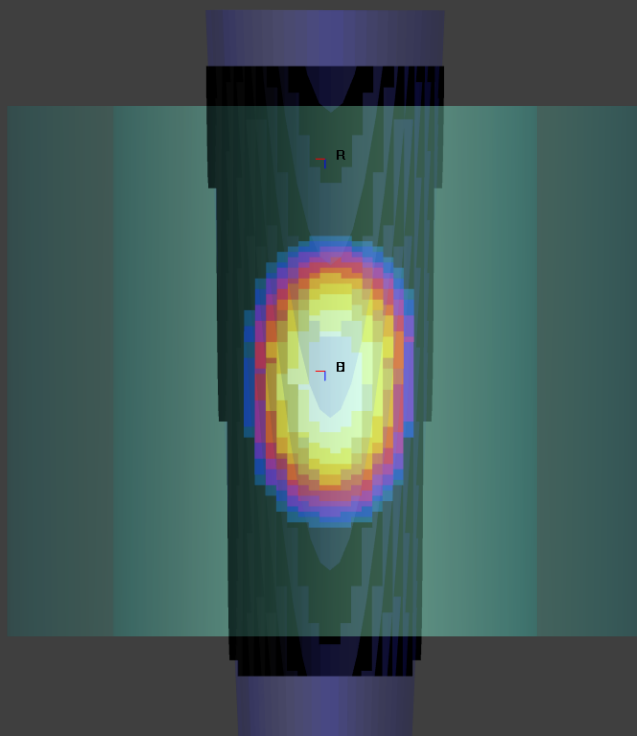

Device Under Test Properties

DUT Type
D2450V2-736

Exposure Conditions

Phantom Section, TSL	Group, UID	Frequency [MHz]	TSL Conductivity [S/m]	TSL Permittivity
Wrist, HSL	CW, 0--	2450.000	1.82	39.0

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
Generic Forearm - 1103	HSL_2450, 2024-03-06	EX3DV4 - SN7822, 2023-08-02	DAE4ip Sn1823, 2023-07-31

Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	80.0 x 80.0	x x
Grid Steps [mm]	5.0 x 5.0	x x
Sensor Surface [mm]	2.5	

SAR Pattern

Measurement Results


	FastVolume Scan	Zoom Scan
Date	2024-04-02	
psSAR1g [W/Kg]	10.2	
psSAR10g [W/Kg]	4.63	
Power Drift [dB]	0.08	

1g IEEE/IEC62704-1 Avg.SAR on surface [dB(10.2W/kg)]

0



-10

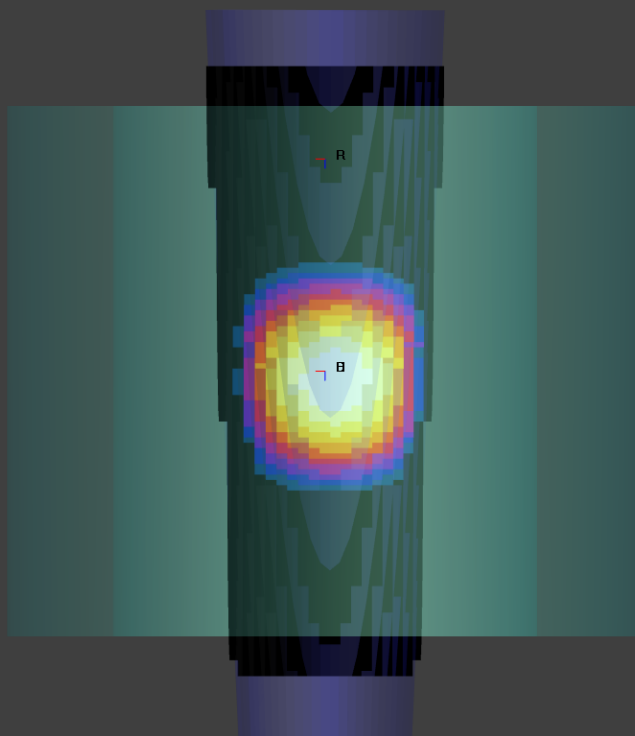

Device Under Test Properties

DUT Type
D5GHzV2-1006

Exposure Conditions

Phantom Section, TSL	Group, UID	Frequency [MHz]	TSL Conductivity [S/m]	TSL Permittivity
Wrist, HSL	CW, 0--	5800.000	5.34	35.8

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
Generic Forearm - 1103	HSL_5G, 2024-03-07	EX3DV4 - SN7822, 2023-08-02	DAE4ip Sn1823, 2023-07-31

Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	100.0 x 100.0	x x
Grid Steps [mm]	5.0 x 5.0	x x
Sensor Surface [mm]	2.5	

SAR Pattern

Measurement Results


	FastVolume Scan	Zoom Scan
Date	2024-04-01	
psSAR1g [W/Kg]	7.65	
psSAR10g [W/Kg]	2.11	
Power Drift [dB]	0.1	

1g IEEE/IEC62704-1 Avg.SAR on surface [dB(7.65W/kg)]

0



-10

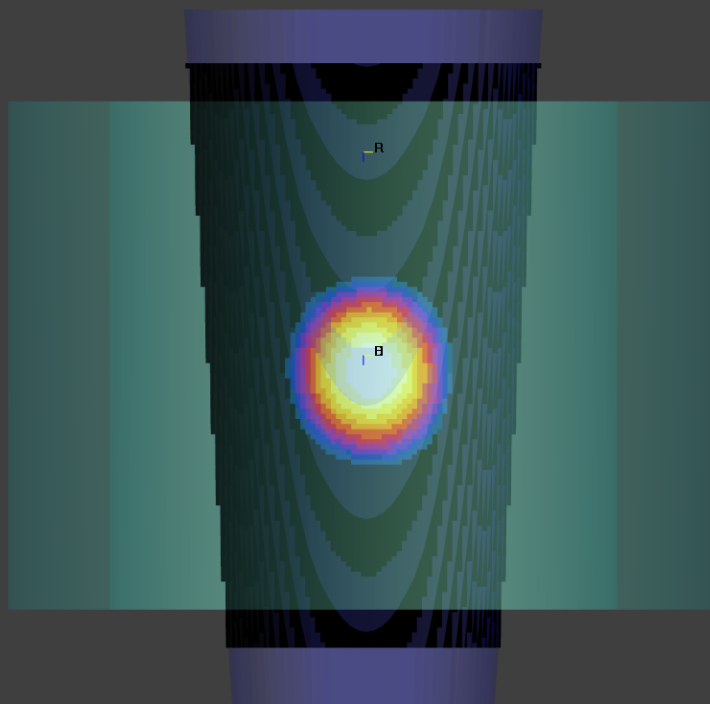

Device Under Test Properties

DUT Type
D6.5GHzV2-1083

Exposure Conditions

Phantom Section, TSL	Group, UID	Frequency [MHz]	TSL Conductivity [S/m]	TSL Permittivity
Wrist, HSL	CW, 0--	6500.000	6.18	34.9

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
Generic Forearm - 1103	HSL_6G, 2024-03-08	EX3DV4 - SN7822, 2023-08-02	DAE4ip Sn1823, 2023-07-31

Scans Setup

	FastVolume Scan	Zoom Scan
Grid Extents [mm]	100.0 x 100.0	x x
Grid Steps [mm]	4.0 x 4.0	x x
Sensor Surface [mm]	2.5	

SAR Pattern

Measurement Results

	FastVolume Scan	Zoom Scan
Date	2024-04-01	
psSAR1g [W/Kg]	27.1	
psSAR10g [W/Kg]	4.82	
Power Drift [dB]	-0.11	

1g IEEE/IEC62704-1 Avg.SAR on surface [dB(27.1W/kg)]

0



-10

