




CP-OFDM Module B

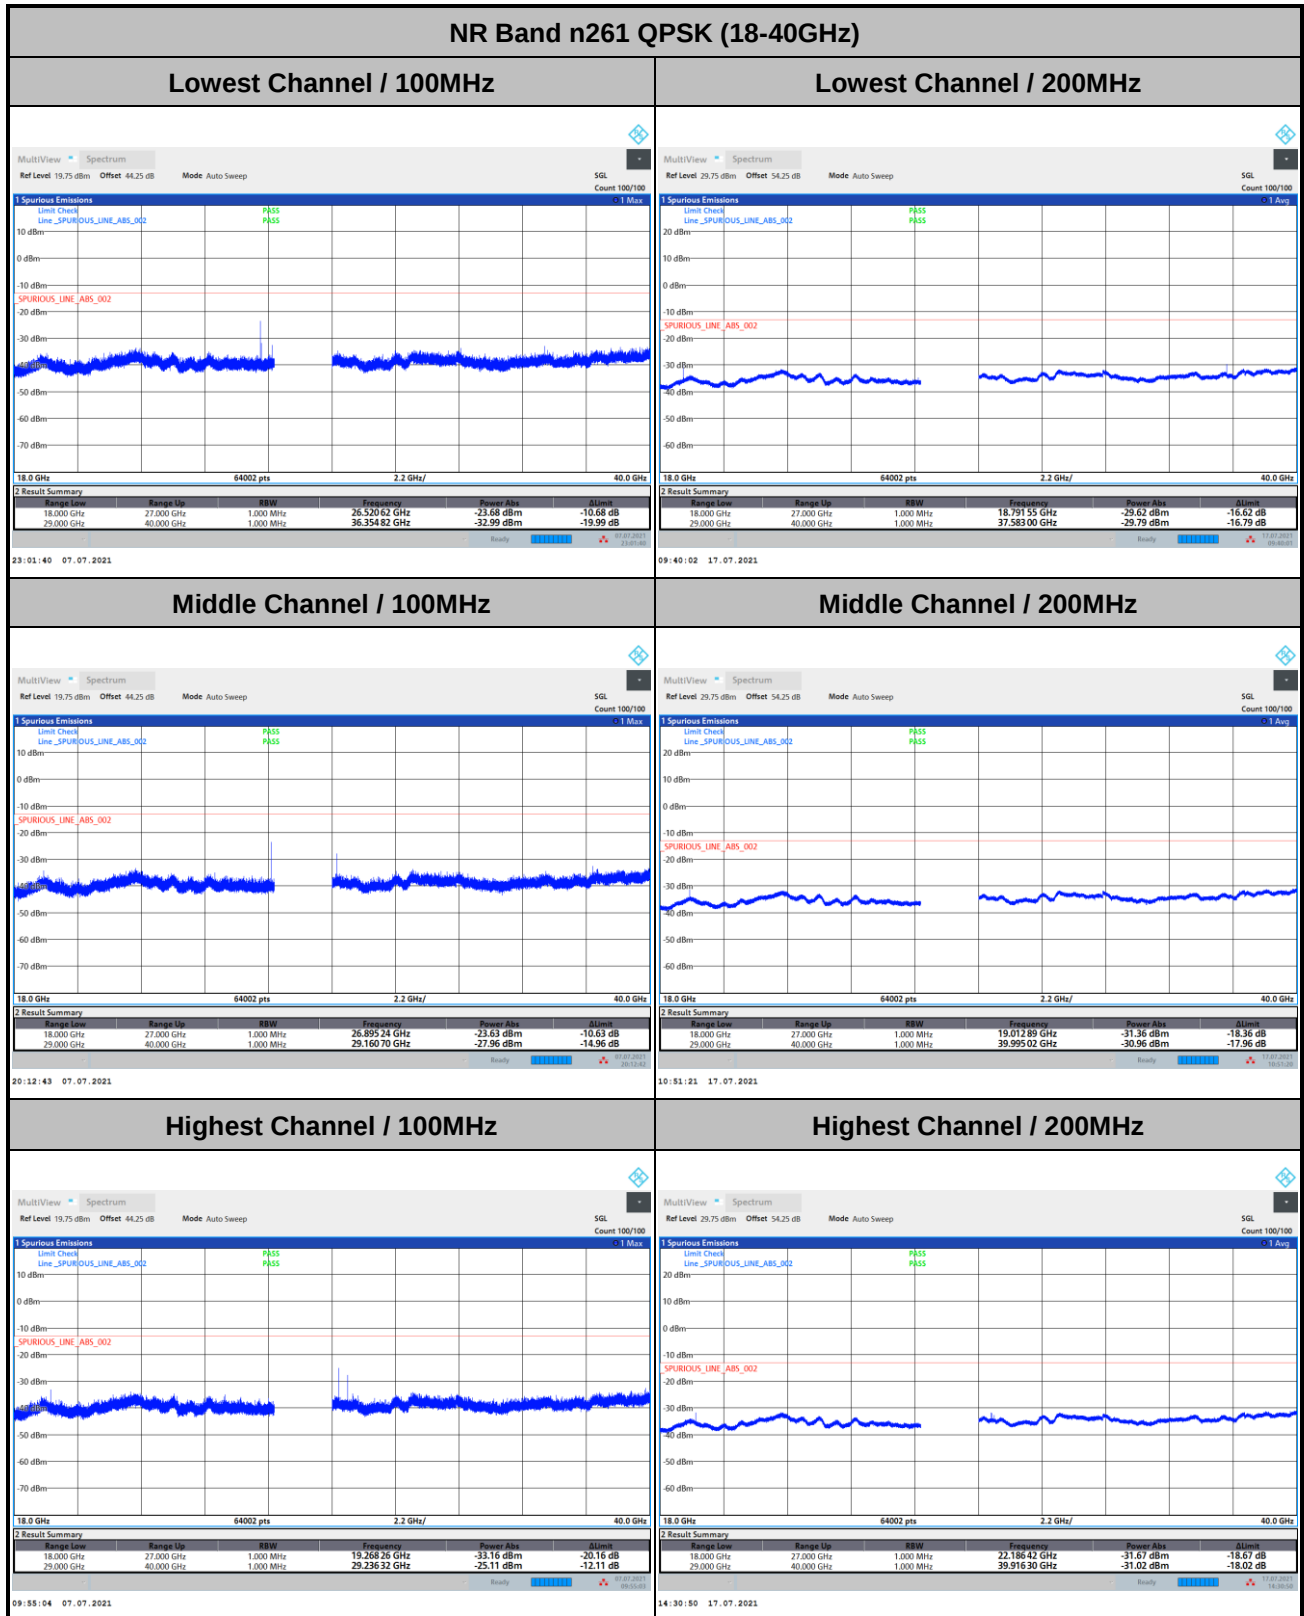

Remark: In band and out of band frequencies that has reported in previous results are omitted.

NR Band n261 Module B Beam H+V

Occupied Bandwidth

Mode	DFT-s-OFDM Module B NR Band n261 : 99%OBW(MHz)					
BW	100MHz			200MHz		
Mod.	QPSK	16QAM	64QAM	QPSK	16QAM	64QAM
Lowest CH	92.34	91.85	91.47	190.69	190.68	190.19
Middle CH	92.62	92.18	91.73	190.64	190.66	190.61
Highest CH	92.18	91.77	91.41	190.82	190.21	190.03


Mode	CP-OFDM Module B NR Band n261 : 99%OBW(MHz)	
BW	100MHz	200MHz
Mod.	QPSK	QPSK
Lowest CH	95.45	194.08
Middle CH	96.03	193.59
Highest CH	95.01	193.76




DFT-s-OFDM Module B

NR Band n261


Lowest Channel / 100MHz / QPSK

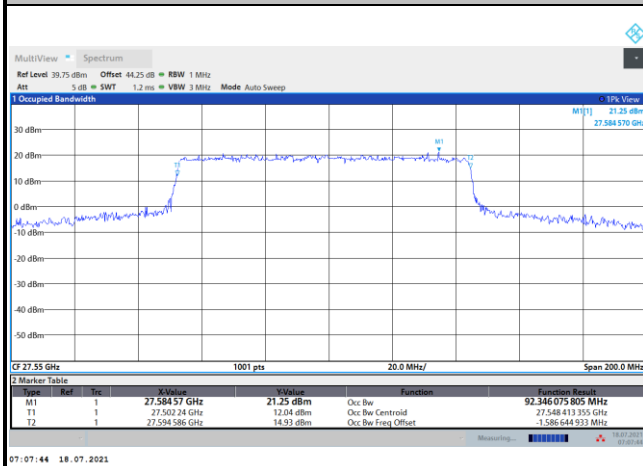


Lowest Channel / 100MHz / 16QAM

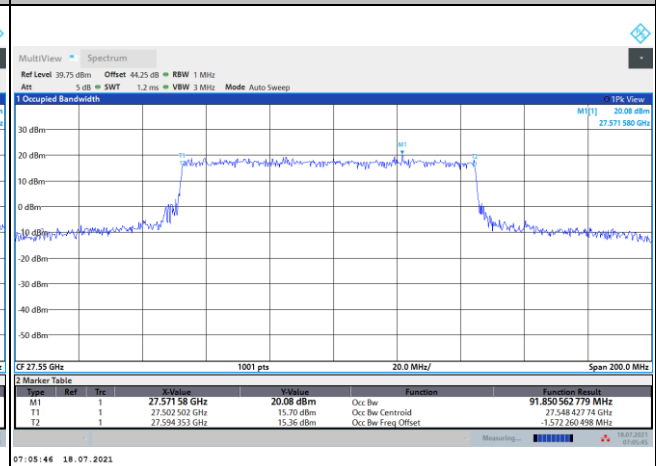


Middle Channel / 100MHz / QPSK

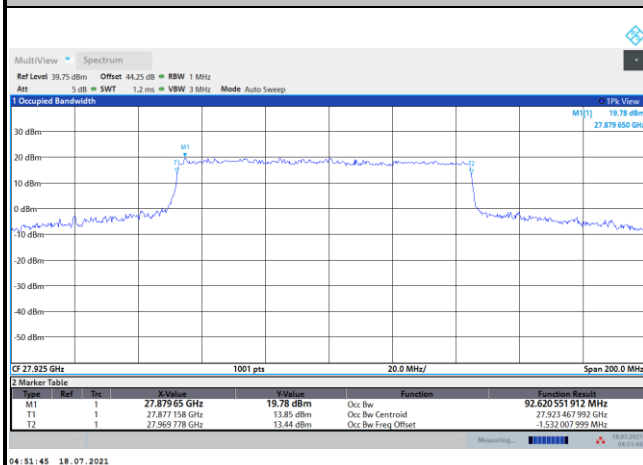


Middle Channel / 100MHz / 16QAM

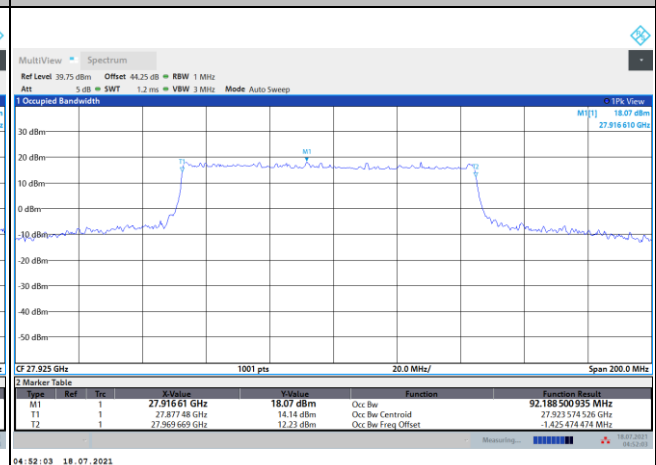

Highest Channel / 100MHz / QPSK

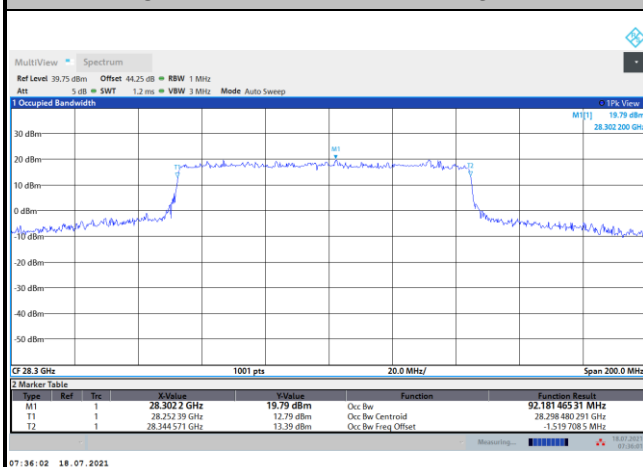

Highest Channel / 100MHz / 16QAM

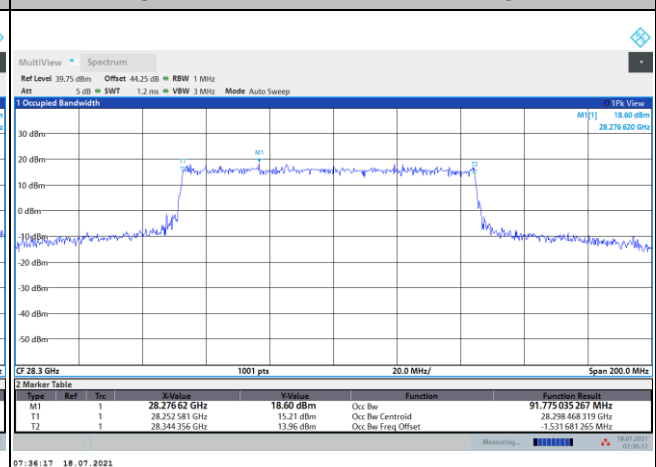





DFT-s-OFDM Module B

NR Band n261


Lowest Channel / 100MHz / 64QAM

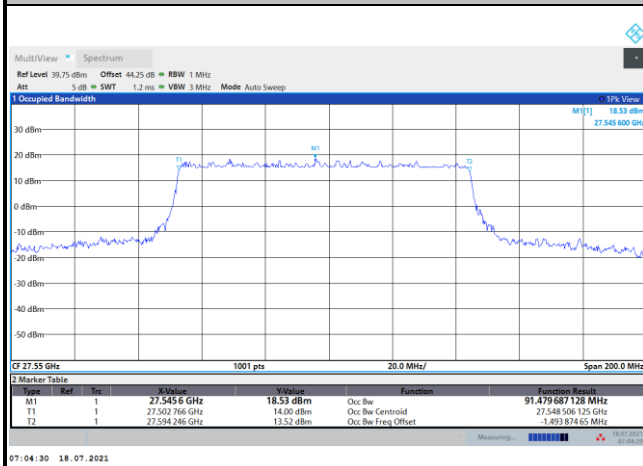

Lowest Channel / 200MHz / QPSK

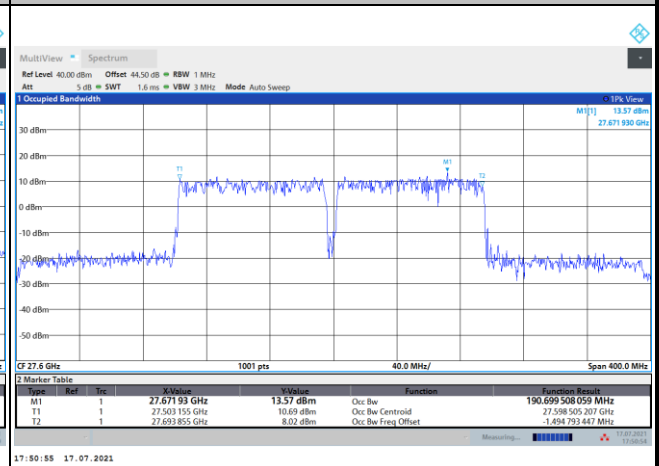


Middle Channel / 100MHz / 64QAM

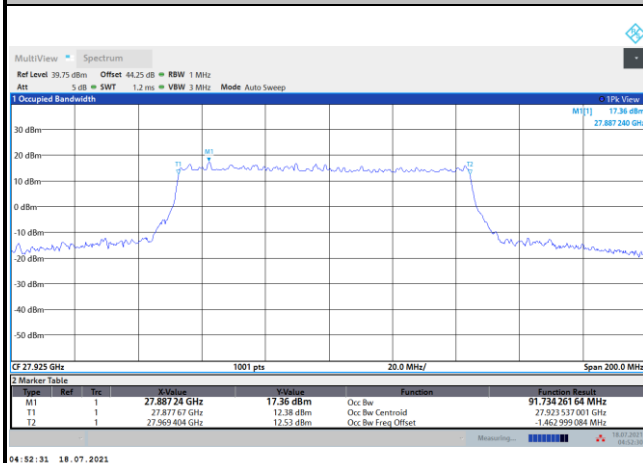


Middle Channel / 200MHz / QPSK



Highest Channel / 100MHz / 64QAM

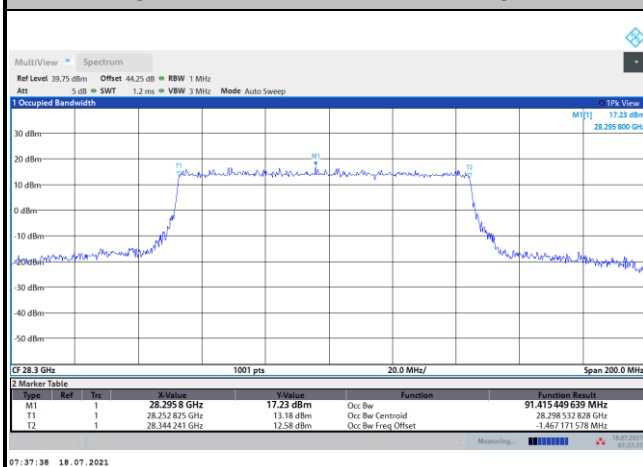

Highest Channel / 200MHz / QPSK

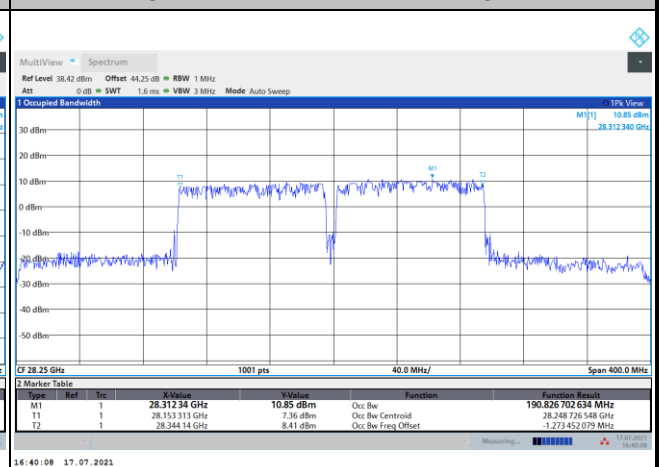





DFT-s-OFDM Module B

NR Band n261


Lowest Channel / 200MHz / 16QAM

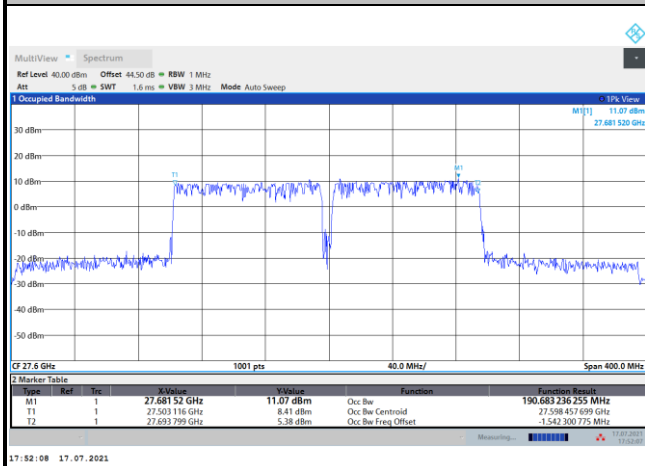


Lowest Channel / 200MHz / 64QAM

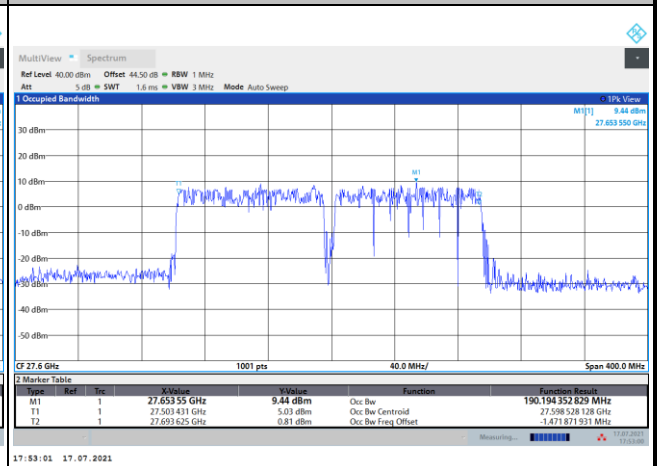


Middle Channel / 200MHz / 16QAM

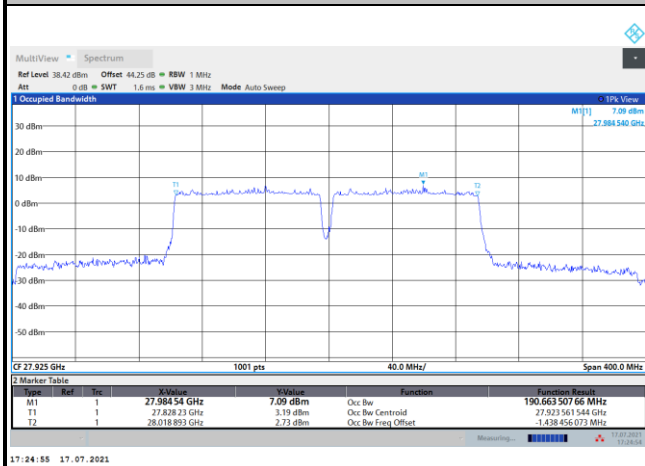


Middle Channel / 200MHz / 64QAM

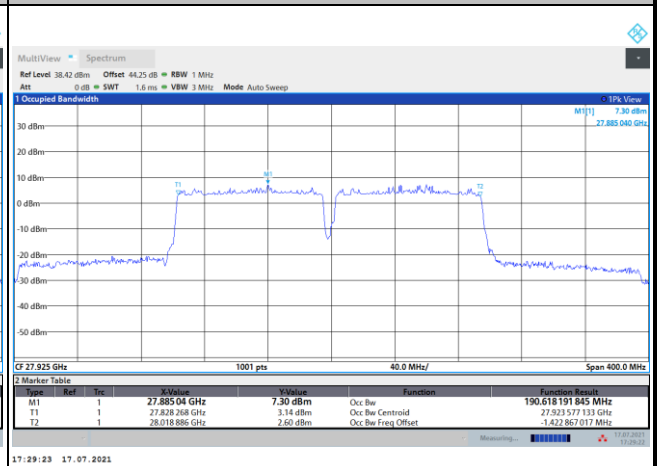

Highest Channel / 200MHz / 16QAM

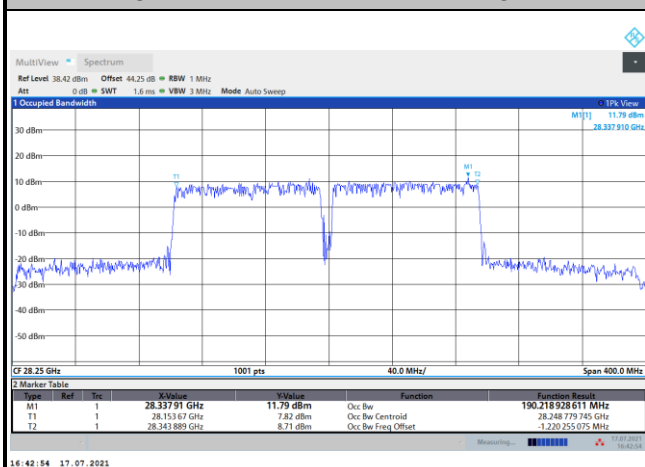

Highest Channel / 200MHz / 64QAM

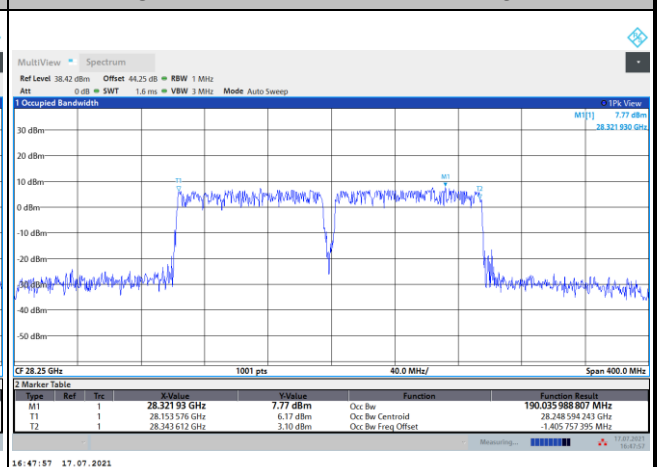





CP-OFDM Module B

NR Band n261


Lowest Channel / 100MHz / QPSK

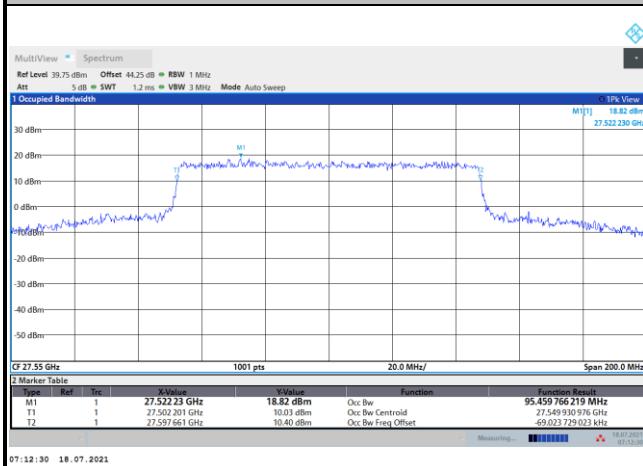


Lowest Channel / 200MHz / QPSK

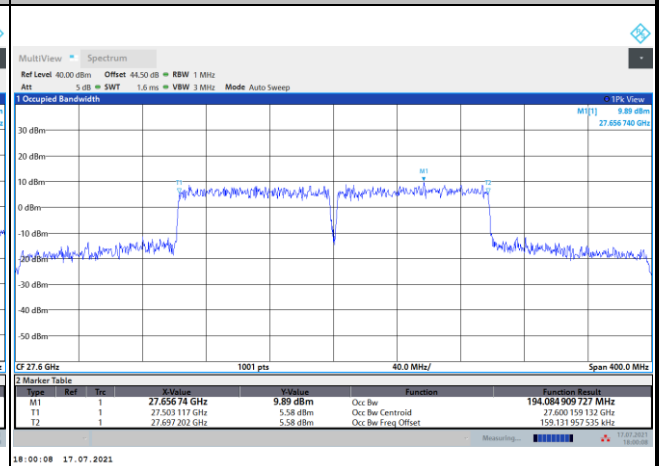


Middle Channel / 100MHz / QPSK

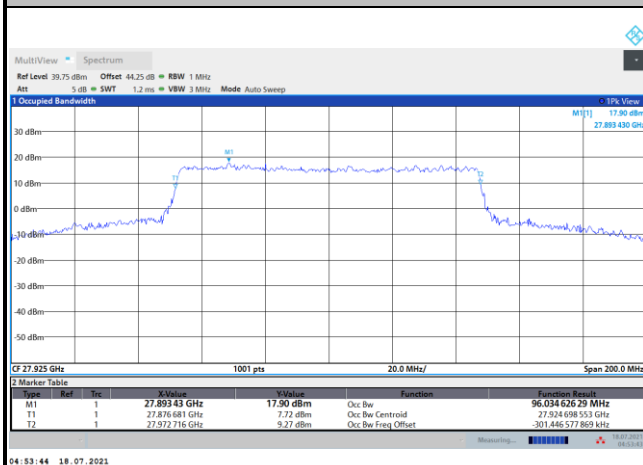


Middle Channel / 200MHz / QPSK

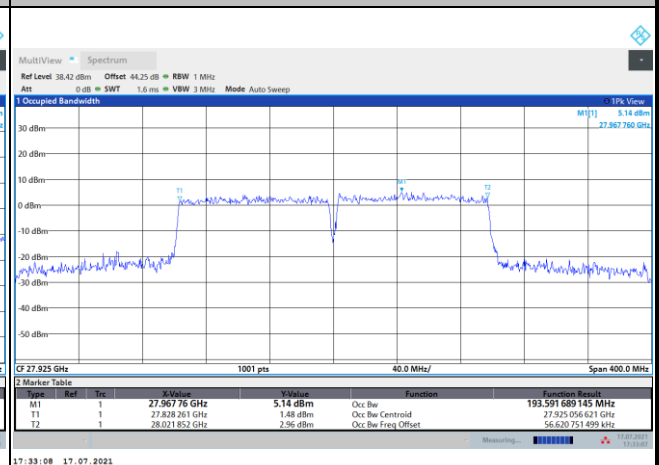

Highest Channel / 100MHz / QPSK

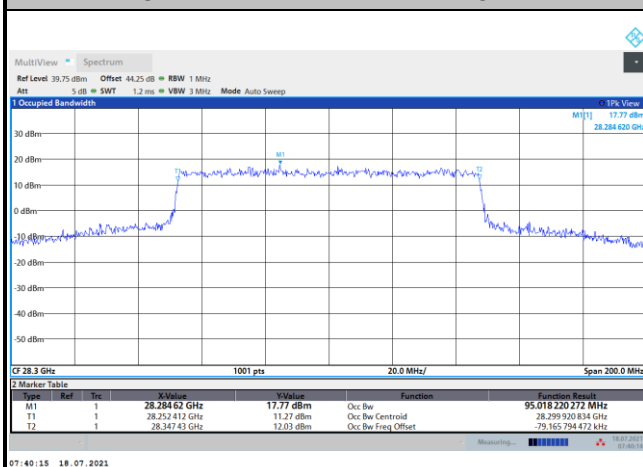

Highest Channel / 200MHz / QPSK

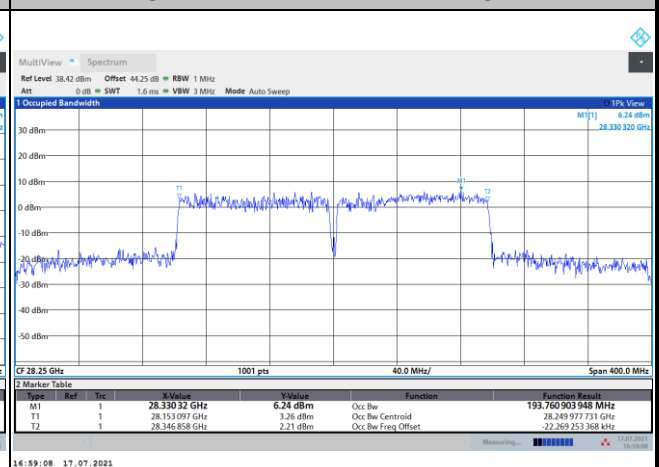

Radiated Out of Band Emissions

Mode			DFT-s-OFDM Module B NR Band n261 : BE (dBm) 1 RB					
BW			100MHz			200MHz		
Limit (dBm)			QPSK	16QAM	64QAM	QPSK	16QAM	64QAM
Low CH	0~10%OB	≤ -5	-19.49	-22.13	-6.20	-12.23	-13.21	-16.27
	>10%OB	≤ -13	-31.56	-31.70	-28.02	-14.31	-16.08	-17.86
High CH	0~10%OB	≤ -5	-18.81	-8.54	-8.88	-14.63	-15.99	-25.40
	>10%OB	≤ -13	-30.36	-34.49	-34.88	-16.76	-16.92	-19.00
Result			Compliance					

Mode			CP-OFDM Module B NR Band n261 : BE (dBm) 1 RB		
BW			100MHz		200MHz
Limit (dBm)			QPSK		QPSK
Low CH	0~10%OB	≤ -5	-20.08		-12.02
	>10%OB	≤ -13	-31.85		-15.51
High CH	0~10%OB	≤ -5	-7.83		-21.49
	>10%OB	≤ -13	-33.20		-16.80
Result			Compliance		

Mode			DFT-s-OFDM Module B NR Band n261 : BE (dBm) Full RB					
BW			100MHz			200MHz		
Limit (dBm)			QPSK	16QAM	64QAM	QPSK	16QAM	64QAM
Low CH	0~10%OB	≤ -5	-21.37	-11.20	-16.65	-18.10	-19.95	-26.27
	>10%OB	≤ -13	-21.31	-14.12	-21.79	-22.51	-25.51	-29.09
High CH	0~10%OB	≤ -5	-21.42	-15.53	-21.70	-22.29	-24.69	-26.98
	>10%OB	≤ -13	-20.92	-17.23	-25.32	-24.27	-27.81	-30.91
Result			Compliance					

Mode			CP-OFDM Module B NR Band n261 : BE (dBm) Full RB		
BW			100MHz		200MHz
Limit (dBm)			QPSK		QPSK
Low CH	0~10%OB	≤ -5	-26.00		-18.20
	>10%OB	≤ -13	-24.84		-20.24
High CH	0~10%OB	≤ -5	-12.09		-21.00
	>10%OB	≤ -13	-15.37		-23.60
Result			Compliance		





DFT-s-OFDM Module B

NR Band n261 / 100MHz / QPSK

Lowest Band Edge / 1 RB



Highest Band Edge / 1 RB

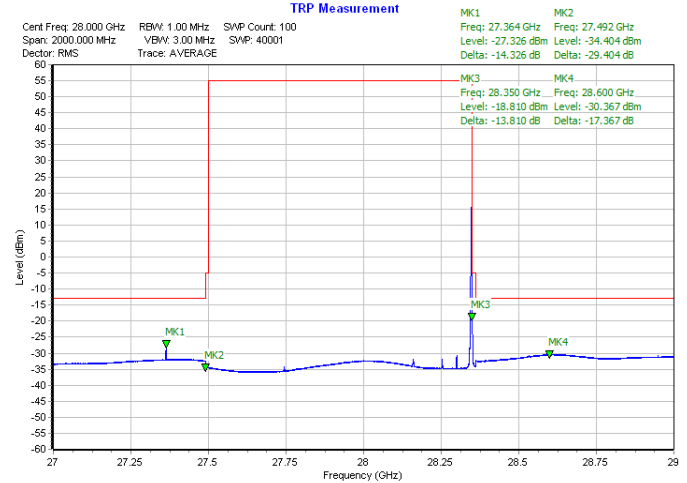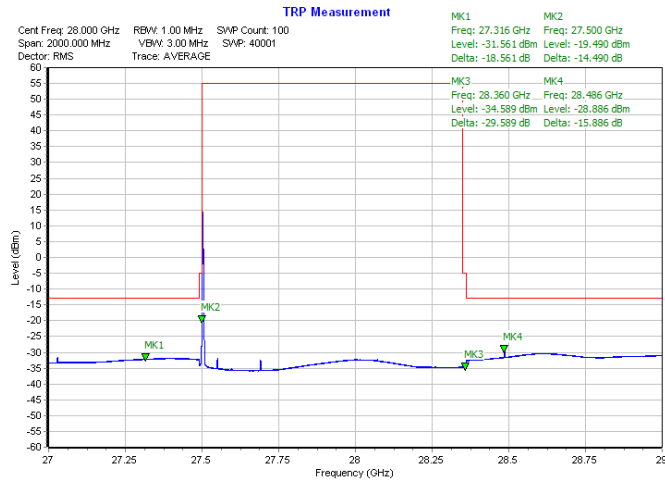

NR Band n261 / 100MHz / 16QAM

Lowest Band Edge / 1 RB

Highest Band Edge / 1 RB

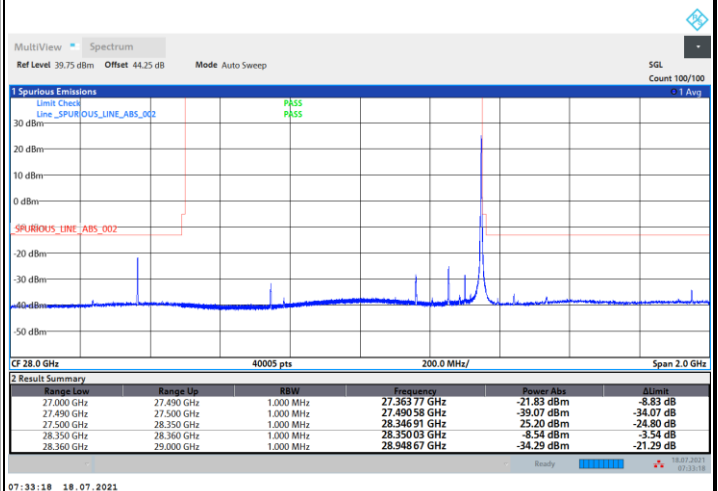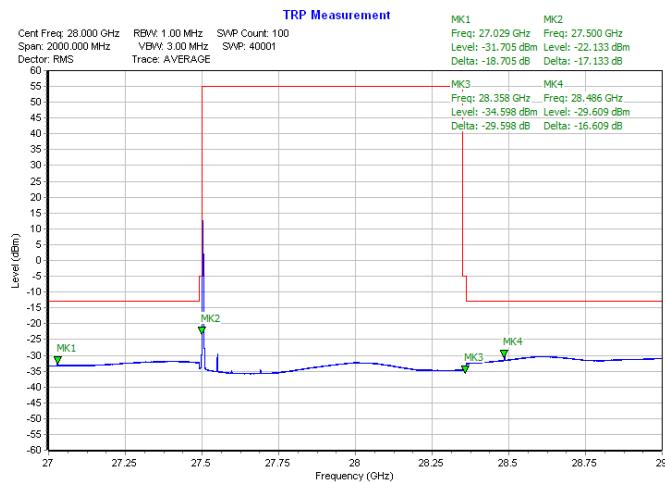





DFT-s-OFDM Module B

NR Band n261 / 100MHz / 64QAM

Lowest Band Edge / 1 RB

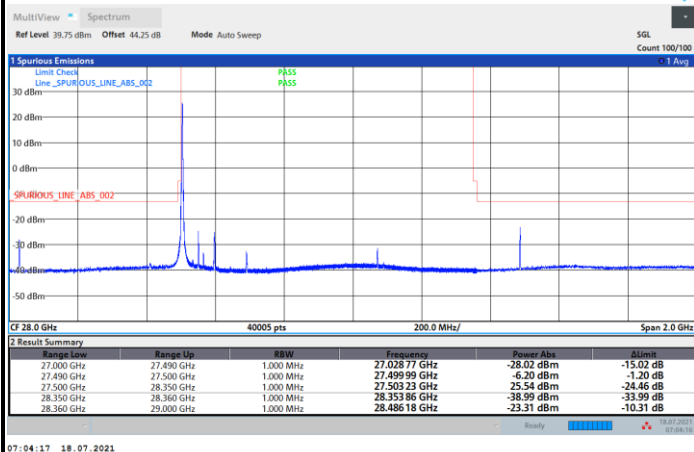


Highest Band Edge / 1 RB

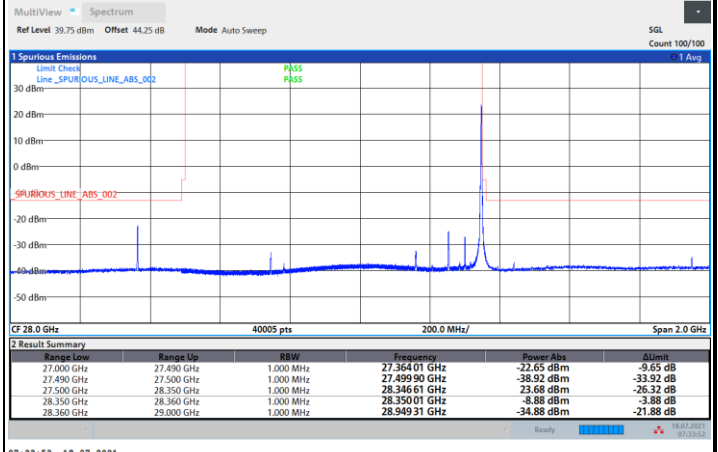


NR Band n261 / 200MHz / QPSK

Lowest Band Edge / 1 RB

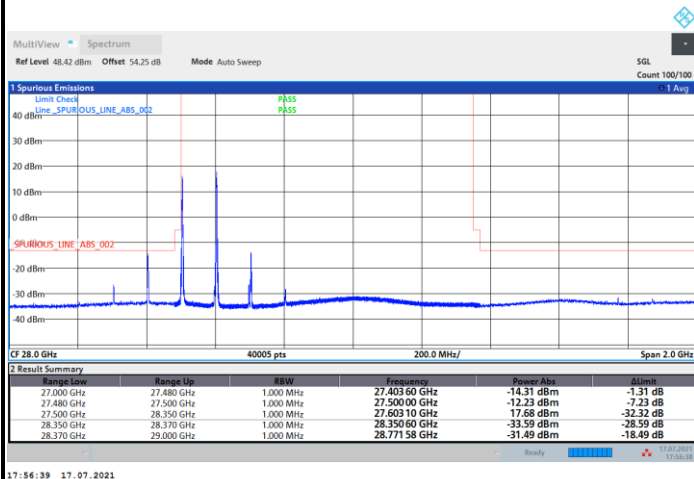

Highest Band Edge / 1 RB

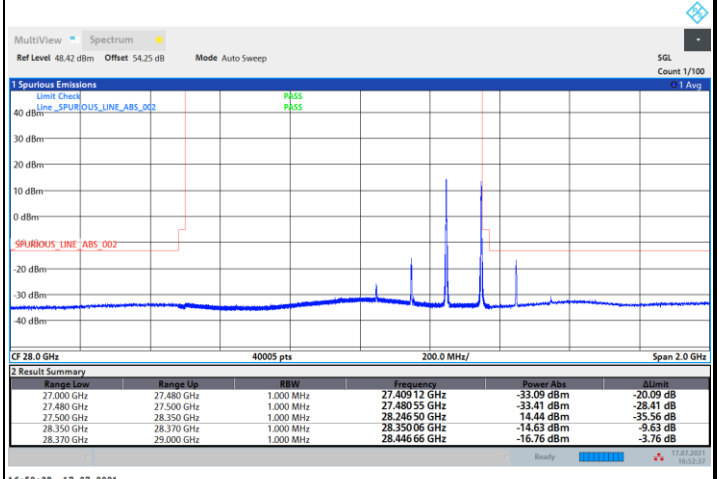





DFT-s-OFDM Module B

NR Band n261 / 200MHz / 16QAM

Lowest Band Edge / 1 RB

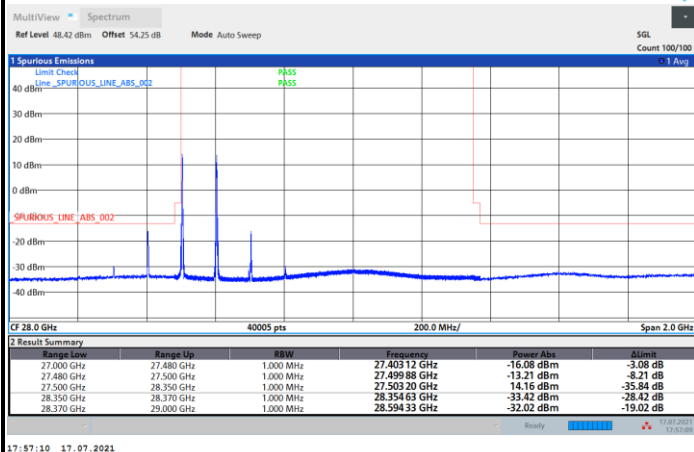


Highest Band Edge / 1 RB

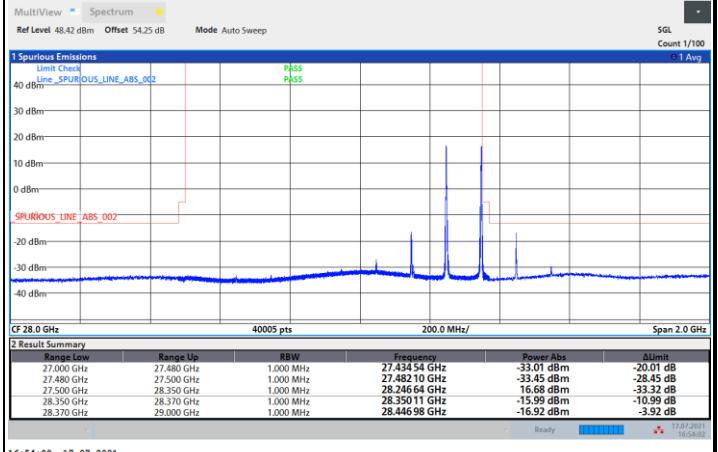


NR Band n261 / 200MHz / 64QAM

Lowest Band Edge / 1 RB

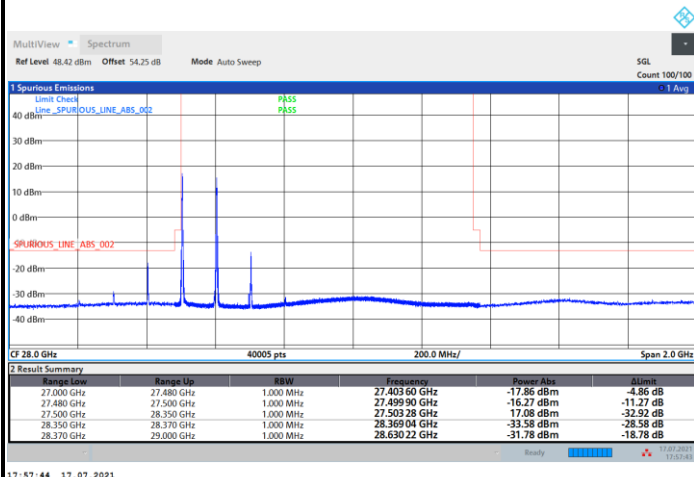

Highest Band Edge / 1 RB

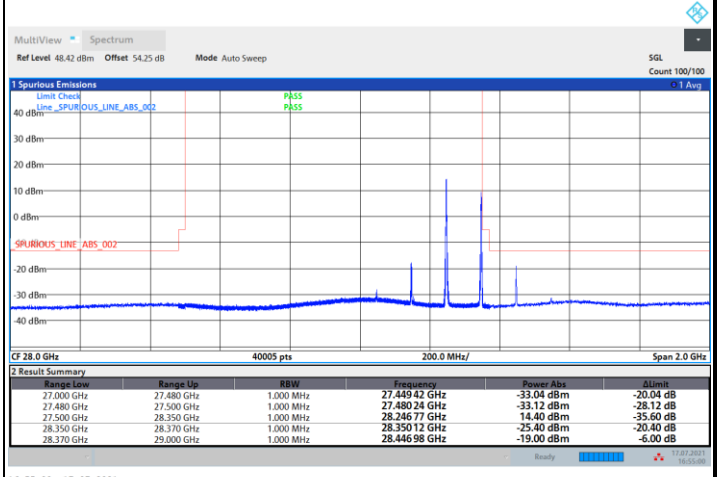





CP-OFDM Module B

NR Band n261 / 100MHz / QPSK

Lowest Band Edge / 1 RB



Highest Band Edge / 1 RB

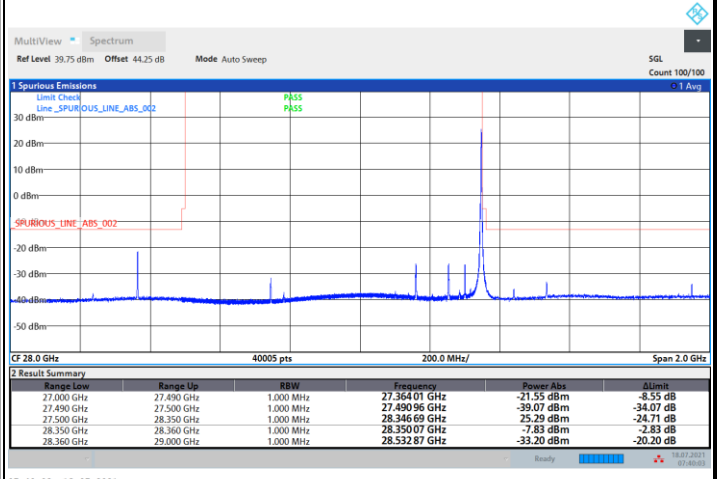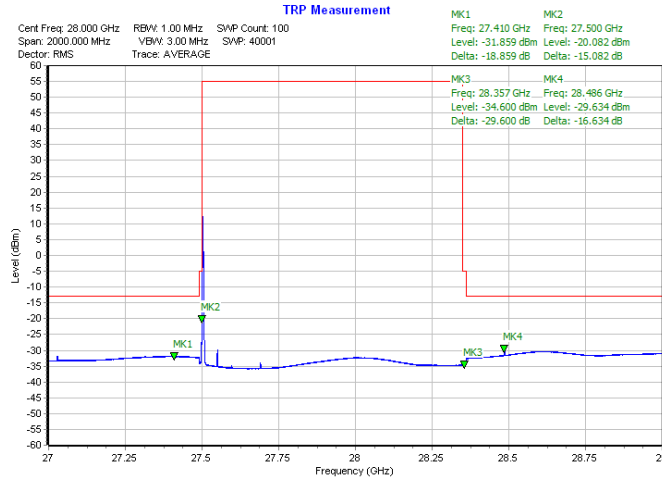

NR Band n261 / 200MHz / QPSK

Lowest Band Edge / 1 RB

Highest Band Edge / 1 RB

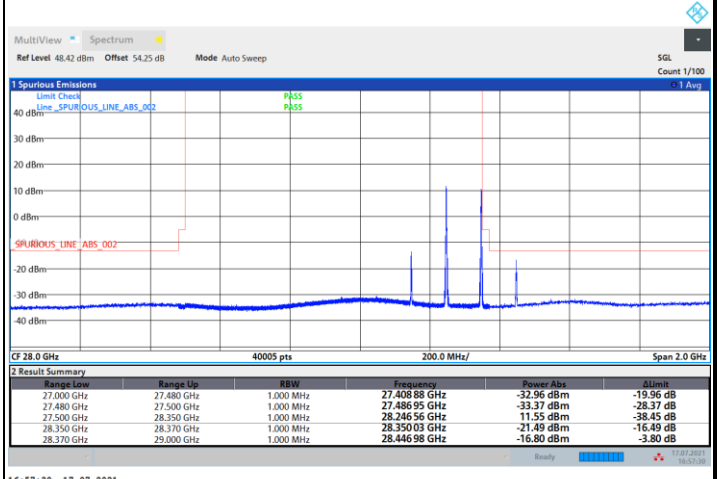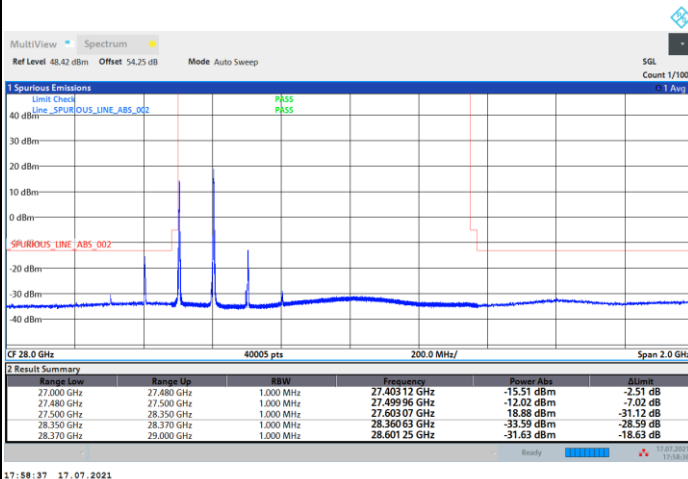





DFT-s-OFDM Module B

NR Band n261 / 100MHz / QPSK

Lowest Band Edge / Full RB

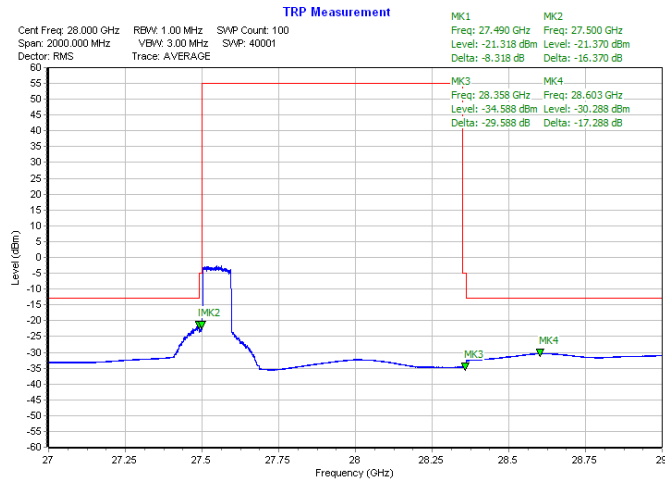


Highest Band Edge / Full RB

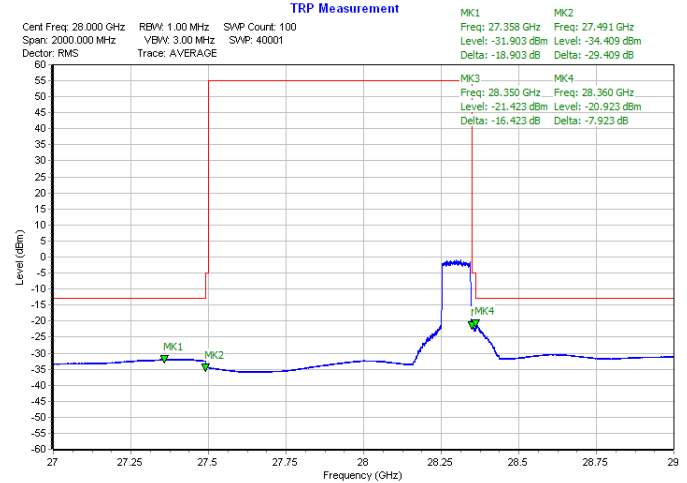


NR Band n261 / 100MHz / 16QAM

Lowest Band Edge / Full RB

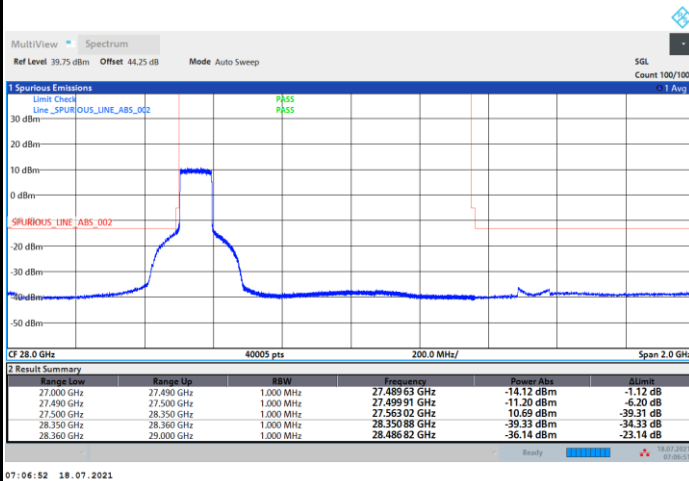

Highest Band Edge / Full RB

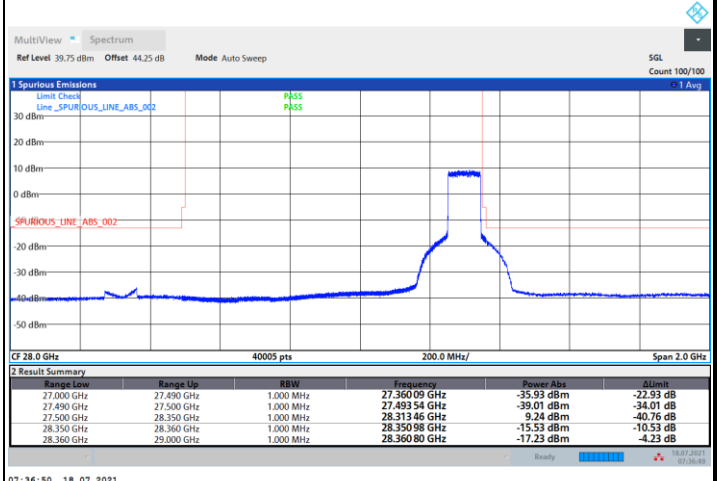





DFT-s-OFDM Module B

NR Band n261 / 100MHz / 64QAM

Lowest Band Edge / Full RB

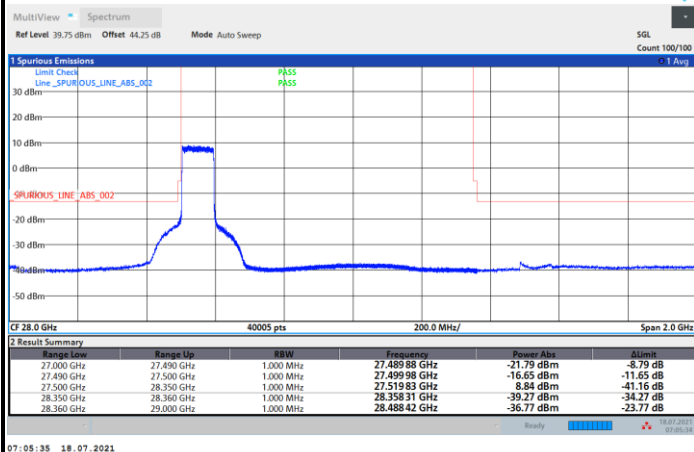


Highest Band Edge / Full RB

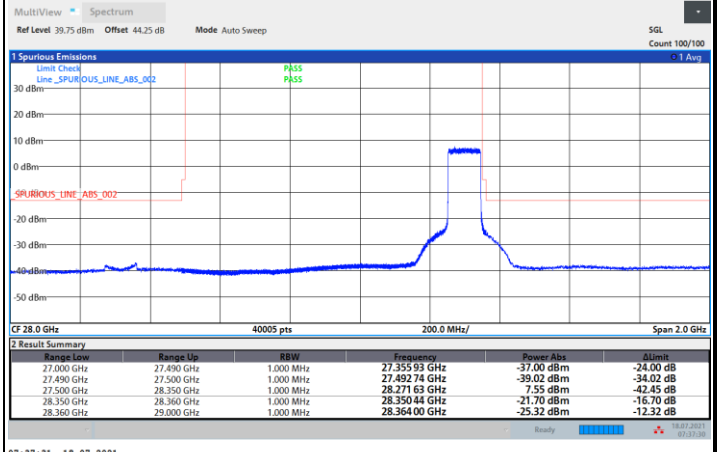


NR Band n261 / 200MHz / QPSK

Lowest Band Edge / Full RB

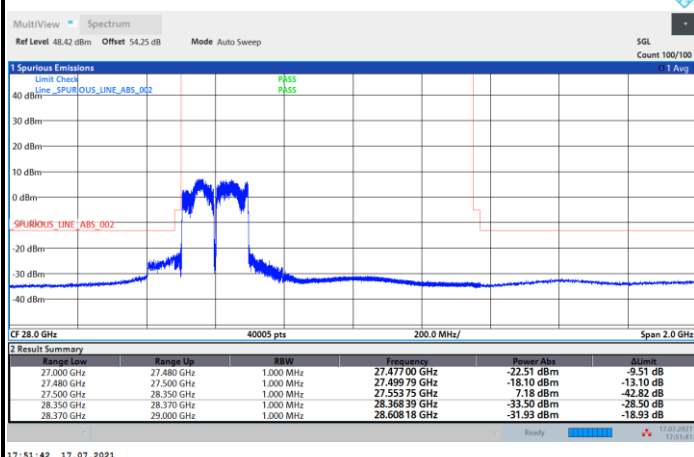

Highest Band Edge / Full RB

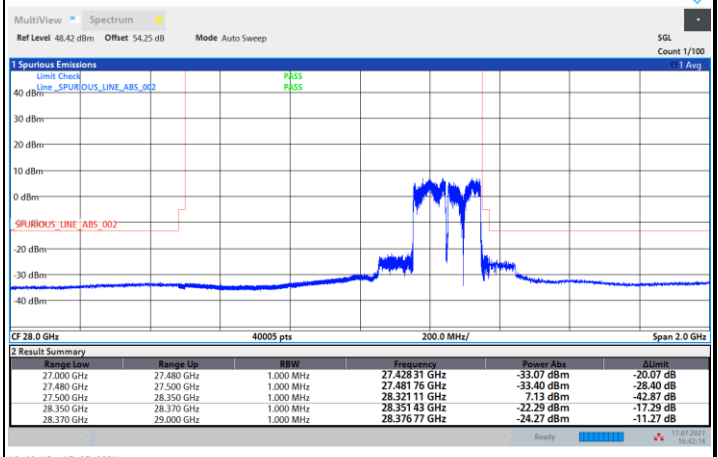





DFT-s-OFDM Module B

NR Band n261 / 200MHz / 16QAM

Lowest Band Edge / Full RB

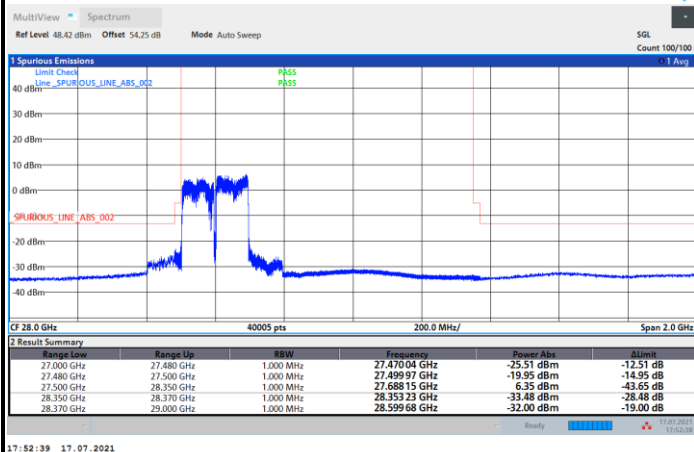


Highest Band Edge / Full RB

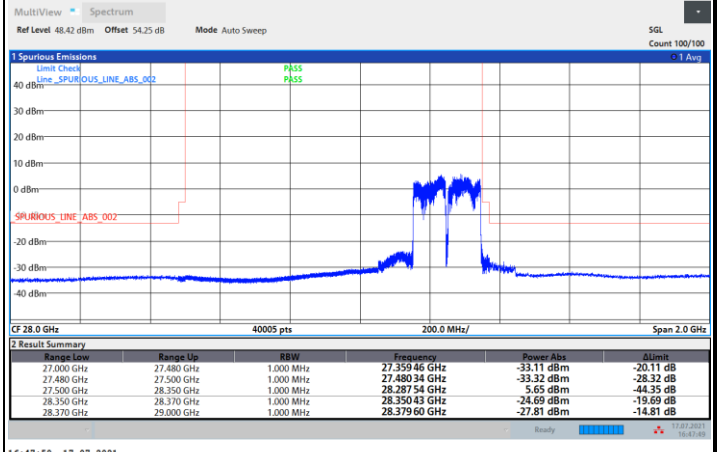


NR Band n261 / 200MHz / 64QAM

Lowest Band Edge / Full RB

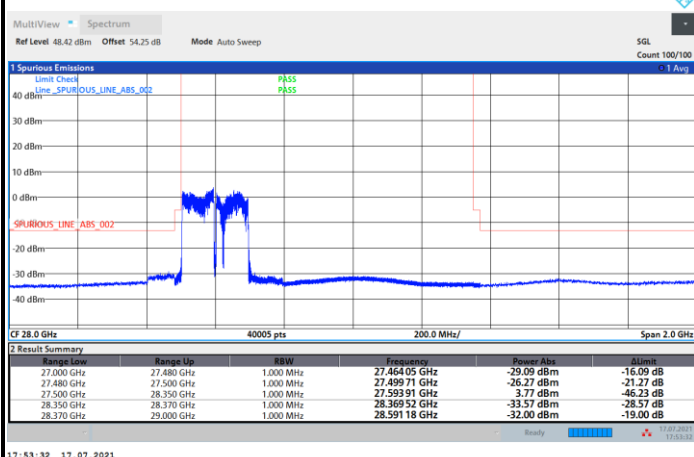


Highest Band Edge / Full RB

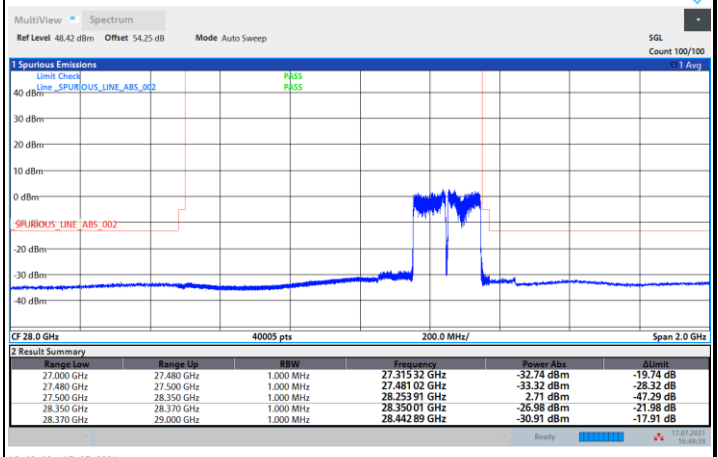




Lowest Band Edge / Full RB



Lowest Band Edge / Full RB




Spurious Emission

There is no significant spurious emission signal found for frequency started from 30MHz up to 18GHz.

Only the noise floor is reported.

NR Band n261 (30MHz-1GHz)


Horizontal

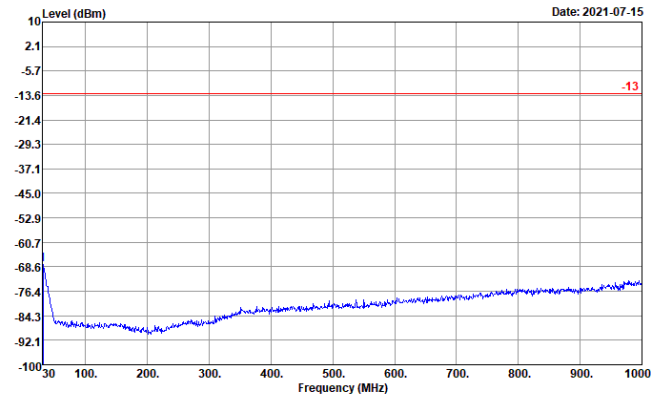

Site : 03CH19-HY
Condition : -13 ERP EIRP_20210305 HORIZONTAL

: n261 MB					
	Freq	Level	Over Limit	Limit Line	Read Level
	MHz	dBm	dB	dBm	dBm
1	30.97	-67.88	-54.88	-13.00	-78.76

Vertical

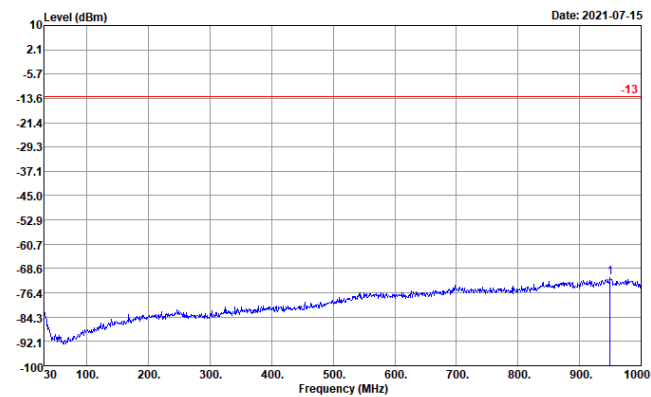


Site : 03CH19-HY
Condition : -13 ERP EIRP_20210305 VERTICAL

: n261 MB					
	Freq	Level	Over Limit	Limit Line	Read Level
	MHz	dBm	dB	dBm	dBm
1	949.56	-71.57	-58.57	-13.00	-81.36



NR Band n261 (1GHz-18GHz)

Horizontal

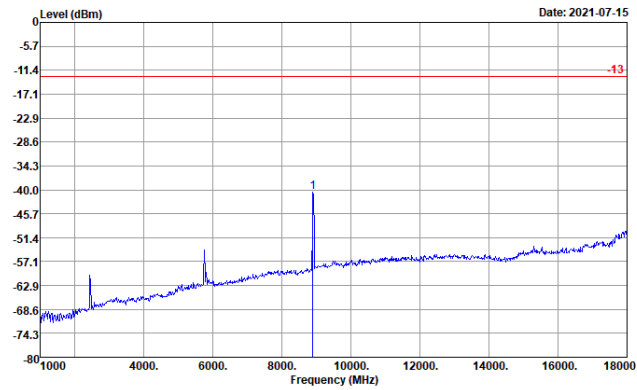


Site : 03CH19-HY
Condition : -13 ERP EIRP_20210305 HORIZONTAL

: n261 MB

Freq	Level	Over Limit	Limit Line	Read Level
MHz	dBm	dB	dBm	dBm
8905.00	-40.53	-27.53	-13.00	-66.17

Vertical

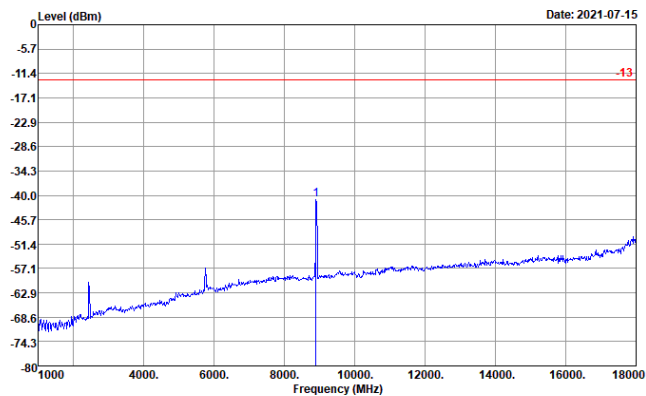

Site : 03CH19-HY
Condition : -13 ERP EIRP_20210305 VERTICAL


: n261 MB

	Freq	Level	Over Limit	Limit Line	Read Level
	MHz	dBm	dB	dBm	dBm
1	8905.00	-41.03	-28.03	-13.00	-66.13



Spurious emission between 18GHz to 40GHz worst case plot is reported as following.


DFT-s-OFDM Module B

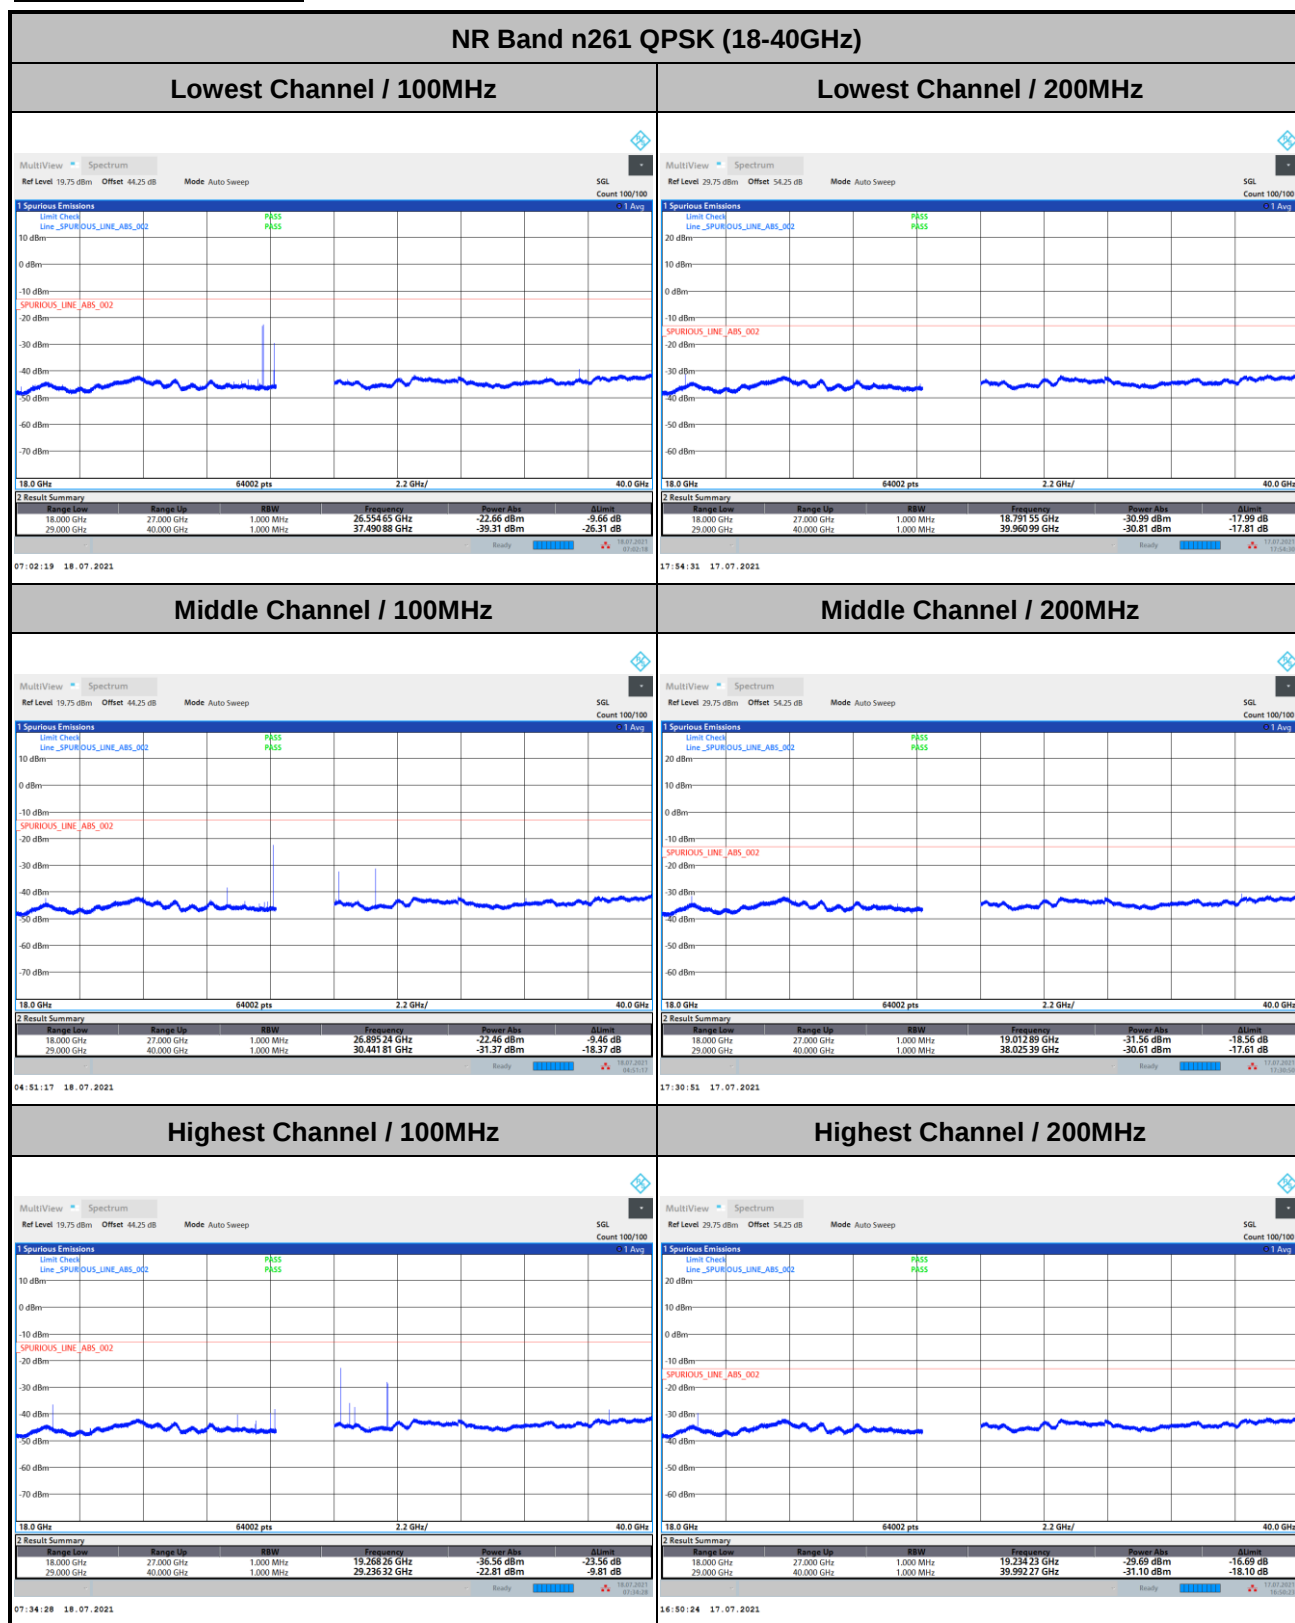

Remark: In band and out of band frequencies that has reported in previous results are omitted.




CP-OFDM Module B

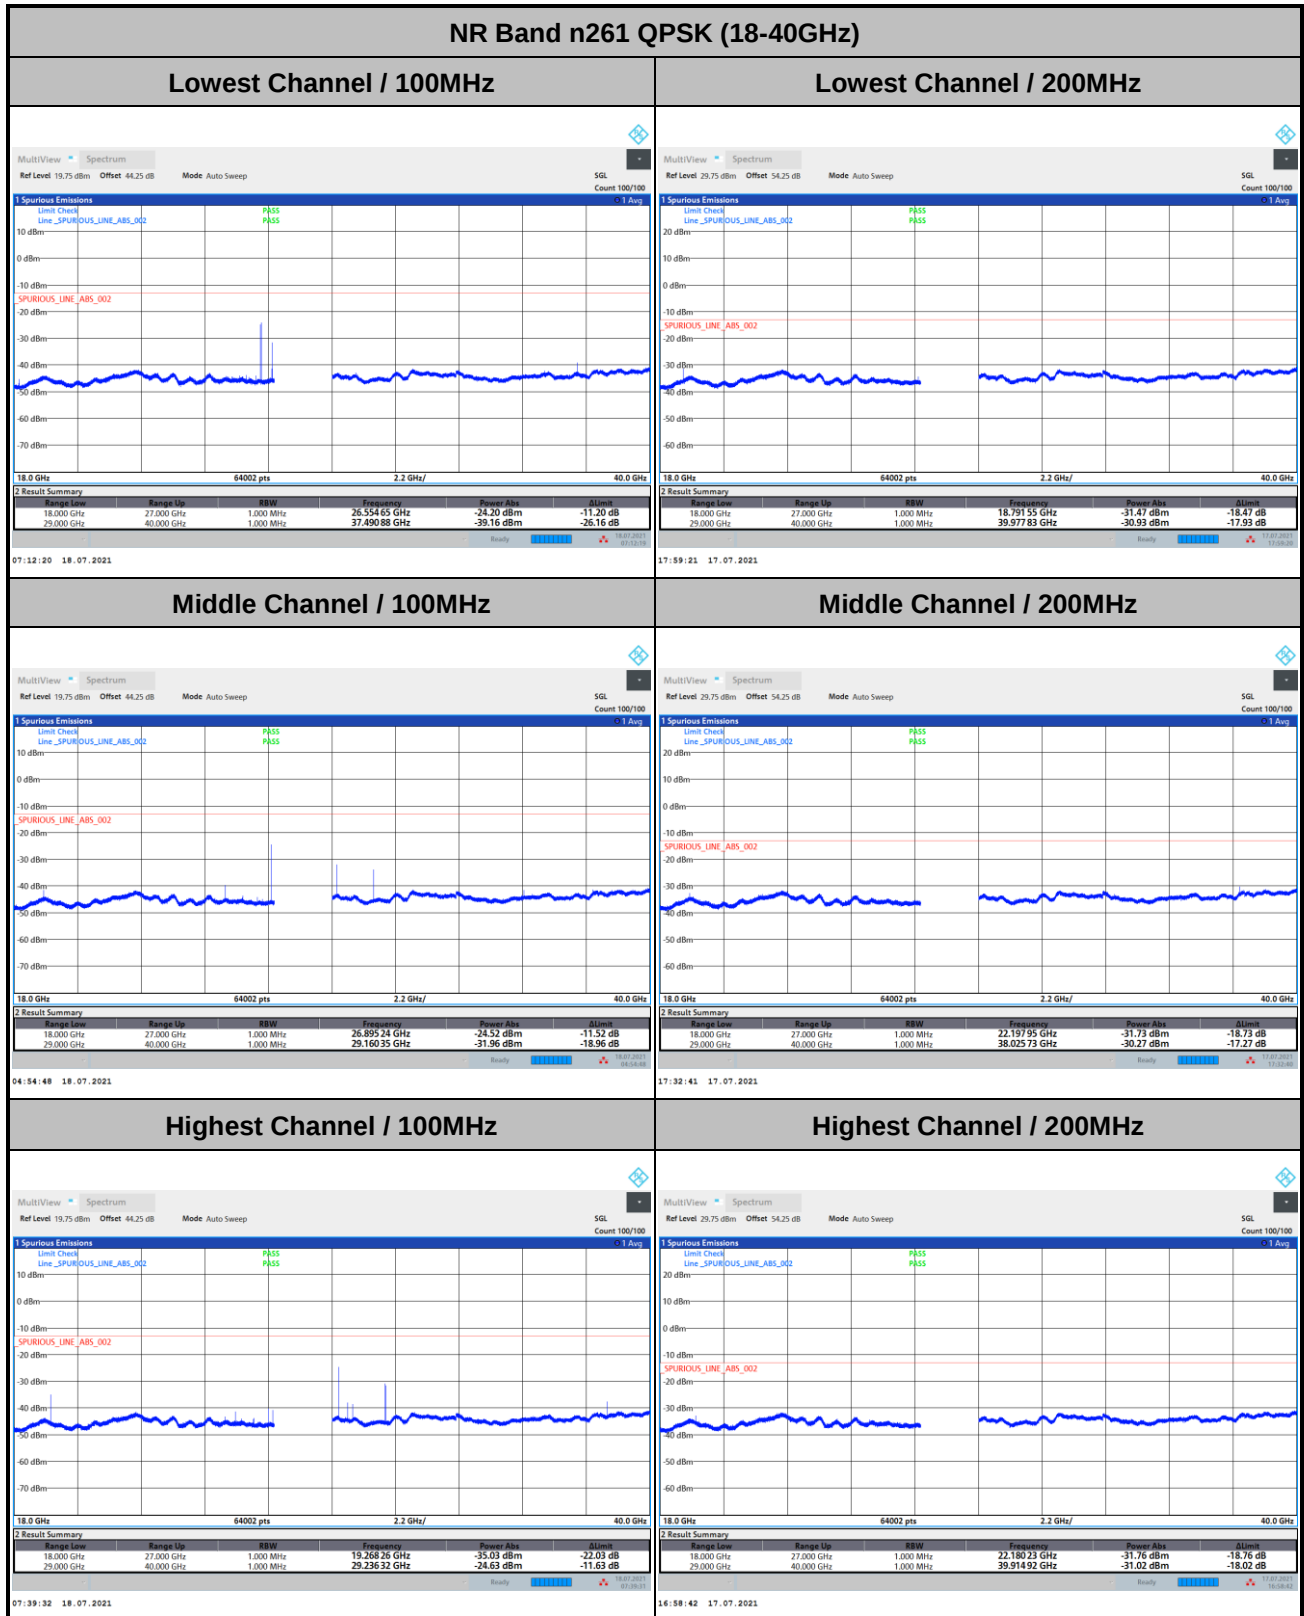


Remark: In band and out of band frequencies that has reported in previous results are omitted.




There is no significant spurious emission signal found for frequency started from 40GHz up to 100GHz.
Only the noise floor is reported.

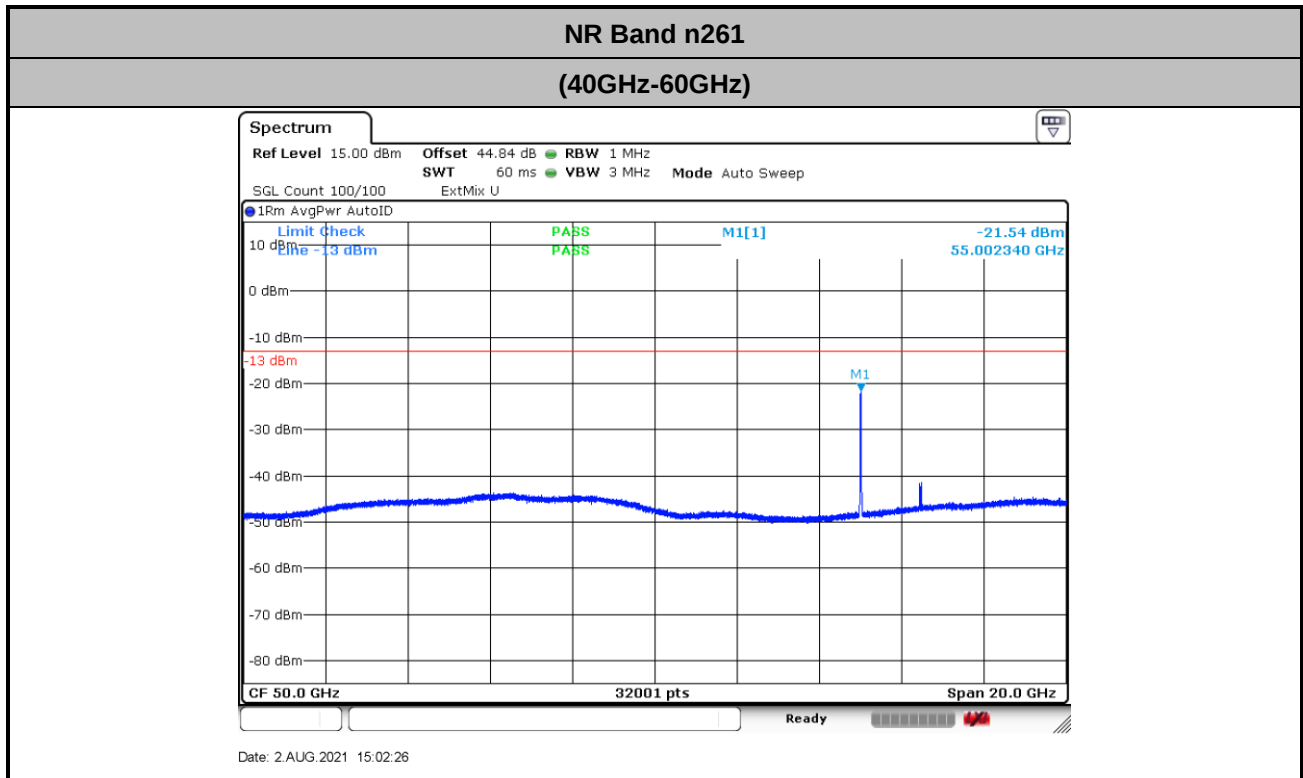

$$\begin{aligned}\text{Offset} &= \text{Antenna Factor (dB/m)} + \text{Cable Loss (dB)} + 107 + 20\log(D) - 104.8 \\ &= 42.3 + 0.34 + 107 + 20\log(1) - 104.8 = 44.84 \text{ (dB)}\end{aligned}$$

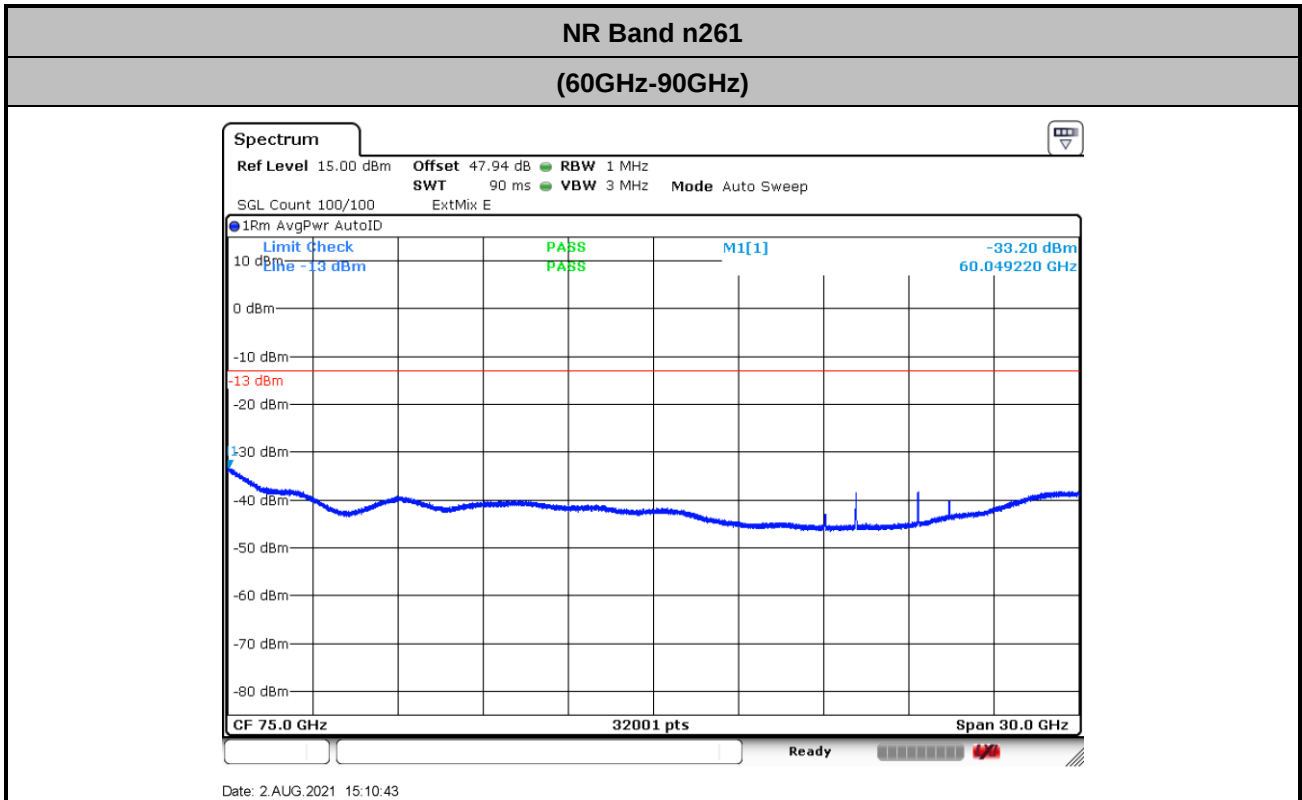

Offset = Antenna Factor (dB/m) + Cable Loss (dB) + 107 + 20log(D) – 104.8
= 45.4 + 0.34 + 107 + 20log(1) – 104.8 = 47.94 (dB)

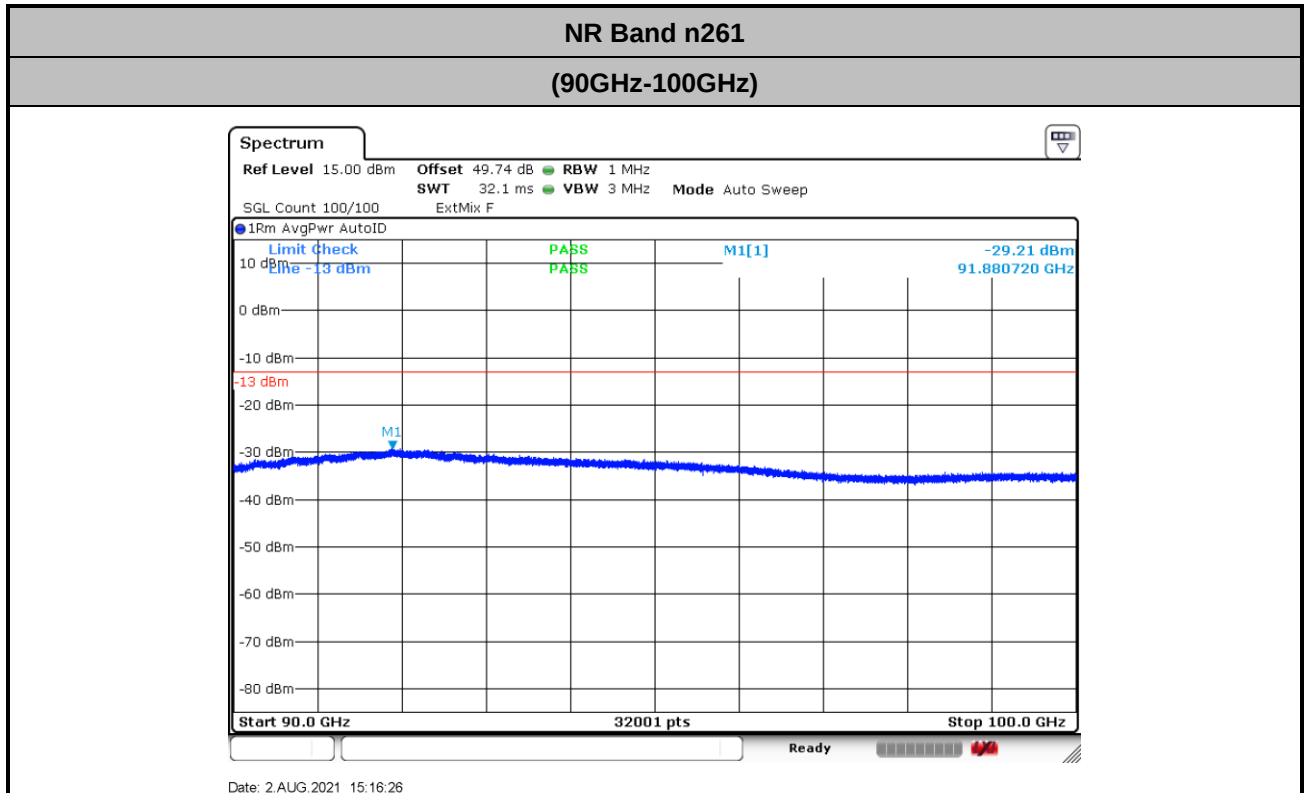

$$\begin{aligned} \text{Offset} &= \text{Antenna Factor (dB/m)} + \text{Cable Loss (dB)} + 107 + 20\log(D) - 104.8 \\ &= 47.2 + 0.34 + 107 + 20\log(1) - 104.8 = 49.74 \text{ (dB)} \end{aligned}$$

Frequency Stability

Test Conditions		NR Band n261 / Middle Channel			Limit
Temperature (°C)	Voltage (Volt)	CW tone			Note 2.
		Frequency (GHz)	Deviation (kHz)	Deviation (ppm)	Result
50	Normal Voltage	27.9260345	-0.500	0.018	Pass
40	Normal Voltage	27.9260345	-0.500	0.018	
30	Normal Voltage	27.9260345	-0.500	0.018	
20(Ref.)	Normal Voltage	27.926034	0.000	0.000	
10	Normal Voltage	27.9260345	-0.500	0.018	
0	Normal Voltage	27.9260345	-0.500	0.018	
-10	Normal Voltage	27.9260345	-0.500	0.018	
-20	Normal Voltage	27.926035	-1.000	0.036	
-30	Normal Voltage	27.926035	-1.000	0.036	
20	Maximum Voltage	27.926034	0.000	0.000	
20	Normal Voltage	27.926034	0.000	0.000	
20	Battery End Point	27.9260345	-0.500	0.018	

Note:

1. Normal Voltage =3.85 V. ; Battery End Point (BEP) =3.60 V. ; Maximum Voltage =4.45 V.
2. The frequency fundamental emissions stay within the authorized frequency block.



Appendix B. R&S Mixer and Horn Antenna Calibration Reports



Calibration Certificate

Kalibrierschein

Certificate Number 24-0060-101033-01

Zertifikatsnummer

Unit Data

Item
Gegenstand
Harmonic Mixer, 40 GHz to 60 GHz

Manufacturer
Hersteller
RPG

Type
Typ
RPG FS-Z60

Material Number
Materialnummer
1048.0171.02

Serial Number
Seriennummer
101033

Asset Number
Inventarnummer

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer
Auftraggeber

Order Number
Bestellnummer

Date of Receipt
Eingangsdatum

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Werteintervall (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Laboratorien. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Performance

Place and Date of Calibration
Ort und Datum der Kalibrierung

Meckenheim, 2020-03-17

Scope of Calibration
Umfang der Kalibrierung

Standard Calibration

Statement of Compliance (Incoming)
Konformitätsaussage (Anlieferung)

New device

Statement of Compliance (Outgoing)
Konformitätsaussage (Auslieferung)

All measured values are within the data sheet specifications.

Extend of Calibration Documents
Umfang des Kalibrierdokuments

**2 pages Calibration Certificate
4 pages Outgoing Results**

Radiometer Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

2020-03-20

Head of Laboratory
Laborleitung

Schulze

Person Responsible
Bearbeiter

Heinze

Page (Seite) 1/2
Vers2010-05-05/
RPG2014-02-28

Calibration Method
Kalibrieranweisung

RPG-PAQA-TN-2014-002

Relative Humidity **20 % - 80 %**
Relative Luftfeuchte

Ambient Temperature
Umgebungstemperatur

(23 ⁺⁷₋₃) °C

Working standards used (having a significant effect on the accuracy)
Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA40	100103	0001-300467129	2021-06-13
Powersensor	R&S® NRP-Z55	140091	509915_D-K-15195-01-01_2019-05	2020-05-22
Powersensor	R&S® NRP-Z57	101423	508173_D-K-15195-01-01_2019-05	2020-05-07

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes

Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

{a}	No measurement uncertainty stated because the errors always add together. So it is sure that a measurement result evaluated as "PASS" is pass.
{b}	The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
{c}	Functional test, therefore no measurement uncertainty is stated.
{d}	Typical value, refer to performance test.
{e}	The measurement uncertainty is taken into account when setting the measuring system.
DL or DT	Data Limit for symmetrical tolerance limits
DLL	Datasheet Lower Limit
DUL	Datasheet Upper Limit
MU	Measurement Uncertainty
MLL or MLV	Measurement Uncertainty Lower Value
MUL or MUV	Measurement Uncertainty Upper Value
Nom.	Nominal Value
Dev.	Deviation
MErr.	Measurement Error
Act.	Actual Value
UGB	Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
UGB1	Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
UGB2	Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
DU	Datasheet Uncertainty

Explanation of charts

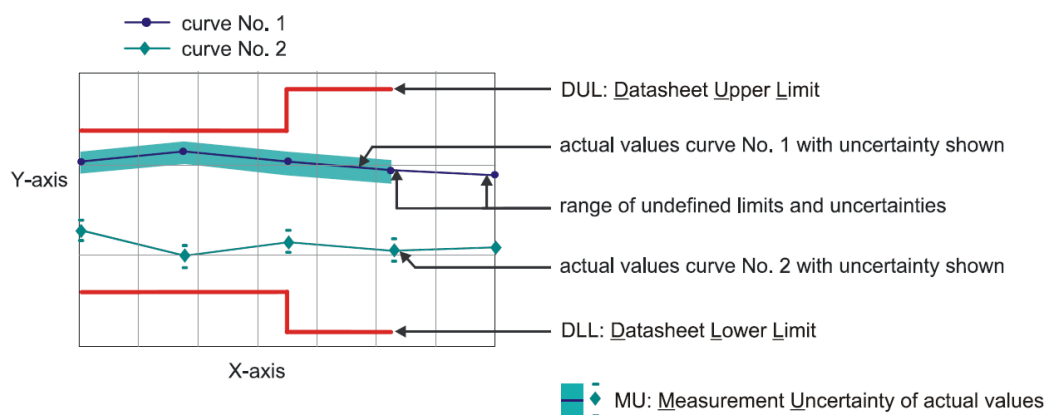

Software used for measurement**Item Type**

Measurement Studio Professional Edition
MixerCertification

Version


2013
7_13

Remark

1.1 Conversion loss

LO level +13 dBm nominal
Bias 0 A

Measurement uncertainty: 1.5 dB

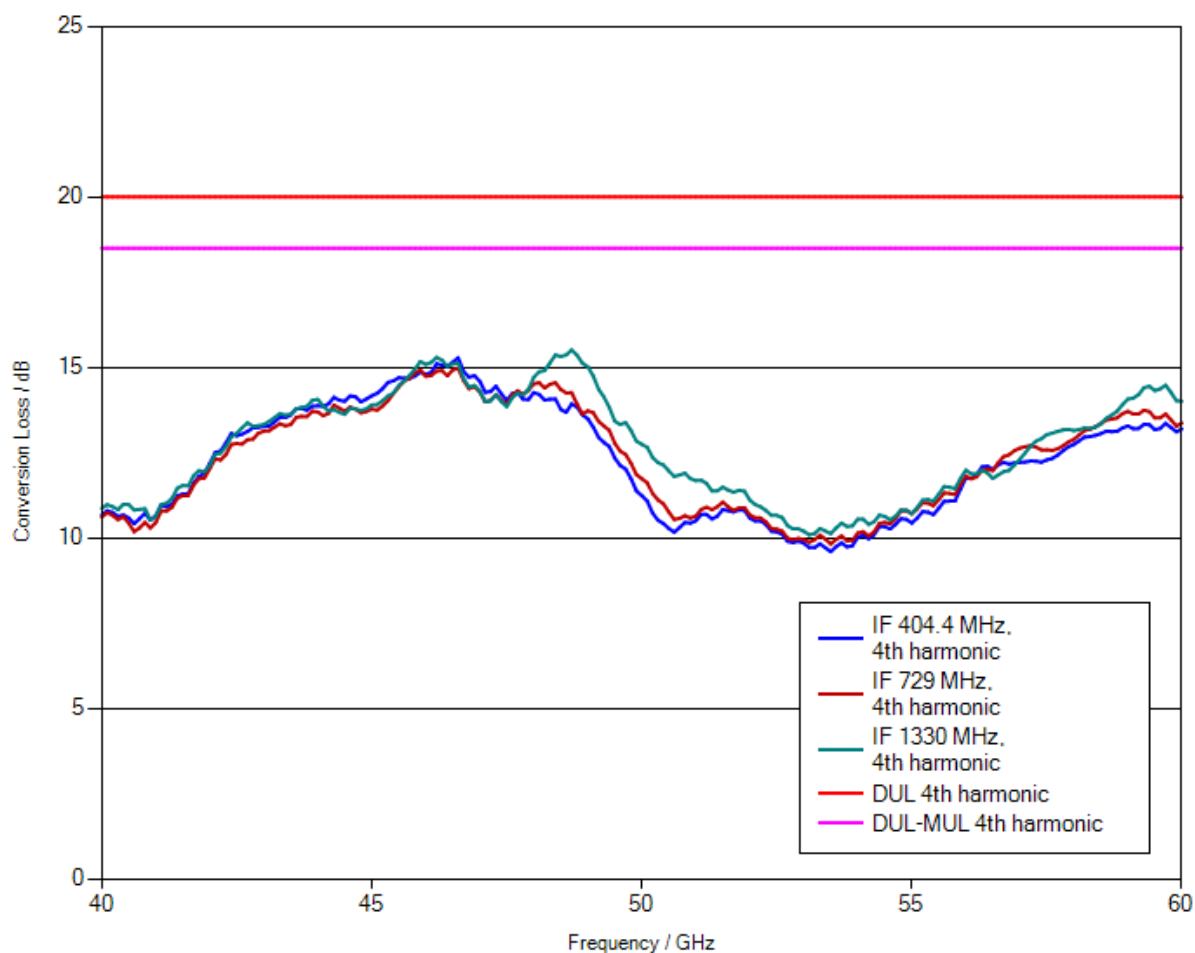

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate. Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.

When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.2 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 4th harmonic	4 dB	2.16 dB	PASS
IF = 729 MHz, 4th harmonic	4 dB	2.04 dB	PASS
IF = 1330 MHz, 4th harmonic	4 dB	2.19 dB	PASS

Calibration Certificate

Kalibrierschein

Certificate Number **24-0090-101867-01**

Zertifikatsnummer

Unit Data

Item
Gegenstand **Harmonic Mixer, 60 GHz to 90 GHz**

Manufacturer
Hersteller **ROHDE & SCHWARZ**

Type
Typ **R&S® FS-Z90**

Material Number
Materialnummer **1048.0371.02** **Serial Number**
Seriennummer **101867**

Asset Number
Inventarnummer

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer
Auftraggeber

Order Number
Bestellnummer

Date of Receipt
Eingangsdatum

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Werteintervall (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Laboratorien. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Performance

Place and Date of Calibration
Ort und Datum der Kalibrierung

Meckenheim, 2019-01-10

Scope of Calibration
Umfang der Kalibrierung

Standard Calibration

Statement of Compliance (Incoming)
Konformitätsaussage (Anlieferung)

New device

Statement of Compliance (Outgoing)
Konformitätsaussage (Auslieferung)

All measured values are within the data sheet specifications.

Extend of Calibration Documents
Umfang des Kalibrierdokuments

**2 pages Calibration Certificate
5 pages Outgoing Results**

Radiometer Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

2019-01-11

Head of Laboratory
Laborleitung



Schulze

Person Responsible
Bearbeiter



Heinze

Page (Seite) 1/2
Vers2010-05-05/
RPG2014-02-28

Calibration Method
Kalibrieranweisung

RPG-PAQA-TN-2014-002

Relative Humidity **20 % - 80 %**
Relative Luftfeuchte

Ambient Temperature
Umgebungstemperatur

(23 ⁺⁷₋₃) °C

Working standards used (having a significant effect on the accuracy)
Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA67	101097	20-300432406	2020-07-21
Powersensor	R&S® NRP-Z55	140093	20-300426315	2019-05-17
Powersensor	R&S® NRP-Z58	101063	0001-300474490	2019-08-06
Calibration kit	WR12	E10001	RPG-PAQA-TN-2014-005	2019-02-01

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes

Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

{a}	No measurement uncertainty stated because the errors always add together. So it is sure that a measurement result evaluated as "PASS" is pass.
{b}	The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
{c}	Functional test, therefore no measurement uncertainty is stated.
{d}	Typical value, refer to performance test.
{e}	The measurement uncertainty is taken into account when setting the measuring system.
DL or DT	Data Limit for symmetrical tolerance limits
DLL	Datasheet Lower Limit
DUL	Datasheet Upper Limit
MU	Measurement Uncertainty
MLL or MLV	Measurement Uncertainty Lower Value
MUL or MUV	Measurement Uncertainty Upper Value
Nom.	Nominal Value
Dev.	Deviation
MErr.	Measurement Error
Act.	Actual Value
UGB	Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
UGB1	Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
UGB2	Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
DU	Datasheet Uncertainty

Explanation of charts

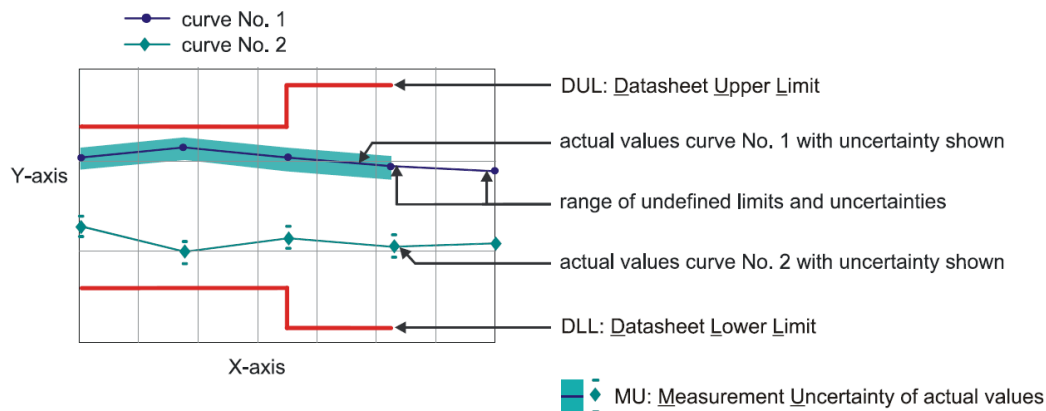

Software used for measurement**Item Type**

Measurement Studio Professional Edition
MixerCertification


Version

2013
7_09

Remark

1.1 RF Input – VSWR

Measurement uncertainty: 0.05 (VSWR)

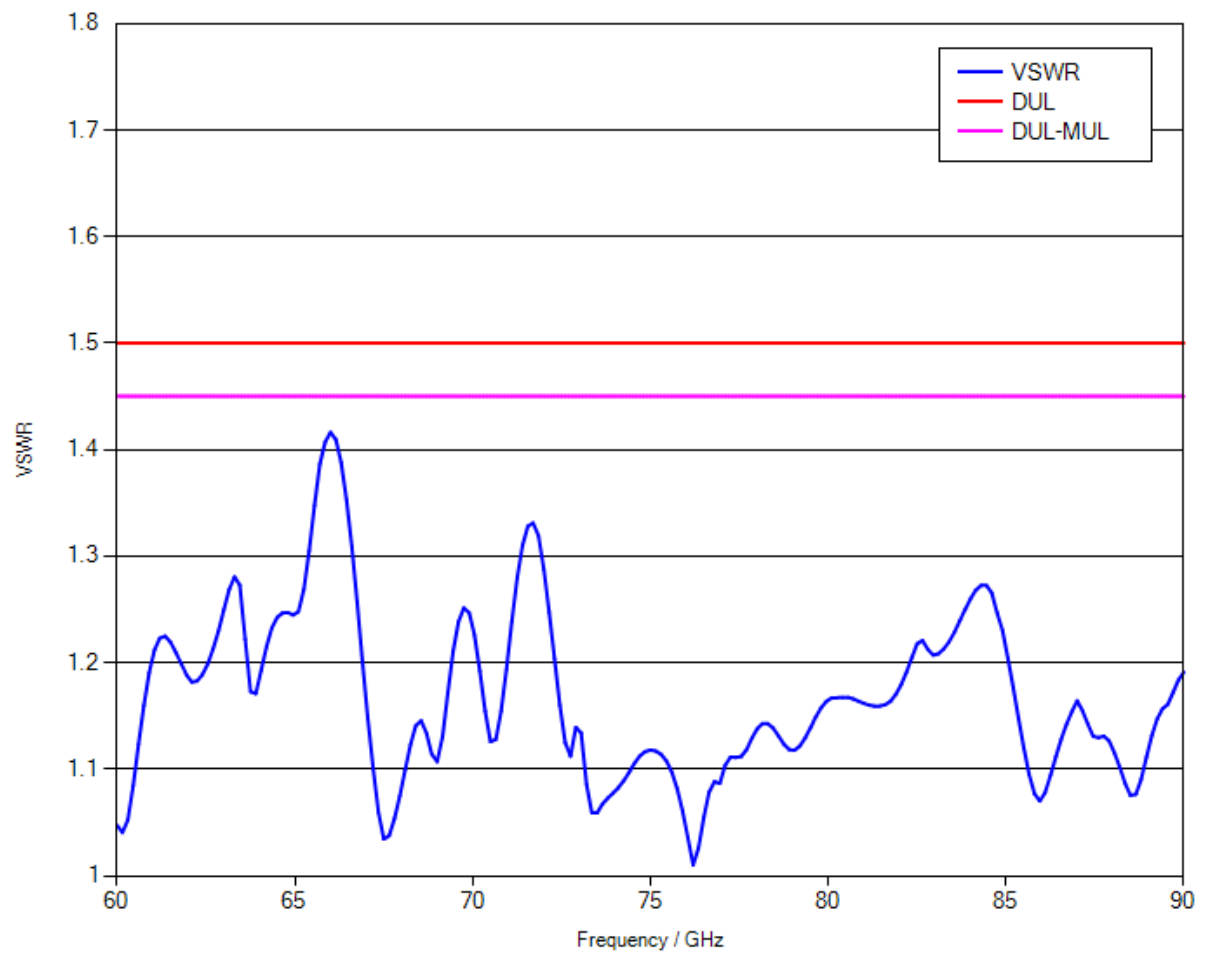


1.2 Conversion loss

LO level +14 dBm nominal

Bias 0 A

Measurement uncertainty: 1.5 dB

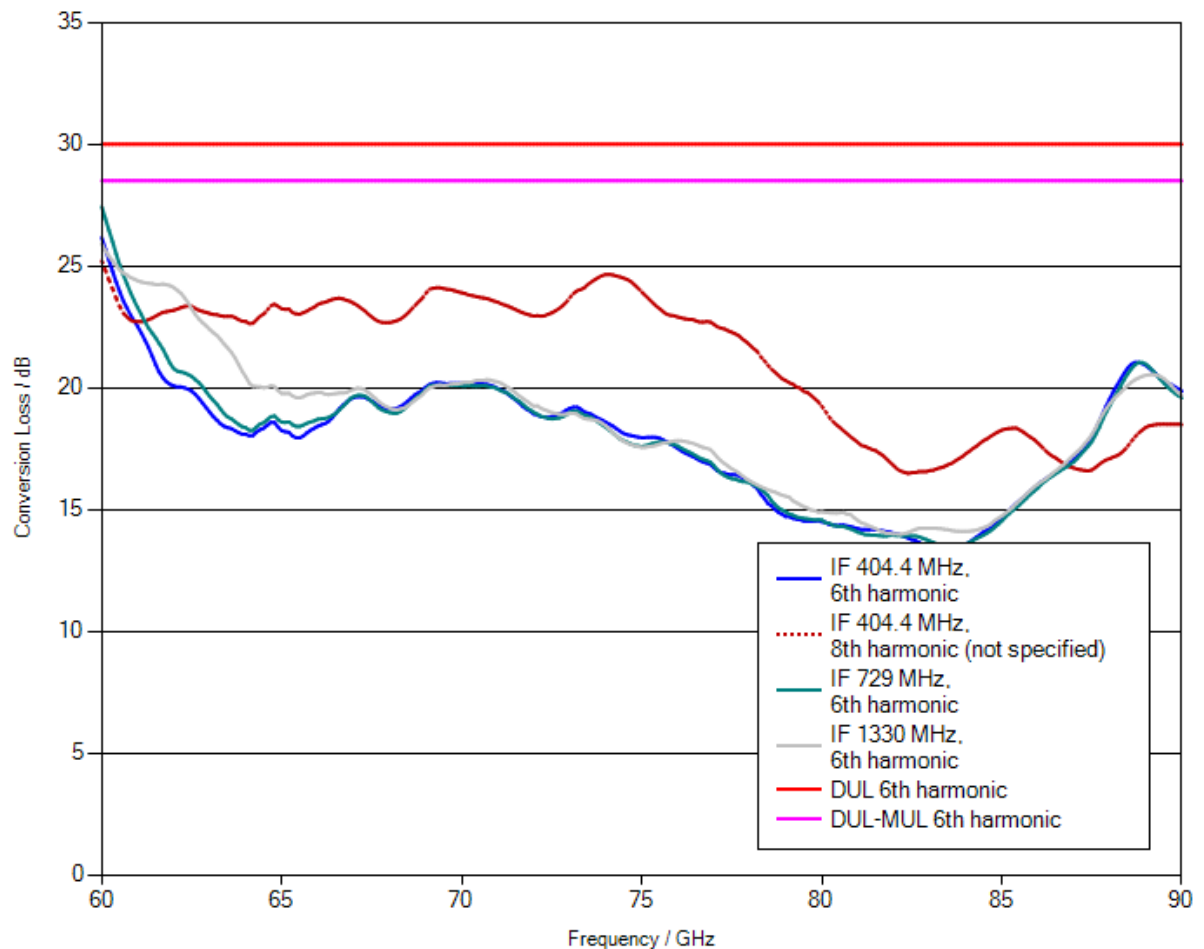

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate. Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.

When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.3 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 6th harmonic	6 dB	3.42 dB	PASS
IF = 404.4 MHz, 8th harmonic	not specified	2.49 dB	not specified
IF = 729 MHz, 6th harmonic	6 dB	3.85 dB	PASS
IF = 1330 MHz, 6th harmonic	6 dB	2.01 dB	PASS



Calibration Certificate

Kalibrierschein

Certificate Number **24-0140-101128-02**

Zertifikatsnummer

Unit Data

Item Harmonic Mixer, 90 GHz to 140 GHz
Gegenstand

Manufacturer RPG Radiometer-Physics GmbH
Hersteller

Type RPG FS-Z140
Typ

Material Number 3622.0708.02 **Serial Number** 101128
Materialnummer **Seriennummer**

Asset Number
Inventarnummer

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer Sporton International Inc.
Auftraggeber No. 106 6F., Sec. 1, Hsin Tai Wu Rd., Xizhi Dist., 000000 NEW TAIPEI CITY-000000 221- TAIWAN

Order Number 8800003072
Bestellnummer

Date of Receipt 2020-10-06
Eingangsdatum

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Werteintervall (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Laboratorien. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Performance

Place and Date of Calibration
Ort und Datum der Kalibrierung

Meckenheim, 2020-10-26

Scope of Calibration
Umfang der Kalibrierung

Standard Calibration

Statement of Compliance (Incoming)
Konformitätsaussage (Anlieferung)

Defective.

Statement of Compliance (Outgoing)
Konformitätsaussage (Auslieferung)

All measured values are within the data sheet specifications.

Extend of Calibration Documents
Umfang des Kalibrierdokuments

2 pages Calibration Certificate
4 pages Outgoing Results

RPG Radiometer-Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

2020-10-27

Head of Laboratory
Laborleitung

Schulze

Person Responsible
Bearbeiter

Gottbehüt

Calibration Method
Kalibrieranweisung

RPG-PAQA-TN-2014-002

Relative Humidity **20 % - 80 %**
Relative Luftfeuchte

Ambient Temperature
Umgebungstemperatur

(23 ⁺⁷₋₃) °C

Working standards used (having a significant effect on the accuracy)
Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA40	100103	0001-300467129	2021-06-13
Powersensor	R&S® NRP-Z55	140093	509916_D-K-15195-01-01_2019-05	2021-05-22

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes

Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

{a}	No measurement uncertainty stated because the errors always add together. So it is sure that a measurement result evaluated as "PASS" is pass.
{b}	The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
{c}	Functional test, therefore no measurement uncertainty is stated.
{d}	Typical value, refer to performance test.
{e}	The measurement uncertainty is taken into account when setting the measuring system.
DL or DT	Data Limit for symmetrical tolerance limits
DLL	Datasheet Lower Limit
DUL	Datasheet Upper Limit
MU	Measurement Uncertainty
MLL or MLV	Measurement Uncertainty Lower Value
MUL or MUV	Measurement Uncertainty Upper Value
Nom.	Nominal Value
Dev.	Deviation
MErr.	Measurement Error
Act.	Actual Value
UGB	Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
UGB1	Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
UGB2	Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
DU	Datasheet Uncertainty

Explanation of charts

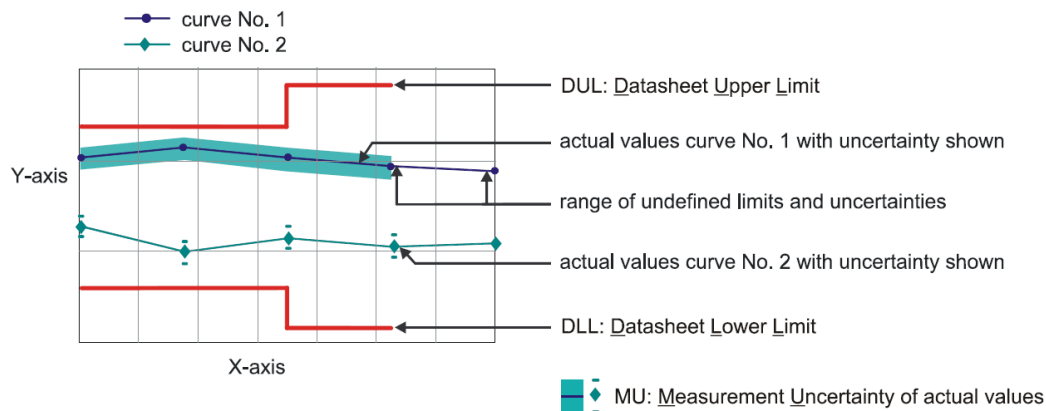

Software used for measurement**Item Type**

Measurement Studio Professional Edition
MixerCertification

Version


2013
7_14

Remark

1.1 Conversion loss

LO level +14 dBm nominal
Bias 0 A

Measurement uncertainty: 3.5 dB

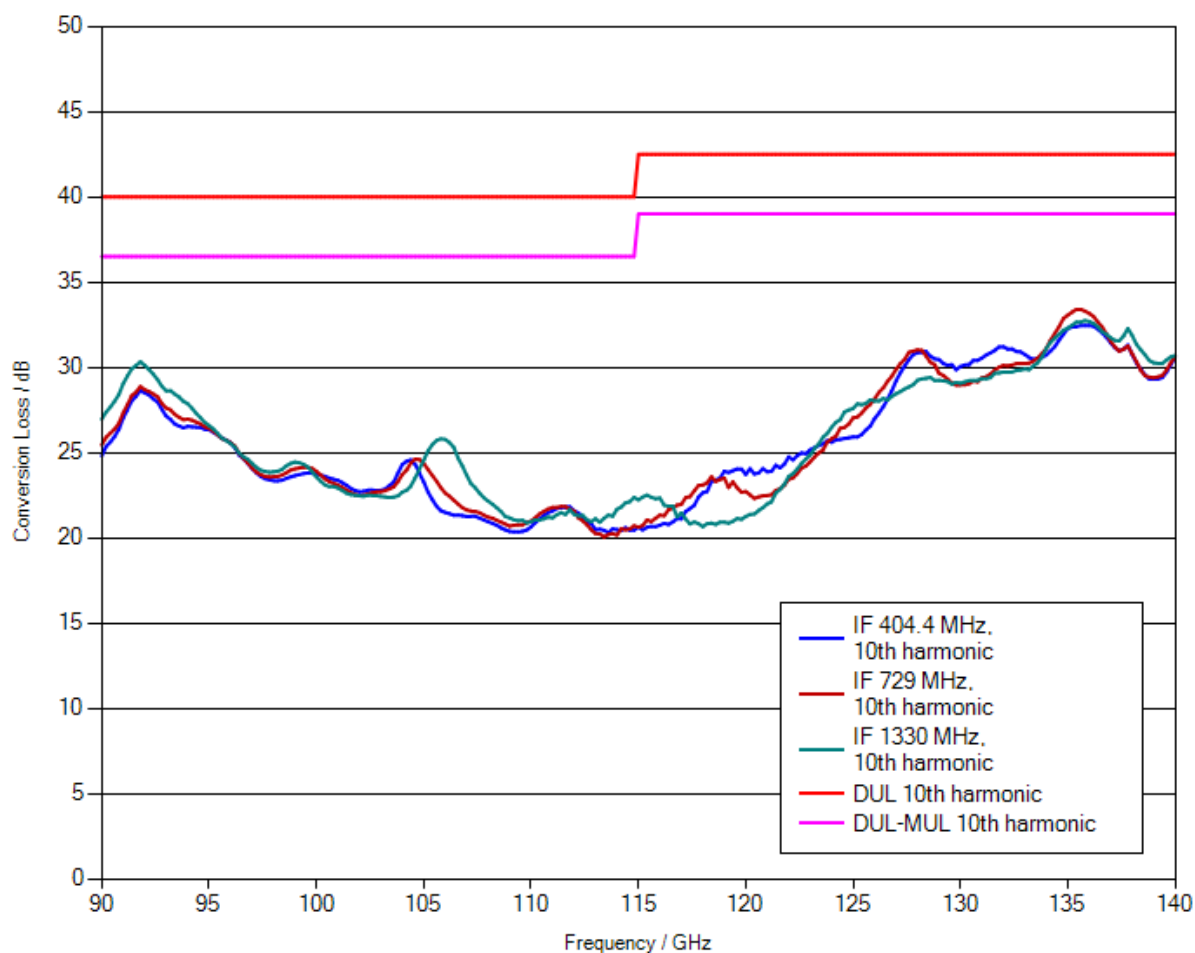

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate. Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.

When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.2 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 10th harmonic	6 dB	2.1 dB	PASS
IF = 729 MHz, 10th harmonic	6 dB	1.96 dB	PASS
IF = 1330 MHz, 10th harmonic	6 dB	2.13 dB	PASS



Calibration Certificate

Kalibrierschein

Certificate Number 24-0220-101014-01

Zertifikatsnummer

Unit Data

Item
Gegenstand
Harmonic Mixer, 140 GHz to 220 GHz

Manufacturer
Hersteller
RPG

Type
Typ
RPG FS-Z220

Material Number
Materialnummer
3593.3250.02

Serial Number
Seriennummer
101014

Asset Number
Inventarnummer

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer
Auftraggeber

Order Number
Bestellnummer

Date of Receipt
Eingangsdatum

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Werteintervall (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Laboratorien. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Performance

Place and Date of Calibration
Ort und Datum der Kalibrierung

Meckenheim, 2018-08-27

Scope of Calibration
Umfang der Kalibrierung

Standard Calibration

Statement of Compliance (Incoming)
Konformitätsaussage (Anlieferung)

New device

Statement of Compliance (Outgoing)
Konformitätsaussage (Auslieferung)

All measured values are within the data sheet specifications.

Extend of Calibration Documents
Umfang des Kalibrierdokuments

**2 pages Calibration Certificate
5 pages Outgoing Results**

Radiometer Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

2018-08-28

Head of Laboratory
Laborleitung

Schulze

Person Responsible
Bearbeiter

Heinze

Page (Seite) 1/2
Vers2010-05-05/
RPG2014-02-28

Calibration Method
Kalibrieranweisung

RPG-PAQA-TN-2014-002

Relative Humidity **20 % - 80 %**
Relative Luftfeuchte

Ambient Temperature
Umgebungstemperatur

(23 ⁺⁷₋₃) °C

Working standards used (having a significant effect on the accuracy)
Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA67	101097	20-300432406	2020-07-21
Powersensor	R&S® NRP-Z55	140093	20-300426315	2019-05-17

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes
Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

{a}	No measurement uncertainty stated because the errors always add together. So it is sure that a measurement result evaluated as "PASS" is pass.
{b}	The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
{c}	Functional test, therefore no measurement uncertainty is stated.
{d}	Typical value, refer to performance test.
{e}	The measurement uncertainty is taken into account when setting the measuring system.
DL or DT	Data Limit for symmetrical tolerance limits
DLL	Datasheet Lower Limit
DUL	Datasheet Upper Limit
MU	Measurement Uncertainty
MLL or MLV	Measurement Uncertainty Lower Value
MUL or MUV	Measurement Uncertainty Upper Value
Nom.	Nominal Value
Dev.	Deviation
MErr.	Measurement Error
Act.	Actual Value
UGB	Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
UGB1	Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
UGB2	Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
DU	Datasheet Uncertainty

Explanation of charts

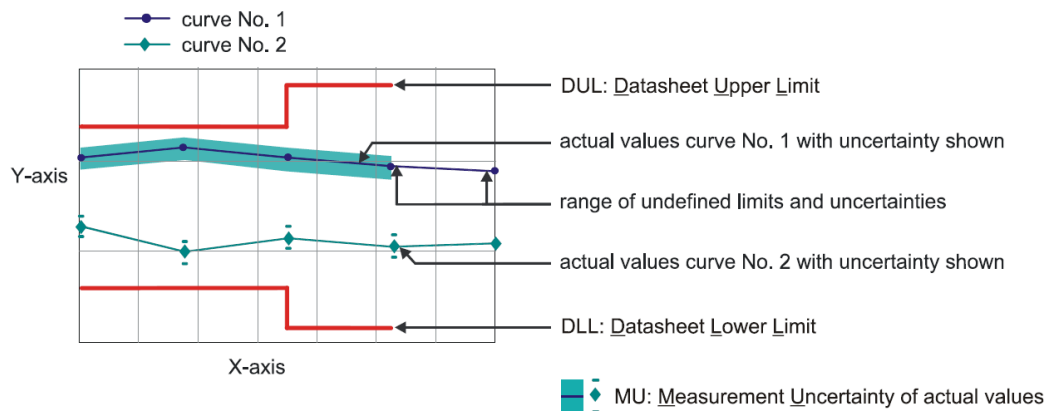

Software used for measurement**Item Type**

Measurement Studio Professional Edition
MixerCertification


Version

2013
7_09

Remark

1.1 RF Input – VSWR


Measurement uncertainty: 0.05 (VSWR)

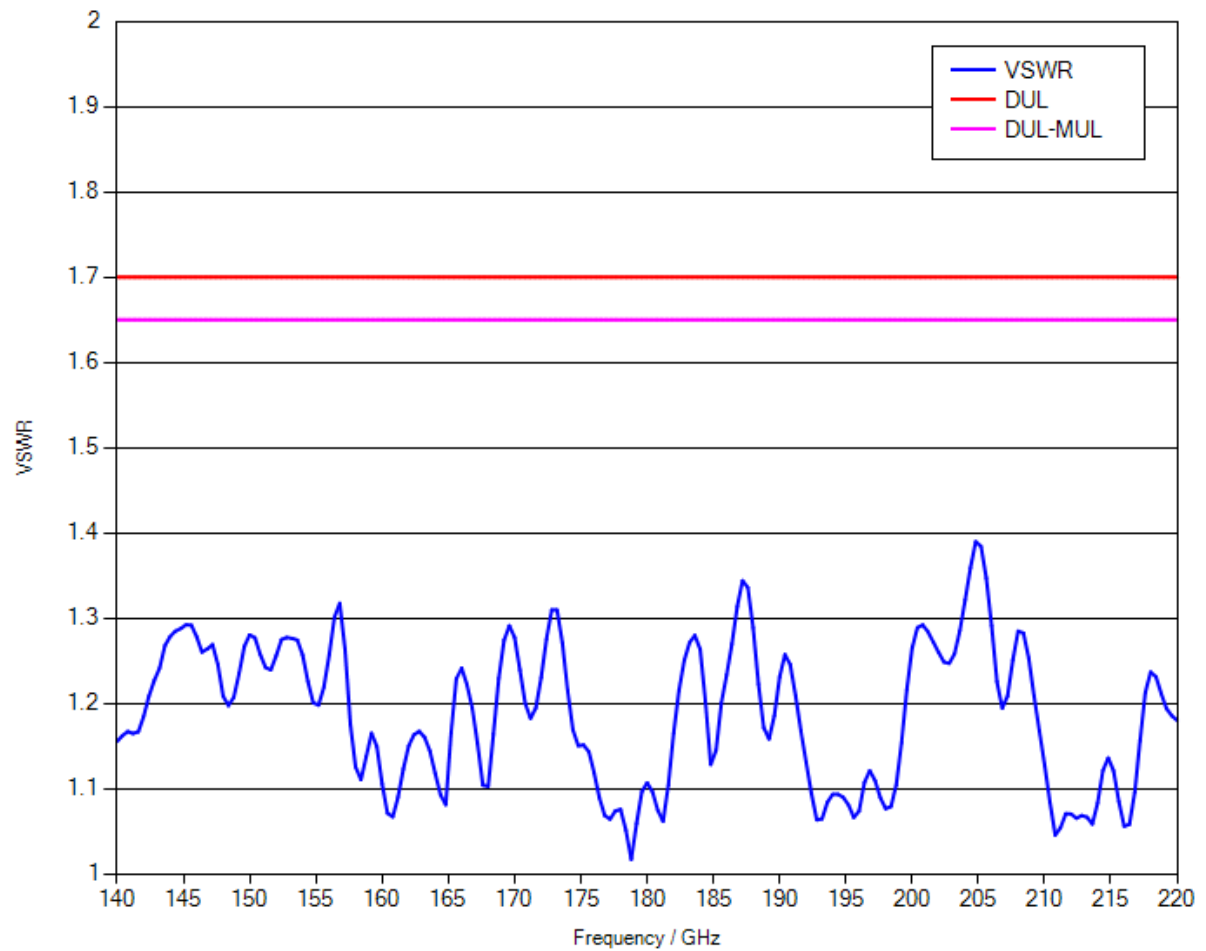

1.2 Conversion loss

LO level +13 dBm nominal
Bias 0 A

Measurement uncertainty: 4 dB

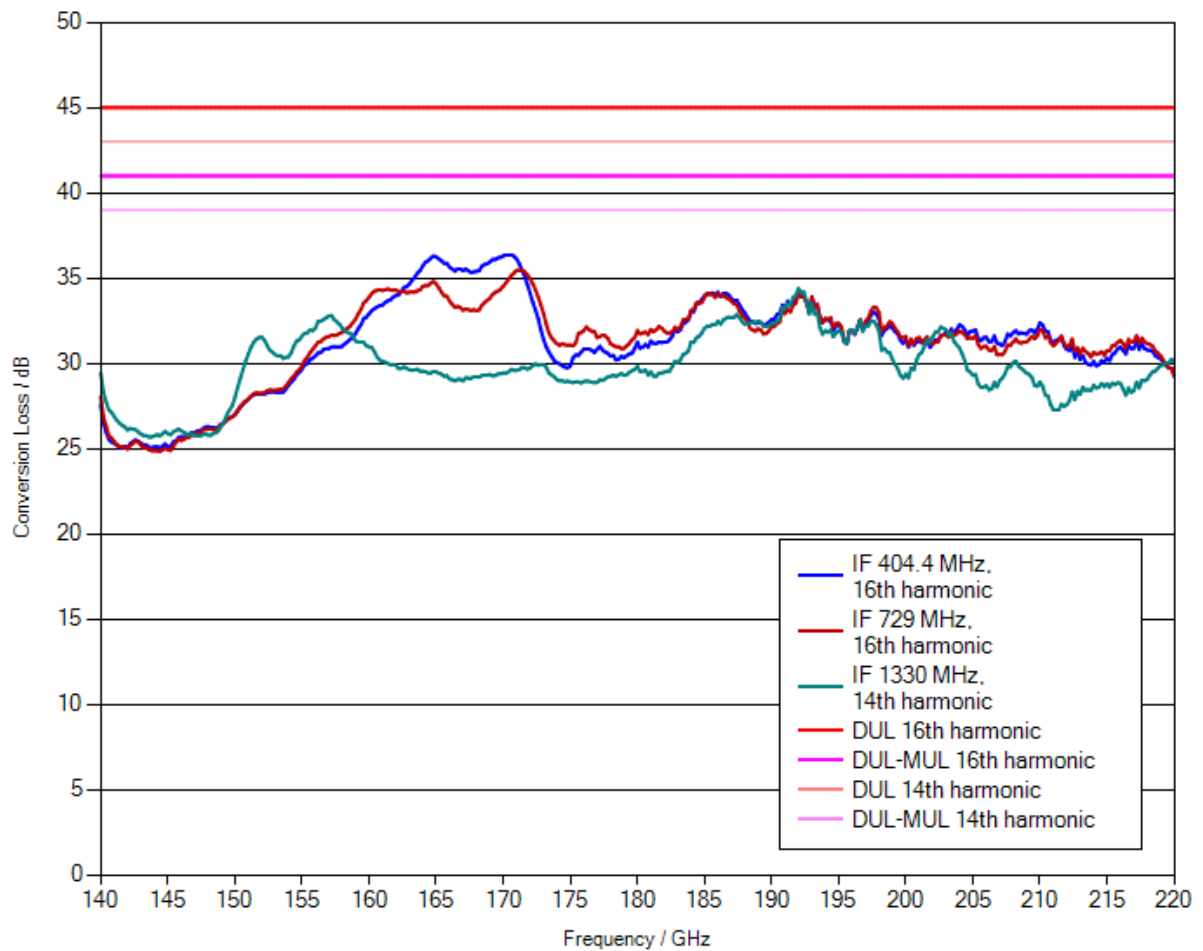

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate. Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.

When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.3 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 16th harmonic	6 dB	2.71 dB	PASS
IF = 729 MHz, 16th harmonic	6 dB	2.61 dB	PASS
IF = 1330 MHz, 14th harmonic	6 dB	2.61 dB	PASS



Calibration certificate



Accreditation certificate No. **№ BY/112 02.5.0.0065** of **09.01.2015**

Certificate number **25-18** Date when calibrated **08/17/2018** Page **1** of **2**

**Item
calibrated**

Antenna QWH-UPRR00 # 923600007

Description of measurement standard / measuring instrument / identification

Customer

Sporton International Inc.

No. 52, HwaYa 1st Road, HwaYa Technology Park, Kwei-Shan District,
TaoYuan City 333, Taiwan, R.O.C.

Name of the customer, address

**Method of
calibration**

GOST 20271.1, MK KL 8.2-16

Name of the method / identification

All measurements are traceable to the SI units which are realized by national measurement standards of NMI and state standards of RF. This certificate shall not be reproduced, except in full. Any publication extracts from the calibration certificate requires written permission of the issuing calibration laboratory of microwave measuring equipment.

**Authorising
signature**



M. Svirid/ Technical manager

Name and position

Date of issue 08/17/2018