



Specific Absorption Rate (SAR) Test Report for

SYMBOL Technologies, INC.

on the

Mobile computer

Report No. : FA691116-1-2-07

Trade Name : Symbol : WT4090

FCC ID : H9PWT4090
Date of Testing : Sep. 21, 2006
Date of Report : Sep. 22, 2006
Date of Review : Sep. 22, 2006

- The test results refer exclusively to the presented test model / sample only.
- Without written approval of SPORTON International Inc., the test report shall not be reproduced except in full.
- Report Version: Rev. 07

SPORTON International Inc.

6F, No.106, Sec. 1, Hsin Tai Wu Rd., Hsi Chih, Taipei Hsien, Taiwan, R.O.C.



Table of Contents

		nent of Compliance							
		istration Data							
	2.1	Testing Laboratory							
	2.2	Detail of Applicant							
	2.3								
	2.4	Application Detail							
3. Sc	ope		3						
	3.1	Description of Device Under Test (DUT)							
	3.2	Product Photo							
	3.3	Applied Standards:	6						
	3.4	Device Category and SAR Limits	7						
	3.5	Test Conditons							
		3.5.1 Ambient Condition:							
		3.5.2 Test Configuration:							
4. Sp	ecific	ic Absorption Rate (SAR)							
	4.1	Introduction							
	4.2	SAR Definition							
5. SA	AR Me	leasurement Setup							
	5.1	DASY4 E-Field Probe System							
		5.1.1 EX3DV3 E-Field Probe Specification	11						
		5.1.2 EX3DV3 E-Field Probe Calibration							
	5.2	DATA Acquisition Electronics (DAE)	12						
	5.3	Robot	13						
	5.4	Measurement Server	13						
	5.5	SAM Twin Phantom	13						
	5.6	Data Storage and Evaluation							
		5.6.1 Data Storage							
		5.6.2 Data Evaluation	15						
	5.7	Test Equipment List	18						
6. Tis	ssue	Simulating Liquids	19						
		ainty Assessment							
8. SA	AR Me	leasurement Evaluation							
	8.1	Purpose of System Performance check							
	8.2	System Setup	22						
	8.3	Validation Results							
		ption for DUT Testing Position							
10.	Meas	surement Procedures							
	10.1								
		10.1.1 For 47 CFR FCC Part 15 Subpart E §15.407 (5150 ~ 5250 MHz)	27						
		10.1.2 For 47 CFR FCC Part 15 Subpart E §15.247 (5725 ~ 5825 MHz)	28						
	10.2	Spatial Peak SAR Evaluation	28						
		Scan Procedures							
		SAR Averaged Methods							
11.	SAR	Test Results	30						
	11.1	Keypad Up with Touch with Scanner A							
	11.2	71.							
	11.3								
	11.4	. All							
		rences	31						
App	endi	lix A – System Performance Check Data							
App	endi	ix B – SAR Measurement Data							
		lix C – Calibration Data							



1. Statement of Compliance

The Specific Absorption Rate (SAR) maximum result found during testing for the **SYMBOL Technologies**, **INC. Mobile computer Symbol WT4090 on the 5 GHz band body SAR** are as follows (with expanded uncertainty 25.9% for 5GHz Band):

5150 ~ 5250 MHz	5725 ~ 5825 MHz
<band 1=""></band>	<band 3=""></band>
Body SAR (W/kg)	Body SAR (W/kg)
0.601	0.68

The co-location of WLAN and Bluetooth were also checked. It is in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1999 and had been tested in accordance with the measurement methods and procedures specified in OET Bulletin 65 Supplement C (Edition 01-01).

Approved by

Dr. Daniel Lee EMC/SAR Director



2. Administration Data

2.1 Testing Laboratory

Company Name : Sporton International Inc. **Department :** Antenna Design/SAR

Address: No.52, Hwa-Ya 1st RD., Hwa Ya Technology Park, Kwei-Shan Hsiang, TaoYuan

Hsien, Taiwan, R.O.C.

Telephone Number: 886-3-327-3456 **Fax Number:** 886-3-327-0973

2.2 Detail of Applicant

Company Name: SYMBOL Technologies, INC.

Address: One Symbol Plaza Holtsville, New York 11742-1300 U.S.A.

2.3 Detail of Manufacturer

Company Name: Universal Scientific Industrial CO., LTD.

Address: 141, Lane 351, Taiping Road, Sec. 1, Tsao Tuen, Nan-Tou, Taiwan

2.4 Application Detail

Date of reception of application: Sep. 11, 2006 Start of test: Sep. 21, 2006 End of test: Sep. 21, 2006



3. Scope

3.1 <u>Description of Device Under Test (DUT)</u>

DUT Type:	Mobile computer
Trade Name :	Symbol
Model Name :	WT4090
FCC ID:	H9PWT4090
Type of Modulation :	802.11a: OFDM Bluetooth: GFSK
Frequency Band:	802.11a: 5150 ~ 5250 MHz (Band 1) / 5725 ~ 5825 MHz (Band 3) Bluetooth: 2400~2483.5
Antenna Connector :	N/A
Antenna Type :	Fixed Internal
Maximum Output Power to Antenna:	13.16 dBm (Band 1) / 17.71 dBm (Band 3)
DUT Stage:	Production Unit
Application Type:	Certification
Accessory:	Battery: DC 3.7V / 2860 mAh



3.2 Product Photo

EUT





Battery





Scanner A







Scanner B





Wrist Mount







3.3 Applied Standards:

The Specific Absorption Rate (SAR) testing specification, method and procedure for this Mobile computer is in accordance with the following standards:

47 CFR Part 2 (2.1093), IEEE C95.1-1999, IEEE C95.3-2002, IEEE P1528 -2003, and OET Bulletin 65 Supplement C (Edition 01-01)



3.4 Device Category and SAR Limits

This device belongs to portable device category because its radiating structure is allowed to be used within 20 centimeters of the body of the user.

Limit for General Population/Uncontrolled exposure should be applied for this device, it is 1.6 W/kg as averaged over any 1 gram of tissue.

3.5 Test Conditions

3.5.1 Ambient Condition:

Ambient Temperature (°C)	20 ~ 24°C
Tissue simulating liquid temperature (°C)	21.0°C
Humidity (%)	< 60%

3.5.2 <u>Test Configuration:</u>

The data rate for SAR testing is 6 Mbps for 802.11a. Engineering testing software installed on notebook can provide continuous transmitting RF signal. This RF signal utilized in SAR measurement has almost 100% duty cycle and its crest factor is 1.



4. Specific Absorption Rate (SAR)

4.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The FCC recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

4.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density.

 ρ). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = C \frac{\delta T}{\delta t}$$

, where C is the specific head capacity, δT is the temperature rise and δt the exposure duration,

or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma |E|^2}{\rho}$$

, where σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.



5. SAR Measurement Setup

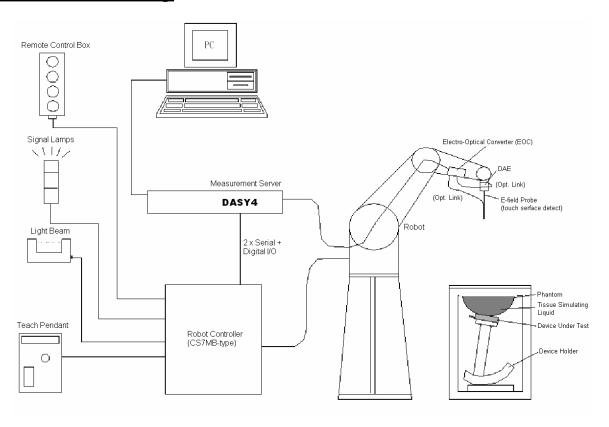


Fig. 5.1 DASY4 system



The DASY4 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- The electro-optical converter (ECO) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the accuracy of the probe positioning
- ➤ A computer operating Windows XP
- DASY4 software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- The SAM twin phantom
- ➤ A device holder
- Tissue simulating liquid
- Dipole for evaluating the proper functioning of the system

Some of the components are described in details in the following sub-sections.

5.1 DASY4 E-Field Probe System

The SAR measurement is conducted with the dosimetric probe EX3DV3 (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency.



5.1.1 <u>EX3DV3 E-Field Probe Specification</u>

<EX3DV3 Probe>

Construction Symmetrical design with triangular core

Built-in shielding against static charges

PEEK enclosure material (resistant to organic solvents)

Calibration Basic Broad Band Calibration in air:

10-3000 MHz Conversion Factors (CF) for HSL 900 and HSL 1800 Additional CF for other liquids and frequencies upon request

Frequency 10 MHz to > 6 GHz; Linearity: $\pm 0.2 \text{ dB}$

(30 MHz to 3 GHz)

Directivity ± 0.3 dB in HSL (rotation around probe

axis)

 \pm 0.5 dB in tissue material (rotation normal

to probe axis)

 $\label{eq:def_power_power} \textbf{Dynamic Range} \qquad \qquad 10~\mu\text{W/g to} > 100~\text{mW/g; Linearity:} \pm 0.2$

dB (noise: typically $< 1 \mu W/g$)

Dimensions Overall length: 330 mm (Tip: 20 mm)

Tip diameter: 2.5 mm (Body: 12 mm)
Typical distance from probe tip to dipole

centers: 1 mm

Application High precision dosimetric measurements in

any exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6 GHz with precision of better 30%.



Test Report No : FA691116-1-2-07

Fig. 5.2 EX3DV3 E-field Probe

5.1.2 EX3DV3 E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy shall be evaluated and within \pm 0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data are as below:



<EX3DV3 Probe>

Sensitivity	X axis : 0.6			s : 0.675 μV	Z axis : 0.598 μV
Diode compression point	X axis : 97			xis : 97 mV	Z axis : 97 mV
	Frequency (MHz)	X axis		Y axis	Z axis
Conversion factor	5100~5300	4.3	5	4.35	4.35
(Body)	5400~5600	4.02		4.02	4.02
	5700~5900	4.09	9	4.09	4.09
	Frequency (MHz)	Alp	ha	Depth	
Boundary effect	5100~5300	0.4	7	1.25	
(Body)	5400~5600	0.4	6	1.14	
	5700~5900	0.52	2	0.92	

NOTE: The probe parameters have been calibrated by the SPEAG.

5.2 DATA Acquisition Electronics (DAE)

The data acquisition electronics (DAE4) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.



5.3 <u>Robot</u>

The DASY4 system uses the high precision robots RX90BL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASYS system, the CS7MB robot controller version from Stäubli is used. The RX robot series have many features that are important for our application:

- ➤ High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- > Low ELF interference (the closed metallic construction shields against motor control fields)
- ► 6-axis controller

5.4 Measurement Server

The DASY4 measurement server is based on a PC/104 CPU board with 166 MHz CPU 32 MB chipset and 64 MB RAM.

Communication with the DAE4 electronic box

the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.

5.5 SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- Left head
- Right head
- > Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections.

Test Report No : FA691116-1-2-07

A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters.

On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids:

- *Water-sugar based liquid
- *Glycol based liquids

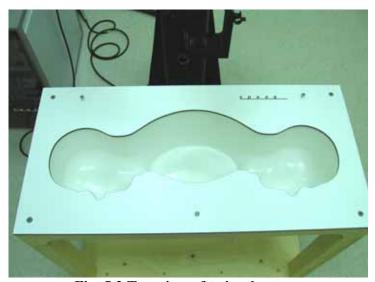


Fig. 5.3 Top view of twin phantom



Fig. 5.4 Bottom view of twin phantom



5.6 <u>Data Storage and Evaluation</u>

5.6.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The postprocessing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a loseless media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

5.6.2 Data Evaluation

The DASY4 postprocessing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters:	- Sensitivity	$Norm_i, a_{i0}, a_{i1}, a_{i2}$
	- Conversion factor	$ConvF_i$
	- Diode compression point	dep_i
Device parameters:	- Frequency	f
	- Crest factor	cf

Media parameters: - Conductivity σ - Density ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used. The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest

factor of the signal must be known to correctly compensate for peak power. The formula for each channel



can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with

 V_i = compensated signal of channel i (i = x, y, z)

 U_i = input signal of channel i (i = x, y, z)

cf = crest factor of exciting field (DASY parameter)

 $dcp_i = diode\ compression\ point\ (DASY\ parameter)$

From the compensated input signals, the primary field data for each channel can be evaluated:

E-field probes : $E_i = \sqrt{\frac{V_i}{Norm_i ConvF}}$

H-field probes: $H_i = \sqrt{V_i} \frac{a_{i0+} a_{i1} f + a_{i2} f^2}{f}$

with

 V_i = compensated signal of channel i (i = x, y, z)

 $Norm_i$ = sensor sensitivity of channel i (i = x, y, z)

 $\mu V/(V/m)$ 2 for E-field Probes

ConvF = sensitivity enhancement in solution

 a_{ii} = sensor sensitivity factors for H-field probes

f = carrier frequency [GHz]

 E_i = electric field strength of channel *i* in V/m

 H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_{v}^{2} + E_{v}^{2} + E_{z}^{2}}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with

SAR = local specific absorption rate in mW/g

Etot = total field strength in V/m

 $\sigma = \text{conductivity in [mho/m] or [Siemens/m]}$

 ρ = equivalent tissue density in g/ cm³



*Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or $P_{pwe} = H_{tot}^2 \cdot 37.7$

with P_{pwe} = equivalent power density of a plane wave in mW/cm²

 E_{tot} = total electric field strength in V/m

 H_{tot} = total magnetic field strength in A/m

FORTON LAB. FCC SAR Test Report Test Report No : FA691116-1-2-07

5.7 Test Equipment List

Manufacture	Name of Equipment	Type/Model	Serial Number	Calibration		
Manufacture	Name of Equipment	aipment Type/Woder Serial Nun		Last Cal.	Due Date	
SPEAG	Dosimetric E-Filed Probe	EX3DV3	3514	Feb. 17, 2006	Feb. 17, 2008	
SPEAG	SPEAG 835MHz System Validation Kit		499	Mar. 15, 2006	Mar. 15, 2008	
SPEAG	900MHz System Validation Kit	D900V2	190	Jul. 19, 2005	Jul. 19, 2007	
SPEAG	1800MHz System Validation Kit	D1800V2	2d076	Jul. 20, 2005	Jul. 20, 2007	
SPEAG	1900MHz System Validation Kit	D1900V2	5d041	Mar. 21, 2006	Mar. 21, 2008	
SPEAG	2000MHz System Validation Kit	D2000V2	1010	Oct. 25, 2004	Oct. 25, 2006	
SPEAG	2450MHz System Validation Kit	D2450V2	736	Jul. 12, 2005	Jul. 12, 2007	
SPEAG	SPEAG 5GHz System Validation Kit		1006	Feb. 10, 2006	Feb. 10, 2008	
SPEAG	SPEAG Data Acquisition Electronics		577	Nov. 11, 2005	Nov. 11, 2006	
SPEAG	Device Holder	N/A	N/A	NCR	NCR	
SPEAG	SPEAG Phantom		TP-1150	NCR	NCR	
SPEAG	SPEAG Robot		F03/5W15A1/A/01	NCR	NCR	
SPEAG			N/A	NCR	NCR	
SPEAG	SPEAG Software		N/A	NCR	NCR	
SPEAG	Measurement Server	SE UMS 001 BA	1021	NCR	NCR	
Agilent	ENA series Network Analyzer	E5071B	MY42403579	Mar. 16, 2006	Mar. 16, 2007	
Agilent	Dielectric Probe Kit	85070D	US01440205	NCR	NCR	
Agilent	Dual Directional Coupler	778D 8449B	50422	NCR	NCR	
Agilent	Agilent Power Amplifier		3008A01917	NCR	NCR	
Agilent Power Meter		E4416A	GB41292344	Jan. 23, 2006	Jan. 23, 2008	
Agilent	Power Sensor	E9327A	US40441548	Feb. 06, 2006	Feb. 06, 2007	
Agilent	Signal Generator	E8247C	MY43320596	Mar. 01, 2006	Mar. 01, 2008	
R&S	Spectrum Analyzer	FSP30	100023	Nov. 26, 2005	Nov. 26, 2006	
R&S	Power Meter	NRVS	100764	Jul. 20, 2006	Jul. 20, 2007	
R&S	Power Sensor	NRV-Z32	100057	Jun. 10, 2006	Jun. 10, 2007	

Table 5.1 Test Equipment List

6. Tissue Simulating Liquids

For the measurement of the field distribution inside the SAM phantom with DASY4, the phantom must be filled with around 25 liters of homogeneous body tissue simulating liquid. The liquid height from the bottom of the phantom body is 15.2 centimeters.

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070D Dielectric Probe Kit and an Agilent Network Analyzer.

Table 6.1 shows the measuring results for muscle simulating liquid.

Bands	Frequency(MHz)	Permittivity (ε_{r})	Conductivity (\sigma)	Measurement date
5150 ~ 5250 MHz	5180	49.0	5.27	
<Band 1>	5200	49.0	5.30	Sep. 21, 2006
Spand 1/	5240	48.9	5.34	_
5705 5005 MII-	5745	48.3	5.94	
5725 ~ 5825 MHz <band 3=""></band>	5785	48.2	5.97	Sep. 21, 2006
Sand 3	5825	48.1	6.02	_

Table 6.1

The measuring data are consistent with ε_r = 49.0 ± 5% and σ = 5.30 ± 5% for 5GHz band 1 and ε_r = 48.2 ± 5% and σ = 6.0 ± 5% for 5GHz band 3.



7. Uncertainty Assessment

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 7.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor ^(a)	1/k (b)	1/√3	1/√6	1/√2

⁽a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity

Table 7.1

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY4 uncertainty Budget is showed in Table 7.2.

⁽b) \mathcal{K} is the coverage factor



Error Description	Uncertainty Value	Probability Distribution	Divisor	Ci (1g)	Standard Unc. (1g)	Vi or Veff
Measurement System						
Probe Calibration	±6.8 %	Normal	1	1	±6.8 %	∞
Axial Isotropy	±4.7 %	Rectangular	√3	0.7	±1.9 %	∞
Hemispherical Isotropy	±9.6 %	Rectangular	√3	0.7	±3.9 %	∞
Boundary Effect	±2.0 %	Rectangular	√3	1	±1.2 %	∞
Linearity	±4.7 %	Rectangular	√3	1	±2.7 %	∞
System Detection Limit	±1.0 %	Rectangular	√3	1	±0.6 %	∞
Readout Electronics	±0.3 %	Normal	1	1	±0.3 %	∞
Response Time	±0.8 %	Rectangular	√3	1	± 0.5 %	∞
Integration Time	±2.6 %	Rectangular	√3	1	± 1.5 %	∞
RF Ambient Noise	±3.0 %	Rectangular	√3	1	±1.7 %	∞
RF Ambient Reflections	±3.0 %	Rectangular	√3	1	±1.7 %	∞
Probe Positioner	±0.8 %	Rectangular	√3	1	±0.5 %	∞
Probe Positioning	±9.9 %	Rectangular	√3	1	±5.7 %	∞
Max. SAR Eval.	±4.0 %	Rectangular	√3	1	±2.3 %	∞
Test Sample Related			•			
Device Positioning	±2.9 %	Normal	1	1	±2.9 %	145
Device Holder	±3.6 %	Normal	1	1	±3.6 %	5
Power Drift	±5.0 %	Rectangular	√3	1	±2.9 %	∞
Phantom and Setup			•			
Phantom Uncertainty	±4.0 %	Rectangular	√3	1	±2.3 %	∞
Liquid Conductivity (target)	±5.0 %	Rectangular	√3	0.64	±1.8 %	∞
Liquid Conductivity (meas.)	±2.5 %	Normal	1	0.64	±1.6 %	∞
Liquid Permittivity (target)	±5.0 %	Rectangular	√3	0.6	±1.7 %	∞
Liquid Permittivity (meas.)	±2.5 %	Normal	1	0.6	±1.5 %	∞
Combined Std. Uncertainty					±12.9 %	330
Expanded STD Uncertainty					±25.9 %	

Table 7.2 Uncertainty Budget of DASY4 for 5GHz Band



8. SAR Measurement Evaluation


Each DASY system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

8.1 Purpose of System Performance check

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

8.2 System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave which comes from a signal generator at frequency 5200 MHz and 5800 MHz. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

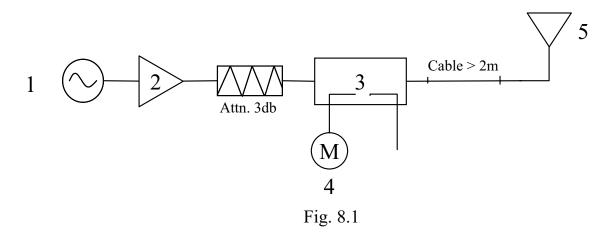



- 1. Signal Generator
- 2. Amplifier
- 3. Directional Coupler
- 4. Power Meter
- 5. 5200 MHz and 5800 MHz Dipole

The output power on dipole port must be calibrated to 100 mW (20 dBm) before dipole is connected.



Fig 8.2 Dipole Setup

8.3 Validation Results

Comparing to the original SAR value provided by Speag, the validation data should within its specification of 10 %. Table 8.1 shows the target SAR and measured SAR after normalized to 1W input power.

Band		Target (W/kg)	Measurement data (W/kg)	Variation	Measurement date	
Band 1	SAR (1g)	73.7	73.8	0.1 %	San 21 2006	
(5200 MHz)	SAR (10g)	20.6	20.5	-0.5 %	Sep. 21, 2006	
Band 3	SAR (1g)	69.8	70.3	0.7 %	San 21 2006	
(5800 MHz)	SAR (10g)	19.7	19.2	-2.5 %	Sep. 21, 2006	

Table 8.1

The table above indicates the system performance check can meet the variation criterion.



9. Description for DUT Testing Position

This DUT was tested in 4 different positions. They are "Keypad Up with Touch with Scanner A" shown in Fig. 9.1, "Keypad Down with Touch with Scanner A" shown in Fig. 9.2, "Keypad Up with Touch with Scanner B" shown in Fig. 9.3 and "Keypad Up with Touch with Scanner B and Wrist Mount" shown in Fig. 9.4. The DUT face to the phantom with 0 mm separation distance.



Fig. 9.1 Keypad Up with Touch with Scanner A



Fig. 9.2 Keypad Down with Touch with Scanner A





Fig. 9.3 Keypad Up with Touch with Scanner B



Fig. 9.4 Keypad Up with Touch with Scanner B and Wrist Mount



10. Measurement Procedures

The measurement procedures are as follows:

- > Using engineering software to transmit RF power continuously (continuous Tx) in the middle channel
- Placing the DUT in the positions described in the last section
- > Setting scan area, grid size and other setting on the DASY4 software
- > Taking data for the middle channel
- Repeat the previous steps for the low and high channels.


According to the IEEE P1528 draft standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- > Power reference measurement
- Area scan
- > Zoom scan
- Power reference measurement

10.1 Conducted Power Measurement

10.1.1 For 47 CFR FCC Part 15 Subpart E §15.407 (5150 ~ 5250 MHz)

10.1.1.1 Test Setup Layout



10.1.1.2 Setting of the Spectrum

Spectrum Parameter	Setting
Attenuation	Auto
Span Frequency	Encompass the entire emissions bandwidth (EBW) of the signal
RB	1000 kHz
VB	3000 kHz
Detector	Sample
Trace	Average
Sweep Time	20ms Trace Average 100 times


10.1.1.3 Test Procedures

- 1. The transmitter output (antenna port) was connected to the spectrum analyzer.
- 2. Test was performed in accordance with method #1 of FCC Public Notice DA 02-2138.



10.1.2 For 47 CFR FCC Part 15 Subpart E §15.247 (5725 ~ 5825 MHz)

10.1.2.1 Test Setup Layout



10.1.2.2 Setting of the Power Meter

- 5000000 01 0000 1 0 00 01 101000	^
Power Meter Parameter	Setting
Filter No.	Auto
Measurement Time	0.135s - 26s
Used Peak Sensor	NRV-Z32 (model 04)

10.1.2.3 Test Procedures

- 1. The transmitter output (antenna port) was connected to the power meter.
- 2. Turn on the EUT and power meter and then record the peak power value.
- 3. Repeat above procedures on all channels needed to be tested.

10.2 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1528-2003 standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

Base on the Draft: SCC-34, SC-2, WG-2-Computational Dosimetry, P1528/D1.2 (Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques), a new algorithm has been implemented. The spatial-peak SAR can be computed over any required mass.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.



The entire evaluation of the spatial peak values is performed within the postprocessing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- extraction of the measured data (grid and values) from the Zoom Scan
- calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- generation of a high-resolution mesh within the measured volume
- interpolation of all measured values form the measurement grid to the high-resolution grid
- extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- calculation of the averaged SAR within masses of 1g and 10g

10.3 Scan Procedures

First **Area Scan** is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an **Area Scan** is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, **Zoom Scan** is required. The **Zoom Scan** measures 5x5x7 points with step size 8, 8 and 5 mm for 2.45GHz Band and 8x8x8 points with step size 4.3, 4.3 and 3 mm for 5GHz Band. The **Zoom Scan** is performed around the highest E-field value to determine the averaged SAR-distribution over 1 g.

10.4 SAR Averaged Methods

In DASY4, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.



11.SAR Test Results

11.1 Keypad Up with Touch with Scanner A

Mode	Chan.	Freq (MHz)	Modulation Type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limit (W/kg)	Results
Band 1	36	5180 (Low)	OFDM	13.16	-	-	-	-
	40	5200 (Mid)	OFDM	13.08	-0.124	0.587	1.6	Pass
	48	5240 (High)	OFDM	12.46	-	-	-	-
Band 3	149	5745 (Low)	OFDM	16.88	-	-	-	-
	157	5785 (Mid)	OFDM	17.71	-	-	-	-
	165	5825 (High)	OFDM	17.68	-	-	-	-

11.2 Keypad Down with Touch with Scanner A

1.2 Acypua Down with Touch with Scattler 11									
Mode	Chan.	Freq (MHz)	Modulation Type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limit (W/kg)	Results	
Band 1	36	5180 (Low)	OFDM	13.16	-	-	-	-	
	40	5200 (Mid)	OFDM	13.08	0.162	0.028	1.6	Pass	
	48	5240 (High)	OFDM	12.46	-	-	-	-	
Band 3	149	5745 (Low)	OFDM	16.88	-	-	-	-	
	157	5785 (Mid)	OFDM	17.71	-	-	-	-	
	165	5825 (High)	OFDM	17.68	-	-	-	-	

11.3 Keypad Up with Touch with Scanner B

$11.5 \frac{\text{Heypt}}{\text{P}}$	$m \circ p$	viin Touch v	viin Scanne	<u>, , , , , , , , , , , , , , , , , , , </u>				
Mode	Chan.	Freq (MHz)	Modulation Type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limit (W/kg)	Results
Band 1	36	5180 (Low)	OFDM	13.16	0.125	0.566	1.6	Pass
	40	5200 (Mid)	OFDM	13.08	-0.117	0.589	1.6	Pass
	48	5240 (High)	OFDM	12.46	0.127	0.601	1.6	Pass
Band 3	149	5745 (Low)	OFDM	16.88	-0.126	0.68	1.6	Pass
	157	5785 (Mid)	OFDM	17.71	0.105	0.666	1.6	Pass
	165	5825 (High)	OFDM	17.68	0.188	0.592	1.6	Pass
Band 3 with BT On	149	5745 (Low)	OFDM	16.88	0.13	0.663	1.6	Pass

11.4 Keypad Up with Touch with Scanner B and Wrist Mount

Mode	Chan.	Freq (MHz)	Modulation Type	Conducted Power (dBm)	Power Drift (dB)	Measured 1g SAR (W/kg)	Limit (W/kg)	Results
Band 1	36	5180 (Low)	OFDM	13.16	-	-	-	-
	40	5200 (Mid)	OFDM	13.08	0.183	0.459	1.6	Pass
	48	5240 (High)	OFDM	12.46	-	-	-	-
Band 3	149	5745 (Low)	OFDM	16.88	-	-	-	-
	157	5785 (Mid)	OFDM	17.71	-	-	-	-
	165	5825 (High)	OFDM	17.68	-	-	-	-

<u>Test Engineer</u>: Gordon Lin



12. References

- [1] FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2] IEEE Std. P1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", April 21,2003.
- [3] Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01), "Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to RF Emissions", June 2001
- [4] IEEE Std. C95.3-2002, "IEEE Recommended Practice for the Meaurement of Potentially Hazardous Electromagnetic Fields-RF and Microwave", 2002
- [5] IEEE Std. C95.1-1999, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", 1999
- [6] Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148
- [7] DAYS4 System Handbook

Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 9/21/2006 9:03:15 AM

System Check Body 5200MHz 20060921

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1006

Communication System: CW; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: MSL_5G Medium parameters used: f = 5200 MHz; $\sigma = 5.3$ mho/m; $\epsilon_r = 49$; $\rho = 1000$ kg/m³

Ambient Temperature: 21.6°C; Liquid Temperature: 21.0°C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.35, 4.35, 4.35); Calibrated: 2/17/2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 15.1 mW/g


Pin=100mW/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 56.8 V/m; Power Drift = -0.119 dB

Peak SAR (extrapolated) = 30.5 W/kg

SAR(1 g) = 7.38 mW/g; SAR(10 g) = 2.05 mW/g

Maximum value of SAR (measured) = 14.2 mW/g

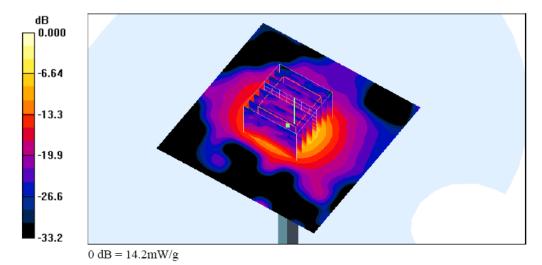

Date/Time: 9/21/2006 9:47:45 AM Test Laboratory: Sporton International Inc. SAR Testing Lab

System Check_Body_5800MHz_20060921

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1006

Communication System: 802.11a; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: MSL_5G Medium parameters used: f = 5800 MHz; $\sigma = 5.99 \text{ mho/m}$; $\varepsilon_r = 48.2$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 21.7 °C; Liquid Temperature: 21.0 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.09, 4.09, 4.09); Calibrated: 2/17/2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161


Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 15.0 mW/g

Pin=100mW/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 50.6 V/m; Power Drift = -0.099 dB

Peak SAR (extrapolated) = 34.5 W/kg

SAR(1 g) = 7.03 mW/g; SAR(10 g) = 1.92 mW/gMaximum value of SAR (measured) = 14.3 mW/g

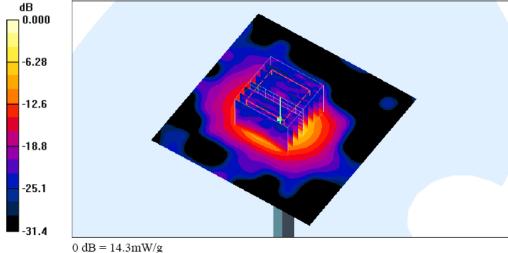

Appendix B - SAR Measurement Data

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 9/21/2006 10:53:16 AM

Body 802.11a Ch40 Keypad Up with Touch with Scanner A 20060921

DUT: 691116

Communication System: 802.11a; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: MSL_5G Medium parameters used: f = 5200 MHz; $\sigma = 5.3$ mho/m; $\epsilon_r = 49$; $\rho = 1000$ kg/m³

Ambient Temperature: 21.4°C; Liquid Temperature: 20.9°C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.35, 4.35, 4.35); Calibrated: 2/17/2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch40/Area Scan (121x171x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 1.14 mW/g


Ch40/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 1.95 V/m; Power Drift = -0.124 dB

Peak SAR (extrapolated) = 2.23 W/kg

SAR(1 g) = 0.587 mW/g; SAR(10 g) = 0.189 mW/g

Maximum value of SAR (measured) = 1.14 mW/g

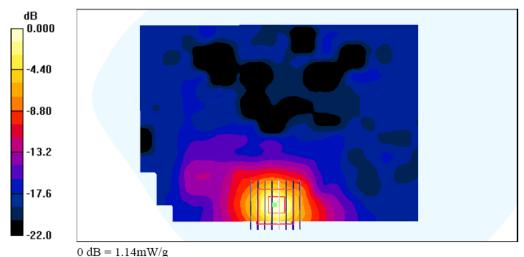

0 dB = 1.14 HeW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 9/21/2006 11:45:15 AM

Body 802.11a Ch40 Keypad Down with Touch with Scanner A 20060921

DUT: 691116

Communication System: 802.11a; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: MSL_5G Medium parameters used: f = 5200 MHz; $\sigma = 5.3$ mho/m; $\varepsilon_r = 49$; $\rho = 1000$ kg/m³

Ambient Temperature: 21.4 °C; Liquid Temperature: 21.0 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.35, 4.35, 4.35); Calibrated: 2/17/2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch40/Area Scan (121x171x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 0.054 mW/g

Ch40/Zoom Scan (8x8x8)/Cube 1: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 1.15 V/m; Power Drift = 0.162 dB

Peak SAR (extrapolated) = 0.063 W/kg


SAR(1 g) = 0.028 mW/g; SAR(10 g) = 0.018 mW/gMaximum value of SAR (measured) = 0.046 mW/g

Ch40/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 1.15 V/m; Power Drift = 0.162 dB

Peak SAR (extrapolated) = 0.086 W/kg

SAR(1 g) = 0.028 mW/g; SAR(10 g) = 0.012 mW/gMaximum value of SAR (measured) = 0.049 mW/g

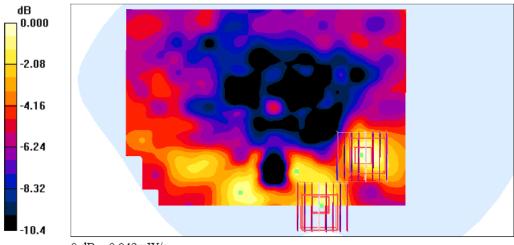

0 dB = 0.049 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 9/21/2006 4:04:41 PM

Body 802.11a Ch48 Keypad Up with Touch with Scanner B 20060921

DUT: 691116

Communication System: 802.11a; Frequency: 5240 MHz; Duty Cycle: 1:1

Medium: MSL_5G Medium parameters used : f = 5240 MHz; $\sigma = 5.34$ mho/m; $\epsilon_r = 48.9$; $\rho = 1000$ kg/m³

Ambient Temperature: 20.1 °C; Liquid Temperature: 21.0 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.35, 4.35, 4.35); Calibrated: 2/17/2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch48/Area Scan (121x171x1): Measurement grid: dx=10mm, dy=10mm


Maximum value of SAR (interpolated) = 1.08 mW/g

Ch48/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 1.44 V/m; Power Drift = 0.127 dB

Peak SAR (extrapolated) = 2.43 W/kg

SAR(1 g) = 0.601 mW/g; SAR(10 g) = 0.189 mW/gMaximum value of SAR (measured) = 1.20 mW/g

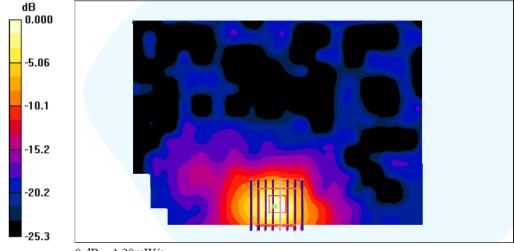

0 dB = 1.20 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 9/21/2006 4:50:34 PM

Body 802.11a Ch149 Keypad Up with Touch with Scanner B 20060921

DUT: 691116

Communication System: 802.11a; Frequency: 5745 MHz; Duty Cycle: 1:1

Medium: MSL_5G Medium parameters used: f = 5745 MHz; $\sigma = 5.94$ mho/m; $\epsilon_r = 48.3$; $\rho = 1000$ kg/m³

Ambient Temperature: 20.0 °C; Liquid Temperature: 21.0 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.09, 4.09, 4.09); Calibrated: 2/17/2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch149/Area Scan (121x171x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 1.37 mW/g


Ch149/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 1.95 V/m; Power Drift = -0.126 dB

Peak SAR (extrapolated) = 3.24 W/kg

SAR(1 g) = 0.680 mW/g; SAR(10 g) = 0.208 mW/g

Maximum value of SAR (measured) = 1.29 mW/g

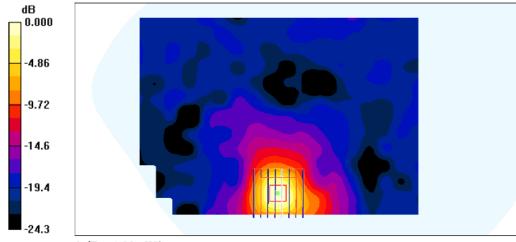

0 dB = 1.29 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 9/21/2006 2:33:47 PM

Body_802.11a Ch40_Keypad Up with Touch with Scanner B and Wrist Mount_20060921

DUT: 691116

Communication System: 802.11a; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: MSL 5G Medium parameters used: f = 5200 MHz; $\sigma = 5.3 \text{ mho/m}$; $\varepsilon_r = 49$; $\rho = 1000 \text{ kg/m}^3$

Ambient Temperature: 20.4 °C; Liquid Temperature: 21.0 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.35, 4.35, 4.35); Calibrated: 2/17/2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161


Ch40/Area Scan (121x171x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.930 mW/g

Ch40/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 1.56 V/m; Power Drift = 0.183 dB

Peak SAR (extrapolated) = 1.79 W/kg

SAR(1 g) = 0.459 mW/g; SAR(10 g) = 0.150 mW/gMaximum value of SAR (measured) = 0.902 mW/g

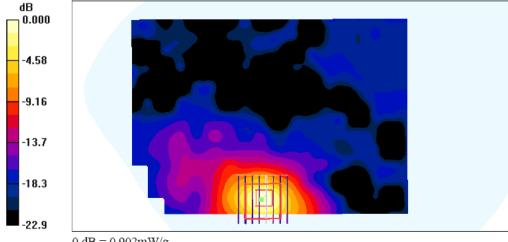

0 dB = 0.902 mW/g



Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 9/21/2006 6:54:26 PM

Body 802.11a Ch149 Keypad Up with Touch with Scanner B 20060921 BT On

DUT: 691116

Communication System: 802.11a; Frequency: 5745 MHz; Duty Cycle: 1:1

Medium: MSL_5G Medium parameters used: f = 5745 MHz; $\sigma = 5.94$ mho/m; $\epsilon_r = 48.3$; $\rho = 1000$ kg/m³

Ambient Temperature: 22.0 °C; Liquid Temperature: 22.0 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.09, 4.09, 4.09); Calibrated: 2/17/2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161

Ch149/Area Scan (121x171x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 1.27 mW/g


Ch149/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 1.57 V/m; Power Drift = 0.13 dB

Peak SAR (extrapolated) = 3.22 W/kg

SAR(1 g) = 0.663 mW/g; SAR(10 g) = 0.204 mW/g

Maximum value of SAR (measured) = 1.32 mW/g

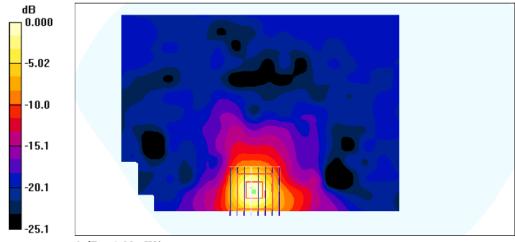

0 dB = 1.32 mW/g

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 9/21/2006 4:04:41 PM

Body_802.11a Ch48_Keypad Up with Touch with Scanner B_20060921_2D

DUT: 691116

Communication System: 802.11a; Frequency: 5240 MHz; Duty Cycle: 1:1

Medium: MSL_5G Medium parameters used : f = 5240 MHz; $\sigma = 5.34$ mho/m; $\varepsilon_r = 48.9$; $\rho = 1000$ kg/m³

Ambient Temperature: 20.1 °C; Liquid Temperature: 21.0 °C

DASY4 Configuration:

- Probe: EX3DV3 SN3514; ConvF(4.35, 4.35, 4.35); Calibrated: 2/17/2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/11/2005
- Phantom: SAM-A; Type: QD 000 P40 C; Serial: TP-1303
- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 161


Ch48/Area Scan (121x171x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 1.08 mW/g

Ch48/Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 1.44 V/m; Power Drift = 0.127 dB

Peak SAR (extrapolated) = 2.43 W/kg

SAR(1 g) = 0.601 mW/g; SAR(10 g) = 0.189 mW/gMaximum value of SAR (measured) = 1.20 mW/g

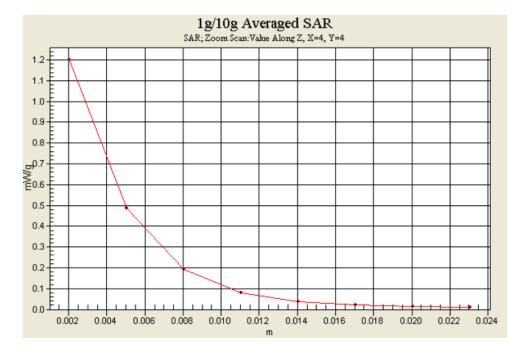



Appendix C – Calibration Data



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swise Federal Office of Metrology and Accreditation.

The Swise Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates.

Client

Sporton (Auden)

Accreditation No.: SCS 108

Cartificate No: D5GHzV2-1006_Feb06

CALIBRATION CERTIFICATE

Object D5GHzV2 - SN; 1006

Calibration procedure(s) QA CAL-22.v1
Calibration procedure for dipole validation kits between 3-6 GHz

Calibration date: February 10, 2006

Condition of the calibrated item In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Call Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	3-May-05 (METAS, No. 251-00466)	May-56
Power sensor E4412A	MY41495277	3-May-05 (METAS, No. 251-00466)	Moy-06
Reference 20 dB Attenuator	SN: S5086 (20b)	3-May-05 (METAS, No. 251-00467)	May-06
Reference 10 dB Attenuator	SN: 5047.2 (10r)	11-Aug-05 (METAS, No 251-00498)	Aug-06
Reference Probe EX3DV4	SN 3503	19-Mar-05 (SPEAG, No. Ex3-3503_Mar05)	Mor-06
DAE4	SN 601	15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	Dec-06
Secondary Standards	ID#	Check Date (in house)	Schoduled Check
Power sensor HP 8481A	MY41093315	10-Aug-03 (SPEAG, in house check Oct-05)	In house check: Oct-06
Power meter E4419B	G843310788	12-Aug-03 (SPEAG, in house check Oct-05)	In house check: Oct-06
RF generator R&S SMT-06	100005	4-Aug-99 (SPEAG, in house check Nov-05)	In house check: Nov-07
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (SPEAG, in house check Nov-05)	In house check: Nov-06
	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	20. Kg
• ************	All No. 14 and 15	# W. M. A	1/15
Approved by:	Niels Kuster	Quality Manager	1.160

Certificate No: D5GHzV2-1006_Feb06

Page 1 of 7

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Issued: February 17, 2006



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43; 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation. The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates.

Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z

N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC Std 62209 Part 2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", Draft Version 0.9, December 2004
- b) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D5GHzV2-1006_Feb06

Page 2 of 7

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 10 mm	
Zoom Scan Resolution	dx, dy = 4.3 mm, dz = 3 mm	
Frequency	5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Body TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	49.0	5.30 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	49.1 ± 6 %	5.11 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		****

SAR result with Body TSL at 5200 MHz

SAR averaged over 1 cm3 (1 g) of Body TSL	condition	
SAR measured	250 mW input power	1840 mW/g
SAR normalized	normalized to 1W	73.6 mW/g
SAR for nominal Body TSL parameters 1	normalized to 1W	73.7 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ² (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.16 mW/g
SAR normalized	normalized to 1W	20.6 mW/g
SAR for nominal Body TSL parameters 1	normalized to 1W	20.6 mW / g ± 19.5 % (k=2)

Certificate No: D5GHzV2-1006_Feb06

Body TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.6	5.65 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.4 ± 6 %	5.50 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		_

SAR result with Body TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	condition	
SAR measured	250 mW input power	18.8 mW / g
SAR normalized	normalized to 1W	75.2 mW / g
SAR for nominal Body TSL parameters 1	normalized to 1W	75.0 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm3 (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.26 mW / g
SAR normalized	normalized to 1W	21.0 mW / g
SAR for nominal Body TSL parameters 1	normalized to 1W	21.0 mW / g ± 19.5 % (k=2)

Body TSL parameters at 5800 MHz
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.2	6.00 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.8 ± 6 %	5.88 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		_

SAR result with Body TSL at 5800 MHz

SAR averaged over 1 cm2 (1 g) of Body TSL	-condition	
SAR measured	250 mW input power	17.5 mW / g
SAR normalized	normalized to 1W	70.0 mW / g
SAR for nominal Body TSL parameters 1	normalized to 1W	69.8 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm3 (10 g) of Body TSL	condition	
SAR measured	250 mW input power	4.94 mW / g
SAR normalized	normalized to 1W	19.8 mW / g
SAR for nominal Body TSL parameters 1	normalized to 1W	19.7 mW / g ± 19.5 % (k=2)

Certificate No: D5GHzV2-1006_Feb06

Page 4 of 7

Appendix

Antenna Parameters with Body TSL at 5200 MHz

Impedance, transformed to feed point	48.3 Ω - 2.2]Ω	
Return Loss	-31.1 dB	

Antenna Parameters with Body TSL at 5500 MHz

Impedance, transformed to feed point	54.1 Ω - 9.4jΩ	
Return Loss	-20.1 dB	

Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	56.3 Ω + 8.3jΩ	
Return Loss	-20.1 dB	-5

General Antenna Parameters and Design

Electrical Delay (one direction)	1.202 ns

After long term use with 40 W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard samirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 28, 2003

Certificate No: D5GHzV2-1006_Feb06

Page 5 of 7

DASY4 Validation Report for Body TSL

Date/Time: 10.02.2006 21:06:10

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1006

Communication System: CW-5GHz; Frequency: 5800 MHz Frequency: 5500 MHz Frequency: 5200 MHz;

Duty Cycle: 1:1

Medium: MSL 5800 MHz:

Medium parameters used: f = 5800 MHz; $\sigma = 5.88 \text{ mho/m}$; $\epsilon_r = 47.8$; $\rho = 1000 \text{ kg/m}^3 \text{ Medium parameters}$ used: f = 5500 MHz; $\sigma = 5.5 \text{ mho/m}$; $\epsilon_r = 48.4$; $\rho = 1000 \text{ kg/m}^2 \text{ Medium parameters used: } f = 5200 \text{ MHz}$; $\sigma =$

5.11 mho/m; $\epsilon_r = 49.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: EX3DV4 SN3503; ConvF(4.69, 4.69, 4.69)ConvF(4.78, 4.78, 4.78)ConvF(5.18, 5.18, 5.18); Calibrated: 19.03.2005
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 15.12.2005
- Phantom: Flat Phantom 5.0 (back); Type: QD000PS0AA
- Measurement SW: DASY4, V4.6 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 160

d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=2mm (8x8x8)/Cube 0:

Measurement grid: dx-4.3mm, dy-4.3mm, dz-3mm Reference Value = 77.8 V/m; Power Drift = -0.025 dB

Peak SAR (extrapolated) = 65.4 W/kg

SAR(1 g) = 18.4 mW/g; SAR(10 g) = 5.16 mW/g

Maximum value of SAR (measured) = 37.8 mW/g

d=10mm, Pin=250mW, f=5500 MHz/Zoom Scan (8x8x8), dist=2mm (8x8x8)/Cube 0:

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 73.9 V/m; Power Drift = 0.003 dB

Peak SAR (extrapolated) = 72.9 W/kg

SAR(1 g) = 18.8 mW/g; SAR(10 g) = 5.26 mW/g

Maximum value of SAR (measured) = 39.6 mW/g

d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=2mm (8x8x8)/Cube 0;

Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 69.5 V/m; Power Drift = -0.024 dB

Peak SAR (extrapolated) = 70.0 W/kg


SAR(1 g) = 17.5 mW/g; SAR(10 g) = 4.94 mW/g

Maximum value of SAR (measured) = 36.7 mW/g

Certificate No: D5GHzV2-1006 Feb06

Page 6 of 7

Impedance Measurement Plot for Body TSL

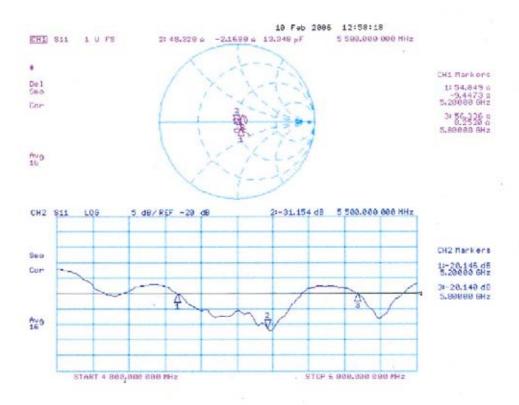

Certificate No: D5GHzV2-1006_Feb06

Page 7 of 7

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

Client Sporton (Auden)

Certificate No: EX3-3514_Feb06

Object	EX3DV3 - SN:3	514	
Calibration procedure(s)	A COMPANY OF THE PROPERTY OF T	and QA CAL-14.v3 edure for dosimetric E-field probes	
Calibration date:	February 17, 20	06	temak port
Condition of the calibrated item	In Tolerance		
CIVIT-CORPONERS THEORY	24.0846	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration May-06
Primary Standards Power meter E4419B	24.0846	3-May-05 (METAS, No. 251-00466)	Scheduled Calibration May-06 May-06
Primary Standards Power meter E4419B Power sensor E4412A	ID # GB41293874		May-06
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A	ID # GB41293874 MY41495277	3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466)	May-06 May-06
Primary Standards Power meter E44196 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	ID # GB41293874 MY41495277 MY41498087	3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466)	May-06 May-06 May-06
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c)	3-Msy-05 (METAS, No. 251-00466) 3-Msy-05 (METAS, No. 251-00466) 3-Msy-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499)	May-06 May-06 May-06 Aug-06
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	3-May-05 (METAS, No. 251-00486) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467)	May-06 May-06 May-06 Aug-06 May-06
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2	ID # GB41293B74 MY41495277 MY414980B7 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b)	3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500)	May-06 May-06 May-06 Aug-06 May-06 Aug-06
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	ID # GB41293874 MY41495277 MY41495087 SN: \$5054 (3c) SN: \$5086 (20b) SN: \$5129 (30b) SN: 3013 SN: 654	3-May-05 (METAS, No. 251-00486) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house)	May-06 May-06 May-06 Aug-06 May-06 Aug-08 Jan-07 Feb-07 Scheduled Check
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5066 (20b) SN: S5129 (30b) SN: 3D13 SN: 654 ID # US3642U01700	3-May-05 (METAS, No. 251-00486) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house)	May-06 May-06 May-06 Aug-06 Aug-06 Aug-06 Jan-07 Feb-07 Scheduled Check In house check: Nov-07
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID # GB41293874 MY41495277 MY41495087 SN: \$5054 (3c) SN: \$5086 (20b) SN: \$5129 (30b) SN: 3013 SN: 654	3-May-05 (METAS, No. 251-00486) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house)	May-06 May-06 May-06 Aug-06 May-06 Aug-08 Jan-07 Feb-07 Scheduled Check
Primary Standards Power meter E44196 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5066 (20b) SN: S5129 (30b) SN: 3D13 SN: 654 ID # US3642U01700	3-May-05 (METAS, No. 251-00486) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00467) 11-Aug-05 (METAS, No. 251-00500) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house)	May-06 May-06 May-06 Aug-06 Aug-06 Aug-06 Jan-07 Feb-07 Scheduled Check In house check: Nov-07
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585	3-May-05 (METAS, No. 251-00486) 3-May-05 (METAS, No. 251-00466) 3-May-05 (METAS, No. 251-00466) 11-Aug-05 (METAS, No. 251-00499) 3-May-05 (METAS, No. 251-00500) 11-Aug-05 (METAS, No. 251-00500) 2-Jan-06 (SPEAG, No. ES3-3013_Jan06) 2-Feb-06 (SPEAG, No. DAE4-654_Feb06) Check Date (in house) 4-Aug-99 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Nov-05)	May-06 May-06 May-06 Aug-06 Aug-06 Aug-06 Jan-07 Feb-07 Scheduled Check In house check: Nov-07 In house check: Nov-06

Certificate No: EX3-3514_Feb06

Page 1 of 9



Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,y,z ConF tissue simulating liquid sensitivity in free space sensitivity in TSL / NORMx,y,z

DCP diode compression point Polarization φ φ rotation around probe axis

Polarization φ φ rotation around probe Polarization 9 9 rotation around an axi

9 rotation around an axis that is in the plane normal to probe axis (at

measurement center), i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This
 linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
 the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Cortificate	Nicos	EX3-3514	E-LOS	
Ceunicare	NO:	EX3-3514	rebub	



EX3DV3 SN:3514

February 17, 2006

Probe EX3DV3

SN:3514

Manufactured:

December 15, 2002 January 23, 2004

Last calibrated: Recalibrated:

February 17, 2006

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: EX3-3514_Feb06

Page 3 of 9

EX3DV3 SN:3514

February 17, 2006

DASY - Parameters of Probe: EX3DV3 SN:3514

|--|

Diode Compression^B

NormX	0.655 ± 10.1%	$\mu V/(V/m)^2$	DCP X	97 mV
NormY	0.675 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	97 mV
NormZ	0.598 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	97 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

TSL

5200 MHz Typical SAR gradient: 25 % per mm

Sensor Center to Phantom Surface Distance		2.0 mm	3.0 mm
SAR _{be} [%]	Without Correction Algorithm	4.5	1.8
SAR _{be} [%]	With Correction Algorithm	0.0	0.0

TSL

5800 MHz Typical SAR gradient: 30 % per mm

Sensor Cente	er to Phantom Surface Distance	2.0 mm	3.0 mm
SAR _{be} [%]	Without Correction Algorithm	1.2	0.8
SAR _{be} [%]	With Correction Algorithm	0.0	0.0

Sensor Offset

Probe Tip to Sensor Center

1.0 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: EX3-3514_Feb06

Page 4 of 9

^h The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).


Numerical linearization parameter: uncertainty not required.

EX3DV3 SN:3514

February 17, 2006

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

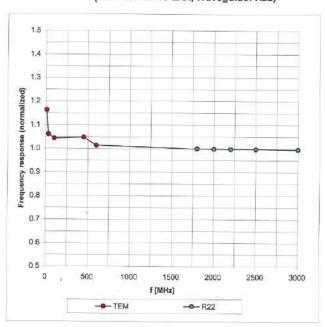

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Certificate No: EX3-3514_Feb06


Page 5 of 9


EX3DV3 SN:3514

February 17, 2006

Receiving Pattern (ϕ), θ = 0°






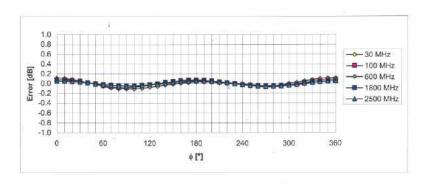

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3514_Feb06


Page 6 of 9

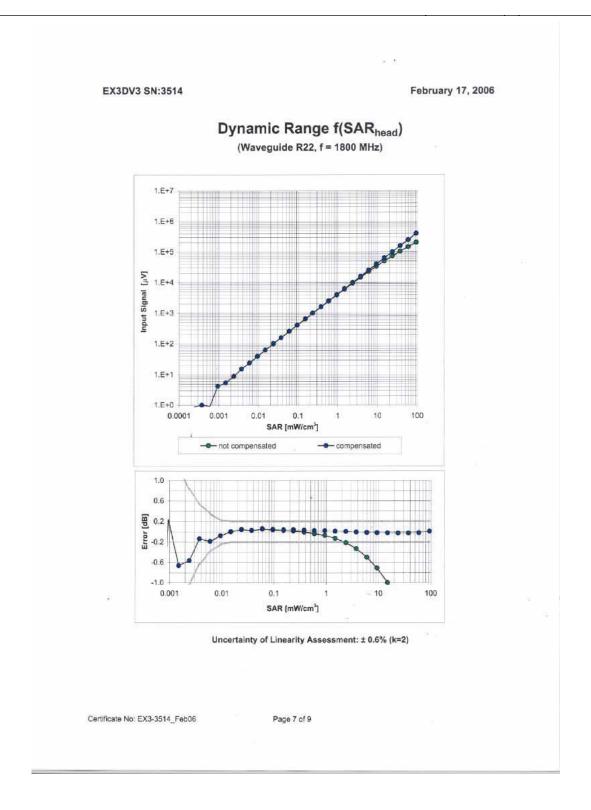


EX3DV3 SN:3514

February 17, 2006

Conversion Factor Assessment





f [MHz]	Validity [MHz]	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF	Uncertainty
5200	$\pm~50~/\pm~100$	Body	49.0 ± 5%	$5.30 \pm 5\%$	0.47	1.25	4.35	± 13.1% (k=2)
5500	\pm 50 / \pm 100	Body	$48.6\pm5\%$	$5.65 \pm 5\%$	0.46	1.14	4.02	± 13.1% (k=2)
5800	\pm 50 / \pm 100	Body	48.2 ± 5%	6.00 ± 5%	0.52	0.92	4.09	± 13.1% (k=2)

Certificate No: EX3-3514 Feb06

Page 8 of 9


 $^{^{\}circ}$ The validity of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

EX3DV3 SN:3514

February 17, 2006

Deviation from Isotropy in HSL

Error (φ, θ), f = 900 MHz

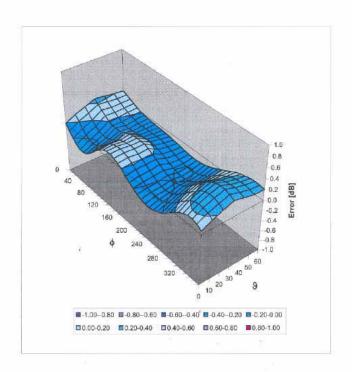

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: EX3-3514_Feb06

Page 9 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client Sporton (Auden)

Certificate No: DAE3-577_Nov05

Accreditation No.: SCS 108

. LIDIOTION O	ERTIFICATE		
Object	DAE3 - SD 000 D	03 AA - SN: 577	
Calibration procedure(e)	QA CAL-06.v12 Calibration proced	dure for the data acquisition electro	onics (DAE)
Calibration date:	November 11, 200	05	
Condition of the calibrated item	In Tolerance		
The measurements and the uncertainty and uncertainty a	tainties with confidence protections and the closed laboratory	onal standards, which realize the physical units obability are given on the following pages and a y facility: environment temperature (22 ± 3)°C a	are part of the certificate.
Calibration Equipment used (M&T)	ii		
Primary Standards Fluke Process Calibrator Type 702	ID# 2 SN: 6295803	Cal Date (Calibrated by, Certificate No.) 7-Oct-05 (Sintrel, No.E-050073)	Scheduled Calibration Oct-06
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Calibrator Box V1.1	SE UMS 006 AB 1002	29-Jun-05 (SPEAG, in house check)	In house check Jun-06
		· · · · · · · · · · · · · · · · · · ·	
	1	*	
×	1		
Calibrated by:	Name Daniel Steinacher	Function Technician	Signature The Senoch
· Calibrated by: Approved by:	and the contract of the contra	Technician	

Certificate No: DAE3-577_Nov05

Page 1 of 5



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE data acquisition electronics

Connector angle information used in DASY system to align probe sensor X to the robot

coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters contain technical information as a result from the performance test and require no uncertainty.
- DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
- Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
- Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
- AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
- Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
- Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
- Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
- Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
- Power consumption: Typical value for information. Supply currents in various operating modes

Certificate No: DAE3-577_Nov05

Page 2 of 5



DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1μV, full range = -100...+300 mV
Low Range: 1LSB = 61nV, full range = -1......+3mV
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Y	Z
High Range	404.445 ± 0.1% (k=2)	403.896 ± 0.1% (k=2)	404.369 ± 0.1% (k=2)
Low Range	3.94241 ± 0.7% (k=2)	3.89919 ± 0.7% (k=2)	3.95427 ± 0.7% (k=2)

Connector Angle

	Selection to the selection of the select
Connector Angle to be used in DASY system	130 ° ± 1 °

Certificate No: DAE3-577_Nov05

Page 3 of 5

Appendix

1. DC Voltage Linearity

High Range	Input (μV)	Reading (μV)	Error (%)
Channel X + Input	200000	199999.3	0.00
Channel X + Input	20000	20006.75	0.03
Channel X - Input	20000	-19997.90	-0.01
Channel Y + Input	200000	200000.3	0.00
Channel Y + Input	20000	20004.58	0.02
Channel Y - Input	20000	-20000.75	0.00
Channel Z + Input	200000	199999.6	0.00
Channel Z + Input	20000	20001.43	0.01
Channel Z - Input	20000	-20003.93	0.02

Low Range	Input (μV)	Reading (μV)	Error (%)
Channel X + Input	2000	2000.1	0.00
Channel X + Input	200	200,42	0.21
Channel X - Input	200	-200.30	0.15
Channel Y + Input	2000	2000.1	0.00
Channel Y + Input	200	199.35	-0.32
Channel Y - Input	200	-200.96	0.48
Channel Z + Input	2000	1999.9	0.00
Channel Z + Input	200	199.37	-0.31
Channel Z - Input	200	-200.62	0.31

2. Common mode sensitivity

2. Common mode sensitivity

2. Common mode sensitivity

2. Sec; Measuring time: 3 sec;

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	13.40	12.55
	- 200	-12.29	-13.06
Channel Y	200	-6.93	-7.43
	- 200	6.72	6.47
Channel Z	200	0.71	0.36
Children	- 200	-1.67	-1.93

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	a l	1.59	0.08
Channel Y	200	1.69	727	3.62
Channel Z	200	-0.73	-1.49	-

Certificate No: DAE3-577_Nov05

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15946	15679
Channel Y	15960	16151
Channel Z	16233	15968

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.08	-1.13	2.31	0.51
Channel Y	-0.35	-2.00	0.81	0.43
Channel Z	-0.38	-2.76	1.68	0.40

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	200.8
Channel Y	0.2000	201.4
Channel Z	0.2001	200.3

8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	+6 -	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE3-577_Nov05

Page 5 of 5