

Front side -middle

Type: Phone measurement (Complete)

Date of measurement:27/9/2024

Measurement duration: 13 minutes 11 seconds

A. Experimental conditions.


<u>Area Scan</u>	<u>dx=15mm dy=15mm</u>
<u>ZoomScan</u>	7x7x7,dx=5mm dy=5mmdz=5mm,Complete
<u>Phantom</u>	<u>Validation plane</u>
<u>Device Position</u>	<u>Body</u>
<u>Band</u>	IEEE 802.11b ISM
<u>Channels</u>	<u>Middle</u>
<u>Signal</u>	IEEE802.b (Crest factor: 1.0)

B. SAR MeasurementResults

Middle Band SAR (Channel 7):

Frequency (MHz)	2442.000000
Relative permittivity (real part)	41.649860
Relative permittivity (imaginary part)	14.743260
Conductivity (S/m)	2.000169
Variation (%)	-1.280000



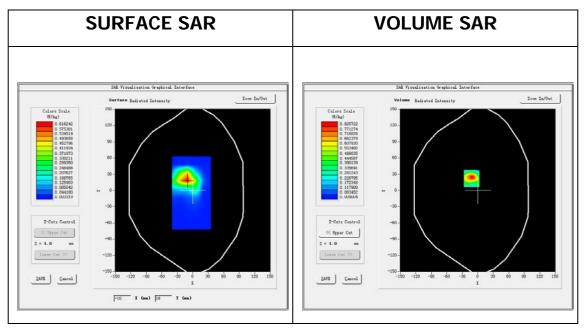



Maximum location: X=-12.00, Y=22.00

SAR Peak: 0.15 W/kg

SAR 10g (W/Kg)	0.305863
SAR1g (W/Kg)	0.757241



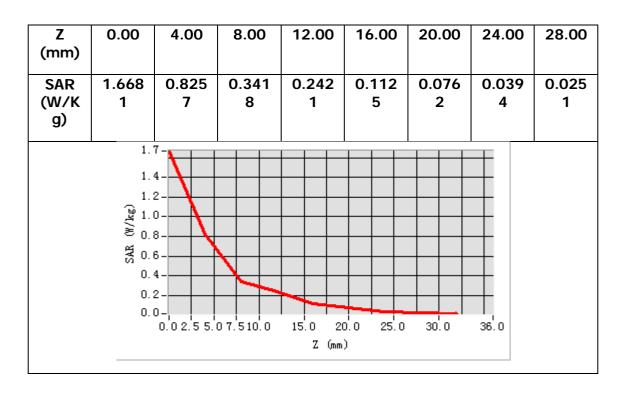

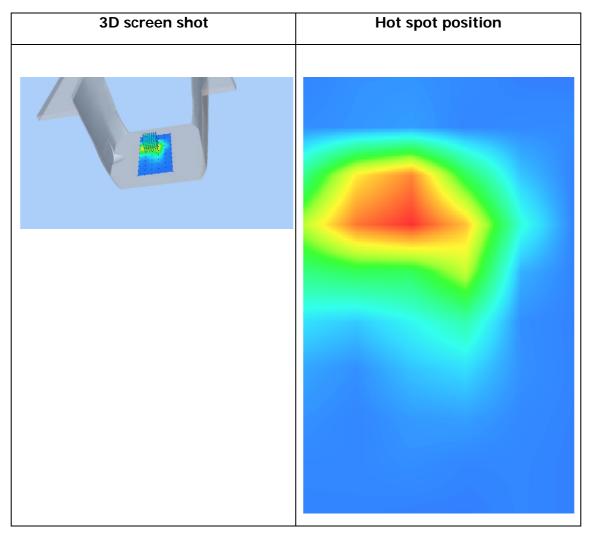



Front-side-middle

Type: Phone measurement (Complete)

Date of measurement: 21/9/2024

Measurement duration: 11 minutes 17 seconds


A. Experimental conditions.

<u>Area Scan</u>	<u>dx=15mm dy=15mm</u>	
<u>ZoomScan</u>	5x5x7,dx=8mm dy=8mm dz=5mm,Complete	
<u>Phantom</u>	Validation plane	
<u>Device Position</u>	Body	
<u>Band</u>	CUSTOM (GPRS850_4Tx)	
<u>Channels</u>	Low	
<u>Signal</u>	Duty Cycle: 2.00 (Crest factor: 2.0)	

B. SAR Measurement Results

Frequency (MHz)	848.800000
Relative permittivity (real part)	53.891621
Relative permittivity (imaginary part)	20.664499
Conductivity (S/m)	0.946204
Variation (%)	-2.160000



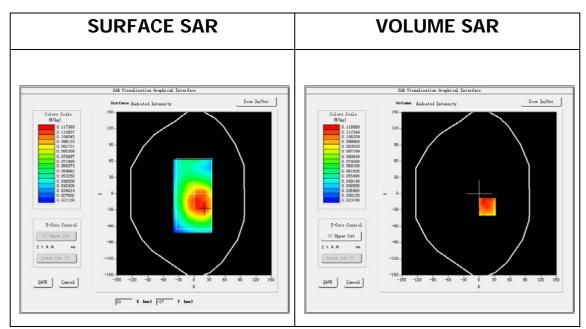



Maximum location: X=16.00, Y=-24.00

SAR Peak: 0.16 W/kg

SAR 10g (W/Kg)	0.147254
SAR 1g (W/Kg)	0.295316



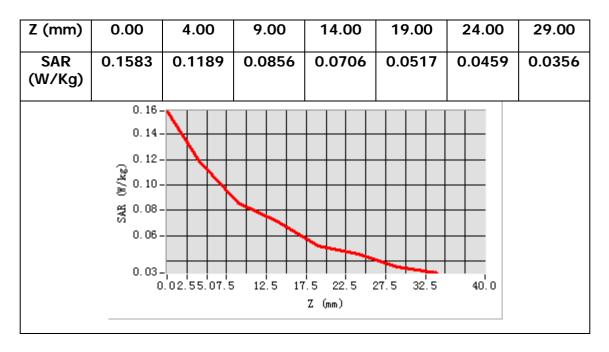

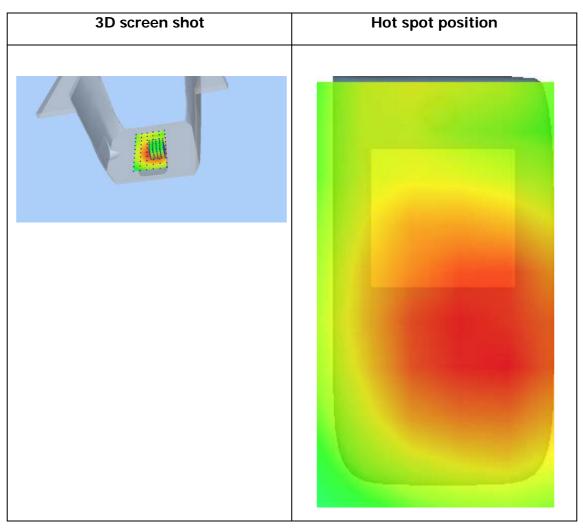



Front-side-middle

Type: Phone measurement (Complete)

Date of measurement:23/9/2024

Measurement duration: 14 minutes 31 seconds

A. Experimental conditions.


Area Scan	<u>dx=15mm dy=15mm</u>
<u>ZoomScan</u>	7x7x7,dx=5mm dy=5mmdz=5mm,Complete
<u>Phantom</u>	<u>Validation plane</u>
<u>Device Position</u>	<u>Body</u>
<u>Band</u>	CUSTOM (GPRS1900 4Tx)
<u>Channels</u>	<u>Middle</u>
<u>Signal</u>	Duty Cycle: 2.0 (Crest factor: 2.0)

B. SAR MeasurementResults

Middle Band SAR (Channel 661):

Frequency (MHz)	1880.000000
Relative permittivity (real part)	44.552711
Relative permittivity (imaginary part)	15.152806
Conductivity (S/m)	1.471001
Variation (%)	-1.230000



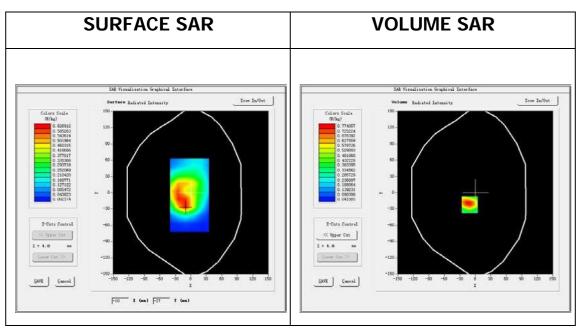



Maximum location: X=-49.00, Y=-8.00

SAR Peak: 0.28 W/kg

SAR 10g (W/Kg)	0.019765
SAR1g (W/Kg)	0.048341



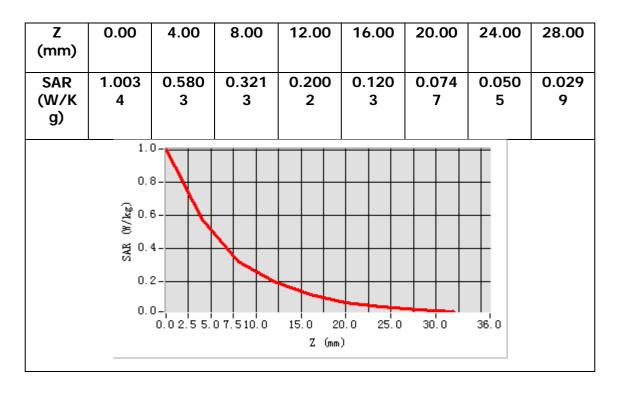

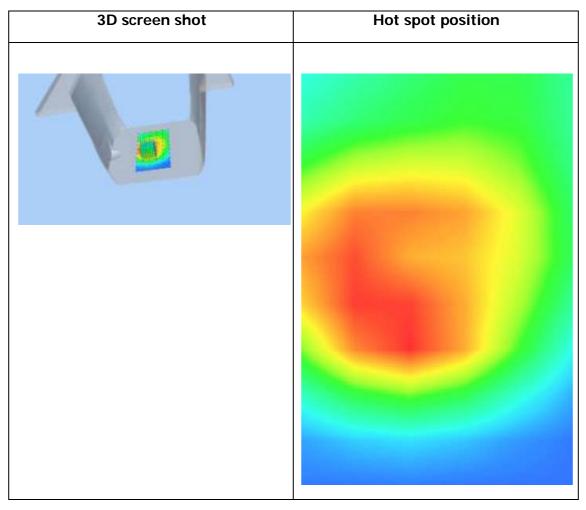



Towards-phantom- Middle

Type: Phone measurement (Complete)

Date of measurement:27/9/2024

Measurement duration: 10 minutes 36 seconds


A. Experimental conditions.

<u>Area Scan</u>	dx=10mm dy=10mm	
<u>ZoomScan</u>	7x7x12,dx=4mm dy=4mmdz=2mm,Complete	
<u>Phantom</u>	Validation plane	
Device Position	Body	
<u>Band</u>	<u>IEEE 802.11a U-NII-1</u>	
<u>Channels</u>	<u>Middle</u>	
<u>Signal</u>	Duty cycle:1:1	

B. SAR MeasurementResults

Frequency (MHz)	5180.000000
Relative permittivity (real part)	35.858526
Relative permittivity (imaginary part)	15.623689
Conductivity (S/m)	4.494532
Variation (%)	1.450000



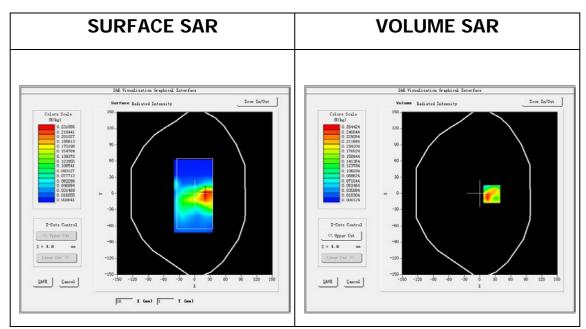



Maximum location: X=23.00, Y=-1.00

SAR Peak: 0.09 W/kg

SAR 10g (W/Kg)	0.350814
SAR1g (W/Kg)	0.719322



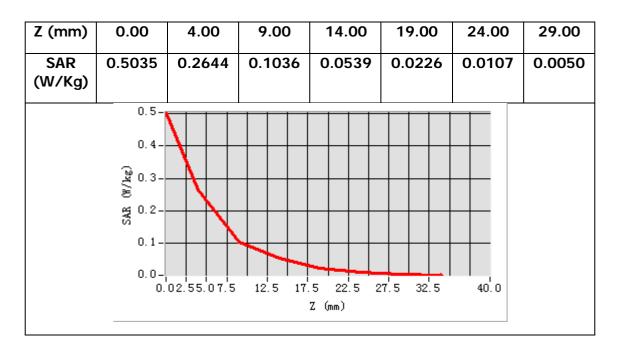

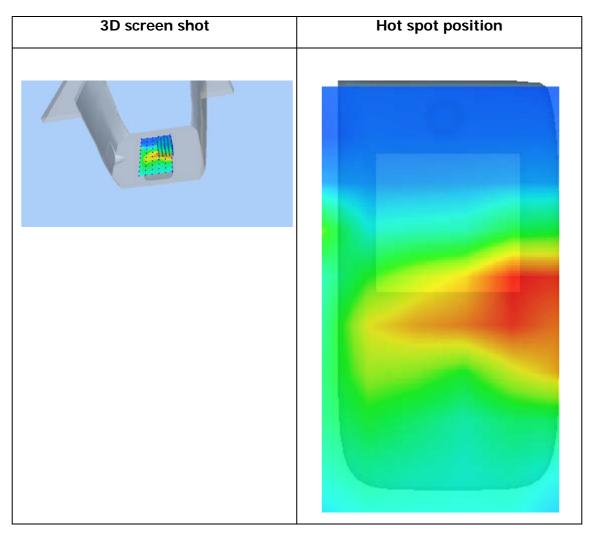



Towards-phantom- Middle

Type: Phone measurement (Complete)

Date of measurement:27/9/2024

Measurement duration:10 minutes 36 seconds


A. Experimental conditions.

Area Scan	dx=10mm dy=10mm	
<u>ZoomScan</u>	7x7x12,dx=4mm dy=4mmdz=2mm,Complete	
<u>Phantom</u>	<u>Validation plane</u>	
<u>Device Position</u>	<u>Body</u>	
<u>Band</u>	<u>IEEE 802.11a U-NII-2a</u>	
<u>Channels</u>	<u>Middle</u>	
<u>Signal</u>	Duty cycle:1:1	

B. SAR MeasurementResults

Frequency (MHz)	5260.000000
Relative permittivity (real part)	35.858526
Relative permittivity (imaginary part)	15.623689
Conductivity (S/m)	4.494532
Variation (%)	2.140000



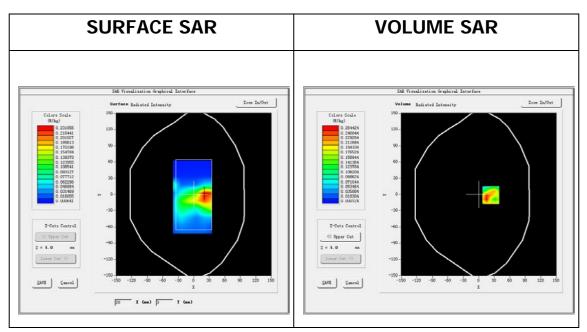



Maximum location: X=23.00, Y=-1.00

SAR Peak: 0.09 W/kg

SAR 10g (W/Kg)	0.328417
SAR1g (W/Kg)	0.691342



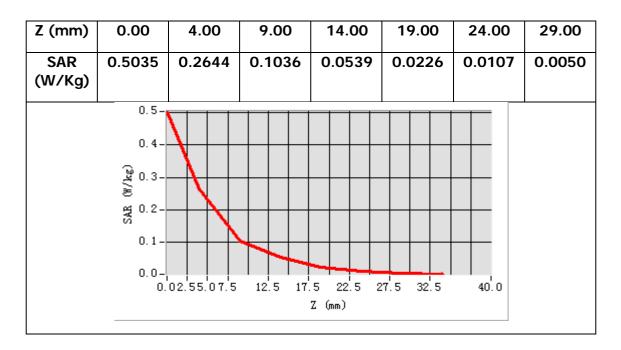

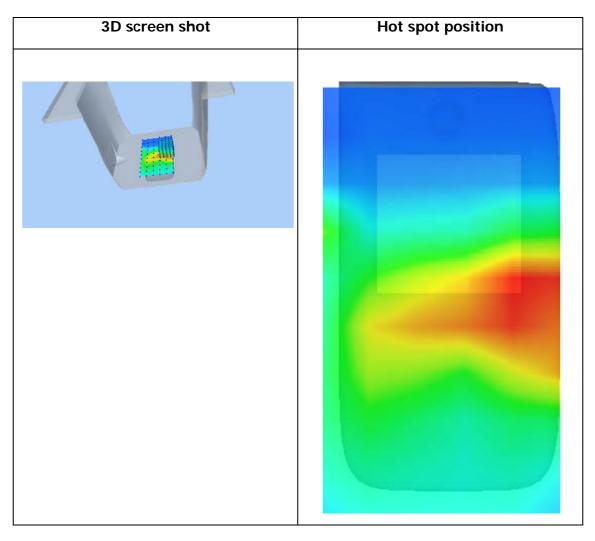



Towards-Phantom-Middle

Type: Phone measurement (Complete)

Date of measurement: 27/9/2024

Measurement duration: 8 minutes 40seconds


A. Experimental conditions.

<u>Area Scan</u>	dx=10mm dy=10mm	
<u>ZoomScan</u>	7x7x12,dx=4mm dy=4mmdz=2mm,Complete	
<u>Phantom</u>	<u>Validation plane</u>	
Device Position	Body	
<u>Band</u>	IEEE 802.11a U-NII-3	
<u>Channels</u>	<u>Middle</u>	
<u>Signal</u>	Duty cycle:1:1	

B. SAR MeasurementResults

Frequency (MHz)	5580.000000
Relative permittivity (real part)	48.235748
Relative permittivity (imaginary part)	19.060800
Conductivity (S/m)	6.173560
Variation (%)	1.730000



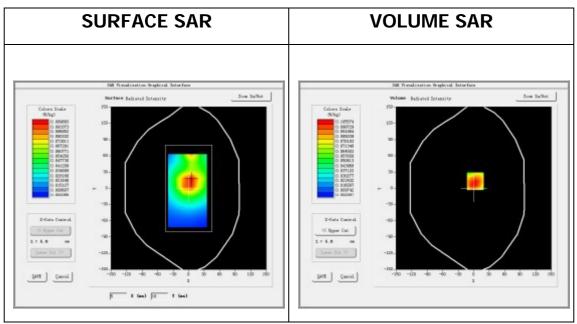



Maximum location: X=3.00, Y=13.00

SAR Peak: 0.33 W/kg

SAR 10g (W/Kg)	0.358435
SAR1g (W/Kg)	0.721836



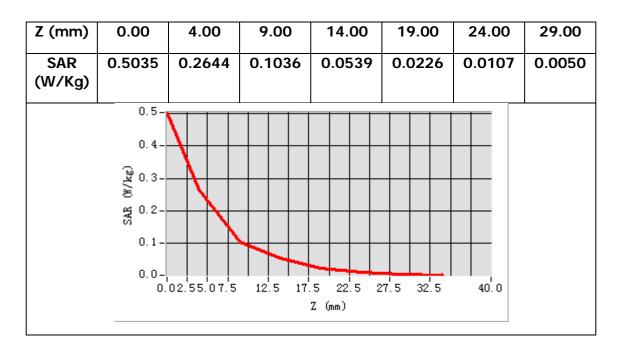

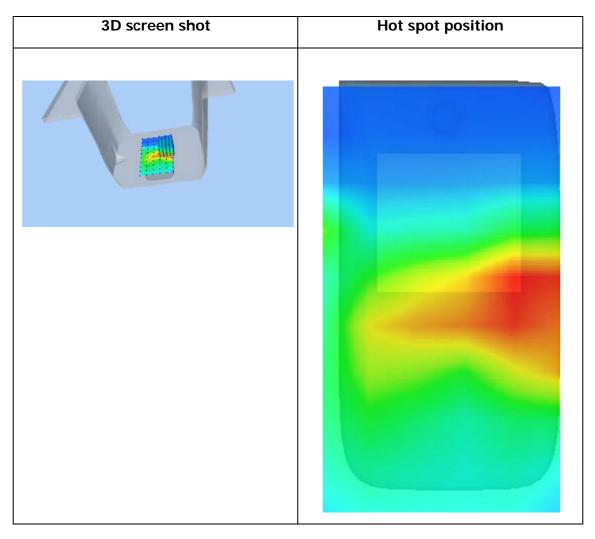



Towards-phantom- Middle

Type: Phone measurement (Complete)

Date of measurement: 27/9/2024

Measurement duration: 9 minutes 32 seconds


A. Experimental conditions.

<u>Area Scan</u>	dx=10mm dy=10mm	
<u>ZoomScan</u>	7x7x12,dx=4mm dy=4mmdz=2mm,Complete	
<u>Phantom</u>	<u>Validation plane</u>	
Device Position	Body	
<u>Band</u>	<u>IEEE 802.11a U-NII-4</u>	
<u>Channels</u>	<u>Middle</u>	
<u>Signal</u>	Duty cycle:1:1	

B. SAR MeasurementResults

Frequency (MHz)	5785.000000
Relative permittivity (real part)	48.235748
Relative permittivity (imaginary part)	19.060800
Conductivity (S/m)	6.173560
Variation (%)	-4.900000



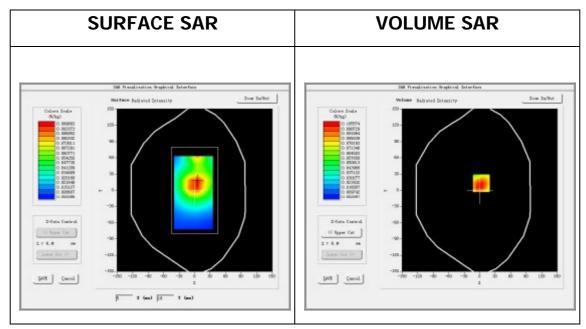



Maximum location: X=3.00, Y=13.00

SAR Peak: 0.25 W/kg

SAR 10g (W/Kg)	0.347386
SAR1g (W/Kg)	0.712435



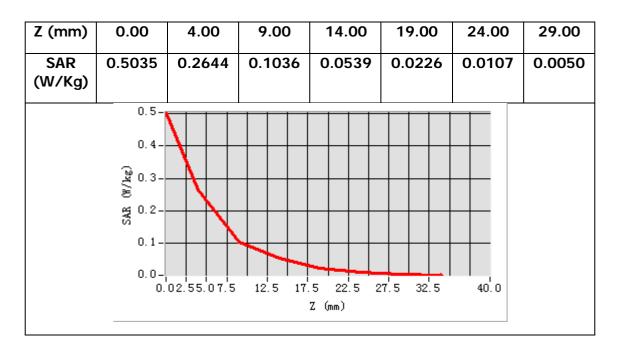

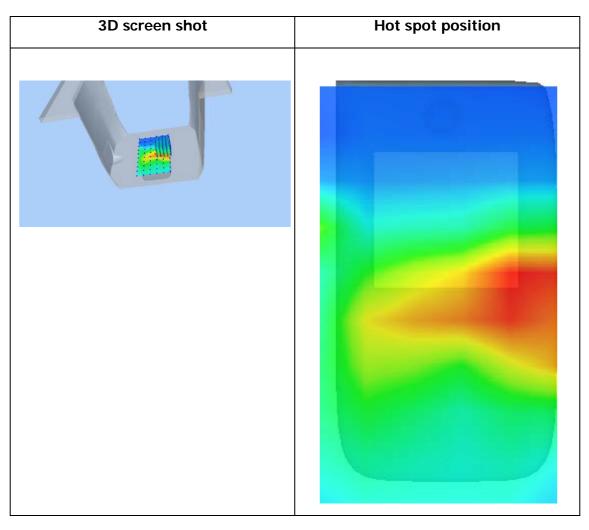



Type: Phone measuremen

Date of measurement: 27/9/2024

Measurement duration: 8 minutes 26 seconds

A. Experimental conditions.


7tt = ZA GOTTITIOTITUAL COL		
<u>Area Scan</u>	<u>dx=15mm dy=15mm</u>	
<u>ZoomScan</u>	5x5x7,dx=8mm dy=8mm	
	<u>dz=5mm</u>	
<u>Phantom</u>	<u>Validation plane</u>	
Device Position	<u>Body</u>	
<u>Band</u>	<u>Bluetooth</u>	
<u>Channels</u>	<u>High</u>	
<u>Signal</u>	Bluetooth (Crest factor: 1.0)	

B. SAR Measurement Results

Higher Band SAR (Channel 78):

Frequency (MHz)	2480.000000
Relative permittivity (real part)	39.160000
Relative permittivity (imaginary	13.290000
Conductivity (S/m)	1.831067
<u>Variation (%)</u>	-2.330000



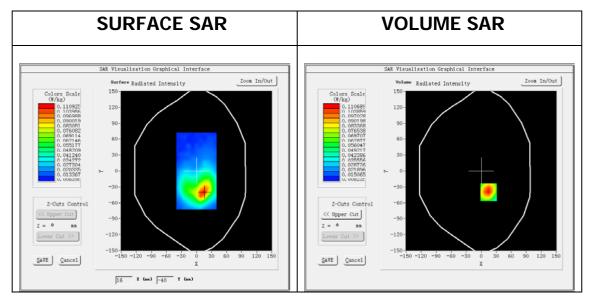


Maximum location: X=15.00, Y=-40.00


SAR Peak: 0.18 W/kg

SAR 10g (W/Kg)	0.004621
SAR 1g (W/Kg)	0.008327



SATIMO 225, rue Pierre Rivoalon 29200 Brest - France Tel:+33 (0)2 98 05 13 34; Fax: +33 (0)2 98 05 53 87; www.satimo.com

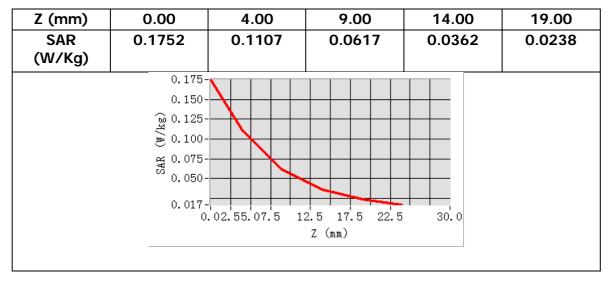

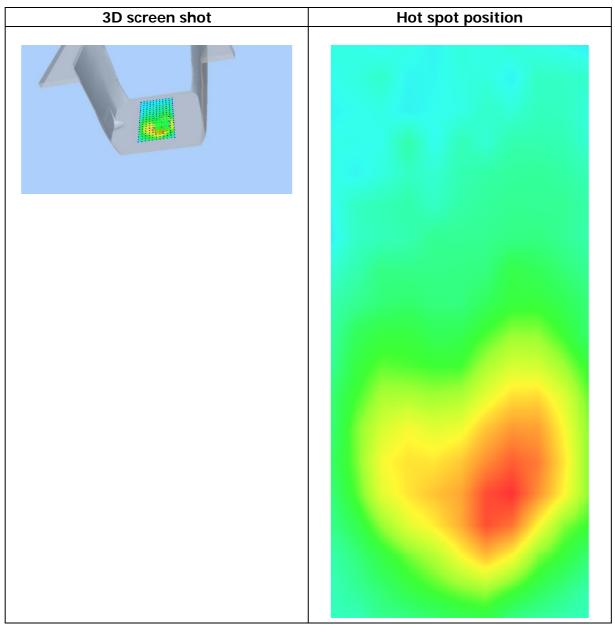



Tested Model: P10003L

Report Number:

WSCT-ANAB-R&E240900047A-SAR



SAR Reference Dipole Calibration Report

Ref: ACR.313.11.23.BES.A

WORLD STANDARDIZATION CERTIFICATION & TESTING GROUP CO .,LTD

BLOCK A, BAO SHI SCIENCE PARK,BAO SHI ROAD, BAO'AN DISTRICT

SHENZHEN 518108, P.R. CHINA

MVG COMOSAR REFERENCE DIPOLE

FREQUENCY: 835 MHZ

SERIAL NO.: 3723-DIP0G835-733

Calibrated at MVG

Z.I. de la pointe du diable

Technopôle Brest Iroise – 295 avenue Alexis de Rochon 29280 PLOUZANE - FRANCE

Calibration date: 09/11/2023



Accreditations #2-6789 and #2-6814 Scope available on www.cofrac.fr

The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.

Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



	Name	Function	Date	Signature
Prepared by :	Cyrille ONNEE	Measurement Responsible	11/9/2023	28
Checked & approved by:	Jérôme Luc	Technical Manager	11/9/2023	Jes
Authorized by:	Yann Toutain	Laboratory Director	11/9/2023	Gann TOUTAN

Yann
Signature numérique de Yann Toutain ID
Date: 2023.11.09
16:42:07 +01'00'

	Customer Name
Distribution :	World
	Standardization
	Certification &
	Testing Group Co
	.,Ltd

Issue	Name	Date	Modifications
A	Cyrille ONNEE	11/9/2023	Initial release



TABLE OF CONTENTS

ł	murc	duction4	
2	Dev	ice Under Test4	
3	Proc	uct Description4	
	3.1	General Information	4
4	Mea	surement Method5	
	4.1	Mechanical Requirements	5
	4.2	S11 parameter Requirements	5
	4.3	SAR Requirements	
5	Mea	surement Uncertainty5	
	5.1	Mechanical dimensions	5
	5.2	S11 Parameter	5
	5.3	SAR	5
6	Cali	pration Results6	
	6.1	Mechanical Dimensions	6
	6.2	S11 parameter	6
	6.3	SAR	6
7	List	of Equipment8	



1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

Device Under Test				
Device Type	COMOSAR 835 MHz REFERENCE DIPOLE			
Manufacturer	MVG			
Model	SID835			
Serial Number	3723-DIP0G835-733			
Product Condition (new / used) New				

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



Figure 1 – MVG COMOSAR Validation Dipole



4 MEASUREMENT METHOD

4.1 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

4.2 S11 PARAMETER REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a S11 of -20 dB or better. The S11 measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

4.3 SAR REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore-mentioned standards.

5 MEASUREMENT UNCERTAINTY

5.1 MECHANICAL DIMENSIONS

For the measurement in the range 0-300mm, the estimated expanded uncertainty (k=2) in calibration for the dimension measurement in mm is +/-0.20 mm with respect to measurement conditions.

For the measurement in the range 300-450mm, the estimated expanded uncertainty (k=2) in calibration for the dimension measurement in mm is +/-0.44 mm with respect to measurement conditions.

5.2 S11 PARAMETER

The estimated expanded uncertainty (k=2) in calibration for the S11 parameter in linear is +/-0.08 with respect to measurement conditions.

5.3 SAR

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

The estimated expanded uncertainty (k=2) in calibration for the 1g and 10g SAR measurement in W/kg is +/-19% with respect to measurement conditions.




6 CALIBRATION RESULTS

6.1 MECHANICAL DIMENSIONS

L	mm	h	mm	d i	mm
Measured	Required	Measured	Required	Measured	Required
161.22	161.00 +/- 2%	89.32	89.80 +/- 2%	3.60	3.60 +/- 2%

6.2 S11 PARAMETER

6.2.1 S11 parameter in Head Liquid

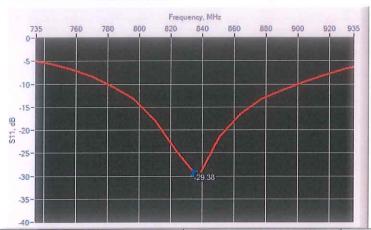

Frequency (MHz)	S11 parameter (dB)	Requirement (dB)	Impedance
835	-29.38	-20	49.7Ω - $2.9j\Omega$

6.3 SAR

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.


6.3.1 SAR with Head Liquid

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.



Software	OPENSAR V5
Phantom	SN 13/09 SAM68
Probe	SN 41/18 EPGO333
Liquid	Head Liquid Values: eps': 45.5 sigma: 0.92
Distance between dipole center and liquid	15.0 mm
Area scan resolution	dx=8mm/dy=8mm
Zoon Scan Resolution	dx=8mm/dy=8mm/dz=5mm
Frequency	835 MHz
Input power	20 dBm
Liquid Temperature 20 +/- 1 °C	
Lab Temperature	20 +/- 1 °C
Lab Humidity 30-70 %	

Frequency	1g SAR (W/kg)			10g SAR (W/kg)		
	Measured	Measured normalized to 1W	Target normalized to 1W	Measured	Measured normalized to 1W	Target normalized to 1W
835 MHz	0.94	9.42	9.56	0.62	6.21	6.22

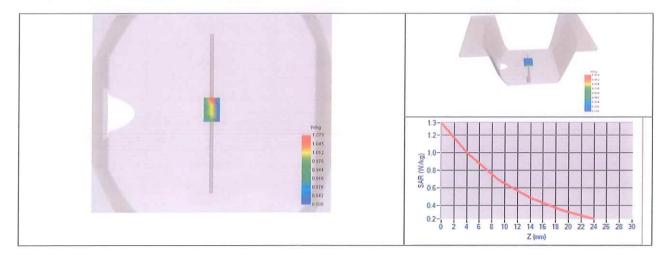



LIST OF EQUIPMENT

THE SHAPE	Equi	pment Summary \$	Sheet		
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date	
SAM Phantom	MVG	SN 13/09 SAM68	Validated. No cal required.	Validated. No cal required.	
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.	
Network Analyzer	Rohde & Schwarz ZVM	100203	08/2021	08/2024	
Network Analyzer – Calibration kit	Rohde & Schwarz ZV-Z235	101223	07/2022	07/2025	
Calipers	Mitutoyo	SN 0009732	11/2022	11/2025	
Reference Probe	MVG	3523-EPGO-429	11/2023	11/2024	
Multimeter	Keithley 2000	4013982	02/2023	02/2026	
Signal Generator	Rohde & Schwarz SMB	106589	03/2022	03/2025	
Amplifier	MVG	MODU-023-C-0002	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.	
Power Meter	NI-USB 5680	170100013	06/2021 06/2024		
Power Meter	Keysight U2000A	SN: MY62340002	10/2022	10/2025	
Directional Coupler	Krytar 158020	131467	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.	
Temperature / Humidity Sensor	Testo 184 H1	44225320	06/2021	06/2024	



SAR Reference Dipole Calibration Report

Ref: ACR.313.13.23.BES.A

WORLD STANDARDIZATION CERTIFICATION & TESTING GROUP CO .,LTD

BLOCK A, BAO SHI SCIENCE PARK, BAO SHI ROAD, BAO'AN DISTRICT

SHENZHEN 518108,P.R. CHINA
MVG COMOSAR REFERENCE DIPOLE

FREQUENCY: 1800 MHZ

SERIAL NO.: 3723-DIP1G800-735

Calibrated at MVG

 $Z.I.\ de\ la\ pointe\ du\ diable$ $Technopôle\ Brest\ Iroise-295\ avenue\ Alexis\ de\ Rochon$

29280 PLOUZANE - FRANCE

Calibration date: 09/11/2023



Accreditations #2-6789 and #2-6814 Scope available on www.cofrac.fr

The use of the Cofrac brand and the accreditation references is prohibited from any reproduction

Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



	Name	Function	Date	Signature
Prepared by :	Cyrille ONNEE	Measurement Responsible	11/9/2023	28
Checked & approved by:	Jérôme Luc	Technical Manager	11/9/2023	JES
Authorized by:	Yann Toutain	Laboratory Director	11/9/2023	Gann TOUTANN

Signature Yann numérique de Yann Toutain ID Toutain ID Date: 2023.11.09 16:43:12 +01'00'

	Customer Name
Distribution :	World
	Standardization
	Certification &
	Testing Group Co
	.,Ltd

Issue	Name	Date	Modifications
A	Cyrille ONNEE	11/9/2023	Initial release



TABLE OF CONTENTS

1	Intr	troduction4		
2	Dev	Device Under Test		
3	Pro	duct Description4		
	3.1	General Information	∠	
4 Me		surement Method5		
	4.1	Mechanical Requirements	5	
	4.2	S11 parameter Requirements		
	4.3	SAR Requirements		
5	Mea	surement Uncertainty5		
	5.1	Mechanical dimensions	5	
	5.2	S11 Parameter		
	5.3	SAR		
6	Cali	bration Results6		
	6.1	Mechanical Dimensions	6	
	6.2	S11 parameter		
	6.3	SAR		
7	List of Equipment8			



1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

Device Under Test						
Device Type	Device Type COMOSAR 1800 MHz REFERENCE DIPOLE					
Manufacturer	MVG					
Model	SID1800					
Serial Number	3723-DIP1G800-735					
Product Condition (new / used)	New					

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



Figure 1 – MVG COMOSAR Validation Dipole



4 MEASUREMENT METHOD

4.1 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

4.2 S11 PARAMETER REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a S11 of -20 dB or better. The S11 measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

4.3 SAR REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore-mentioned standards.

5 MEASUREMENT UNCERTAINTY

5.1 MECHANICAL DIMENSIONS

For the measurement in the range 0-300mm, the estimated expanded uncertainty (k=2) in calibration for the dimension measurement in mm is +/-0.20 mm with respect to measurement conditions.

For the measurement in the range 300-450mm, the estimated expanded uncertainty (k=2) in calibration for the dimension measurement in mm is +/-0.44 mm with respect to measurement conditions.

5.2 S11 PARAMETER

The estimated expanded uncertainty (k=2) in calibration for the S11 parameter in linear is +/-0.08 with respect to measurement conditions.

5.3 <u>SAR</u>

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

The estimated expanded uncertainty (k=2) in calibration for the 1g and 10g SAR measurement in W/kg is +/-19% with respect to measurement conditions.




6 CALIBRATION RESULTS

6.1 MECHANICAL DIMENSIONS

L mm		L mm h mm		d mm	
Measured	Required	Measured	Required	Measured	Required
72.12	72.00 +/- 2%	41.48	41.70 +/- 2%	3.60	3.60 +/- 2%

6.2 S11 PARAMETER

6.2.1 S11 parameter in Head Liquid

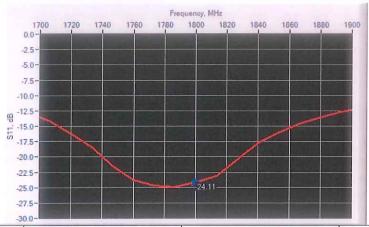

Frequency (MHz)	S11 parameter (dB)	Requirement (dB)	Impedance
1800	-24.11	-20	$47.6\Omega + 5.6j\Omega$

6.3 **SAR**

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.


6.3.1 SAR with Head Liquid

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.



Software	OPENSAR V5
Phantom	SN 13/09 SAM68
Probe	SN 41/18 EPGO333
Liquid	Head Liquid Values: eps': 41.7 sigma: 1.47
Distance between dipole center and liquid	10.0 mm
Area scan resolution	dx=8mm/dy=8mm
Zoon Scan Resolution	dx=8mm/dy=8mm/dz=5mm
Frequency	1800 MHz
Input power	20 dBm
Liquid Temperature	20 +/- 1 °C
Lab Temperature	20 +/- 1 °C
Lab Humidity	30-70 %

Frequency		1g SAR (W/kg	W/kg) 10g SAR (W/kg)			g)
	Measured	Measured normalized to 1W	Target normalized to 1W	Measured	Measured normalized to 1W	Target normalized to 1W
1800 MHz	3.92	39.22	38.40	2.09	20.93	20.10

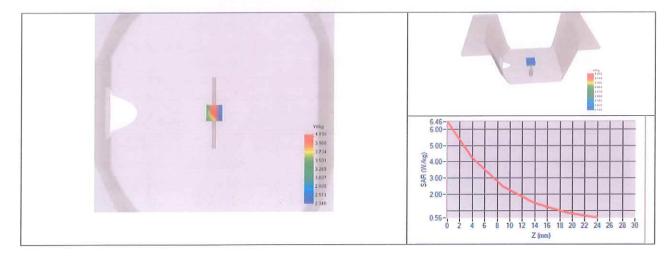



LIST OF EQUIPMENT

Equipment Summary Sheet							
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date			
SAM Phantom	MVG	SN 13/09 SAM68	Validated. No cal required.	Validated. No ca required.			
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No ca required.			
Network Analyzer	Rohde & Schwarz ZVM	100203	08/2021	08/2024			
Network Analyzer – Calibration kit	Rohde & Schwarz ZV-Z235	101223	07/2022	07/2025			
Calipers	Mitutoyo	SN 0009732	11/2022	11/2025			
Reference Probe	MVG	3523-EPGO-429	11/2023	11/2024			
Multimeter	Keithley 2000	4013982	02/2023	02/2026			
Signal Generator	Rohde & Schwarz SMB	106589	03/2022	03/2025			
Amplifier	MVG	MODU-023-C-0002	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.			
Power Meter	NI-USB 5680	170100013	06/2021	06/2024			
Power Meter	Keysight U2000A	SN: MY62340002	10/2022	10/2025			
Directional Coupler	Krytar 158020	131467	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.			
Temperature / Humidity Sensor	Testo 184 H1	44225320	06/2021	06/2024			



SAR Reference Dipole Calibration Report

Ref: ACR.313.14.23.BES.A

WORLD STANDARDIZATION CERTIFICATION & TESTING GROUP CO.,LTD

BLOCK A, BAO SHI SCIENCE PARK,BAO SHI ROAD, BAO'AN DISTRICT

SHENZHEN 518108, P.R. CHINA

MVG COMOSAR REFERENCE DIPOLE

FREQUENCY: 1900 MHZ

SERIAL NO.: 3723-DIP1G900-736

Calibrated at MVG

 $Z.I.\ de\ la\ pointe\ du\ diable$ $Technopôle\ Brest\ Iroise-295\ avenue\ Alexis\ de\ Rochon$

29280 PLOUZANE - FRANCE

Calibration date: 09/11/2023



Accreditations #2-6789 and #2-6814 Scope available on www.cofrac.fr

The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.

Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



	Name	Function	Date	Signature	
Prepared by :	Cyrille ONNEE	Measurement Responsible	11/9/2023	28	
Checked & approved by:	Jérôme Luc	Technical Manager	11/9/2023	JES	
Authorized by:	Yann Toutain	Laboratory Director	11/9/2023	Yann TOUTAAN	

Signature Yann numérique de Toutain ID Date: 2023.11.09 16:43:45 +01'00'

	Customer Name
Distribution:	World
	Standardization
	Certification &
	Testing Group Co
	.,Ltd

Issue	Name	Date	Modifications
A	Cyrille ONNEE	11/9/2023	Initial release



TABLE OF CONTENTS

Ţ	Intr	oduction4	
2	Dev	ice Under Test4	
3	Pro	luct Description4	
	3.1	General Information	4
4	Mea	surement Method5	
	4.1	Mechanical Requirements	5
	4.2	S11 parameter Requirements	5
	4.3	SAR Requirements	5
5	Mea	surement Uncertainty5	
	5.1	Mechanical dimensions	5
	5.2	S11 Parameter	5
	5.3	SAR	5
6	Cali	bration Results6	
	6.1	Mechanical Dimensions	6
	6.2	S11 parameter	6
	6.3	SAR	
7	List	of Equipment8	



1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

2 DEVICE UNDER TEST

Device Under Test					
Device Type COMOSAR 1900 MHz REFERENCE DIPO					
Manufacturer	MVG				
Model	SID1900				
Serial Number	3723-DIP1G900-736				
Product Condition (new / used)	New				

3 PRODUCT DESCRIPTION

3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



Figure 1 – MVG COMOSAR Validation Dipole



4 MEASUREMENT METHOD

4.1 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

4.2 S11 PARAMETER REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a S11 of -20 dB or better. The S11 measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

4.3 SAR REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore-mentioned standards.

5 MEASUREMENT UNCERTAINTY

5.1 MECHANICAL DIMENSIONS

For the measurement in the range 0-300mm, the estimated expanded uncertainty (k=2) in calibration for the dimension measurement in mm is +/-0.20 mm with respect to measurement conditions.

For the measurement in the range 300-450mm, the estimated expanded uncertainty (k=2) in calibration for the dimension measurement in mm is +/-0.44 mm with respect to measurement conditions.

5.2 S11 PARAMETER

The estimated expanded uncertainty (k=2) in calibration for the S11 parameter in linear is +/-0.08 with respect to measurement conditions.

5.3 SAR

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

The estimated expanded uncertainty (k=2) in calibration for the 1g and 10g SAR measurement in W/kg is +/-19% with respect to measurement conditions.




6 CALIBRATION RESULTS

6.1 MECHANICAL DIMENSIONS

L mm		h mm		d mm	
Measured	Required	Measured	Required	Measured	Required
68.06	68.00 +/- 2%	39.42	39.50 +/- 2%	3.60	3.60 +/- 2%

6.2 S11 PARAMETER

6.2.1 S11 parameter in Head Liquid

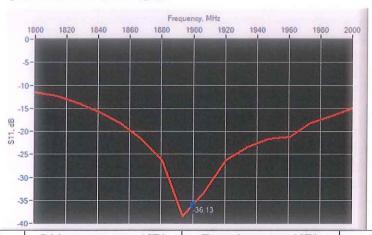

Frequency (MHz)	S11 parameter (dB)	Requirement (dB)	Impedance
1900	-36.13	-20	$51.0\Omega + 0.2j\Omega$

6.3 SAR

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

6.3.1 SAR with Head Liquid


The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.



SAR REFERENCE DIPOLE CALIBRATION REPORT

Software	OPENSAR V5
Phantom	SN 13/09 SAM68
Probe	SN 41/18 EPGO333
Liquid	Head Liquid Values: eps': 43.5 sigma: 1.44
Distance between dipole center and liquid	10.0 mm
Area scan resolution	dx=8mm/dy=8mm
Zoon Scan Resolution	dx=8mm/dy=8mm/dz=5mm
Frequency	1900 MHz
Input power	20 dBm
Liquid Temperature	20 +/- 1 °C
Lab Temperature	20 +/- 1 °C
Lab Humidity	30-70 %

Frequency	1g SAR (W/kg)			10g SAR (W/kg)		
	Measured	Measured normalized to 1W	Target normalized to 1W	Measured	Measured normalized to 1W	Target normalized to 1W
1900 MHz	3.93	39.25	39.70	2.06	20.63	20.50

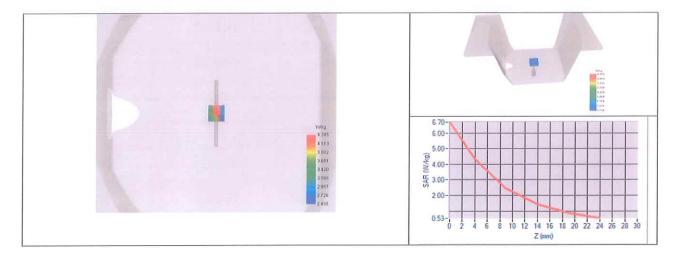



LIST OF EQUIPMENT

Name of Street	Equi	pment Summary S	Sheet		
Equipment Description	Manufacturer / Model	Identification No.	Current Calibration Date	Next Calibration Date	
SAM Phantom	MVG	SN 13/09 SAM68	Validated. No cal required.	Validated. No cal required.	
COMOSAR Test Bench	Version 3	NA	Validated. No cal required.	Validated. No cal required.	
Network Analyzer	Rohde & Schwarz ZVM	100203	08/2021	08/2024	
Network Analyzer – Calibration kit	Rohde & Schwarz ZV-Z235	101223	07/2022	07/2025	
Calipers	Mitutoyo	SN 0009732	11/2022	11/2025	
Reference Probe	MVG	3523-EPGO-429	11/2023	11/2024	
Multimeter	Keithley 2000	4013982	02/2023	02/2026	
Signal Generator	Rohde & Schwarz SMB	106589	03/2022	03/2025	
Amplifier	MVG	MODU-023-C-0002	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.	
Power Meter	NI-USB 5680	170100013	06/2021	06/2024	
Power Meter	Keysight U2000A	SN: MY62340002	10/2022	10/2025	
Directional Coupler	Krytar 158020	131467	Characterized prior to test. No cal required.	Characterized prior to test. No cal required.	
Temperature / Humidity Sensor	Testo 184 H1	44225320	06/2021	06/2024	



SAR Reference Dipole Calibration Report

Ref: ACR.313.16.23.BES.A

WORLD STANDARDIZATION CERTIFICATION & TESTING GROUP CO.,LTD

BLOCK A, BAO SHI SCIENCE PARK,BAO SHI ROAD, BAO'AN DISTRICT

SHENZHEN 518108, P.R. CHINA

MVG COMOSAR REFERENCE DIPOLE

FREQUENCY: 2450 MHZ

SERIAL NO.: 3723-DIP2G450-738

Calibrated at MVG

Z.I. de la pointe du diable

Technopôle Brest Iroise – 295 avenue Alexis de Rochon 29280 PLOUZANE - FRANCE

Calibration date: 09/11/2023



Accreditations #2-6789 and #2-6814 Scope available on www.cofrac.fr

The use of the Cofrac brand and the accreditation references is prohibited from any reproduction

Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



	Name	Function	Date	Signature
Prepared by :	Cyrille ONNEE	Measurement Responsible	11/9/2023	28
Checked & approved by:	Jérôme Luc	Technical Manager	11/9/2023	JES
Authorized by:	Yann Toutain	Laboratory Director	11/9/2023	Gann TOUTAAN

Signature Yann numérique de Yann Toutain ID Date: 2023.11.09
16:44:40 +01'00'

	Customer Name
Distribution :	World
	Standardization
	Certification &
	Testing Group Co
	.,Ltd

Name	Date	Modifications
rille ONNEE	11/9/2023	Initial release



TABLE OF CONTENTS

1	Intro	duction4	
2	Devi	ce Under Test4	
3	Prod	uct Description4	
	3.1	General Information	4
4	Mea	surement Method5	
	4.1	Mechanical Requirements	
	4.2	S11 parameter Requirements	
	4.3	SAR Requirements	
5	Mea	surement Uncertainty5	
	5.1	Mechanical dimensions	
	5.2	S11 Parameter	5
	5.3	SAR	5
6	Calil	oration Results6	
	6.1	Mechanical Dimensions	(
	6.2	S11 parameter	(
	6.3	SAR	6
7	List	of Equipment8	