



Test Setup Photographs

FOR:

iRhythm Technologies, Inc.

Model Name:

A101A5001

Product Description:

Zio AT ECG Patch

FCC ID: 2AFBP-AT17P

IC ID: N/A

Date: November 18, 2016



CETECOM Inc.

411 Dixon Landing Road • Milpitas, CA 95035 • U.S.A.


Phone: + 1 (408) 586 6200 • Fax: + 1 (408) 586 6299 • E-mail: info@cetecom.com • <http://www.cetecom.com>

CETECOM Inc. is a Delaware Corporation with Corporation number: 2905571


Table of Contents

| | | |
|-----------|--|----------|
| 1 | <i>EUT setup for conducted measurement.....</i> | 3 |
| 2 | <i>Conducted measurement</i> | 4 |
| 3 | <i>Radiated Emissions 9KHz- 30MHz Measurement</i> | 5 |
| 4 | <i>Radiated Emissions 30MHz- 1GHz Measurement</i> | 6 |
| 8. | <i>Radiated Emissions 1GHz- 3GHz Measurement.....</i> | 7 |
| 5 | <i>Radiated Emissions 3GHz- 18GHz Measurement.....</i> | 8 |
| 6 | <i>Radiated Emissions above 18GHz.....</i> | 9 |


1 EUT setup for conducted measurement

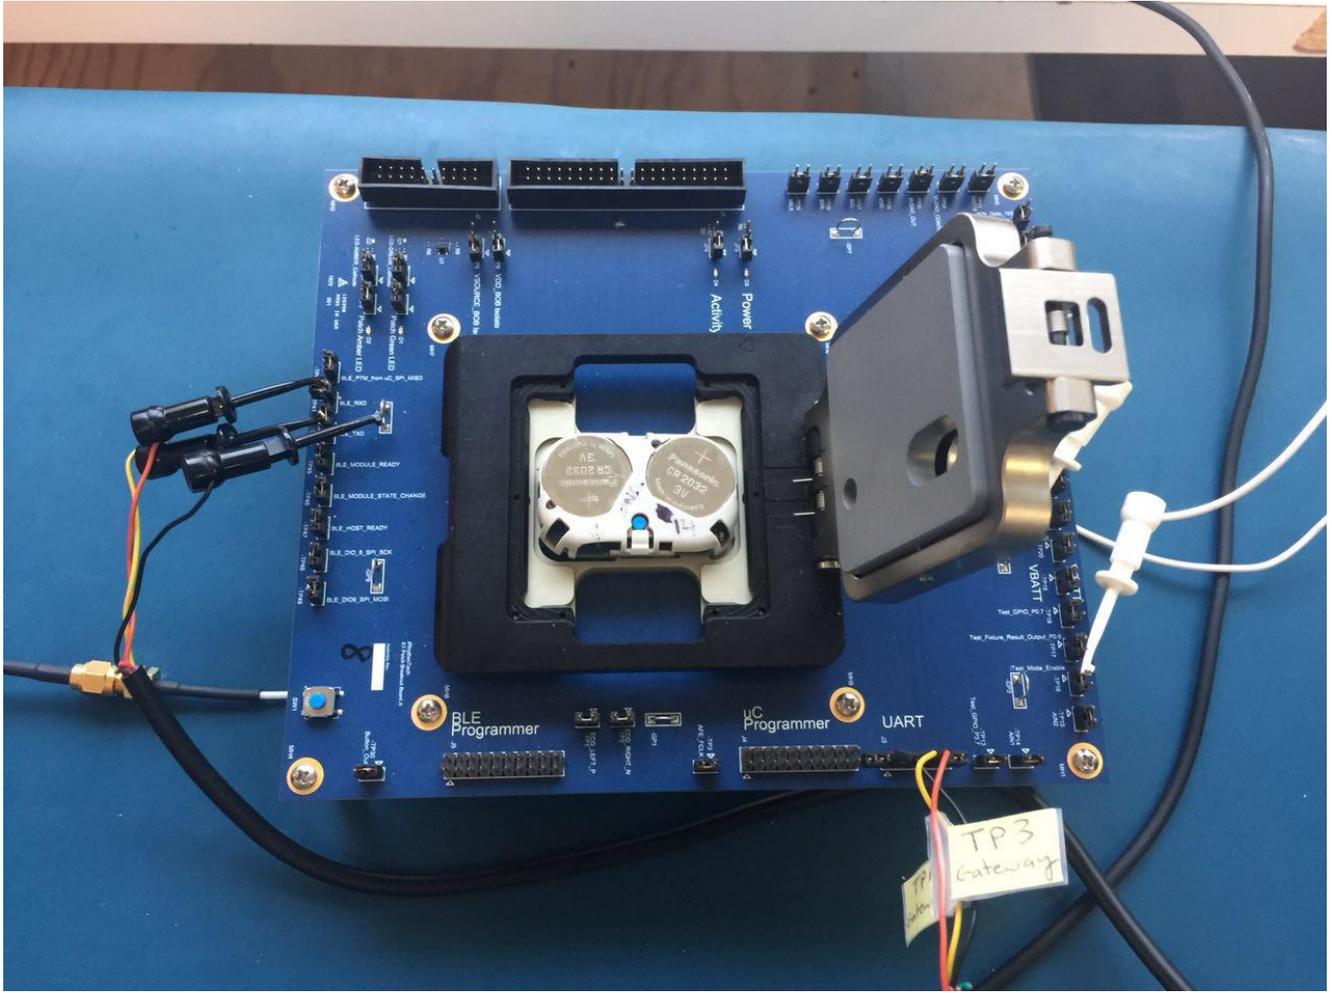


2 Conducted measurement

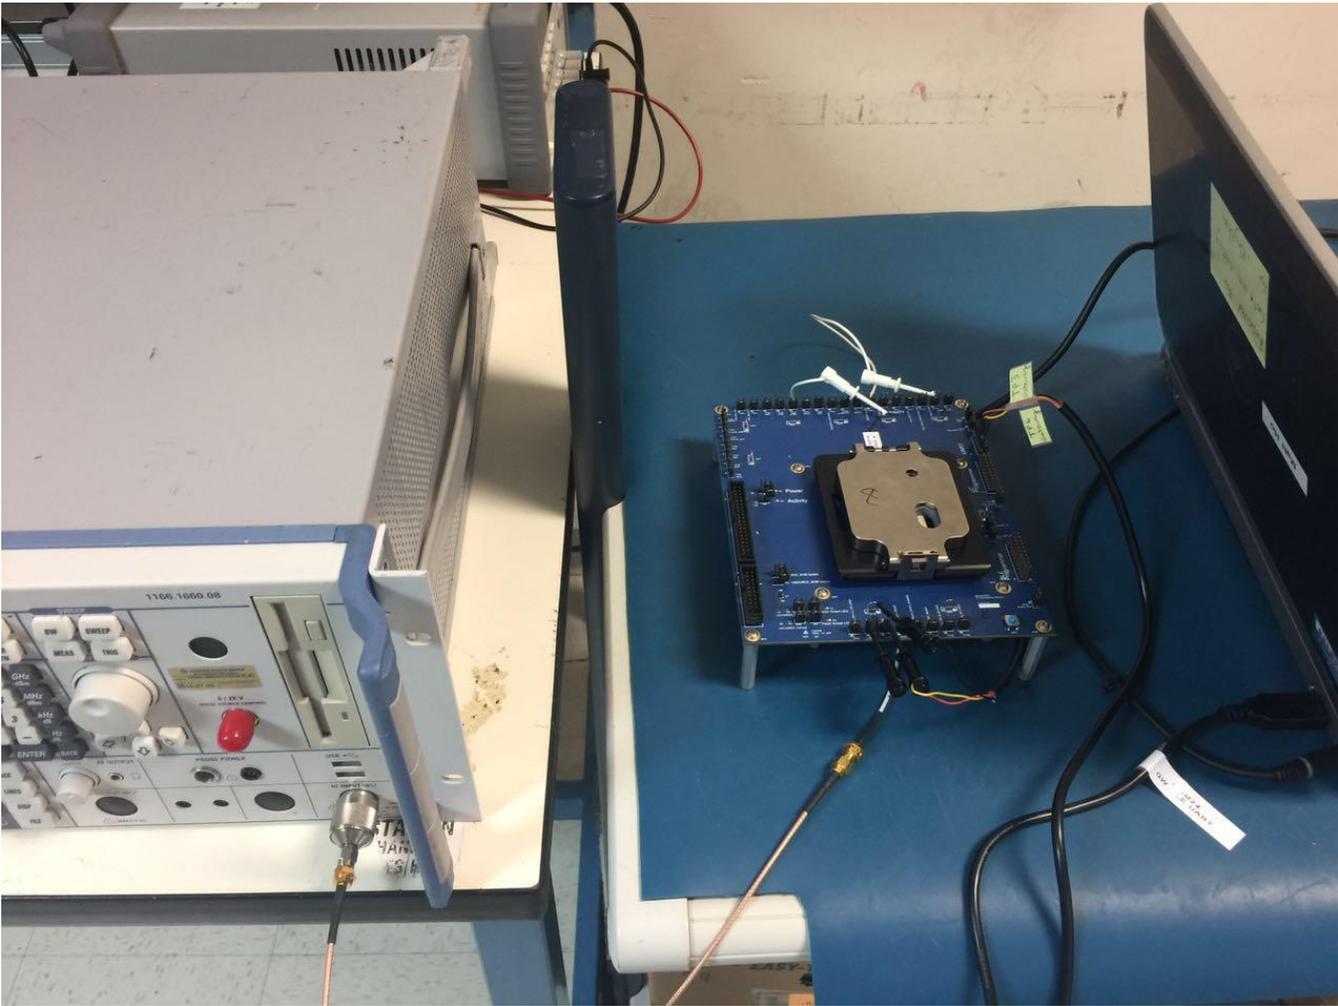

3 Radiated Emissions 9KHz- 30MHz Measurement

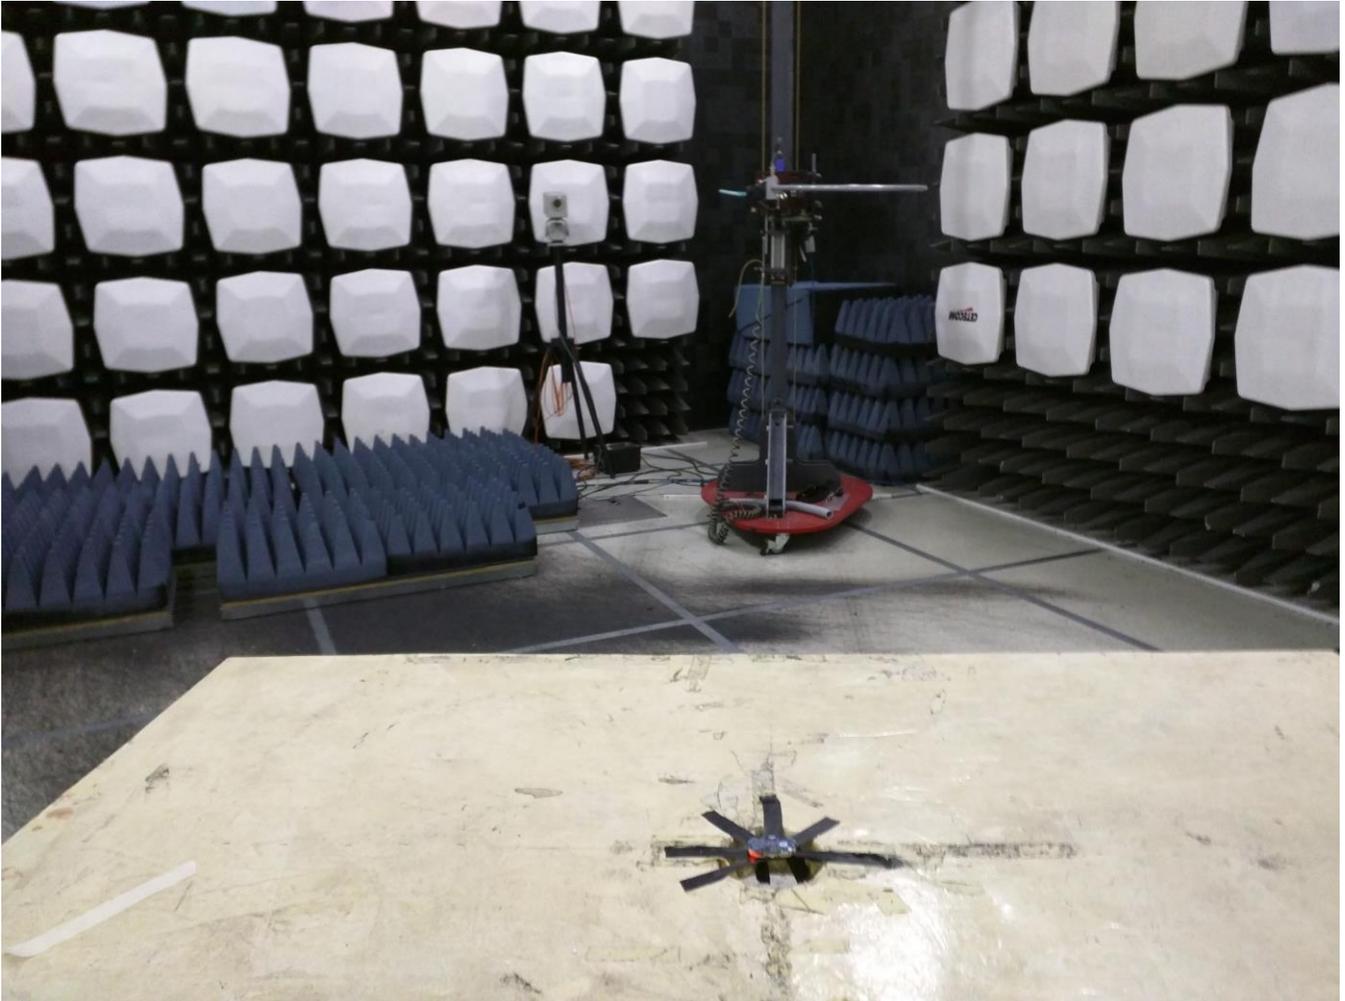


4 Radiated Emissions 30MHz- 1GHz Measurement

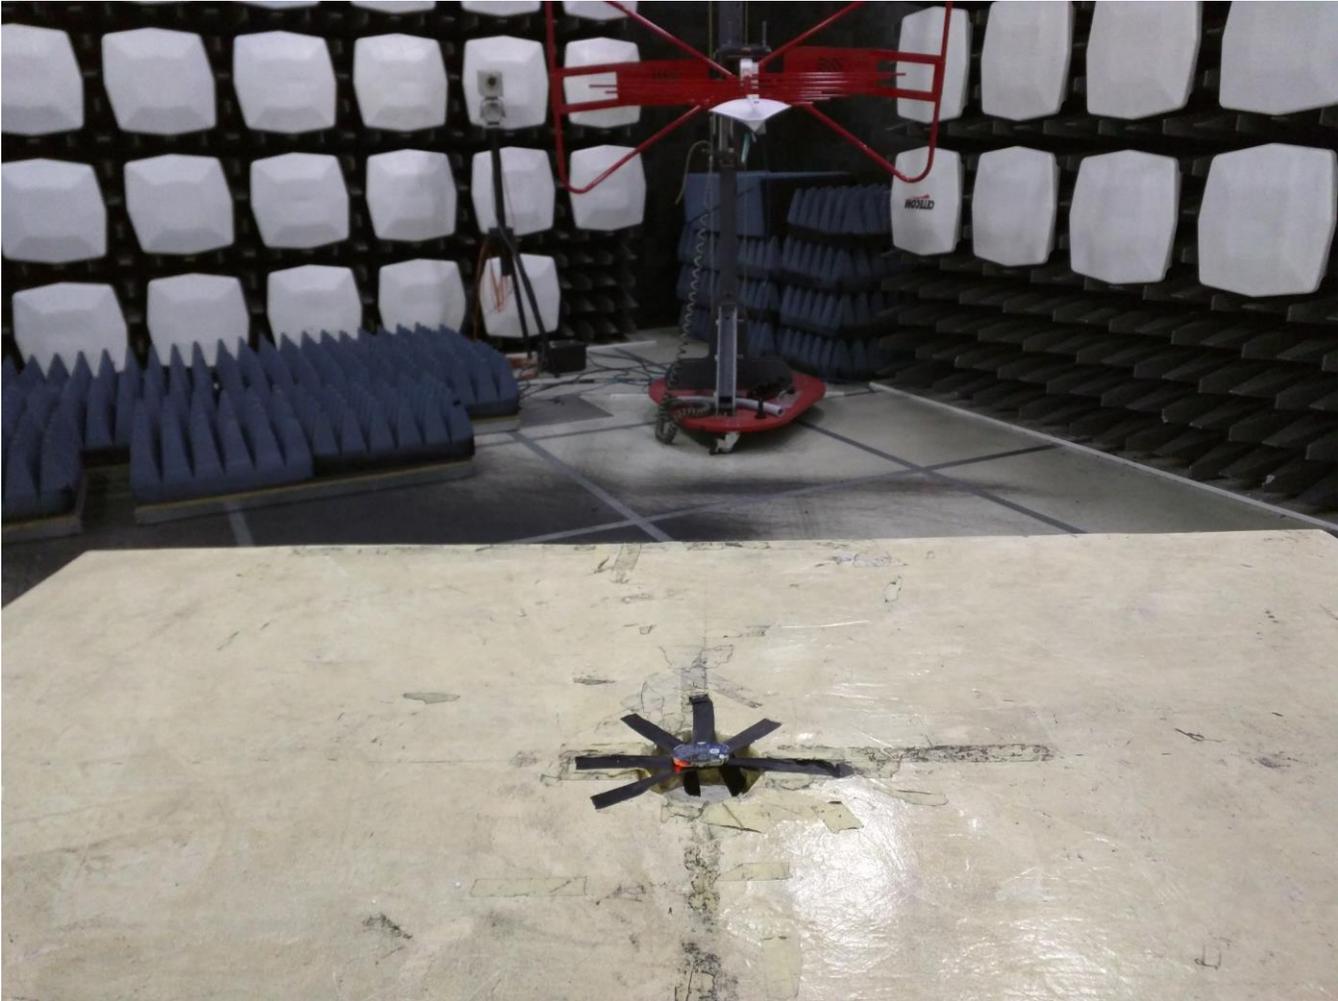

8. Radiated Emissions 1GHz- 3GHz Measurement



5 Radiated Emissions 3GHz- 18GHz Measurement

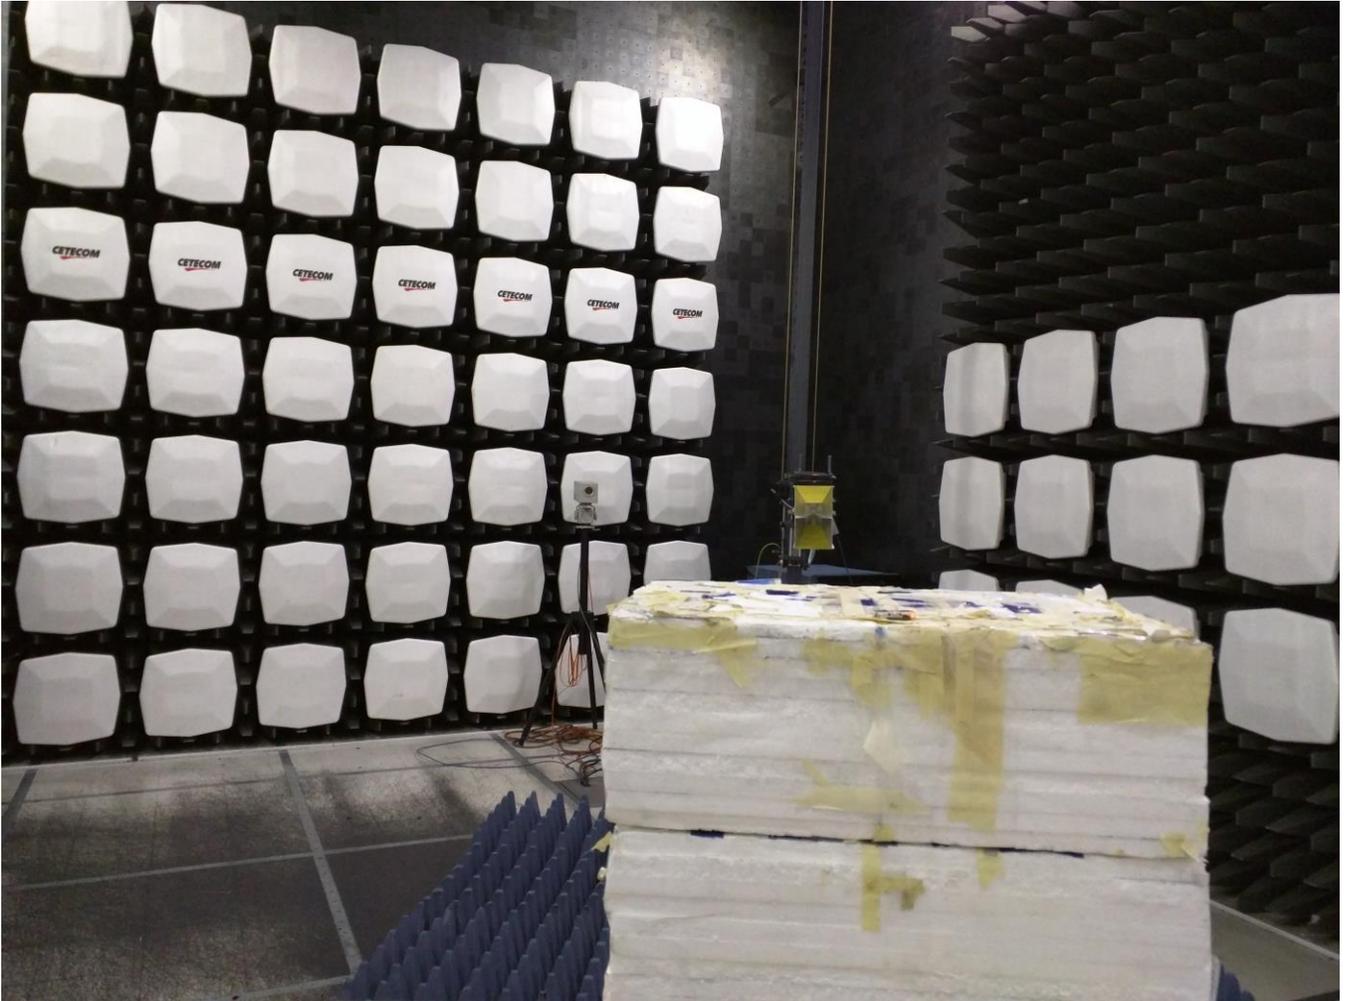

6 Radiated Emissions above 18GHz

