

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid








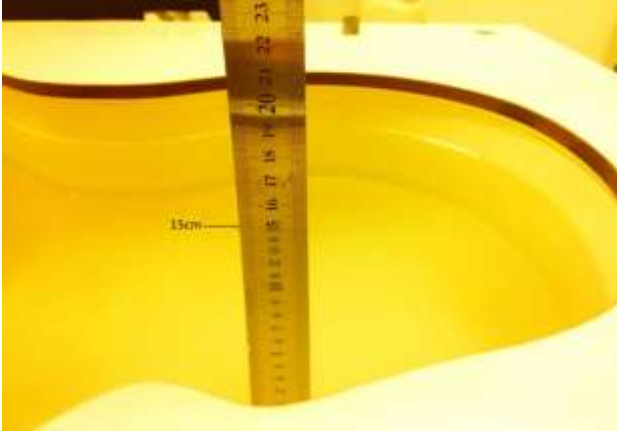
<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Body 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Body 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Body 2450</p>
	

Photo 7: Tissue Simulant Liquid for Head 2600	Photo 8: Tissue Simulant Liquid for Body 2600
	

3. Photographs of EUT test position


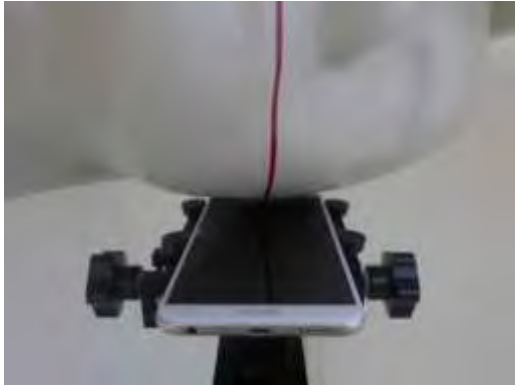


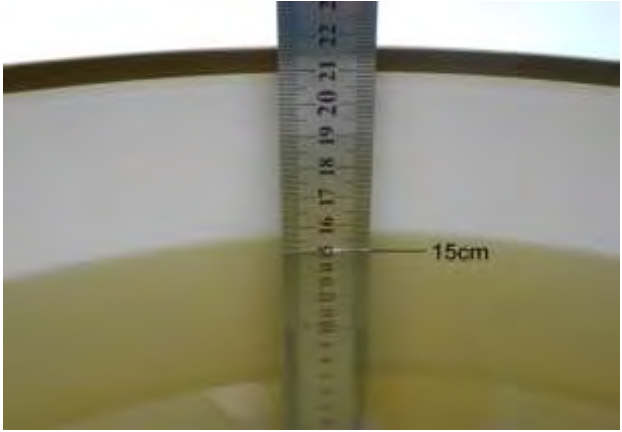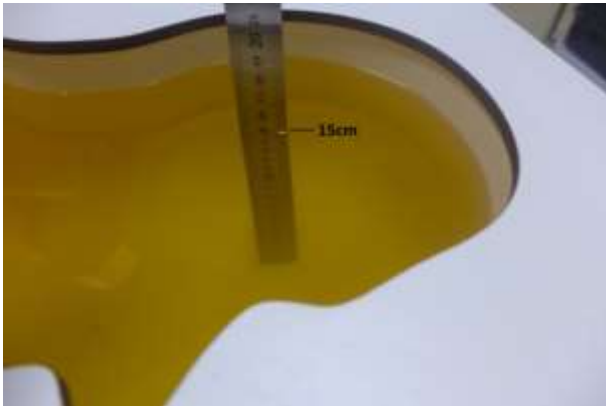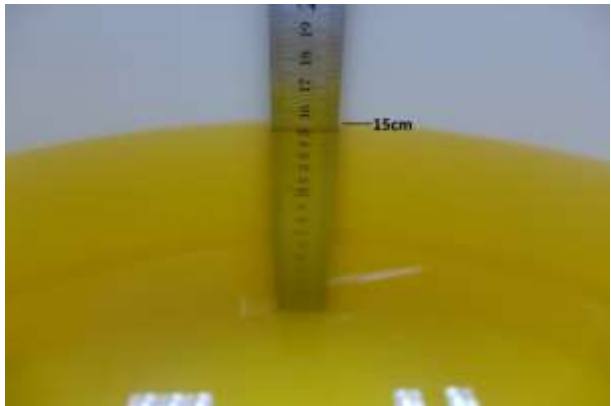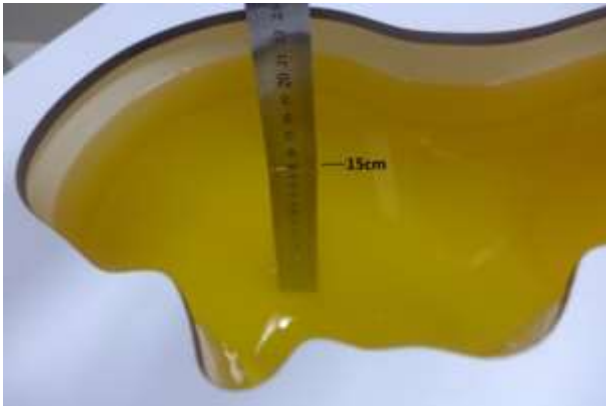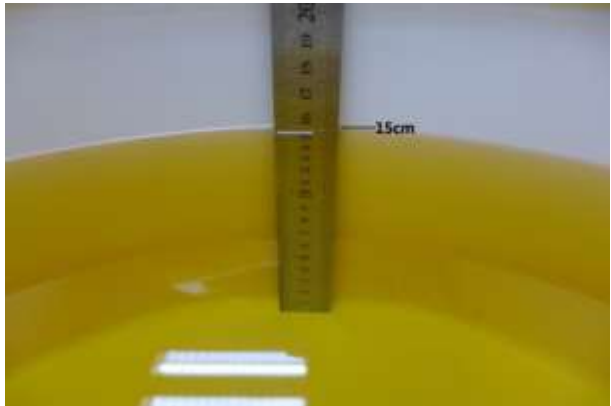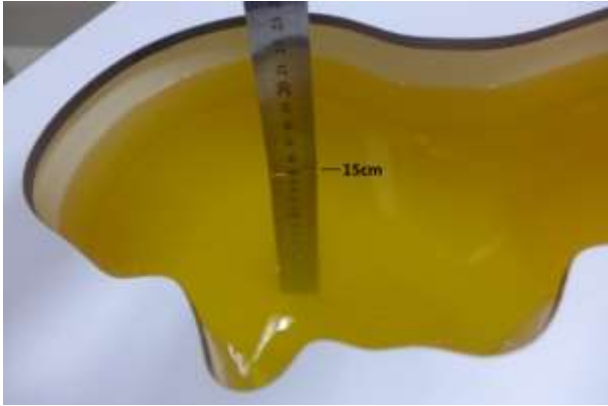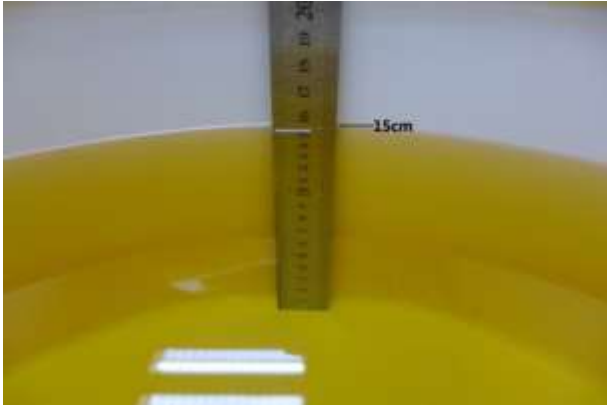

<p>Photo 9: Left touch cheek</p> 	<p>Photo 10: Left tilted 15 degree</p> 
<p>Photo 11: Right touch cheek</p> 	<p>Photo 12: Right tilted 15 degree</p> 
<p>Photo 13: Front side 15mm</p> 	<p>Photo 14: Back side 15mm</p> 






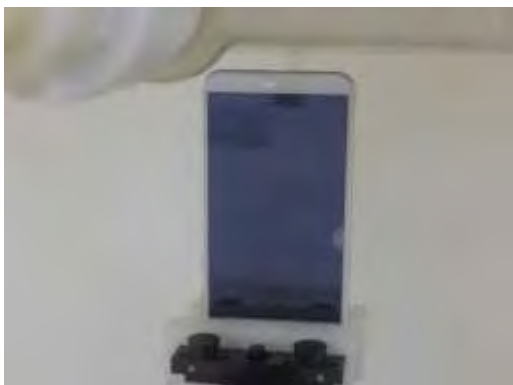



Photo 15: Front side 10mm	Photo 16: Back side 10mm
	
Photo 17: Left side 10mm	Photo 18: Right side 10mm
	
Photo 19: Top side 10mm	Photo 20: Bottom side 10mm
	

Photo 21: Front side 17mm	Photo 22: Back side 17mm
	
Photo 23: Bottom side 17mm	N/A
	N/A

4. EUT Constructional Details




Photo 24: Front View	Photo 25: Back View
	

Photo 26: Accessory	N/A
	<p>N/A</p>