

Test Laboratory: Compliance Certification Services

System Performance Check @ 2450MHz (Body Tissue)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:748

Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.97$ mho/m; $\epsilon_r = 53.1$; $\rho = 1000$ kg/m³
Phantom section: Flat Section


Room Ambient Temperature: 24.0 deg. C; Liquid Temperature: 23.0 deg. C

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV4 - SN3552 ; ConvF(6.94, 6.94, 6.94); Calibrated: 3/19/2005
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 2/7/2005
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

d=10mm, Pin=250mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (measured) = 17.8 mW/g

d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm
Reference Value = 97.2 V/m; Power Drift = 0.044 dB
Peak SAR (extrapolated) = 24.6 W/kg
SAR(1 g) = 12.7 mW/g; SAR(10 g) = 5.97 mW/g
Maximum value of SAR (measured) = 17.4 mW/g

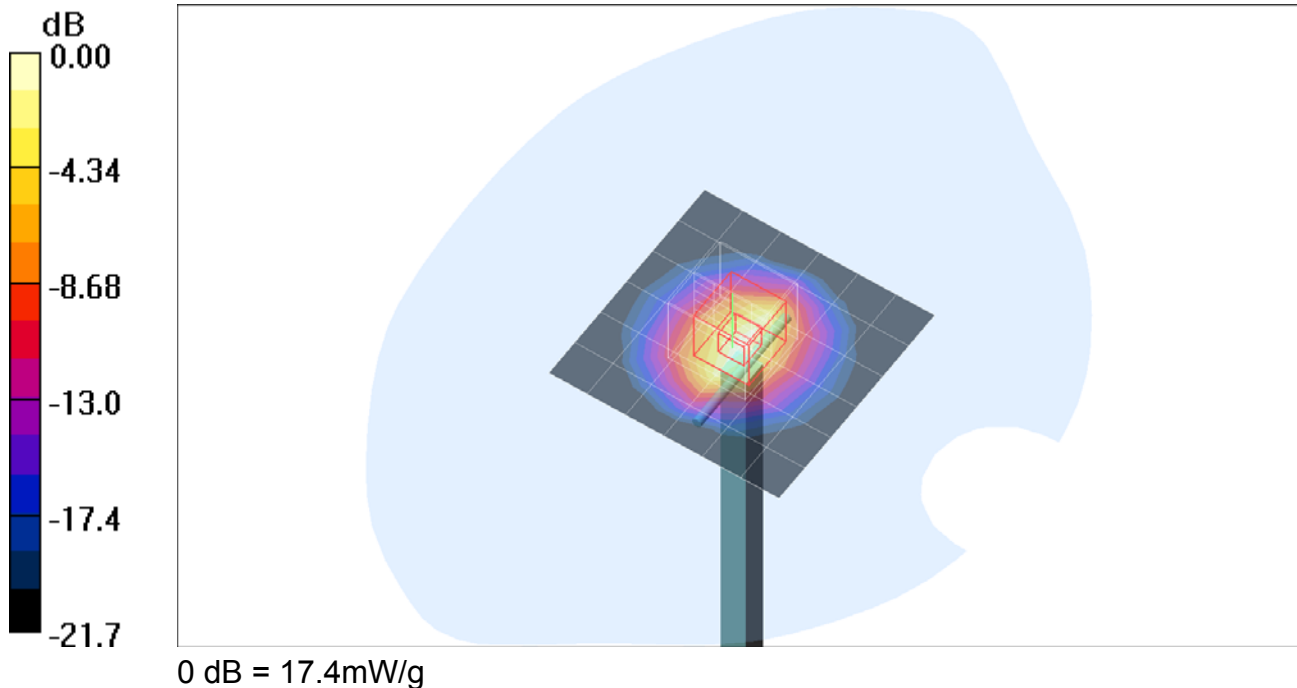


Test Laboratory: Compliance Certification Services

System Performance Check @ 2450MHz (Body Tissue)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:748

Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1

d=10mm, Pin=250mW/Z Scan (1x1x41): Measurement grid: dx=20mm, dy=20mm, dz=2.5mm
Maximum value of SAR (measured) = 16.6 mW/g

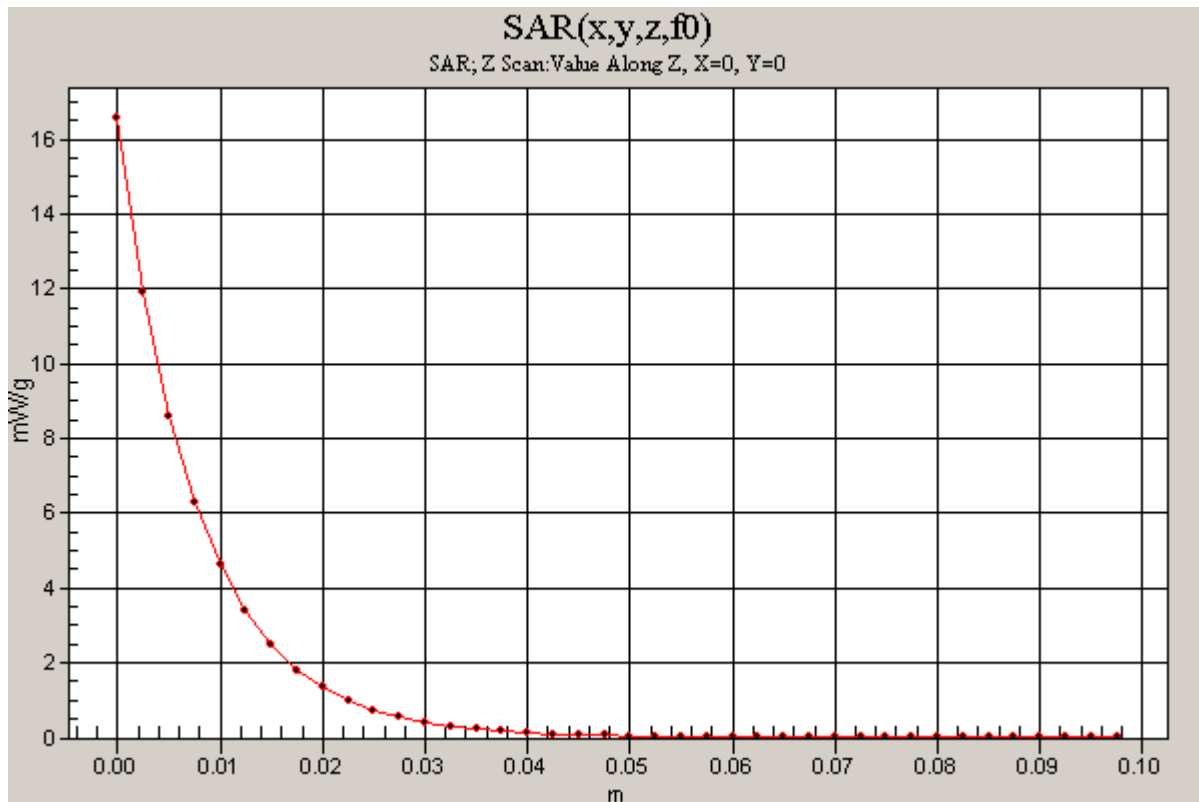

Test Laboratory: Compliance Certification Services

System Performance Check @ 5.2GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5200MHz; Frequency: 5200 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5200$ MHz; $\sigma = 5.4$ mho/m; $\epsilon_r = 50$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Room Ambient Temperature: 25.0 deg. C; Liquid Temperature: 24.5 deg. C

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV4 - SN3552 ; ConvF(4.28, 4.28, 4.28); Calibrated: 3/19/2005
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 2/7/2005
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

d=10mm, Pin=250mW/Area Scan (8x8x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 22.3 mW/g


d=10mm, Pin=250mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 91.1 V/m; Power Drift = -0.040 dB

Peak SAR (extrapolated) = 69.2 W/kg

SAR(1 g) = 18.7 mW/g; SAR(10 g) = 5.29 mW/g

Maximum value of SAR (measured) = 35.8 mW/g

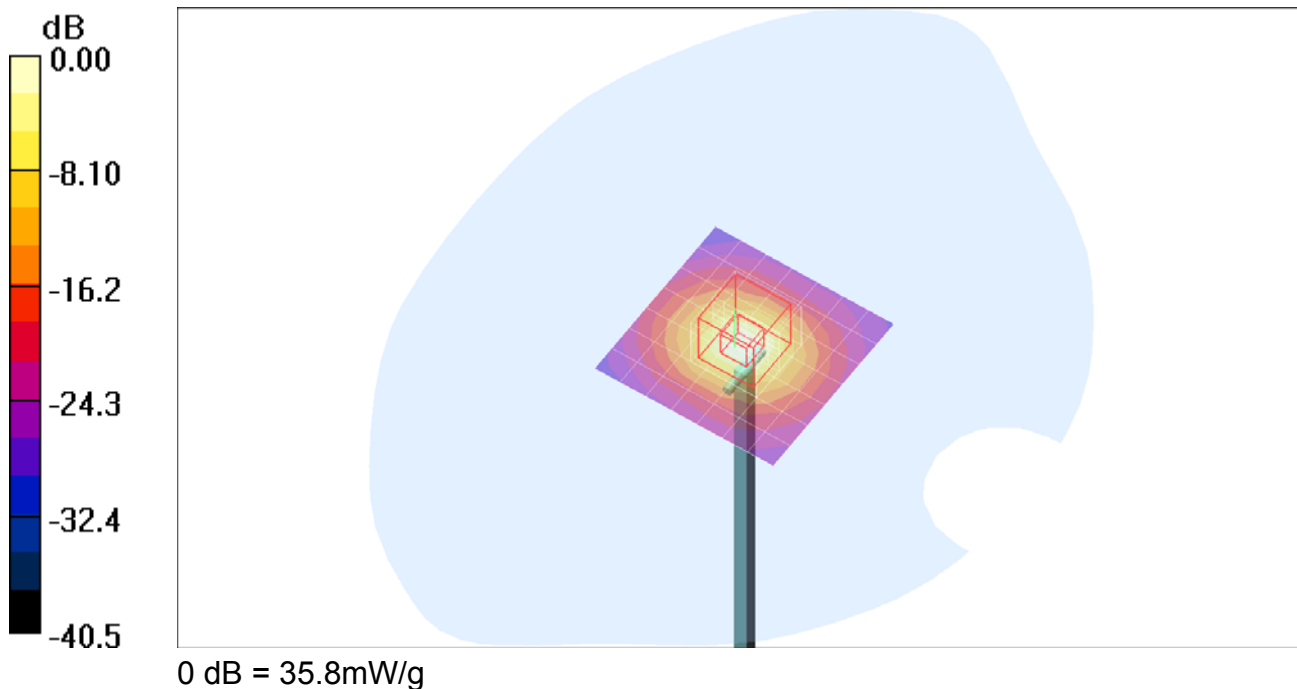


Test Laboratory: Compliance Certification Services

System Performance Check @ 5.2GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5200MHz; Frequency: 5200 MHz;Duty Cycle: 1:1

d=10mm, Pin=250mW/Z Scan (1x1x41): Measurement grid: dx=20mm, dy=20mm, dz=2.5mm
Maximum value of SAR (measured) = 26.5 mW/g

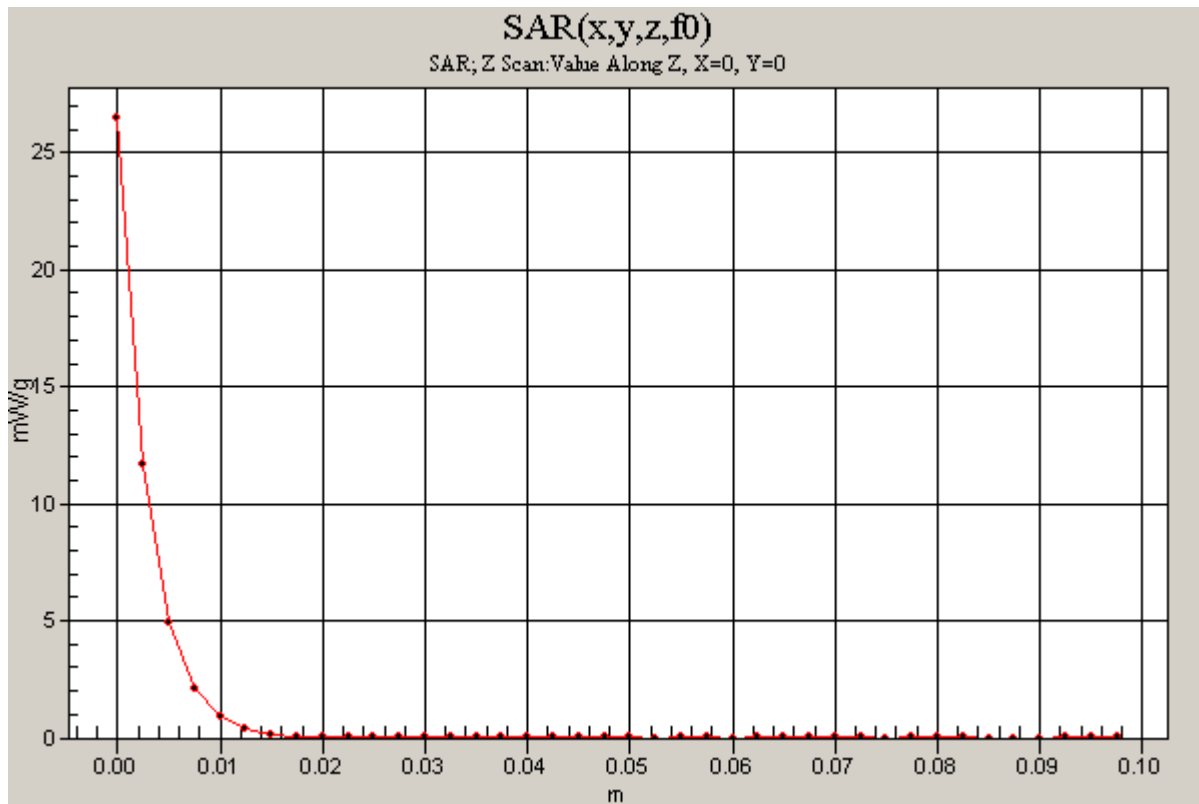

Test Laboratory: Compliance Certification Services

System Performance Check @ 5.8GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5800MHz; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 5800$ MHz; $\sigma = 6.28$ mho/m; $\epsilon_r = 48.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Room Ambient Temperature: 25 deg. C; Liquid Temperature: 24.5 deg. C

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV4 - SN3552 ; ConvF(3.61, 3.61, 3.61); Calibrated: 3/19/2005
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 2/7/2005
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

d=10mm, Pin=250mW/Area Scan (8x8x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 27.2 mW/g


d=10mm, Pin=250mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 87.8 V/m; Power Drift = 0.047 dB

Peak SAR (extrapolated) = 81.4 W/kg

SAR(1 g) = 19.7 mW/g; SAR(10 g) = 5.54 mW/g

Maximum value of SAR (measured) = 39.4 mW/g

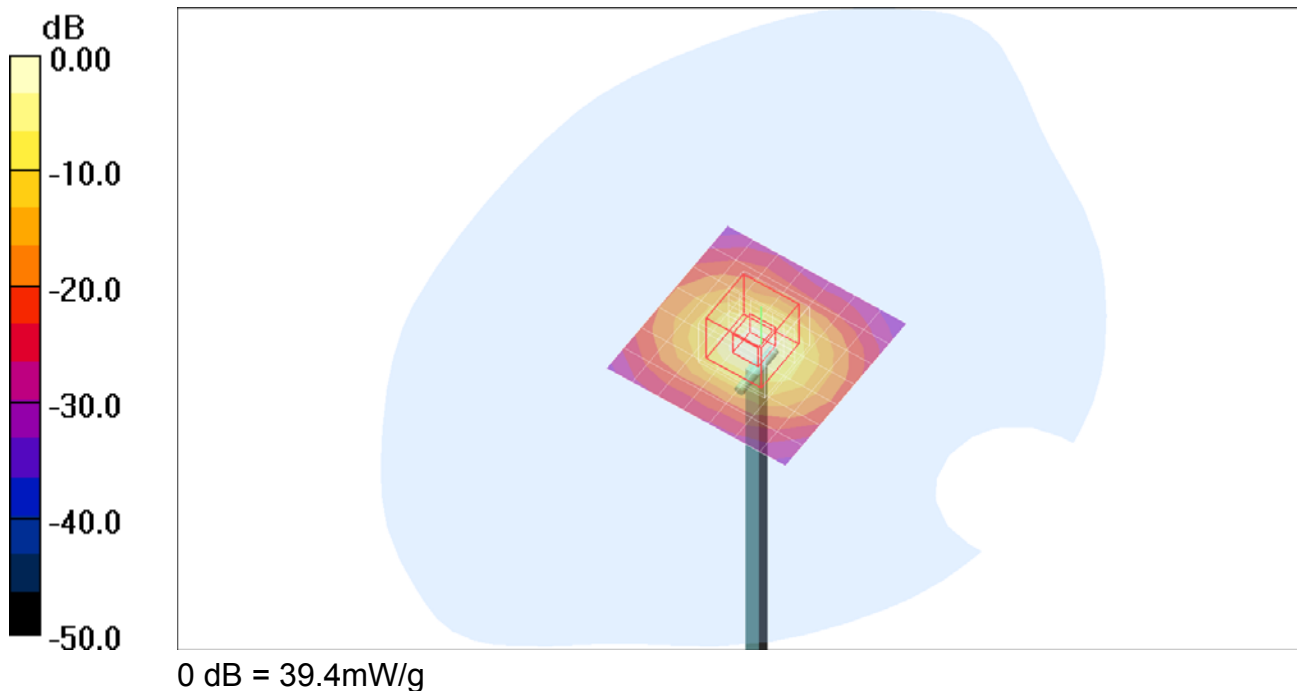


Test Laboratory: Compliance Certification Services

System Performance Check @ 5.8GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5800MHz; Frequency: 5800 MHz;Duty Cycle: 1:1

d=10mm, Pin=250mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 16.0 mW/g

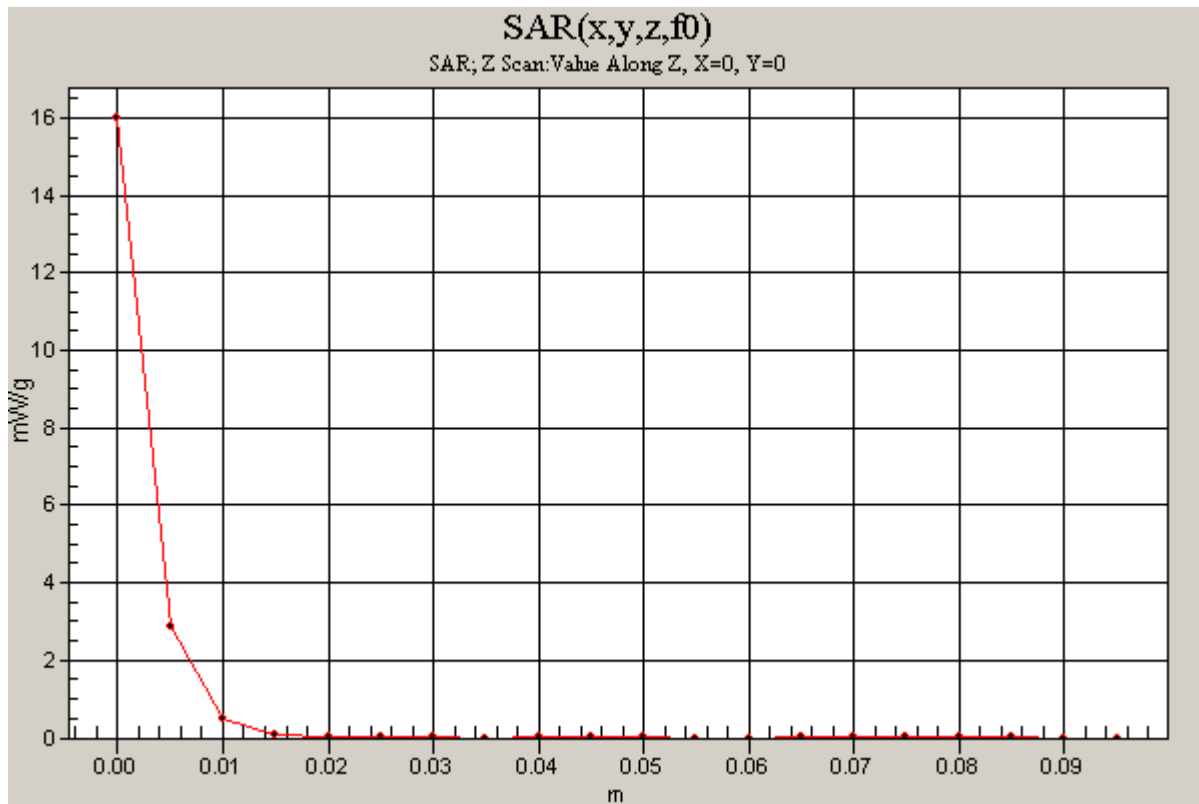

Test Laboratory: Compliance Certification Services

System Performance Check @ 5.2GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5200MHz; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 5200$ MHz; $\sigma = 5.42$ mho/m; $\epsilon_r = 50.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Room Ambient Temperature: 25 deg. C; Liquid Temperature: 24 deg. C

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV4 - SN3552 ; ConvF(4.28, 4.28, 4.28); Calibrated: 3/19/2005
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 2/7/2005
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

d=10mm, Pin=250mW/Area Scan (8x8x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 24.4 mW/g


d=10mm, Pin=250mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 89.6 V/m; Power Drift = 0.158 dB

Peak SAR (extrapolated) = 70.0 W/kg

SAR(1 g) = 18.3 mW/g; SAR(10 g) = 5.16 mW/g

Maximum value of SAR (measured) = 35.6 mW/g

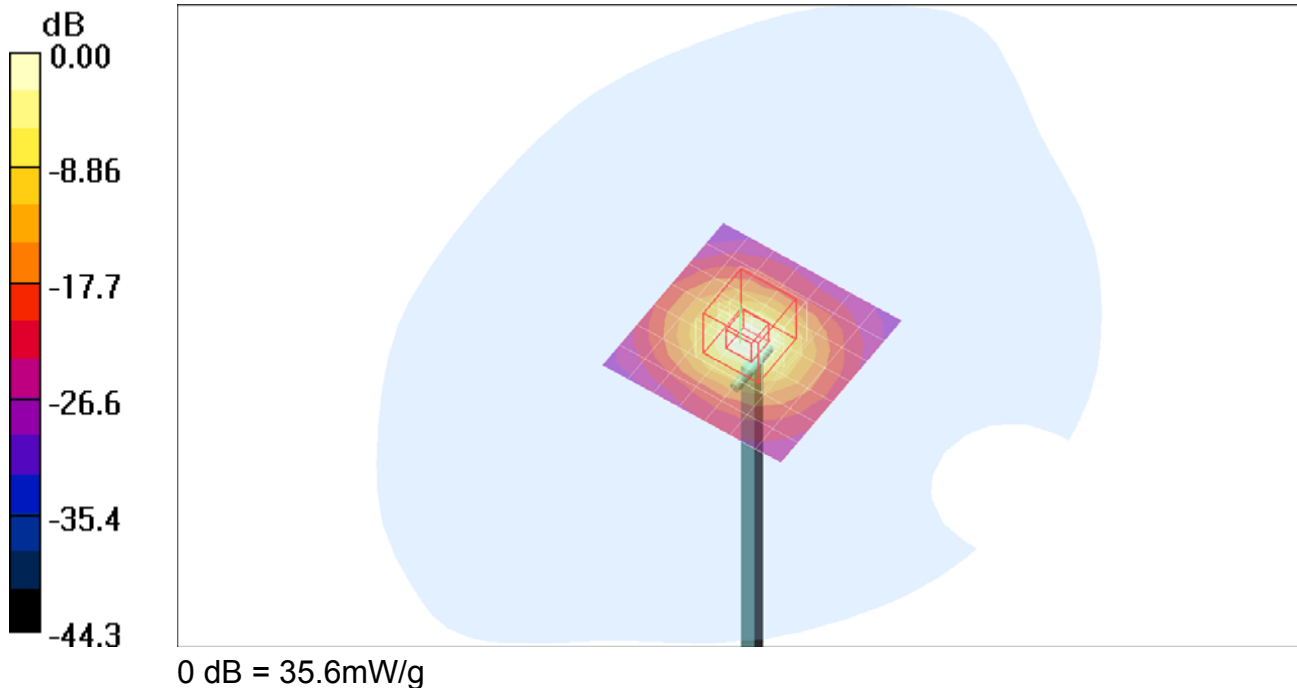


Test Laboratory: Compliance Certification Services

System Performance Check @ 5.2GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5200MHz; Frequency: 5200 MHz;Duty Cycle: 1:1

d=10mm, Pin=250mW/Z Scan (1x1x41): Measurement grid: dx=20mm, dy=20mm, dz=2.5mm
Maximum value of SAR (measured) = 32.9 mW/g

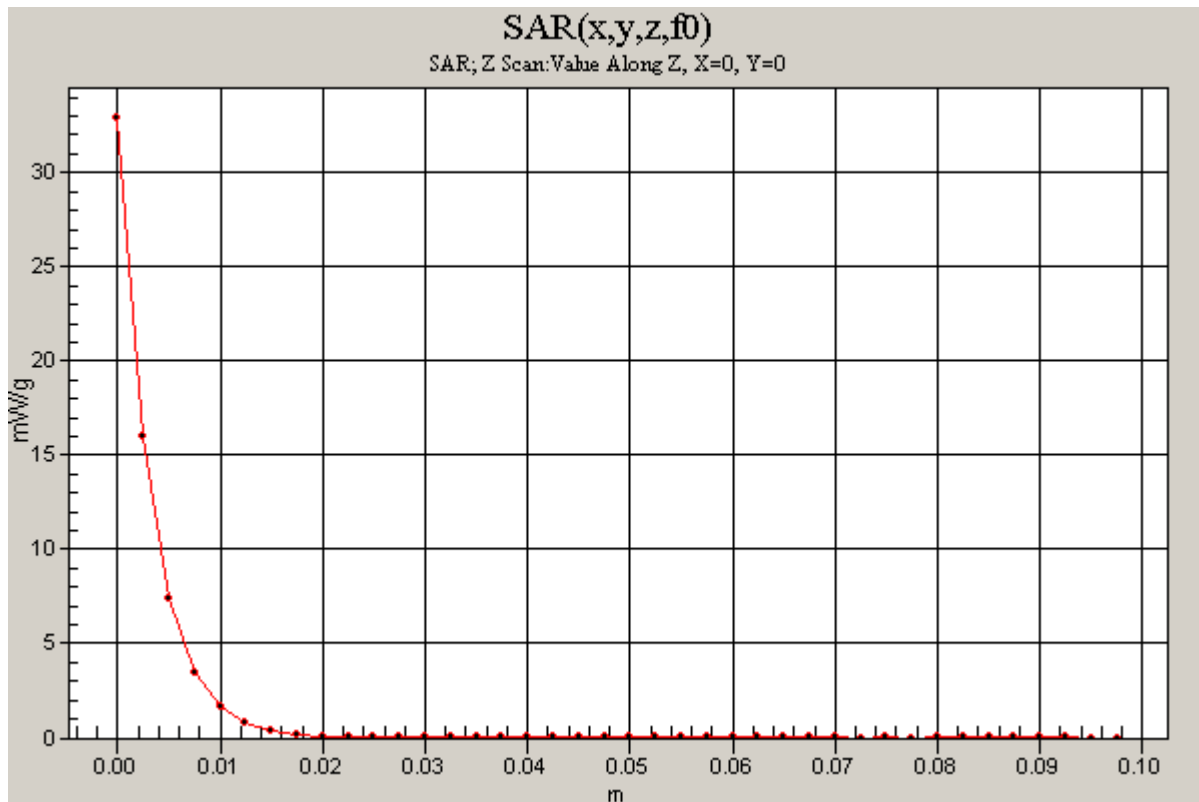

Test Laboratory: Compliance Certification Services

System Performance Check @ 5.8GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5800MHz; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 5800 \text{ MHz}$; $\sigma = 6.29 \text{ mho/m}$; $\epsilon_r = 48.9$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Room Ambient Temperature: 25.0 deg. C; Liquid Temperature: 24.0 deg. C

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV4 - SN3552 ; ConvF(3.61, 3.61, 3.61); Calibrated: 3/19/2005
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 2/7/2005
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

d=10mm, Pin=250mW/Area Scan (8x8x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 25.4 mW/g


d=10mm, Pin=250mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 89.8 V/m; Power Drift = -0.035 dB

Peak SAR (extrapolated) = 81.2 W/kg

SAR(1 g) = 19.5 mW/g; SAR(10 g) = 5.49 mW/g

Maximum value of SAR (measured) = 38.1 mW/g

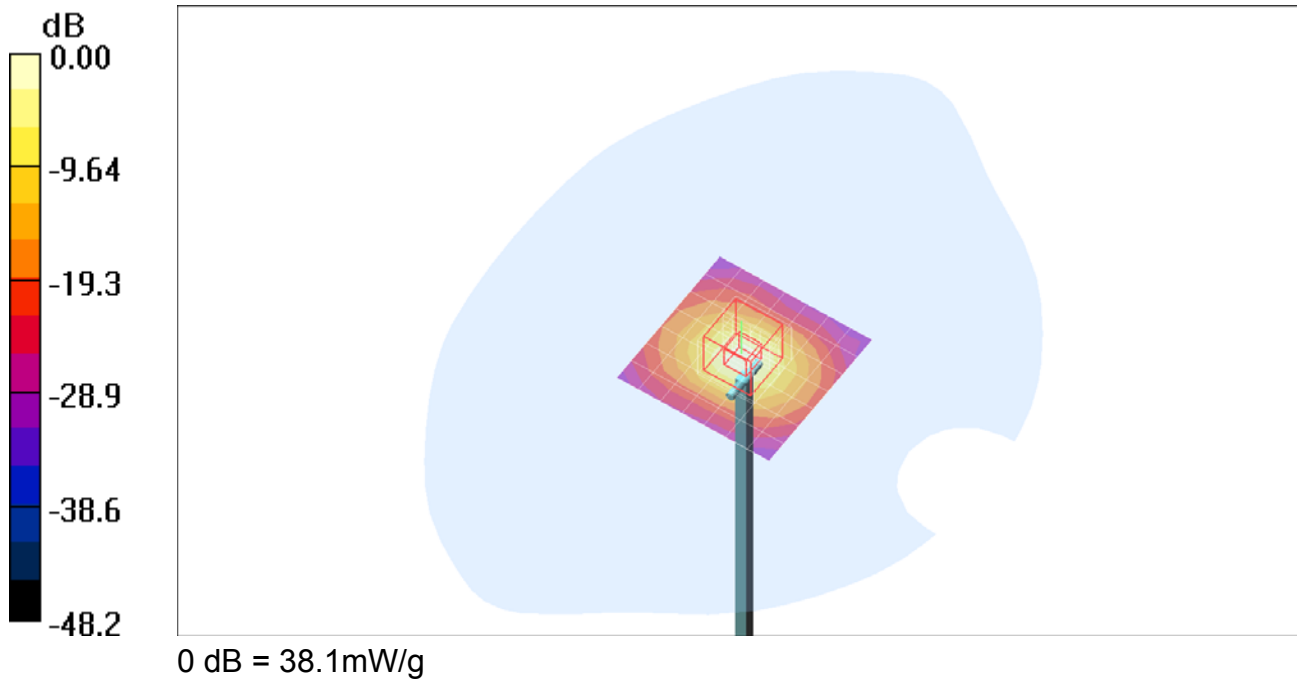


Test Laboratory: Compliance Certification Services

System Performance Check @ 5.8GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5800MHz; Frequency: 5800 MHz;Duty Cycle: 1:1

d=10mm, Pin=250mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 15.4 mW/g

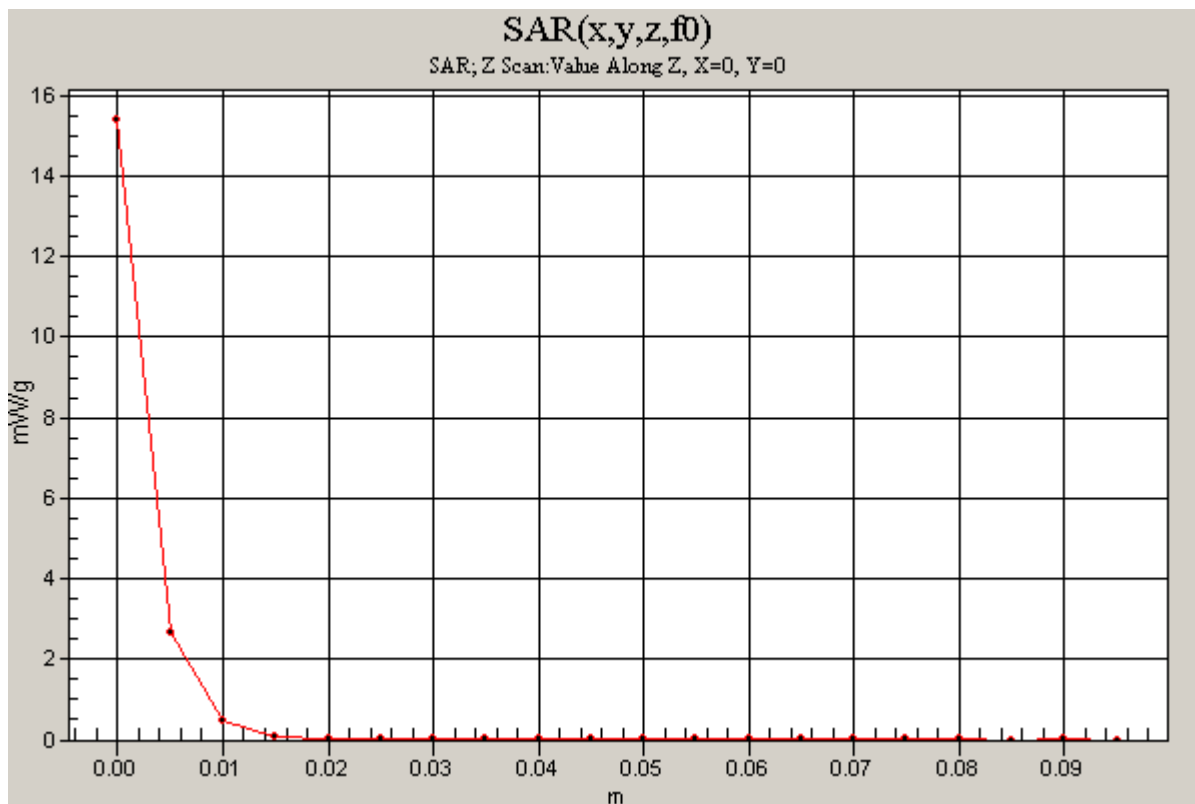

Test Laboratory: Compliance Certification Services

System Performance Check @ 2450MHz (Body Tissue)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:748

Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.93$ mho/m; $\epsilon_r = 52.4$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

Room Ambient Temperature: 25.0 deg. C; Liquid Temperature: 24.0 deg. C

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV4 - SN3552 ; ConvF(6.94, 6.94, 6.94); Calibrated: 3/19/2005
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 2/7/2005
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

d=10mm, Pin=250mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 17.2 mW/g


d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 95.9 V/m; Power Drift = 0.112 dB

Peak SAR (extrapolated) = 24.2 W/kg

SAR(1 g) = 12.5 mW/g; SAR(10 g) = 5.86 mW/g

Maximum value of SAR (measured) = 16.9 mW/g

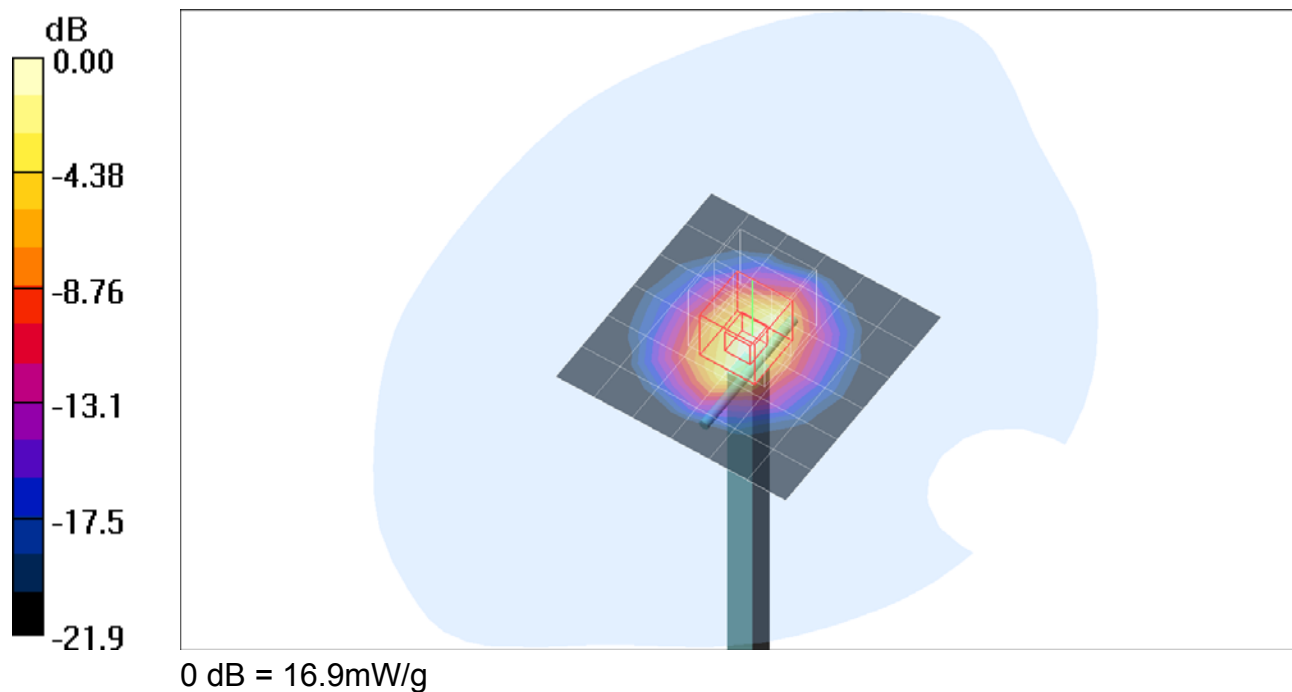


Test Laboratory: Compliance Certification Services

System Performance Check @ 2450MHz (Body Tissue)

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:748

Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1

d=10mm, Pin=250mW/Z Scan (1x1x41): Measurement grid: dx=20mm, dy=20mm, dz=2.5mm
Maximum value of SAR (measured) = 17.7 mW/g

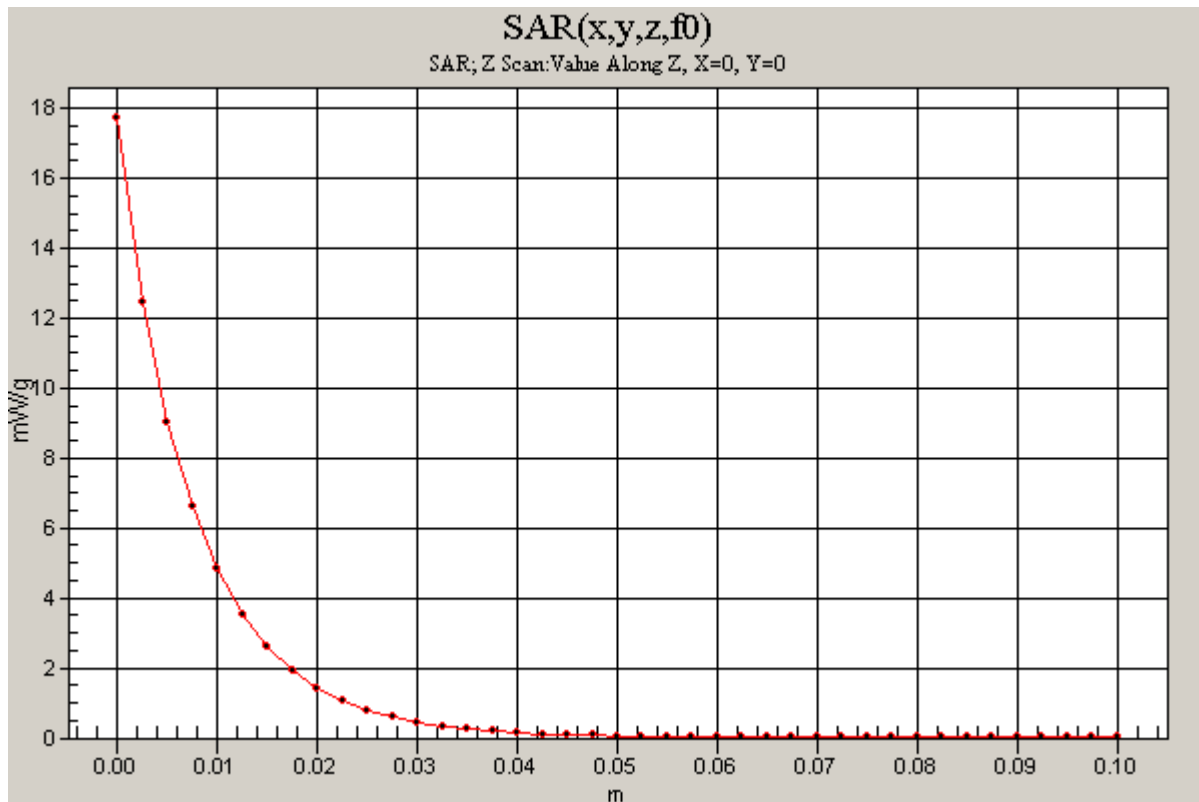

Test Laboratory: Compliance Certification Services

System Performance Check @ 5.8GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5800MHz; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 5800 \text{ MHz}$; $\sigma = 6.29 \text{ mho/m}$; $\epsilon_r = 48.8$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Room Ambient Temperature: 25.0 deg. C; Liquid Temperature: 24.5 deg. C

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV4 - SN3552 ; ConvF(3.61, 3.61, 3.61); Calibrated: 3/19/2005
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 2/7/2005
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

d=10mm, Pin=250mW/Area Scan (8x8x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 22.9 mW/g


d=10mm, Pin=250mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm

Reference Value = 88.5 V/m; Power Drift = -0.024 dB

Peak SAR (extrapolated) = 79.3 W/kg

SAR(1 g) = 19.1 mW/g; SAR(10 g) = 5.36 mW/g

Maximum value of SAR (measured) = 37.5 mW/g

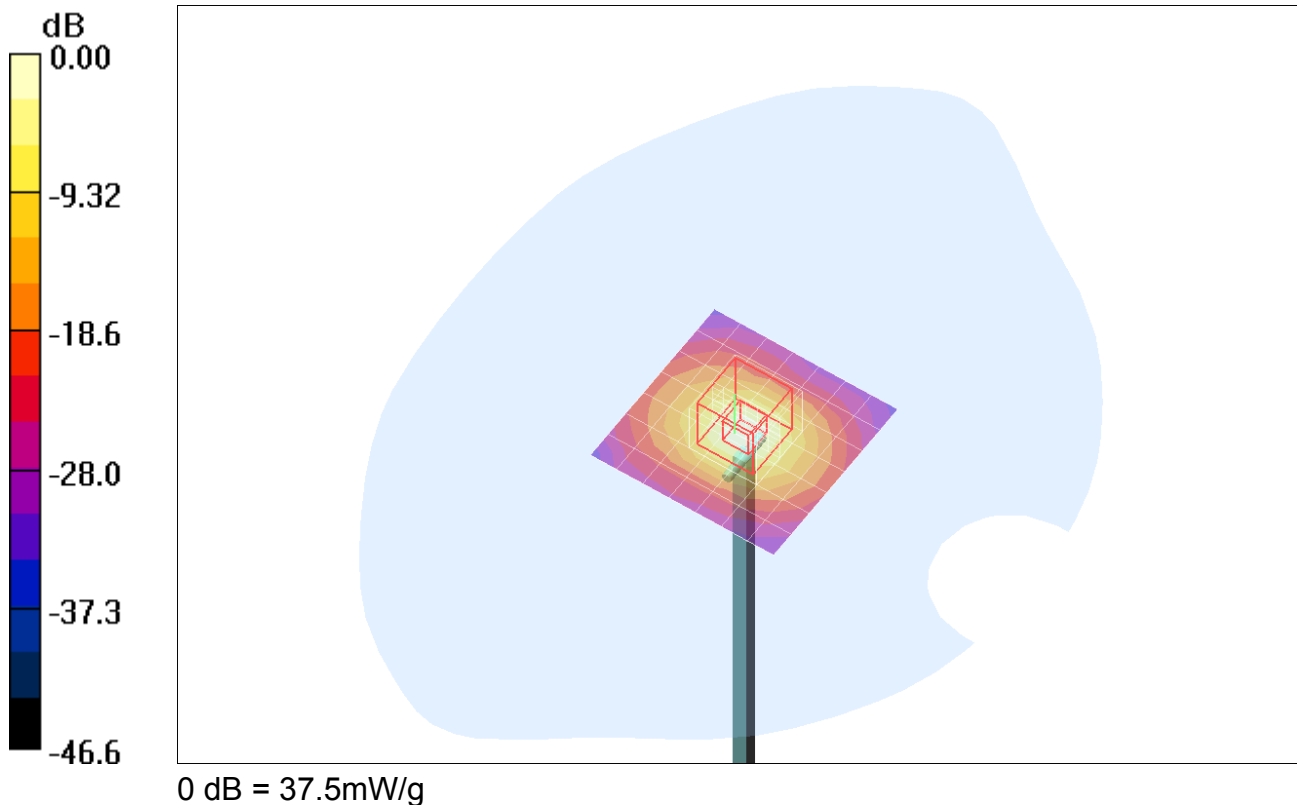

Test Laboratory: Compliance Certification Services

System Performance Check @ 5.8GHz (Body Tissue)

DUT: Dipole 5200-5800MHz; Type: D5GHzV2; Serial: 1003

Communication System: CW 5800MHz; Frequency: 5800 MHz;Duty Cycle: 1:1

d=10mm, Pin=250mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 15.2 mW/g

