

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1148

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.34 S/m; perm = 41.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/26/2022; Ambient Temp: 21.5°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7670; ConvF:(8.53,8.53,8.53); Calibrated: 2021-08-05
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2021-08-03
Phantom: Twin-SAM V8.0; Serial: 1630
Measurement SW: DASY Module SAR V16.0.2.136

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.85 W/kg

SAR(1 g) = 3.63 W/kg

Deviation (1 g) = -2.42%

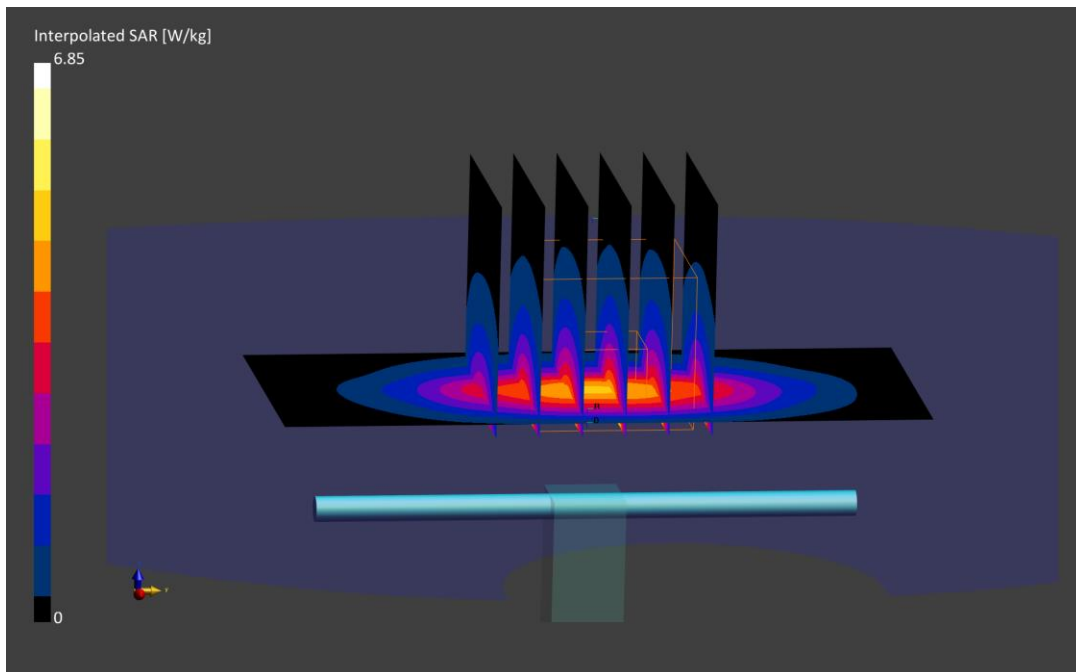

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1150

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.38 S/m; perm = 39.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/01/2022; Ambient Temp: 22.0°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7527; ConvF:(8.21,8.21,8.21); Calibrated: 2022-03-21
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1272; Calibrated: 2022-03-16
Phantom: Twin-SAM V5.0; Serial: 1757
Measurement SW: DASY Module SAR V16.0.0.116

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.11 W/kg

SAR(1 g) = 3.74 W/kg

Deviation (1 g) = 1.36%

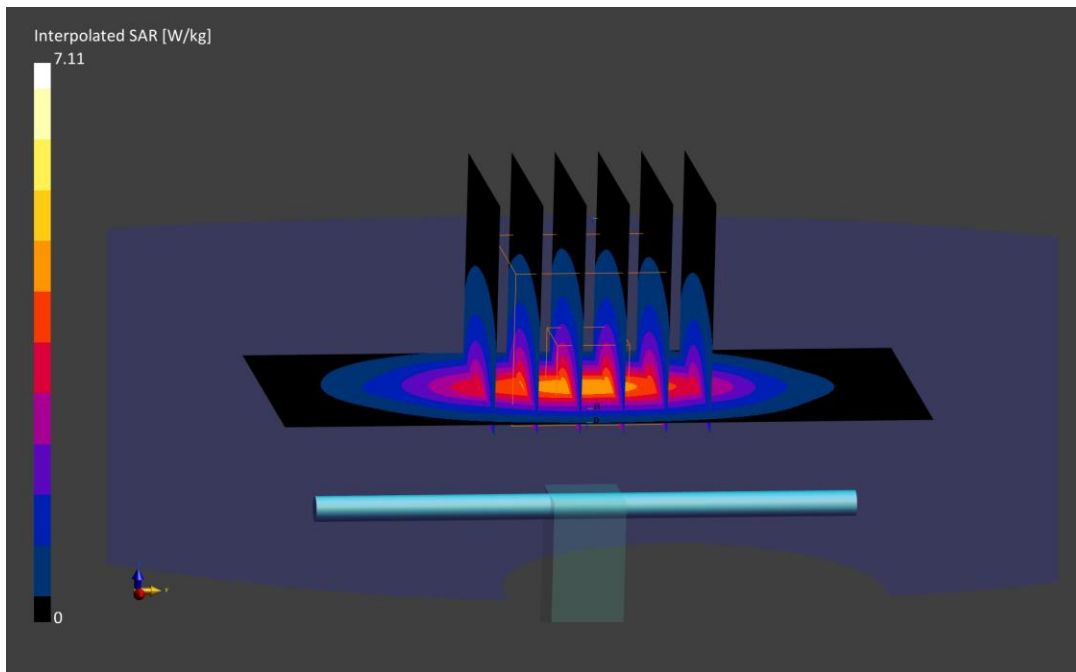

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1073

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2300.0 MHz; cond = 1.65 S/m; perm = 40.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/02/2022; Ambient Temp: 19.7°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7409; ConvF:(7.52,7.52,7.52); Calibrated: 2022-06-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14
Phantom: Twin-SAM V5.0; Serial: 1792
Measurement SW: DASY Module SAR V16.0.2.136

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.3 W/kg

SAR(1 g) = 4.84 W/kg

Deviation (1 g) = -2.22%

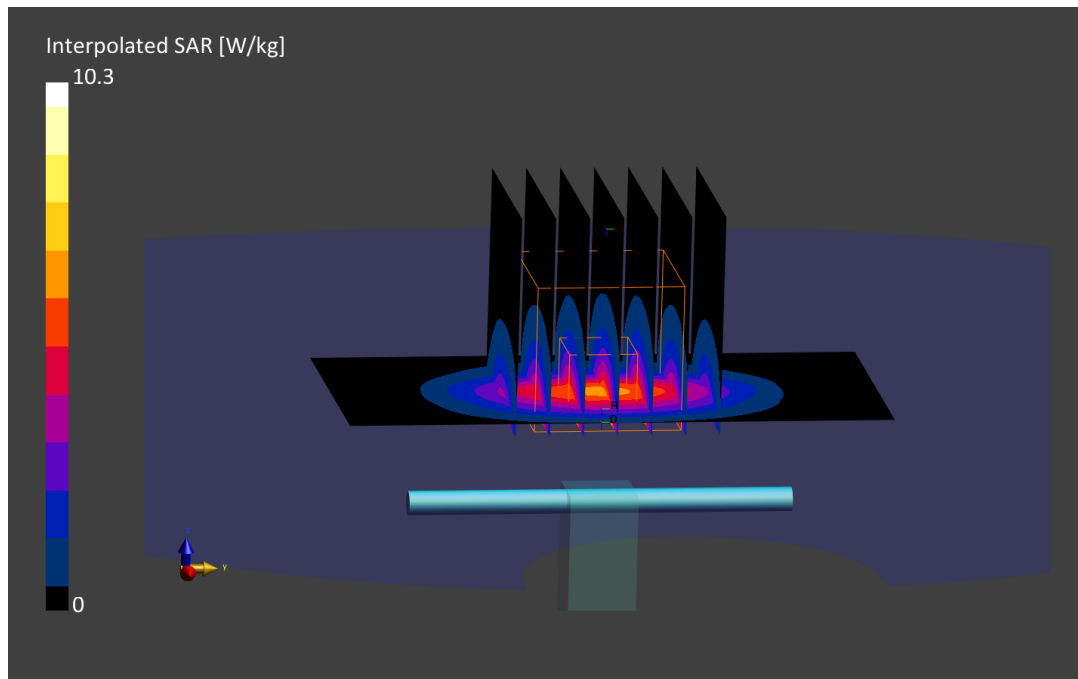

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1073

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2300.0 MHz; cond = 1.67 S/m; perm = 40.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/04/2022; Ambient Temp: 23.5°C; Tissue Temp: 23.8°C

Probe: EX3DV4 - SN7409; ConvF:(7.52,7.52,7.52); Calibrated: 2022-06-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14
Phantom: Twin-SAM V5.0; Serial: 1792
Measurement SW: DASY Module SAR V16.0.2.136

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.3 W/kg

SAR(1 g) = 5.04 W/kg

Deviation (1 g) = 1.82%

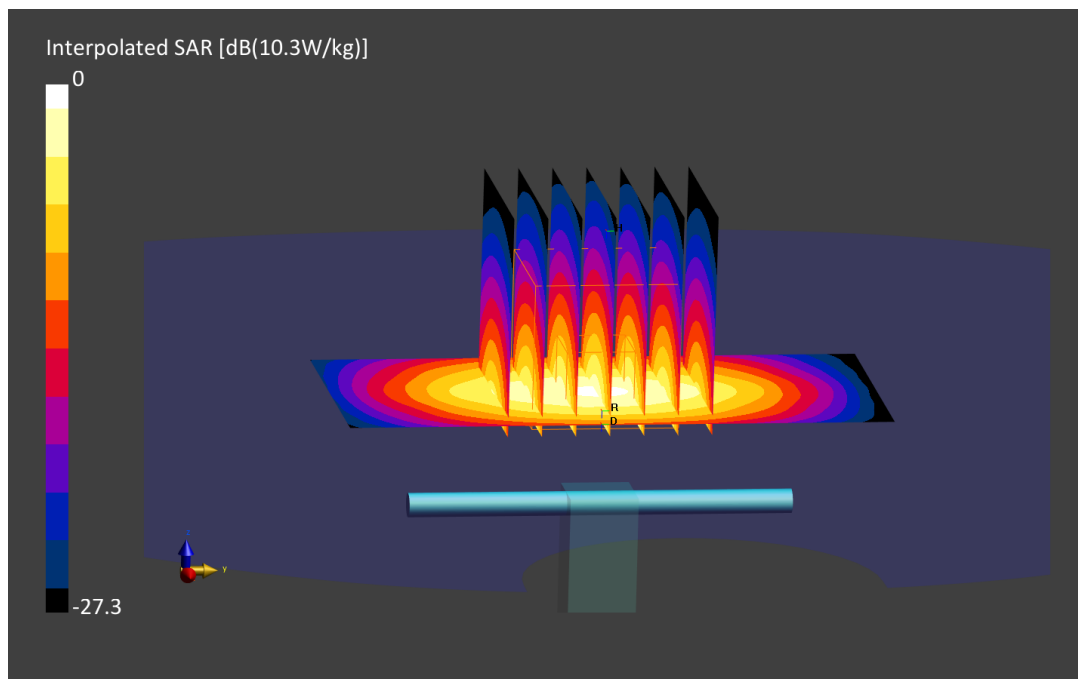

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN719

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.85 S/m; perm = 40.2; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/01/2022; Ambient Temp: 19.9°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7417; ConvF:(7.5,7.5,7.5); Calibrated: 2022-02-22

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn665; Calibrated: 2022-02-22

Phantom: Twin-SAM V8.0; Serial: 2060

Measurement SW: DASY Module SAR V16.0.2.83

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.1 W/kg

SAR(1 g) = 5.22 W/kg

Deviation (1 g) = -5.09%

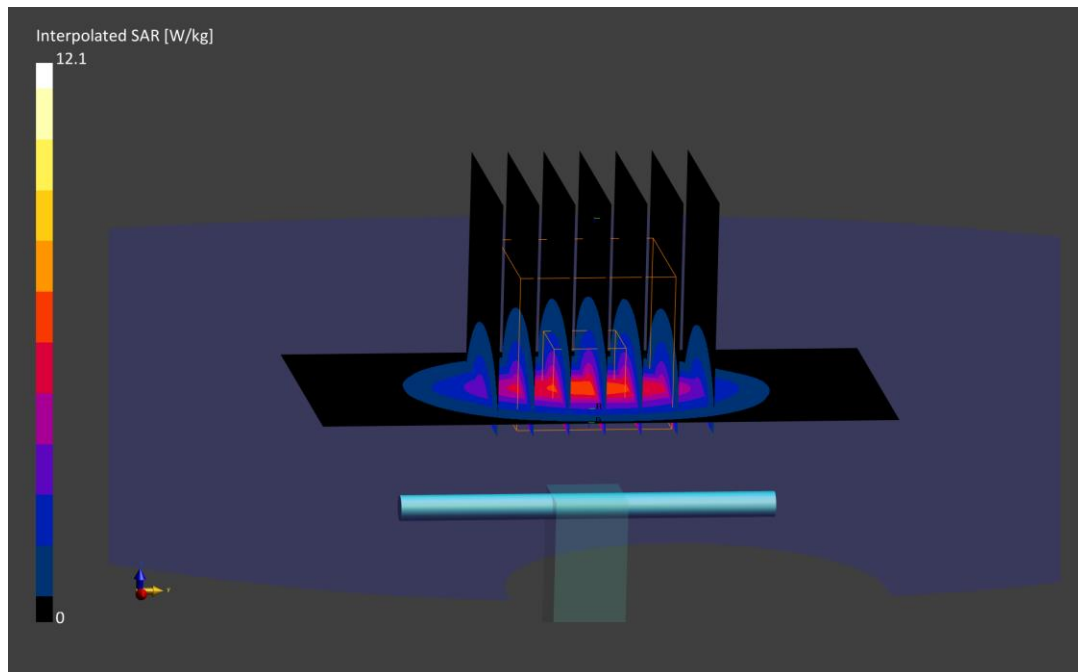

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN797

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.82 S/m; perm = 40.0; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/02/2022; Ambient Temp: 19.7°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7409; ConvF:(7.21,7.21,7.21); Calibrated: 2022-06-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1334; Calibrated: 2022-06-14

Phantom: Twin-SAM V5.0; Serial: 1792

Measurement SW: DASY Module SAR V16.0.2.136

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.9 W/kg

SAR(1 g) = 5.27 W/kg

Deviation (1 g) = 0.57%

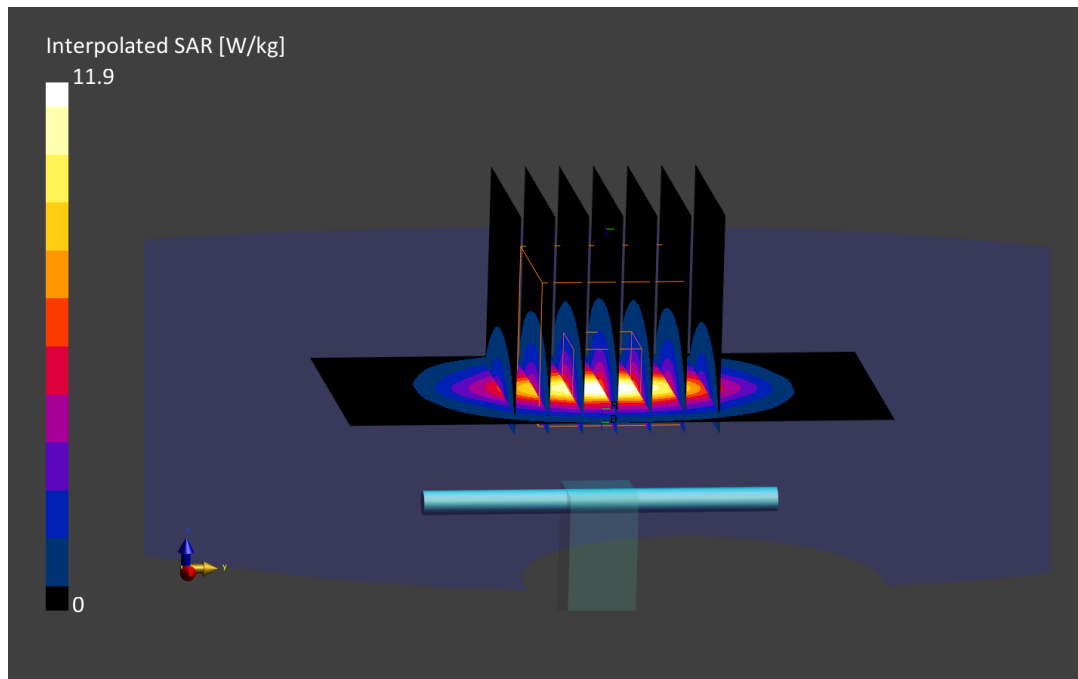

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN981

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.82 S/m; perm = 40.4; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/07/2022; Ambient Temp: 22.3°C; Tissue Temp: 22.2°C

Probe: EX3DV4 - SN7538; ConvF:(7.58,7.58,7.58); Calibrated: 2021-11-16

Sensor-Surface: 1.4mm (All points)

Electronics: DAE4 Sn1323; Calibrated: 2021-11-10

Phantom: Twin-SAM V8.0; Serial: 2056

Measurement SW: DASY Module SAR V16.0.2.83

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.4 W/kg

SAR(1 g) = 5.18 W/kg

Deviation (1 g) = -3.90%

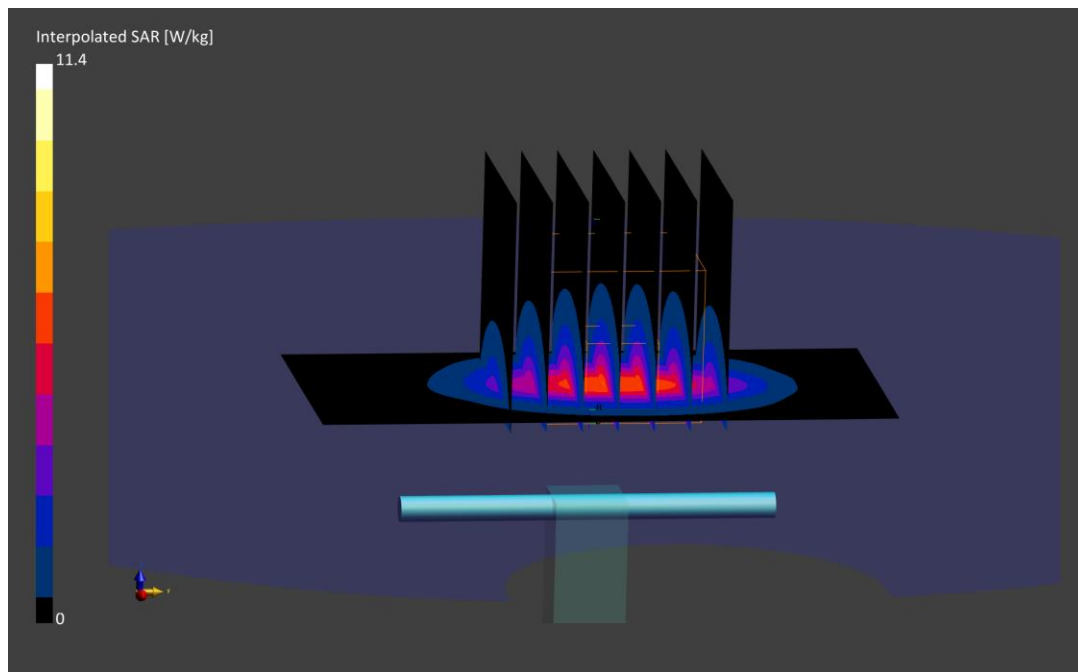

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN981

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.86 S/m; perm = 40.0; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/09/2022; Ambient Temp: 20.3°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7409; ConvF:(7.21,7.21,7.21); Calibrated: 2022-06-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1334; Calibrated: 2022-06-14

Phantom: Twin-SAM V5.0; Serial: 1792

Measurement SW: DASY Module SAR V16.0.2.136

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.2 W/kg

SAR(1 g) = 5.32 W/kg

Deviation (1 g) = -1.30%

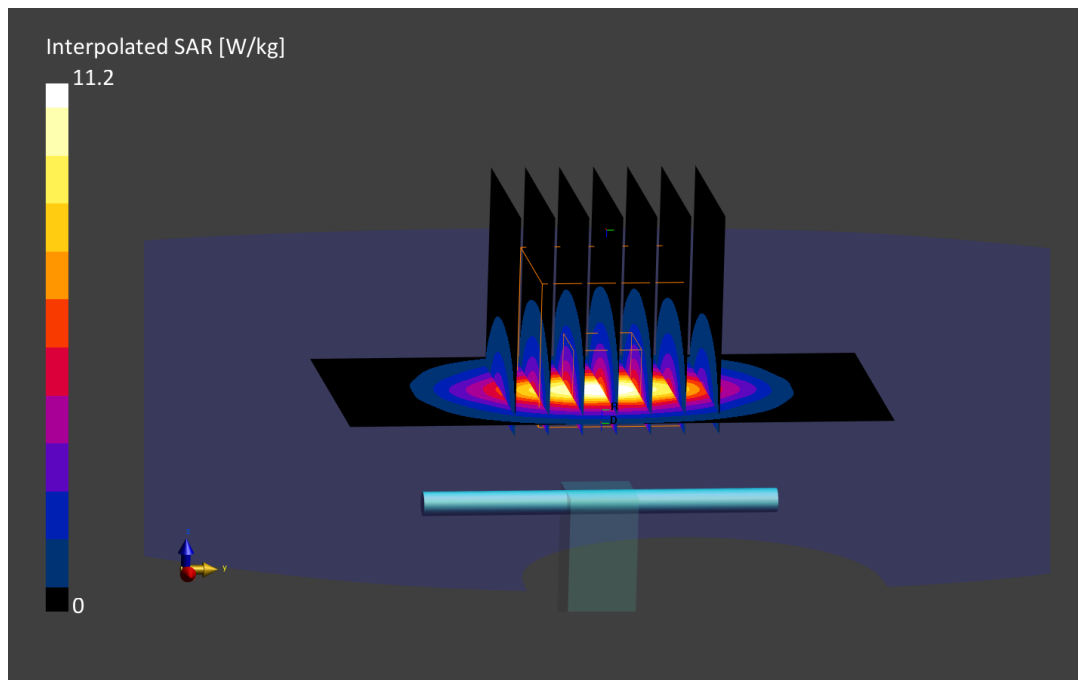

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1064

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.00 S/m; perm = 39.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/02/2022; Ambient Temp: 19.7°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7409; ConvF:(6.97,6.97,6.97); Calibrated: 2022-06-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14
Phantom: Twin-SAM V5.0; Serial: 1792
Measurement SW: DASY Module SAR V16.0.2.136

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 13.2 W/kg

SAR(1 g) = 5.50 W/kg

Deviation (1 g) = -2.48%

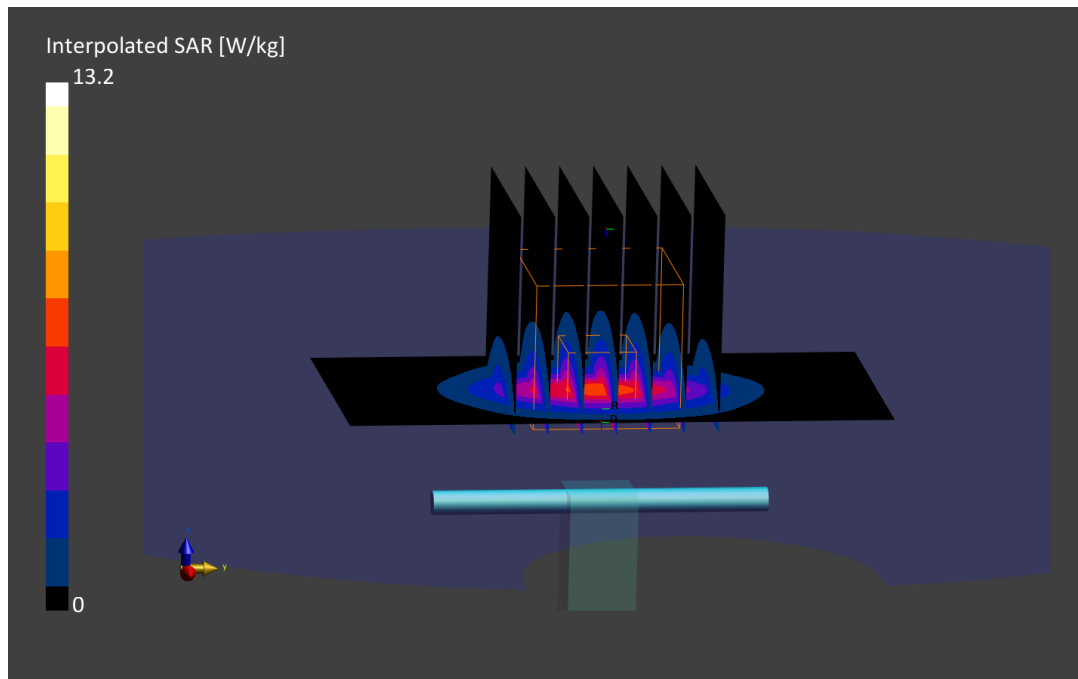

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1071

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 1.99 S/m; perm = 39.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/07/2022; Ambient Temp: 22.3°C; Tissue Temp: 22.2°C

Probe: EX3DV4 - SN7538; ConvF:(7.34,7.34,7.34); Calibrated: 2021-11-16
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn1323; Calibrated: 2021-11-10
Phantom: Twin-SAM V8.0; Serial: 2056
Measurement SW: DASY Module SAR V16.0.2.83

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.5 W/kg

SAR(1 g) = 5.50 W/kg

Deviation (1 g) = -1.96%

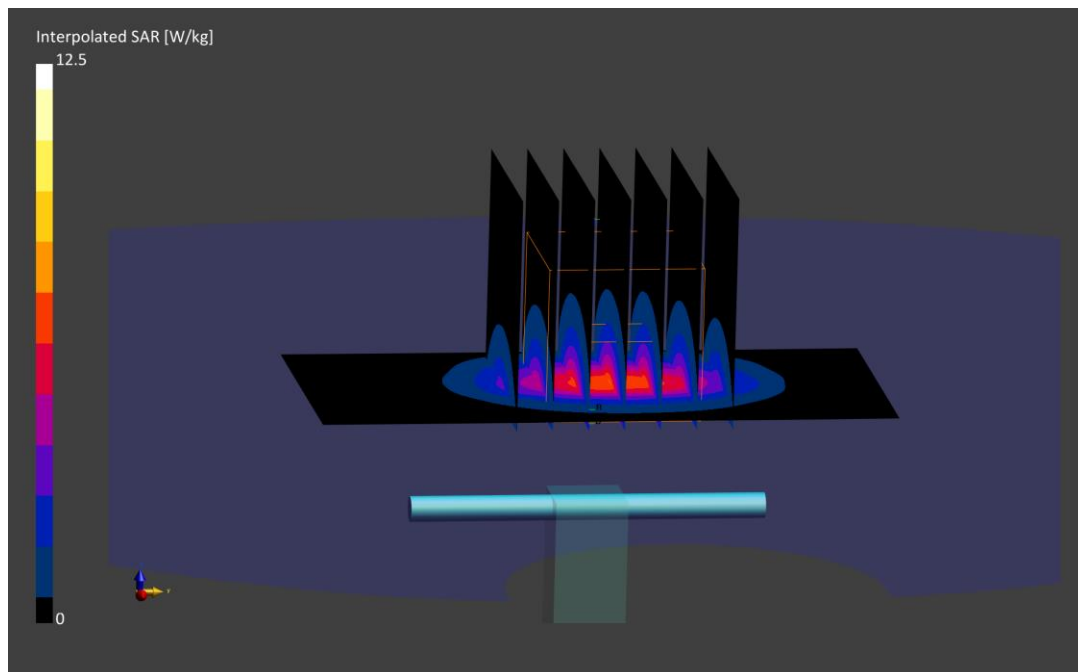

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1004

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 1.99 S/m; perm = 39.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/09/2022; Ambient Temp: 20.3°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7409; ConvF:(6.97,6.97,6.97); Calibrated: 2022-06-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1334; Calibrated: 2022-06-14
Phantom: Twin-SAM V5.0; Serial: 1792
Measurement SW: DASY Module SAR V16.0.2.136

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 13.6 W/kg

SAR(1 g) = 6.07 W/kg

Deviation (1 g) = 5.02%

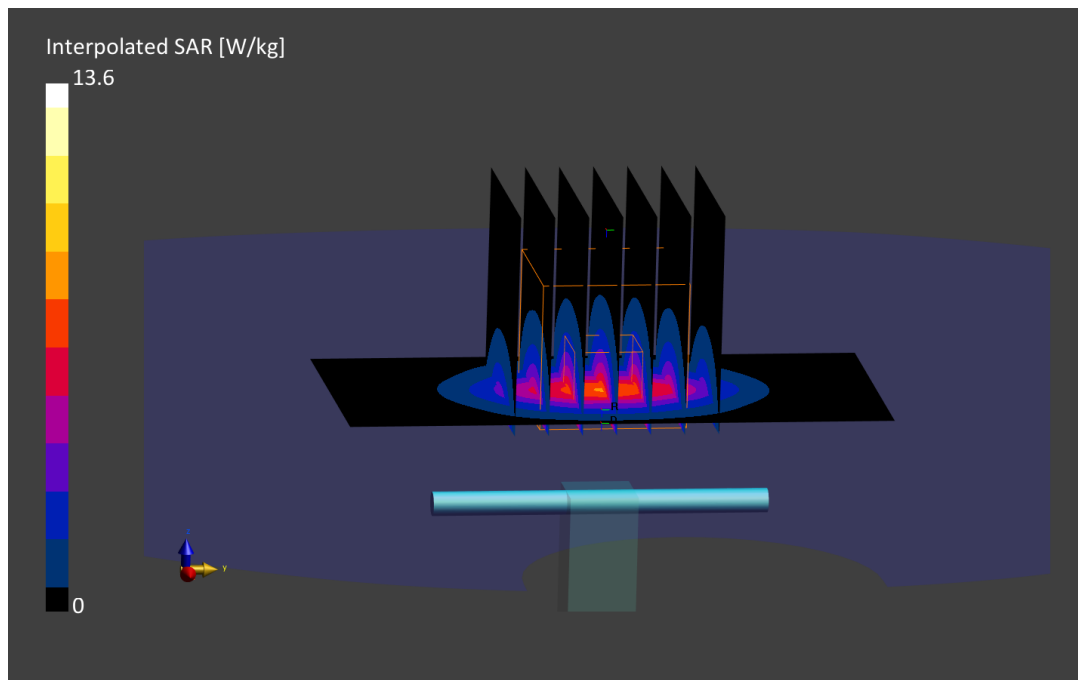

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1150

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Body; Medium parameters used:
f = 1750.0 MHz; cond = 1.50 S/m; perm = 52.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/24/2022; Ambient Temp: 23.4°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7660; ConvF:(9.22,9.22,9.22); Calibrated: 2022-05-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1678; Calibrated: 2022-05-10
Phantom: Twin-SAM V5.0; Serial: 1692rightback
Measurement SW: DASY Module SAR V16.0.2.136

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.17 W/kg

SAR(1 g) = 3.85 W/kg; SAR(10 g) = 2.04 W/kg

Deviation (1 g) = 1.85%; Deviation (10 g) = 2.00%

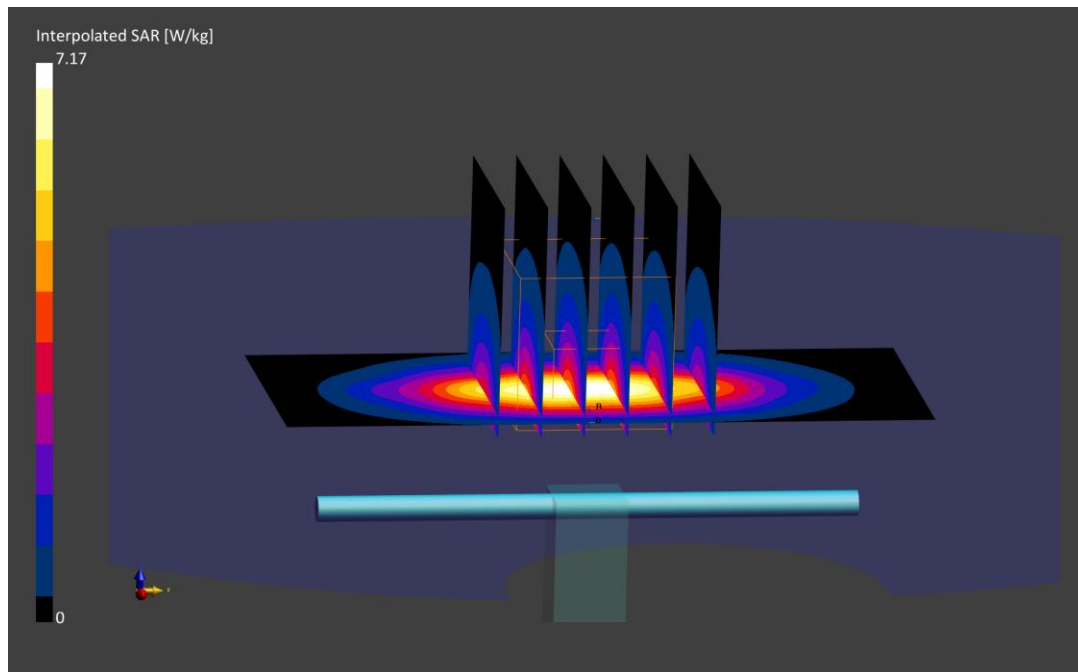

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1150

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Body; Medium parameters used:
f = 1750.0 MHz; cond = 1.48 S/m; perm = 52.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/26/2022; Ambient Temp: 21.9°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7660; ConvF:(9.22,9.22,9.22); Calibrated: 2022-05-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1678; Calibrated: 2022-05-10
Phantom: Twin-SAM V5.0; Serial: 1692rightback
Measurement SW: DASY Module SAR V16.0.2.136

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.89 W/kg

SAR(1 g) = 3.62 W/kg; SAR(10 g) = 1.92 W/kg

Deviation (1 g) = -4.23%; Deviation (10 g) = -4.00%

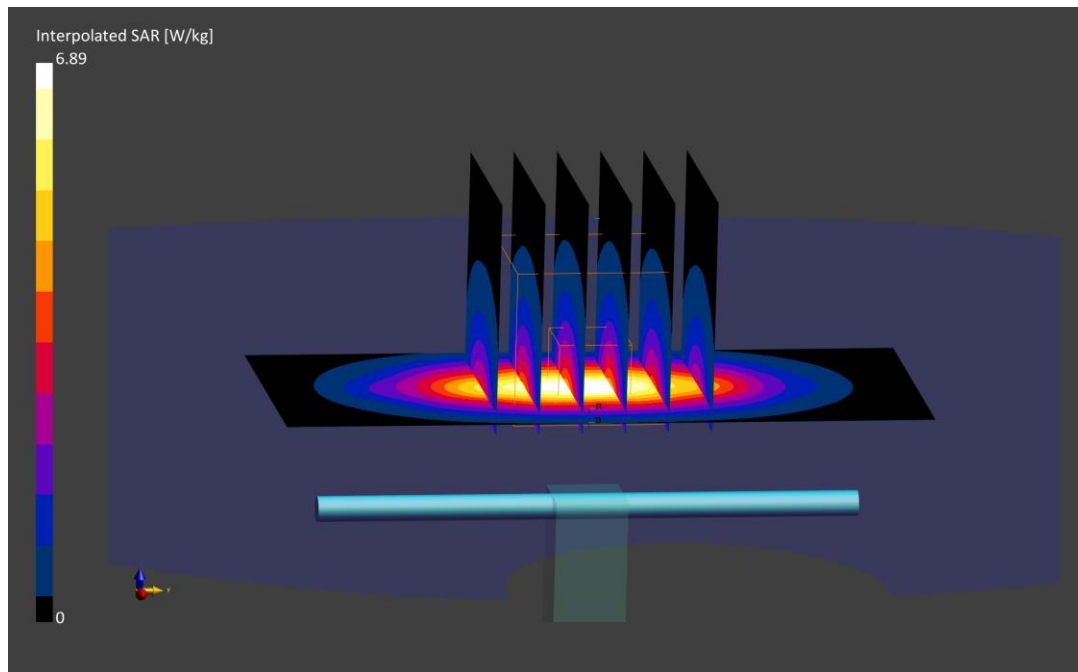

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1765V2 - SN1008

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Body; Medium parameters used:
f = 1750.0 MHz; cond = 1.50 S/m; perm = 52.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/28/2022; Ambient Temp: 22.6°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7660; ConvF:(9.22,9.22,9.22); Calibrated: 2022-05-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1678; Calibrated: 2022-05-10
Phantom: Twin-SAM V5.0; Serial: 1692rightback
Measurement SW: DASY Module SAR V16.0.2.136

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.82 W/kg

SAR(1 g) = 3.61 W/kg; SAR(10 g) = 1.90 W/kg

Deviation (1 g) = -4.50%; Deviation (10 g) = -4.52%

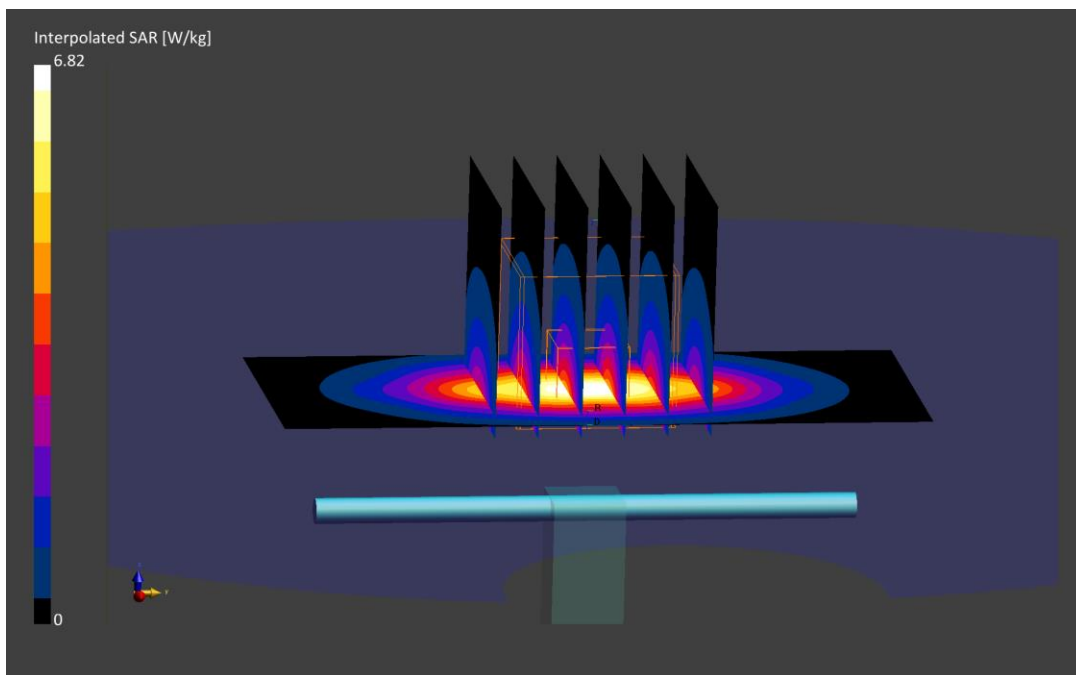

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1150

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Body; Medium parameters used:
f = 1750.0 MHz; cond = 1.54 S/m; perm = 52.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/01/2022; Ambient Temp: 20.9°C; Tissue Temp: 20.2°C

Probe: EX3DV4 - SN7660; ConvF:(9.22,9.22,9.22); Calibrated: 2022-05-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1678; Calibrated: 2022-05-10
Phantom: Twin-SAM V5.0; Serial: 1692rightback
Measurement SW: DASY Module SAR V16.0.2.136

1750 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.07 W/kg

SAR(1 g) = 3.73 W/kg

Deviation (1 g) = -1.32%

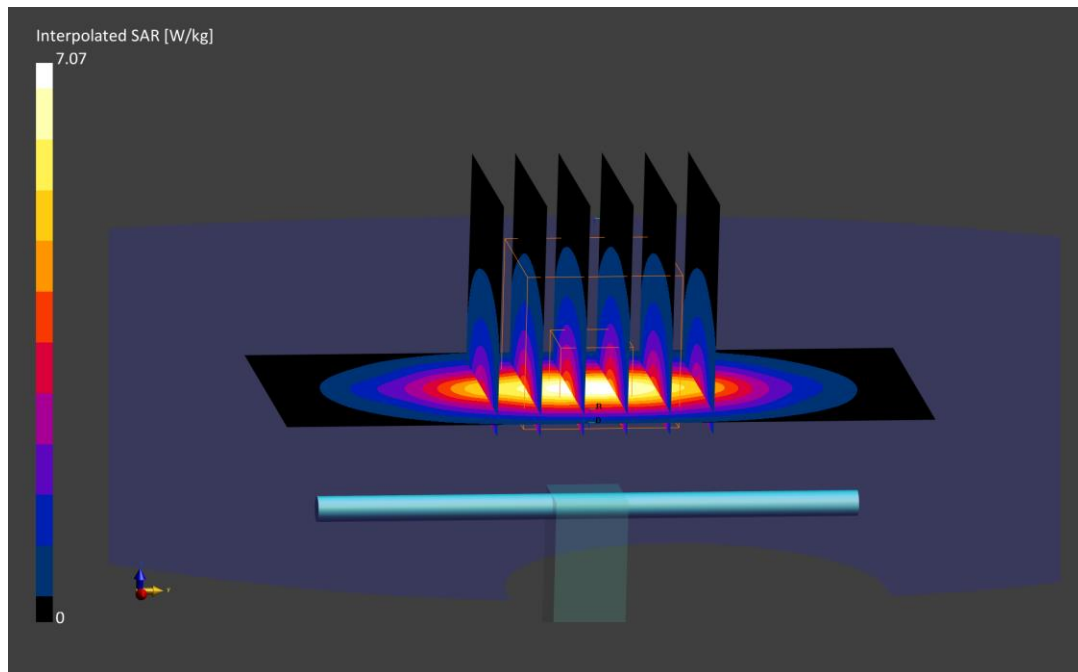

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1073

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2300.0 MHz; cond = 1.86 S/m; perm = 50.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/24/2022; Ambient Temp: 22.3°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7538; ConvF:(7.6,7.6,7.6); Calibrated: 2021-11-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1323; Calibrated: 2021-11-10
Phantom: Twin-SAM V8.0; Serial: 2056
Measurement SW: DASY Module SAR V16.0.2.83

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.1 W/kg

SAR(1 g) = 4.89 W/kg; SAR(10 g) = 2.33 W/kg

Deviation (1 g) = 1.03%; Deviation (10 g) = -0.43%

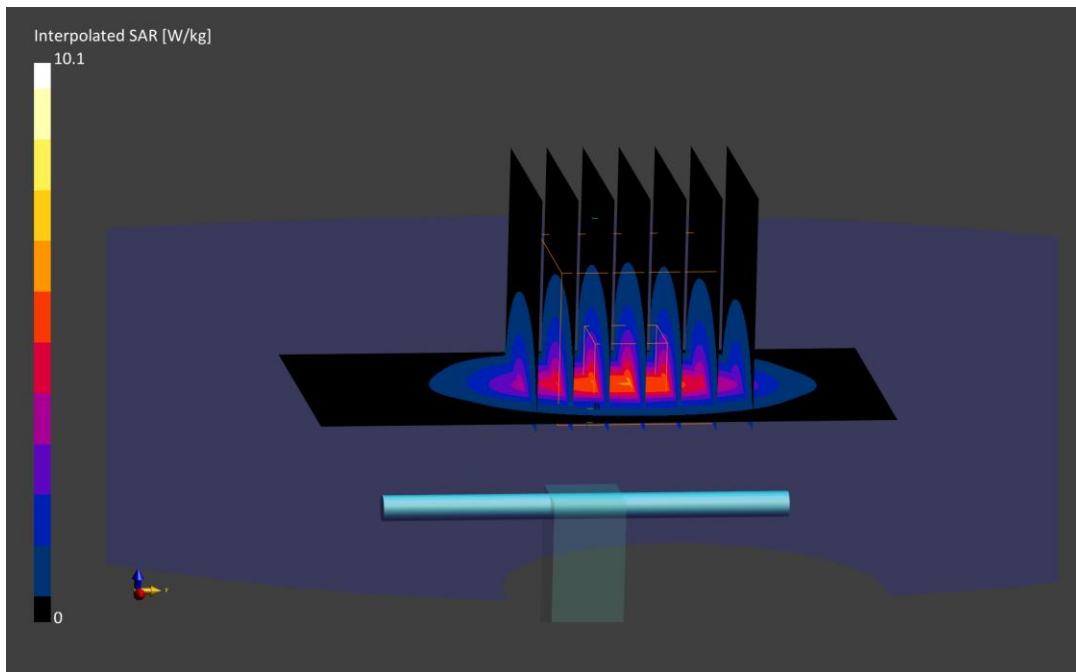

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1073

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2300.0 MHz; cond = 1.86 S/m; perm = 50.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/26/2022; Ambient Temp: 21.5°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7538; ConvF:(7.6,7.6,7.6); Calibrated: 2021-11-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1323; Calibrated: 2021-11-10
Phantom: Twin-SAM V8.0; Serial: 2056
Measurement SW: DASY Module SAR V16.0.2.83

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.84 W/kg

SAR(1 g) = 4.91 W/kg

Deviation (1 g) = 1.45%

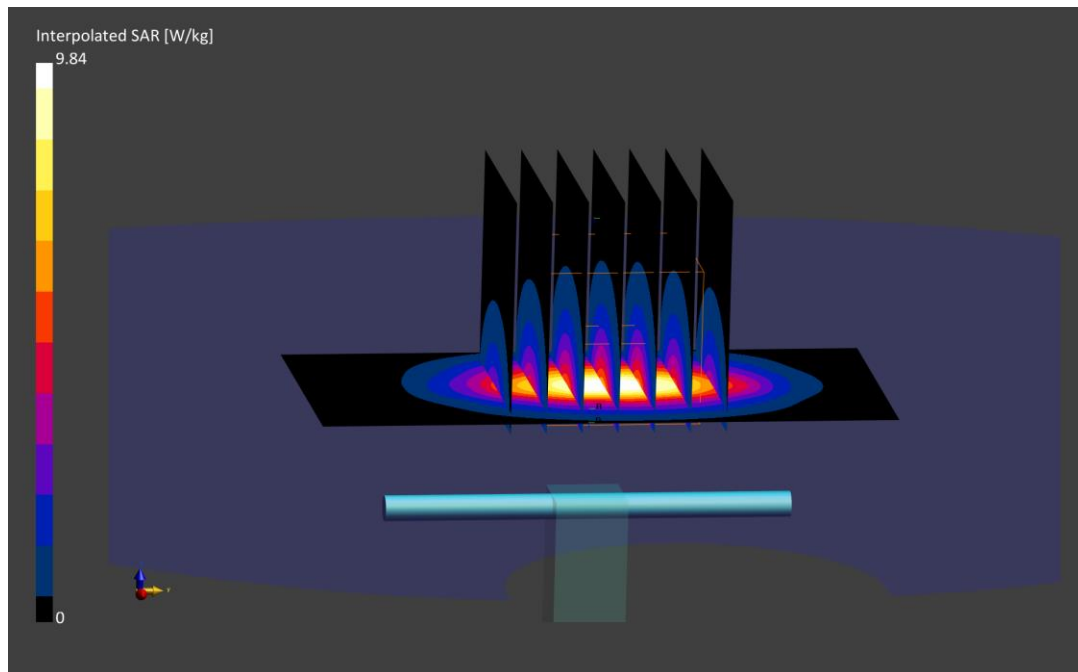

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1116

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2300.0 MHz; cond = 1.82 S/m; perm = 52.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/15/2022; Ambient Temp: 22.0°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7570; ConvF:(7.75,7.75,7.75); Calibrated: 2022-01-19
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1558; Calibrated: 2022-01-14
Phantom: Twin-SAM V8.0; Serial: 20063
Measurement SW: DASY Module SAR V16.0.2.136

2300 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.96 W/kg

SAR(10 g) = 2.30 W/kg

Deviation (10 g) = -2.95%

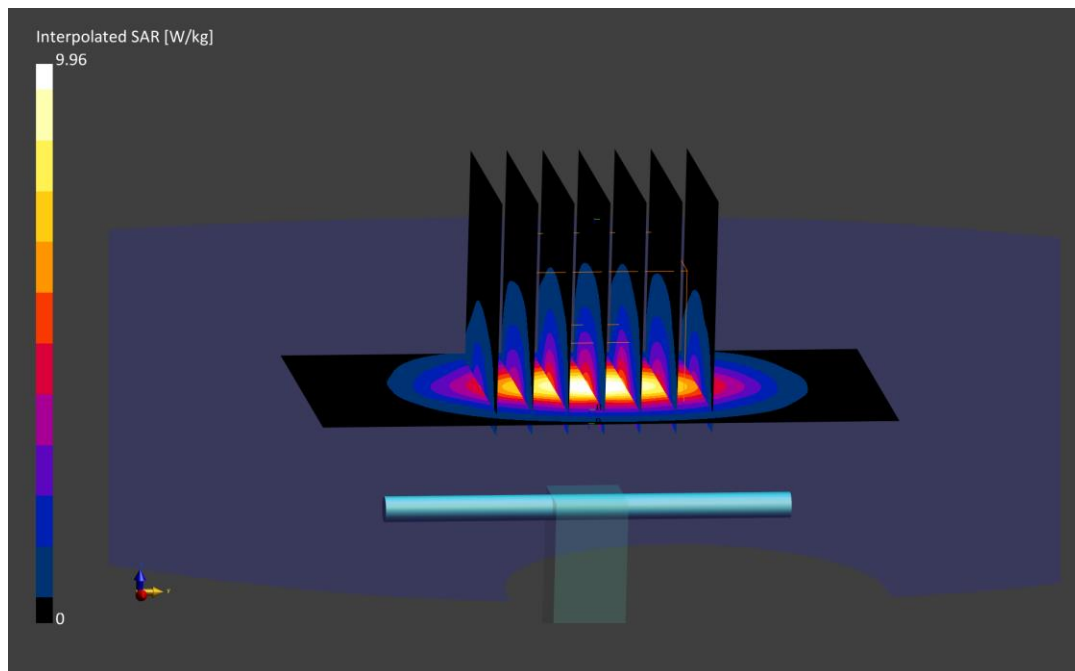

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN797

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2450.0 MHz; cond = 2.03 S/m; perm = 52.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/01/2022; Ambient Temp: 21.0°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7538; ConvF:(7.43,7.43,7.43); Calibrated: 2021-11-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1323; Calibrated: 2021-11-10
Phantom: Twin-SAM V8.0; Serial: 2056
Measurement SW: DASY Module SAR V16.0.2.83

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.2 W/kg

SAR(1 g) = 4.98 W/kg

Deviation (1 g) = 0.81%

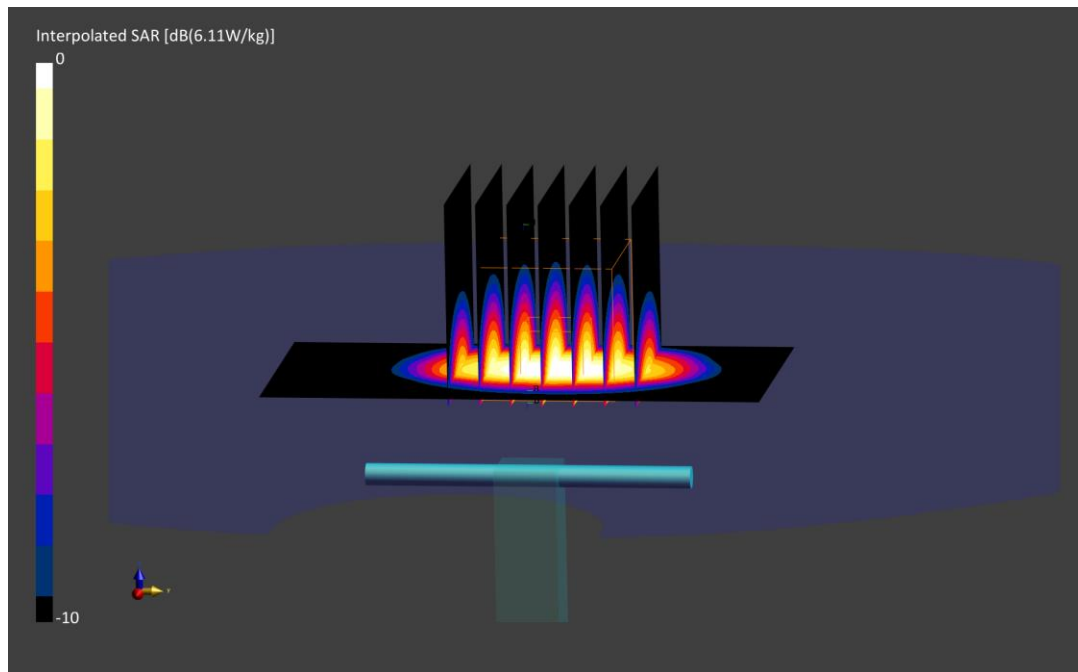

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN981

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

f = 2450.0 MHz; cond = 2.00 S/m; perm = 52.3; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/06/2022; Ambient Temp: 21.8°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7417; ConvF:(7.57,7.57,7.57); Calibrated: 2022-02-22

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn665; Calibrated: 2022-02-22

Phantom: Twin-SAM V8.0; Serial: 2060

Measurement SW: DASY Module SAR V16.0.2.83

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.96 W/kg

SAR(1 g) = 4.78 W/kg

Deviation (1 g) = -4.97%

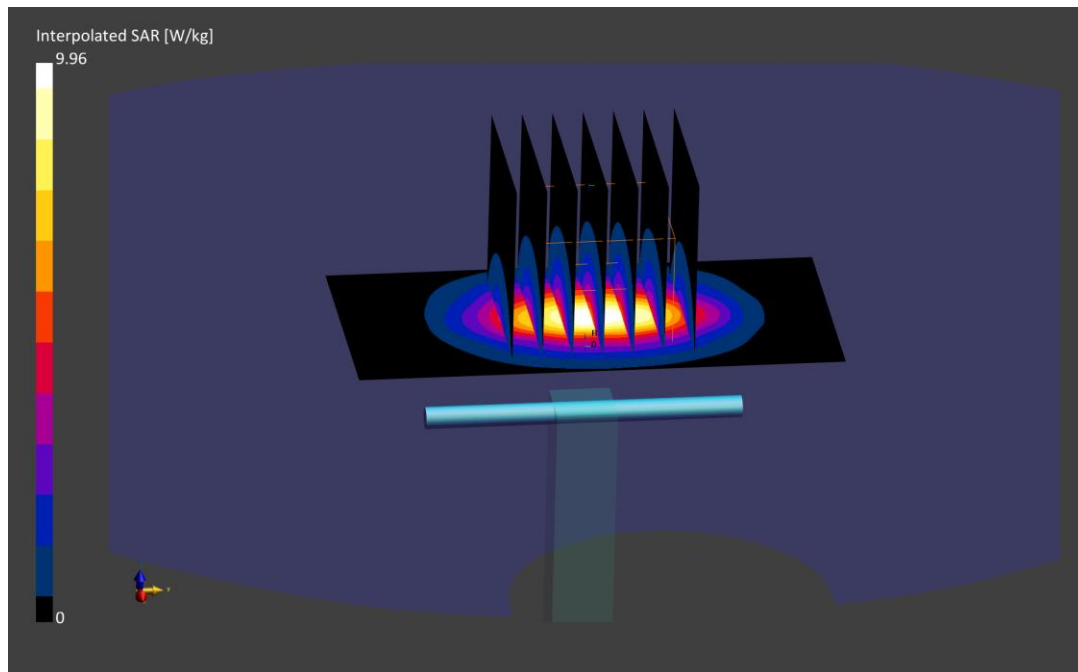

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN797

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

f = 2450.0 MHz; cond = 1.99 S/m; perm = 51.9; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/08/2022; Ambient Temp: 22.4°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7417; ConvF:(7.57,7.57,7.57); Calibrated: 2022-02-22

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn665; Calibrated: 2022-02-22

Phantom: Twin-SAM V8.0; Serial: 2060

Measurement SW: DASY Module SAR V16.0.2.83

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.83 W/kg

SAR(1 g) = 4.78 W/kg

Deviation (1 g) = -3.24%

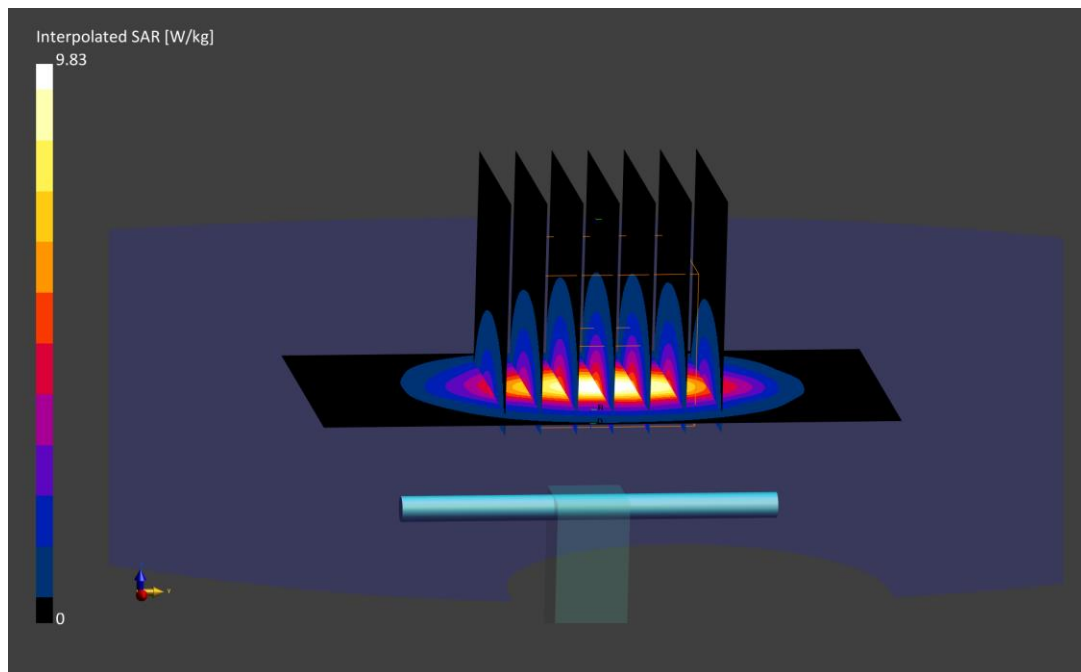

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN719

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

f = 2450.0 MHz; cond = 2.03 S/m; perm = 51.8; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/08/2022; Ambient Temp: 23.5°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7570; ConvF:(7.66,7.66,7.66); Calibrated: 2022-01-19

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1558; Calibrated: 2022-01-14

Phantom: Twin-SAM V8.0; Serial: 20063

Measurement SW: DASY Module SAR V16.0.2.136

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.3 W/kg

SAR(1 g) = 5.26 W/kg

Deviation (1 g) = -1.15%

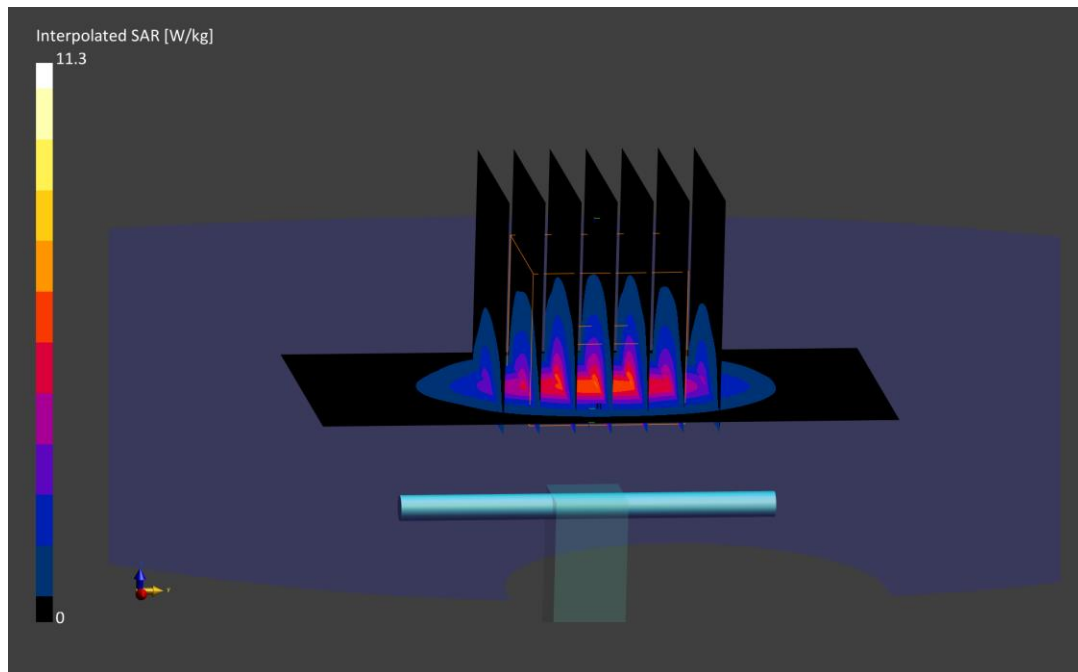

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN797

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

f = 2450.0 MHz; cond = 2.03 S/m; perm = 51.1; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/11/2022; Ambient Temp: 21.9°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7417; ConvF:(7.57,7.57,7.57); Calibrated: 2022-02-22

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn665; Calibrated: 2022-02-22

Phantom: Twin-SAM V8.0; Serial: 2060

Measurement SW: DASY Module SAR V16.0.2.83

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.82 W/kg

SAR(10 g) = 2.23 W/kg

Deviation (10 g) = -4.70%

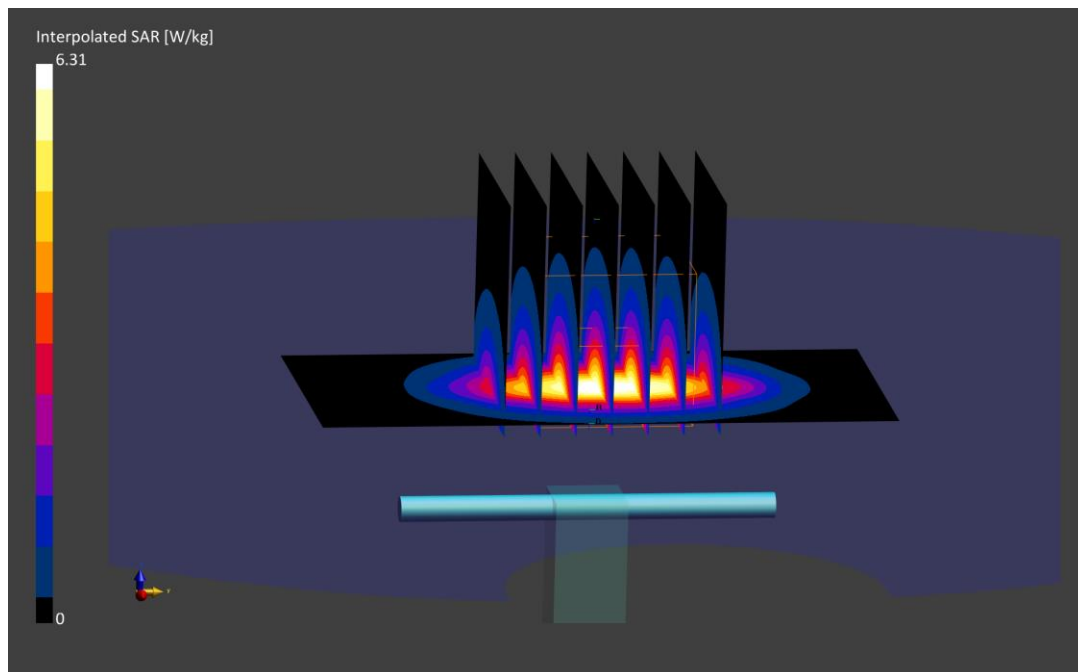

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN981

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Body; Medium parameters used:

f = 2450.0 MHz; cond = 2.01 S/m; perm = 52.0; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/28/2022; Ambient Temp: 22.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7488; ConvF:(7.95,7.95,7.95); Calibrated: 2022-02-21

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn1415; Calibrated: 2022-02-23

Phantom: Twin-SAM V8.0; Serial: 2065

Measurement SW: DASY Module SAR V16.0.2.83

2450 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.8 W/kg

SAR(10 g) = 2.39 W/kg

Deviation (10 g) = 0.84%

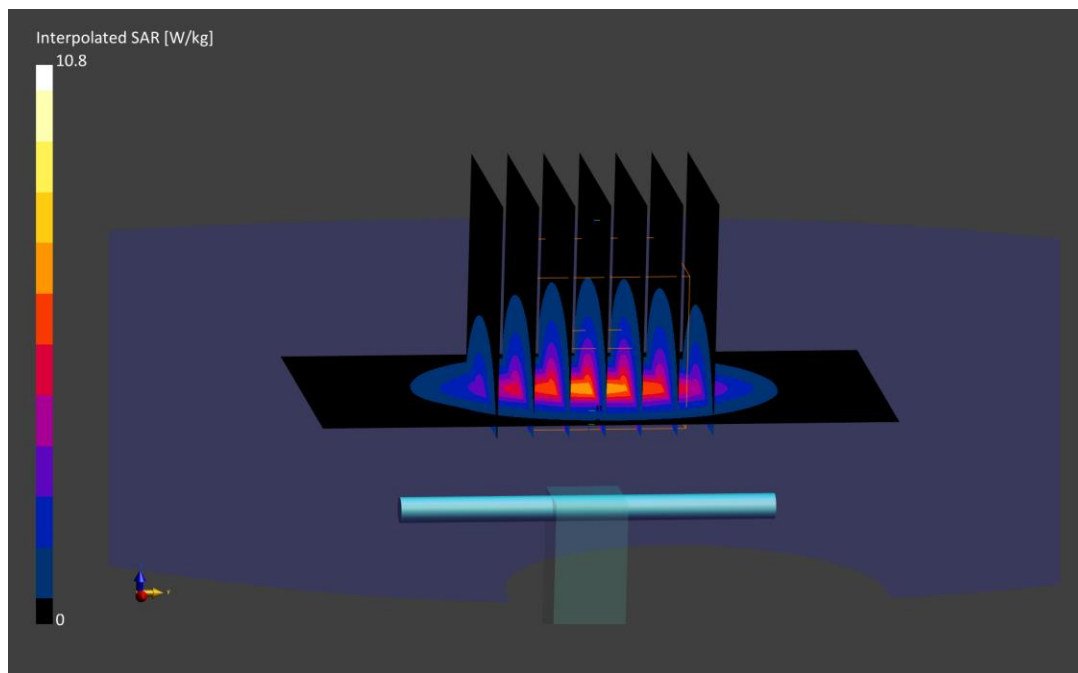

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1071

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2600.0 MHz; cond = 2.21 S/m; perm = 51.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/06/2022; Ambient Temp: 21.8°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7417; ConvF:(7.4,7.4,7.4); Calibrated: 2022-02-22
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn665; Calibrated: 2022-02-22
Phantom: Twin-SAM V8.0; Serial: 2060
Measurement SW: DASY Module SAR V16.0.2.83

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.9 W/kg

SAR(1 g) = 5.46 W/kg

Deviation (1 g) = 0.55%

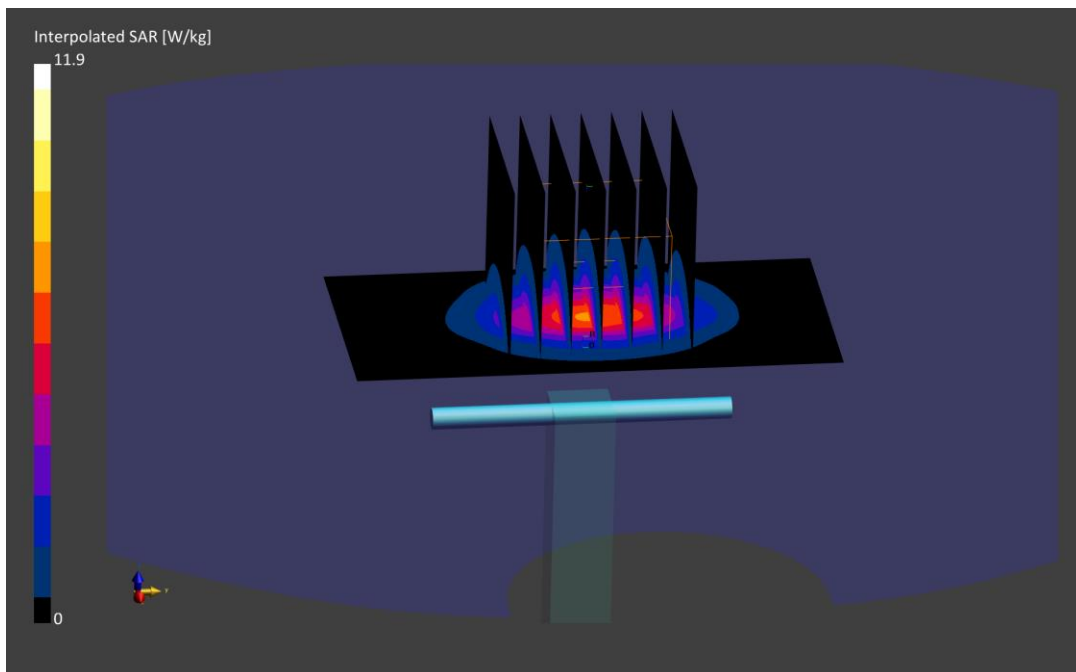

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1064

Communication System: UID: 0, CW; Frequency: 2600.0 MHz

Medium: 2450 Body; Medium parameters used:

f = 2600.0 MHz; cond = 2.19 S/m; perm = 51.4; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 08/08/2022; Ambient Temp: 22.4°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7417; ConvF:(7.4,7.4,7.4); Calibrated: 2022-02-22

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn665; Calibrated: 2022-02-22

Phantom: Twin-SAM V8.0; Serial: 2060

Measurement SW: DASY Module SAR V16.0.2.83

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.8 W/kg

SAR(1 g) = 5.46 W/kg; SAR(10 g) = 2.43 W/kg

Deviation (1 g) = 0.00%; Deviation (10 g) = -0.41%

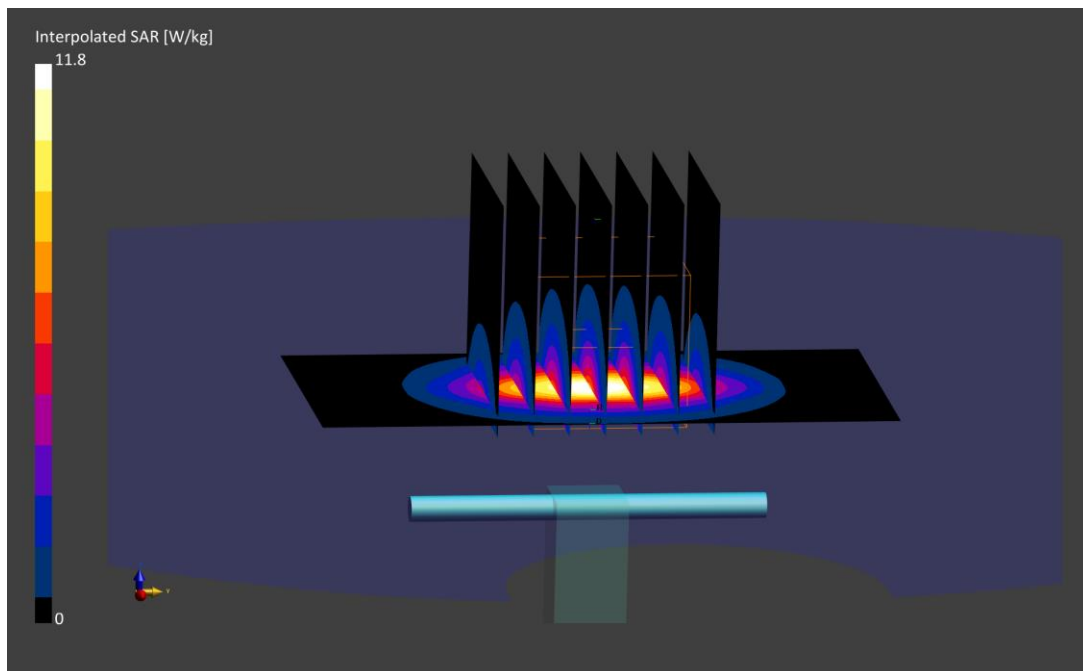

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1071

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2600.0 MHz; cond = 2.24 S/m; perm = 51.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/08/2022; Ambient Temp: 23.5°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7570; ConvF:(7.37,7.37,7.37); Calibrated: 2022-01-19
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1558; Calibrated: 2022-01-14
Phantom: Twin-SAM V8.0; Serial: 20063
Measurement SW: DASY Module SAR V16.0.2.136

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.9 W/kg

SAR(1 g) = 5.58 W/kg

Deviation (1 g) = 2.76%

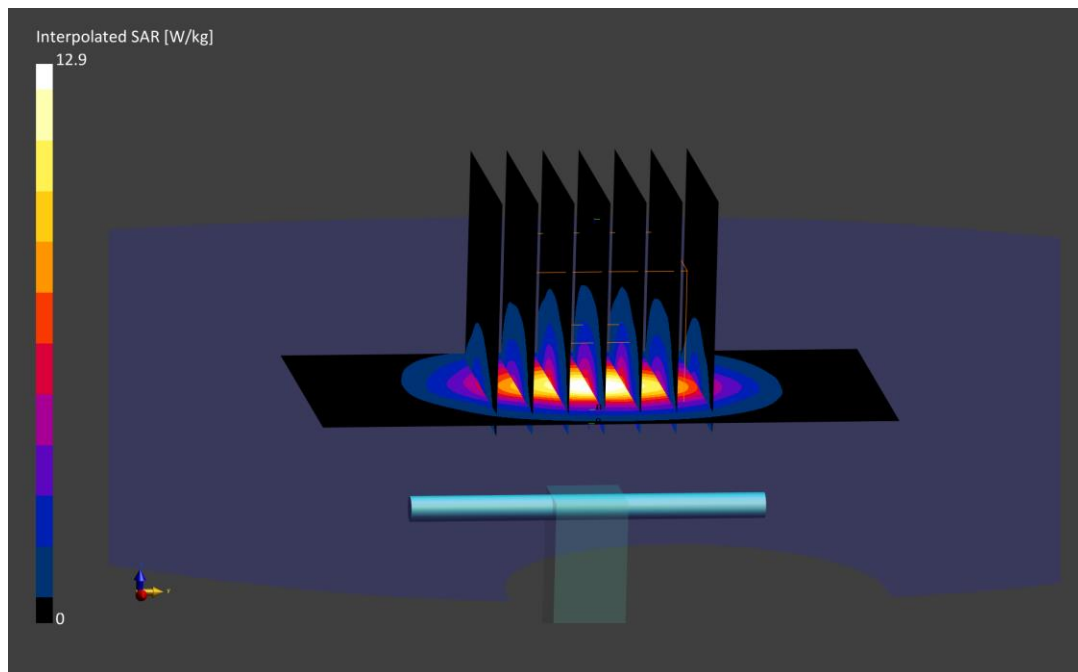

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1064

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2600.0 MHz; cond = 2.24 S/m; perm = 50.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/11/2022; Ambient Temp: 21.9°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7417; ConvF:(7.4,7.4,7.4); Calibrated: 2022-02-22
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn665; Calibrated: 2022-02-22
Phantom: Twin-SAM V8.0; Serial: 2060
Measurement SW: DASY Module SAR V16.0.2.83

2600 MHz System Verification at 20 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.1 W/kg

SAR(10 g) = 2.49 W/kg

Deviation (10 g) = 2.05%

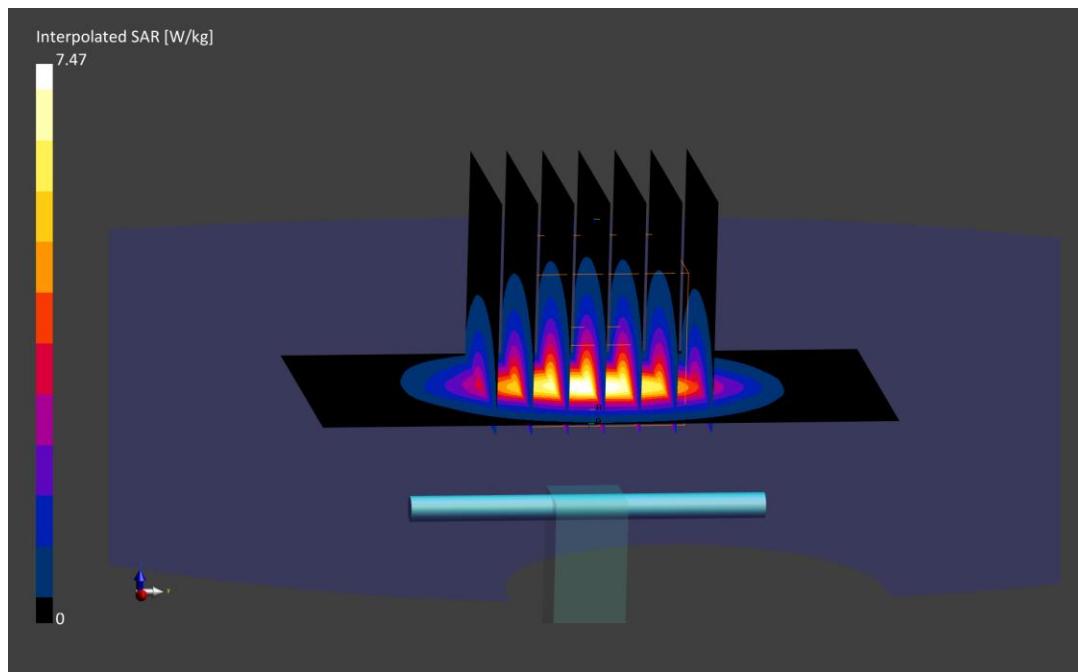

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1004

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Body; Medium parameters used:
f = 2600.0 MHz; cond = 2.22 S/m; perm = 51.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 08/28/2022; Ambient Temp: 22.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7488; ConvF:(7.57,7.57,7.57); Calibrated: 2022-02-21
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1415; Calibrated: 2022-02-23
Phantom: Twin-SAM V8.0; Serial: 2065
Measurement SW: DASY Module SAR V16.0.2.83

2600 MHz System Verification at 20 dBm (100 mW)

Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.2 W/kg

SAR(10 g) = 2.24W/kg

Deviation (10 g) = -9.68%

