

## APPENDIX

### 11. Photographs of Test Setup



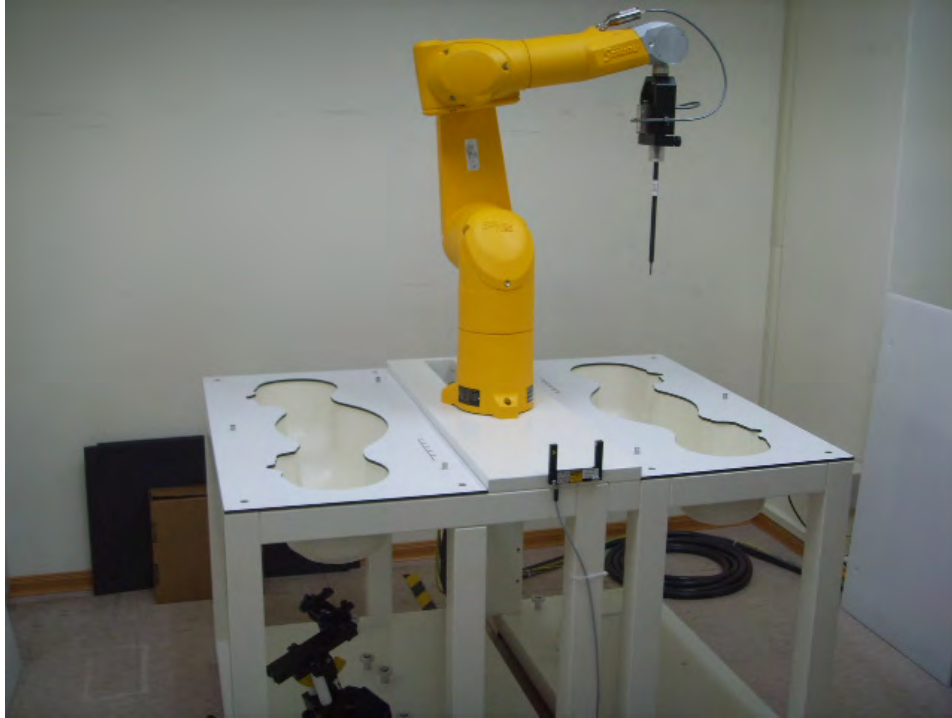


Fig.1 Photograph of the SAR measurement system


**Photograph of the Tissue Simulant Fluid Liquid Depth**

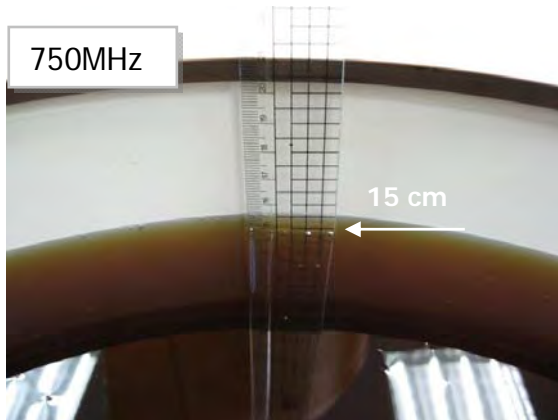


**Fig.2.1**

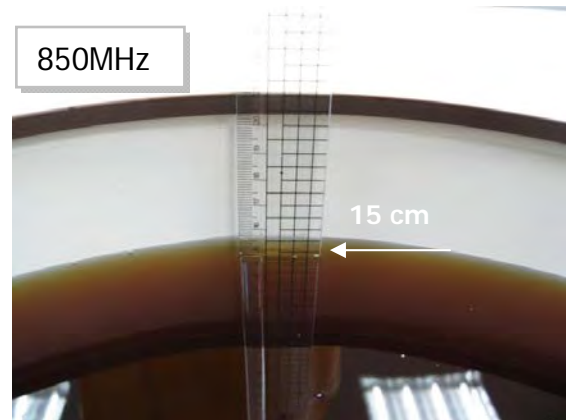


**Fig.2.2**

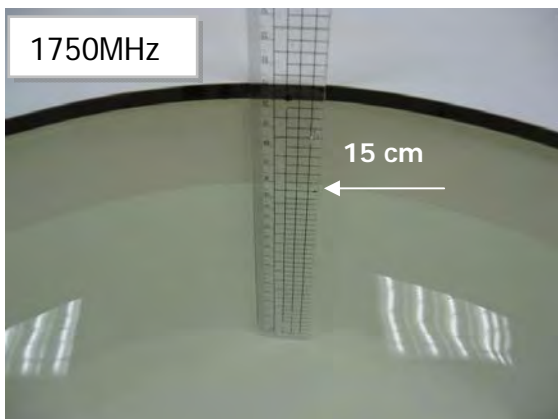


**Fig.2.3**

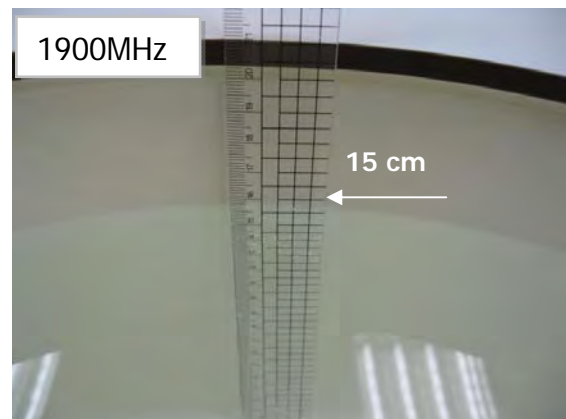

**Fig.2.4**

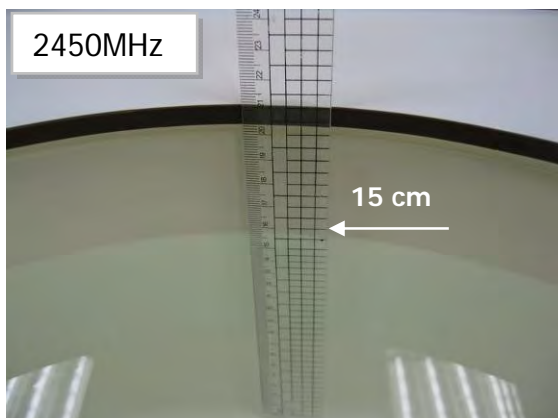


**Fig.2.5**


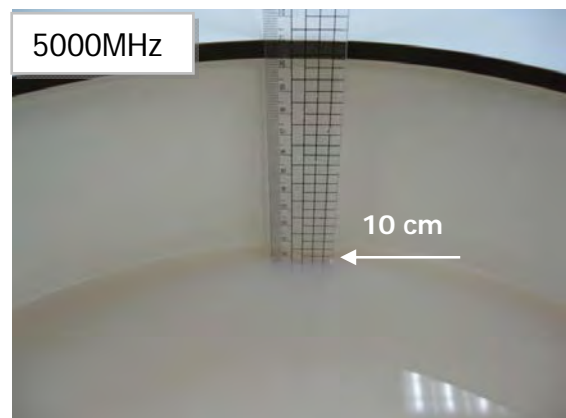


**Fig.2.6**


**Body - distance between flat phantom and EUT is 0 mm**

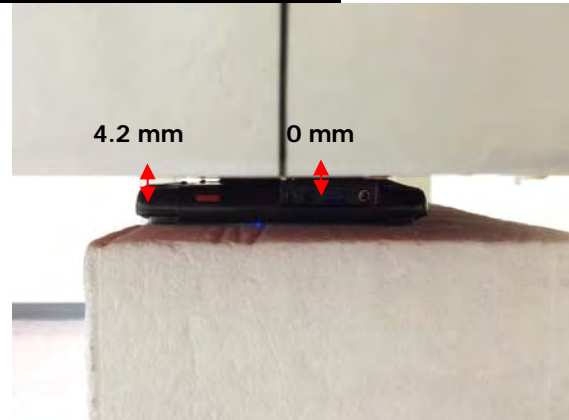


**Fig.3 EUT Back side to flat phantom**

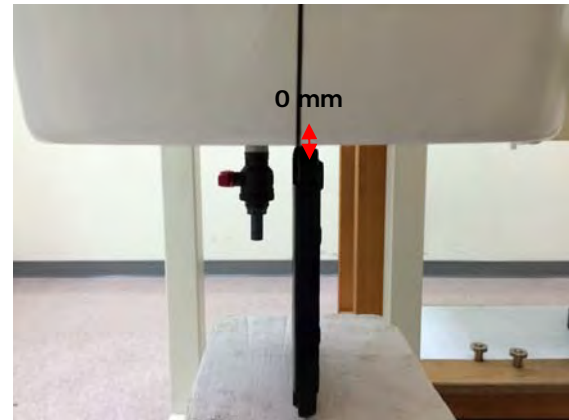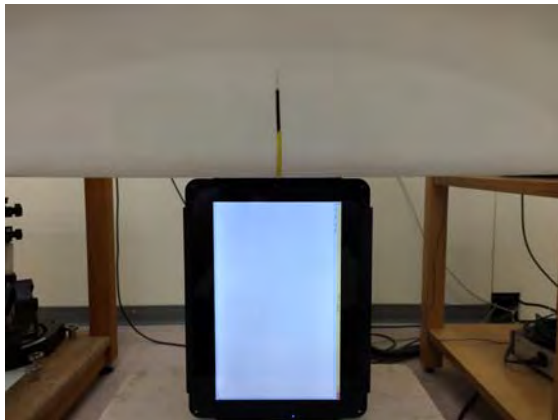

**Fig.4 EUT Left side to flat phantom**

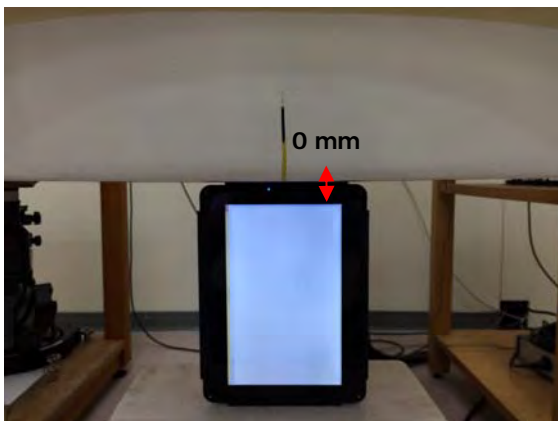

**Fig.5 EUT Right side to flat phantom**

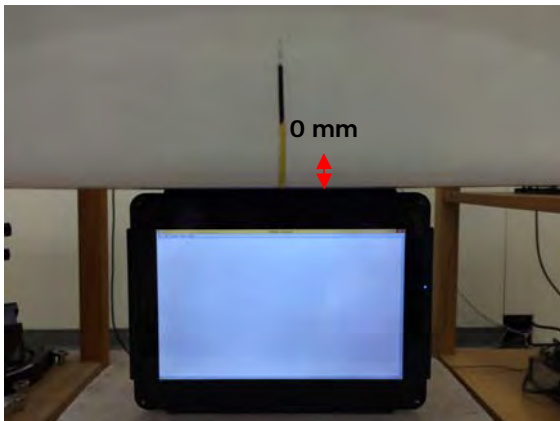

**Fig.6 EUT Top side to flat phantom**


## 12. Photographs of the EUT




**Fig.7 Front view of EUT**



**Fig.8 Back view of EUT**

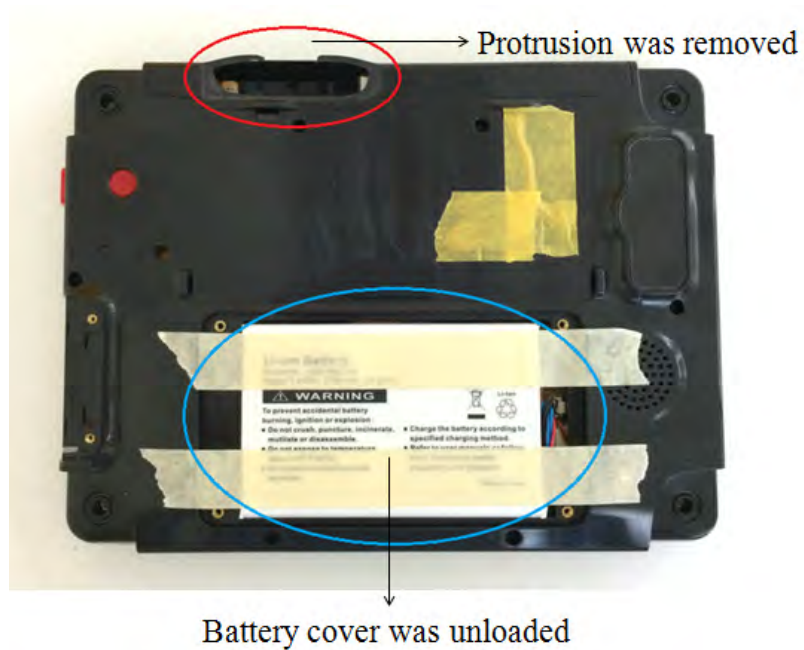

**Fig.9 Back view of EUT for SAR testing  
(Protrusion was removed and battery cover was unloaded)**

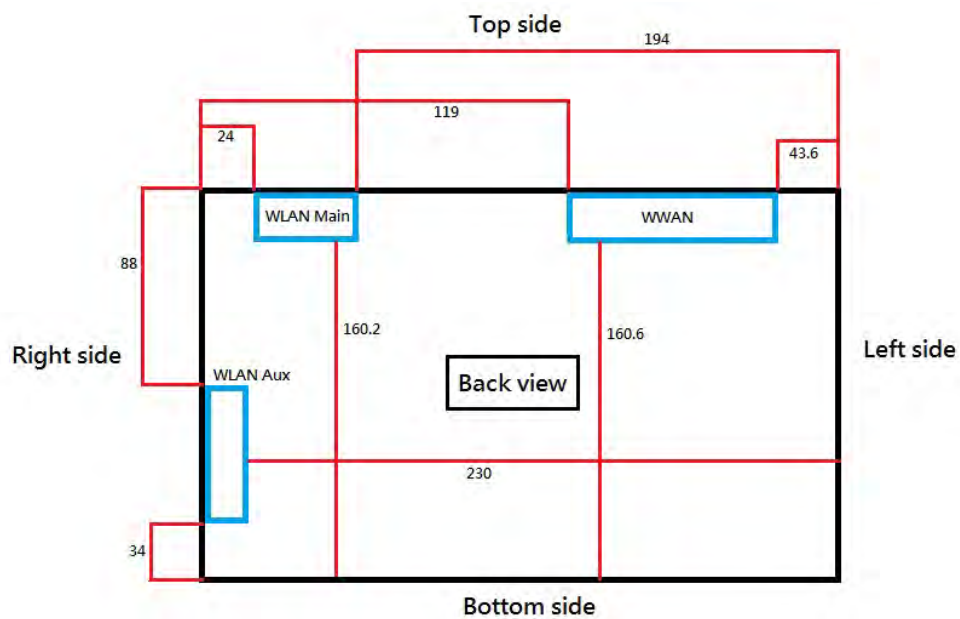

**Fig.10 Antenna position of EUT (Back view)**

- End of Report -