



PCTEST Engineering Laboratory, Inc.

6660-B Dobbin Road • Columbia, MD 21045 • U.S.A.

TEL (410) 290-6652 • FAX (410) 290-6654

<http://www.pctestlab.com>



CERTIFICATE OF COMPLIANCE (SAR EVALUATION)

Vertex Standard Co., Ltd.
4-8-8 Nakameguro, Meguro-Ku,
Tokyo, 153-8644
Attn: Tomiro Ohmoto, Export Manager

Dates of Tests: December 11-12, 2000
Test Report S/N: SAR.201208627.K66
Test Site: PCTEST Lab, Columbia MD

FCC ID

K66VX-900U

APPLICANT

VERTEX STANDARD CO., LTD.

EUT Type:	UHF Mobile Radio
Tx Frequency:	450.025MHz – 484.975MHz
Rx Frequency:	450.025MHz – 484.975MHz
Max. Conducted Power:	5.0 Watts
Max. SAR Measurement:	3.085mW/g (1g) AMPS MOUTH SAR <i>including a 50% Duty Cycle</i> ;
(with 50% Duty Cycle)	5.600mW/g (1g) AMPS BODY SAR <i>including a 50% Duty Cycle</i>
Trade Name/Model(s):	VERTEX STANDARD VX-900U
FCC Classification:	Licensed Non-Broadcast Transmitter Held to Face (TNF)
Application Type:	Certification
Serial Number:	n/a (pre production)
FCC Rule Part(s):	2.1093; ET Docket 96.326
Modulation:	FM

This wireless portable device has been shown to be capable of compliance for localized specific absorption rate (SAR) for Controlled Environment/Occupational exposure limits specified in ANSI/IEEE Std. C95.1-1992 and had been tested in accordance with the measurement procedures specified in ANSI/IEEE Std. C95.3-1992. (See Test Report).

I attest to the accuracy of data. All measurements reported herein were performed by me or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

NVLAP accreditation does not constitute any product endorsement by NVLAP or any agency of the United States Government.

PCTEST certifies that no party to this application has been denied the FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 853(a).



NVLAP[®]
LAB CODE 100431-0


Randy Ortanez
President & Chief Engineer

200214067.OWD

Table of Contents

1.1 SCOPE	1
2.1 INTRODUCTION / SAR DEFINITION	2
3.1 SAR MEASUREMENT SET-UP	3
4.1 E-FIELD PROBE SYSTEM	4
5.1 E-FIELD PROBE CALIBRATION PROCESS	5
5.3 DATA EXTRAPOLATION	6
6.1 PHANTOM, HOLDER & EQUIVALENT TISSUES	7
7.1 SYSTEM SPECIFICATIONS	8
8.1 MEASUREMENT PROCESS	9
9.1 TEST POSITION OF THE RADIO	10
10.1 BODY-WORN CONFIGURATION	11
11.1 ANSI/IEEE C95.1 RF EXPOSURE LIMITS	12
12.1 MEASUREMENT UNCERTAINTIES	13
13.1 SAR TEST DATA SUMMARY	14-15
14.1 SAR TEST EQUIPMENT LIST	16
15.1 CONCLUSION	17
16.1 REFERENCES	18
APPENDIX A – SAR TEST PLOTS	
APPENDIX B – SAR TEST SETUP PHOTOGRAPHS	
APPENDIX C – DIPOLE VALIDATION DATA	
APPENDIX D – PROBE CALIBRATION DATA	
APPENDIX E – EUT EXTERNAL PHOTOGRAPHS	

SAR MEASUREMENT REPORT

1.1 Scope

Environmental evaluation measurements of specific absorption rate¹ (SAR) distributions in simulated human tissues exposed to radiofrequency (RF) radiation from wireless portable devices for compliance with the rules and regulations of the U.S. Federal Communications Commission (FCC).²

Applicant Name:	VERTEX STANDARD CO., LTD.
Address:	4-8-8 Nakameguro, Meguro-Ku Tokyo, 153-8644, Japan
Attention:	Tomiro Ohmoto, Export Manager

- | | |
|-------------------------|--|
| • EUT Type: | UHF Mobile Radio |
| • Trade Name: | Vertex Standard |
| • Model(s): | VX-900U |
| • FCC IDENTIFIER: | K66VX-900U |
| • S/N: | Pre-production |
| • Tx Frequency: | 450.025MHz – 484.975MHz |
| • Rx Frequency : | 450.025MHz – 484.975MHz |
| • Application Type: | Certification |
| • FCC Classification: | Licensed Non-Broadcast
Transmitter Held to Face (TNF) |
| • Modulation(s): | FM |
| • FCC Rule Part(s): | § 2.1093, Docket 96-326 |
| • Max. Conducted Power: | 5.0 Watts |
| • Dates of Tests: | December 11-12, 2000 |
| • Place of Tests: | PCTEST Engineering Lab.
Columbia, MD, U.S.A. |
| • Report Serial No.: | SAR.201208627.K66 |



Fig. 1 SAR Test Setup

NVLAP
Lab Code 100431-0

¹ Specific Absorption Rate (SAR) is a measure of the rate of energy absorption due to exposure to an RF transmitting source (wireless portable device).

² IEEE/ANSI Std. C95.1-1992 limits are used to determine compliance with FCC ET Docket 93-62.

2.1 INTRODUCTION

The FCC has adopted the guidelines for evaluating the environmental effects of radiofrequency radiation in ET Docket 93-62 on Aug. 6, 1996 to protect the public and workers from the potential hazards of RF emissions due to FCC-regulated portable devices.[1]

The safety limits used for the environmental evaluation measurements are based on the criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate (SAR) in *IEEE/ANSI C95.1-1992 Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz*. (c) 1992 by the Institute of Electrical and Electronics Engineers, Inc., New York, New York 10017.[2] The measurement procedure described in *IEEE/ANSI C95.3-1992 Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields - RF and Microwave*[3] is used for guidance in measuring SAR due to the RF radiation exposure from the Equipment Under Test (EUT). These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in *Biological Effects and Exposure Criteria for Radiofrequency Electromagnetic Fields*, NCRP Report No. 86 (c) NCRP, 1986, Bethesda, MD 20814.[4] SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards.

2.2 SAR Definition

Specific Absorption Rate (SAR) is defined as the time derivative (rate) of the incremental energy (dU) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density (r). It is also defined as the rate of RF energy absorption per unit mass at a point in an absorbing body (see Fig. 2).

$$SAR = \frac{d}{dt} \left(\frac{dU}{dm} \right) = \frac{d}{dt} \left(\frac{dU}{r dV} \right)$$

Figure 2. SAR Mathematical Equation

SAR is expressed in units of Watts per Kilogram (W/kg).

$$SAR = \sigma E^2 / r$$

where:

σ	=	conductivity of the tissue-simulant material (S/m)
r	=	mass density of the tissue-simulant material (kg/m ³)
E	=	Total RMS electric field strength (V/m)

NOTE: The primary factors that control rate of energy absorption were found to be the wavelength of the incident field in relations to the dimensions and geometry of the irradiated organism, the orientation of the organism in relation to the polarity of field vectors, the presence of reflecting surfaces, and whether conductive contact is made by the organism with a ground plane.[4]

3.1 SAR MEASUREMENT SET-UP

These measurements are performed using the DASY3 automated dosimetric assessment system. It is made by Schmid & Partner Engineering AG (SPEAG) in Zurich, Switzerland. It consists of high precision robotics system (Staubli), robot controller, Pentium III computer, near-field probe, probe alignment sensor, and the generic twin phantom containing the brain or muscle equivalent material. The robot is a six-axis industrial robot performing precise movements to position the probe to the location (points) of maximum electromagnetic field (EMF) (see Fig. 2).

A cell controller system contains the power supply, robot controller, teach pendant (Joystick), and remote control, is used to drive the robot motors. The PC consists of the Micron Pentium III 500 MHz computer with Windows NT system and SAR Measurement Software DASY3, A/D interface card, monitor, mouse, and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card. The DAE3 consists of a

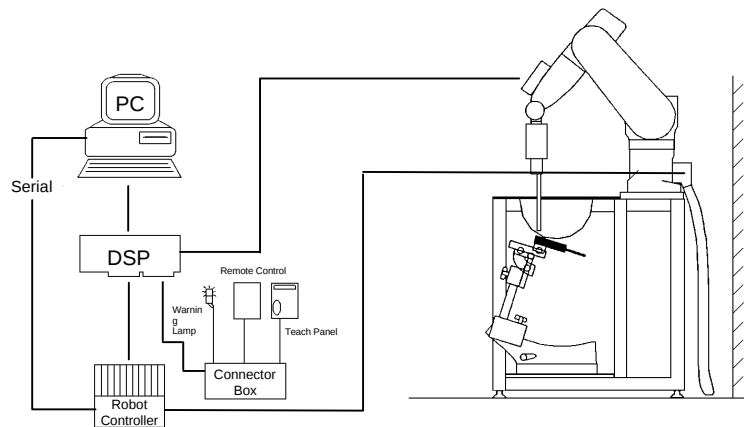


Figure 3. PCTEST SAR Lab II Test Measurement Set-up

highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts.

They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer. The system is described in detail in [5].

4.1 DASY3 E-FIELD PROBE SYSTEM

4.2 ET3DV5 Probe Specification

Construction	Symmetrical design with triangular core Built-in optical fiber for surface detection System Built-in shielding against static charges
Calibration	In air from 10 MHz to 2.5 GHz In brain and muscle simulating tissue at Frequencies of 450 MHz, 900 MHz and 1.8 GHz (accuracy $\pm 8\%$)
Frequency	10 MHz to > 6 GHz; Linearity: ± 0.2 dB (30 MHz to 3 GHz)
Directivity	± 0.2 dB in brain tissue (rotation around probe axis) ± 0.4 dB in brain tissue (rotation normal probe axis)
Dynamic Range	$5 \mu\text{W/g}$ to $> 100 \text{ mW/g}$; Linearity: ± 0.2 dB
Surface Detection	± 0.2 mm repeatability in air and clear liquids over diffuse reflecting surfaces.
Dimensions	Overall length: 330 mm Tip length: 16 mm Body diameter: 12 mm Tip diameter: 6.8 mm Distance from probe tip to dipole centers: 2.7 mm
Application	General dosimetry up to 3 GHz Compliance tests of mobile phones Fast automatic scanning in arbitrary phantoms

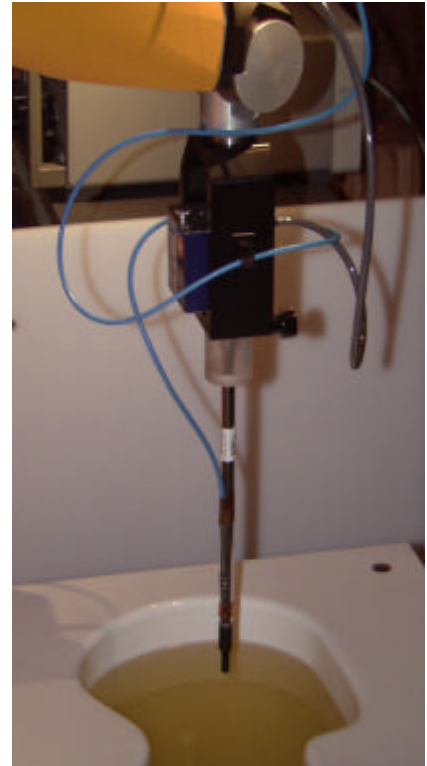


Figure 4. Photograph of the Probe and the Phantom

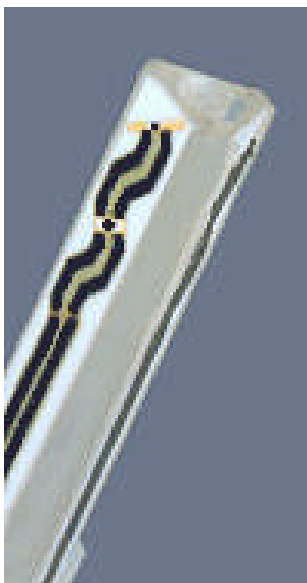


Fig. 5. ET3DV5 E-field Probe

The SAR measurements were conducted with the dosimetric probe ET3DV5, designed in the classical triangular configuration [5] and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multifiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches a maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY3 software reads the reflection during a software approach and looks for the maximum using a 2nd order fitting. The approach is stopped at reaching the maximum.

5.1 E-FIELD PROBE CALIBRATION PROCESS

5.2 E-Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure described in [6] with an accuracy better than +/- 10%. The spherical isotropy was evaluated with the procedure described in [7] and found to be better than +/-0.25dB. The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe is tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies below 1 GHz, and in a waveguide above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulating tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$SAR = C \frac{\Delta T}{\Delta t}$$

where:

Δt = exposure time (30 seconds),

C = heat capacity of tissue (brain or muscle),

ΔT = temperature increase due to RF exposure.

SAR is proportional to $\Delta T / \Delta t$, the initial rate of tissue heating, before thermal diffusion takes place. Now it's possible to quantify the electric field in the simulated tissue by equating the thermally derived SAR to the E- field;

$$SAR = \frac{|E|^2 \cdot s}{r}$$

where:

σ = simulated tissue conductivity,

ρ = Tissue density (1.25 g/cm³ for brain tissue)

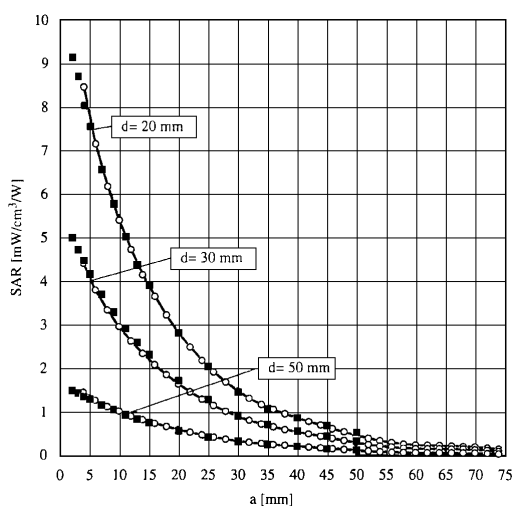


Figure 6. E-Field and Temperature measurements at 900MHz [5]

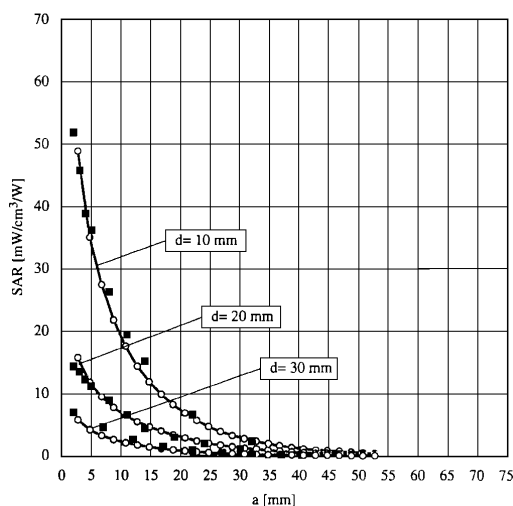


Figure 7. E-Field and temperature measurements at 1.8GHz [5]

5.3 Data Extrapolation

The DASY3 software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as [8]:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with V_i = compensated signal of channel i (i=x,y,z)
 U_i = input signal of channel i (i=x,y,z)
 cf = crest factor of exciting field (DASY parameter)
 dcp_i = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:

$$E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

with V_i = compensated signal of channel i (i = x,y,z)
 $Norm_i$ = sensor sensitivity of channel i (i = x,y,z)
 $\mu V/(V/m)^2$ for E-field probes
 $ConvF$ = sensitivity of enhancement in solution
 E_i = electric field strength of channel i in V/m

The RSS value of the field components gives the total field strength (Hermetian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{S}{r \cdot 1000}$$

with SAR = local specific absorption rate in W/g
 E_{tot} = total field strength in V/m
 σ = conductivity in [mho/m] or [Siemens/m]
 ρ = equivalent tissue density in g/cm³

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$

with P_{pwe} = equivalent power density of a plane wave in W/cm²
 E_{tot} = total electric field strength in V/m

6.1 PHANTOM, HOLDER AND THE EQUIVALENT TISSUES

6.2 Generic Twin Phantom

The Generic Twin Phantom is constructed of a fiberglass shell integrated in a wooden table. The shape of the shell is based on data from an anatomical study designed to determine the maximum exposure in at least 90% of all users [9][10]. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents the evaporation of the liquid. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. See Figure 8.



Fig. 8 Generic Twin Phantom

Shell Thickness	2 ± 0.1 mm
Filling Volume	Volume Approx. 20 liters
Dimensions	810 x 1000 x 500 mm (H x L x W)

6.3 Tissue Simulating Mixture Characterization

The mixtures consist of a viscous gel using hydroxyethylcellulose (HEC) gelling agent and saline solution (see Table 1). Preservation with a bactericide is added and visual inspection is made to make sure air bubbles are not trapped during the mixing process. The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of brain or muscle tissue. The mixture characterizations used for the tissue simulating liquids are according to the data by C. Gabriel and G. Hartsgrove [11].

MIXTURE %	FREQUENCY (Muscle) 450 MHz
WATER	40.4
SUGAR	57.0
SALT	1.5
BACTERIACIDE	0.1
HEC	1.0

Table 1. Composition of the Tissue Equivalent Matters

6.4 Device Holder for Transmitters

In combination with the Generic Twin Phantom V3.0, the Mounting Device (POM) enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation points is the ear opening. The devices can be easily, accurately, and repeatably positioned according to the FCC and CENELEC specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).



Fig. 9. Device Holder

* Note: A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produced infinite number of configurations [10]. To produce the worst-case condition (the hand absorbs antenna output power), the hand is omitted during the tests.

7.1 SYSTEM SPECIFICATIONS

7.2 Robotic System Specifications

Specifications

POSITIONER: Stäubli Unimation Corp. Robot Model: RX60L
Repeatability: 0.02 mm
No. of axis: 6

Data Acquisition Electronic (DAE) System

Cell Controller

Processor: Pentium III
Clock Speed: 450 MHz
Operating System: Windows NT
Data Card: DASY3 PC-Board

Data Converter

Features: Signal Amplifier, multiplexer, A/D converter, and control logic
Software: DASY3 software
Connecting Lines: Optical downlink for data and status info.
Optical uplink for commands and clock

PC Interface Card

Function: 24 bit (64 MHz) DSP for real time processing
Link to DAE3
16 bit A/D converter for surface detection system
serial link to robot
direct emergency stop output for robot

E-Field Probes

Model: ET3DV5 S/N: 1368 S/N: 1370
Construction: Triangular core fiber optic detection system
Frequency: 10 MHz to 6 GHz
Linearity: ± 0.2 dB (30 MHz to 3 GHz)

Phantom

Phantom: Generic Twin
Shell Material: Fiberglass
Thickness: 2.0 ± 0.1 mm

Tissue Parameters

450 MHz (Muscle)

Dielectric Constant: ϵ 57.5
Conductivity: σ 0.82

8.1 MEASUREMENT PROCESS

8.2 System Verification

Prior to assessment, the system is verified to the $\pm 5\%$ of the specifications by using the system validation kit. (Graphics plots attached)

Validation Kit D835V2, S/N: 406	Muscle	Targeted SAR _{1g} (mW/g) 2.11	Measured SAR _{1g} (mW/g) 2.19
------------------------------------	--------	---	---

8.3 Dosimetric Assessment Setup

The evaluation was performed with the following procedure:

1. The SAR value at a fixed location above the ear point was measured and was used as a reference value for assessing the power drop.
2. The SAR distribution at the exposed side of the head was measured at a distance of 3.9mm from the inner surface of the shell. The area covered the entire dimension of the head and the horizontal grid spacing was 20mm x 20mm. Based on this data, the area of the maximum absorption was determined by spline interpolation.
3. Around this point, a volume of 32mm x 32mm x 34mm was assessed by measuring 5 x 5 x 7 points. On this basis of this data set, the spatial peak SAR value was evaluated with the following procedure:
 - a. The data at the surface were extrapolated, since the center of the dipoles is 2.7mm away from the tip of the probe and the distance between the surface and the lowest measuring point is 1.2mm. The extrapolation was based on a least square algorithm [13]. A polynomial of the fourth order was calculated through the points in z-axes. This polynomial was then used to evaluate the points between the surface and the probe tip.
 - b. The maximum interpolated value was searched with a straight-forward algorithm. Around this maximum the SAR values averaged over the spatial volumes (1g or 10g) were computed using the 3D-Spline interpolation algorithm. The 3D-spline is composed of three one-dimensional splines with the "Not a knot" condition (in x,y, and z directions) [13][14]. The volume was integrated with the trapezoidal algorithm. One thousand points (10 x 10 x 10) were interpolated to calculate the average.
 - c. All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.
4. The SAR value, at the same location as procedure #1, was re-measured. If the value changed by more than 5%, the evaluation is repeated.

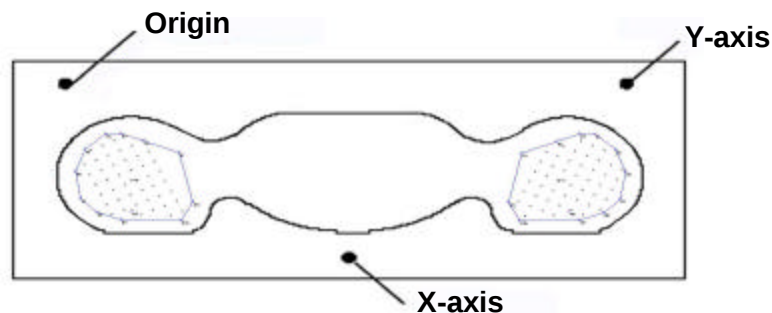


Fig 10. SAR Measurement Points in Area Scan

9.1 TEST POSITION OF THE RADIO

9.2 FACE-HELD TEST SETUP

The radio was placed in a normal operating position with the center of the mouthpiece aligned with the mouth and parallel to the face of the phantom (See figure 8.) Testing is performed with the use of a head/torso, or flat phantom, as applicable, filled with a muscle equivalent tissue. SAR test is then performed in antenna in and out (if applicable), or fixed antenna position using the low, middle and high channels.

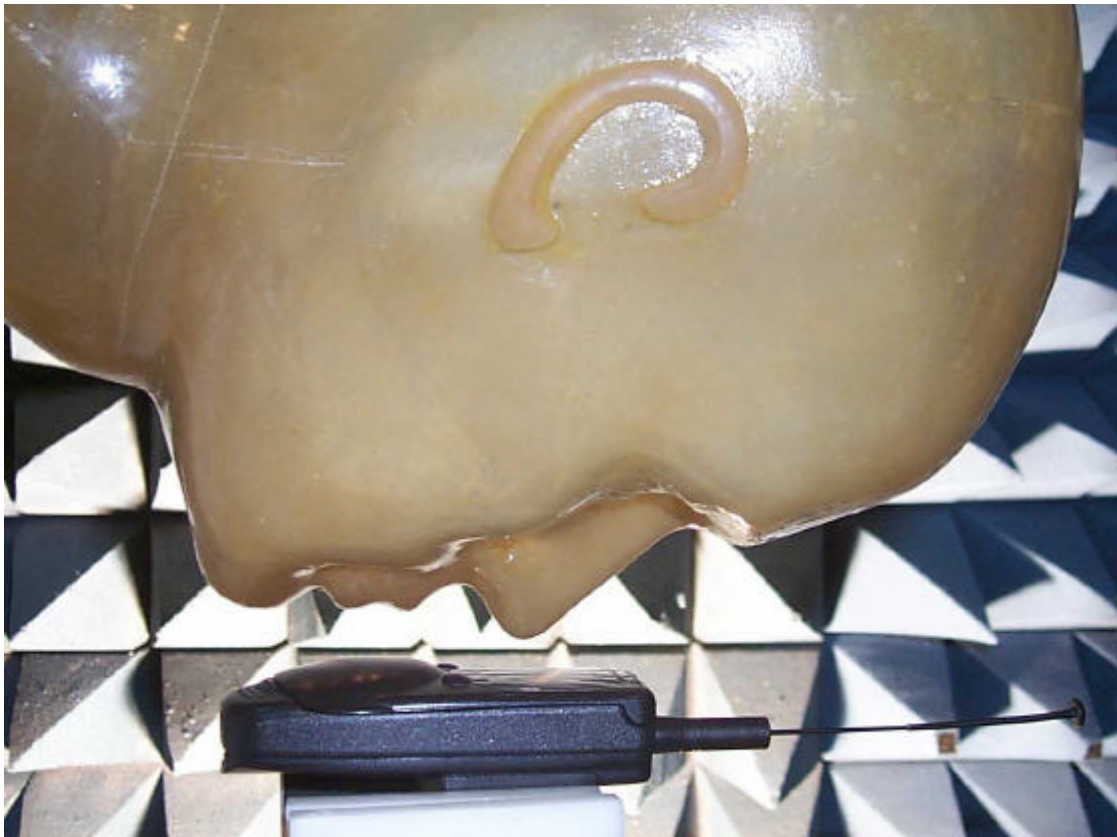


Figure 11. Diagram showing typical alignment of radio held to face.

10.1 BODY-WORN CONFIGURATION TEST SETUP

10.2 Ear-Microphone Jack

Portable transmitting devices which have an Ear-Microphone jack must be evaluated for RF exposure in a body-worn configuration. The testing is performed with the use of a torso phantom filled with muscle equivalent tissue. The EUT is positioned with the keypad facing away from the phantom, and the Ear-Microphone wire attached to the phone jack, simulating the device placed in a shirt pocket or attached to a body holster. The SAR tests are then performed in both the antenna in and antenna out positions using the low, middle, and high channels to investigate the worst case SAR value (see Figure 12). Please note that body-worn configurations which have not been SAR tested may result in operating conditions that could exceed FCC RF exposure limits, therefore, users are cautioned to use tested and/or approved accessories.

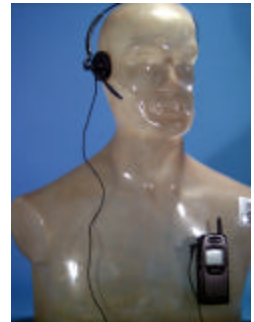


Figure 12.
Ear-Microphone Jack

A. Shirt Pocket Configuration

The shirt pocket configuration is used for devices designed to be body-worn, and small enough to be placed inside a shirt pocket. To simulate the worst-case configuration, the EUT is placed in a torso position on the phantom with the keypad facing away from the phantom, and the Ear-Microphone wire connected to the phone to simulate hands-free operation in a shirt-pocket configuration (see Figure 13).

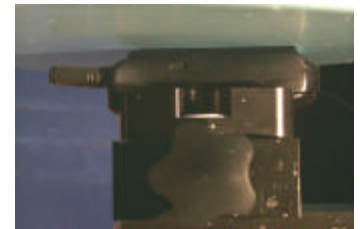


Figure 13.
Shirt Pocket Configuration

B. Body Holster Configuration

The body holster configuration is used for body-worn devices which have a body holster accessory. Typically, a holster or carrying case is provided or available as an accessory item for supporting headset and body-worn operations. SAR may vary depending on the body separation distance provided by the type of holster and batteries supplied for a phone. In most cases, the antenna may become closer to the user's body than next to the head. The design of the holster permits the phone to be positioned only with the keypad facing away from the phantom. Proper usage of the holster restricts the antenna to a specified distance away from the surface of the body. For this test the EUT is placed into the holster and the holster is positioned against the torso of the phantom in a normal operating position. The Ear-Microphone wire is then connected to the phone to simulate hands-free operation in a body holster configuration (see Figure 14).



Figure 14.
Body Holster Configuration

C. Other Configurations

If other operating configurations are possible (i.e.: pants pocket, car adapter kit, etc), it will be indicated to users in the instruction manual about untested conditions and the possibility of exceeding FCC RF exposure limits for such use or the use of third-party accessories. If there is a high potential for exceeding limits in certain unintended configurations, a warning statement will be included in the manual, warning the user to avoid such operating conditions.

11.1 ANSI/IEEE C95.1 - 1992 RF EXPOSURE LIMITS

HUMAN EXPOSURE	UNCONTROLLED ENVIRONMENT General Population (W/kg) or (mW/g)	CONTROLLED ENVIRONMENT Occupational (W/kg) or (mW/g)
SPATIAL PEAK SAR * (Brain)	1.60	8.00
SPATIAL AVERAGE SAR ** (Whole Body)	0.08	0.40
SPATIAL PEAK SAR *** (Hands / Feet / Ankle / Wrist)	4.00	20.00

Table 2. Safety Limits for Partial Body Exposure [2]

NOTES:

- * The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
- ** The Spatial Average value of the SAR averaged over the whole-body.
- *** The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure.

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation).

12.1 MEASUREMENT UNCERTAINTIES

Measurement uncertainties in SAR measurements are difficult to quantify due to several variables including biological, physiological, and environmental. However, we estimate the measurement uncertainties in SAR to be less than 15-25 % [16].

According to ANSI/IEEE C95.3, the overall uncertainties are difficult to assess and will vary with the type of meter and usage situation. However, accuracy's of ± 1 to 3 dB can be expected in practice, with greater uncertainties in near-field situations and at higher frequencies (shorter wavelengths), or areas where large reflecting objects are present. Under optimum measurement conditions, SAR measurement uncertainties of at least ± 2 dB can be expected.[3]

According to CENELEC [17], typical worst-case uncertainty of field measurements is ± 5 dB. For well-defined modulation characteristics the uncertainty can be reduced to ± 3 dB.

Uncertainty Description	Error	Distribution	Weight	Std. Deviation	Offset
Probe Uncertainty					
Axial isotropy	± 0.2 dB	U-Shaped	0.5	± 2.4 %	
Spherical isotropy	± 0.4 dB	U-Shaped	0.5	± 4.8 %	
Isotropy from gradient	± 0.5 dB	U-Shaped	0	$\pm$	
Spatial resolution	± 0.5 %	Normal	1	± 0.5 %	
Linearity error	± 0.2 dB	Rectangle	1	± 2.7 %	
Calibration error	± 3.3 %	Normal	1	± 3.3 %	
SAR Evaluation Uncertainty					
Data acquisition error	± 1 %	Rectangle	1	± 0.6 %	
ELF and RF disturbances	± 0.25 %	Normal	1	± 0.25 %	
Conductivity assessment	± 10 %	Rectangle	1	± 5.8 %	
Spatial Peak SAR Evaluation Uncertainty					
Extrapolated boundary effect	± 3 %	Normal	1	± 3 %	± 5 %
Probe positioning error	± 0.1 mm	Normal	1	± 1 %	
Integrated and cube orientation	± 3 %	Normal	1	± 3 %	
Cube Shape inaccuracies	± 2 %	Rectangle	1	± 1.2 %	
Device positioning	± 6 %	Normal	1	± 6 %	
Combined Uncertainties				± 11.7 %	± 5 %

Table 3. Breakdown of Errors [18]

13.1 SAR TEST DATA SUMMARY

Ambient TEMPERATURE (°C)	20.1
Relative HUMIDITY (%)	58.7
Atmospheric PRESSURE (kPa)	99.7

Mixture Type: Muscle

Dielectric Constant: 57.5

Conductivity: 0.82 S/m

13.2 Measurement Results (Mouth SAR including 50% Duty Cycle)

Frequency		Modulation	Power* (Watts)	Separation Distance (cm)	Antenna Position	SAR** (W/kg)
MHz	Ch.					
450.025	00	FM	5.0	2.5 cm	Fixed	3.085
467.525	08	FM	5.0	2.5 cm	Fixed	2.605
484.975	16	FM	5.0	2.5 cm	Fixed	2.015
ANSI / IEEE C95.1 1992 - SAFETY LIMIT Spatial Peak (Muscle) Controlled Environment/Occupational Exposure Limits				Mouth/Face 8.0 W/kg (mW/g) averaged over 1 gram for Controlled Environment / Occupational Exposure Limits; including 50% Duty Cycle		

NOTES:

- All modes of operation were investigated and the worst-case are reported.
- Battery condition is fully charged for all readings.
- Battery ☒ Standard ☐ Extended
- *Power Measured ☒ Conducted ☐ EIRP ☐ ERP
- SAR Measurement System ☒ SPEAG ☐ IDX
- SAR Configuration ☒ Mouth ☐ Body ☐ Hand
- **SAR Test Data includes a 50% Duty Cycle


Randy Ortanez
President & Chief Engineer



Figure 15.
MOUTH SAR Test Setup

13.1 SAR TEST DATA SUMMARY

Ambient TEMPERATURE (°C)	20.1
Relative HUMIDITY (%)	58.7
Atmospheric PRESSURE (kPa)	99.7

Mixture Type: Muscle

Dielectric Constant: 57.5

Conductivity: 0.82 S/m

13.3 Measurement Results (Body SAR including 50% Duty Cycle)

Frequency		Modulation	Power* (W)	Separation Distance (cm)	Antenna Position	SAR*** (W/kg)
MHz	Ch.					
450.025	00	FM	5.0	1.5 cm	Fixed	5.600
467.525	08	FM	5.0	1.5 cm	Fixed	4.985
484.975	16	FM	5.0	1.5 cm	Fixed	4.360
ANSI / IEEE C95.1 1992 - SAFETY LIMIT Spatial Peak (Muscle) Controlled Environment/Occupational Exposure Limits				Body 8.0 W/kg (mW/g) averaged over 1 gram for Controlled Environment / Occupational Exposure Limits; including 50% Duty Cycle		

NOTES:

- All modes of operation were investigated and the worst-case are reported.
- Battery condition is fully charged for all readings.
- Battery Type ☒ Standard ☐ Extended
- * Power Measured ☒ Conducted ☐ EIRP ☐ ERP
- SAR Measurement System ☒ SPEAG ☐ IDX
- SAR Configuration ☐ Mouth ☒ Body ☐ Hand
- ** Test Configuration ☒ Belt Clip ☐ Without Belt Clip
- ***SAR Test Data includes a 50% Duty Cycle


Randy Ortanez
President & Chief Engineer



Figure 16.
BODY SAR Test Setup w/ Belt Clip

14.1 SAR TEST EQUIPMENT

14.2 Type / Model	Calib. Date	S/N:
Stäubli Robot RX60L	Feb. 00	599131-01
Stäubli Robot Controller	Feb. 00	PCT592
Stäubli Teach Pendant (Joystick)	Feb. 00	3323-00161
Micron Computer 450 MHz Pentium III, Windows NT	Feb. 00	PCT577
SPEAG EDC3	Feb. 00	321
SPEAG DAE3	Feb. 00	330
SPEAG E-Field Probe ET3DV5	Feb. 00	1368
SPEAG E-Field Probe ET3DV5	Feb. 00	1370
SPEAG Dummy Probe	Feb. 00	PCT583
SPEAG Generic Twin Phantom	Feb. 00	PCT587
SPEAG Light Alignment Sensor	Feb. 00	205
SPEAG Validation Dipole D1900V2	Feb. 00	PCT593
Muscle Equivalent Matter (450MHz)	Dec. 00	PCTBEM10
Muscle Equivalent Matter (835MHz)	Dec. 00	PCTBEM14
Robot Table		PCT586
Phone Holder		PCT588
A/B Power Indicator		PCT589
Remote Power Switch		PCT590
Phantom Cover		PCT591
HP Spectrum Analyzer	Dec. 99	PCT200
IFI TEM Cell Model: CC110EXX (DC - 2000 MHz)	Jan. 00	A427-0697
Microwave Amp. Model: 5S1G4 (800MHz - 4.2GHz, 5 Watts)	Jan. 00	22332

NOTE:

The E-field probe was calibrated by SPEAG. The SAR calibration of the E-field probe is performed by temperature measurement procedure. A TEM cell is used for the free space calibration of the probe. The tissue simulating material is calibrated by PCTEST using the dielectric probe system and network analyzer to determine the conductivity and permittivity (dielectric constant) of the desired equivalent material.

The following list of equipment was used to calibrate the equivalent materials:

Power Meter	Gigatronics 8651A
Signal Generator	HP-8648D (9kHz ~ 4GHz)
Power Amp	Amplifier Research 5S1G4 (5 Watts, 800MHz ~ 4.2GHz)
Network Analyzer	HP-8753E (30kHz ~ 3GHz)
Dielectric Probe Kit	HP85070B

15.1 CONCLUSION

The SAR measurement indicates that the EUT complies with the RF radiation exposure limits of the FCC. These measurements are taken to simulate the RF effects exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests.

Please note that the absorption and distribution of electromagnetic energy in the body are very complex phenomena that depend on the mass, shape, and size of the body, the orientation of the body with respect to the field vectors, and the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables.[3]

16.1 REFERENCES:

- [1] Federal Communications Commission, ET Docket 93-62, Guidelines for Evaluating the Environmental Effects of Radiofrequency Radiation, Aug. 1996.
- [2] ANSI/IEEE C95.1 - 1991, *American National Standard safety levels with respect to human exposure to radio frequency electromagnetic fields, 300kHz to 100GHz*, New York: IEEE, Aug. 1992
- [3] ANSI/IEEE C95.3 - 1991, *IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields - RF and Microwave*, New York: IEEE, 1992.
- [4] NCRP, National Council on Radiation Protection and Measurements, *Biological Effects and Exposure Criteria for RadioFrequency Electromagnetic Fields*, NCRP Report No. 86, 1986. Reprinted Feb. 1995.
- [5] T. Schmid, O. Egger, N. Kuster, *Automated E-field scanning system for dosimetric assessments*, IEEE Transaction on Microwave Theory and Techniques, vol. 44, Jan. 1996, pp. 105-113.
- [6] K. Pokovic, T. Schmid, N. Kuster, *Robust setup for precise calibration of E-field probes in tissue simulating liquids at mobile communications frequencies*, ICECOM97, Oct. 1997, pp. 120-124.
- [7] K. Poković, T. Schmid, and N. Kuster, *E-field Probe with improved isotropy in brain simulating liquids*, Proceedings of the ELMAR, Zadar, Croatia, June 23-25, 1996, pp. 172-175.
- [8] Schmid & Partner Engineering AG, Application Note: Data Storage and Evaluation, June 1998, p2.
- [9] V. Hombach, K. Meier, M. Burkhardt, E. Kuhn, N. Kuster, *The Dependence of EM Energy Absorption upon Human Head Modeling at 900 MHz*, IEEE Transaction on Microwave Theory and Techniques, vol. 44 no. 10, Oct. 1996, pp. 1865-1873.
- [10] N. Kuster and Q. Balzano, *Energy absorption mechanism by biological bodies in the near field of dipole antennas above 300MHz*, IEEE Transaction on Vehicular Technology, vol. 41, no. 1, Feb. 1992, pp. 17-23.
- [11] G. Hartsgrrove, A. Kraszewski, A. Surowiec, *Simulated Biological Materials for Electromagnetic Radiation Absorption Studies*, University of Ottawa, Bioelectromagnetics, Canada: 1987, pp. 29-36.
- [12] Q. Balzano, O. Garay, T. Manning Jr., *Electromagnetic Energy Exposure of Simulated Users of Portable Cellular Telephones*, IEEE Transactions on Vehicular Technology, vol. 44, no.3, Aug. 1995.
- [13] W. Gander, *Computermathematick*, Birkhaeuser, Basel, 1992.
- [14] W.H. Press, S.A. Teukolsky, W.T. Vetterling, and B.P. Flannery, *Numerical Recepies in C*, The Art of Scientific Computing, Second edition, Cambridge University Press, 1992.
- [15] Federal Communications Commission, OET Bulletin 65, *Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields*. Supplement C, Dec. 1997.
- [16] N. Kuster, R. Kastle, T. Schmid, *Dosimetric evaluation of mobile communications equipment with known precision*, IEEE Transaction on Communications, vol. E80-B, no. 5, May 1997, pp. 645-652.
- [17] CENELEC CLC/SC111B, European Prestandard (prENV 50166-2), *Human Exposure to Electromagnetic Fields High-frequency: 10kHz-300GHz*, Jan. 1995.
- [18] Prof. Dr. Niels Kuster, ETH, Eidgenössische Technische Hochschule Zürich, *Dosimetric Evaluation of the Cellular Phone*.

APPENDIX A – SAR TEST PLOTS

VERTEX STANDARD FCC ID:K66VX-900U -- FM Mouth SAR

Generic Twin Phantom; Flat Section; Probe: ET3DV5 - SN1370 -- Probe Cal Date 02/00

Med. Parameters 450 MHz Muscle: $\sigma = 0.82 \text{ mho/m}$ $\epsilon_r = 57.5$ $\rho = 1.00 \text{ g/cm}^3$; Antenna Position -- Out; Crest Factor 1.0


SAR (1g): 6.17 mW/g, SAR (10g): 4.80 mW/g

Vertex Standard Portable Radio Model: VX-9000U

FM Low Channel 450.025MHz

High Conducted Power = 5 Watts; Spacing = 2.5cm from flat phantom to radio front

Test Date -- 12-11-2000

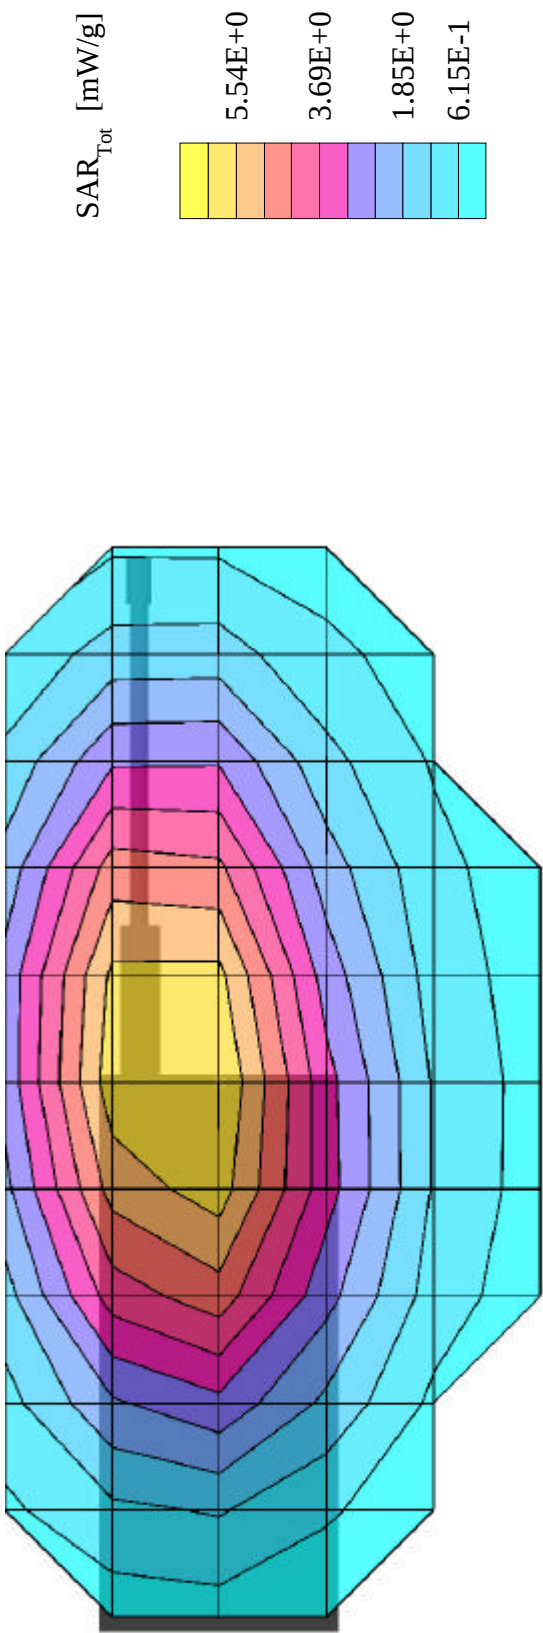

VERTEX STANDARD FCC ID:K66VX-900U -- FM Mouth SAR

Generic Twin Phantom; Flat Section; Probe: ET3DV5 - SN1370 -- Probe Cal Date 02/00

Med. Parameters 450 MHz Muscle: $\sigma = 0.82 \text{ mho/m}$ $\epsilon_r = 57.5$ $\rho = 1.00 \text{ g/cm}^3$; Antenna Position -- Out; Crest Factor 1.0


SAR (1g): 5.21 mW/g, SAR (10g): 4.07 mW/g

Vertex Standard Portable Radio Model: VX-9000U

FM Mid Channel 467.525MHz

High Conducted Power = 5 Watts; Spacing = 2.5cm from flat phantom to radio front

Test Date -- 12-11-2000

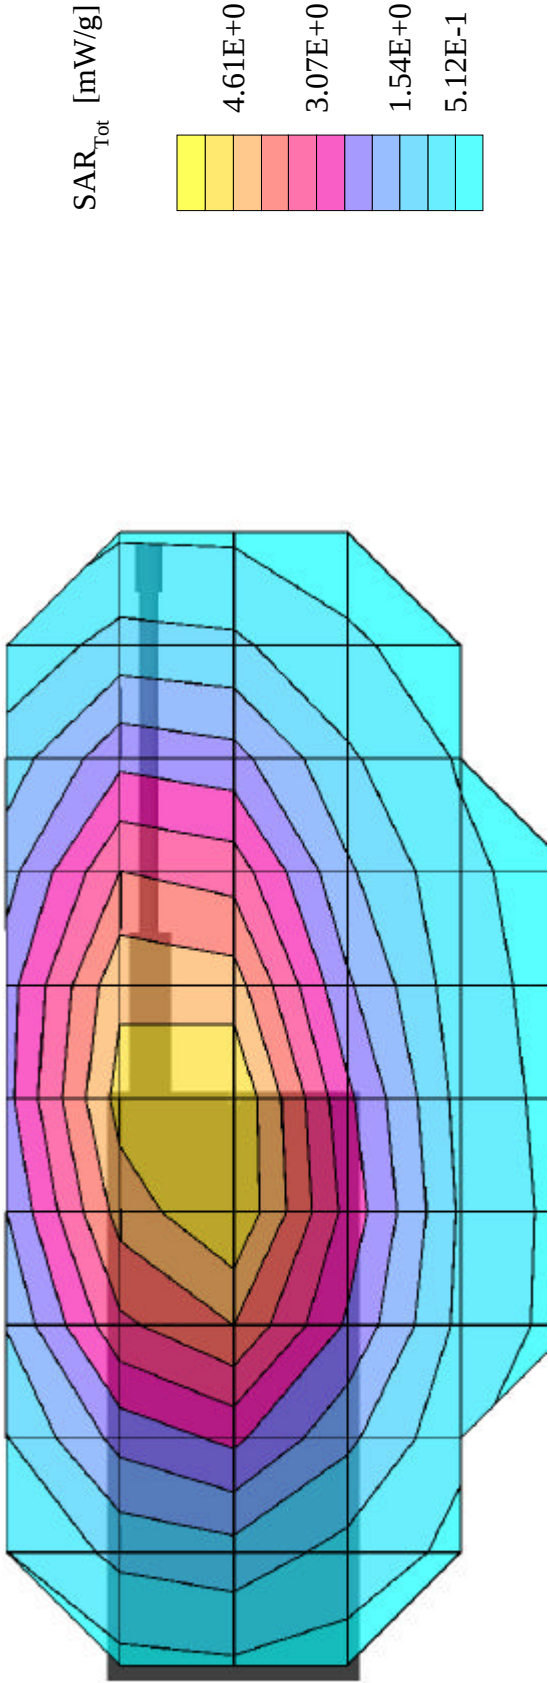

VERTEX STANDARD FCC ID:K66VX-900U -- FM Mouth SAR

Generic Twin Phantom; Flat Section; Probe: ET3DV5 - SN1370 -- Probe Cal Date 02/00

Med. Parameters 450 MHz Muscle: $\sigma = 0.82 \text{ mho/m}$ $\epsilon_r = 57.5$ $\rho = 1.00 \text{ g/cm}^3$; Antenna Position -- Out; Crest Factor 1.0


SAR (1g): 4.03 mW/g, SAR (10g): 3.19 mW/g

Vertex Standard Portable Radio Model: VX-9000U

FM High Channel 484.975MHz

High Conducted Power = 5 Watts; Spacing = 2.5cm from flat phantom to radio front

Test Date -- 12-11-2000

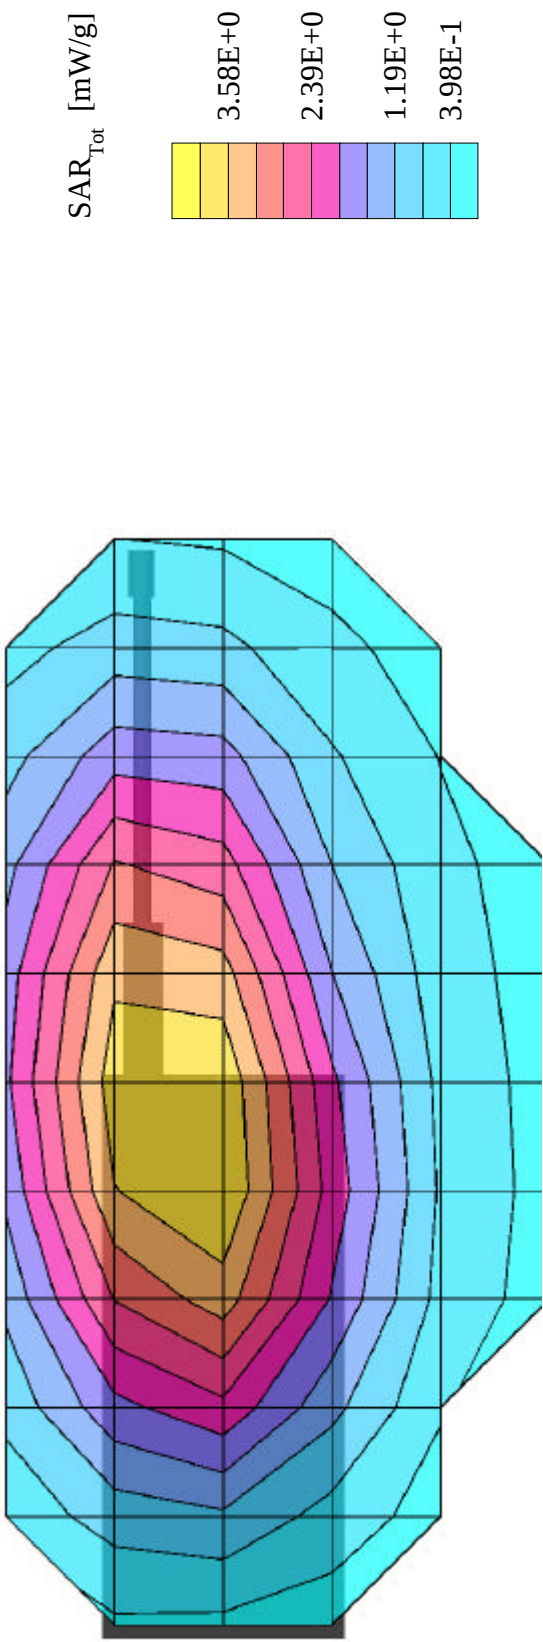

VERTEX STANDARD FCC ID:K66VX-900U -- FM Body SAR

Generic Twin Phantom; Flat Section; Probe: ET3DV5 - SN1370 -- Probe Cal Date 02/00

Med. Parameters 450 MHz Muscle: $\sigma = 0.82 \text{ mho/m}$ $\epsilon_r = 57.5$ $\rho = 1.00 \text{ g/cm}^3$; Antenna Position -- Out; Crest Factor 1.0


SAR (1g): 11.2 mW/g, SAR (10g): 8.10 mW/g

Vertex Standard Portable Radio Model: VX-9000U

FM Low Channel 450.025MHz

High Conducted Power = 5 Watts; Spacing = 1.5cm from flat phantom to radio back, w/Beltclip

Test Date -- 12-11-200

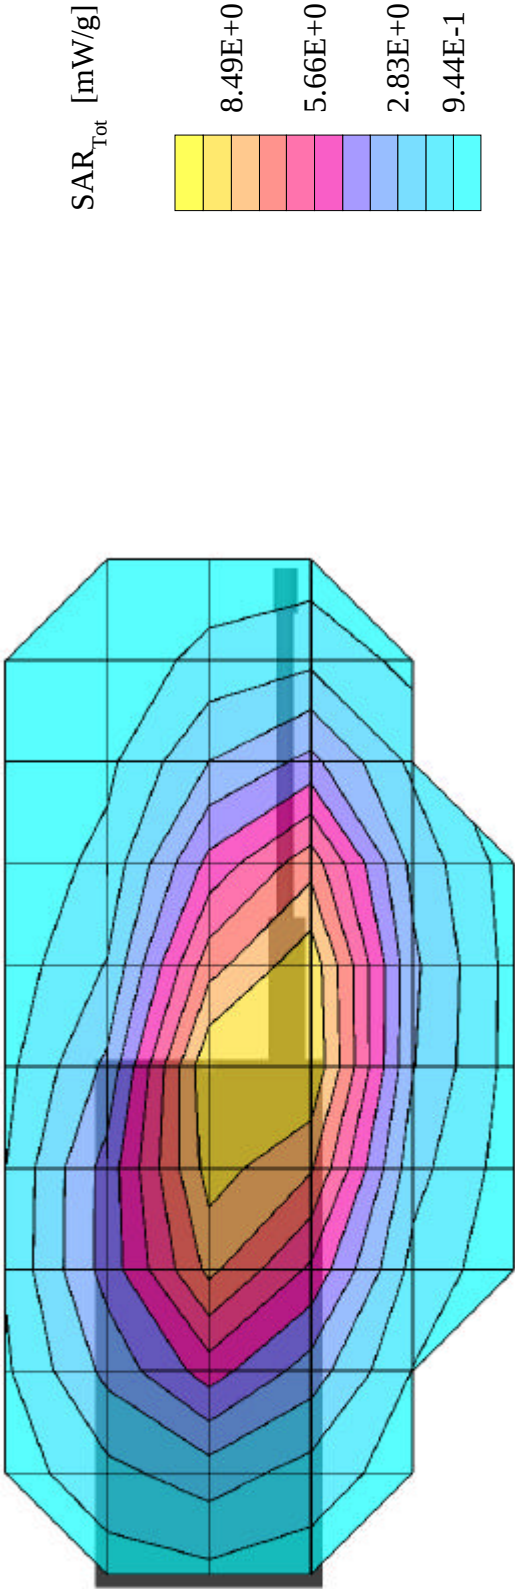

VERTEX STANDARD FCC ID:K66VX-900U -- FM Body SAR

Generic Twin Phantom; Flat Section; Probe: ET3DV5 - SN1370 -- Probe Cal Date 02/00

Med. Parameters 450 MHz Muscle: $\sigma = 0.82 \text{ mho/m}$ $\epsilon_r = 57.5$ $\rho = 1.00 \text{ g/cm}^3$; Antenna Position -- Out; Crest Factor 1.0


SAR (1g): 9.97 mW/g, SAR (10g): 7.26 mW/g

Vertex Standard Portable Radio Model: VX-9000U

FM Mid Channel 467.525MHz

High Conducted Power = 5 Watts; Spacing = 1.5cm from flat phantom to radio back, w/Beltclip

Test Date -- 12-11-200

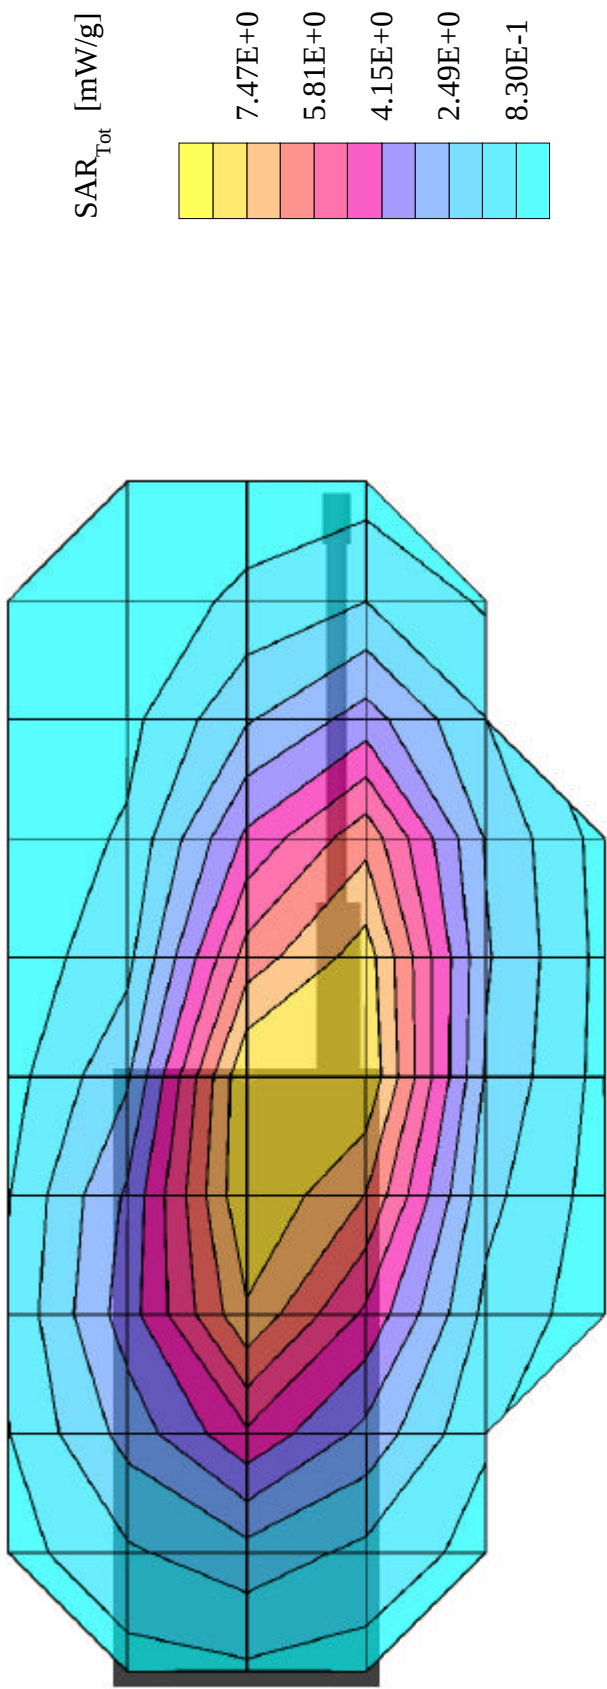

VERTEX STANDARD FCC ID:K66VX-900U -- FM Body SAR

Generic Twin Phantom; Flat Section; Probe: ET3DV5 - SN1370 -- Probe Cal Date 02/00

Med. Parameters 450 MHz Muscle: $\sigma = 0.82 \text{ mho/m}$ $\epsilon_r = 57.5$ $\rho = 1.00 \text{ g/cm}^3$; Antenna Position -- Out; Crest Factor 1.0


SAR (1g): 8.72 mW/g, SAR (10g): 6.22 mW/g

Vertex Standard Portable Radio Model: VX-9000U


FM High Channel 484.975MHz

High Conducted Power = 5 Watts; Spacing = 1.5cm from flat phantom to radio back, w/Beltclip


Test Date -- 12-11-200

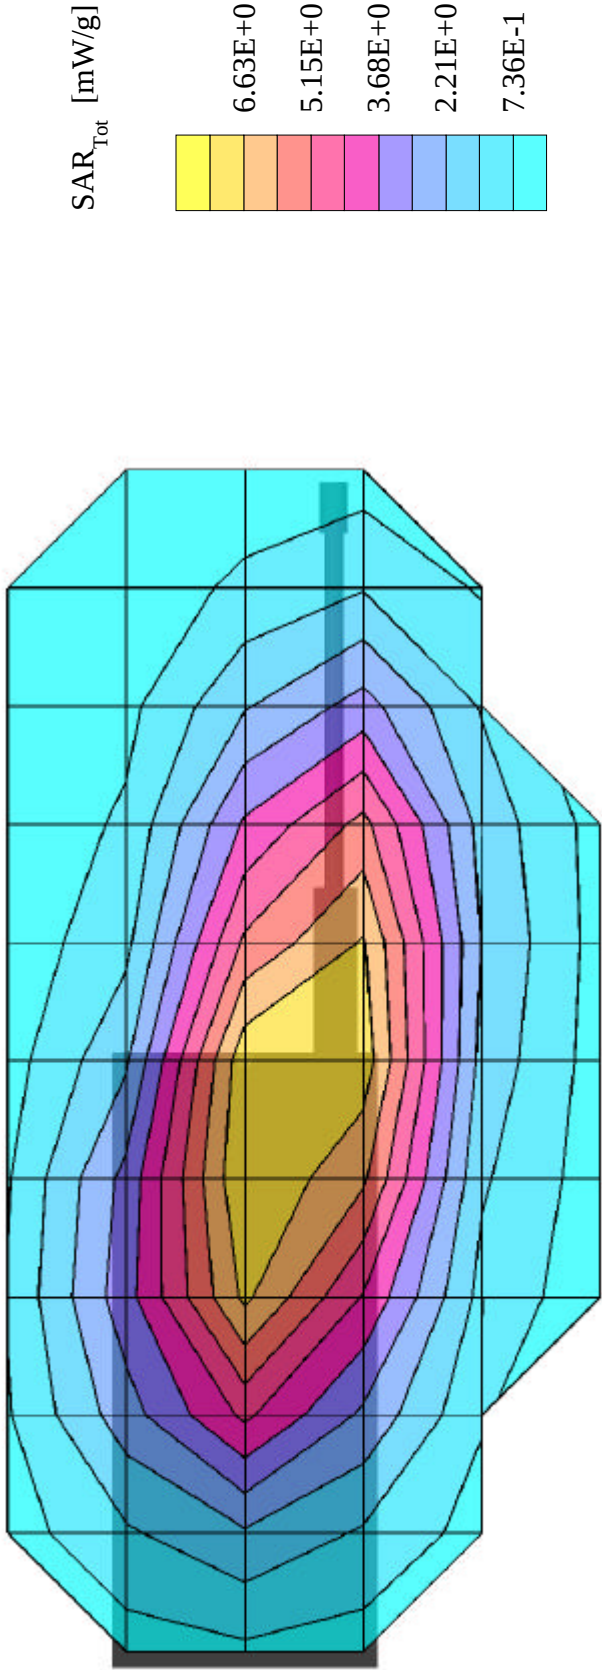


APPENDIX B – SAR TEST SETUP PHOTOGRAPHS

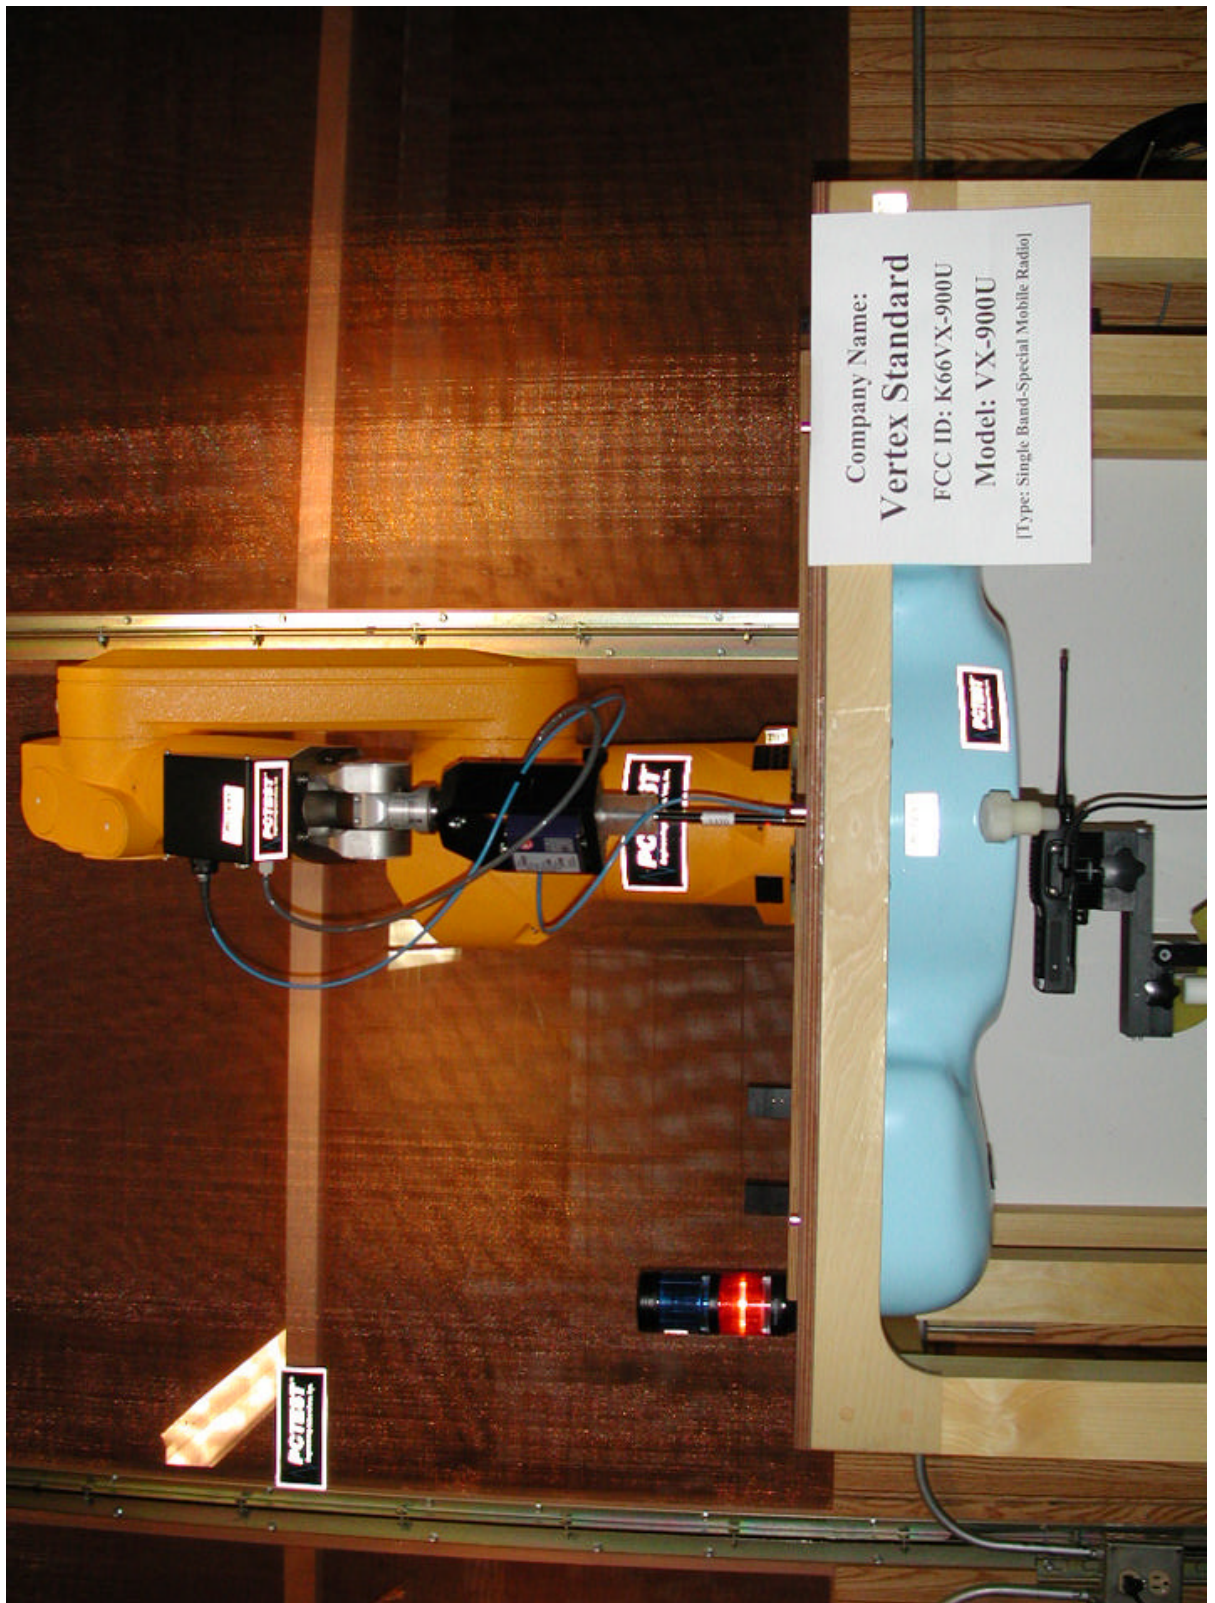



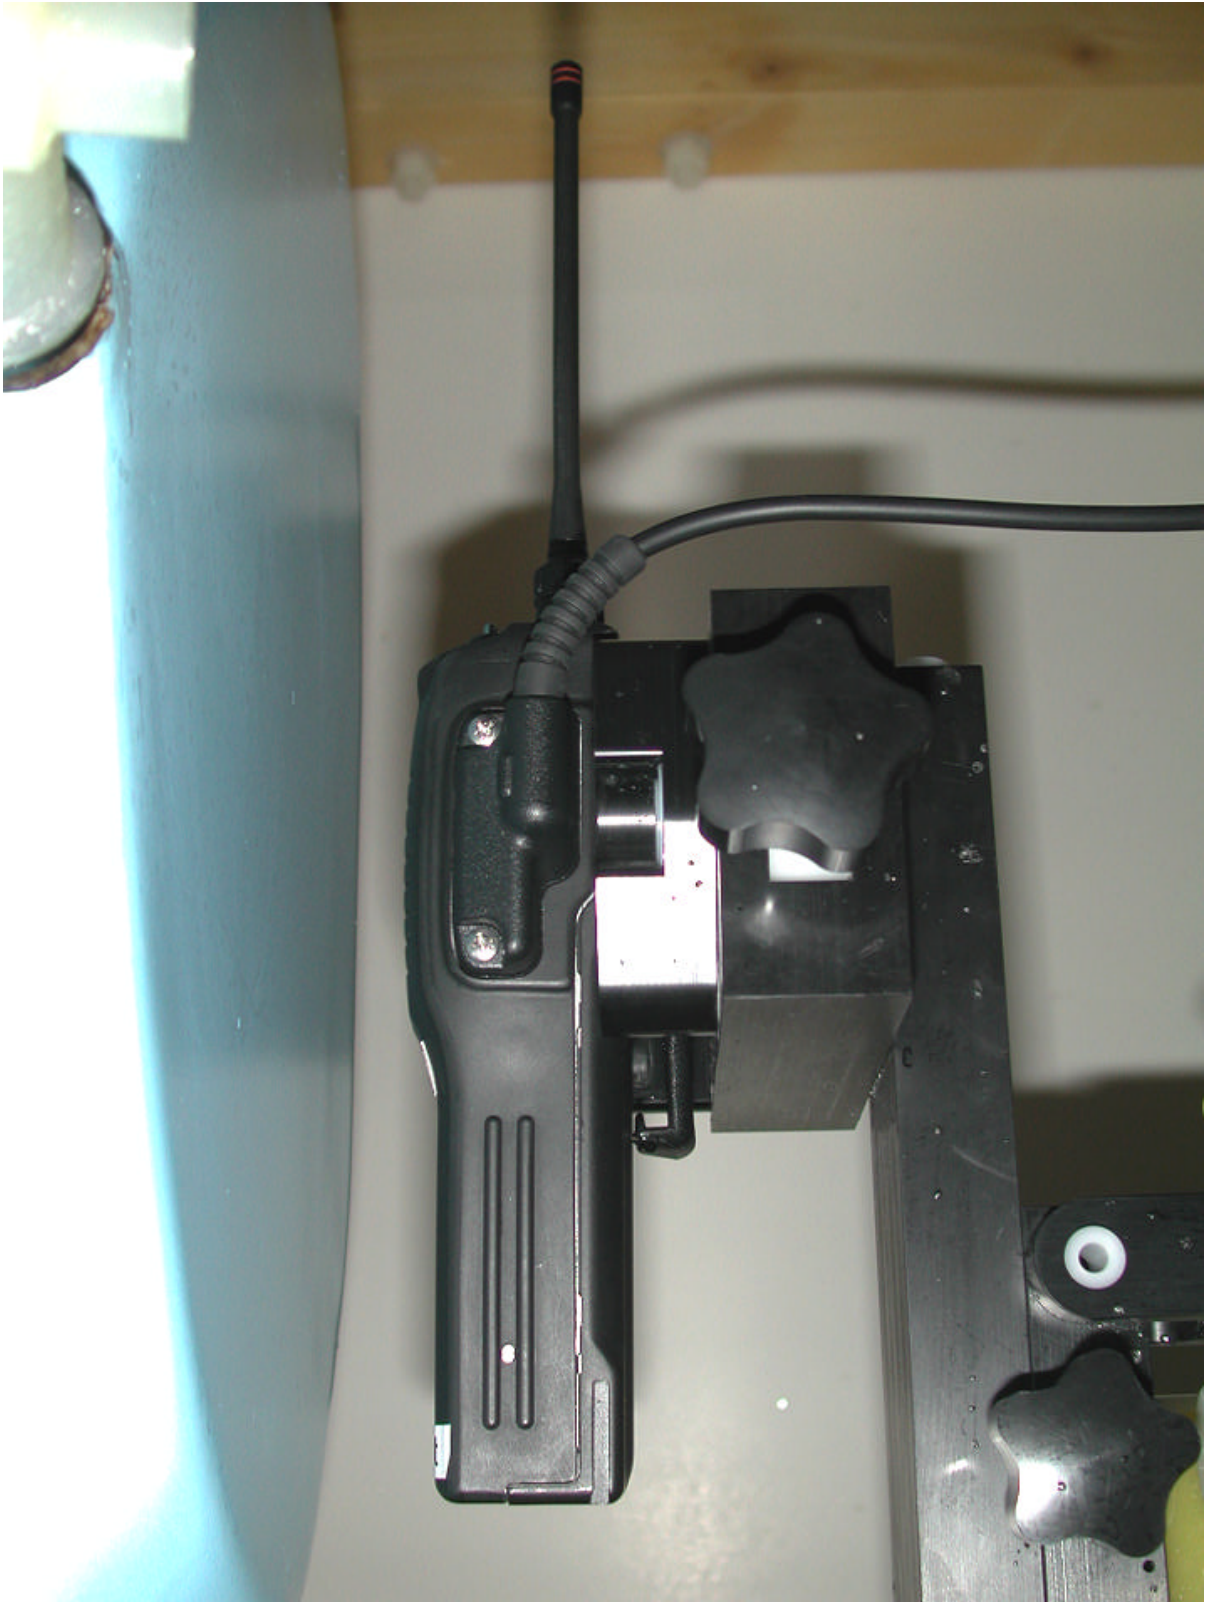

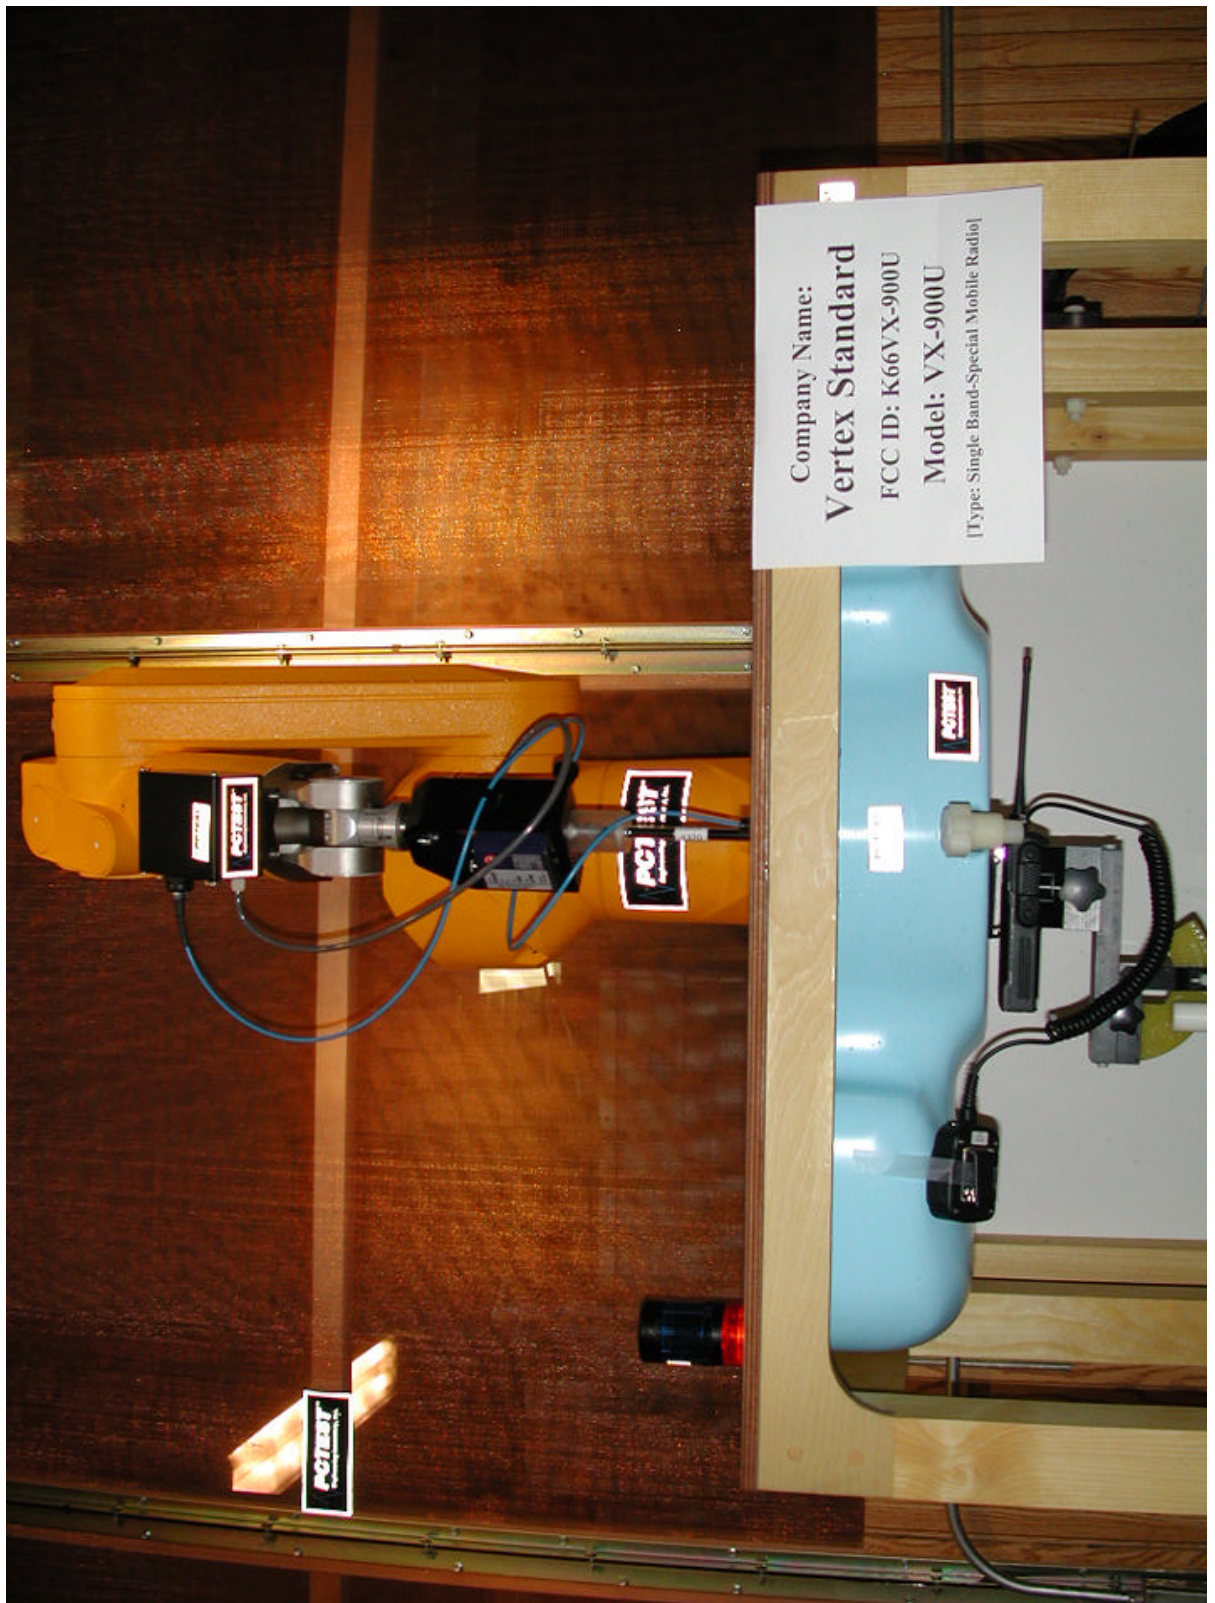






APPENDIX C – DIPOLE VALIDATION DATA

835MHz Muscle Dipole Validation

Generic Twin Phantom; Flat Section; Probe: ET3DV5 - SN1370 -- Probe Cal Date 02/00
Med. Parameters 835 MHz Muscle: $\sigma = 0.95 \text{ mho/m}$ $\epsilon_r = 56.2$ $\rho = 1.00 \text{ g/cm}^3$; Antenna Position -- Out; Crest Factor 1.0
SAR (1g): 2.19 mW/g, SAR (10g): 1.44 mW/g

835MHz Muscle Dipole Validation (D835V2 S/N: 406)
Frequency: 835 MHz; Antenna Input Power: 250 [mW]
PCTEST Muscle Tissue Simulating Liquid

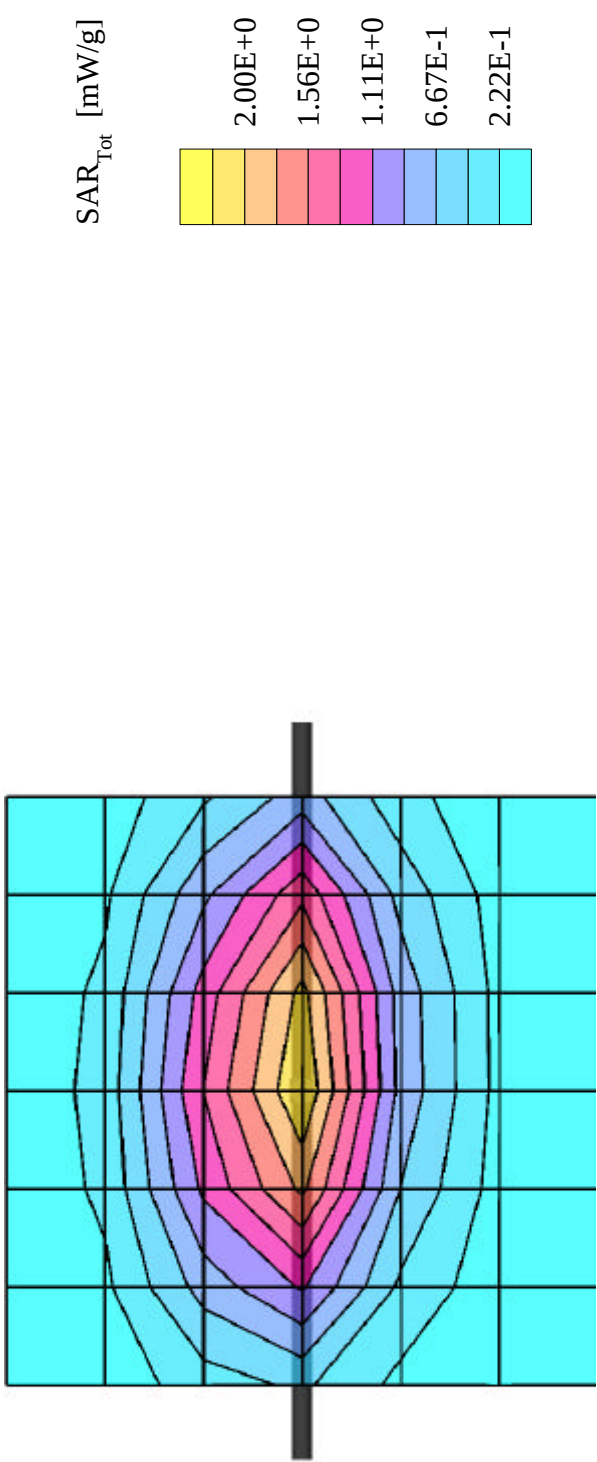

APPENDIX D – PROBE CALIBRATION DATA

Probe ET3DV5

SN:1370

Manufactured:	February 1999
Calibrated:	February 2000

Calibrated for System DASY3

Introduction

The performance of all probes is measured before delivery. This includes an assessment of the characteristic parameters, receiving patterns as a function of frequency, frequency response and relative accuracy. Furthermore, each probe is tested in use according to a dosimetric assessment protocol. The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe and some of the measurement diagrams are given in the following.

The performance of the individual probes varies slightly due to tolerances arising from the manufacturing process. Since the lines are highly resistive (several MOhms), the offset and noise problem is greatly increased if signals in the low μV range are measured. Accurate measurement below 10 $\mu\text{W/g}$ are possible if the following precautions are taken. 1) check the current grounding with the *multimeter*¹, i.e., low noise levels, 2) compensate the current *offset*¹, 3) use long integration time (approx. 10 seconds), 4) *calibrate*¹ before each measurement, 5) persons should avoid moving around the lab while measuring.

Since the field distortion caused by the supporting material and the sheath is quite high in the θ direction, the receiving pattern is poor in air. However, the distortion in tissue equivalent material is much less because of its high dielectricity. In addition, the fields induced in the phantoms by dipole structures close to the body are dominantly parallel to the surface. Thus, the error due to non-isotropy is much better than 1 dB for dosimetric assessments.

The probes are calibrated in the TEM cell if 110 although the field distribution in the cell is not very uniform and the frequency response is not very flat. To ensure consistency, a strict protocol is followed. The conversion factor (ConF) between this calibration and the measurement in the tissue simulation solution is performed by comparison with temperature measurements and computer simulations. This conversion factor is only valid for the specified tissue simulating liquids at the specified frequencies. If measurements have to be performed in solutions with other electrical properties or at other frequencies, the conversion factor has to be assessed by the same procedure.

As the probes have been constructed with printed resistive lines on ceramic substrates (thick film technique), the probe is very delicate with respect to mechanical shocks.

Attention:

Do not drop the probe or let the probe collide with any solid object. Never let the robot move without first activating the emergency stop feature (i.e., without first turning the data acquisition electronics on).

¹ Feature of the DASY Software Tool.

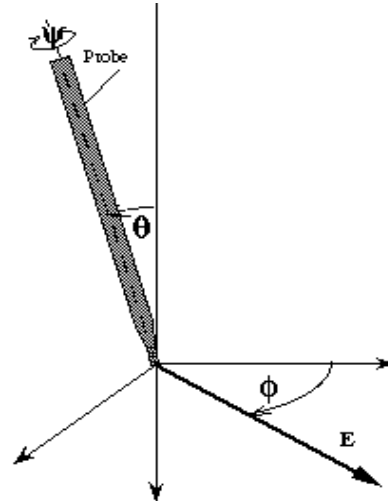


Fig 1: Due to the field distortion caused by the supporting material, the probe has two characteristic directions, referred to as angle ψ and θ .

DASY3 - Parameters of Probe: ET3DV5 SN:1370

Sensitivity in Free Space

NormX	1.58	$\mu\text{V}/(\text{V}/\text{m})^2$
NormY	1.64	$\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	1.80	$\mu\text{V}/(\text{V}/\text{m})^2$

Diode Compression

DCP X	96	mV
DCP Y	96	mV
DCP Z	96	mV

Sensitivity in Tissue Simulating Liquid

450 MHz	ConvF X	6.5	extrapolated
	ConvF Y	6.5	extrapolated
	ConvF Z	6.5	extrapolated

$\epsilon_r =$	$48 \pm 5\%$
$\sigma =$	$0.50 \pm 10\% \text{ mho/m}$
(brain tissue simulating liquid)	

900 MHz	ConvF X	6.0	$\pm 10\%$
	ConvF Y	6.0	$\pm 10\%$
	ConvF Z	6.0	$\pm 10\%$

$\epsilon_r =$	$42.5 \pm 5\%$
$\sigma =$	$0.86 \pm 10\% \text{ mho/m}$
(brain tissue simulating liquid)	

1500 MHz	ConvF X	5.4	interpolated
	ConvF Y	5.4	interpolated
	ConvF Z	5.4	interpolated

$\epsilon_r =$	$41 \pm 5\%$
$\sigma =$	$1.32 \pm 10\% \text{ mho/m}$
(brain tissue simulating liquid)	

1800 MHz	ConvF X	5.1	$\pm 10\%$
	ConvF Y	5.1	$\pm 10\%$
	ConvF Z	5.1	$\pm 10\%$


$\epsilon_r =$	$41 \pm 5\%$
$\sigma =$	$1.69 \pm 10\% \text{ mho/m}$
(brain tissue simulating liquid)	

Sensor Offset


Probe Tip to Sensor Center	2.7	mm
Surface to Probe Tip	1.6 ± 0.2	mm

Receiving Pattern (ϕ), $\theta = 0^\circ$


f = 30 MHz, TEM cell ifi110

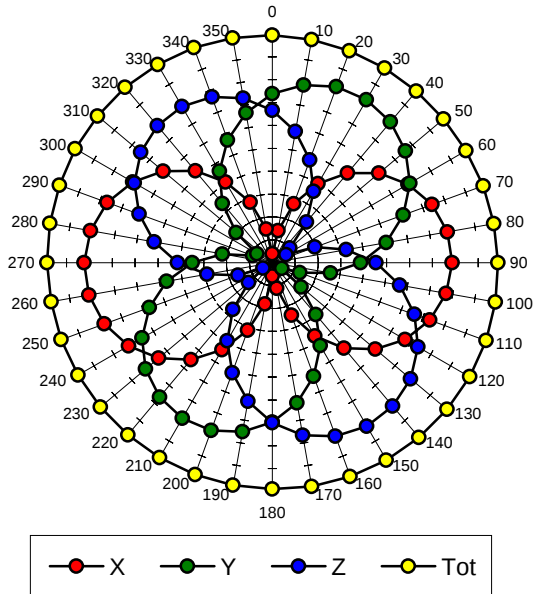


f = 100 MHz, TEM cell ifi110

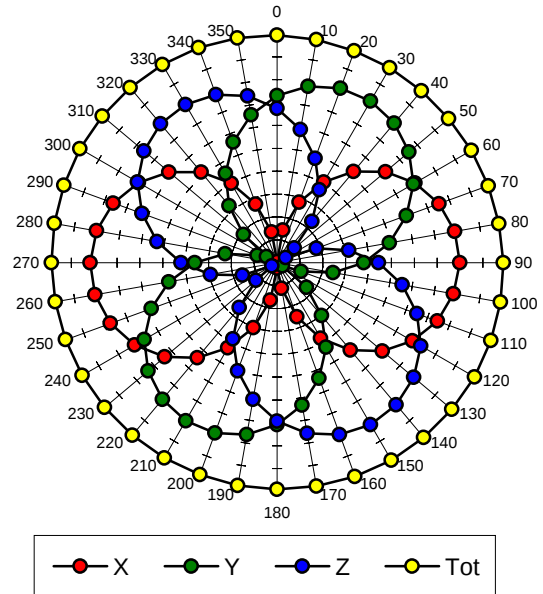


f = 300 MHz, TEM cell ifi110

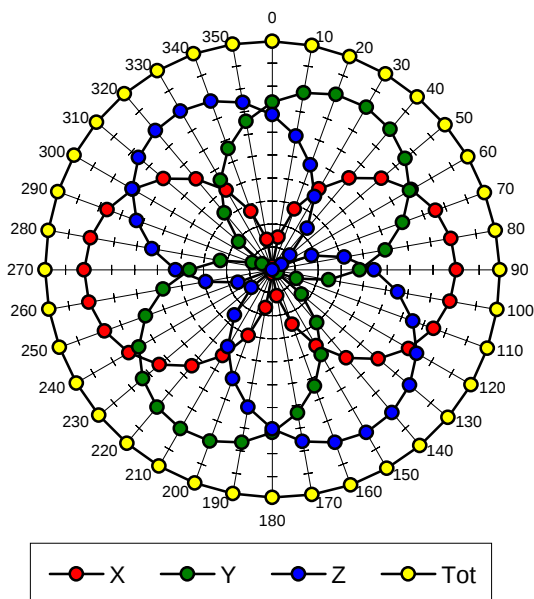


f = 900 MHz, TEM cell ifi110

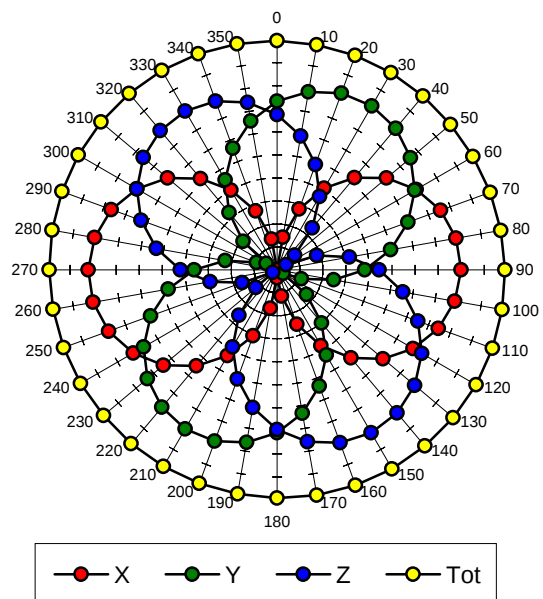

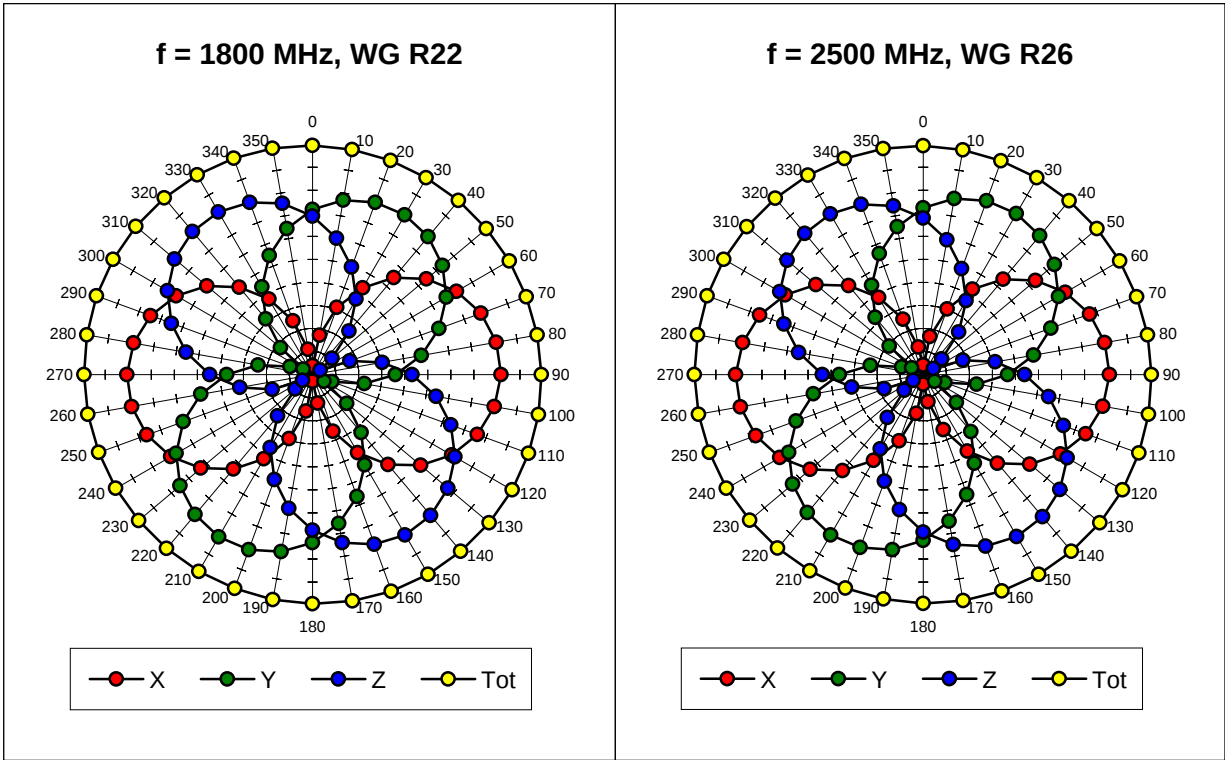


Isotropy Error (ϕ), $\theta = 0^\circ$


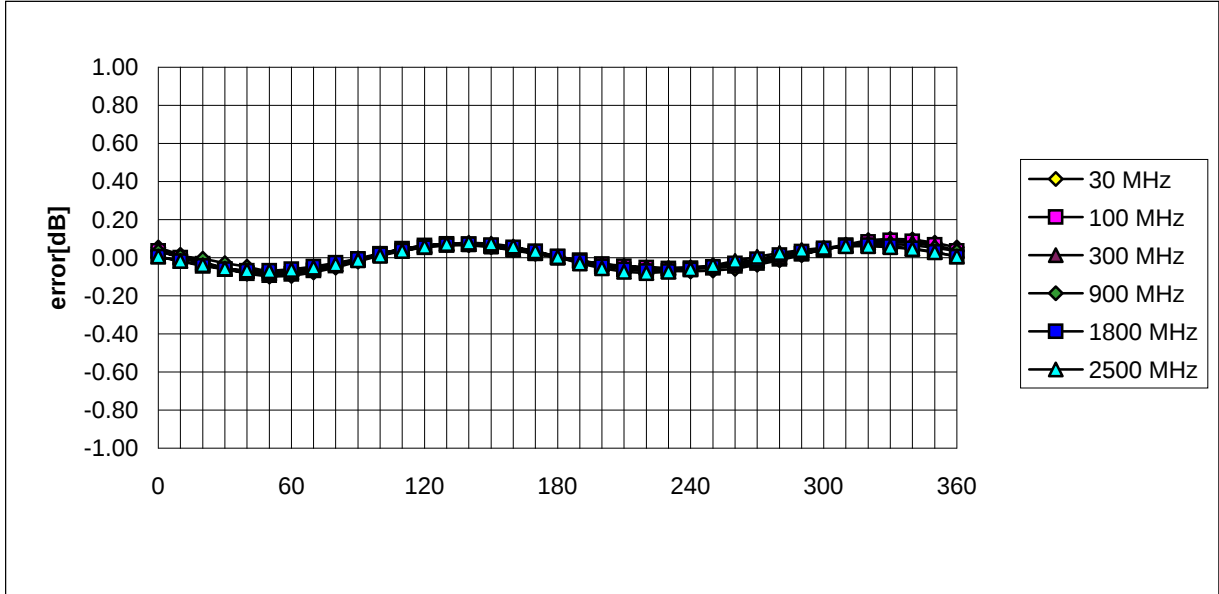


Frequency Response of E-Field


(TEM-Cell:ifi110, Waveguide R22, R26)

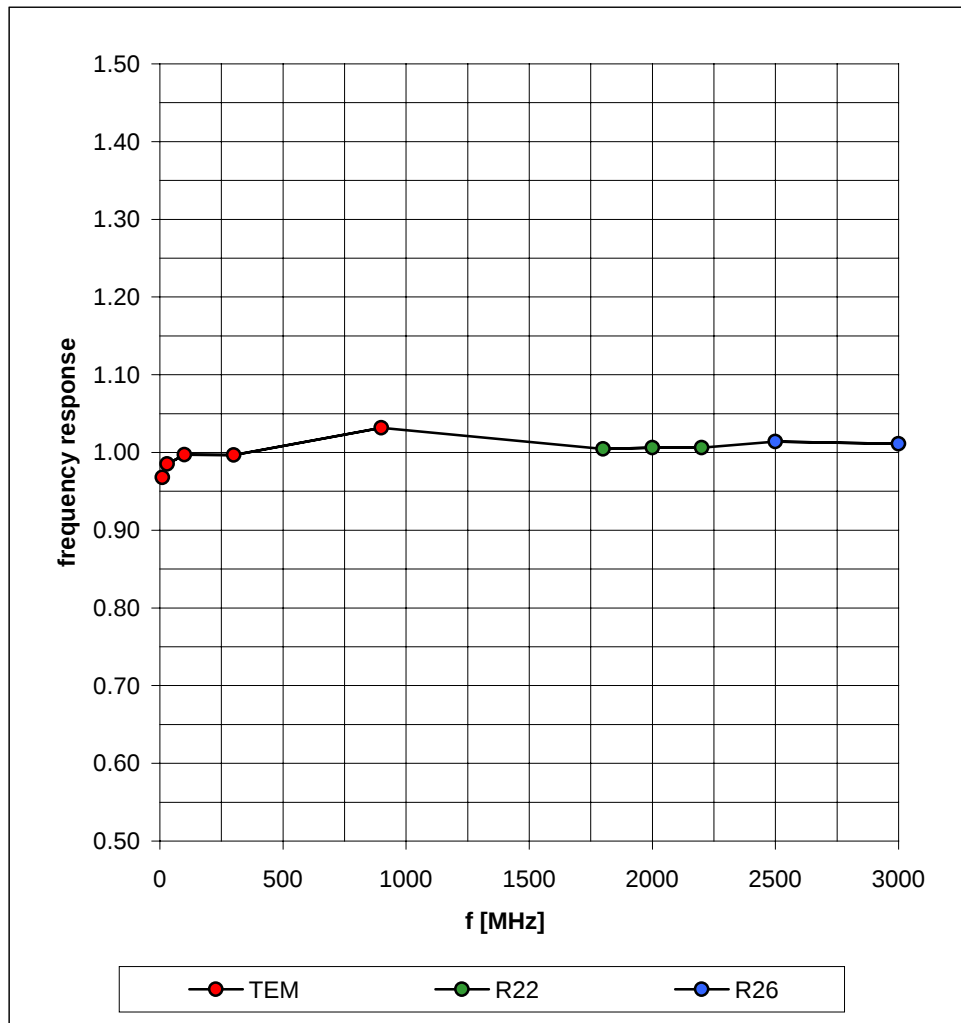


Dynamic Range f(SAR_{brain})
(TEM-Cell:ifi1110)

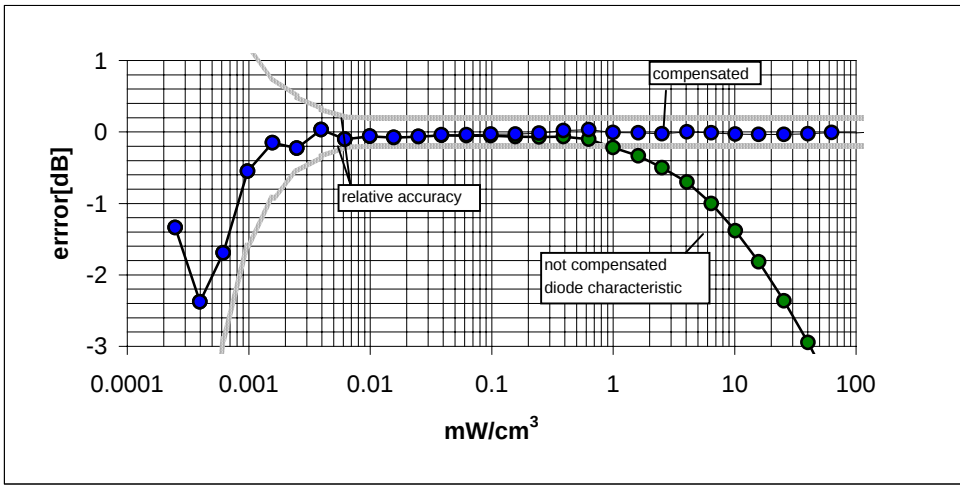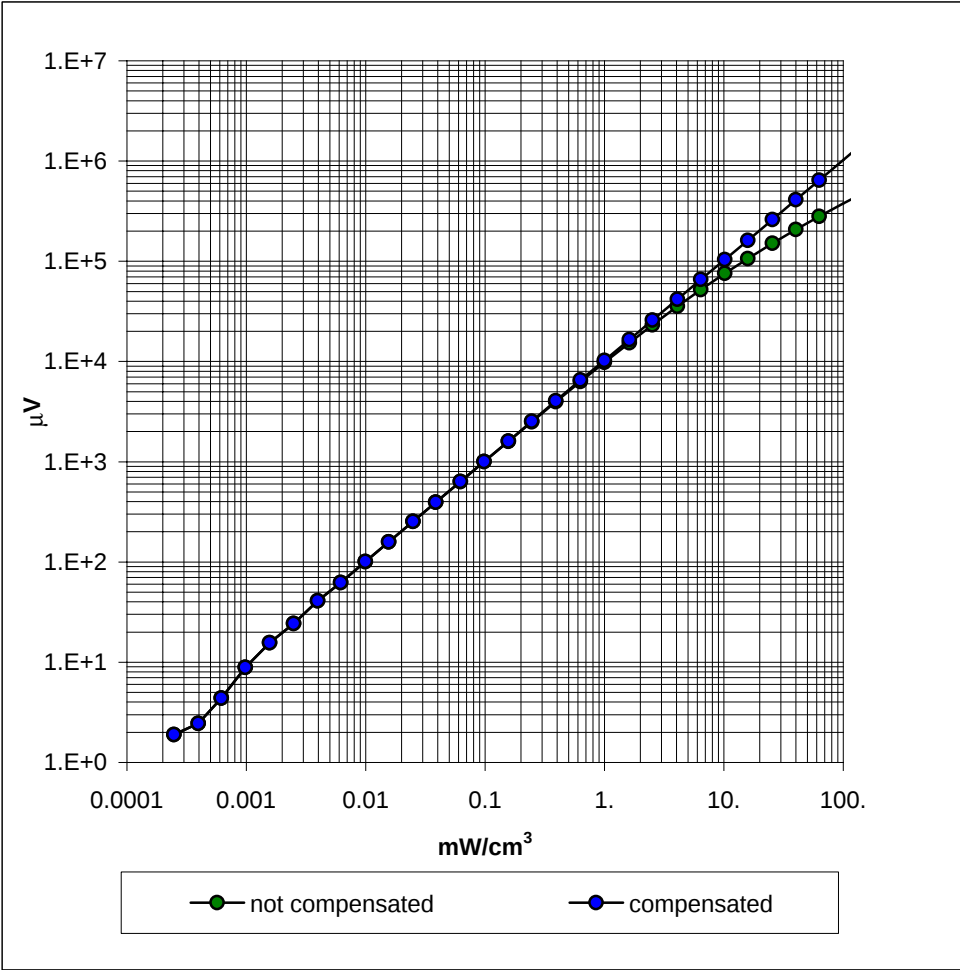

Conversion Factor Assessment

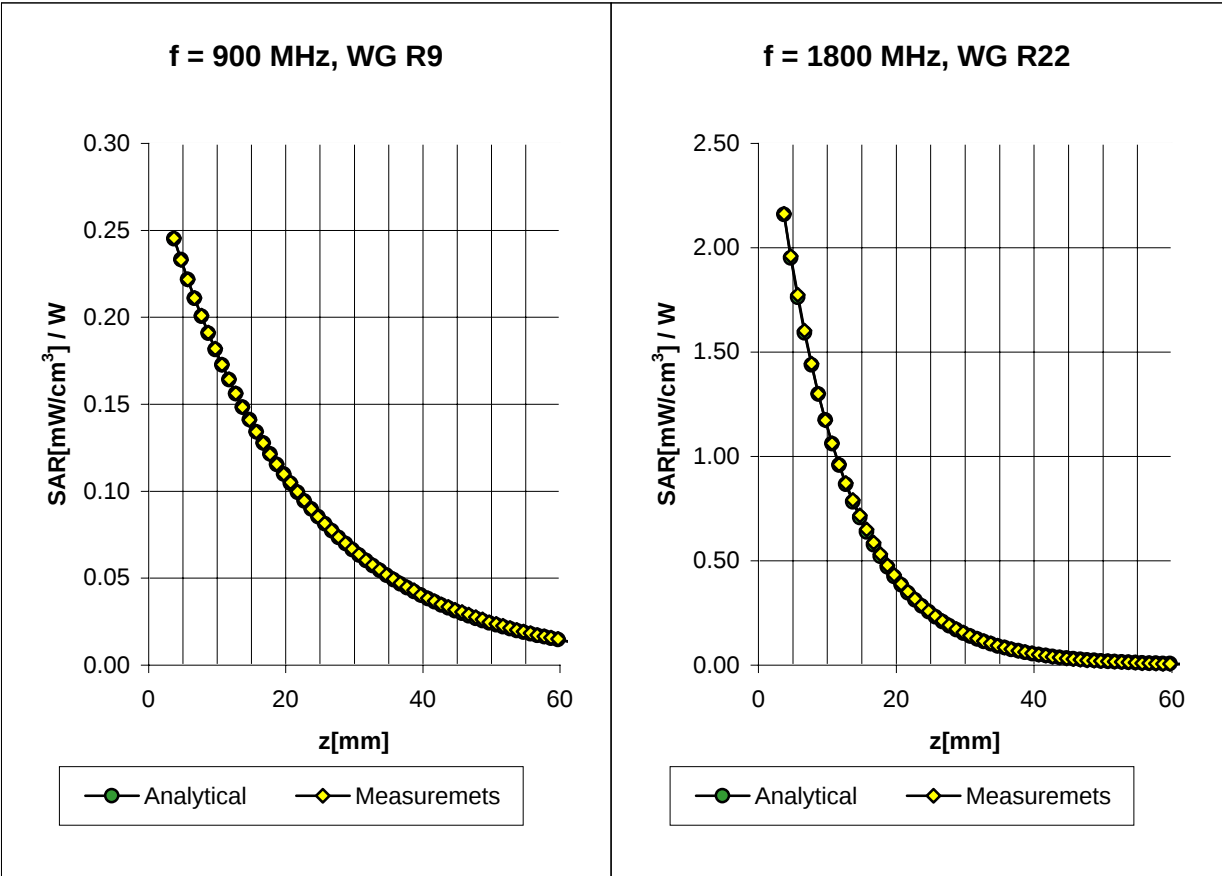

Receiving Pattern (ϕ) (in brain tissue, $z = 5 \text{ mm}$)

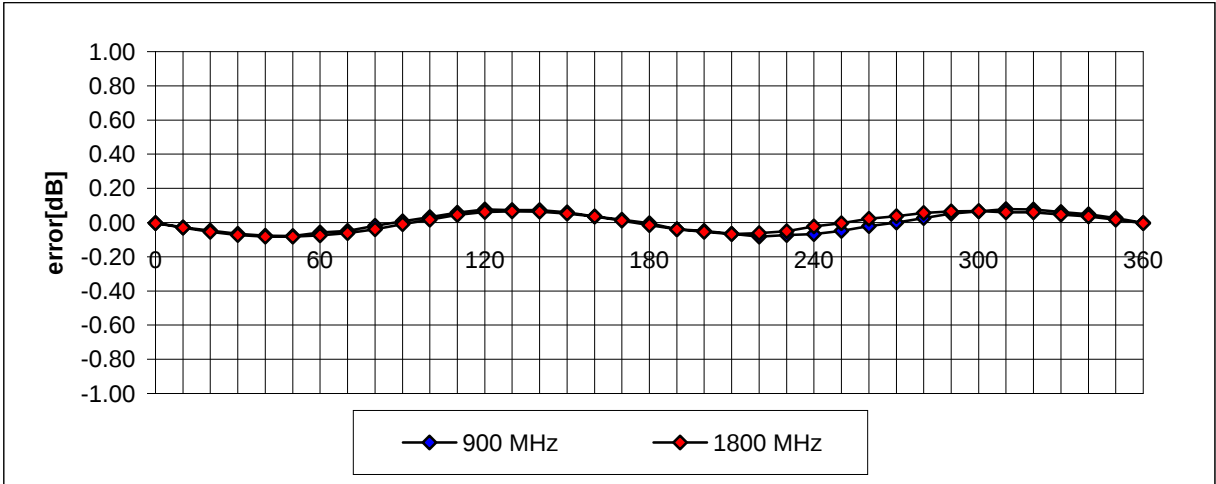

APPENDIX E – EUT EXTERNAL PHOTOGRAPHS











