





Plot 1.3.13
Spurious emissions



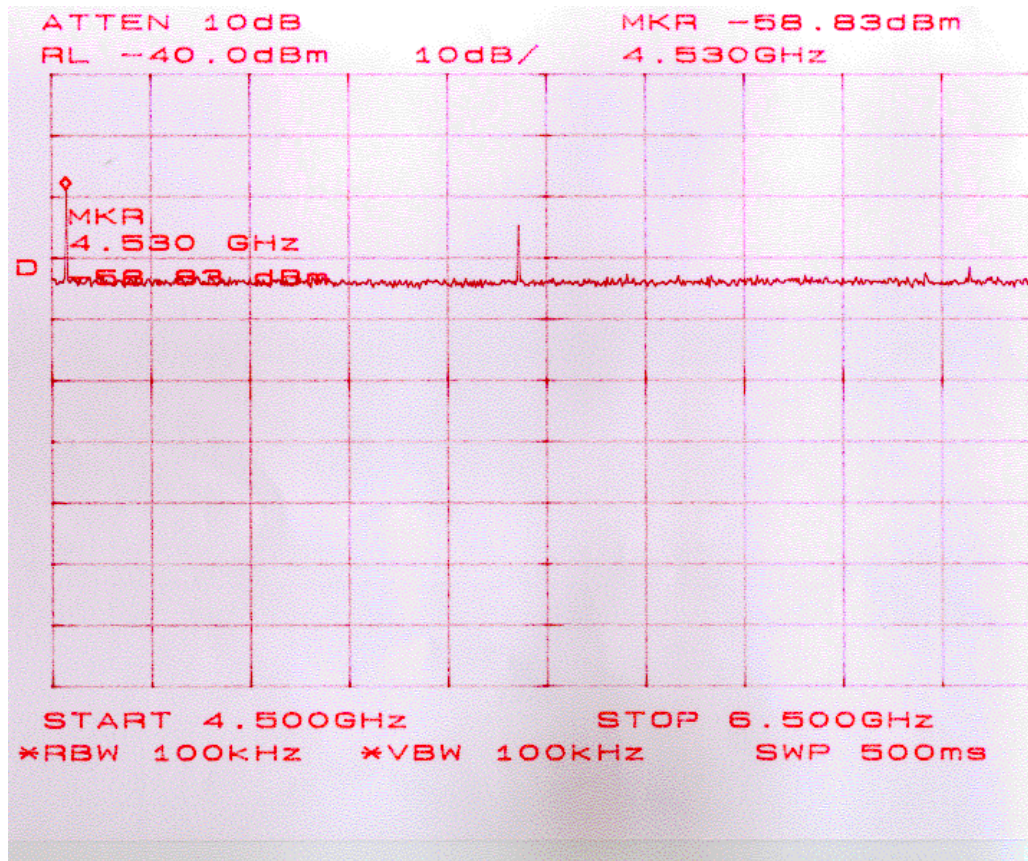


Plot 1.3.14
Spurious emissions

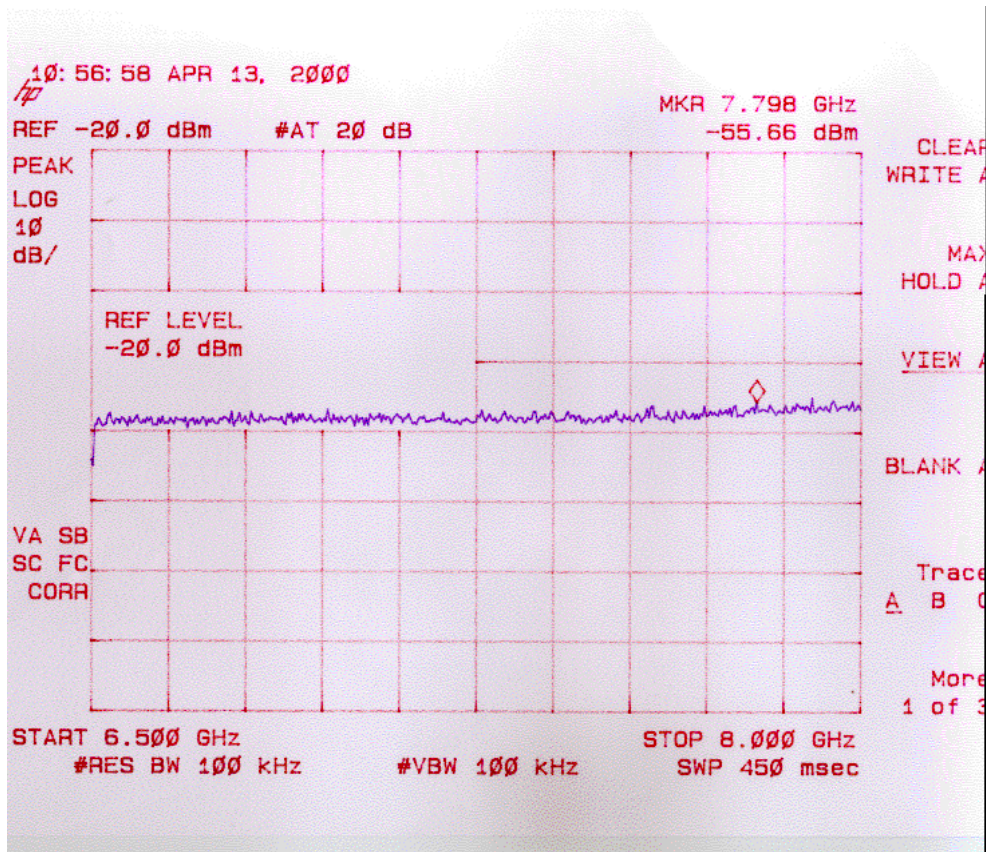



Plot 1.3.15
Spurious emissions

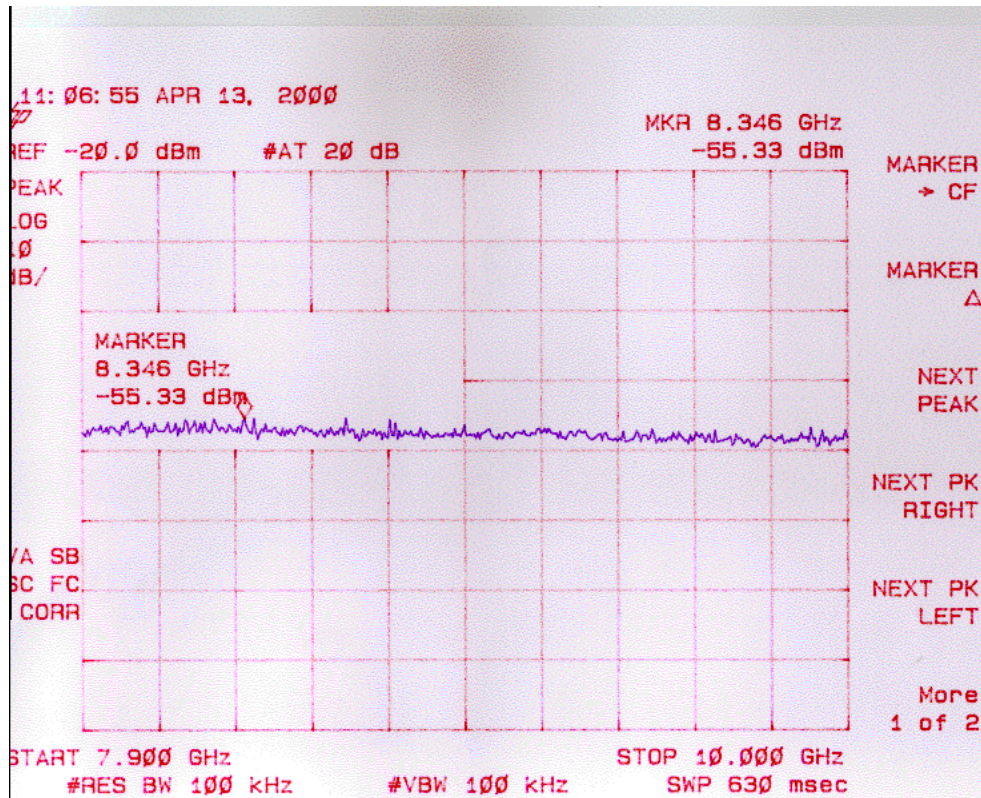



APPENDIX A - Test equipment and ancillaries used for tests

HL Serial No.	Serial No.	Description	Manufacturer	Model No.	Due Calibr.
0025	5837	Spectrum Analyzer, 10 kHz-23 GHz	Anritsu	MS-710C	8/00
0053	7538	Attenuator, 50 Ohm, 2W, 0-18 GHz, 10 dB	Hewlett Packard	8492A	2/00
0056	2627	Attenuator, 50 Ohm, 2W, 0-18 GHz, 30 dB	Hewlett Packard	8492A	2/00
0507	2926U 00162	Spectrum analyzer, 9 kHz - 1.8 GHz	Hewlett Packard	HP 8591A	5/00
0872	8767	Cable coax	Amplifier Research	PFP01P0103 94	7/00