

FCC TEST REPORT FCC 47 CFR Part 95I Medical Device Radiocommunication Service (MedRadio) Industry Canada RSS-243 Medical Devices Operating in the 401 – 406 MHz Frequency Band	
Report Reference No.	G0M-1412-4360-TFC95IMR-V02
Testing Laboratory	Eurofins Product Service GmbH
Address	Storkower Str. 38c 15526 Reichenwalde Germany
Accreditation	  A2LA Accredited Testing Laboratory, Certificate No.: 1983.01 FCC Filed Test Laboratory, Reg.-No.: 96970 IC OATS Filing assigned code: 3470A
Applicant's name	Biotronik SE & Co. KG
Address	Woermannkehre 1 12359 Berlin GERMANY
Test specification:	
Standard	47 CFR Part 95E 47 CFR Part 95I 47 CFR Part 15C RSS-243, Issue 3, 2010-02 RSS-Gen, Issue 4, 2014-11 ANSI C63.4:2009 EN 301 839-1 V1.3.1:2009-10
Equipment under test (EUT):	
Product description	ICD / Implantable Cardioverter Defibrillator
Model No.	Inlexa 1 HF-T
Additional Model(s)	Inlexa 1 DR-T (SN: 60508939) Inlexa 1 VR-T (SN: 60508940)
Brand Name(s)	Inlexa 1
Hardware version	Rev.: 01
Firmware / Software version	ROM: 4.1 / RAM: 3.0
	FCC-ID: QRITACHBORAX IC: 4708A-TACHBORAX
Test result	Passed

Possible test case verdicts:

- neither assessed nor tested: N/N
- required by standard but not appl. to test object.....: N/A
- required by standard but not tested.....: N/T
- not required by standard for the test object: N/R
- test object does meet the requirement.....: P (Pass)
- test object does not meet the requirement.....: F (Fail)

Testing:

Test Lab Temperature.....: 20 – 23 °C

Test Lab Humidity: 32 – 38 %

Date of receipt of test item: 2015-01-26

Date (s) of performance of tests: 2015-01-26 – 2015-01-28

Compiled by: Wilfried Treffke

Tested by (+ signature).....: Wilfried Treffke
(Responsible for Test) *W. Treffke*

Approved by (+ signature): Christian Weber *C. Weber*

Date of issue: 2016-02-12

Total number of pages: 76

General remarks:

The test results presented in this report relate only to the object tested.

The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.

This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.

Additional comments :

All devices feature the two RF-Telemetry functions Home Monitoring and wireless Wand.

RF-Telemetry functions are using the MICS-Band (402MHz – 405MHz).

A „-T“ inside the name of the device represents a device containing RF-Telemetry.

HF-T are triple-chamber devices.

DR-T are dual-chamber devices.

VR-T are single chamber devices without additional atrial detection.

All variants are available with DF-1.

All of these differences are only relevant in terms of medical aspects. They do not interfere the RF performance.

Evaluation measurements were performed for worst case antenna selection and the Inlexa 1 HF-T was selected. The model Inlexa 1 HF-T, as the most complex model, was selected for the measurements.

Tach_Borax Family Explanation (G0M-1412-4360)

1. Family Letter


	Product Name	Type	no. of chambers	Connector	max.stored energy	SN
1	Inlexa 1 HF-T	CRT	3	DF-1	40J	60508938 (Master)
2	Inlexa 1 DR-T	DR	2	DF-1	40J	60508939
3	Inlexa 1 VR-T	VR	1	DF-1	40J	60508940

2. Family description

2.1 PC-Board

All family devices are using the same electronic. This means all active and all passive electrical components are the same.

PC Board (4190)
10pol feedthrough
Schematic file SCH-0160_01.pdf

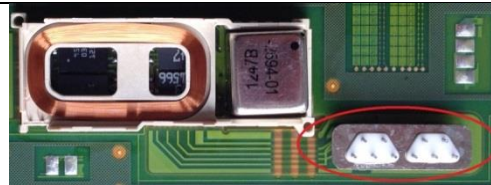

2.2 RF-Antenna

The family members are equipped with the identical RF antenna.

DF-1 header with antenna



Signature:

Date: 2/12/2016

Mark Briesemeister
Junior Manager Regulatory Affairs
BIOTRONIK SE & Co. KG
Woermannkehre 1
12359 Berlin
Germany

Version History

Version	Issue Date	Remarks	Revised by
01	2015-02-24	Initial Release	
02	2016-02-12	Certification numbers corrected	C. Weber

REPORT INDEX


1	EQUIPMENT (TEST ITEM) DESCRIPTION	7
1.1	Photos - Equipment external	9
1.2	Photos - Equipment internal	12
1.3	Photos – Test setup	14
1.4	Supporting Equipment Used During Testing	15
1.5	Test Modes	16
1.6	Test Equipment Used During Testing	17
1.7	Sample emission level calculation	18
1.8	Simulated human body	19
2	RESULT SUMMARY	20
3	TEST CONDITIONS AND RESULTS	21
3.1	Test Conditions and Results – Occupied Bandwidth	21
3.2	Test Conditions and Results – Emission Bandwidth	25
3.3	Test Conditions and Results – Frequency stability	29
3.4	Test Conditions and Results – Transmitter output power	31
3.5	Test Conditions and Results – Band-edge compliance	33
3.6	Test Conditions and Results – Transmitter unwanted emissions	35
3.7	Test Conditions and Results – Receiver spurious emissions	37
ANNEX A	Transmitter radiated power	39
ANNEX B	Transmitter radiated spurious emissions	47
ANNEX C	Receiver radiated spurious emissions	71

1 Equipment (Test item) Description

Description	ICD / Implantable Cardioverter Defibrillator	
Model	Inlexa 1 HF-T	
Additional Model(s)	Inlexa 1 DR-T (SN: 60508939) Inlexa 1 VR-T (SN: 60508940)	
Brand Name(s)	Inlexa 1	
Serial number	60508938	
Hardware version	Rev.: 01	
Software / Firmware version	ROM: 4.1 / RAM: 3.0	
FCC-ID	QRITACHBORAX	
IC	4708A-TACHBORAX	
Equipment type	End product	
Radio type	Transceiver	
Number of Radios	1	
Radio technology	MedRadio (MICS) active medical implant	
Operating frequency range	402.45 - 404.85 MHz	
Assigned frequency band	402 - 405 MHz	
Main test frequencies	F _{LOW}	402.45 MHz
	F _{MID}	403.65 MHz
	F _{HIGH}	404.85 MHz
Modulations	2FSK	
Emission designator	F1D	
Number of channels	9	
Channel spacing	300 kHz	
Spectrum access	LBT/AFA (channel access controlled by ULP-AMI-P device outside the human body)	
Number of antennas	2	
Antenna 1	Type	integrated
	Model	loop antenna Inlexa 1
	Manufacturer	see Manufacturer
	Gain	-29.1 dBi (Determined by measurements)
Manufacturer	Biotronik SE & Co. KG Woermannkehre 1 12359 Berlin GERMANY	


Power supply	V _{NOM}	3.0 VDC
	V _{MIN}	2.5 VDC
	V _{MAX}	3.2 VDC
Temperature	T _{NOM}	37 °C
	T _{MIN}	25 °C
	T _{MAX}	45 °C
AC/DC-Adaptor	Model	N/A
	Vendor	N/A
	Input	N/A
	Output	N/A

1.1 Photos - Equipment external

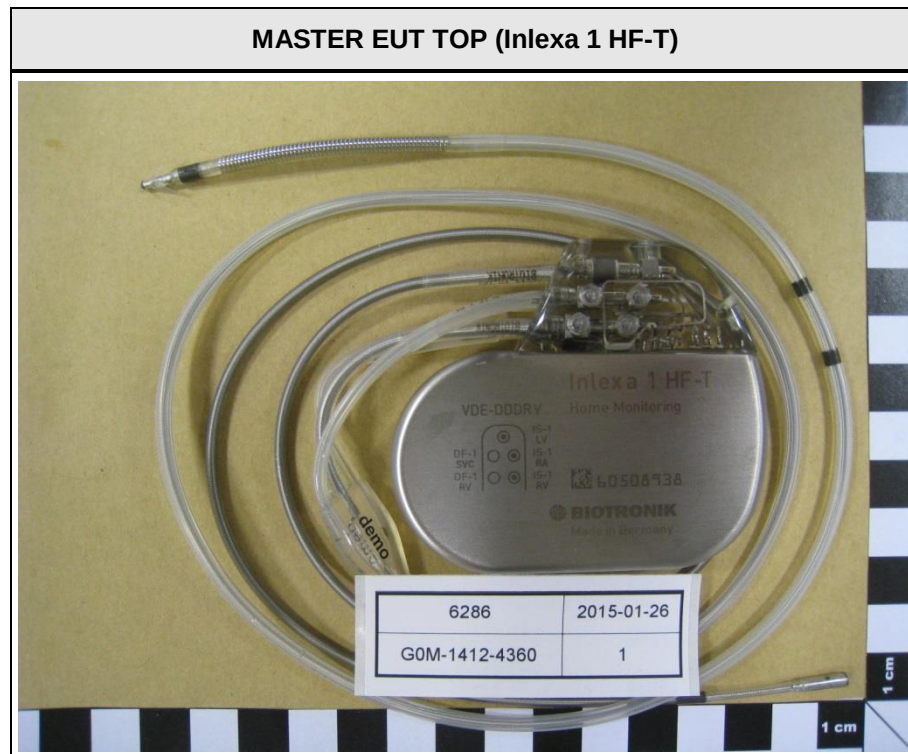

Test Report No.: G0M-1412-4360-TFC95IMR-V02



Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

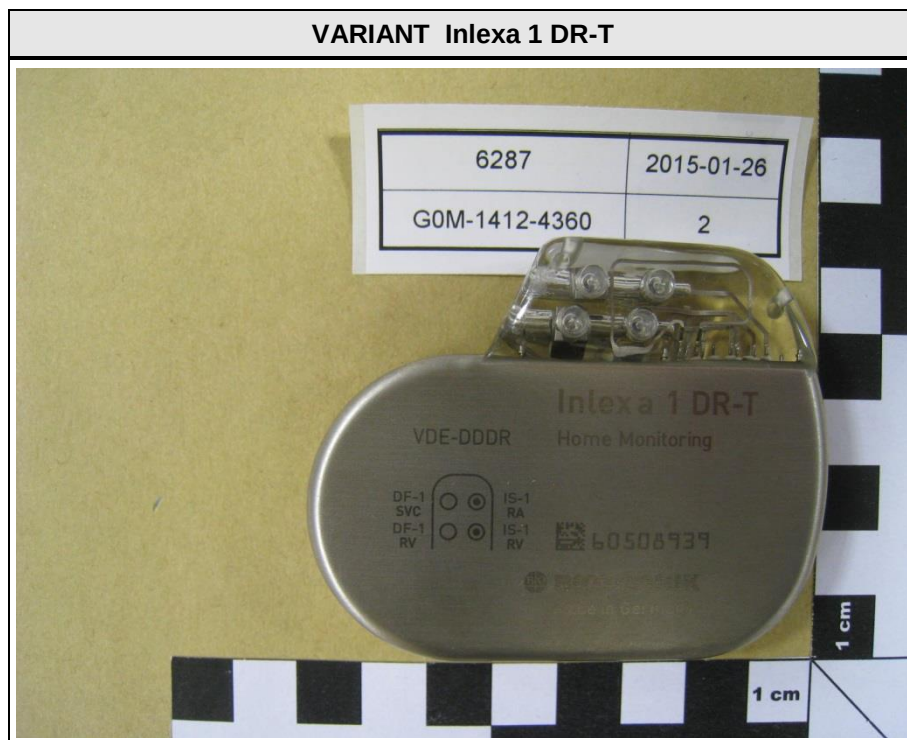


AE WIRELESS WAND TelBoxII





1.2 Photos - Equipment internal

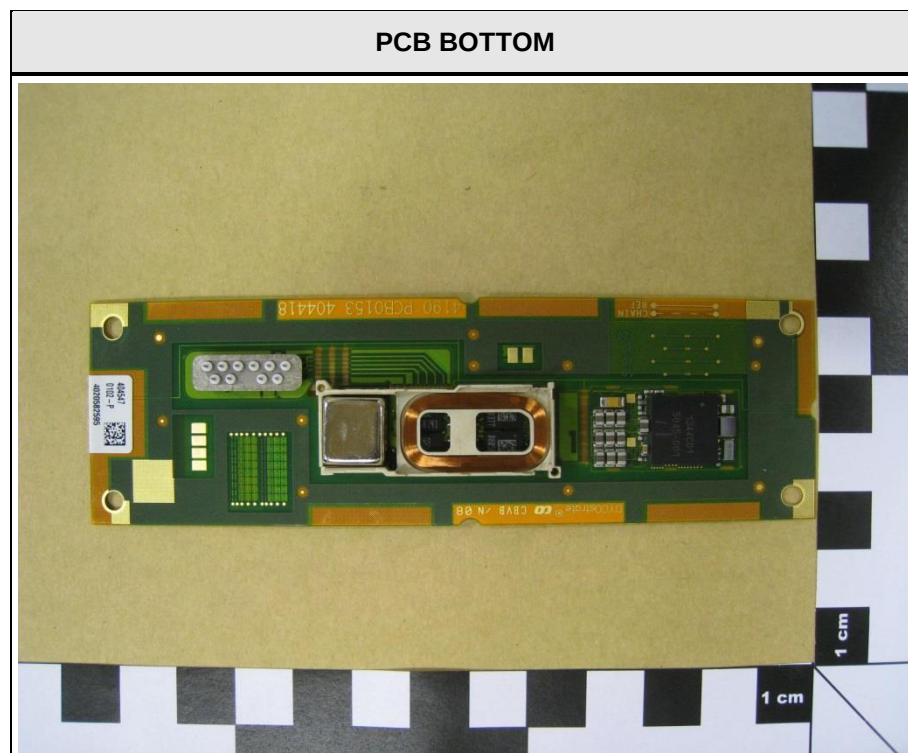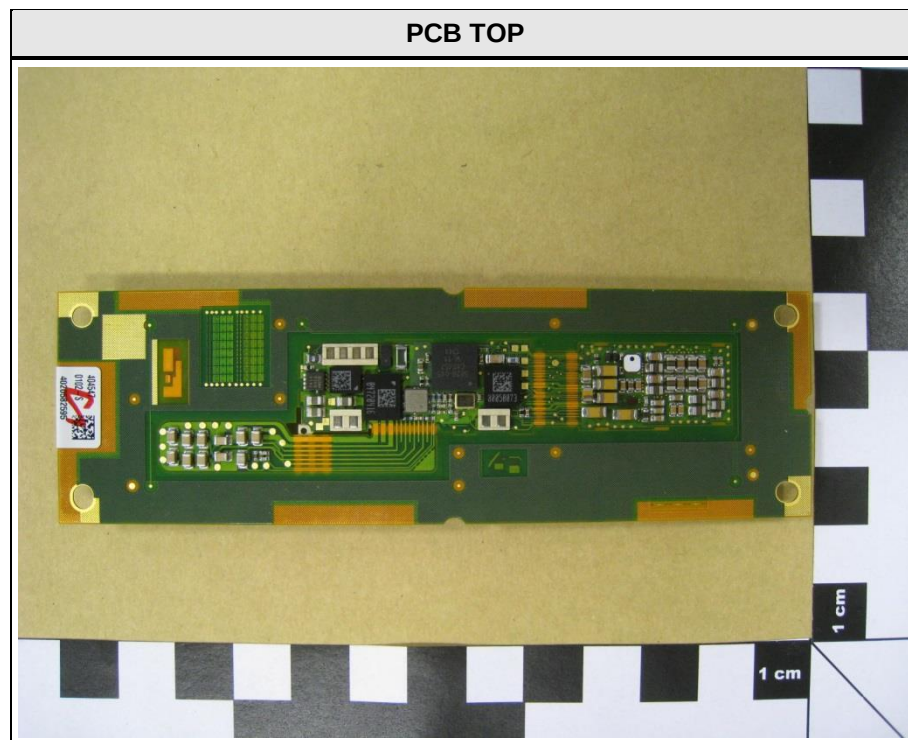

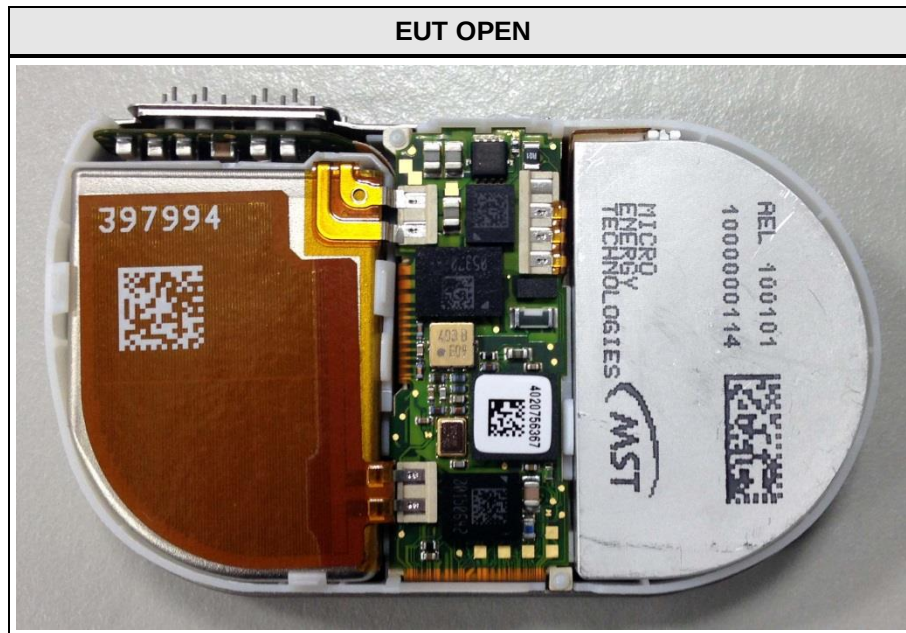

1.3 Photos – Test setup

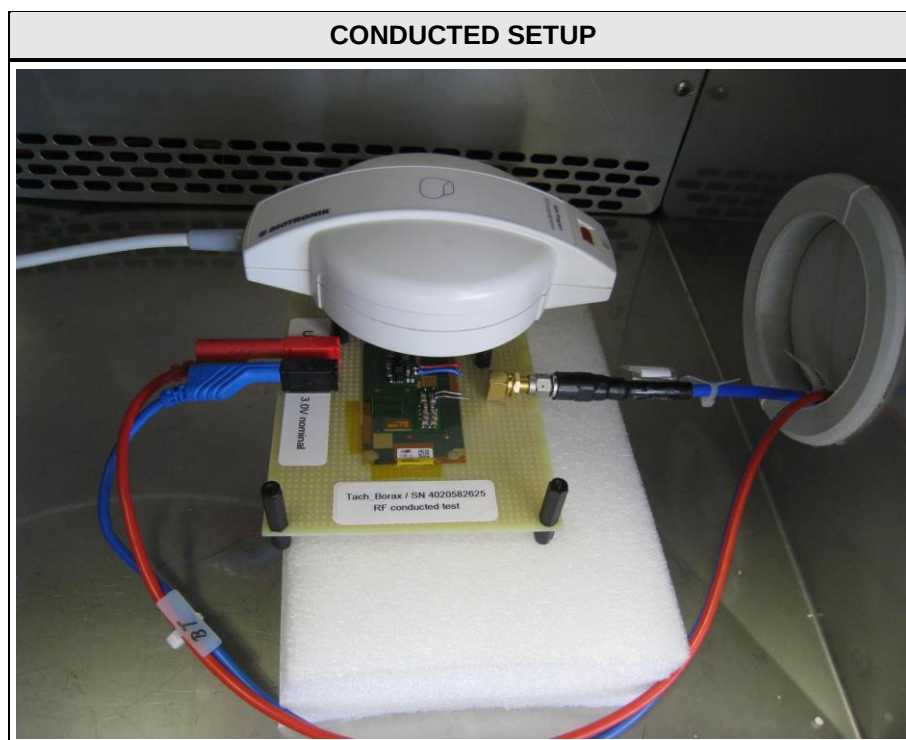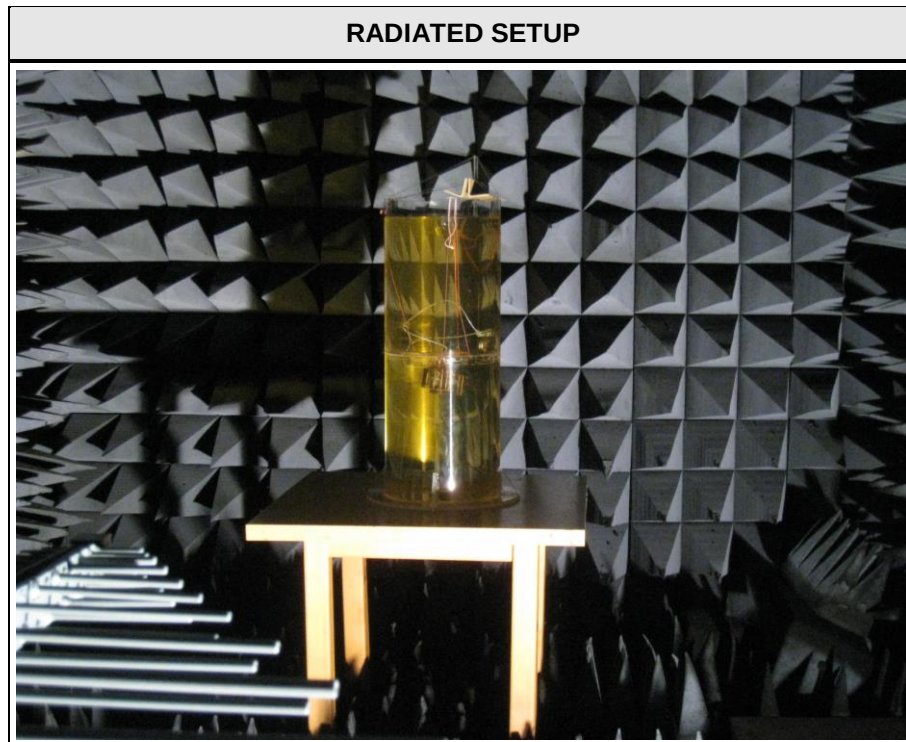

1.4 Supporting Equipment Used During Testing

Product Type*	Device	Manufacturer	Model No.	Comments
AE	Enginnering communication box	BIOTRONIK	TelBoxII	for test mode
AE	Electrode	Biotronik	Lincox Smart	-

***Note:** Use the following abbreviations:

AE : Auxiliary/Associated Equipment, or

SIM : Simulator (Not Subjected to Test)

CABL : Connecting cables

1.5 Test Modes

Mode #	Description	
Unmodulated	General conditions:	EUT powered on.
	Radio conditions:	Mode = standalone transmit Spreading = None Modulation = None Duty cycle = 100 % Power level = Maximum
Modulated	General conditions:	EUT powered on.
	Radio conditions:	Mode = standalone transmit Modulation = 2FSK Duty cycle = 100 % Power level = Maximum
Receive	General conditions:	EUT powered on.
	Radio conditions:	Mode = standalone receive Modulation = 2FSK

1.6 Test Equipment Used During Testing

Measurement Software			
Description	Manufacturer	Name	Version
EMC Test Software	Dare Instruments	Radimation	2014.1.15

Occupied Bandwidth					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSIQ26	EF00242	2014-03	2015-03

Emission Bandwidth					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSIQ26	EF00242	2014-03	2015-03

Frequency Stability					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSIQ26	EF00242	2014-03	2015-03

Effective radiated power					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Fully-anechoic chamber	Frankonia	AC 4	EF00200	-	-
Spectrum Analyzer	R&S	FSEK30	EF00168	2015-01	2016-01
LPD Antenna	R&S	HL 223	EF00212	2013-02	2016-02

Radiated spurious emissions					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Semi-anechoic chamber	Frankonia	AC 5	EF00395	-	-
Spectrum Analyzer	R&S	FSIQ26	EF00242	2014-03	2015-03
Biconical Antenna	R&S	HK 116	EF00012	2013-02	2016-02
LPD Antenna	R&S	HL 223	EF00212	2013-02	2016-02
LPD Antenna	R&S	HL 025	EF00327	2013-02	2016-02

Discontinuation of MICS session					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSIQ26	EF00242	2014-03	2015-03
Signal Generator	R&S	SMP 02	EF00165	2013-05	2015-05

1.7 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyzer in dBμV. Any external preamplifiers used are taken into account through internal analyzer settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyzer. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyzer (dB}\mu\text{V)} + \text{A.F. (dB)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dBμV/m). The FCC limits are given in units of μV/m. The following formula is used to convert the units of μV/m to dBμV/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 \cdot \log (\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

$$\begin{array}{rclcl} \text{Reading} & + & \text{AF} & = & \text{Net Reading} & : & \text{Net reading - FCC limit} & = & \text{Margin} \\ 21.5 \text{ dB}\mu\text{V} & + & 26 \text{ dB} & = & 47.5 \text{ dB}\mu\text{V/m} & : & 47.5 \text{ dB}\mu\text{V/m} - 57.0 \text{ dB}\mu\text{V/m} & = & -9.5 \text{ dB} \end{array}$$

1.8 Simulated human body

For radiated tests the implant was placed in a simulated human body.

Liquid components	
Component	percentage per weight
Deionized water	52.4
Bactericide	0.08
Hydroxy ethyl cellulose (HCE)	1.0
Sodium chloride	1.4
Sucrose	45.0

Measured tissue parameters:

Tissue parameters – 403.5MHz			
Component	Target	Measured	Tolerance [%]
Dielectric constant ϵ	62.5	63.01	0.82
Conductivity σ [ms/cm]	9.0	8.9	-1.11

2 Result Summary

FCC 47 CFR Part 95E, 95I, 15C, IC RSS-243, IC RSS-Gen				
Product Specific Standard Section	Requirement – Test	Reference Method	Result	Remarks
IC RSS-243 3.2 IC RSS-Gen 6.6	Occupied bandwidth	RSS-Gen 6.6	N/A	Informational only
FCC 95.628(d) FCC § 95.633(e) IC RSS-243 3.6, 5.1	Emission bandwidth	FCC § 95.628(a)(6)(i) FCC § 95.633(e)(3)	PASS	
FCC 95.628(e) IC RSS-243 3.3, 5.3 RSS-Gen 6.11	Frequency stability	EN 301 839-1 8.1	PASS	
FCC § 95.6369(f) IC RSS-243 § 5.4	Transmitter output power	EN 301 839-1 8.3	PASS	
FCC § 95.635(d) IC RSS-243 § 3.4, 5.5	Band edge compliance	FCC § 95.635(d) ANSI C63.4	PASS	
FCC § 95.635(d) IC RSS-243 § 3.4, 5.5 RSS-Gen 6.13	Transmitter unwanted emissions	FCC § 95.635(d) ANSI C63.4	PASS	
IC RSS-243 3.5, 5.6 IC RSS-Gen 7.1	Receiver spurious emissions	ANSI C63.4	PASS	
FCC § 15.207 IC RSS-Gen 8.8	AC power line conducted emissions	ANSI C63.4	N/R	EUT battery powered
FCC § 95.628(a)(3) IC RSS-243 3.6, 5.7.1	System threshold power levels	EN 301 839-1 10.1	N/R	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(1) IC RSS-243 3.6, 5.7.2	Monitoring system bandwidth	EN 301 839-1 10.2	N/R	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(2) IC RSS-243 3.6, 5.7.3	Scan cycle time	EN 301 839-1 10.3	N/R	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(2) IC RSS-243 3.6, 5.7.4	Minimum channel monitoring period	EN 301 839-1 10.3	N/R	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(4) IC RSS-243 3.6, 5.7.5	Channel Access	EN 301 839-1 10.4	N/R	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(4) IC RSS-243 3.6, 5.7.6	Discontinuation of MICS or MEDS session	EN 301 839-1 10.5	N/R	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(5) IC RSS-243 3.6, 5.7.7	Use of the pre-scanned alternate channel	EN 301 839-1 10.6	N/R	Not used
Remarks:				

3 Test Conditions and Results

3.1 Test Conditions and Results – Occupied Bandwidth


Occupied Bandwidth acc. to IC RSS-243			Verdict: PASS
Test according to measurement reference	Reference Method		
	RSS-Gen 6.6		
Test frequency range	Tested frequencies		
	F _{LOW} / F _{MID} / F _{HIGH}		
EUT test mode	Modulated		
Limits			
None (Informational only)			
Test setup			
Spectrum Analyzer EUT			
Test procedure			
1. EUT set to test mode (Communication tester is used if needed) 2. Span set to at least twice the emission spectrum 3. Resolution bandwidth set to 1 % of span 4. Occupied Bandwidth (99 %) measurement with spectrum analyzer built in measurement function			
Test results			
Channel	Frequency [MHz]	Occupied Bandwidth [kHz]	
F _{LOW}	402.45	169.9	
F _{MID}	403.65	198.7	
F _{HIGH}	404.85	170.8	
Comments:			

Occupied Bandwidth – F_{Low}

Occupied Bandwidth acc. to RSS-Gen

Project Number: G0M-1412-4360

Applicant: Biotronik SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 402.45 MHz, 2FSK
 Test Date: 2015-01-28
 Verdict: PASS
 Note 1: A spectrum analyzer with an integrated 99% power bandwidth function is used

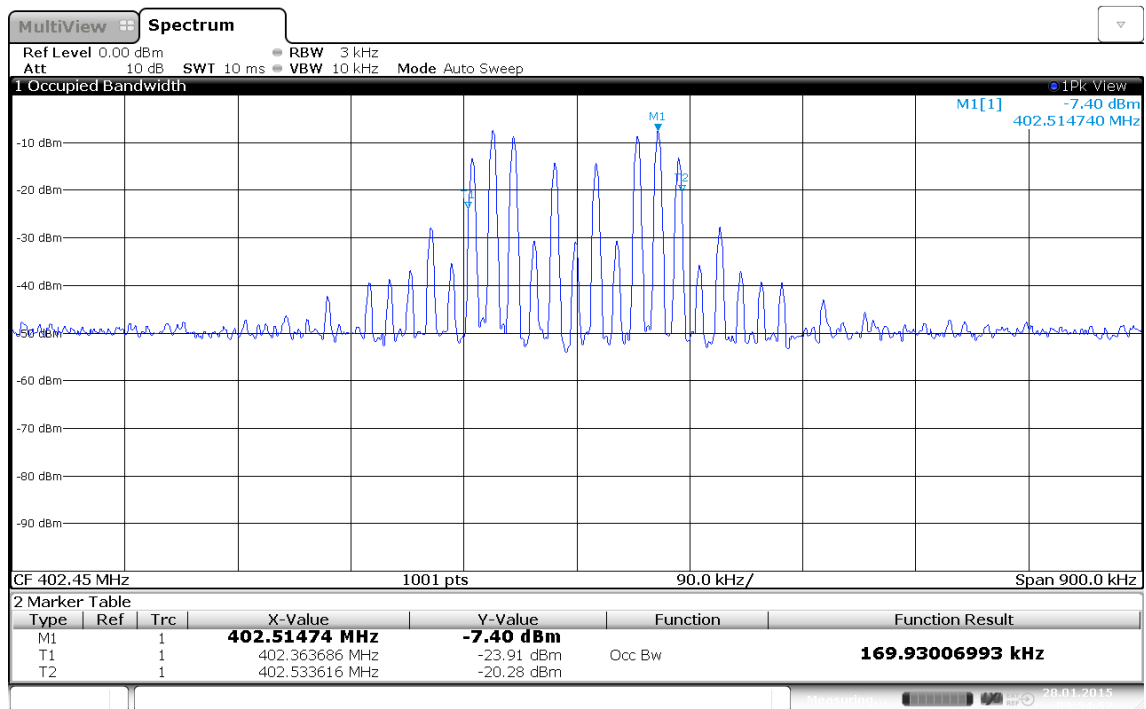

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Occupied Bandwidth - F_{MID}

Occupied Bandwidth acc. to RSS-Gen

Project Number: G0M-1412-4360

Applicant: Biotronik SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 403.65 MHz, 2FSK
 Test Date: 2015-01-28
 Verdict: PASS
 Note 1: A spectrum analyzer with an integrated 99% power bandwidth function is used

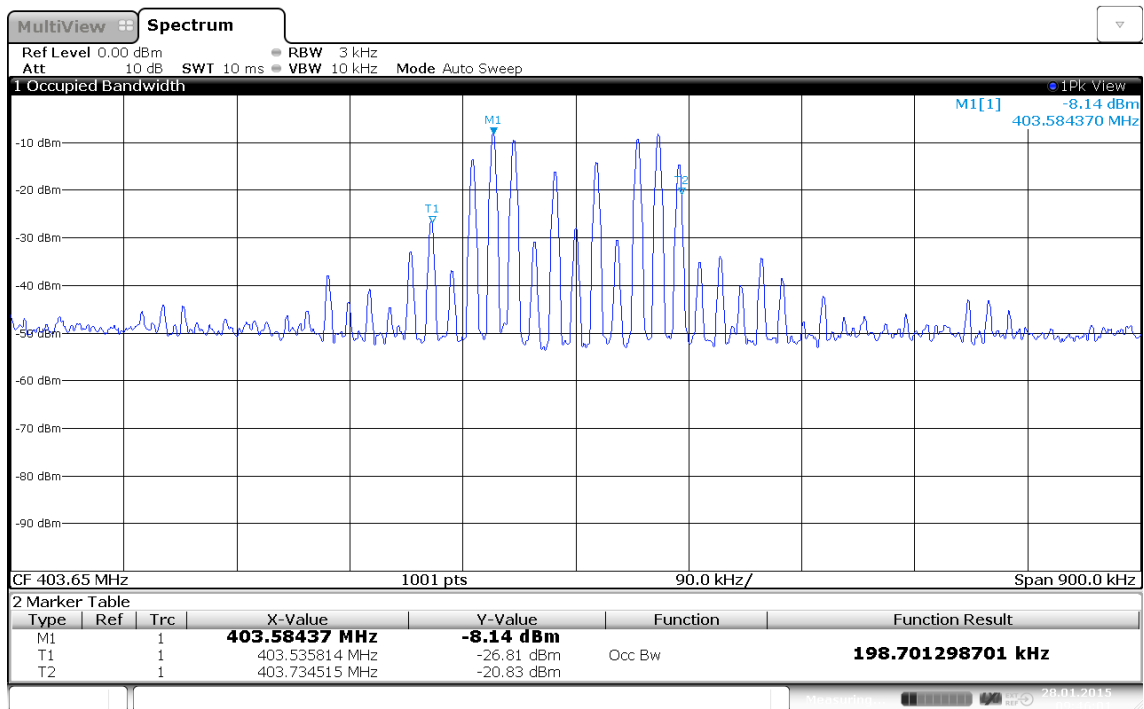

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Occupied Bandwidth - F_{HIGH}

Occupied Bandwidth acc. to RSS-Gen

Project Number: G0M-1412-4360

Applicant: Biotronik SE & Co.KG
EUT Name: ICD / Implantable Cardioverter Defibrillator
Model: Inlexa 1
Test Site: Eurofins Product Service GmbH
Operator: Wilfried Treffke
Test Conditions: Tnom / Vnom
Mode: Tx 404.85 MHz, 2FSK
Test Date: 2015-01-28
Verdict: PASS
Note 1: A spectrum analyzer with an integrated 99% power bandwidth function is used

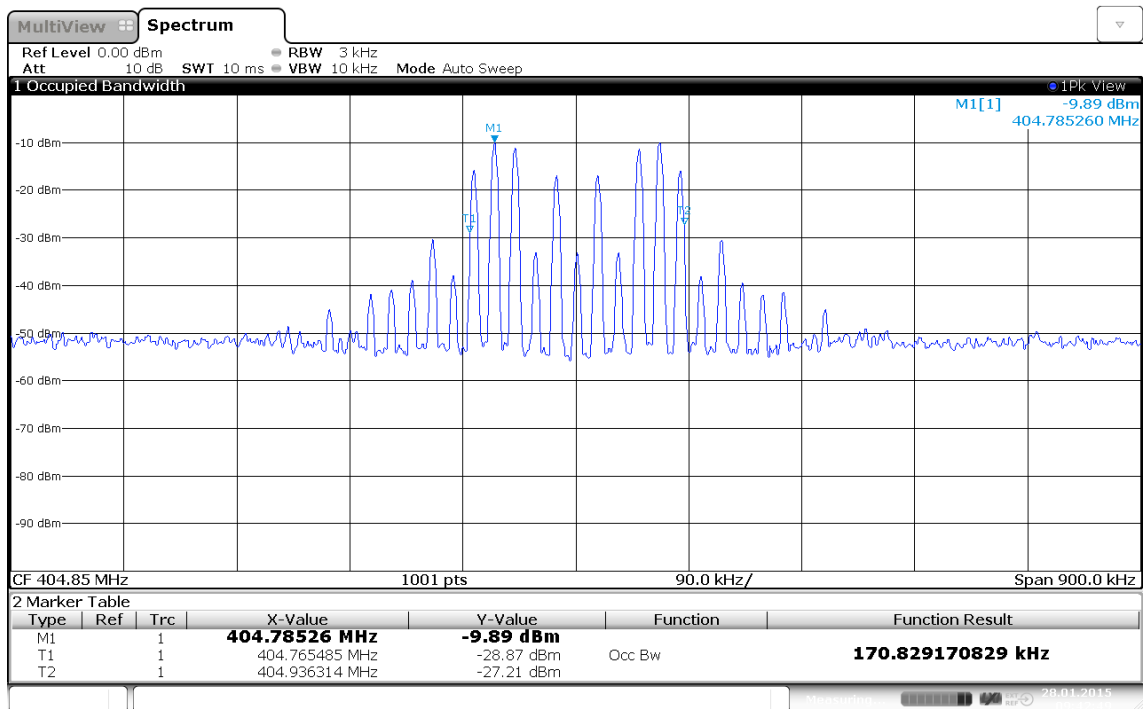

Test Report No.: G0M-1412-4360-TFC95IMR-V02

Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

3.2 Test Conditions and Results – Emission Bandwidth


Emission Bandwidth acc. to FCC Part 95 / IC RSS-243				Verdict: PASS
EUT requirement rule parts and clause	Reference			
	FCC 95.628(d) / FCC 95.633(e) / IC RSS-243 3.3 5.1			
Test according to measurement reference	Reference Method			
	FCC 95.628(a)(6)(i) / FCC 95.633(e)(3)			
Test frequency range	Tested frequencies			
	F _{LOW} / F _{MID} / F _{HIGH}			
EUT test mode	Modulated			
Limits				
≤ 300 kHz				
Test setup				
Spectrum Analyzer EUT				
Test procedure				
1. EUT set to test mode 2. Span set to at least twice the emission spectrum 3. Detector set to peak and max hold 4. Envelope peak value of emission spectrum is selected 5. Marker on envelope of spectrum is set to level of -20 dB to the left of the peak 6. Marker on envelope of spectrum is set to level of -20 dB to the right of the peak 7. 20 dB Emission Bandwidth is determined by marker frequency separation				
Test results				
Channel	Frequency [MHz]	Emission Bandwidth [kHz]	Limit [kHz]	Result
F _{LOW}	402.45	229.5	≤ 300	PASS
F _{MID}	403.65	231.4	≤ 300	PASS
F _{HIGH}	404.85	230.4	≤ 300	PASS
Comments:				

Emission Bandwidth – F_{Low}

Emission Bandwidth acc. to FCC Part 95.633

Project Number: G0M-1412-4360

Applicant: Biotronik SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 402.45 MHz, 2FSK
 Test Date: 2015-01-28
 Verdict: PASS
 Note 1: 20 dB bandwidth

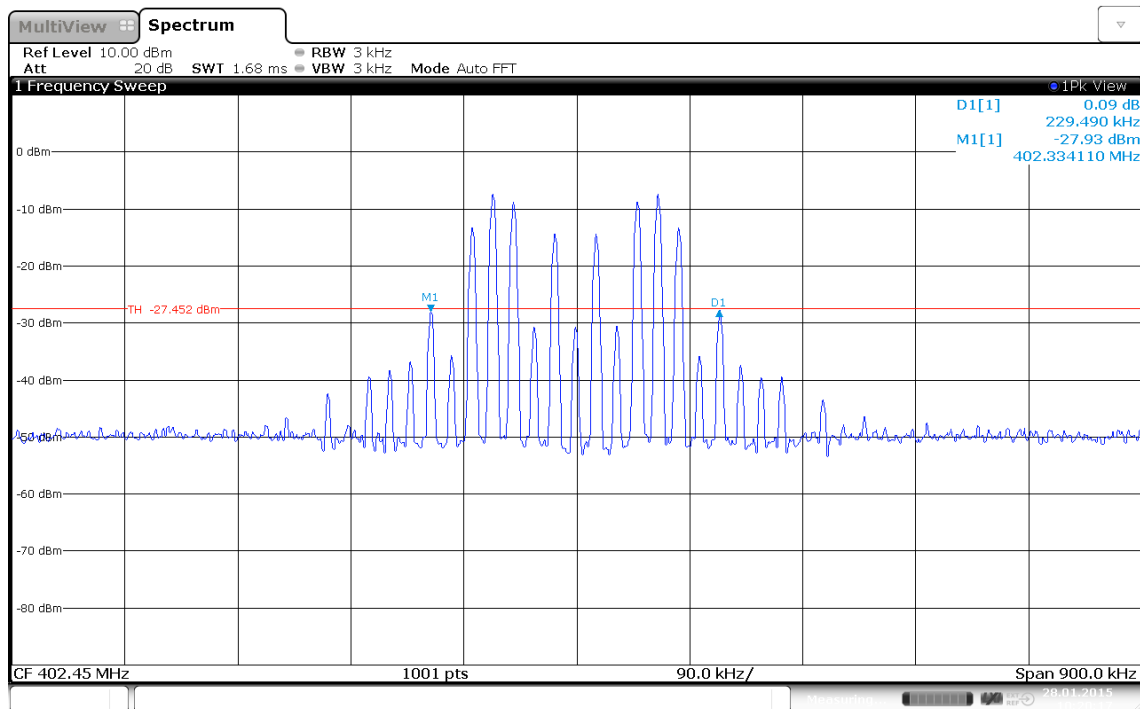


Emission Bandwidth – F_{MID}

Emission Bandwidth acc. to FCC Part 95.633

Project Number: G0M-1412-4360

Applicant: Biotronik SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 403.65 MHz, 2FSK
 Test Date: 2015-01-28
 Verdict: PASS
 Note 1: 20 dB bandwidth

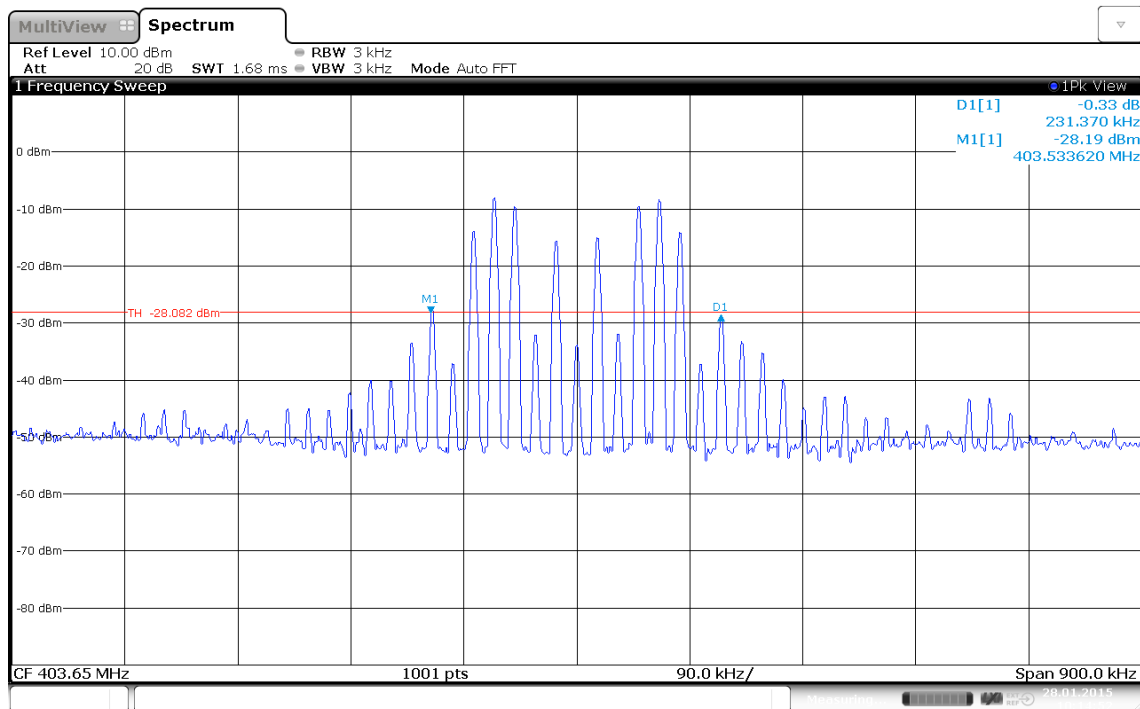

Date: 28.JAN.2015 10:14:52


Test Report No.: G0M-1412-4360-TFC95IMR-V02

Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Emission Bandwidth – F_{HIGH}
Emission Bandwidth acc. to FCC Part 95.633

Project Number: G0M-1412-4360

Applicant: Biotronik SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 404.85 MHz, 2FSK
 Test Date: 2015-01-28
 Verdict: PASS
 Note 1: 20 dB bandwidth

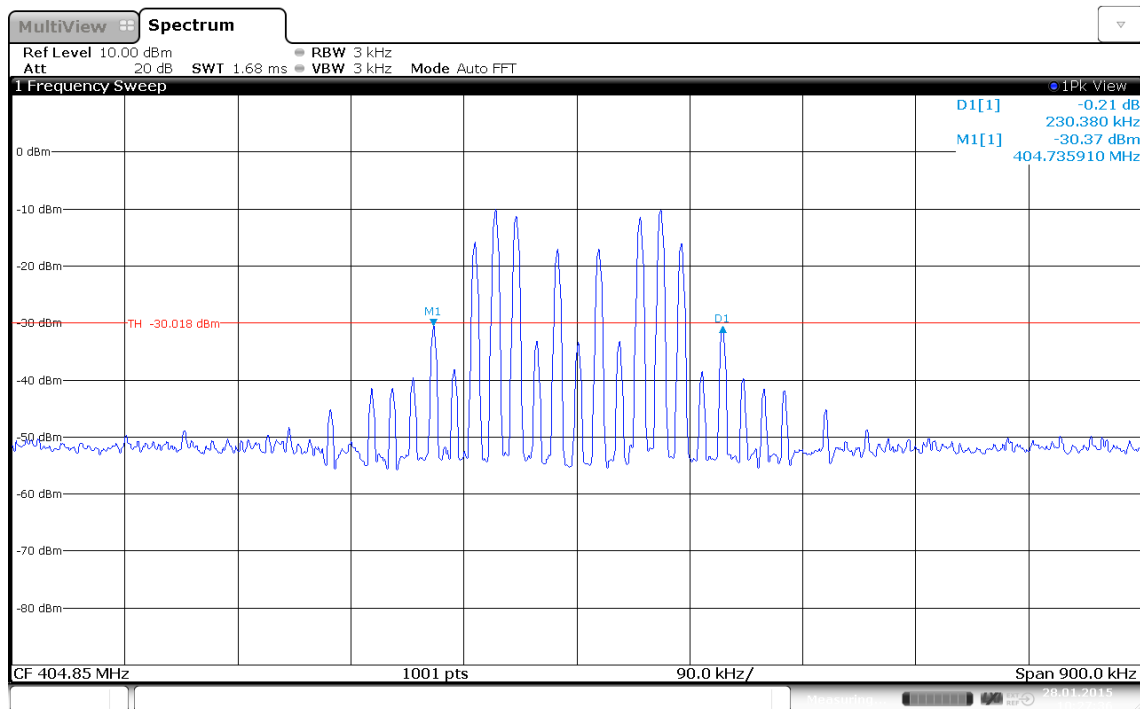


3.3 Test Conditions and Results – Frequency stability

Frequency stability acc. FCC Part 95 / IC RSS-243		Verdict: PASS
EUT requirement rule parts and clause	Reference	
	FCC 95.628(e) / IC RSS-243 3.3 5.3 / RSS-Gen 6.11	
Test according to measurement reference	Reference Method	
	EN 301 839-1 8.1	
Test frequency range	Tested frequencies	
	F _{LOW} / F _{MID} / F _{HIGH}	
EUT test mode	Unmodulated	
Limits		
≤ ±100 ppm		
Test setup		
Power Spectrum Analyzer Rubidium Reference EUT (Test fixture) Climatic Chamber		
Test procedure		
1. EUT set to test mode with supply voltage and temperature set to nominal conditions 2. EUT transmits without modulation 3. Detector set to peak and max hold 4. Peak of emission is measured using a frequency counter 5. The frequency error is determined as the deviation of the emission frequency from the nominal frequency stated by the customer.		


Test results					
Channel	Nominal Frequency [MHz]	Temperature	Supply voltage	Frequency [MHz]	Drift [ppm]
F _{LOW}	402.45	T _{NOM} = 37 °C	V _{NOM} = 3.0 VDC	402.448814	-2.95
F _{LOW}	402.45	T _{MIN} = 25 °C	V _{NOM} = 3.0 VDC	402.448621	-3.43
F _{LOW}	402.45	T _{MAX} = 45 °C	V _{NOM} = 3.0 VDC	402.448849	-2.86
F _{MID}	403.65	T _{NOM} = 37 °C	V _{NOM} = 3.0 VDC	403.649927	-0.18
F _{MID}	403.65	T _{MIN} = 25 °C	V _{NOM} = 3.0 VDC	403.649635	-0.90
F _{MID}	403.65	T _{MAX} = 45 °C	V _{NOM} = 3.0 VDC	403.649874	-0.31
F _{HIGH}	404.85	T _{NOM} = 37 °C	V _{NOM} = 3.0 VDC	404.850865	2.14
F _{HIGH}	404.85	T _{MIN} = 25 °C	V _{NOM} = 3.0 VDC	404.850714	1.76
F _{HIGH}	404.85	T _{MAX} = 45 °C	V _{NOM} = 3.0 VDC	404.850941	2.32
Comments:					

3.4 Test Conditions and Results – Transmitter output power

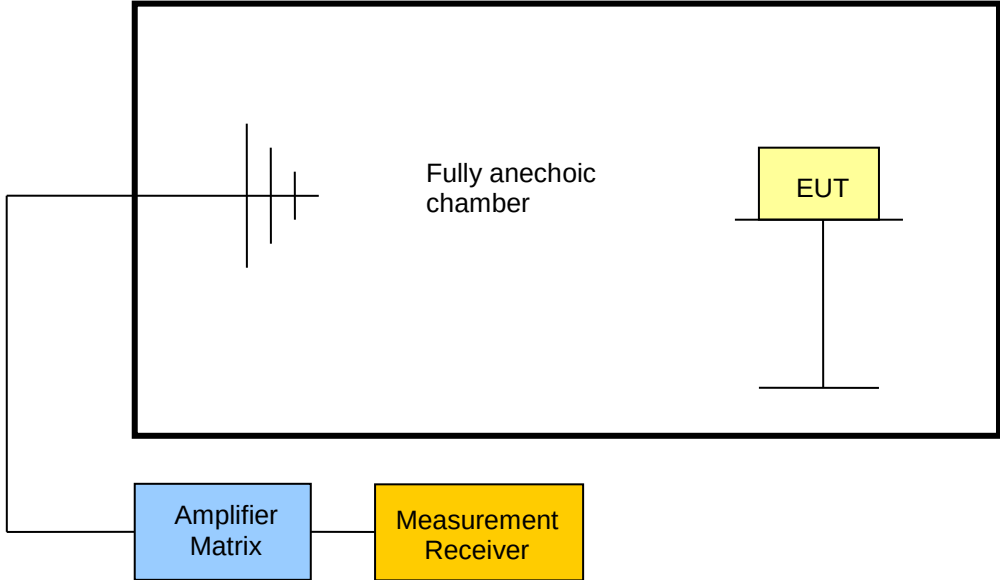Transmitter output power acc. to FCC Part 95 / IC RSS-243		Verdict: PASS
EUT requirement rule parts and clause	Reference	
	FCC 95.639(f) / IC RSS-243 5.4	
Test according to measurement reference	Reference Method	
	EN 301 839-1 8.3	
Test frequency range	Tested frequencies	
	F _{LOW} / F _{HIGH}	
EUT test mode	Modulated	
Limits		
≤ 25 μW (-16 dBm) e.i.r.p.		
Test setup		
		
Test procedure		
1. EUT set to test frequency with modulation 2. Measurement polarization is set to vertical 3. Span it set according to measurement range and detector is set to peak and max hold 4. Resolution bandwidth is set two be at least twice the emission bandwidth 5. During the sweep the EUT is rotated to obtain maximum emission level 6. Measurement is repeated with horizontal measurement polarization		


Test results					
Channel	Frequency [MHz]	Emission Level [dbm e.i.r.p.]	Detector	Limit [dbm e.i.r.p.]	Margin [dB]
F _{LOW}	402.45	-31.6	pk	-16	-15.60
F _{HIGH}	404.85	-33.7	pk	-16	-17.70
Comments:					

3.5 Test Conditions and Results – Band-edge compliance

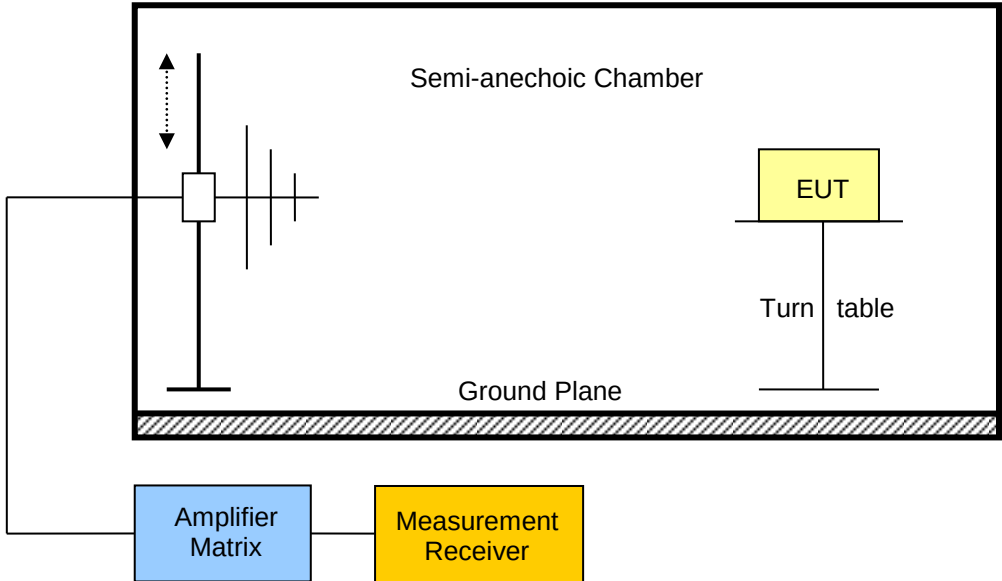Band-edge compliance acc. to FCC Part 95 / IC RSS-243		Verdict: PASS
EUT requirement rule parts and clause	Reference	
	FCC 95.635(d) / IC RSS-243 3.5 5.5 / RSS-Gen 4.9	
Test according to measurement reference	Reference Method	
	FCC 95.635(d) / ANSI C 63.4	
Test frequency range	Tested frequencies	
	F _{LOW} / F _{HIGH}	
EUT test mode	Modulated	
Limits - FCC		
Frequency range	Limit	
402 MHz – 250 kHz ≤ f ≤ 402 MHz	20 dB below maximum permitted output power	
402 MHz < f < 150 kHz - f _C	20 dB below transmitter output power	
150 kHz + f _C < f < 405 Mhz	20 dB below transmitter output power	
405 MHz ≤ f ≤ 405 MHz + 250 kHz	20 dB below maximum permitted output power	
Limits - IC		
Frequency range	Limit	
402 MHz – 250 kHz < f < 150 kHz-f _C	20 dB below maximum permitted output power	
150 kHz+f _C < f < 405 MHz + 250 kHz	20 dB below maximum permitted output power	
Because the FCC limits are more stringent than the Industry Canada limits, the FCC limits are used to show compliance with the band-edge emission requirements.		
Test setup		
		


Test procedure					
1. EUT set to test frequency with modulation 2. Measurement polarization is set to vertical 3. Span it set according to measurement range 4. Resolution bandwidth is set to 1% of the emission bandwidth and detector is set to peak 5. During the sweep the EUT is rotated to obtain maximum emission level 6. Measurement is repeated with horizontal measurement polarization					
Test results					
Channel	Frequency [MHz]	Max. Emission Level [dBμV/m]	Max. Carrier Level [dBμV/m]	In-band Limit [dBμV/m]	Result
F _{LOW}	402.286	21.16	73.8	53.8	PASS
F _{LOW}	402.614	21.48	73.8	53.8	PASS
F _{LOW}	403.649	19.52	73.8	53.8	PASS
F _{HIGH}	403.652	26.20	71.9	51.8	PASS
F _{HIGH}	404.689	19.54	71.9	51.8	PASS
F _{HIGH}	405.000	20.28	71.9	51.8	PASS
Comments: see attached diagrams					

3.6 Test Conditions and Results – Transmitter unwanted emissions

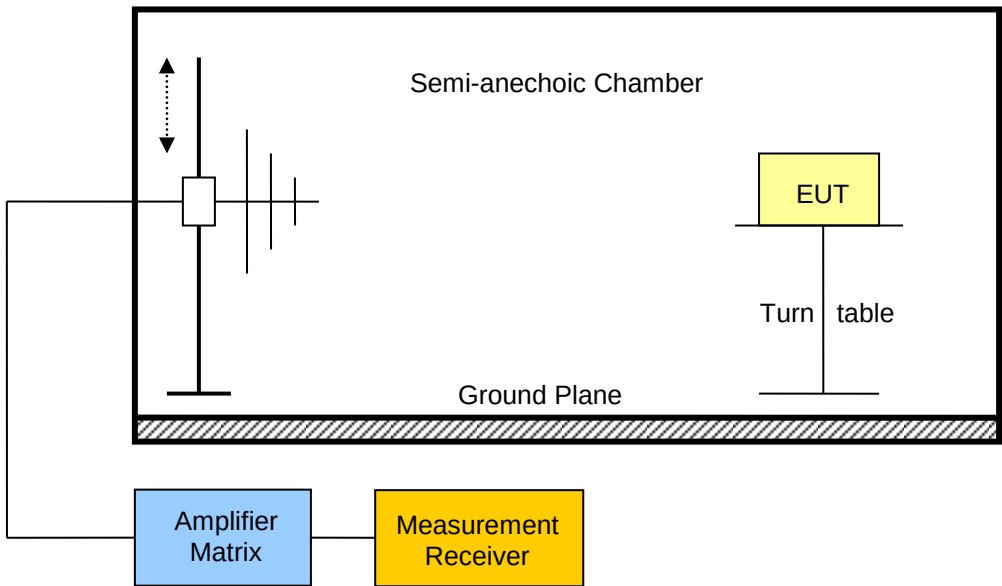Transmitter unwanted emissions acc. to FCC Part 95 / IC RSS-243				Verdict: PASS	
Test according referenced standards		Reference Method			
		FCC 95.635(d) / IC RSS-243 3.4 5.5 / IC RSS-Gen 6.13			
Test according to measurement reference		Reference Method			
		FCC 95.635(d) / ANSI C 63.4			
Test frequency range		Tested frequencies			
		30 MHz – 10 th Harmonic			
Limits					
Frequency range [MHz]	Detector	Limit [μV/m]	Limit [dBμV/m]	Limit Distance [m]	
30 – 88	Quasi-Peak	100	40	3	
88 – 216	Quasi-Peak	150	43.5	3	
216 – 960	Quasi-Peak	200	46	3	
960 – 1000	Quasi-Peak	500	54	3	
> 1000	Average	500	54	3	
Test setup					
					

Test procedure									
1. EUT set to test mode 2. Span it set according to measurement range 3. Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector and RBW of 1 MHz with peak/average detector is used above 1 GHz 4. Markers are set to peak emission levels within restricted bands									
Test results									
Channel	Frequency [MHz]	Mode	Emission [MHz]	Level [dBμV/m]	Det.	Pol.	Limit [dBμV/m]	Limit dist. [m]*	Margin [dB]
F _{LOW}	402.45	Modulated	401.347	27.19	pk	ver	46.00	3	-18.81
F _{LOW}	402.45	Modulated	406.44	20.20	pk	hor	46.00	3	-25.80
F _{LOW}	402.45	Modulated	406.44	22.80	pk	ver	46.00	3	-23.20
F _{LOW}	402.45	Modulated	1695	35.62	pk	hor	54.00	3	-18.38
F _{HIGH}	404.85	Modulated	399.95	23.04	pk	hor	46.00	3	-22.96
F _{HIGH}	404.85	Modulated	400.136	27.34	pk	ver	46.00	3	-18.66
F _{HIGH}	404.85	Modulated	405	14.98	pk	hor	59.40	3	-44.42
F _{HIGH}	404.85	Modulated	405	20.28	pk	ver	40.50	3	-20.22
F _{HIGH}	404.85	Modulated	405.001	19.34	pk	ver	59.40	3	-40.06
F _{HIGH}	404.85	Modulated	405.017	19.36	pk	ver	59.40	3	-40.04
F _{HIGH}	404.85	Modulated	406.44	18.09	pk	hor	46.00	3	-27.91
Comments: * Physical distance between EUT and measurement antenna.									

3.7 Test Conditions and Results – Receiver spurious emissions

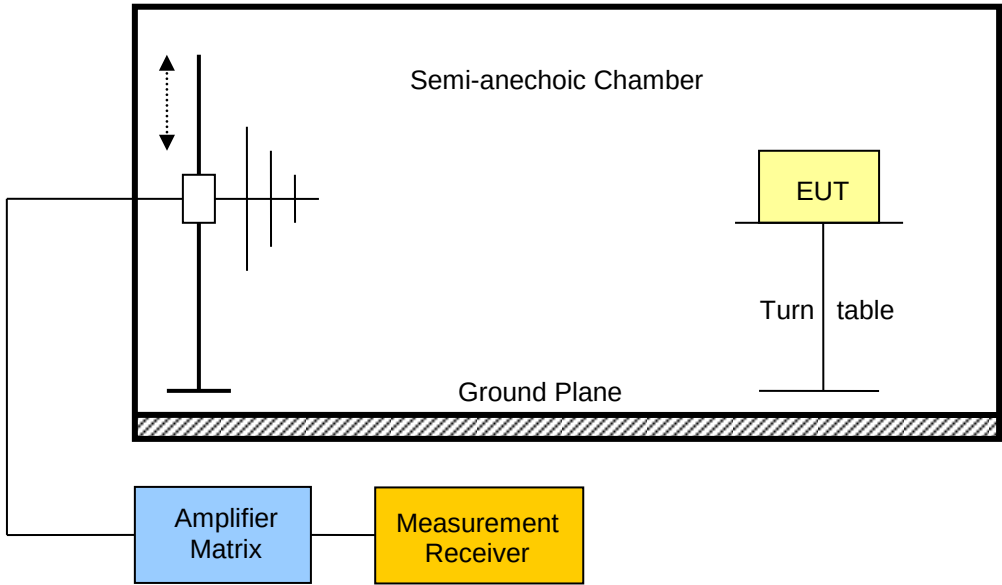Receiver spurious emissions acc. to IC RSS-243				Verdict: PASS
Test according referenced standards	Reference Method			
	IC RSS-243 3.5 5.6 / IC RSS-Gen 7.1			
Test according to measurement reference	Reference Method			
	ANSI C 63.4			
Test frequency range	Tested frequencies			
	30 MHz – 3 th Harmonic			
EUT test mode	Receive			
Limits				
Frequency range [MHz]	Detector	Limit [μV/m]	Limit [dBμV/m]	Limit Distance [m]
30 – 88	Quasi-Peak	100	40	3
88 – 216	Quasi-Peak	150	43.5	3
216 – 960	Quasi-Peak	200	46	3
960 – 1000	Quasi-Peak	500	54	3
> 1000	Average	500	54	3
Test setup				
				

Test procedure							
1. EUT set to receive mode (Communication tester is used if needed) 2. Span it set according to measurement range 3. Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector and RBW of 1 MHz with peak/average detector is used above 1 GHz 4. Markers are set to peak emission levels							
Test results							
Channel	Frequency [MHz]	Emission [MHz]	Emission Level [dBμV/m]	Det.	Pol.	Limit [dBμV/m]	Margin [dBμV/m]
F _{MID}	403.65	984	19.60	pk	hor	54	-34.40
F _{MID}	403.65	1696	35.11	pk	ver	54	-18.89
F _{MID}	403.65	1702	34.64	pk	hor	54	-19.36
Comments: * Physical distance between EUT and measurement antenna. ** Emission level corresponds to ambient noise floor							


ANNEX A Transmitter radiated power

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: Tx; 402.45 MHz, 2FSK
 Test Date: 2015-01-26
 Note: Tx Power EIRP

Index 52

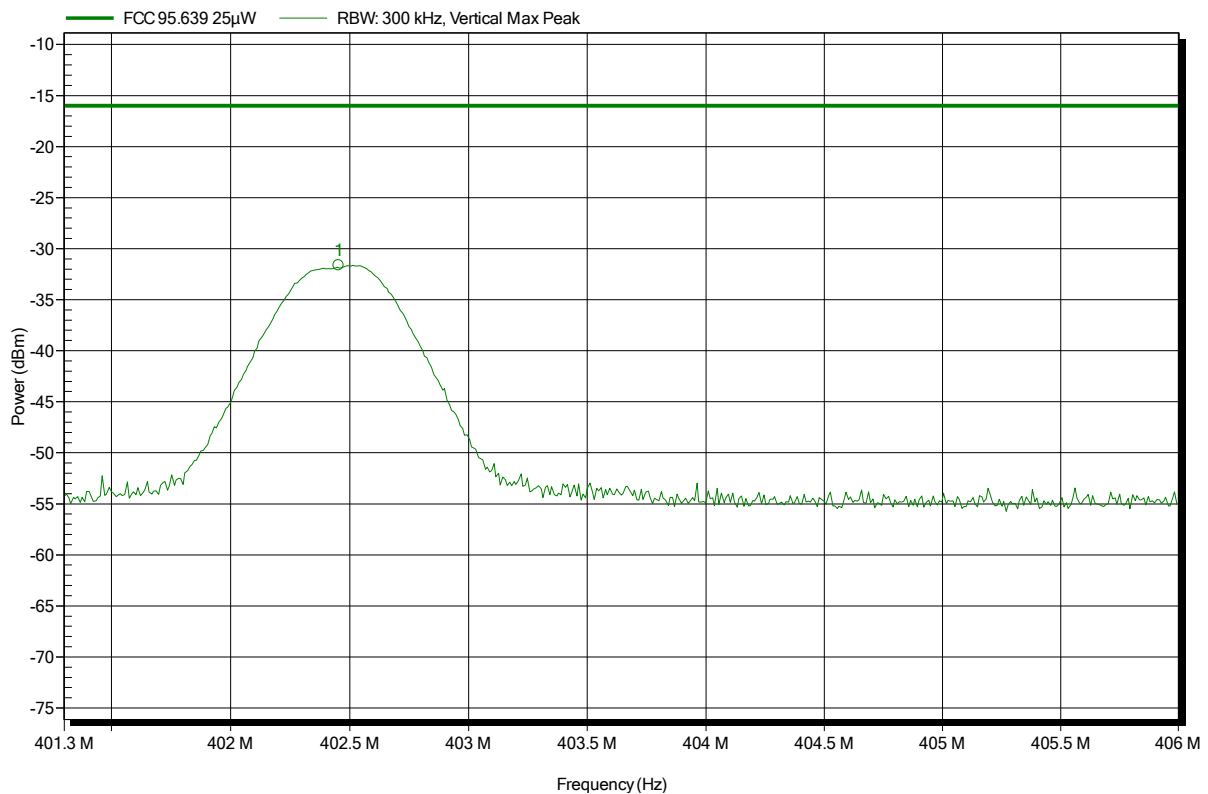

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.453 MHz	-31.6 dBm	-16 dBm	-15.64 dB	Pass

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: Tx; 402.45 MHz, 2FSK
 Test Date: 2015-01-26
 Note: Tx Power EIRP

Index 54

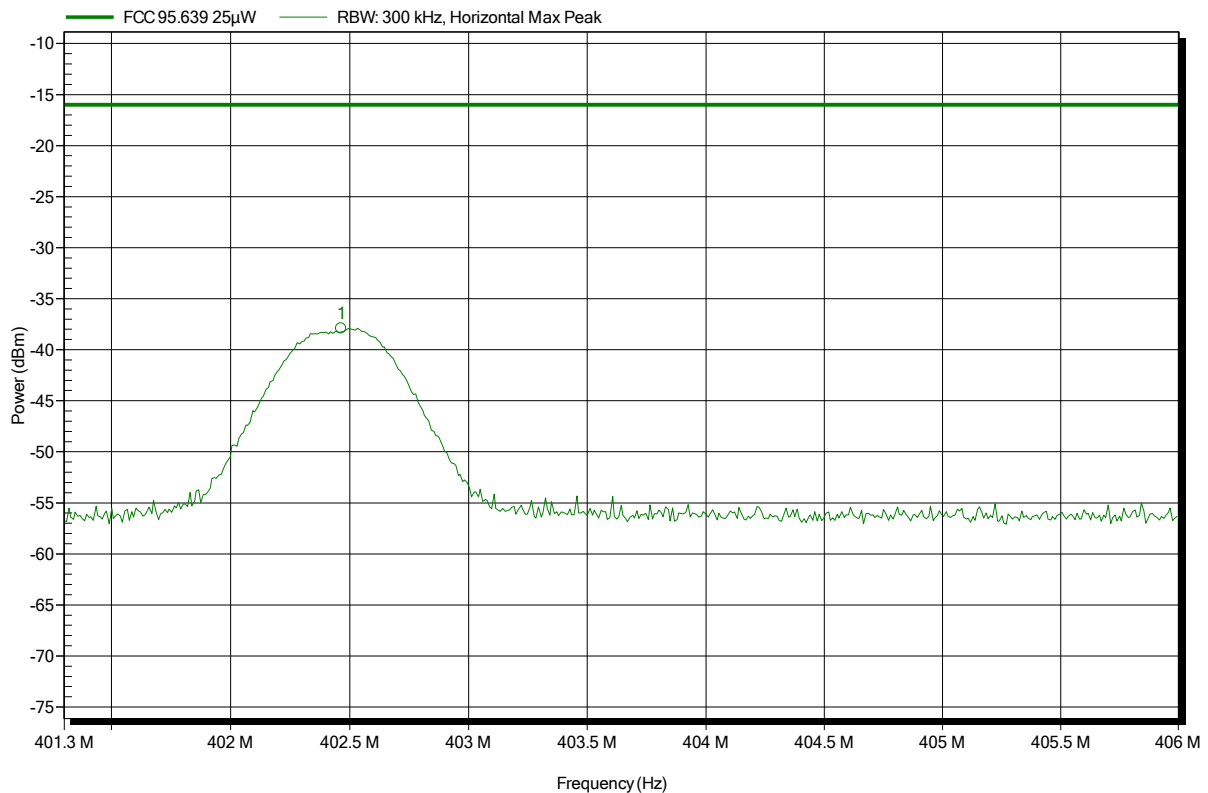

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.464 MHz	-37.9 dBm	-16 dBm	-21.93 dB	Pass

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: Tx; 404.85 MHz, 2FSK
 Test Date: 2015-01-26
 Note: Tx Power EIRP

Index 48

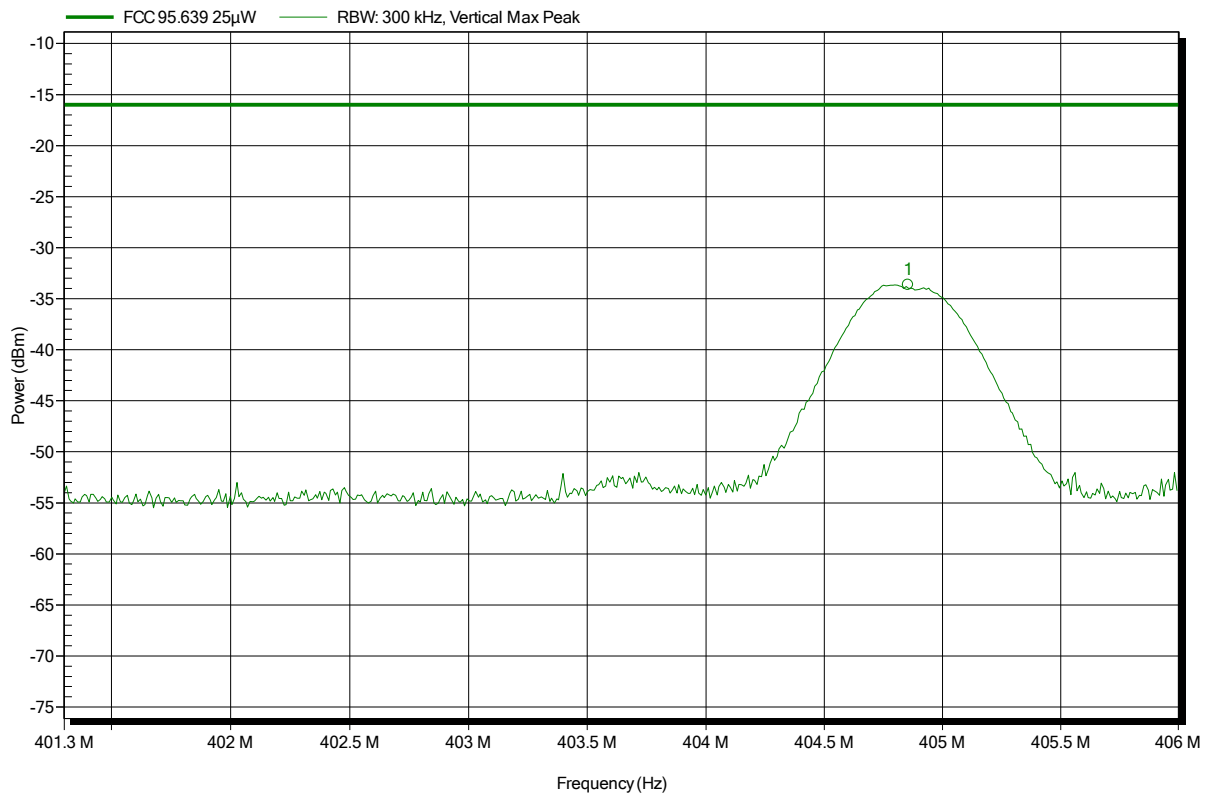

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
404.853 MHz	-33.7 dBm	-16 dBm	-17.65 dB	Pass

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: Tx; 404.85 MHz, 2FSK
 Test Date: 2015-01-26
 Note: Tx Power EIRP

Index 50

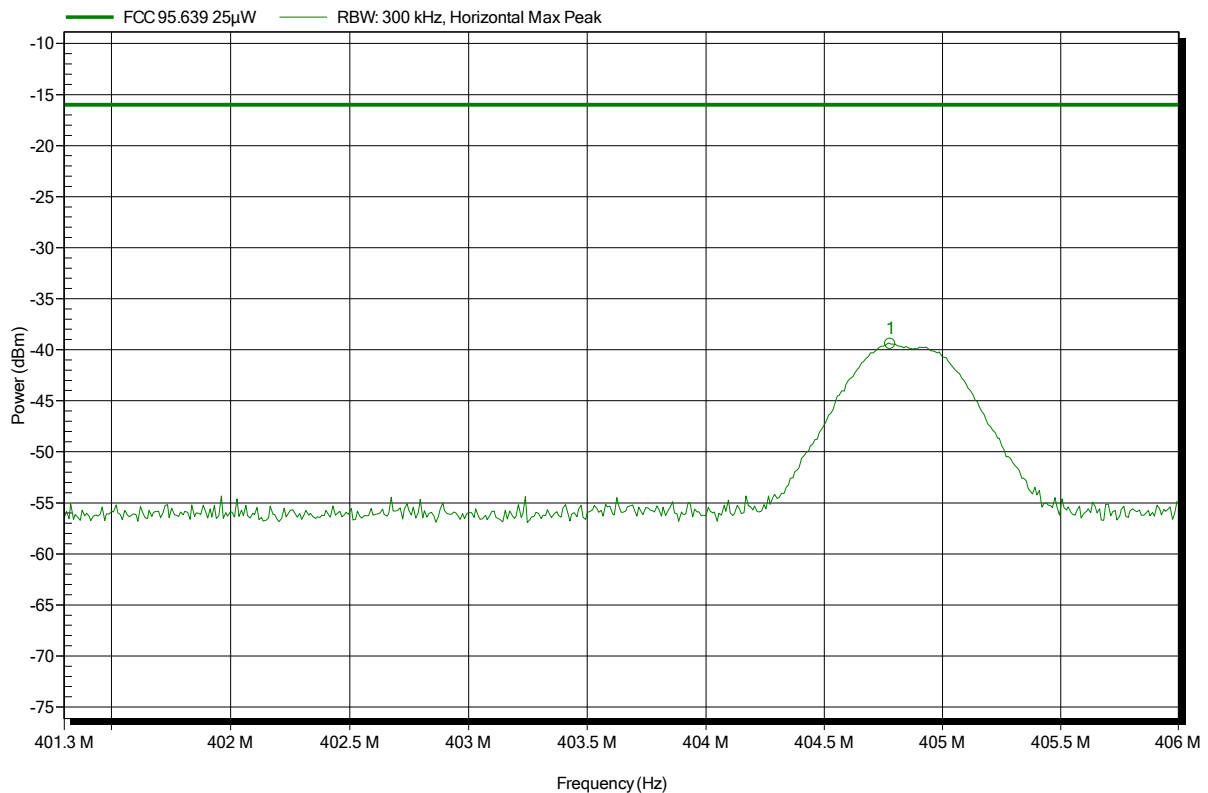

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
404.778 MHz	-39.4 dBm	-16 dBm	-23.44 dB	Pass

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1412-4360

Applicant:	BIOTRONIK SE & Co.KG
EUT Name:	ICD / Implantable Cardioverter Defibrillator
Model:	Inlexa 1
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 25°C, Vnom: 3.0 VDC lithium battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	Tx; 402.45 MHz, 2FSK
Test Date:	2015-01-26
Note:	Power dBμV/m ERP

Index 53

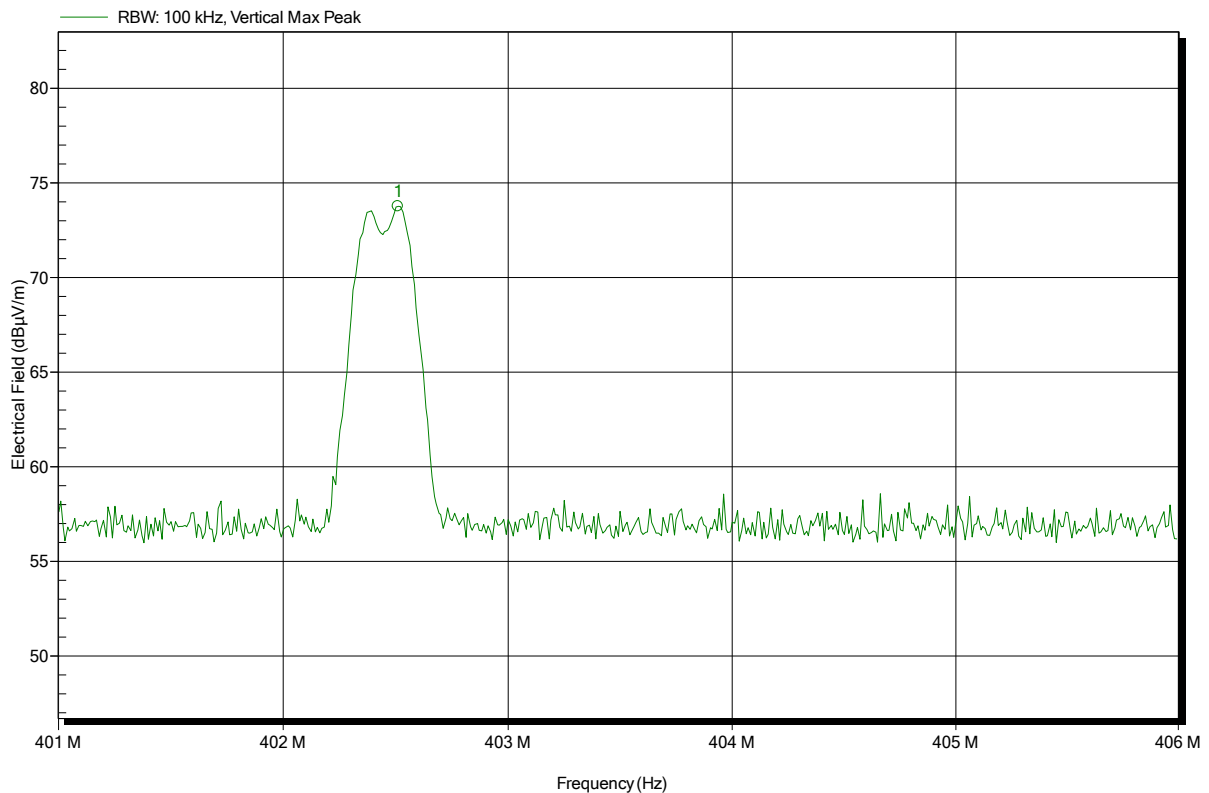

Frequency
402.51 MHz

Peak
73.77 dBμV/m

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1412-4360

Applicant:	BIOTRONIK SE & Co.KG
EUT Name:	ICD / Implantable Cardioverter Defibrillator
Model:	Inlexa 1
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 25°C, Vnom: 3.0 VDC lithium battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	Tx; 402.45 MHz, 2FSK
Test Date:	2015-01-26
Note:	Power dBμV/m ERP

Index 55

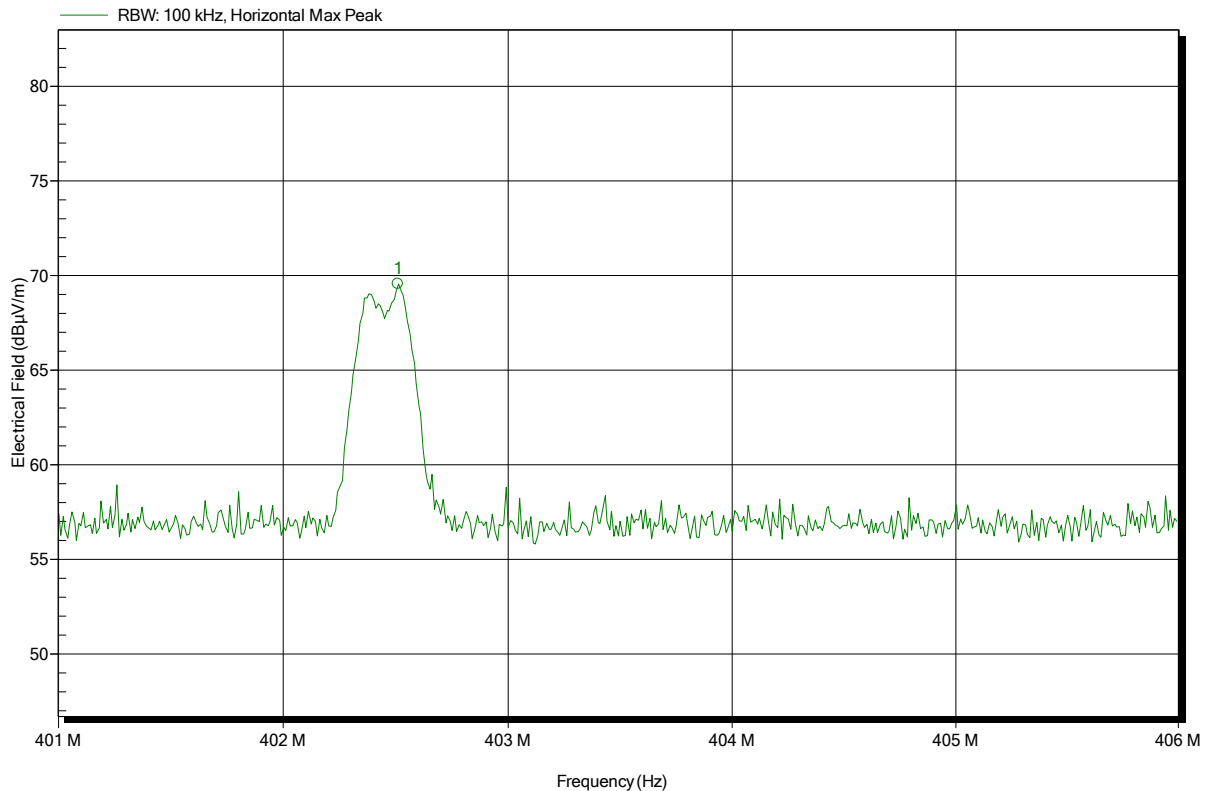

Frequency
402.51 MHz


Peak
69.57 dBμV/m

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1412-4360

Applicant:	BIOTRONIK SE & Co.KG
EUT Name:	ICD / Implantable Cardioverter Defibrillator
Model:	Inlexa 1
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 25°C, Vnom: 3.0 VDC lithium battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	Tx; 404.85 MHz, 2FSK
Test Date:	2015-01-26
Note:	Power dBμV/m ERP

Index 49

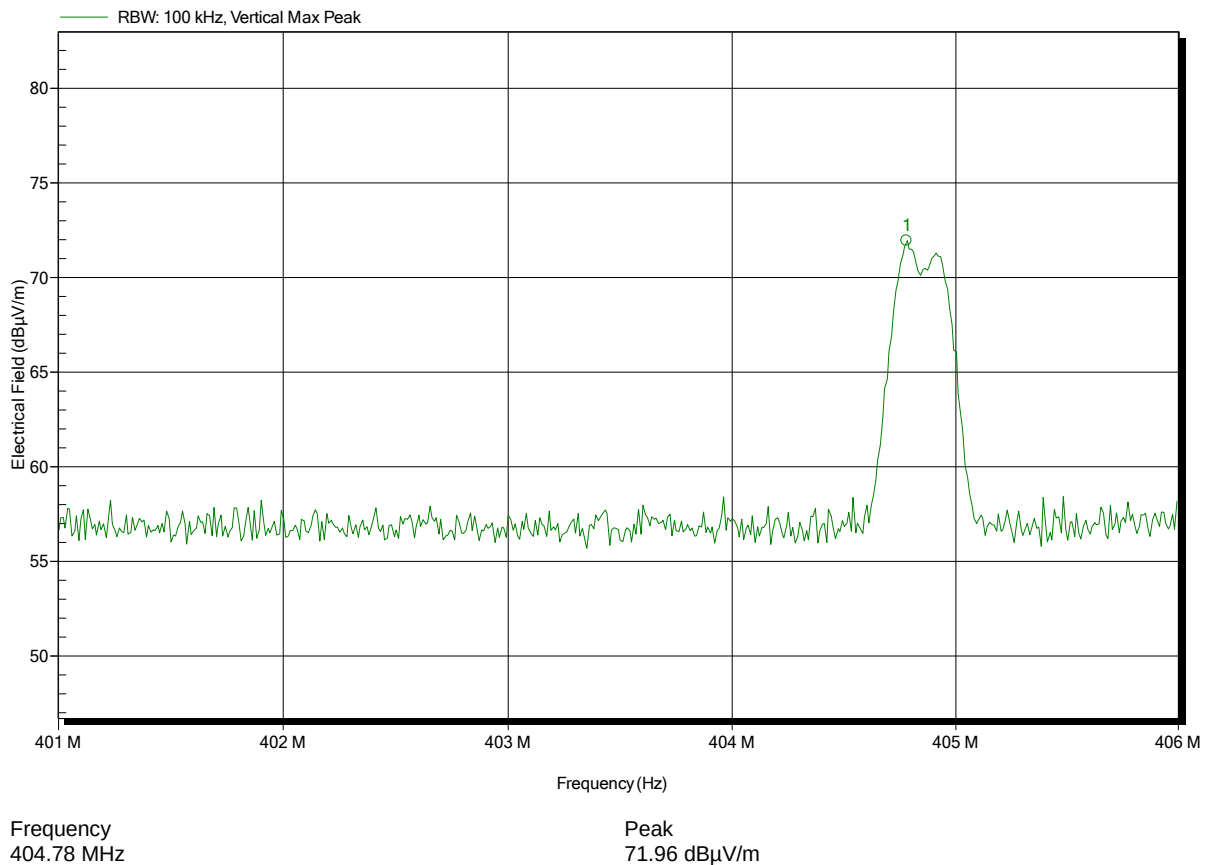


Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1412-4360

Applicant:	BIOTRONIK SE & Co.KG
EUT Name:	ICD / Implantable Cardioverter Defibrillator
Model:	Inlexa 1
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 25°C, Vnom: 3.0 VDC lithium battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	Tx; 404.85 MHz, 2FSK
Test Date:	2015-01-26
Note:	Power dBµV/m ERP

Index 51

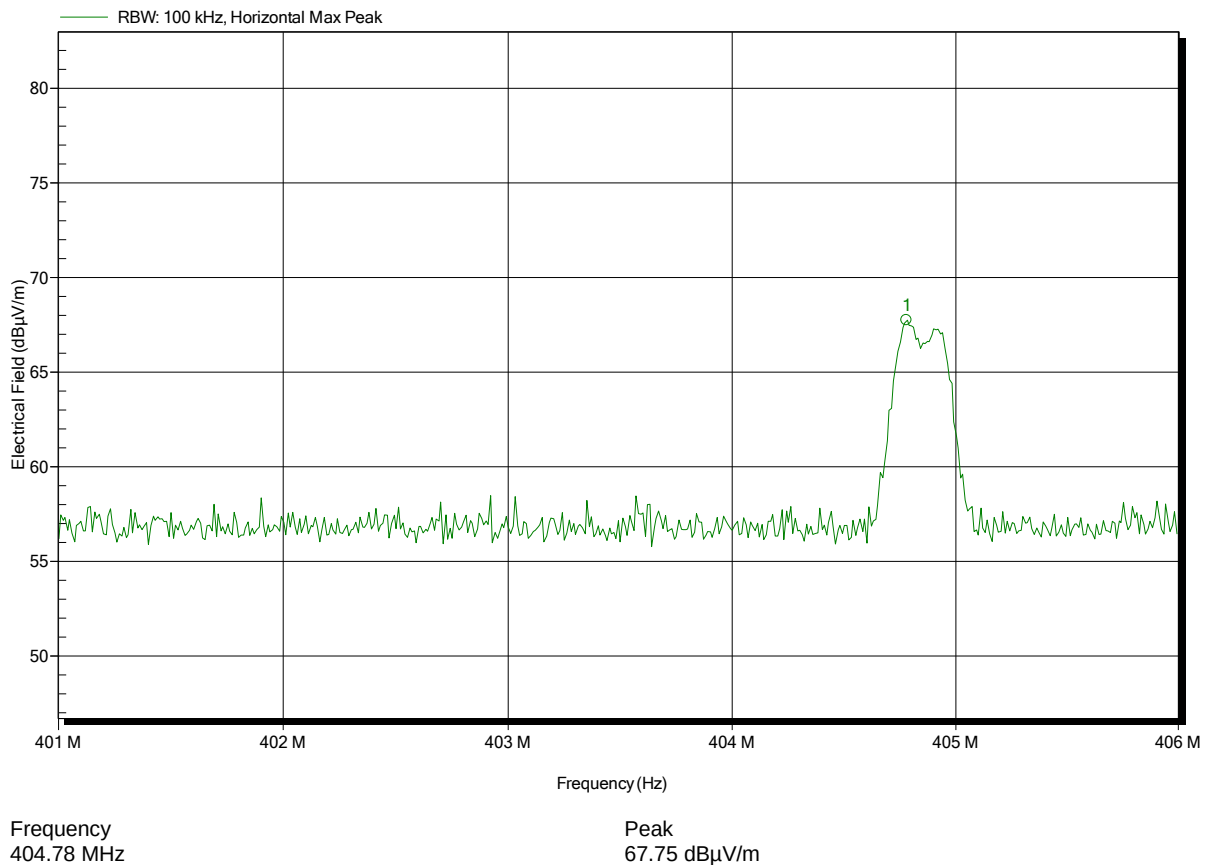


ANNEX B Transmitter radiated spurious emissions

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HK116, Horizontal
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 62

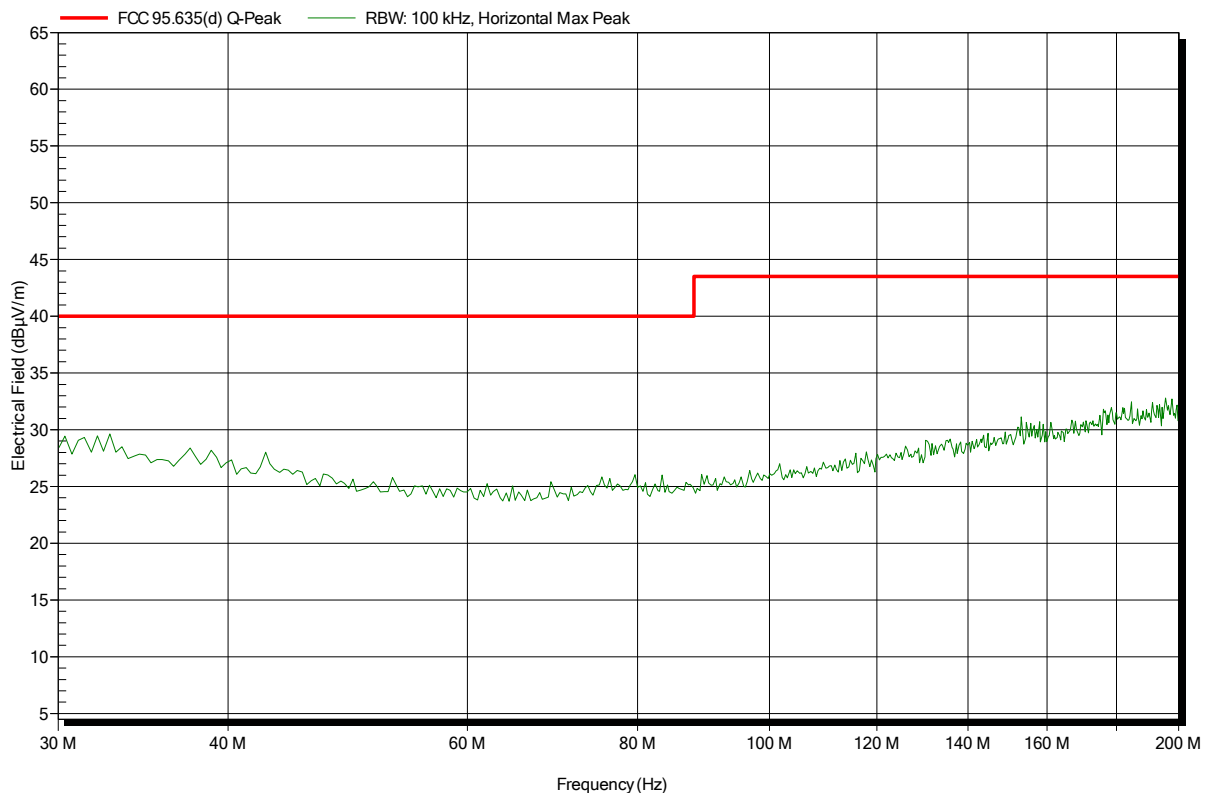


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HK116, Vertical
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 63

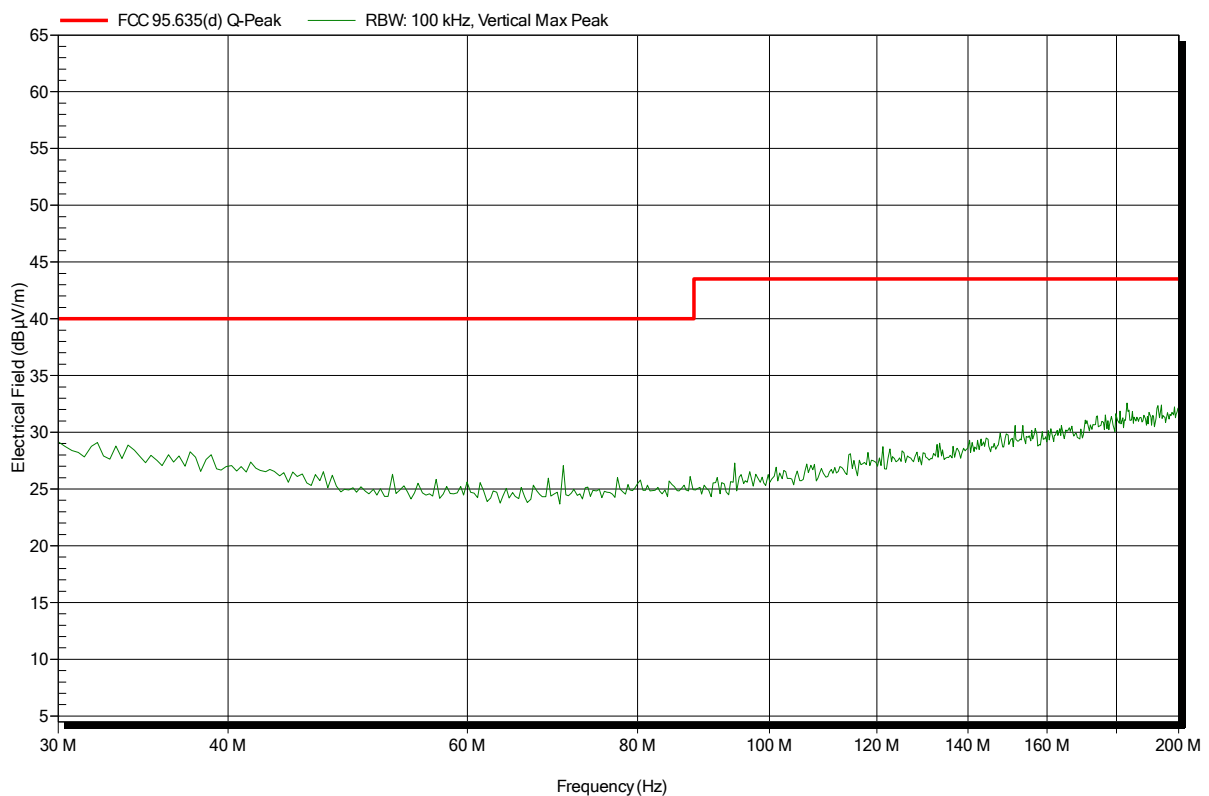


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant:	BIOTRONIK SE & Co.KG
EUT Name:	ICD / Implantable Cardioverter Defibrillator
Model:	Inlexa 1
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 25°C, Vnom: 3.0 VDC lithium battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	TX; 402.45 MHz, 2FSK
Test Date:	2015-01-27
Note:	

Index 56

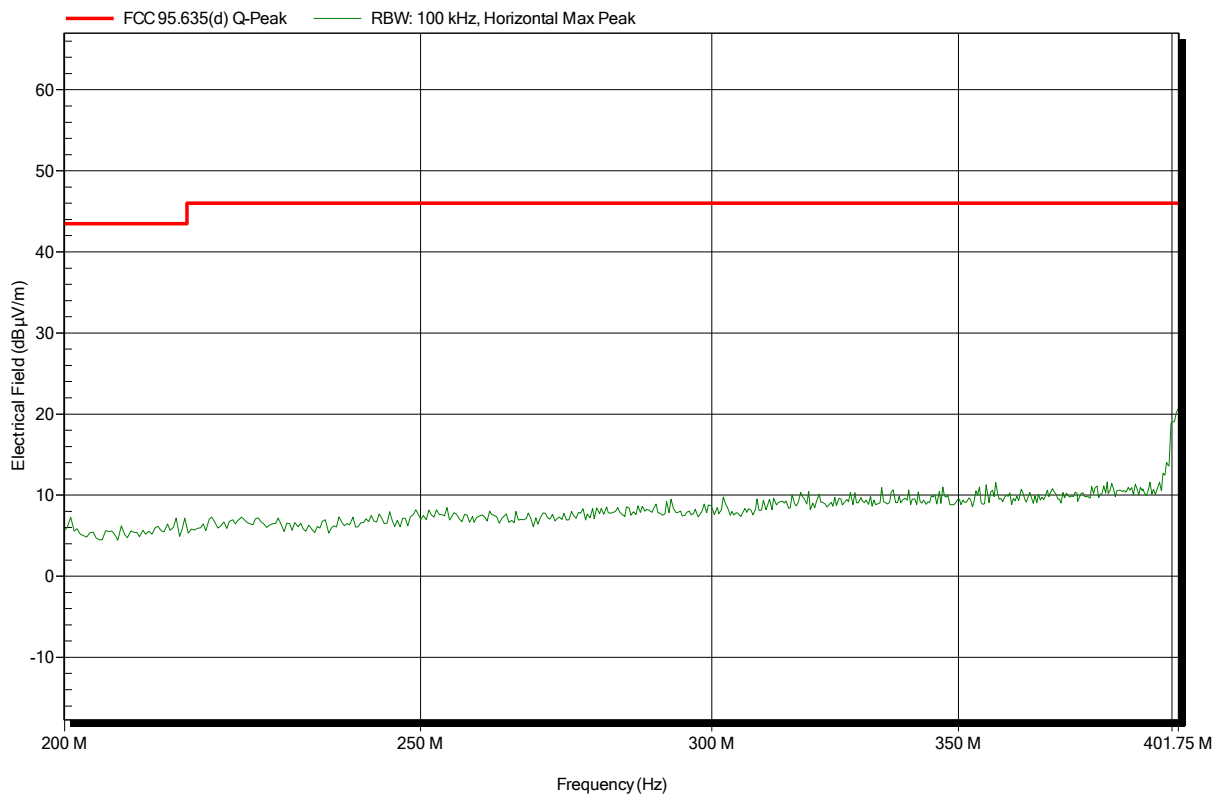


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 64

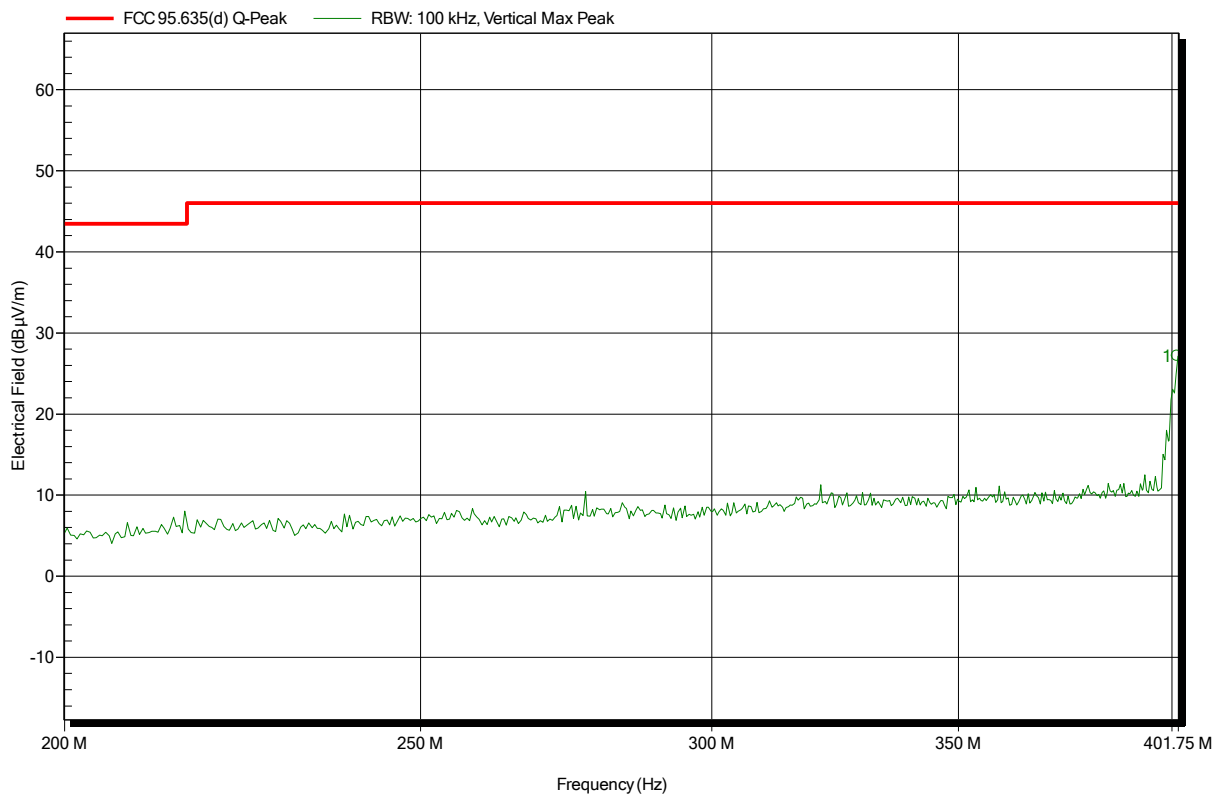


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
401.347 MHz	27.19 dBµV/m	46 dBµV/m	-18.81 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant:	BIOTRONIK SE & Co.KG
EUT Name:	ICD / Implantable Cardioverter Defibrillator
Model:	Inlexa 1
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 25°C, Vnom: 3.0 VDC lithium battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	TX; 402.45 MHz, 2FSK
Test Date:	2015-01-27
Note:	Band-edge

Index 58

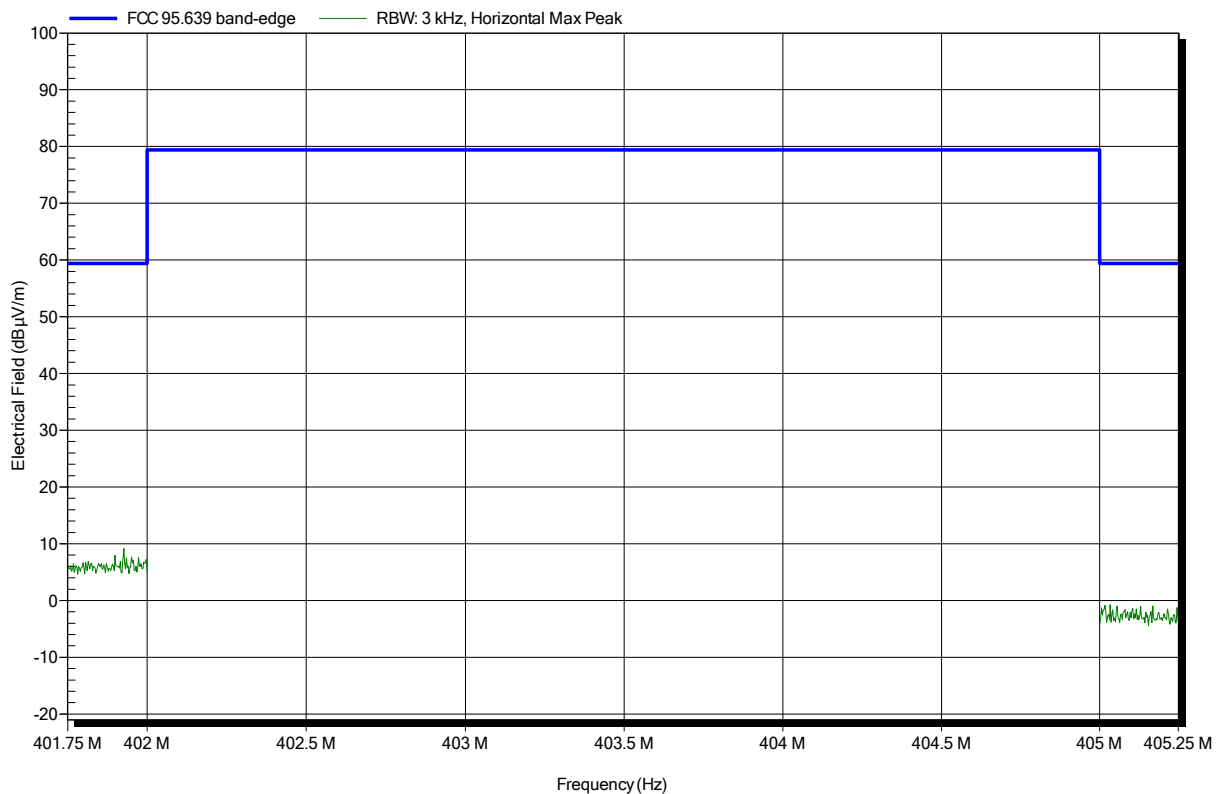


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant:	BIOTRONIK SE & Co.KG
EUT Name:	ICD / Implantable Cardioverter Defibrillator
Model:	Inlexa 1
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 25°C, Vnom: 3.0 VDC lithium battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	TX; 402.45 MHz, 2FSK
Test Date:	2015-01-27
Note:	Band-edge

Index 65

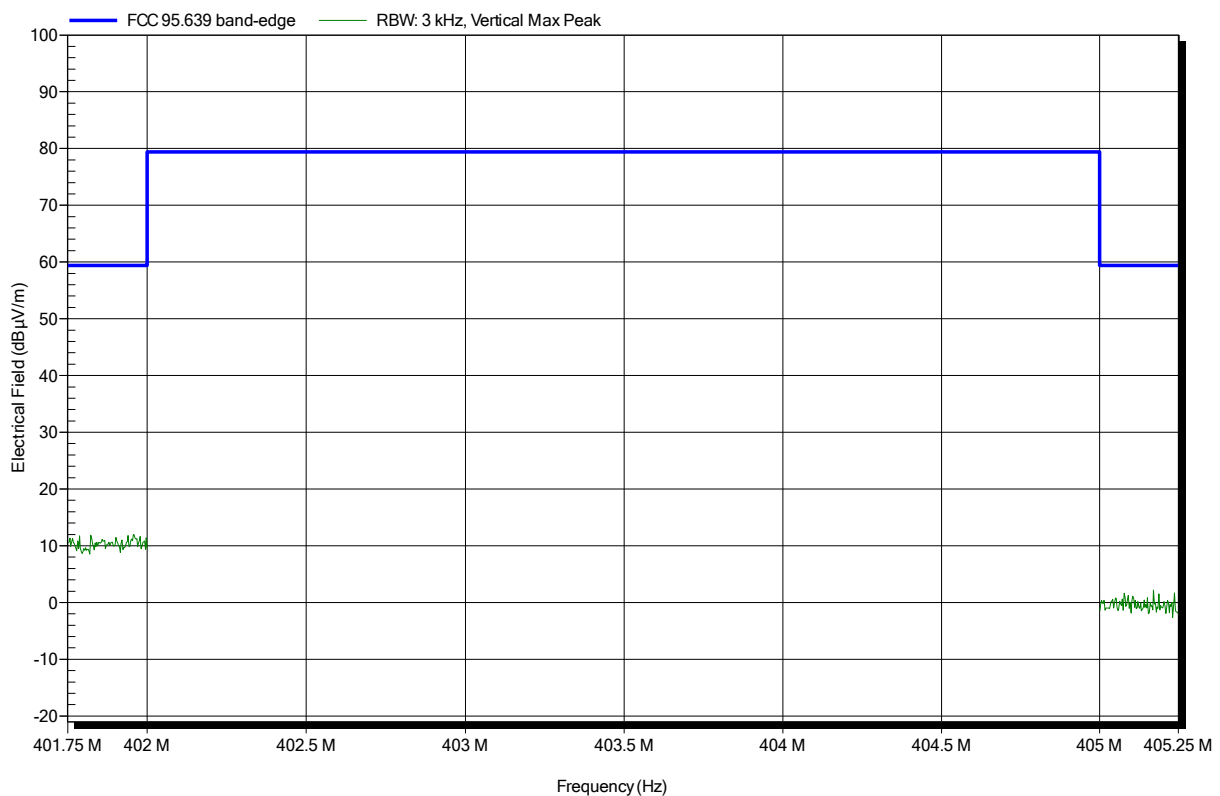


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz, 2FSK
 Test Date: 2015-01-27
 Note: In-band emissions

Index 59

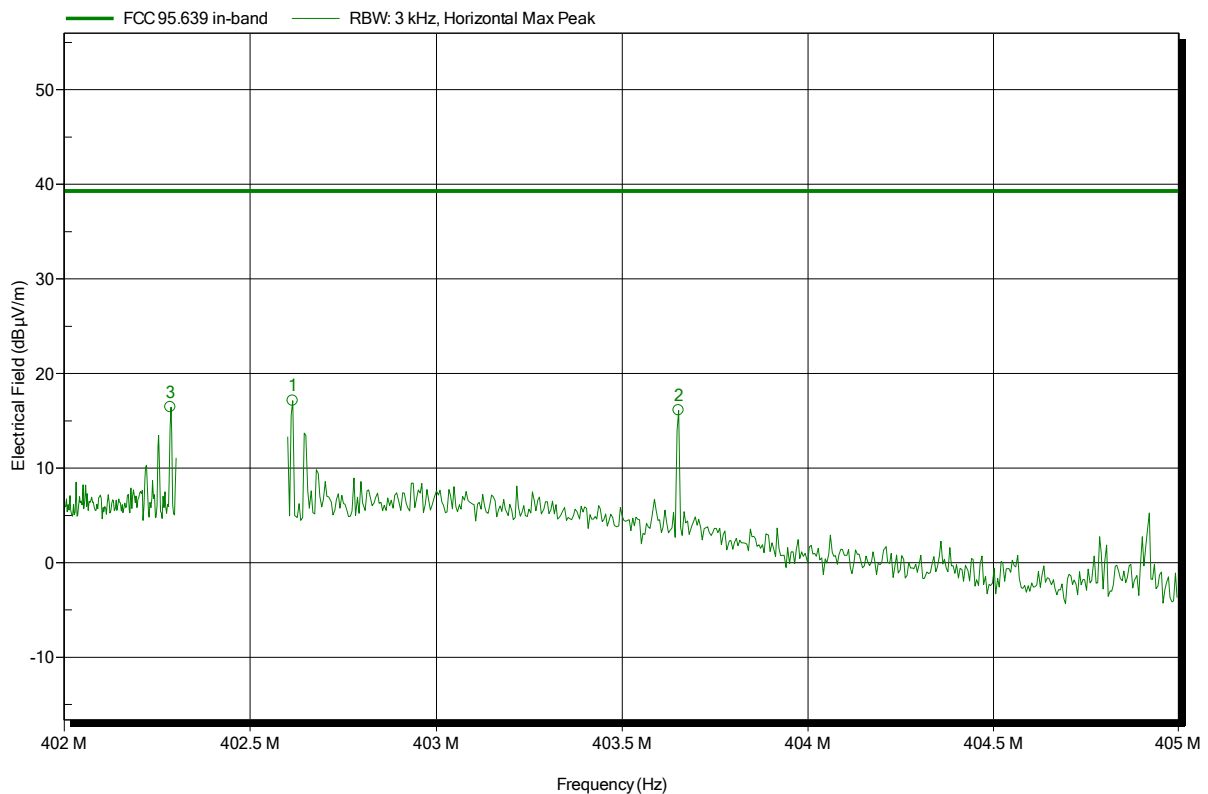


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.286 MHz	16.45 dBµV/m	39.3 dBµV/m	-22.85 dB	Pass
402.614 MHz	17.13 dBµV/m	39.3 dBµV/m	-22.17 dB	Pass
403.651 MHz	16.11 dBµV/m	39.3 dBµV/m	-23.19 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz, 2FSK
 Test Date: 2015-01-27
 Note: In-band emissions

Index 66

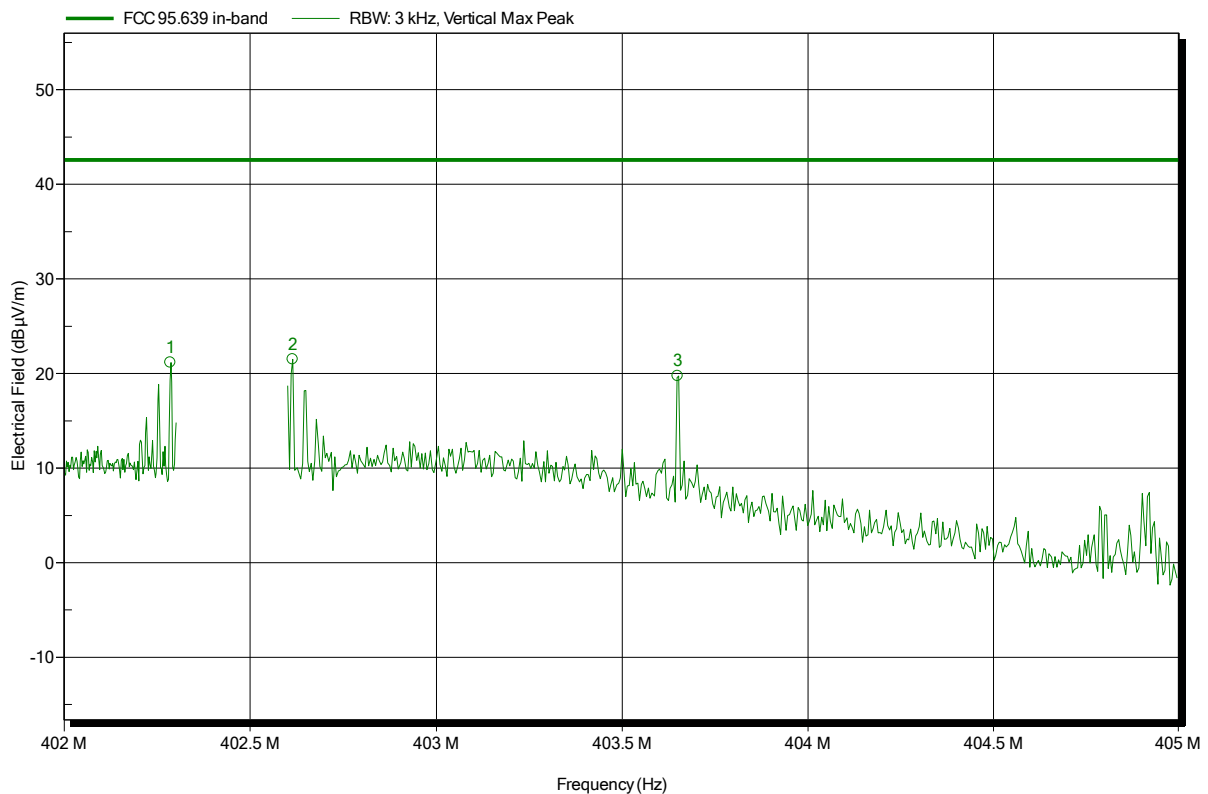


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.286 MHz	21.16 dBµV/m	42.6 dBµV/m	-21.44 dB	Pass
402.614 MHz	21.48 dBµV/m	42.6 dBµV/m	-21.12 dB	Pass
403.649 MHz	19.72 dBµV/m	42.6 dBµV/m	-22.88 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 60

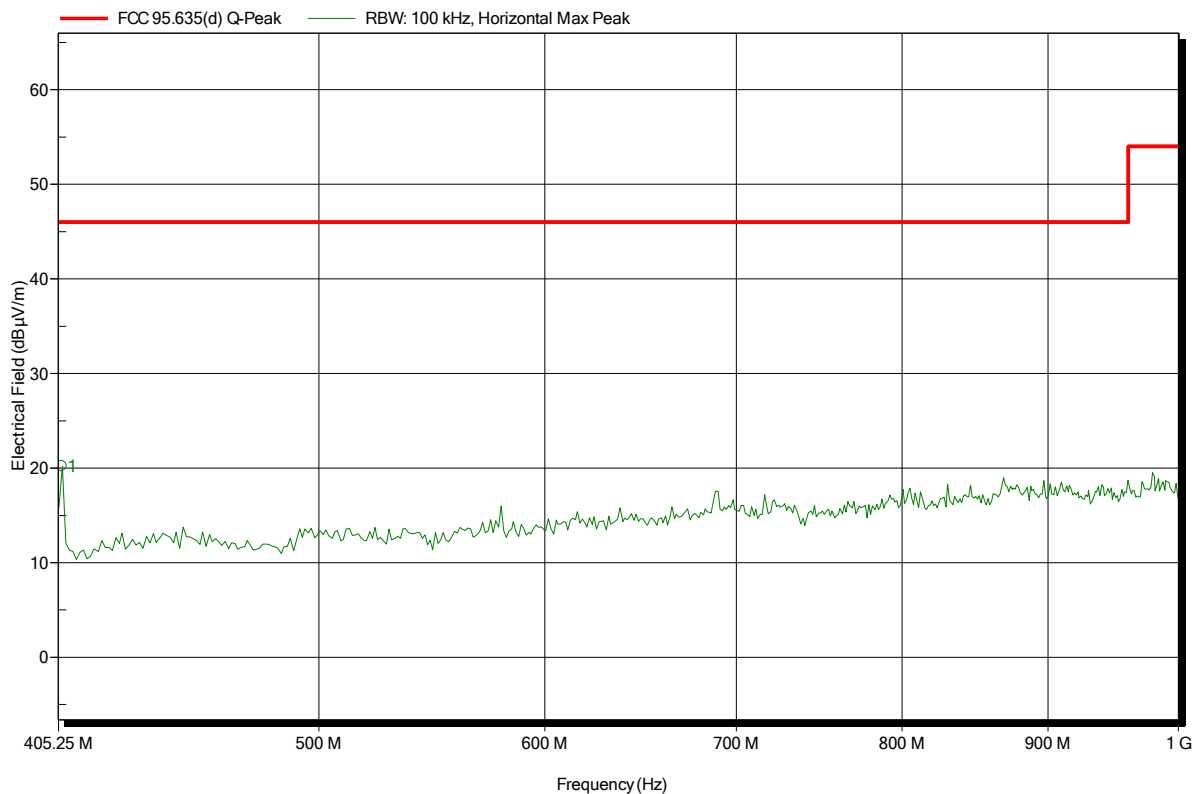


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
406.44 MHz	20.2 dBµV/m	46 dBµV/m	-25.8 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 67

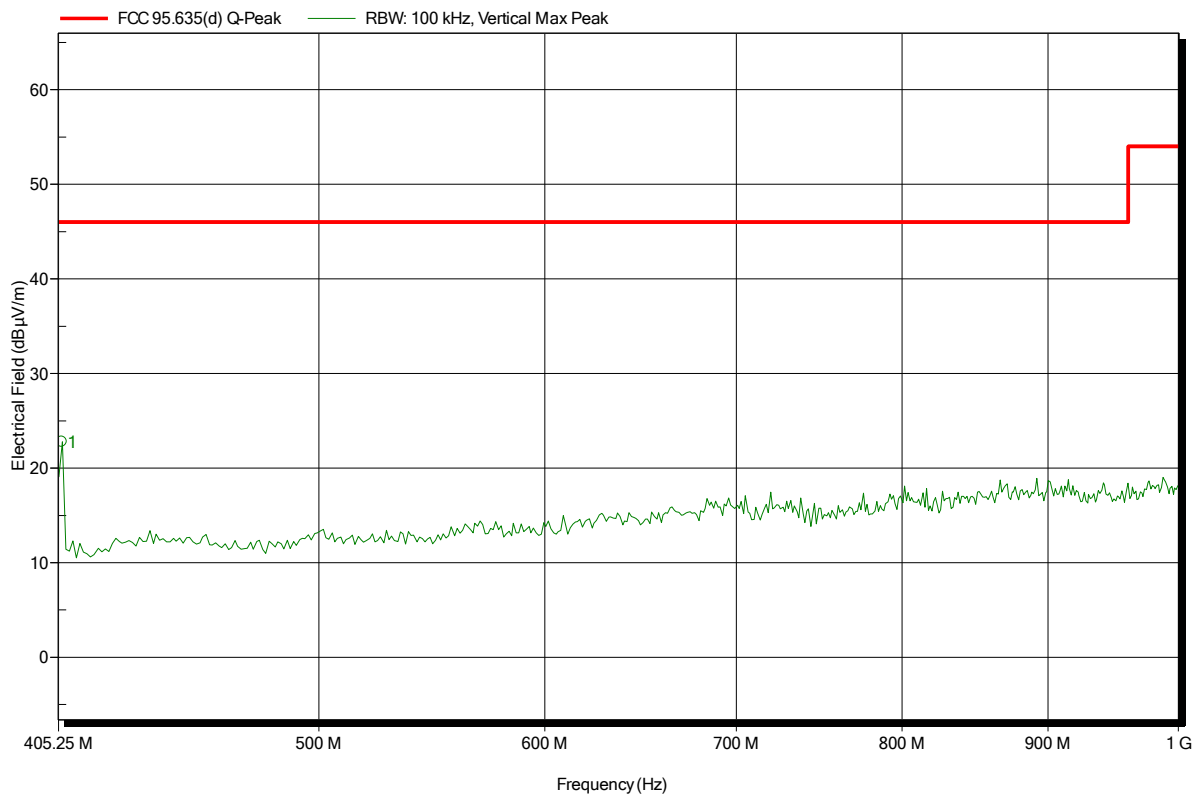


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
406.44 MHz	22.8 dBµV/m	46 dBµV/m	-23.2 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL025, Horizontal
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 61

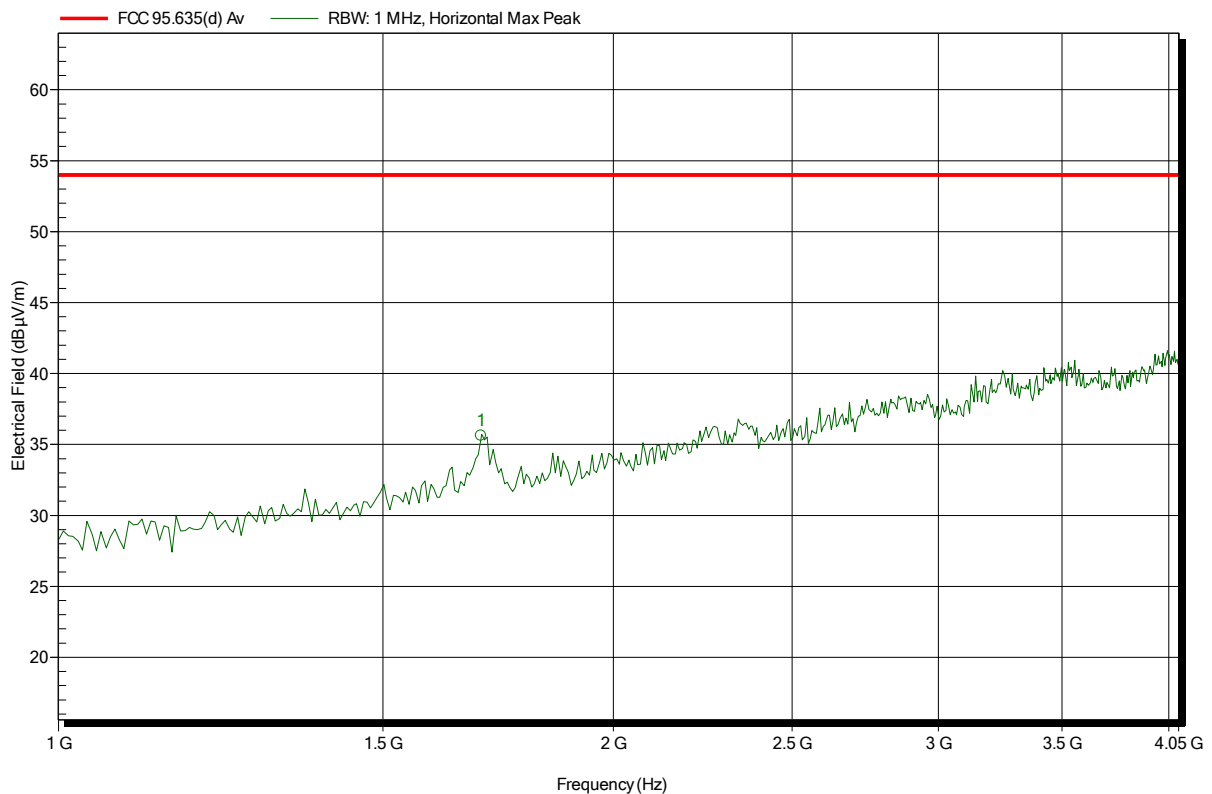

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
1.695 GHz	35.62 dBµV/m	54 dBµV/m	-18.38 dB	Pass

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL025, Vertical
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 68

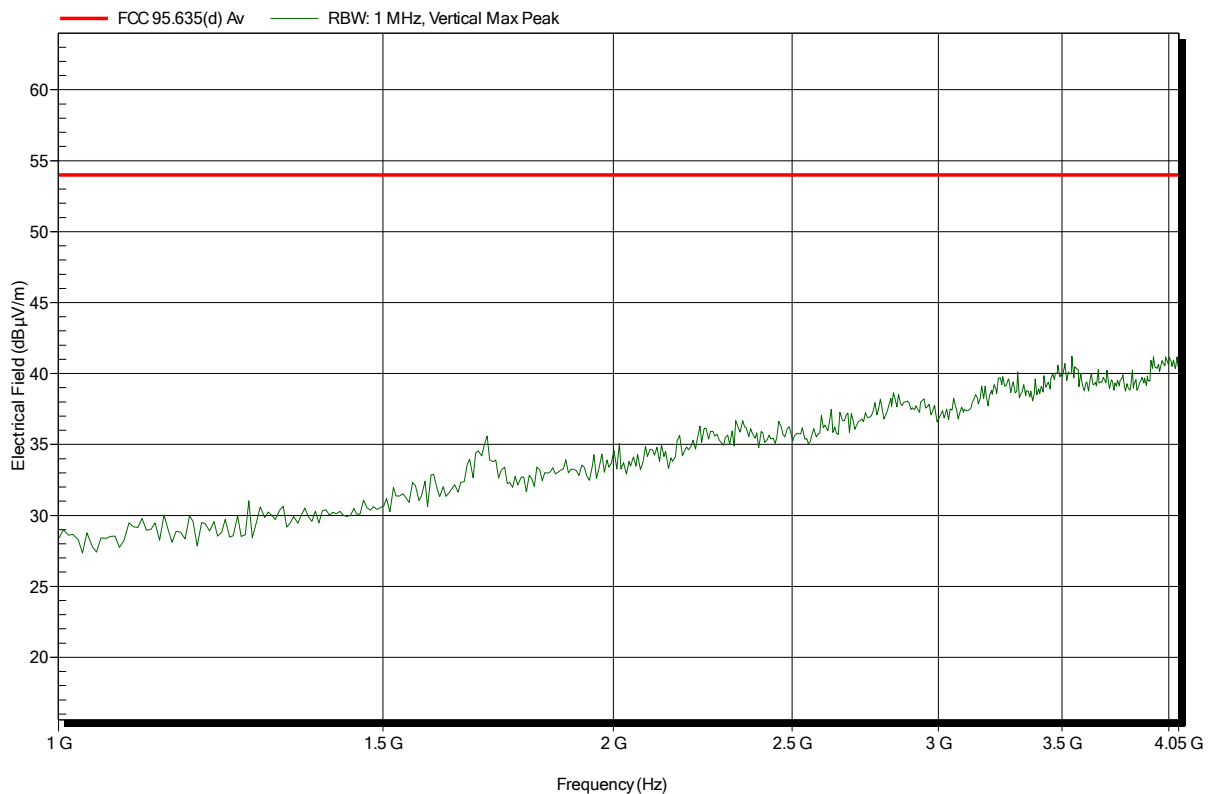


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HK116, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 78

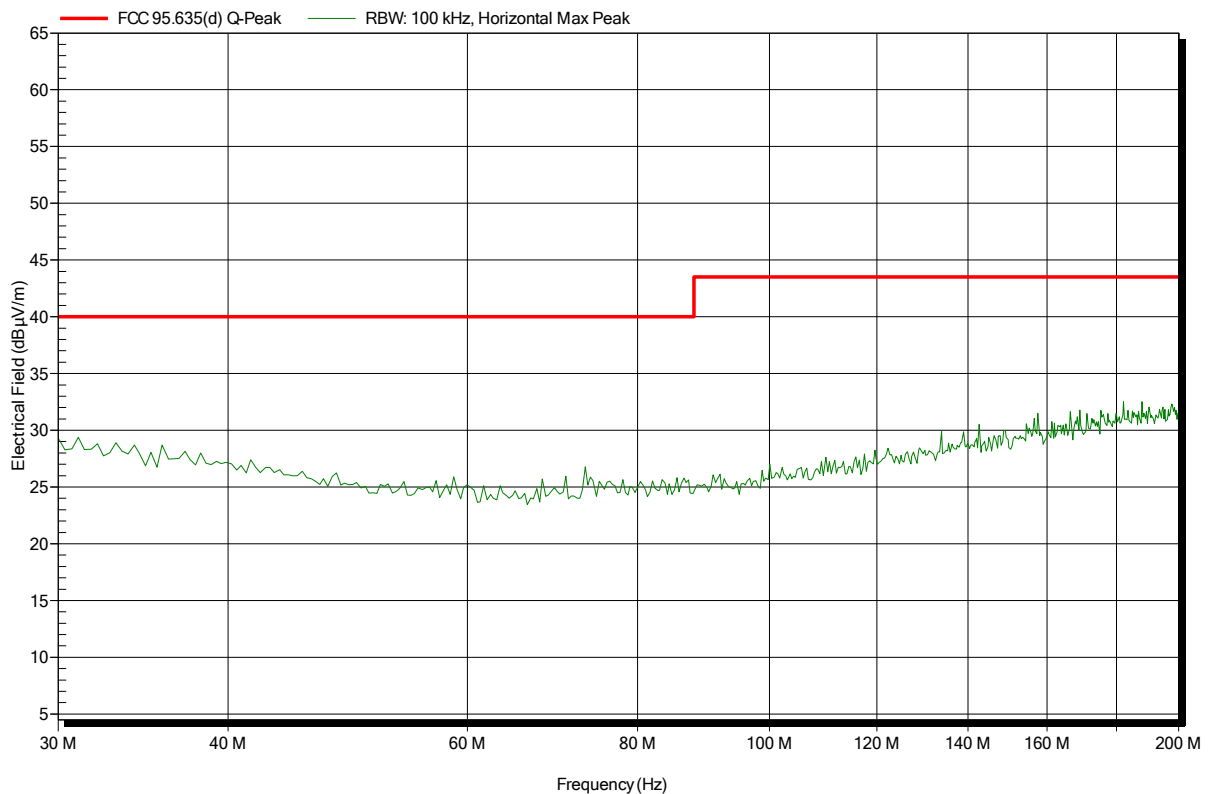


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HK116, Vertical
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 79

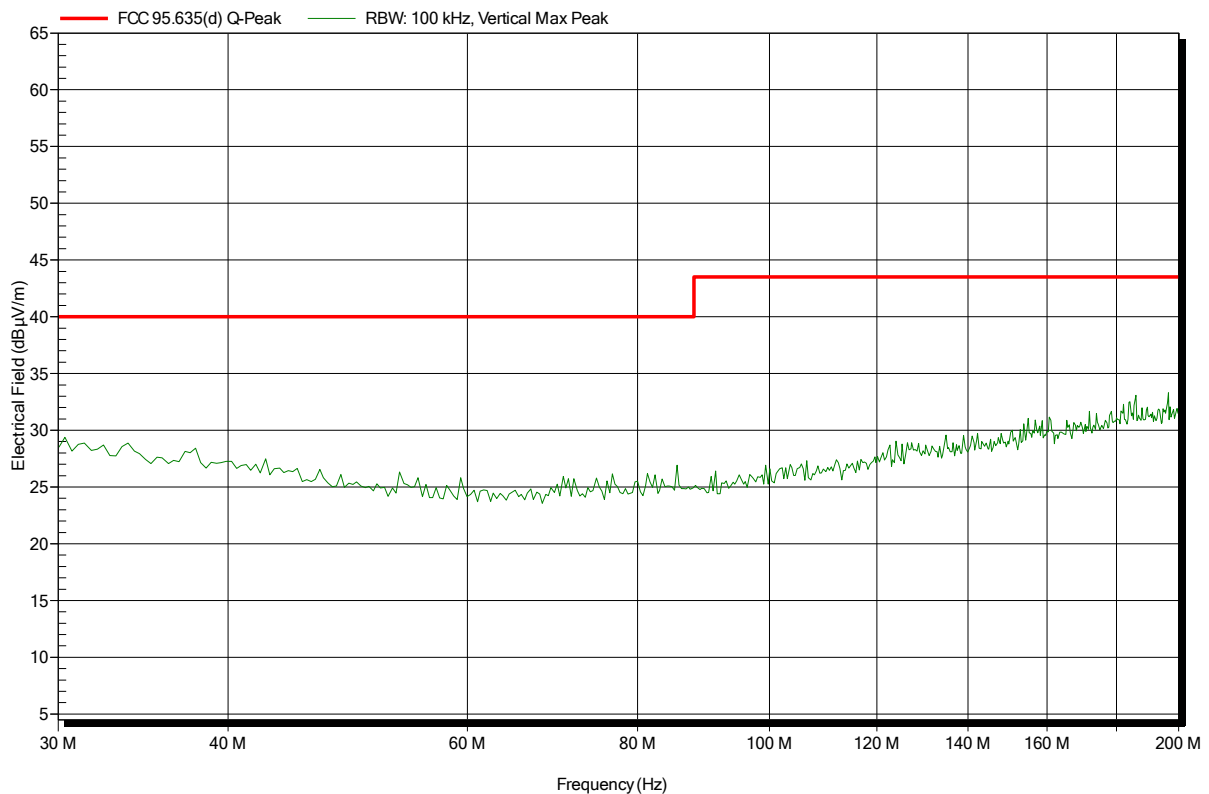


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 71

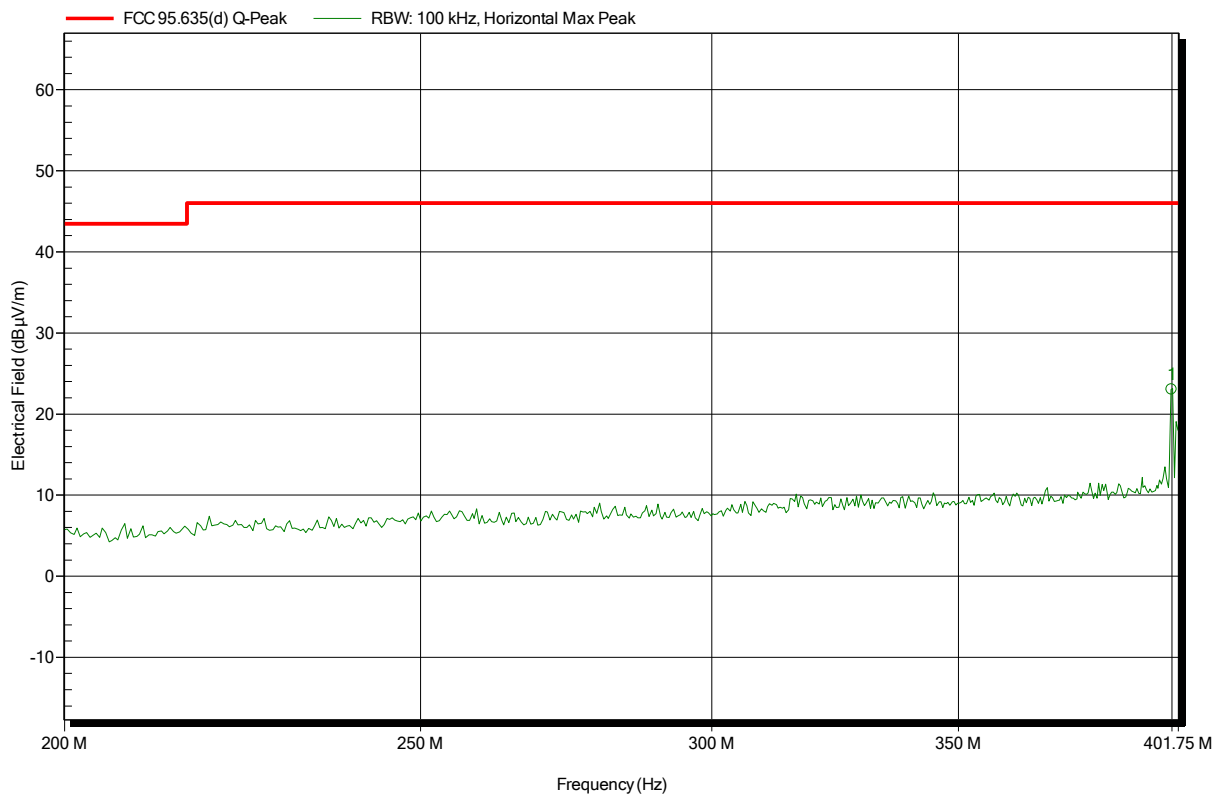


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
399.95 MHz	23.04 dBµV/m	46 dBµV/m	-22.96 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 75

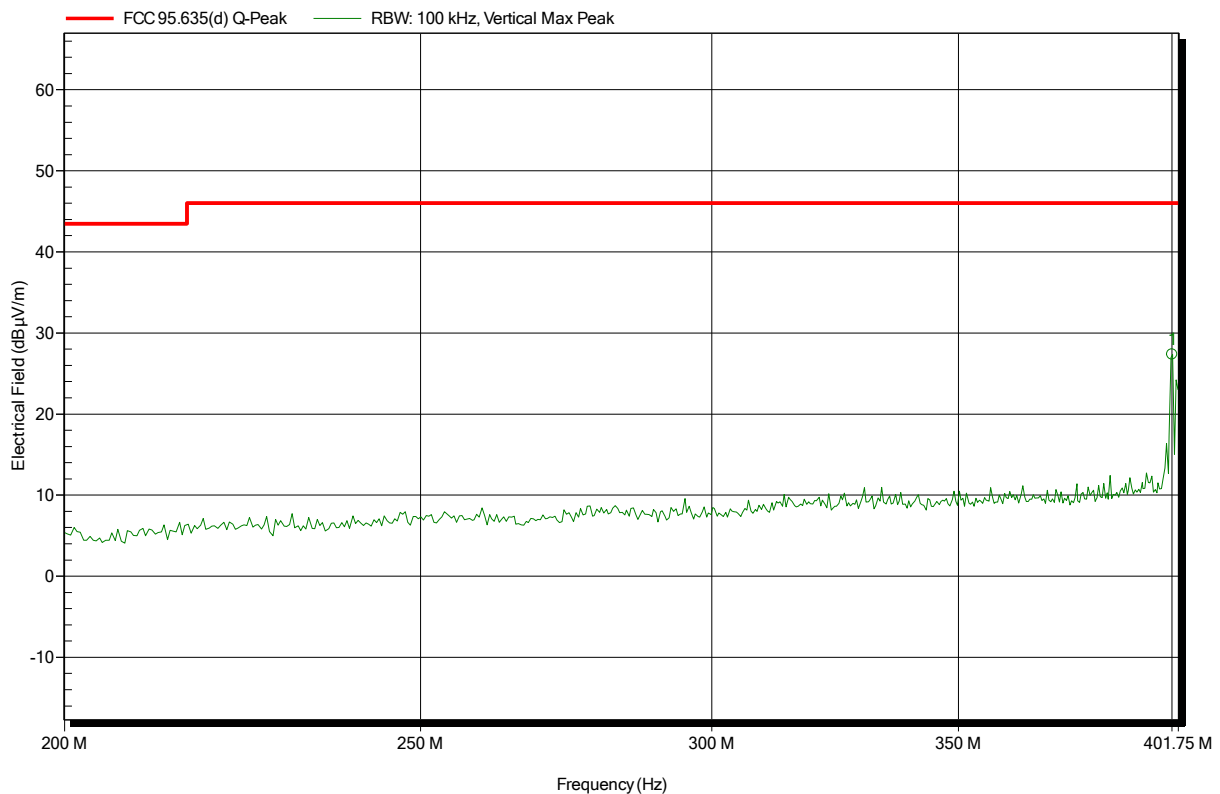


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
400.136 MHz	27.34 dBµV/m	46 dBµV/m	-18.66 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note: Band-edge

Index 72

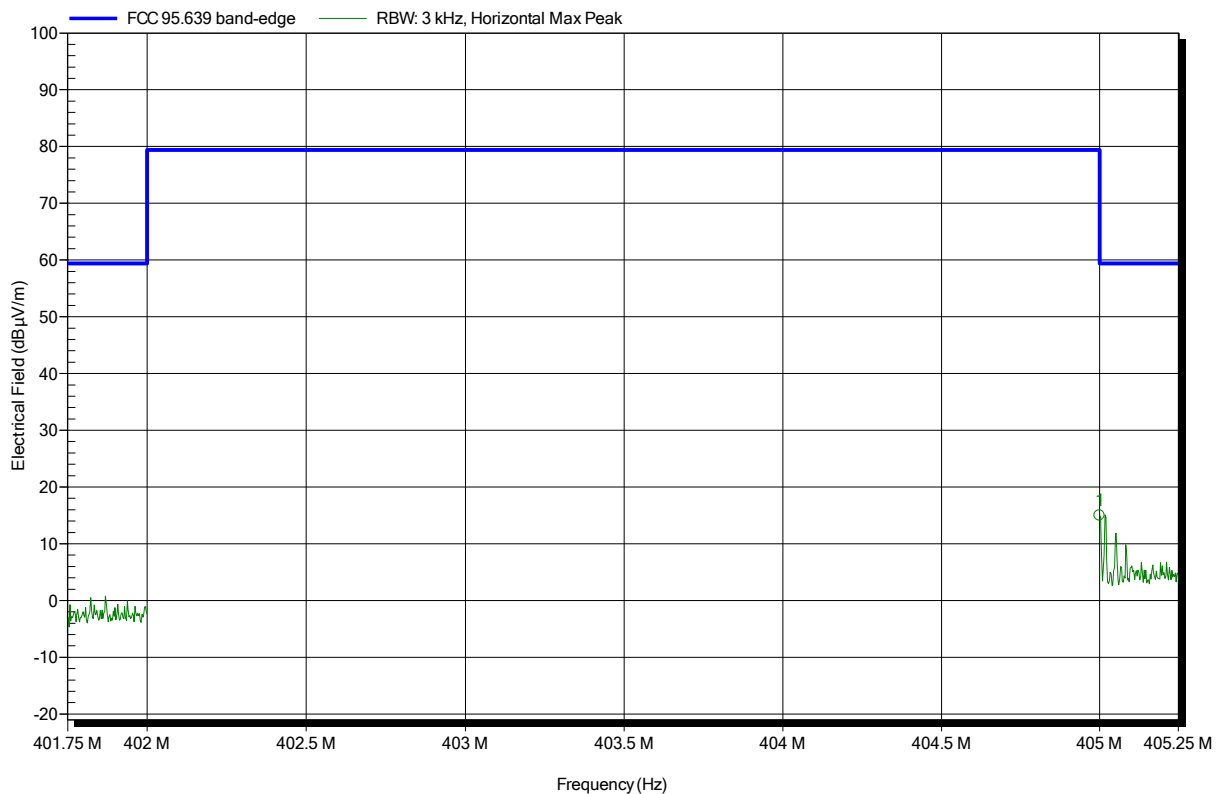


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
405 MHz	14.98 dBµV/m	59.4 dBµV/m	-44.42 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note: Band-edge

Index 76

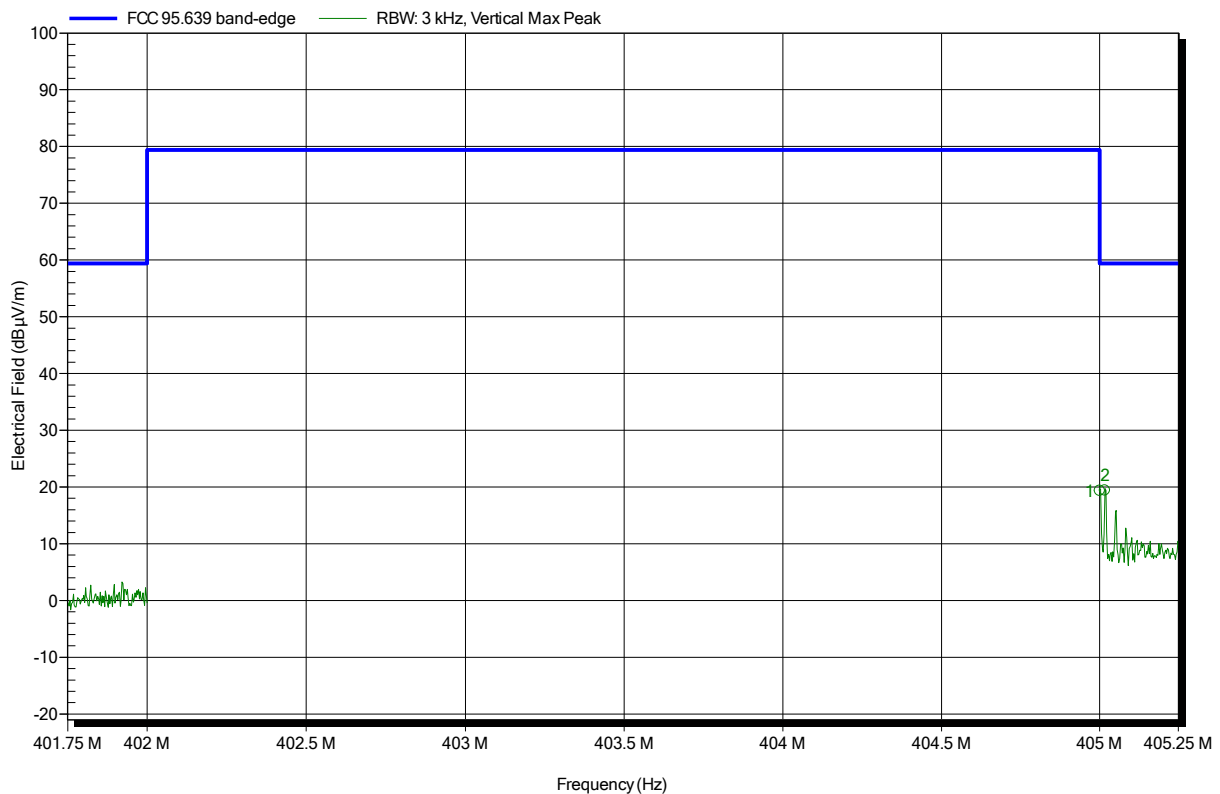


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
405.001 MHz	19.34 dBµV/m	59.4 dBµV/m	-40.06 dB	Pass
405.017 MHz	19.36 dBµV/m	59.4 dBµV/m	-40.04 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note: In-band emissions

Index 73

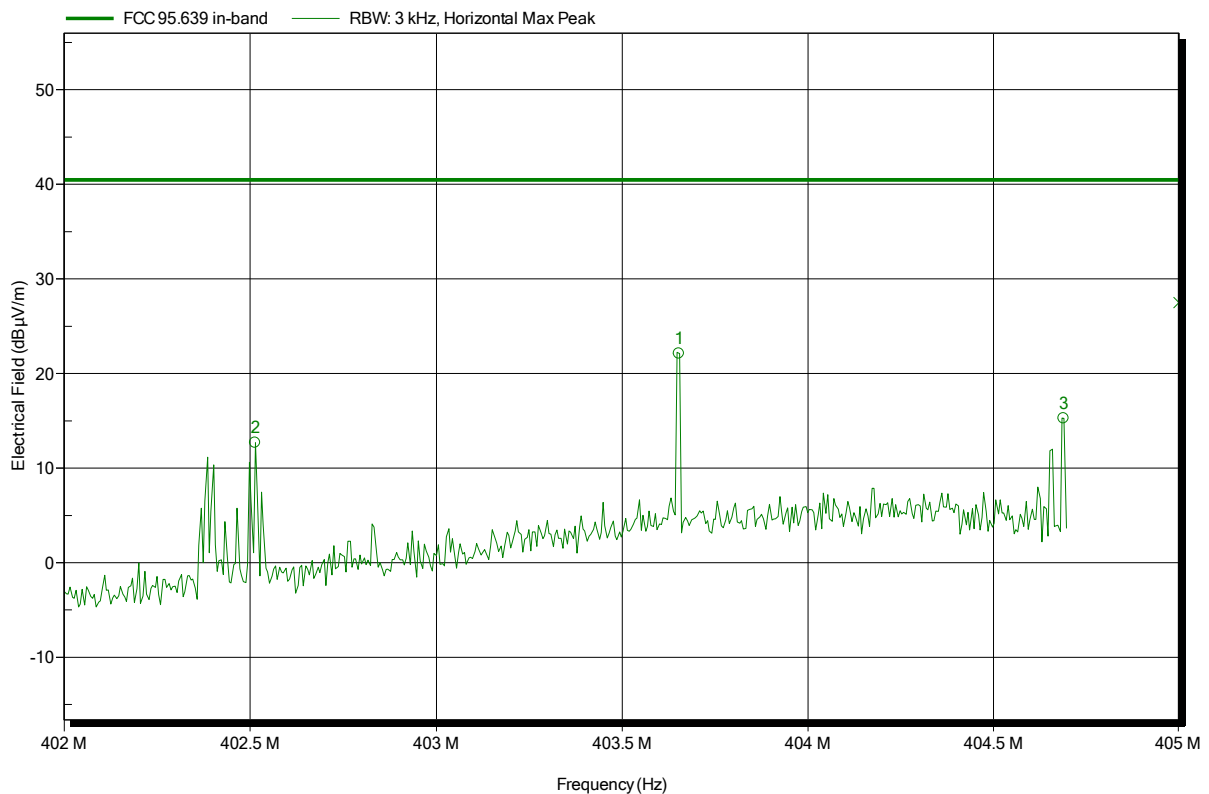

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.513 MHz	12.67 dBµV/m	40.5 dBµV/m	-27.83 dB	Pass
403.652 MHz	22.12 dBµV/m	40.5 dBµV/m	-18.38 dB	Pass
404.689 MHz	15.25 dBµV/m	40.5 dBµV/m	-25.25 dB	Pass

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note: In-band emissions

Index 77

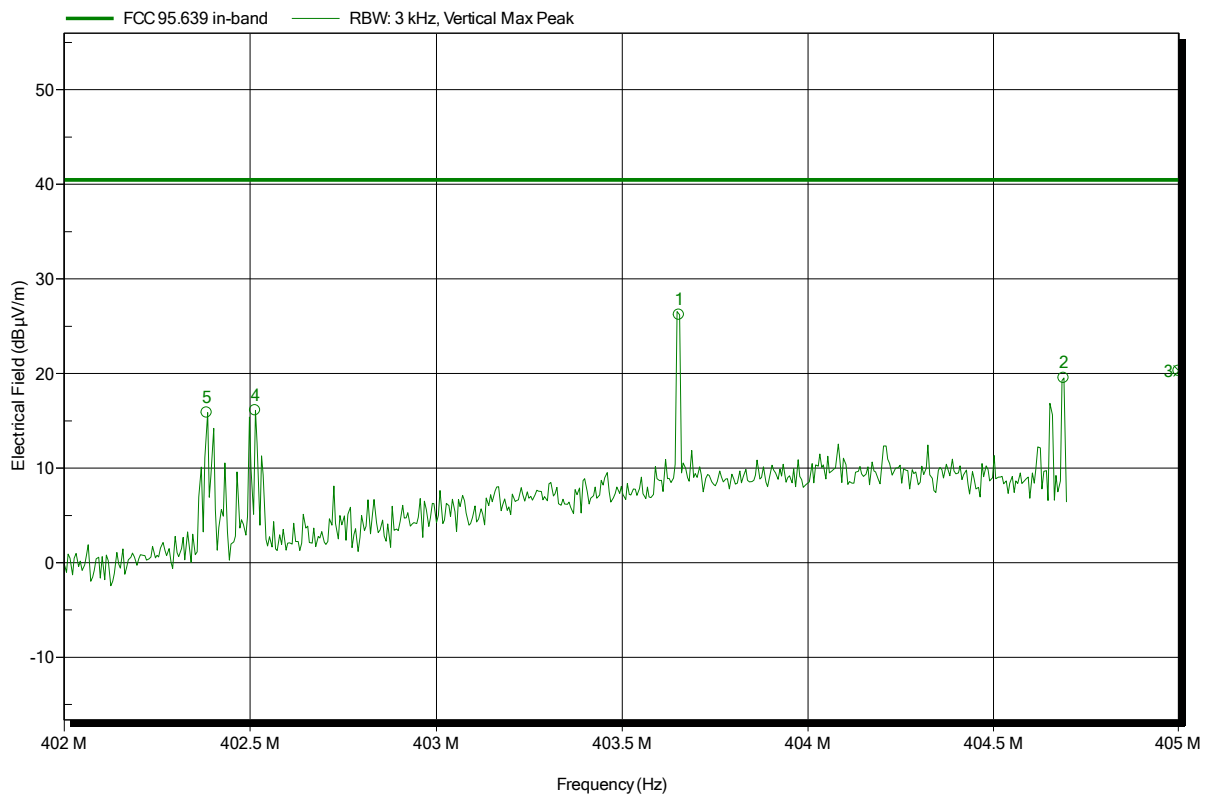

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.383 MHz	15.88 dBµV/m	40.5 dBµV/m	-24.62 dB	Pass
402.513 MHz	16.09 dBµV/m	40.5 dBµV/m	-24.41 dB	Pass
403.652 MHz	26.2 dBµV/m	40.5 dBµV/m	-14.3 dB	Pass
404.689 MHz	19.54 dBµV/m	40.5 dBµV/m	-20.96 dB	Pass
405 MHz	20.28 dBµV/m	40.5 dBµV/m	-20.22 dB	Pass

Test Report No.: G0M-1412-4360-TFC95IMR-V02


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 74

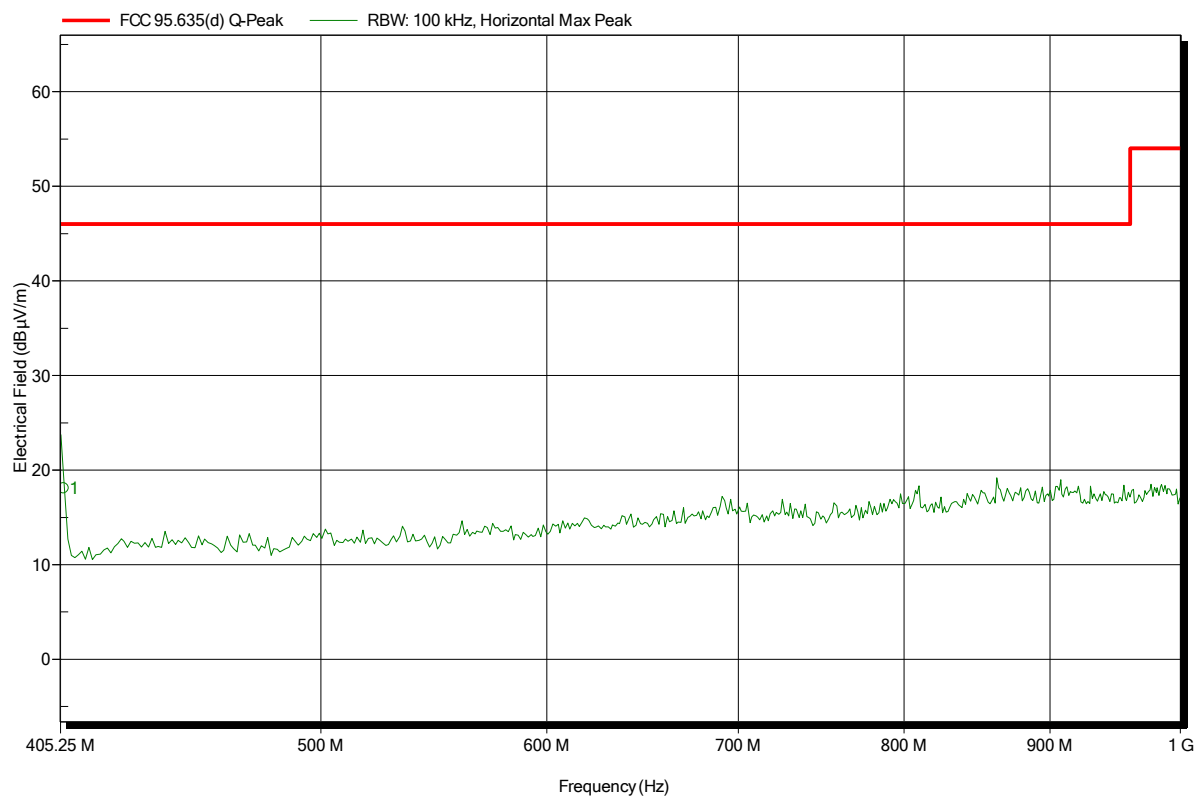


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
406.44 MHz	18.09 dBµV/m	46 dBµV/m	-27.91 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant:	BIOTRONIK SE & Co.KG
EUT Name:	ICD / Implantable Cardioverter Defibrillator
Model:	Inlexa 1
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 25°C, Vnom: 3.0 VDC lithium battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	TX; 404.85 MHz, 2FSK
Test Date:	2015-01-27
Note:	

Index 80

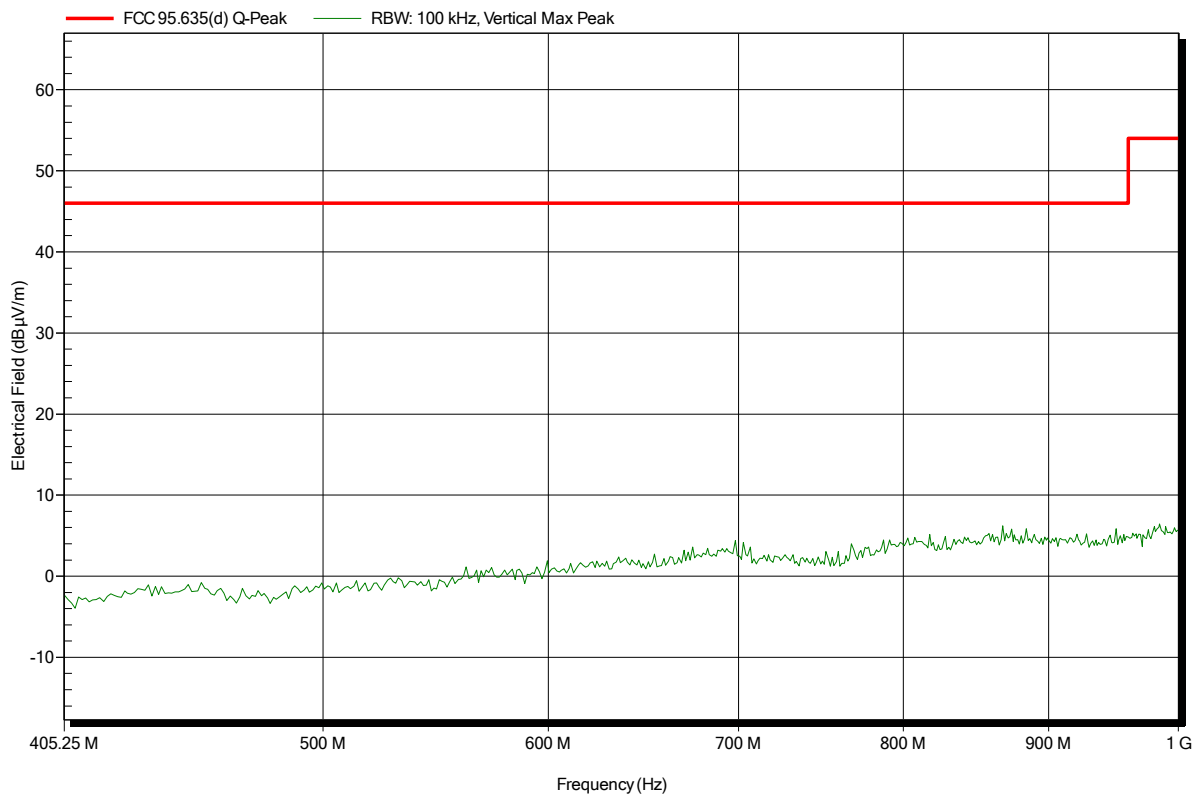


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL025, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 70

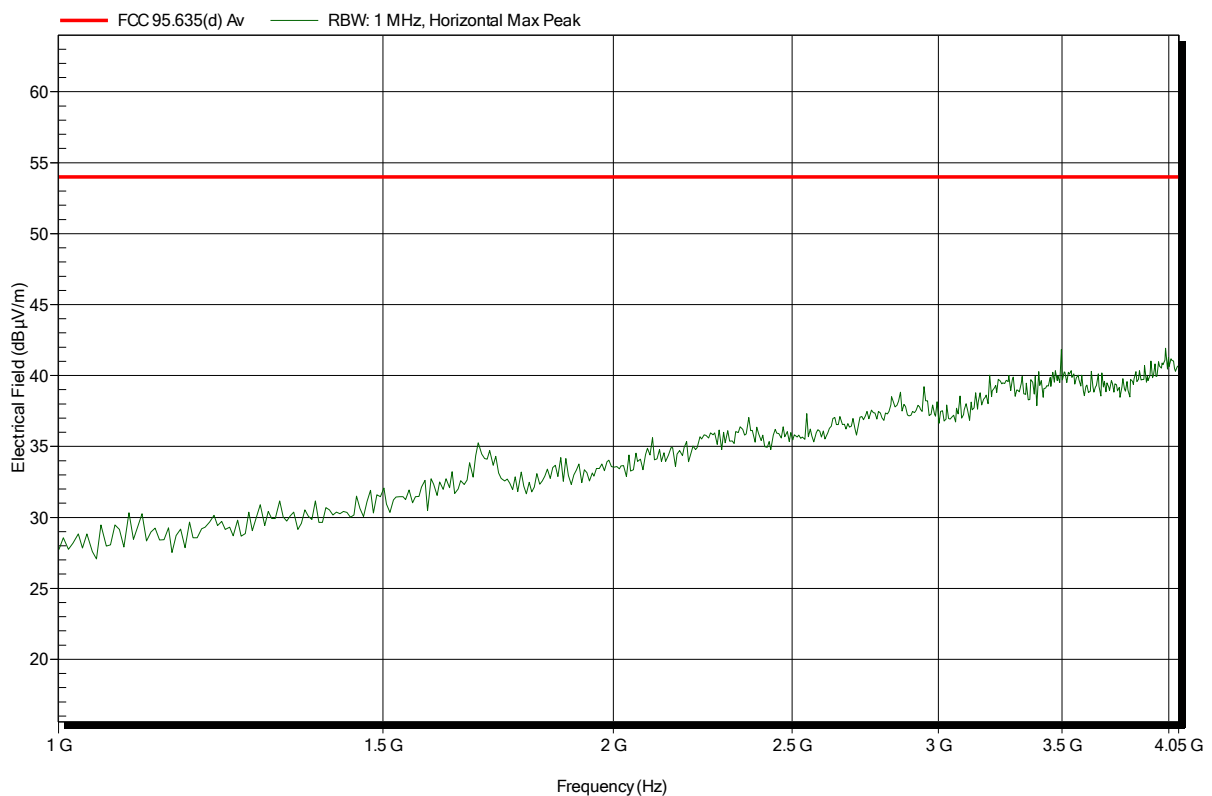


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL025, Vertical
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz, 2FSK
 Test Date: 2015-01-27
 Note:

Index 69

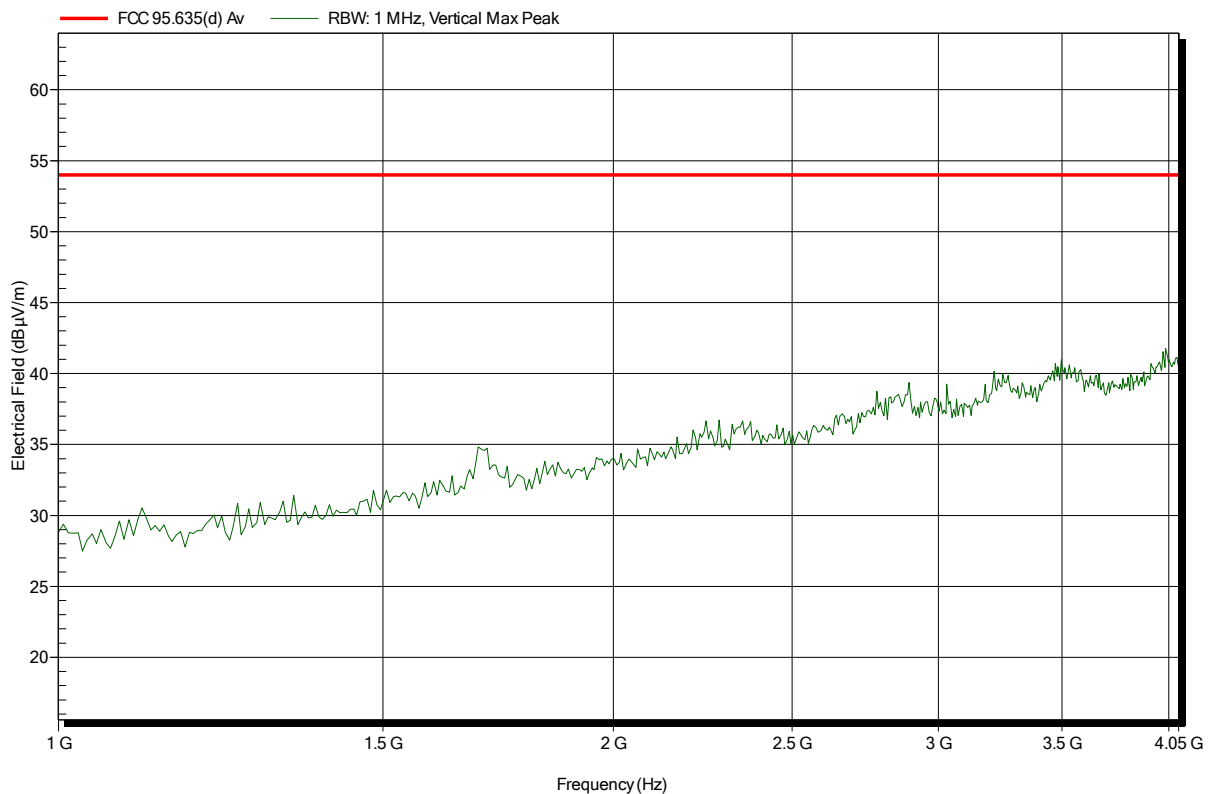


ANNEX C Receiver radiated spurious emissions

Spurious emissions according to RSS-Gen

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HK116, Horizontal
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2015-01-26
 Note:

Index 40

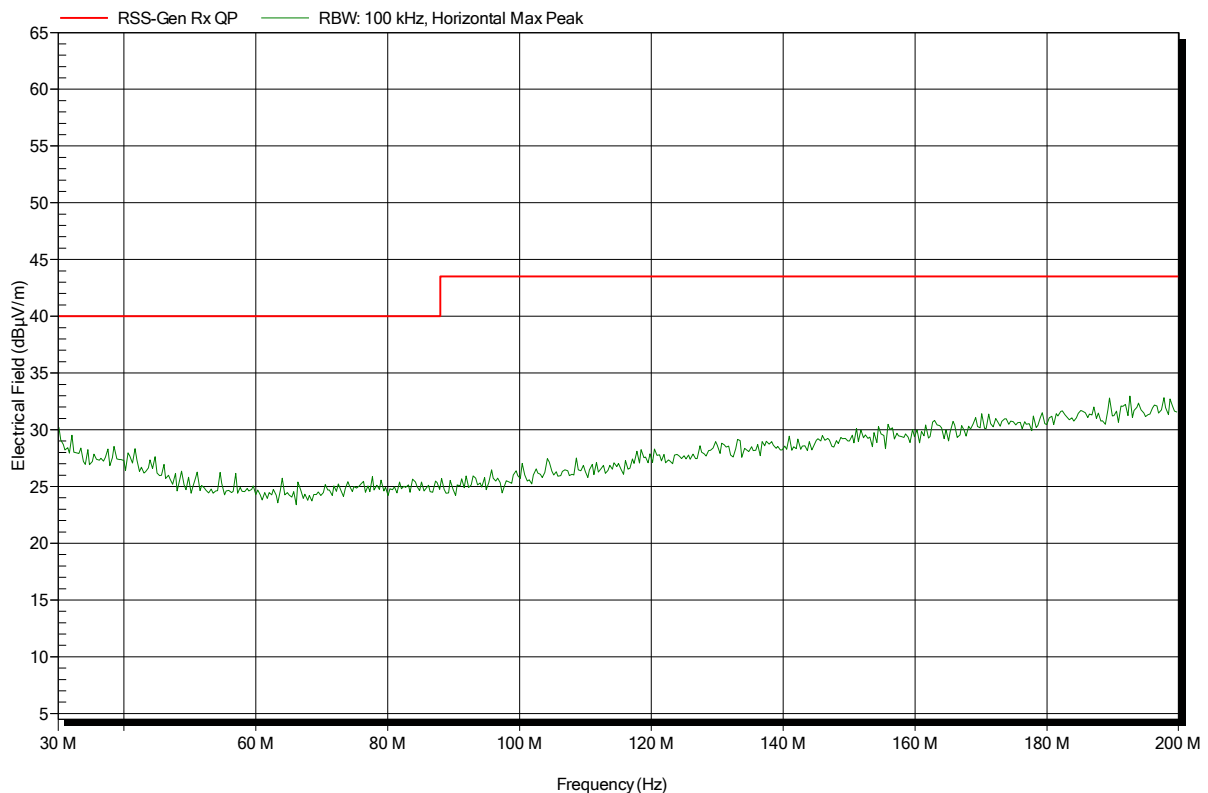


Spurious emissions according to RSS-Gen

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HK116, Vertical
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2015-01-26
 Note:

Index 41

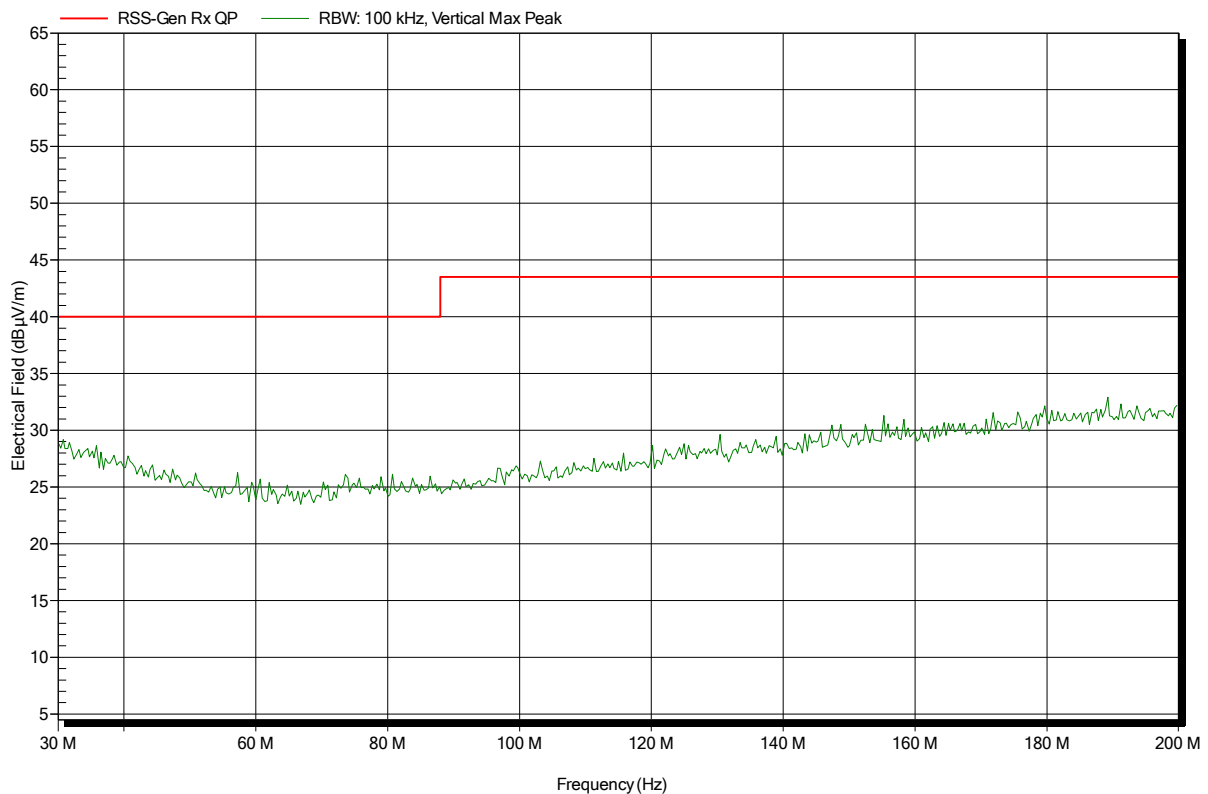


Spurious emissions according to RSS-Gen

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2015-01-26
 Note:

Index 38

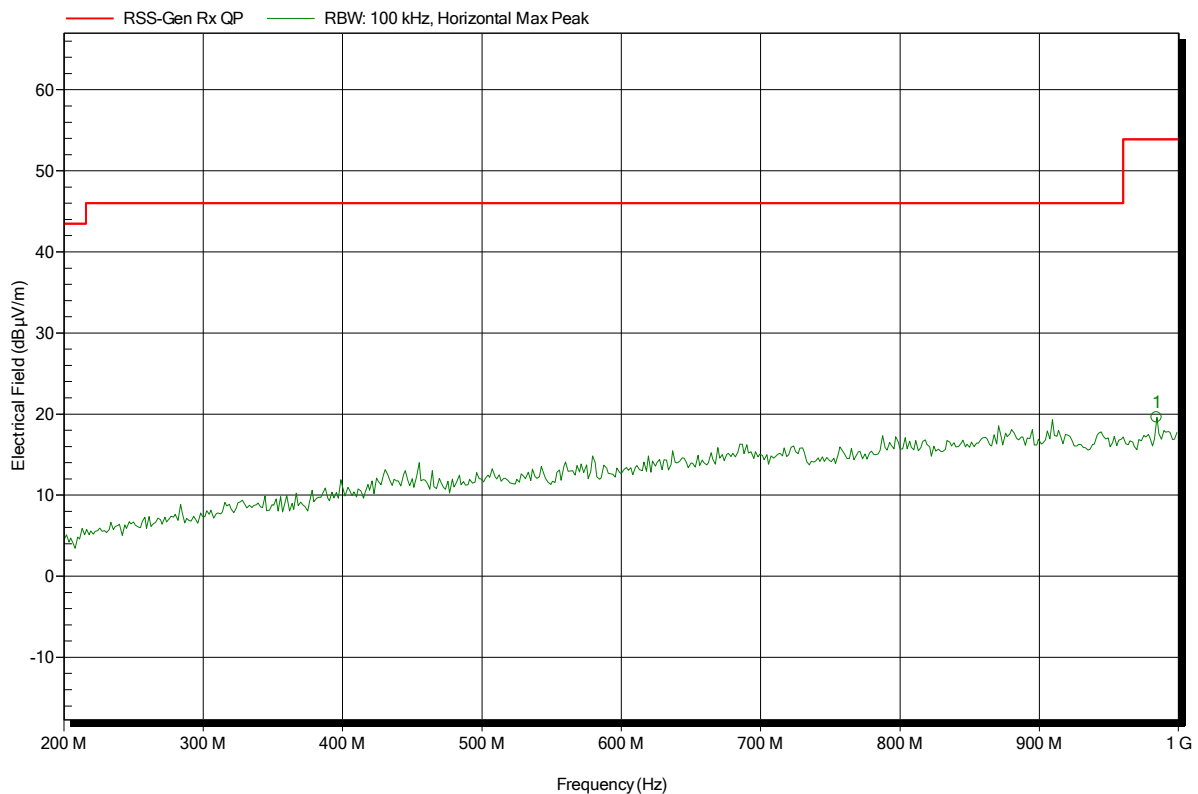


Frequency	Peak	Peak Limit	Peak Difference	Status
984 MHz	19.6 dBµV/m	53.9 dBµV/m	-34.3 dB	Pass

Spurious emissions according to RSS-Gen

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2015-01-26
 Note:

Index 39

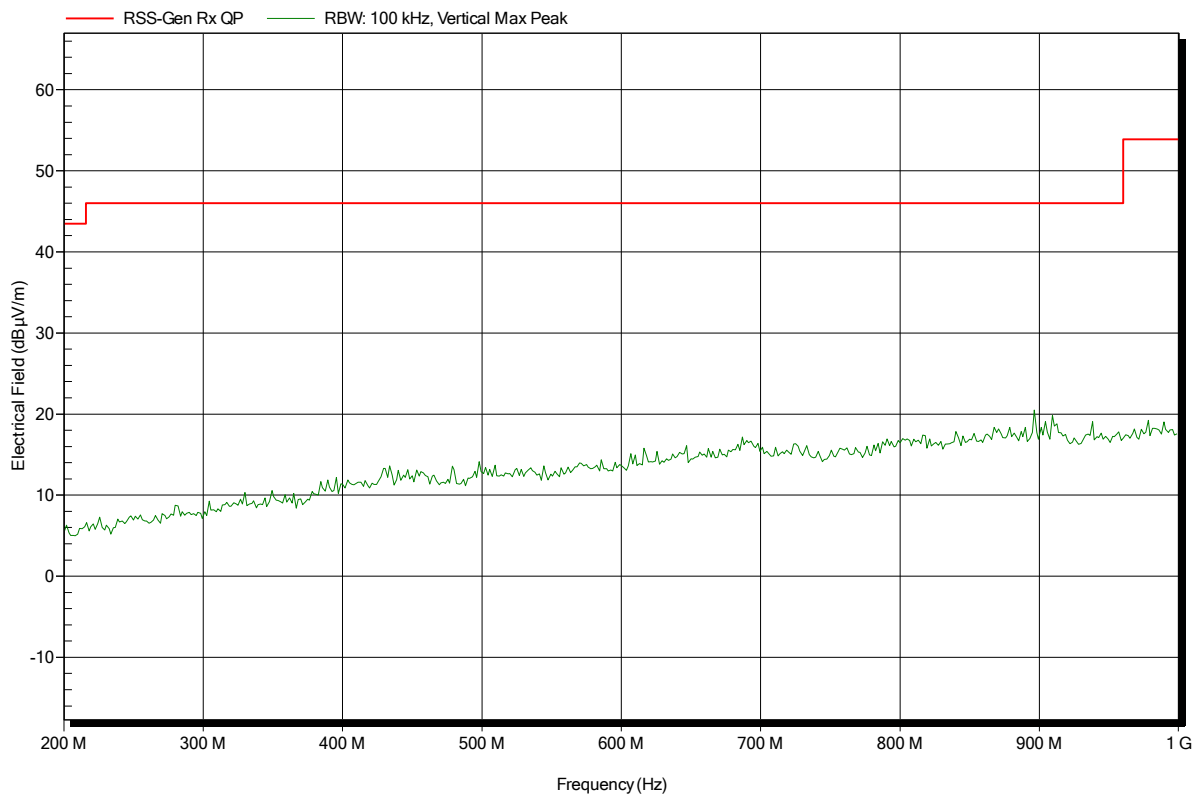


Spurious emissions according to RSS-Gen

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL025, Horizontal
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2015-01-26
 Note:

Index 42

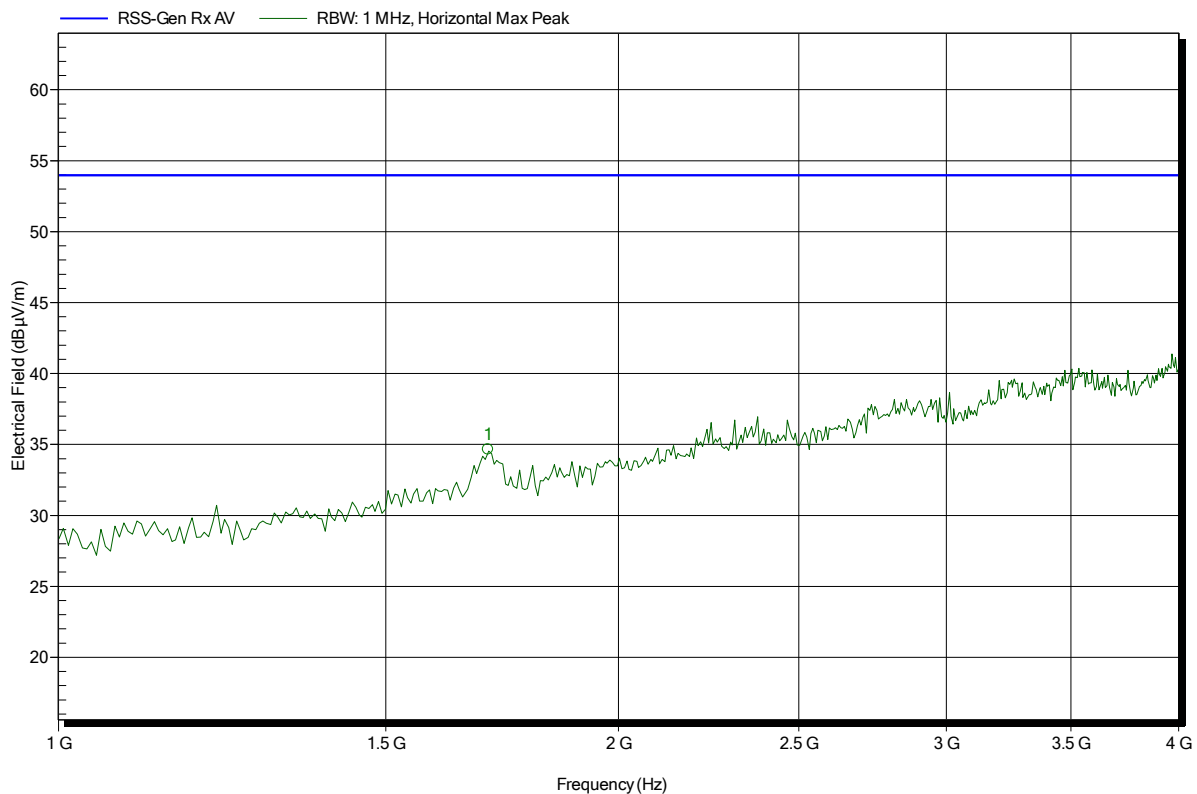


Frequency	Peak	Peak Limit	Peak Difference	Status
1.702 GHz	34.64 dBµV/m	53.98 dBµV/m	-19.34 dB	Pass

Spurious emissions according to RSS-Gen

Project number: G0M-1412-4360

Applicant: BIOTRONIK SE & Co.KG
 EUT Name: ICD / Implantable Cardioverter Defibrillator
 Model: Inlexa 1
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 25°C, Vnom: 3.0 VDC lithium battery
 Antenna: HL025, Vertical
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2015-01-26
 Note:

Index 43

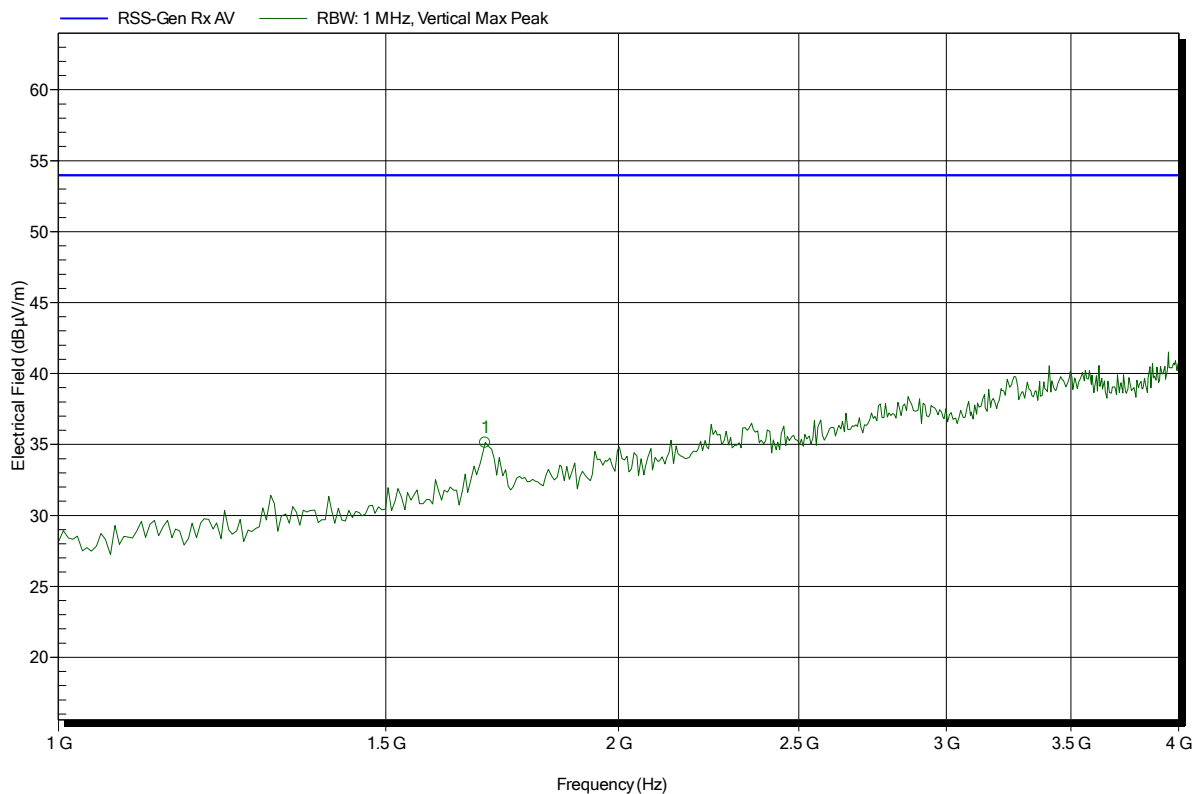

Frequency	Peak	Peak Limit	Peak Difference	Status
1.696 GHz	35.11 dBµV/m	53.98 dBµV/m	-18.87 dB	Pass