

Test Laboratory: Compliance Certification Services

File Name: [D2450V2SN748\\_ES3DV2SN3021\\_070604.da4](#)

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:748**

**Program Name: System Performance Check at 2450 MHz**

**Ambient Temp.: 24.0 deg. C; Liquid Temp.: 23.0 deg. C**

Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.99$  mho/m;  $\epsilon_r = 52.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV2 - SN3021; ConvF(4.1, 4.1, 4.1); Calibrated: 7/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 12/23/2003
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.2 Build 44; Postprocessing SW: SEMCAD, V1.8 Build 112

**d=10mm, Pin=250mW/Area Scan (7x7x1):** Measurement grid: dx=15mm, dy=15mm

Reference Value = 87.4 V/m; Power Drift = 0.0 dB

Maximum value of SAR (measured) = 14.4 mW/g


**d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 87.4 V/m; Power Drift = 0.0 dB

Maximum value of SAR (measured) = 14.3 mW/g

Peak SAR (extrapolated) = 25.1 W/kg

**SAR(1 g) = 12.8 mW/g; SAR(10 g) = 6.02 mW/g**

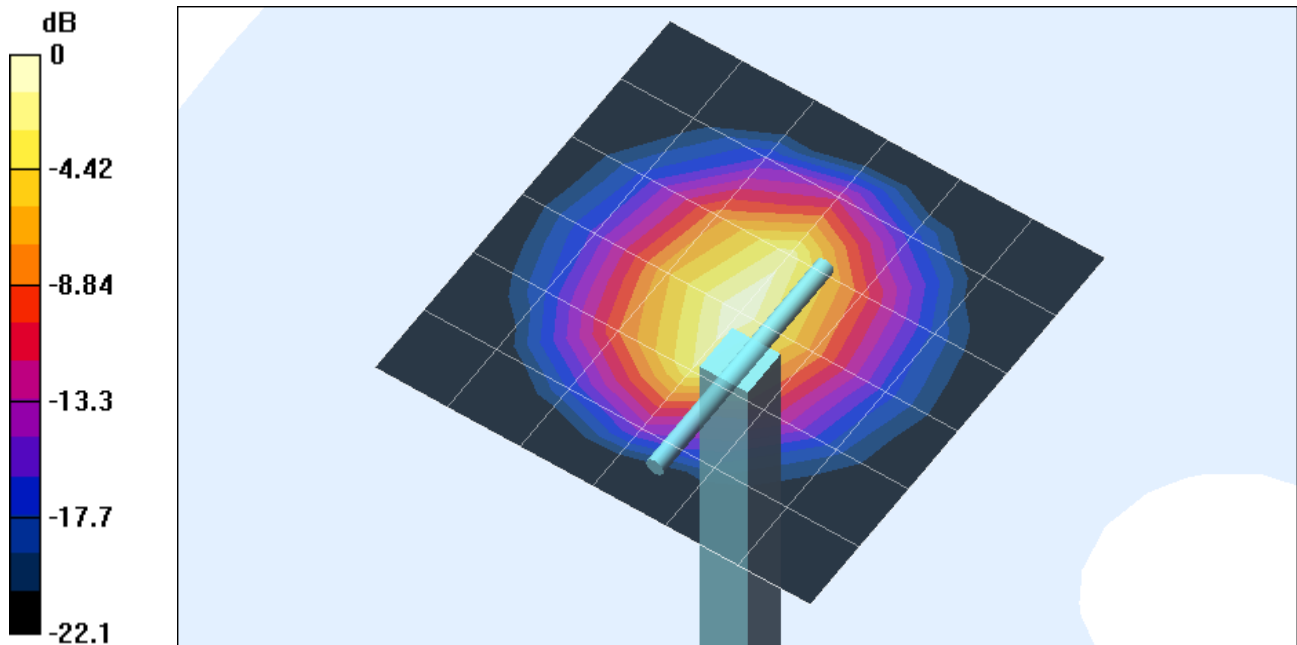

0 dB = 14.3mW/g

Test Laboratory: Compliance Certification Services

File Name: [D2450V2SN748\\_ES3DV2SN3021\\_070604.da4](#)

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:748**

**Program Name: System Performance Check at 2450 MHz**

Communication System: CW - 2450 MHz; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.99$  mho/m;  $\epsilon_r = 52.9$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

**d=10mm, Pin=250mW/Z Scan (1x1x51):** Measurement grid: dx=20mm, dy=20mm, dz=2mm

Reference Value = 87.4 V/m; Power Drift = 0.0 dB

Maximum value of SAR (measured) = 14.6 mW/g

