


## APPENDIX

### 01. Photographs of Test Setup




**Fig.1 Photograph of the SAR measurement system**

**Photograph of the tissue simulant fluid liquid depth (Body)**

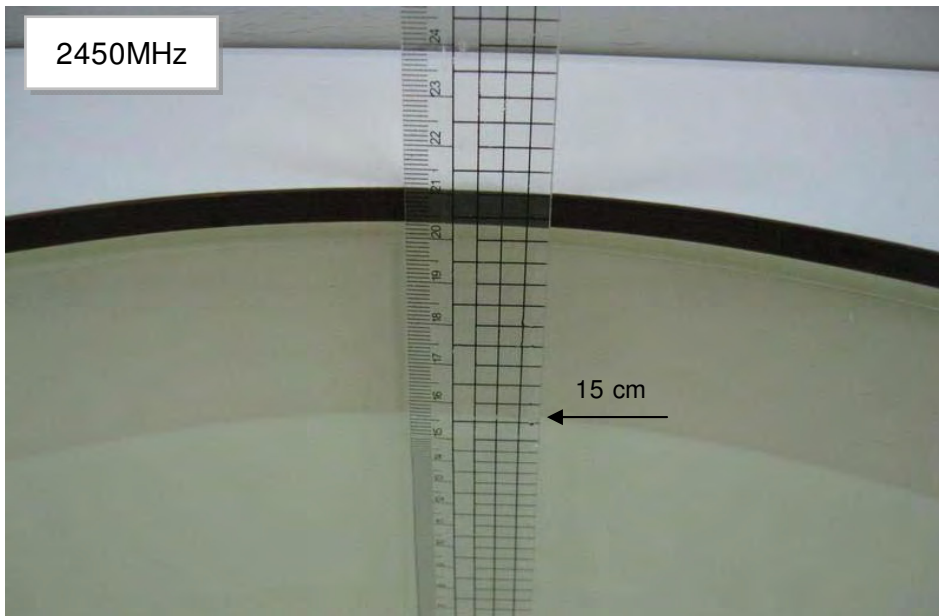


**Fig.2.1**

**Body - distance between flat phantom and EUT is 0 mm**

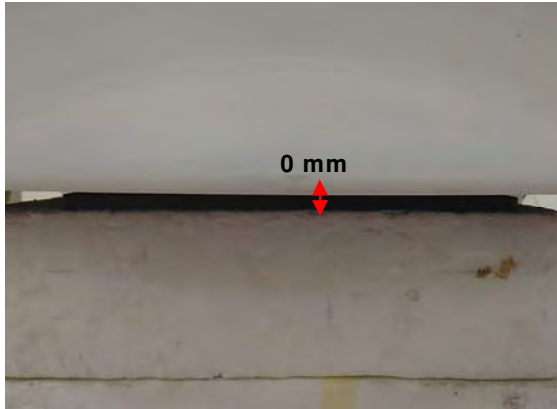

**Fig.3 EUT Back side to flat phantom**

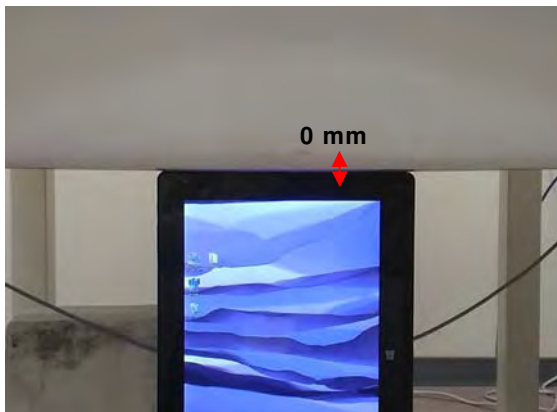

**Fig.4 EUT Right side to flat phantom**


## 11. Photographs of the EUT



**Fig.5 Front view of EUT**



**Fig.6 Back view of EUT**

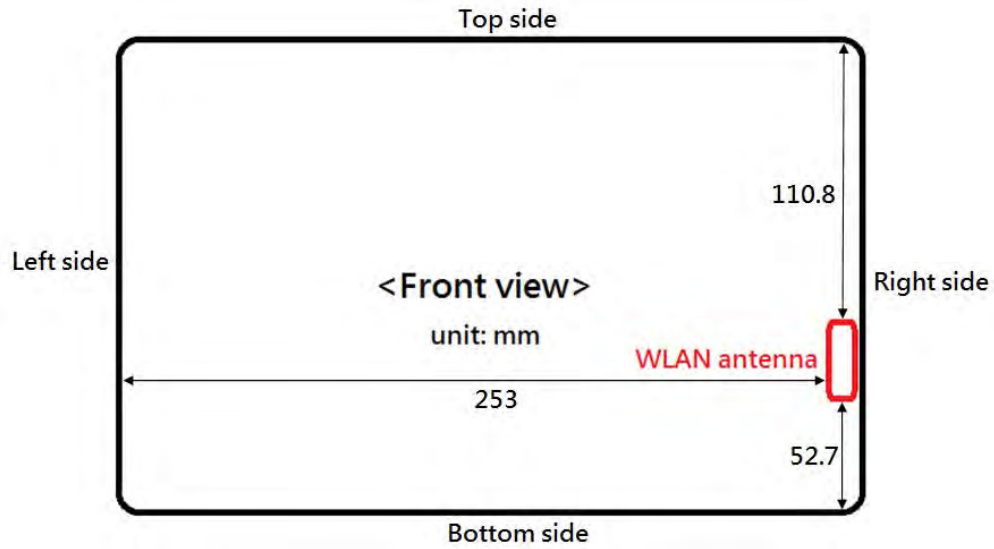

**Fig.7 Antenna position of EUT (Front view)**

**- End of Report -**