
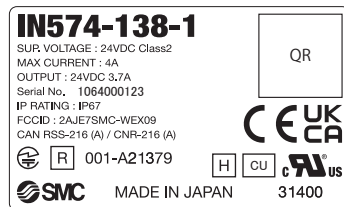


* JP/US


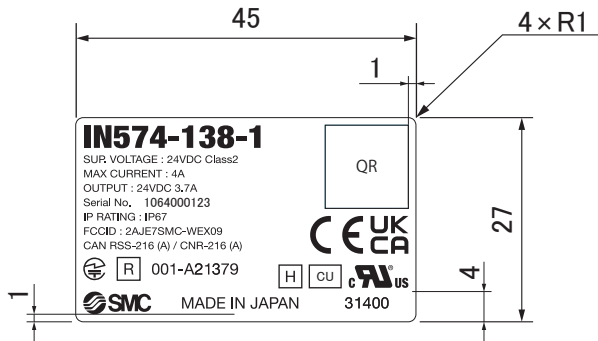


Unit: mm

The label is placed at the rear side of the device.

The label is permanently affixed on the device with an acrylic type adhesive.

* JP/US

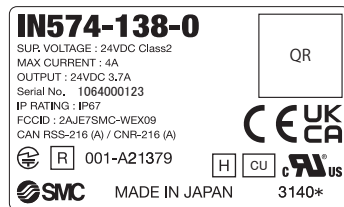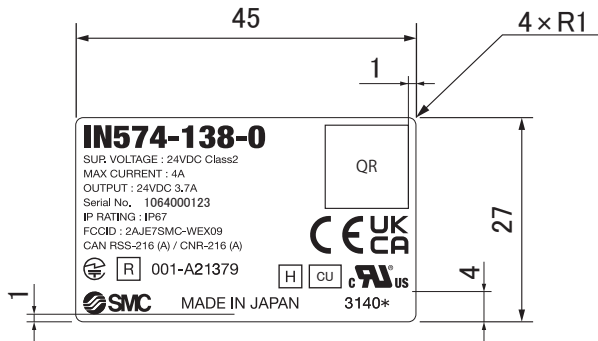

Unit: mm

The label is placed at the rear side of the device.

The label is permanently affixed on the device with an acrylic type adhesive.