

# Probe ET3DV6

SN:1559

Manufactured:	December 1, 2000
Last calibrated:	April 16, 2003
Recalibrated:	July 18, 2004

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1559

July 18, 2004

**DASY - Parameters of Probe: ET3DV6 SN:1559****Sensitivity in Free Space****Diode Compression<sup>A</sup>**

NomX	<b>1.76</b> $\mu\text{V}/(\text{V}/\text{m})^2$
NomY	<b>1.56</b> $\mu\text{V}/(\text{V}/\text{m})^2$
NomZ	<b>1.71</b> $\mu\text{V}/(\text{V}/\text{m})^2$

DCP X	<b>94</b>	mV
DCP Y	<b>94</b>	mV
DCP Z	<b>94</b>	mV

**Sensitivity in Tissue Simulating Liquid (Conversion Factors)**

Please see Page 7.

**Boundary Effect****Head**                      **900 MHz**      Typical SAR gradient: 5 % per mm

Sensor Center to Phantom Surface Distance		<b>3.7 mm</b>	<b>4.7 mm</b>
SAR <sub>ref</sub> [%]	Without Correction Algorithm	8.5	4.7
SAR <sub>ref</sub> [%]	With Correction Algorithm	0.0	0.1

**Head**                      **1750 MHz**      Typical SAR gradient: 10 % per mm

Sensor Center to Phantom Surface Distance		<b>3.7 mm</b>	<b>4.7 mm</b>
SAR <sub>ref</sub> [%]	Without Correction Algorithm	12.2	7.7
SAR <sub>ref</sub> [%]	With Correction Algorithm	0.0	0.3

**Sensor Offset**

Probe Tip to Sensor Center	<b>2.7</b> mm
Optical Surface Detection	<b>in tolerance</b>


The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> numerical linearization parameter, uncertainty not required

ET3DV6 SN:1559

July 18, 2004


**Frequency Response of E-Field**  
( TEM-Cell:ifi110, Waveguide R22)

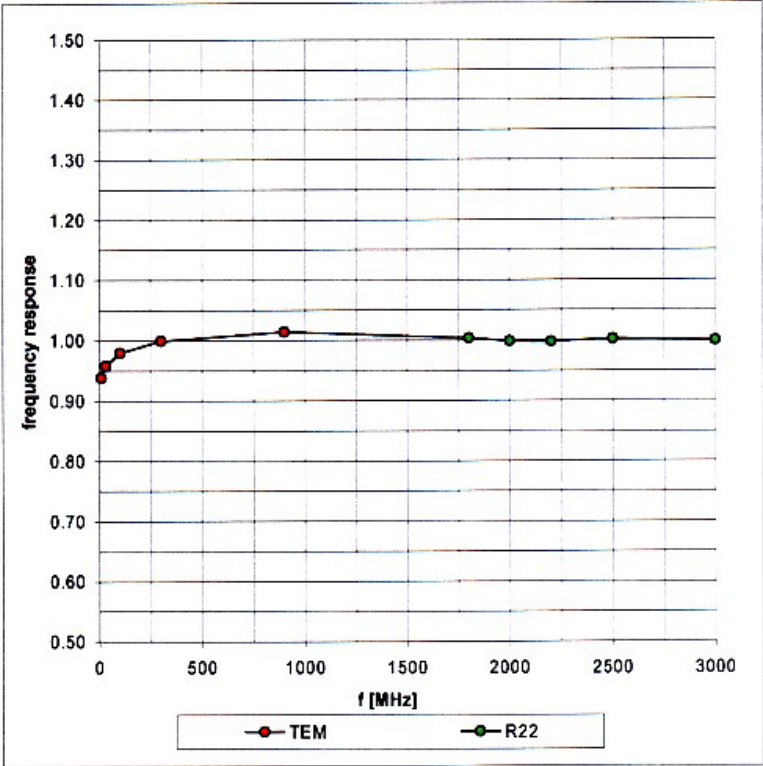

ET3DV6 SN:1559

July 18, 2004

Receiving Pattern ( $\phi$ ),  $\theta = 0^\circ$

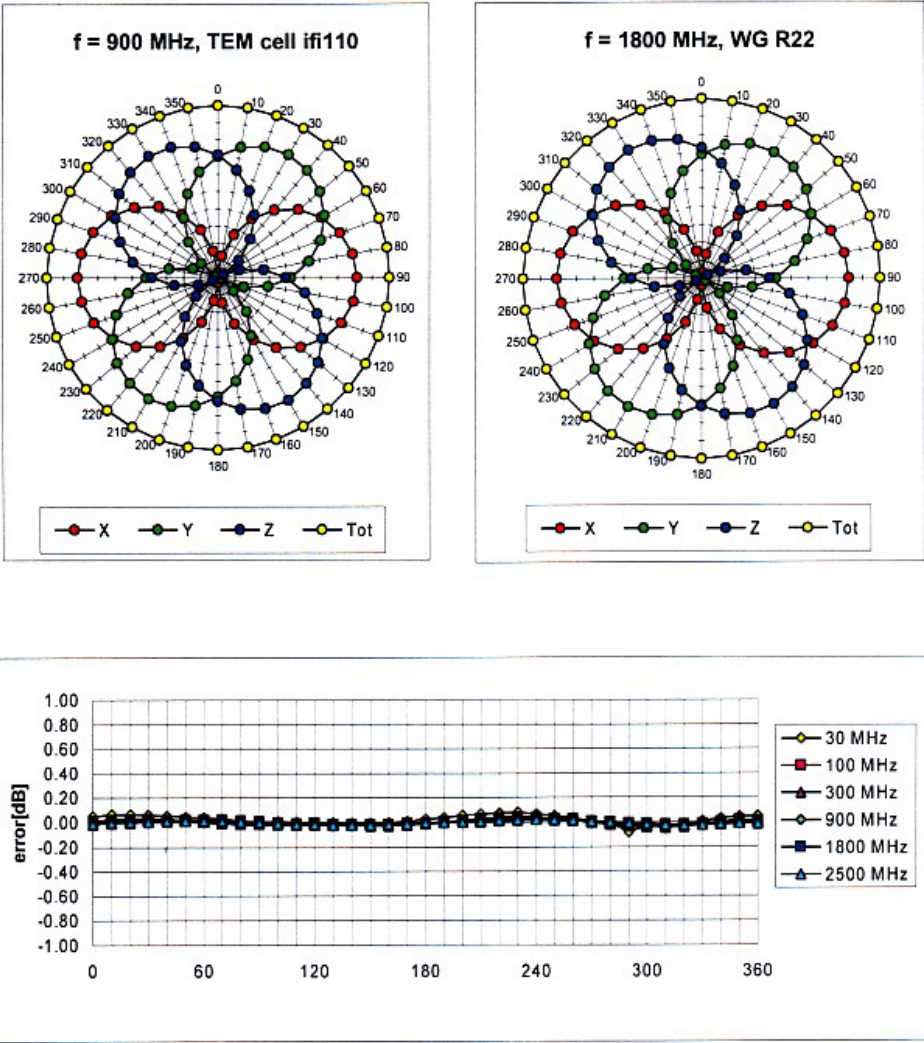


Axial Isotropy Error  $< \pm 0.2 \text{ dB}$

ET3DV6 SN:1559

July 18, 2004

Dynamic Range f(SAR<sub>head</sub>)  
( Waveguide R22 )


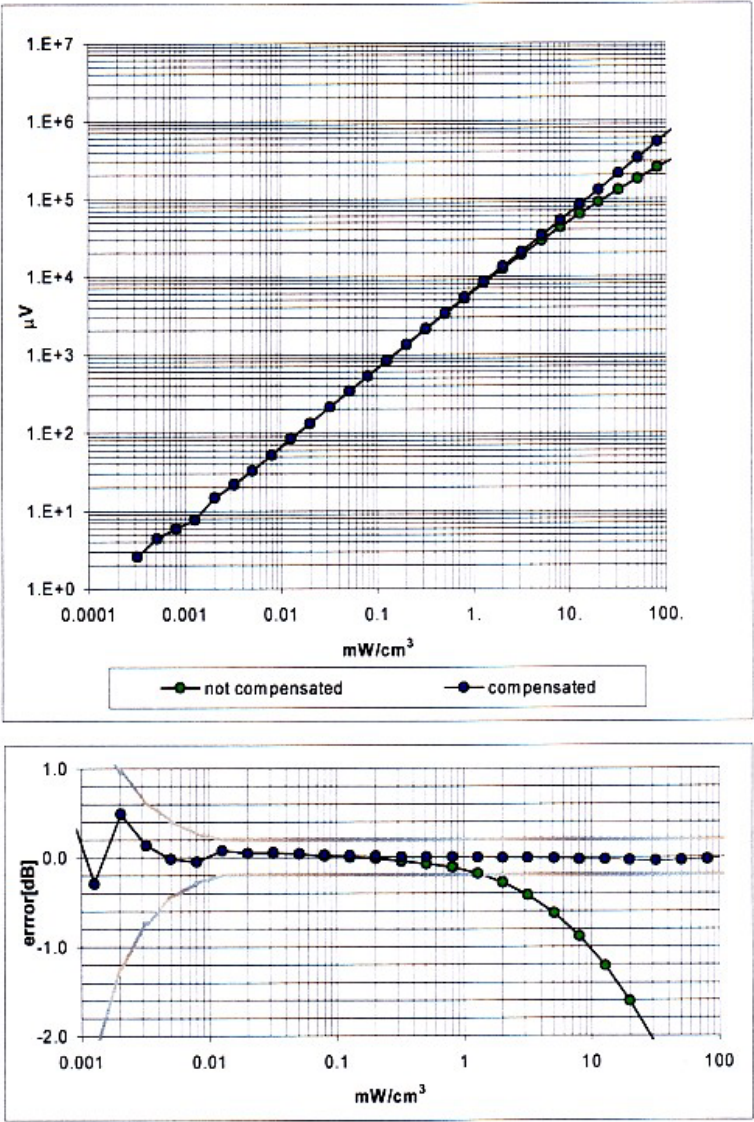


Probe Linearity Error <  $\pm 0.2$  dB

ET3DV6 SN:1559

July 18, 2004

## Conversion Factor Assessment

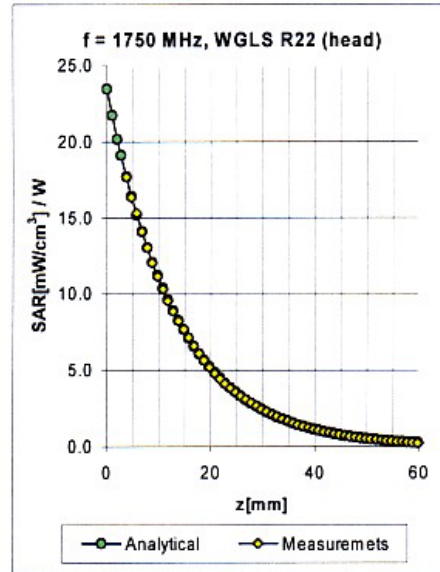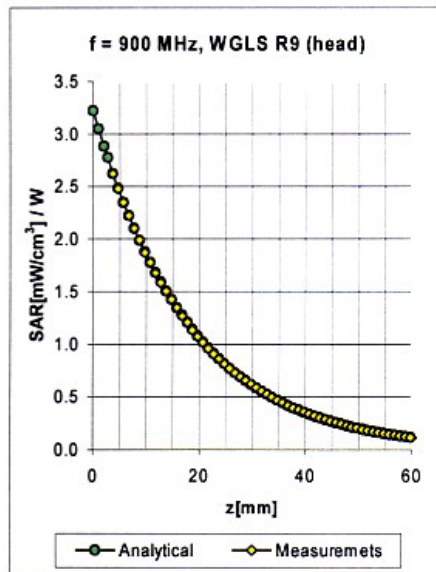


f [MHz]	Validity [MHz] <sup>B</sup>	Tissue	Permittivity	Conductivity	Alpha	Depth	ConvF	Uncertainty
900	850-950	Head	41.5 ± 5%	0.97 ± 5%	0.53	1.93	6.59 ± 9.7% (k=2)	
1750	1700-1800	Head	40.0 ± 5%	1.40 ± 5%	0.46	2.58	5.37 ± 9.7% (k=2)	
1900	1850-1950	Head	40.0 ± 5%	1.40 ± 5%	0.48	2.79	5.13 ± 9.7% (k=2)	
2450	2400-2500	Head	39.2 ± 5%	1.80 ± 5%	0.81	1.92	4.56 ± 9.7% (k=2)	
450	400-500	Body	56.7 ± 5%	0.94 ± 5%	0.29	2.46	7.13 ± 15.5% (k=2)	
900	850-950	Body	55.0 ± 5%	1.05 ± 5%	0.46	2.26	6.21 ± 9.7% (k=2)	
1750	1700-1800	Body	53.3 ± 5%	1.52 ± 5%	0.48	2.94	4.60 ± 9.7% (k=2)	
1900	1850-1950	Body	53.3 ± 5%	1.52 ± 5%	0.53	2.90	4.40 ± 9.7% (k=2)	
2450	2400-2500	Body	52.7 ± 5%	1.95 ± 5%	1.11	1.55	4.21 ± 9.7% (k=2)	

<sup>B</sup> The total standard uncertainty is calculated as root-sum-square of standard uncertainty of the Conversion Factor at calibration frequency and the standard uncertainty for the indicated frequency band.

ET3DV6 SN:1559

July 18, 2004

**Deviation from Isotropy in HSL**  
Error ( $\theta, \phi$ ),  $f = 900\text{ MHz}$

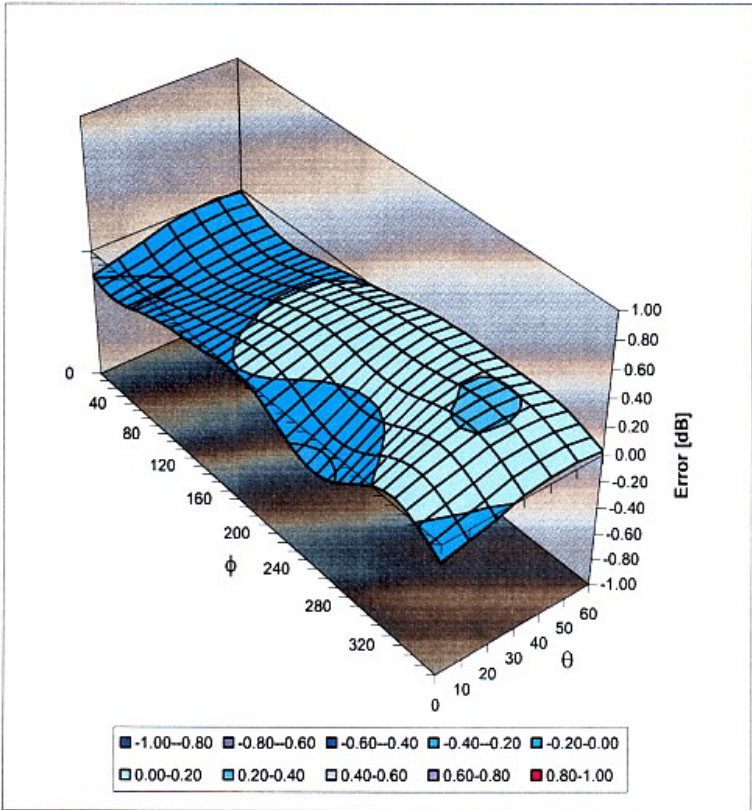



**Spherical Isotropy Error  $< \pm 0.4\text{ dB}$**

### 3 Calibration report "900 MHz System validation dipole"

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland

Client **Cetecomm**

CALIBRATION CERTIFICATE			
Object(s)	D900V2 - SN:102		
Calibration procedure(s)	QA CAL-05.v2 Calibration procedure for dipole validation kits		
Calibration date:	February 4, 2003		
Condition of the calibrated item	In Tolerance (according to the specific calibration document)		
This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.			
All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.			
Calibration Equipment used (M&TE critical for calibration)			
Model Type	ID #	Cal Date	Scheduled Calibration
RF generator HP 8684C	US3642U01700	4-Aug-99 (in house check Aug-02)	In house check: Aug-05
Power sensor E4412A	MY41495277	8-Mar-02	Mar-03
Power sensor HP 8481A	MY41092180	18-Sep-02	Sep-03
Power meter EPM E4419B	GB41293874	13-Sep-02	Sep-03
Network Analyzer HP 8753E	US38432426	3-May-00	In house check: May 03
Fluke Process Calibrator Type 702	SN: 6295803	3-Sep-01	Sep-03
Calibrated by:	Name Nico Vetterli	Function Technician	Signature 
Approved by:	Katja Pokovic	Laboratory Director	
Date issued: February 7, 2003			
This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.			

**Schmid & Partner  
Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

**DASY**

**Dipole Validation Kit**

**Type: D900V2**

**Serial: 102**

**Manufactured: January 24, 2001**

**Calibrated: February 4, 2003**

## **1. Measurement Conditions**

The measurements were performed in the flat section of the SAM twin phantom filled with head simulating solution of the following electrical parameters at 900 MHz:

Relative Dielectricity	<b>40.8</b>	$\pm 5\%$
Conductivity	<b>0.95 mho/m</b>	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.6 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was  $250\text{mW} \pm 3\%$ . The results are normalized to 1W input power.

## **2. SAR Measurement with DASY4 System**

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over $1\text{ cm}^3$ (1 g) of tissue:	<b>10.6 mW/g</b>
averaged over $10\text{ cm}^3$ (10 g) of tissue:	<b>6.68 mW/g</b>

### **3. Dipole Impedance and Return Loss**

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:	<b>1.405 ns</b>	(one direction)
Transmission factor:	<b>0.999</b>	(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 900 MHz:	$\text{Re}\{Z\} = 49.6 \Omega$
	$\text{Im}\{Z\} = -4.9 \Omega$
Return Loss at 900 MHz	<b>-26.3 dB</b>

### **4. Measurement Conditions**

The measurements were performed in the flat section of the SAM twin phantom filled with body simulating solution of the following electrical parameters at 900 MHz:

Relative Dielectricity	<b>53.5</b>	$\pm 5\%$
Conductivity	<b>1.03 mho/m</b>	$\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.3 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was 250mW  $\pm 3\%$ . The results are normalized to 1W input power.



Date/Time: 02/07/03 17:05:43

Test Laboratory: SPEAG, Zurich, Switzerland  
File Name: SN102\_SN1507\_HSL900\_030203.da4


**DUT: Dipole 900 MHz** Type & Serial Number: D900V2 - SN102  
**Program: Dipole Calibration; Pin = 250 mW; d = 15 mm**


Communication System: CW-900; Frequency: 900 MHz; Duty Cycle: 1:1  
Medium: HSL 900 MHz ( $\sigma = 0.95$  mho/m,  $\epsilon = 40.75$ ,  $\rho = 1000$  kg/m<sup>3</sup>)  
Phantom section: FlatSection

**DASY4 Configuration:**

- Probe: ET3DV6 - SN1507; ConvF(6.6, 6.6, 6.6); Calibrated: 1/18/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 - SN410; Calibrated: 1/14/2003
- Phantom: SAM 4.0 - TP:1006
- Software: DASY4, V4.0 Build 51

**Area Scan (81x81x1):** Measurement grid: dx=15mm, dy=15mm  
**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm  
Reference Value = 57.2 V/m  
Peak SAR = 3.94 mW/g  
SAR(1 g) = 2.64 mW/g; SAR(10 g) = 1.67 mW/g  
Power Drift = 0.005 dB

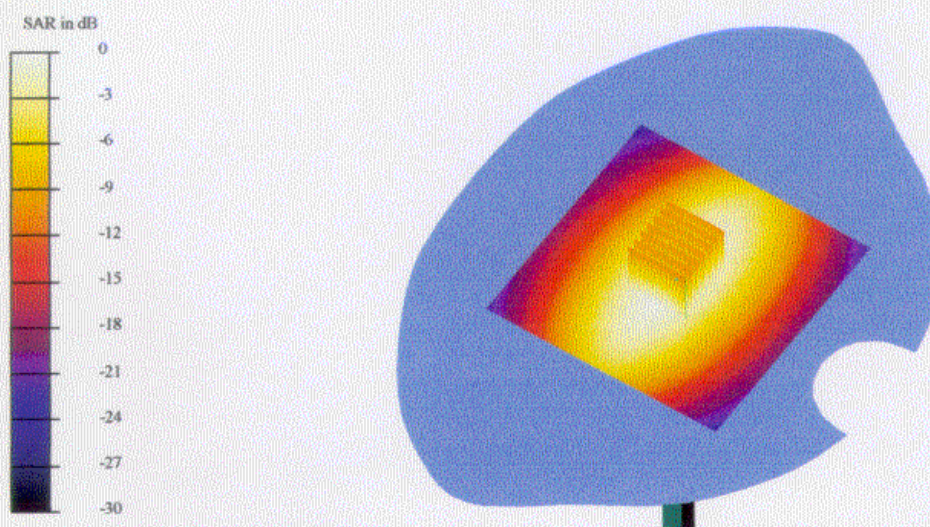

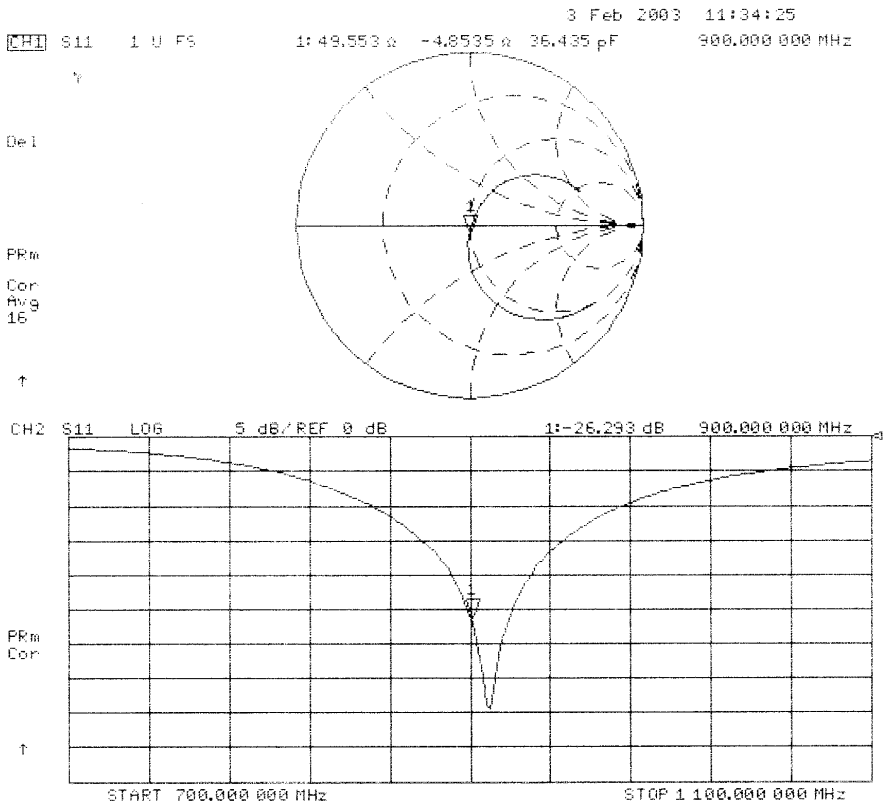

Date/Time: 02/07/03 17:14:19

Test Laboratory: SPEAG, Zurich, Switzerland  
File Name: SN102\_SN1507\_M900\_040203.da4


**DUT: Dipole 900 MHz** Type & Serial Number: D900V2 - SN102  
**Program: Dipole Calibration; Pin = 250 mW; d = 15 mm**


Communication System: CW-900; Frequency: 900 MHz; Duty Cycle: 1:1  
Medium: Muscle 900 MHz ( $\sigma = 1.03$  mho/m,  $\epsilon = 53.48$ ,  $\rho = 1000$  kg/m<sup>3</sup>)  
Phantom section: FlatSection

**DASY4 Configuration:**

- Probe: ET3DV6 - SN1507; ConvF(6.3, 6.3, 6.3); Calibrated: 1/18/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 - SN410; Calibrated: 1/14/2003
- Phantom: SAM 4.0 - TP:1006
- Software: DASY4, V4.0 Build 51

**Area Scan (81x81x1):** Measurement grid: dx=15mm, dy=15mm  
**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm  
Reference Value = 56.3 V/m  
Peak SAR = 4.07 mW/g  
SAR(1 g) = 2.77 mW/g; SAR(10 g) = 1.77 mW/g  
Power Drift = -0.0008 dB

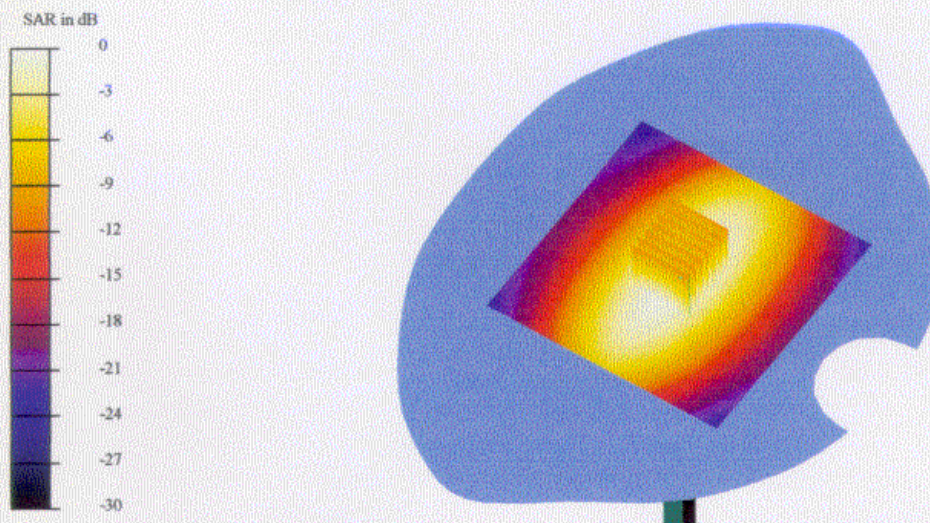

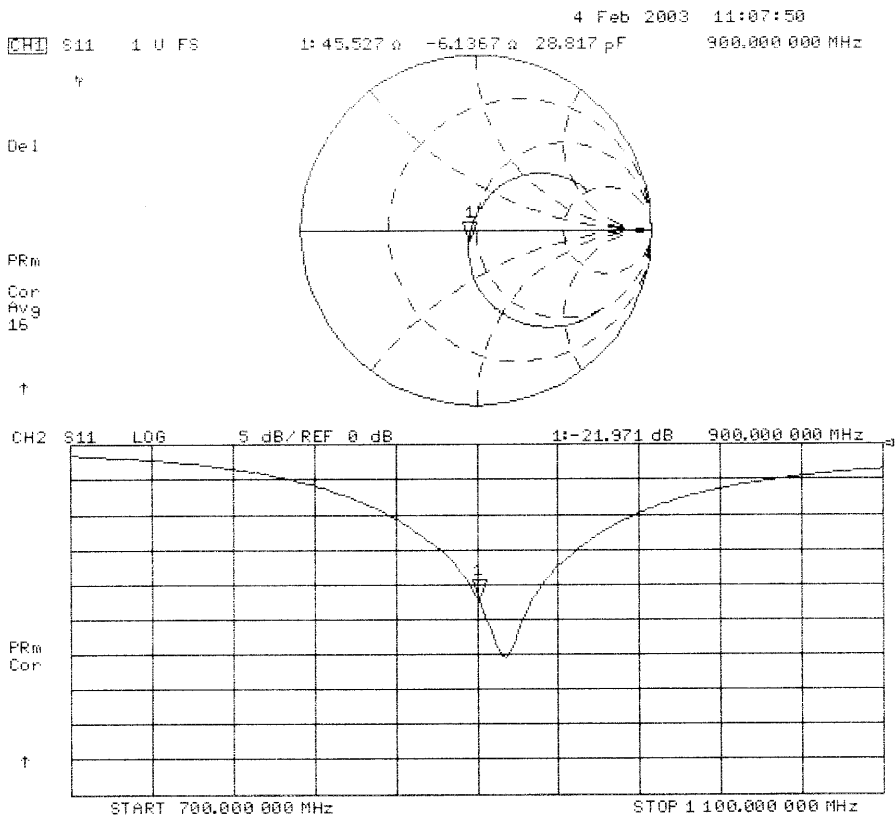

Scor Muscle

