




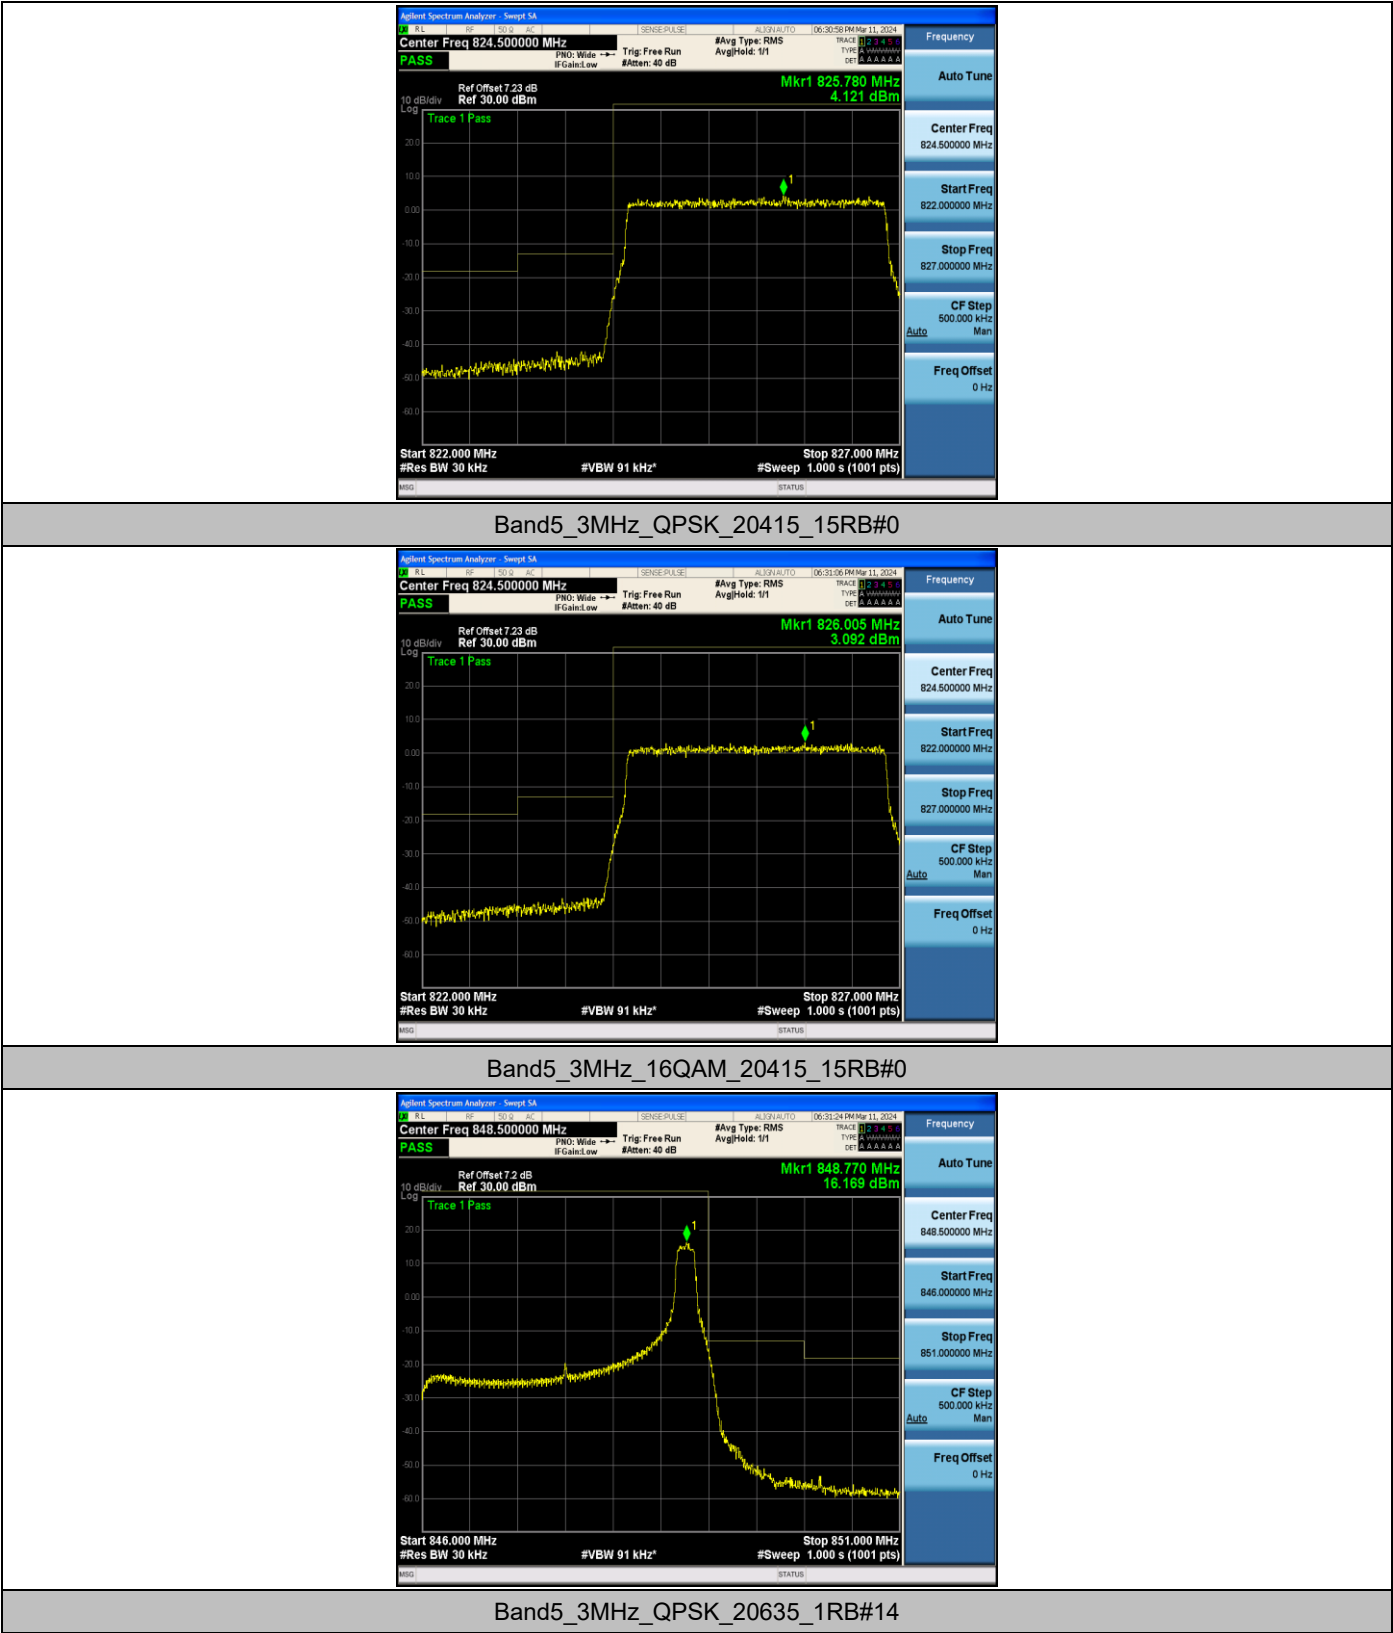

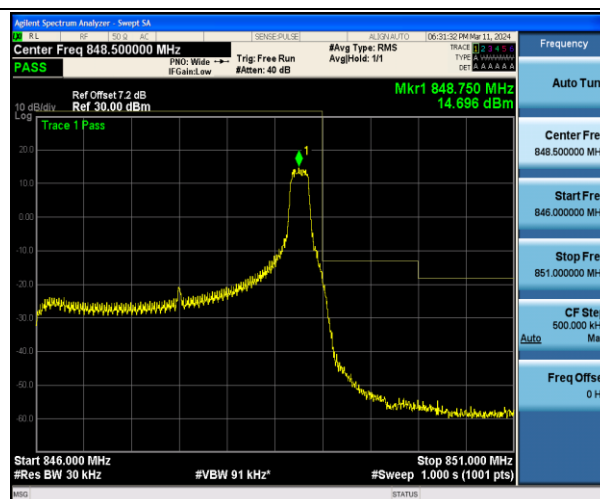


Band5 3MHz 16QAM 20635 1RB#14

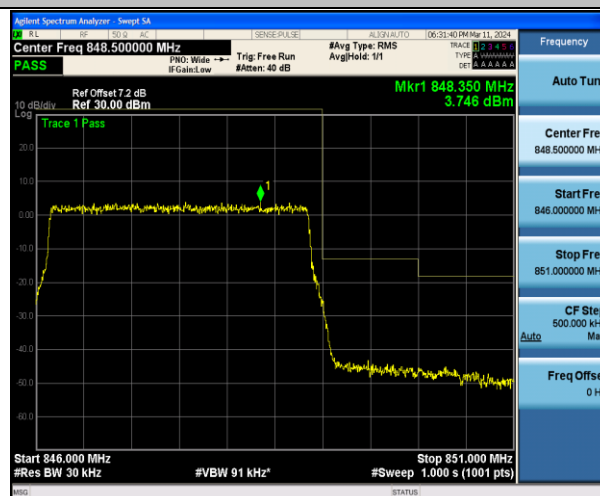


Band5 3MHz QPSK 20635 15RB#0



Band5	3MHz	16QAM	20635	15RB#0
-------	------	-------	-------	--------

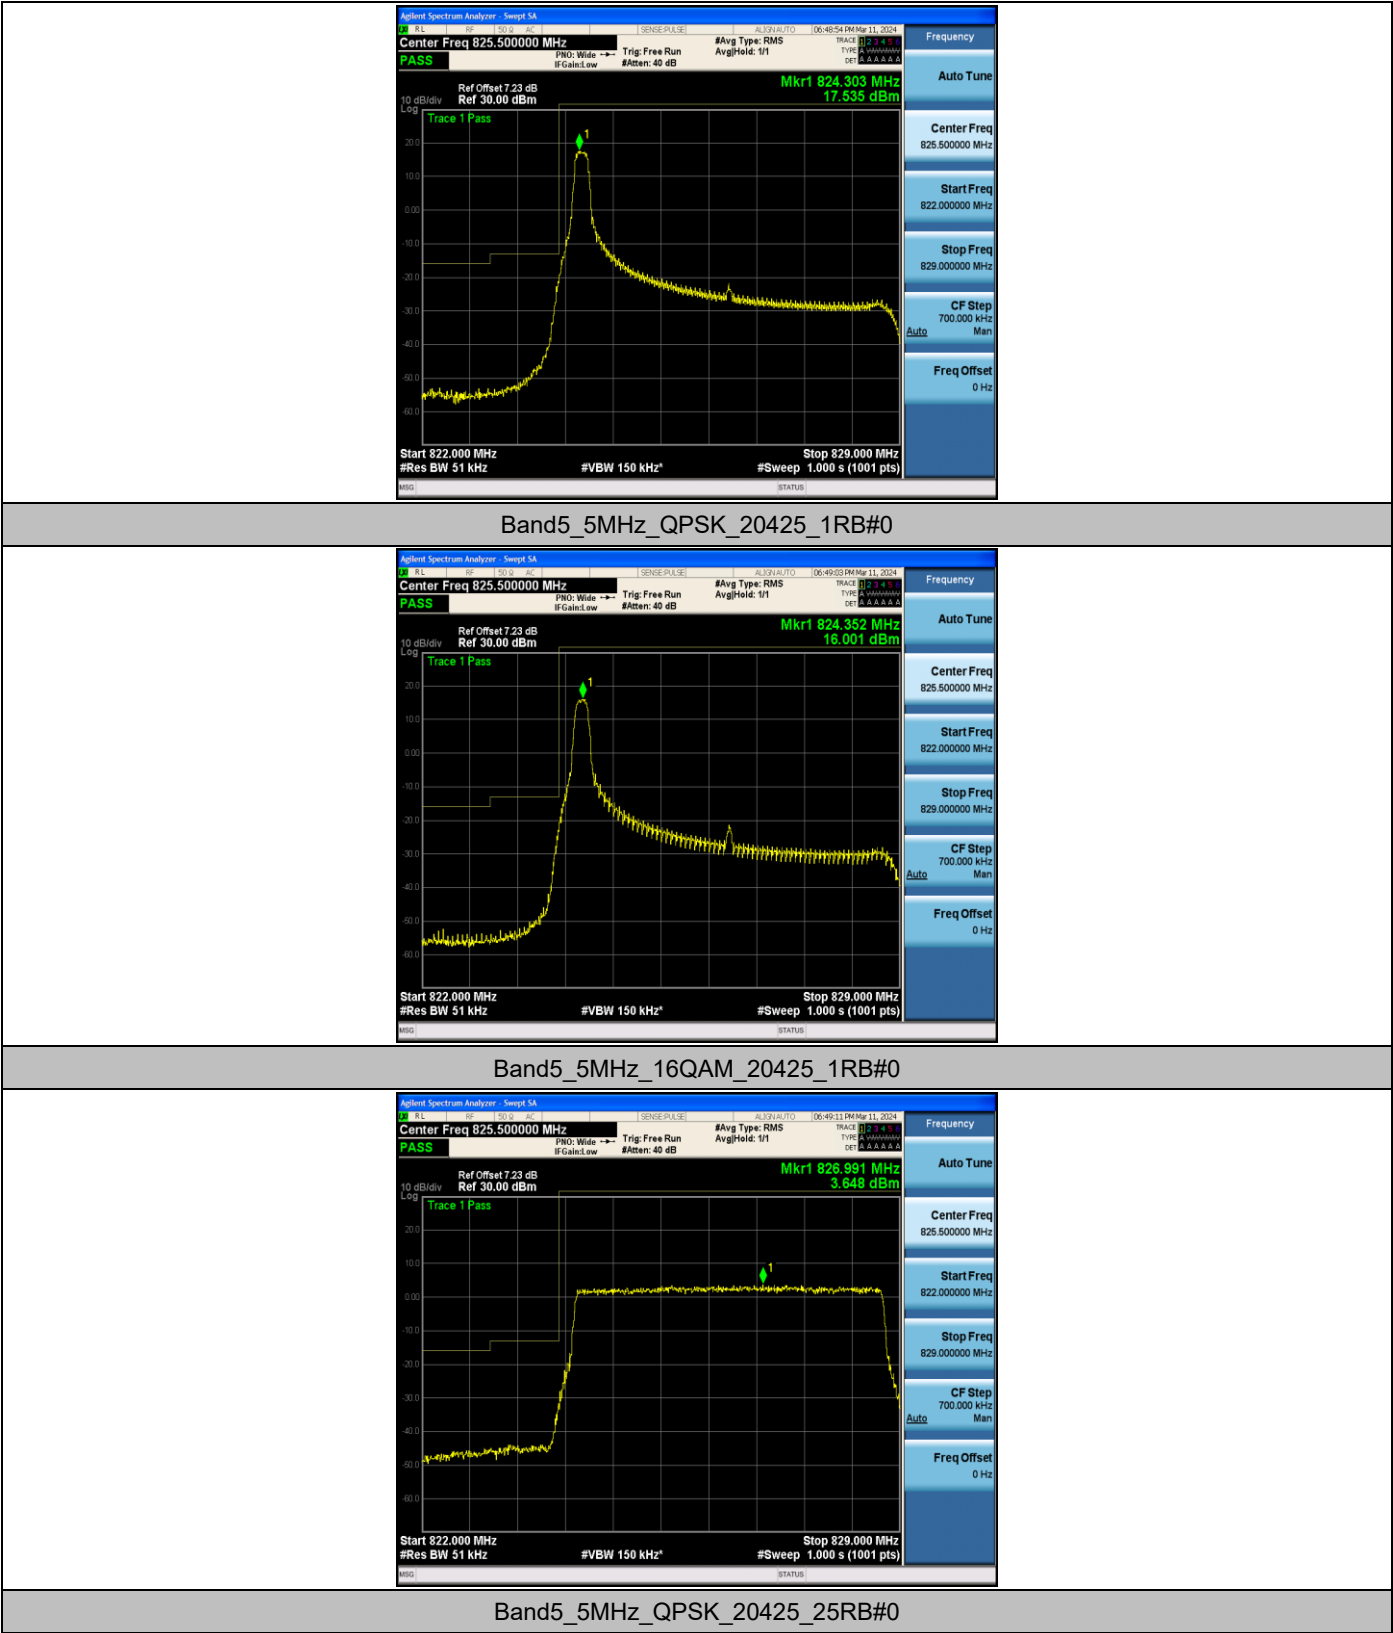

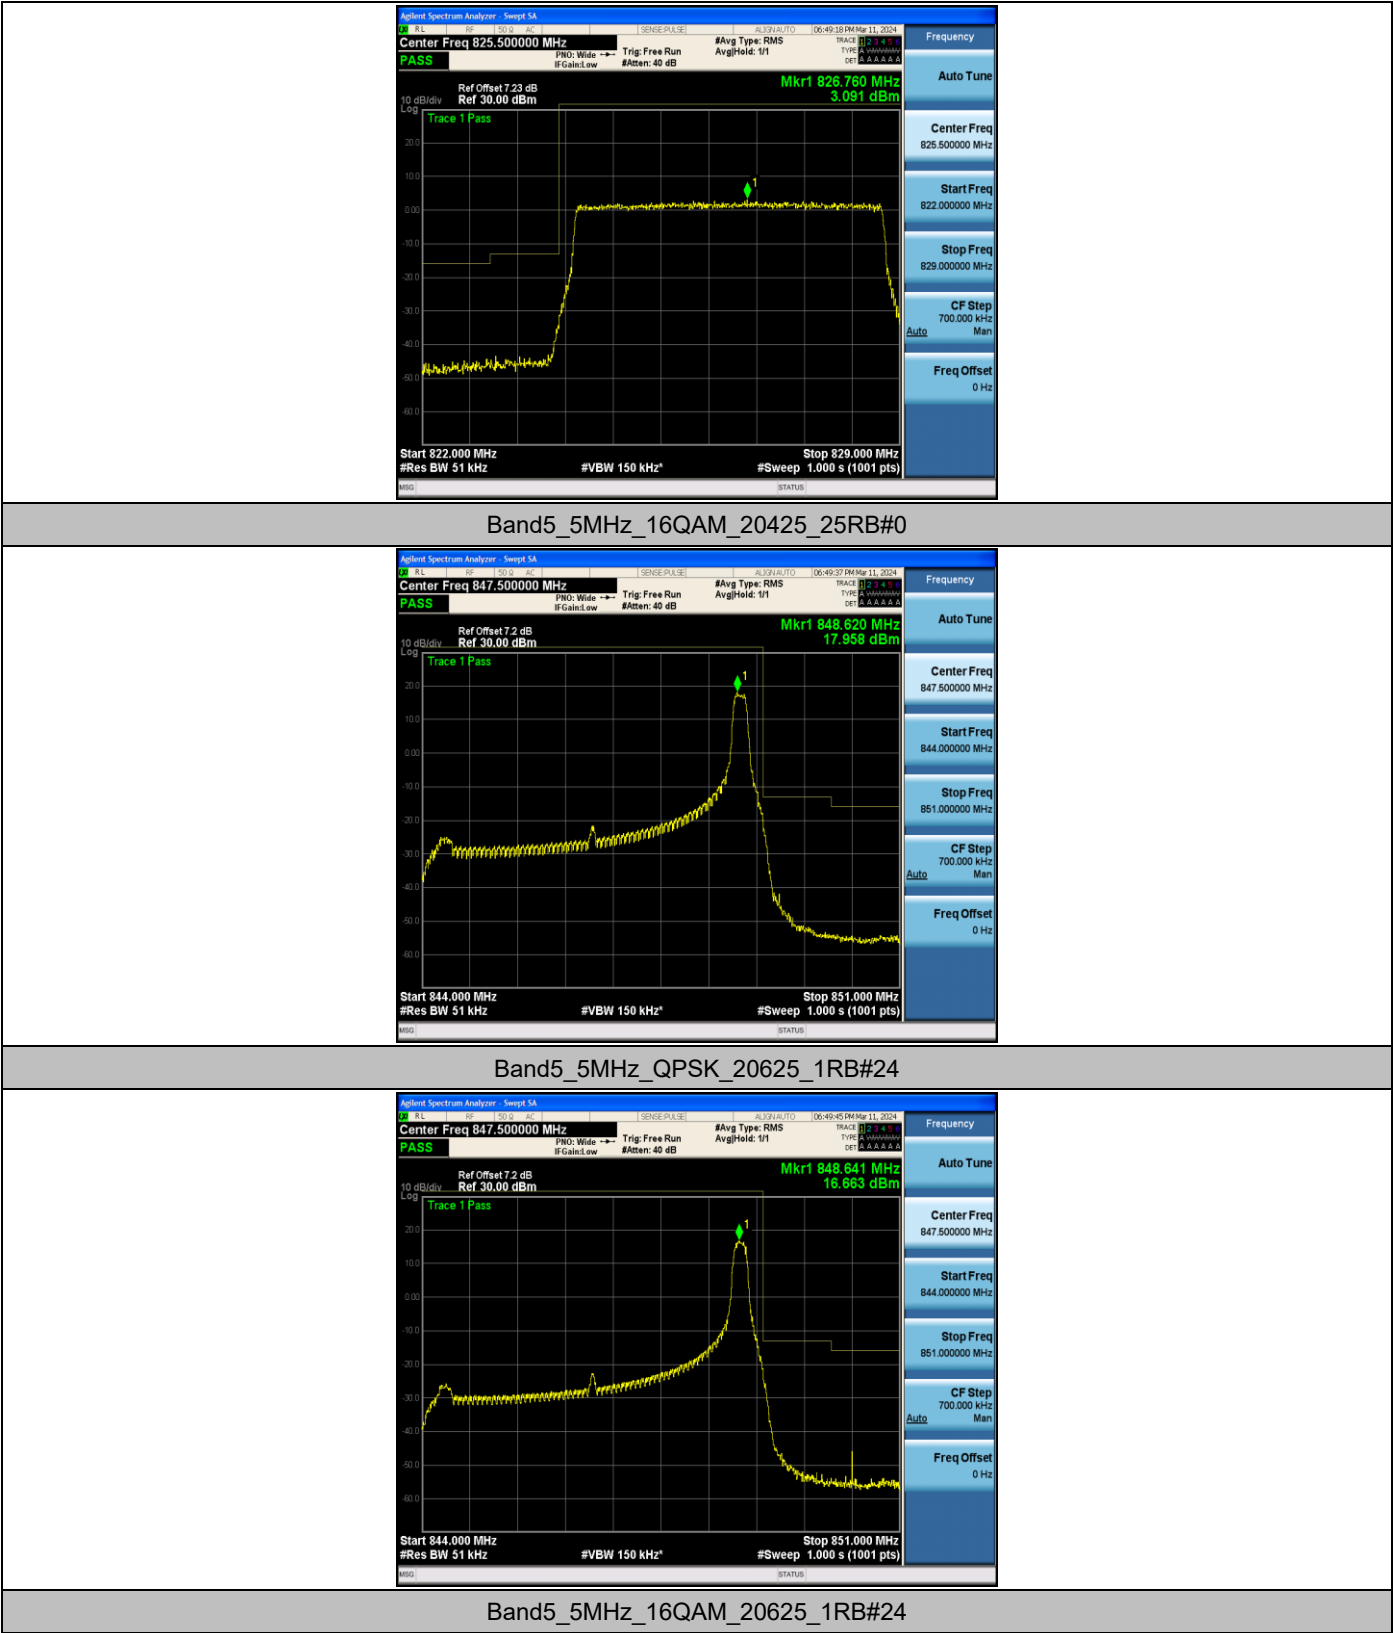

Agilent Spectrum Analyzer - Sweep 5A

Center Freq 847.500000 MHz

PASS

Ref Offset 7.2 dB

Ref 30.00 dBm

Trace 1 Pass

Start 844.000 MHz

#Res BW 51 kHz

#VBW 150 kHz

Stop 851.000 MHz

#Sweep 1.000 s (1001 pts)

Mkr1 848.641 MHz

16.663 dBm

Frequency

Auto Tune

Center Freq 847.500000 MHz

Start Freq 844.000000 MHz


Stop Freq 851.000000 MHz

CF Step 700.000 kHz

Auto

Freq Offset 0 Hz

Band5_5MHz_16QAM_20625_1RB#24

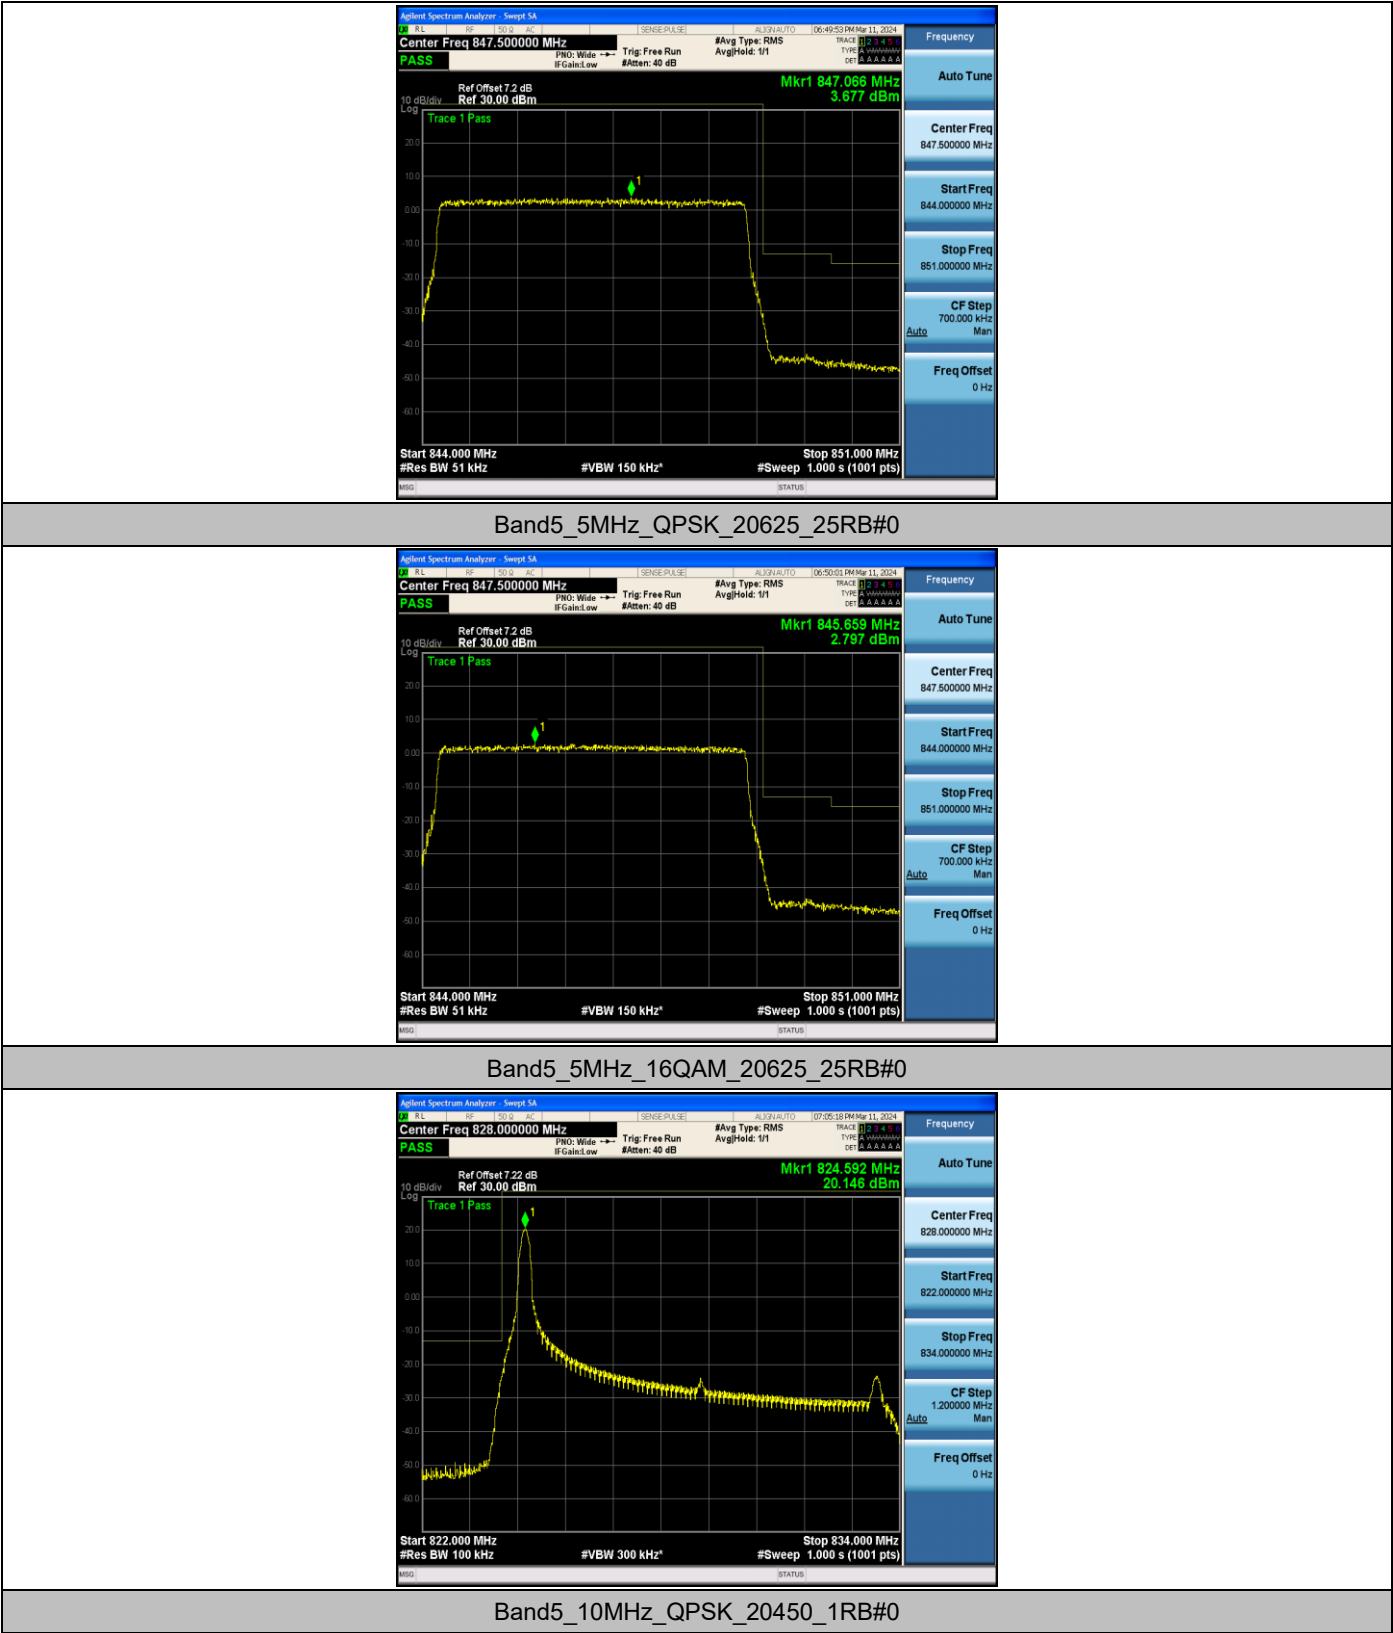

Agilent Spectrum Analyzer - Sweep SA

Center Freq 828.000000 MHz

PASS

Ref Offset 7.22 dB

Ref 30.00 dBm

Trace 1 Pass

Start 822.000 MHz

#Res BW 100 kHz

#VBW 300 kHz

#Sweep 1.000 s (1001 pts)

SENSE PULSE

06/21/2024

07:06:38 PM Mar 11, 2024

TYPE A

DEF 2.0, 0.5, 0.5

Frequency

Auto Tune

Center Freq 828.000000 MHz

Start Freq 822.000000 MHz

Stop Freq 834.000000 MHz

CF Step 1200000 MHz

Auto

Freq Offset 0 Hz

Mkr1 824.592 MHz

20.146 dBm

1

Band5_10MHz_QPSK_20450_1RB#0

