


# PCTEST Engineering Laboratory, Inc.

6660-B Dobbin Road • Columbia, MD 21045 • U.S.A.

TEL (410) 290-6652 • FAX (410) 290-6654

<http://www.pctestlab.com>



## CERTIFICATE OF COMPLIANCE FCC Part 95 Certification

Medtronic, Inc.  
7000 Central Ave.  
Minneapolis, MN 55432-3576  
Attention: Mr. Len Twetan,  
Senior Product Development Manager

Dates of Tests: July 21, 2002  
Test Report S/N: 95.220719375.LF5  
Test Site: PCTEST Lab, MD U.S.A.

FCC ID

**LF5MICS**

APPLICANT


**Medtronic, Inc.**

Classification:	Licensed Non-Broadcast Transmitter Worn on the Body
FCC Rule Part(s):	§§§ 95
EUT Type:	Carelink Programmer
Trade Name(s):	<i>Medtronic</i>
Model(s):	<i>2090</i>
Tx/Rx Frequency Range:	402.15 – 404.85 MHz
Max. RF Output Power:	21.6 µW
Frequency Tolerance:	16 ppm
Emission Designator:	46K0F1D
Channel Capacity:	10

This equipment has been shown to be capable of compliance with the applicable technical standards as indicated in the measurement report and was tested in accordance with the measurement procedures specified in §2.947.

I attest to the accuracy of data. All measurements reported herein were performed by me or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualifications of all persons taking them.

*PCTEST certifies that no party to this application has been denied the FCC benefits pursuant to Section 5301 of the Anti-Drug Abuse Act of 1988, 21 U.S.C. 862.*

  
Randy Ortanez  
President





## TABLE OF CONTENTS

---

ATTACHMENT A:	COVER LETTER(S)	
ATTACHMENT B:	ATTESTATION STATEMENT(S)	
ATTACHMENT C:	TEST REPORT	
	SCOPE	1
	INTRODUCTION	2
	INSERTS	3
	DESCRIPTION OF TESTS	4-6
	RADIATED MEASUREMENTS	7
	FREQUENCY STABILITY	8-9
	PLOTS OF EMISSIONS	10
	LIST OF TEST EQUIPMENT	11
	SAMPLE CALCULATIONS	12
	CONCLUSION	13
ATTACHMENT D:	TEST PLOTS	
ATTACHMENT E:	FCC ID LABEL & LOCATION	
ATTACHMENT F:	TEST SETUP PHOTOGRAPHS	
ATTACHMENT G:	EUT PHOTOGRAPHS	
ATTACHMENT H:	BLOCK DIAGRAM(S)	
ATTACHMENT I:	SCHEMATIC DIAGRAM(S)	
ATTACHMENT J:	USER'S MANUAL	

# MEASUREMENT REPORT



## 1.1 Scope

*Measurement and determination of electromagnetic emissions (EME) of radio frequency devices including intentional and/or unintentional radiators for compliance with the technical rules and regulations of the Federal Communications Commission.*

## General Information

<b>Applicant Name:</b>	<b>Medtronic, Inc.</b>
<b>Address:</b>	<b>7000 Central Ave. Minneapolis, MN 55432-3576</b>
<b>Attention:</b>	<b>Mr. Len Twetan, Senior Product Development Manager</b>

- **FCC ID:** LF5MICS
- **Model(s):** 2090
- **Quantity:** Quantity production is planned
- **Tx/Rx Freq. Range:** 402.15 – 404.85 MHz
- **Equipment Class:** Licensed Non-Broadcast Transmitter Worn on the Body
- **Equipment Type:** Carelink Programmer
- **Emission Designator:** 46K0F1D
- **Modulation:** FM
- **Frequency Tolerance:** 16 ppm
- **Max. Power:** 21.6  $\mu$ W
- **FCC Rule Part(s):** §§§§ 95
- **Dates of Tests:** July 21, 2002
- **Place of Tests:** PCTEST Lab, Columbia, MD U.S.A.
- **Test Report S/N:** 95.220719375.LF5

## 2.1 INTRODUCTION

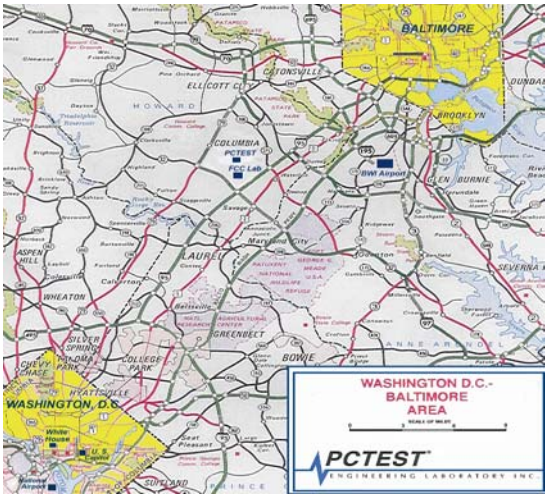


Figure 1. Map of the Greater Baltimore and Metropolitan Washington, D.C. area.

These measurement tests were conducted at **PCTEST Engineering Laboratory, Inc.** facility in New Concept Business Park, Guilford Industrial Park, Columbia, Maryland. The site address is 6660-B Dobbin Road, Columbia, MD 21045. The test site is one of the highest points in the Columbia area with an elevation of 390 feet above mean sea level. The site coordinates are 39° 11'15" N latitude and 76° 49'38" W longitude. The facility is 1.5 miles North of the FCC laboratory, and the ambient signal and ambient signal strength are approximately equal to those of the FCC laboratory. There are no FM or TV transmitters within 15 miles of the site. The detailed description of the measurement facility was found to be in compliance with the requirements of § 2.948 according to ANSI C63.4 on October 19, 1992.

### Measurement Procedure

The radiated and spurious measurements were made outdoors at a 3-meter test range (see Figure2). The equipment under testing was placed on a wooden turntable, 3-meters from the receive antenna. The receive antenna height and turntable rotations was adjusted for the highest reading on the receive spectrum analyzer. A half-wave dipole was substituted in place of the EUT. This dipole antenna was driven by a signal generator and the level of the signal generator was adjusted to obtain the same receive spectrum analyzer reading. This level was recorded.

For readings above 1 GHZ, the above procedure would be repeated using horn antennas and the difference between the gain of the horn and an isotropic antenna are taken into consideration.

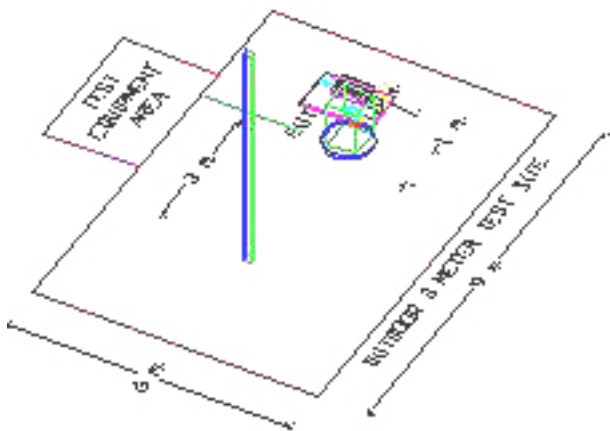


Figure 2. 3-meter outdoor test site

### 3.1 INSERTS

---

#### **Block Diagram(s) & Circuit Diagram(s)**

The block diagram is shown in Attachment I, and the circuit diagram is shown in Attachment J.

#### **Operating Instructions**

The instruction manual is shown in Attachment K.

## 4.1 DESCRIPTION OF TESTS

---

### **4.2 Transmitter Audio Frequency Response**

N/A

### **4.3 Modulation Limiting**

N/A

## 4.1 DESCRIPTION OF TESTS (CONTINUED)

---

### **4.4 20dB Bandwidth**

The unit was internally modulated and the Spectrum Analyzer was set with a Resolution Bandwidth of 100Hz and a Video Bandwidth of 100Hz.

### **4.5 Spurious and Harmonic Emissions at Antenna Terminal**

N/A

### **4.6 Radiation Spurious and Harmonic Emissions**

Radiation and harmonic emissions above 1 GHz is measured at out 3-meter outdoor site. The EUT is placed on the turntable connected to a dummy load in normal operation using the intended power source. A receiving antenna located 3 meters from the turntable receives any signal radiated from the transmitter and its operating accessories. The antenna is varied from 1 to 4 meters and the polarization is varied (horizontal and vertical) to determine the worst-case emission level. A signal generator and antenna replace the EUT and is adjusted in output until a reading identical to that obtained with the actual transmitter is obtained at the receiver. Signal strength is read from the generator and recorded on the attached table.

## 4.1 DESCRIPTION OF TESTS (CONTINUED)

---

### 4.7 Frequency Stability/Temperature Variation

The frequency stability of the transmitter is measured by:

- a.) **Temperature:** The temperature is varied from -30°C to +55°C using an environmental chamber.
  - b.) **Primary Supply Voltage:** The primary supply voltage is varied from 85% to 115% of the voltage normally at the input to the device or at the power supply terminals if cables are not normally supplied.
- Specification – The minimum frequency stability shall be +/- 0.0010% at any time during normal operation.*

**Time Period and Procedure:**

1. The carrier frequency of the transmitter and the individual oscillators is measured at room temperature (25°C to 27°C to provide a reference).
2. The equipment is subjected to an overnight "soak" at -30°C without any power applied.
3. After the overnight "soak" at 30°C (usually 14-16 hours), the equipment is turned on in a "standby" condition for one minute before applying power to the transmitter. Measurement of the carrier frequency of the transmitter and the individual oscillators is made within a three minute interval after applying power to the transmitter.
4. Frequency measurements are made at 10°C interval up to room temperature. At least a period of one and one half-hour is provided to allow stabilization of the equipment at each temperature level.
5. Again the transmitter carrier frequency and the individual oscillators is measured at room temperature to begin measurement of the upper temperature levels.
6. Frequency were made at 10 intervals starting at 30°C up to +50°C allowing at least two hours at each temperature for stabilization. In all measurements the frequency is measured within three minutes after applying power to the transmitter.
7. The artificial load is mounted external to the temperature chamber.

**NOTE: The EUT is tested down to the battery endpoint.**



## 5.1 TEST DATA

### 5.2 Emissions Measurements

#### Strength of Radiation –Low

Frequency (MHz)	Level (dBm)	AFCL (dB)	POL (H/V)	F/S (dBμV/m)	F/S (μV/m)	Power (W)	Margin (dB)
402.15	- 50.000	23.72	V	80.72	10864.26	2.16E-05	N/A
804.30	- 97.200	31.45	V	41.25	115.4782	2.44E-09	- 4.75
1206.50	- 115.000	32.10	V	24.10	16.03245	4.70E-11	- 29.9
1608.60	- 125.000	34.50	V	16.50	6.683439	8.17E-12	- 37.5
2010.80	- 133.000	36.00	V	10.00	3.162278	1.83E-12	- 44.0

#### Strength of Radiation –Medium

Frequency (MHz)	Level (dBm)	AFCL (dB)	POL (H/V)	F/S (dBμV/m)	F/S (μV/m)	Power (W)	Margin (dB)
403.35	- 50.100	23.77	V	80.67	10801.9	2.13E-05	N/A
806.70	- 97.100	31.50	V	41.40	117.4898	2.53E-09	- 4.6
1210.10	- 114.600	32.20	V	24.60	16.98244	5.28E-11	- 29.4
1613.40	- 125.100	34.60	V	16.50	6.683439	8.17E-12	- 37.5
2016.80	- 132.100	36.10	V	11.00	3.548134	2.30E-12	- 43.0

#### Strength of Radiation –High

Frequency (MHz)	Level (dBm)	AFCL (dB)	POL (H/V)	F/S (dBμV/m)	F/S (μV/m)	Power (W)	Margin (dB)
404.85	- 50.300	23.82	V	80.52	10616.96	2.06E-05	N/A
809.70	- 97.200	31.60	V	41.40	117.4898	2.53E-09	- 4.6
1214.60	- 115.000	32.30	V	24.30	16.40590	4.92E-11	- 29.7
1619.40	- 126.100	34.70	V	15.60	6.025596	6.64E-12	- 38.4
2024.30	- 132.000	36.20	V	11.20	3.630781	2.41E-12	- 42.8

## 6.1 Test Data


### 6.2 FREQUENCY STABILITY

OPERATING FREQUENCY: 403,350,000 Hz  
 CHANNEL: 005  
 REFERENCE VOLTAGE: 115 VDC  
 DEVIATION LIMIT: ± 0.0100 % or 100 ppm

VOLTAGE (% )	POWER (VDC )	TEMP (°C)	FREQ . (Hz)	Deviation (% )
100 %	115.00	+ 20 (Ref)	403,350,000	0.000000
100 %		- 30	403,343,546	0.001600
100 %		- 20	403,344,353	0.001400
100 %		- 10	403,345,967	0.001000
100 %		0	403,346,410	0.000890
100 %		+ 10	403,347,713	0.000567
100 %		+ 20	403,350,000	0.000000
100 %		+ 25	403,349,996	0.000001
100 %		+ 30	403,347,298	0.000670
100 %		+ 40	403,353,590	-0.000890
100 %		+ 50	403,354,840	-0.001200
100 %		+ 60	403,356,454	-0.001600
85 %	97.75	+ 20	403,350,000	0.000000
115 %	132.25	+ 20	403,350,000	0.000000
BATT.ENDPOINT	N/A	+ 20	403,350,000	0.000000

## 6.1 Test Data (Continued)

### 6.3 FREQUENCY STABILITY

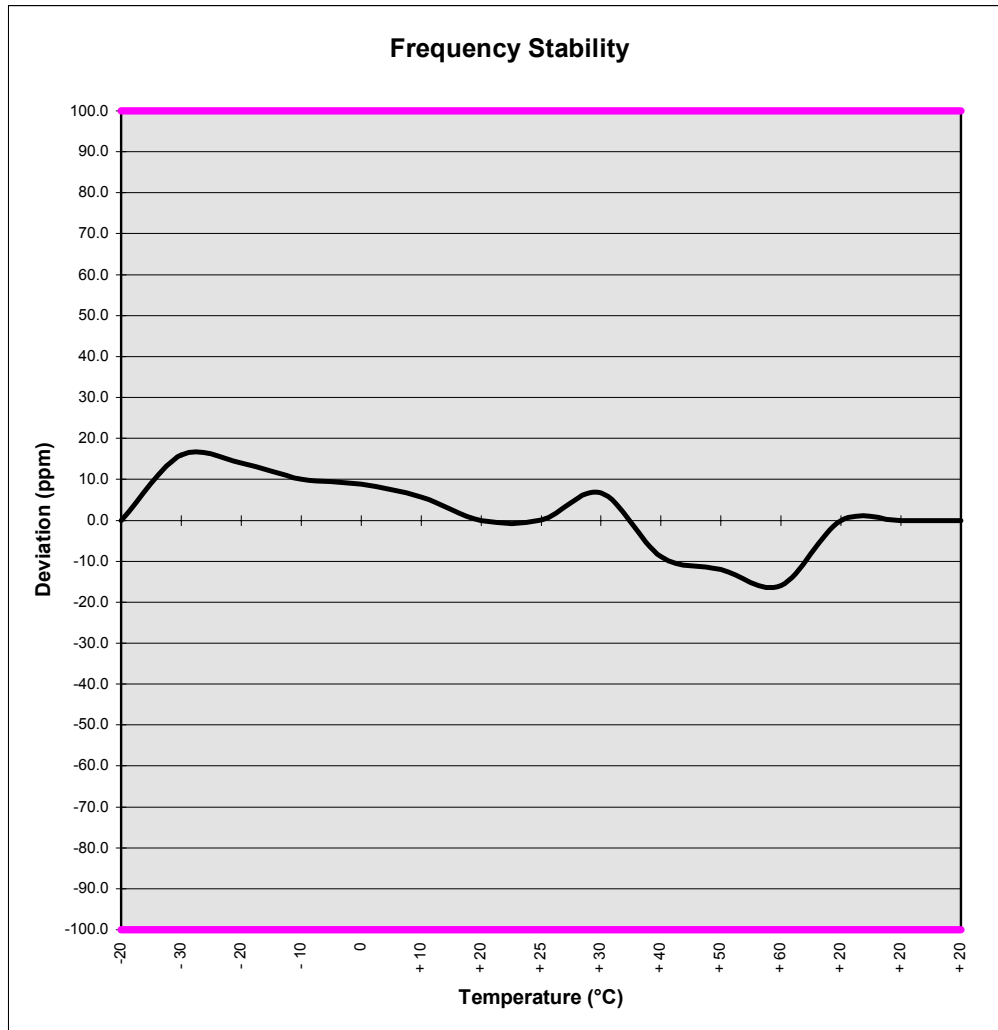

## 7.1 PLOT(S) OF EMISSIONS

---

SEE ATTACHMENT D

## 8.1 TEST EQUIPMENT

8.2 Type	Model	Cal. Due Date	S/N
Microwave Spectrum Analyzer	HP 8566B (100Hz-22GHz)	08/15/03	3638A08713
Microwave Spectrum Analyzer	HP 8566B (100Hz-22GHz)	04/17/03	2542A11898
Spectrum Analyzer/Tracking Gen.	HP 8591A (100Hz-1.8GHz)	08/10/03	3144A02458
Signal Generator*	HP 8640B (500Hz-1GHz)	06/03/03	2232A19558
Signal Generator*	HP 8640B (500Hz-1GHz)	06/03/03	1851A09816
Signal Generator*	Rohde & Schwarz (0.1-1000MHz)	09/11/02	894215/012
Ailtech/Eaton Receiver	NM 37/57A-SL (30-1000MHz)	04/12/03	0792-03271
Ailtech/Eaton Receiver	NM 37/57A (30-1000MHz)	03/11/03	0805-03334
Ailtech/Eaton Receiver	NM 17/27A (0.1-32MHz)	09/17/02	0608-03241
Quasi-Peak Adapter	HP 85650A	08/15/02	2043A00301
Ailtech/Eaton Adapter	CCA-7 CISPR/ANSI QP Adapter	03/11/03	0194-04082
RG58 Coax Test Cable	No. 167		n/a
Harmonic/Flicker Test System	HP 6841A (IEC 555-2/3)		3531A00115
Broadband Amplifier (2)	HP 8447D		1145A00470, 1937A03348
Broadband Amplifier	HP 8447F		2443A03784
Transient Limiter	HP 11947A (9kHz-200MHz)		2820A00300
Horn Antenna	EMCO Model 3115 (1-18GHz)	9704-5182	
Horn Antenna	EMCO Model 3115 (1-18GHz)	9205-3874	
Horn Antenna	EMCO Model 3116 (18-40GHz)		9203-2178
Biconical Antenna (4)	Eaton 94455/Eaton 94455-1/Singer 94455-1/Compliance Design 1295, 1332, 0355		
Log-Spiral Antenna (3)	Ailtech/Eaton 93490-1		0608, 1103, 1104
Roberts Dipoles	Compliance Design (1 set)		
Ailtech Dipoles	DM-105A (1 set)		33448-111
EMCO LISN	3816/2		1079
EMCO LISN	3816/2		1077
EMCO LISN	3725/2		2009
Microwave Preamplifier 40dB Gain	HP 83017A (0.5-26.5GHz)		3123A00181
Microwave Cables	MicroCoax (1.0-26.5GHz)		
Ailtech/Eaton Receiver	NM37/57A-SL		0792-03271
Spectrum Analyzer	HP 8594A		3051A00187
Spectrum Analyzer (2)	HP 8591A		3034A01395, 3108A02053
Modulation Analyzer	HP 8901A		2432A03467
NTSC Pattern Generator	Leader 408		0377433
Noise Figure Meter	HP 8970B		3106A02189
Noise Figure Meter	Ailtech 7510		TE31700
Noise Generator	Ailtech 7010		1473
Microwave Survey Meter	Holaday Model 1501 (2.450GHz)		80931
Digital Thermometer	Extech Instruments 421305		426966
Attenuator	HP 8495A (0-70dB) DC-4GHz		
Bi-Directional Coax Coupler	Narda 3020A (50-1000MHz)		
Shielded Screen Room	RF Lindgren Model 26-2/2-0		6710 (PCT270)
Shielded Semi-Anechoic Chamber	Ray Proof Model S81		R2437 (PCT278)
Environmental Chamber	Associated Systems Model 1025 (Temperature/Humidity)		PCT285

\* Calibration traceable to the National Institute of Standards and Technology (NIST).

## 9.1 SAMPLE CALCULATIONS

---

The EIRP for channel 05 (403.35 MHz) was measured at a 3 meter distance on our OATS. The turn table and antenna mast were adjusted to obtain the highest reading on a receiver spectrum analyzer with RBW and VBW set at 3MHz each. A dipole antenna driven by a signal generator was substituted in place of the EUT and adjusted to match the -50.1 dBm receiver spectrum analyzer reading. (The dipole antenna used during the substitution has a gain of 2.14 dBi at 403.35 MHz.) The power at the antenna terminals of the substituted dipole was -18.87 dBm. This value was corrected by adding the 2.14 dBi gain of the substituted dipole to yield - 16.73 dBm for EIRP.

## 10.1 CONCLUSION

---

The data collected shows that the Medtronic Carelink Programmer **FCC ID: LF5MICS** complies with all the requirements of Parts 2 and 95 of the FCC rules.