

Date: 2025-02-16

**System Check\_Head\_750MHz****DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_750\_250216 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.893$  S/m;  $\epsilon_r = 41.5$ 

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.17, 8.96, 10.01); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.410 W/kg; SAR (10g) = 0.276 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.414 W/kg; SAR (8g) = 0.291 W/kg; SAR (10g) = 0.276 W/kg

Smallest distance from peaks to all points 3 dB below = &gt; 15.0 mm

Ratio of SAR at M2 to SAR at M1 = 88.3 %

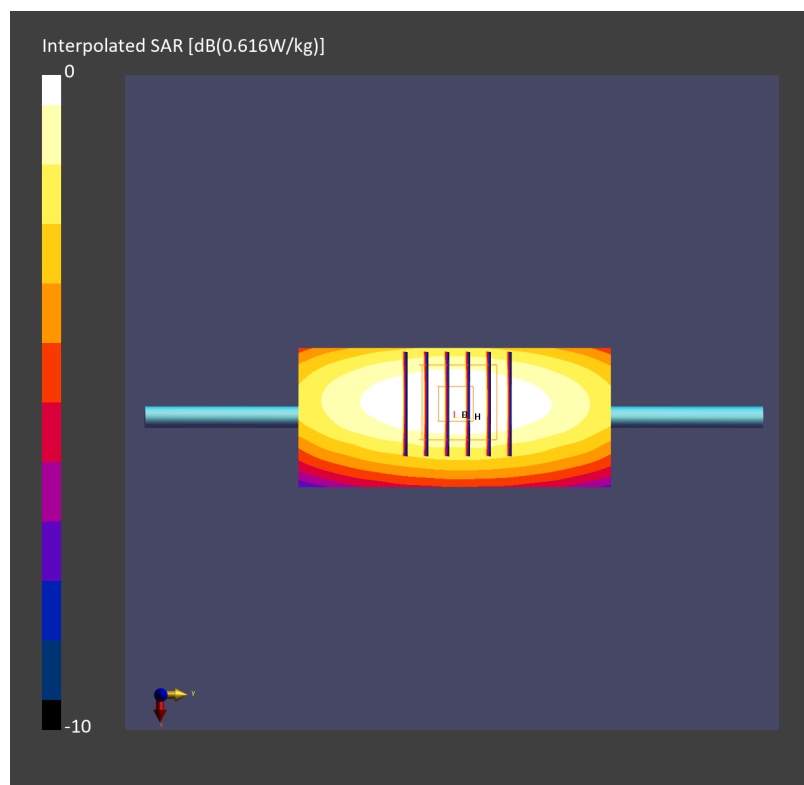

Date: 2025-02-19

**System Check\_Head\_750MHz****DUT: D750V3 - SN1107**

Communication System: CW; Frequency: 750.000 MHz

Medium: HSL\_750\_250219 Medium parameters used:  $f = 750.000$  MHz;  $\sigma = 0.893$  S/m;  $\epsilon_r = 41.8$ 

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(9.17, 8.96, 10.01); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.417 W/kg; SAR (10g) = 0.280 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.415 W/kg; SAR (8g) = 0.291 W/kg; SAR (10g) = 0.276 W/kg

Smallest distance from peaks to all points 3 dB below = 19.0 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

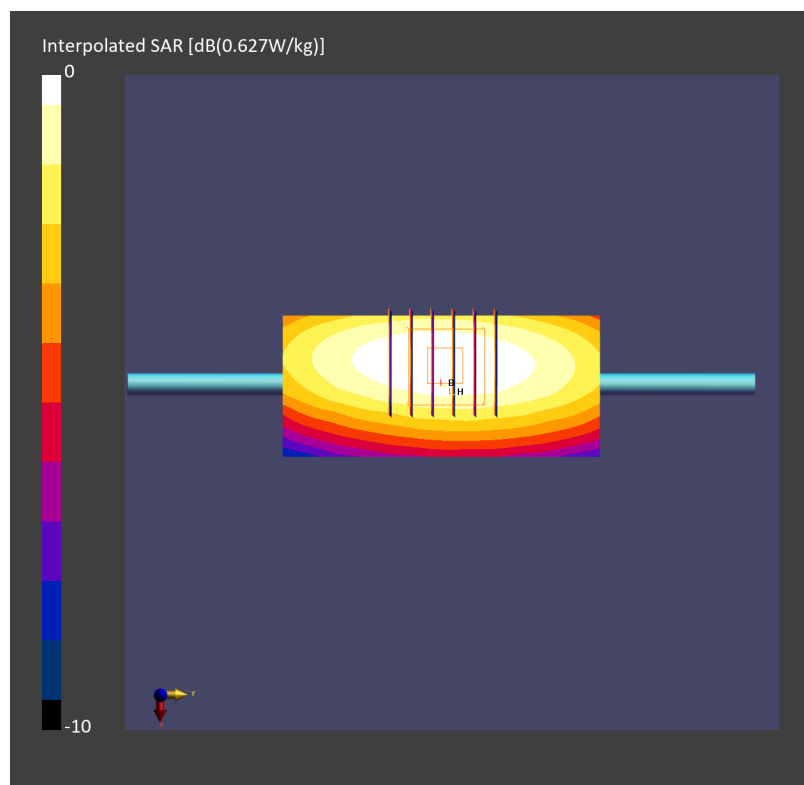

Date: 2025-02-16

## System Check\_Head\_850MHz

### DUT: D835V2 - SN499

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL\_850\_250216 Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.927$  S/m;  $\epsilon_r = 41.2$

Ambient Temperature: 23.6°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.87, 8.66, 9.68); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.484 W/kg; SAR (10g) = 0.321 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.05 dB

SAR (1g) = 0.484 W/kg; SAR (8g) = 0.336 W/kg; SAR (10g) = 0.319 W/kg

Smallest distance from peaks to all points 3 dB below = 17.8 mm

Ratio of SAR at M2 to SAR at M1 = 87.9 %

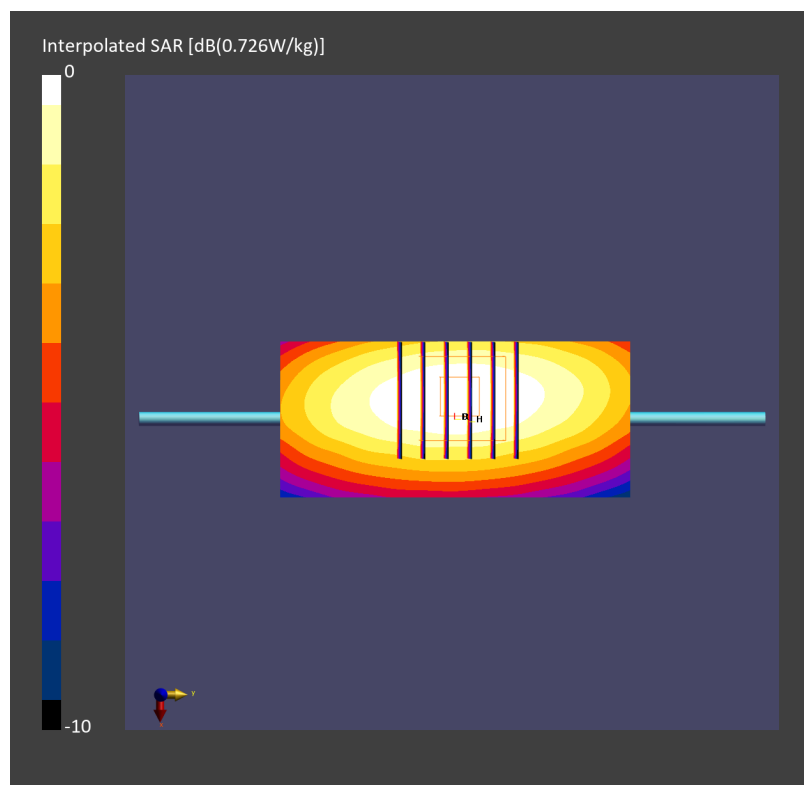

Date: 2025-02-19

**System Check\_Head\_850MHz****DUT: D835V2 - SN499**

Communication System: CW; Frequency: 835.000 MHz

Medium: HSL\_850\_250219 Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.927$  S/m;  $\epsilon_r = 41.5$ 

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(8.87, 8.66, 9.68); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.494 W/kg; SAR (10g) = 0.329 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.500 W/kg; SAR (8g) = 0.348 W/kg; SAR (10g) = 0.330 W/kg

Smallest distance from peaks to all points 3 dB below = 18.8 mm

Ratio of SAR at M2 to SAR at M1 = 88.2 %

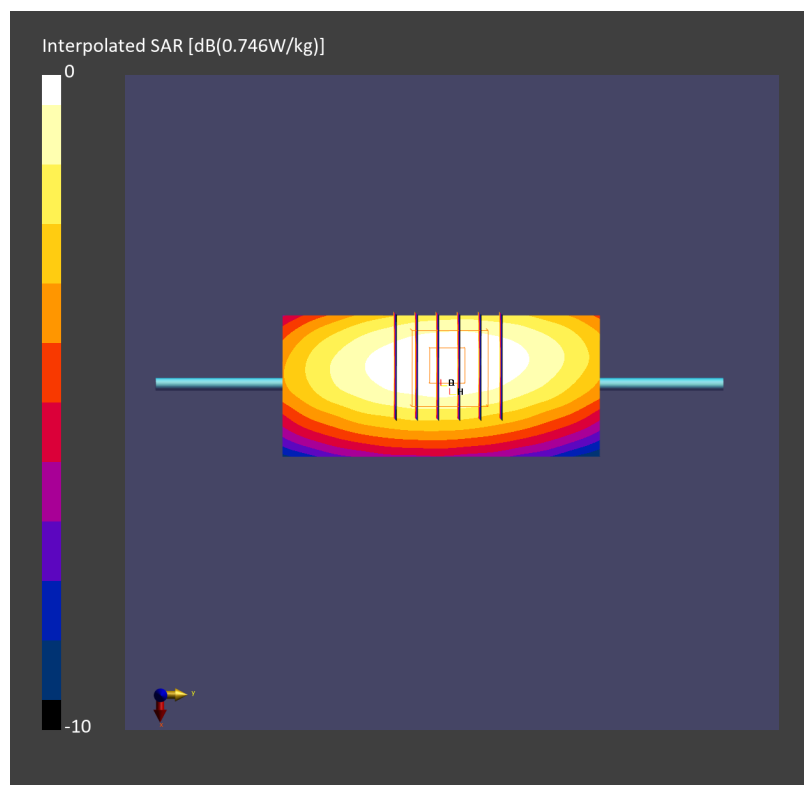

Date: 2025-02-15

**System Check\_Head\_1750MHz****DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL\_1750\_250215 Medium parameters used:  $f = 1750.000$  MHz;  $\sigma = 1.37$  S/m;  $\epsilon_r = 40.9$ 

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

**DASY6 Configuration:**

- Probe: EX3DV4 - SN7694; ConvF(7.86, 7.67, 8.57); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.82 W/kg; SAR (10g) = 1.01 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.83 W/kg; SAR (8g) = 1.06 W/kg; SAR (10g) = 0.981 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.0 %

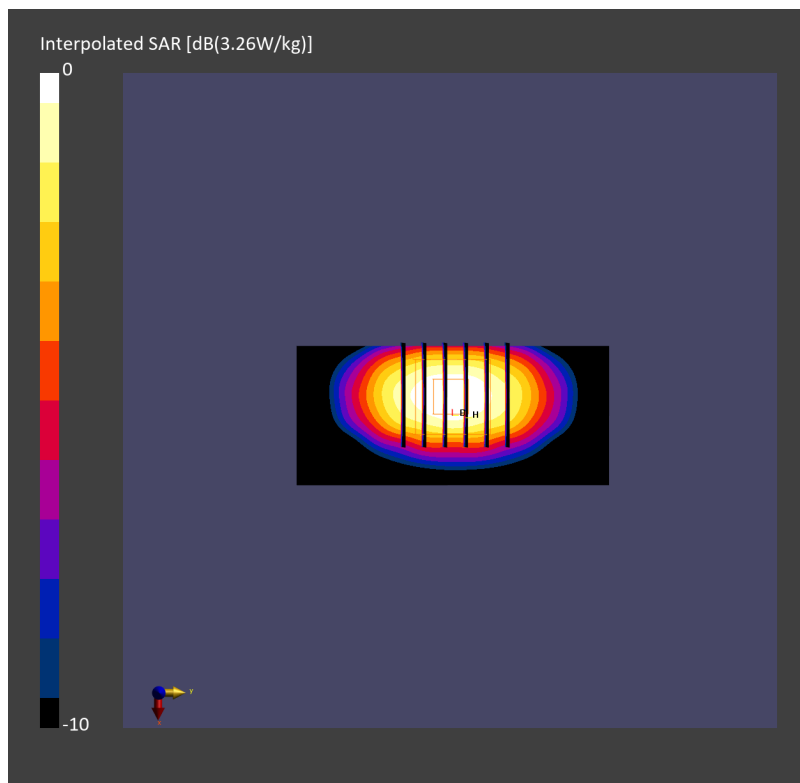

Date: 2025-02-18

**System Check\_Head\_1750MHz****DUT: D1750V2 - SN1112**

Communication System: CW; Frequency: 1750.000 MHz

Medium: HSL\_1750\_250218 Medium parameters used:  $f = 1750.000$  MHz;  $\sigma = 1.36$  S/m;  $\epsilon_r = 40.5$ 

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.86, 7.67, 8.57); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.80 W/kg; SAR (10g) = 0.998 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.00 dB

SAR (1g) = 1.81 W/kg; SAR (8g) = 1.05 W/kg; SAR (10g) = 0.970 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.8 %

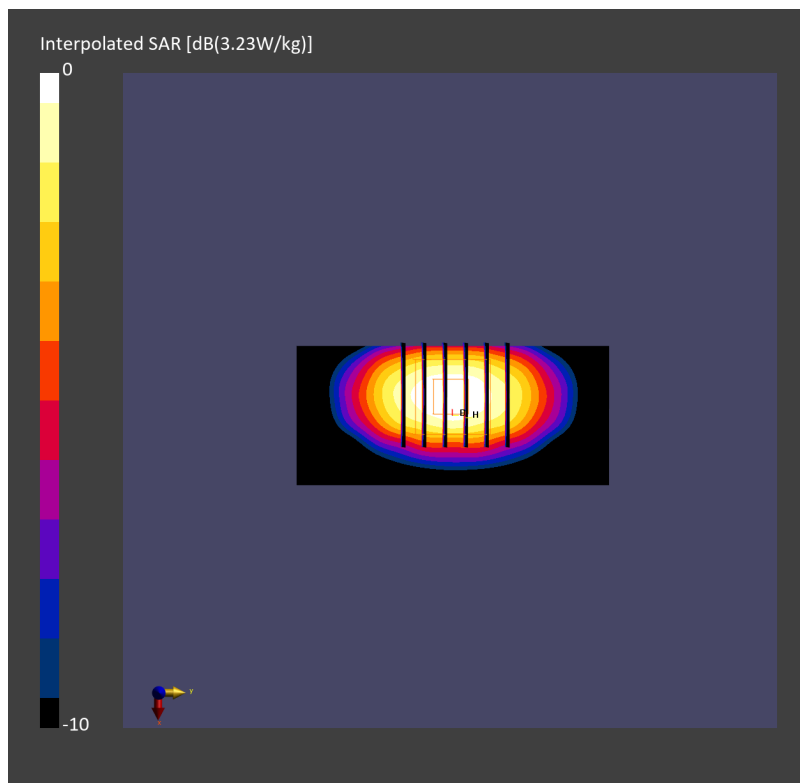

Date: 2025-02-15

**System Check\_Head\_1900MHz****DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL\_1900\_250215 Medium parameters used:  $f = 1900.000$  MHz;  $\sigma = 1.45$  S/m;  $\epsilon_r = 39.3$ 

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.62, 7.44, 8.32); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.86 W/kg; SAR (10g) = 1.00 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 1.91 W/kg; SAR (8g) = 1.09 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.5 %

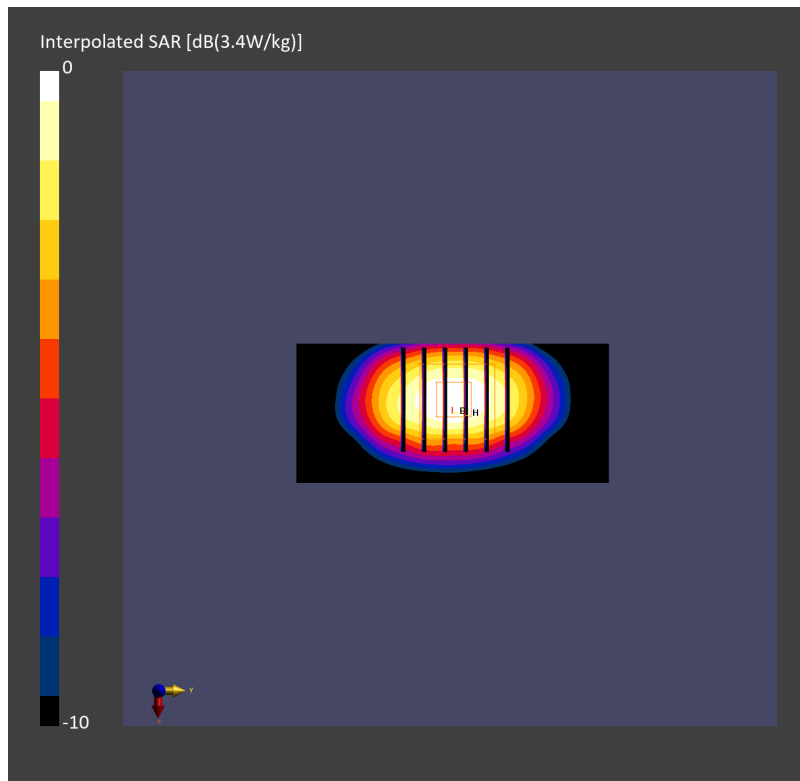

Date: 2025-02-18

**System Check\_Head\_1900MHz****DUT: D1900V2 - SN5d185**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL\_1900\_250218 Medium parameters used:  $f = 1900.000$  MHz;  $\sigma = 1.44$  S/m;  $\epsilon_r = 39.0$ 

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.62, 7.44, 8.32); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.84 W/kg; SAR (10g) = 0.991 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.89 W/kg; SAR (8g) = 1.08 W/kg; SAR (10g) = 0.995 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 84.2 %

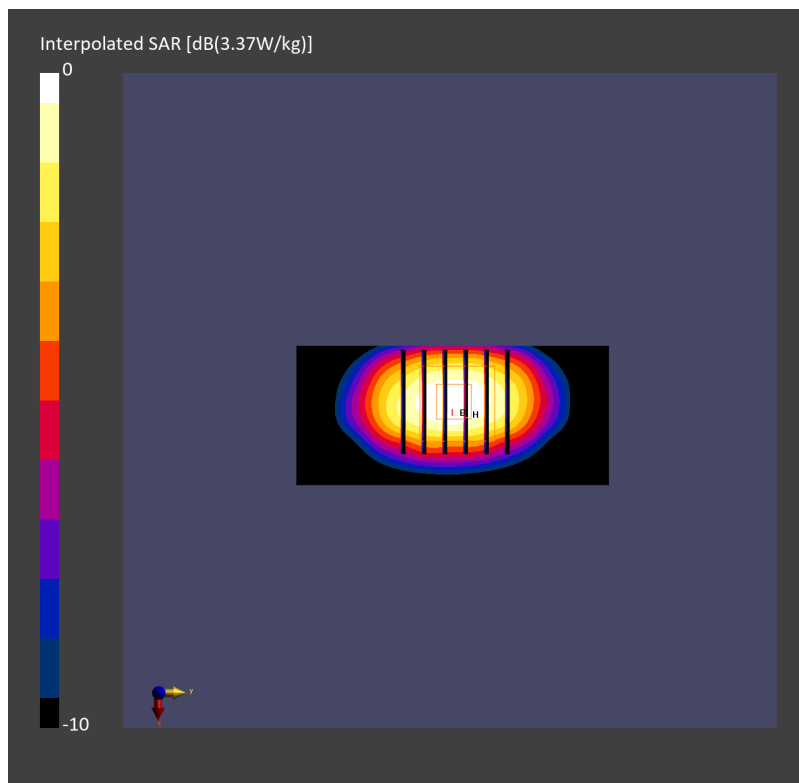

Date: 2025-02-20

**System Check\_Head\_1900MHz****DUT: D1900V2 - SN5d093**

Communication System: CW; Frequency: 1900.000 MHz

Medium: HSL\_1900\_250220 Medium parameters used:  $f = 1900.000$  MHz;  $\sigma = 1.40$  S/m;  $\epsilon_r = 40.1$ 

Ambient Temperature: 23.8°C; Liquid Temperature: 22.8°C

**DASY6 Configuration:**

- Probe: EX3DV4 - SN3931; ConvF(7.67, 7.38, 7.28); Calibrated: 2024-11-19
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn703; Calibrated: 2024-04-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.93 W/kg; SAR (10g) = 1.02 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.94 W/kg; SAR (8g) = 1.10 W/kg; SAR (10g) = 1.01 W/kg

Smallest distance from peaks to all points 3 dB below = 9.6 mm

Ratio of SAR at M2 to SAR at M1 = 83.8 %

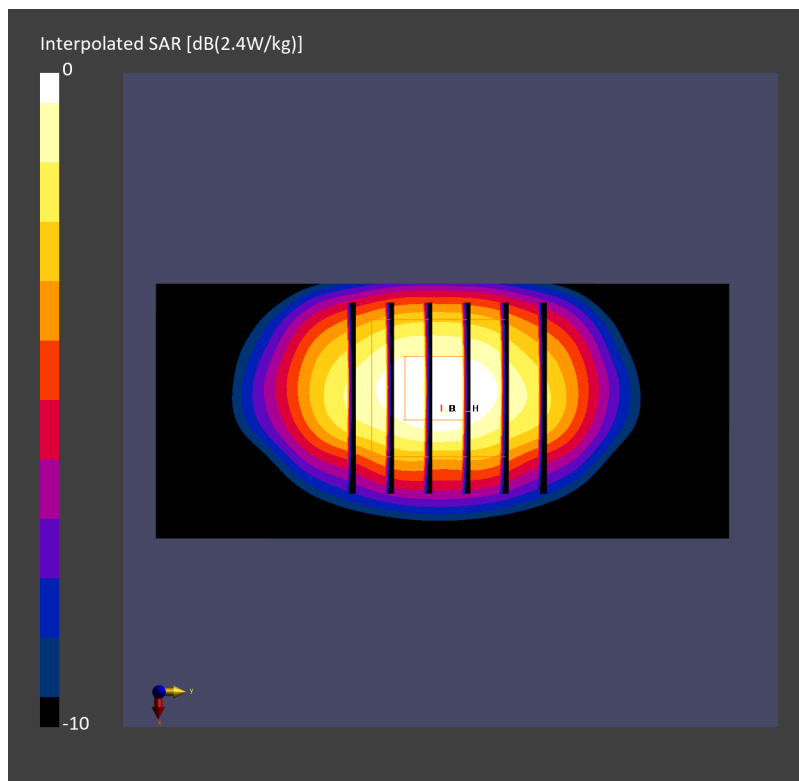

Date: 2025-02-17

**System Check\_Head\_2300MHz****DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz

Medium: HSL\_2300\_250217 Medium parameters used:  $f = 2300.000$  MHz;  $\sigma = 1.67$  S/m;  $\epsilon_r = 39.4$ 

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.4, 7.22, 8.07); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.27 W/kg; SAR (10g) = 1.12 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.28 W/kg; SAR (8g) = 1.20 W/kg; SAR (10g) = 1.09 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 81.5 %

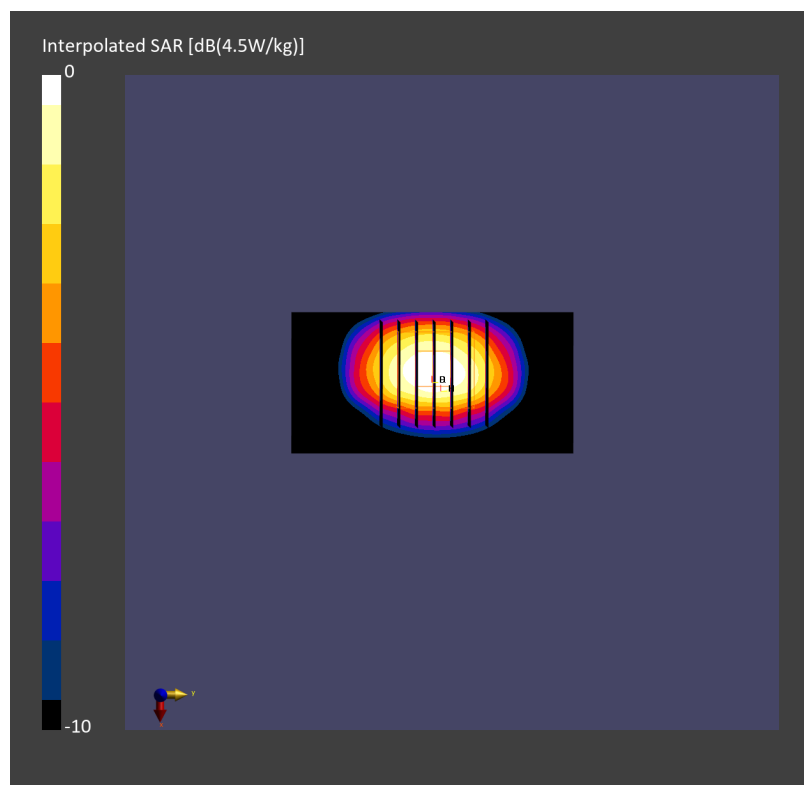

Date: 2025-02-21

**System Check\_Head\_2300MHz****DUT: D2300V2 - SN1088**

Communication System: CW; Frequency: 2300.000 MHz;

Medium: HSL\_2300\_250221 Medium parameters used:  $f = 2300.000$  MHz;  $\sigma = 1.64$  S/m;  $\epsilon_r = 40.6$  Ambient

Temperature: 23.0°C; Liquid Temperature: 22.0°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.4, 7.22, 8.07); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.24 W/kg; SAR (10g) = 1.10 W/kg;

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5


mm

Power Drift = -0.01 dB

SAR (1g) = 2.25 W/kg; SAR (8g) = 1.19 W/kg; SAR (10g) = 1.08 W/kg

Smallest distance from peaks to all points 3 dB below = 9.3 mm

Ratio of SAR at M2 to SAR at M1 = 82.7 %

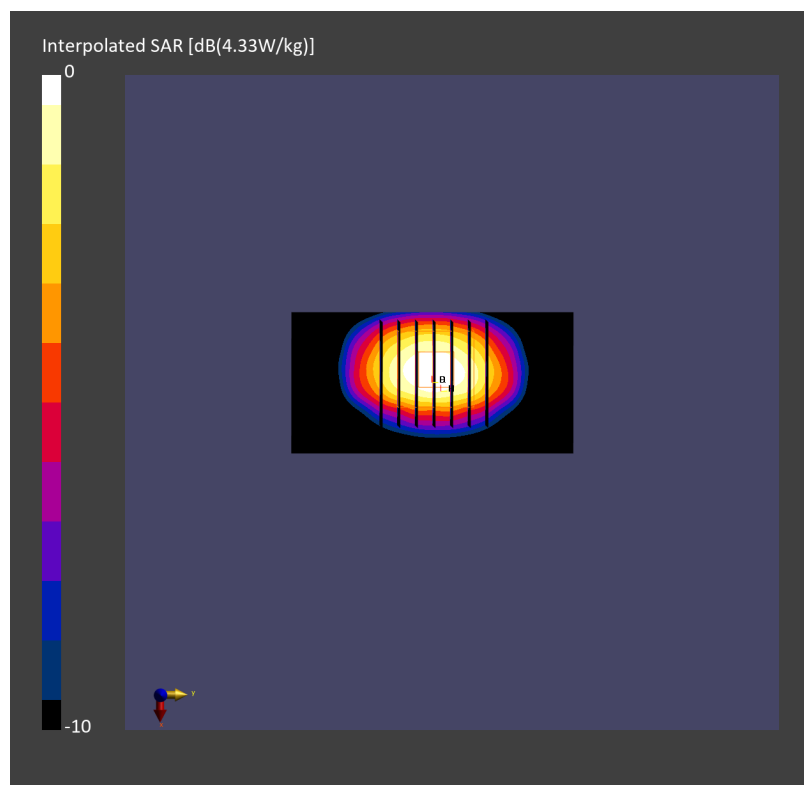

Date: 2025-02-17

**System Check\_Head\_2600MHz****DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_2600\_250217 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 2.00$  S/m;  $\epsilon_r = 38.3$ 

Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.12, 6.95, 7.76); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.27 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.75 W/kg; SAR (8g) = 1.38 W/kg; SAR (10g) = 1.25 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 80.2 %

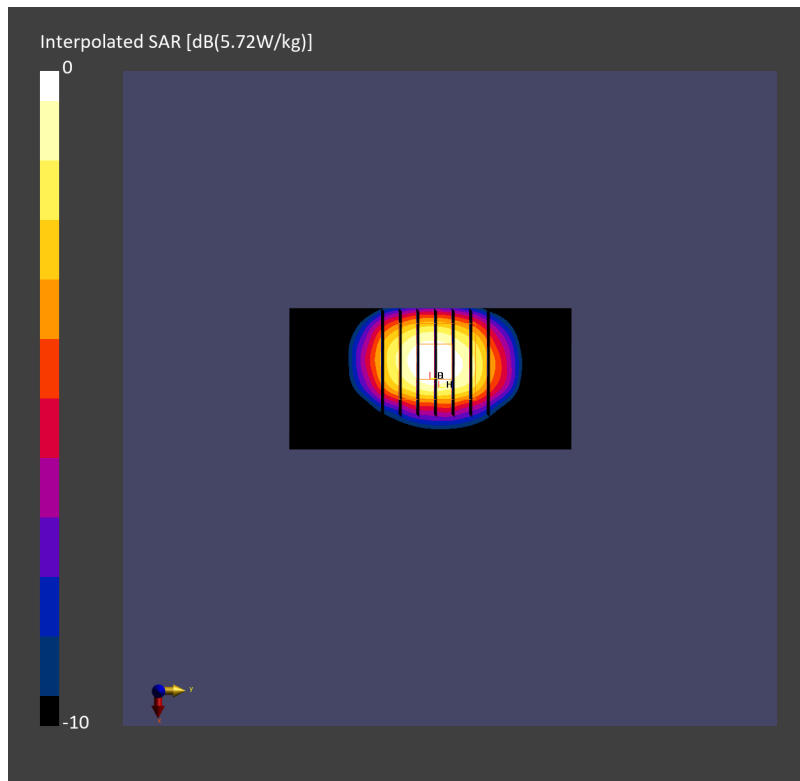

Date: 2025-02-21

**System Check\_Head\_2600MHz****DUT: D2600V2 - SN1078**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_2600\_250221 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.97$  S/m;  $\epsilon_r = 39.4$ 

Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN7694; ConvF(7.12, 6.95, 7.76); Calibrated: 2024-11-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1697; Calibrated: 2024-11-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.25 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 2.71 W/kg; SAR (8g) = 1.36 W/kg; SAR (10g) = 1.23 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 80.3 %

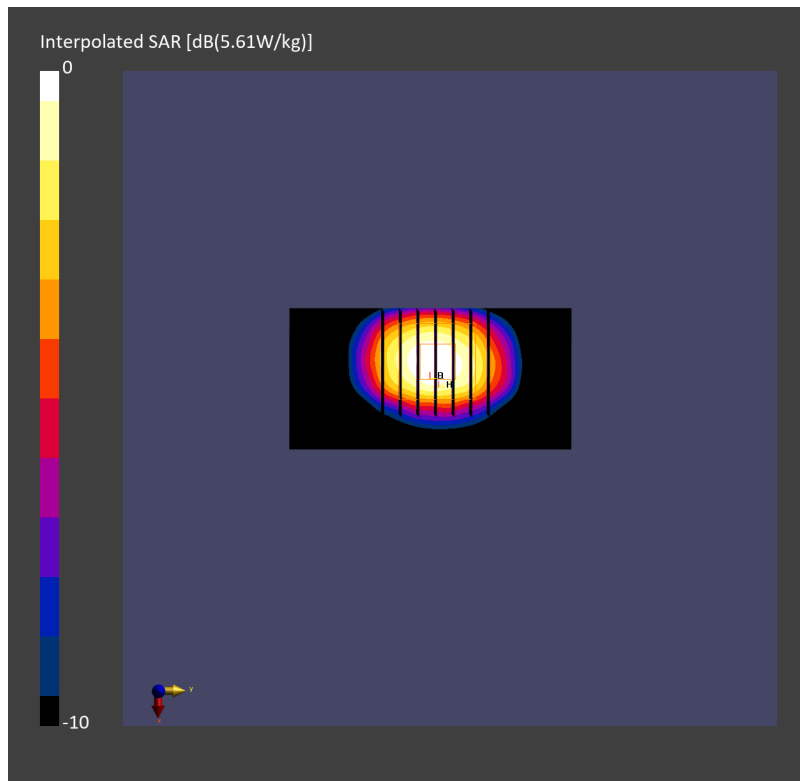

Date: 2025-03-03

**System Check\_Head\_2600MHz****DUT: D2600V2 - SN1008**

Communication System: CW; Frequency: 2600.000 MHz

Medium: HSL\_2600\_250303 Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 2.01$  S/m;  $\epsilon_r = 38.5$ 

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

## DASY6 Configuration:

- Probe: EX3DV4 - SN3976; ConvF(7.15, 7.68, 7.04); Calibrated: 2025-01-23
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1805; Calibrated: 2024-05-22
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2055; Section: Flat
- Measurement Software: 16.4.0.5005
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.73 W/kg; SAR (10g) = 1.25 W/kg;

**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.74 W/kg; SAR (8g) = 1.37 W/kg; SAR (10g) = 1.24 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 79.8 %

