

System Performance Check Report for D750V3 - SN1122

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	750.000	TSL Permittivity	42.0
Group / UID	CW / 0--	TSL Conductivity [S/m]	0.903
Conversion Factor	9.25	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7313 2025-02-24	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1671 2024-04-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.828	0.826
psSAR10g [W/Kg]	0.551	0.547
Power Drift [dB]		0.00
Dist 3dB Peak [mm]		20.5
M2/M1 [%]		89.1

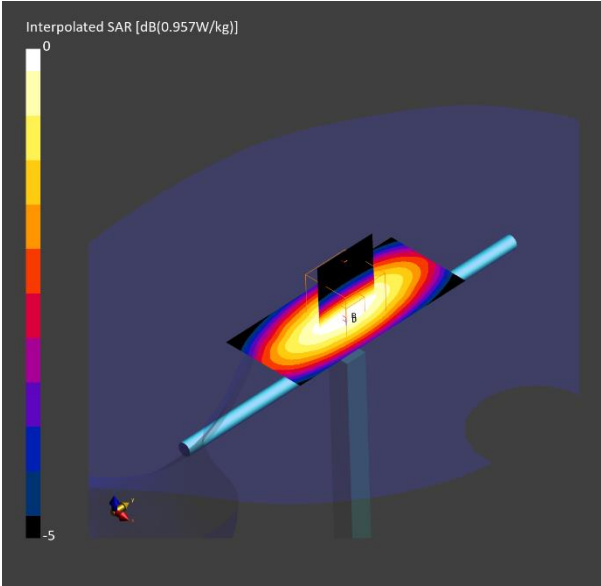

System Performance Check Report for D835V2 - SN4d174

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	835.000	TSL Permittivity	41.5
Group / UID	CW / 0--	TSL Conductivity [S/m]	0.938
Conversion Factor	8.69	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7313 2025-02-24	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1671 2024-04-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	0.978	0.982
psSAR10g [W/Kg]	0.642	0.644
Power Drift [dB]		0.00
Dist 3dB Peak [mm]		19.0
M2/M1 [%]		88.9

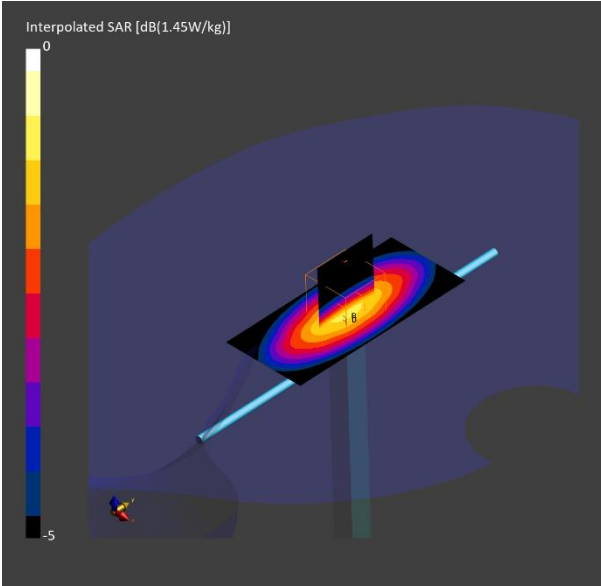

System Performance Check Report for D2450V2 - SN939

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2450.000	TSL Permittivity	38.1
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.82
Conversion Factor	6.92	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7313 2025-02-24	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1671 2024-04-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	5.26	5.05
psSAR10g [W/Kg]	2.44	2.37
Power Drift [dB]		-0.03
Dist 3dB Peak [mm]		9.0
M2/M1 [%]		81.4

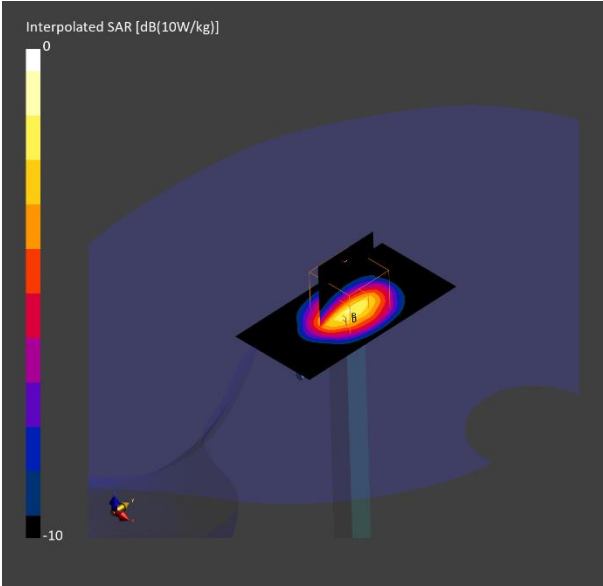

System Performance Check Report for D1900V2 - SN5d199

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1900.000	TSL Permittivity	40.5
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.45
Conversion Factor	7.51	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7313 2025-02-24	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1671 2024-04-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	4.11	4.06
psSAR10g [W/Kg]	2.13	2.11
Power Drift [dB]		-0.02
Dist 3dB Peak [mm]		10.8
M2/M1 [%]		84.1

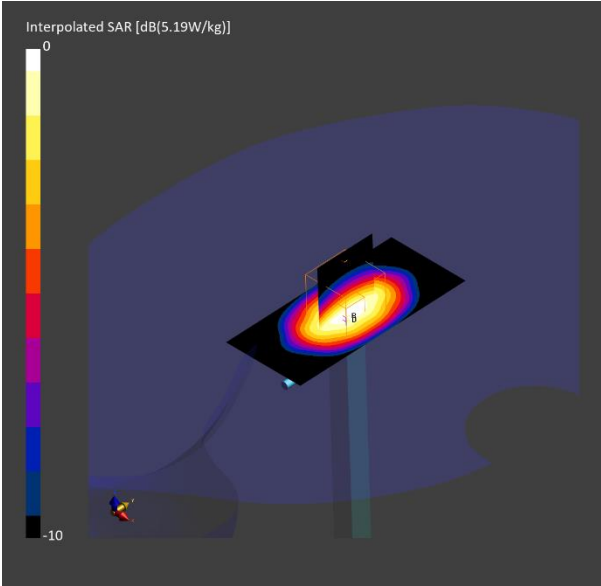

System Performance Check Report for D2600V2 - SN1097

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2600.000	TSL Permittivity	38.2
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.93
Conversion Factor	7.06	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7313 2025-02-24	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1671 2024-04-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	5.62	5.39
psSAR10g [W/Kg]	2.51	2.45
Power Drift [dB]		-0.14
Dist 3dB Peak [mm]		9.0
M2/M1 [%]		80.6

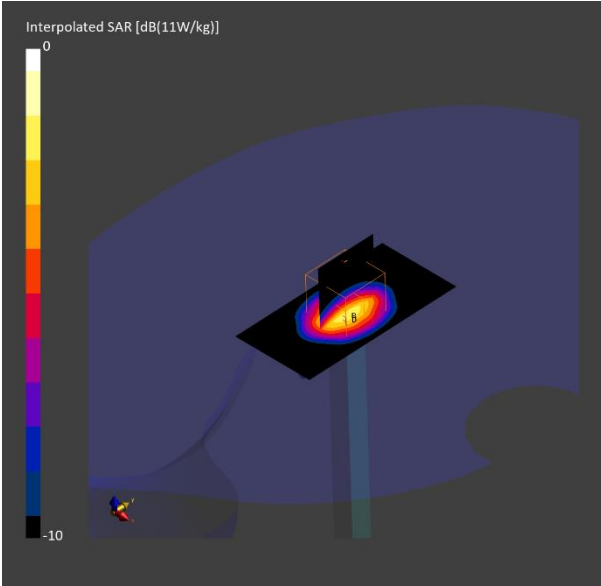

System Performance Check Report for D5GHzV2 - SN1184

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	5800.000	TSL Permittivity	35.2
Group / UID	CW / 0--	TSL Conductivity [S/m]	5.30
Conversion Factor	4.96	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7313 2025-02-24	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1667 2025-03-19	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	7.48	8.20
psSAR10g [W/Kg]	2.14	2.35
Power Drift [dB]		-0.06
Dist 3dB Peak [mm]		7.9
M2/M1 [%]		57.9

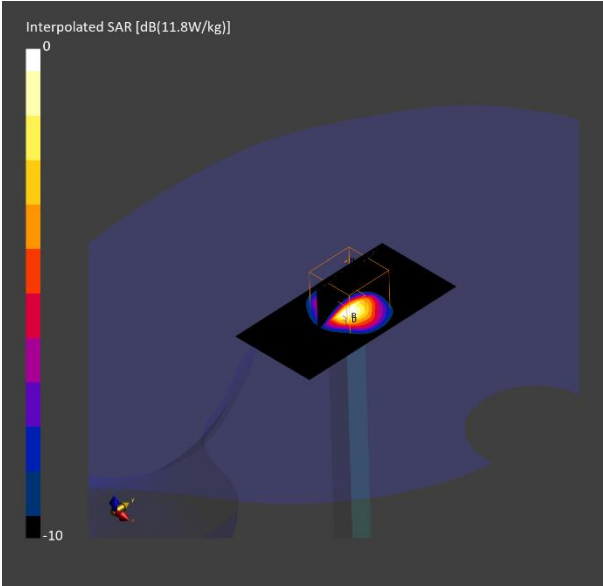

System Performance Check Report for D1750V2 - SN1125

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	1750.000	TSL Permittivity	41.2
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.35
Conversion Factor	7.74	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration

Probe Calibration Date	EX3DV4 - SN7313 2025-02-24	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1667 2025-03-19	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	3.51	3.41
psSAR10g [W/Kg]	1.88	1.83
Power Drift [dB]		-0.03
Dist 3dB Peak [mm]		10.8
M2/M1 [%]		84.9

