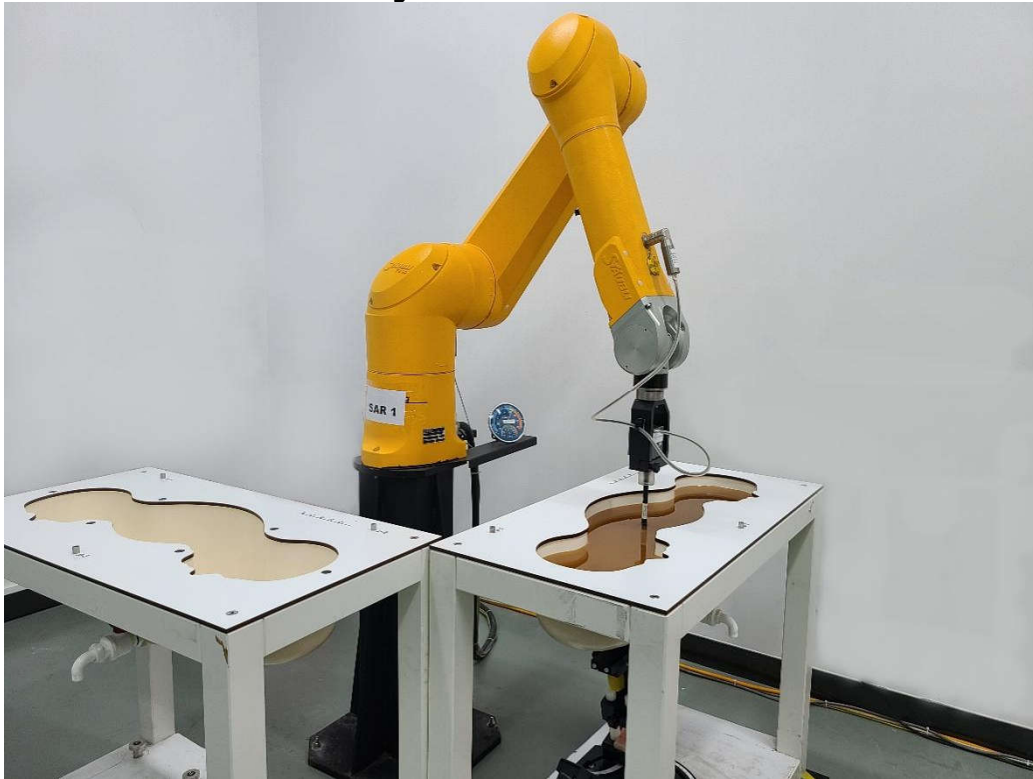


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 A photograph showing a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically next to the container, with the 10 cm mark visible. The container has a blue outer rim and a white inner lining. The liquid level is approximately 8 cm high.	NA

3. Photographs of EUT test position

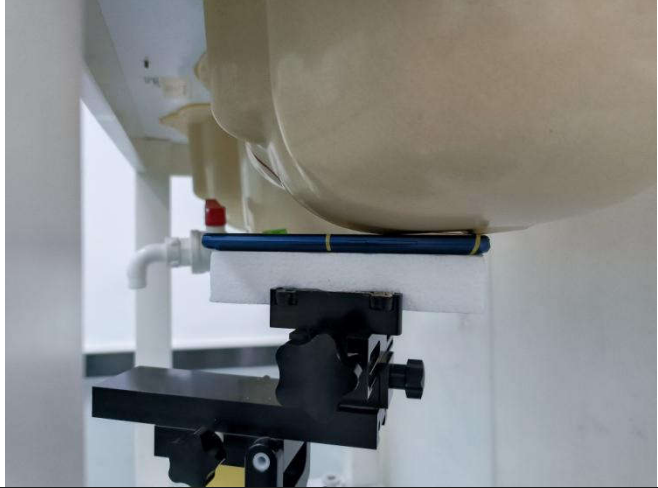
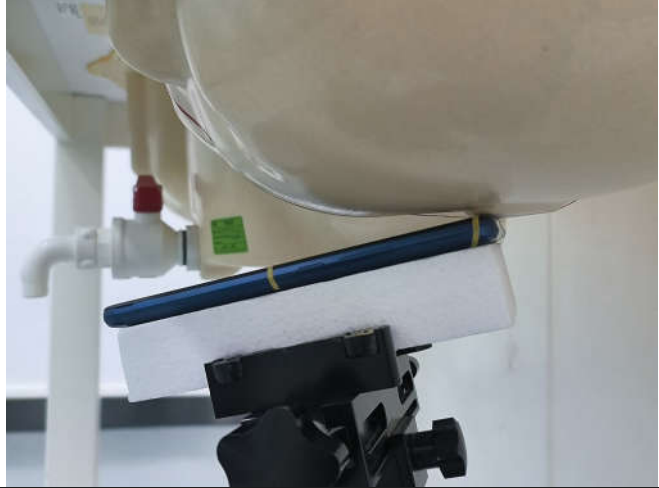
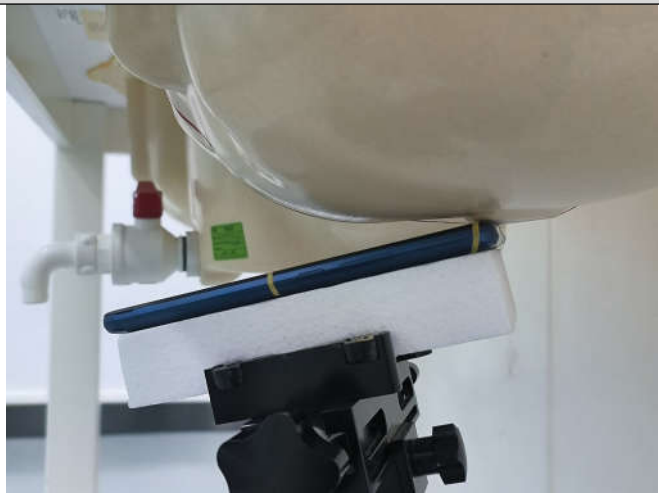
Photo 2: Left Cheek	Photo 3: Left Tilted
	
Photo 4: Right Cheek	Photo 5: Right Tilted
	
Photo 6: Front Side 15mm	Photo 7: Back Side 15mm



Photo 8: Front Side 10mm



Photo 9: Back Side 10mm



Photo 10: Left Side 10mm



Photo 11: Right Side 10mm



Photo 12: Top Side 10mm



Photo 13: Bottom Side 10mm



4. EUT Constructional Details

