

SETUP PHOTO EXHIBIT

Report Number: R14665749-EP1

Applicant : Stryker Medical
3800 E Centre Ave
Portage, MI 49002-5826

Model : LBCA1KU1WA

Contains FCC ID : Z7ALBCA1KU1WA

Contains IC : 4919E-LBCA1KU1WA

EUT Description : Bluetooth Room Interface Board

Test Standard(s) : FCC 47 CFR PART 15 SUBPART C: 2023
ISED RSS-247 ISSUE 2: 2017
ISED RSS-GEN ISSUE 5 + A2: 2021

Date Of Issue:
2023-07-06

Prepared by:
UL LLC
12 Laboratory Dr.
Research Triangle Park, NC 27709 U.S.A.
TEL: (919) 549-1400




REPORT REVISION HISTORY

Rev.	Issue Date	Revisions	Revised By
V1	2023-06-30	Initial Issue	Charles Moody
V2	2023-07-06	Updated IC and FCC ID and Model Number	Charles Moody

TABLE OF CONTENTS


REPORT REVISION HISTORY	2
TABLE OF CONTENTS	3
1. SETUP DIAGRAMS	4
2. SETUP PHOTOS.....	5
END OF TEST REPORT	11

1. SETUP DIAGRAMS


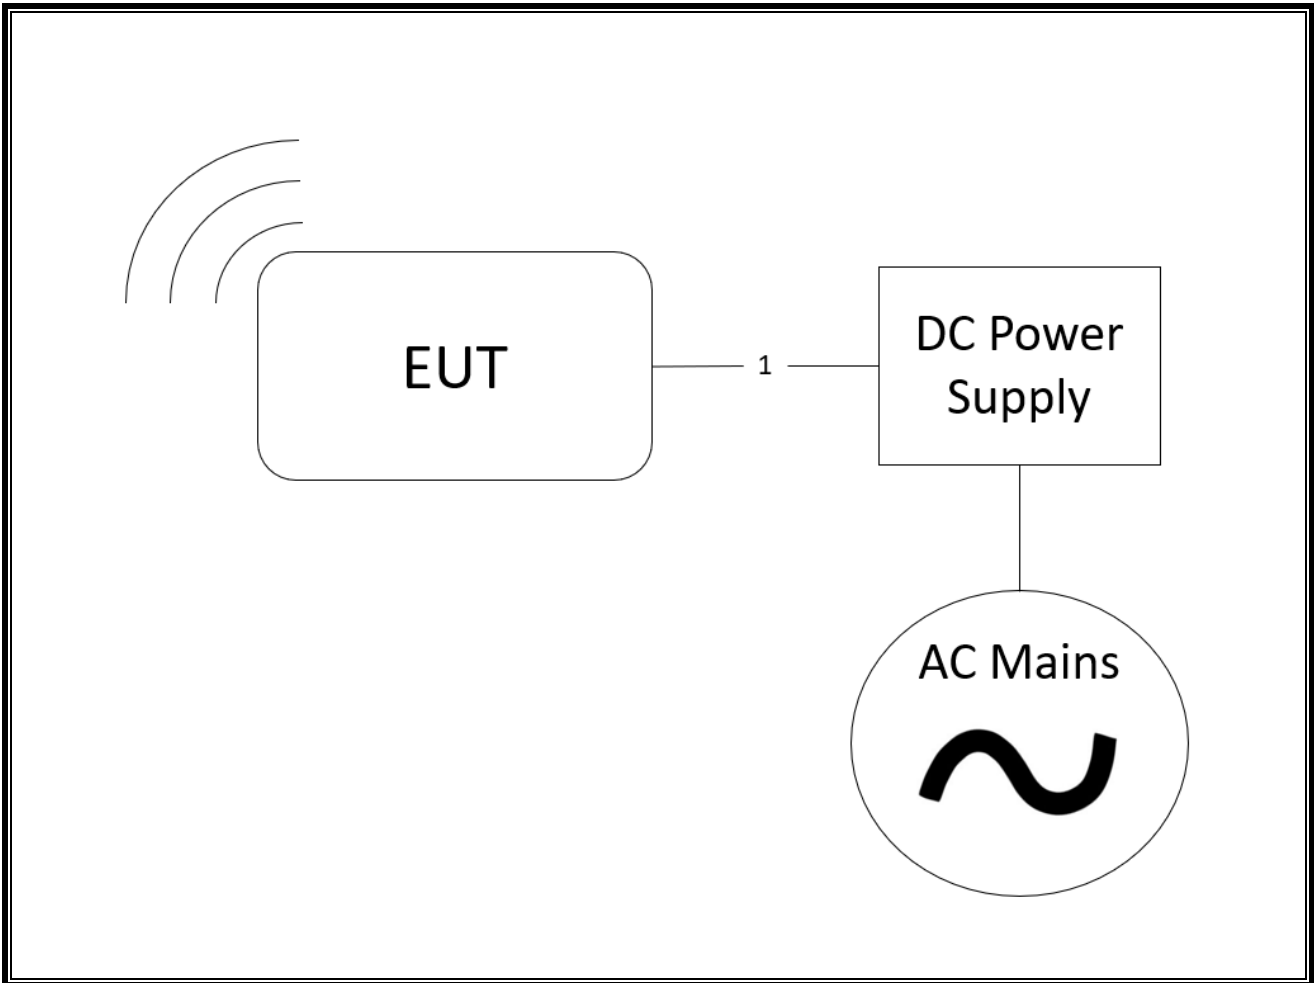


2. SETUP PHOTOS



RADIATED RF MEASUREMENT SETUP

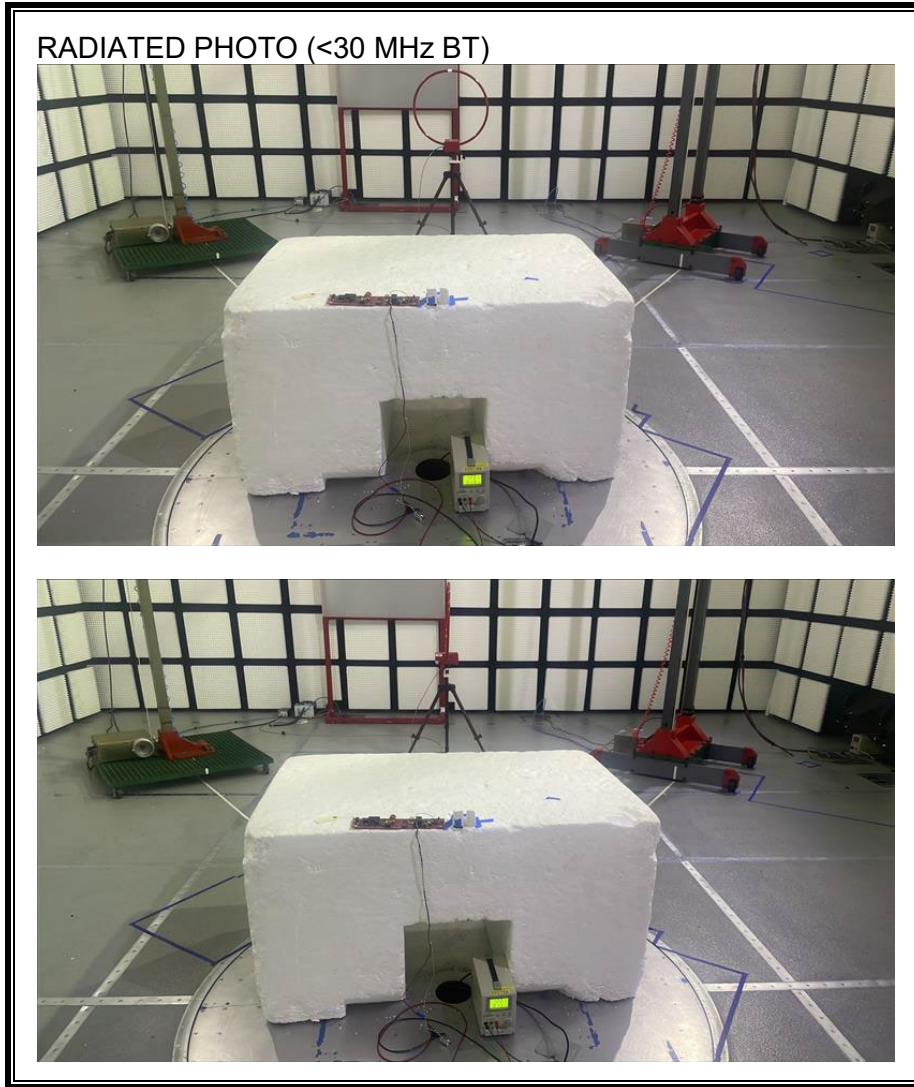



RADIATED PHOTO (<30 MHz BT)

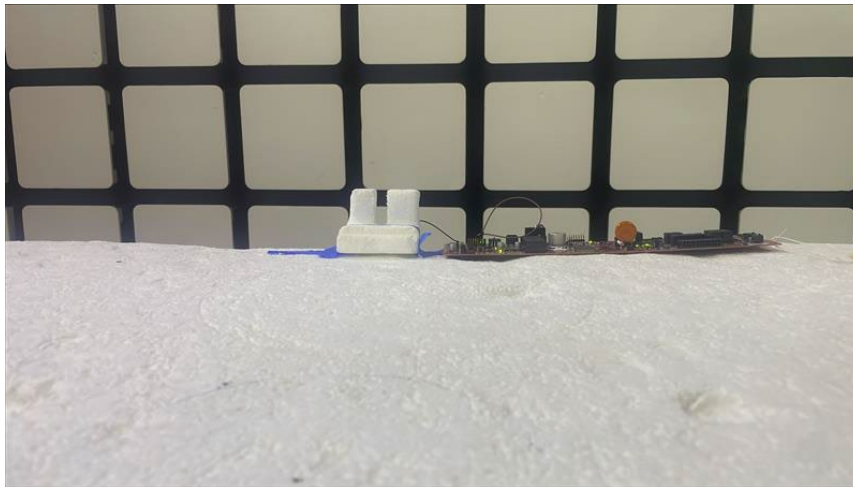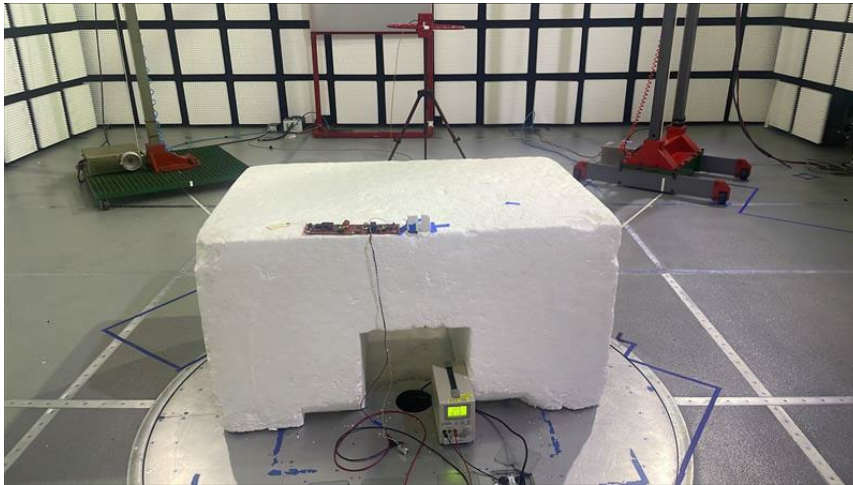

RADIATED PHOTO (30-1000MHz BT)

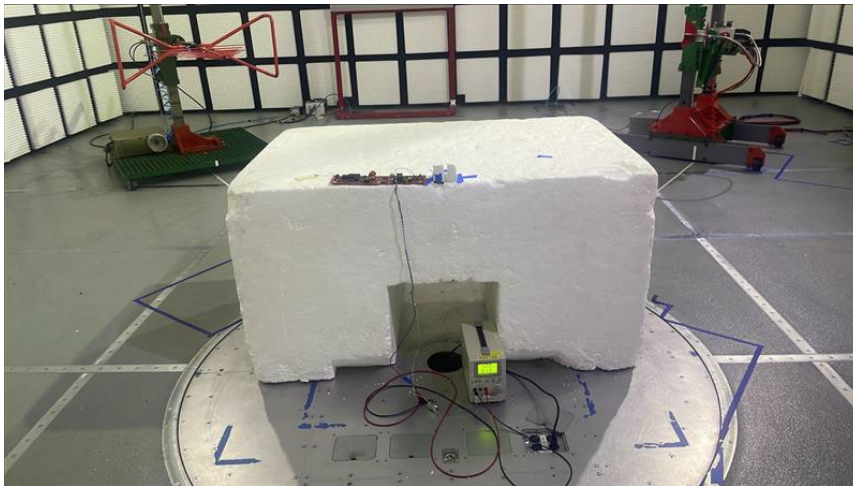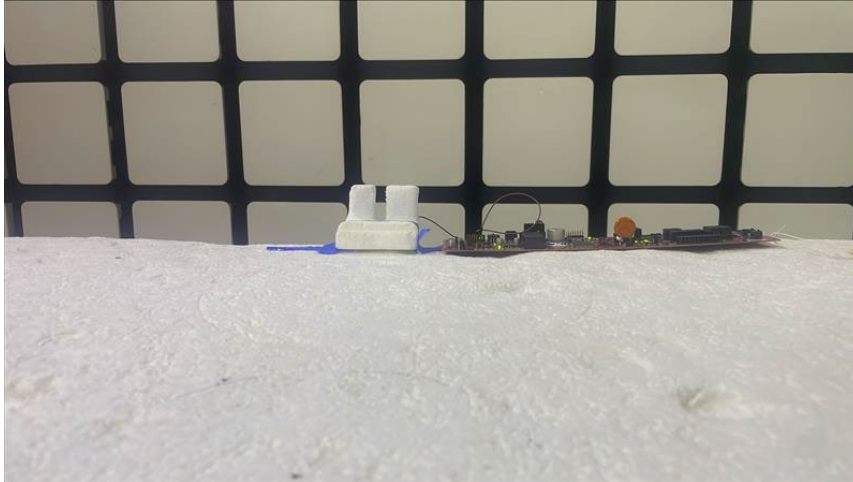


RADIATED PHOTO (>1GHz BT)

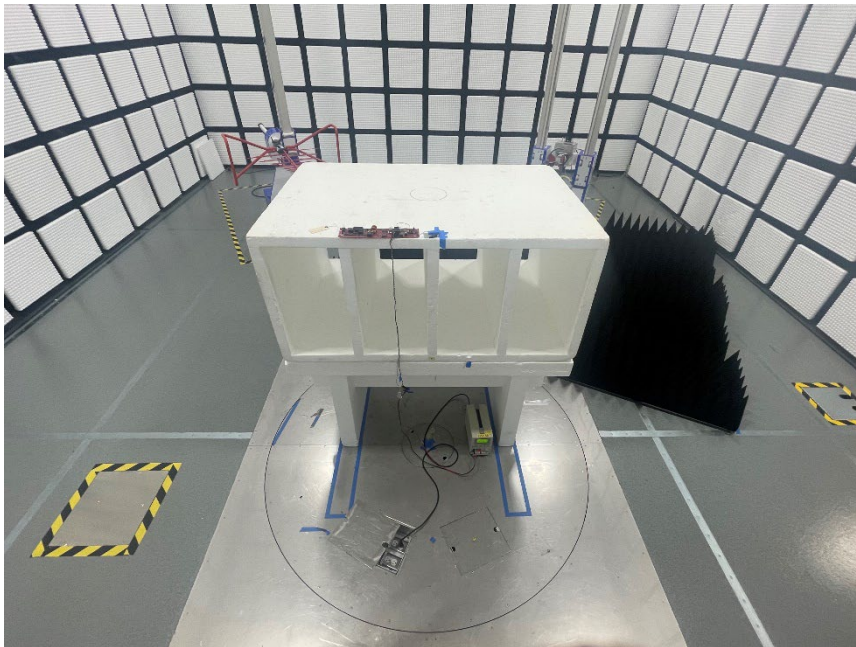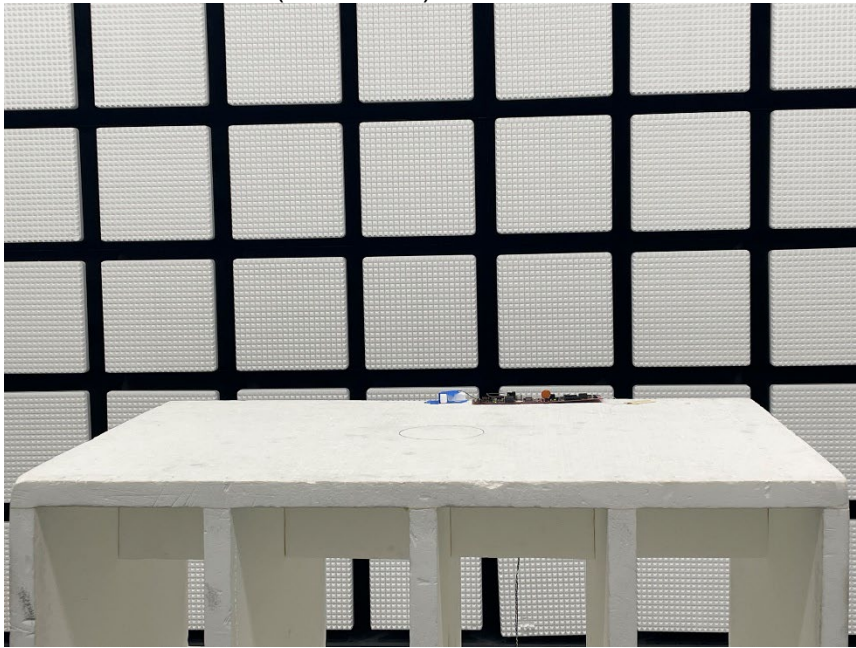


XYZ SETUP PHOTOS


X-ORIENTATION

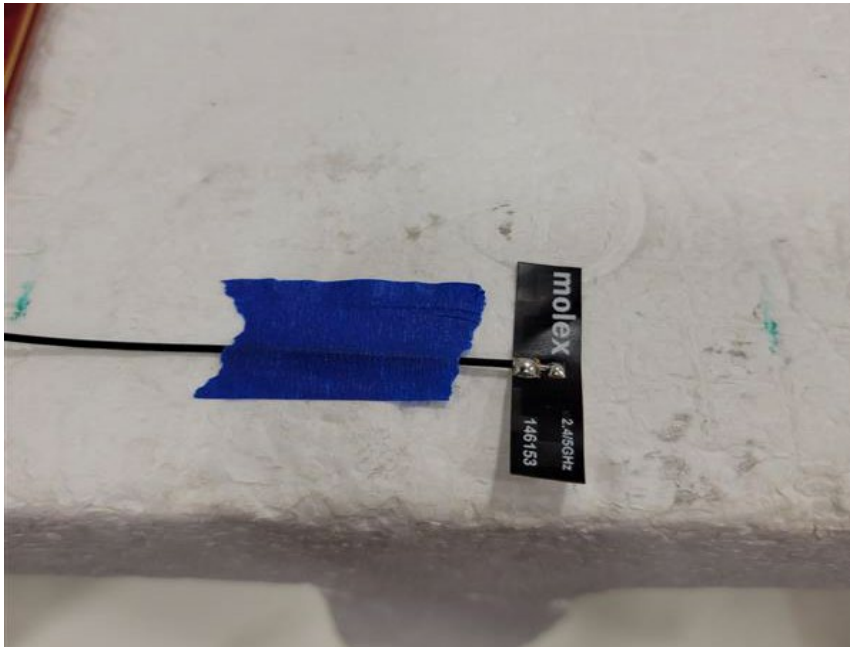

Y-ORIENTATION

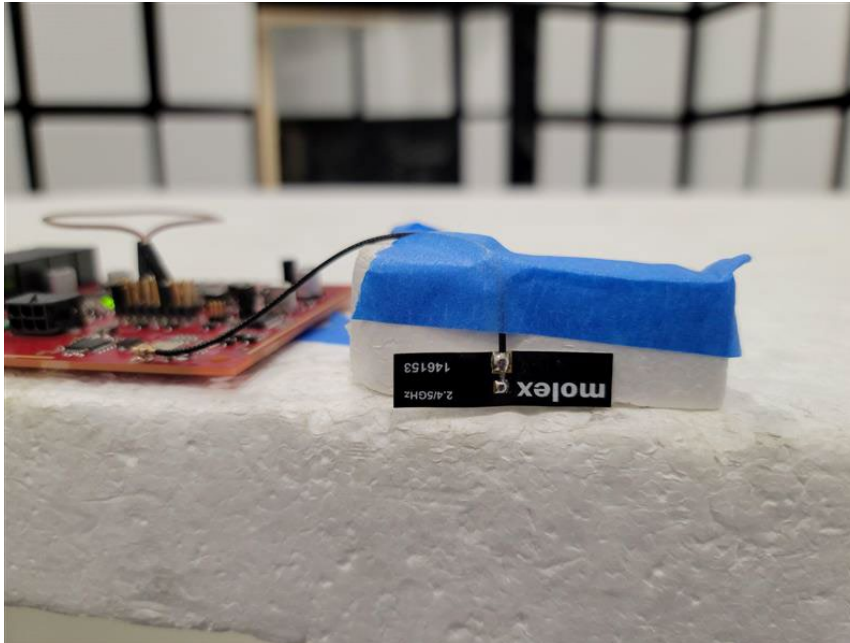

Z-ORIENTATION

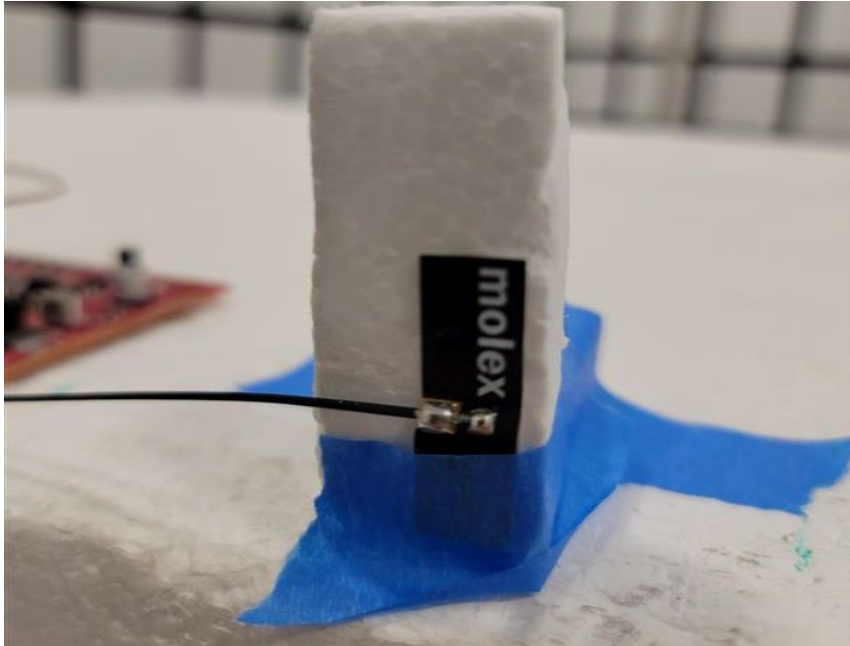

AC MAINS LINE CONDUCTED MEASUREMENT SETUP



END OF TEST REPORT