



**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
Swiss Calibration Service

Glossary

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

CW Continuous wave

Calibration is Performed According to the Following Standards

- Internal procedure QA CAL-45, Calibration procedure for sources in air above 6 GHz.
- IEC/IEEE 63195-1, "Assessment of power density of human exposure to radio frequency fields from wireless devices in close proximity to the head and body (frequency range of 6 GHz to 300 GHz)", May 2022

Methods Applied and Interpretation of Parameters

- *Coordinate System:* z-axis orthogonal to the top surface of P6500, y-axis is in the direction of the SMA connector, x-axis normal to y and z.
- *Measurement Conditions:* During the measurements, the source is directly connected to the cable and measured without the spacer. Fields are measured at the stated antenna input power. Absorbers are used around the probe cup and at the ceiling to minimize reflections.
- *Positioning:* The source is placed on the phantom and measured with the EUmmW probes at the measurement planes stated. The planes are parallel to the phantom and source surfaces. The probe distance is verified using mechanical gauges positioned on the surface of the source.
- *E- field distribution:* E field is measured in two x-y-planes with an EUmmW probe. The E-field value stated as calibration value represents the E-field-maxima and the averaged (1cm² and 4cm²) power density values at 2mm and 8mm from top surface of the source or 4mm and 10mm from top surface of the antenna patch.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the source radiating into air and absorbers present. The impedance stated is the impedance measured at the SMA connector.

Calibrated Quantity

- Local peak E-field (V/m) and average of peak spatial components of the Poynting vector (W/m²) averaged over the surface area of 1 cm² and 4cm² at the nominal operational frequency of the source. Both square and circular averaging results are listed.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY8 Module mmWave	V3.2
Phantom	5G Phantom	
Distance patch - plane	4 mm	
Number of measured planes	2 (4 mm, 4 mm + $\lambda/4$)	
Frequency	6.5 GHz $\pm$ 1 MHz	

Calibration Parameters, 6.5 GHz

Circular Averaging

Distance Antenna to Measured Plane	<i>Pin</i> (mW)	Max E-field (V/m)	Uncertainty (k = 2)	Avg Power Density Avg (psPDn+, psPDtot+, psPDmod+) (W/m ²)		Uncertainty (k = 2)
				1 cm ²	4 cm ²	
4 mm	100	453	1.27 dB	232	166	1.28 dB
	1000 ¹	1433	1.27 dB	2317	1663	1.28 dB

Distance Antenna to Measured Plane	<i>Pin</i> (mW)	Max E-field (V/m)	Uncertainty (k = 2)	Power Density psPDn+, psPDtot+, psPDmod+ (W/m ²)		Uncertainty (k = 2)
				1 cm ²	4 cm ²	
4 mm	100	453	1.27 dB	201, 219, 275	131, 156, 212	1.28 dB
	1000 ¹	1433	1.27 dB	2010, 2190, 2750	1310, 1560, 2120	1.28 dB

Square Averaging

Distance Antenna to Measured Plane	<i>Pin</i> (mW)	Max E-field (V/m)	Uncertainty (k = 2)	Avg Power Density Avg (psPDn+, psPDtot+, psPDmod+) (W/m ²)		Uncertainty (k = 2)
				1 cm ²	4 cm ²	
4 mm	100	453	1.27 dB	233	167	1.28 dB
	1000 ¹	1433	1.27 dB	2330	1670	1.28 dB

Distance Antenna to Measured Plane	<i>Pin</i> (mW)	Max E-field (V/m)	Uncertainty (k = 2)	Power Density psPDn+, psPDtot+, psPDmod+ (W/m ²)		Uncertainty (k = 2)
				1 cm ²	4 cm ²	
4 mm	100	453	1.27 dB	202, 220, 277	132, 156, 213	1.28 dB
	1000 ¹	1433	1.27 dB	2020, 2200, 2770	1320, 1560, 2130	1.28 dB

¹ Measured result normalized to 1W input power.



Max Power Density


Distance Antenna to Measured Plane	<i>Pin</i> (mW)	Max E-field (V/m)	Uncertainty (k = 2)	Max Power Density Sn, Stot, Stot (W/m ²)	Uncertainty (k = 2)
4 mm	100	453	1.27 dB	257, 278, 348	1.28 dB
	1000 ¹	1433	1.27 dB	2570, 2780, 3480	1.28 dB

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters

Impedance, transformed to feed point	72.7 Ω - 16.1 j Ω
Return Loss	- 13.0 dB

Impedance Measurement Plot

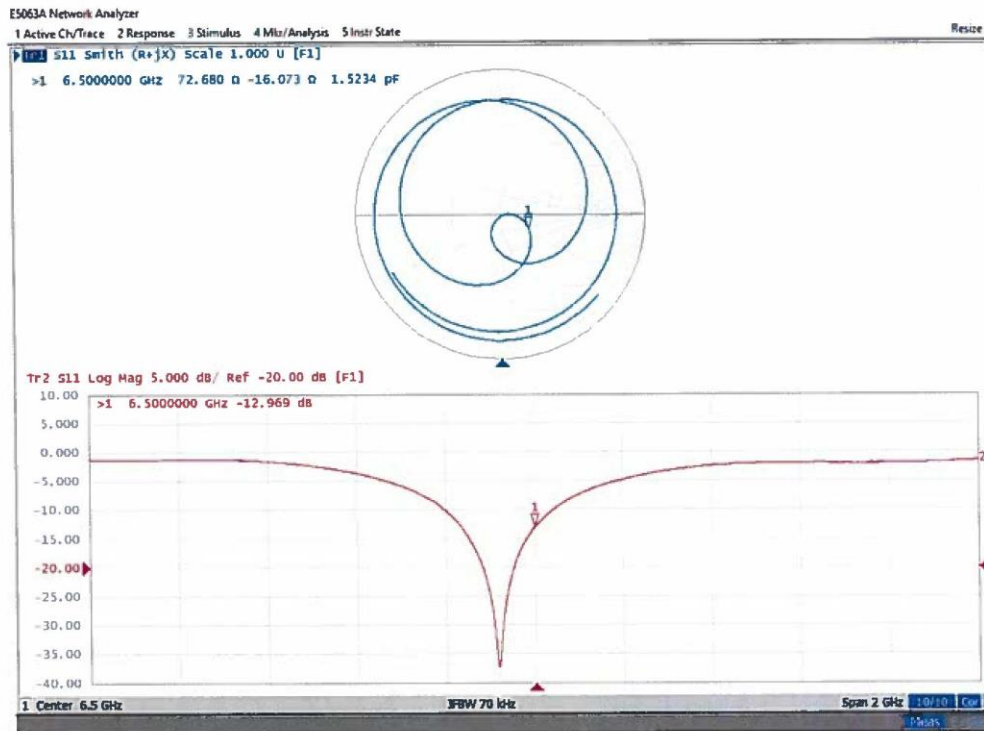



DASY Report

Measurement Report for P6500V2, UID 0 -, Channel 6500 (6500.0MHz)

Device under Test Properties

Name, Manufacturer	Dimensions [mm]	IMEI	DUT Type
P6500V2	100.0 x 100.0 x 100.0	SN: 1018	-

Exposure Conditions

Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
5G -	2.0 mm	Validation band	CW	6500.0, 6500	1.0

Hardware Setup


Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave Phantom - 1002	Air	EUmmWV4 - SN9374_F1-55GHz, 2023-05-22	DAE4 Sn1215, 2023-06-29

Scan Setup

	5G Scan
Grid Extents (auto extend) [mm]	50.0 x 90.0
Grid Steps (automatic) [lambda]	0.044 x 0.044
Sensor Surface [mm]	2.0
MAIA	MAIA not used

Measurement Results

	5G Scan
Date	2023-11-07, 11:45
Avg. Area [cm²]	1.00
Avg. Type	Circular Averaging
psPDn+ [W/m²]	201
psPDtot+ [W/m²]	219
psPDmod+ [W/m²]	275
Max(Sn) [W/m²]	257
Max(Stot) [W/m²]	278
Max(Stot) [W/m²]	348
E _{max} [V/m]	453
Power Drift [dB]	0.01

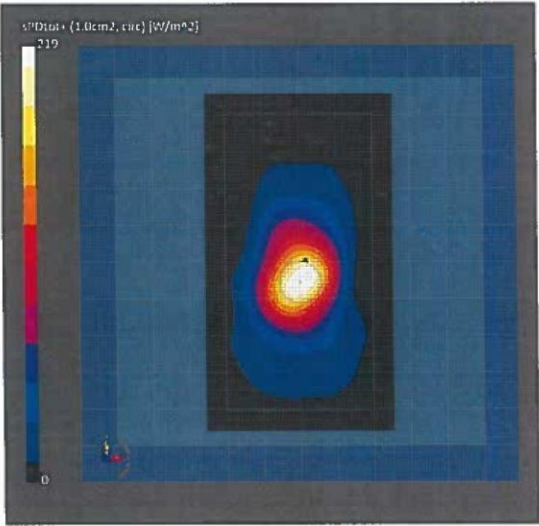



DASY Report


Measurement Report for P6500V2, UID 0 -, Channel 6500 (6500.0MHz)

Device under Test Properties			
Name, Manufacturer	Dimensions [mm]	IMEI	DUT Type
P6500V2	100.0 x 100.0 x 100.0	SN: 1018	-

Exposure Conditions					
Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
5G -	2.0 mm	Validation band	CW	6500.0, 6500	1.0

Hardware Setup			
Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave Phantom - 1002	Air	EUmmWV4 - SN9374_F1-55GHz, 2023-05-22	DAE4 Sn1215, 2023-06-29

Scan Setup		Measurement Results	
	5G Scan		5G Scan
Grid Extents (auto extend) [mm]	50.0 x 90.0	Date	2023-11-07, 11:45
Grid Steps (automatic) [lambda]	0.044 x 0.044	Avg. Area [cm²]	4.00
Sensor Surface [mm]	2.0	Avg. Type	Circular Averaging
MAIA	MAIA not used	psPDn+ [W/m²]	131
		psPDtot+ [W/m²]	156
		psPDmod+ [W/m²]	212
		Max(Sn) [W/m²]	257
		Max(Stot) [W/m²]	278
		Max(Stot) [W/m²]	348
		E _{max} [V/m]	453
		Power Drift [dB]	0.01

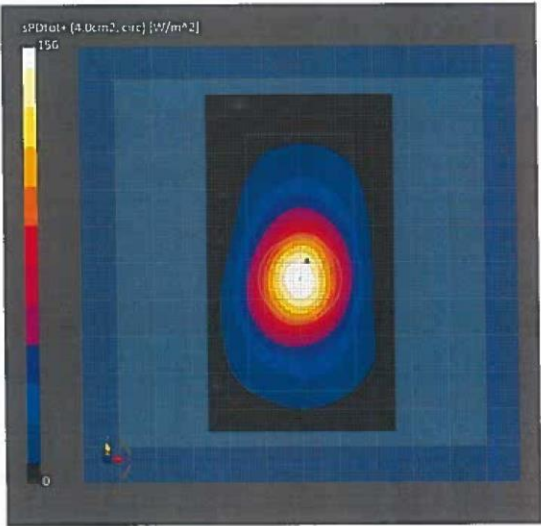



DASY Report


Measurement Report for P6500V2, UID 0 -, Channel 6500 (6500.0MHz)

Device under Test Properties			
Name, Manufacturer	Dimensions (mm)	IMEI	DUT Type
P6500V2	100.0 x 100.0 x 100.0	SN: 1018	-

Exposure Conditions					
Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
SG -	2.0 mm	Validation band	CW	6500.0, 6500	1.0

Hardware Setup			
Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date
mmWave Phantom - 1002	Air	EUmmWV4 - SN9374_F1-55GHz, 2023-05-22	DAE4 Sn1215, 2023-06-29

Scan Setup		Measurement Results	
	5G Scan		5G Scan
Grid Extents (auto extend) [mm]	50.0 x 90.0	Date	2023-11-07, 11:45
Grid Steps (automatic) [lambda]	0.044 x 0.044	Avg. Area [cm²]	1.00
Sensor Surface [mm]	2.0	Avg. Type	Square Averaging
MAIA	MAIA not used	psPDn+ [W/m²]	202
		psPDtot+ [W/m²]	220
		psPDmod+ [W/m²]	277
		Max(Sn) [W/m²]	257
		Max(Stot) [W/m²]	278
		Max(Stot) [W/m²]	348
		E _{max} [V/m]	453
		Power Drift [dB]	0.01

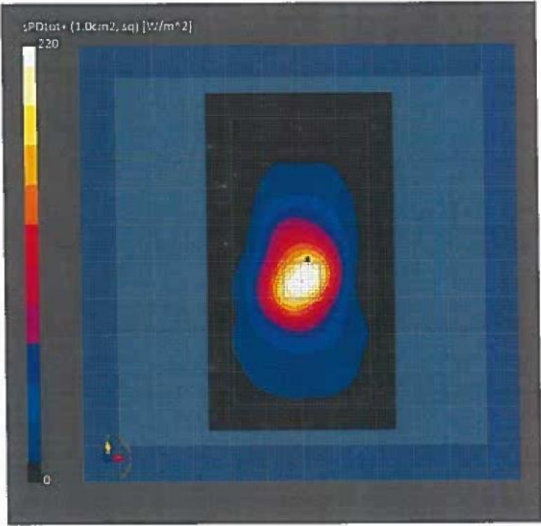



DASY Report


Measurement Report for P6500V2, UID 0 -, Channel 6500 (6500.0MHz)

Device under Test Properties			
Name, Manufacturer	Dimensions [mm]	IMEI	DUT Type
P6500V2	100.0 x 100.0 x 100.0	SN: 1018	-

Exposure Conditions	Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
5G -		2.0 mm	Validation band	CW	6500.0, 6500	1.0

Hardware Setup		Probe, Calibration Date		DAE, Calibration Date	
Phantom	Medium	Probe, Calibration Date	DAE, Calibration Date		
mmWave Phantom - 1002	Air	EUmmWV4 - SN9374_F1-55GHz, 2023-05-22	DAE4 Sn1215, 2023-06-29		

Scan Setup		Measurement Results	
		5G Scan	
Grid Extents (auto extend) [mm]	50.0 x 90.0	Date	2023-11-07, 11:45
Grid Steps (automatic) [lambda]	0.044 x 0.044	Avg. Area [cm²]	4.00
Sensor Surface [mm]	2.0	Avg. Type	Square Averaging
MAIA	MAIA not used	psPDn+ [W/m²]	132
		psPDtot+ [W/m²]	156
		psPDmod+ [W/m²]	213
		Max(Sn) [W/m²]	257
		Max(Stot) [W/m²]	278
		Max(Stot) [W/m²]	348
		E _{max} [V/m]	453
		Power Drift [dB]	0.01

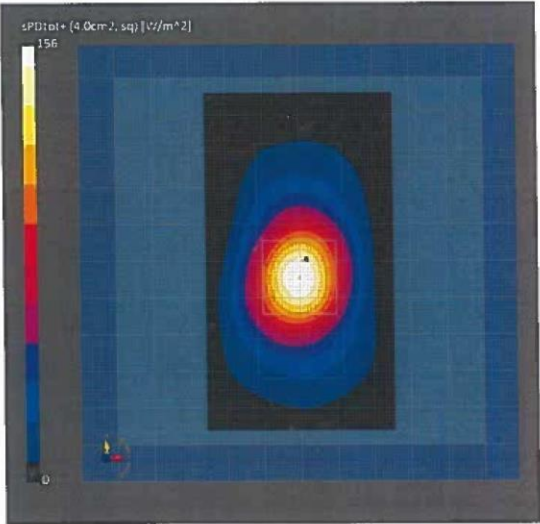



**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S S S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **TÜV SÜD**
Fareham, United Kingdom

Certificate No. **D2450V2-715_Dec23**

CALIBRATION CERTIFICATE

Object **D2450V2 - SN:715**

Calibration procedure(s) **QA CAL-05.v12
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **December 07, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP2	SN: 104778	30-Mar-23 (No. 217-03804/03805)	Mar-24
Power sensor NRP-Z91	SN: 103244	30-Mar-23 (No. 217-03804)	Mar-24
Power sensor NRP-Z91	SN: 103245	30-Mar-23 (No. 217-03805)	Mar-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Type-N mismatch combination	SN: 310982 / 06327	30-Mar-23 (No. 217-03810)	Mar-24
Reference Probe EX3DV4	SN: 7349	03-Nov-23 (No. EX3-7349_Nov23)	Nov-24
DAE4	SN: 601	03-Oct-23 (No. DAE4-601_Oct23)	Oct-24
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
Power sensor HP 8481A	SN: MY41093315	07-Oct-15 (in house check Oct-22)	In house check: Oct-24
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-22)	In house check: Oct-24
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-22)	In house check: Oct-24

Calibrated by:	Name Paulo Pina	Function Laboratory Technician	Signature
Approved by:	Sven Kühn	Technical Manager	

Issued: December 8, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:** This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.3 $\pm$ 6 %	1.85 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.4 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.6 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.21 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	53.0 $\pm$ 6 %	2.01 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	---	---

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.5 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	49.3 W/kg $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.93 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.6 W/kg $\pm$ 16.5 % (k=2)



Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$51.7 \Omega + 2.1 j\Omega$
Return Loss	- 31.6 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$49.4 \Omega + 2.5 j\Omega$
Return Loss	- 31.8 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.157 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 07.12.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:715

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 38.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.96, 7.96, 7.96) @ 2450 MHz; Calibrated: 03.11.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 116.1 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 26.5 W/kg

SAR(1 g) = 13.4 W/kg; SAR(10 g) = 6.21 W/kg

Smallest distance from peaks to all points 3 dB below = 9 mm


Ratio of SAR at M2 to SAR at M1 = 50.6%

Maximum value of SAR (measured) = 21.9 W/kg

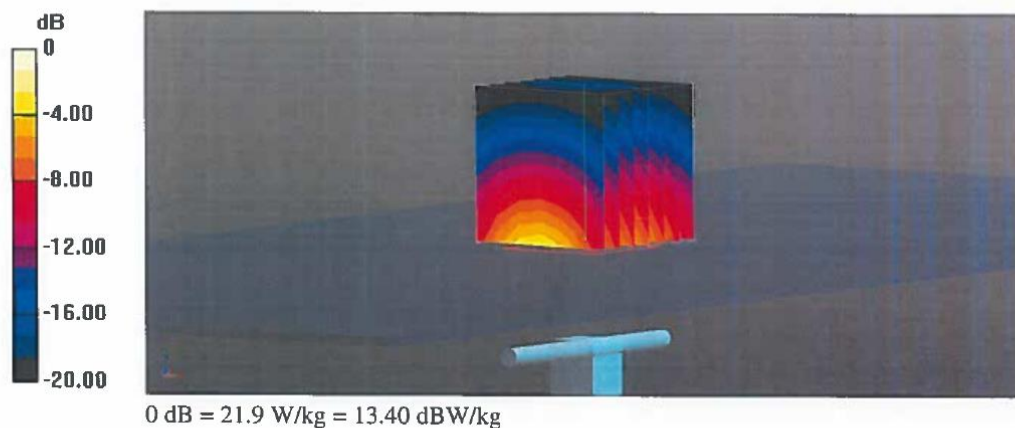



Impedance Measurement Plot for Head TSL

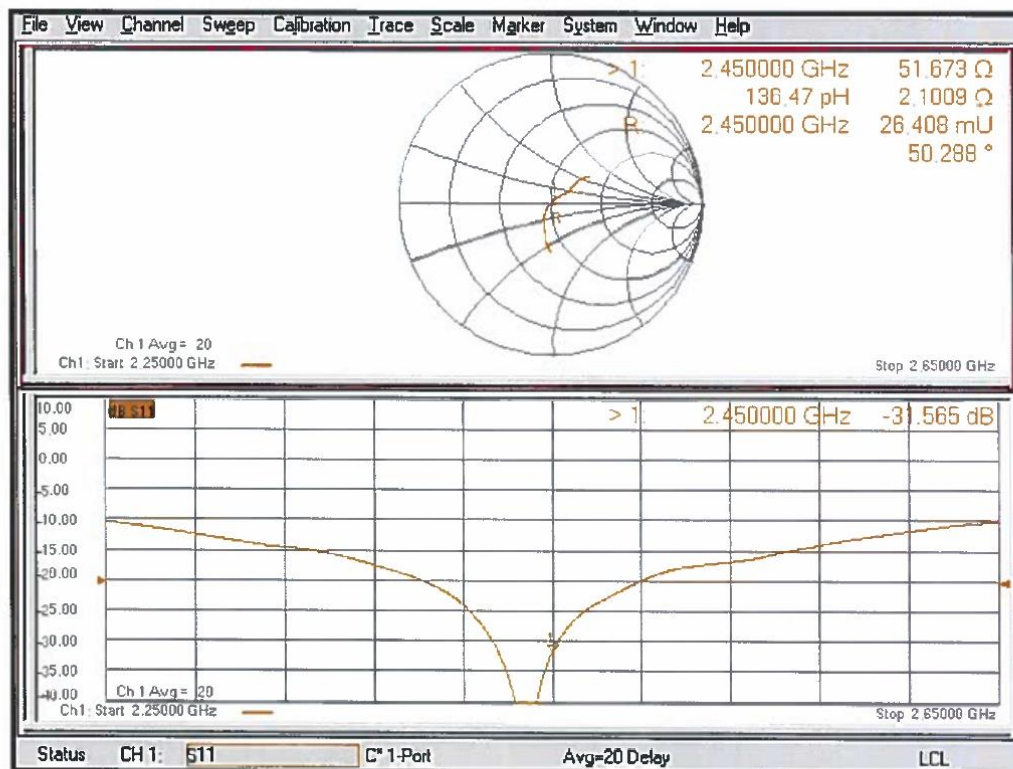

DASY5 Validation Report for Body TSL

Date: 06.12.2023

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:715

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 2.01$ S/m; $\epsilon_r = 53$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.12, 8.12, 8.12) @ 2450 MHz; Calibrated: 03.11.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.10.2023
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 107.3 V/m; Power Drift = 0.08 dB


Peak SAR (extrapolated) = 23.3 W/kg

SAR(1 g) = 12.5 W/kg; SAR(10 g) = 5.93 W/kg

Smallest distance from peaks to all points 3 dB below = 8.9 mm


Ratio of SAR at M2 to SAR at M1 = 54.6%

Maximum value of SAR (measured) = 20.0 W/kg

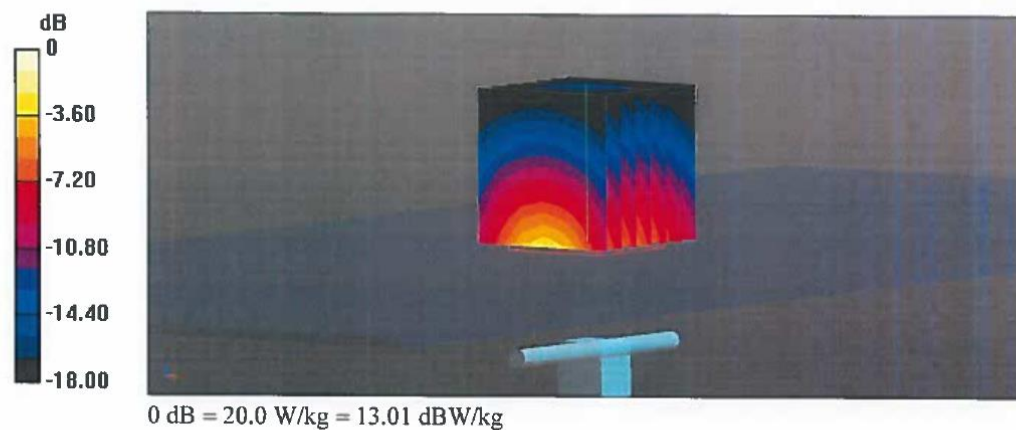



Impedance Measurement Plot for Body TSL

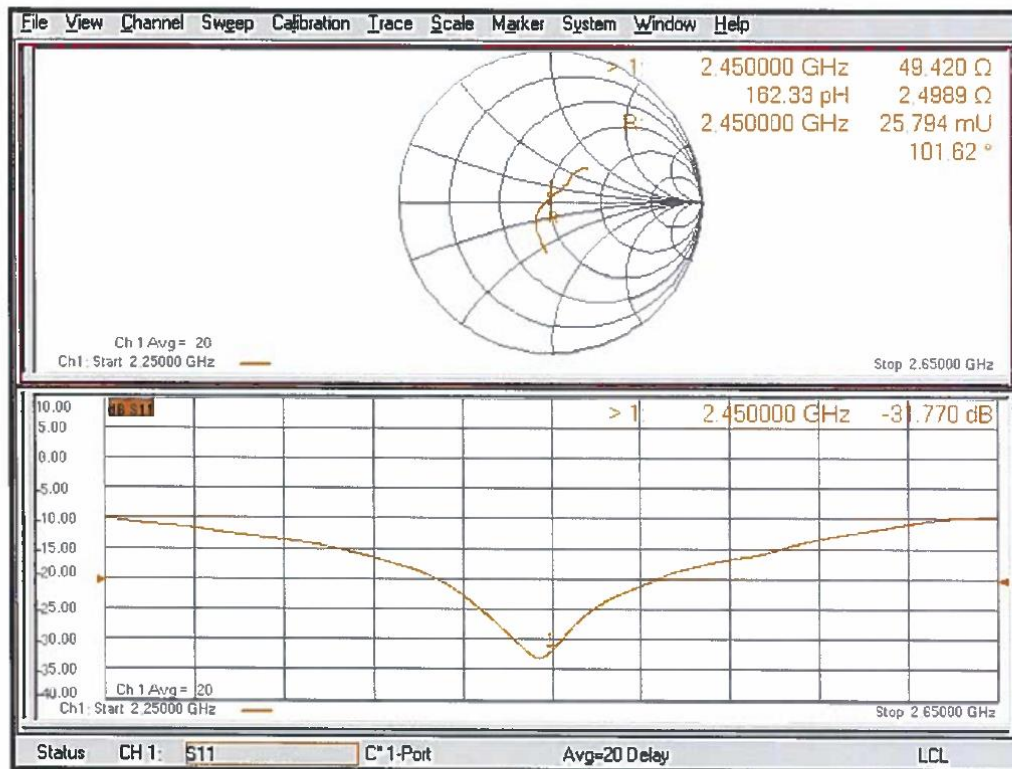



**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **TÜV SÜD**
Fareham, United Kingdom

Certificate No. **D6.5GHzV2-1070_Nov23**

CALIBRATION CERTIFICATE

Object **D6.5GHzV2 - SN:1070**

Calibration procedure(s) **QA CAL-22.v7
Calibration Procedure for SAR Validation Sources between 3-10 GHz**

Calibration date: **November 02, 2023**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power sensor R&S NRP33T	SN: 100967	03-Apr-23 (No. 217-03806)	Apr-24
Reference 20 dB Attenuator	SN: BH9394 (20k)	30-Mar-23 (No. 217-03809)	Mar-24
Mismatch combination	SN: 84224 / 360D	03-Apr-23 (No. 217-03812)	Apr-24
Reference Probe EX3DV4	SN: 7405	12-Jun-23 (No. EX3-7405_Jun23)	Jun-24
DAE4	SN: 908	03-Jul-23 (No. DAE4-908_Jul23)	Jul-24
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator Anapico APSIN20G	SN: 827	18-Dec-18 (in house check Dec-21)	In house check: Dec-23
Power sensor NRP-Z23	SN: 100169	10-Jan-19 (in house check Nov-22)	In house check: Nov-23
Power sensor NRP-18T	SN: 100950	28-Sep-22 (in house check Nov-22)	In house check: Nov-23
Network Analyzer Keysight E5063A	SN:MY54504221	31-Oct-19 (in house check Oct-22)	In house check: Oct-25

Calibrated by:	Name Aldonia Georgiadou	Function Laboratory Technician	Signature
Approved by:	Sven Kühn	Technical Manager	

Issued: November 2, 2023

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range Of 4 MHz To 10 GHz)", October 2020.

Additional Documentation:

- b) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The Return Loss ensures low reflected power. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.
- *The absorbed power density (APD):* The absorbed power density is evaluated according to Samaras T, Christ A, Kuster N, "Compliance assessment of the epithelial or absorbed power density above 6 GHz using SAR measurement systems", Bioelectromagnetics, 2021 (submitted). The additional evaluation uncertainty of 0.55 dB (rectangular distribution) is considered.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY6	V16.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	5 mm	with Spacer
Zoom Scan Resolution	dx, dy = 3.4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	6500 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	34.5	6.07 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	34.6 $\pm$ 6 %	6.18 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	29.6 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	296 W/kg $\pm$ 24.7 % (k=2)

SAR averaged over 8 cm ³ (8 g) of Head TSL	Condition	
SAR measured	100 mW input power	6.66 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	66.6 W/kg $\pm$ 24.4 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	5.46 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	54.6 W/kg $\pm$ 24.4 % (k=2)



Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.1 Ω - 3.5 j Ω
Return Loss	- 28.8 dB

APD (Absorbed Power Density)

APD averaged over 1 cm ²	Condition	
APD measured	100 mW input power	296 W/m ²
APD measured	normalized to 1W	2960 W/m ² $\pm$ 29.2 % (k=2)

APD averaged over 4 cm ²	condition	
APD measured	100 mW input power	133 W/m ²
APD measured	normalized to 1W	1330 W/m ² $\pm$ 28.9 % (k=2)

*The reported APD values have been derived using the psSAR1g and psSAR8g.

General Antenna Parameters and Design

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------



DASY6 Validation Report for Head TSL


Measurement Report for D6.5GHz-1070, UID 0 -, Channel 6500 (6500.0MHz)

Device under Test Properties			
Name, Manufacturer	Dimensions [mm]	IMEI	DUT Type
D6.5GHz	10.0 x 10.0 x 10.0	SN: 1070	-


Exposure Conditions							
Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz]	Conversion Factor	TSL Cond. [S/m]	TSL Permittivity
Flat, HSL	5.00	Band	CW,	6500	5.50	6.18	34.6

Hardware Setup			
Phantom	TSL	Probe, Calibration Date	DAE, Calibration Date
MFP V8.0 Center - 1182	HBBL600-10000V6	EX3DV4 - SN7405, 2023-06-12	DAE4 Sn908, 2023-07-03

Scan Setup		Measurement Results	
	Zoom Scan		Zoom Scan
Grid Extents [mm]	22.0 x 22.0 x 22.0	Date	2023-11-02, 12:59
Grid Steps [mm]	3.4 x 3.4 x 1.4	psSAR1g [W/Kg]	29.6
Sensor Surface [mm]	1.4	psSAR8g [W/Kg]	6.66
Graded Grid	Yes	psSAR10g [W/Kg]	5.46
Grading Ratio	1.4	Power Drift [dB]	0.02
MAIA	N/A	Power Scaling	Disabled
Surface Detection	VMS + 6p	Scaling Factor [dB]	
Scan Method	Measured	TSL Correction	No correction
		M2/M1 [%]	51.2
		Dist 3dB Peak [mm]	4.6

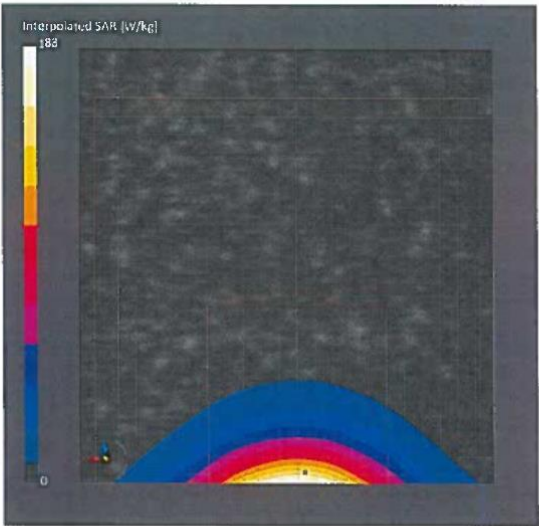

Impedance Measurement Plot for Head TSL

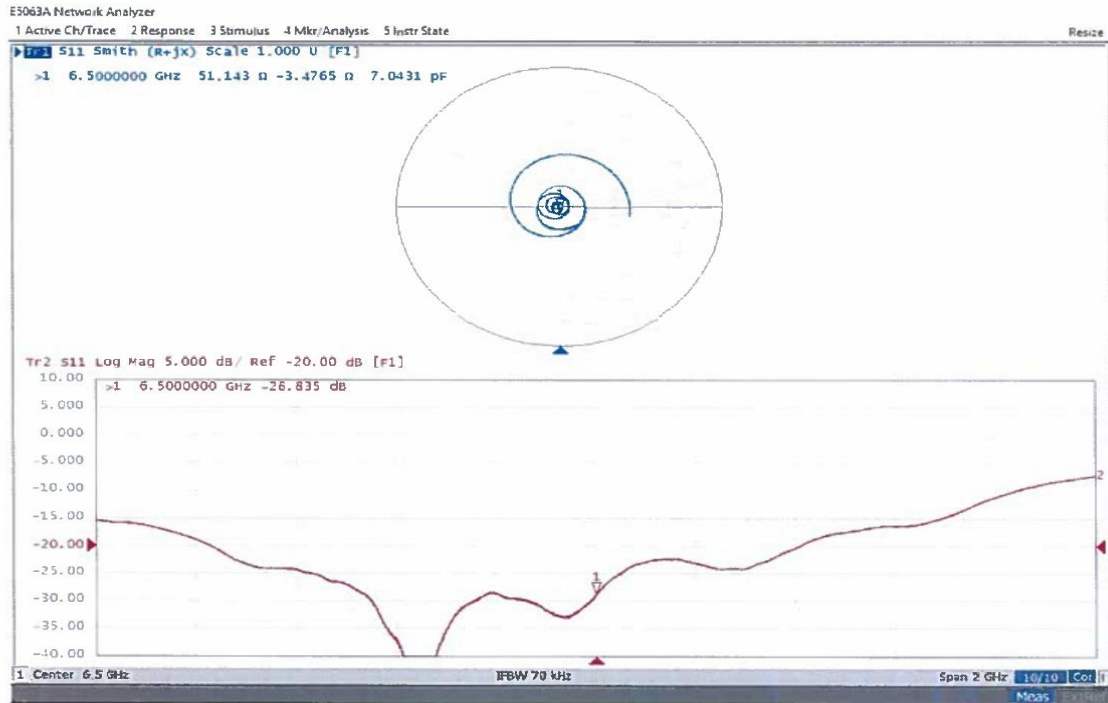



ANNEX C

TEST RESULTS



Measurement Report for A3185, BACK, ISM 2.4 GHz Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 78 (2480.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	ISM 2.4 GHz Band	Bluetooth, 10032-CAA	2480.0, 78	7.22	1.83	39.4

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2102	HBBL-600-10000 DAK 3.5 Head ELI 20.66 deg.C 2024-Sep-09 SYS3 B3.prn, 2024-Sep-09	EX3DV4 - SN7804, 2024-08-14	DAE4ip Sn1786, 2024-08-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
MAIA	N/A	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-09, 21:54	2024-09-09, 22:05
psSAR1g [W/Kg]	0.225	0.235
psSAR10g [W/Kg]	0.109	0.105
Power Drift [dB]	-0.02	-0.04
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		73.8
Dist 3dB Peak [mm]		8.0

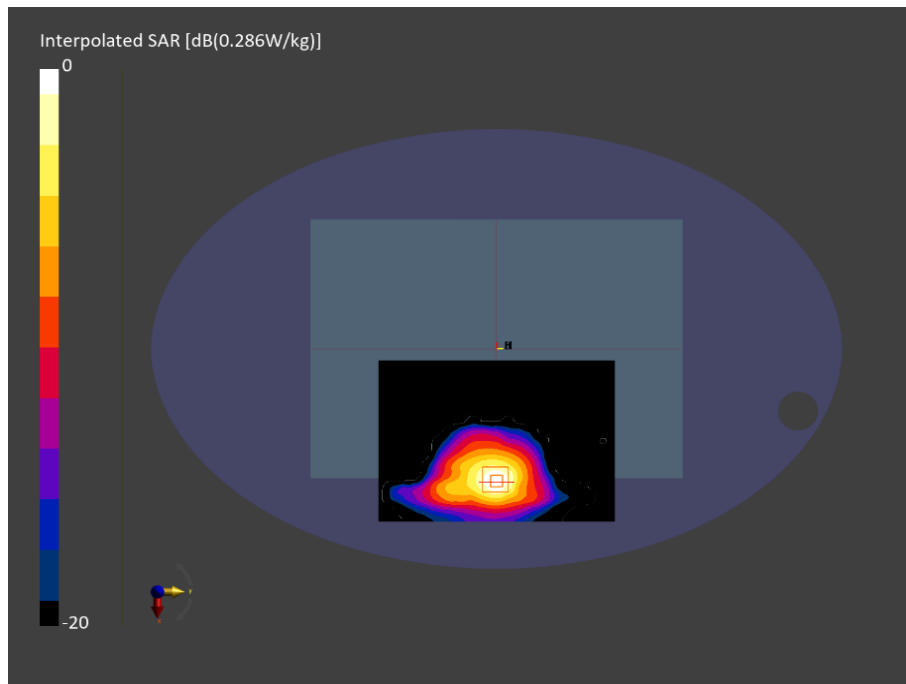


Figure C.01: SAR testing results for the A3185 at 2480 MHz core 0



Measurement Report for A3185, BACK, ISM 2.4 GHz Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 78 (2480.000 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	ISM 2.4 GHz Band	Bluetooth, 10032-CAA	2480.000, 78	7.22	1.83	39.4

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2102	HBBL-600-10000 DAK 3.5 Head ELI 20.66 deg.C 2024-Sep-09 SYS3 B3.prn, 2024-Sep-09	EX3DV4 - SN7804, 2024-08-14	DAE4ip Sn1786, 2024-08-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5
MAIA	Y	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-10, 00:11	2024-09-10, 00:22
psSAR1g [W/Kg]	0.165	0.160
psSAR10g [W/Kg]	0.078	0.070
Power Drift [dB]	0.04	0.04
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		74.5
Dist 3dB Peak [mm]		8.6

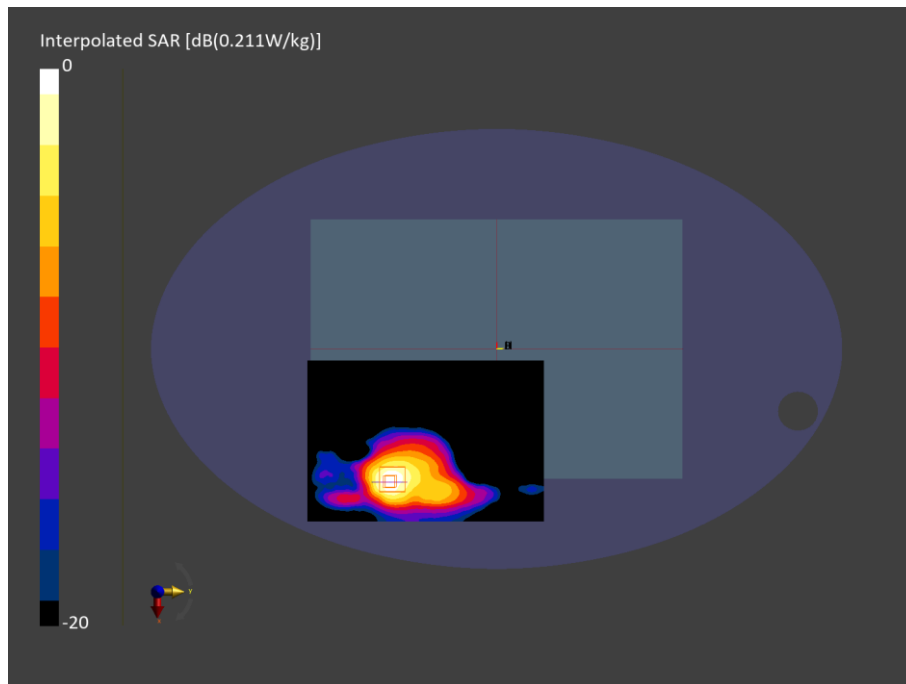


Figure C.02: SAR testing results for the A3185 at 2480 MHz core 1



Measurement Report for A3185, BACK, ISM 2.4 GHz Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 39 (2441.000 MHz)

Device Under Test Properties

del, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	ISM 2.4 GHz Band	Bluetooth, 10032-CAA	2441.0, 39	7.22	1.79	39.4

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) – 2102	HBBL-600-10000 DAK 3.5 Head ELI 20.66 deg.C 2024-Sep-09 SYS3 B3.prn, 2024-Sep-09	EX3DV4 – SN7804, 2024-08-14	DAE4ip Sn1786, 2024-08-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.5
MAIA	Y	Y
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-10, 04:12	2024-09-10, 04:30
psSAR1g [W/Kg]	0.087	0.084
SAR10g [W/Kg]	0.042	0.038
Power Drift [dB]	0.11	-0.03
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		73.2
Dist 3dB Peak [mm]		7.9

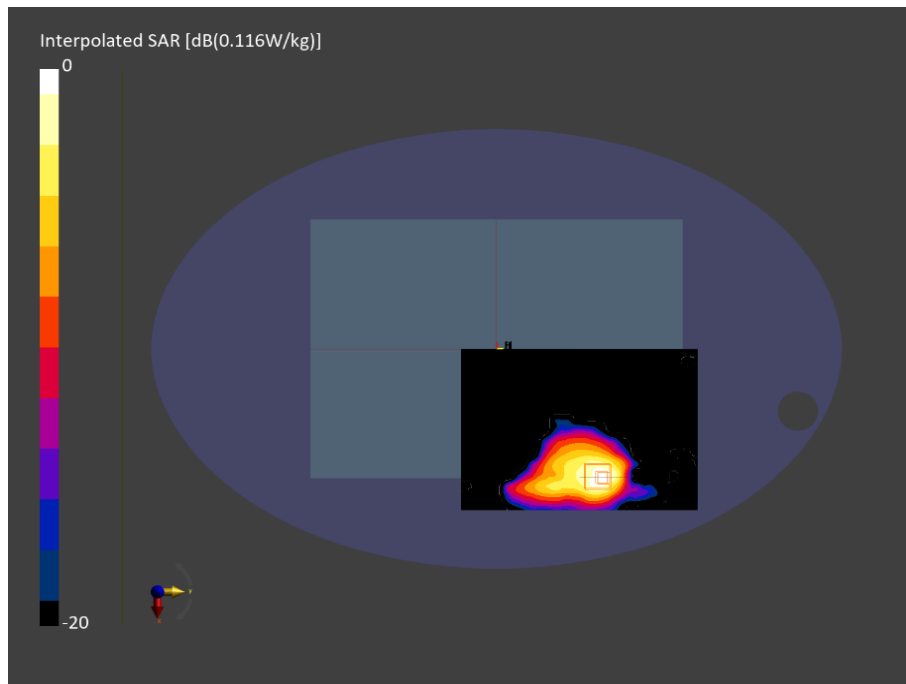


Figure C.03: SAR testing results for the A3185 at 2441 MHz core 2



Measurement Report for A3185, BACK, Custom Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 5250000 (5250.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 10032-CAA	5250.0, 5250000	5.18	4.55	35.2

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) – 2202	HBBL-600-10000 DAK 3.5 Head ELI 20.68 deg.C 2024-Sep-09 SYS5 B5 .prn, 2024-Sep-09	EX3DV4 – SN7805, 2024-02-14	DAE4ip Sn1785, 2024-02-13

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	n/a	Yes
ading Ratio	n/a	1.4
MAIA	Y	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-11, 06:30	2024-09-11, 06:38
psSAR1g [W/Kg]	0.564	0.630
psSAR10g [W/Kg]	0.210	0.212
Power Drift [dB]	0.17	0.04
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		59.6
Dist 3dB Peak [mm]		8.7

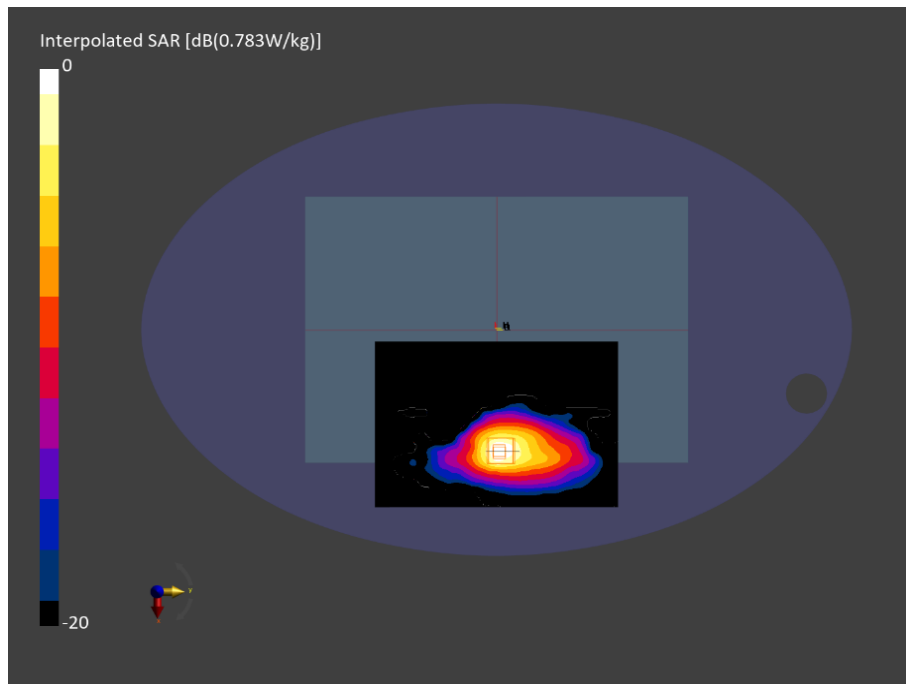


Figure C.04: SAR testing results for the A3185 at 5250 MHz core 0



Measurement Report for A3185, BACK, Custom Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 5250000 (5250.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 10032-CAA	5250.0, 5250000	5.18	4.55	35.2

Hardware Setup

antom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) – 2202	HBBL-600-10000 DAK 3.5 Head ELI 20.68 deg.C 2024-Sep-09 SYS5 B5 .prn, 2024-Sep-09	EX3DV4 – SN7805, 2024-02-14	DAE4ip Sn1785, 2024-02-13

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
MAIA	Y	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-11, 07:29	2024-09-11, 07:39
psSAR1g [W/Kg]	0.600	0.667
psSAR10g [W/Kg]	0.223	0.228
Power Drift [dB]	0.04	0.01
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		60.3
Dist 3dB Peak [mm]		8.1

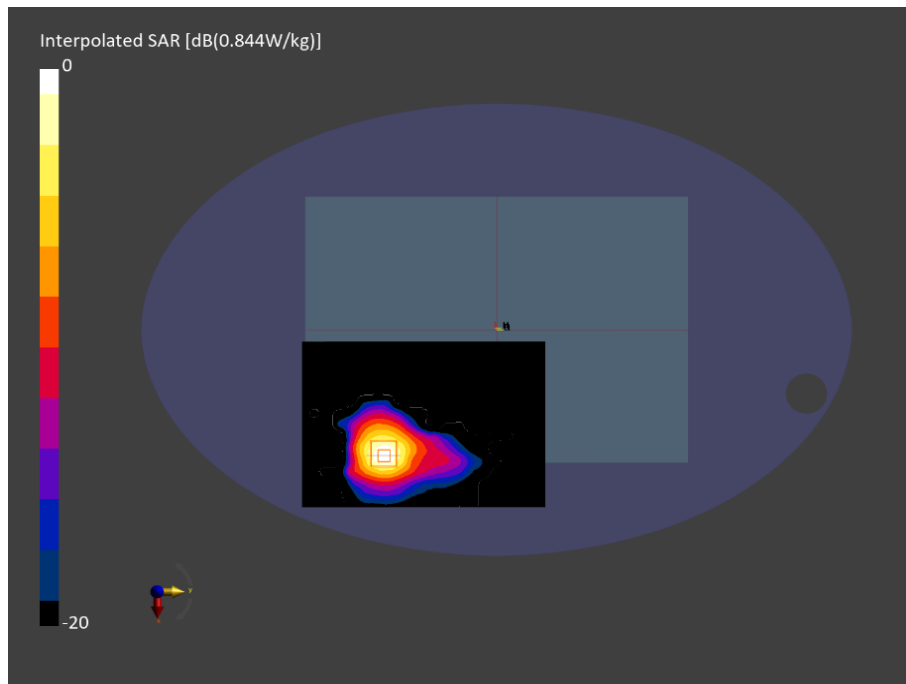


Figure C.05: SAR testing results for the A3185 at 5250 MHz core 1



Measurement Report for A3185, BACK, Custom Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 5850000 (5850.0 z)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 10032-CAA	5850.0, 5850000	4.63	5.18	34.1

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2202	HBBL-600-10000 DAK 3.5 Head ELI 21.36 deg.C 2024-Sep-11 SYS5 B5.prn, 2024-Sep-11	EX3DV4 - SN7805, 2024-02-14	DAE4ip Sn1785, 2024-02-13

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
MAIA	Y	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-11, 12:54	2024-09-11, 13:03
psSAR1g [W/Kg]	0.474	0.549
psSAR10g [W/Kg]	0.171	0.183
Power Drift [dB]	-0.15	0.13
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		54.3
Dist 3dB Peak [mm]		7.9

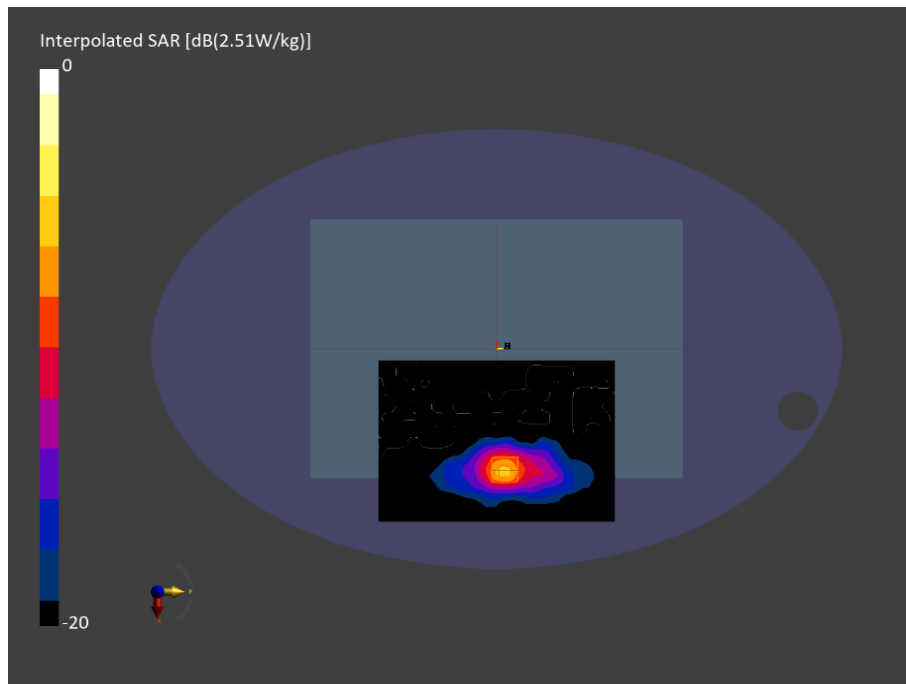


Figure C.06: SAR testing results for the A3185 at 5850 MHz core 0



Measurement Report for A3185, BACK, Custom Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 5725000 (5725.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 10032-CAA	5725.0, 5725000	4.63	5.03	34.4

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2202	HBBL-600-10000 DAK 3.5 Head ELI 21.36 deg.C 2024-Sep-11 SYS5 B5.prn, 2024-Sep-11	EX3DV4 - SN7805, 2024-02-14	DAE4ip Sn1785, 2024-02-13

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
MAIA	Y	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-11, 14:13	2024-09-11, 14:22
SAR1g [W/Kg]	0.616	0.679
psSAR10g [W/Kg]	0.227	0.249
Power Drift [dB]	0.12	0.05
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		57.6
Dist 3dB Peak [mm]		8.4

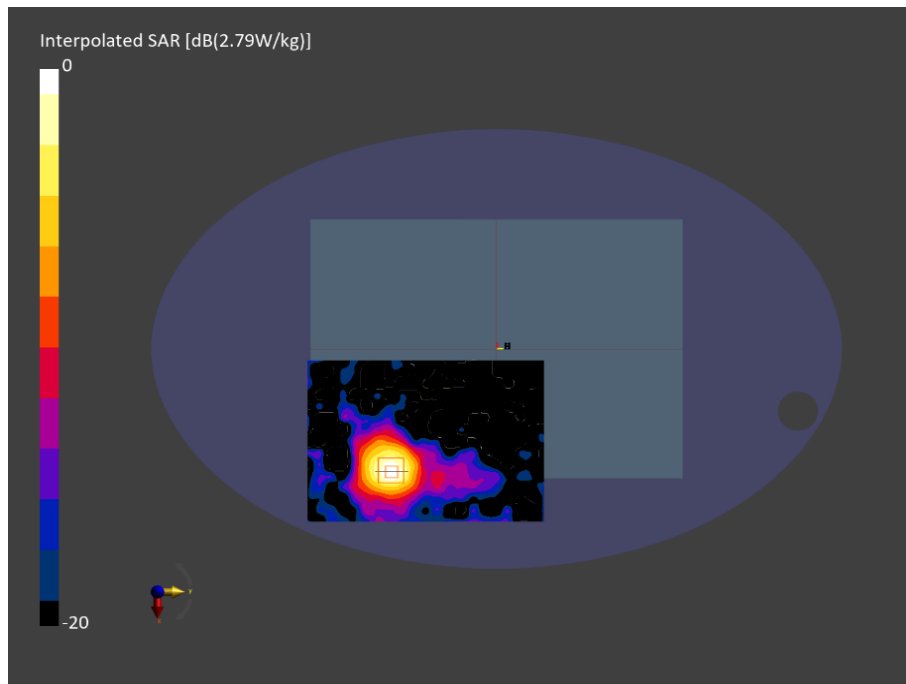


Figure C.07: SAR testing results for the A3185 at 5725 MHz core 1



Measurement Report for A3185, BACK, Custom Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 5250000 (5250.000 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 10032-CAA	5250.000, 5250000	5.18	4.55	35.2

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) – 2202	HBBL-600-10000 DAK 3.5 Head ELI 20.68 deg.C 2024-Sep-09 SYS5 B5 .prn, 2024-Sep-09	EX3DV4 – SN7805, 2024-02-14	DAE4ip Sn1785, 2024-02-13

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
aded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	Y	Y
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-10, 18:58	2024-09-10, 19:06
psSAR1g [W/Kg]	0.239	0.266
psSAR10g [W/Kg]	0.083	0.084
Power Drift [dB]	0.11	0.10
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		57.5
Dist 3dB Peak [mm]		7.4

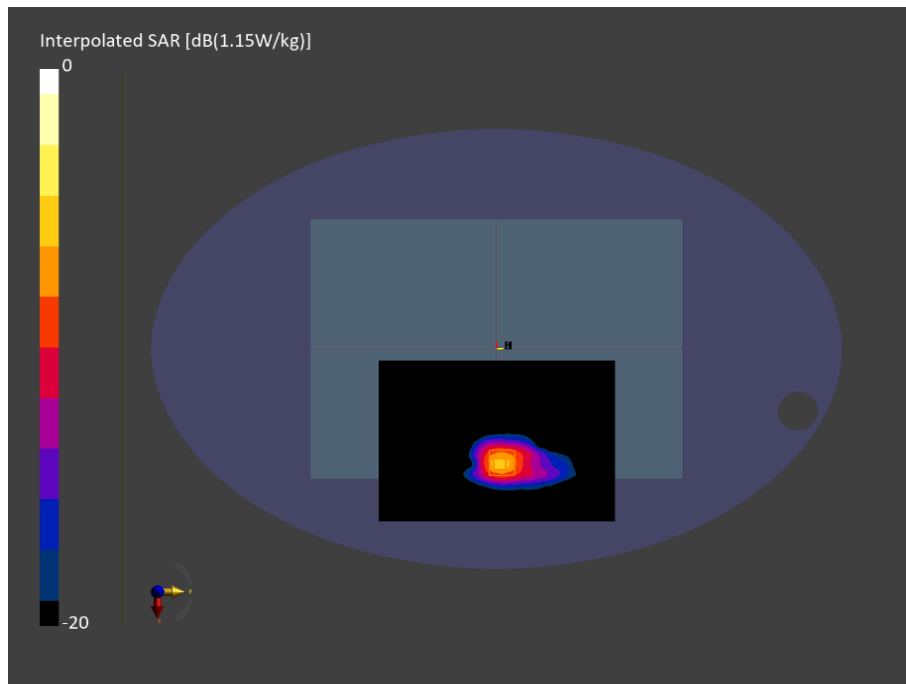


Figure C.08: SAR testing results for the A3185 at 5250 MHz core 0



Measurement Report for A3185, BACK, Custom Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 5250000 (5250.000 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 10032-CAA	5250.000, 5250000	5.18	4.55	35.2

rdware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2202	HBBL-600-10000 DAK 3.5 Head ELI 20.68 deg.C 2024-Sep-09 SYS5 B5 .prn, 2024-Sep-09	EX3DV4 - SN7805, 2024-02-14	DAE4ip Sn1785, 2024-02-13

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.4
MAIA	Y	Y
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-10, 20:49	2024-09-10, 21:01
psSAR1g [W/Kg]	0.328	0.354
psSAR10g [W/Kg]	0.116	0.125
Power Drift [dB]	0.18	-0.11
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		59.4
Dist 3dB Peak [mm]		8.0

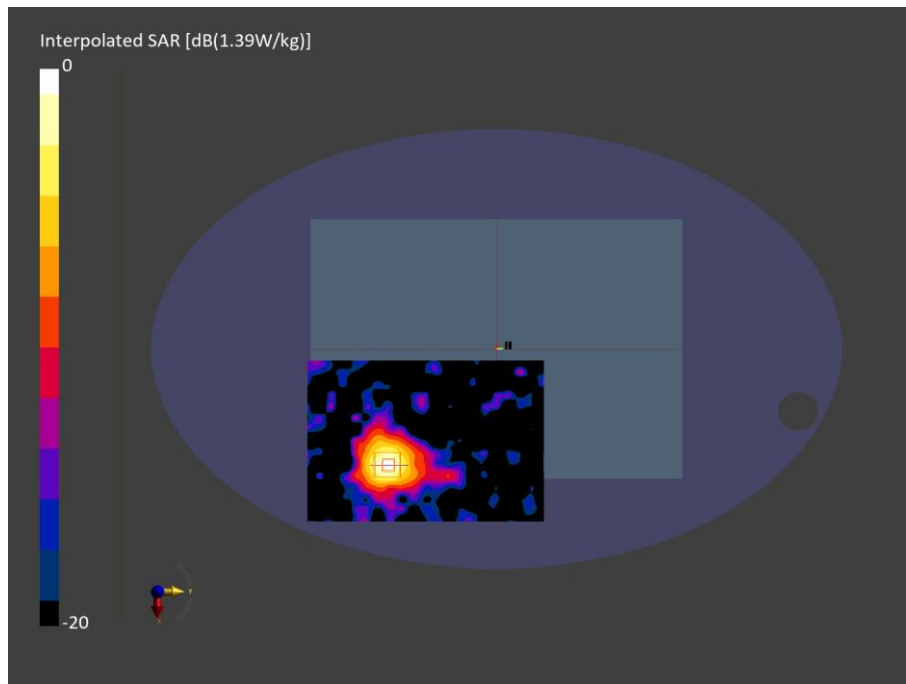


Figure C.09: SAR testing results for the A3185 at 5250 MHz core 1



Measurement Report for A3185, BACK, Custom Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 5725000 (5725.0MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 10032-CAA	5725.0, 5725000	4.63	5.09	34.4

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2202	HBBL-600-10000 DAK 3.5 Head ELI 20.68 deg.C 2024-Sep-09 SYS5 B5 .prn, 2024-Sep-09	EX3DV4 - SN7805, 2024-02-14	DAE4ip Sn1785, 2024-02-13

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
MAIA	Y	Y
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-10, 22:01	2024-09-10, 22:12
psSAR1g [W/Kg]	0.188	0.218
psSAR10g [W/Kg]	0.065	0.075
Power Drift [dB]	-0.67	-0.38
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		55.7
Dist 3dB Peak [mm]		7.2

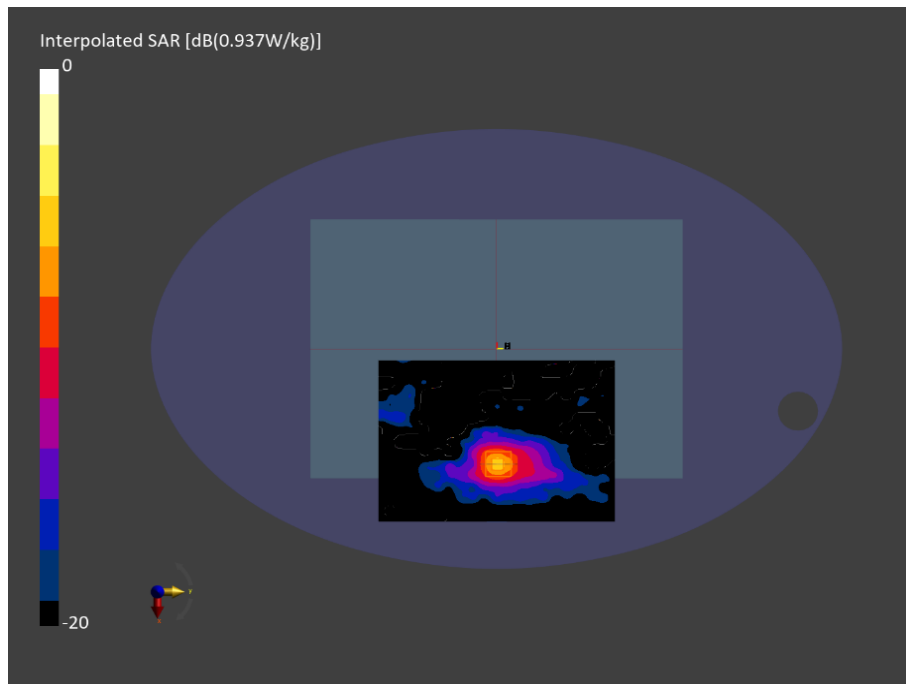


Figure C.10: SAR testing results for the A3185 at 5725 MHz core 0



Measurement Report for A3185, BACK, Custom Band, IEEE 802.15.1 Bluetooth (GFSK, DH5), Channel 5725000 (5725.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 10032-CAA	5725.0, 5725000	4.63	5.09	34.4

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2202	HBBL-600-10000 DAK 3.5 Head ELI 20.68 deg.C 2024-Sep-09 SYS5 B5 .prn, 2024-Sep-09	EX3DV4 - SN7805, 2024-02-14	DAE4ip Sn1785, 2024-02-13

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4
Graded Grid	n/a	Yes
Grading Ratio	n/a	1.4
MAIA	Y	Y
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-11, 02:03	2024-09-11, 02:11
SAR1g [W/Kg]	0.337	0.338
psSAR10g [W/Kg]	0.119	0.108
Power Drift [dB]	-0.03	0.35
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		56.6
Dist 3dB Peak [mm]		8.8

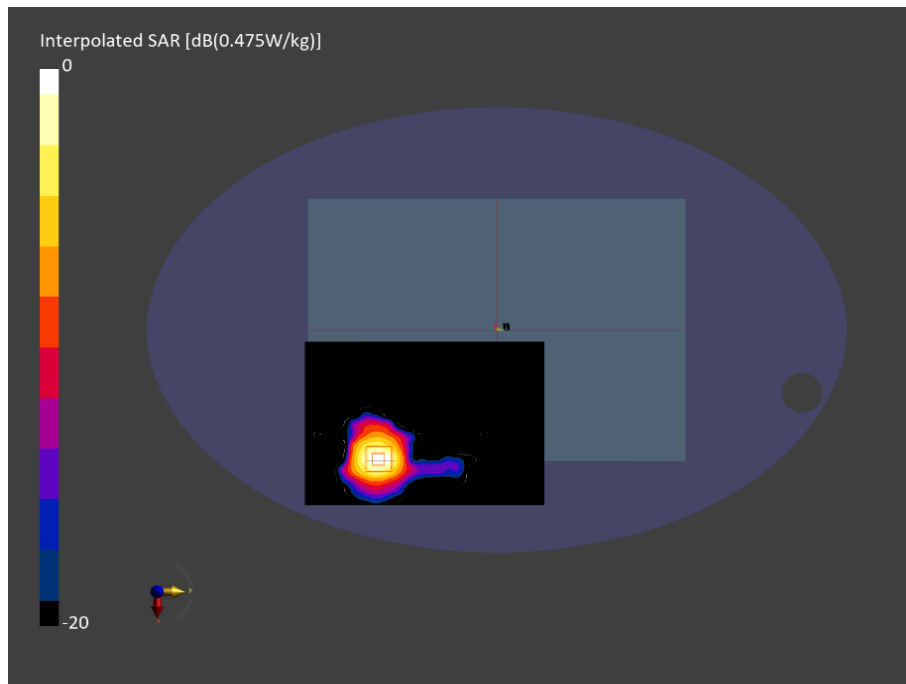


Figure C.11: SAR testing results for the A3185 at 5725 MHz core 1



Measurement Report for A3185, BACK, Custom Band, CW, Channel 2440000 (2440.0 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 0--	2440.0, 2440000	7.22	1.79	39.4

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) – 2102	HBBL-600-10000 DAK 3.5 Head ELI 20.66 deg.C 2024-Sep-09 SYS3 B3.prn, 2024-Sep-09	EX3DV4 – SN7804, 2024-08-14	DAE4ip Sn1786, 2024-08-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
aded Grid	n/a	Yes
Grading Ratio	n/a	1.5
MAIA	N/A	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-10, 14:17	2024-09-10, 14:28
psSAR1g [W/Kg]	0.934	0.964
psSAR10g [W/Kg]	0.461	0.447
Power Drift [dB]	0.03	0.01
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		75.3
Dist 3dB Peak [mm]		8.6

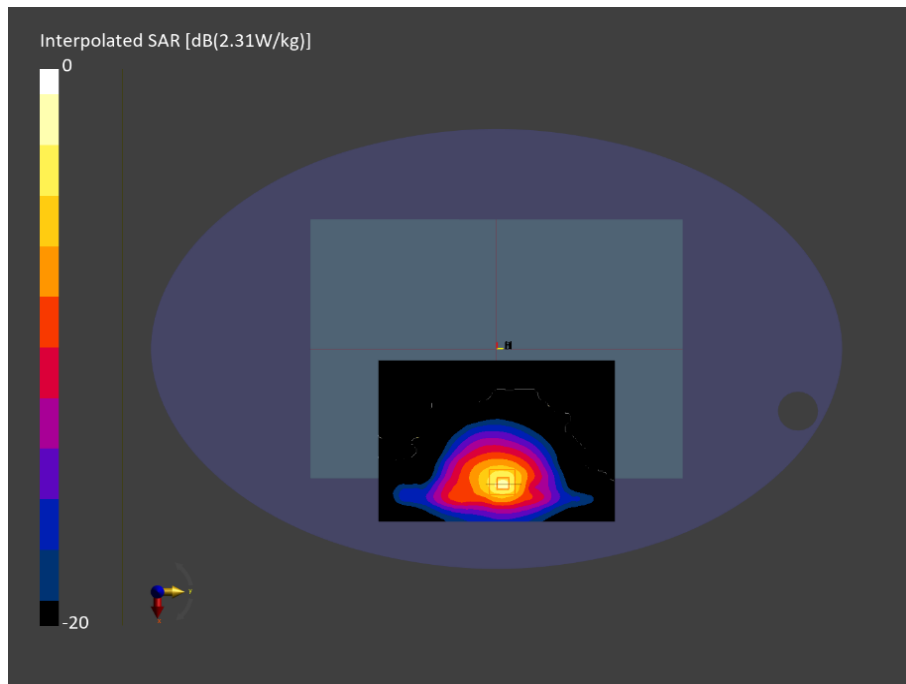


Figure C.12: SAR testing results for the A3185 at 2440 MHz core 0



Measurement Report for A3185, BACK, Custom Band, CW, Channel 2480000 (2480.000 MHz)

Device Under Test Properties

Model, Manufacturer	Dimensions [mm]	IMEI	DUT Type
A3185,	315.0 x 225.0 x 15.0		Laptop

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL	BACK, 0.00	Custom Band	CW, 0--	2480.000, 2480000	7.22	1.83	39.4

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V8.0 (20deg probe tilt) - 2102	HBBL-600-10000 DAK 3.5 Head ELI 20.66 deg.C 2024-Sep-09 SYS3 B3.prn, 2024-Sep-09	EX3DV4 - SN7804, 2024-08-14	DAE4ip Sn1786, 2024-08-07

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	140.0 x 200.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4
Graded Grid	N/A	Yes
Grading Ratio	N/A	1.5
MAIA	N/A	N/A
Surface Detection	VMS + 6p	VMS + 6p
Scan Method	Measured	Measured

Measurement Results

	Area Scan	Zoom Scan
Date	2024-09-10, 16:45	2024-09-10, 16:56
psSAR1g [W/Kg]	0.646	0.658
psSAR10g [W/Kg]	0.313	0.296
Power Drift [dB]	0.01	-0.00
Power Scaling	Disabled	Disabled
Scaling Factor [dB]		
TSL Correction	Positive only	Positive only
M2/M1 [%]		74.9
Dist 3dB Peak [mm]		8.5