



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid




<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1750</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Head 2600</p>
	

Photo 7: Tissue Simulant Liquid for Head 5G	NA
	<p>NA</p>

3. Photographs of EUT test position

<p>Photo 8: Front side 10mm</p>	<p>Photo 9: Back side 10mm</p>
	
<p>Photo 10: Left side 10mm</p>	<p>Photo 11: Right side 10mm</p>
	
<p>Photo 12: Top side 10mm</p>	<p>Photo 13: Bottom side 10mm</p>
	

4. EUT Constructional Details

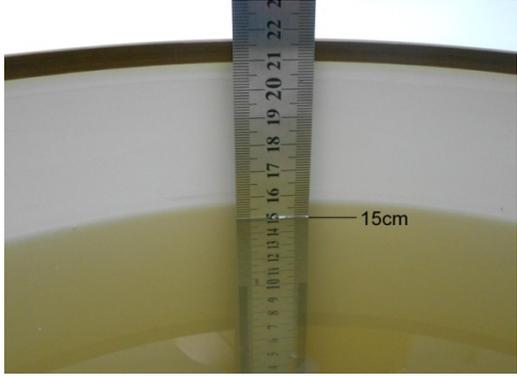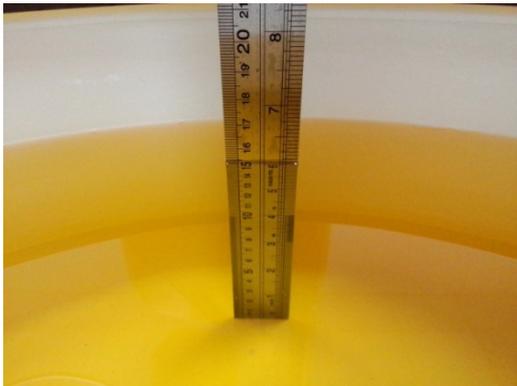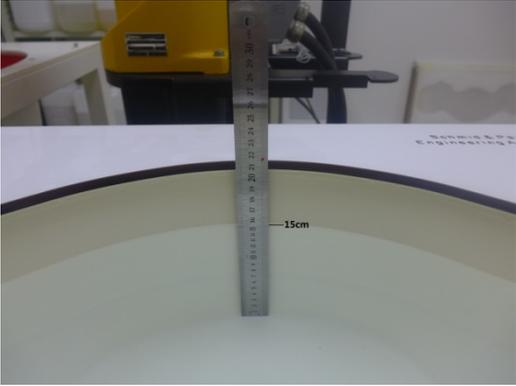