



DECLARATION OF COMPLIANCE SAR ASSESSMENT PCII Report Part 1 of 2

Motorola Solutions Inc.
EME Test Laboratory
 Motorola Solutions Malaysia Sdn Bhd
 Plot 2A, Medan Bayan Lepas,
 Mukim 12 SWD 11900 Bayan Lepas Penang, Malaysia.

Date of Report: 04/11/2020
Report Revision: A

Responsible Engineer: Ch'ng Jian Sheng
Report Author: Ch'ng Jian Sheng
Date/s Tested: 09/27/2019 - 09/28/2019, 10/21/2019 - 10/22/2019, 10/24/2019, 11/17/2019, 12/29/2019 - 12/31/2019, 01/13/2020, 01/16/202 - 01/17/2020, 03/29/2020 - 03/30/2020, 04/05/2020, 04/11/2020
Manufacturer: Motorola Solutions Inc.
DUT Description: Handheld Portable - 136-174MHz, 5W rated power, 6.25kHz/12.5kHz/25kHz, Capable of digital and analog FM transmission. Also capable of TDMA transmission.
Test TX mode(s): CW (PTT)
Max. Power output: 5.9W
Nominal Power: 5.0W
Tx Frequency Bands: 136-174MHz
Signaling type: FM, TDMA
Model(s) Tested: H84KDD9PW5AN (MUD3305) & H84KDH9PW7AN (MUD3277)
Model(s) Certified: H84KDD9PW5AN (MUD3305), H84KDH9PW7AN (MUD3277) & H84KDF9PW6AN (MUD3318)
Serial Number(s): 837CQT0048, 837CQT0045
Classification: Occupational/Controlled
Applicant Name: Motorola Solutions Inc.
Applicant Address: 8000 West Sunrise Boulevard, Fort Lauderdale, Florida 33322
FCC ID: AZ489FT3834; LMR 150.8-173.4MHz
 This report contains results that are immaterial for FCC equipment approval, which are clearly identified.
IC: 109U-89FT3834
 This report contains results that are immaterial for ISSED equipment approval, which are clearly identified.
Applicant Name: Motorola Solutions Inc.
Applicant Address: 8000 West Sunrise Boulevard, Fort Lauderdale, Florida 33322
ISSED Test Site registration: 24843
FCC Test Firm Registration Number: 823256

The test results clearly demonstrate compliance with FCC Occupational/Controlled RF Exposure limits of 8 W/kg averaged over 1 gram per the requirements of FCC 47 CFR § 2.1093 and RSS-102 (Issue 5).

Based on the information and the testing results provided herein, the undersigned certifies that when used as stated in the operating instructions supplied, said product complies with the national and international reference standards and guidelines listed in section 4.0 of this report (no deviation from standard methods). This report shall not be reproduced without written approval from an officially designated representative of the Motorola Solutions Inc EME Laboratory. I attest to the accuracy of the data and assume full responsibility for the completeness of these measurements. This reporting format is consistent with the suggested guidelines of the TIA TSB-150 December 2004. The results and statements contained in this report pertain only to the device(s) evaluated.

Tiong Nguk Ing
Deputy Technical Manager (Approved Signatory)
Approval Date: 4/15/2020

Part 1 of 2

1.0	Introduction.....	4
2.0	FCC SAR Summary.....	4
3.0	Abbreviations / Definitions.....	4
4.0	Referenced Standards and Guidelines	5
5.0	SAR Limits	6
6.0	Description of Device Under Test (DUT)	6
7.0	Optional Accessories and Test Criteria	6
7.1	Antenna.....	7
7.2	Batteries	7
7.3	Body worn Accessory.....	7
7.4	Audio Accessory.....	7
8.0	Description of Test System.....	8
8.1	Descriptions of Robotics/Probes/Readout Electronics	8
8.2	Description of Phantom(s).....	9
8.3	Description of Simulated Tissue.....	9
9.0	Additional Test Equipment.....	10
10.0	SAR Measurement System Validation and Verification	11
10.1	System Validation.....	11
10.2	System Verification	12
10.3	Equivalent Tissue Test Results.....	12
11.0	Environmental Test Conditions	14
12.0	DUT Test Setup and Methodology	14
12.1	Measurements	14
12.2	DUT Configuration(s)	15
12.3	DUT Positioning Procedures	15
12.3.1	Body.....	15
12.3.2	Head.....	15
12.3.3	Face.....	15
12.4	DUT Test Channels	16
12.5	SAR Result Scaling Methodology.....	16
12.6	DUT Test Plan	16
13.0	DUT Test Data.....	17
13.1	Assessment for FCC (150.8 - 173.4MHz)	17
13.2	Assessment for ISED, Canada (138 - 174MHz).....	18
13.3	Shortened Scan Assessment	19
	Results Summary	20
14.0	Variability Assessment	20
15.0	System Uncertainty.....	20

APPENDICES

A	Measurement Uncertainty Budget	21
B	Probe Calibration Certificates.....	24
C	Dipole Calibration Certificates	113

Part 2 of 2**APPENDICES**

D	System Verification Check Scans.....	2
E	DUT Scans.....	16
F	Shorten Scan of Highest SAR Configuration	21
G	DUT Test Position Photos	23
H	Battery Photos.....	25

Report Revision History

Date	Revision	Comments
04/11/2020	A	Release of PCII results

1.0 Introduction

This report details the utilization, test setup, test equipment, and test results of the Specific Absorption Rate (SAR) measurements performed at the Motorola Solutions Inc. EME Test Laboratory for handheld portable model number H84KDD9PW5AN (MUD3305) and H84KDH9PW7AN (MUD3277). These devices are classified as Occupational/Controlled. The information herein is to show evidence of Class II Permissive Change compliance based on the SAR evaluation of newly offered battery PMNN4424B, PMNN4448B, NNTN8128C and PMNN4491C.

2.0 FCC SAR Summary

Table 1

Equipment Class	Frequency band (MHz)	Max Calc at Body (W/kg)	Max Calc at Face (W/kg)
		1g-SAR	1g-SAR
TNF	150.8-173.4MHz (LMR)	1.12*	0.80*

Note:

* indicates that “Max Calc at Body” and “Max Calc at Face” reflects the new SAR compliance value at the body and head for this FCC ID (Previous filed SAR value for body and head are 1.02 & 0.60W/kg)

3.0 Abbreviations / Definitions

CNR: Calibration Not Required
 EME: Electromagnetic Energy
 DUT: Device Under Test
 NA: Not Applicable
 PTT: Push to Talk
 SAR: Specific Absorption Rate
 RSM: Remote Speaker Microphone
 4FSK: 4 Level Frequency Shift Keying
 TDMA: Time Division Multiple Access
 DSP: Digital Signal Processor
 TNF: Licensed Non-Broadcast Transmitter Held to Face

Audio accessories: These accessories allow communication while the DUT is worn on the body.

Body worn accessories: These accessories allow the DUT to be worn on the body of the user.

Maximum Power: Defined as the upper limit of the production line final test station.

4.0 Referenced Standards and Guidelines

This product is designed to comply with the following applicable national and international standards and guidelines.

- IEC62209-1 (2016) Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)
- Federal Communications Commission, “Evaluating Compliance with FCC Guidelines for Human Exposure to Radio frequency Electromagnetic Fields”, OET Bulletin 65, FCC, Washington, D.C.: 1997.
- IEEE 1528 (2013), Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
- American National Standards Institute (ANSI) / Institute of Electrical and Electronics Engineers (IEEE) C95. 1-1992
- Institute of Electrical and Electronics Engineers (IEEE) C95.1-2005
- International Commission on Non-Ionizing Radiation Protection (ICNIRP) 1998
- Ministry of Health (Canada) Safety Code 6 (2015), Limits of Human Exposure to Radio frequency Electromagnetic Fields in the Frequency Range from 3 kHz to 300 GHz
- RSS-102 (Issue 5) – Radio Frequency (RF) Exposure Compliance of Radio communication Apparatus (All Frequency Bands)
- Australian Communications Authority Radio communications (Electromagnetic Radiation - Human Exposure) Standard (2014)
- ANATEL, Brazil Regulatory Authority, Resolution No. 303 of July 2, 2002 "Regulation of the limitation of exposure to electrical, magnetic, and electromagnetic fields in the radio frequency range between 9 kHz and 300 GHz." and “Attachment to resolution # 303 from July 2, 2002”
- IEC62209-2 Edition 1.0 2010-03, Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices – Human models, instrumentation, and procedures – Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz).
- FCC KDB – 643646 D01 SAR Test for PTT Radios v01r03
- FCC KDB – 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r04
- FCC KDB – 865664 D02 RF Exposure Reporting v01r02
- FCC KDB – 447498 D01 General RF Exposure Guidance v06

5.0 SAR Limits

Table 2

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average - ANSI - (averaged over the whole body)	0.08	0.4
Spatial Peak - ANSI - (averaged over any 1-g of tissue)	1.6	8.0
Spatial Peak – ICNIRP/ANSI - (hands/wrists/feet/ankles averaged over 10-g)	4.0	20.0
Spatial Peak - ICNIRP - (Head and Trunk 10-g)	2.0	10.0

6.0 Description of Device Under Test (DUT)

These portable devices operate in the LMR band using either frequency modulation (FM) with 100% transmit duty cycle or TDMA signal with 50% transmit duty cycle. For conservative assessment, FM signal with higher average power was tested.

These devices operate in a half duplex system. A half duplex system only allows the user to transmit or receive. This device cannot transmit and receive simultaneously. The user must stop transmitting in order to receive a signal or listen for a response, regardless of PTT button or use of voice activated audio accessories. This type of operation, along with the RF safety booklet, which instructs the user to transmit no more than 50% of the time, justifies the use of 50% duty factor for this device.

The models represented under this filing utilize removable antennas capable of transmitting in the 136-174 MHz band. The nominal output powers are 5.0 W with maximum output powers of 5.9 W as defined by upper limit of the production line final test station.

The intended operating positions are “at the face” with the DUT at least 2.5cm inch from the mouth, and “at the body” by means of the offered body worn accessories. Body worn audio and PTT operation is accomplished by means of optional remote accessories that are connected to the radio.

7.0 Optional Accessories and Test Criteria

These devices are offered with optional accessories. The following sections identify the test criteria and details for each accessory category applicable for this PCII filing only. Detailed listings of all the approved offered accessories are available in the original filing report.

7.1 Antenna

Only one antenna applicable for this PCII filing. The Table below lists its descriptions.

Table 3

Antenna No.	Antenna Models	Description	Selected for test	Tested
1	NAR6593A	Antenna VHF/GPS, 136-174 MHz, ¼ wave, -7.0 dBi gain	Yes	Yes

7.2 Batteries

There are four new batteries applicable for this PCII filing. The Table below lists its descriptions.

Table 4

Battery No.	Battery Models	Description	Selected for test	Tested	Comments
1	PMNN4424B	Battery IMPRES Li-ION 2350mAh Typical	Yes	Yes	
2	PMNN4448B	Battery IMPRES Li-ION 2800mAh Typical	Yes	Yes	
3	PMNN4491C	Battery IMPRES Li-ION 2100mAh Typical	Yes	Yes	
4	NNTN8128C	Battery IMPRES Li-ION 2000mAh Typical	Yes	Yes	

7.3 Body worn Accessory

Only one body worn applicable for this PCII filing. The Table below lists the body worn accessory and its descriptions.

Table 5

Body worn No.	Body worn Models	Description	Selected for test	Tested	Comments
1	PMLN4651A	2" Belt Clip	Yes	Yes	

7.4 Audio Accessory

Only one audio accessory is applicable for this PCII filing. The Table below lists its descriptions.

Table 6

Audio No.	Audio Acc. Models	Description	Selected for test	Tested	Comments
1	PMLN6130A	Impress 2 Wire with Translucent Tube, Beige	Yes	Yes	

8.0 Description of Test System



8.1 Descriptions of Robotics/Probes/Readout Electronics

Table 7

Dosimetric System type	System version	DAE type	Probe Type
Schmid & Partner Engineering AG SPEAG DASY 5	52.10.2.1495	DAE4	EX3DV4 (E-Field)

The DASY5™ system is operated per the instructions in the DASY5™ Users Manual. The complete manual is available directly from SPEAG™. All measurement equipment used to assess SAR compliance was calibrated according to ISO/IEC 17025 A2LA guidelines. Section 9.0 presents additional test equipment information. Appendices B and C present the applicable calibration certificates. The E-field probe first scans a coarse grid over a large area inside the phantom in order to locate the interpolated maximum SAR distribution. After the coarse scan measurement, the probe is automatically moved to a position at the interpolated maximum. The subsequent scan can directly use this position as reference for the cube evaluations.

8.2 Description of Phantom(s)

Table 8

Phantom Type	Phantom(s) Used	Material Parameters	Phantom Dimensions LxWxD (mm)	Material Thickness (mm)	Support Structure Material	Loss Tangent (wood)
Triple Flat	NA	200MHz -6GHz; Er = 3-5, Loss Tangent = ≤ 0.05	280x175x175	2mm +/- 0.2mm	Wood	< 0.05
SAM	NA	300MHz -6GHz; Er = < 5, Loss Tangent = ≤ 0.05	Human Model			
Oval Flat	√	300MHz -6GHz; Er = 4+/- 1, Loss Tangent = ≤ 0.05	600x400x190			

8.3 Description of Simulated Tissue

The sugar based simulate tissue is produced by placing the correct measured amount of De-ionized water into a large container. Each of the dried ingredients are weighed and added to the water carefully to avoid clumping. If the solution has a high sugar concentration the water is pre-heated to aid in dissolving the ingredients.

The simulated tissue mixture was mixed based on the Simulated Tissue Composition indicated in Table 9. During the daily testing of this product, the applicable mixture was used to measure the Di-electric parameters at each of the tested frequencies to verify that the Di-electric parameters were within the tolerance of the tissue specifications.

Simulated Tissue Composition (percent by mass)

Table 9

Ingredients	150MHz	
	Head	Body
Sugar	55.4	49.7
De ionized Water	38.35	46.2
Salt	5.15	3.0
HEC	1.0	1.0
Bact.	0.1	0.1

9.0 Additional Test Equipment

The Table below lists additional test equipment used during the SAR assessment.

Table 10

Equipment Type	Model Number	Serial Number	Calibration Date	Calibration Due Date
SPEAG Probe	EX3DV4	7534	07/25/2019	07/25/2020
SPEAG Probe*	EX3DV4	7364	01/23/2019	01/23/2020
SPEAG Probe*	EX3DV4	7485	01/23/2019	01/23/2020
SPEAG Probe	EX3DV4	7533	11/06/2019	11/06/2020
SPEAG Probe	EX3DV4	7486	10/24/2019	10/24/2020
SPEAG Probe	EX3DV4	7511	10/24/2019	10/24/2020
SPEAG DAE	DAE4	374	07/17/2019	07/17/2020
SPEAG DAE*	DAE4	1483	01/10/2019	01/10/2020
SPEAG DAE*	DAE4	688	01/10/2019	01/10/2020
SPEAG DAE	DAE4	1488	07/23/2019	07/23/2020
SPEAG DAE	DAE4	850	10/16/2019	10/16/2020
SPEAG DAE	DAE4	729	10/16/2019	10/16/2020
Amplifier	10W1000C	312859	CNR	CNR
Amplifier	5S1G4	313326	CNR	CNR
Amplifier	50W 1000A	312859	CNR	CNR
Amplifier	50W 1000A	14715	CNR	CNR
Bi-Directional Coupler	3020A	40295	09/12/2019	09/12/2020
Bi-Directional Coupler	3020A	41931	07/11/2019	07/11/2020
Power Meter	E4418B	MY45100911	08/30/2019	08/30/2021
Power Meter	E4419B	MY45103725	06/10/2019	06/10/2021
Power Meter	E4416A	MY50001037	08/30/2019	08/30/2021
Power Meter	E4419B	MY40330364	09/21/2018	09/21/2020
Power Meter	E4418B	MY45107917	07/01/2019	07/01/2021
Power Meter	E4418B	MY45100739	12/09/2019	12/09/2020
Power Sensor	E9301B	MY55210003	04/26/2019	04/26/2020
Power Sensor*	E9301B	MY55210006	12/19/2018	12/19/2019
Power Sensor	E9301B	MY50290001	05/06/2019	05/06/2020
Power Sensor*	8481B	SG41090248	12/20/2018	12/20/2019
Power Sensor	E9301B	MY41495733	04/19/2019	04/19/2020
Power Sensor*	E4412A	US38488023	03/24/2019	03/24/2020
Power Sensor	8481B	MY41091243	12/17/2019	12/17/2020
Power Sensor	8481B	3318A10982	02/05/2020	02/05/2021
Vector Signal Generator	E4438C	MY42081753	09/05/2019	09/05/2021
Vector Signal Generator	E4438C	MY45091270	08/13/2018	08/13/2020
Vector Signal Generator	SMA100A	111386	07/19/2019	07/19/2021
Vector Signal Generator	E4438C	MY47272101	10/29/2019	10/29/2021
Temperature & Humidity Logger*	TM320	12253047	10/30/2018	10/30/2019
Temperature & Humidity Logger*	DSB	16326831	11/28/2018	11/28/2019
Temperature & Humidity Logger	DSB	16326820	11/20/2019	11/20/2020
Temperature & Humidity Logger	DSB	16326831	11/25/2019	11/25/2020

Table 10 (Continued)

Equipment Type	Model Number	Serial Number	Calibration Date	Calibration Due Date
Thermometer*	HH806AU	080307	12/05/2018	12/05/2019
Thermometer*	HH202A	35881	12/26/2018	12/26/2019
Thermometer	1523	3492108	05/03/2019	05/03/2020
Temperature Probe*	80PK-22	06032017	12/05/2018	12/05/2019
Temperature Probe*	80PK-22	05032017	12/26/2018	12/26/2019
Temperature Probe	PR-10-3-100-1/4-6-E	WNWR020579	07/06/2019	07/06/2020
Dielectric Assessment Kit*	DAK-12	1069	01/08/2019	01/08/2020
Dielectric Assessment Kit	DAK-12	1051	07/11/2019	07/11/2020
Network Analyzer*	E5071B	MY42403147	12/19/2018	12/19/2019
Network Analyzer	E5071B	MY42403218	09/13/2019	09/13/2020
SPEAG Dipole*	CLA150	4005	02/09/2018	02/09/2020
SPEAG Dipole	CLA150	4016	10/10/2018	10/10/2020

Note: * indicates that the equipment is used for SAR assessment before calibration due date

10.0 SAR Measurement System Validation and Verification

DASY output files of the probe/dipole calibration certificates and system verification test results are included in appendices B, C & D respectively.

10.1 System Validation

The SAR measurement system was validated according to procedures in KDB 865664. The validation status summary Table is below.

Table 11

Dates	Probe Calibration Point		Probe SN	Measured Tissue Parameters		Validation		
				σ	ϵ_r	Sensitivity	Linearity	Isotropy
CW								
09/24/2019	Body	150	7534	0.83	59.3	Pass	Pass	Pass
09/11/2019	Head	150		0.73	50.9	Pass	Pass	Pass
*03/09/2019	Body	150	7364	0.79	59.1	Pass	Pass	Pass
*03/14/2019	Head	150		0.73	50.5	Pass	Pass	Pass
*03/08/2019	Body	150	7485	0.81	59.2	Pass	Pass	Pass
*03/07/2019	Head	150		0.75	51.2	Pass	Pass	Pass
11/22/2019	Body	150	7533	0.82	59.7	Pass	Pass	Pass
11/20/2019	Head	150		0.74	51.7	Pass	Pass	Pass
11/04/2019	Body	150	7486	0.77	59.7	Pass	Pass	Pass
11/05/2019	Head	150		0.77	51.3	Pass	Pass	Pass
11/26/2019	Body	150	7511	0.79	59.6	Pass	Pass	Pass
11/26/2019	Head	150		0.73	49.8	Pass	Pass	Pass

Note: * indicates that the probe verification check covers until the due date and replace with new probe

10.2 System Verification

System verification checks were conducted each day during the SAR assessment. The results are normalized to 1W. Appendix D includes DASY plots for each day during the SAR assessment. The Table below summarizes the daily system check results used for the SAR assessment.

Table 12

Probe Serial #	Tissue Type	Dipole Kit / Serial #	Ref SAR @ 1W (W/kg)	System Check Results Measured (W/kg)	System Check Test Results when normalized to 1W (W/kg)	Tested Date
7534	FCC Body	SPEAG CLA150 /4005	3.84 +/- 10%	3.92	3.92	10/24/2019
	IEEE/IEC Head		3.77 +/- 10%	3.86	3.86	10/21/2019
				3.77	3.77	10/22/2019
7364	IEEE/IEC Head		3.77 +/- 10%	3.85	3.85	11/17/2019
7485	FCC Body		3.84 +/- 10%	4.12	4.12	09/27/2019#
	IEEE/IEC Head		3.77 +/- 10%	3.94	3.94	09/27/2019#
7533	FCC Body		3.84 +/- 10%	4.13	4.13	12/30/2019#
	IEEE/IEC Head		3.77 +/- 10%	4.12	4.12	12/29/2019#
7486	FCC Body		3.84 +/- 10%	4.06	4.06	01/13/2020
	IEEE/IEC Head		3.77 +/- 10%	4.01	4.01	01/16/2020#
7511	FCC Body	SPEAG CLA150 /4016	3.95 +/- 10%	4.25	4.25	04/11/2020
	IEEE/IEC Head		3.64 +/- 10%	3.76	3.76	03/30/2020#
7533	FCC Body		3.95 +/- 10%	4.31	4.31	04/05/2020

Note: # indicates that the system verification check covers next testing day (within 24 hours)

10.3 Equivalent Tissue Test Results

Simulated tissue prepared for SAR measurements is measured daily and within 24 hours prior to actual SAR testing to verify that the tissue is within +/- 5% of target parameters at the center of the transmit band. This measurement is done using the applicable equipment indicated in section 9.0. The Table below summarizes the measured tissue parameters used for the SAR assessment.

Table 13

Frequency (MHz)	Tissue Type	Conductivity Target (S/m)	Dielectric Constant Target	Conductivity Meas. (S/m)	Dielectric Constant Meas.	Tested Date
138	FCC Body	0.79 (0.75-0.83)	62.2 (59.1-65.3)	0.78	60.0	04/11/2020
	IEEE/ IEC Head	0.75 (0.71-0.79)	52.9 (50.2-55.5)	0.72	54.7	03/11/2020#
144	FCC Body	0.8 (0.76-0.84)	62.1 (58.9-65.2)	0.82	59.5	10/24/2019
				0.78	59.4	09/27/2019#
				0.78	59.0	12/30/2019#
				0.78	59.1	04/05/2020
	IEEE/ IEC Head	0.76 (0.72-0.79)	52.6 (49.9-55.2)	0.79	53.0	10/22/2019
				0.79	53.0	09/26/2019#
				0.77	52.0	12/29/2019
				0.74	50.1	01/16/2020#
150	FCC Body	0.80 (0.76-0.84)	61.9 (58.8-65.0)	0.83	59.3	10/24/2019
				0.78	59.2	09/27/2019#
				0.78	58.9	12/30/2019#
				0.81	58.9	01/13/2020
				0.78	59.0	04/05/2020
				0.79	59.6	04/11/2020
	IEEE/ IEC Head	0.76 (0.72-0.80)	52.3 (49.7-54.9)	0.75	51.7	10/21/2019
				0.80	52.8	10/22/2019
				0.79	52.7	09/26/2019#
				0.73	50.0	11/17/2019
				0.77	51.8	12/29/2019#
				0.74	49.8	01/16/2020#
151	FCC Body	0.8 (0.76-0.84)	61.9 (58.8-65)	0.72	54.1	03/29/2020#
				0.83	59.3	10/24/2019
				0.78	59.2	09/27/2019#
				0.78	58.8	12/30/2019#
				0.81	58.9	01/13/2020
				0.79	59.6	04/11/2020
	IEEE/ IEC Head	0.76 (0.72-0.80)	52.3 (49.6-54.9)	0.75	51.7	10/21/2019
				0.74	49.9	11/17/2019
				0.74	49.8	01/16/2020#
173	FCC Body	0.82 (0.78-0.86)	61.3 (58.3-64.4)	0.80	59.0	04/11/2020
	IEEE/ IEC Head	0.78 (0.74-0.82)	51.2 (48.7-53.8)	0.74	53.0	03/29/2020#

Note: # indicates that tissue date is covered for next test day (within 24 hours)

11.0 Environmental Test Conditions

The EME Laboratory's ambient environment is well controlled resulting in very stable simulated tissue temperature and therefore stable dielectric properties. Simulated tissue temperature is measured prior to each scan to insure it is within $\pm 2^{\circ}\text{C}$ of the temperature at which the dielectric properties were determined. The liquid depth within the phantom used for measurements was at least 15cm. Additional precautions are routinely taken to ensure the stability of the simulated tissue such as covering the phantoms when scans are not actively in process in order to minimize evaporation. The lab environment is continuously monitored. The Table below presents the range and average environmental conditions during the SAR tests reported herein:

Table 14

	Target	Measured
Ambient Temperature	18 – 25 °C	Range: 18.0 – 25.0°C Avg. 22.8 °C
Tissue Temperature	18 – 25 °C	Range: 19.2 – 22.5°C Avg. 21.2°C

Relative humidity target range is a recommended target

The EME Lab RF environment uses a Spectrum Analyzer to monitor for extraneous large signal RF disturbances that could possibly affect the test results. If such unwanted signals are discovered the SAR scans are repeated.

12.0 DUT Test Setup and Methodology

12.1 Measurements

SAR measurements were performed using the DASY system described in section 8.0 using zoom scans. Oval flat phantoms filled with applicable simulated tissue were used for body and face testing.

The Table below includes the step sizes and resolution of area and zoom scans per KDB 865664 requirements.

Table 15

Description		≤ 3 GHz	> 3 GHz
Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface		5 ± 1 mm	$\frac{1}{2} \cdot \delta \cdot \ln(2) \pm 0.5$ mm
Maximum probe angle from probe axis to phantom surface normal at the measurement location		$30^\circ \pm 1^\circ$	$20^\circ \pm 1^\circ$
Maximum area scan spatial resolution: Δx_{Area} , Δy_{Area}		≤ 2 GHz: ≤ 15 mm 2 – 3 GHz: ≤ 12 mm	3 – 4 GHz: ≤ 12 mm 4 – 6 GHz: ≤ 10 mm
		When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be $\leq$ the corresponding x or y dimension of the test device with at least one measurement point on the test device.	
Maximum zoom scan spatial resolution: Δx_{Zoom} , Δy_{Zoom}		≤ 2 GHz: ≤ 8 mm 2 – 3 GHz: ≤ 5 mm*	3 – 4 GHz: ≤ 5 mm* 4 – 6 GHz: ≤ 4 mm*
Maximum zoom scan spatial resolution, normal to phantom surface	uniform grid: $\Delta z_{Zoom}(n)$	≤ 5 mm	3 – 4 GHz: ≤ 4 mm 4 – 5 GHz: ≤ 3 mm 5 – 6 GHz: ≤ 2 mm
Note: δ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details. * When zoom scan is required and the reported SAR from the area scan based 1-g SAR estimation procedures of KDB 447498 is ≤ 1.4 W/kg, ≤ 8 mm, ≤ 7 mm and ≤ 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.			

12.2 DUT Configuration(s)

The DUT is a portable device operational at the body and face as described in section 6.0 while using the applicable accessories listed in section 7.0.

12.3 DUT Positioning Procedures

The positioning of the device for each body location is described below and illustrated in Appendix G.

12.3.1 Body

The DUT was positioned in normal use configuration against the phantom with the offered body worn accessory as well as with the offered audio accessories as applicable.

12.3.2 Head

Not applicable.

12.3.3 Face

The DUT was positioned with its' front side separated 2.5cm from the phantom.

12.4 DUT Test Channels

The number of test channels was determined by using the following IEEE 1528 equation. The use of this equation produces the same or more test channels compared to the FCC KDB 447498 number of test channels formula.

$$N_c = 2 * \text{roundup}[10 * (f_{\text{high}} - f_{\text{low}}) / f_c] + 1$$

Where

N_c = Number of channels

F_{high} = Upper channel

F_{low} = Lower channel

F_c = Center channel

12.5 SAR Result Scaling Methodology

The calculated 1-gram and 10-gram averaged SAR results indicated as “Max Calc. 1g-SAR” in the data Tables is determined by scaling the measured SAR to account for power leveling variations and drift. Appendix F includes a shortened scan to justify SAR scaling for drift. For this device the “Max Calc. 1g-SAR” are scaled using the following formula:

$$\text{Max_Calc} = \text{SAR_meas} \cdot 10^{\frac{-\text{Drift}}{10}} \cdot \frac{P_{\text{max}}}{P_{\text{int}}} \cdot \text{DC}$$

P_{max} = Maximum Power (W)

P_{int} = Initial Power (W)

Drift = DASY drift results (dB)

SAR_meas = Measured 1-g or 10-g Avg. SAR (W/kg)

DC = Transmission mode duty cycle in % where applicable

50% duty cycle is applied for PTT operation

Note: for conservative results, the following are applied:

If $P_{\text{int}} > P_{\text{max}}$, then $P_{\text{max}}/P_{\text{int}} = 1$.

Drift = 1 for positive drift

Additional SAR scaling was applied using the methodologies outlined in FCC KDB 865664 using tissue sensitivity values. SAR was scaled for conditions where the tissue permittivity was measured above the nominal target and for tissue conductivity that was measured below the nominal target. Negative or reduced SAR scaling is not permitted.

12.6 DUT Test Plan

The DUT was assessed at the body and face using the highest applicable configuration found during initial compliance assessment on filed with the FCC and ISED. All modes of operation identified in section 6.0 were considered during the development of the test plan. All tests were performed in CW 50% duty cycle was applied to PTT configurations in the final results.

13.0 DUT Test Data

13.1 Assessment for FCC

The new batteries PMNN4424B, PMNN4448B, PMNN4491C & NNTN8128C were assessed using the accessories indicated in section 7.0 which represent the highest applicable configurations at the body and face found during the initial compliance assessment on file with the FCC. SAR plots of the highest body and face results (bolded) are presented in Appendix E.

Table 16

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Body									
NAR6593A	PMNN4424B	PMLN4651A	PMLN6130A	150.8000	5.41	-0.57	1.36	0.85	FAZ-AB-191024-07
	PMNN4448B				5.90	-0.45	1.30	0.72	BL-AB-190928-03#
	PMNN4491C				5.78	-0.75	1.75	1.06	IZ-AB-191231-05#
	NNTN8128C				5.82	-0.63	1.91	1.12	FAZ-AB-200113-07
Face									
NAR6593A	PMNN4424B	Front @ 2.5cm	None	150.8000	5.40	-0.46	1.31	0.80	ZZ(NZ)-FACE-191021-07
	PMNN4448B				5.86	-0.60	1.24	0.72	ZZ-FACE-191117-13
	PMNN4491C				5.80	-0.44	1.38	0.78	IZ-FACE-191230-01#
	NNTN8128C				5.83	-0.46	1.42	0.80	ZZ(MA)-FACE-200117-03#

13.2 Assessment for ISED, Canada

The new batteries PMNN4424B, PMNN4448B, PMNN4491C & NNTN8128C were assessed using the accessories indicated in section 7.0 which represent the highest applicable configurations at the body and face found during the initial compliance assessment on file with ISED. SAR plots of the highest body and face results (bolded) are presented in Appendix E.

Table 17

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Body									
NAR6593A	PMNN4424B	PMLN4651A	PMLN6130A	144.4000	5.43	-0.39	3.23	1.92	FAZ-AB-191024-08
	PMNN4448B				5.87	-0.58	2.69	1.55	BL-AB-190928-04#
	PMNN4491C				5.88	-0.85	2.66	1.62	IZ-AB-191231-06#
	NNTN8128C				5.70	-0.57	3.03	1.79	AM-AB-200405-12
Face									
NAR6593A	PMNN4424B	Front @ 2.5cm	None	144.4000	5.72	-0.07	2.60	1.36	BL-FACE-191022-13
	PMNN4448B				5.90	0.31	2.60	1.30	AM-FACE-190927-06#
	PMNN4491C				5.55	0.03	2.64	1.40	AM-FACE-191229-06
	NNTN8128C				5.90	0.03	2.56	1.28	ZZ(MA)-FACE-200117-04#

As per ISED Notice 2016-DRS001, additional tests were required for the low, mid and high frequency channels for the configuration with the highest SAR value as shown below.

Table 18

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
Body									
NAR6593A	PMNN4424B	PMLN4651A	PMLN6130A	138.0000	5.44	0.18	2.07	1.12	ZZ(MA)-AB-200411-18
				144.4000	5.43	-0.39	3.23	1.92	FAZ-AB-191024-08
				173.4000	5.39	-0.78	1.40	0.92	ZZ(MA)-AB-200411-19
Face									
NAR6593A	PMNN4491C	Front @ 2.5cm	None	138.0000	5.82	0.30	0.86	0.44	AM-FACE-200330-09#
				144.4000	5.55	0.03	2.64	1.40	AM-FACE-191229-06
				173.4000	5.86	-0.57	1.33	0.76	AM-FACE-200330-11#

13.3 Shortened Scan Assessment

A “shortened” scan using the highest FCC SAR configuration from above was performed to validate the SAR drift of the full DASY5™ coarse and zoom scans. Note that the shortened scan represents the zoom scan performance result; this is obtained by first running a coarse scan to find the peak area and then, using a newly charged battery, a zoom scan only was performed. The results of the shortened cube scan presented in Appendix F demonstrate that the scaling methodology used to determine the calculated SAR results presented herein are valid. The SAR result from the Table below is provided in Appendix F.

Table 19

Antenna	Battery	Carry Accessory	Cable Accessory	Test Freq (MHz)	Init Pwr (W)	SAR Drift (dB)	Meas. 1g-SAR (W/kg)	Max Calc. 1g-SAR (W/kg)	Run#
NAR6593A	NNTN8128C	PMLN4651A	PMLN6130A	150.8000	5.65	-0.26	2.02	1.12	ZZ(MA)-AB-200411-17

Results Summary

The highest Operational Maximum Calculated 1-gram average SAR value found for this filing. The test results clearly demonstrate compliance with FCC Occupational/Controlled RF Exposure limits of 8 W/kg averaged over 1 gram per the requirements of FCC 47 CFR § 2.1093.

Table 20

Designator	Frequency band (MHz)	Max Calc at Body (W/kg)	Max Calc at Face (W/kg)
		1g-SAR	1g-SAR
FCC US			
LMR	150.8-173.4	1.12*	0.80*
ISED Canada			
LMR	138-174	1.92**	1.40**
Overall			
LMR	136-174	1.92	1.40

All results are scaled to the maximum output power.

Note:

* indicates that “Max Calc at Body” & “Max Calc at Face” reflects the new SAR compliance value at the Face and body for FCC US (Previous filed SAR value for body and Face is 1.02 W/kg & 0.60 W/kg respectively)

** indicates that “Max Calc at Body” & “Max Calc at Face” reflects the new SAR compliance value at the Face and body for ISED Canada (Previous filed SAR value for body and Face is 1.42 W/kg & 1.09 W/kg respectively)

14.0 Variability Assessment

Per the guidelines in KDB 865664 SAR variability assessment is not required because SAR results are below 4.0W/kg (Occupational).

15.0 System Uncertainty

A system uncertainty analysis is not required for this report per KDB 865664 because the highest report SAR value Occupational exposure is less than 7.5W/kg.

Per the guidelines of ISO 17025 a reported system uncertainty is required and therefore measurement uncertainty budget is included in Appendix A.

Appendix A

Measurement Uncertainty Budget

Uncertainty Budget for Device Under Test, for 150 MHz

<i>a</i>	<i>b</i>	<i>c</i>	<i>d</i>	$e = f(d,k)$	<i>f</i>	<i>g</i>	$h = c \times f / e$	$i = c \times g / e$	<i>k</i>
Uncertainty Component	IEEE 1528 section	Tol. ($\pm$ %)	Prob Dist	Div.	c_i (1 g)	c_i (10 g)	1 g u_i ($\pm$ %)	10 g u_i ($\pm$ %)	v_i
Measurement System									
Probe Calibration	E.2.1	6.7	N	1.00	1	1	6.7	6.7	∞
Axial Isotropy	E.2.2	4.7	R	1.73	0.707	0.707	1.9	1.9	∞
Hemispherical Isotropy	E.2.2	9.6	R	1.73	0.707	0.707	3.9	3.9	∞
Boundary Effect	E.2.3	1.0	R	1.73	1	1	0.6	0.6	∞
Linearity	E.2.4	4.7	R	1.73	1	1	2.7	2.7	∞
System Detection Limits	E.2.5	1.0	R	1.73	1	1	0.6	0.6	∞
Readout Electronics	E.2.6	0.3	N	1.00	1	1	0.3	0.3	∞
Response Time	E.2.7	1.1	R	1.73	1	1	0.6	0.6	∞
Integration Time	E.2.8	1.1	R	1.73	1	1	0.6	0.6	∞
RF Ambient Conditions - Noise	E.6.1	3.0	R	1.73	1	1	1.7	1.7	∞
RF Ambient Conditions - Reflections	E.6.1	0.0	R	1.73	1	1	0.0	0.0	∞
Probe Positioner Mech. Tolerance	E.6.2	0.4	R	1.73	1	1	0.2	0.2	∞
Probe Positioning w.r.t Phantom	E.6.3	1.4	R	1.73	1	1	0.8	0.8	∞
Max. SAR Evaluation (ext., int., avg.)	E.5	3.4	R	1.73	1	1	2.0	2.0	∞
Test sample Related									
Test Sample Positioning	E.4.2	3.2	N	1.00	1	1	3.2	3.2	29
Device Holder Uncertainty	E.4.1	4.0	N	1.00	1	1	4.0	4.0	8
SAR drift	6.6.2	5.0	R	1.73	1	1	2.9	2.9	∞
Phantom and Tissue Parameters									
Phantom Uncertainty	E.3.1	4.0	R	1.73	1	1	2.3	2.3	∞
Liquid Conductivity (target)	E.3.2	5.0	R	1.73	0.64	0.43	1.8	1.2	∞
Liquid Conductivity (measurement)	E.3.3	3.3	N	1.00	0.64	0.43	2.1	1.4	∞
Liquid Permittivity (target)	E.3.2	5.0	R	1.73	0.6	0.49	1.7	1.4	∞
Liquid Permittivity (measurement)	E.3.3	1.9	N	1.00	0.6	0.49	1.1	0.9	∞
Combined Standard Uncertainty			RSS				12	11	482
Expanded Uncertainty (95% CONFIDENCE LEVEL)			$k=2$				23	23	

Notes for uncertainty budget Tables:

- Column headings a-k are given for reference.
- Tol. - tolerance in influence quantity.
- Prob. Dist. – Probability distribution
- N, R - normal, rectangular probability distributions
- Div. - divisor used to translate tolerance into normally distributed standard uncertainty
- c_i - sensitivity coefficient that should be applied to convert the variability of the uncertainty component into a variability of SAR.
- u_i – SAR uncertainty
- v_i - degrees of freedom for standard uncertainty and effective degrees of freedom for the expanded uncertainty

Uncertainty Budget for System Validation(Dipole & flat phantom) for 150 MHz

<i>a</i>	<i>b</i>	<i>c</i>	<i>d</i>	<i>e = f(d,k)</i>	<i>f</i>	<i>g</i>	<i>h = c x f / e</i>	<i>i = c x g / e</i>	<i>k</i>
Uncertainty Component	IEEE 1528 section	Tol. (± %)	Prob. Dist.	Div.	<i>c_i</i> (1 g)	<i>c_i</i> (10 g)	1 g <i>u_i</i> (±%)	10 g <i>u_i</i> (±%)	<i>v_i</i>
Measurement System									
Probe Calibration	E.2.1	6.7	N	1.00	1	1	6.7	6.7	∞
Axial Isotropy	E.2.2	4.7	R	1.73	1	1	2.7	2.7	∞
Spherical Isotropy	E.2.2	9.6	R	1.73	0	0	0.0	0.0	∞
Boundary Effect	E.2.3	1.0	R	1.73	1	1	0.6	0.6	∞
Linearity	E.2.4	4.7	R	1.73	1	1	2.7	2.7	∞
System Detection Limits	E.2.5	1.0	R	1.73	1	1	0.6	0.6	∞
Readout Electronics	E.2.6	0.3	N	1.00	1	1	0.3	0.3	∞
Response Time	E.2.7	1.1	R	1.73	1	1	0.6	0.6	∞
Integration Time	E.2.8	0.0	R	1.73	1	1	0.0	0.0	∞
RF Ambient Conditions - Noise	E.6.1	3.0	R	1.73	1	1	1.7	1.7	∞
RF Ambient Conditions - Reflections	E.6.1	0.0	R	1.73	1	1	0.0	0.0	∞
Probe Positioner Mechanical Tolerance	E.6.2	0.4	R	1.73	1	1	0.2	0.2	∞
Probe Positioning w.r.t. Phantom	E.6.3	1.4	R	1.73	1	1	0.8	0.8	∞
Max. SAR Evaluation (ext., int., avg.)	E.5	3.4	R	1.73	1	1	2.0	2.0	∞
Dipole									
Dipole Axis to Liquid Distance	8, E.4.2	2.0	R	1.73	1	1	1.2	1.2	∞
Input Power and SAR Drift Measurement	8, 6.6.2	5.0	R	1.73	1	1	2.9	2.9	∞
Phantom and Tissue Parameters									
Phantom Uncertainty	E.3.1	4.0	R	1.73	1	1	2.3	2.3	∞
Liquid Conductivity (target)	E.3.2	5.0	R	1.73	0.64	0.43	1.8	1.2	∞
Liquid Conductivity (measurement)	E.3.3	3.3	R	1.73	0.64	0.43	1.2	0.8	∞
Liquid Permittivity (target)	E.3.2	5.0	R	1.73	0.6	0.49	1.7	1.4	∞
Liquid Permittivity (measurement)	E.3.3	1.9	R	1.73	0.6	0.49	0.6	0.5	∞
Combined Standard Uncertainty			RSS				10	9	99999
Expanded Uncertainty (95% CONFIDENCE LEVEL)			<i>k</i> =2				19	18	

Notes for uncertainty budget Tables:

- Column headings a-k are given for reference.
- Tol. - tolerance in influence quantity.
- Prob. Dist. – Probability distribution
- N, R - normal, rectangular probability distributions
- Div. - divisor used to translate tolerance into normally distributed standard uncertainty
- c_i* - sensitivity coefficient that should be applied to convert the variability of the uncertainty component into a variability of SAR.
- u_i* – SAR uncertainty
- v_i* - degrees of freedom for standard uncertainty and effective degrees of freedom for the expanded uncertainty

Appendix B

Probe Calibration Certificates

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **EX3-7534_Jul19**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:7534**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v5, QA CAL-23.v5,
QA CAL-25.v7
Calibration procedure for dosimetric E-field probes**

Calibration date: **July 25, 2019**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-19 (No. 217-02894)	Apr-20
DAE4	SN: 660	19-Dec-18 (No. DAE4-660_Dec18)	Dec-19
Reference Probe ES3DV2	SN: 3013	31-Dec-18 (No. ES3-3013_Dec18)	Dec-19
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	09-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41406067	09-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

	Name	Function	Signature
Calibrated by:	Manu Seitz	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
			Issued: July 25, 2019
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: EX3-7534_Jul19

Page 1 of 17

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization ϕ	ϕ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 – SN:7534

July 25, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7534**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.48	0.40	0.50	± 10.1 %
DCP (mV) ^B	95.7	98.1	103.0	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^C (k=2)
0	CW	X	0.0	0.0	1.0	0.00	114.8	±2.5 %
		Y	0.0	0.0	1.0		141.6	
		Z	0.0	0.0	1.0		127.4	

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).^B Numerical linearization parameter; uncertainty not required.^C Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:7534

July 25, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7534**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	85.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4- SN:7534

July 25, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7534

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^e	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^h (mm)	Unc (k=2)
150	52.3	0.76	13.79	13.79	13.79	0.00	1.00	± 13.3 %
300	45.3	0.87	12.60	12.60	12.60	0.08	1.20	± 13.3 %
450	43.5	0.87	11.59	11.59	11.59	0.12	1.30	± 13.3 %
750	41.9	0.89	10.17	10.17	10.17	0.35	1.04	± 12.0 %
835	41.5	0.90	9.90	9.90	9.90	0.49	0.83	± 12.0 %
900	41.5	0.97	9.84	9.84	9.84	0.49	0.80	± 12.0 %
1450	40.5	1.20	8.73	8.73	8.73	0.37	0.80	± 12.0 %
1810	40.0	1.40	8.13	8.13	8.13	0.34	0.88	± 12.0 %
1900	40.0	1.40	8.05	8.05	8.05	0.33	0.88	± 12.0 %
2100	39.8	1.49	8.04	8.04	8.04	0.33	0.85	± 12.0 %
2300	39.5	1.67	7.83	7.83	7.83	0.31	0.90	± 12.0 %
2450	39.2	1.80	7.58	7.58	7.58	0.36	0.90	± 12.0 %
2600	39.0	1.96	7.29	7.29	7.29	0.34	0.90	± 12.0 %
3500	37.9	2.91	6.61	6.61	6.61	0.30	1.30	± 13.1 %
3700	37.7	3.12	6.48	6.48	6.48	0.30	1.30	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^e At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^h Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7534

July 25, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7534

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^h (mm)	Unc (k=2)
150	61.9	0.80	13.36	13.36	13.36	0.00	1.00	± 13.3 %
300	58.2	0.92	12.35	12.35	12.35	0.03	1.20	± 13.3 %
450	56.7	0.94	11.87	11.87	11.87	0.06	1.30	± 13.3 %
750	55.5	0.96	10.23	10.23	10.23	0.42	0.89	± 12.0 %
835	55.2	0.97	10.04	10.04	10.04	0.47	0.80	± 12.0 %
900	55.0	1.05	9.80	9.80	9.80	0.49	0.80	± 12.0 %
1450	54.0	1.30	8.59	8.59	8.59	0.33	0.80	± 12.0 %
1810	53.3	1.52	8.16	8.16	8.16	0.42	0.88	± 12.0 %
1900	53.3	1.52	7.95	7.95	7.95	0.36	0.88	± 12.0 %
2100	53.2	1.62	7.93	7.93	7.93	0.36	0.85	± 12.0 %
2300	52.9	1.81	7.88	7.88	7.88	0.34	0.90	± 12.0 %
2450	52.7	1.95	7.68	7.68	7.68	0.33	0.90	± 12.0 %
2600	52.5	2.16	7.59	7.59	7.59	0.23	0.90	± 12.0 %
3500	51.3	3.31	6.37	6.37	6.37	0.40	1.30	± 13.1 %
3700	51.0	3.55	6.13	6.13	6.13	0.40	1.30	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^h Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7534

July 25, 2019



Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

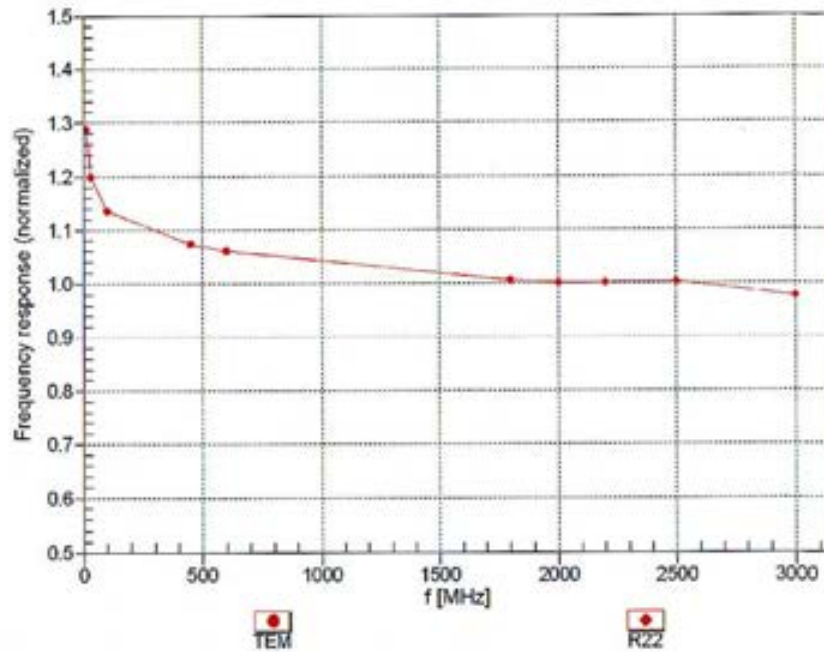Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

EX3DV4- SN:7534

July 25, 2019

Receiving Pattern (ϕ), $\theta = 0^\circ$

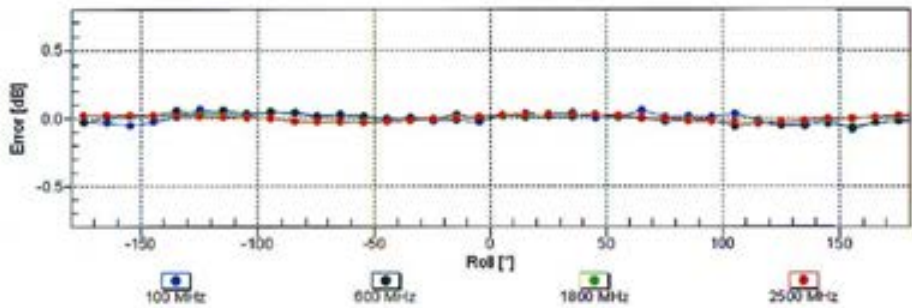
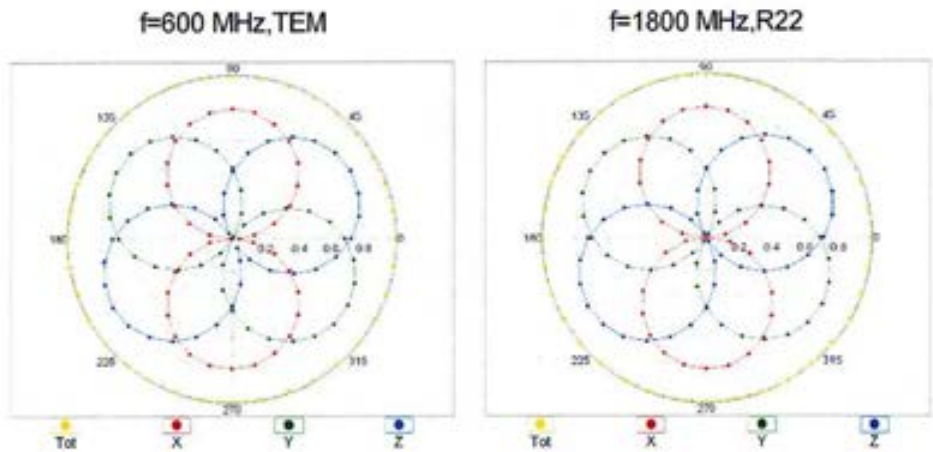


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

EX3DV4- SN:7534

July 25, 2019

Dynamic Range f(SAR_{head})
(TEM cell , f_{eval}= 1900 MHz)

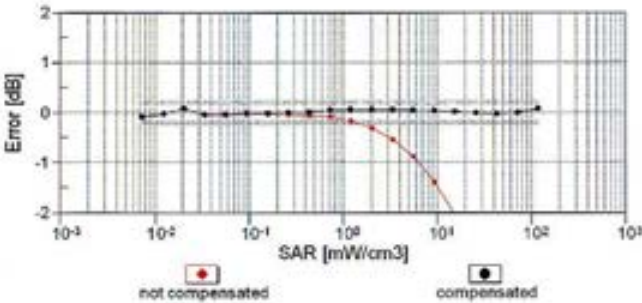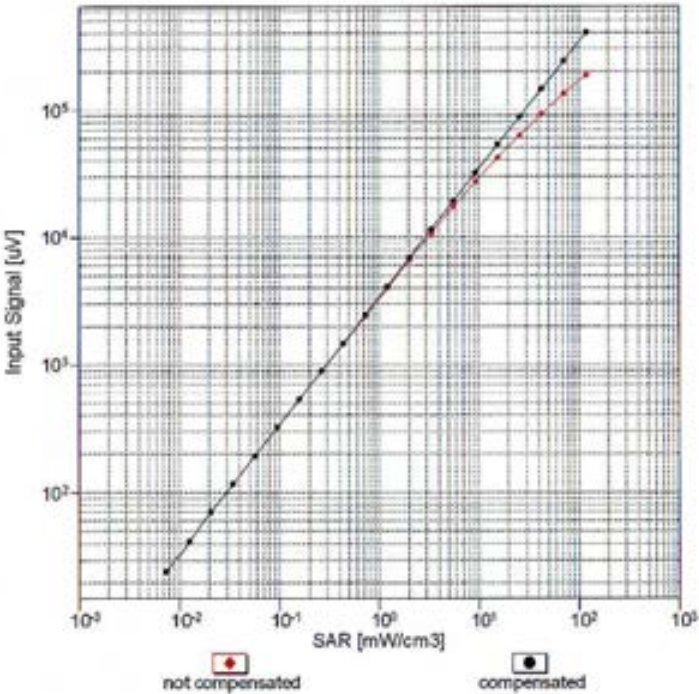


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


EX3DV4- SN:7534

July 25, 2019

Conversion Factor Assessment

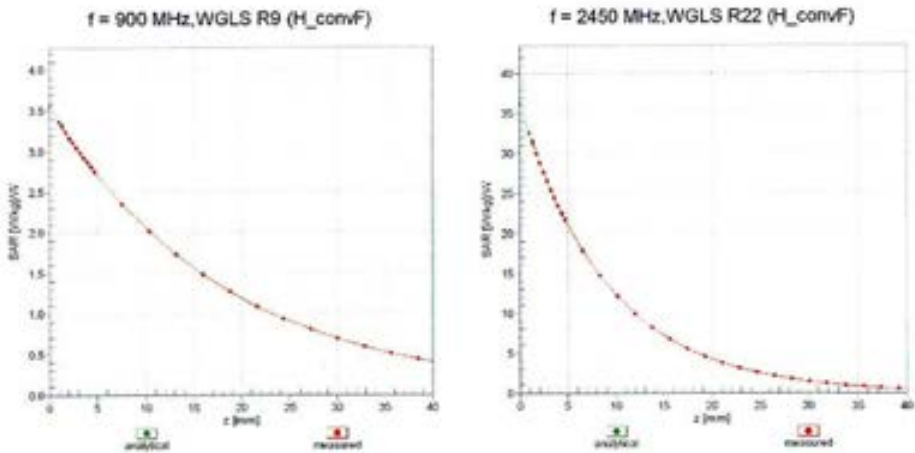

Deviation from Isotropy in Liquid
Error (ϕ, θ), f = 900 MHz

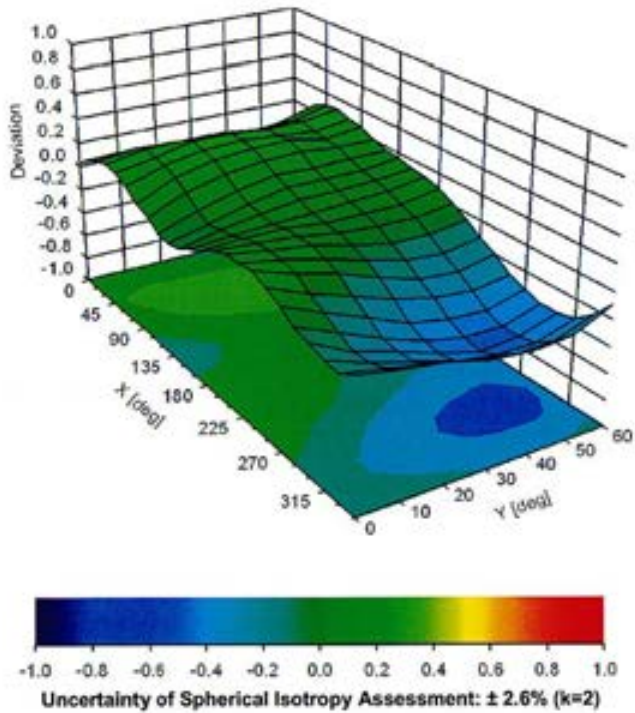

EX3DV4-- SN:7534

July 25, 2019

Appendix: Modulation Calibration Parameters

UID	Communication System Name		A dB	B dBV _{μV}	C	D dB	VR mV	Unc ^L (k=2)
0	CW	X	0.0	0.0	1.0	0.00	114.8	±2.5 %
		Y	0.0	0.0	1.0		141.6	
		Z	0.0	0.0	1.0		127.4	
10011-CAB	UMTS-FDD (WCDMA)	X	3.14	64.9	17.0	2.91	123.6	±0.7 %
		Y	2.93	64.5	17.1		110.4	
		Z	3.59	69.6	20.1		137.7	
10097-CAB	UMTS-FDD (HSDPA)	X	4.49	65.6	17.8	3.98	130.9	±0.9 %
		Y	4.14	64.7	17.5		115.6	
		Z	4.74	68.2	19.6		145.7	
10098-CAB	UMTS-FDD (HSUPA, Subtest 2)	X	4.54	65.8	18.0	3.98	131.5	±0.9 %
		Y	4.19	65.0	17.6		116.2	
		Z	4.73	68.1	19.5		146.4	
10100-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.37	66.8	19.2	5.67	138.6	±1.4 %
		Y	5.80	65.1	18.3		120.5	
		Z	5.96	66.1	19.2		109.1	
10101-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	7.51	67.4	19.9	6.42	147.7	±1.7 %
		Y	6.92	65.9	19.0		128.1	
		Z	7.01	66.6	19.6		115.7	
10108-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.24	66.4	19.2	5.80	135.8	±1.2 %
		Y	5.70	64.9	18.4		118.3	
		Z	5.83	65.8	19.1		107.3	
10109-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	7.25	67.2	19.9	6.43	143.2	±1.7 %
		Y	6.64	65.6	18.9		123.8	
		Z	6.76	66.4	19.6		112.2	
10110-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	5.94	66.0	19.0	5.75	132.1	±1.2 %
		Y	5.42	64.6	18.2		115.7	
		Z	5.97	67.3	20.0		146.9	
10111-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	6.96	67.0	19.8	6.44	138.0	±1.4 %
		Y	6.39	65.5	18.9		119.4	
		Z	6.50	66.4	19.6		108.4	
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	9.93	68.0	20.8	8.07	125.4	±2.2 %
		Y	9.20	66.5	19.9		105.4	
		Z	10.03	68.9	21.5		140.9	
10140-CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	7.71	67.7	20.1	6.49	149.5	±1.7 %
		Y	7.05	66.0	19.1		129.0	
		Z	7.17	66.8	19.8		116.6	
10142-CAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	5.75	65.9	19.0	5.73	129.0	±1.2 %
		Y	5.24	64.4	18.1		112.8	
		Z	5.77	67.2	19.9		143.4	
10143-CAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	6.69	67.0	19.7	6.35	134.2	±1.4 %
		Y	6.08	65.4	18.8		115.5	
		Z	6.71	68.2	20.6		148.6	

Certificate No: EX3-7534_Jul19

Page 11 of 17

EX3DV4- SN:7534

July 25, 2019

10145-CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	5.53	66.1	19.1	5.76	124.5	±1.2 %
		Y	5.03	64.6	18.2		108.8	
		Z	5.56	67.5	20.1		137.7	
10146-CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	6.37	67.1	19.8	6.41	127.2	±1.4 %
		Y	5.77	65.6	18.9		108.8	
		Z	6.41	68.6	20.8		140.5	
10149-CAE	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	7.24	67.2	19.9	6.42	143.4	±1.4 %
		Y	6.65	65.6	18.9		124.0	
		Z	6.73	66.3	19.6		111.7	
10154-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	5.93	66.0	19.0	5.75	131.8	±1.2 %
		Y	5.44	64.6	18.2		115.4	
		Z	5.97	67.2	19.9		147.1	
10155-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	6.97	67.1	19.8	6.43	138.0	±1.7 %
		Y	6.38	65.5	18.9		118.9	
		Z	6.46	66.3	19.6		108.1	
10156-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	5.69	65.8	18.9	5.79	127.9	±1.2 %
		Y	5.23	64.5	18.2		111.8	
		Z	5.73	67.2	20.0		141.7	
10157-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	6.66	67.0	19.8	6.49	131.7	±1.4 %
		Y	6.09	65.5	18.9		113.7	
		Z	6.72	68.3	20.8		146.2	
10160-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.37	66.6	19.3	5.82	137.1	±1.4 %
		Y	5.80	64.9	18.4		119.2	
		Z	5.93	65.9	19.1		107.4	
10161-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	7.27	67.3	19.9	6.43	143.5	±1.4 %
		Y	6.68	65.8	19.0		123.6	
		Z	6.78	66.5	19.7		112.0	
10166-CAF	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	4.92	65.6	18.7	5.46	119.3	±0.9 %
		Y	4.74	65.5	18.7		144.1	
		Z	4.98	67.4	20.0		132.3	
10167-CAF	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	5.77	67.0	19.7	6.21	120.3	±1.2 %
		Y	5.56	66.9	19.7		144.3	
		Z	5.80	68.5	20.8		132.4	
10169-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.74	65.6	18.9	5.73	113.7	±1.2 %
		Y	4.59	65.5	18.9		138.0	
		Z	4.74	67.0	20.1		125.7	
10170-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	5.35	66.3	19.7	6.52	111.5	±1.2 %
		Y	5.17	66.2	19.6		135.2	
		Z	5.35	67.8	20.8		123.4	
10175-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4.73	65.5	18.9	5.72	113.4	±0.9 %
		Y	4.56	65.4	18.8		137.6	
		Z	4.74	67.0	20.1		125.7	
10176-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	5.34	66.3	19.7	6.52	111.6	±1.2 %
		Y	5.16	66.1	19.6		135.1	
		Z	5.34	67.7	20.8		123.8	

Certificate No: EX3-7534_Jul19

Page 12 of 17

EX3DV4- SN:7534

July 25, 2019

10177-CAI	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	4.75	65.6	19.0	5.73	113.3	±0.9 %
		Y	4.58	65.4	18.9		137.6	
		Z	4.77	67.2	20.2		125.9	
10178-CAG	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	5.35	66.3	19.7	6.52	111.6	±1.2 %
		Y	5.17	66.2	19.6		135.2	
		Z	5.33	67.7	20.7		123.7	
10181-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	4.73	65.5	18.9	5.72	113.5	±1.2 %
		Y	4.61	65.6	19.0		137.6	
		Z	4.75	67.1	20.1		125.4	
10182-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	5.35	66.4	19.7	6.52	111.8	±1.2 %
		Y	5.16	66.2	19.6		135.1	
		Z	5.37	67.9	20.9		123.6	
10184-CAE	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	4.72	65.4	18.8	5.73	113.4	±1.2 %
		Y	4.60	65.6	19.0		138.0	
		Z	4.76	67.1	20.1		125.7	
10185-CAE	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	5.32	66.3	19.6	6.51	111.7	±1.2 %
		Y	5.19	66.4	19.7		135.4	
		Z	5.36	67.8	20.8		123.8	
10187-CAF	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	4.73	65.5	18.9	5.73	113.3	±0.9 %
		Y	4.60	65.6	18.9		137.8	
		Z	4.76	67.1	20.1		125.8	
10188-CAF	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	5.34	66.3	19.6	6.52	111.7	±1.2 %
		Y	5.16	66.1	19.5		135.5	
		Z	5.38	67.8	20.8		123.8	
10196-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.51	67.7	20.8	8.10	118.9	±2.2 %
		Y	9.41	67.9	20.8		145.9	
		Z	9.59	68.7	21.4		133.1	
10225-CAB	UMTS-FDD (HSPA+)	X	7.07	67.3	19.6	5.97	145.5	±1.4 %
		Y	6.45	65.9	18.7		124.9	
		Z	6.56	66.7	19.4		113.3	
10274-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	X	5.94	66.7	18.7	4.87	140.9	±1.2 %
		Y	5.41	65.5	18.0		122.0	
		Z	5.63	66.8	19.0		109.8	
10275-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	4.31	65.5	17.8	3.96	127.3	±0.7 %
		Y	3.94	64.4	17.4		111.9	
		Z	4.44	67.5	19.3		141.2	
10297-AAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	6.26	66.5	19.2	5.81	135.5	±1.4 %
		Y	5.67	64.7	18.2		116.9	
		Z	6.28	67.6	20.1		150.0	
10298-AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	5.54	65.8	18.9	5.72	126.1	±1.2 %
		Y	5.04	64.4	18.1		109.6	
		Z	5.56	67.2	19.9		138.9	
10299-AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	6.48	67.2	19.8	6.39	129.9	±1.4 %
		Y	5.88	65.7	19.0		110.4	
		Z	6.53	68.6	20.8		143.0	

Certificate No: EX3-7534_Jul19

Page 13 of 17

EX3DV4- SN:7534

July 25, 2019

10311-AAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.79	66.9	19.5	6.06	140.5	±1.4 %
		Y	6.24	65.4	18.7		122.4	
		Z	6.33	66.2	19.3		110.2	
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.56	65.8	16.8	1.54	127.6	±0.5 %
		Y	2.32	65.0	16.6		113.0	
		Z	3.18	72.3	20.8		141.3	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	9.46	67.7	20.8	8.14	118.5	±2.5 %
		Y	9.37	67.9	20.8		143.7	
		Z	9.53	68.5	21.4		131.7	
10435-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.60	68.3	21.8	7.82	132.6	±1.7 %
		Y	4.90	65.6	20.2		114.4	
		Z	5.54	69.6	22.8		143.8	
10457-AAA	UMTS-FDD (DC-HSDPA)	X	7.92	65.9	19.1	6.62	115.8	±1.4 %
		Y	7.95	66.5	19.3		142.3	
		Z	8.00	66.9	19.8		128.8	
10460-AAA	UMTS-FDD (WCDMA, AMR)	X	2.76	65.6	17.2	2.39	121.7	±0.5 %
		Y	2.62	65.7	17.5		148.3	
		Z	3.27	71.2	20.7		134.2	
10461-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.60	68.3	21.7	7.82	132.4	±1.9 %
		Y	4.89	65.5	20.1		114.5	
		Z	5.54	69.6	22.8		144.3	
10462-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.02	69.1	22.3	8.30	129.7	±1.7 %
		Y	5.54	67.8	21.6		147.7	
		Z	5.96	70.5	23.4		141.0	
10464-AAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.58	68.2	21.7	7.82	131.9	±1.7 %
		Y	4.90	65.6	20.2		115.3	
		Z	5.57	69.8	22.9		143.8	
10465-AAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.02	69.1	22.3	8.32	129.4	±1.7 %
		Y	5.55	67.8	21.6		147.7	
		Z	5.99	70.5	23.4		141.2	
10467-AAE	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.57	68.2	21.6	7.82	131.7	±1.7 %
		Y	4.92	65.7	20.2		115.6	
		Z	5.54	69.6	22.8		143.4	
10468-AAE	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.03	69.1	22.4	8.32	129.6	±1.7 %
		Y	5.55	67.8	21.6		147.8	
		Z	5.99	70.6	23.5		141.2	
10470-AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.57	68.2	21.6	7.82	132.2	±1.7 %
		Y	4.90	65.6	20.2		115.1	
		Z	5.52	69.5	22.7		143.8	
10471-AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.03	69.1	22.3	8.32	130.0	±1.9 %
		Y	5.54	67.7	21.6		147.7	
		Z	5.99	70.5	23.5		141.0	

Certificate No: EX3-7534_Jul19

Page 14 of 17

EX3DV4- SN:7534

July 25, 2019

10473-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.56	68.2	21.7	7.82	131.5	±1.7 %
		Y	4.88	65.5	20.1		115.4	
		Z	5.55	69.6	22.8		143.9	
10474-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.03	69.2	22.4	8.32	129.7	±1.9 %
		Y	5.56	67.8	21.6		147.9	
		Z	6.02	70.7	23.5		141.6	
10477-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.02	69.1	22.3	8.32	130.1	±1.7 %
		Y	5.56	67.8	21.7		148.4	
		Z	5.99	70.5	23.5		141.8	
10479-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.86	67.8	21.3	7.74	138.5	±1.7 %
		Y	5.21	65.6	20.1		121.3	
		Z	5.51	67.6	21.5		111.1	
10480-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.54	69.2	22.2	8.18	140.8	±1.7 %
		Y	5.70	66.5	20.6		120.5	
		Z	6.13	68.9	22.2		111.5	
10482-AAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.26	67.8	21.3	7.71	146.1	±1.7 %
		Y	5.53	65.3	19.8		126.5	
		Z	5.90	67.5	21.3		117.2	
10483-AAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.87	67.5	21.2	8.39	109.9	±1.7 %
		Y	6.44	66.6	20.7		129.7	
		Z	6.88	68.8	22.2		120.2	
10485-AAE	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.26	67.7	21.2	7.59	149.1	±1.7 %
		Y	5.54	65.3	19.8		128.9	
		Z	5.91	67.4	21.3		119.3	
10486-AAE	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.00	67.3	21.2	8.38	112.9	±1.9 %
		Y	6.56	66.4	20.6		133.1	
		Z	7.00	68.5	22.0		123.8	
10488-AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.27	66.3	20.3	7.70	113.1	±1.7 %
		Y	5.90	65.4	19.9		133.5	
		Z	6.25	67.3	21.2		123.4	
10489-AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.28	67.3	21.1	8.31	118.7	±1.9 %
		Y	6.82	66.2	20.5		139.4	
		Z	7.24	68.2	21.8		130.2	
10491-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.66	66.7	20.5	7.74	117.4	±1.7 %
		Y	6.23	65.7	20.0		138.2	
		Z	6.67	67.8	21.4		128.6	
10492-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.74	67.6	21.3	8.41	124.1	±2.2 %
		Y	7.25	66.5	20.7		144.6	
		Z	7.72	68.5	22.0		136.0	
10494-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.65	66.8	20.6	7.74	117.0	±1.7 %
		Y	6.19	65.6	20.0		137.3	
		Z	6.67	67.9	21.5		128.3	
10495-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.66	67.4	21.2	8.37	124.2	±2.2 %
		Y	7.15	66.2	20.5		144.7	
		Z	7.66	68.4	22.0		136.0	

Certificate No: EX3-7534_Jul19

Page 15 of 17

EX3DV4- SN:7534

July 25, 2019

10497-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.18	67.9	21.2	7.67	145.5	±1.7 %
		Y	5.45	65.5	19.9		125.5	
		Z	5.82	67.6	21.3		116.2	
10498-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.18	69.3	22.2	8.40	149.4	±1.9 %
		Y	6.32	66.7	20.7		126.7	
		Z	6.76	68.8	22.2		118.6	
10500-AAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.08	66.2	20.3	7.67	110.6	±1.7 %
		Y	5.70	65.3	19.8		130.2	
		Z	6.06	67.3	21.2		120.7	
10501-AAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.18	67.4	21.2	8.44	115.2	±1.9 %
		Y	6.74	66.5	20.7		134.8	
		Z	7.16	68.4	22.0		125.5	
10503-AAE	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.30	66.3	20.4	7.72	113.1	±1.7 %
		Y	5.89	65.3	19.8		133.2	
		Z	6.29	67.4	21.3		124.1	
10504-AAE	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.27	67.2	21.1	8.31	118.8	±1.9 %
		Y	6.83	66.3	20.5		139.5	
		Z	7.27	68.2	21.9		129.9	
10506-AAE	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.63	66.7	20.5	7.74	116.8	±1.7 %
		Y	6.17	65.6	19.9		137.5	
		Z	6.66	67.9	21.5		128.5	
10507-AAE	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.66	67.5	21.2	8.36	124.2	±1.9 %
		Y	7.16	66.4	20.6		145.1	
		Z	7.66	68.4	22.0		136.1	
10509-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.26	67.3	20.9	7.99	122.4	±1.9 %
		Y	6.73	66.1	20.3		142.7	
		Z	7.30	68.4	21.8		134.5	
10510-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.19	67.9	21.5	8.49	130.0	±2.2 %
		Y	7.33	65.5	20.0		111.1	
		Z	8.17	68.8	22.2		143.1	
10512-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.96	67.3	20.8	7.74	120.4	±1.9 %
		Y	6.44	65.9	20.1		141.5	
		Z	7.01	68.4	21.6		132.9	
10513-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.03	67.7	21.4	8.42	129.6	±2.2 %
		Y	7.47	66.4	20.6		149.7	
		Z	8.03	68.6	22.1		142.1	
10515-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)	X	2.56	65.8	16.8	1.56	127.2	±0.5 %
		Y	2.33	65.4	16.9		113.2	
		Z	3.31	73.3	21.3		139.9	
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	2.72	66.3	17.3	1.99	124.0	±0.7 %
		Y	2.48	65.6	17.1		108.9	
		Z	3.56	74.0	21.8		137.0	

Certificate No: EX3-7534_Jul19

Page 16 of 17

EX3DV4– SN:7534

July 25, 2019

10572-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	2.65	65.9	17.0	1.99	123.7	±0.5 %
		Y	2.37	65.1	16.9		149.6	
		Z	3.37	73.1	21.3		136.5	
10575-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	9.66	67.7	21.0	8.59	116.3	±2.5 %
		Y	9.59	68.0	21.2		140.9	
		Z	9.79	68.8	21.8		129.6	
10591-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	9.84	67.9	21.2	8.63	118.1	±2.5 %
		Y	9.69	68.0	21.2		142.7	
		Z	9.93	68.8	21.9		131.7	
10599-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	10.43	68.4	21.4	8.79	124.7	±2.7 %
		Y	10.24	68.4	21.4		150.0	
		Z	10.54	69.3	22.1		138.8	

² Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **EX3-7364_Jan19**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:7364**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v5, QA CAL-23.v5,
QA CAL-25.v7
Calibration procedure for dosimetric E-field probes**

Calibration date: **January 23, 2019**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
DAE4	SN: 660	19-Dec-18 (No. DAE4-660_Dec18)	Dec-19
Reference Probe ES3DV2	SN: 3013	31-Dec-18 (No. ES3-3013_Dec18)	Dec-19
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
Issued: January 26, 2019			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: EX3-7364_Jan19

Page 1 of 15

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}:** Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)/_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}:** DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}:** A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle:** The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

Certificate No: EX3-7364_Jan19

Page 2 of 15

EX3DV4 – SN:7364

January 23, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7364**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V/m})^2$) ^A	0.46	0.46	0.57	$\pm 10.1 \%$
DCP (mV) ^B	99.7	97.6	99.3	

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Max dev.	Unc ^C (k=2)
0	CW	X	0.0	0.0	1.0	0.00	114.6	+ 2.7 %	$\pm 4.7 \%$
		Y	0.0	0.0	1.0		112.4		
		Y	0.0	0.0	1.0		127.7		

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).^B Numerical linearization parameter: uncertainty not required.^C Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:7364

January 23, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7364**Sensor Model Parameters****Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	129.9
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4- SN:7364

January 23, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7364

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth (mm) ^g	Unc (k=2)
150	52.3	0.76	12.97	12.97	12.97	0.00	1.00	± 13.3 %
300	45.3	0.87	12.05	12.05	12.05	0.09	1.20	± 13.3 %
450	43.5	0.87	10.75	10.75	10.75	0.13	1.30	± 13.3 %
750	41.9	0.89	10.42	10.42	10.42	0.56	0.80	± 12.0 %
835	41.5	0.90	10.23	10.23	10.23	0.30	1.09	± 12.0 %
900	41.5	0.97	9.78	9.78	9.78	0.31	1.08	± 12.0 %
1810	40.0	1.40	8.25	8.25	8.25	0.35	0.87	± 12.0 %
1900	40.0	1.40	8.19	8.19	8.19	0.37	0.85	± 12.0 %
2100	39.8	1.49	8.15	8.15	8.15	0.25	1.09	± 12.0 %
2450	39.2	1.80	7.38	7.38	7.38	0.40	0.85	± 12.0 %
5250	35.9	4.71	5.08	5.08	5.08	0.40	1.80	± 13.1 %
5500	35.6	4.96	4.86	4.86	4.86	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.68	4.68	4.68	0.40	1.80	± 13.1 %
5750	35.4	5.22	4.72	4.72	4.72	0.40	1.80	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7364

January 23, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7364

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
150	61.9	0.80	12.37	12.37	12.37	0.00	1.00	± 13.3 %
300	58.2	0.92	11.79	11.79	11.79	0.05	1.20	± 13.3 %
450	56.7	0.94	11.17	11.17	11.17	0.14	1.30	± 13.3 %
750	55.5	0.96	10.24	10.24	10.24	0.50	0.83	± 12.0 %
835	55.2	0.97	9.94	9.94	9.94	0.41	0.90	± 12.0 %
900	55.0	1.05	9.93	9.93	9.93	0.35	0.96	± 12.0 %
1810	53.3	1.52	7.97	7.97	7.97	0.44	0.85	± 12.0 %
1900	53.3	1.52	7.89	7.89	7.89	0.46	0.85	± 12.0 %
2100	53.2	1.62	7.96	7.96	7.96	0.46	0.90	± 12.0 %
2450	52.7	1.95	7.48	7.48	7.48	0.34	0.98	± 12.0 %
5250	48.9	5.36	4.47	4.47	4.47	0.45	1.90	± 13.1 %
5500	48.6	5.65	4.07	4.07	4.07	0.45	1.90	± 13.1 %
5600	48.5	5.77	3.89	3.89	3.89	0.45	1.90	± 13.1 %
5750	48.3	5.94	4.19	4.19	4.19	0.45	1.90	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7364

January 23, 2019

Frequency Response of E-Field
(TEM-Cell:ifi110 EXX, Waveguide: R22)

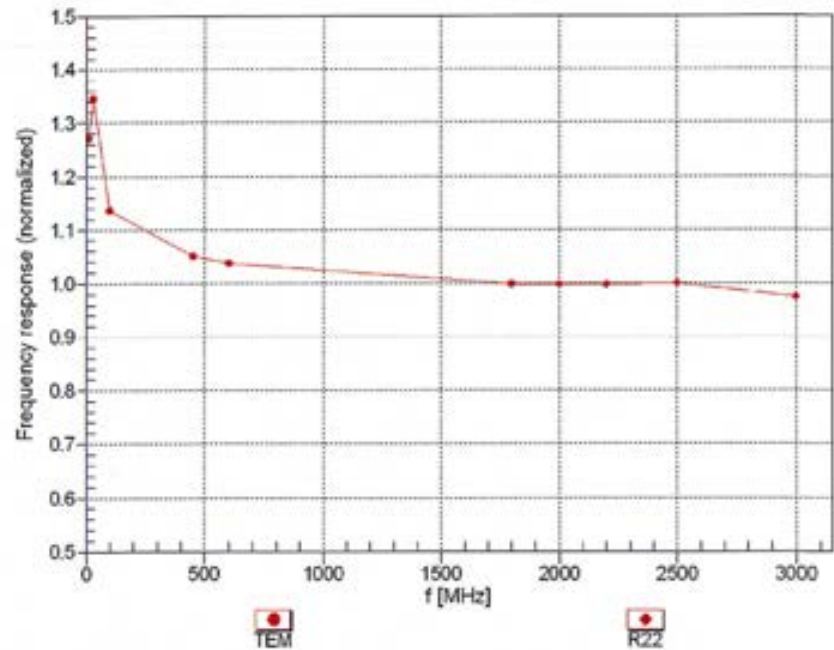


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

EX3DV4- SN:7364

January 23, 2019

Receiving Pattern (ϕ), $\theta = 0^\circ$


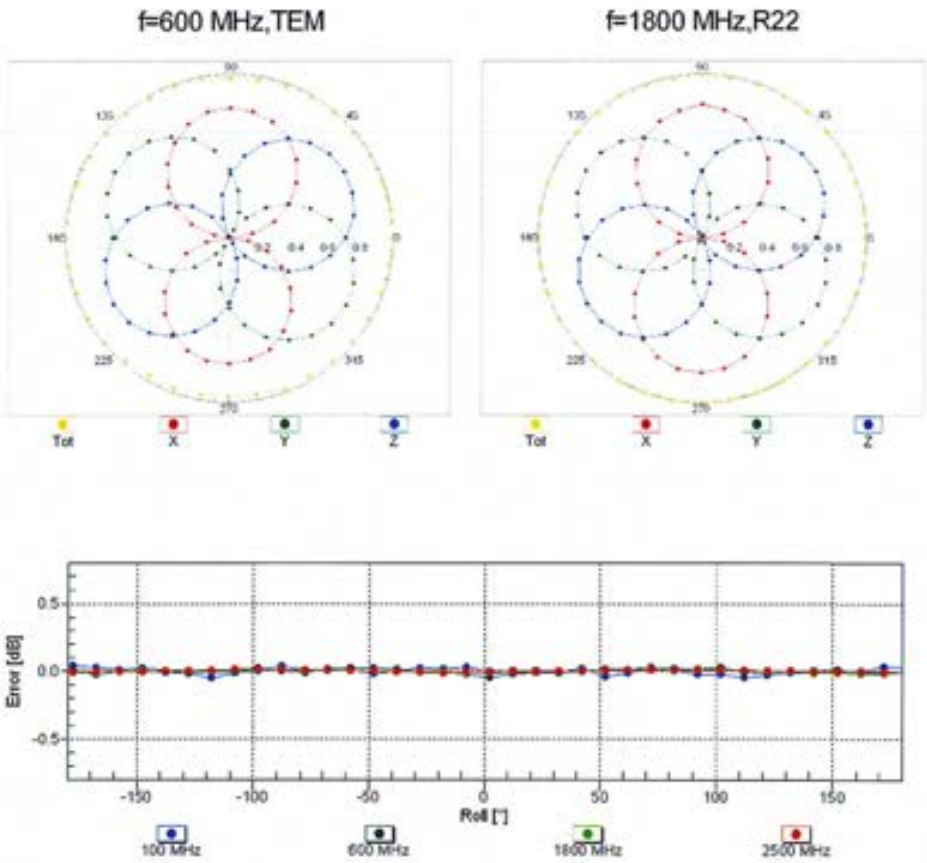


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

EX3DV4- SN:7364

January 23, 2019

Dynamic Range f(SAR_{head})
(TEM cell , f_{eval}= 1900 MHz)

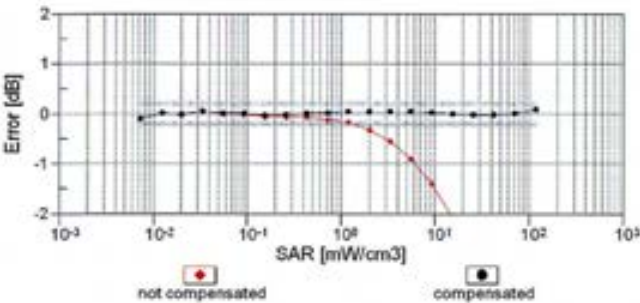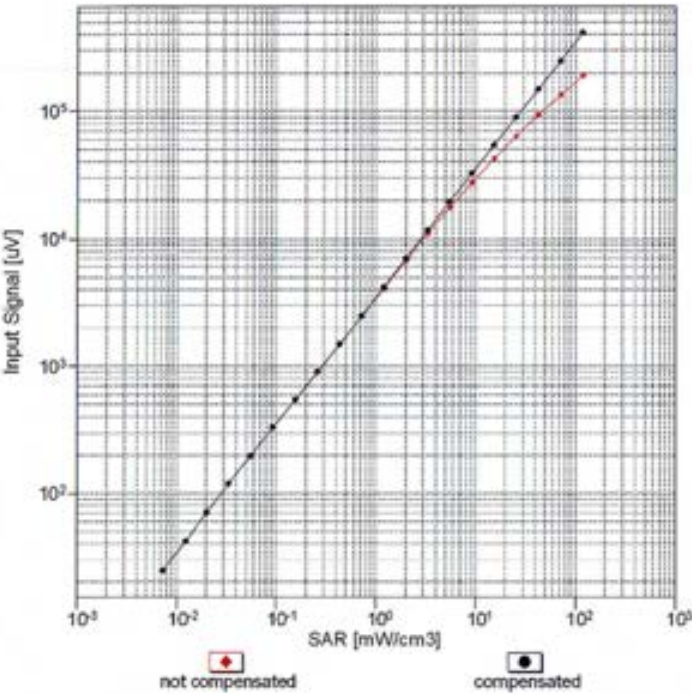


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


EX3DV4- SN:7364

January 23, 2019

Conversion Factor Assessment

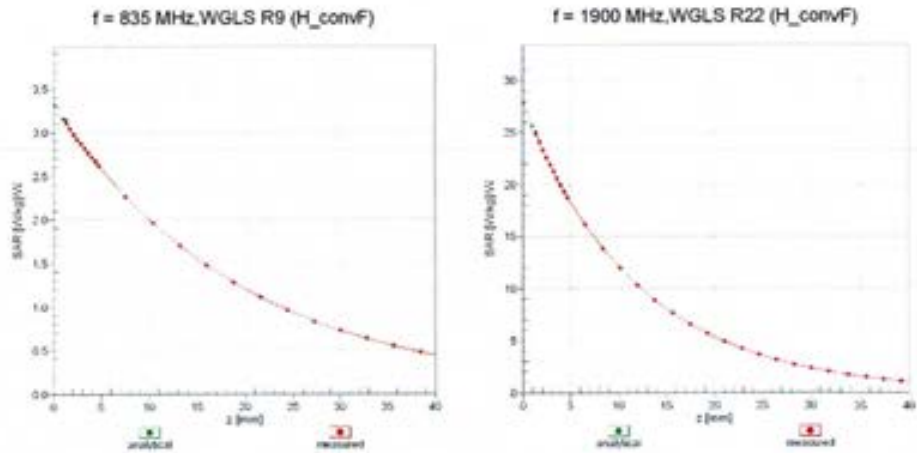

Deviation from Isotropy in Liquid
Error (ϕ, θ), f = 900 MHz

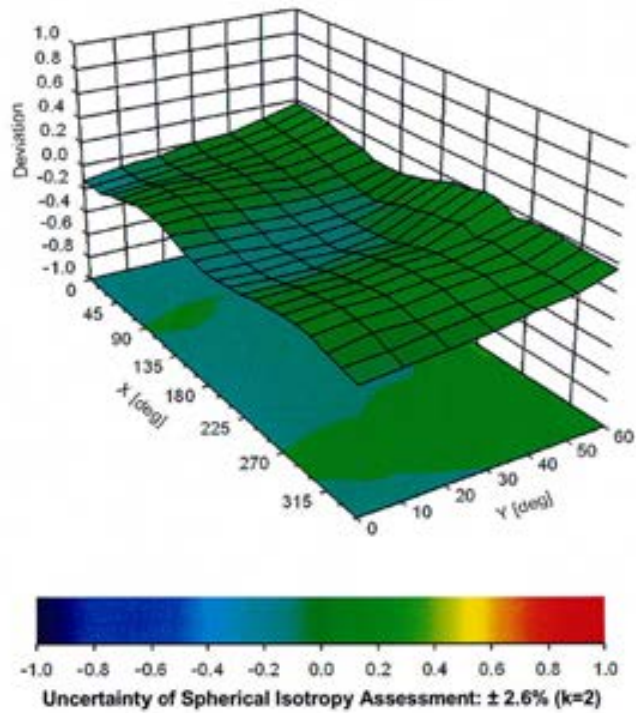

EX3DV4- SN:7364

January 23, 2019

Appendix: Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu V}$	C	D dB	VR mV	Unc ⁿ (k=2)
0	CW	X	0.0	0.0	1.0	0.00	114.6	$\pm 2.7\%$
		Y	0.0	0.0	1.0		112.4	
		Z	0.0	0.0	1.0		127.7	
10021-DAC	GSM-FDD (TDMA, GMSK)	X	1.72	63.0	12.0	9.39	94.6	$\pm 1.9\%$
		Y	1.71	65.4	13.2		68.7	
		Z	2.22	65.7	13.5		108.0	
10023-DAC	GPRS-FDD (TDMA, GMSK, TN 0)	X	1.75	63.4	12.3	9.57	91.5	$\pm 1.7\%$
		Y	1.83	65.6	13.2		67.1	
		Z	2.26	65.5	13.3		104.9	
10024-DAC	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	1.71	64.7	10.9	6.56	147.1	$\pm 1.2\%$
		Y	4.98	81.5	18.4		127.8	
		Z	2.35	69.4	14.0		131.0	
10025-DAC	EDGE-FDD (TDMA, 8PSK, TN 0)	X	5.28	72.4	25.7	12.62	61.2	$\pm 1.2\%$
		Y	4.38	68.1	23.6		44.2	
		Z	5.84	75.3	27.6		69.5	
10026-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1)	X	5.13	74.3	24.8	9.55	140.7	$\pm 1.9\%$
		Y	4.43	71.4	23.6		100.8	
		Z	5.35	74.8	25.1		128.7	
10027-DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	1.22	62.4	8.8	4.80	140.5	$\pm 1.7\%$
		Y	29.58	100.0	21.9		130.1	
		Z	34.45	99.7	22.2		118.2	
10028-DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	54.30	99.7	20.4	3.55	116.7	$\pm 1.9\%$
		Y	0.97	66.1	10.9		148.2	
		Z	43.93	99.7	21.0		131.0	
10029-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	X	4.59	72.8	23.2	7.78	137.7	$\pm 1.4\%$
		Y	3.83	68.9	21.1		125.2	
		Z	5.87	78.6	26.0		118.8	
10039-CAB	CDMA2000 (1xRTT, RC1)	X	4.72	66.7	19.1	4.57	123.7	$\pm 0.9\%$
		Y	4.44	65.3	18.2		121.2	
		Z	4.88	67.4	19.4		140.2	
10056-CAA	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	X	4.17	68.9	23.5	11.01	89.7	$\pm 1.4\%$
		Y	3.52	65.8	22.2		64.7	
		Z	4.64	71.3	24.8		101.7	
10058-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	X	4.77	75.3	23.9	6.52	116.4	$\pm 1.4\%$
		Y	4.03	71.6	22.1		147.1	
		Z	5.32	76.9	24.4		133.3	
10081-CAB	CDMA2000 (1xRTT, RC3)	X	4.00	66.6	18.9	3.97	120.2	$\pm 0.5\%$
		Y	3.78	65.2	18.0		118.1	
		Z	4.11	67.0	19.1		136.1	

EX3DV4- SN:7364

January 23, 2019

10090-DAC	GPRS-FDD (TDMA, GMSK, TN 0-4)	X	1.59	64.6	11.2	6.56	144.9	±1.9 %
		Y	1.86	68.3	12.9		126.4	
		Z	2.87	71.7	14.8		131.1	
10099-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-4)	X	5.33	75.9	25.9	9.55	139.0	±2.2 %
		Y	4.36	71.0	23.4		99.7	
		Z	5.59	76.5	26.3		126.6	
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	9.95	68.2	21.0	8.07	124.6	±2.2 %
		Y	9.62	67.4	20.5		119.2	
		Z	10.30	69.2	21.6		143.9	
10196-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.61	68.0	21.0	8.10	119.9	±1.9 %
		Y	9.28	67.1	20.4		114.4	
		Z	9.94	69.0	21.6		137.6	
10290-AAB	CDMA2000, RC1, SO55, Full Rate	X	4.41	67.8	19.3	3.91	123.6	±0.7 %
		Y	4.02	65.7	18.1		120.5	
		Z	4.58	68.5	19.6		139.9	
10291-AAB	CDMA2000, RC3, SO55, Full Rate	X	3.79	67.8	19.3	3.46	120.1	±0.5 %
		Y	3.37	65.1	17.7		117.4	
		Z	3.91	68.2	19.5		135.9	
10292-AAB	CDMA2000, RC3, SO32, Full Rate	X	3.75	67.9	19.4	3.39	120.3	±0.5 %
		Y	3.35	65.3	17.8		117.1	
		Z	3.86	68.3	19.5		135.5	
10293-AAB	CDMA2000, RC3, SO3, Full Rate	X	3.86	68.0	19.4	3.50	120.3	±0.5 %
		Y	3.44	65.4	17.9		117.0	
		Z	3.91	68.0	19.4		135.8	
10295-AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	X	5.27	66.0	23.4	12.49	74.0	±1.4 %
		Y	4.56	62.5	21.4		53.0	
		Z	5.70	68.1	24.8		84.1	
10403-AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	5.20	70.4	19.9	3.76	126.4	±0.5 %
		Y	4.56	67.7	18.4		123.3	
		Z	5.28	70.5	19.9		143.5	
10404-AAB	CDMA2000 (1xEV-DO, Rev. A)	X	5.38	71.6	20.6	3.77	124.9	±0.7 %
		Y	4.42	67.3	18.2		121.9	
		Z	5.02	69.8	19.6		142.4	
10406-AAB	CDMA2000, RC3, SO32, SCH0, Full Rate	X	6.70	71.0	20.9	5.22	129.5	±0.7 %
		Y	5.85	67.9	19.2		125.2	
		Z	6.66	70.6	20.7		148.5	
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	3.44	72.9	21.1	1.54	126.4	±0.5 %
		Y	2.56	67.0	17.9		123.5	
		Z	3.20	71.3	20.2		142.2	
10416-AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	X	9.70	68.1	21.2	8.23	119.3	±1.9 %
		Y	9.38	67.2	20.5		114.1	
		Z	10.02	69.0	21.7		137.1	

Certificate No: EX3-7364_Jan19

Page 12 of 15

EX3DV4- SN:7364

January 23, 2019

10417-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	X	9.70	68.1	21.2	8.23	119.3	±1.9 %
		Y	9.42	67.3	20.6		114.1	
		Z	10.03	69.0	21.7		137.4	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	9.58	68.0	21.1	8.14	118.4	±1.9 %
		Y	9.30	67.2	20.5		113.4	
		Z	9.87	68.9	21.6		136.2	
10458-AAA	CDMA2000 (1xEV-DO, Rev. B, 2 carriers)	X	7.83	67.4	19.9	6.55	108.2	±1.2 %
		Y	7.69	67.0	19.4		104.5	
		Z	8.11	68.2	20.3		124.3	
10459-AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	X	10.63	69.2	21.7	8.25	130.7	±2.2 %
		Y	10.48	68.9	21.4		123.4	
		Z	10.07	67.8	20.9		101.8	
10515-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)	X	3.51	73.4	21.3	1.58	125.8	±0.5 %
		Y	2.68	68.0	18.5		122.8	
		Z	3.41	72.6	20.8		142.5	
10518-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 99pc duty cycle)	X	9.68	68.0	21.1	8.23	118.9	±1.9 %
		Y	9.42	67.3	20.6		114.1	
		Z	10.04	69.1	21.7		137.4	
10525-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)	X	9.92	68.2	21.3	8.36	120.5	±1.9 %
		Y	9.66	67.6	20.8		116.3	
		Z	10.24	69.2	21.9		139.1	
10526-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 99pc duty cycle)	X	10.00	68.3	21.4	8.42	120.7	±1.9 %
		Y	9.69	67.5	20.8		116.2	
		Z	10.32	69.3	22.0		139.3	
10534-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)	X	10.41	68.7	21.5	8.45	125.5	±2.2 %
		Y	10.06	67.8	20.9		120.8	
		Z	10.78	69.7	22.1		145.9	
10535-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle)	X	10.43	68.7	21.5	8.45	126.5	±2.2 %
		Y	10.08	67.9	20.9		121.2	
		Z	10.78	69.7	22.1		146.0	
10544-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	X	10.74	69.0	21.5	8.47	130.5	±2.2 %
		Y	10.26	67.9	20.8		123.8	
		Z	10.20	67.7	20.8		101.3	
10545-AAB	IEEE 802.11ac WiFi (80MHz, MCS1, 99pc duty cycle)	X	10.83	69.1	21.6	8.55	130.8	±2.2 %
		Y	10.36	68.1	21.0		124.5	
		Z	10.28	67.8	20.9		101.7	
10564-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty cycle)	X	9.76	68.2	21.2	8.25	119.0	±1.9 %
		Y	9.46	67.4	20.7		114.6	
		Z	10.08	69.1	21.8		137.5	
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	3.65	73.3	21.4	1.99	123.5	±0.5 %
		Y	2.71	67.4	18.4		120.2	
		Z	3.53	72.6	21.0		138.6	

Certificate No: EX3-7364_Jan19

Page 13 of 15

EX3DV4- SN:7364

January 23, 2019

10572-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	3.80	74.3	21.8	1.99	122.7	±0.5 %
		Y	2.83	68.4	18.9		120.1	
		Z	3.60	73.2	21.2		138.7	
10575-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	9.84	68.2	21.5	8.59	117.1	±1.9 %
		Y	9.55	67.4	20.9		112.7	
		Z	10.17	69.1	22.0		134.4	
10576-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	X	9.84	68.2	21.5	8.60	116.5	±1.9 %
		Y	9.55	67.4	20.9		112.4	
		Z	10.18	69.2	22.1		134.2	
10583-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	X	9.87	68.3	21.5	8.59	117.1	±1.9 %
		Y	9.55	67.4	20.9		112.6	
		Z	10.18	69.2	22.1		134.3	
10584-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)	X	9.87	68.3	21.5	8.60	116.6	±1.9 %
		Y	9.54	67.4	20.9		112.3	
		Z	10.17	69.2	22.1		134.1	
10591-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	9.98	68.3	21.5	8.63	118.4	±1.9 %
		Y	9.66	67.4	20.9		113.7	
		Z	10.29	69.2	22.1		136.0	
10592-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)	X	10.14	68.4	21.7	8.79	118.6	±2.2 %
		Y	9.83	67.6	21.1		113.8	
		Z	10.49	69.5	22.3		136.9	
10599-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	10.57	68.8	21.8	8.79	124.4	±2.2 %
		Y	10.16	67.8	21.1		118.7	
		Z	10.89	69.7	22.4		143.5	
10600-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle)	X	10.65	68.9	21.9	8.88	123.9	±2.2 %
		Y	10.24	67.9	21.2		118.8	
		Z	10.98	69.9	22.5		143.9	
10607-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle)	X	9.99	68.3	21.5	8.64	118.6	±2.2 %
		Y	9.67	67.4	20.9		113.5	
		Z	10.33	69.3	22.1		136.4	
10608-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle)	X	10.13	68.4	21.7	8.77	118.9	±1.9 %
		Y	9.80	67.6	21.1		113.5	
		Z	10.48	69.5	22.3		137.0	
10616-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	X	10.58	68.8	21.8	8.82	124.5	±2.2 %
		Y	10.21	67.9	21.2		118.8	
		Z	10.94	69.8	22.4		143.9	
10617-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle)	X	10.59	68.8	21.8	8.81	124.8	±2.2 %
		Y	10.21	67.9	21.2		118.9	
		Z	10.93	69.8	22.4		144.1	
10626-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)	X	10.89	69.1	21.8	8.83	128.8	±2.2 %
		Y	10.39	68.0	21.1		121.6	
		Z	11.24	70.1	22.4		149.4	

Certificate No: EX3-7364_Jan19

Page 14 of 15

EX3DV4- SN:7364

January 23, 2019

10627-AAB	IEEE 802.11ac WiFi (80MHz, MCS1, 90pc duty cycle)	X	10.94	69.1	21.9	8.88	129.3	±2.2 %
		Y	10.43	68.0	21.1		121.2	
		Z	11.32	70.2	22.5		149.9	
10648-AAA	CDMA2000 (1x Advanced)	X	3.77	67.8	19.4	3.45	120.1	±0.7 %
		Y	3.51	66.0	18.3		117.6	
		Z	3.94	68.6	19.8		136.8	

[†] Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **EX3-7485_Jan19**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:7485**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v5, QA CAL-23.v5,
QA CAL-25.v7
Calibration procedure for dosimetric E-field probes**

Calibration date: **January 23, 2019**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
DAE4	SN: 660	19-Dec-18 (No. DAE4-660_Dec18)	Dec-19
Reference Probe ES3DV2	SN: 3013	31-Dec-18 (No. ES3-3013_Dec18)	Dec-19
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: January 26, 2019			

Certificate No: EX3-7485_Jan19

Page 1 of 17

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

Certificate No: EX3-7485_Jan19

Page 2 of 17

EX3DV4 – SN:7485

January 23, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7485**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.46	0.45	0.46	$\pm 10.1 \%$
DCP (mV) ^B	100.5	94.4	103.1	

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Max dev.	Unc ^C (k=2)
0	CW	X	0.0	0.0	1.0	0.00	132.5	+ 3.8 %	$\pm 4.7 \%$
		Y	0.0	0.0	1.0		129.0		
		Y	0.0	0.0	1.0		131.8		

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).^B Numerical linearization parameter: uncertainty not required.^C Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:7485

January 23, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7485**Sensor Model Parameters****Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	1.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4- SN:7485

January 23, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7485

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^e	Conductivity (S/m) ^e	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
150	52.3	0.76	14.29	14.29	14.29	0.00	1.00	± 13.3 %
300	45.3	0.87	13.10	13.10	13.10	0.08	1.10	± 13.3 %
450	43.5	0.87	11.95	11.95	11.95	0.13	1.20	± 13.3 %
750	41.9	0.89	10.90	10.90	10.90	0.42	0.89	± 12.0 %
835	41.5	0.90	10.53	10.53	10.53	0.38	0.97	± 12.0 %
900	41.5	0.97	10.26	10.26	10.26	0.33	1.01	± 12.0 %
1450	40.5	1.20	9.56	9.56	9.56	0.40	0.83	± 12.0 %
1810	40.0	1.40	8.95	8.95	8.95	0.35	0.84	± 12.0 %
1900	40.0	1.40	8.70	8.70	8.70	0.32	0.84	± 12.0 %
2100	39.8	1.49	8.80	8.80	8.80	0.31	0.84	± 12.0 %
2300	39.5	1.67	8.21	8.21	8.21	0.29	0.88	± 12.0 %
2450	39.2	1.80	7.84	7.84	7.84	0.36	0.90	± 12.0 %
2600	39.0	1.96	7.64	7.64	7.64	0.39	0.85	± 12.0 %
3500	37.9	2.91	7.36	7.36	7.36	0.25	1.25	± 13.1 %
3700	37.7	3.12	7.03	7.03	7.03	0.24	1.30	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^e At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7485

January 23, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7485

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth ^g (mm)	Unc (k=2)
150	61.9	0.80	13.55	13.55	13.55	0.00	1.00	± 13.3 %
300	58.2	0.92	12.62	12.62	12.62	0.04	1.10	± 13.3 %
450	56.7	0.94	12.52	12.52	12.52	0.08	1.20	± 13.3 %
750	55.5	0.96	10.75	10.75	10.75	0.27	1.13	± 12.0 %
835	55.2	0.97	10.43	10.43	10.43	0.45	0.84	± 12.0 %
900	55.0	1.05	10.32	10.32	10.32	0.31	0.99	± 12.0 %
1450	54.0	1.30	9.01	9.01	9.01	0.29	0.80	± 12.0 %
1810	53.3	1.52	8.47	8.47	8.47	0.37	0.84	± 12.0 %
1900	53.3	1.52	8.23	8.23	8.23	0.28	0.98	± 12.0 %
2100	53.2	1.62	8.41	8.41	8.41	0.29	0.96	± 12.0 %
2300	52.9	1.81	8.10	8.10	8.10	0.39	0.82	± 12.0 %
2450	52.7	1.95	8.09	8.09	8.09	0.21	1.15	± 12.0 %
2600	52.5	2.16	7.88	7.88	7.88	0.25	0.99	± 12.0 %
3500	51.3	3.31	7.11	7.11	7.11	0.25	1.20	± 13.1 %
3700	51.0	3.55	7.06	7.06	7.06	0.23	1.25	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7485

January 23, 2019

Frequency Response of E-Field


(TEM-Cell: ifi110 EXX, Waveguide: R22)

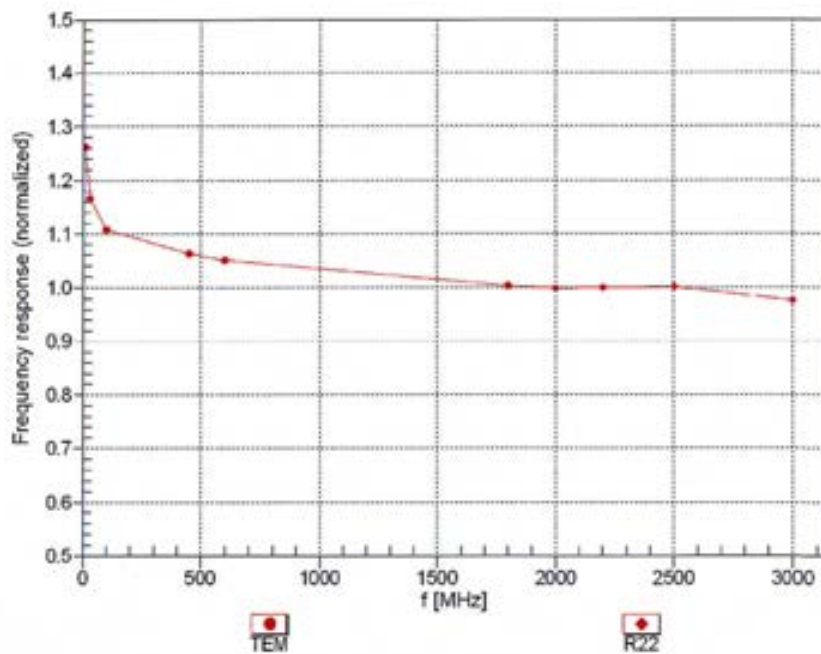

Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4- SN:7485



January 23, 2019

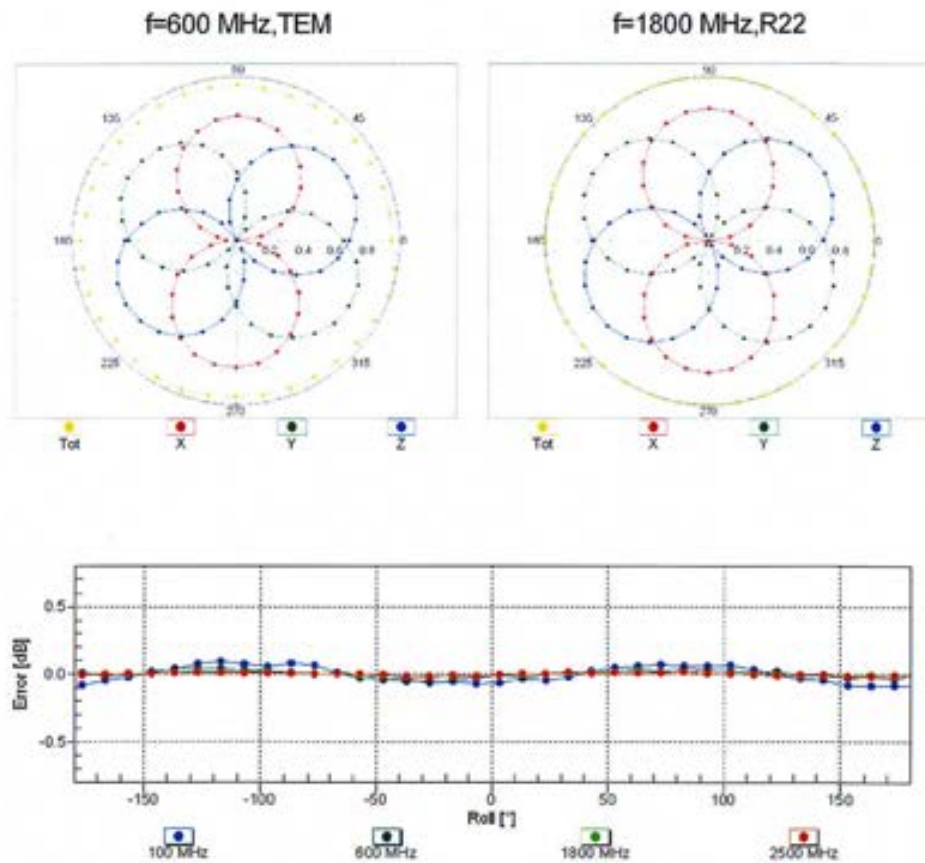Receiving Pattern (ϕ), $\theta = 0^\circ$ **Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)**

EX3DV4- SN:7485

January 23, 2019

Dynamic Range f(SAR_{head})
(TEM cell , f_{eval}= 1900 MHz)

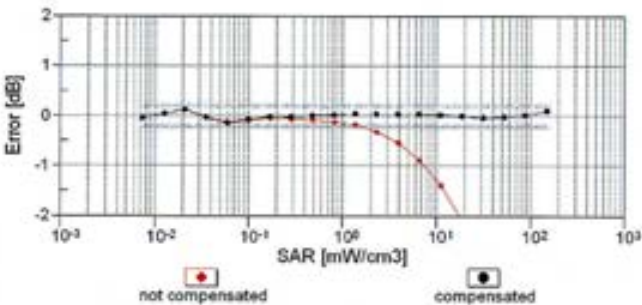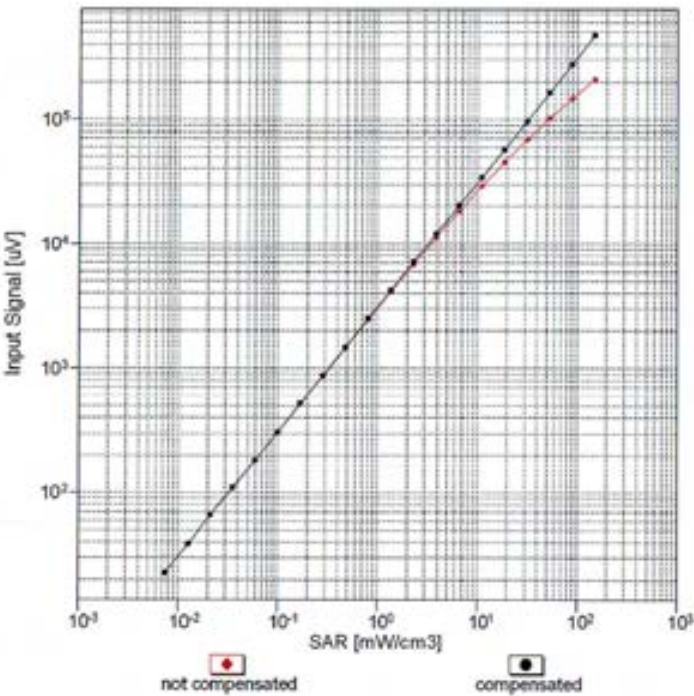


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


EX3DV4- SN:7485

January 23, 2019

Conversion Factor Assessment

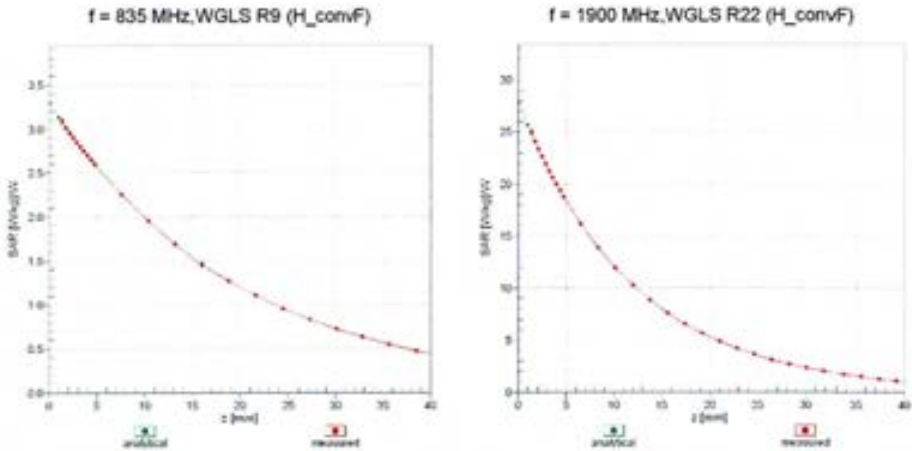

Deviation from Isotropy in Liquid
Error (ϕ , θ), f = 900 MHz

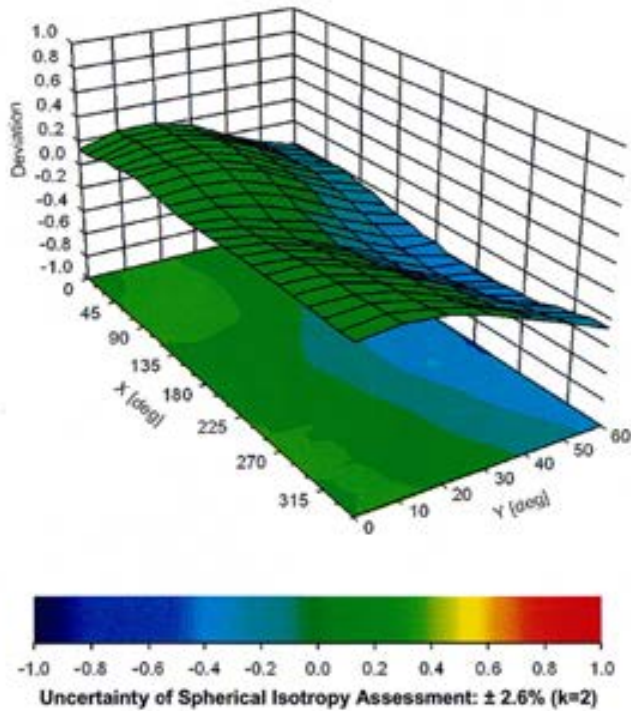

EX3DV4- SN:7485

January 23, 2019

Appendix: Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu V}$	C	D dB	VR mV	Unc ^c (k=2)
0	CW	X	0.0	0.0	1.0	0.00	132.5	$\pm 3.8\%$
		Y	0.0	0.0	1.0		129.0	
		Z	0.0	0.0	1.0		131.8	
10011-CAB	UMTS-FDD (WCDMA)	X	3.27	66.4	17.8	2.91	142.4	$\pm 1.7\%$
		Y	3.02	64.5	16.8		138.7	
		Z	3.61	69.5	20.0		142.8	
10097-CAB	UMTS-FDD (HSDPA)	X	4.42	65.9	17.9	3.98	127.9	$\pm 1.7\%$
		Y	4.26	64.8	17.3		146.5	
		Z	4.62	67.5	19.1		128.2	
10098-CAB	UMTS-FDD (HSPA, Subtest 2)	X	4.42	65.9	18.0	3.98	128.1	$\pm 1.7\%$
		Y	4.29	64.9	17.4		146.2	
		Z	4.62	67.4	19.1		128.2	
10100-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.11	66.2	18.9	5.67	134.3	$\pm 2.2\%$
		Y	5.88	65.2	18.4		129.8	
		Z	6.26	67.2	19.7		134.6	
10101-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	7.24	67.0	19.6	6.42	142.9	$\pm 2.2\%$
		Y	7.02	66.2	19.2		137.8	
		Z	7.31	67.5	20.1		143.9	
10106-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.03	66.1	19.0	5.80	131.6	$\pm 1.7\%$
		Y	6.09	66.3	19.2		149.4	
		Z	6.12	66.9	19.7		132.1	
10109-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	6.99	66.9	19.6	6.43	138.2	$\pm 2.5\%$
		Y	6.85	66.3	19.4		133.8	
		Z	7.07	67.4	20.1		136.7	
10110-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	5.71	65.7	18.8	5.75	127.7	$\pm 2.5\%$
		Y	5.77	65.8	19.0		145.1	
		Z	5.84	66.7	19.6		128.5	
10111-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	6.73	66.8	19.6	6.44	133.1	$\pm 1.9\%$
		Y	6.57	66.0	19.2		129.1	
		Z	6.81	67.4	20.2		133.7	
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	9.93	68.4	21.0	8.07	144.8	$\pm 3.0\%$
		Y	9.73	67.9	20.8		138.9	
		Z	9.98	68.7	21.3		145.4	
10140-CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	7.42	67.2	19.8	6.49	144.3	$\pm 2.2\%$
		Y	7.18	66.4	19.4		139.1	
		Z	7.48	67.7	20.3		144.7	
10142-CAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	5.74	66.5	19.3	5.73	147.7	$\pm 1.9\%$
		Y	5.58	65.6	18.9		142.1	
		Z	5.83	67.3	20.0		148.4	
10143-CAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	6.43	66.7	19.5	6.35	128.7	$\pm 2.2\%$
		Y	6.51	66.8	19.6		148.1	
		Z	6.55	67.5	20.1		130.0	
10145-CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	5.52	66.7	19.4	5.76	142.0	$\pm 1.9\%$

Certificate No: EX3-7485_Jan19

Page 11 of 17

EX3DV4- SN:7485

January 23, 2019

		Y	5.39	65.9	19.0		137.0	
		Z	5.58	67.3	20.0		143.0	
10146-CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	6.37	67.9	20.1	6.41	144.3	±2.2 %
		Y	6.29	67.4	20.0		140.4	
		Z	6.47	68.5	20.7		145.8	
10149-CAE	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	6.99	66.8	19.6	6.42	138.3	±1.9 %
		Y	6.83	66.2	19.3		133.5	
		Z	7.05	67.4	20.1		138.4	
10154-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	5.73	65.8	18.9	5.75	127.6	±2.2 %
		Y	5.79	65.9	19.0		145.4	
		Z	5.82	66.6	19.6		128.0	
10155-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	6.70	66.7	19.5	6.43	132.8	±2.2 %
		Y	6.60	66.2	19.4		129.3	
		Z	6.81	67.4	20.2		133.7	
10156-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	5.71	66.5	19.3	5.79	146.3	±2.2 %
		Y	5.57	65.7	19.0		140.8	
		Z	5.76	67.1	19.9		146.6	
10157-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	6.43	66.8	19.6	6.49	127.0	±1.9 %
		Y	6.56	67.1	19.9		145.4	
		Z	6.54	67.5	20.3		127.6	
10160-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.14	66.3	19.1	5.82	132.4	±1.9 %
		Y	6.03	65.8	18.9		128.5	
		Z	6.23	67.0	19.7		133.1	
10161-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	7.01	66.9	19.6	6.43	138.3	±1.9 %
		Y	6.86	66.3	19.4		133.4	
		Z	7.11	67.6	20.2		138.1	
10166-CAF	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	4.95	66.6	19.3	5.46	136.3	±1.9 %
		Y	4.87	65.9	19.0		132.2	
		Z	5.07	67.5	20.1		136.7	
10167-CAF	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	5.72	67.5	20.0	6.21	136.4	±2.2 %
		Y	5.66	67.0	19.8		132.4	
		Z	5.93	68.7	20.9		137.5	
10169-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.75	66.3	19.4	5.73	130.0	±1.7 %
		Y	4.89	66.6	19.6		148.6	
		Z	4.88	67.5	20.3		130.7	
10170-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	5.56	68.0	20.6	6.52	149.7	±2.2 %
		Y	5.49	67.3	20.3		146.3	
		Z	5.48	68.0	20.9		128.0	
10175-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4.74	66.3	19.3	5.72	129.5	±1.9 %
		Y	4.88	66.6	19.6		148.5	
		Z	4.89	67.5	20.4		130.4	
10176-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	5.56	68.0	20.6	6.52	149.7	±2.2 %
		Y	5.47	67.2	20.2		146.3	
		Z	5.47	68.0	20.9		127.7	

Certificate No: EX3-7485_Jan19

Page 12 of 17

EX3DV4- SN:7485

January 23, 2019

10177-CAI	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	4.76	66.4	19.4	5.73	130.1	±1.9 %
		Y	4.88	66.6	19.6		147.9	
		Z	4.91	67.6	20.4		130.5	
10178-CAG	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	5.55	68.0	20.6	6.52	149.9	±2.2 %
		Y	5.49	67.2	20.2		146.3	
		Z	5.52	68.2	21.0		127.7	
10181-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	4.77	66.4	19.4	5.72	130.0	±1.9 %
		Y	4.88	66.6	19.6		148.3	
		Z	4.92	67.7	20.4		130.7	
10182-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	5.56	68.0	20.6	6.52	149.6	±2.2 %
		Y	5.51	67.4	20.4		146.1	
		Z	5.49	68.1	20.9		127.7	
10184-CAE	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	4.77	66.4	19.4	5.73	129.7	±2.2 %
		Y	4.88	66.6	19.6		148.3	
		Z	4.89	67.5	20.4		130.2	
10185-CAE	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	5.58	68.1	20.7	6.51	149.8	±2.2 %
		Y	5.49	67.3	20.3		146.4	
		Z	5.46	68.0	20.9		127.4	
10187-CAF	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	4.76	66.4	19.4	5.73	129.5	±1.9 %
		Y	4.87	66.4	19.5		148.5	
		Z	4.91	67.6	20.4		130.3	
10188-CAF	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	5.57	68.0	20.6	6.52	149.6	±2.2 %
		Y	5.48	67.2	20.2		146.6	
		Z	5.49	68.1	21.0		127.7	
10196-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.55	68.3	21.1	8.10	137.2	±2.7 %
		Y	9.39	67.9	20.9		131.6	
		Z	9.60	68.6	21.4		138.2	
10225-CAB	UMTS-FDD (HSPA+)	X	6.77	67.0	19.4	5.97	138.3	±2.2 %
		Y	6.67	66.6	19.2		134.5	
		Z	6.89	67.7	20.0		138.6	
10274-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	X	5.75	66.7	18.7	4.87	135.3	±0.9 %
		Y	5.54	65.6	18.2		131.4	
		Z	5.92	67.7	19.4		136.5	
10275-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	4.40	66.6	18.5	3.96	145.9	±0.9 %
		Y	4.23	65.6	18.0		140.7	
		Z	4.57	68.1	19.6		145.8	
10297-AAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	6.08	66.3	19.2	5.81	130.5	±1.7 %
		Y	6.25	67.2	19.9		146.9	
		Z	6.19	67.2	19.9		130.9	
10298-AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	5.57	66.7	19.4	5.72	143.9	±1.9 %
		Y	5.54	66.5	19.4		138.4	
		Z	5.70	67.7	20.2		144.4	
10299-AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	6.50	68.0	20.2	6.39	147.5	±1.9 %
		Y	6.41	67.5	20.1		142.6	
		Z	6.60	68.6	20.8		148.1	

Certificate No: EX3-7485_Jan19

Page 13 of 17

EX3DV4- SN:7485

January 23, 2019

10311-AAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.60	66.7	19.4	6.06	136.5	±1.9 %
		Y	6.48	66.3	19.3		131.5	
		Z	6.67	67.4	20.0		136.0	
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.93	69.1	18.6	1.54	146.6	±1.7 %
		Y	2.73	67.8	18.0		141.9	
		Z	3.99	76.8	22.9		146.2	
10416-AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	X	9.64	68.3	21.1	8.23	137.7	±2.7 %
		Y	9.44	67.8	20.9		131.7	
		Z	9.69	68.7	21.5		138.3	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	9.50	68.2	21.1	8.14	136.1	±2.7 %
		Y	9.32	67.7	20.8		130.9	
		Z	9.55	68.5	21.4		136.7	
10435-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.59	69.0	22.2	7.82	149.8	±2.5 %
		Y	5.34	67.4	21.4		142.3	
		Z	5.47	68.8	22.3		129.6	
10457-AAA	UMTS-FDD (DC-HSDPA)	X	8.03	66.7	19.5	6.62	134.0	±2.2 %
		Y	7.91	66.3	19.3		129.2	
		Z	8.08	67.1	19.9		134.2	
10460-AAA	UMTS-FDD (WCDMA, AMR)	X	3.07	68.6	18.9	2.39	139.3	±1.7 %
		Y	2.84	67.0	18.1		135.5	
		Z	3.70	73.8	22.0		139.1	
10461-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.42	68.1	21.7	7.82	128.9	±1.7 %
		Y	5.36	67.5	21.5		141.9	
		Z	5.50	68.9	22.3		129.2	
10462-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.02	69.9	22.7	8.30	146.8	±1.9 %
		Y	5.73	68.1	21.9		139.1	
		Z	6.08	70.5	23.4		146.9	
10464-AAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.59	69.0	22.1	7.82	149.3	±1.9 %
		Y	5.30	67.1	21.1		142.3	
		Z	5.66	69.7	22.8		150.0	
10465-AAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.01	69.7	22.7	8.32	146.1	±1.9 %
		Y	5.73	67.9	21.8		139.2	
		Z	6.14	70.6	23.4		147.9	
10467-AAE	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.57	68.9	22.1	7.82	149.2	±1.9 %
		Y	5.30	67.1	21.1		142.1	
		Z	5.46	68.7	22.2		128.9	
10468-AAE	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.02	69.8	22.7	8.32	146.5	±1.9 %
		Y	5.72	67.9	21.7		139.4	
		Z	6.13	70.6	23.4		147.0	
10470-AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.57	68.9	22.1	7.82	149.1	±2.2 %
		Y	5.31	67.2	21.1		142.3	
		Z	5.45	68.7	22.2		128.8	

Certificate No: EX3-7485_Jan19

Page 14 of 17

EX3DV4- SN:7485

January 23, 2019

10471-AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.01	69.7	22.7	8.32	146.6	±1.9 %
		Y	5.71	67.9	21.7		139.6	
		Z	6.11	70.6	23.4		147.5	
10473-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.58	69.0	22.1	7.82	149.2	±2.5 %
		Y	5.30	67.1	21.1		142.7	
		Z	5.47	68.8	22.3		128.8	
10474-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.02	69.8	22.8	8.32	146.4	±2.5 %
		Y	5.71	67.9	21.7		139.4	
		Z	6.10	70.5	23.3		147.8	
10477-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.00	69.7	22.7	8.32	146.7	±2.5 %
		Y	5.71	67.8	21.6		139.8	
		Z	6.11	70.6	23.4		147.7	
10479-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.69	67.7	21.3	7.74	134.3	±2.2 %
		Y	5.57	66.9	20.9		149.5	
		Z	5.72	68.2	21.8		134.7	
10480-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.31	69.0	22.0	8.18	135.9	±2.2 %
		Y	6.13	67.9	21.5		149.8	
		Z	6.38	69.5	22.6		136.7	
10482-AAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.09	67.7	21.2	7.71	141.8	±2.5 %
		Y	5.76	66.0	20.3		135.6	
		Z	6.11	68.1	21.7		142.5	
10483-AAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.06	69.0	22.1	8.39	147.0	±2.7 %
		Y	6.68	67.2	21.1		139.8	
		Z	7.10	69.3	22.5		147.6	
10485-AAE	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.05	67.4	21.0	7.59	144.1	±2.2 %
		Y	5.75	65.9	20.2		137.6	
		Z	6.09	67.9	21.5		144.7	
10486-AAE	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.99	67.9	21.5	8.38	128.4	±2.2 %
		Y	6.84	67.2	21.2		143.1	
		Z	7.05	68.4	22.0		129.3	
10488-AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.27	66.8	20.7	7.70	127.9	±2.7 %
		Y	6.10	66.0	20.3		142.8	
		Z	6.33	67.4	21.3		128.7	
10489-AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.25	67.7	21.3	8.31	135.3	±2.5 %
		Y	7.07	67.0	21.0		149.8	
		Z	7.29	68.2	21.8		135.8	
10491-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.65	67.2	20.8	7.74	133.4	±2.5 %
		Y	6.43	66.3	20.4		147.9	
		Z	6.71	67.8	21.4		133.7	
10492-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.72	68.0	21.5	8.41	141.6	±2.7 %
		Y	7.35	66.6	20.8		134.4	
		Z	7.74	68.4	21.9		141.9	
10494-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.63	67.2	20.9	7.74	132.7	±2.7 %
		Y	6.39	66.3	20.4		147.1	
		Z	6.67	67.8	21.4		133.2	

Certificate No: EX3-7485_Jan19

Page 15 of 17

EX3DV4- SN:7485

January 23, 2019

10495-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.65	67.9	21.5	8.37	141.2	±2.5 %
		Y	7.27	66.5	20.7		134.2	
		Z	7.66	68.2	21.8		141.8	
10497-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.00	67.8	21.2	7.67	141.2	±2.5 %
		Y	5.69	66.2	20.3		134.7	
		Z	6.05	68.4	21.8		141.5	
10498-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	6.95	69.1	22.1	8.40	144.1	±1.9 %
		Y	6.61	67.4	21.2		137.4	
		Z	6.99	69.4	22.5		145.3	
10500-AAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.24	67.5	21.1	7.67	146.1	±2.2 %
		Y	5.92	65.9	20.2		139.9	
		Z	6.29	68.1	21.7		146.9	
10501-AAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.18	68.0	21.6	8.44	130.5	±2.7 %
		Y	6.98	67.1	21.1		145.4	
		Z	7.22	68.4	22.0		131.6	
10503-AAE	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.29	66.9	20.7	7.72	128.0	±2.7 %
		Y	6.10	66.0	20.3		142.7	
		Z	6.35	67.4	21.3		129.0	
10504-AAE	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.27	67.8	21.4	8.31	135.4	±1.9 %
		Y	7.06	66.9	21.0		150.0	
		Z	7.32	68.2	21.8		136.2	
10506-AAE	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.63	67.2	20.9	7.74	132.8	±2.5 %
		Y	6.42	66.4	20.5		147.8	
		Z	6.67	67.8	21.4		133.2	
10507-AAE	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	7.65	67.9	21.4	8.36	141.2	±2.5 %
		Y	7.28	66.6	20.8		133.9	
		Z	7.67	68.3	21.8		141.9	
10509-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.25	67.8	21.2	7.99	138.9	±2.5 %
		Y	6.82	66.2	20.4		131.6	
		Z	7.29	68.3	21.7		139.1	
10510-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.17	68.3	21.7	8.49	148.7	±2.5 %
		Y	7.71	66.7	20.9		136.9	
		Z	8.16	68.6	22.0		147.6	
10512-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.97	67.7	21.0	7.74	137.5	±2.2 %
		Y	6.56	66.2	20.3		130.3	
		Z	7.01	68.3	21.5		137.7	
10513-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	8.02	68.1	21.6	8.42	146.5	±2.5 %
		Y	7.60	66.7	20.9		137.7	
		Z	8.03	68.4	21.9		146.8	
10515-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)	X	3.03	69.9	19.0	1.58	146.0	±1.4 %
		Y	2.57	66.6	17.3		140.8	
		Z	4.02	77.1	23.0		145.7	

Certificate No: EX3-7485_Jan19

Page 16 of 17

EX3DV4- SN:7485

January 23, 2019

10564-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	X	9.64	68.3	21.1	8.25	137.0	±2.7 %
		Y	9.51	68.0	21.0		131.9	
		Z	9.72	68.7	21.5		138.2	
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	3.10	69.6	19.1	1.99	142.2	±1.9 %
		Y	2.67	66.9	17.8		137.5	
		Z	4.15	76.9	23.0		142.1	
10572-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	3.11	69.9	19.2	1.99	141.9	±1.7 %
		Y	2.68	67.0	17.8		137.4	
		Z	4.00	76.4	22.8		141.9	
10575-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	9.73	68.3	21.4	8.59	134.3	±3.0 %
		Y	9.58	67.9	21.2		128.5	
		Z	9.80	68.7	21.7		135.7	
10576-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	X	9.73	68.4	21.4	8.60	134.1	±3.0 %
		Y	9.53	67.8	21.2		128.1	
		Z	9.81	68.8	21.8		135.2	
10591-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	9.86	68.4	21.5	8.63	136.2	±3.0 %
		Y	9.66	67.8	21.2		130.3	
		Z	9.93	68.7	21.8		137.4	
10592-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)	X	10.04	68.6	21.7	8.79	136.6	±3.0 %
		Y	9.83	68.1	21.4		130.4	
		Z	10.09	68.9	21.9		137.9	
10599-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	10.50	69.0	21.7	8.79	144.3	±3.0 %
		Y	10.20	68.3	21.4		135.9	
		Z	10.52	69.2	22.0		144.8	
10600-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle)	X	10.58	69.1	21.9	8.88	144.7	±3.0 %
		Y	10.29	68.4	21.5		136.9	
		Z	10.61	69.3	22.1		145.0	

* Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **EX3-7533_Nov19**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:7533**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v5, QA CAL-23.v5,
 QA CAL-25.v7
 Calibration procedure for dosimetric E-field probes**

Calibration date: **November 6, 2019**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-19 (No. 217-02894)	Apr-20
DAE4	SN: 660	07-Oct-19 (No. DAE4-660_Oct19)	Oct-20
Reference Probe ES3DV2	SN: 3013	31-Dec-18 (No. ES3-3013_Dec18)	Dec-19
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-18 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	06-Apr-18 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-18 (in house check Jun-18)	In house check: Jun-20
RF generator HP 6648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-19)	In house check: Oct-20

	Name	Function	Signature
Calibrated by:	Jeton Kastati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
Issued: November 8, 2019			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: EX3-7533_Nov19

Page 1 of 12

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
 Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E^2 -field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 – SN:7533

November 6, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7533**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.42	0.47	0.41	± 10.1 %
DCP (mV) ^B	96.5	99.1	103.6	

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Max dev.	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	145.2	±3.8 %	±4.7 %
		Y	0.0	0.0	1.0		159.8		
		Z	0.0	0.0	1.0		148.5		

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).^B Numerical linearization parameter: uncertainty not required.^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4-- SN:7533

November 6, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7533**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	88.9
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4- SN:7533

November 6, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7533

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth (mm) ^g	Unc (k=2)
150	52.3	0.76	13.81	13.81	13.81	0.00	1.00	± 13.3 %
300	45.3	0.87	12.94	12.94	12.94	0.08	1.20	± 13.3 %
450	43.5	0.87	11.84	11.84	11.84	0.12	1.30	± 13.3 %
750	41.9	0.89	10.71	10.71	10.71	0.38	0.93	± 12.0 %
835	41.5	0.90	10.47	10.47	10.47	0.46	0.86	± 12.0 %
900	41.5	0.97	10.25	10.25	10.25	0.31	1.01	± 12.0 %
2450	39.2	1.80	7.67	7.67	7.67	0.32	0.92	± 12.0 %
5250	35.9	4.71	5.35	5.35	5.35	0.40	1.80	± 13.1 %
5500	35.6	4.96	4.89	4.89	4.89	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.74	4.74	4.74	0.40	1.80	± 13.1 %
5750	35.4	5.22	4.90	4.90	4.90	0.40	1.80	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7533

November 6, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7533

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k=2)
150	61.9	0.80	13.50	13.50	13.50	0.00	1.00	± 13.3 %
300	58.2	0.92	12.69	12.69	12.69	0.03	1.20	± 13.3 %
450	56.7	0.94	12.06	12.06	12.06	0.06	1.30	± 13.3 %
750	55.5	0.96	10.58	10.58	10.58	0.44	0.86	± 12.0 %
835	55.2	0.97	10.23	10.23	10.23	0.45	0.80	± 12.0 %
900	55.0	1.05	9.95	9.95	9.95	0.50	0.80	± 12.0 %
2450	52.7	1.95	7.79	7.79	7.79	0.35	0.92	± 12.0 %
5250	48.9	5.36	4.80	4.80	4.80	0.50	1.90	± 13.1 %
5500	48.6	5.65	4.22	4.22	4.22	0.50	1.90	± 13.1 %
5600	48.5	5.77	4.10	4.10	4.10	0.50	1.90	± 13.1 %
5750	48.3	5.94	4.23	4.23	4.23	0.50	1.90	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7533

November 6, 2019

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

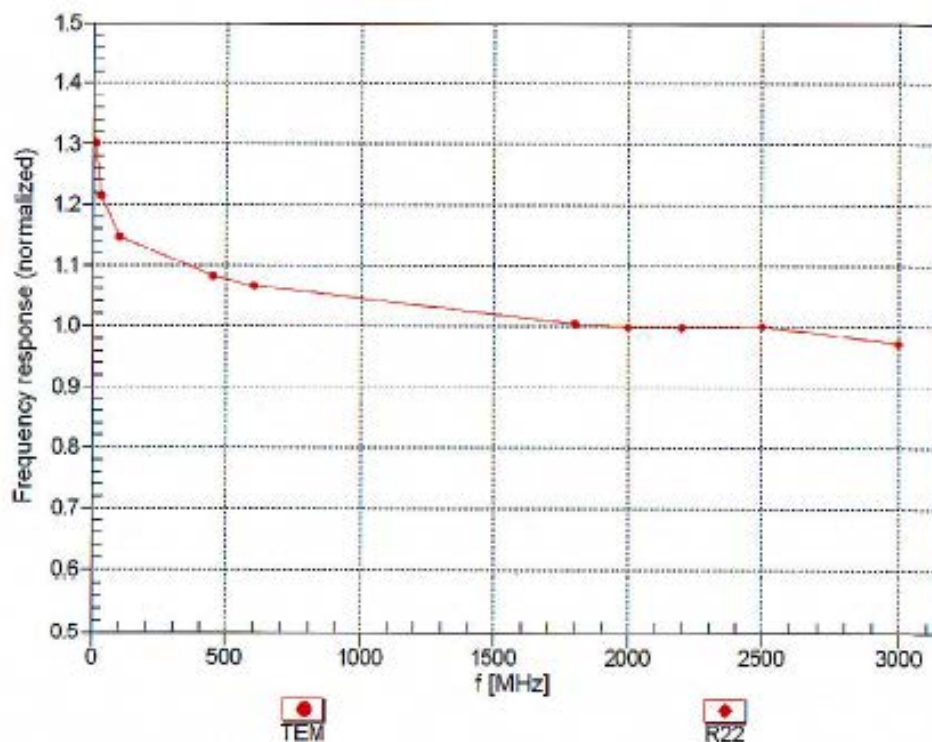


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4- SN:7533

November 6, 2019

Receiving Pattern (ϕ), $\theta = 0^\circ$


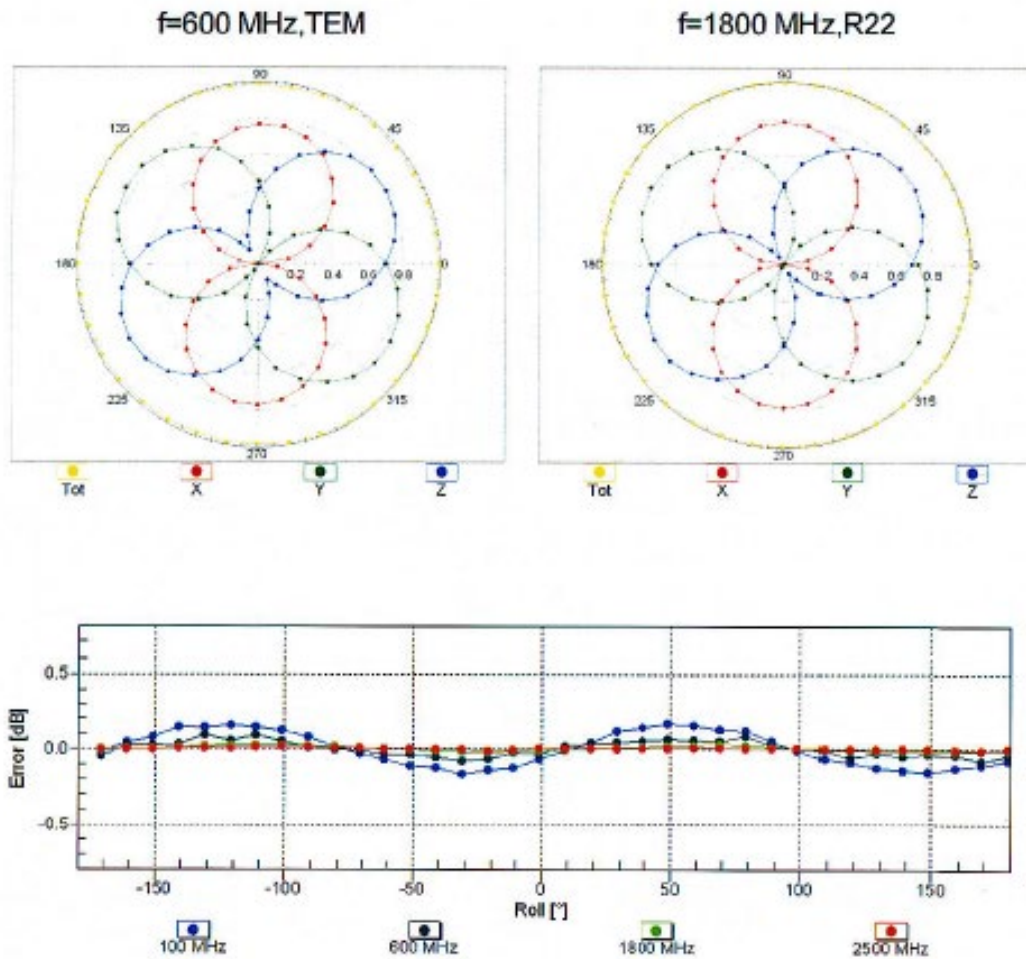


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

EX3DV4- SN:7533

November 6, 2019


Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f_{\text{eval}} = 1900 \text{ MHz}$)

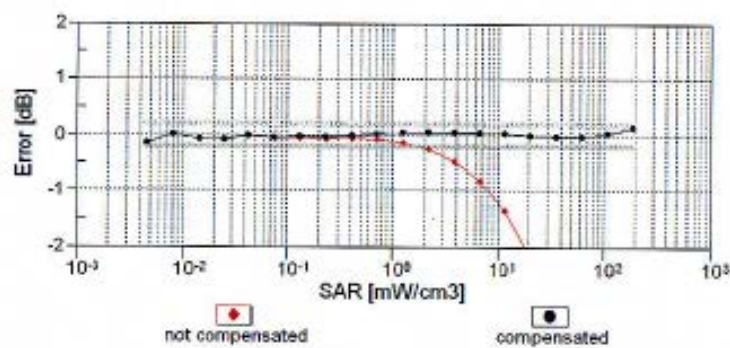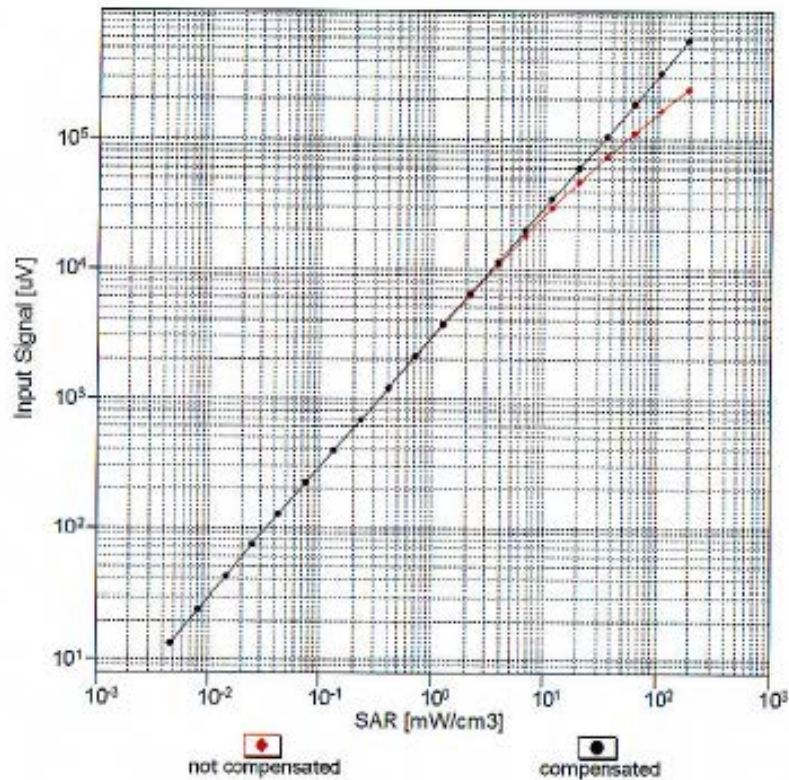Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)


EX3DV4- SN:7533

November 6, 2019

Conversion Factor Assessment

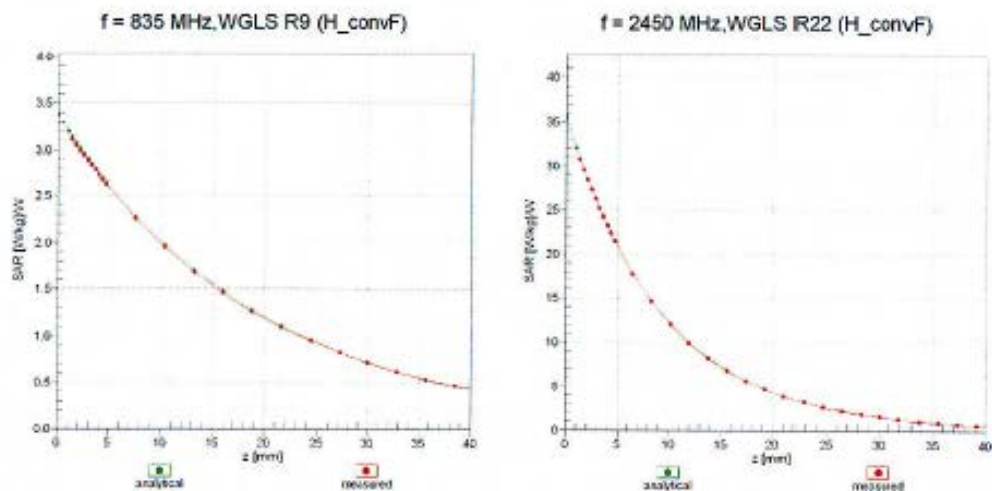

Deviation from Isotropy in Liquid
Error (ϕ, ϑ), $f = 900 \text{ MHz}$

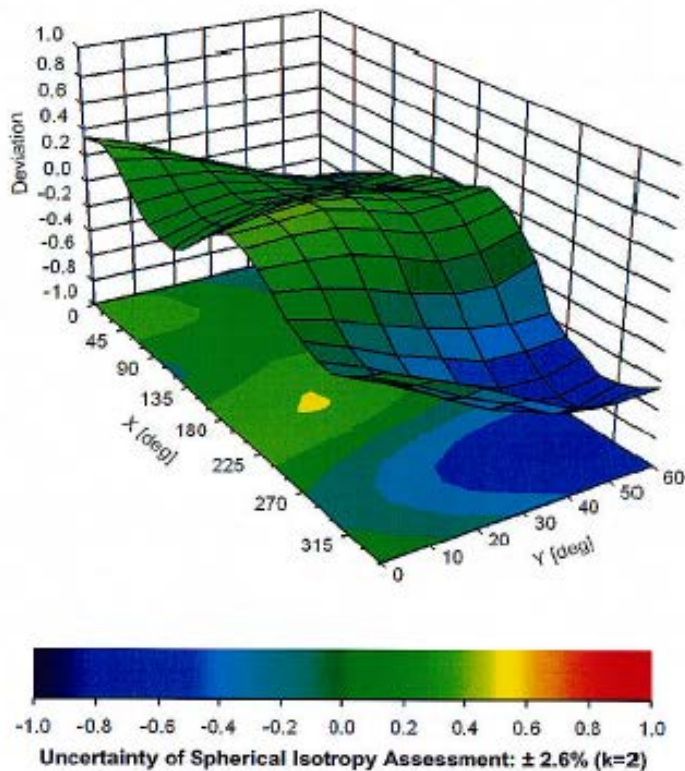

EX3DV4-- SN:7533

November 6, 2019

Appendix: Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu V}$	C	D dB	VR mV	Max dev.	Unc ^e (k=2)
0	CW	X	0.0	0.0	1.0	0.00	145.2	±3.8 %	± 4.7 %
		Y	0.0	0.0	1.0		159.8		
		Z	0.0	0.0	1.0		148.5		
10117- CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	9.83	67.8	20.7	8.07	135.6	±3.0 %	± 4.7 %
		Y	9.76	68.0	20.8		149.2		
		Z	9.86	68.3	21.0		139.0		
10196- CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.44	67.6	20.6	8.10	129.3	±2.7 %	± 4.7 %
		Y	9.40	67.9	20.8		141.8		
		Z	9.49	68.2	21.0		132.6		
10415- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.53	65.8	16.9	1.54	136.9	±0.5 %	± 4.7 %
		Y	2.47	66.8	17.8		149.8		
		Z	3.39	72.8	20.7		140.5		
10417- AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	X	9.51	67.6	20.7	8.23	127.8	±2.5 %	± 4.7 %
		Y	9.49	67.9	20.9		141.8		
		Z	9.56	68.1	21.0		131.6		
10525- AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)	X	9.74	67.8	20.9	8.36	130.1	±2.7 %	± 4.7 %
		Y	9.69	68.1	21.1		143.5		
		Z	9.78	68.3	21.2		133.9		
10534- AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)	X	10.28	68.3	21.1	8.45	137.0	±3.0 %	± 4.7 %
		Y	9.85	67.6	20.7		124.3		
		Z	10.31	68.7	21.4		140.8		
10544- AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	X	10.60	68.5	21.1	8.47	142.9	±3.3 %	± 4.7 %
		Y	10.09	67.7	20.7		128.7		
		Z	10.63	69.0	21.4		147.0		
10571- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	2.60	65.8	17.0	1.99	132.6	±0.7 %	± 4.7 %
		Y	2.58	67.1	18.2		144.9		
		Z	3.64	73.7	21.4		136.4		
10583- AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	X	9.64	67.7	21.0	8.59	125.3	±2.5 %	± 4.7 %
		Y	9.55	67.8	21.1		136.8		
		Z	9.65	68.1	21.3		128.7		
10591- AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	9.75	67.7	21.0	8.63	126.7	±2.7 %	± 4.7 %
		Y	9.69	67.9	21.2		139.7		
		Z	9.82	68.3	21.4		131.0		
10599- AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	10.38	68.3	21.4	8.79	134.2	±3.3 %	± 4.7 %
		Y	10.24	68.4	21.4		146.7		
		Z	10.37	68.6	21.6		137.3		

EX3DV4- SN:7533

November 6, 2019

10607-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle)	X	9.78	67.8	21.1	8.64	126.9	±3.3 %	± 4.7 %
		Y	9.69	67.9	21.2		138.6		
		Z	9.83	68.3	21.4		131.1		
10616-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	X	10.41	68.3	21.4	8.82	134.4	±3.3 %	± 4.7 %
		Y	10.26	68.4	21.4		146.8		
		Z	10.43	68.8	21.6		138.7		
10626-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)	X	10.71	68.5	21.4	8.83	138.9	±3.5 %	± 4.7 %
		Y	10.17	67.6	20.8		125.5		
		Z	10.74	69.0	21.6		143.7		

² Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **Motorola Solutions MY**

Certificate No: **EX3-7486_Oct19**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:7486**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v5, QA CAL-23.v5,
QA CAL-25.v7
Calibration procedure for dosimetric E-field probes**

Calibration date: **October 24, 2019**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-19 (No. 217-02894)	Apr-20
DAE4	SN: 660	07-Oct-19 (No. DAE4-660_Oct19)	Oct-20
Reference Probe ES3DV2	SN: 3013	31-Dec-18 (No. ES3-3013_Dec18)	Dec-19
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41496067	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: October 24, 2019			

Certificate No: EX3-7486_Oct19

Page 1 of 14

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E^2 -field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 – SN:7486

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7486**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.37	0.47	0.48	$\pm 10.1 \%$
DCP (mV) ^B	105.6	93.2	97.9	

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Max dev.	Unc ^C (k=2)
0	CW	X	0.0	0.0	1.0	0.00	137.7	$\pm 3.8 \%$	$\pm 4.7 \%$
		Y	0.0	0.0	1.0		152.0		
		Z	0.0	0.0	1.0		161.5		

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).^B Numerical linearization parameter: uncertainty not required.^C Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:7486

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7486**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	19.4
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4-- SN:7486

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7486

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth (mm) ^g	Unc (k=2)
150	52.3	0.76	13.49	13.49	13.49	0.00	1.00	± 13.3 %
300	45.3	0.87	12.20	12.20	12.20	0.07	1.20	± 13.3 %
450	43.5	0.87	11.40	11.40	11.40	0.10	1.30	± 13.3 %
750	41.9	0.89	10.68	10.68	10.68	0.34	1.06	± 12.0 %
835	41.5	0.90	10.46	10.46	10.46	0.45	0.85	± 12.0 %
900	41.5	0.97	10.31	10.31	10.31	0.32	1.00	± 12.0 %
1810	40.0	1.40	8.50	8.50	8.50	0.31	0.87	± 12.0 %
1900	40.0	1.40	8.46	8.46	8.46	0.34	0.87	± 12.0 %
2100	39.8	1.49	8.36	8.36	8.36	0.34	0.87	± 12.0 %
2450	39.2	1.80	7.59	7.59	7.59	0.34	0.90	± 12.0 %
5250	35.9	4.71	5.60	5.60	5.60	0.40	1.80	± 13.1 %
5500	35.6	4.96	5.07	5.07	5.07	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.85	4.85	4.85	0.40	1.80	± 13.1 %
5750	35.4	5.22	5.02	5.02	5.02	0.40	1.80	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7486

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7486

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth (mm) ^g	Unc (k=2)
150	61.9	0.80	13.04	13.04	13.04	0.00	1.00	± 13.3 %
300	58.2	0.92	11.99	11.99	11.99	0.04	1.20	± 13.3 %
450	56.7	0.94	11.73	11.73	11.73	0.08	1.30	± 13.3 %
750	55.5	0.96	10.49	10.49	10.49	0.25	1.08	± 12.0 %
835	55.2	0.97	10.28	10.28	10.28	0.32	0.94	± 12.0 %
900	55.0	1.05	10.03	10.03	10.03	0.26	1.01	± 12.0 %
1810	53.3	1.52	8.48	8.48	8.48	0.36	0.87	± 12.0 %
1900	53.3	1.52	8.37	8.37	8.37	0.38	0.87	± 12.0 %
2100	53.2	1.62	8.34	8.34	8.34	0.34	0.87	± 12.0 %
2450	52.7	1.95	7.67	7.67	7.67	0.37	0.90	± 12.0 %
5250	48.9	5.36	4.72	4.72	4.72	0.50	1.90	± 13.1 %
5500	48.6	5.65	4.28	4.28	4.28	0.50	1.90	± 13.1 %
5600	48.5	5.77	4.12	4.12	4.12	0.50	1.90	± 13.1 %
5750	48.3	5.94	4.26	4.26	4.26	0.50	1.90	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7486

October 24, 2019



Frequency Response of E-Field
(TEM-Cell:ifi110 EXX, Waveguide: R22)

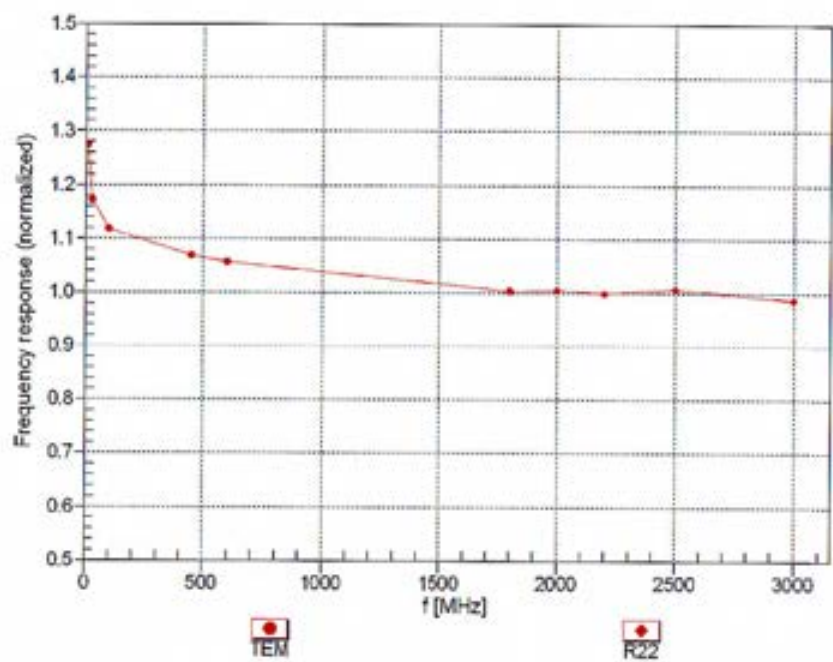

Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4-SN:7486



October 24, 2019

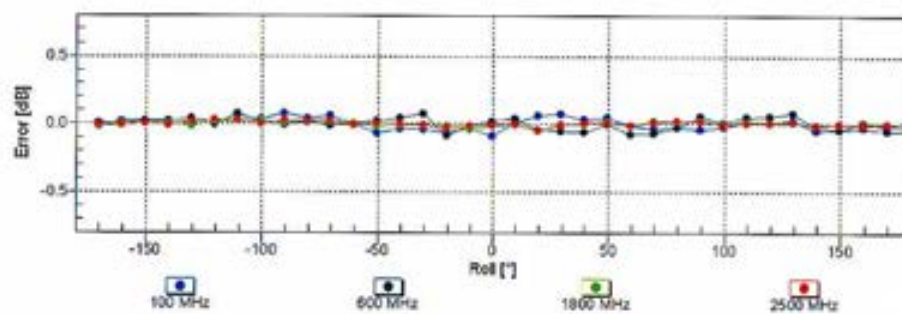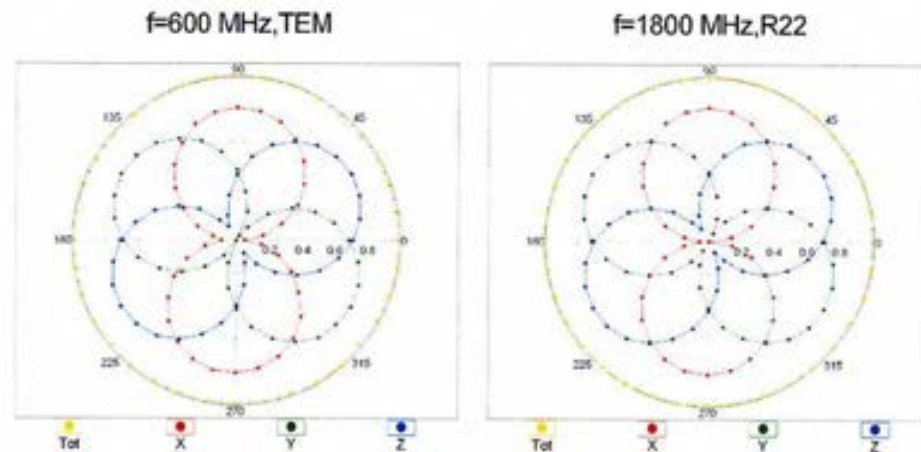Receiving Pattern (ϕ), $\theta = 0^\circ$ **Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)**

EX3DV4- SN:7486

October 24, 2019

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f_{\text{eval}} = 1900 \text{ MHz}$)

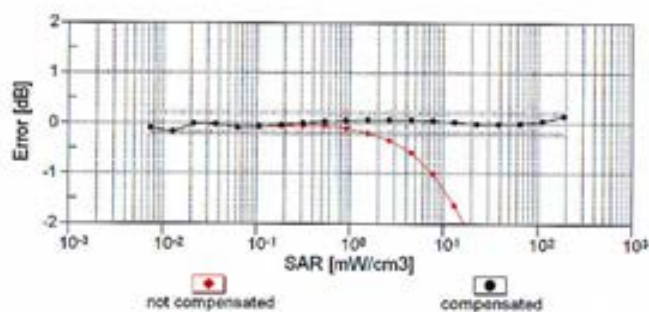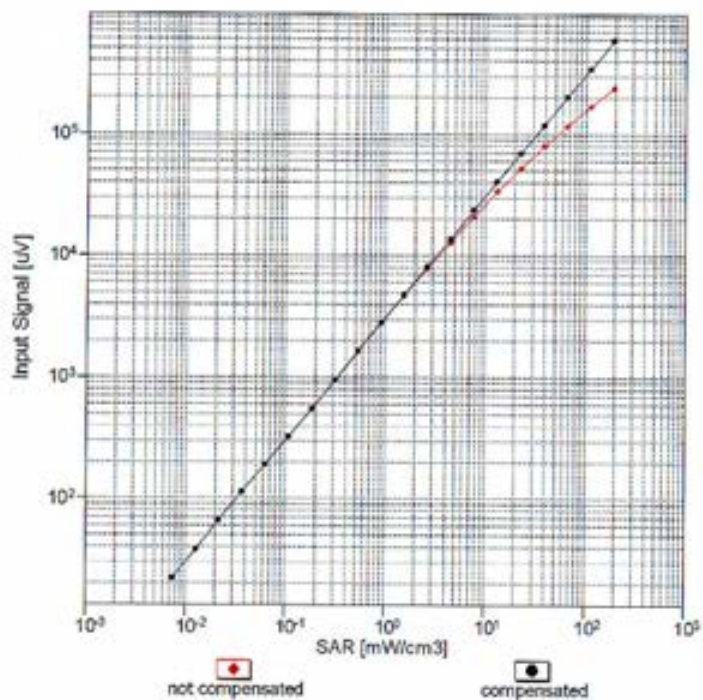


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)


EX3DV4- SN:7486

October 24, 2019

Conversion Factor Assessment

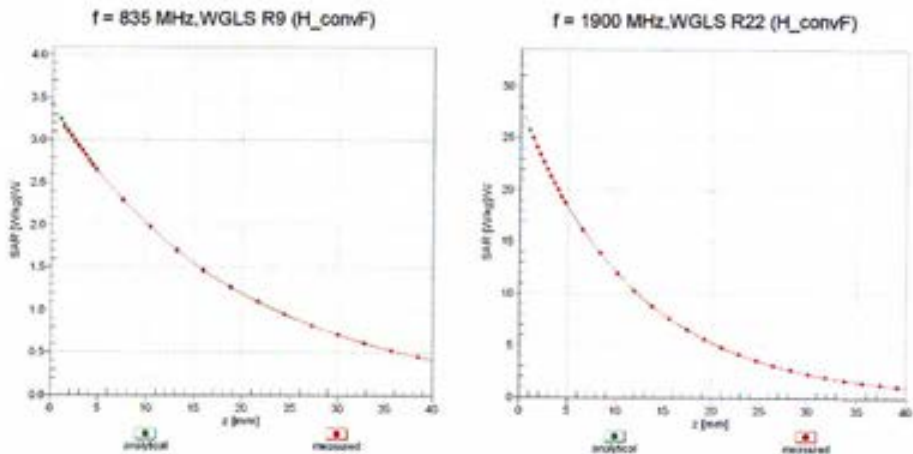

Deviation from Isotropy in Liquid
Error (ϕ, θ), $f = 900 \text{ MHz}$

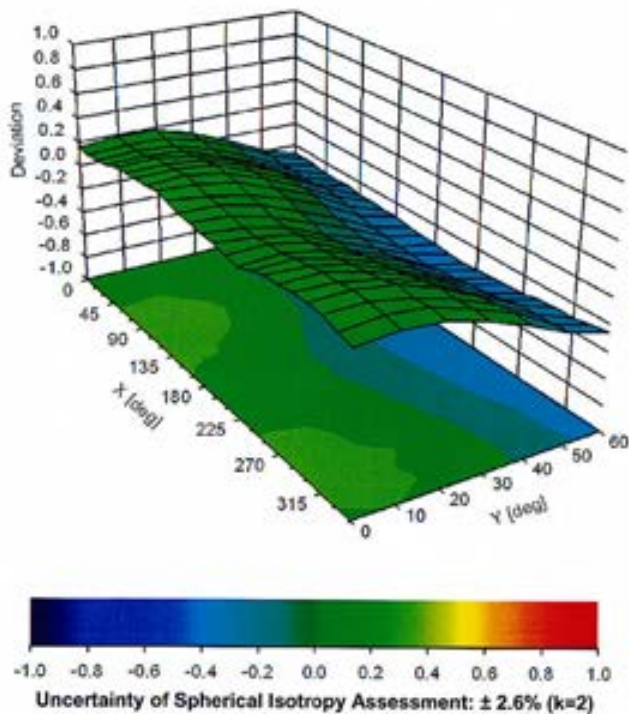

EX3DV4-- SN:7486

October 24, 2019

Appendix: Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu V}$	C	D dB	VR mV	Max dev.	Unc ^h (k=2)
0	CW	X	0.0	0.0	1.0	0.00	137.7	$\pm 3.8\%$	$\pm 4.7\%$
		Y	0.0	0.0	1.0		152.0		
		Z	0.0	0.0	1.0		161.5		
10021-DAC	GSM-FDD (TDMA, GMSK)	X	15.47	100.0	26.2	9.39	82.1	$\pm 3.5\%$	$\pm 4.7\%$
		Y	14.51	99.4	26.0		66.7		
		Z	10.49	99.5	28.8		96.2		
10023-DAC	GPRS-FDD (TDMA, GMSK, TN 0)	X	1.66	65.0	12.6	9.57	80.2	$\pm 2.7\%$	$\pm 4.7\%$
		Y	29.46	99.7	23.7		64.9		
		Z	10.83	98.5	28.3		93.5		
10024-DAC	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	0.99	60.7	8.4	6.56	125.8	$\pm 3.0\%$	$\pm 4.7\%$
		Y	21.05	99.6	23.1		122.6		
		Z	2.48	74.1	17.0		147.2		
10025-DAC	EDGE-FDD (TDMA, 8PSK, TN 0)	X	8.37	69.3	34.3	12.62	52.9	$\pm 1.7\%$	$\pm 4.7\%$
		Y	5.46	77.1	29.2		42.7		
		Z	8.46	91.9	37.4		62.0		
10026-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1)	X	5.58	79.9	28.0	9.55	119.8	$\pm 1.9\%$	$\pm 4.7\%$
		Y	4.75	75.8	26.8		96.9		
		Z	5.41	78.1	27.7		141.1		
10027-DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	34.47	99.9	21.2	4.80	121.3	$\pm 3.0\%$	$\pm 4.7\%$
		Y	29.06	99.9	21.4		126.1		
		Z	13.02	99.2	24.7		142.4		
10028-DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	29.63	98.9	20.4	3.55	136.1	$\pm 2.7\%$	$\pm 4.7\%$
		Y	15.01	99.2	22.1		144.3		
		Z	9.31	99.4	25.2		120.3		
10029-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	X	9.47	96.7	36.4	7.78	117.6	$\pm 2.2\%$	$\pm 4.7\%$
		Y	5.43	82.2	29.6		149.9		
		Z	10.13	99.2	36.7		139.4		
10039-CAB	CDMA2000 (1xRTT, RC1)	X	6.17	76.0	24.7	4.57	146.7	$\pm 1.4\%$	$\pm 4.7\%$
		Y	4.90	69.1	21.1		118.1		
		Z	5.98	74.2	23.7		126.2		
10056-CAA	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	X	4.87	78.5	30.0	11.01	77.6	$\pm 2.2\%$	$\pm 4.7\%$
		Y	3.98	73.0	28.0		62.2		
		Z	4.65	75.3	28.7		90.2		
10058-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	X	6.68	87.2	29.7	6.52	134.1	$\pm 1.7\%$	$\pm 4.7\%$
		Y	5.19	81.2	27.9		142.8		
		Z	4.96	79.0	26.7		118.1		
10081-CAB	CDMA2000 (1xRTT, RC3)	X	6.20	79.7	26.3	3.97	143.7	$\pm 1.4\%$	$\pm 4.7\%$
		Y	4.66	71.7	22.4		115.6		
		Z	5.76	76.7	24.8		123.9		
10090-DAC	GPRS-FDD (TDMA, GMSK, TN 0-4)	X	15.43	99.6	24.4	6.56	125.4	$\pm 3.5\%$	$\pm 4.7\%$
		Y	18.16	99.6	23.6		121.1		
		Z	9.82	99.2	27.4		147.6		

Certificate No: EX3-7486_Oct19

Page 11 of 14

EX3DV4-- SN:7486

October 24, 2019

10099-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-4)	X	10.19	99.2	37.2	9.55	118.7	±2.7 %	±4.7 %
		Y	5.22	79.1	28.7		95.2		
		Z	8.20	92.9	35.7		139.5		
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	9.78	68.8	21.6	8.07	103.7	±1.7 %	±4.7 %
		Y	9.82	68.4	21.5		117.8		
		Z	10.24	69.7	22.2		128.2		
10198-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	10.17	71.0	23.1	8.10	144.0	±1.4 %	±4.7 %
		Y	9.71	69.1	22.2		112.3		
		Z	10.03	70.3	22.8		122.1		
10290-AAB	CDMA2000, RC1, SO55, Full Rate	X	11.62	94.6	32.3	3.91	146.3	±1.9 %	±4.7 %
		Y	7.57	82.8	27.6		117.6		
		Z	7.76	83.3	27.7		126.1		
10291-AAB	CDMA2000, RC3, SO55, Full Rate	X	11.80	99.2	34.4	3.46	143.4	±1.9 %	±4.7 %
		Y	12.94	99.3	34.1		115.2		
		Z	12.08	97.1	33.1		123.5		
10292-AAB	CDMA2000, RC3, SO32, Full Rate	X	11.92	99.8	34.6	3.39	143.5	±1.9 %	±4.7 %
		Y	12.32	98.8	34.0		114.9		
		Z	13.37	99.8	33.9		123.6		
10293-AAB	CDMA2000, RC3, SO3, Full Rate	X	11.76	99.1	34.4	3.50	143.5	±2.2 %	±4.7 %
		Y	12.62	99.4	34.5		115.0		
		Z	10.86	94.7	32.3		123.6		
10295-AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	X	4.92	66.4	23.8	12.49	63.0	±0.9 %	±4.7 %
		Y	4.52	63.4	22.8		50.7		
		Z	5.29	67.5	24.8		74.0		
10403-AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	17.21	99.8	32.2	3.76	147.7	±1.4 %	±4.7 %
		Y	8.19	81.9	25.6		119.6		
		Z	13.55	93.3	30.0		127.1		
10404-AAB	CDMA2000 (1xEV-DO, Rev. A)	X	15.68	99.4	32.6	3.77	146.5	±1.9 %	±4.7 %
		Y	15.19	96.4	31.5		118.1		
		Z	16.70	99.3	32.4		126.4		
10406-AAB	CDMA2000, RC3, SO32, SCH0, Full Rate	X	17.03	97.6	33.1	5.22	148.4	±1.9 %	±4.7 %
		Y	11.79	86.9	29.1		120.1		
		Z	10.22	84.1	27.9		129.0		
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	7.42	98.4	34.5	1.54	109.8	±2.5 %	±4.7 %
		Y	9.91	100.0	33.3		120.8		
		Z	9.73	98.5	32.6		131.8		
10417-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	X	10.51	72.0	23.9	8.23	143.9	±1.7 %	±4.7 %
		Y	10.07	70.1	23.0		111.5		
		Z	10.21	70.7	23.2		122.5		
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	10.40	72.0	23.9	8.14	142.3	±1.7 %	±4.7 %
		Y	9.82	69.6	22.6		110.3		
		Z	10.06	70.6	23.2		121.0		

Certificate No: EX3-7486_Oct19

Page 12 of 14

EX3DV4- SN:7486

October 24, 2019

10458-AAA	CDMA2000 (1xEV-DO, Rev. B, 2 carriers)	X	10.47	77.6	25.7	6.55	124.7	±1.7 %	±4.7 %
		Y	8.97	72.5	23.3		142.6		
		Z	9.40	74.2	24.0		107.3		
10459-AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	X	11.67	74.4	24.9	8.25	148.1	±1.7 %	±4.7 %
		Y	11.22	72.3	24.0		117.0		
		Z	11.08	72.4	23.9		127.1		
10515-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)	X	7.34	98.4	34.5	1.58	109.7	±2.2 %	±4.7 %
		Y	9.17	98.7	33.0		121.1		
		Z	10.32	99.6	32.8		131.4		
10525-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)	X	10.70	72.1	24.0	8.36	145.4	±1.7 %	±4.7 %
		Y	10.29	70.4	23.3		113.0		
		Z	10.39	70.8	23.3		123.1		
10534-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)	X	10.76	71.1	23.4	8.45	103.9	±1.7 %	±4.7 %
		Y	10.58	70.0	22.9		118.6		
		Z	10.94	71.1	23.4		130.0		
10544-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	X	10.82	70.4	22.8	8.47	108.4	±1.4 %	±4.7 %
		Y	10.78	69.9	22.7		122.2		
		Z	11.31	71.4	23.5		135.6		
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	9.46	100.0	33.9	1.99	147.9	±1.9 %	±4.7 %
		Y	10.20	99.9	33.2		116.6		
		Z	9.81	98.7	33.1		128.4		
10572-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	8.79	99.6	34.2	1.99	147.3	±1.9 %	±4.7 %
		Y	9.98	99.8	33.3		116.9		
		Z	9.76	98.8	33.1		128.1		
10575-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	10.53	71.8	24.1	8.59	140.2	±1.7 %	±4.7 %
		Y	10.12	70.2	23.3		108.9		
		Z	10.31	70.8	23.6		119.3		
10583-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	X	10.55	71.9	24.1	8.59	140.7	±1.4 %	±4.7 %
		Y	10.01	69.7	23.0		109.4		
		Z	10.33	70.8	23.6		119.4		
10591-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	10.61	71.7	24.0	8.63	142.4	±1.4 %	±4.7 %
		Y	10.04	69.4	22.7		110.8		
		Z	10.41	70.7	23.5		120.8		
10599-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	10.70	70.7	23.4	8.79	102.9	±1.4 %	±4.7 %
		Y	10.60	69.8	22.9		116.5		
		Z	10.98	71.0	23.6		128.0		
10607-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle)	X	10.72	72.0	24.3	8.64	142.1	±1.7 %	±4.7 %
		Y	10.03	69.4	22.8		110.2		
		Z	10.48	70.9	23.7		121.0		
10616-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	X	10.73	70.7	23.5	8.82	103.0	±1.4 %	±4.7 %
		Y	10.55	69.6	22.8		116.4		
		Z	11.04	71.1	23.7		128.5		

Certificate No: EX3-7486_Oct19

Page 13 of 14

EX3DV4-- SN:7486

October 24, 2019

10626-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)	X	10.86	70.2	22.9	8.83	106.8	±1.4 %	±4.7 %
		Y	10.78	69.6	22.7		119.8		
		Z	11.41	71.4	23.7		133.4		
10648-AAA	CDMA2000 (1x Advanced)	X	12.74	100.0	34.1	3.45	144.2	±1.9 %	±4.7 %
		Y	8.46	88.8	29.9		115.0		
		Z	13.18	99.5	34.0		124.5		

^g Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **EX3-7511_Oct19**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:7511**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v5, QA CAL-23.v5,
QA CAL-25.v7
Calibration procedure for dosimetric E-field probes**

Calibration date: **October 24, 2019**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-19 (No. 217-02894)	Apr-20
DAE4	SN: 660	07-Oct-19 (No. DAE4-660_Oct19)	Oct-20
Reference Probe ES3DV2	SN: 3013	31-Dec-18 (No. ES3-3013_Dec18)	Dec-19
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter F4419B	SN: GB41293874	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642UD1700	04-Aug-09 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
Issued: October 24, 2019			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: EX3-7511_Oct19

Page 1 of 13

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization ϕ	ϕ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E^2 -field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 – SN:7511

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7511**Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.46	0.37	0.44	± 10.1 %
DCP (mV) ^B	99.0	96.6	99.9	

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Max dev.	Unc ^C (k=2)
0	CW	X	0.0	0.0	1.0	0.00	118.4	±3.8 %	± 4.7 %
		Y	0.0	0.0	1.0		133.1		
		Z	0.0	0.0	1.0		117.4		

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).^B Numerical linearization parameter; uncertainty not required.^C Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4--SN:7511

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7511**Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	0.8
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

EX3DV4—SN:7511

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7511

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^e	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth (mm) ^g	Unc (k=2)
150	52.3	0.76	12.15	12.15	12.15	0.00	1.00	± 13.3 %
300	45.3	0.87	10.87	10.87	10.87	0.08	1.20	± 13.3 %
450	43.5	0.87	10.30	10.30	10.30	0.10	1.30	± 13.3 %
750	41.9	0.89	9.57	9.57	9.57	0.46	0.80	± 12.0 %
835	41.5	0.90	9.28	9.28	9.28	0.33	1.01	± 12.0 %
900	41.5	0.97	9.06	9.06	9.06	0.49	0.81	± 12.0 %
1450	40.5	1.20	8.17	8.17	8.17	0.10	0.80	± 12.0 %
1810	40.0	1.40	7.94	7.94	7.94	0.28	0.80	± 12.0 %
1900	40.0	1.40	7.69	7.69	7.69	0.34	0.80	± 12.0 %
2100	39.8	1.49	7.73	7.73	7.73	0.33	0.80	± 12.0 %
2300	39.5	1.67	7.35	7.35	7.35	0.36	0.90	± 12.0 %
2450	39.2	1.80	7.06	7.06	7.06	0.33	0.90	± 12.0 %
2600	39.0	1.96	6.81	6.81	6.81	0.39	0.90	± 12.0 %
3500	37.9	2.91	6.66	6.66	6.66	0.35	1.30	± 13.1 %
3700	37.7	3.12	6.56	6.56	6.56	0.35	1.30	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^e At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7511

October 24, 2019

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7511

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^g	Depth (mm) ^g	Unc (k=2)
150	61.9	0.80	11.72	11.72	11.72	0.00	1.00	± 13.3 %
300	58.2	0.92	11.12	11.12	11.12	0.04	1.20	± 13.3 %
450	56.7	0.94	10.59	10.59	10.59	0.08	1.30	± 13.3 %
750	55.5	0.96	9.52	9.52	9.52	0.49	0.80	± 12.0 %
835	55.2	0.97	9.26	9.26	9.26	0.40	0.80	± 12.0 %
900	55.0	1.05	9.14	9.14	9.14	0.42	0.84	± 12.0 %
1450	54.0	1.30	7.97	7.97	7.97	0.30	0.80	± 12.0 %
1810	53.3	1.52	7.64	7.64	7.64	0.34	0.80	± 12.0 %
1900	53.3	1.52	7.37	7.37	7.37	0.44	0.80	± 12.0 %
2100	53.2	1.62	7.46	7.46	7.46	0.31	0.86	± 12.0 %
2300	52.9	1.81	7.21	7.21	7.21	0.35	0.90	± 12.0 %
2450	52.7	1.95	6.97	6.97	6.97	0.36	0.90	± 12.0 %
2600	52.5	2.16	6.88	6.88	6.88	0.32	0.90	± 12.0 %
3500	51.3	3.31	6.11	6.11	6.11	0.40	1.35	± 13.1 %
3700	51.0	3.55	6.02	6.02	6.02	0.40	1.35	± 13.1 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 8 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^f At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^g Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:7511



October 24, 2019

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

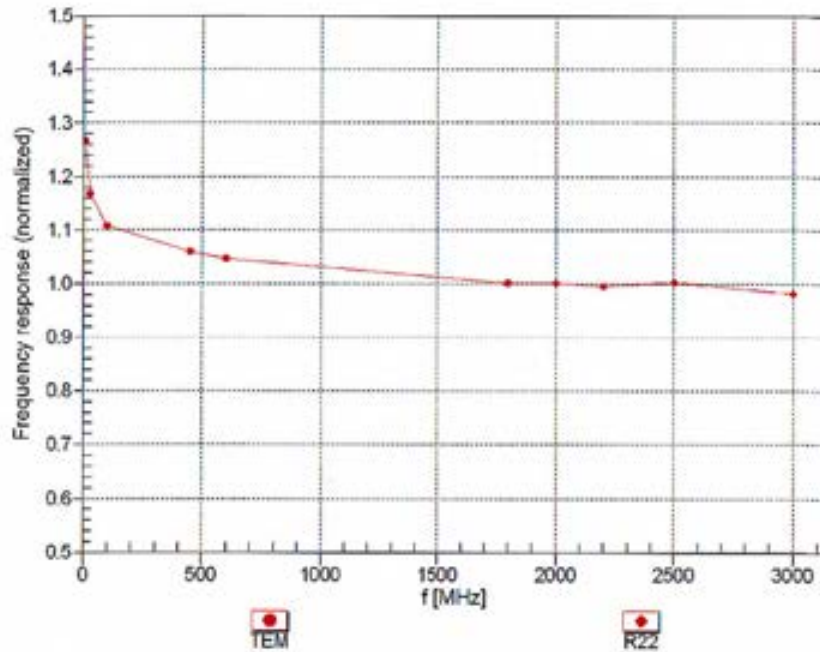Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

EX3DV4- SN:7511



October 24, 2019

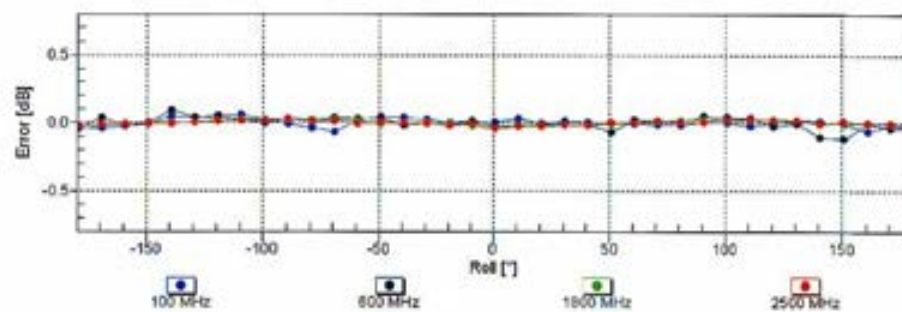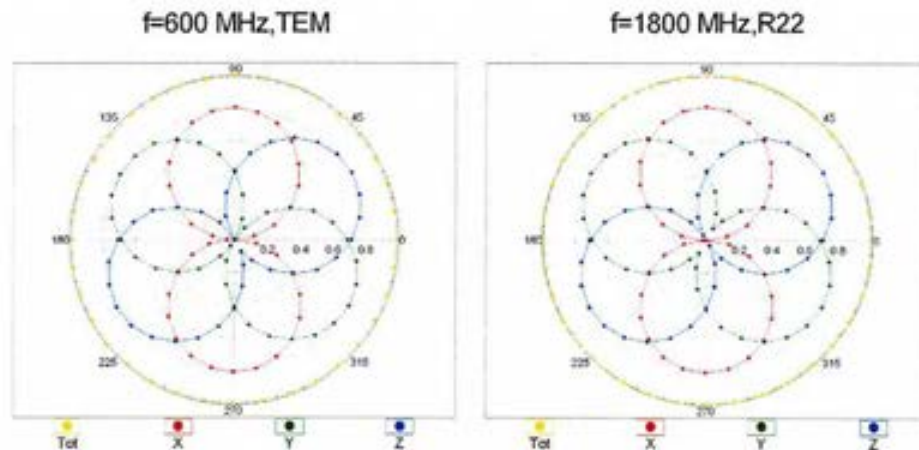Receiving Pattern (ϕ), $\theta = 0^\circ$ **Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)**

EX3DV4-SN:7511

October 24, 2019


Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f_{\text{eval}} = 1900 \text{ MHz}$)

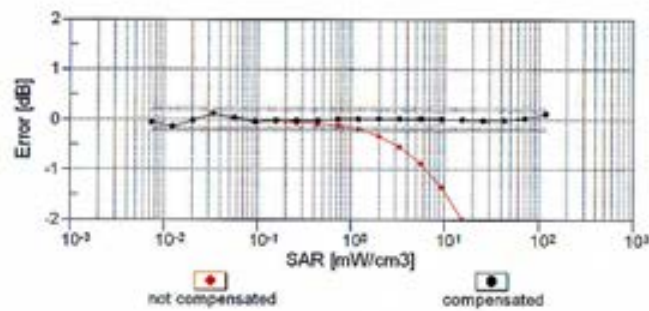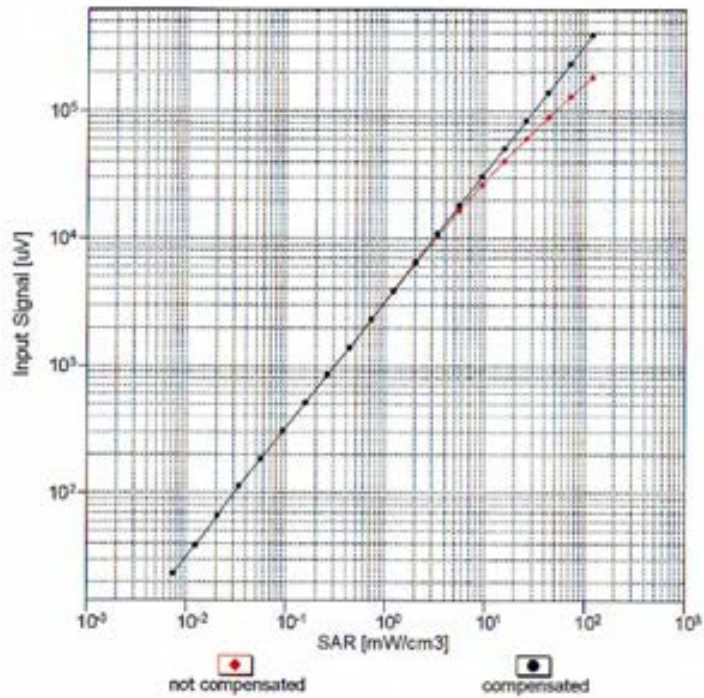Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)


EX3DV4-- SN:7511

October 24, 2019

Conversion Factor Assessment

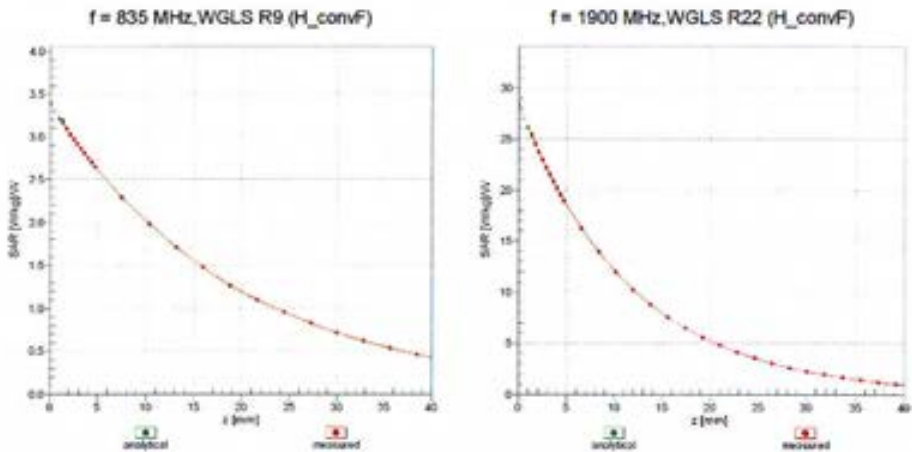

Deviation from Isotropy in Liquid
Error (ϕ, θ), f = 900 MHz

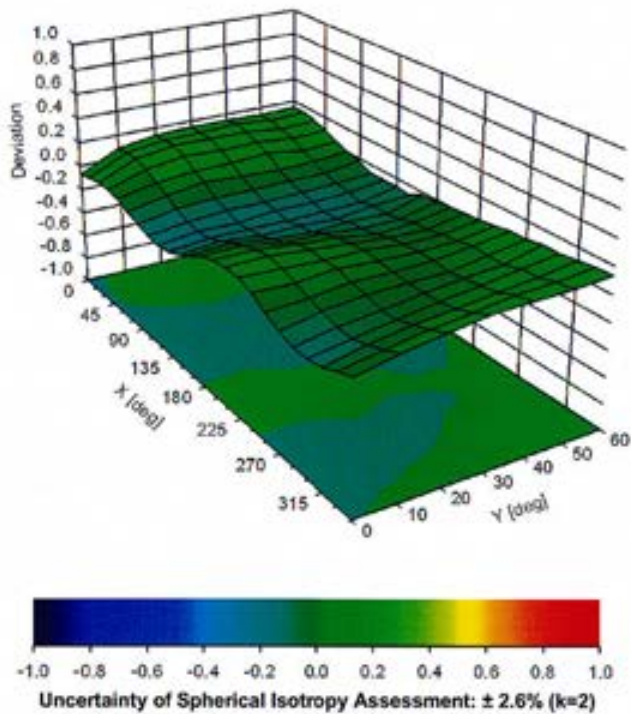

EX3DV4--SN:7511

October 24, 2019

Appendix: Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB- $\sqrt{\mu V}$	C	D dB	VR mV	Max dev.	Unc ^B (k=2)
0	CW	X	0.0	0.0	1.0	0.00	118.4	$\pm 3.8 \%$	$\pm 4.7 \%$
		Y	0.0	0.0	1.0		133.1		
		Z	0.0	0.0	1.0		117.4		
10100-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.43	67.6	19.8	5.67	141.8	$\pm 1.4 \%$	$\pm 4.7 \%$
		Y	6.81	70.2	22.1		112.8		
		Z	6.38	67.4	19.7		140.0		
10108-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.29	67.3	19.8	5.80	138.5	$\pm 2.2 \%$	$\pm 4.7 \%$
		Y	7.56	73.7	24.5		110.1		
		Z	6.28	67.3	19.8		136.5		
10110-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	5.97	67.0	19.8	5.75	134.4	$\pm 2.5 \%$	$\pm 4.7 \%$
		Y	6.87	72.6	24.2		149.0		
		Z	5.93	66.8	19.6		132.2		
10154-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	5.97	67.0	19.8	5.75	134.3	$\pm 2.5 \%$	$\pm 4.7 \%$
		Y	6.95	73.0	24.5		149.0		
		Z	5.95	66.9	19.6		132.6		
10156-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	5.77	67.1	19.8	5.79	129.9	$\pm 2.5 \%$	$\pm 4.7 \%$
		Y	6.92	74.0	25.2		144.8		
		Z	5.72	66.8	19.7		128.0		
10160-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.41	67.5	20.0	5.82	140.2	$\pm 2.5 \%$	$\pm 4.7 \%$
		Y	8.27	76.0	25.8		111.2		
		Z	6.37	67.4	19.9		137.5		
10169-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.81	67.0	20.0	5.73	116.5	$\pm 2.7 \%$	$\pm 4.7 \%$
		Y	7.29	81.0	29.2		129.3		
		Z	4.77	66.7	19.8		114.7		
10175-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4.80	66.9	20.0	5.72	116.1	$\pm 2.5 \%$	$\pm 4.7 \%$
		Y	6.87	79.0	28.1		129.3		
		Z	4.80	66.9	19.9		114.1		
10177-CAI	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	4.82	67.1	20.1	5.73	115.5	$\pm 2.5 \%$	$\pm 4.7 \%$
		Y	6.68	78.1	27.6		129.4		
		Z	4.78	66.8	19.9		113.9		
10181-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	4.88	67.4	20.3	5.72	116.3	$\pm 2.5 \%$	$\pm 4.7 \%$
		Y	6.81	78.7	27.9		129.1		
		Z	4.80	66.8	19.9		114.1		
10297-AAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	6.37	67.7	20.2	5.81	138.2	$\pm 2.5 \%$	$\pm 4.7 \%$
		Y	7.95	75.1	25.4		110.4		
		Z	6.32	67.5	20.0		136.2		
10311-AAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.90	68.1	20.4	6.06	144.1	$\pm 2.5 \%$	$\pm 4.7 \%$
		Y	8.57	75.6	25.7		113.8		
		Z	6.90	68.0	20.4		140.7		

EX3DV4- SN:7511

October 24, 2019

10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	3.27	71.5	20.0	1.54	130.5	±3.0 %	±4.7 %
		Y	7.44	100.0	36.1		146.5		
		Z	3.30	71.7	20.1		128.2		
10435-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.67	70.0	23.2	7.82	134.0	±2.2 %	±4.7 %
		Y	6.40	76.6	28.9		142.3		
		Z	5.66	69.8	23.0		132.2		
10467-AAF	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.67	70.0	23.2	7.82	133.7	±1.4 %	±4.7 %
		Y	5.81	72.6	26.0		142.6		
		Z	5.65	69.7	22.9		131.7		
10470-AAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.64	69.8	23.0	7.82	133.5	±1.4 %	±4.7 %
		Y	5.73	71.9	25.4		142.7		
		Z	5.69	69.9	23.0		131.9		
10473-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	5.67	70.1	23.2	7.82	133.5	±1.2 %	±4.7 %
		Y	5.65	71.4	25.1		142.7		
		Z	5.67	69.8	23.0		131.5		
10485-AAF	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.02	67.8	21.6	7.59	110.4	±1.2 %	±4.7 %
		Y	6.00	69.0	23.2		121.1		
		Z	6.30	68.9	22.1		149.7		
10488-AAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.35	67.6	21.5	7.70	114.9	±1.2 %	±4.7 %
		Y	6.26	68.5	22.9		124.7		
		Z	6.37	67.6	21.4		113.3		
10491-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.74	68.0	21.6	7.74	119.3	±1.2 %	±4.7 %
		Y	6.58	68.6	22.9		129.0		
		Z	6.73	67.8	21.5		117.8		
10494-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.75	68.1	21.7	7.74	119.1	±1.2 %	±4.7 %
		Y	6.56	68.6	23.0		128.9		
		Z	6.74	67.9	21.6		117.6		
10503-AAF	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.37	67.7	21.5	7.72	114.8	±1.4 %	±4.7 %
		Y	6.34	68.9	23.2		124.8		
		Z	6.36	67.4	21.3		113.4		
10506-AAF	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	6.72	68.0	21.7	7.74	118.9	±1.4 %	±4.7 %
		Y	6.56	68.6	23.0		128.6		
		Z	6.73	67.9	21.6		117.8		
10509-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.35	68.6	22.0	7.99	124.0	±1.4 %	±4.7 %
		Y	7.06	68.7	23.0		133.6		
		Z	7.37	68.5	22.0		122.9		

Certificate No: EX3-7511_Oct19

Page 12 of 13

EX3DV4- SN:7511

October 24, 2019

10512-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	7.09	68.6	21.9	7.74	122.9	±1.4 %	±4.7 %
		Y	6.83	69.0	23.0		131.8		
		Z	7.10	68.5	21.8		121.3		
10571-AAA	IEEE 802.11b WIFI 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	3.42	71.9	20.4	1.99	127.1	±1.9 %	±4.7 %
		Y	9.13	99.3	33.8		140.7		
		Z	3.61	72.9	21.0		124.4		

⁶ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Appendix C

Dipole Calibration Certificates

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **CLA150-4005_Feb18**

CALIBRATION CERTIFICATE

Object **CLA150 - SN: 4005**

Calibration procedure(s) **QA CAL-15.v8
Calibration procedure for system validation sources below 700 MHz**

Calibration date: **February 09, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5277 (20x)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX3DV4	SN: 3877	30-Dec-17 (No. EX3-3877_Dec17)	Dec-18
DAE4	SN: 654	24-Jul-17 (No. DAE4-654_Jul17)	Jul-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (No. 217-02285/02284)	In house check: Jun-18
Power sensor E4412A	SN: MY41498087	06-Apr-16 (No. 217-02285)	In house check: Jun-18
Power sensor E4412A	SN: 000110210	06-Apr-16 (No. 217-02284)	In house check: Jun-18
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-16)	In house check: Jun-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: February 12, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: **CLA150-4005_Feb18**

Page 1 of 8

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:** This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.0
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	$dx, dy = 4.0$ mm, $dz = 1.4$ mm	Graded Ratio = 1.4 (Z direction)
Frequency	150 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	52.3	0.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	$50.3 \pm 6 \%$	$0.76 \text{ mho/m} \pm 6 \%$
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.80 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	$3.77 \text{ W/kg} \pm 18.4 \%$ (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.52 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	$2.50 \text{ W/kg} \pm 18.0 \%$ (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	61.9	0.80 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	$62.1 \pm 6 \%$	$0.81 \text{ mho/m} \pm 6 \%$
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	1 W input power	3.87 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	$3.84 \text{ W/kg} \pm 18.4 \%$ (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	1 W input power	2.57 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	$2.55 \text{ W/kg} \pm 18.0 \%$ (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	$41.9 \Omega + 2.0 j\Omega$
Return Loss	- 20.8 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$42.9 \Omega + 0.8 j\Omega$
Return Loss	- 22.3 dB

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 23, 2013

DASY5 Validation Report for Head TSL

Date: 09.02.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4005

Communication System: UID 0 - CW; Frequency: 150 MHz

Medium parameters used: $f = 150$ MHz; $\sigma = 0.76$ S/m; $\epsilon_r = 50.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(12.12, 12.12, 12.12); Calibrated: 30.12.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 24.07.2017
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan(81x81x1): Interpolated grid: $dx=1.500$ mm, $dy=1.500$ mm

Maximum value of SAR (interpolated) = 5.37 W/kg


CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan,**dist=1.4mm (8x10x7)/Cube 0:** Measurement grid: $dx=4$ mm, $dy=4$ mm, $dz=1.4$ mm

Reference Value = 83.36 V/m; Power Drift = -0.05 dB


Peak SAR (extrapolated) = 7.14 W/kg

SAR(1 g) = 3.8 W/kg; SAR(10 g) = 2.52 W/kg

Maximum value of SAR (measured) = 5.33 W/kg

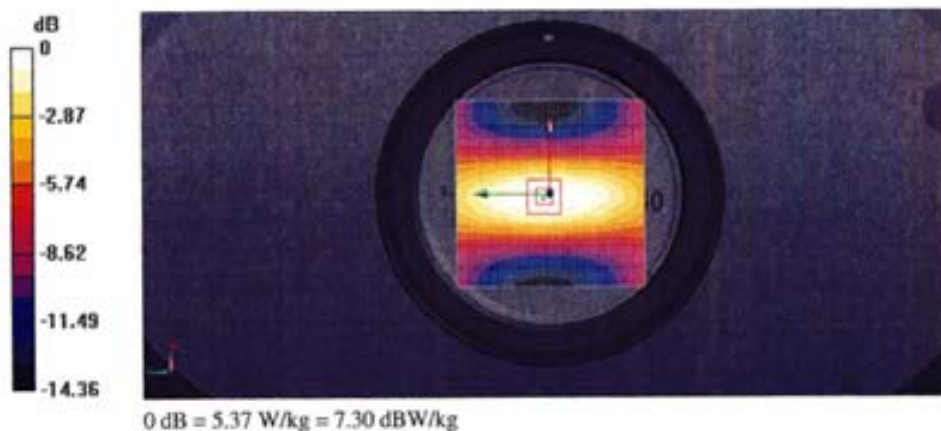

Impedance Measurement Plot for Head TSL

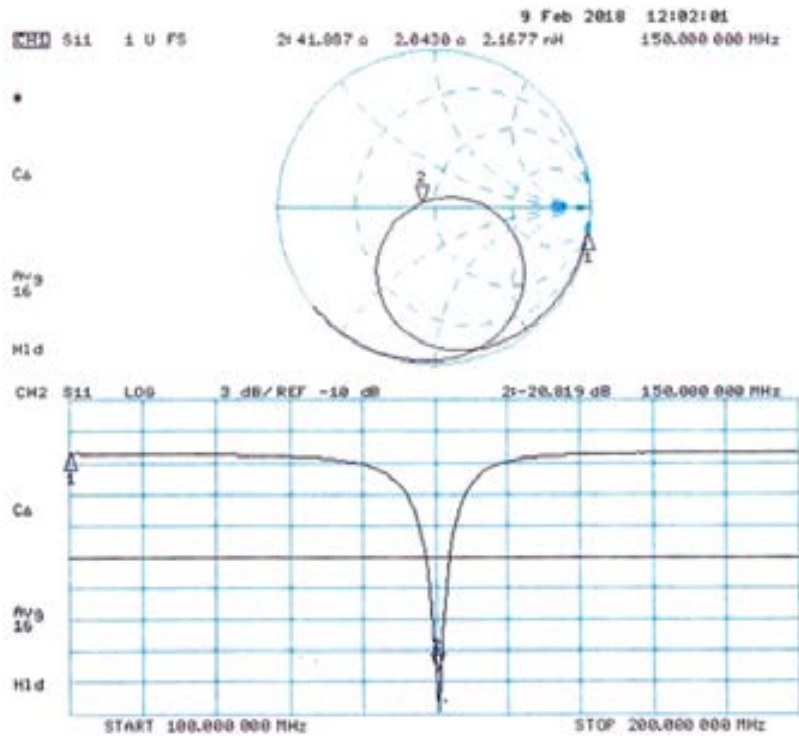

DASY5 Validation Report for Body TSL

Date: 09.02.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4005

Communication System: UID 0 - CW; Frequency: 150 MHz

Medium parameters used: $f = 150 \text{ MHz}$; $\sigma = 0.81 \text{ S/m}$; $\epsilon_r = 62.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(11.57, 11.57, 11.57); Calibrated: 30.12.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 24.07.2017
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan**(81x81x1):** Interpolated grid: $dx=1.500 \text{ mm}$, $dy=1.500 \text{ mm}$

Maximum value of SAR (interpolated) = 5.47 W/kg


CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan,**dist=1.4mm (8x10x7)/Cube 0:** Measurement grid: $dx=4\text{mm}$, $dy=4\text{mm}$, $dz=1.4\text{mm}$

Reference Value = 81.25 V/m; Power Drift = 0.01 dB


Peak SAR (extrapolated) = 7.26 W/kg

SAR(1 g) = 3.87 W/kg; SAR(10 g) = 2.57 W/kg

Maximum value of SAR (measured) = 5.37 W/kg

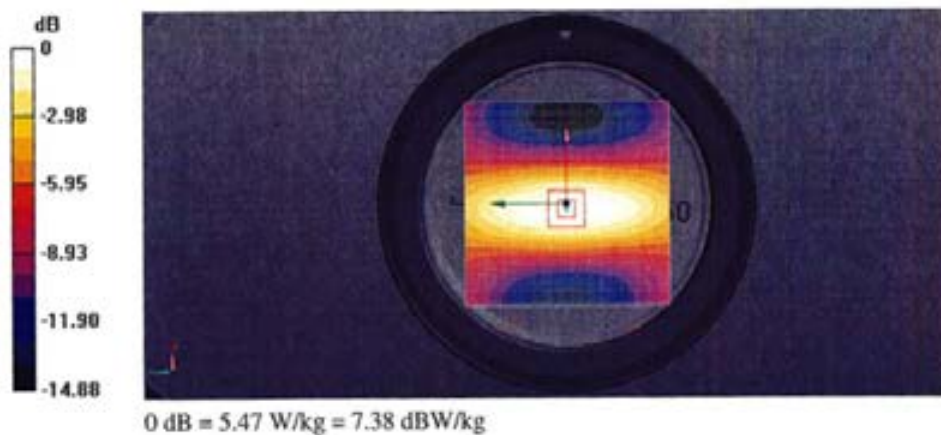

Impedance Measurement Plot for Body TSL

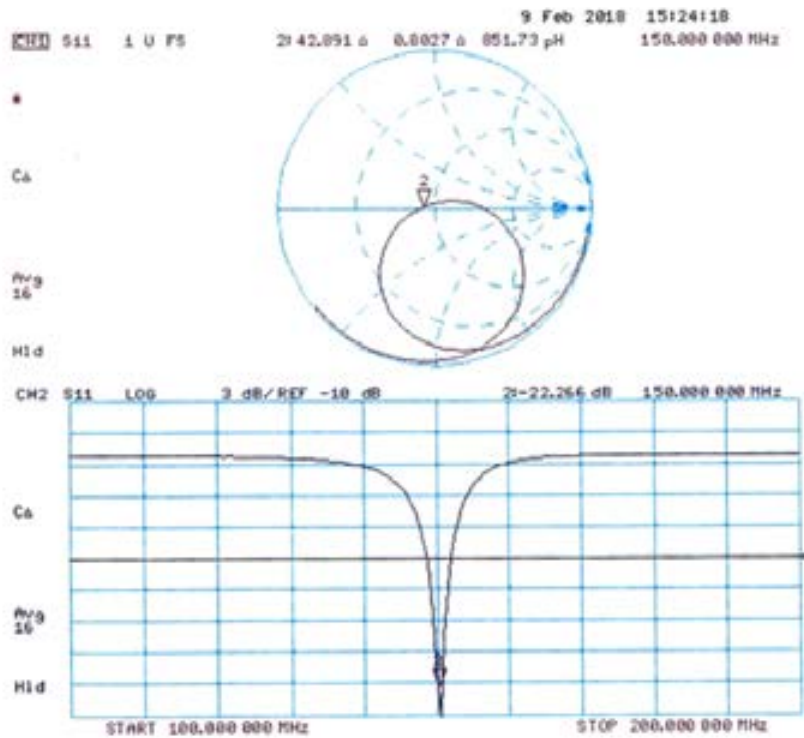

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Motorola Solutions MY**

Certificate No: **CLA150-4016_Oct18**

CALIBRATION CERTIFICATE

Object **CLA150 - SN: 4016**

Calibration procedure(s) **QA CAL-15.v8**
Calibration procedure for system validation sources below 700 MHz

Calibration date: **October 10, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: 5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-18 (No. 217-02683)	Apr-19
Reference Probe EX3DV4	SN: 3877	30-Dec-17 (No. EX3-3877_Dec17)	Dec-18
DAE4	SN: 654	05-Jul-18 (No. DAE4-654_Jul18)	Jul-19
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	12-Jun-18 (No. 217-02285/02284)	In house check: Jun-20
Power sensor E4412A	SN: MY41498067	12-Jun-18 (No. 217-02285)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	12-Jun-18 (No. 217-02284)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

	Name	Function	Signature
Calibrated by:	Michael Weber	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: October 15, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: CLA150-4016_Oct18

Page 1 of 8

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss:** This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.2
Extrapolation	Advanced Extrapolation	
Phantom	ELI4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	$dx, dy = 4.0$ mm, $dz = 1.4$ mm	Graded Ratio = 1.4 (Z direction)
Frequency	150 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	52.3	0.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	$50.3 \pm 6 \%$	$0.76 \text{ mho/m} \pm 6 \%$
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.67 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.64 W/kg $\pm 18.4 \%$ (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.45 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	2.43 W/kg $\pm 18.0 \%$ (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	61.9	0.80 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	$63.3 \pm 6 \%$	$0.82 \text{ mho/m} \pm 6 \%$
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	1 W input power	4.01 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	3.95 W/kg $\pm 18.4 \%$ (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	1 W input power	2.65 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	2.61 W/kg $\pm 18.0 \%$ (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)**Antenna Parameters with Head TSL**

Impedance, transformed to feed point	47.0 Ω - 4.4 j Ω
Return Loss	- 25.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.9 Ω - 1.7 j Ω
Return Loss	- 35.5 dB

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 28, 2014

DASY5 Validation Report for Head TSL

Date: 10.10.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4016

Communication System: UID 0 - CW; Frequency: 150 MHz

Medium parameters used: $f = 150$ MHz; $\sigma = 0.76$ S/m; $\epsilon_r = 50.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(12.12, 12.12, 12.12) @ 150 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 05.07.2018
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.2(1495); SEMCAD X 14.6.12(7450)

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan(81x81x1): Interpolated grid: $dx=1.500$ mm, $dy=1.500$ mm

Maximum value of SAR (interpolated) = 5.21 W/kg


CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan,**dist=1.4mm (8x10x7)/Cube 0:** Measurement grid: $dx=4$ mm, $dy=4$ mm, $dz=1.4$ mm

Reference Value = 80.01 V/m; Power Drift = -0.09 dB


Peak SAR (extrapolated) = 7.05 W/kg

SAR(1 g) = 3.67 W/kg; SAR(10 g) = 2.45 W/kg

Maximum value of SAR (measured) = 5.15 W/kg

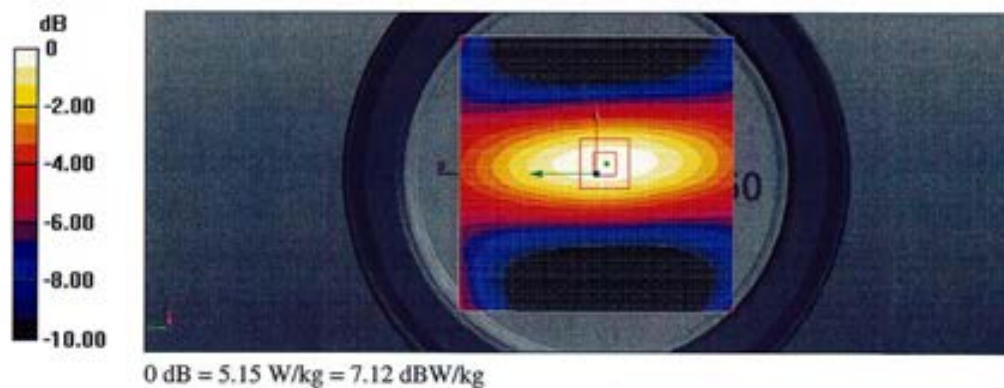

Impedance Measurement Plot for Head TSL

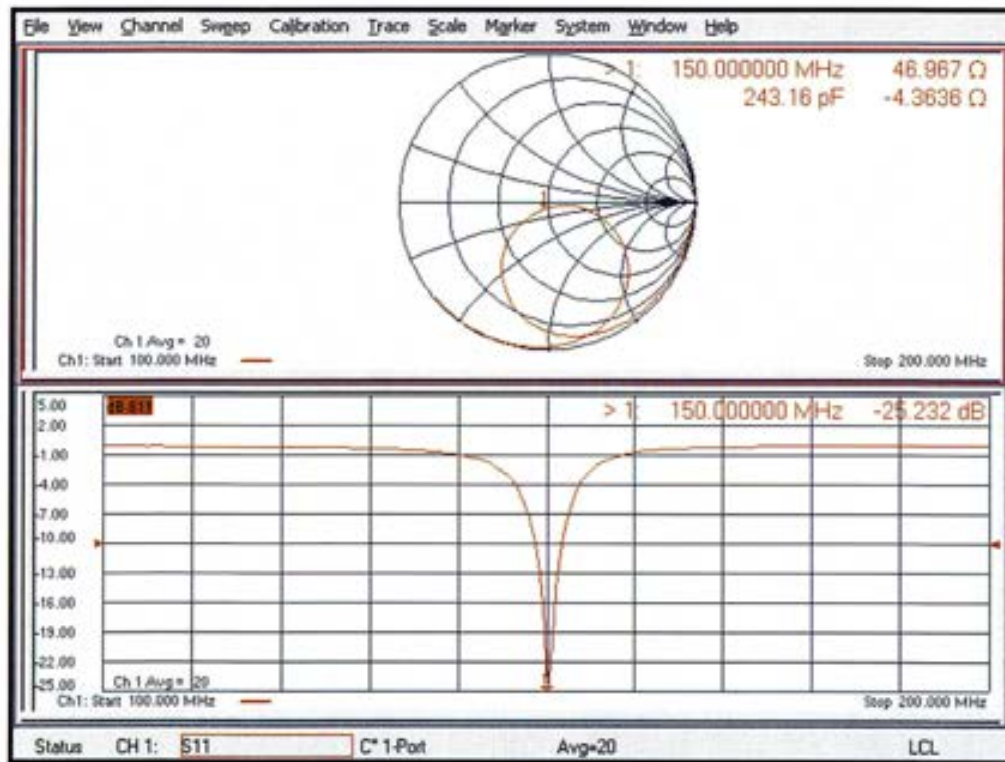

DASY5 Validation Report for Body TSL

Date: 10.10.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4016

Communication System: UID 0 - CW; Frequency: 150 MHz

Medium parameters used: $f = 150$ MHz; $\sigma = 0.82$ S/m; $\epsilon_r = 63.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(11.57, 11.57, 11.57) @ 150 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 05.07.2018
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.2(1495); SEMCAD X 14.6.12(7450)

CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Area Scan(81x81x1): Interpolated grid: $dx=1.500$ mm, $dy=1.500$ mm

Maximum value of SAR (interpolated) = 5.75 W/kg


CLA Calibration for MSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan, dist=1.4mm (8x10x7)/Cube 0: Measurement grid: $dx=4$ mm, $dy=4$ mm, $dz=1.4$ mm

Reference Value = 82.91 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 7.87 W/kg

SAR(1 g) = 4.01 W/kg; SAR(10 g) = 2.65 W/kg


Maximum value of SAR (measured) = 5.67 W/kg

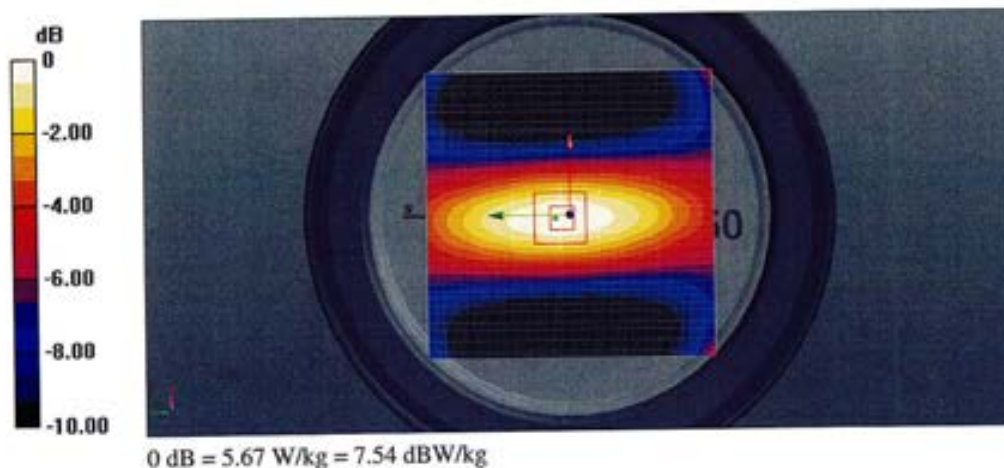

Certificate No: CLA150-4016_Oct18

Page 7 of 8

Impedance Measurement Plot for Body TSL

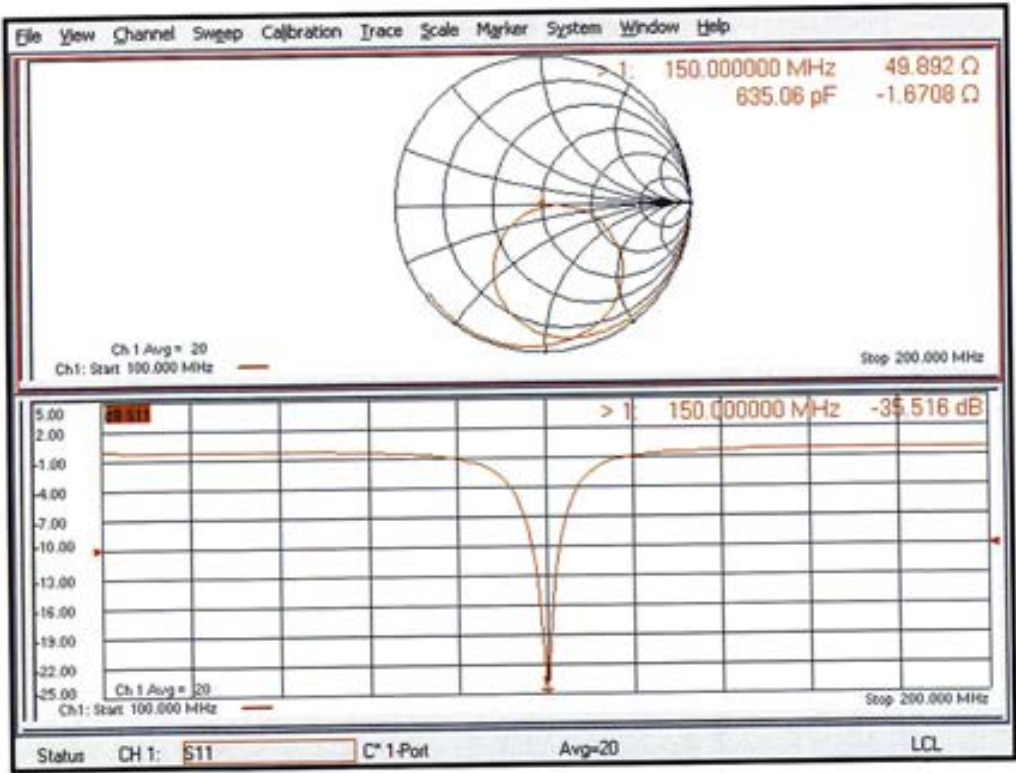

Dipole Data

As stated in KDB 865664, only dipoles used for longer calibration intervals required to provide supporting information and measurement to qualify for extended calibration interval.

The table below includes dipole impedance and return loss measurement data measured by Motorola Solutions' EME lab. The results meet the requirements stated in KDB 865664.

Dipole CLA150-4005	Head			Body		
	Impedance		Return Loss	Impedance		Return Loss
Date Measured	real Ω	imag $j\Omega$	dB	real Ω	imag $j\Omega$	dB
02/26/2018	43.11	4.56	-21.01	46.25	-0.63	-28.16
02/09/2019	43.62	5.59	-20.87	46.18	-2.20	-26.77

Dipole CLA150-4016	Head			Body		
	Impedance		Return Loss	Impedance		Return Loss
Date Measured	real Ω	imag $j\Omega$	dB	real Ω	imag $j\Omega$	dB
12/18/2018	44.51	6.18	-21.21	44.94	5.98	-21.59
11/09/2019	42.03	9.19	-21.64	45.01	6.36	-21.45