




Appendix D





Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

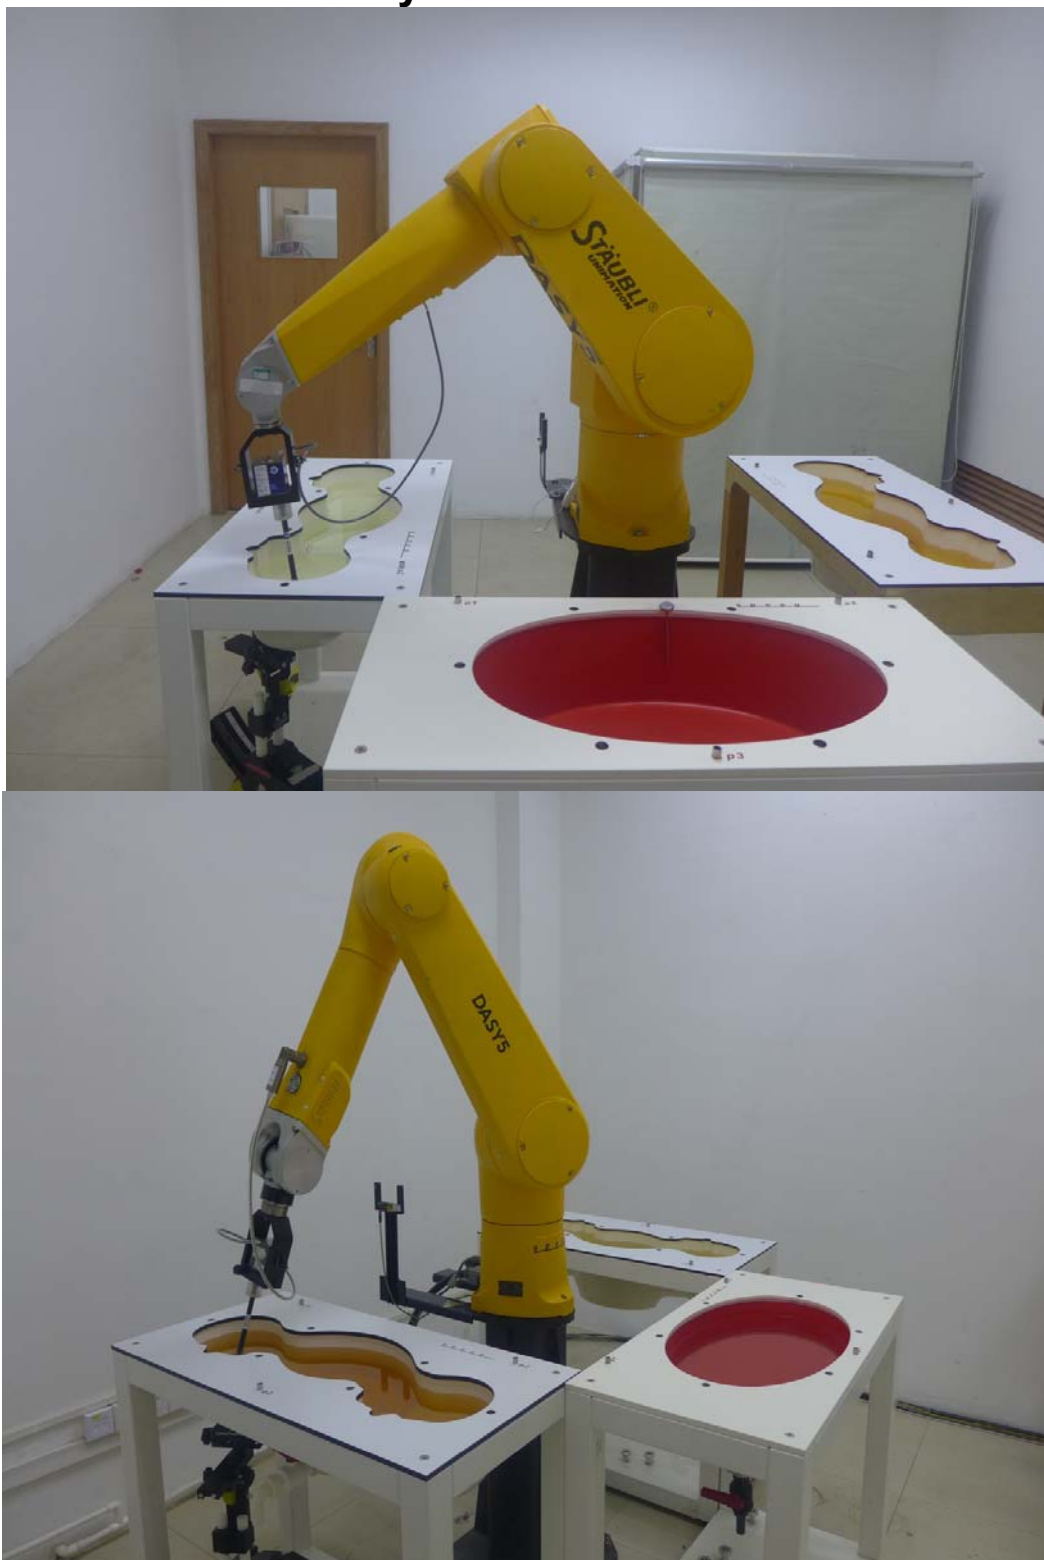

2. Photographs of Tissue Simulate Liquid

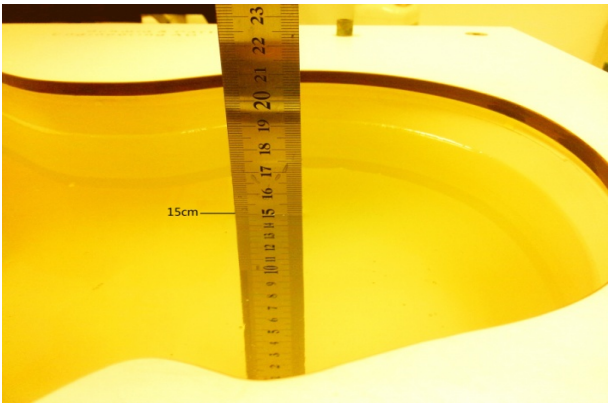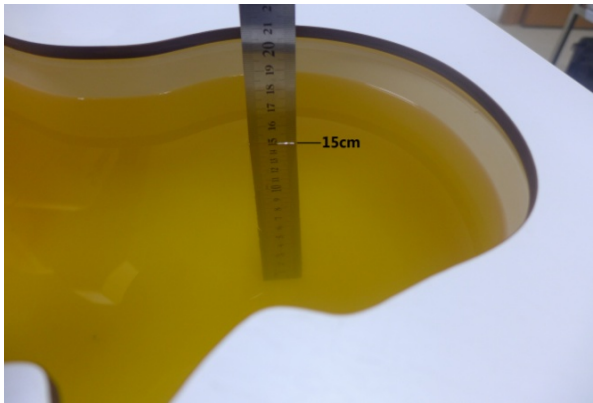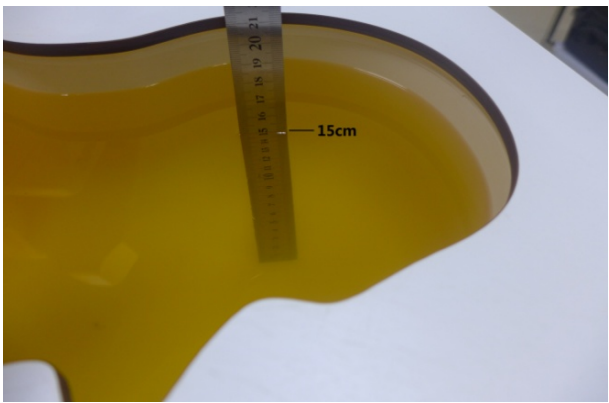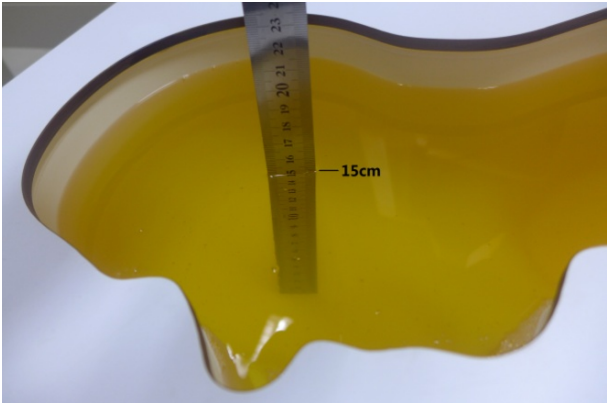Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1750
	
Photo 3: issue Simulant Liquid for Head 1900	Photo 4: Tissue Simulant Liquid for Head 2600
	

3. Photographs of EUT test position

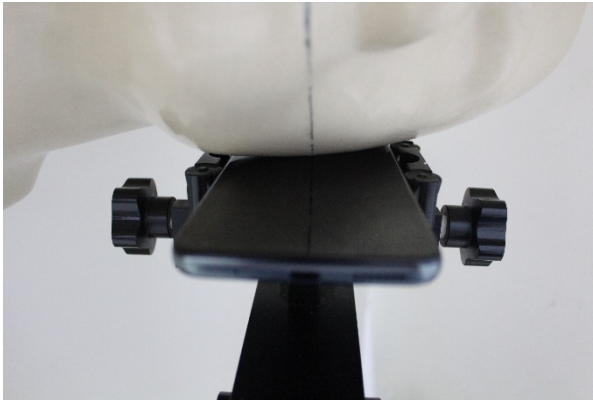
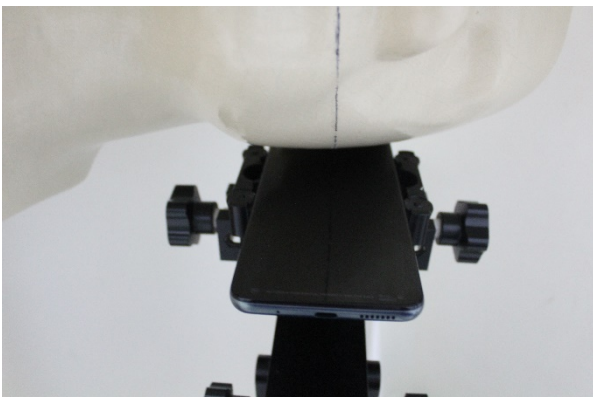
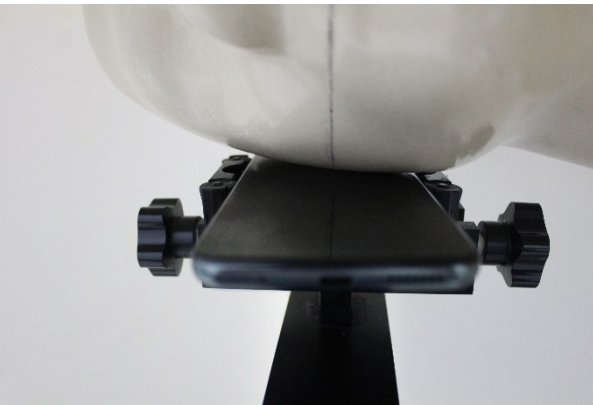
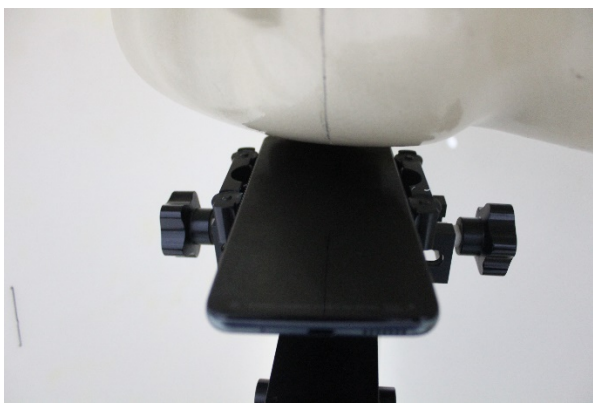
Photo 5: Left cheek	Photo 6: Left tilted
	
Photo 7: Right cheek	Photo 8: Right tilted
	
Photo 9: Front side 5mm	Photo 10: Back side 5mm
	

Photo 11: Left side 5mm	Photo 12: Right side 5mm
	
Photo 13: Bottom side 5mm	Photo 14: Back side 0mm
	
Photo 15: Bottom side 0mm	Photo 16: Back side with headset 5mm
	

Photo 17: Front side 10mm	Photo 18: Back side 17mm
	

4. EUT Constructional Details

Photo 19: Front View	Photo 20: Back View
	