


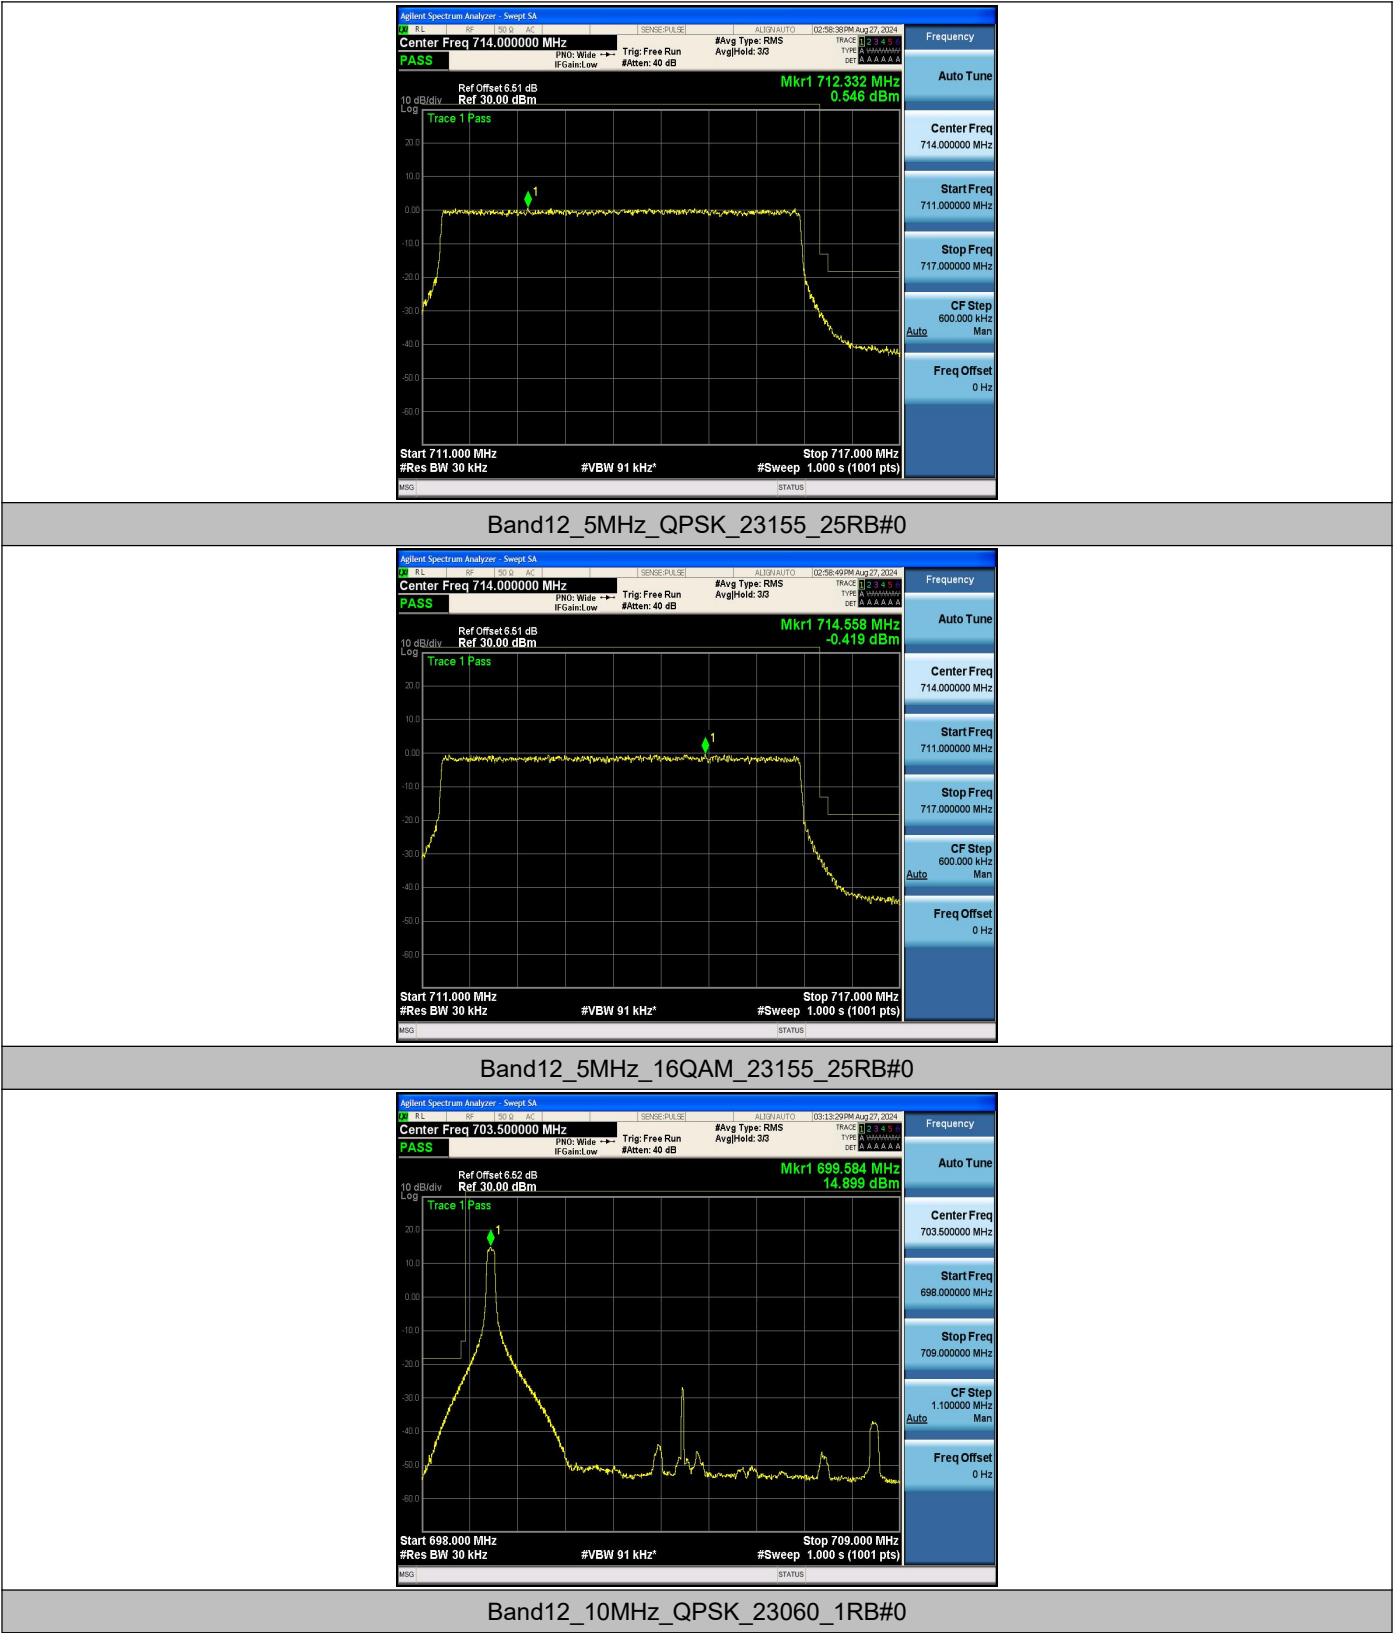

Agilent Spectrum Analyzer - Sweep SA

Center Freq 703.500000 MHz

PASS

Ref Offset 6.52 dB

Ref 30.00 dBm

Trace 1 Pass

Start 698.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 709.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 703.500000 MHz

Start Freq 698.000000 MHz

Stop Freq 709.000000 MHz

CF Step 1.100000 MHz


Auto

Freq Offset 0 Hz


Mkr1 699.584 MHz

14.899 dBm

Band12_10MHz_QPSK_23060_1RB#0

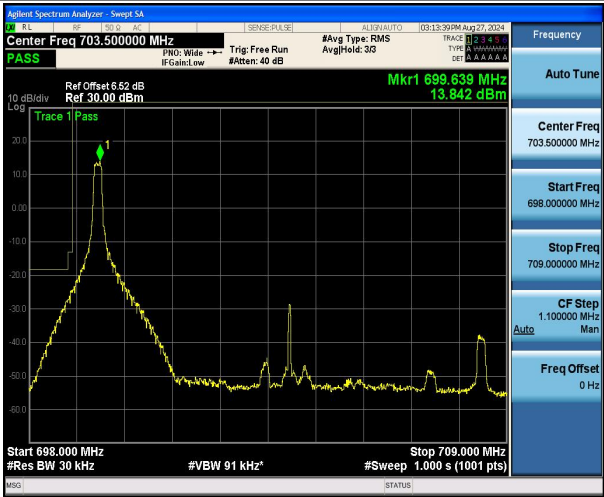


Band12_10MHz_16QAM_23060_1RB#0

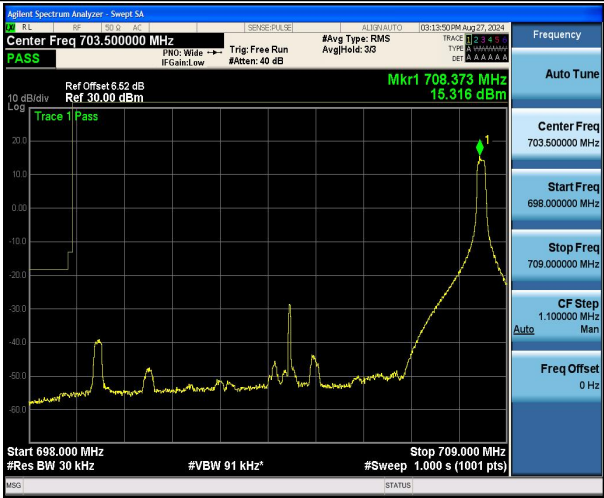

Band12_10MHz_QPSK_23060_1RB#49



Band12_10MHz_16QAM_23060_1RB#49

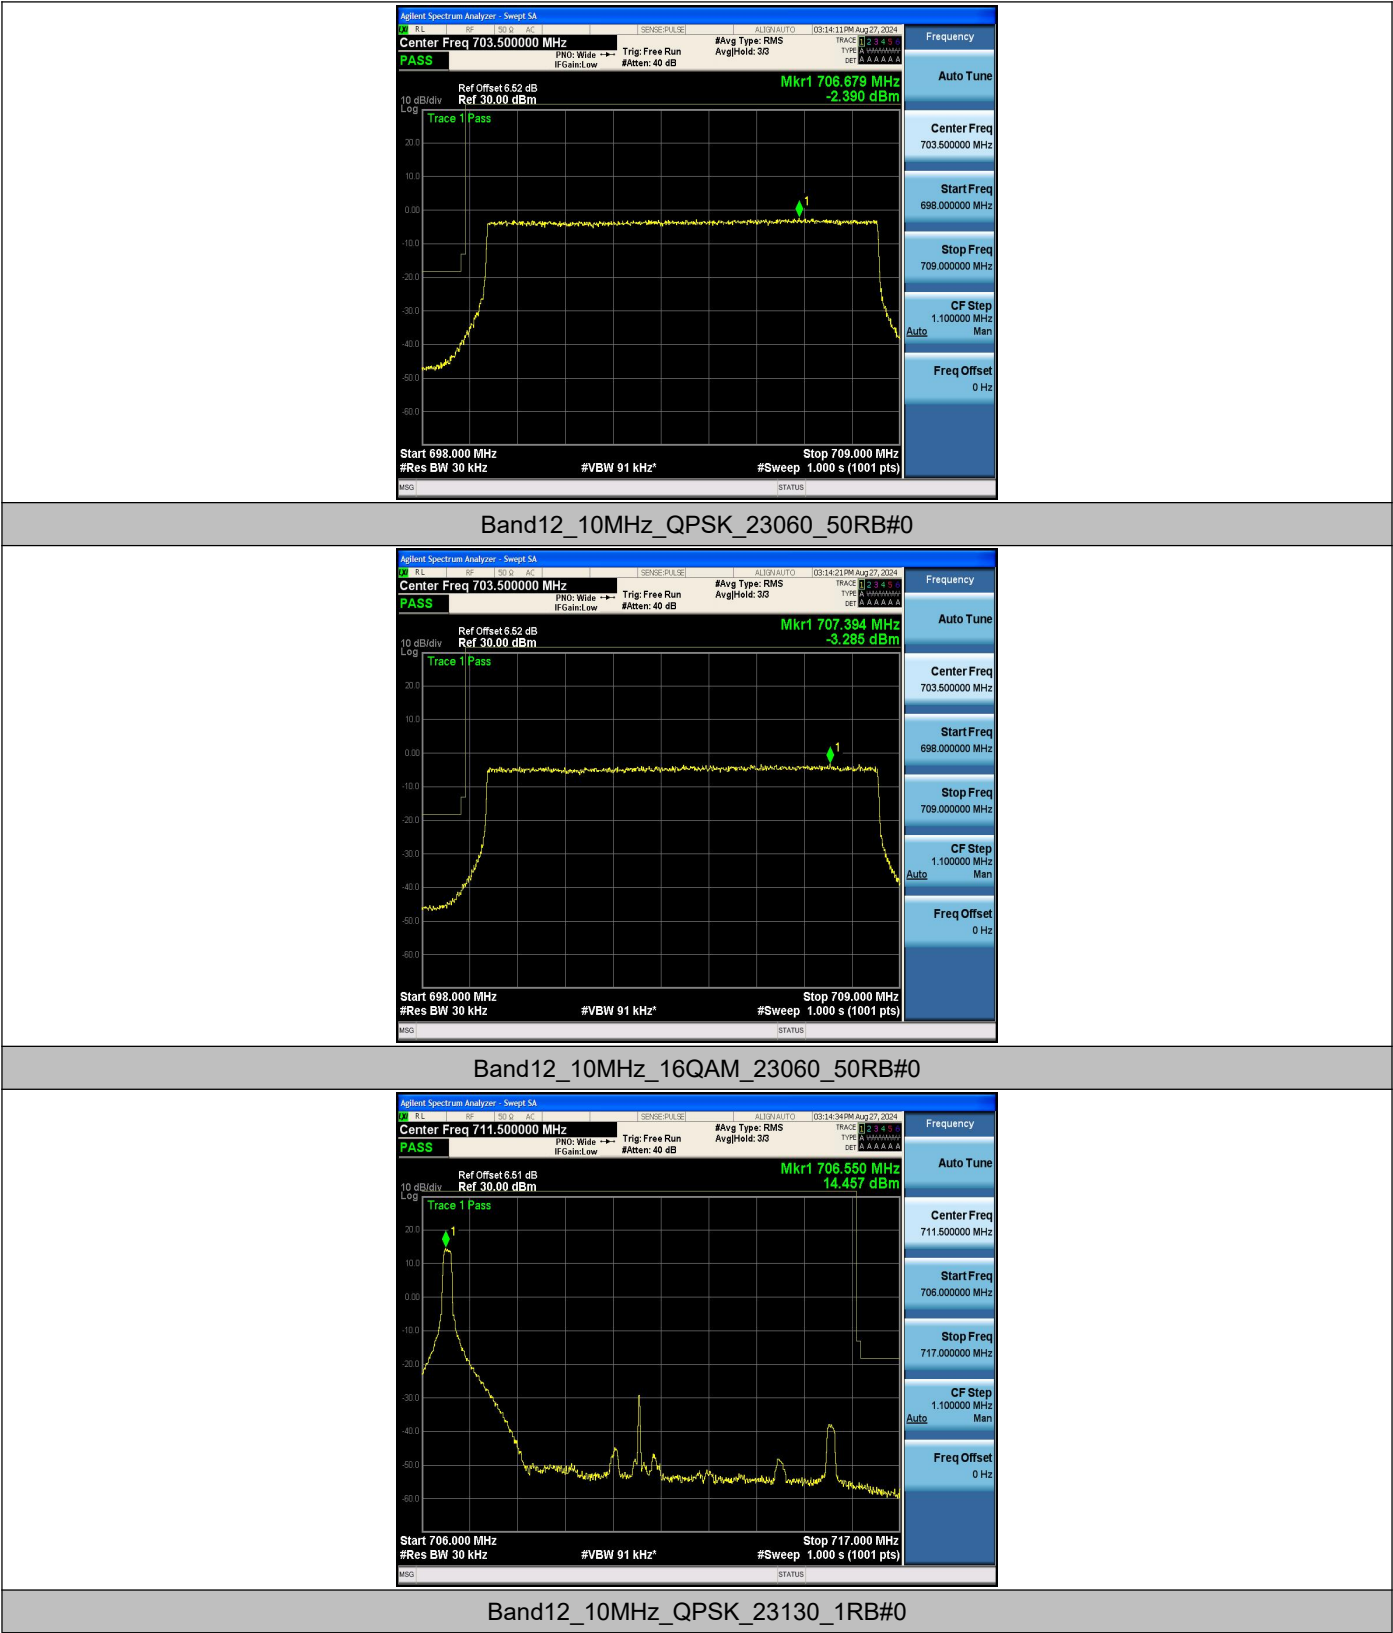

Agilent Spectrum Analyzer - Sweep SA

Center Freq 711.500000 MHz

PASS

Ref Offset 6.51 dB

Ref 30.00 dBm

Trace 1 Pass

Start 706.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 711.500000 MHz

Start Freq 706.000000 MHz

Stop Freq 717.000000 MHz

CF Step 1.100000 MHz


Auto


Freq Offset 0 Hz

Mkr1 706.550 MHz

14.457 dBm

Band12_10MHz_QPSK_23130_1RB#0

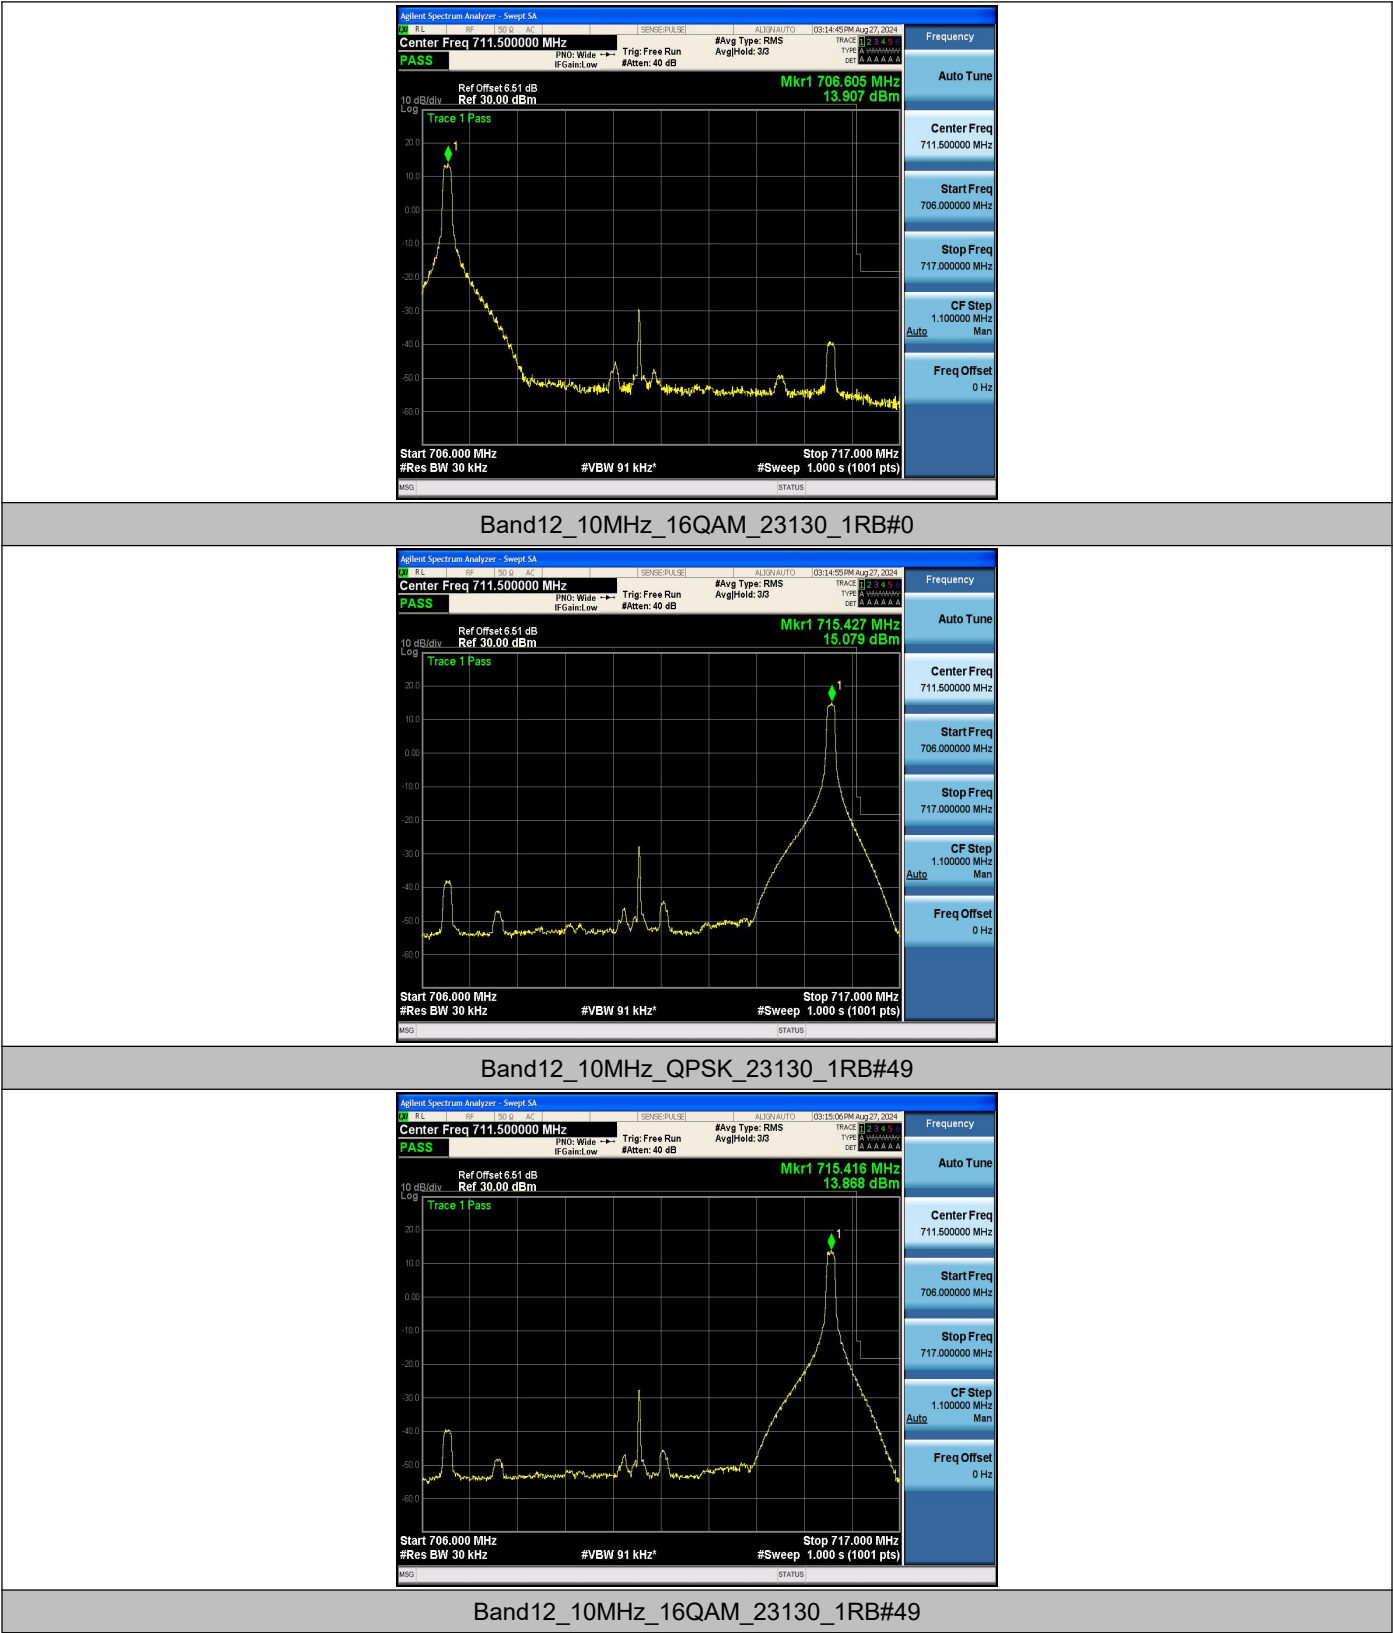

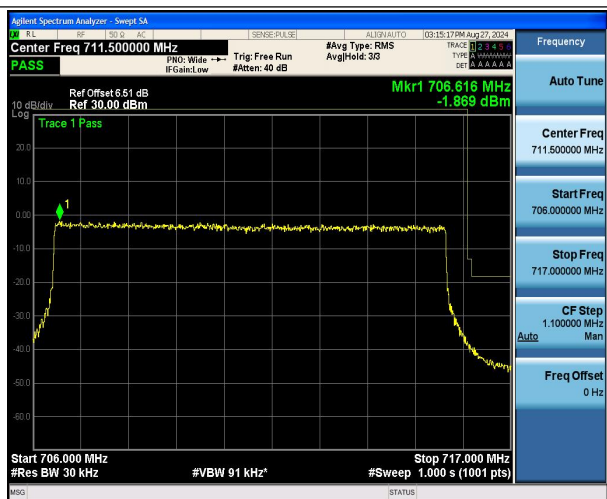


Band12_10MHz_QPSK_23130_50RB#0



Band12_10MHz_16QAM_23130_50RB#0



Band17_5MHz_16QAM_23825_25RB#0

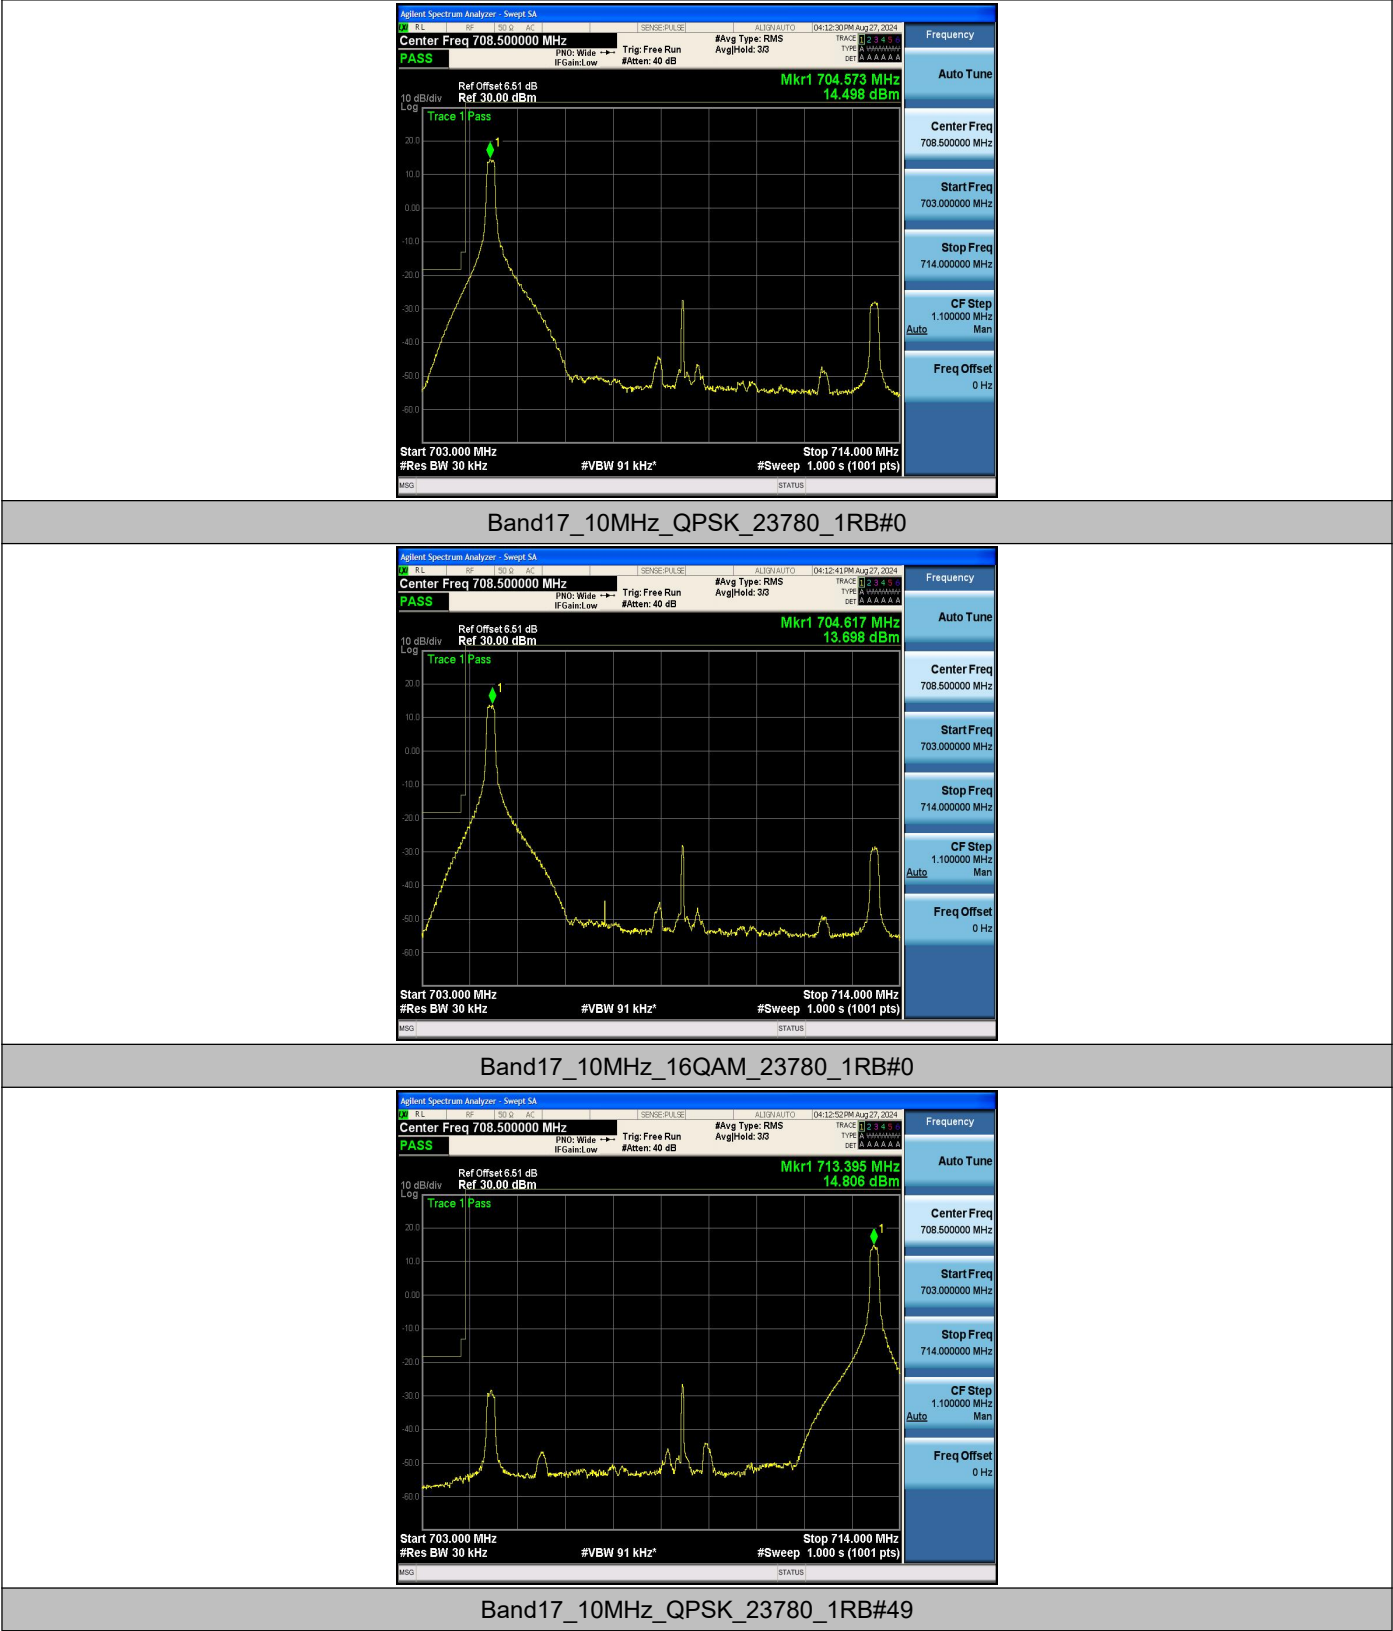

Agilent Spectrum Analyzer - Swept SA

Center Freq 708.500000 MHz

PASS

Ref Offset 6.51 dB

Ref 30.00 dBm

Trace 1 Pass

Start 703.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 708.500000 MHz

Start Freq 703.000000 MHz

Stop Freq 714.000000 MHz

CF Step 1.100000 MHz


Auto


Freq Offset 0 Hz

Mkr1 713.395 MHz


14.806 dBm

Band17_10MHz_QPSK_23780_1RB#49

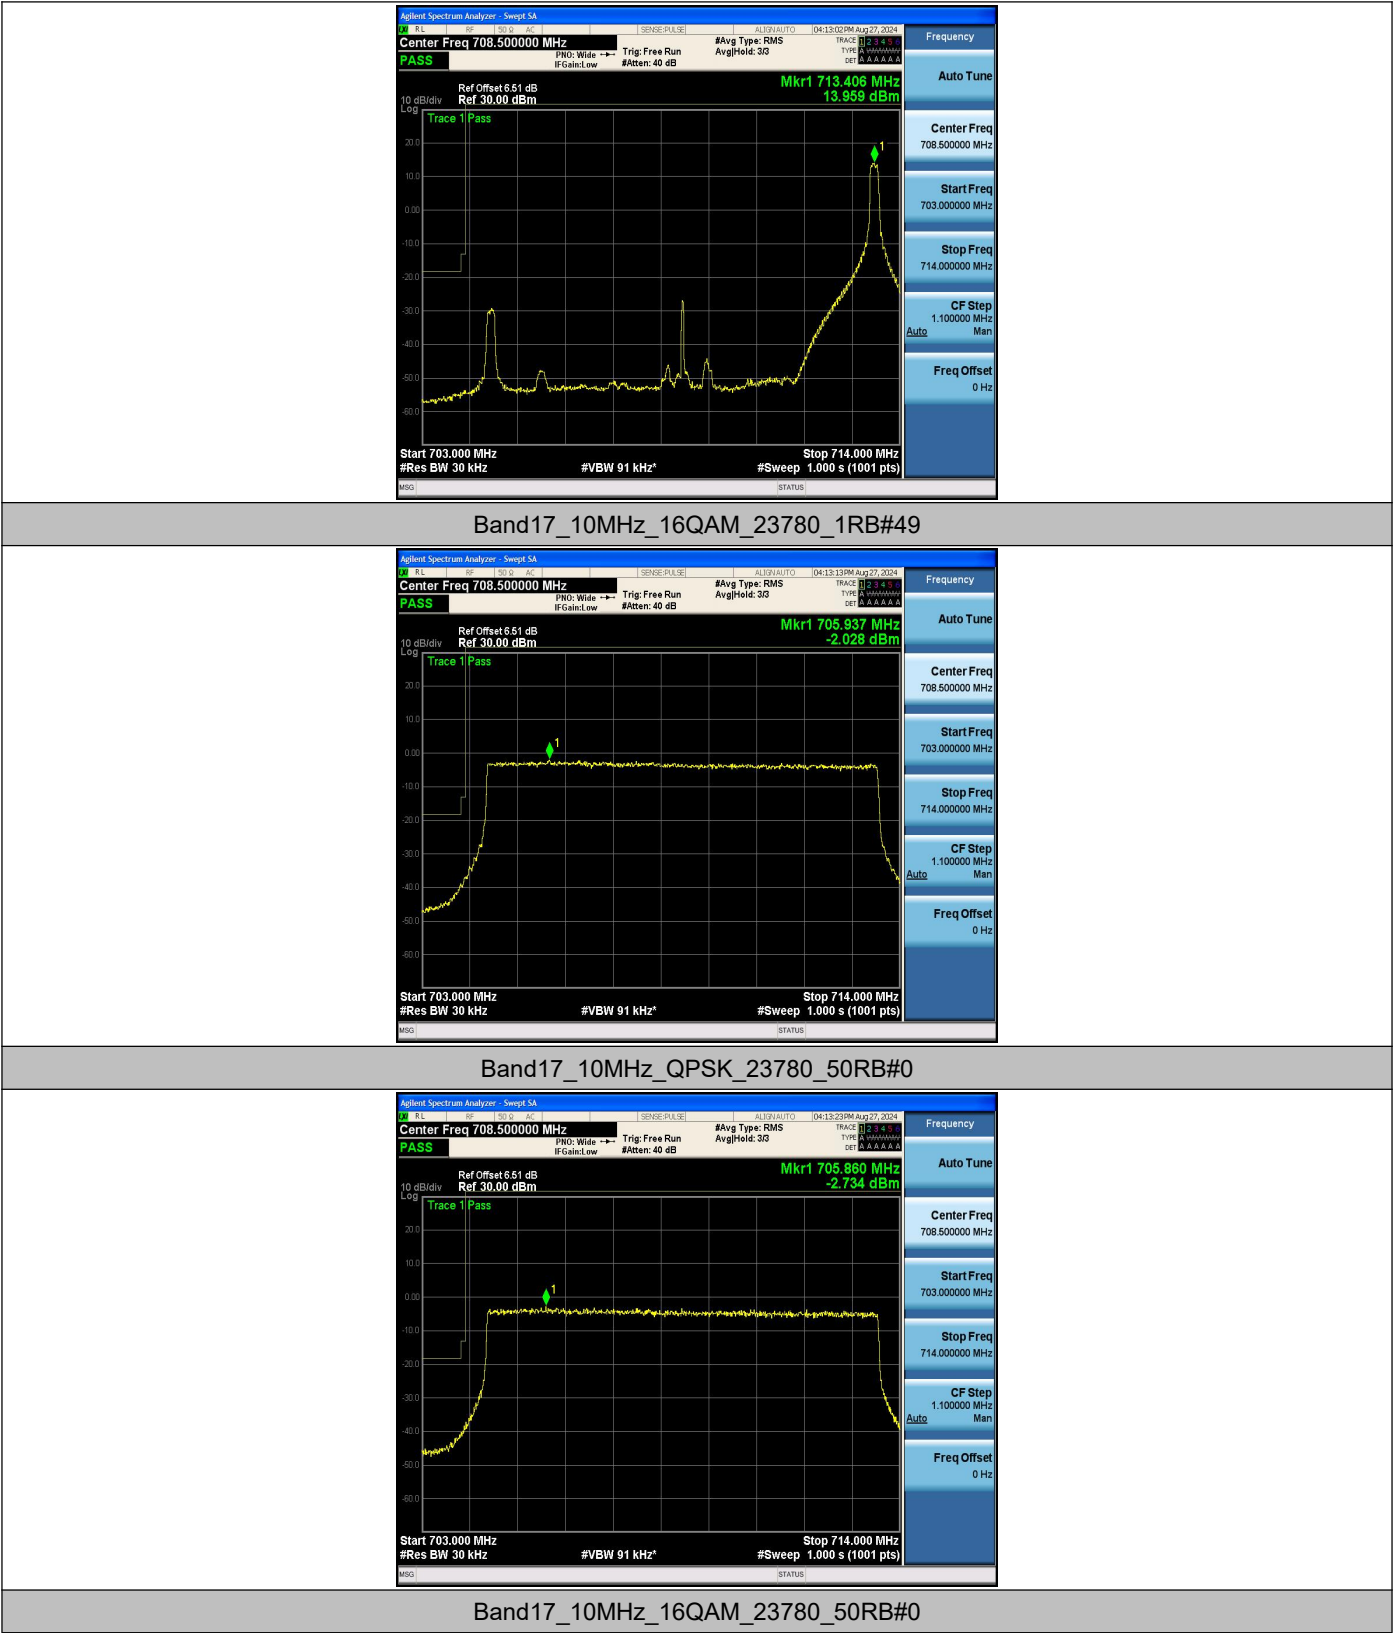


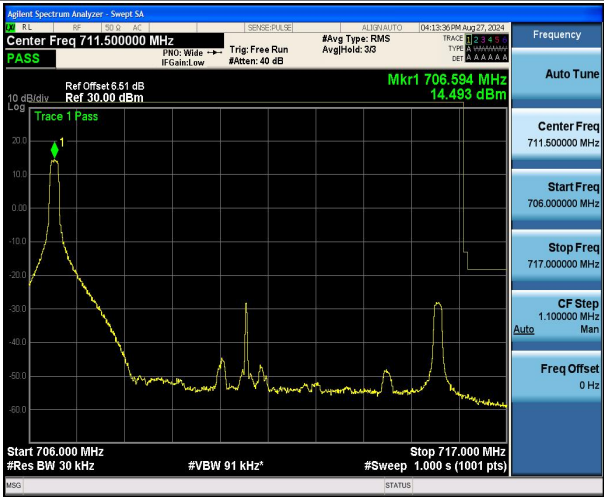


Band17_10MHz_QPSK_23800_1RB#0

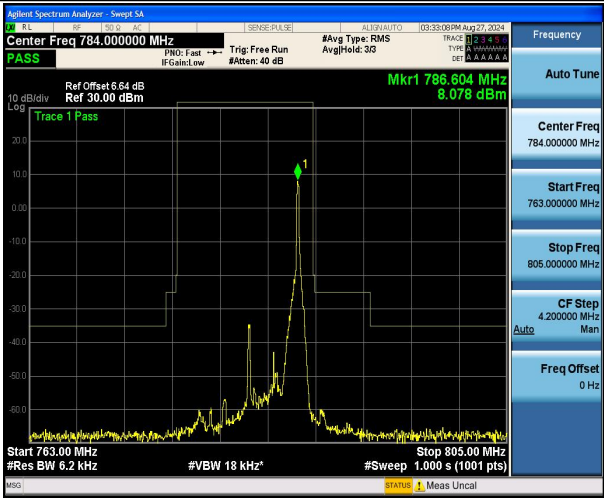



Band13_5MHz_QPSK_23255_1RB#24

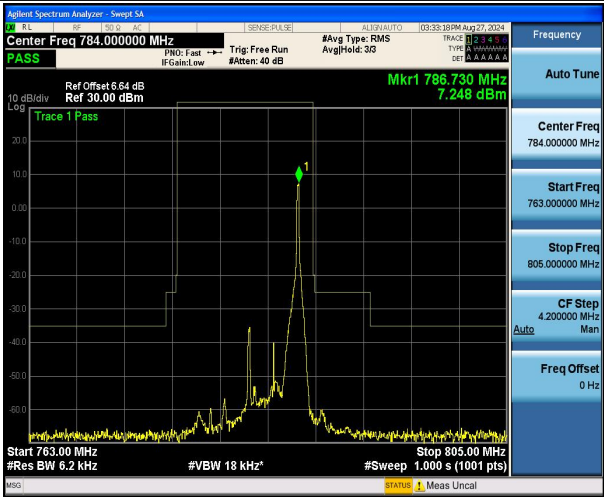

Band13_5MHz_16QAM_23255_1RB#24

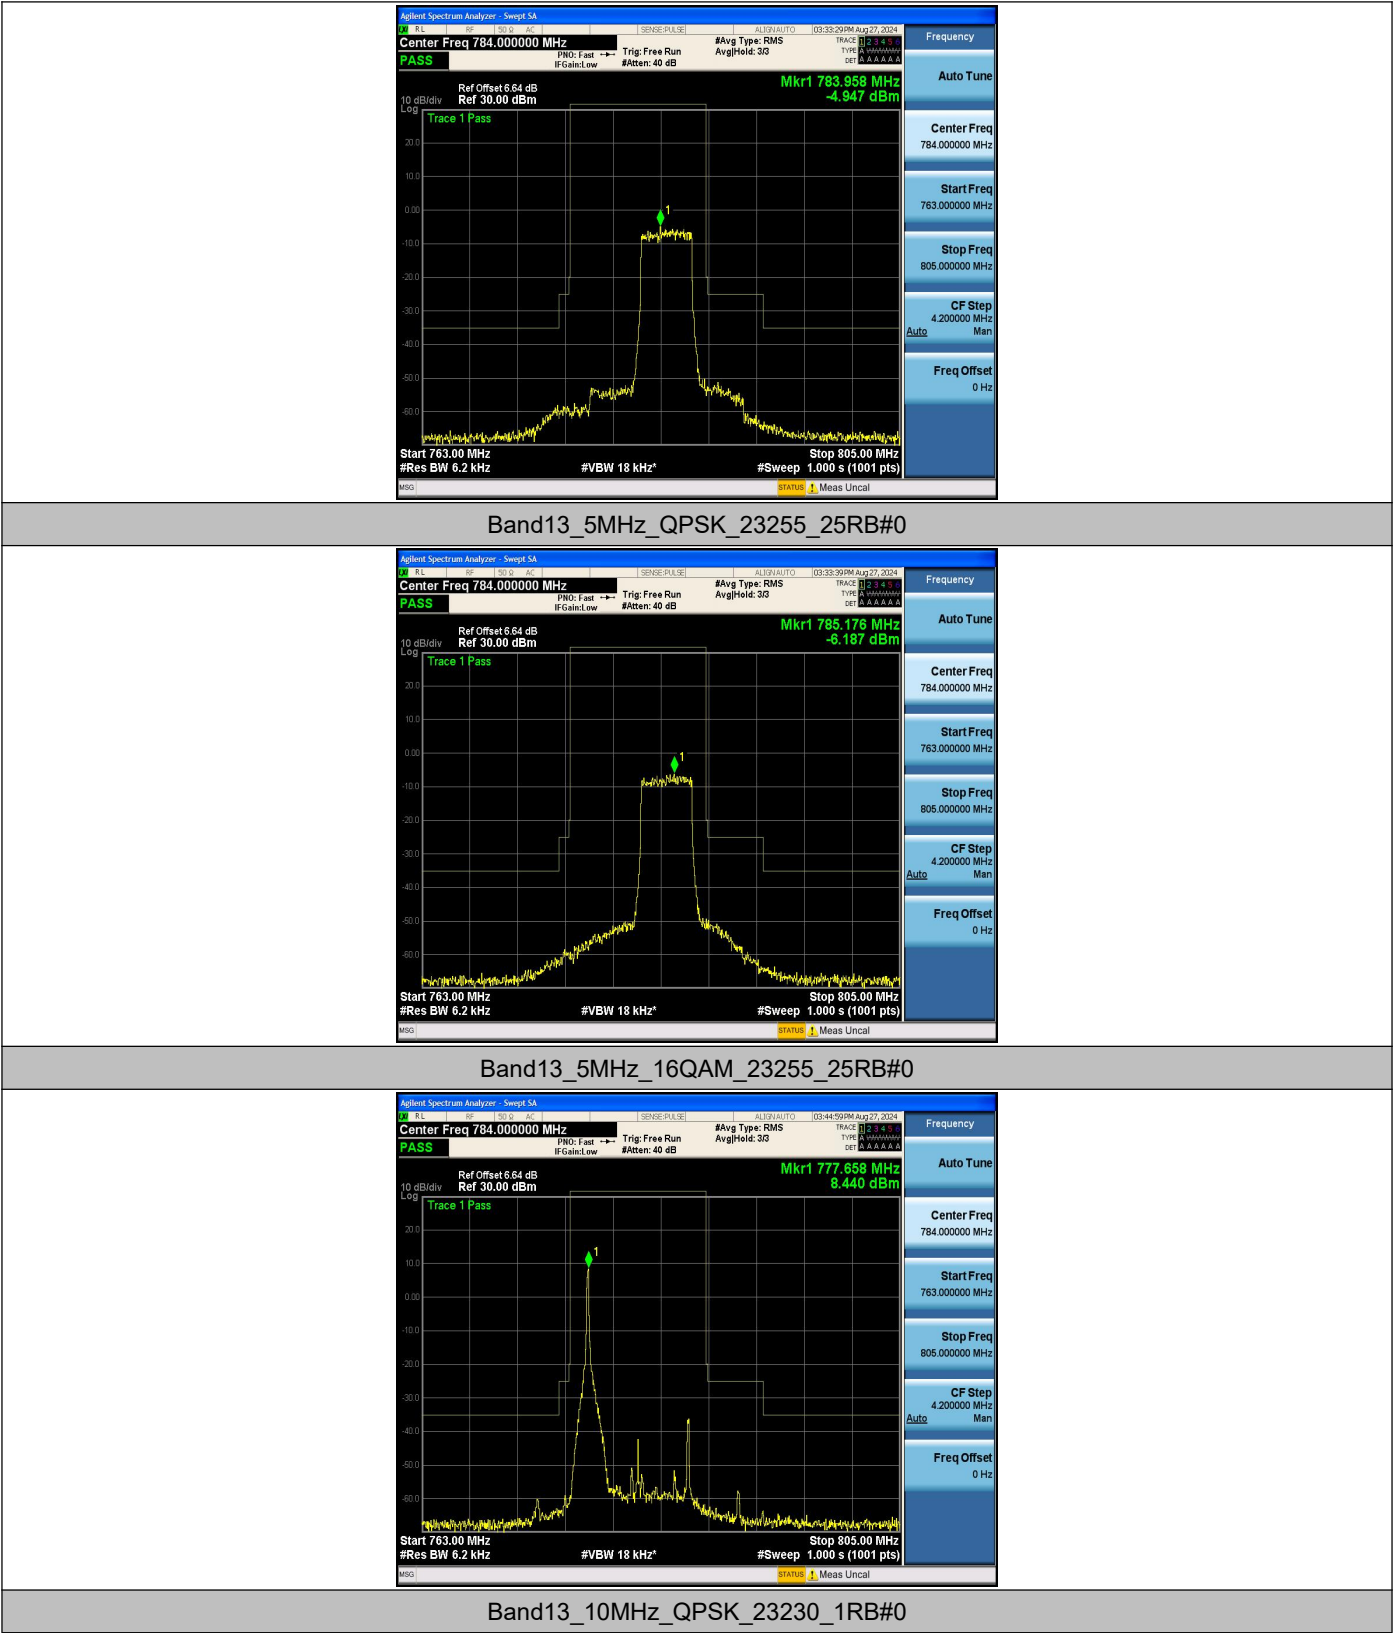

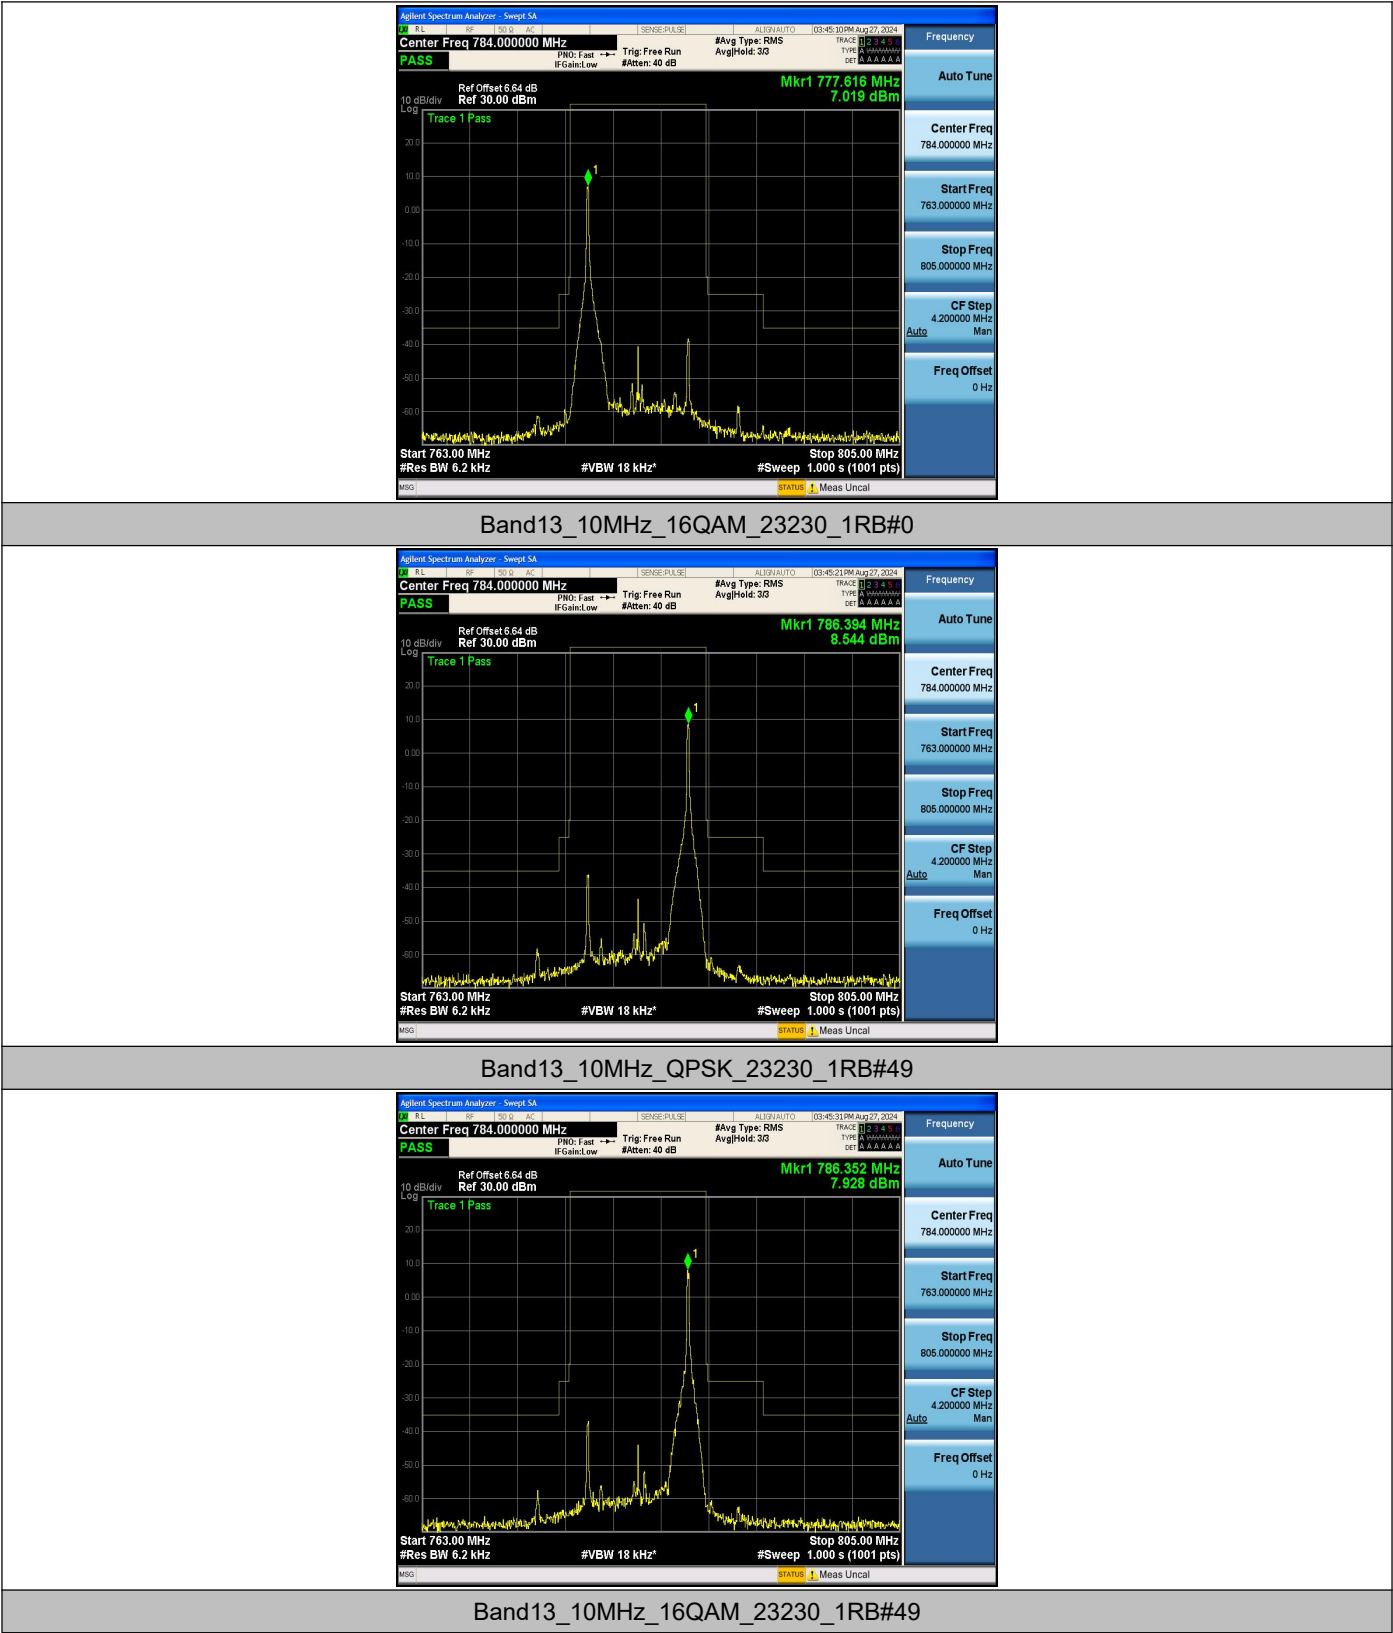

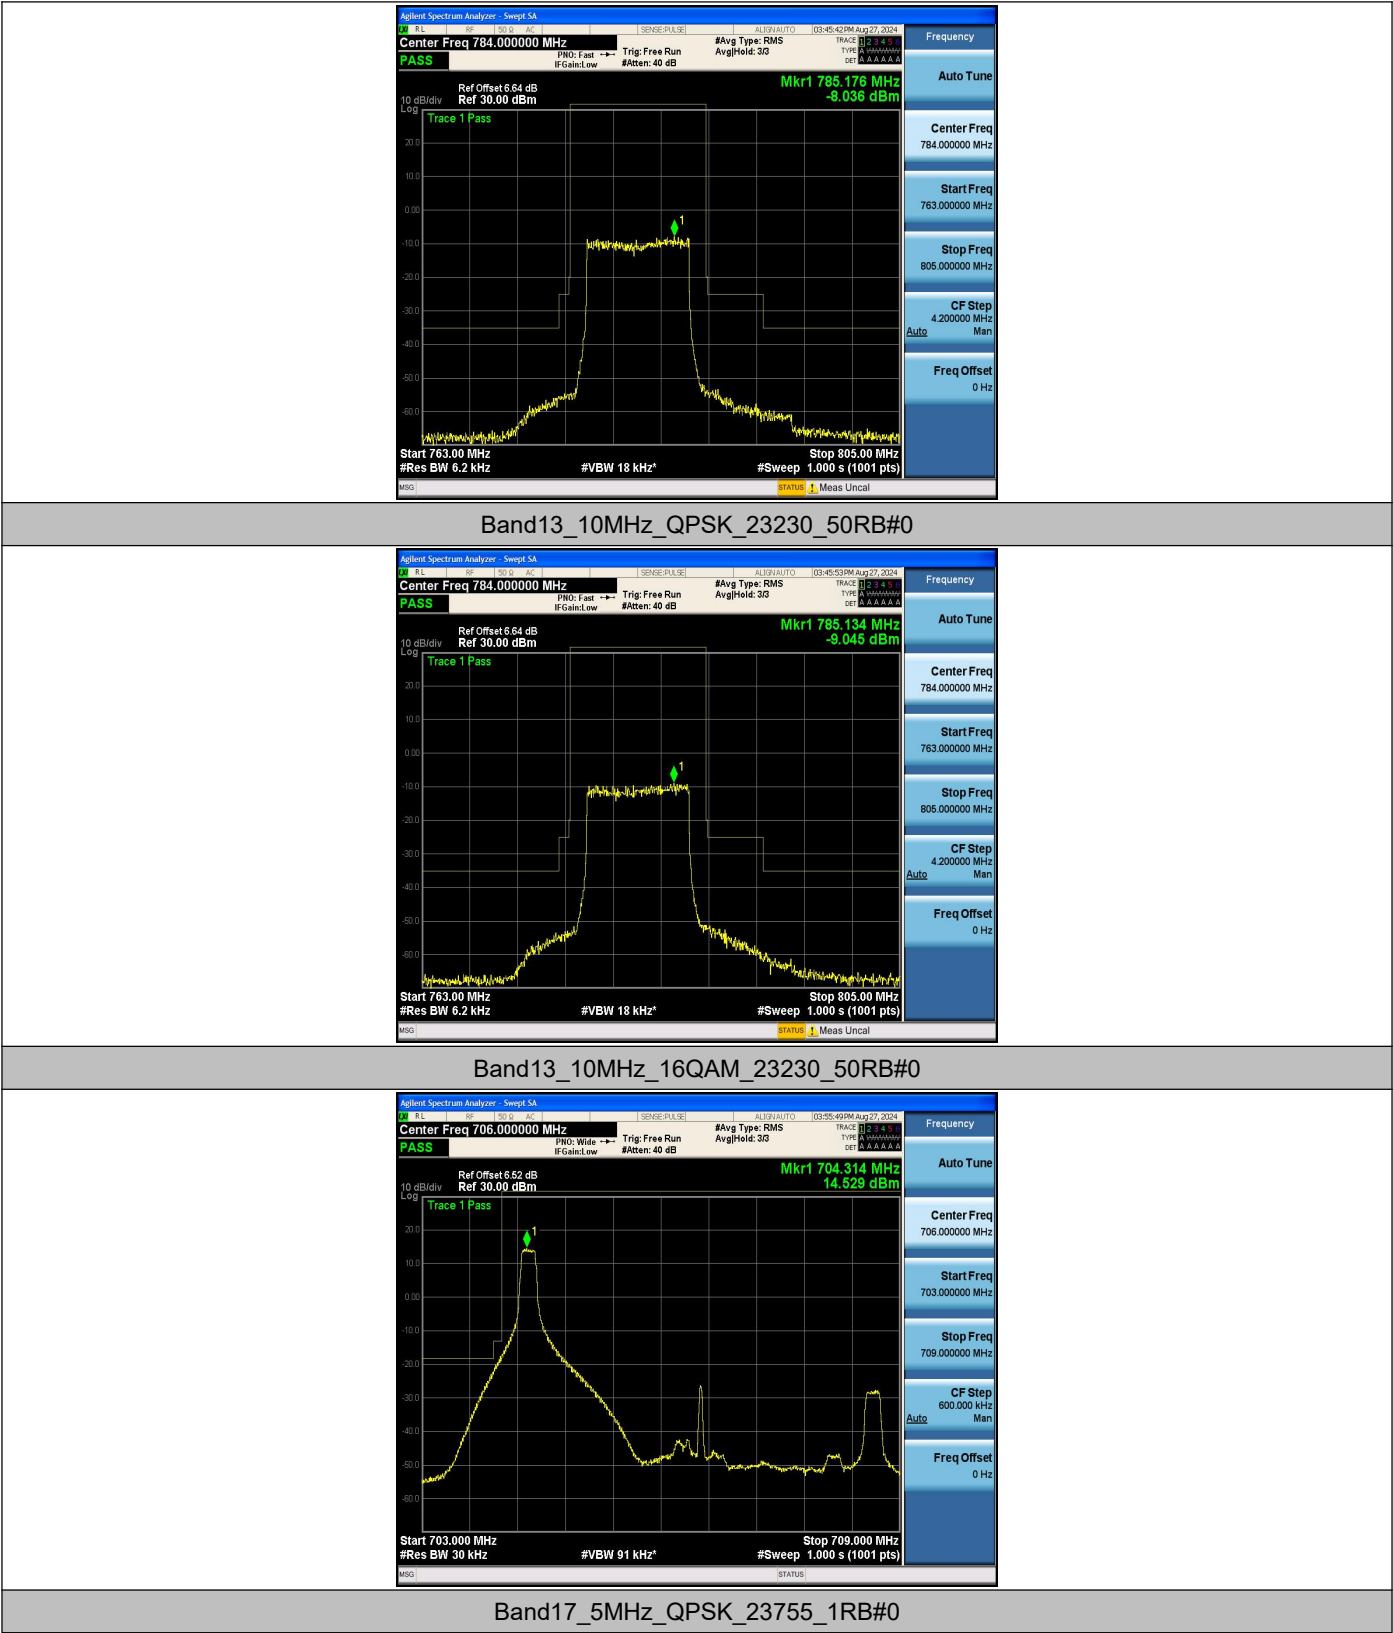

Agilent Spectrum Analyzer - Sweep SA

AL

SENSE (PLA SE)

AL (10) AUTO

03-55:49 PM Aug 27, 2024

Center Freq 706.000000 MHz

PASS

PRD: Wide

IF Gain: Low

Trig: Free Run

#Atten: 40 dB

#Avg Type: RMS

Avg Hold: 30

TRACE 1 3 1

TYPE A

DEF A

Ref Offset 6.52 dB

Ref 30.00 dBm

Mkr1 704.314 MHz

14.529 dBm

10 dB/div

Log

Trace 1 Pass

Start 703.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 709.000 MHz

#Sweep 1.000 s (1001 pts)

MSG

STATUS

Meas Uncal

Frequency

Auto Tune

Center Freq
706.000000 MHz


Start Freq
703.000000 MHz

Stop Freq
709.000000 MHz

CF Step
600.000 kHz
Auto Man

Freq Offset
0 Hz

Band17_5MHz_QPSK_23755_1RB#0

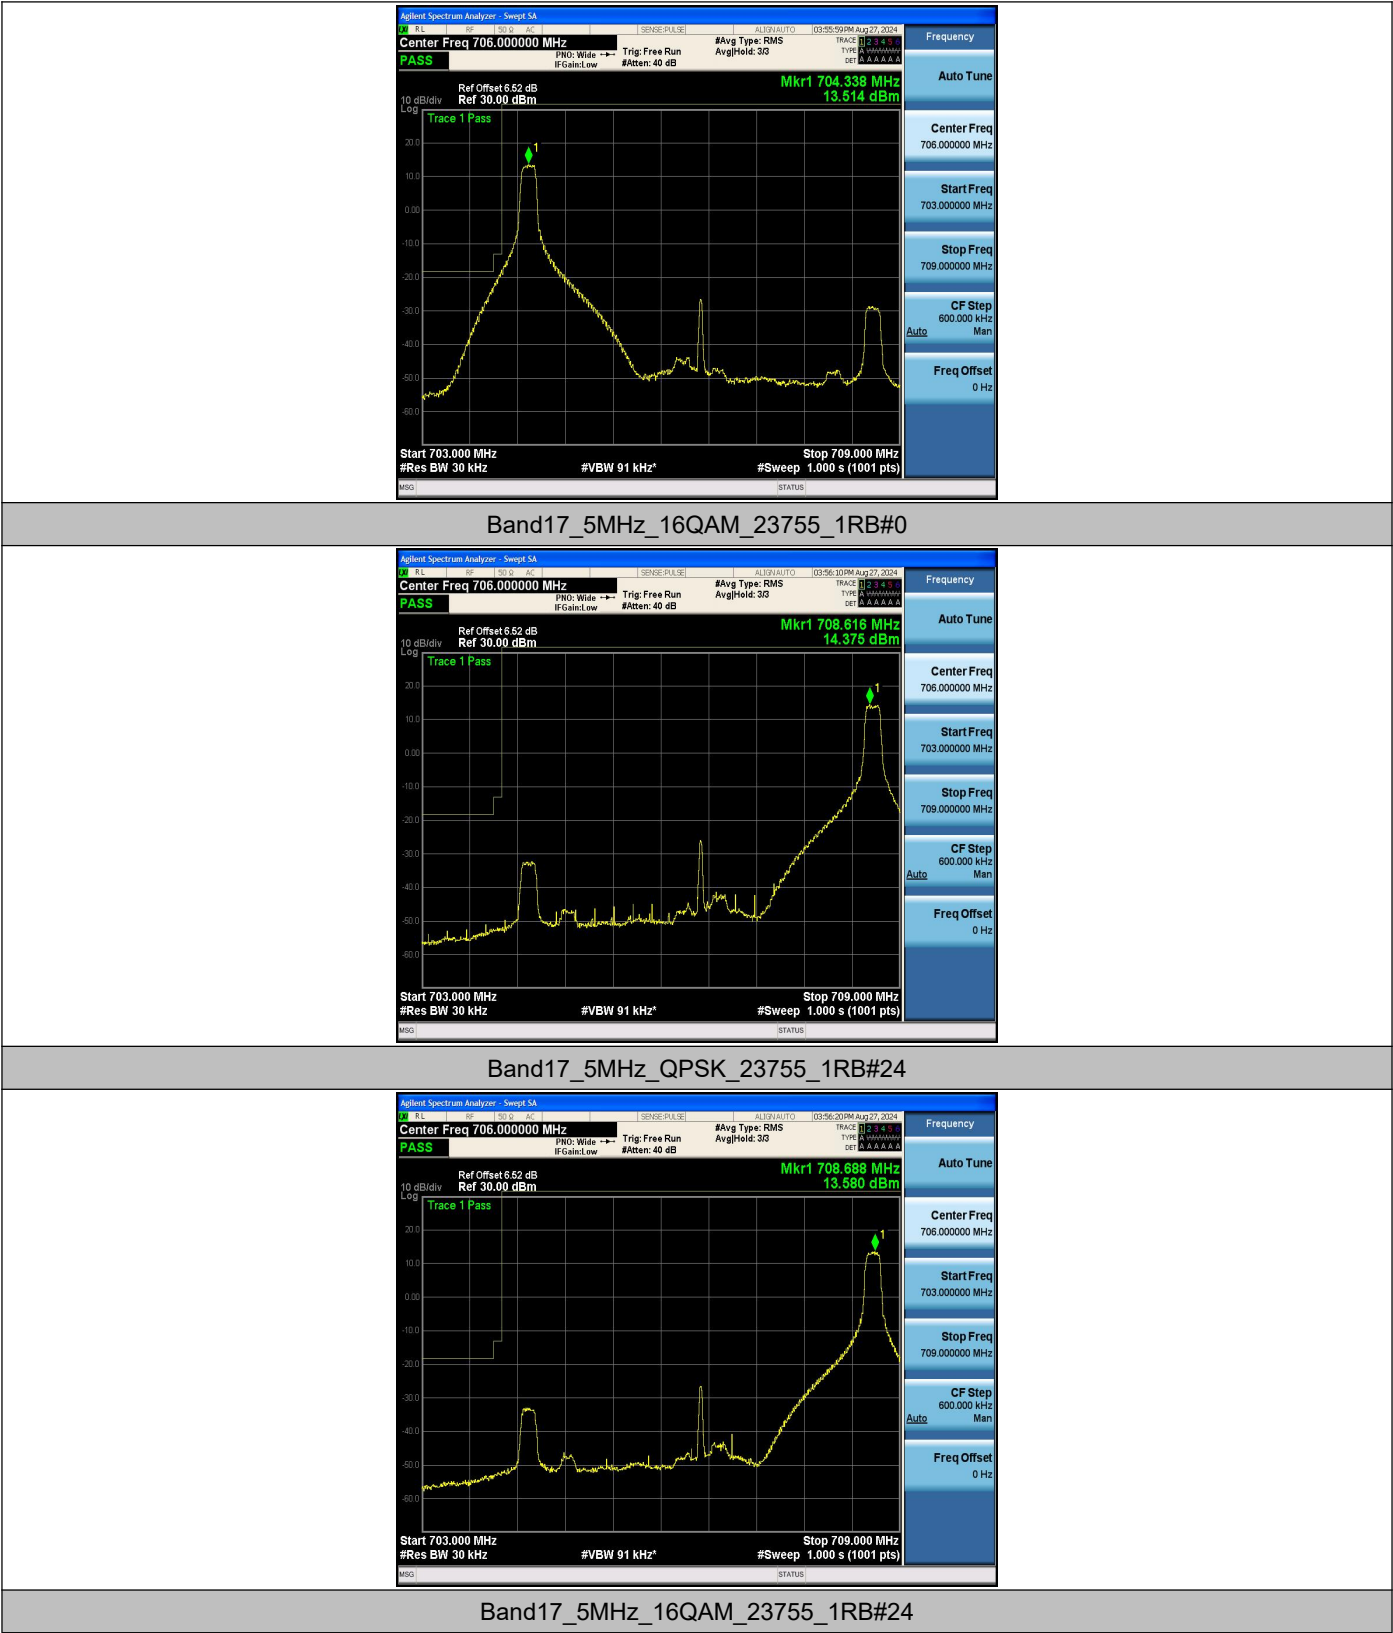

Agilent Spectrum Analyzer - Sweep SA

Center Freq 706.000000 MHz

PASS

Ref Offset 6.52 dB

Ref 30.00 dBm

Trace 1 Pass

Start 703.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 709.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 706.000000 MHz

Start Freq 703.000000 MHz

Stop Freq 709.000000 MHz


CF Step 600.000 kHz

Auto


Freq Offset 0 Hz

Mkr1 708.688 MHz

13.580 dBm

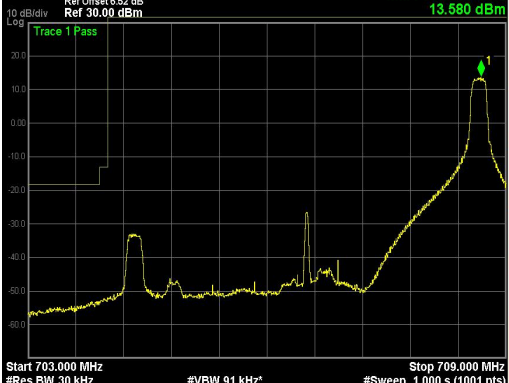

Band17_5MHz_16QAM_23755_1RB#24

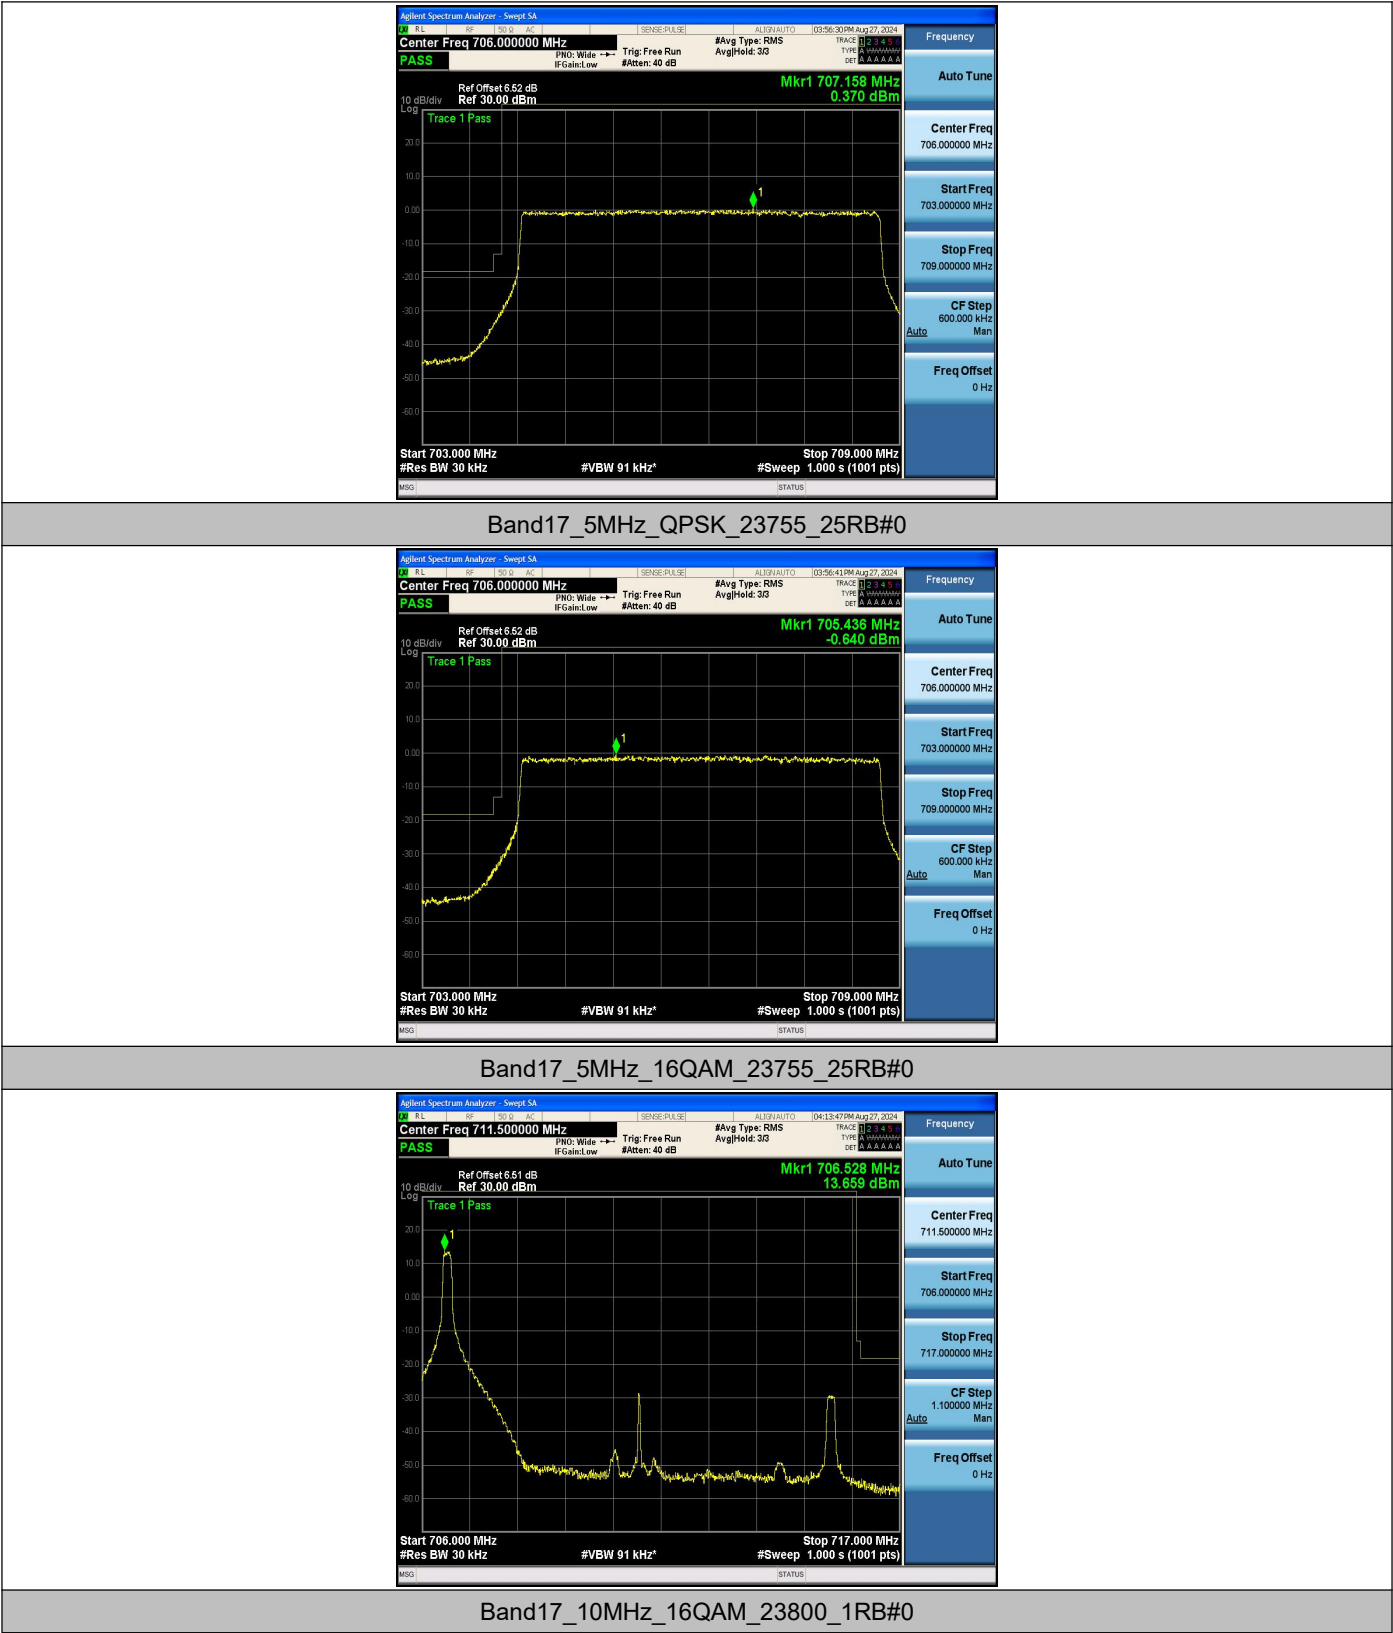

Agilent Spectrum Analyzer - Sweep SA

Center Freq 711.500000 MHz

PASS

Ref Offset 6.51 dB

Ref 30.00 dBm

Trace 1 Pass

Start 706.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 711.500000 MHz

Start Freq 706.000000 MHz

Stop Freq 717.000000 MHz

CF Step 1.100000 MHz

Auto


Freq Offset 0 Hz

Mkr1 706.528 MHz

13.659 dBm

1

Band17_10MHz_16QAM_23800_1RB#0

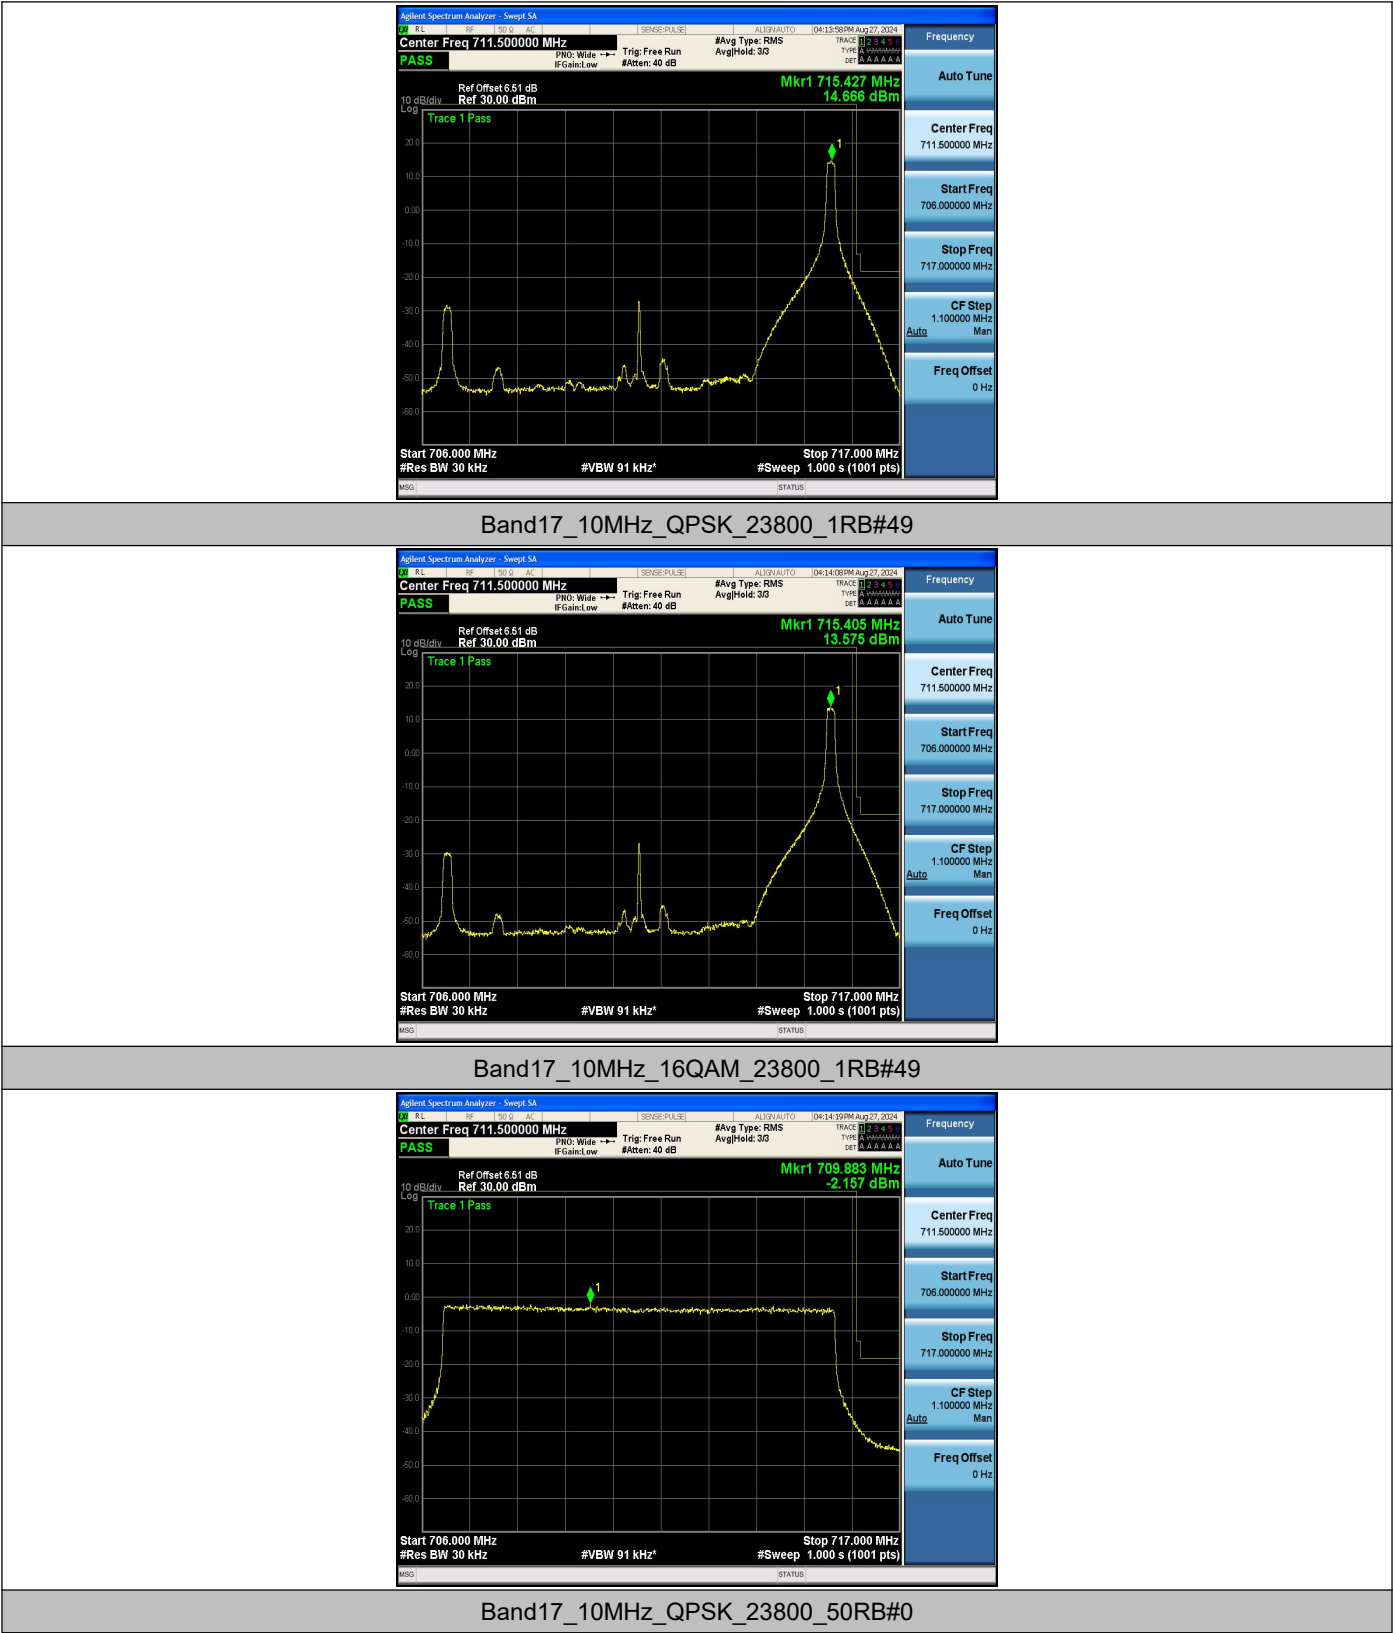

Agilent Spectrum Analyzer - Sweep SA

Center Freq 711.500000 MHz

PASS

Ref Offset 6.51 dB

Ref 30.00 dBm

Trace 1 Pass

Start 706.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 717.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 711.500000 MHz

Start Freq 706.000000 MHz

Stop Freq 717.000000 MHz

CF Step 1.100000 MHz

Auto

Freq Offset 0 Hz

Mkr1 709.883 MHz

-2.167 dBm

Trace 1 Pass

Band17_10MHz_QPSK_23800_50RB#0

