

APPENDIX B: SYSTEM VERIFICATION PLOTS

ELEMENT

DUT: Dipole 6500.0 MHz; Type: D6.5GHzV2 - SN1018

Communication System: UID: 0, CW; Frequency: 6500.0 MHz
Medium: 6000 Head; Medium parameters used:
f = 6500.0 MHz; cond = 6.11 S/m; perm = 33.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 5 mm

Test Date: 07/12/2023; Ambient Temp: 24.0°C; Tissue Temp: 22.1°C

Probe: EX3DV4 - SN7718; ConvF:(5.15,5.15,5.15); Calibrated: 2023-04-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1368; Calibrated: 2023-04-14
Phantom: Twin-SAM V5.0; Serial: 1759
Measurement SW: DASY Module SAR V16.2.0.1425

6500.0 MHz System Verification at 14.0 dBm (25 mW)


Area Scan (51.0 x 85.0): Measurement grid: dx=8.5 mm, dy=8.5 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=3.4 mm, dy=3.4 mm, dz=1.4 mm; Graded
Ratio: 1.4

Peak SAR (extrapolated) = 45.4 W/kg

SAR(1 g) = 7.11 W/kg; SAR(10 g) = 1.32 W/kg; APD(4 cm²) = 32.2 W/m²

Deviation (1 g) = -2.94%; Deviation (10 g) = -2.40%; Deviation (4 cm²) = -1.68%

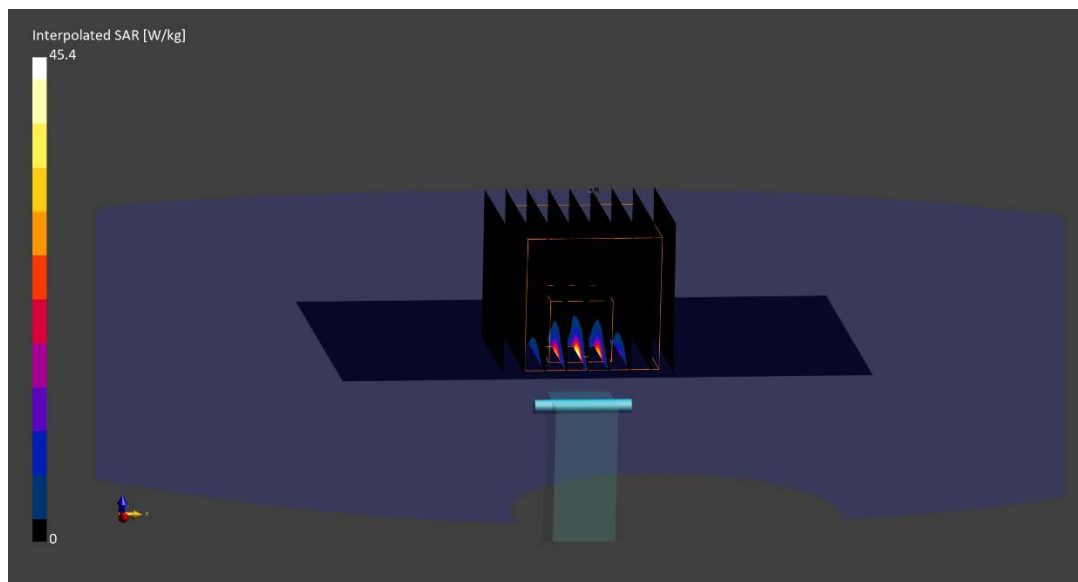

ELEMENT

DUT: Dipole 6500.0 MHz; Type: D6.5GHzV2 - SN1018

Communication System: UID: 0, CW; Frequency: 6500.0 MHz
Medium: 6000 Head; Medium parameters used:
f = 6500.0 MHz; cond = 6.01 S/m; perm = 33.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 5 mm

Test Date: 07/16/2023; Ambient Temp: 22.0°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN7718; ConvF:(5.15,5.15,5.15); Calibrated: 2023-04-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1368; Calibrated: 2023-04-14
Phantom: Twin-SAM V5.0; Serial: 1759
Measurement SW: DASY Module SAR V16.2.0.1425

6500.0 MHz System Verification at 14.0 dBm (25 mW)


Area Scan (51.0 x 85.0): Measurement grid: dx=8.5 mm, dy=8.5 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=3.4 mm, dy=3.4 mm, dz=1.4 mm; Graded
Ratio: 1.4

Peak SAR (extrapolated) = 46.1 W/kg

SAR(1 g) = 7.09 W/kg; SAR(10 g) = 1.31 W/kg; APD(4 cm²) = 31.9 W/m²

Deviation (1 g) = -3.21%; Deviation (10 g) = -3.14%; Deviation (4 cm²) = -2.60%

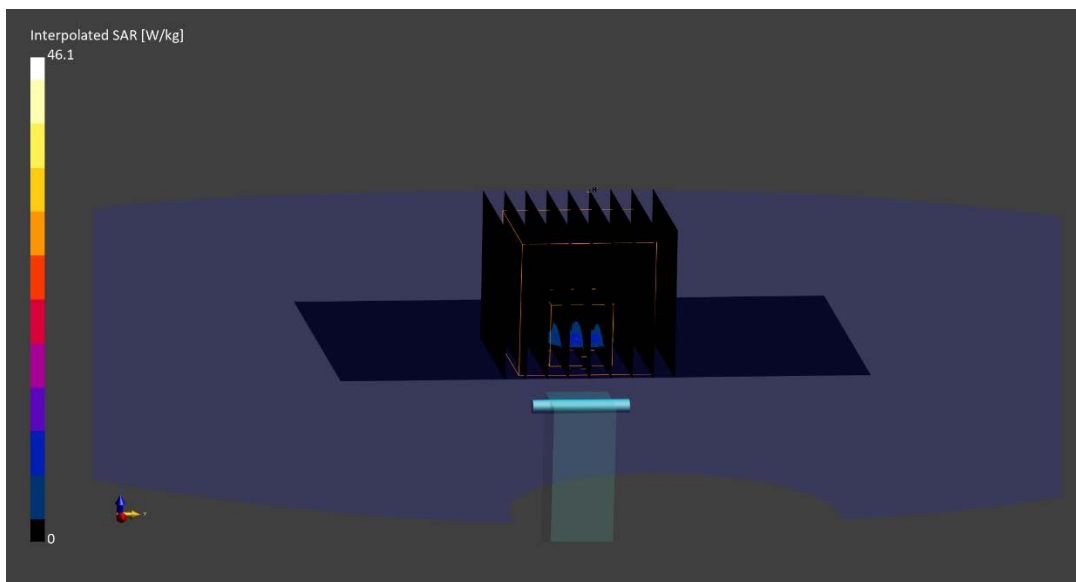

Date: 2023-07-06

10 GHz System Verification

Device Under Test Properties

DUT	Serial Number
10 GHz Verification Source	1004

Exposure Conditions

Phantom Section	Position	Test Distance [mm]	Band	Frequency [MHz]
5G	FRONT	10.00	CW	10000.0

Hardware/Software Setup

Probe, Calibration Date	DAE, Calibration Date	Software	Software Version
EUmmWV3 – SN9407, 2022-10-17	DAE4ip – SN1638, 2022-10-13	cDASY6 Module mmWave	3.2.0.1840

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	120.0 x 120.0
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.0

Measurement Results

Scan Type	5G Scan
Avg. Area [cm²]	4.00
pS _{tot} avg [W/m²]	55.4
pS _n avg [W/m²]	55.3
E _{peak} [V/m]	153
Deviation [dB] pS _{tot}	0.50
Deviation [dB] pS _n	0.49

