

System Performance Check Report for D2450V2 - SN939

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2450.000	TSL Permittivity	40.2
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.76
Conversion Factor	6.92	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7313 2025-02-24	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1667 2025-03-19	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	5.32	5.15
psSAR10g [W/Kg]	2.48	2.41
Power Drift [dB]		-0.10
Dist 3dB Peak [mm]		9.0
M2/M1 [%]		80.7

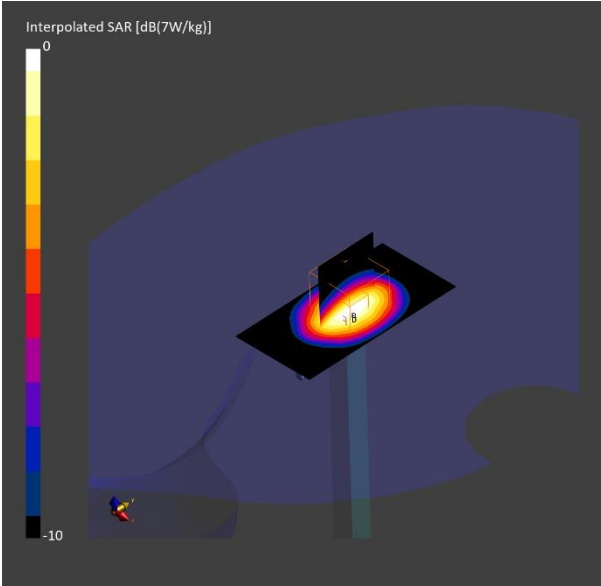

System Performance Check Report for D5GHzV2 - SN1184

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	5800.000	TSL Permittivity	35.2
Group / UID	CW / 0--	TSL Conductivity [S/m]	5.37
Conversion Factor	4.96	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration

Probe Calibration Date	EX3DV4 - SN7313 2025-02-24	Phantom	Twin-SAM V8.0 (30deg probe tilt)
DAE Calibration Date	DAE4 Sn1667 2025-03-19	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	7.47	8.23
psSAR10g [W/Kg]	2.14	2.37
Power Drift [dB]		-0.01
Dist 3dB Peak [mm]		7.6
M2/M1 [%]		58.1

