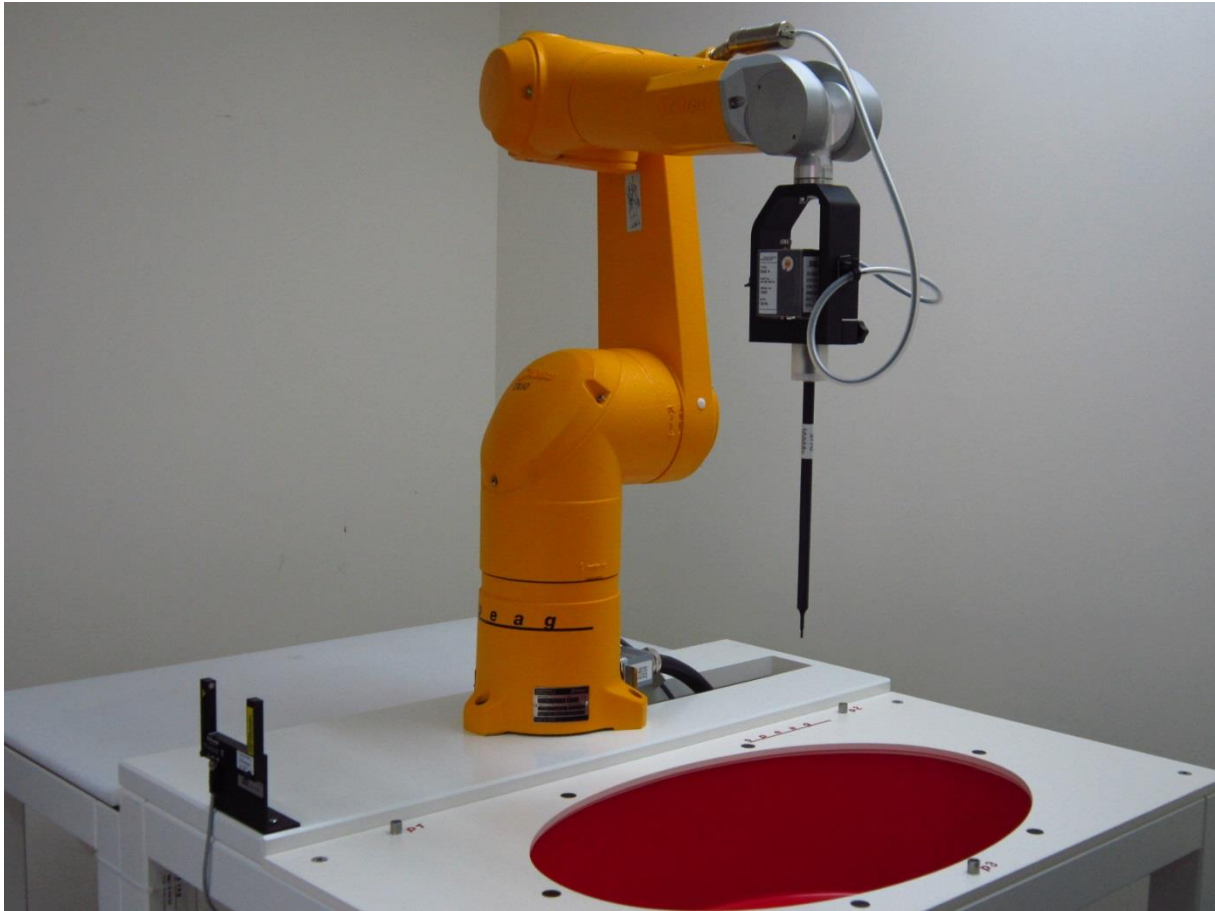


Appendix D






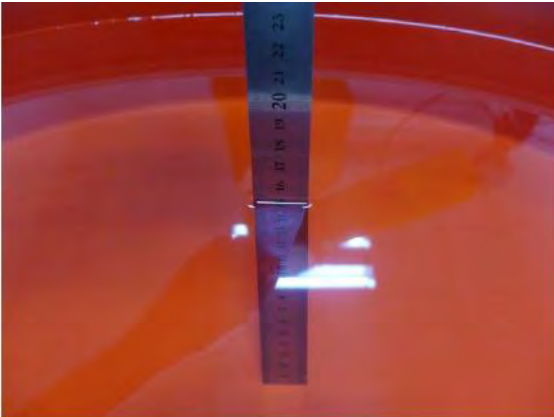
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

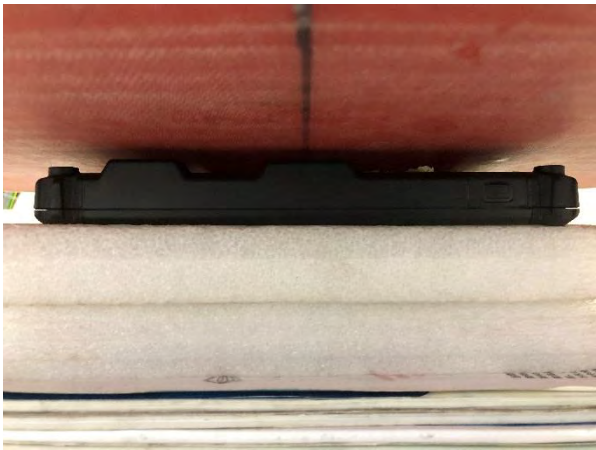
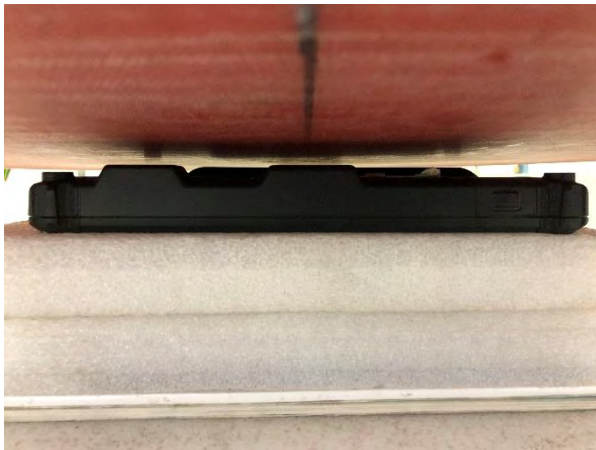
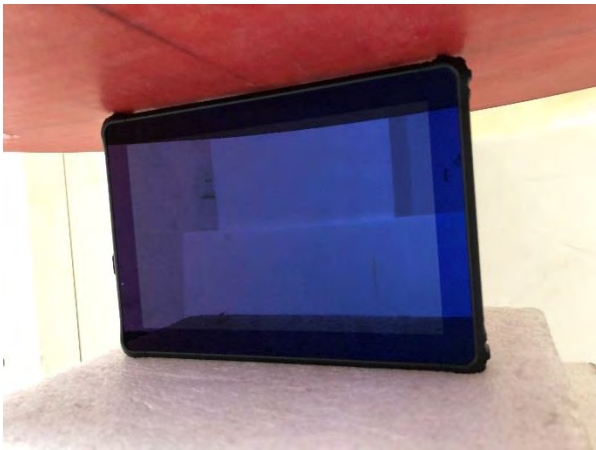



1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1800	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 5GHz
	

3. Photographs of EUT test position

Photo 7: Bottom Face 0mm	Photo 8: Bottom Face 4mm
	
Photo 9: Edge 1 0mm	Photo 10: Edge 3 0mm
	
Photo 11: Edge 2 0mm	Photo 12: Edge 2 4mm
	

4. EUT Constructional Details


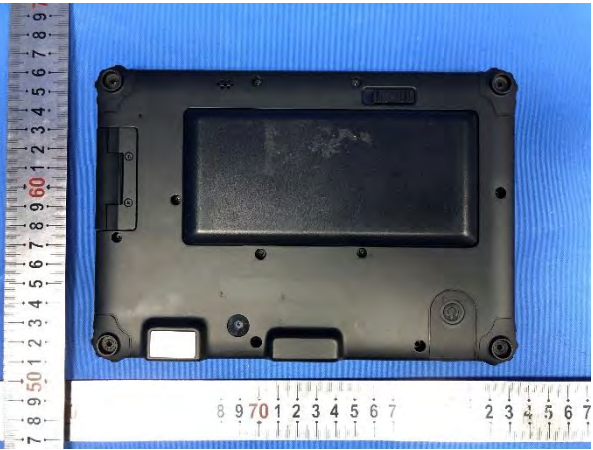




<p>Photo 13: Front View</p>	<p>Photo 14: Back View</p>
	
<p>Photo 15: Left View</p>	<p>Photo 16: Right View</p>
	
<p>Photo 17: Top View</p>	<p>Photo 18: Bottom View</p>
	

Photo 19: Back View

