

20221022_System Performance Check D5GHzV2 SN 1209

Frequency: 5600 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

Medium parameters used: $f = 5600$ MHz; $\sigma = 4.946$ S/m; $\epsilon_r = 34.836$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1667; Calibrated: 4/27/2022
- Probe: EX3DV4 - SN7330; ConvF(4.95, 4.95, 4.95) @ 5600 MHz; Calibrated: 1/28/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (20deg probe tilt); Type: QD 000 P40 CD; Serial: 1751

Head/5.6 GHz, Pin=100mW/Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 19.2 W/kg


Head/5.6 GHz, Pin=100mW/Zoom Scan (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 67.26 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 29.9 W/kg

SAR(1 g) = 7.52 W/kg; SAR(10 g) = 2.19 W/kg

Maximum value of SAR (measured) = 17.2 W/kg

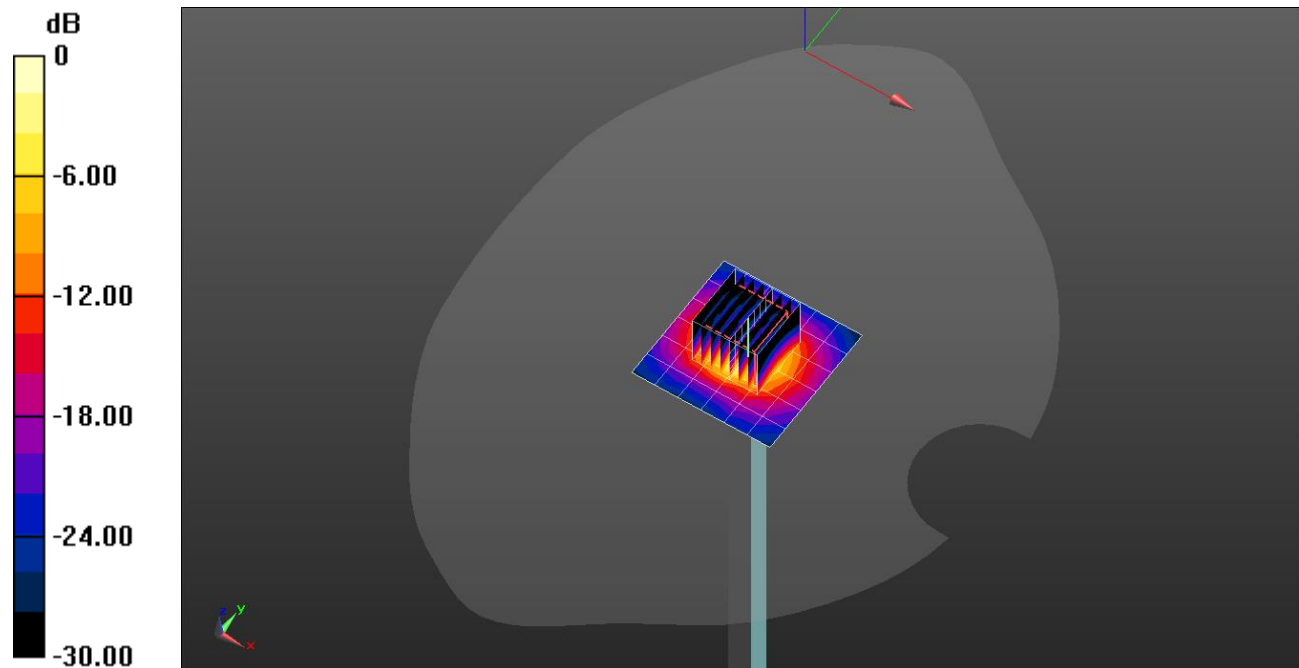

0 dB = 17.2 W/kg = 12.36 dBW/kg

20221021_System Performance check D2450V2 SN960

Frequency: 2450 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C
Medium parameters used (interpolated): $f = 2450$ MHz; $\sigma = 1.752$ S/m; $\epsilon_r = 40.708$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1668; Calibrated: 4/27/2022
- Probe: EX3DV4 - SN7646; ConvF(8.34, 8.34, 8.34) @ 2450 MHz; Calibrated: 3/29/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: SAM (20deg probe tilt) with CRP v5.0(Right); Type: QD000P40CD; Serial: TP:xxxx

Head/2450MHz/Pin=100mW/Area Scan (6x8x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 7.30 W/kg



Head/2450MHz/Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 60.38 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 10.1 W/kg

SAR(1 g) = 4.9 W/kg; SAR(10 g) = 2.31 W/kg

Maximum value of SAR (measured) = 8.15 W/kg

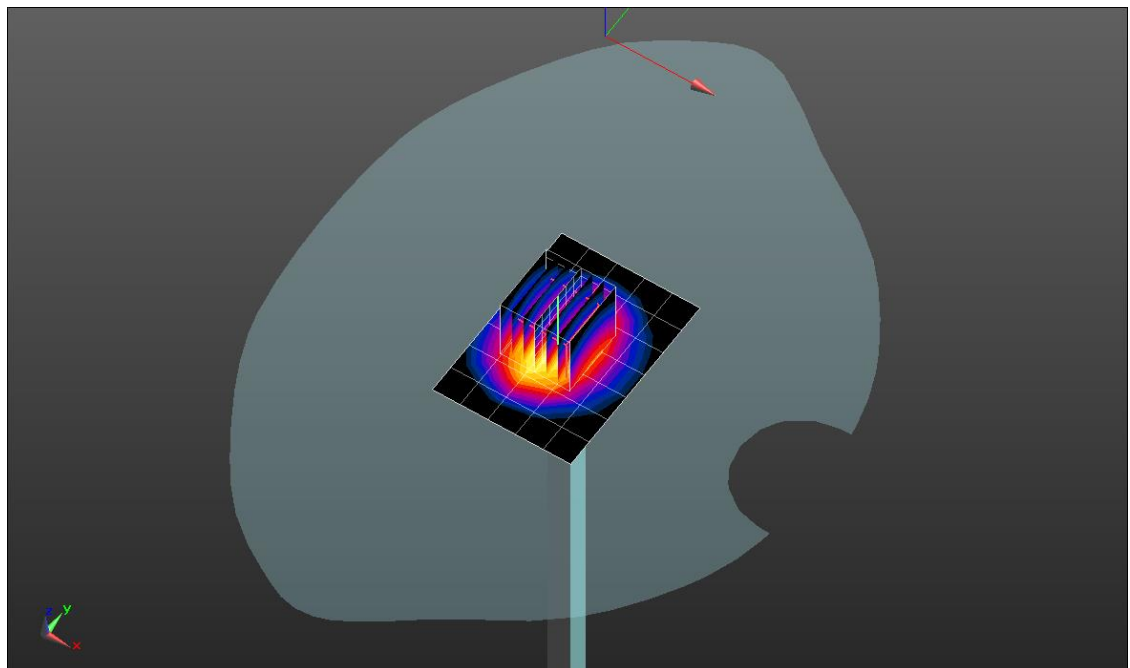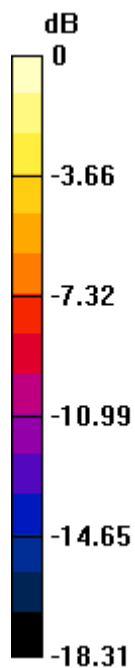

0 dB = 8.15 W/kg = 9.11 dBW/kg

20221003_System Performance Check D3500V2 SN1121

Frequency: 3500 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

Medium parameters used: $f = 3500$ MHz; $\sigma = 2.949$ S/m; $\epsilon_r = 39.225$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1671; Calibrated: 5/31/2022
- Probe: EX3DV4 - SN7313; ConvF(6.9, 6.9, 6.9) @ 3500 MHz; Calibrated: 3/2/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (Right); Type: QD 000 P40 CD; Serial: 1855

Head/3500MHz, Pin=100mW/Area Scan (5x7x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 11.5 W/kg


Head/3500MHz, Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=1.4mm

Reference Value = 67.66 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 16.5 W/kg

SAR(1 g) = 6.16 W/kg; SAR(10 g) = 2.35 W/kg

Maximum value of SAR (measured) = 12.0 W/kg

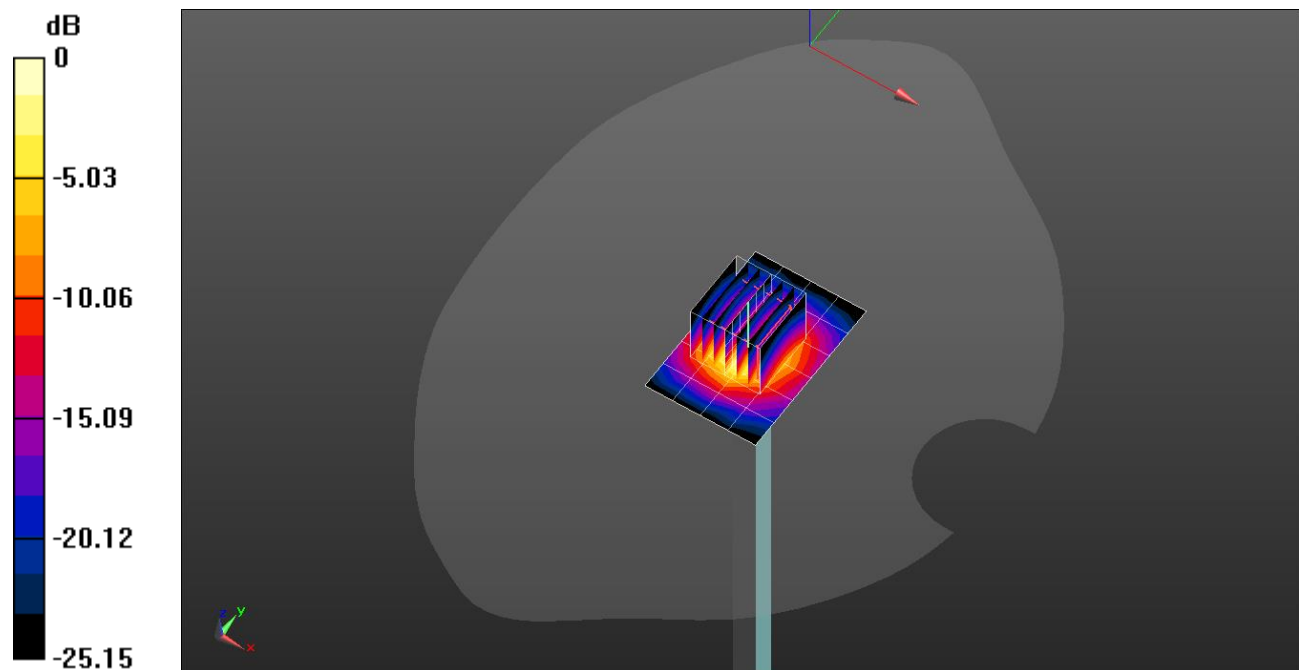

0 dB = 12.0 W/kg = 10.79 dBW/kg

20221019_System Performance Check D1900V2 SN 5d199

Frequency: 1900 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.395$ S/m; $\epsilon_r = 41.253$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1671; Calibrated: 5/31/2022
- Probe: EX3DV4 - SN7376; ConvF(8.51, 8.51, 8.51) @ 1900 MHz; Calibrated: 7/27/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (Right); Type: QD 000 P40 CD; Serial: 1855

Head/1900MHz, Pin=100 mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 4.64 W/kg


Head/1900MHz, Pin=100 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 58.37 V/m; Power Drift = 0.15 dB

Peak SAR (extrapolated) = 6.48 W/kg

SAR(1 g) = 3.73 W/kg; SAR(10 g) = 1.98 W/kg

Maximum value of SAR (measured) = 5.59 W/kg

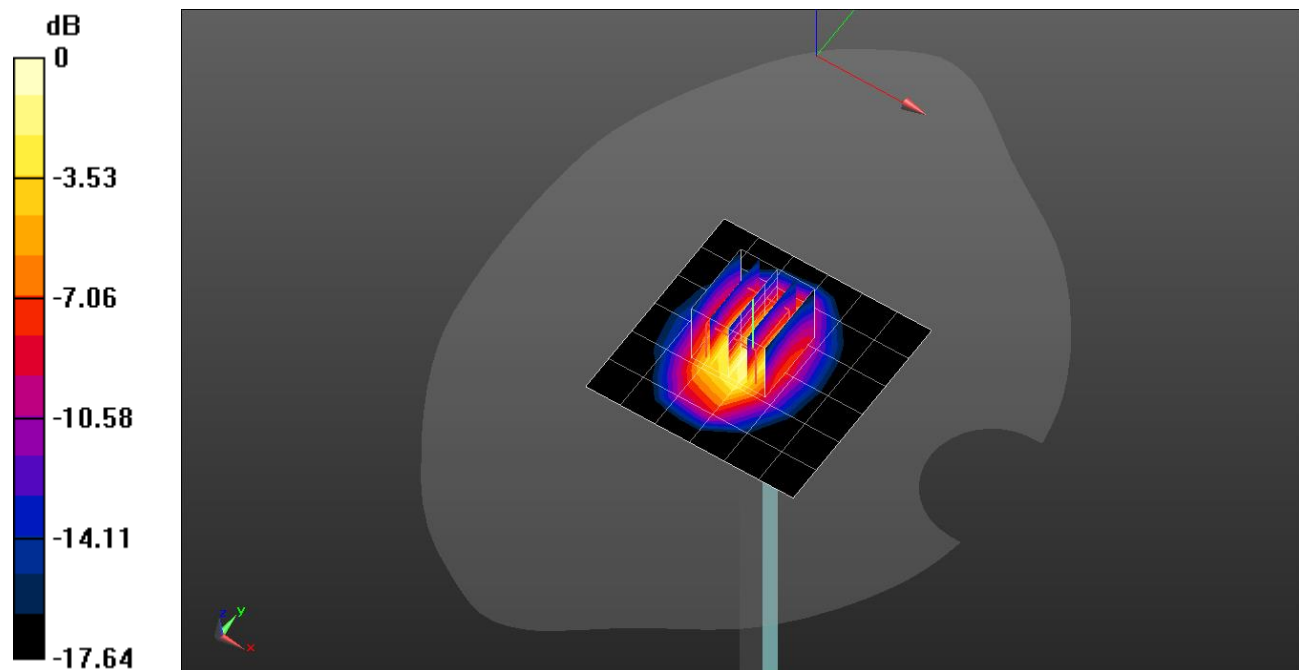

0 dB = 5.59 W/kg = 7.47 dBW/kg

20220913_SystemPerformanceCheck-D1900V2 SN 5d190

Frequency: 1900 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C
Medium parameters used: $f = 1900$ MHz; $\sigma = 1.408$ S/m; $\epsilon_r = 41.083$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Electronics: DAE4 Sn1468; Calibrated: 8/18/2022
- Probe: EX3DV4 - SN7545; ConvF(8.02, 8.02, 8.02) @ 1900 MHz; Calibrated: 8/19/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Type: QD 000 P40 CE; Serial: xxxx

Head/Pin=100 mW CW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 5.93 W/kg

Head/Pin=100 mW CW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 59.44 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 7.23 W/kg

SAR(1 g) = 3.82 W/kg; SAR(10 g) = 1.95 W/kg

Ratio of SAR at M2 to SAR at M1 = 52.6%

Maximum value of SAR (measured) = 6.03 W/kg

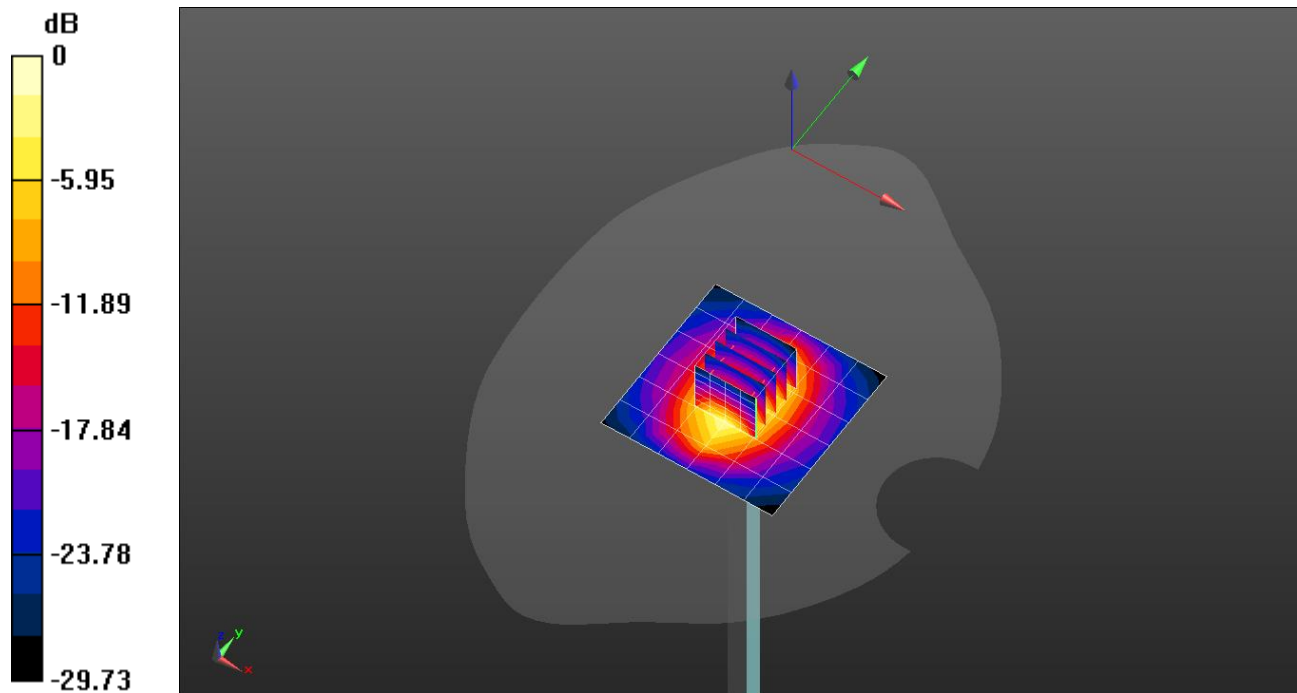

0 dB = 5.93 W/kg = 7.73 dBW/kg

20221003_System Performance Check D5GHzV2 SN 1209

Frequency: 5800 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C
Medium parameters used: $f = 5800$ MHz; $\sigma = 5.194$ S/m; $\epsilon_r = 35.977$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1468; Calibrated: 8/18/2022
- Probe: EX3DV4 - SN7545; ConvF(4.6, 4.6, 4.6) @ 5800 MHz; Calibrated: 8/19/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V8.0 (20deg probe tilt); Type: QD 000 P41 AA; Serial: 1991

Head/5.8 GHz, Pin=100mW/Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm
Maximum value of SAR (measured) = 21.4 W/kg


Head/5.8 GHz, Pin=100mW/Zoom Scan (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 71.08 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 38.1 W/kg

SAR(1 g) = 8.54 W/kg; SAR(10 g) = 2.42 W/kg

Maximum value of SAR (measured) = 20.6 W/kg

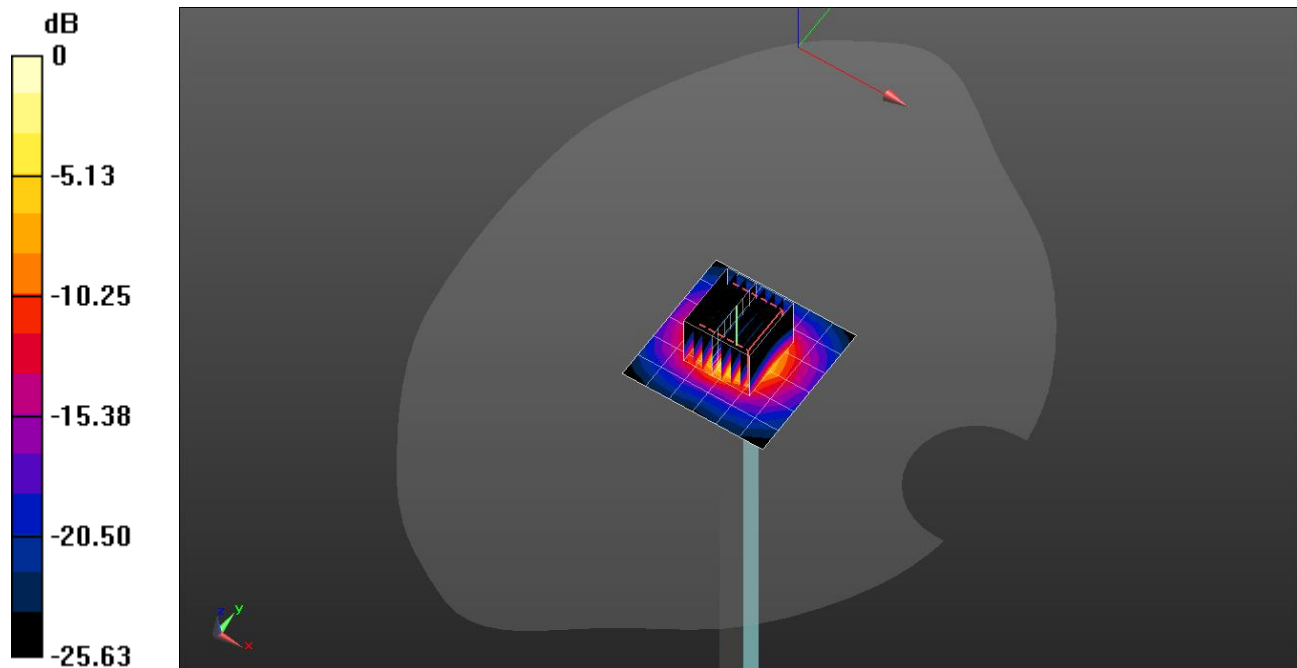

0 dB = 20.6 W/kg = 13.14 dBW/kg

20221004_System Performance Check D1750V2 SN 1125

Frequency: 1750 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C
Medium parameters used: $f = 1750$ MHz; $\sigma = 1.365$ S/m; $\epsilon_r = 39.513$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1468; Calibrated: 8/18/2022
- Probe: EX3DV4 - SN7545; ConvF(8.38, 8.38, 8.38) @ 1750 MHz; Calibrated: 8/19/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V8.0 (20deg probe tilt); Type: QD 000 P41 AA; Serial: 1991

Head/1750MHz, Pin=100 mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (measured) = 5.22 W/kg


Head/1750MHz, Pin=100 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 58.56 V/m; Power Drift = -0.13 dB

Peak SAR (extrapolated) = 6.29 W/kg

SAR(1 g) = 3.38 W/kg; SAR(10 g) = 1.78 W/kg

Maximum value of SAR (measured) = 5.27 W/kg

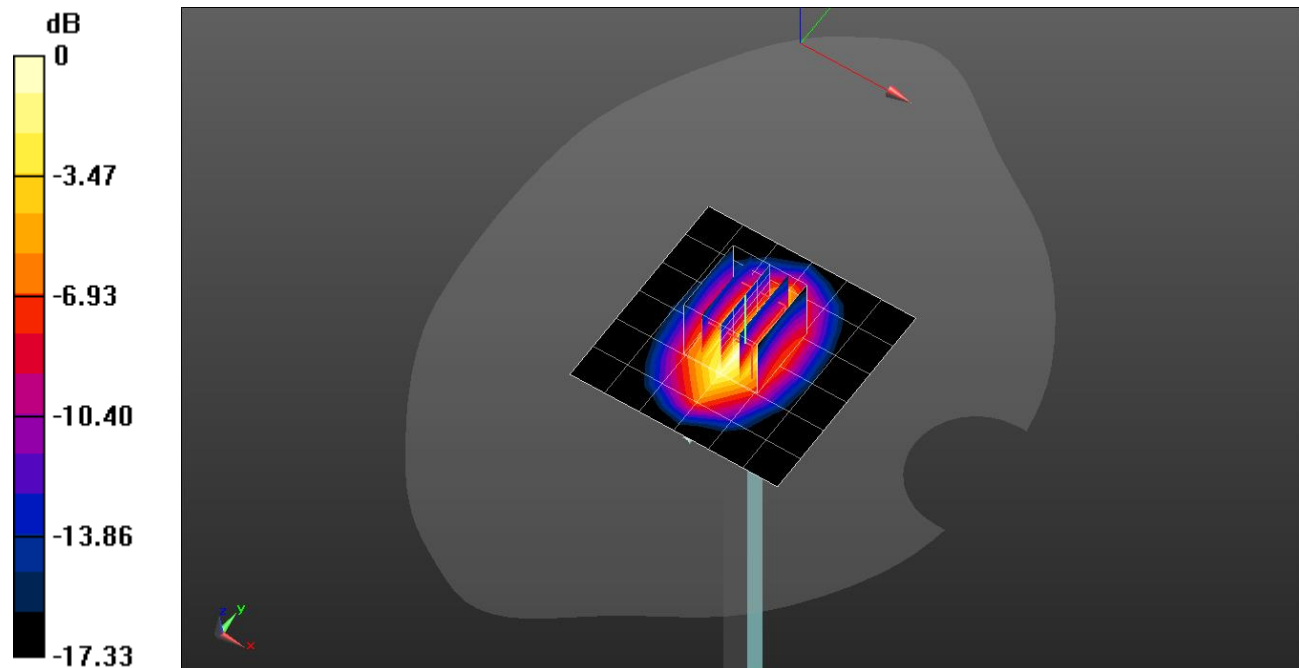

0 dB = 5.27 W/kg = 7.22 dBW/kg

20220913_System Performance Check D835V2 SN 4d194

Frequency: 835 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.91 \text{ S/m}$; $\epsilon_r = 41.868$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1343; Calibrated: 8/18/2022
- Probe: EX3DV4 - SN7376; ConvF(10.12, 10.12, 10.12) @ 835 MHz; Calibrated: 7/27/2022
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (20deg probe tilt); Type: QD 000 P40 CD; Serial: 1751

Head/835MHz, Pin=100 mW/Area Scan (7x13x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 1.19 W/kg



Head/835MHz, Pin=100 mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 36.68 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 1.48 W/kg

SAR(1 g) = 1.02 W/kg; SAR(10 g) = 0.684 W/kg

Maximum value of SAR (measured) = 1.23 W/kg

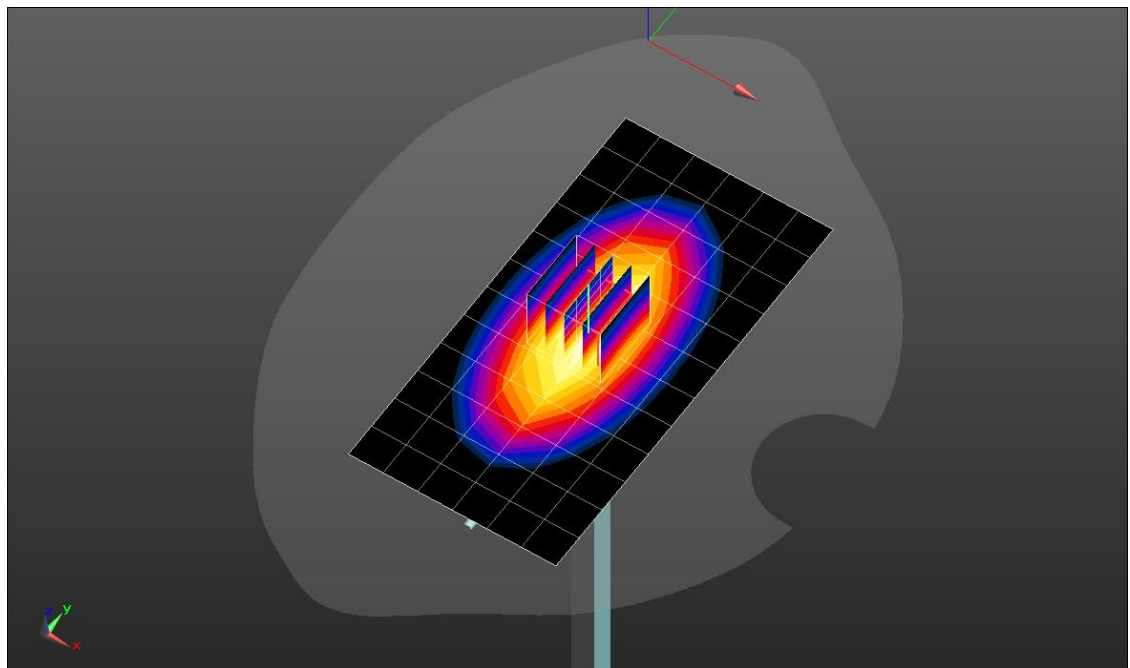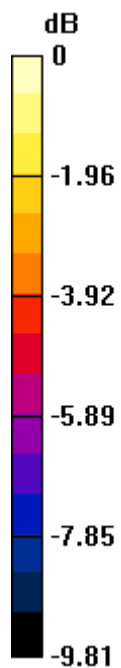

0 dB = 1.23 W/kg = 0.90 dBW/kg

20220920_System Performance Check D3700V2 SN1036

Frequency: 3700 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C
Medium parameters used: $f = 3700$ MHz; $\sigma = 3.071$ S/m; $\epsilon_r = 37.406$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1343; Calibrated: 8/18/2022
- Probe: EX3DV4 - SN7376; ConvF(7.05, 7.05, 7.05) @ 3700 MHz; Calibrated: 7/27/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (20deg probe tilt); Type: QD 000 P40 CD; Serial: 1751

Head/3700MHz, Pin=100mW/Area Scan (5x7x1): Measurement grid: dx=12mm, dy=12mm
Maximum value of SAR (measured) = 11.6 W/kg


Head/3700MHz, Pin=100mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=5mm, dy=5mm,
dz=1.4mm

Reference Value = 65.54 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 14.6 W/kg

SAR(1 g) = 6.39 W/kg; SAR(10 g) = 2.52 W/kg

Maximum value of SAR (measured) = 11.5 W/kg

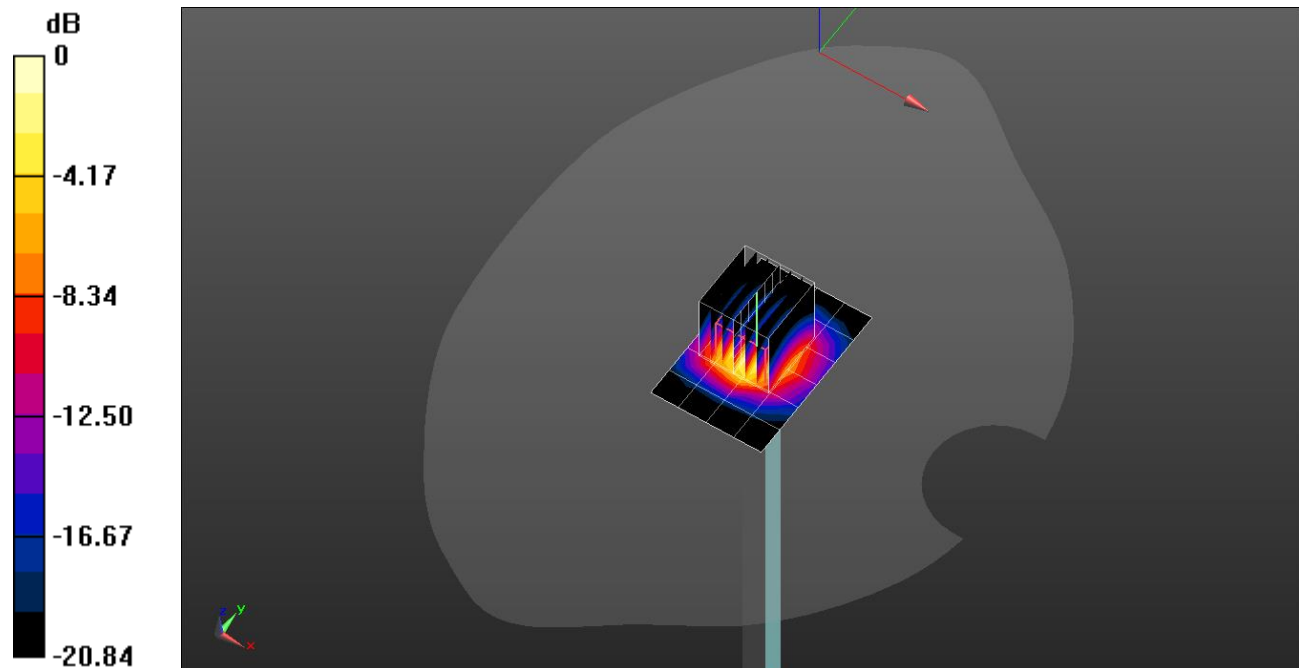

0 dB = 11.5 W/kg = 10.61 dBW/kg

20220926_System Performance Check D3900V2 SN1069

Frequency: 3900 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C

Medium parameters used: $f = 3900$ MHz; $\sigma = 3.338$ S/m; $\epsilon_r = 38.535$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1343; Calibrated: 8/18/2022
- Probe: EX3DV4 - SN7376; ConvF(6.75, 6.75, 6.75) @ 3900 MHz; Calibrated: 7/27/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (20deg probe tilt); Type: QD 000 P40 CD; Serial: 1751

Head/3900MHz, Pin=100mW/Area Scan (5x7x1): Measurement grid: dx=12mm, dy=12mm

Maximum value of SAR (measured) = 11.1 W/kg

Head/3900MHz, Pin=100mW/Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=5mm, dy=5mm,


dz=1.4mm

Reference Value = 64.80 V/m; Power Drift = 0.17 dB

Peak SAR (extrapolated) = 17.0 W/kg

SAR(1 g) = 6.68 W/kg; SAR(10 g) = 2.41 W/kg

Maximum value of SAR (measured) = 13.3 W/kg

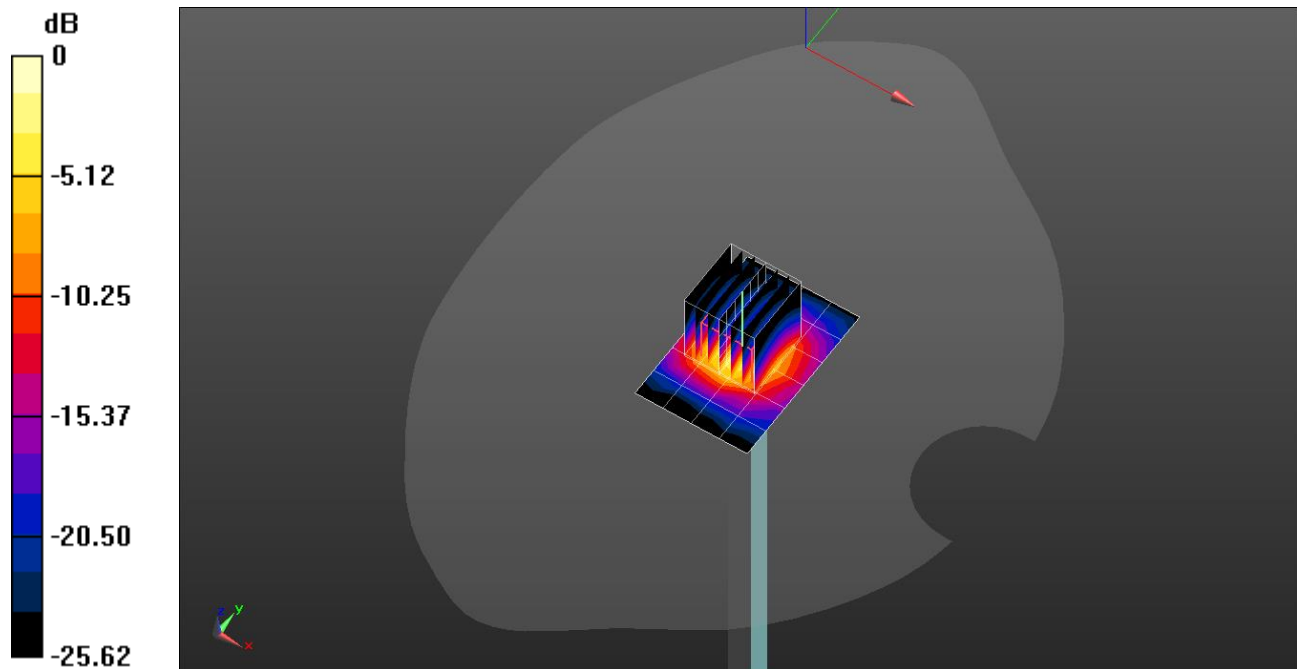

20221012_System Performance check D2450V2 SN960

Frequency: 2450 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 23.0°C; Liquid Temperature: 22.0°C
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.729$ S/m; $\epsilon_r = 37.725$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.012W/kg
- Averaged Fast SAR: Polynomial fit
- Electronics: DAE4 Sn1343; Calibrated: 8/18/2022
- Probe: EX3DV4 - SN7651; ConvF(7.82, 7.82, 7.82) @ 2450 MHz; Calibrated: 5/30/2022
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Phantom: Twin-SAM V5.0 (20deg probe tilt); Type: QD 000 P40 CD; Serial: 1751

Head/2450MHz, Pin=100mW/Area Scan (6x8x1): Measurement grid: dx=12mm, dy=12mm
Maximum value of SAR (measured) = 7.20 W/kg


Head/2450MHz, Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.48 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 9.51 W/kg

SAR(1 g) = 4.76 W/kg; SAR(10 g) = 2.4 W/kg

Maximum value of SAR (measured) = 7.36 W/kg

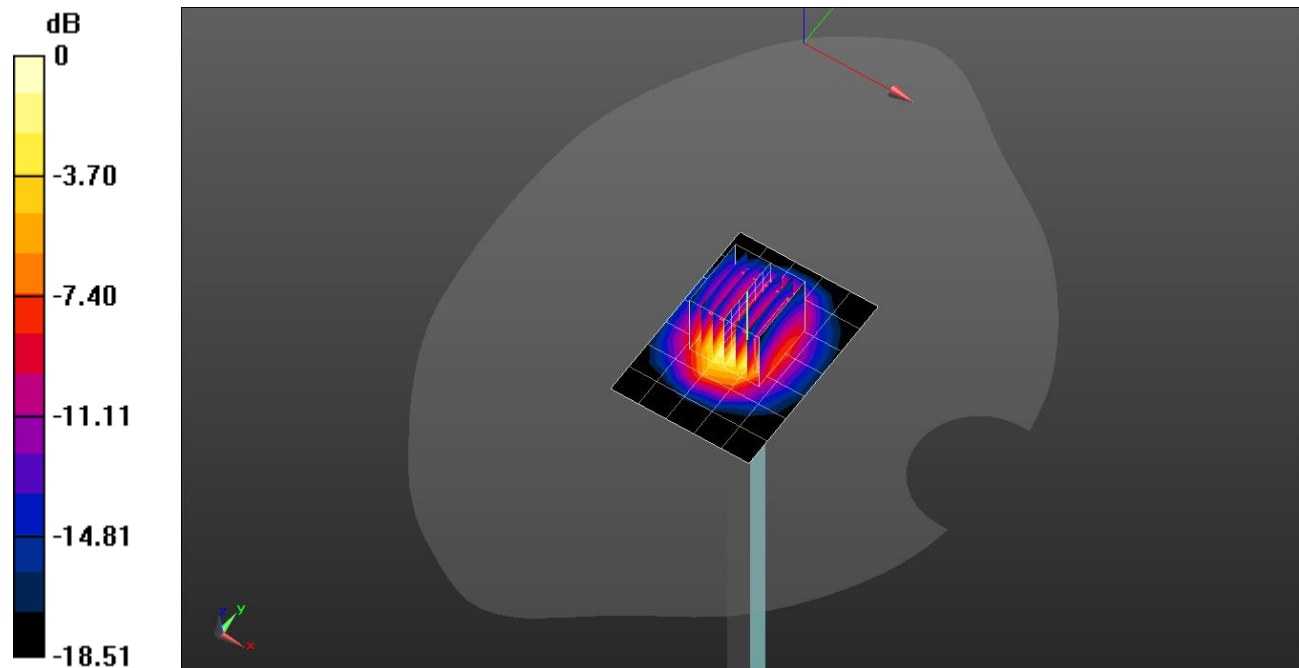

0 dB = 7.36 W/kg = 8.67 dBW/kg

20221020_System Performance Check D1900V2 SN5d199

Measurement Report for Device, UID 0 -, 1900.0MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL			0--	1900.0, 0	8.18	1.44	40.7

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
Twin-SAM V8.0 (30deg probe tilt) - 2043	HBBL-600-10000, 2022-Oct-20	EX3DV4 - SN7313, 2022-03-02	DAE4 Sn1494, 2022-07-18

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
Date	2022-10-20	2022-10-20
psSAR1g [W/kg]	4.02	3.98
psSAR10g [W/kg]	2.10	2.04
Power Drift [dB]	-0.00	-0.02

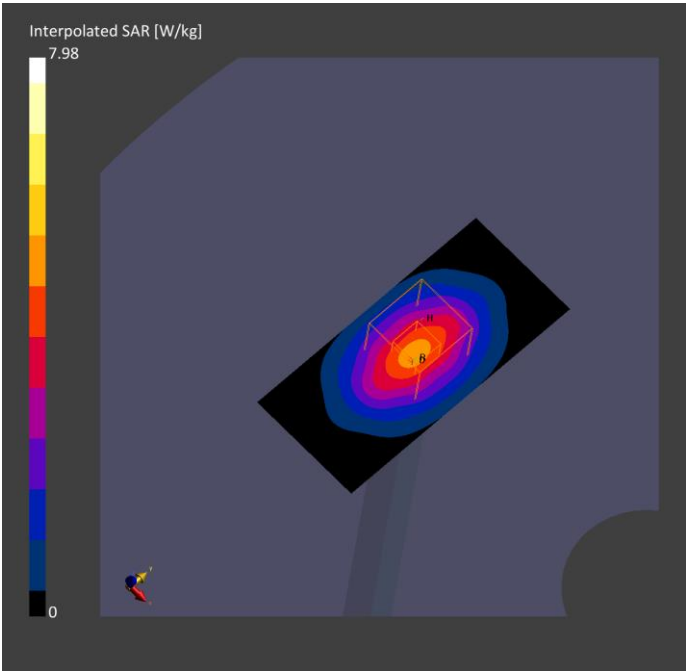

Measurement Report for Device, UID 0 -, 13.0MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL				13.0, 0	17.91	0.757	53.7

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
ELI V6.0 (20deg probe tilt) - 2005	HBBL-600-10000, 2022-Sep-13	EX3DV4 - SN7313, 2022-03-02	DAE4 Sn1591, 2022-03-24

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
Date	2022-09-13	2022-09-13
psSAR1g [W/kg]	0.056	0.055
psSAR10g [W/kg]	0.045	0.033
Power Drift [dB]	-0.02	-0.02

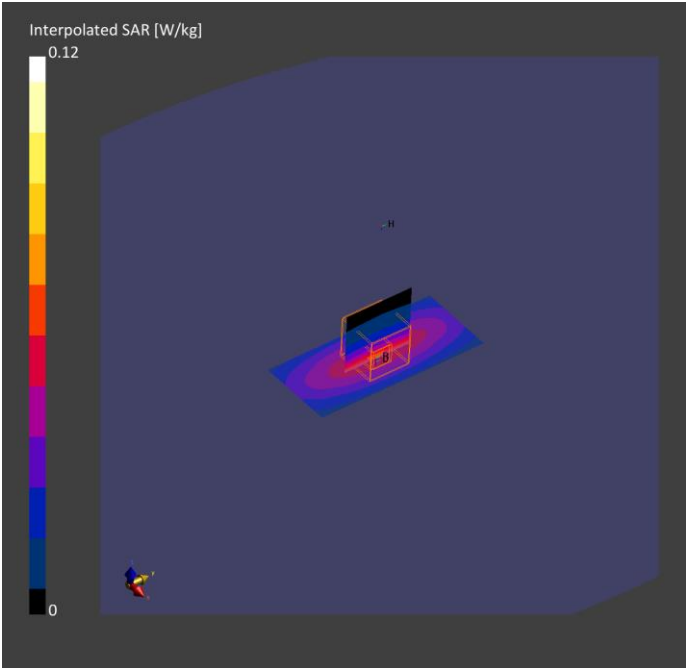

Measurement Report for Device, UID 0 -, 750.0MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL				750.0,0	9.91	0.868	42.6

Hardware Setup


Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
Twin-SAM V8.0 (30deg probe tilt) - 2039	HBBL-600-10000, 2022-Sep-14	EX3DV4 - SN7313, 2022-03-02	DAE4 Sn1591, 2022-03-24

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 90.0	32.0 x 32.0 x 30.0
Grid Steps [mm]	10.0 x 15.0	6.0 x 6.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
Date	2022-09-14	2022-09-14
psSAR1g [W/kg]	0.822	0.813
psSAR10g [W/kg]	0.548	0.527
Power Drift [dB]	0.00	0.03

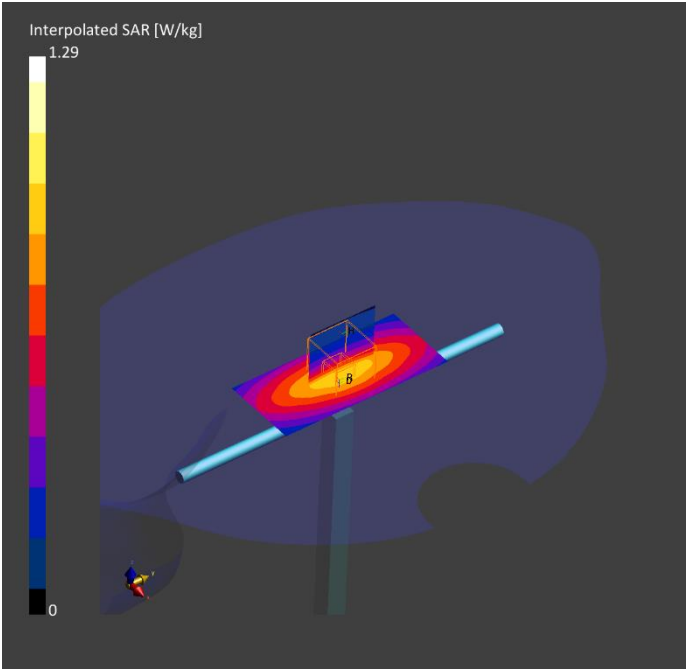

20220926_System Performance Check D2600V2 SN1097

Measurement Report for Device , UID 0 -, 2600.0MHz

Exposure Conditions

Phantom Section, TSL	Position, Test Distance [mm]	Band	Group, UID	Frequency [MHz], Channel Number	Conversion Factor	TSL Conductivity [S/m]	TSL Permittivity
Flat, HSL				2600.0, 0	7.4	1.94	39.3

Hardware Setup

Phantom	TSL, Measured Date	Probe, Calibration Date	DAE, Calibration Date
Twin-SAM V8.0 (30deg probe tilt) - 2039	HBBL-600-10000, 2022-Sep-26	EX3DV4 - SN7313, 2022-03-02	DAE4 Sn1591, 2022-03-24

Scan Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
Date	2022-09-26	2022-09-26
psSAR1g [W/kg]	5.95	6.06
psSAR10g [W/kg]	2.75	2.73
Power Drift [dB]	-0.04	-0.08

