



# **Appendix D**







## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details







## 1. SAR measurement System

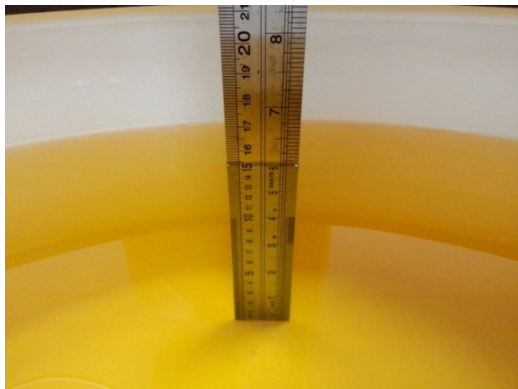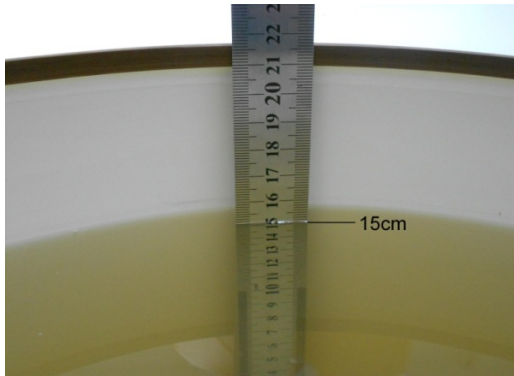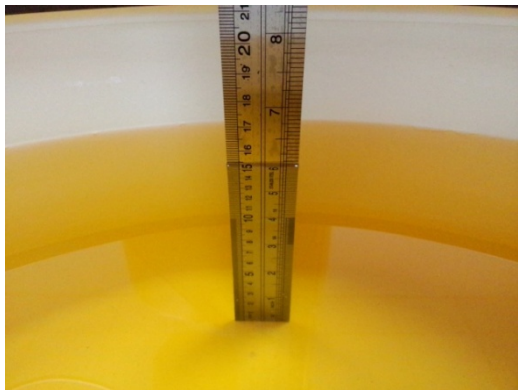



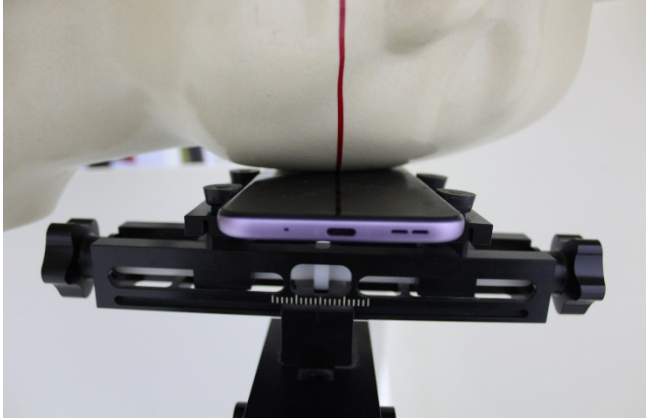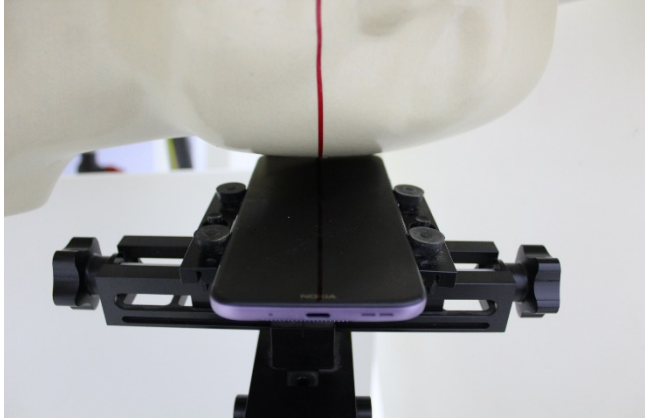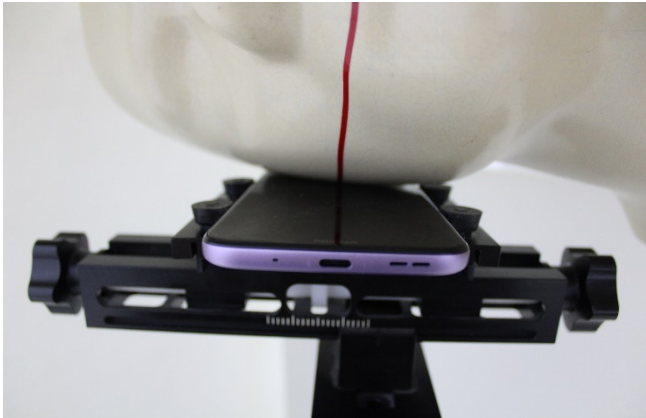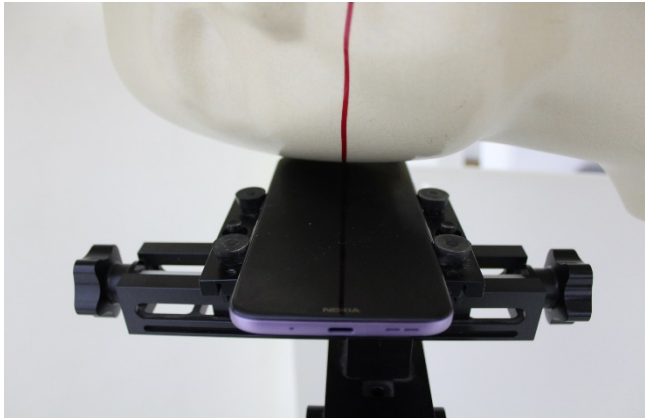

## 2. Photographs of Tissue Simulate Liquid

<p><b>Photo 1: Tissue Simulant Liquid for Head 750</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Head 835</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 1750</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Head 1900</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Head 2450</b></p>	<p><b>Photo 6: Tissue Simulant Liquid for Head 2600</b></p>
	

### 3. Photographs of EUT test position

<p><b>Photo 7: Left touch cheek</b></p>	<p><b>Photo 8: Left tilted 15 degree</b></p>
	
<p><b>Photo 9: Right touch cheek</b></p>	<p><b>Photo 10: Right tilted 15 degree</b></p>
	
<p><b>Photo 11: Front side 10mm</b></p>	<p><b>Photo 12: Back side 10mm</b></p>
	



<p><b>Photo 13: Left side 10mm</b></p>	<p><b>Photo 14: Right side 10mm</b></p>
	
<p><b>Photo 15: Top side 10mm</b></p>	<p><b>Photo 16: Bottom side 10mm</b></p>
	

## 4. EUT Constructional Details

