

Appendix C for KSCR220900175701

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date
Dipole	<input type="checkbox"/>	1	CLA150	4025	2021/04/26
	<input type="checkbox"/>	2	D450V3	1103	2021/04/21
	<input type="checkbox"/>	3	D750V3	1188	2022/03/29
	<input type="checkbox"/>	4	D835V2	4d114	2022/03/31
	<input type="checkbox"/>	5	D900V2	1d079	2022/06/07
	<input type="checkbox"/>	6	D1800V2	2d170	2022/03/31
	<input type="checkbox"/>	7	D1900V2	5d136	2022/06/07
	<input type="checkbox"/>	8	D2000V2	1041	2022/06/06
	<input type="checkbox"/>	9	D2300V2	1096	2022/03/31
	<input checked="" type="checkbox"/>	10	D2450V2	817	2022/04/01
	<input type="checkbox"/>	11	D2600V2	1158	2022/03/31
	<input type="checkbox"/>	12	D5GHzV2	1095	2022/06/01
DAE	<input checked="" type="checkbox"/>	13	DAE4	1245	2022/05/30
Probe	<input checked="" type="checkbox"/>	14	EX3DV4	7346	2022/03/30



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1 Dipole

1.1 CLA150 - SN 4025

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Client: SGS-CN (Auden)		Certificate No: CLA150-4025_Apr21	
CALIBRATION CERTIFICATE			
Object: CLA150 - SN: 4025			
Calibration procedure(s): QA CAL-15-v9 Calibration Procedure for SAR Validation Sources below 700 MHz			
Calibration date: April 26, 2021			
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature $22 \pm 3^\circ\text{C}$ and humidity $< 70\%$.			
Calibration Equipment used (M&E critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 10476	09-Apr-21 (No. 217-03201/03202)	Apr-22
Power sensor NRP Z91	SN: 10344	09-Apr-21 (No. 217-03201)	Apr-22
Power sensor NRP Z91	SN: 10345	09-Apr-21 (No. 217-03202)	Apr-22
Reference 20 dB Attenuator	SN: C22862 (203)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310952 / 00357	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX30N4	SN: 3877	30-Dec-20 (No. C3X3077_Dec20)	Dec-21
EXE4	SN: 684	26-Jun-20 (No. D458-658_Jun20)	Jun-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter S441S6	SN: G841203074	06-Apr-19 (in house check Jun-20)	In house check Jun-22
Power sensor E4113A	SN: MY4149067	06-Apr-19 (in house check Jun-20)	In house check Jun-22
Power sensor E4113A	SN: 00010010	06-Apr-19 (in house check Jun-20)	In house check Jun-22
RF generator HP 8440D	SN: US484010709	04-Aug-19 (in house check Jun-20)	In house check Jun-22
Network Analyser Agilent E8363A	SN: US41000477	31-Mar-14 (in house check Oct-20)	In house check Oct-21
Calibrated by:	Name: Jeffrey Katsman	Function: Laboratory Technician	Signature:
Approved by:	Name: Kaja Polovic	Function: Technical Manager	Signature:
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: April 26, 2021			
Certificate No: CLA150-4025_Apr21		Page 1 of 6	

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Glossary:			
TSL	Issue simulating liquid		
ConvF	sensitivity in TSL / NORM x,y,z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Technique", June 2013			
b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016			
c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010			
d) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
e) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom.			
• Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: CLA150-4025_Apr21		Page 2 of 6	

Measurement Conditions			
DASY system configuration, as far as not given on page 1.			
DASY Version	DASY5	V52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	ELIA Flat Phantom	Shell thickness: 2 ± 0.2 mm	
EUT Positioning	Touch Position		
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)	
Frequency	150 MHz \pm 1 MHz		


Head TSL parameters			
The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0°C	52.3	0.75 mho/m
Measured Head TSL parameters	$(22.0 \pm 0.2)^\circ\text{C}$	$51.1 \pm 6\%$	0.75 mho/m $\pm 6\%$
Head TSL temperature change during test	$< 0.5^\circ\text{C}$	---	---

SAR result with Head TSL		
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.90 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	$3.88\text{ W/kg} \pm 19.4\%$ (k=2)
SAR averaged over 10 cm^3 (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.60 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	$2.59\text{ W/kg} \pm 18.0\%$ (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)	
Antenna Parameters with Head TSL	
Impedance, transformed to feed point	$47.9\Omega \pm 1.5\Omega$
Return Loss	-31.4 dB
Additional EUT Data	
Manufactured by	SPLEAG

Certificate No: CLA150-4025_Apr21 Page 3 of 6

Certificate No: CLA150-4025_Apr21 Page 4 of 6

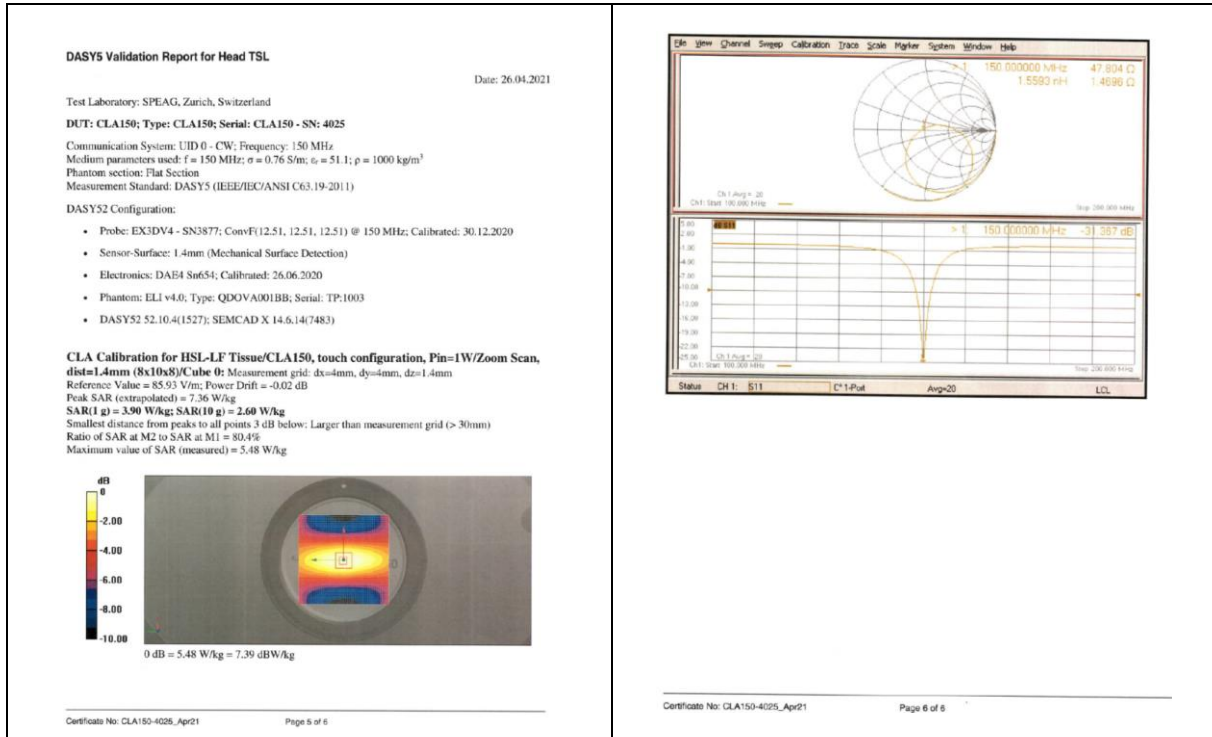

1.2 D450V3 - SN 1103

Calibration Laboratory of Schmid & Partner Engineering AG
Zugstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aude)** Certificate No: **D450V3-1103_Apr21**

CALIBRATION CERTIFICATE

Object: **D450V3 - SN: 1103**

Calibration procedure(s): **QA CAL-15-v9**
Calibration Procedure for SAR Validation Sources below 700 MHz

Calibration date: **April 21, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 2) °C and humidity < 70%.

Calibration Equipment used (MPE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03021/03020)	Apr-22
Power sensor NRP-291	SN: 102344	09-Apr-21 (No. 217-03021)	Apr-22
Power sensor NRP-291	SN: 102345	09-Apr-21 (No. 217-03020)	Apr-22
Reference 20 dB Attenuator	SN: CG2852 (200)	09-Apr-21 (No. 217-03345)	Apr-22
Type-N mismatch combination	SN: 310852 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 3877	30-Dec-20 (No. EX3-3877 Dec20)	Dec-21
DA84	SN: 654	26-Jun-20 (No. DA84-654 Jun20)	Jun-21

Secondary Standards	ID #	Check Date (In House)	Scheduled Check
Power meter E4118B	SN: GB41200274	06-Apr-16 (In house check Jun-20)	In house check Jun-22
Power sensor E4112A	SN: MY41496027	06-Apr-16 (In house check Jun-20)	In house check Jun-22
Power sensor E4112A	SN: 00018010	06-Apr-16 (In house check Jun-20)	In house check Jun-22
RF generator HP 8446C	SN: U03460.01700	06-Aug-19 (In house check Jun-20)	In house check Jun-22
Network Analyzer Agilent E8358A	SN: U841980477	31-Mar-14 (In house check Oct-20)	In house check Oct-21

Calibrated by: **Christoph Leubner** Function: **Laboratory Technician**

Approved by: **Kelly Polovic** Technical Manager

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D450V3-1103_Apr21 Page 1 of 6

Calibration Laboratory of Schmid & Partner Engineering AG
Zugstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aude)** Certificate No: **D450V3-1103_Apr21**

CALIBRATION CERTIFICATE

Object: **D450V3 - SN: 1103**

Calibration procedure(s): **QA CAL-15-v9**
Calibration Procedure for SAR Validation Sources below 700 MHz

Calibration date: **April 21, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 2) °C and humidity < 70%.

Calibration Equipment used (MPE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03021/03020)	Apr-22
Power sensor NRP-291	SN: 102344	09-Apr-21 (No. 217-03021)	Apr-22
Power sensor NRP-291	SN: 102345	09-Apr-21 (No. 217-03020)	Apr-22
Reference 20 dB Attenuator	SN: CG2852 (200)	09-Apr-21 (No. 217-03345)	Apr-22
Type-N mismatch combination	SN: 310852 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX3DV4	SN: 3877	30-Dec-20 (No. EX3-3877 Dec20)	Dec-21
DA84	SN: 654	26-Jun-20 (No. DA84-654 Jun20)	Jun-21

Secondary Standards	ID #	Check Date (In House)	Scheduled Check
Power meter E4118B	SN: GB41200274	06-Apr-16 (In house check Jun-20)	In house check Jun-22
Power sensor E4112A	SN: MY41496027	06-Apr-16 (In house check Jun-20)	In house check Jun-22
Power sensor E4112A	SN: 00018010	06-Apr-16 (In house check Jun-20)	In house check Jun-22
RF generator HP 8446C	SN: U03460.01700	06-Aug-19 (In house check Jun-20)	In house check Jun-22
Network Analyzer Agilent E8358A	SN: U841980477	31-Mar-14 (In house check Oct-20)	In house check Oct-21

Calibrated by: **Christoph Leubner** Function: **Laboratory Technician**

Approved by: **Kelly Polovic** Technical Manager

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D450V3-1103_Apr21 Page 1 of 6

Glossary:

TSL: Issue simulating liquid sensitivity in TSL / NORM x,y,z

ConvF: not applicable or not measured

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1103_Apr21 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

Measurement Conditions		
DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V62.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELJ Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters			
The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.57 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	43.1 ± 6 %	0.07 mho/m ± 8 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL		
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.55 W/kg ± 18.1 % (k=2)

SAR result with Head TSL		
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	0.757 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg ± 17.6 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0106)		
Antenna Parameters with Head TSL		
Impedance, transformed to feed point	57.1 Ω - 2.8 jΩ	
Return Loss	-23.0 dB	

General Antenna Parameters and Design	
Electrical Delay (one direction)	1.346 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data	
Manufactured by	SPEAG

Certificate No: D450V3-1103_Apr21 Page 3 of 6

Certificate No: D450V3-1103_Apr21 Page 4 of 6

DASY5 Validation Report for Head TSL		
Test Laboratory: SPEAG, Zurich, Switzerland		
Date: 21.04.2021		
DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103		
Communication System: UID 0 - CW; Frequency: 450 MHz		
Medium parameters used: f = 450 MHz; α = 0.87 S/m; ε = 43.1; ρ = 1000 kg/m ³		
Phantom section: Flat Section		
Measurement Standard: DASY5 (IEC/IEC/ANSI C63.19-2011)		
DASY52 Configuration:		
<ul style="list-style-type: none">Probe: EX3DV4 - SN3877; ConvF(10.64, 10.64) @ 450 MHz; Calibrated: 30.12.2020Sensor-Surface: 1.4mm Mechanical Surface DetectionElectronics: DAE4 Sn654; Calibrated: 26.06.2020Phantom: ELJ v4.0; Type: QDOVA001BB; Serial: TP:1003DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)		
Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:		
Measurement grid: dx=5mm, dy=5mm, dz=5mm		
Reference Value = 39.18 V/m; Power Drift = -0.08 dB		
Peak SAR (extrapolated) = 1.76 W/kg		
SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.767 W/kg		
Smallest distance from peaks to all points 3 dB below: Larger than measurement grid		
Ratio of SAR at M2 to SAR at M1 = 64.9%		
Maximum value of SAR (measured) = 1.53 W/kg		



Certificate No: D450V3-1103_Apr21 Page 5 of 6

Certificate No: D450V3-1103_Apr21 Page 6 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.3 D750V3 - SN 1188

TTL Speag CALIBRATION LABORATORY		CAICT																					
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn																					
Client: SGS-CN		Certificate No: Z22-60103																					
CALIBRATION CERTIFICATE																							
Object: D750V3 - SN: 1188																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: March 28, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.																							
Calibration Equipment used (M&TE critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by: Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>104277</td><td>24-Sep-21 (CTTL No.J21X08328)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP88</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08328)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX30V4</td><td>SN 7307</td><td>26-May-21(SPEAG No EX3-7307_May21)</td><td>May-22</td></tr><tr><td>DAE4</td><td>SN 1556</td><td>12-Jan-22(CTTL-SPEAG No Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration	Power Meter NRP2	104277	24-Sep-21 (CTTL No.J21X08328)	Sep-22	Power sensor NRP88	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22	Reference Probe EX30V4	SN 7307	26-May-21(SPEAG No EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	104277	24-Sep-21 (CTTL No.J21X08328)	Sep-22																				
Power sensor NRP88	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22																				
Reference Probe EX30V4	SN 7307	26-May-21(SPEAG No EX3-7307_May21)	May-22																				
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by: Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator S4438C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY48110673</td><td>14-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration	Signal Generator S4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration																				
Signal Generator S4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Calibrated by: Zhao Jing SAR Test Engineer		Signature:																					
Reviewed by: Lin Hao SAR Test Engineer		Signature:																					
Approved by: Qi Dianyan SAR Project Leader		Signature:																					
Issued: April 3, 2022																							
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-60103		Page 1 of 5																					


TTL Speag CALIBRATION LABORATORY		CAICT																						
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn																						
Measurement Conditions DASY system configuration, as far as not given on page 1:																								
<table border="1"><thead><tr><th>DASY Version</th><th>DASY52</th><th>V52.10.4</th></tr></thead><tbody><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>15 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>750 MHz ± 1 MHz</td><td></td></tr></tbody></table>				DASY Version	DASY52	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	750 MHz ± 1 MHz				
DASY Version	DASY52	V52.10.4																						
Extrapolation	Advanced Extrapolation																							
Phantom	Triple Flat Phantom 5.1C																							
Distance Dipole Center - TSL	15 mm	with Spacer																						
Zoom Scan Resolution	dx, dy, dz = 5 mm																							
Frequency	750 MHz ± 1 MHz																							
Head TSL parameters The following parameters and calculations were applied:																								
<table border="1"><thead><tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr></thead><tbody><tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>42.0</td><td>0.90 mho/m</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>41.4 ± 6 %</td><td>0.89 mho/m ± 6 %</td></tr><tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>---</td><td>---</td></tr></tbody></table>					Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---					
	Temperature	Permittivity	Conductivity																					
Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m																					
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %																					
Head TSL temperature change during test	<1.0 °C	---	---																					
SAR result with Head TSL																								
<table border="1"><thead><tr><th></th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR averaged over 1 cm² (1 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>2.07 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>8.27 W/kg ± 18.8 % (k=2)</td></tr><tr><td>SAR averaged over 10 cm² (10 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>1.37 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>5.48 W/kg ± 18.7 % (k=2)</td></tr></tbody></table>					Condition		SAR averaged over 1 cm ² (1 g) of Head TSL			SAR measured	250 mW input power	2.07 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL			SAR measured	250 mW input power	1.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)
	Condition																							
SAR averaged over 1 cm ² (1 g) of Head TSL																								
SAR measured	250 mW input power	2.07 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)																						
SAR averaged over 10 cm ² (10 g) of Head TSL																								
SAR measured	250 mW input power	1.37 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)																						

TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NORMx.y.z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60103		Page 2 of 5	

TTL Speag CALIBRATION LABORATORY		CAICT					
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn					
Appendix (Additional assessments outside the scope of CNAS L0570)							
Antenna Parameters with Head TSL							
<table border="1"><thead><tr><th>Impedance, transformed to feed point</th><th>53.60- 1.13jΩ</th></tr></thead><tbody><tr><td>Return Loss</td><td>-28.7dB</td></tr></tbody></table>				Impedance, transformed to feed point	53.60- 1.13jΩ	Return Loss	-28.7dB
Impedance, transformed to feed point	53.60- 1.13jΩ						
Return Loss	-28.7dB						
General Antenna Parameters and Design							
<table border="1"><thead><tr><th>Electrical Delay (one direction)</th><th>0.947 ns</th></tr></thead></table>				Electrical Delay (one direction)	0.947 ns		
Electrical Delay (one direction)	0.947 ns						
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.							
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.							
Additional EUT Data							
<table border="1"><thead><tr><th>Manufactured by</th><th>SPEAG</th></tr></thead></table>				Manufactured by	SPEAG		
Manufactured by	SPEAG						
Certificate No: Z22-60103		Page 3 of 5					

TTL Speag CALIBRATION LABORATORY		CAICT																						
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn																						
Measurement Conditions DASY system configuration, as far as not given on page 1:																								
<table border="1"><thead><tr><th>DASY Version</th><th>DASY52</th><th>V52.10.4</th></tr></thead><tbody><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>15 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>750 MHz ± 1 MHz</td><td></td></tr></tbody></table>				DASY Version	DASY52	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	750 MHz ± 1 MHz				
DASY Version	DASY52	V52.10.4																						
Extrapolation	Advanced Extrapolation																							
Phantom	Triple Flat Phantom 5.1C																							
Distance Dipole Center - TSL	15 mm	with Spacer																						
Zoom Scan Resolution	dx, dy, dz = 5 mm																							
Frequency	750 MHz ± 1 MHz																							
Head TSL parameters The following parameters and calculations were applied:																								
<table border="1"><thead><tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr></thead><tbody><tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>42.0</td><td>0.90 mho/m</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>41.4 ± 6 %</td><td>0.89 mho/m ± 6 %</td></tr><tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>---</td><td>---</td></tr></tbody></table>					Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---					
	Temperature	Permittivity	Conductivity																					
Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m																					
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %																					
Head TSL temperature change during test	<1.0 °C	---	---																					
SAR result with Head TSL																								
<table border="1"><thead><tr><th></th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR averaged over 1 cm² (1 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>2.07 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>8.27 W/kg ± 18.8 % (k=2)</td></tr><tr><td>SAR averaged over 10 cm² (10 g) of Head TSL</td><td></td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>1.37 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>5.48 W/kg ± 18.7 % (k=2)</td></tr></tbody></table>					Condition		SAR averaged over 1 cm ² (1 g) of Head TSL			SAR measured	250 mW input power	2.07 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ² (10 g) of Head TSL			SAR measured	250 mW input power	1.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)
	Condition																							
SAR averaged over 1 cm ² (1 g) of Head TSL																								
SAR measured	250 mW input power	2.07 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)																						
SAR averaged over 10 cm ² (10 g) of Head TSL																								
SAR measured	250 mW input power	1.37 W/kg																						
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)																						

TTL Speag CALIBRATION LABORATORY		CAICT					
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn					
Appendix (Additional assessments outside the scope of CNAS L0570)							
Antenna Parameters with Head TSL							
<table border="1"><thead><tr><th>Impedance, transformed to feed point</th><th>53.60- 1.13jΩ</th></tr></thead><tbody><tr><td>Return Loss</td><td>-28.7dB</td></tr></tbody></table>				Impedance, transformed to feed point	53.60- 1.13jΩ	Return Loss	-28.7dB
Impedance, transformed to feed point	53.60- 1.13jΩ						
Return Loss	-28.7dB						
General Antenna Parameters and Design							
<table border="1"><thead><tr><th>Electrical Delay (one direction)</th><th>0.947 ns</th></tr></thead></table>				Electrical Delay (one direction)	0.947 ns		
Electrical Delay (one direction)	0.947 ns						
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.							
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.							
Additional EUT Data							
<table border="1"><thead><tr><th>Manufactured by</th><th>SPEAG</th></tr></thead></table>				Manufactured by	SPEAG		
Manufactured by	SPEAG						
Certificate No: Z22-60103		Page 4 of 5					

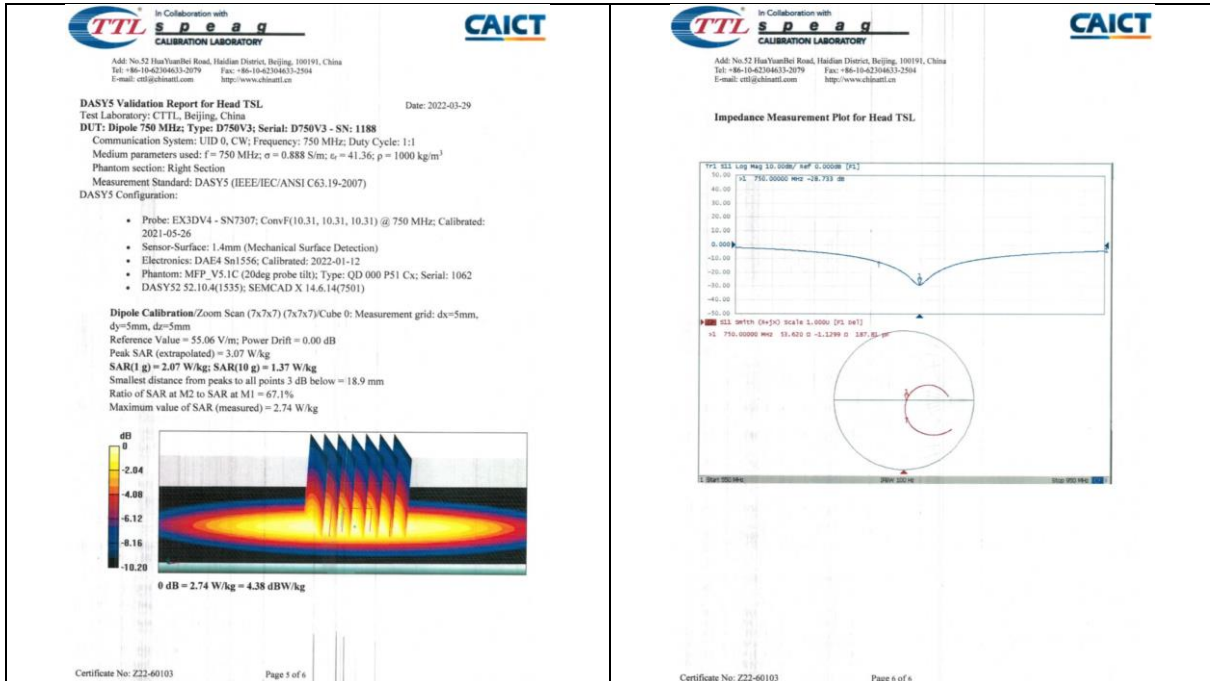

1.4 D835V2 - SN 4d114

TTL Speaq CALIBRATION LABORATORY		CAICT																					
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2079 Fax: +86-10-4204633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2079 Fax: +86-10-4204633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com																					
Client: SGS-CN		Certificate No: Z22-60104																					
CALIBRATION CERTIFICATE																							
Object: D835V2 - SN: 4d114																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: March 31, 2022																							
This Calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.																							
Calibration Equipment used (M&TE critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by, Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>106277</td><td>24-Sep-21 (CTTL, No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Power sensor NRPBS</td><td>104261</td><td>24-Sep-21 (CTTL, No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX3DV4</td><td>SN 7307</td><td>26-May-21 (SPEAG, No.EX3-7307_May21)</td><td>May-22</td></tr><tr><td>DAE4</td><td>SN 1556</td><td>12-Jan-22 (CTTL-SPEAG, No.Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Power sensor NRPBS	104261	24-Sep-21 (CTTL, No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG, No.EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG, No.Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																				
Power sensor NRPBS	104261	24-Sep-21 (CTTL, No.J21X08326)	Sep-22																				
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG, No.EX3-7307_May21)	May-22																				
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG, No.Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by, Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator E4438C</td><td>MY46071430</td><td>13-Jan-22 (CTTL, No.J22X00409)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY46110673</td><td>14-Jan-22 (CTTL, No.J22X00409)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY46071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X00409)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																				
Signal Generator E4438C	MY46071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23																				
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X00409)	Jan-23																				
Calibrated by: Zhao Jing SAR Test Engineer																							
Reviewed by: Lin Hao SAR Test Engineer																							
Approved by: Qi Dianyan SAR Project Leader																							
Issued: April 6, 2022																							
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							

Certificate No: Z22-60104 Page 1 of 6

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2079 Fax: +86-10-4204633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4204633-2079 Fax: +86-10-4204633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
Glossary:			
TSL		tissue simulating liquid	
ConvF		sensitivity in TSL / NORMx.y.z	
N/A		not applicable or not measured	
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			

Certificate No: Z22-60104 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

TTL Calibration Laboratory		CAICT	
<p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com</p>			
<p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p>			
DASY Version	DASY52	VS2 10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	835 MHz ± 1 MHz		
<p>Head TSL parameters The following parameters and calculations were applied.</p>			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 5 %	0.91 mho/m ± 5 %
Head TSL temperature change during test	<1.0 °C	---	---
<p>SAR result with Head TSL</p>			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.37 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	9.40 W/kg ± 18.5 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.54 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 18.7 % (k=2)	
<p>Certificate No: Z22-60104 Page 3 of 6</p>			

TTL Calibration Laboratory		CAICT	
<p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com</p>			
<p>Appendix (Additional assessments outside the scope of CNAS L0570)</p>			
<p>Antenna Parameters with Head TSL</p>			
Impedance, transformed to feed point	48.70 - j22.0Q		
Return Loss	-25.3dB		
<p>General Antenna Parameters and Design</p>			
Electrical Delay (one direction)	1.307 ns		
<p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p>			
<p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.</p>			
<p>No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p>			
<p>Additional EUT Data</p>			
Manufactured by	SPEAG		
<p>Certificate No: Z22-60104 Page 4 of 6</p>			

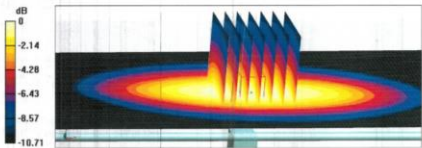TTL Calibration Laboratory		CAICT	
<p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com</p>			
<p>DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-03-31</p>			
<p>DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114 Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: f = 835 MHz; σ = 0.907 S/m; ε_r = 40.98; ρ = 1000 kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:</p>			
<ul style="list-style-type: none">Probe: EX3DV4 - SN7307; ConvF(10.13, 10.13, 10.13) @ 835 MHz; Calibrated: 2021-05-26Sensor-Surface: 1.4mm (Mechanical Surface Detection)Electronics: DA-E4 Sn1556; Calibrated: 2022-01-12Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062DASY52 52.10.4(1535); SEMCAD X 14.6(147501)			
<p>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.88 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 3.56 W/kg SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg Smallest distance from peaks to all points 3 dB below = 15.8 mm Ratio of SAR at M2 to SAR at M1 = 66.2% Maximum value of SAR (measured) = 3.17 W/kg</p>			
			
<p>Certificate No: Z22-60104 Page 5 of 6</p>			

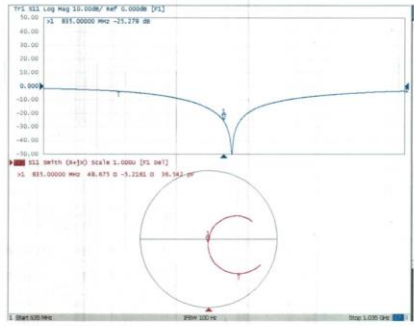TTL Calibration Laboratory		CAICT	
<p>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com</p>			
<p>Impedance Measurement Plot for Head TSL</p>			
			
<p>Certificate No: Z22-60104 Page 6 of 6</p>			



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 t(86-512)57370818 www.sgs.com
t(86-512)57355888 t(86-512)57370818 sgs.china@sgs.com

1.5 D900V2 - SN 1d079

In Collaboration with TTL speag CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION LABORATORY																																	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn																																	
Client: SGS-CN		Certificate No: Z22-60184																																	
CALIBRATION CERTIFICATE																																			
Object: D900V2 - SN: 1d079																																			
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																																			
Calibration date: June 7, 2022																																			
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																																			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.																																			
Calibration Equipment used (M&TE critical for calibration)																																			
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>106277</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP85</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Reference Probe EX3DV4</td><td>SN 7464</td><td>28-Jan-22 (SPEAG No EX3-7464_Jan22)</td><td>Jan-23</td></tr><tr><td>DAE4</td><td>SN 1556</td><td>12-Jan-22 (CTTL-SPEAG No Z22-60007)</td><td>Jan-23</td></tr><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by Certificate No.)</th><th>Scheduled Calibration</th></tr><tr><td>Signal Generator E4438C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY48110673</td><td>14-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7464	28-Jan-22 (SPEAG No EX3-7464_Jan22)	Jan-23	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																																
Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																																
Reference Probe EX3DV4	SN 7464	28-Jan-22 (SPEAG No EX3-7464_Jan22)	Jan-23																																
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23																																
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration																																
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																																
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23																																
Calibrated by: Zhao Jing SAR Test Engineer																																			
Reviewed by: Lin Hao SAR Test Engineer																																			
Approved by: Qi Dianyan SAR Project Leader																																			
Issued: June 13, 2022																																			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																																			
Certificate No: Z22-60184		Page 1 of 6																																	

In Collaboration with TTL speag CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION LABORATORY																			
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn																			
Measurement Conditions DASY system configuration, as far as not given on page 1.																					
<table border="1"><thead><tr><th>DASY Version</th><th>DASY2</th><th>52.10.4</th></tr></thead><tbody><tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr><tr><td>Phantom</td><td>Triple Flat Phantom S 1C</td><td></td></tr><tr><td>Distance Dipole Center - TSL</td><td>15 mm</td><td>with Spacer</td></tr><tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr><tr><td>Frequency</td><td>900 MHz ± 1 MHz</td><td></td></tr></tbody></table>				DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom S 1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	900 MHz ± 1 MHz	
DASY Version	DASY2	52.10.4																			
Extrapolation	Advanced Extrapolation																				
Phantom	Triple Flat Phantom S 1C																				
Distance Dipole Center - TSL	15 mm	with Spacer																			
Zoom Scan Resolution	dx, dy, dz = 5 mm																				
Frequency	900 MHz ± 1 MHz																				
Head TSL parameters The following parameters and calculations were applied.																					
<table border="1"><thead><tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr></thead><tbody><tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>41.5</td><td>0.97 nS/m</td></tr><tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>42.1 ± 6 %</td><td>0.98 nS/m ± 6 %</td></tr><tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>---</td><td>---</td></tr></tbody></table>					Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	41.5	0.97 nS/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 nS/m ± 6 %	Head TSL temperature change during test	<1.0 °C	---	---		
	Temperature	Permittivity	Conductivity																		
Nominal Head TSL parameters	22.0 °C	41.5	0.97 nS/m																		
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 nS/m ± 6 %																		
Head TSL temperature change during test	<1.0 °C	---	---																		
SAR result with Head TSL																					
<table border="1"><thead><tr><th>SAR averaged over 1 cm³ (1 g) of Head TSL</th><th>Condition</th><th></th></tr></thead><tbody><tr><td>SAR measured</td><td>250 mW input power</td><td>2.70 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>11.0 W/kg ± 18.8 % (k=2)</td></tr><tr><td>SAR averaged over 10 cm³ (10 g) of Head TSL</td><td>Condition</td><td></td></tr><tr><td>SAR measured</td><td>250 mW input power</td><td>1.73 W/kg</td></tr><tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>7.09 W/kg ± 18.7 % (k=2)</td></tr></tbody></table>				SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	2.70 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	1.73 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																				
SAR measured	250 mW input power	2.70 W/kg																			
SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)																			
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																				
SAR measured	250 mW input power	1.73 W/kg																			
SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)																			
Certificate No: Z22-60184		Page 3 of 6																			

In Collaboration with TTL speag CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION LABORATORY	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn	
Glossary: TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx,y,z N/A: not applicable or not measured			
Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz" c) DASY4/5 System Handbook			
Additional Documentation: c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters: • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60184		Page 2 of 6	

In Collaboration with TTL speag CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION LABORATORY							
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn							
Appendix (Additional assessments outside the scope of CNAS L0570)									
Antenna Parameters with Head TSL									
<table border="1"><thead><tr><th></th><th>48.10-8.49G</th></tr></thead><tbody><tr><td>Impedance, transformed to feed point</td><td></td></tr><tr><td>Return Loss</td><td>-23.3 dB</td></tr></tbody></table>					48.10-8.49G	Impedance, transformed to feed point		Return Loss	-23.3 dB
	48.10-8.49G								
Impedance, transformed to feed point									
Return Loss	-23.3 dB								
General Antenna Parameters and Design									
<table border="1"><thead><tr><th>Electrical Delay (one direction)</th><th>1.312 ns</th></tr></thead><tbody><tr><td></td><td></td></tr></tbody></table>				Electrical Delay (one direction)	1.312 ns				
Electrical Delay (one direction)	1.312 ns								
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.									
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.									
Additional EUT Data									
<table border="1"><thead><tr><th>Manufactured by</th><th>SPEAG</th></tr></thead><tbody><tr><td></td><td></td></tr></tbody></table>				Manufactured by	SPEAG				
Manufactured by	SPEAG								
Certificate No: Z22-60184		Page 4 of 6							




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

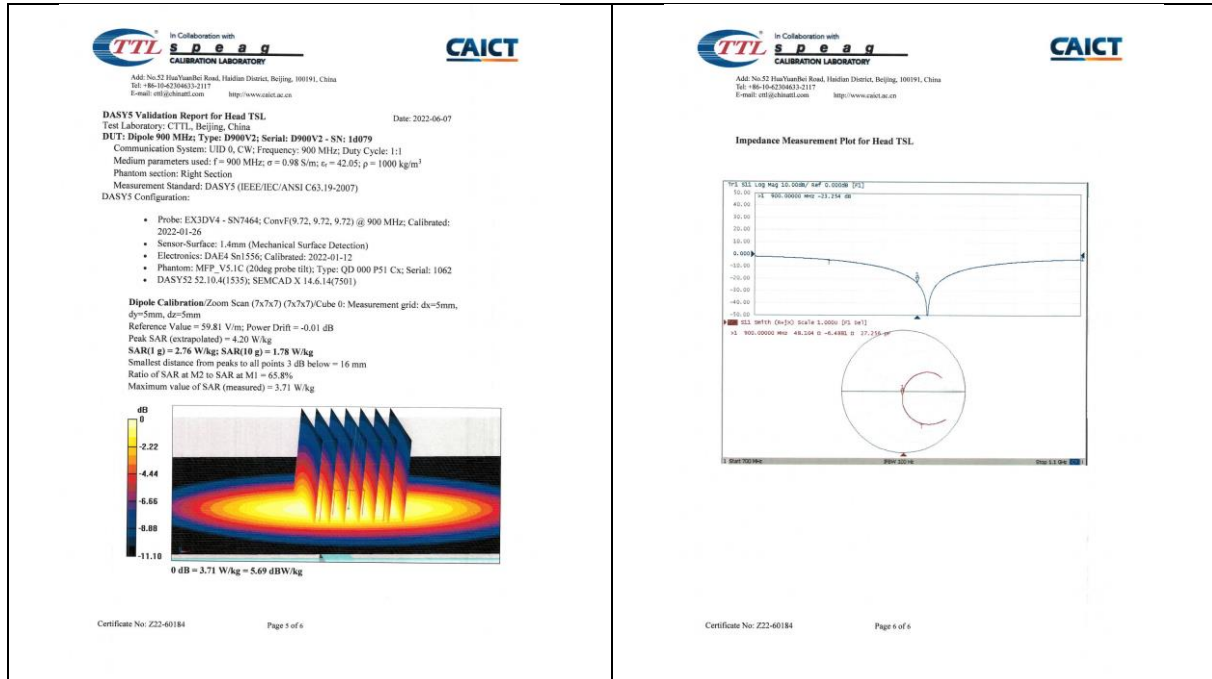

1.6 D1800V2 - SN 2d170

TTL In Collaboration with **CAICT**
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4230603-2117 Fax: +86-10-4230603-2118
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60105**

CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d170**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer

Reviewed by: **Lin Hao** SAR Test Engineer

Approved by: **Qi Dianyan** SAR Project Leader

Issued April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

TTL In Collaboration with **CAICT**
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4230603-2079 Fax: +86-10-4230603-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

TTL Speaq Calibration Laboratory		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	1800 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.8 ± 6 %	1.41 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	9.73 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	38.9 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.11 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	20.4 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60105 Page 3 of 6			

TTL Speaq Calibration Laboratory		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	47.90-2.54jΩ		
Return Loss	-29.4dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.116 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60105 Page 4 of 6			

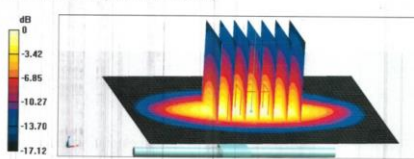TTL Speaq Calibration Laboratory		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
DASY5 Validation Report for Head TSL Test Laboratory: TTL, Beijing, China Date: 2022-03-31 DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d170 Communication System: UID 0, CW; Frequency: 1800 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1800 MHz; σ = 1.411 S/m; ε = 40.62; ρ = 1000 kg/m ³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/ANSI C63.19-2007) DASY5 Configuration: <ul style="list-style-type: none">Probe: EX3DV4 - SN7307; ConvF(8.34, 8.34, 8.34) @ 1800 MHz; Calibrated: 2021-05-26Sensor-Surface: 1.4mm (Mechanical Surface Detection)Electronics: DAE4 Sn1556; Calibrated: 2022-01-12Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 98.14 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 18.2 W/kg SAR(1 g) = 9.73 W/kg; SAR(10 g) = 5.11 W/kg Smallest distance from peaks to all points 3 dB below = 10 mm Ratio of SAR at M2 to SAR at M1 = 54% Maximum value of SAR (measured) = 15.2 W/kg			
			
Certificate No: Z22-60105 Page 5 of 6			

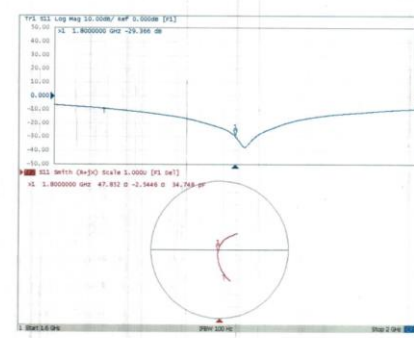TTL Speaq Calibration Laboratory		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
Impedance Measurement Plot for Head TSL			
			
Certificate No: Z22-60105 Page 6 of 6			


1.7 D1900V2 - SN 5d136

TTL S p e a g CALIBRATION LABORATORY		CAICT																					
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: cti@china.com.cn		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: cti@china.com.cn																					
Client: SGS-CN		Certificate No: Z22-60185																					
CALIBRATION CERTIFICATE																							
Object: D1900V2 - SN: 5d136																							
Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits																							
Calibration date: June 7, 2022																							
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																							
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±1)°C and humidity <70%.																							
Calibration Equipment used (M&TE critical for calibration)																							
<table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Calibrated by: Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Power Meter NRP2</td><td>106277</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Power sensor NRP6S</td><td>104291</td><td>24-Sep-21 (CTTL No.J21X08326)</td><td>Sep-22</td></tr><tr><td>Reference Probe EXSDV4</td><td>SN 7464</td><td>28-Jan-22 (SPEAG No EX3-7464_Jan22)</td><td>Jan-23</td></tr><tr><td>DAE4</td><td>SN 1656</td><td>12-Jan-22 (CTTL-SPEAG No Z22-60007)</td><td>Jan-23</td></tr></tbody></table>				Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration	Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRP6S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EXSDV4	SN 7464	28-Jan-22 (SPEAG No EX3-7464_Jan22)	Jan-23	DAE4	SN 1656	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration																				
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Power sensor NRP6S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22																				
Reference Probe EXSDV4	SN 7464	28-Jan-22 (SPEAG No EX3-7464_Jan22)	Jan-23																				
DAE4	SN 1656	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23																				
<table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Cal Date (Calibrated by: Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Signal Generator E4438C</td><td>MY48071430</td><td>13-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr><tr><td>Network Analyzer E5071C</td><td>MY48110073</td><td>14-Jan-22 (CTTL No.J22X00409)</td><td>Jan-23</td></tr></tbody></table>				Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyzer E5071C	MY48110073	14-Jan-22 (CTTL No.J22X00409)	Jan-23								
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration																				
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Network Analyzer E5071C	MY48110073	14-Jan-22 (CTTL No.J22X00409)	Jan-23																				
Calibrated by: Name: Zhao Jing, Function: SAR Test Engineer, Signature: [Signature]																							
Reviewed by: Name: Lin Hao, Function: SAR Test Engineer, Signature: [Signature]																							
Approved by: Name: Qi Diqian, Function: SAR Project Leader, Signature: [Signature]																							
Issued: June 13, 2022																							
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																							
Certificate No: Z22-60185		Page 1 of 6																					

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: cti@china.com.cn		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: cti@china.com.cn	
Measurement Conditions		Appendix (Additional assessments outside the scope of CNAS L0570)	
DASY Version: DASY52		Antenna Parameters with Head TSL	
Extrapolation: Advanced Extrapolation		Impedance, transformed to feed point: 51.02 ± 7.58Ω	
Phantom: Triple Flat Phantom 5.1C		Return Loss: -22.4dB	
Distance Dipole Center - TSL: 10 mm		General Antenna Parameters and Design	
Zoom Scan Resolution: 6x, 6y, 6z = 5 mm		Electrical Delay (one direction): 1.109 ns	
Frequency: 1900 MHz ± 1 MHz		After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.	
Head TSL parameters		The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.	
The following parameters and calculations were applied:		Additional EUT Data	
Nominal Head TSL parameters: Temperature: 22.0 °C, Permittivity: 40.0, Conductivity: 1.40 return		Manufactured by: SPEAG	
Measured Head TSL parameters: (22.0 ± 0.5) °C, 39.9 ± 6 %, 1.39 return ± 6 %			
Head TSL temperature change during test: <+1.0 °C			
SAR result with Head TSL			
SAR averaged over 1 cm² (1 g) of Head TSL			
SAR measured: 250 mW input power			
SAR for nominal Head TSL parameters: normalized to 1W			
SAR averaged over 10 cm² (10 g) of Head TSL			
SAR measured: 250 mW input power			
SAR for nominal Head TSL parameters: normalized to 1W			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60185		Page 2 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: cti@china.com.cn		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: cti@china.com.cn	
Measurement Conditions		Appendix (Additional assessments outside the scope of CNAS L0570)	
DASY Version: DASY52		Antenna Parameters with Head TSL	
Extrapolation: Advanced Extrapolation		Impedance, transformed to feed point: 51.02 ± 7.58Ω	
Phantom: Triple Flat Phantom 5.1C		Return Loss: -22.4dB	
Distance Dipole Center - TSL: 10 mm		General Antenna Parameters and Design	
Zoom Scan Resolution: 6x, 6y, 6z = 5 mm		Electrical Delay (one direction): 1.109 ns	
Frequency: 1900 MHz ± 1 MHz		After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.	
Head TSL parameters		The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.	
The following parameters and calculations were applied:		Additional EUT Data	
Nominal Head TSL parameters: Temperature: 22.0 °C, Permittivity: 40.0, Conductivity: 1.40 return		Manufactured by: SPEAG	
Measured Head TSL parameters: (22.0 ± 0.5) °C, 39.9 ± 6 %, 1.39 return ± 6 %			
Head TSL temperature change during test: <+1.0 °C			
SAR result with Head TSL			
SAR averaged over 1 cm² (1 g) of Head TSL			
SAR measured: 250 mW input power			
SAR for nominal Head TSL parameters: normalized to 1W			
SAR averaged over 10 cm² (10 g) of Head TSL			
SAR measured: 250 mW input power			
SAR for nominal Head TSL parameters: normalized to 1W			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60185		Page 3 of 6	

TTL S p e a g CALIBRATION LABORATORY		CAICT	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: cti@china.com.cn		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: cti@china.com.cn	
Measurement Conditions		Appendix (Additional assessments outside the scope of CNAS L0570)	
DASY Version: DASY52		Antenna Parameters with Head TSL	
Extrapolation: Advanced Extrapolation		Impedance, transformed to feed point: 51.02 ± 7.58Ω	
Phantom: Triple Flat Phantom 5.1C		Return Loss: -22.4dB	
Distance Dipole Center - TSL: 10 mm		General Antenna Parameters and Design	
Zoom Scan Resolution: 6x, 6y, 6z = 5 mm		Electrical Delay (one direction): 1.109 ns	
Frequency: 1900 MHz ± 1 MHz		After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.	
Head TSL parameters		The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.	
The following parameters and calculations were applied:		Additional EUT Data	
Nominal Head TSL parameters: Temperature: 22.0 °C, Permittivity: 40.0, Conductivity: 1.40 return		Manufactured by: SPEAG	
Measured Head TSL parameters: (22.0 ± 0.5) °C, 39.9 ± 6 %, 1.39 return ± 6 %			
Head TSL temperature change during test: <+1.0 °C			
SAR result with Head TSL			
SAR averaged over 1 cm² (1 g) of Head TSL			
SAR measured: 250 mW input power			
SAR for nominal Head TSL parameters: normalized to 1W			
SAR averaged over 10 cm² (10 g) of Head TSL			
SAR measured: 250 mW input power			
SAR for nominal Head TSL parameters: normalized to 1W			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60185		Page 4 of 6	

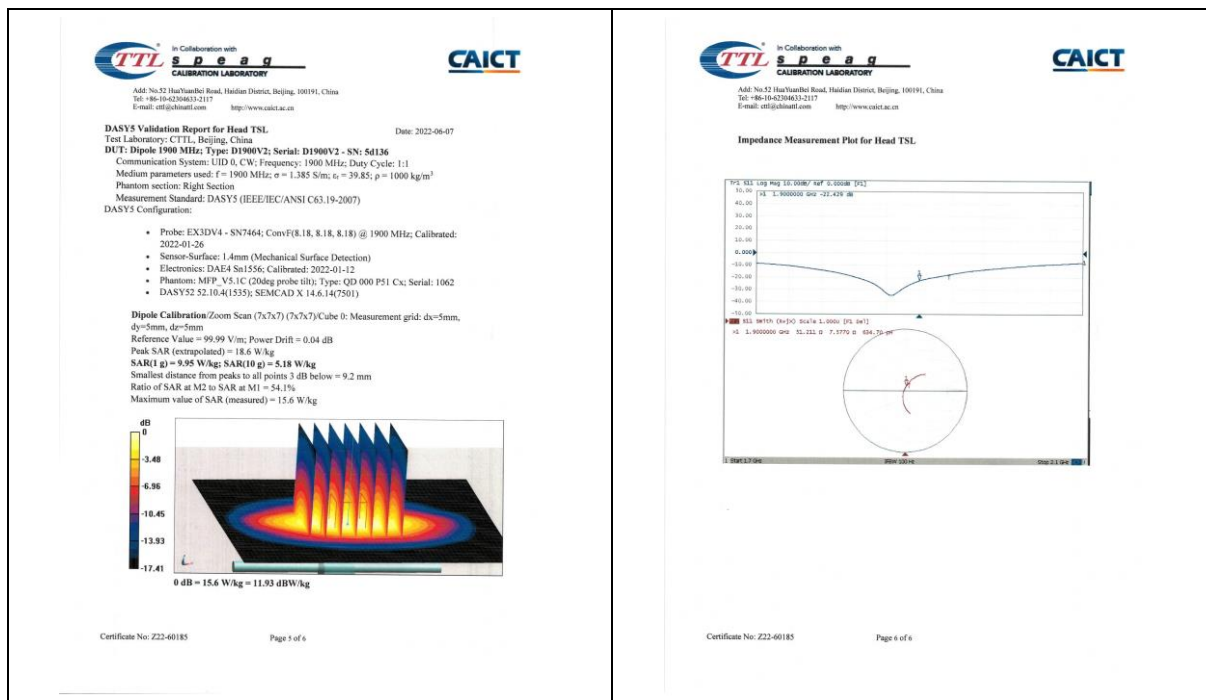

1.8 D2000V2 - SN 1041

Page 1 of 6: CALIBRATION CERTIFICATE

Client: SGS-CN Certificate No: Z22-60186
Object: D2000V2 - SN 1041
Calibration Procedure(s): FF-Z11-003-01
Calibration date: June 8, 2022
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (B). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.
All calibrations have been conducted in the closed laboratory facility; environment temperature (22±3)°C and humidity <70%.
Calibration Equipment used (MATE critical for calibration):
Primary Standards: ID #, Cal Date (Calibrated by Certificate No.), Scheduled Calibration
Secondary Standards: ID #, Cal Date (Calibrated by Certificate No.), Scheduled Calibration
Calibrated by: Zhao Jing, SAR Test Engineer
Reviewed by: Lin Hao, SAR Test Engineer
Approved by: Qi Danyuan, SAR Project Leader
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Page 2 of 6: Glossary

TSL: Issue simulating liquid
SAR: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured
Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz), October 2020
b) KOB 865964, "SAR Measurement Requirements for 100 MHz to 6 GHz"
Additional Documentation:
c) DASY4/5 System Handbook
Methods Applied and Interpretation of Parameters:
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
• SAR measured: SAR measured at the stated antenna input power.
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>, and, for electronic formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

In Collaboration with TTL CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239632-2117 E-mail: ott@china.ttl.com http://www.caict.ac.cn			
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom S.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2000 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.39 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	10.4 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 16.8 % (n=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.30 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 18.7 % (n=2)	
Certificate No: Z22-60186 Page 3 of 6			

In Collaboration with TTL CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239632-2117 E-mail: ott@china.ttl.com http://www.caict.ac.cn			
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48.4Ω ± 0.74Ω		
Return Loss	-34.9dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.088 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60186 Page 4 of 6			

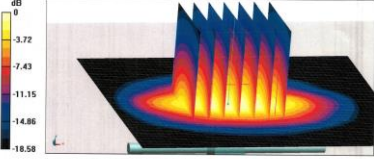In Collaboration with TTL CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239632-2117 E-mail: ott@china.ttl.com http://www.caict.ac.cn			
DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041 Communication System: UTD 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2000 MHz; σ = 1.392 S/m; ε _r = 40.21; ρ = 1000 kg/m ³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:			
• Probe: EX3DV4 - SN7464; ConvF(8.2, 8.2, 8.2) @ 2000 MHz; Calibrated: 2022-01-26			
• Sensor-Surface: 1.4mm (Mechanical Surface Detection)			
• Electronics: DA64 Sn1556; Calibrated: 2022-01-12			
• Phantom: MPP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062			
• DASY52 52.10.4(1555); SEMCAD X 14.6.14(7501)			
Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 103.4 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 19.6 W/kg SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg Smallest distance from peaks to all points 3 dB below = 9.1 mm Ratio of SAR at M2 to SAR at M1 = 53.6% Maximum value of SAR (measured) = 16.3 W/kg			
			
Certificate No: Z22-60186 Page 5 of 6			

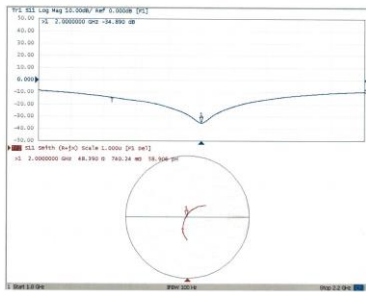In Collaboration with TTL CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4239632-2117 E-mail: ott@china.ttl.com http://www.caict.ac.cn			
Impedance Measurement Plot for Head TSL			
			
Certificate No: Z22-60186 Page 6 of 6			



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1.9 D2300V2 - SN 1096

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Client: SGS-CN		Certificate No: Z22-60106	
CALIBRATION CERTIFICATE			
Object	D2300V2 - SN: 1096		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRPBS	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX30V4	SN 7307	26-May-21 (SPEAG No.EK3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Diqian	SAR Project Leader	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60106		Page 1 of 6	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2300 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.70 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	—	—
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	12.4 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.88 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60106		Page 3 of 6	


TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	49.20 - 4.56jΩ		
Return Loss	-26.6dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.083 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60106		Page 4 of 6	



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 t(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 t(86-512)57370818 sgs.china@sgs.com

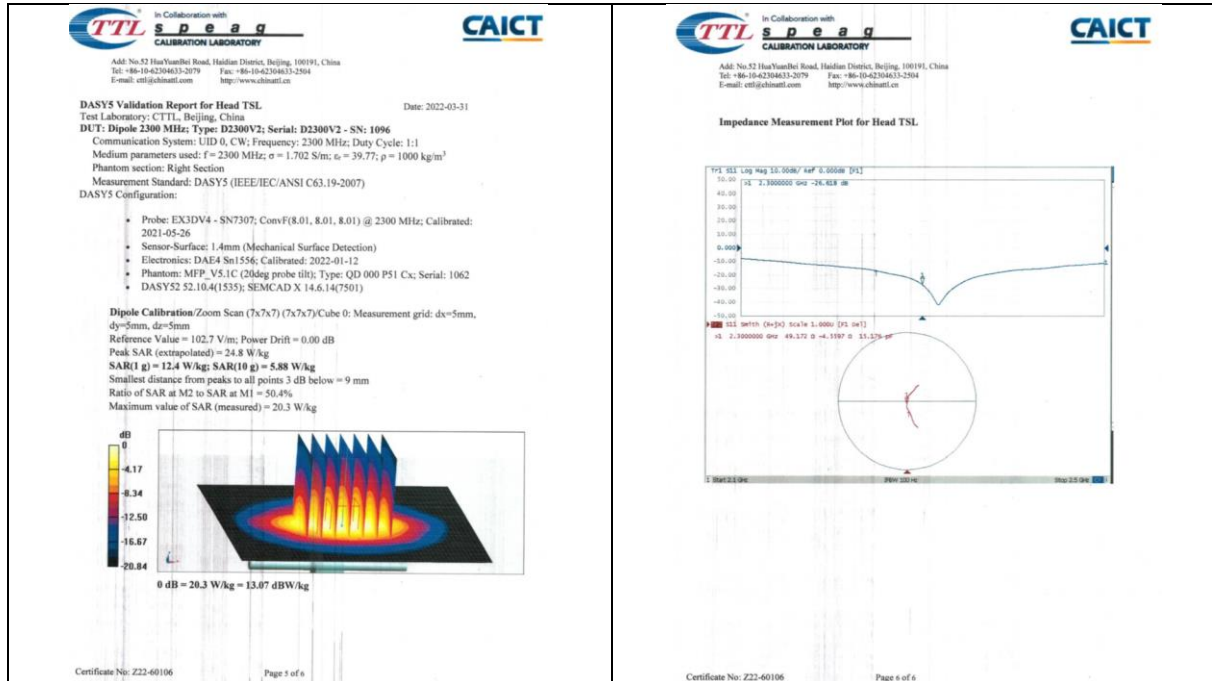

1.10 D2450V2 - SN 817

TTL *speaq* **CAICT**

In Collaboration with
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-2079 Fax: +86-10-62504633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60107**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN: 817**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **April 1, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Power sensor: NRP8S	104291	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG.No EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. J22X00406)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer Signature: *[Signature]*

Reviewed by: **Lin Hao** SAR Test Engineer Signature: *[Signature]*

Approved by: **Qi Dianyan** SAR Project Leader Signature: *[Signature]*

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 6

TTL *speaq* **CAICT**

In Collaboration with
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-2079 Fax: +86-10-62504633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60107 Page 2 of 6



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com


TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2450 MHz ± 1 MHz		

Head TSL parameters			
The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL		
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.15 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)

Certificate No: Z22-60107 Page 3 of 6

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn	
DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-04-01 DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817 Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; σ = 1.79 S/m; ε _r = 39.52; ρ = 1000 kg/m ³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: <ul style="list-style-type: none">Probe: EX3DV4 - SN7307; ConvF(7.75, 7.75, 7.75) @ 2450 MHz; Calibrated: 2021-05-26Sensor-Surface: 1.4mm (Mechanical Surface Detection)Electronics: DA14 Sni556; Calibrated: 2022-01-12Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 104.6 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 27.0 W/kg SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.15 W/kg Smallest distance from peaks to all points 3 dB below = 8.9 mm Ratio of SAR at M2 to SAR at M1 = -49.2% Maximum value of SAR (measured) = 22.1 W/kg			

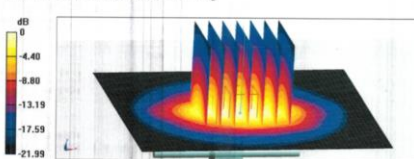

0 dB = 22.1 W/kg = 13.44 dBW/kg

Certificate No: Z22-60107 Page 5 of 6

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn	
Appendix (Additional assessments outside the scope of CNAS L0570) Antenna Parameters with Head TSL			
Impedance, transformed to feed point	52.10 ± 3.20 Ω		
Return Loss	-28.5 dB		


General Antenna Parameters and Design	
Electrical Delay (one direction)	1.066 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data	
Manufactured by	SPEAG

Certificate No: Z22-60107 Page 6 of 6

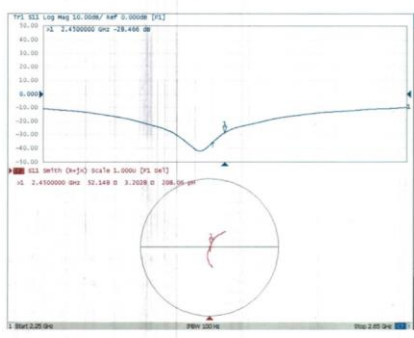TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn	
Impedance Measurement Plot for Head TSL			
			



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 t(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 t(86-512)57370818 sgs.china@sgs.com


1.11 D2600V2 - SN 1158

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaast.com.cn http://www.chinaast.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaast.com.cn http://www.chinaast.com	
Client: SGS-CN		Certificate No: Z22-60108	
CALIBRATION CERTIFICATE			
Object	D2600V2 - SN: 1158		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor: NRPBS	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DVA	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22
DAE4	SN 1158	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyuan	SAR Project Leader	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60108		Page 1 of 6	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaast.com.cn http://www.chinaast.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaast.com.cn http://www.chinaast.com	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2600 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.7 ± 6 %	1.96 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
	Condition		
SAR averaged over 1 cm² (1 g) of Head TSL			
SAR measured	250 mW input power	13.7 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm² (10 g) of Head TSL			
SAR measured	250 mW input power	6.12 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60108		Page 3 of 6	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaast.com.cn http://www.chinaast.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaast.com.cn http://www.chinaast.com	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NORMx.y.z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/S System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60108		Page 2 of 6	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaast.com.cn http://www.chinaast.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaast.com.cn http://www.chinaast.com	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	49.90-6.49jΩ		
Return Loss	-23.8dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.053 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60108		Page 4 of 6	

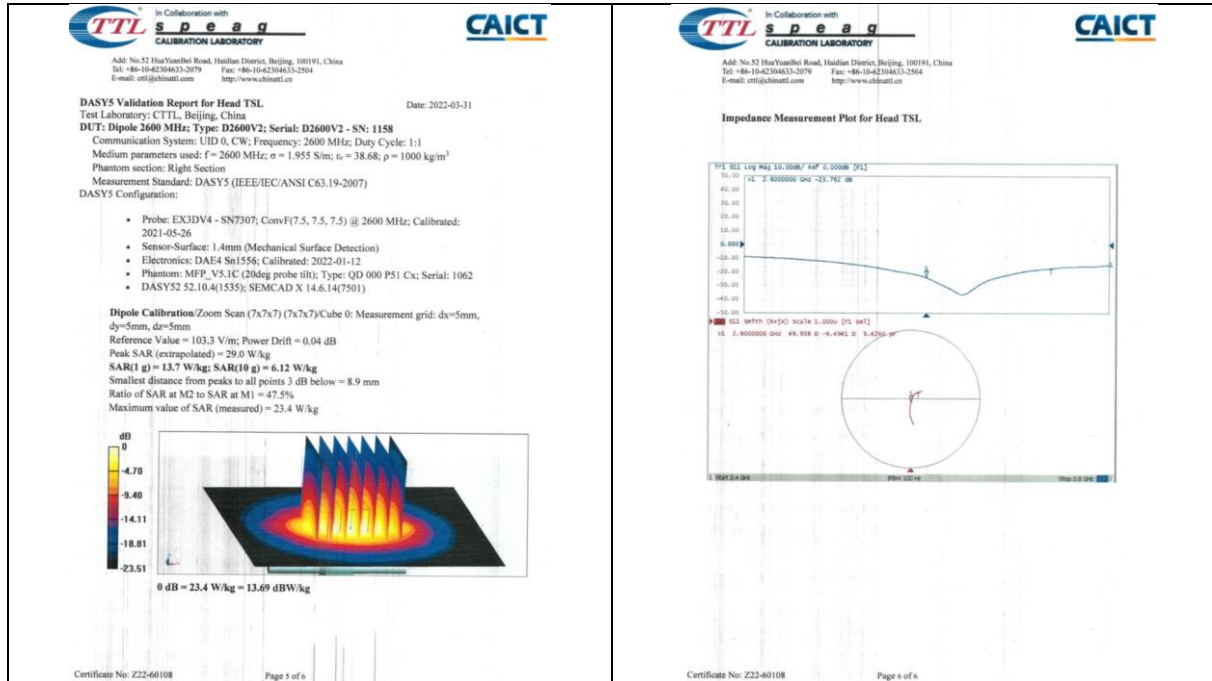

1.12 D5GHzV2 - SN 1095

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

Client: SGS-CN Certificate No: Z22-60187

CALIBRATION CERTIFICATE

Object: D5GHzV2 - SN: 1095

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: June 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21008328)	Sep-22
Power sensor NRP8S	104201	24-Sep-21 (CTTL No.J21008328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7464, Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00408)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyan SAR Project Leader

Issued: June 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

Glossary:

TSL Issue simulating liquid
Sensitivity in TSL / NORM_{Mx,y,z} not applicable or not measured
N/A

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 2 of 10



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>; and, for electronic formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

In Collaboration with TTL s p e a q CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62362117 E-mail: csl@caict.ac.cn http://www.caict.ac.cn			
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)	
Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz		
Head TSL parameters at 5200MHz The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5200MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	7.79 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	77.8 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.22 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)	
Certificate No: Z22-60187 Page 3 of 10			

In Collaboration with TTL s p e a q CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62362117 E-mail: csl@caict.ac.cn http://www.caict.ac.cn			
Head TSL parameters at 5300MHz The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5300MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	7.94 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.27 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)	
Head TSL parameters at 5500MHz The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.8	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.94 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5500MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	8.29 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	82.6 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.34 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)	
Certificate No: Z22-60187 Page 4 of 10			

In Collaboration with TTL s p e a q CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62362117 E-mail: csl@caict.ac.cn http://www.caict.ac.cn			
Head TSL parameters at 5600MHz The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5600MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	8.12 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.30 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 24.2 % (k=2)	
Head TSL parameters at 5800MHz The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL at 5800MHz			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	100 mW input power	7.71 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	100 mW input power	2.16 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	21.6 W/kg ± 24.2 % (k=2)	
Certificate No: Z22-60187 Page 5 of 10			

In Collaboration with TTL s p e a q CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62362117 E-mail: csl@caict.ac.cn http://www.caict.ac.cn			
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL at 5200MHz			
Impedance, transformed to feed point	48.1D-5.03jΩ		
Return Loss	-23.6dB		
Antenna Parameters with Head TSL at 5300MHz			
Impedance, transformed to feed point	47.8D-2.42jΩ		
Return Loss	-28.5dB		
Antenna Parameters with Head TSL at 5500MHz			
Impedance, transformed to feed point	50.3D-4.26jΩ		
Return Loss	-27.4dB		
Antenna Parameters with Head TSL at 5600MHz			
Impedance, transformed to feed point	54.5D-4.80jΩ		
Return Loss	-24.0dB		
Antenna Parameters with Head TSL at 5800MHz			
Impedance, transformed to feed point	51.5D-5.61jΩ		
Return Loss	-24.9dB		
Certificate No: Z22-60187 Page 6 of 10			



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

<p>In Collaboration with TTL s p e a q CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62920117 E-mail: cs@sgs.com http://www.caict.ac.cn</p> <p>General Antenna Parameters and Design</p> <p>Electrical Delay (one direction) 1.101 ns</p> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.</p> <p>No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <p>Manufactured by SPEAG</p> <p>Certificate No: Z22-60187 Page 7 of 10</p>	<p>In Collaboration with TTL s p e a q CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62920117 E-mail: cs@sgs.com http://www.caict.ac.cn</p> <p>DASY5 Validation Report for Head TSL</p> <p>Test Laboratory: CTTL, Beijing, China Date: 2022-06-01</p> <p>DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095</p> <p>Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: $f = 5200$ MHz; $\sigma = 4.62$ S/m; $\epsilon_r = 35.19$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5300$ MHz; $\sigma = 4.73$ S/m; $\epsilon_r = 35.19$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5500$ MHz; $\sigma = 4.939$ S/m; $\epsilon_r = 34.83$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5600$ MHz; $\sigma = 5.051$ S/m; $\epsilon_r = 34.88$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5800$ MHz; $\sigma = 5.247$ S/m; $\epsilon_r = 34.42$; $\rho = 1000$ kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:</p> <ul style="list-style-type: none">Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz; Calibrated: 2022-01-26Sensor-Surface: 1.4mm (Mechanical Surface Detection)Electronics: DA64 Sn1556; Calibrated: 2022-01-12Phantom: MPF_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) <p>Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 60.80 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 18.3 W/kg</p> <p>Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg</p> <p>Certificate No: Z22-60187 Page 8 of 10</p>
<p>In Collaboration with TTL s p e a q CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62920117 E-mail: cs@sgs.com http://www.caict.ac.cn</p> <p>Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.7 W/kg SAR(1 g) = 8.28 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg</p> <p>Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.2 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg</p> <p>Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 62.13 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 34.8 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg</p> <p>0 dB = 16.7 W/kg = 12.72 dBW/kg</p> <p>Certificate No: Z22-60187 Page 9 of 10</p>	<p>In Collaboration with TTL s p e a q CALIBRATION LABORATORY</p> <p>CAICT</p> <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62920117 E-mail: cs@sgs.com http://www.caict.ac.cn</p> <p>Impedance Measurement Plot for Head TSL</p> <p>TP1: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP2: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP3: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP4: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP5: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP6: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP7: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP8: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP9: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP10: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP11: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP12: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP13: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP14: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP15: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP16: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP17: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP18: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP19: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP20: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP21: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP22: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP23: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP24: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP25: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP26: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP27: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP28: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP29: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP30: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP31: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP32: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP33: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP34: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP35: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP36: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP37: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP38: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP39: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP40: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP41: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP42: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP43: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP44: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP45: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP46: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP47: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP48: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP49: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP50: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP51: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP52: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP53: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP54: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP55: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP56: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP57: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP58: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP59: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP60: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP61: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP62: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP63: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP64: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP65: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP66: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP67: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP68: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP69: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP70: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP71: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP72: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP73: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP74: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP75: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP76: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP77: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP78: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP79: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP80: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP81: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP82: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP83: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP84: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP85: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP86: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP87: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP88: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP89: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP90: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP91: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP92: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP93: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP94: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP95: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP96: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP97: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP98: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP99: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>TP100: S11 [dB] mag 13.00000 / ref 0.00000 [dB]</p> <p>Certificate No: Z22-60187 Page 10 of 10</p>



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgs.com
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

2 DAE4 - SN 1245

<p>Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9770 www.spgs.ch, info@spgs.ch</p> <p style="text-align: center;">s p e a g</p> <p style="text-align: center;">IMPORTANT NOTICE</p> <p>USAGE OF THE DAE4</p> <p>The DAE4 unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE4. Special attention shall be given to the following points:</p> <p>Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw, over tightening the screw may cause the threads inside the DAE4 to wear out.</p> <p>Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an anti-static bag. This anti-static bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.</p> <p>E-stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE4 carefully and keep the DAE4 unit in a non-dusty environment if not used for measurements.</p> <p>Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.</p> <p>DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE4 unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.</p> <p>Important Note: Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.</p> <p>Important Note: Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.</p> <p>Important Note: To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.</p> <p>TN_EH190306AE DAE4.docx 07.03.2019</p>	<p>Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Accreditation No.: SCS 0108</p> <p>Client: SGS-CN (Auden) Certificate No.: DAE4-1245_May22</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: DAE4 - SD 000 D04 BM - SN: 1245</p> <p>Calibration procedure(s): QA CAL-06 v30 Calibration procedure for the data acquisition electronics (DAE)</p> <p>Calibration date: May 30, 2022</p> <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3) °C and humidity < 70%.</p> <p>Calibration Equipment used (MATE critical for calibration)</p> <table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Ketley Multimeter Type 2001</td><td>SN: 0810276</td><td>31-Aug-21 (No.31368)</td><td>Aug-22</td></tr></tbody></table> <table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Check Date (in house)</th><th>Scheduled Check</th></tr></thead><tbody><tr><td>Auto DAE Calibration Unit</td><td>SE LWS 003 AA 1001</td><td>24-Jan-22 (in house check)</td><td>In house check: Jan-23</td></tr><tr><td>Calibrator Blue V2.1</td><td>SE LWS 006 AA 1002</td><td>24-Jan-22 (in house check)</td><td>In house check: Jan-23</td></tr></tbody></table> <p>Calibrated by: Dominique Stettin Function: Laboratory Technician Signature: <i>[Signature]</i></p> <p>Approved by: Ben Kohn Technical Manager Signature: <i>[Signature]</i></p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: May 30, 2022</p> <p>Certificate No: DAE4-1245_May22 Page 1 of 5</p>	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Ketley Multimeter Type 2001	SN: 0810276	31-Aug-21 (No.31368)	Aug-22	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Auto DAE Calibration Unit	SE LWS 003 AA 1001	24-Jan-22 (in house check)	In house check: Jan-23	Calibrator Blue V2.1	SE LWS 006 AA 1002	24-Jan-22 (in house check)	In house check: Jan-23
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																		
Ketley Multimeter Type 2001	SN: 0810276	31-Aug-21 (No.31368)	Aug-22																		
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																		
Auto DAE Calibration Unit	SE LWS 003 AA 1001	24-Jan-22 (in house check)	In house check: Jan-23																		
Calibrator Blue V2.1	SE LWS 006 AA 1002	24-Jan-22 (in house check)	In house check: Jan-23																		
<p>Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Accreditation No.: SCS 0108</p> <p>Glossary DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system.</p> <p>Methods Applied and Interpretation of Parameters</p> <ul style="list-style-type: none">• DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.• Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.• The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.<ul style="list-style-type: none">• DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.• Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.• Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.• AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage.• Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.• Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.• Input resistance: Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement.• Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.• Power consumption: Typical value for information. Supply currents in various operating modes. <p>Certificate No: DAE4-1245_May22 Page 2 of 5</p>	<p>DC Voltage Measurement</p> <p>AD - Converter Resolution nominal High Range: 1LSB = 6.1 μV, full range = -190...+320 mV Low Range: 1LSB = 61 μV, full range = -1...+3 mV DASY measurement parameters: Auto Zero-Time: 3 sec; Measuring time: 3 sec</p> <table border="1"><thead><tr><th>Calibration Factors</th><th>X</th><th>Y</th><th>Z</th></tr></thead><tbody><tr><td>High Range</td><td>405.265 ± 0.02% (k=2)</td><td>403.974 ± 0.02% (k=2)</td><td>406.092 ± 0.02% (k=2)</td></tr><tr><td>Low Range</td><td>3.99534 ± 1.50% (k=2)</td><td>3.99508 ± 1.50% (k=2)</td><td>4.01015 ± 1.50% (k=2)</td></tr></tbody></table> <p>Connector Angle</p> <table border="1"><thead><tr><th>Connector Angle to be used in DASY system</th><th>30.0° ± 1°</th></tr></thead></table> <p>Certificate No: DAE4-1245_May22 Page 3 of 5</p>	Calibration Factors	X	Y	Z	High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)	Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)	Connector Angle to be used in DASY system	30.0° ± 1°						
Calibration Factors	X	Y	Z																		
High Range	405.265 ± 0.02% (k=2)	403.974 ± 0.02% (k=2)	406.092 ± 0.02% (k=2)																		
Low Range	3.99534 ± 1.50% (k=2)	3.99508 ± 1.50% (k=2)	4.01015 ± 1.50% (k=2)																		
Connector Angle to be used in DASY system	30.0° ± 1°																				



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	19994.45	1.52	0.00
Channel X - Input	20004.58	2.22	0.01
Channel X + Input	-20001.14	1.12	-0.01
Channel Y + Input	19994.72	1.58	0.00
Channel Y - Input	20001.22	-1.00	-0.00
Channel Y + Input	-20003.05	-1.57	0.01
Channel Z + Input	19992.44	0.19	0.00
Channel Z - Input	20003.09	0.58	0.00
Channel Z + Input	-20001.73	-0.27	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2001.91	0.41	0.02
Channel X - Input	202.54	0.65	0.32
Channel X + Input	-197.86	0.07	-0.04
Channel Y + Input	2002.05	0.58	0.03
Channel Y - Input	201.27	-0.57	-0.28
Channel Y + Input	-196.23	-0.06	0.03
Channel Z + Input	2001.96	0.08	0.00
Channel Z - Input	200.09	-1.53	-0.76
Channel Z + Input	-199.85	-1.57	0.79

2. Common mode sensitivity

Common mode Input Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)
Channel X	-5.87	-7.69
-200	9.12	7.79
Channel Y	-8.68	-9.28
-200	8.52	6.36
Channel Z	-5.36	-5.60
-200	3.58	3.06

3. Channel separation

Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	-	4.07
Channel Y	200	9.36	-
Channel Z	200	7.14	-

Certificate No: DAE4-1245, May22

Page 4 of 5

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15984	17040
Channel Y	16562	16768
Channel Z	16035	15968

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input (mV)	Average (µV)	min. Offset (µV)	max. Offset (µV)	Std. Deviation (µV)
Channel X	1.00	-0.15	1.93	0.45
Channel Y	-0.18	-1.28	0.94	0.45
Channel Z	-0.58	-2.61	0.58	0.60

6. Input Offset Current

Nominal input circuitry offset current on all channels: <25nA

7. Input Resistance (Typical values for information)

	Zeroing (Ohm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+8	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1245, May22

Page 5 of 5

3 EX3DV4 - SN 7346

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zugstrasse 6, 8684 Zurich, SwitzerlandS Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration ServiceAccredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client: Auden

Certificate No: EX3-7346_Mar22

CALIBRATION CERTIFICATE

Object: EX3DV4 - SN 7346

Calibration procedure(s): QA CAL-01 v8; QA CAL-14 v6; QA CAL-23 v5; QA CAL-25 v7
Calibration procedure for dosimetric E-field probes

Calibration date: March 30, 2022

This calibration certificate documents the traceability to national standards, which involve the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3) °C and humidity < 70%.

Calibration Equipment used (MATE critical for calibration):

Primary Standards	SI	Cal Date (Certificate No.)	Scheduled Calibration
Power meter MNP	SR 10478	08-Apr-21 (No. 217-02501-02502)	Apr-22
Power sensor MNP-291	SR 10304	08-Apr-21 (No. 217-02501)	Apr-22
Power sensor MNP-291	SR 10304	08-Apr-21 (No. 217-02502)	Apr-22
Reference 20 dB attenuator	SR C2253 (20)	08-Apr-21 (No. 217-02503)	Apr-22
DAEA	SR 460	13-Dec-21 (No. DAE4-485, 04031)	Dec-22
Reference Probe (S3302)	SR 3013	27-Dec-21 (No. E53-3013, Dec21)	Dec-22

Secondary Standards	SI	Check Date (in house)	Scheduled Calibration
Power meter E4415B	SR G84125074	08-Apr-21 (in house check Jun-20)	In house check Jun-22
Power sensor E4412A	SR MY4148687	08-Apr-21 (in house check Jun-20)	In house check Jun-22
Power sensor E4412A	SR 40011010	08-Apr-21 (in house check Jun-20)	In house check Jun-22
RF generator HP 8446C	SR US340101709	04-Apr-20 (in house check Jun-20)	In house check Jun-22
Network Analyzer E5730A	SR US41050477	31-Mar-14 (in house check Dec-20)	In house check Dec-22

Calibrated by: Name: Sven Kuhn, Function: Laboratory Technician, Signature: [Signature]
Approved by: Sven Kuhn, Deputy Manager, Signature: [Signature]

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-7346_Mar22

Page 1 of 24

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zugstrasse 6, 8684 Zurich, SwitzerlandS Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration ServiceAccredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary:

TSL	Issue simulating liquid
NORM _{M,x,y,z}	sensitivity in free space
Conf _F	sensitivity in TSL / NORM _{M,x,y,z}
DCP	diode compression point
CF	crest factor (10µs duty cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization ψ	ψ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62208-1:2018, "Measurement Procedure For the Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1:351: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020
- b) KOB 805664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{M,x,y,z}: Assessed for E-field polarization $\psi = 0$ (if $f < 800$ MHz in TEM-cell; $f > 800$ MHz: R22 waveguide). NORM_{M,x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{M,x,y,z} do not affect the E-field uncertainty inside TSL (see below Conf_F).
- NORM_{M,x,y,z} = NORM_{M,x,y,z} * Frequency response (see Frequency Response Chart). This linearization is implemented in DASY4 software version later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of Conf_F.
- DCP_{M,x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAC: PAC is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A_{x,y,z}, B_{x,y,z}, C_{x,y,z}, D_{x,y,z}, V_{th,x,y,z}: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. V_{th} is the maximum calibration range expressed in RMS voltage across the diode.
- Conf_F and Boundary Effect Parameters: Assessed in far phantom using E-field (or Temperature Transfer Standard for $f < 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same values are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are to NORM_{M,x,y,z} * Conf_F whereby the uncertainty corresponds to that given for Conf_F. A frequency dependent Conf_F is used in DASY4 version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy / DCP deviation from isotropy: ψ in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORM_M (no uncertainty required).

Certificate No: EX3-7346_Mar22

Page 2 of 24



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weyue Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

EX3DV4 - SN:7346

March 30, 2022

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc. (k=2)
Norm. $\mu V/(V/m)^2$	0.46	0.47	0.61	$\pm 10.1\%$
DCP (mV) ²	101.4	106.0	106.9	

Calibration Results for Modulation Response

UID	Communication System Name	A dB	B dB- μV	C dB	VR mV	Max dev.	Max Unc ¹ (k=2)
0	CW	X: 0.00 Y: 0.00 Z: 0.00	0.00 0.00 0.00	1.00 1.00 1.00	0.00 0.00 0.00	143.5 135.3 139.0	$\pm 3.5\%$ $\pm 3.5\%$ $\pm 3.5\%$
10035-AAA	Pulse Waveform (200Hz, 10%)	X: 3.33 Y: 4.03 Z: 1.63	68.90 79.70 61.25	11.66 12.35 6.76	10.00 66.0 66.0	$\pm 3.5\%$ $\pm 3.5\%$ $\pm 3.5\%$	$\pm 9.6\%$ $\pm 9.6\%$ $\pm 9.6\%$
10035-AAA	Pulse Waveform (200Hz, 20%)	X: 3.30 Y: 11.31 Z: 0.83	79.65 81.32 69.90	11.31 14.72 5.11	6.99 86.0 86.0	$\pm 2.4\%$ $\pm 2.7\%$ $\pm 2.7\%$	$\pm 9.6\%$ $\pm 9.6\%$ $\pm 9.6\%$
10035-AAA	Pulse Waveform (200Hz, 40%)	X: 7.41 Y: 26.03 Z: 0.18	79.85 81.42 138.38	12.51 15.51 0.01	3.88 95.0 95.0	$\pm 2.7\%$ $\pm 2.7\%$ $\pm 1.7\%$	$\pm 9.6\%$ $\pm 9.6\%$ $\pm 9.6\%$
10035-AAA	Pulse Waveform (200Hz, 60%)	X: 22.77 Y: 20.90 Z: 7.84	71.13 81.58 138.51	9.52 16.29 16.47	2.32 120.0 120.0	$\pm 1.7\%$ $\pm 1.7\%$ $\pm 1.7\%$	$\pm 9.6\%$ $\pm 9.6\%$ $\pm 9.6\%$
10037-AAA	GRK Waveform, 1 MHz	X: 1.47 Y: 1.56 Z: 0.43	64.88 66.27 67.88	13.82 14.65 11.05	1.00 0.00 150.0	$\pm 4.2\%$ $\pm 4.2\%$ $\pm 1.1\%$	$\pm 9.6\%$ $\pm 9.6\%$ $\pm 9.6\%$
10038-AAA	GRK Waveform, 10 MHz	X: 2.08 Y: 2.08 Z: 2.08	67.33 67.33 67.33	13.38 13.38 13.38	150.0 150.0 150.0	$\pm 1.1\%$ $\pm 1.1\%$ $\pm 1.1\%$	$\pm 9.6\%$ $\pm 9.6\%$ $\pm 9.6\%$
10036-AAA	64-QAM Waveform, 100 MHz	X: 2.43 Y: 2.43 Z: 1.70	68.51 68.51 64.72	18.25 18.25 15.99	3.01 150.0 150.0	$\pm 1.0\%$ $\pm 1.0\%$ $\pm 2.0\%$	$\pm 9.6\%$ $\pm 9.6\%$ $\pm 9.6\%$
10036-AAA	64-QAM Waveform, 40 MHz	X: 3.38 Y: 3.38 Z: 2.70	66.82 66.82 65.72	15.96 15.96 14.74	0.00 150.0 150.0	$\pm 2.0\%$ $\pm 2.0\%$ $\pm 3.6\%$	$\pm 9.6\%$ $\pm 9.6\%$ $\pm 9.6\%$
10041-AAA	WLAN CDDF, 64-QAM, 40MHz	X: 4.11 Y: 4.70 Z: 3.83	65.35 65.54 66.16	15.77 15.41 15.28	0.00 150.0 150.0	$\pm 3.6\%$ $\pm 3.6\%$ $\pm 3.6\%$	$\pm 9.6\%$ $\pm 9.6\%$ $\pm 9.6\%$

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

* The uncertainties of Norm. V, Z do not affect the E-field uncertainty inside T10, (see Pages 5 and 6)

* Numerical simulation parameter, uncertainty not required

* Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX3-7346_Mar22

Page 3 of 34

EX3DV4 - SN:7346

March 30, 2022

DASY/EASY - Parameters of Probe: EX3DV4 - SN:7346

Sensor Model Parameters

C1	C2	a	T1	T2	T3	T4	T5	T6
IP	IP	V ²	ms.V ²	ms.V ²	ms	V ²	V ²	V ²
X	39.2	291.80	35.10	5.63	0.33	5.02	1.42	0.12
Y	37.1	270.84	34.12	5.29	0.30	5.01	1.82	0.05
Z	9.7	69.74	33.37	4.96	0.30	4.94	0.61	0.00


Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-166.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Note: Measurement distance from surface can be increased to 3-4 mm for an Area Scan job.

Certificate No: EX3-7346_Mar22

Page 4 of 34

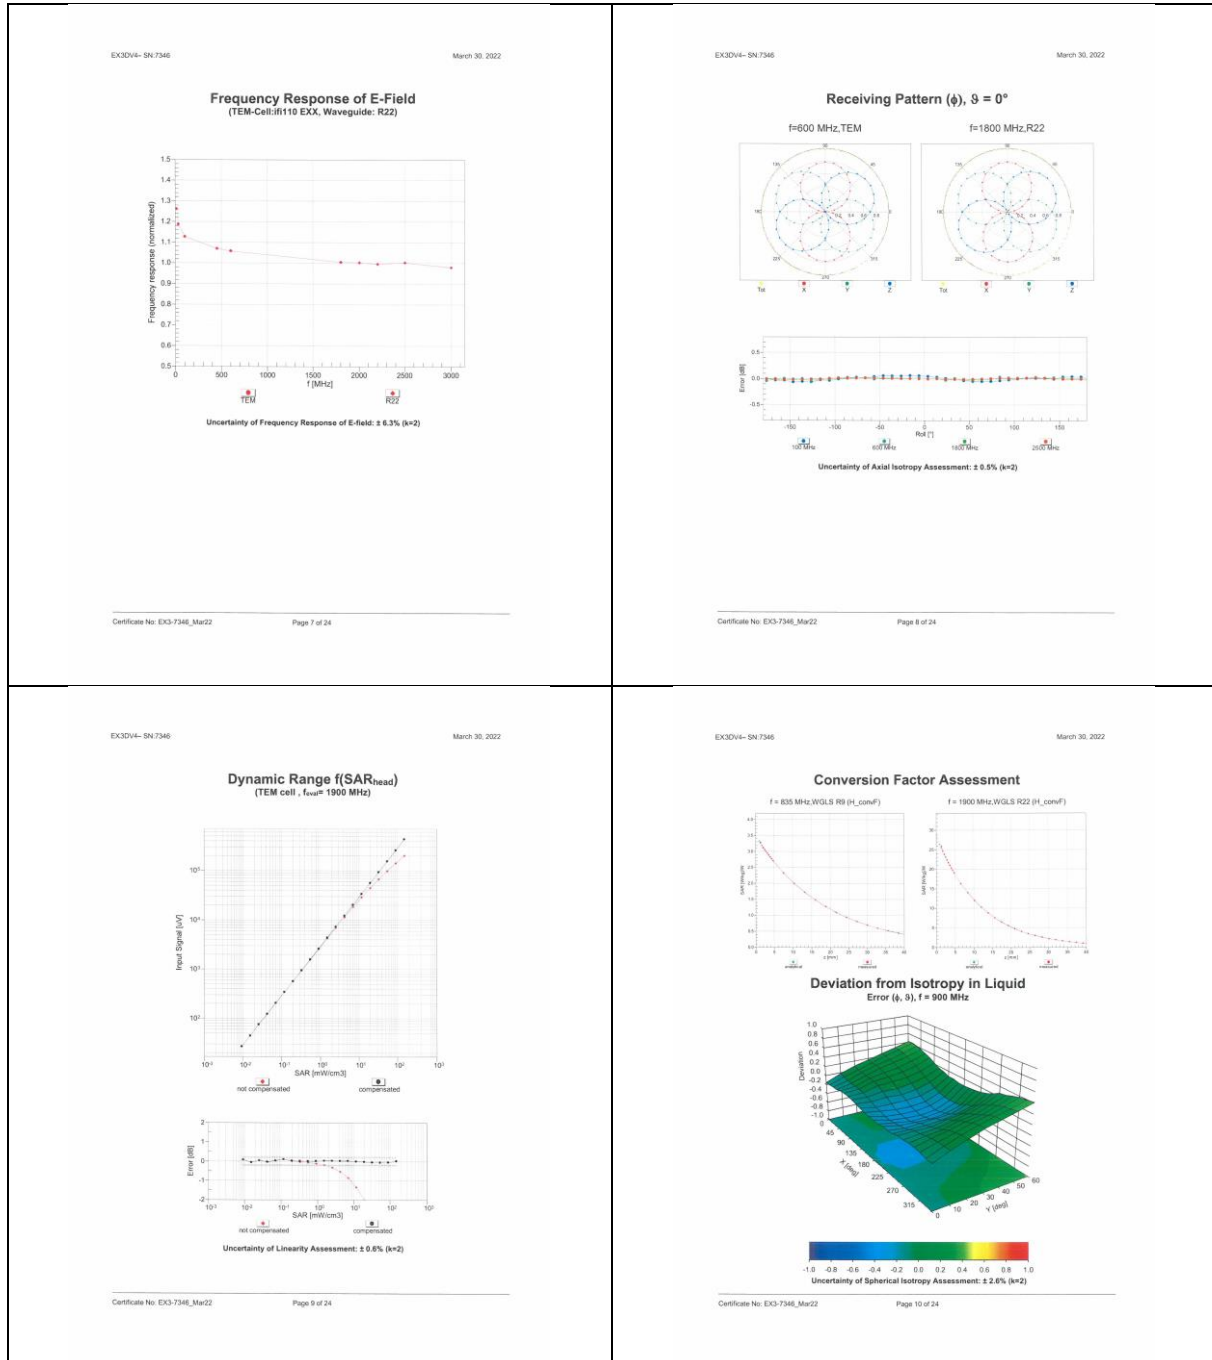

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学院创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



EKC3V4-SN-7346				March 30, 2022				EKC3V4-SN-7346				March 30, 2022			
Appendix: Modulation Calibration Parameters															
Uplink	Rev	Communication System Name	Group	FAR (dB)	Unc' (dB)										
10015	CAB	SAR Validation (SARmax: 100mW, 100mW)	CW	0.00	+4.7 dB			10100	CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	LTE-FDD	5.67	+3.6 dB		
10011	CAB	LAMTS FDD (WCDMA)	WCDMA	2.91	+3.6 dB			10101	CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	LTE-FDD	6.42	+3.6 dB		
10012	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS-OFDM, 1 Mbps)	WLAN	1.87	+3.6 dB			10102	CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	LTE-FDD	6.60	+3.6 dB		
10013	CAB	IEEE 802.11g WPAN 2.4 GHz (DSSS-OFDM, 6 Mbps)	WLAN	9.46	+3.6 dB			10103	CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	LTE-TDD	9.29	+3.6 dB		
10014	DAC	GSM-FDD (TDMA, GSM)	GSM	9.39	+3.6 dB			10104	CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	LTE-TDD	9.87	+3.6 dB		
10023	DAC	GPRS-FDD (TDMA, GPRS, TN-0)	GSM	9.57	+3.6 dB			10105	CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	LTE-TDD	10.01	+3.6 dB		
10024	DAC	GPRS-FDD (TDMA, GPRS, TN-0-1)	GSM	6.56	+3.6 dB			10106	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	LTE-FDD	3.80	+3.6 dB		
10025	DAC	EDGE-FDD (TDMA, GPRS, TN-0)	GSM	12.62	+3.6 dB			10107	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	LTE-FDD	6.43	+3.6 dB		
10026	DAC	EDGE-FDD (TDMA, GPRS, TN-0-1)	GSM	9.45	+3.6 dB			10108	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	LTE-FDD	5.75	+3.6 dB		
10027	DAC	GPRS-FDD (TDMA, GPRS, TN-0-2)	GSM	4.80	+3.6 dB			10109	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	LTE-FDD	6.43	+3.6 dB		
10028	DAC	GPRS-FDD (TDMA, GPRS, TN-0-2b)	GSM	3.55	+3.6 dB			10110	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	LTE-FDD	6.43	+3.6 dB		
10029	DAC	EDGE-FDD (TDMA, GPRS, TN-0-3)	GSM	7.78	+3.6 dB			10111	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	LTE-FDD	6.43	+3.6 dB		
10030	CAA	IEEE 802.15.1 Bluetooth (GFSK, DSSS)	Bluetooth	5.20	+3.6 dB			10112	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	LTE-FDD	6.59	+3.6 dB		
10031	CAA	IEEE 802.15.1 Bluetooth (GFSK, DSSS)	Bluetooth	1.87	+3.6 dB			10113	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	LTE-FDD	6.62	+3.6 dB		
10032	CAA	IEEE 802.15.1 Bluetooth (PSS-OFDM, DSSS)	Bluetooth	1.16	+3.6 dB			10114	CAG	IEEE 802.11n (HT Overhead, 13.5 Mbps, BPSK)	WLAN	8.30	+3.6 dB		
10033	CAA	IEEE 802.15.1 Bluetooth (PSS-OFDM, DSSS)	Bluetooth	7.74	+3.6 dB			10115	CAG	IEEE 802.11n (HT Overhead, 13.5 Mbps, 16-QAM)	WLAN	8.46	+3.6 dB		
10034	CAA	IEEE 802.15.1 Bluetooth (PSS-OFDM, DSSS)	Bluetooth	4.53	+3.6 dB			10116	CAG	IEEE 802.11n (HT Overhead, 13.5 Mbps, 64-QAM)	WLAN	8.15	+3.6 dB		
10035	CAA	IEEE 802.15.1 Bluetooth (PSS-OFDM, DSSS)	Bluetooth	3.83	+3.6 dB			10117	CAG	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	WLAN	8.07	+3.6 dB		
10036	CAA	IEEE 802.15.1 Bluetooth (8-PSK, DSSS)	Bluetooth	8.01	+3.6 dB			10118	CAG	IEEE 802.11n (HT Mixed, 13.5 Mbps, 16-QAM)	WLAN	8.39	+3.6 dB		
10037	CAA	IEEE 802.15.1 Bluetooth (8-PSK, DSSS)	Bluetooth	4.77	+3.6 dB			10119	CAG	IEEE 802.11n (HT Mixed, 13.5 Mbps, 64-QAM)	WLAN	8.13	+3.6 dB		
10038	CAA	IEEE 802.15.1 Bluetooth (8-PSK, DSSS)	Bluetooth	4.10	+3.6 dB			10120	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	6.49	+3.6 dB		
10039	CAB	CDMA2000 (1XRTT, RCT)	CDMA2000	4.57	+3.6 dB			10121	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.53	+3.6 dB		
10040	CAB	IS-94 (IS-94-FDD) TDMA/FDD (PSS-OFDM, Full Rate)	AMPS	7.78	+3.6 dB			10122	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	5.73	+3.6 dB		
10041	CAB	IS-94 (IS-94-FDD) TDMA/FDD (PSS-OFDM, Full Rate)	AMPS	6.00	+3.6 dB			10123	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.25	+3.6 dB		
10042	CAB	IS-94 (IS-94-FDD) TDMA/FDD (PSS-OFDM, Full Rate)	AMPS	13.80	+3.6 dB			10124	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	6.49	+3.6 dB		
10043	CAB	IS-94 (IS-94-FDD) TDMA/FDD (PSS-OFDM, Full Rate)	AMPS	10.79	+3.6 dB			10125	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.41	+3.6 dB		
10044	CAB	LAMTS FDD (WCDMA, 1.28 Mbps)	WCDMA	11.01	+3.6 dB			10126	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	10.05	+3.6 dB		
10045	CAB	EDGE-FDD (TDMA, GPRS, TN-0-3)	GSM	6.82	+3.6 dB			10127	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	10.05	+3.6 dB		
10046	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 2 Mbps)	WLAN	2.12	+3.6 dB			10128	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	6.43	+3.6 dB		
10047	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 5.5 Mbps)	WLAN	2.83	+3.6 dB			10129	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.79	+3.6 dB		
10048	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	3.86	+3.6 dB			10130	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	6.43	+3.6 dB		
10049	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	8.68	+3.6 dB			10131	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.62	+3.6 dB		
10050	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	8.63	+3.6 dB			10132	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.66	+3.6 dB		
10051	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.09	+3.6 dB			10133	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.82	+3.6 dB		
10052	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.38	+3.6 dB			10134	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	6.43	+3.6 dB		
10053	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.12	+3.6 dB			10135	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10054	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.24	+3.6 dB			10136	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	5.73	+3.6 dB		
10055	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.56	+3.6 dB			10137	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.49	+3.6 dB		
10056	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.56	+3.6 dB			10138	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.49	+3.6 dB		
10057	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10139	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10058	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.62	+3.6 dB			10140	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10059	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	9.34	+3.6 dB			10141	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.49	+3.6 dB		
10060	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.30	+3.6 dB			10142	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10061	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.77	+3.6 dB			10143	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.49	+3.6 dB		
10062	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	10.84	+3.6 dB			10144	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.49	+3.6 dB		
10063	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10145	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10064	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10146	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10065	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10147	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10066	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10148	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10067	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10149	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10068	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10150	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10069	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10151	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10070	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10152	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10071	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10153	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10072	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10154	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10073	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10155	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10074	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10156	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10075	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10157	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10076	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10158	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10077	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10159	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10078	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10160	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10079	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10161	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10080	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10162	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10081	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10163	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10082	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10164	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10083	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10165	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10084	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10166	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10085	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10167	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10086	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10168	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10087	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10169	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10088	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10170	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10089	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10171	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		
10090	CAB	IEEE 802.11b WPAN 2.4 GHz (DSSS, 11 Mbps)	WLAN	11.00	+3.6 dB			10172	CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	5.73	+3.6 dB		

EX3034-SN-7346				March 30, 2022				EX3034-SN-7346				March 30, 2022			
10414	AAA	WLAN CDF: 64-QAM, 40MHz	Generic	8.54	> 9.8%			10489	AAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.31	> 9.8%		
10415	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS, 1 Mbps, R90c-d)	WLAN	1.54	> 9.8%			10490	AAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.54	> 9.8%		
10416	AAA	IEEE 802.11g WFI 2.4 GHz (OFDM, 6 Mbps, R90c-d)	WLAN	8.23	> 9.8%			10491	AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	7.74	> 9.8%		
10417	AAC	IEEE 802.11n WFI 5 GHz (OFDM, 6 Mbps, R90c-d)	WLAN	8.23	> 9.8%			10492	AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.41	> 9.8%		
10418	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS-OFDM, 6 Mbps, R90c, Long)	WLAN	8.14	> 9.8%			10493	AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.55	> 9.8%		
10419	AAA	IEEE 802.11g WFI 2.4 GHz (DSSS-OFDM, 6 Mbps, R90c, Short)	WLAN	8.19	> 9.8%			10494	AAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	7.74	> 9.8%		
10420	AAC	IEEE 802.11n HT Overhead, 7.2 Mbps, R90c-d	WLAN	8.32	> 9.8%			10495	AAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.37	> 9.8%		
10421	AAC	IEEE 802.11n HT Overhead, 6.3 Mbps, 16-QAM	WLAN	8.47	> 9.8%			10496	AAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.54	> 9.8%		
10424	AAO	IEEE 802.11n HT Overhead, 7.2 Mbps, 64-QAM	WLAN	8.40	> 9.8%			10497	AAB	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK, UL, Sub)	LTE-TDD	7.67	> 9.8%		
10425	AAC	IEEE 802.11n HT Overhead, 15 Mbps, R90c-d	WLAN	8.34	> 9.8%			10498	AAB	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.40	> 9.8%		
10428	AAC	IEEE 802.11n HT Overhead, 30 Mbps, 16-QAM	WLAN	8.45	> 9.8%			10499	AAB	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.68	> 9.8%		
10427	AAC	IEEE 802.11n HT Overhead, 150 Mbps, 64-QAM	WLAN	8.41	> 9.8%			10500	AAC	LTE-TDD (SC-FDMA, 100% RB, 3 Mbps, QPSK, UL, Sub)	LTE-TDD	7.67	> 9.8%		
10432	AAO	LTE-FDD (OFDMA, 5 MHz, E-TRP 3.1)	LTE-FDD	8.38	> 9.8%			10501	AAE	LTE-TDD (SC-FDMA, 100% RB, 3 Mbps, 16-QAM, UL, Sub)	LTE-TDD	8.44	> 9.8%		
10431	AAO	LTE-FDD (OFDMA, 10 MHz, E-TRP 3.1)	LTE-FDD	8.38	> 9.8%			10502	AAC	LTE-TDD (SC-FDMA, 100% RB, 3 Mbps, 64-QAM, UL, Sub)	LTE-TDD	8.52	> 9.8%		
10432	AAC	LTE-FDD (OFDMA, 15 MHz, E-TRP 3.1)	LTE-FDD	8.34	> 9.8%			10503	AAF	LTE-TDD (SC-FDMA, 100% RB, 3 Mbps, QPSK, UL, Sub)	LTE-TDD	7.72	> 9.8%		
10433	AAC	LTE-FDD (OFDMA, 20 MHz, E-TRP 3.1)	LTE-FDD	8.34	> 9.8%			10504	AAF	LTE-TDD (SC-FDMA, 100% RB, 3 Mbps, 16-QAM, UL, Sub)	LTE-TDD	8.31	> 9.8%		
10434	AAA	WCDMA (BS Test Model 1, 64 DPCCH)	WCDMA	8.80	> 9.8%			10505	AAF	LTE-TDD (SC-FDMA, 100% RB, 3 Mbps, 64-QAM, UL, Sub)	LTE-TDD	8.54	> 9.8%		
10435	AAF	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL, Sub)	LTE-TDD	7.82	> 9.8%			10506	AAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL, Sub)	LTE-TDD	7.74	> 9.8%		
10447	AAO	LTE-FDD (OFDMA, 5 MHz, E-TRP 3.1, Clipping 44%)	LTE-FDD	7.56	> 9.8%			10507	AAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.36	> 9.8%		
10448	AAO	LTE-FDD (OFDMA, 10 MHz, E-TRP 3.1, Clipping 44%)	LTE-FDD	7.53	> 9.8%			10508	AAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.35	> 9.8%		
10449	AAC	LTE-FDD (OFDMA, 15 MHz, E-TRP 3.1, Clipping 44%)	LTE-FDD	7.51	> 9.8%			10509	AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL, Sub)	LTE-TDD	7.99	> 9.8%		
10450	AAC	LTE-FDD (OFDMA, 20 MHz, E-TRP 3.1, Clipping 44%)	LTE-FDD	7.48	> 9.8%			10510	AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.49	> 9.8%		
10451	AAA	WCDMA (BS Test Model 1, 64 DPCCH, Clipping 44%)	WCDMA	7.59	> 9.8%			10511	AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.51	> 9.8%		
10452	AAD	Validation (Spurious, 10ms, 1ms)	Test	10.90	> 9.8%			10512	AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL, Sub)	LTE-TDD	7.74	> 9.8%		
10453	AAC	IEEE 802.11ac WFI (160MHz, 64-QAM, R90c-d)	WLAN	8.63	> 9.8%			10513	AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.42	> 9.8%		
10457	AAA	UMTS FDD (SC-FDMA)	WCDMA	6.62	> 9.8%			10514	AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.45	> 9.8%		
10458	AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	CDMA2000	8.58	> 9.8%			10515	AAA	IEEE 802.11a WFI 2.4 GHz (DSSS, 2 Mbps, R90c-d)	WLAN	1.58	> 9.8%		
10459	AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	CDMA2000	8.25	> 9.8%			10516	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS, 5.5 Mbps, R90c-d)	WLAN	1.57	> 9.8%		
10462	AAA	UMTS FDD (HSPA, R99)	WCDMA	2.39	> 9.8%			10517	AAA	IEEE 802.11b WFI 2.4 GHz (DSSS, 11 Mbps, R90c-d)	WLAN	1.58	> 9.8%		
10461	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL, Sub)	LTE-TDD	7.82	> 9.8%			10518	AAC	IEEE 802.11a WFI 5 GHz (OFDM, 9 Mbps, R90c-d)	WLAN	8.73	> 9.8%		
10462	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.30	> 9.8%			10519	AAC	IEEE 802.11a WFI 5 GHz (OFDM, 12 Mbps, R90c-d)	WLAN	8.39	> 9.8%		
10463	AAB	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.30	> 9.8%			10520	AAC	IEEE 802.11a WFI 5 GHz (OFDM, 18 Mbps, R90c-d)	WLAN	8.12	> 9.8%		
10464	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, QPSK, UL, Sub)	LTE-TDD	7.82	> 9.8%			10521	AAC	IEEE 802.11a WFI 5 GHz (OFDM, 24 Mbps, R90c-d)	WLAN	7.97	> 9.8%		
10465	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10522	AAC	IEEE 802.11a WFI 5 GHz (OFDM, 36 Mbps, R90c-d)	WLAN	8.45	> 9.8%		
10466	AAC	LTE-TDD (SC-FDMA, 1 RB, 3.1 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10523	AAC	IEEE 802.11a WFI 5 GHz (OFDM, 48 Mbps, R90c-d)	WLAN	8.38	> 9.8%		
10467	AAF	LTE-TDD (SC-FDMA, 1 RB, 5.1 MHz, QPSK, UL, Sub)	LTE-TDD	7.82	> 9.8%			10524	AAC	IEEE 802.11a WFI 5 GHz (OFDM, 54 Mbps, R90c-d)	WLAN	8.27	> 9.8%		
10468	AAF	LTE-TDD (SC-FDMA, 1 RB, 5.1 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10525	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	2.36	> 9.8%		
10469	AAF	LTE-TDD (SC-FDMA, 1 RB, 5.1 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10526	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.42	> 9.8%		
10470	AAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL, Sub)	LTE-TDD	7.82	> 9.8%			10527	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.21	> 9.8%		
10471	AAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10528	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.39	> 9.8%		
10472	AAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10529	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.36	> 9.8%		
10473	AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL, Sub)	LTE-TDD	7.82	> 9.8%			10530	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.36	> 9.8%		
10474	AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10531	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.36	> 9.8%		
10475	AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10532	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.29	> 9.8%		
10476	AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10533	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.30	> 9.8%		
10477	AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10534	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.45	> 9.8%		
10478	AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.32	> 9.8%			10535	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.45	> 9.8%		
10479	AAB	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL, Sub)	LTE-TDD	7.74	> 9.8%			10536	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.32	> 9.8%		
10480	AAB	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.18	> 9.8%			10537	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.44	> 9.8%		
10481	AAB	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.18	> 9.8%			10538	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.34	> 9.8%		
10482	AAC	LTE-TDD (SC-FDMA, 50% RB, 3.1 MHz, QPSK, UL, Sub)	LTE-TDD	7.71	> 9.8%			10540	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.39	> 9.8%		
10483	AAC	LTE-TDD (SC-FDMA, 50% RB, 3.1 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.39	> 9.8%			10541	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.46	> 9.8%		
10484	AAC	LTE-TDD (SC-FDMA, 50% RB, 3.1 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.47	> 9.8%			10542	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.45	> 9.8%		
10485	AAF	LTE-TDD (SC-FDMA, 50% RB, 5.1 MHz, QPSK, UL, Sub)	LTE-TDD	7.79	> 9.8%			10543	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.55	> 9.8%		
10486	AAF	LTE-TDD (SC-FDMA, 50% RB, 5.1 MHz, 16-QAM, UL, Sub)	LTE-TDD	8.47	> 9.8%			10544	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.47	> 9.8%		
10487	AAF	LTE-TDD (SC-FDMA, 50% RB, 5.1 MHz, 64-QAM, UL, Sub)	LTE-TDD	8.40	> 9.8%			10545	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.55	> 9.8%		
10488	AAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL, Sub)	LTE-TDD	7.70	> 9.8%			10546	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.35	> 9.8%		

Certificate No: EX3-7346_Mar22Page 15 of 24

EX3034-SN-7346				March 30, 2022				EX3034-SN-7346				March 30, 2022			
10547	AAC	IEEE 802.11a WFI (80MHz, MCS1, R90c-d)	WLAN	8.49	> 9.8%			10595	AAC	IEEE 802.11n HT Mxwd, 40MHz, MCS1, R90c-d)	WLAN	8.57	> 9.8%		
10548	AAC	IEEE 802.11a WFI (80MHz, MCS1, R90c-d)	WLAN	8.37	> 9.8%			10596	AAC	IEEE 802.11n HT Mxwd, 40MHz, MCS1, R90c-d)	WLAN	8.62	> 9.8%		
10550	AAC	IEEE 802.11a WFI (80MHz, MCS1, R90c-d)	WLAN	8.39	> 9.8%			10597	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.64	> 9.8%		
10551	AAC	IEEE 802.11a WFI (80MHz, MCS1, R90c-d)	WLAN	8.39	> 9.8%			10598	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.77	> 9.8%		
10552	AAC	IEEE 802.11a WFI (80MHz, MCS1, R90c-d)	WLAN	8.42	> 9.8%			10599	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.57	> 9.8%		
10553	AAC	IEEE 802.11a WFI (80MHz, MCS1, R90c-d)	WLAN	8.48	> 9.8%			10600	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.58	> 9.8%		
10554	AAD	IEEE 802.11a WFI (160MHz, MCS1, R90c-d)	WLAN	8.48	> 9.8%			10601	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.78	> 9.8%		
10555	AAD	IEEE 802.11a WFI (160MHz, MCS1, R90c-d)	WLAN	8.47	> 9.8%			10602	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.70	> 9.8%		
10556	AAD	IEEE 802.11a WFI (160MHz, MCS1, R90c-d)	WLAN	8.47	> 9.8%			10603	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.77	> 9.8%		
10557	AAD	IEEE 802.11a WFI (160MHz, MCS1, R90c-d)	WLAN	8.52	> 9.8%			10604	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.84	> 9.8%		
10558	AAD	IEEE 802.11a WFI (160MHz, MCS1, R90c-d)	WLAN	8.50	> 9.8%			10605	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.59	> 9.8%		
10559	AAD	IEEE 802.11a WFI (160MHz, MCS1, R90c-d)	WLAN	8.73	> 9.8%			10606	AAC	IEEE 802.11a WFI (20MHz, MCS1, R90c-d)	WLAN	8.62	> 9.8%		
10560	AAD	IEEE 802.11a WFI (160MHz, MCS1, R90c-d)	WLAN	8.56	> 9.8%			10607	AAC	IEEE 802.11a WFI (40MHz, MCS1, R90c-d)	WLAN	8.81	> 9.8%		
10561	AAD	IEEE 802.11a WFI (160MHz, MCS1, R90c													


 Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated, the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
 中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

(t86-512)67355888 (t86-512)67370818 www.sgsgroup.com.cn
 (t86-512)67355888 (t86-512)67370818 sgs.china@sgs.com

Test Report Form Version: Rev01

Member of the SGS Group (SGS SA)

<p>EXC304--SN 7346</p> <p>March 30, 2022</p> <p>15985 AAA 50 NR DL (CP-CFOM, TM 3.1, 40 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.54 ± 9.8 %</p> <p>15986 AAA 50 NR DL (CP-CFOM, TM 3.1, 50 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.50 ± 9.8 %</p> <p>15987 AAA 50 NR DL (CP-CFOM, TM 3.1, 60 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.50 ± 9.8 %</p> <p>15988 AAA 50 NR DL (CP-CFOM, TM 3.1, 70 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.38 ± 9.8 %</p> <p>15989 AAA 50 NR DL (CP-CFOM, TM 3.1, 80 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.33 ± 9.8 %</p> <p>15990 AAA 50 NR DL (CP-CFOM, TM 3.1, 90 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.52 ± 9.8 %</p> <p>¹ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.</p> <p>Certificate No. EXC3-7346_Mar22</p> <p>Page 24 of 24</p>	<p>EXC304--SN 7346</p> <p>March 30, 2022</p> <p>15985 AAA 50 NR DL (CP-CFOM, TM 3.1, 40 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.54 ± 9.8 %</p> <p>15986 AAA 50 NR DL (CP-CFOM, TM 3.1, 50 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.50 ± 9.8 %</p> <p>15987 AAA 50 NR DL (CP-CFOM, TM 3.1, 60 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.50 ± 9.8 %</p> <p>15988 AAA 50 NR DL (CP-CFOM, TM 3.1, 70 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.38 ± 9.8 %</p> <p>15989 AAA 50 NR DL (CP-CFOM, TM 3.1, 80 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.33 ± 9.8 %</p> <p>15990 AAA 50 NR DL (CP-CFOM, TM 3.1, 90 MHz, 64-QAM, 30 kHz) SG NR PR1 TDD 9.52 ± 9.8 %</p> <p>¹ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.</p> <p>Certificate No. EXC3-7346_Mar22</p> <p>Page 24 of 24</p>
--	--

4 Impedance and return loss

Dipole CLA150 SN 4025				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/26	-31.4	/	47.8	/
Dipole D450V3 SN 1103				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/21	-23	/	57.1	/



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com