

System Performance Check Report for D2450V2 - SN960

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	2450.000	TSL Permittivity	39.9
Group / UID	CW / 0--	TSL Conductivity [S/m]	1.74
Conversion Factor	7.39	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration


Probe Calibration Date	EX3DV4 - SN7646 2025-01-22	Phantom	ELI V8.0 (20deg probe tilt)
DAE Calibration Date	DAE4 Sn1591 2025-02-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	30.0 x 30.0 x 30.0
Grid Steps [mm]	10.0 x 10.0	5.0 x 5.0 x 1.5
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	5.29	5.36
psSAR10g [W/Kg]	2.49	2.64
Power Drift [dB]		0.04
Dist 3dB Peak [mm]		9.5
M2/M1 [%]		84.6

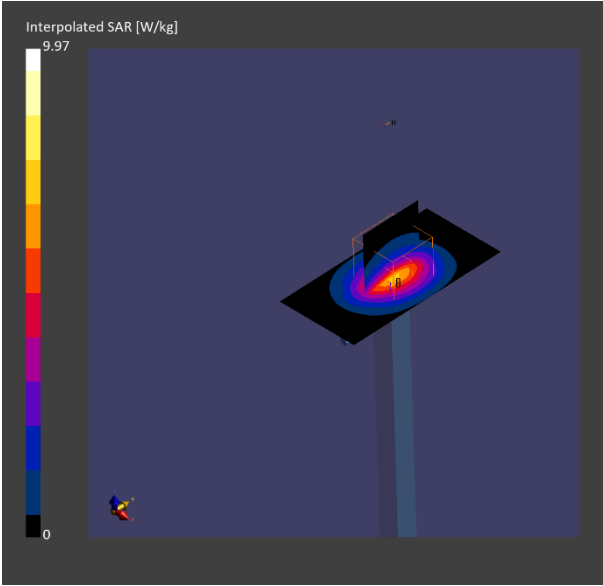

System Performance Check Report for D5GHzV2 - SN1209

Room Ambient Temperature: 23.0°C, Liquid Temperature: 22.0°C

Exposure Conditions

Frequency [MHz]	5750.000	TSL Permittivity	35.3
Group / UID	CW / 0--	TSL Conductivity [S/m]	5.16
Conversion Factor	5.06	Phantom Section / TSL	Flat / Head Simulating Liquid

DASY Configuration

Probe Calibration Date	EX3DV4 - SN7646 2025-01-22	Phantom	ELI V8.0 (20deg probe tilt)
DAE Calibration Date	DAE4 Sn1591 2025-02-18	TSL Type	HBBL-600-10000
Software Version	16.4.0.5005		

Scans Setup

	Area Scan	Zoom Scan
Grid Extents [mm]	40.0 x 80.0	22.0 x 22.0 x 22.0
Grid Steps [mm]	10.0 x 10.0	4.0 x 4.0 x 1.4
Sensor Surface [mm]	3.0	1.4

Measurement Results

	Area Scan	Zoom Scan
psSAR1g [W/Kg]	6.92	8.09
psSAR10g [W/Kg]	1.96	2.34
Power Drift [dB]		0.14
Dist 3dB Peak [mm]		7.4
M2/M1 [%]		57.6

