# Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 10/4/2005 08:42:42 AM

# System Check\_Body\_2450MHz\_20051004

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:736

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL 2450 Medium parameters used: f = 2450 MHz;  $\sigma = 1.98 \text{ mho/m}$ ;  $\epsilon_r = 52.6$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Ambient Temperature: 22.4 °C; Liquid Temperature: 22.0 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.26, 4.26, 4.26); Calibrated: 9/30/2004
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/17/2004
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146


Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 6.44 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 54.7 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 12.4 W/kg

SAR(1 g) = 5.54 mW/g; SAR(10 g) = 2.55 mW/gMaximum value of SAR (measured) = 6.25 mW/g

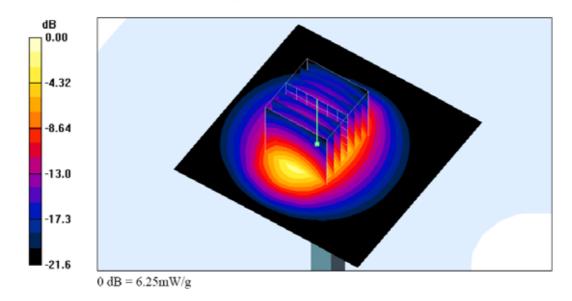

# Appendix B - SAR Measurement Data

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 10/4/2005 6:28:21 PM

### Body\_802.11b Ch1\_Keypad Up with Touch\_20051004

DUT: 592128; Type: Pocket PC

Communication System: 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma = 1.94$  mho/m;  $\epsilon_e = 52.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature : 23.0 °C; Liquid Temperature : 22.7 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.26, 4.26, 4.26); Calibrated: 9/30/2004
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/17/2004
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146


Ch1/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.193 mW/g

Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.90 V/m; Power Drift = 0.056 dB

Peak SAR (extrapolated) = 0.378 W/kg

SAR(1 g) = 0.177 mW/g; SAR(10 g) = 0.091 mW/gMaximum value of SAR (measured) = 0.190 mW/g

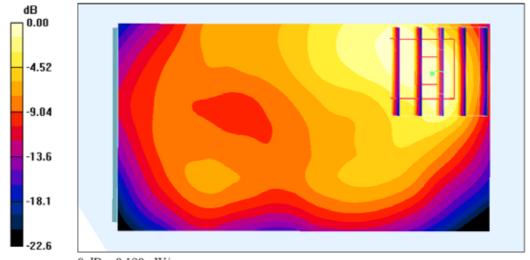

 $0~dB=0.190m\mathrm{W/g}$ 

-CC SAR Test Report No : FA592128-1-2-01

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 10/4/2005 6:01:48 PM

# Body\_802.11b Ch6\_Keypad Down with Touch\_20051004

DUT: 592128; Type: Pocket PC

Communication System: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.97$  mho/m;  $\varepsilon_r = 52.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.2 °C; Liquid Temperature: 22.9 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.26, 4.26, 4.26); Calibrated: 9/30/2004
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/17/2004
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146


Ch6/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.164 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.74 V/m; Power Drift = -0.057 dB

Peak SAR (extrapolated) = 0.301 W/kg

SAR(1 g) = 0.143 mW/g; SAR(10 g) = 0.074 mW/gMaximum value of SAR (measured) = 0.151 mW/g

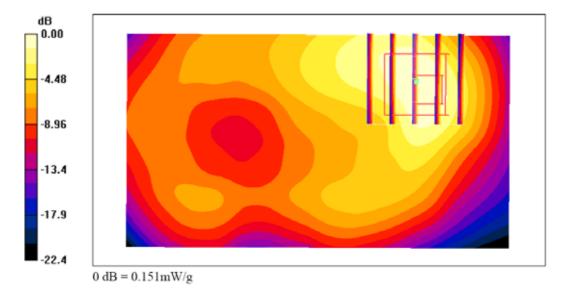

FCC SAR Test Report No : FA592128-1-2-01

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 10/4/2005 7:51:23 PM

## Body\_802.11g Ch6\_Keypad Up with Touch\_20051004

DUT: 592128; Type: Pocket PC

Communication System: 802.11g; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.97$  mho/m;  $\epsilon_r = 52.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.9 °C; Liquid Temperature: 22.6 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.26, 4.26, 4.26); Calibrated: 9/30/2004
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/17/2004
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

# Ch6/Area Scan (51x91x1): Measurement grid: dx=15mm, dy=15mm


Maximum value of SAR (interpolated) = 0.127 mW/g

Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.16 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 0.259 W/kg

SAR(1 g) = 0.120 mW/g; SAR(10 g) = 0.061 mW/gMaximum value of SAR (measured) = 0.131 mW/g

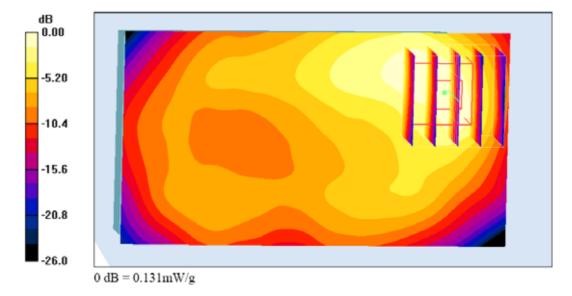

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 10/4/2005 6:34:28 PM

# Body\_802.11b Ch1\_Keypad Up with Touch\_20051004\_2D

DUT: 592128; Type: Pocket PC

Communication System: 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2412 MHz;  $\sigma = 1.94$  mho/m;  $\varepsilon_r = 52.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 23.0 °C; Liquid Temperature: 22.7 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.26, 4.26, 4.26); Calibrated: 9/30/2004
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/17/2004
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

# Ch1/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.90 V/m; Power Drift = 0.056 dB

Peak SAR (extrapolated) = 0.378 W/kg

SAR(1 g) = 0.177 mW/g; SAR(10 g) = 0.091 mW/g

Maximum value of SAR (measured) = 0.190 mW/g



FCC SAR Test Report Test Report No : FA592128-1-2-01

Test Laboratory: Sporton International Inc. SAR Testing Lab Date/Time: 10/4/2005 7:56:54 PM

# Body 802.11g Ch6 Keypad Up with Touch 20051004\_2D

DUT: 592128; Type: Pocket PC

Communication System: 802.11g; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium: MSL\_2450 Medium parameters used: f = 2437 MHz;  $\sigma = 1.97$  mho/m;  $\varepsilon_e = 52.6$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Ambient Temperature: 22.9 °C; Liquid Temperature: 22.6 °C

### DASY4 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.26, 4.26, 4.26); Calibrated: 9/30/2004
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn577; Calibrated: 11/17/2004
- Phantom: SAM 12; Type: QD 000 P40 C; Serial: TP-1150
- Measurement SW: DASY4, V4.5 Build 19; Postprocessing SW: SEMCAD, V1.8 Build 146

### Ch6/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 6.16 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 0.259 W/kg

SAR(1 g) = 0.120 mW/g; SAR(10 g) = 0.061 mW/gMaximum value of SAR (measured) = 0.131 mW/g



# Appendix C - Calibration Data

Calibration Laboratory of Schmid & Partner Engineering AG Zeugheusstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client Sporton (Auden)



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Certificate No: D2450V2-736\_Jul05

CALIBRATION C	ERTIFICATE		
Object	D2450V2 - SN: 7	36	
Calibration procedure(s)	QA CAL-05.v6 Calibration procedure for dipole validation kits		
Calibration date:	July 12, 2005		
Condition of the calibrated item	In Tolerance		
		y facility: environment temperature (22 ± 3)°C an	d humidity < 70%.
Calibration Equipment used (M&)		y facility: environment temperature (22 ± 3)°C and Call Date (Calibrated by, Certificate No.)	d humidity < 70%. Scheduled Calibration
Calibration Equipment used (M&)	TE dritical for calibration)		
Calibration Equipment used (M&1 Primary Standards	TE chitical for calibration)	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Calibration Equipment used (M&1 Primary Standards Power meter EPM E442 Power sensor HP 8481A	TE chitical for calibration)  ID #  GB37480704	Cal Date (Calibrated by, Certificate No.) 12-Oct-04 (METAS, No. 251-00412)	Scheduled Calibration Oct-05
Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator	TE chitical for calibration)  ID #  GB37480704  US37292783	Cai Date (Calibrated by, Certificate No.) 12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412)	Scheduled Calibration Oct-05 Oct-05
Calibration Equipment used (M&1 Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator	ID # GB37480704 US37292783 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025	Cai Date (Calibrated by, Certificate No.) 12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No. 251-00402)	Scheduled Calibration Oct-05 Oct-05 Aug-05
Calibration Equipment used (M&I Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2	ID #  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r)	Cai Date (Calibrated by, Certificate No.) 12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No 251-00402) 10-Aug-04 (METAS, No 251-00402)	Scheduled Calibration Oct-05 Oct-05 Aug-05 Aug-05
Calibration Equipment used (M&I Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4	TE dritical for calibration)  ID #  GB37480704  US37292783  SN: 5086 (20g)  SN: 5047.2 (10r)  SN 3025  SN 601	Cal Date  Calibrated by, Certificate No.) 12-Oct-04 (METAS, No. 251-00412) 12-Oct-04 (METAS, No. 251-00412) 10-Aug-04 (METAS, No. 251-00402) 10-Aug-04 (METAS, No. 251-00402) 29-Oct-04 (SPEAG, No. ES3-3025_Oct04) 07-Jan-05 (SPEAG, No. DAE4-601_Jan05)	Scheduled Calibration Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06
Calibration Equipment used (M&1 Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	ID #  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN 3025 SN 601	Cal Date  Calibrated by, Certificate No.)  12-Oct-04 (METAS, No. 251-00412)  12-Oct-04 (METAS, No. 251-00412)  10-Aug-04 (METAS, No. 251-00402)  10-Aug-04 (METAS, No. 251-00402)  29-Oct-04 (SPEAG, No. ES3-3025_Oct04)  07-Jan-05 (SPEAG, No. DAE4-601_Jan05)  Check Date (in house)	Scheduled Calibration Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check
Primary Standards Power meter EPM E442 Power sensor HP 8461A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A	ID #  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN 3025 SN 601  ID #  MY41092317	Cal Date (Calibrated by, Certificate No.)  12-Oct-04 (METAS, No. 251-00412)  12-Oct-04 (METAS, No. 251-00412)  10-Aug-04 (METAS, No. 251-00402)  10-Aug-04 (METAS, No. 251-00402)  29-Oct-04 (METAS, No. 251-00402)  29-Oct-04 (METAS, No. 251-00402)  29-Oct-04 (METAS, No. 251-00402)  Check Date (in house)  18-Oct-02 (SPEAG, In house check Oct-03)	Scheduled Calibration Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06
Calibration Equipment used (M&1 Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4	ID #  GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 (10r) SN 3025 SN 601	Cal Date  Calibrated by, Certificate No.)  12-Oct-04 (METAS, No. 251-00412)  12-Oct-04 (METAS, No. 251-00412)  10-Aug-04 (METAS, No. 251-00402)  10-Aug-04 (METAS, No. 251-00402)  29-Oct-04 (SPEAG, No. ES3-3025_Oct04)  07-Jan-05 (SPEAG, No. DAE4-601_Jan05)  Check Date (in house)	Scheduled Calibration Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05
Calibration Equipment used (M&T Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SML-03	ID # GB37480704 US37292783 SN: 5047.2 (10r) SN 3025 SN 601 ID # MY41092317 100698 US37390585 S4206	Cal Date [Calibrated by, Certificate No.)  12-Oct-04 (METAS, No. 251-00412)  12-Oct-04 (METAS, No. 251-00412)  10-Aug-04 (METAS, No 251-00402)  10-Aug-04 (METAS, No 251-00402)  29-Oct-04 (SPEAG, No. ES3-3025_Oct04)  07-Jan-05 (SPEAG, No. DAE4-601_Jan05)  Check Date (in house)  18-Oct-02 (SPEAG, in house check Oct-03)  27-Mar-02 (SPEAG, in house check Nov-04)	Scheduled Calibration Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05 In house check: Nav-05
Calibration Equipment used (M&T Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SML-03	TE dritical for calibration)  ID #  GB37480704  US37292783  SN: 5085 (20g)  SN: 5047.2 (10r)  SN 3025  SN 601  ID #  MY41092317  100698	Cal Date  Calibrated by, Certificate No.)  12-Oct-04 (METAS, No. 251-00412)  12-Oct-04 (METAS, No. 251-00412)  10-Aug-04 (METAS, No. 251-00402)  10-Aug-04 (METAS, No. 251-00402)  29-Oct-04 (SPEAG, No. ES3-3025_Oct04)  07-Jan-05 (SPEAG, No. DAE4-601_Jan05)  Check Date (in house)  18-Oct-02 (SPEAG, in house check Oct-03)  27-Mar-02 (SPEAG, in house check Nov-04)  Function  Laboratory Technician	Scheduled Calibration Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05 In house check: Nav-05 Signature
Calibration Equipment used (M&T Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SML-03 Network Analyzer HP 8753E	TE dritical for calibration)  ID # GB37480704 US37292783 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025 SN 601  ID # MY41092317 100698 US37390585 \$4206 Name	Cal Date  Calibrated by, Certificate No.)  12-Oct-04 (METAS, No. 251-00412)  12-Oct-04 (METAS, No. 251-00412)  10-Aug-04 (METAS, No. 251-00402)  10-Aug-04 (METAS, No. 251-00402)  29-Oct-04 (SPEAG, No. ES3-3025_Oct04)  07-Jan-05 (SPEAG, No. DAE4-601_Jan05)  Check Date (in house)  18-Oct-02 (SPEAG, in house check Oct-03)  27-Mar-02 (SPEAG, in house check Nov-04)  Function  Laboratory Technician	Scheduled Calibration Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05 In house check: Nav-05 Signature
Calibration Equipment used (M&T Primary Standards Power meter EPM E442 Power sensor HP 8481A Reference 20 dB Attenuator Reference 10 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SML-03 Network Analyzer HP 8753E	TE dritical for calibration)  ID # GB37480704 US37292783 SN: 5085 (20g) SN: 5047.2 (10r) SN 3025 SN 601  ID # MY41092317 100698 US37390585 \$4206 Name	Cal Date  Calibrated by, Certificate No.)  12-Oct-04 (METAS, No. 251-00412)  12-Oct-04 (METAS, No. 251-00412)  10-Aug-04 (METAS, No. 251-00402)  10-Aug-04 (METAS, No. 251-00402)  29-Oct-04 (SPEAG, No. ES3-3025_Oct04)  07-Jan-05 (SPEAG, No. DAE4-601_Jan05)  Check Date (in house)  18-Oct-02 (SPEAG, in house check Oct-03)  27-Mar-02 (SPEAG, in house check Nov-04)  Function  Laboratory Technician	Scheduled Calibration Oct-05 Oct-05 Aug-05 Aug-05 Oct-05 Jan-06 Scheduled Check In house check: Oct-05 In house check: Nov-05 Signature

Certificate No: D2450V2-736\_Jul05

Page 1 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland ONISS OF PRATE

S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

### Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z

N/A not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

# Additional Documentation:

d) DASY4 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D2450V2-735\_Jul05

Page 2 of 9

### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.6
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat IPhantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 15 mm	
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	:22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.5 ± 6 %	1.73 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	condition	
SAR measured	250 mW input power	13.1 mW / g
SAR normalized	normalized to 1W	52.4 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	52.8 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>2</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.13 mW / g
SAR normalized	normalized to 1W	24.5 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	24.7 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-736\_Jul05 Page 3 of 9

<sup>&</sup>lt;sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Body TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.2 ± 0.2) °C	52.5 ± 6 %	2.02 mho/m ± 8 %
Body TSL temperature during test	(22.2 ± 0.2) °C	'	

# SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	condition	
SAR measured	250 mW input power	13.5 mW / g
SAR normalized	normalized to 1W	54.0 mW / g
SAR for nominal Body TSL parameters 2	normalized to 1W	52.8 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.26 mW / g
SAR normalized	normalized to 1W	25.0 mW / g
SAR for nominal Body TSL parameters 2	normalized to 1W	24.5 mW / g ± 16.5 % (k=2)

Certificate No: D2450V2-736\_Jul05

<sup>&</sup>lt;sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

### Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.6 Ω + 3.7 jΩ
Return Loss	-26.0 dB

# Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.9 Ω + 5.3 jΩ
Return Loss	- 25.5 dB

# General Antenna Parameters and Design

Electrical Delay (one direction)	1.157 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 26, 2003

Certificate No: D2450V2-736\_Jul05 Page 5 of 9

### DASY4 Validation Report for Head TSL

Date/Time: 12.07.2005 12:53:00

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U10 BB

Medium parameters used: f = 2450 MHz;  $\sigma = 1.73$  mho/m;  $\epsilon_r = 38.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

### DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.4, 4.4, 4.4); Calibrated: 29.10.2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 22.07.2004
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA
- Measurement SW: DASY4, V4.5 Build 30; Postprocessing SW: SEMCAD, V1.8 Build 149

### Pin = 250 mW; d = 10 mm 2/Area Scan (41x61x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 16.6 mW/g

### Pin = 250 mW; d = 10 mm 2/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 91.6 V/m; Power Drift = 0.077 dB

Peak SAR (extrapolated) = 27.0 W/kg

### SAR(1 g) = 13.1 mW/g; SAR(10 g) = 6.13 mW/g


Maximum value of SAR (measured) = 15.0 mW/g

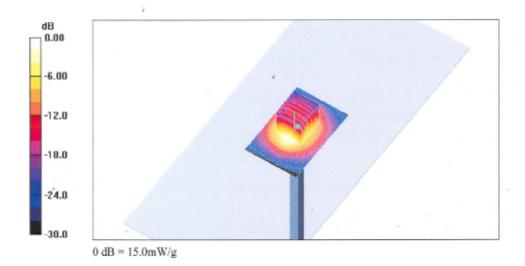

Certificate No: D2450V2-736\_Jul05



# Impedance Measurement Plot for Head TSL

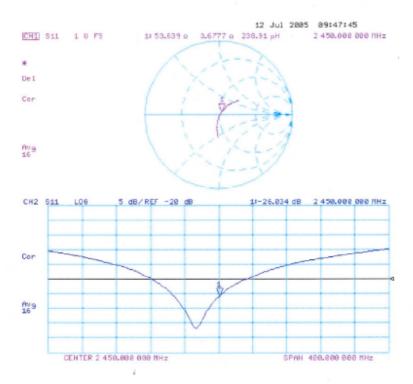

Certificate No: D2450V2-736\_Jul05

Page 7 of 9

### DASY4 Validation Report for Body TSL

Date/Time: 11.07.2005 17:33:35

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN736

Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL 2450

Medium parameters used: f = 2450 MHz;  $\sigma = 2.02$  mho/m;  $\varepsilon_r = 52.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

### DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.13, 4.13, 4.13); Calibrated: 29.10.2004
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 22.07.2004
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA
- Measurement SW: DASY4, V4.6 Build 4; Postprocessing SW: SEMCAD, V1.8 Build 149

### Pin = 250 mW; d = 10 mm/Area Scan (81x81x1):

Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (interpolated) = 15.8 mW/g

### Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx-5mm, dy-5mm, dz-5mm

Reference Value = 85.9 V/m; Power Drift = 0.160 dB

Peak SAR (extrapolated) = 27.6 W/kg

### SAR(1 g) = 13.5 mW/g; SAR(10 g) = 6.26 mW/g


Maximum value of SAR (measured) = 15.5 mW/g

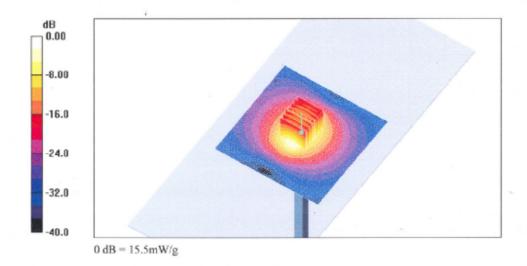

Certificate No: D2450V2-736\_Jul05



# Impedance Measurement Plot for Body TSL

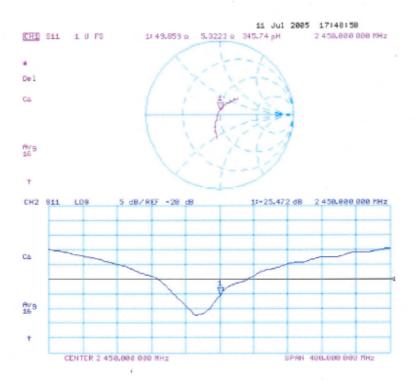

Certificate No: D2450V2-736\_Jul05

Page 9 of 9