
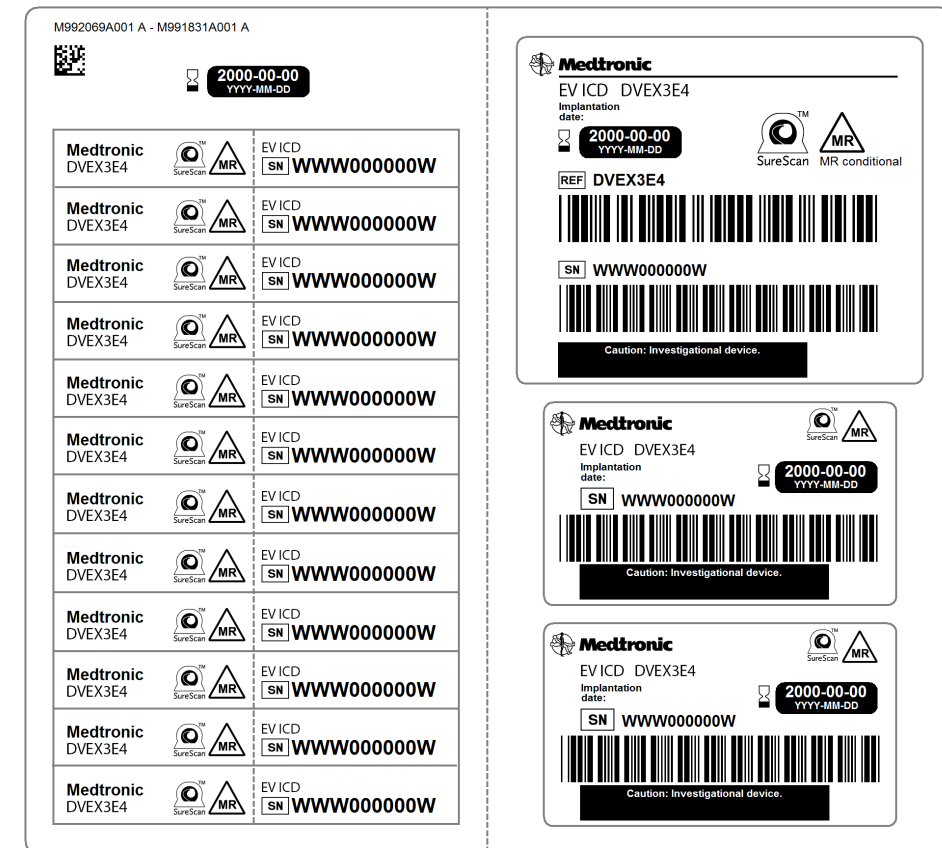
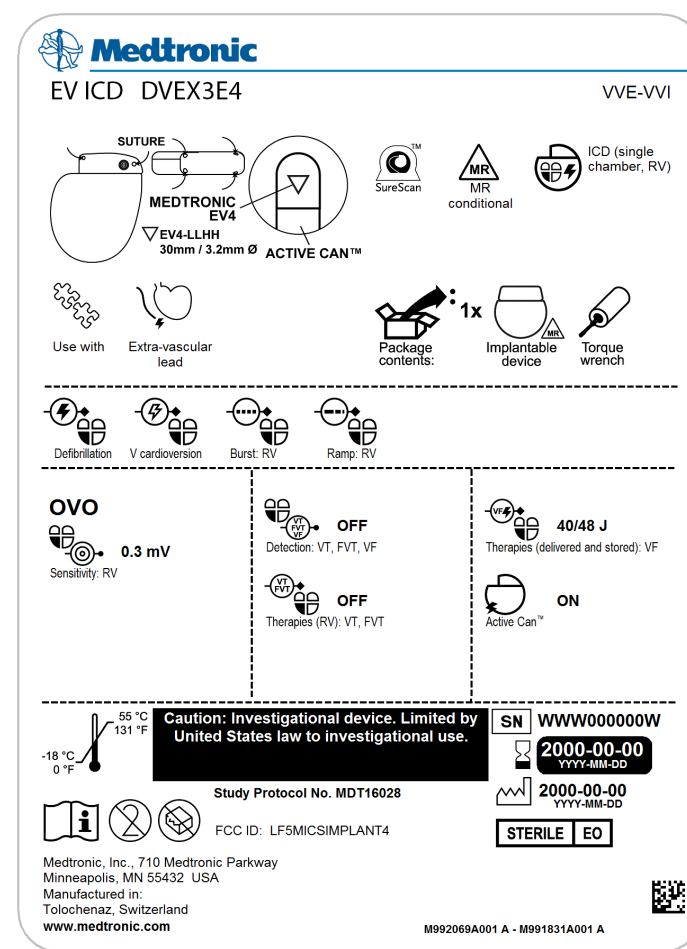


1. THIS SPECIFICATION IS CONTROLLED BY CRHF PACKAGE ENGINEERING. THIS SPECIFICATION IS INTENDED TO BE THE FINAL LABEL DESIGN OUTPUT GENERATED FROM A COMBINATION OF LABEL PARTS WITHIN THE ASSOCIATED PDM BOM.
2. THESE LABEL IMAGES ARE THE COMBINATION OF THE TEMPLATE FILE, MODEL DATA RECORD, SAMPLE TRIGGER DATA AND REPRESENTATIVE VIEWS OF THE LABEL DIE LINES.
3. PRINTING REQUIREMENTS - THE LABELS ARE TO BE PRINTED USING A 300 DPI ZEBRA THERMAL TRANSFER PRINTER.
4. THE LOT OR SERIAL NUMBER, USE BY DATE, DATE OF MANUFACTURE, PIN NUMBER, ADDRESS CODE, GTIN, PRODUCT NUMBER (REF) AND BAR CODES ARE SHOWN FOR EXAMPLE ONLY. THESE FIELDS ARE VARIABLE AND ARE TO BE SUPPLIED BY MANUFACTURING AT THE TIME OF PRINTING.
5. SPACING AND TEXT WRAPPING SHOWN IN THE IMAGES MAY DIFFER SLIGHTLY FROM ACTUAL PRINTED LABEL, AS LONG AS CONTENT OF PRINTED VERSION IS ACCURATE. THE IMAGES INCLUDE REPRESENTATION OF THE PRE-PRINTED LABEL STOCK. BRANDING, PART NUMBER BAR CODES (2D OR OTHER) AND OTHER PRE-PRINTED AREAS OR ADDITIONAL STICKERS MAY CHANGE AND ARE ACCEPTABLE.
6. THE LABEL PRINTED IN MANUFACTURING MUST BE AT AN EQUAL OR LATER MODEL DATA AND TEMPLATE REVISION AS SHOWN ON THE IMAGE.
7. (FOR LABEL SET ONLY) THE TRIGGER DATA SHOWN ON THE LABEL SET IMAGE MAY NOT MATCH THE PRINTED LABEL.

SPEC TAB	MFG ADDRESS
A95703-001	Tolochenaz, Switzerland

DeviceImageSpec_03

Medtronic MEDTRONIC, INC. MINNEAPOLIS, MINNESOTA USA MEDTRONIC CONFIDENTIAL THIS DOCUMENT IS THE PROPERTY OF MEDTRONIC, INC. AND MUST BE ACCOUNTED FOR. INFORMATION HEREON IS CONFIDENTIAL. DO NOT REPRODUCE IT, REVEAL IT TO UNAUTHORIZED PERSONS OR SEND IT OUTSIDE MEDTRONIC WITHOUT PROPER AUTHORIZATION.	TITLE LABEL IMAGE SPEC - EV ICD PIVOTAL CLINICAL US				
	LABEL IMAGE SPEC TEMPLATE: A83320 REV D				
	DATE 22-Jan-2019	SCALE N/A	ENGINEERING JIMMY FLYNN		
	MODEL DVEX3E4	Size B	PART NUMBER A95703	REV A	SHEET 1 of 2

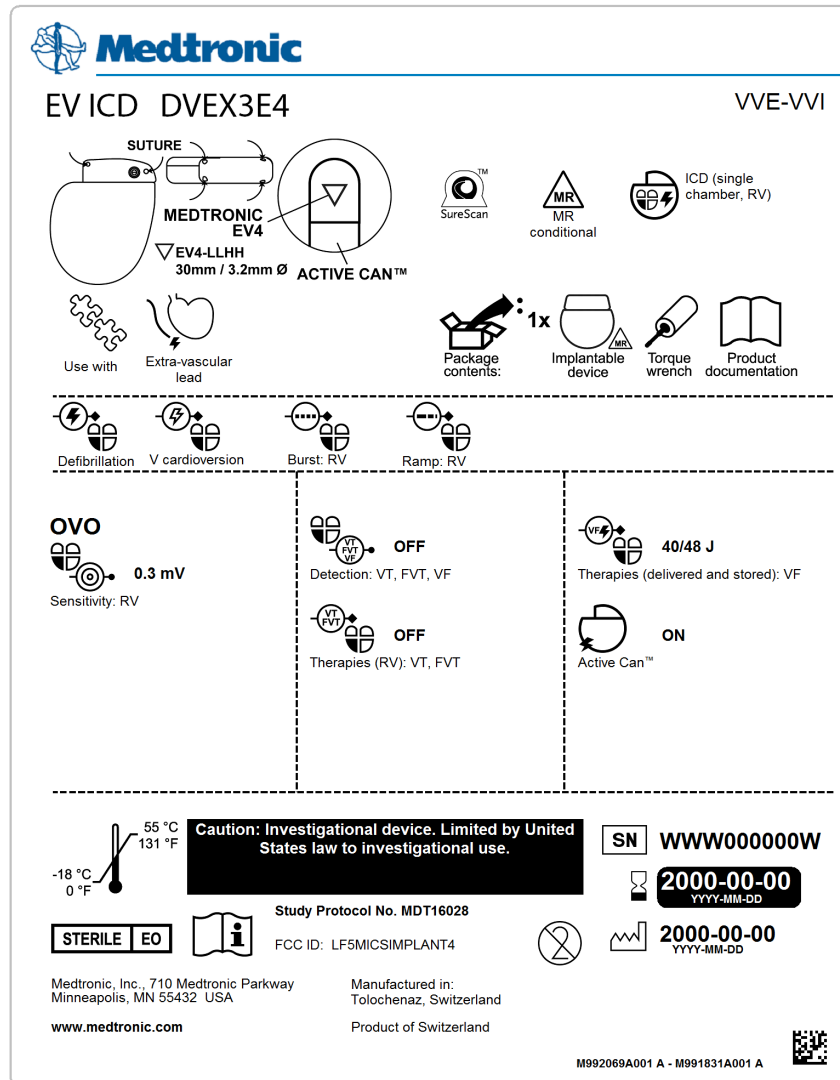

Shelf Box Label



End Label 1

End Label 2

FYR Labels