

S-039-18

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

EMC Technologies

CALIBRATION CERTIFICATE

Object(s) **D5GHzV2 - SN:1008**

Calibration procedure(s) **QA CAL-05.v2
Calibration procedure for dipole validation kits**

Calibration date: **October 5, 2003**

Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 ± 2 degrees Celsius and humidity $< 75\%$.

Calibration Equipment used (M&TE critical for calibration)

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM E4419B	GB41293874	2-Apr-03 (METAS, No 252-0250)	Apr-04
Power sensor E4412A	MY41495277	2-Apr-03 (METAS, No 252-0250)	Apr-04
Reference 20 dB Attenuator	SN: 5086 (20b)	3-Apr-03 (METAS No. 251-0340)	Apr-04
Fluke Process Calibrator Type 702	SN: 8295803	8-Sep-03 (Sintrel SCS No. E-030020)	Sep-04
Power sensor HP 8481A	MY41092180	18-Sep-02 (Agilent, No. 20020918)	In house check: Oct 03
RF generator R&S SMT06	100058	23-May-01 (SPEAG, in house check May-03)	In house check: May-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (Agilent, No. 24BR1033101)	In house check: Oct 03

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Laboratory Director	
Approved by:	Nils Kuster	Quality Manager	

Date issued: October 6, 2003

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

Schmid & Partner Engineering AG

s p e a g

Zeughausstrasse 43, 8004 Zurich, Switzerland
Phone +41 1 245 9700, Fax +41 1 245 9779
info@speag.com, <http://www.speag.com>

DASY

Dipole Validation Kit

Type: D5GHzV2

Serial: 1008

Manufactured: August 28, 2003

Calibrated: October 5, 2003

1. Measurement Conditions

The measurements were performed in the flat section of the SAM twin phantom filled with **body simulating solution** of the following electrical parameters:

Frequency:	5200 MHz	
Relative Dielectricity	49.7	$\pm 5\%$
Conductivity	5.18 mho/m	$\pm 5\%$
Frequency:	5800 MHz	
Relative Dielectricity	48.5	$\pm 5\%$
Conductivity	6.01 mho/m	$\pm 5\%$

The DASY3 System with a dosimetric E-field probe ES3DV3 - SN:3025 was used for the measurements. The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. Lossless spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10mm was aligned with the dipole. The 8x8x8 fine cube was chosen for cube integration ($dx=dy=4.3\text{mm}$, $dz=3\text{mm}$). Distance between probe sensors and phantom surface was set to 3.0 mm. The dipole input power (forward power) was $250\text{mW} \pm 3\%$. The results are normalized to 1W input power.

2. SAR Measurement with DASY System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figures supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured at **5200 MHz (Body Tissue)** with the dosimetric probe ES3DV3 SN:3025 and applying the advanced extrapolation are:

averaged over 1 cm^3 (1 g) of tissue: **$84.8\text{ mW/g} \pm 32.0\% (k=2)^1$**

averaged over 10 cm^3 (10 g) of tissue: **$23.5\text{ mW/g} \pm 31.7\% (k=2)^1$**

The resulting averaged SAR-values measured at **5800 MHz (Body Tissue)** with the dosimetric probe ES3DV3 SN:3025 and applying the advanced extrapolation are:

averaged over 1 cm^3 (1 g) of tissue: **$80.8\text{ mW/g} \pm 32.0\% (k=2)^2$**

averaged over 10 cm^3 (10 g) of tissue: **$22.0\text{ mW/g} \pm 31.7\% (k=2)^2$**

¹ Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR_1g=71.8 mW/g, SAR_10g=20.1 mW/g and SAR_peak=284.7 mW/g.

² Target dipole values determined by FDTD (feedpoint impedance set to 50 Ohm). The values are SAR_1g=74.1 mW/g, SAR_10g=20.5 mW/g and SAR_peak=324.7 mW/g.

SPEAG Calibration Laboratory

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1008

Communication System: CW-5GHz; Frequency: 5200 MHz; Duty Cycle: 1:1

Medium: MSL5800 ($\sigma = 5.18$ mho/m, $\epsilon_r = 49.73$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV3 - SN3025-Y2003; ConvF(1.93, 1.93, 1.93); Calibrated: 9/19/2003
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn410; Calibrated: 4/22/2003
- Phantom: SAM 12b; Type: SAM 4.0; Serial: TP:1197
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 60

d=10mm, Pin=250mW, f=5200 MHz/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 88 V/m

Power Drift = 0.0 dB

Maximum value of SAR = 32.5 mW/g

d=10mm, Pin=250mW, f=5200 MHz/Zoom Scan (8x8x8), dist=3mm (7x7x8)/Cube 0: Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm


Peak SAR (extrapolated) = 82.1 W/kg

SAR(1 g) = 21.2 mW/g; SAR(10 g) = 5.88 mW/g

Reference Value = 88 V/m

Power Drift = 0.0 dB

Maximum value of SAR = 31.1 mW/g

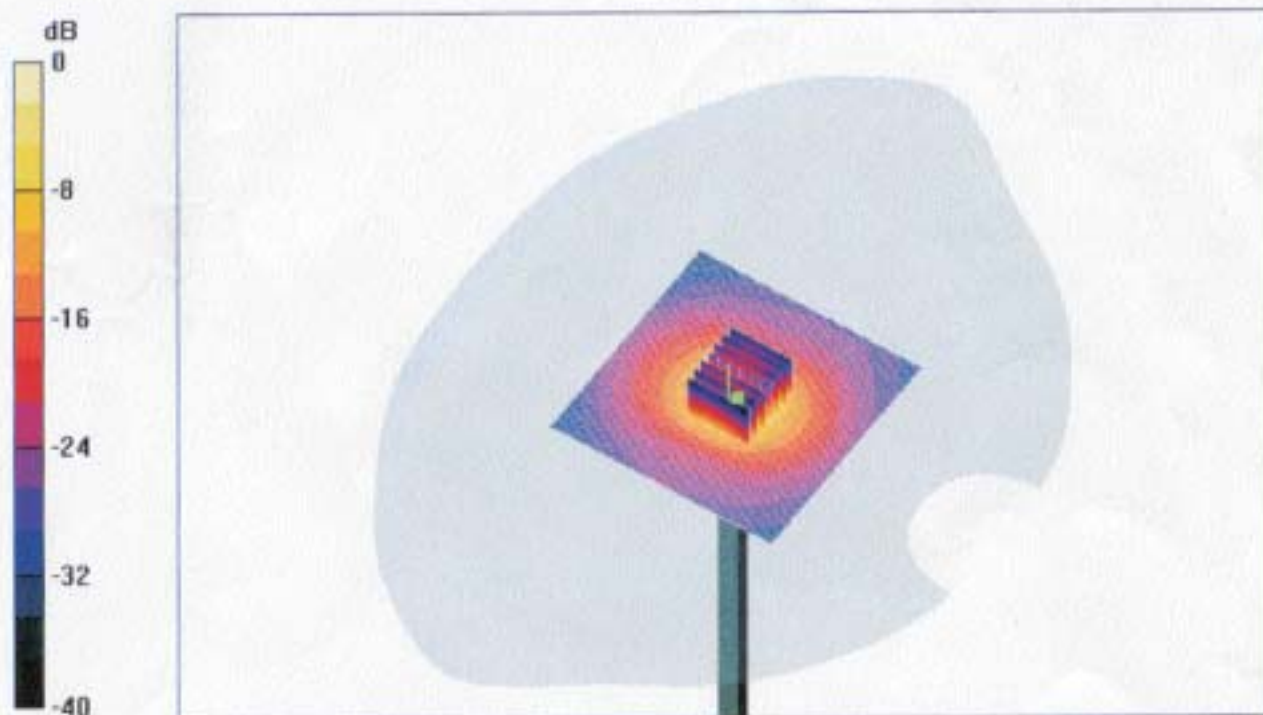

0 dB = 31.1mW/g

SPEAG Calibration Laboratory

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1008

Communication System: CW-5GHz; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: MSL5800 ($\sigma = 6.01$ mho/m, $\epsilon_r = 48.51$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ES3DV3 - SN3025-Y2003; ConvF(1.65, 1.65, 1.65); Calibrated: 9/19/2003
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn410; Calibrated: 4/22/2003
- Phantom: SAM 12b; Type: SAM 4.0; Serial: TP:1197
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 60

d=10mm, Pin=250mW, f=5800 MHz/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 80.2 V/m

Power Drift = -0.1 dB

Maximum value of SAR = 31.9 mW/g

d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=3mm (7x7x8)/Cube 0: Measurement

grid: dx=4.3mm, dy=4.3mm, dz=3mm



Peak SAR (extrapolated) = 85.7 W/kg

SAR(1 g) = 20.2 mW/g; SAR(10 g) = 5.51 mW/g

Reference Value = 80.2 V/m

Power Drift = -0.1 dB

Maximum value of SAR = 29.7 mW/g

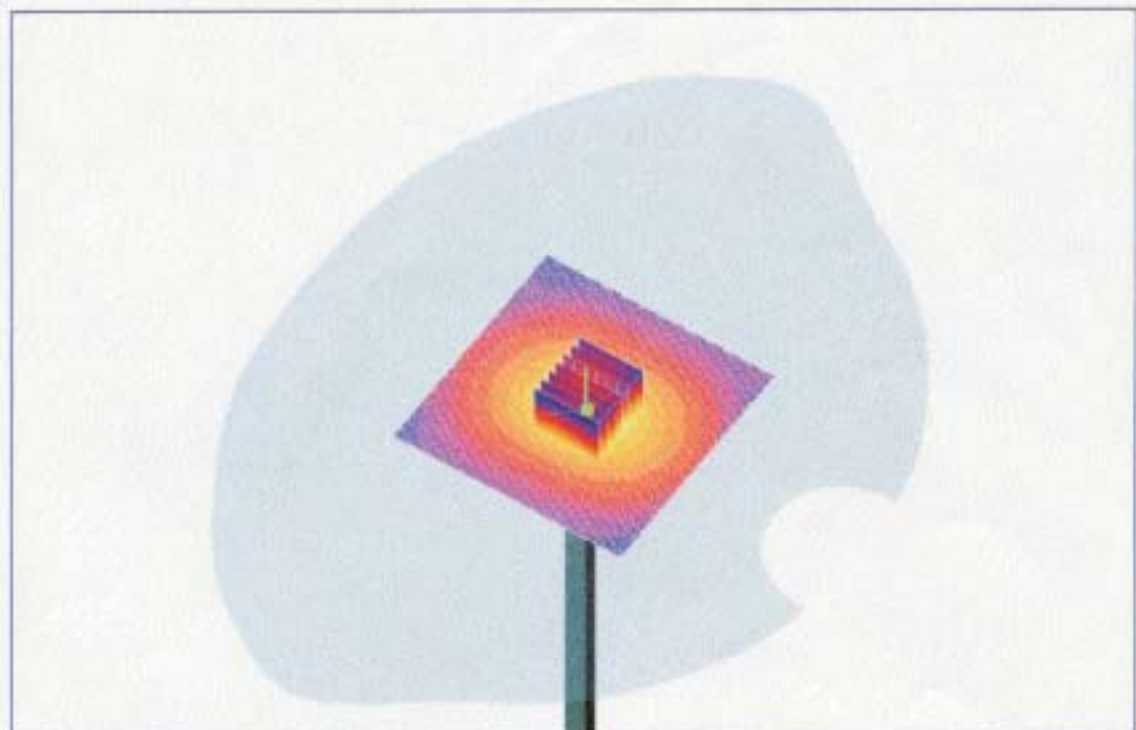


0 dB = 29.7mW/g

1008
Body

5 Oct 2003 12:39:02
CH1 S11 1 V F9 21 51.703 a -12.469 a 2.4547 pF 5 200.000 000 MHz

Del

Cor

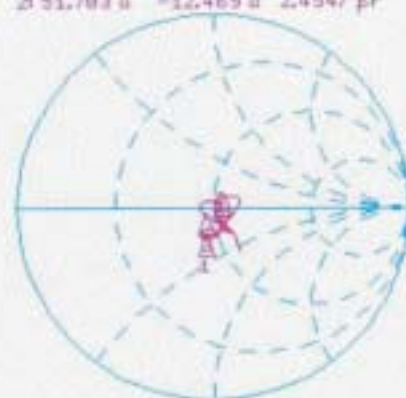

CH1 Markers

1: 43.588 a
-13.525 a
5.10000 GHz
3: 45.600 a
-3.6797 a
5.50000 GHz
4: 54.217 a
6.8410 a
5.00000 GHz

CH2 S11 LOG 5 dB/REF -20 dB 2: -18.227 dB 5 200.000 000 MHz

Sw

Cor

avg

16

↑



CH2 Markers

1: -15.993 dB
5.10000 GHz
3: -24.485 dB
5.50000 GHz
4: -22.259 dB
5.00000 GHz

START 4 000.000 000 MHz

STOP 6 000.000 000 MHz