


ANNEX D. ANTENNA INFORMATION

< Antenna location >

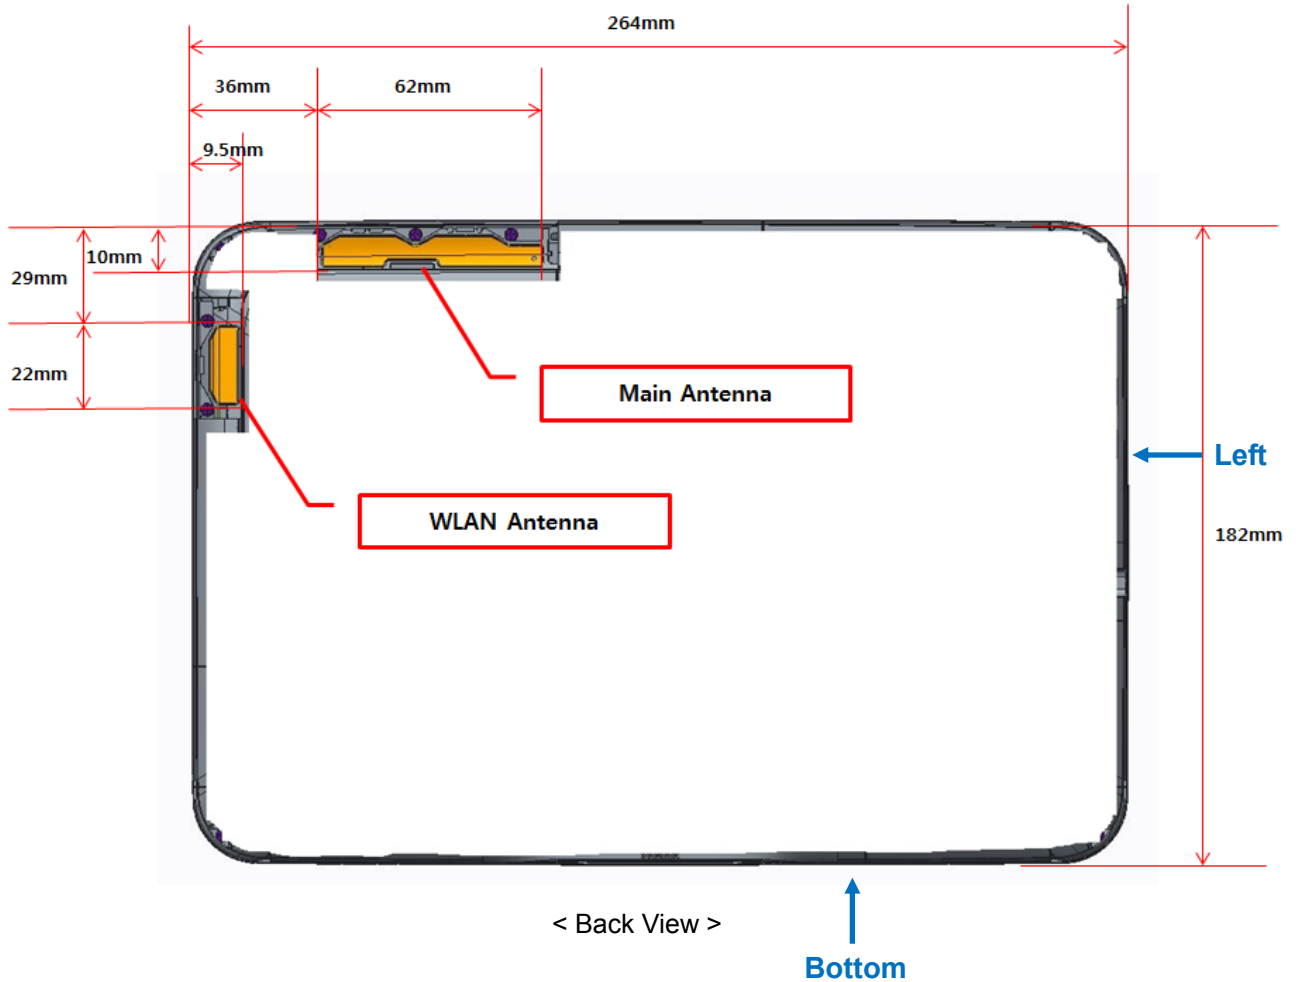

< Antenna Data Sheet >

1. WWAN Antenna Data Sheet



Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	1 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A

APPROVAL SHEET

Customer : BLUEBIRD

Company : DONGNAM

Item : INTENNA

Model : BP80S (MAIN)

Customer P/N :

Maker Code : KIN-MAIN-BS1401



Department	Investigation	Verification	Approval
RF			
Machine			

KRD01-00A10-01A

1

EMC-003 (Rev.2)



Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	2 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A

► Contents ◀

1. Revision History of Product Specification -----	03/13
1.1 History List of Approval Sheet -----	03/13
2. Circuit Specification -----	04/13
2.1 Test Setting -----	04/13
2.1.1 Test Environment (Condition/Method) -----	04/13
2.2 Electrical Specification -----	06/13
2.2.1 Electrical Spec. of SET (With VSWR) -----	07/13
2.2.2 Passive Gain & 3D Pattern -----	08/13
3. Mechanical Specification -----	10/13
3.1 Material Certification -----	10/13
3.2 Mechanical Specification -----	11/13
3.2.1 Part List -----	11/13
3.2.2 Assy Drawing -----	12/13
3.2.3 Packing Spec. & Drawing -----	13/13



Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A

[illegible]



Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	4 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A

2. Circuit Specification

2.1 Test Setting

2.1.1 Test Environment (Condition PROTEK A333)

① VSWR

Step 1. Connect ANT port with cable included adaptor to port1 of Network analyzer.

Step 2. Point out markers on network analyzer display at target frequencies.

Step 3. Inspect VSWR



KRD01-00A10-01A

4



Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	5 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A


② Radiation Pattern and Gain

Step 1. Calibrate chamber system for gain measurement using horn antenna.

At the same time set up software program for chamber system control.

Step 2. Change over from a horn antenna to measuring antenna on target positioner

Step 3. Start a software program for chamber system control & measuring.

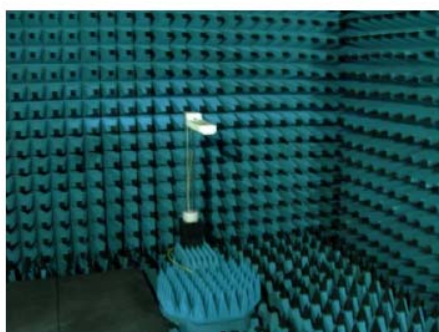

KRD01-00A10-01A



5



Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	6 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A

2.2 Electrical Specification

Frequency Band	GSM850, GSM900			
	824MHz	880MHz	894MHz	960MHz
VSWR	≤ 6.0	≤ 3.5	≤ 3.0	≤ 5.0
Average Gain	$\geq -9.5\text{dBi}$	$\geq -5.5\text{dBi}$	$\geq -5.0\text{dBi}$	$\geq -10.0\text{dBi}$
Frequency Band	DCS, PCS, WCDMA2100			
	1710MHz	1850MHz	1880MHz	2170MHz
VSWR	≤ 5.5	≤ 2.5	≤ 2.0	≤ 5.0
Average Gain	$\geq -9.0\text{dBi}$	$\geq -5.0\text{dBi}$	$\geq -5.5\text{dBi}$	$\geq -9.0\text{dBi}$
Directivity	Omni-directional			
Polarization	Linear			
Matching Value	  Port #2 Matching value  Port #1 Matching value			

KRD01-00A10-01A

6

EMC-003 (Rev.2)




Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	7 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	ANTENNA		BLUEBIRD	A


2.2.1 Electrical Spec. of Set (With VSWR)

Tr1 S11 Smith(R+jX) Scale 1.000U [F1 Del]

1	824.000000MHZ	44.282Ω	-83.294Ω	2.3165 pF
2	894.000000MHZ	26.644Ω	-12.843Ω	13.862 pF
3	960.000000MHZ	30.924Ω	54.516Ω	9.0380 nH
4	1.71000000GHZ	12.064Ω	-8.7535Ω	10.633 pF
5	1.85000000GHZ	38.296Ω	4.9337Ω	424.44 pF
6	1.88000000GHZ	50.790Ω	3.0378Ω	257.17 pF
7	1.99000000GHZ	35.416Ω	-26.110Ω	3.0631 pF
8	2.17000000GHZ	20.148Ω	-39.459Ω	1.8587 pF

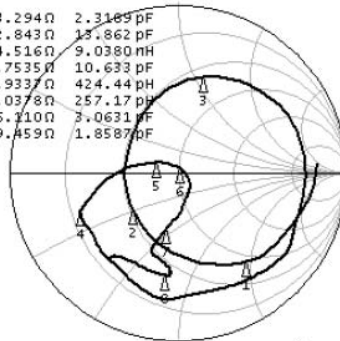

Tr2 S11 SWR 1.000 / 1.000 [F1]

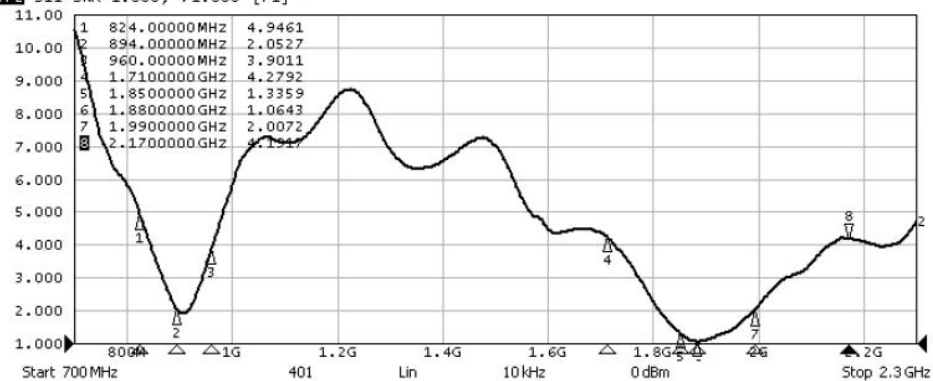

KRD01-00A10-01A

7




Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	8 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A

2.2.2 Passive Gain & 3D Pattern

GSM850, GSM900 Band

3D Pattern

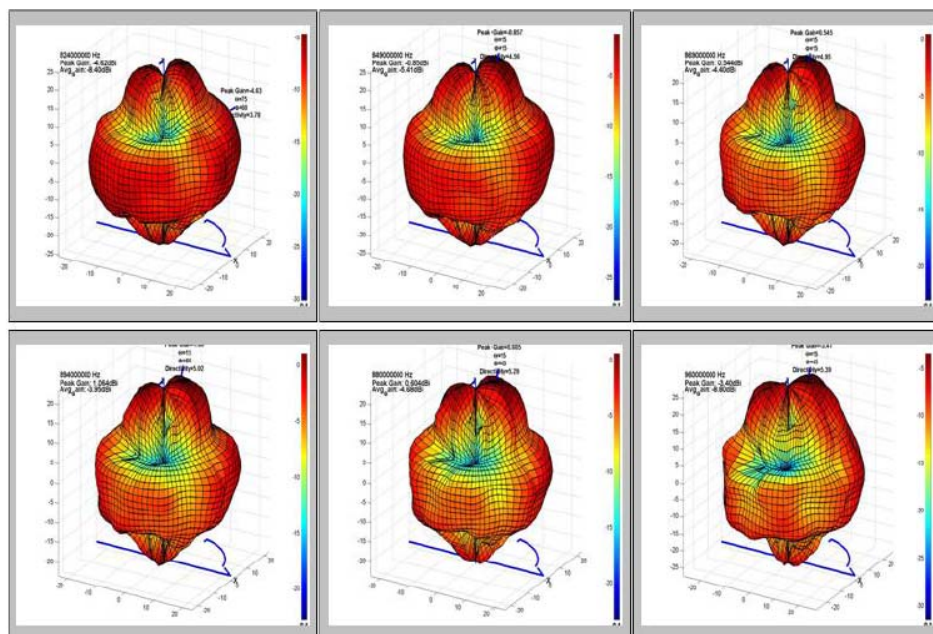

3D Gain

Frequency	Efficiency	Average Gain			Max Gain			Max Position	Directivity
		Ver	Hor	Total	Ver	Hor	Total		
824,000,000 Hz	14.4 %	-13.5 dBi	-10.0 dBi	-8.4 dBi	-11.2 dBi	-5.7 dBi	-4.6 dBi	Theta75/Pie60	3.78 dB
849,000,000 Hz	28.7 %	-9.7 dBi	-7.4 dBi	-5.4 dBi	-2.8 dBi	-5.3 dBi	-0.9 dBi	Theta15/Pie15	4.56 dB
869,000,000 Hz	36.3 %	-8.4 dBi	-6.6 dBi	-4.4 dBi	-1.5 dBi	-3.8 dBi	0.5 dBi	Theta15/Pie15	4.95 dB
894,000,000 Hz	40.2 %	-8.3 dBi	-6.0 dBi	-4.0 dBi	-1.5 dBi	-2.4 dBi	1.1 dBi	Theta15/Pie60	5.02 dB
880,000,000 Hz	34.0 %	-8.4 dBi	-7.1 dBi	-4.7 dBi	-1.9 dBi	-3.0 dBi	0.6 dBi	Theta15/Pie45	5.29 dB
960,000,000 Hz	13.2 %	-12.6 dBi	-11.1 dBi	-8.8 dBi	-7.3 dBi	-5.7 dBi	-3.4 dBi	Theta15/Pie45	5.39 dB

KRD01-00A10-01A

8




Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	9 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A

2.2.2 Passive Gain & 3D Pattern

DCS, PCS Band , WCDMA2100

3D Pattern

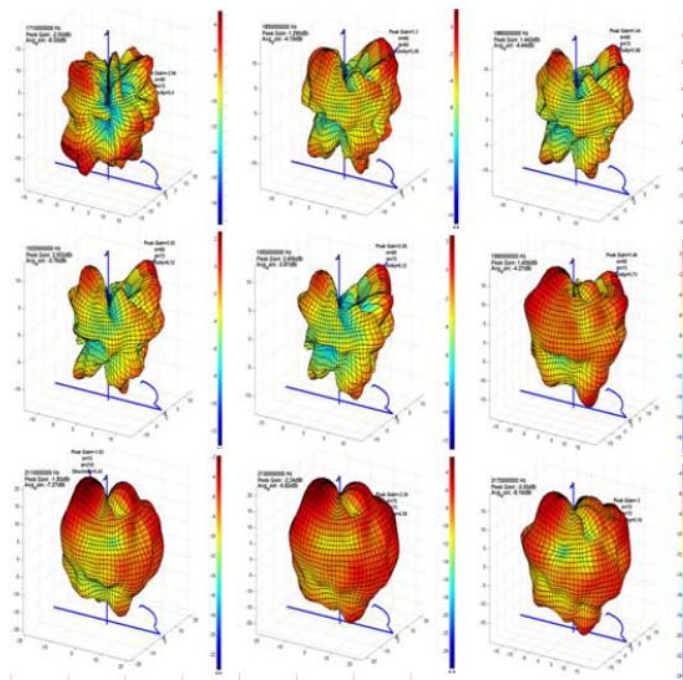

3D Gain

Frequency	Efficiency	Average Gain			Max Gain			Max Position	Directivity
		Ver	Hor	Total	Ver	Hor	Total		
1,710,000,000 Hz	14.7 %	-12.0 dBi	-10.8 dBi	-8.3 dBi	-6.6 dBi	-5.4 dBi	-2.9 dBi	Theta90/Pie75	5.40 dB
1,850,000,000 Hz	38.0 %	-8.4 dBi	-6.3 dBi	-4.2 dBi	-4.4 dBi	-0.1 dBi	1.3 dBi	Theta60/Pie60	5.48 dB
1,870,000,000 Hz	38.3 %	-9.2 dBi	-6.4 dBi	-4.2 dBi	-4.1 dBi	0.2 dBi	1.6 dBi	Theta60/Pie60	5.77 dB
1,880,000,000 Hz	36.0 %	-8.5 dBi	-6.6 dBi	-4.4 dBi	-4.3 dBi	0.1 dBi	1.4 dBi	Theta60/Pie75	5.88 dB
1,900,000,000 Hz	52.6 %	-6.7 dBi	-5.1 dBi	-2.8 dBi	-2.5 dBi	2.1 dBi	3.4 dBi	Theta60/Pie75	6.17 dB
1,920,000,000 Hz	42.0 %	-7.6 dBi	-6.1 dBi	-3.8 dBi	-3.7 dBi	1.4 dBi	2.6 dBi	Theta60/Pie75	6.32 dB
1,950,000,000 Hz	41.0 %	-7.9 dBi	-6.0 dBi	-3.9 dBi	-4.2 dBi	1.4 dBi	2.5 dBi	Theta60/Pie75	6.33 dB
1,990,000,000 Hz	37.4 %	-8.3 dBi	-6.5 dBi	-4.3 dBi	-5.6 dBi	0.5 dBi	1.5 dBi	Theta60/Pie75	5.73 dB
2,110,000,000 Hz	18.7 %	-10.3 dBi	-10.3 dBi	-7.3 dBi	-5.9 dBi	-4.0 dBi	-1.8 dBi	Theta15/Pie210	5.45 dB
2,130,000,000 Hz	20.8 %	-10.0 dBi	-8.7 dBi	-6.8 dBi	-5.3 dBi	-5.2 dBi	-2.2 dBi	Theta75/Pie75	4.58 dB
2,140,000,000 Hz	20.7 %	-10.1 dBi	-9.6 dBi	-6.8 dBi	-5.0 dBi	-5.0 dBi	-2.0 dBi	Theta75/Pie75	4.86 dB
2,170,000,000 Hz	15.3 %	-11.7 dBi	-10.7 dBi	-8.2 dBi	-6.4 dBi	-5.6 dBi	-3.0 dBi	Theta75/Pie75	5.16 dB

KRD01-00A10-01A

9



Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	10 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A

3. Mechanical Specification

3.1 Material Certification

Model		BP80S (MAIN)						
Ant Type		Main Intenna						
No	Part Name	Raw Material (Plating Spec.)	Raw Material color	Raw Material Company	Manufacture Company	Post Processing	Post Processing Company	Cavity
1	Carrier	Polycarbonate (SC1004A-KPA1)	Black	LG chemical	HANKOOK QDM	-	-	1X1
2	Pattern	Cu Plating (9~15μm)	-	EC TECH	Bukwang Plating	-	-	-
		Ni Plating (2~3.5μm)	-	EC TECH	Bukwang Plating	-	-	-

KRD01-00A10-01A

10



Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	11 / 13

Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	INTENNA		BLUEBIRD	A

3.2 Mechanical Specification

3.2.1 Part List


PARTS LIST											
PRODUCT NAME/MODEL			KIN-MAIN-BS1401 / BP80S INTENNA			ESTABLISH. DATE		2015.01.28			
CUSTOMER			BLUEBIRD			REVISION DATE		-			
FREQUENCY			MAIN			REVISION No		IR			
No.	PART NAME	PART NO.	PART SIZE (mm)	MATERIAL	MATERIAL PROVIDER	Q'TY	Rev.	CHANGE CONTENT	SECTION	COMPANY	REMARK
1	CARRIER	BS-1401PCRRP1	61.93 X 8.64 X 1.0	PC	LG chemical	1EA	IR	-	MOLD	HANKOOK QDM	1X1
2	PATTERN	BS-1401PELPID	57.7 x 5.1	LDP (Cu : 9+15um Ni : 2+3.5um)	EC TECH	1EA	IR	-	-	Bukwang Plating	
3	TRAY	-	420 X 300 X 11.5	PP	-	1EA	IR	-	-		
4	OUT BOX	-	445 X 442 X 360	DW2	-	1EA	IR	-	-		



Document NO.	KAT-1501-IN001P
Maker Code	KIN-MAIN-BS1401
DATE	2015. 01. 29
Page	12 / 13


Model	Type	Rev.	DONGNAM	IR
BP80S (MAIN)	ANTENNA		BLUEBIRD	A

3.2.2 Assy Drawing

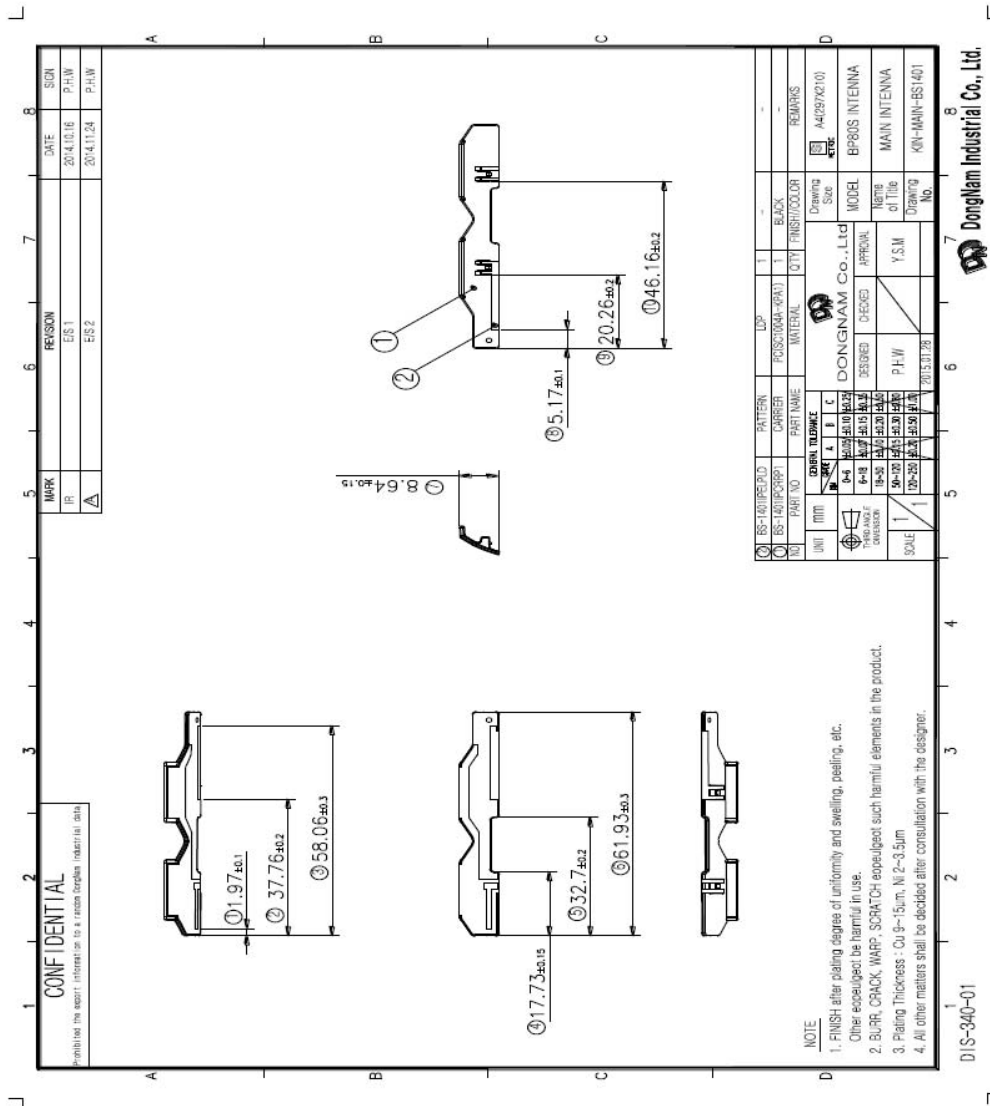

KRD01-00A10-01A

12

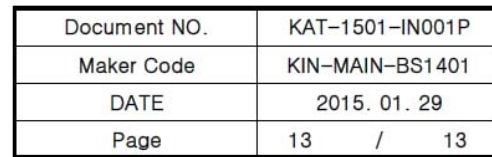

3.2.3 Packing Spec. & Drawing



2. WLAN Antenna Data Sheet



Document NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	1 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	INTENNA		BLUEBIRD	A

APPROVAL SHEET

Customer : BLUEBIRD

Company : DONGNAM




Item : INTENNA

Model : BP80S (WiFi)

Customer P/N :

Maker Code : KIN-MAIN-BS1401



Department	Investigation	Verification	Approval
RF			
Machine			
Safety			

KRD01-00A10-01A

1

EMC-003 (Rev.2)




PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	2 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	INTENNA		BLUEBIRD	A

► Contents ◀

1. Revision History of Product Specification	03/13
1.1 History List of Approval Sheet	03/13
2. Circuit Specification	04/13
2.1 Test Setting	04/13
2.1.1 Test Environment (Condition/Method)	04/13
2.2 Electrical Specification	06/13
2.2.1 Electrical Spec. of SET (With VSWR)	07/13
2.2.2 2.4GHz Passive Gain & 3D Pattern	08/13
2.2.3 5GHz Passive Gain & 3D Pattern	09/13
3. Mechanical Specification	10/13
3.1 Material Certification	10/13
3.2 Mechanical Specification	11/13
3.2.1 Part List	11/13
3.2.2 Assy Drawing	12/13
3.2.3 Packing Spec. & Drawing	13/13



1.1 History List of Approval Sheet



PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	4 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	ANTENNA		BLUEBIRD	A

2. Circuit Specification

2.1 Test Setting


2.1.1 Test Environment (Condition/Method)

① VSWR

Step 1. Connect ANT port with cable included adaptor to port1 of Network analyzer

Step 2. Point out markers on network analyzer display at target frequencies.

Step 3. Inspect VSWR

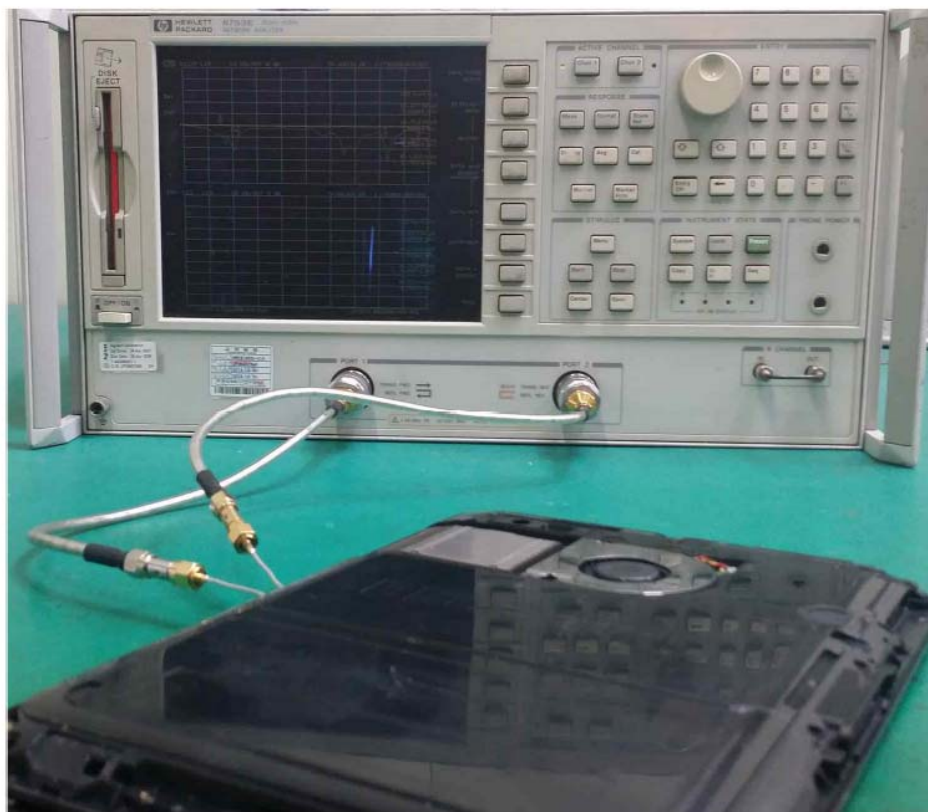

KRD01-00A10-01A

4



PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	5 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	INTENNA		BLUEBIRD	A


② Radiation Pattern and Gain

Step 1. Calibrate chamber system for gain measurement using horn antenna.

At the same time set up software program for chamber system control.

Step 2. Change over from a horn antenna to measuring antenna on target positioner

Step 3. Start a software program for chamber system control & measuring.

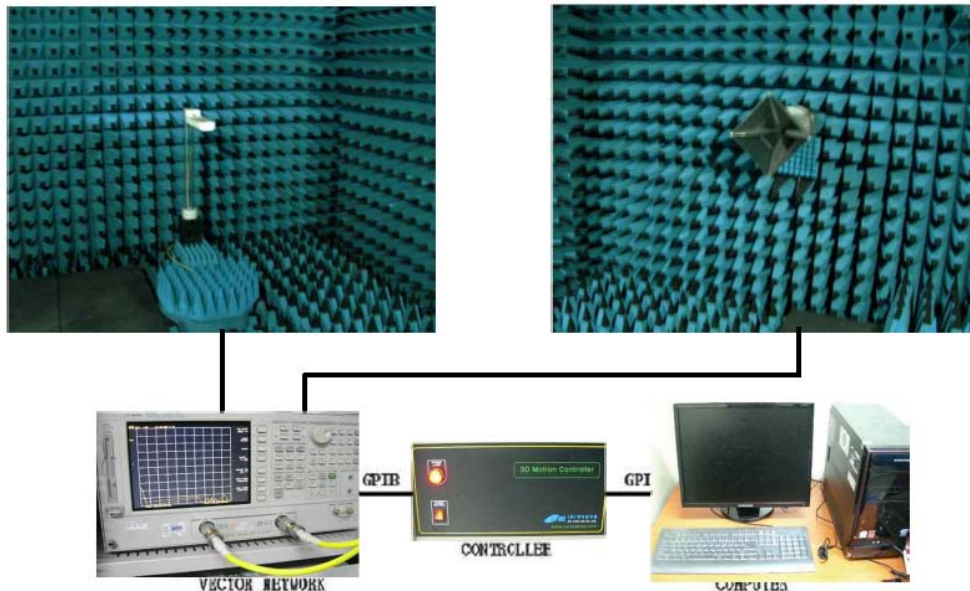

KRD01-00A10-01A


5



PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	6 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	Cable Antenna		BLUEBIRD	A

2.2 Electrical Specification

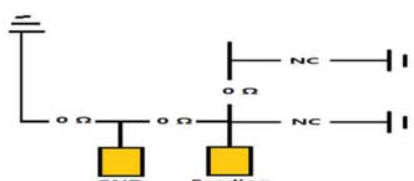Frequency	2400MHz	2480MHz	5200MHz	5800MHz
VSWR	≤ 1.61	≤ 1.50	≤ 1.37	≤ 4.04
Peak Gain (dBi)	≤ 1.3	≤ 2.6	≤ 1.7	≤ 3.6
Average Gain (dBi)	≥ -3.7	≥ -3.3	≥ -5.0	≥ -2.7
Directivity	Omni-directional			
Polarization	Linear			
Matching Value	 			

KRD01-00A10-01A


6



PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	7 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	Cable Antenna		BLUEBIRD	A

2.2.1 Electrical Spec. of Set (With VSWR)

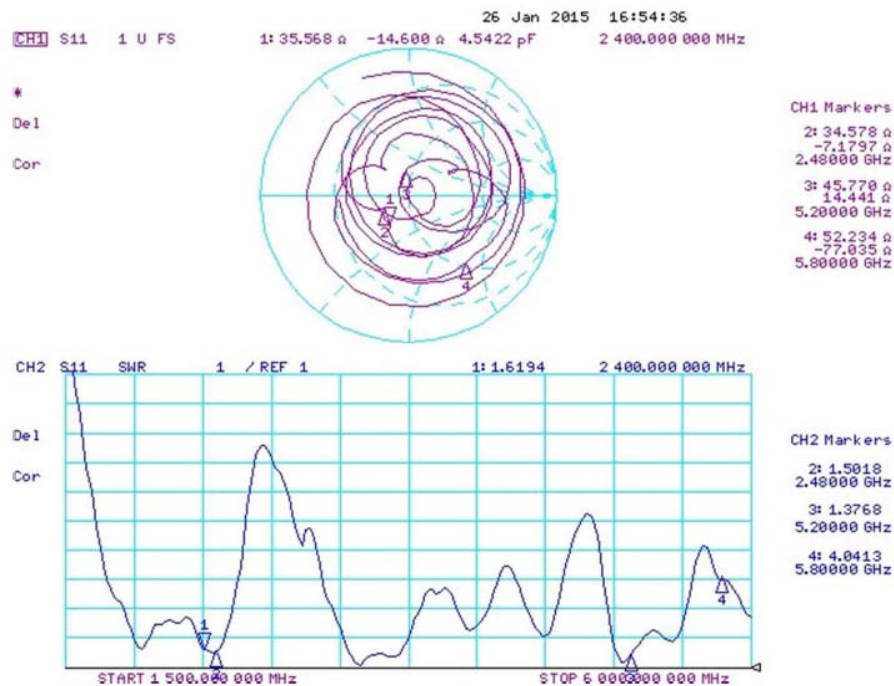

KRD01-00A10-01A

7




PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	8 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	Cable Antenna		BLUEBIRD	A

2.2.2 2.4GHz Passive Gain & 3D Pattern

3D Pattern

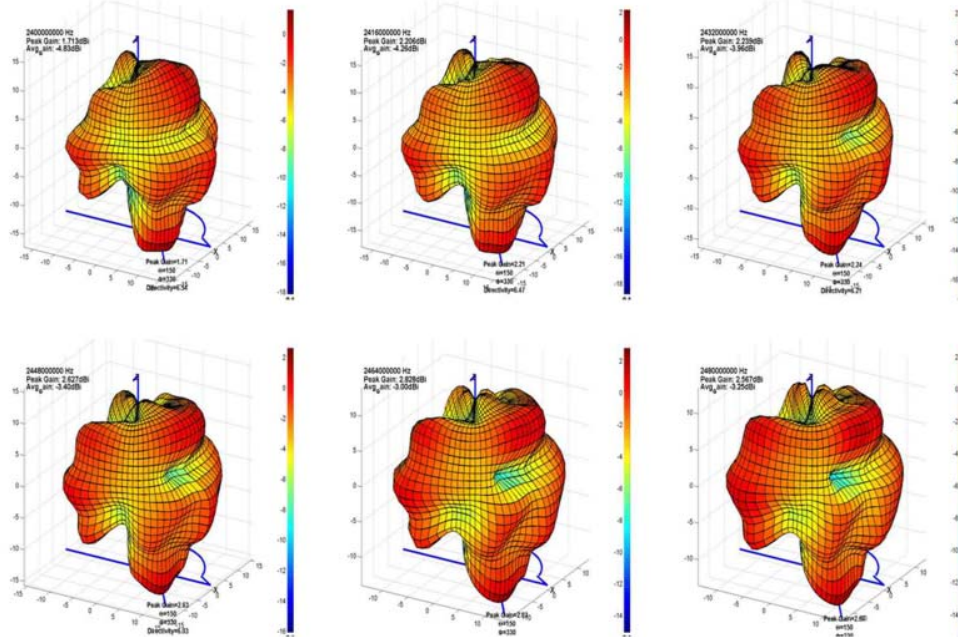

Passive Gain

Frequency	Efficiency	Average Gain			Max Gain			Max Position	Directivity
		Ver	Hor	Total	Ver	Hor	Total		
2,400,000,000 Hz	42.5 %	-7.3 dBi	-6.2 dBi	-3.7 dBi	-0.7 dBi	0.7 dBi	1.3 dBi	Theta150/Pie60	6.54 dB
2,416,000,000 Hz	43.0 %	-7.5 dBi	-6.0 dBi	-3.6 dBi	-0.3 dBi	2.5 dBi	2.5 dBi	Theta150/Pie60	6.47 dB
2,432,000,000 Hz	45.6 %	-6.8 dBi	-6.1 dBi	-3.4 dBi	0.0 dBi	0.7 dBi	1.6 dBi	Theta150/Pie60	6.21 dB
2,448,000,000 Hz	45.7 %	-7.9 dBi	-5.3 dBi	-3.4 dBi	-0.1 dBi	2.6 dBi	2.6 dBi	Theta150/Pie60	6.03 dB
2,464,000,000 Hz	50.0 %	-7.7 dBi	-4.8 dBi	-3.0 dBi	0.2 dBi	2.8 dBi	2.8 dBi	Theta150/Pie60	5.84 dB
2,480,000,000 Hz	47.3 %	-8.3 dBi	-4.9 dBi	-3.3 dBi	-0.5 dBi	2.5 dBi	2.6 dBi	Theta150/Pie60	5.82 dB

KRD01-00A10-01A

8




PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	9 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WIFI)	Cable Antenna		BLUEBIRD	A

2.2.3 5GHz Passive Gain & 3D Pattern

3D Pattern

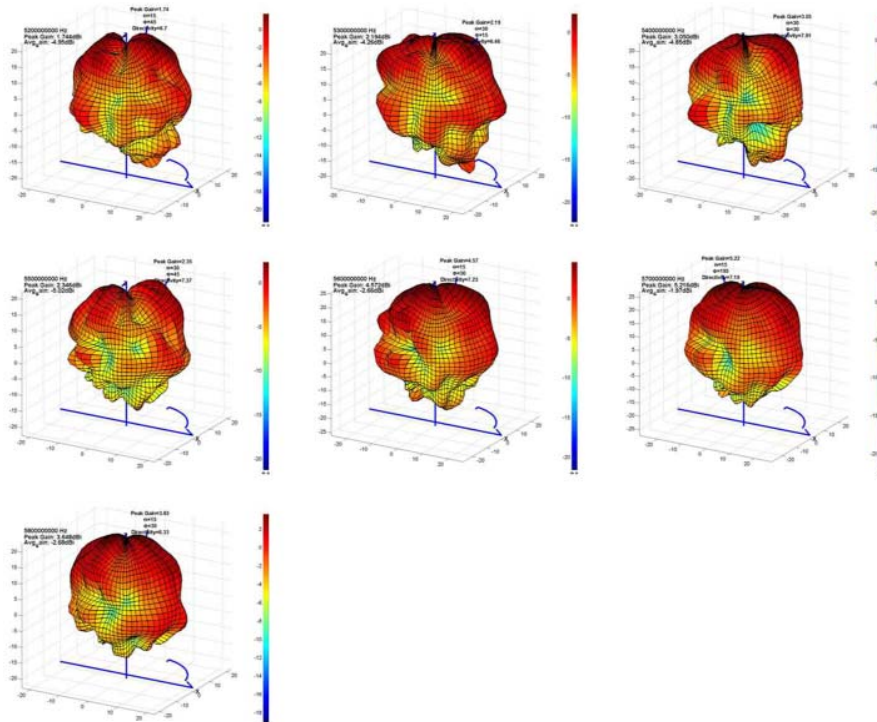

Passive Gain

Frequency	Efficiency	Average Gain			Max Gain			Max Position	Directivity
		Ver	Hor	Total	Ver	Hor	Total		
5,200,000,000 Hz	31.9 %	-8.0 dBi	-7.9 dBi	-5.0 dBi	-1.0 dBi	1.3 dBi	1.7 dBi	Theta15/Pie135	6.70 dB
5,300,000,000 Hz	37.5 %	-7.3 dBi	-7.2 dBi	-4.3 dBi	-0.3 dBi	0.8 dBi	2.2 dBi	Theta30/Pie105	6.46 dB
5,400,000,000 Hz	32.7 %	-9.6 dBi	-6.6 dBi	-4.9 dBi	-3.0 dBi	2.0 dBi	3.1 dBi	Theta30/Pie120	7.91 dB
5,500,000,000 Hz	31.4 %	-8.4 dBi	-7.7 dBi	-5.0 dBi	-2.3 dBi	1.6 dBi	2.3 dBi	Theta30/Pie135	7.37 dB
5,600,000,000 Hz	54.2 %	-7.6 dBi	-4.3 dBi	-2.7 dBi	-1.6 dBi	4.0 dBi	4.6 dBi	Theta15/Pie120	7.23 dB
5,700,000,000 Hz	63.5 %	-5.5 dBi	-4.5 dBi	-2.0 dBi	1.0 dBi	4.2 dBi	5.2 dBi	Theta15/Pie285	7.19 dB
5,800,000,000 Hz	53.9 %	-5.4 dBi	-6.0 dBi	-2.7 dBi	1.1 dBi	2.6 dBi	3.6 dBi	Theta15/Pie120	6.33 dB

KRD01-00A10-01A

9



PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	10 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	Cable Antenna		BLUEBIRD	A

3. Mechanical Specification

3.1 Material Certification

Model		BP80S (WiFi)						
Ant Type		WiFi Intenna						
No	Part Name	Raw Material (Plating Spec.)	Raw Material color	Raw Material Company	Manufacture Company	Post Processing	Post Processing Company	Cavity
1	Carrier	Polycarbonate (SC1004A-KPA1)	Black	LG chemical	HANKOOK QDM	—	—	1X1
2	Pattern	Cu Plating (9~15 μ m)	—	EC TECH	Bukwang Plating	—	—	—
		Ni Plating (2~3.5 μ m)	—	EC TECH	Bukwang Plating	—	—	—

KRD01-00A10-01A

10



Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	Cable Antenna		BLUEBIRD	A


[illegible]



PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	12 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	Cable Antenna		BLUEBIRD	A

3.2.2 Assy Drawing

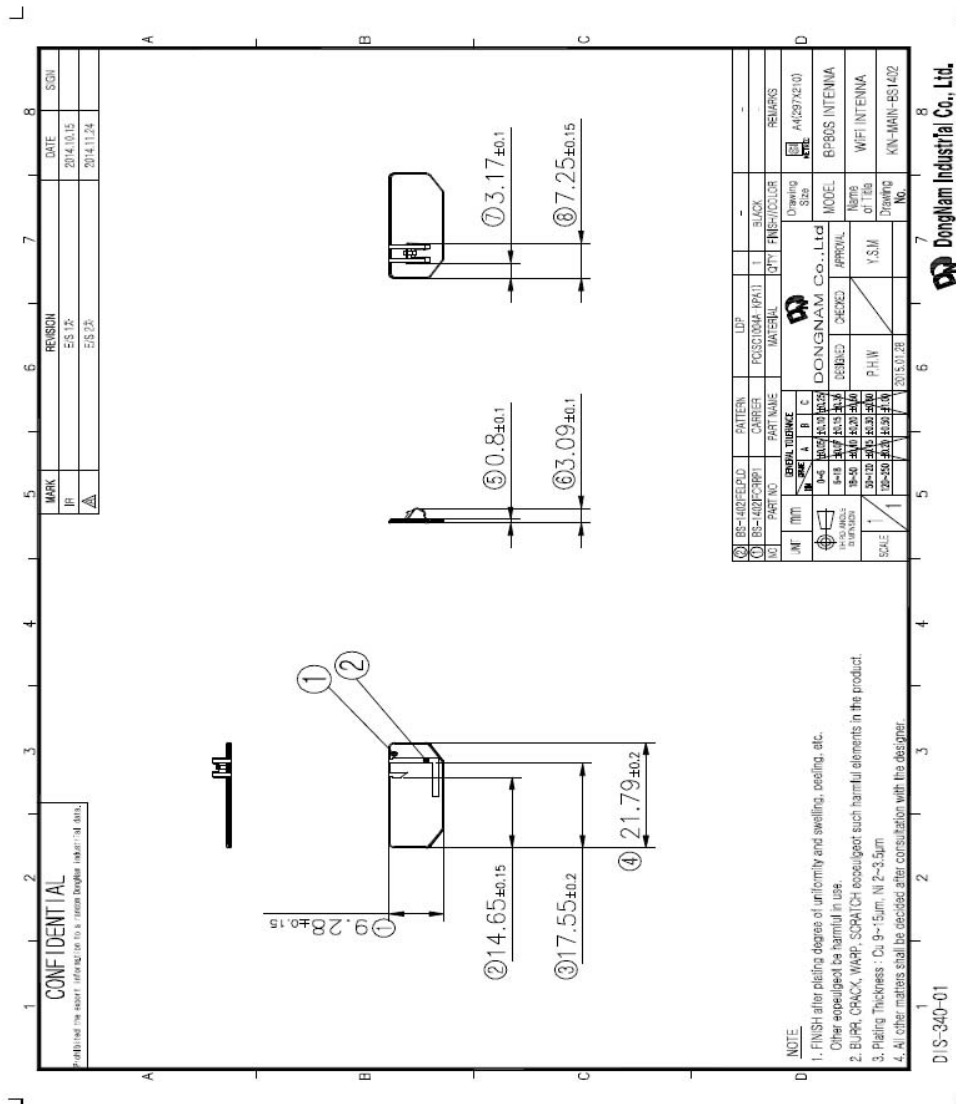

KRD01-00A10-01A


12



PART NO.	KAT-1501-IN002P
Maker Code	KIN-WIFI-BS1402
DATE	2015. 1. 29
Page	13 / 13

Model	Type	Rev.	DONGNAM	IR
BP 80S (WiFi)	Cable Antenna		BLUEBIRD	A

3.2.3 Packing Spec. & Drawing

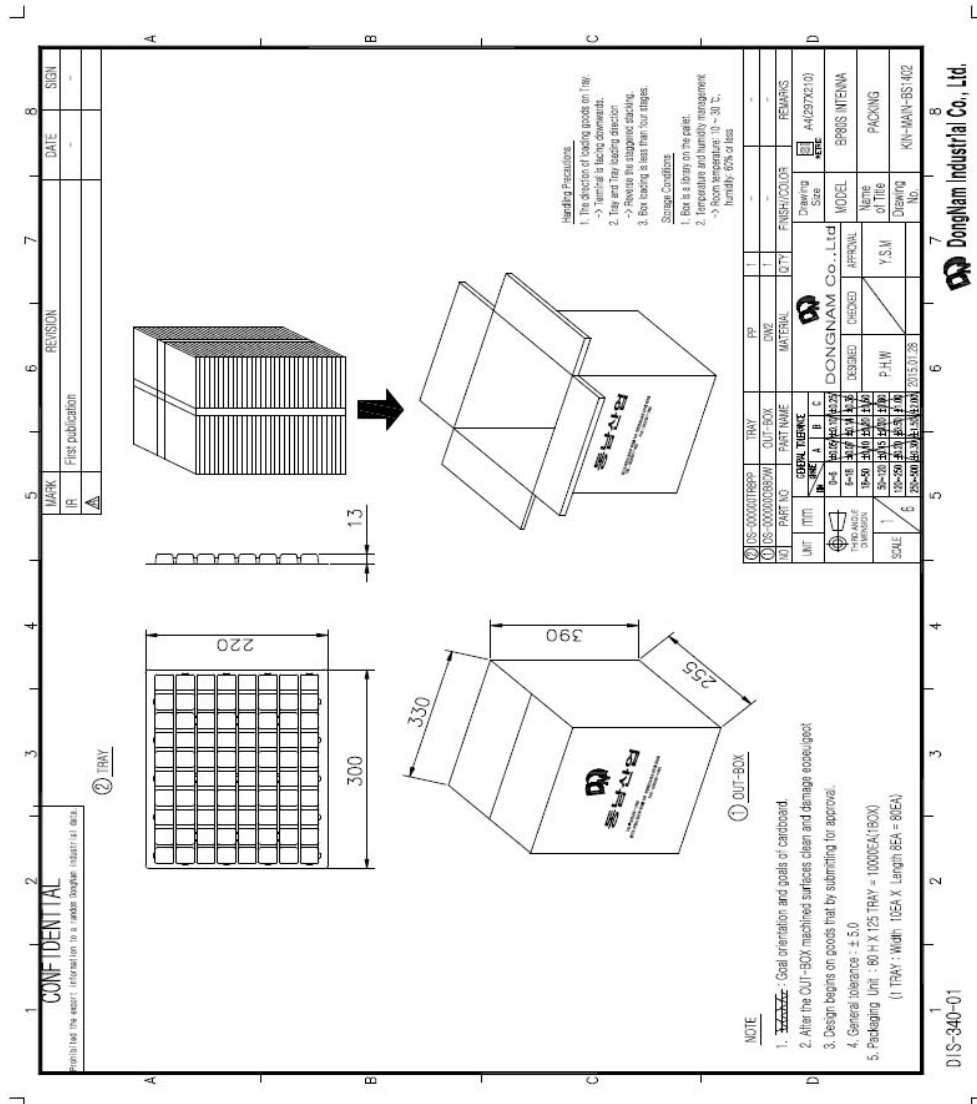

KRD01-00A10-01A

13

ANNEX E. PROBE AND DIPOLE CALIBRATION CERTIFICATES

< E-Field Probe : ES3DV3 – SN 3171 >

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client **One-Tech (Dymstec)**

Certificate No: **ES3-3171_Jul14**

CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3171**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6
Calibration procedure for dosimetric E-field probes**

Calibration date: **July 18, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498087	03-Apr-14 (No. 217-01911)	Apr-15
Reference 3 dB Attenuator	SN: S5054 (3c)	03-Apr-14 (No. 217-01915)	Apr-15
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Apr-15
Reference Probe ES3DV2	SN: 3013	30-Dec-13 (No. ES3-3013_Dec13)	Dec-14
DAE4	SN: 660	13-Dec-13 (No. DAE4-660_Dec13)	Dec-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
Issued: July 22, 2014			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

Certificate No: ES3-3171_Jul14

Page 1 of 11

EMC-003 (Rev.2)

HEAD OFFICE : 301-14 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-799-9500, FAX: 82-31-799-9599)
EMC Testing Div. : 307-51 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-765-8289, FAX: 82-31-766-2904)

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization ϕ	ϕ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E^2 -field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}**: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

ES3DV3 – SN:3171

July 18, 2014

Probe ES3DV3

SN:3171

Manufactured: January 23, 2008
Calibrated: July 18, 2014

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

Certificate No: ES3-3171_Jul14

Page 3 of 11

ES3DV3- SN:3171

July 18, 2014

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3171

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	1.06	1.20	1.20	$\pm 10.1 \%$
DCP (mV) ^B	103.5	98.0	101.8	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	195.4	$\pm 3.8 \%$
		Y	0.0	0.0	1.0		204.9	
		Z	0.0	0.0	1.0		205.0	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E^2 -field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3- SN:3171

July 18, 2014

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3171

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth (mm) ^G	Unct. (k=2)
835	41.5	0.90	6.20	6.20	6.20	0.57	1.33	± 12.0 %
1750	40.1	1.37	5.35	5.35	5.35	0.80	1.15	± 12.0 %
1950	40.0	1.40	4.92	4.92	4.92	0.76	1.17	± 12.0 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- SN:3171

July 18, 2014

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3171

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
835	55.2	0.97	6.08	6.08	6.08	0.31	1.90	± 12.0 %
1750	53.4	1.49	5.03	5.03	5.03	0.47	1.77	± 12.0 %
1950	53.3	1.52	4.86	4.86	4.86	0.60	1.47	± 12.0 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Certificate No: ES3-3171_Jul14

Page 6 of 11

ES3DV3- SN:3171

July 18, 2014

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

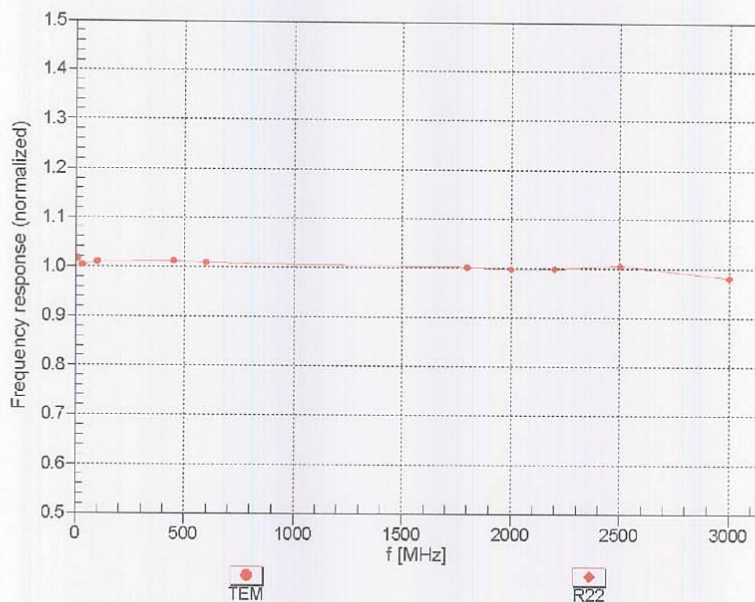

Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

Certificate No: ES3-3171_Jul14

Page 7 of 11

EMC-003 (Rev.2)

HEAD OFFICE : 301-14 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-799-9500, FAX: 82-31-799-9599)
EMC Testing Div. : 307-51 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-765-8289, FAX: 82-31-766-2904)



ES3DV3- SN:3171

July 18, 2014

Receiving Pattern (ϕ), $\theta = 0^\circ$

f=600 MHz,TEM

f=1800 MHz,R22

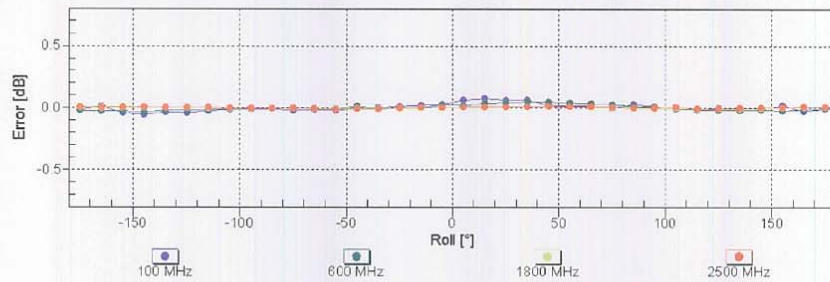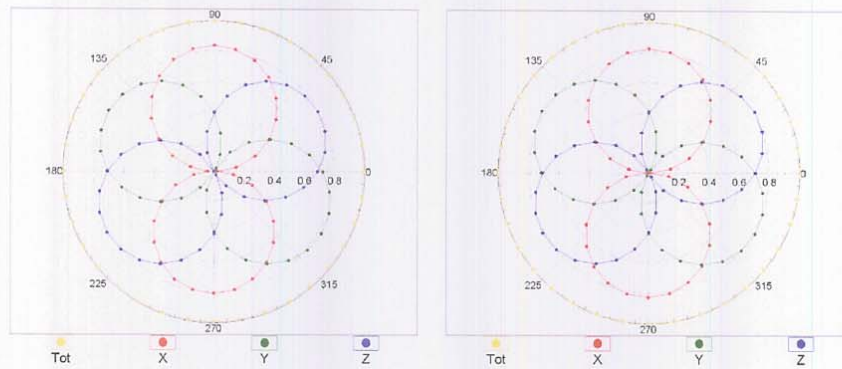

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)

Certificate No: ES3-3171_Jul14

Page 8 of 11


EMC-003 (Rev.2)

HEAD OFFICE : 301-14 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-799-9500, FAX: 82-31-799-9599)
 EMC Testing Div. : 307-51 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-765-8289, FAX: 82-31-766-2904)

ES3DV3- SN:3171

July 18, 2014

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f_{\text{eval}} = 1900 \text{ MHz}$)

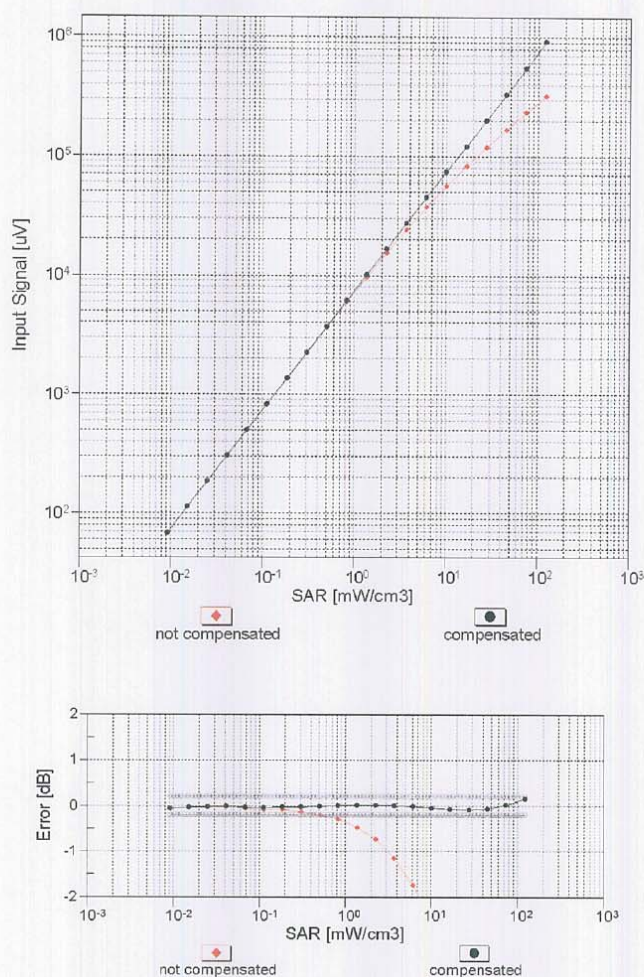

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Certificate No: ES3-3171_Jul14

Page 9 of 11


EMC-003 (Rev.2)

HEAD OFFICE : 301-14 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-799-9500, FAX: 82-31-799-9599)
EMC Testing Div. : 307-51 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-765-8289, FAX: 82-31-766-2904)


ES3DV3- SN:3171

July 18, 2014

Conversion Factor Assessment

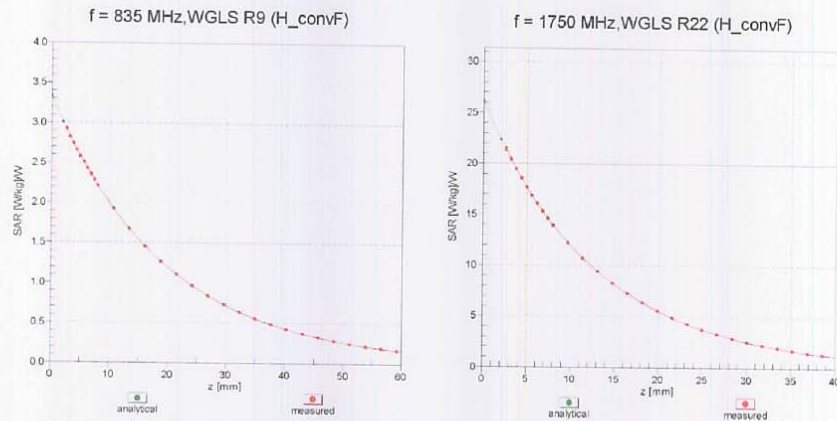

Deviation from Isotropy in Liquid Error (ϕ, θ), $f = 900$ MHz

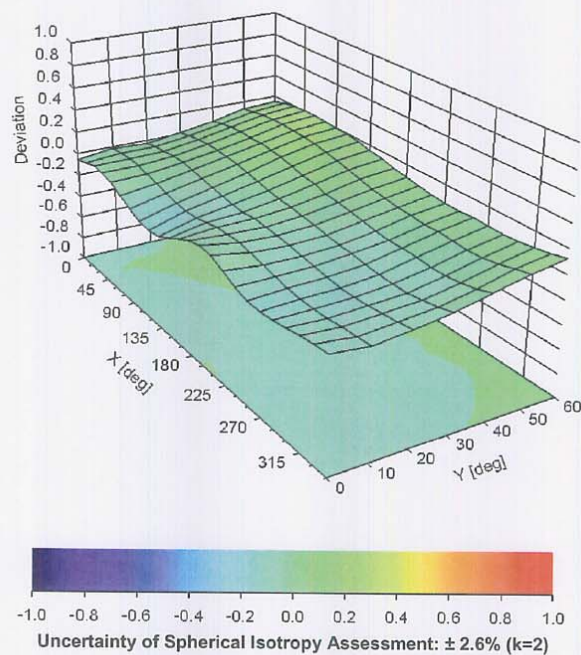

Certificate No: ES3-3171_Jul14

Page 10 of 11

EMC-003 (Rev.2)

HEAD OFFICE : 301-14 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-799-9500, FAX: 82-31-799-9599)
EMC Testing Div. : 307-51 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-765-8289, FAX: 82-31-766-2904)

ES3DV3- SN:3171

July 18, 2014

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3171

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-74.8
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

< Probe : EX3DV4 – SN 3716 >

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **One-Tech (Dymstec)**

Certificate No: **EX3-3716_Nov14**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3716**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6
Calibration procedure for dosimetric E-field probes**

Calibration date: **November 18, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498087	03-Apr-14 (No. 217-01911)	Apr-15
Reference 3 dB Attenuator	SN: S5054 (3c)	03-Apr-14 (No. 217-01915)	Apr-15
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Apr-15
Reference Probe ES3DV2	SN: 3013	30-Dec-13 (No. ES3-3013_Dec13)	Dec-14
DAE4	SN: 660	13-Dec-13 (No. DAE4-660_Dec13)	Dec-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Calibrated by:	Name Claudio Leubler	Function Laboratory Technician	Signature
Approved by:	Katja Pokovic	Technical Manager	
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: November 18, 2014			

Certificate No: EX3-3716_Nov14

Page 1 of 11

Calibration Laboratory of

Schmid & Partner

Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization ϕ	ϕ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E^2 -field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

EX3DV4 – SN:3716

November 18, 2014

Probe EX3DV4

SN:3716

Manufactured: August 14, 2009
Calibrated: November 18, 2014

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

Certificate No: EX3-3716_Nov14

Page 3 of 11

EX3DV4- SN:3716

November 18, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3716

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.48	0.54	0.48	± 10.1 %
DCP (mV) ^B	97.9	98.9	97.7	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	137.7	±2.5 %
		Y	0.0	0.0	1.0		134.9	
		Z	0.0	0.0	1.0		135.3	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4- SN:3716

November 18, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3716

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
2450	39.2	1.80	6.94	6.94	6.94	0.54	0.70	± 12.0 %
5200	36.0	4.66	4.97	4.97	4.97	0.35	1.80	± 13.1 %
5300	35.9	4.76	4.74	4.74	4.74	0.35	1.80	± 13.1 %
5500	35.6	4.96	4.56	4.56	4.56	0.35	1.80	± 13.1 %
5600	35.5	5.07	4.30	4.30	4.30	0.35	1.80	± 13.1 %
5800	35.3	5.27	4.29	4.29	4.29	0.40	1.80	± 13.1 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3716

November 18, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3716

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
2450	52.7	1.95	7.13	7.13	7.13	0.76	0.58	± 12.0 %
5200	49.0	5.30	4.41	4.41	4.41	0.45	1.90	± 13.1 %
5300	48.9	5.42	4.22	4.22	4.22	0.45	1.90	± 13.1 %
5500	48.6	5.65	3.89	3.89	3.89	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.85	3.85	3.85	0.50	1.90	± 13.1 %
5800	48.2	6.00	4.03	4.03	4.03	0.50	1.90	± 13.1 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4- SN:3716

November 18, 2014

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

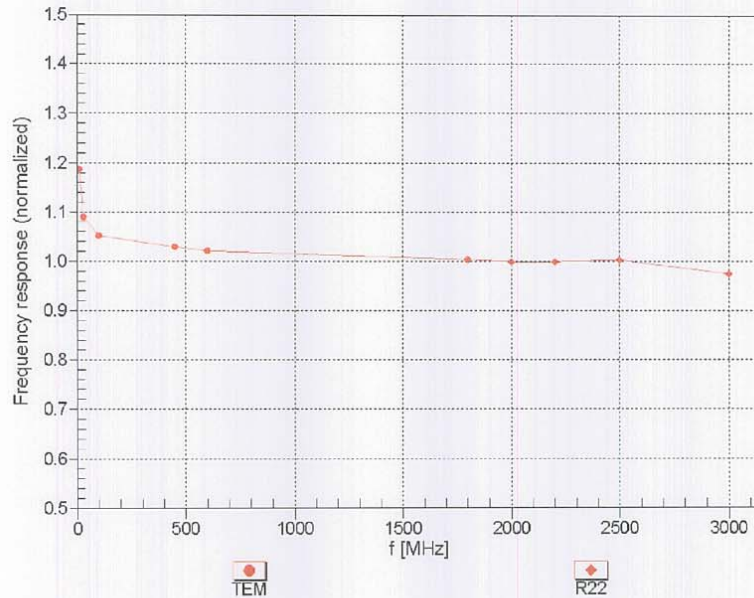


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

EX3DV4- SN:3716

November 18, 2014

Receiving Pattern (ϕ), $\theta = 0^\circ$

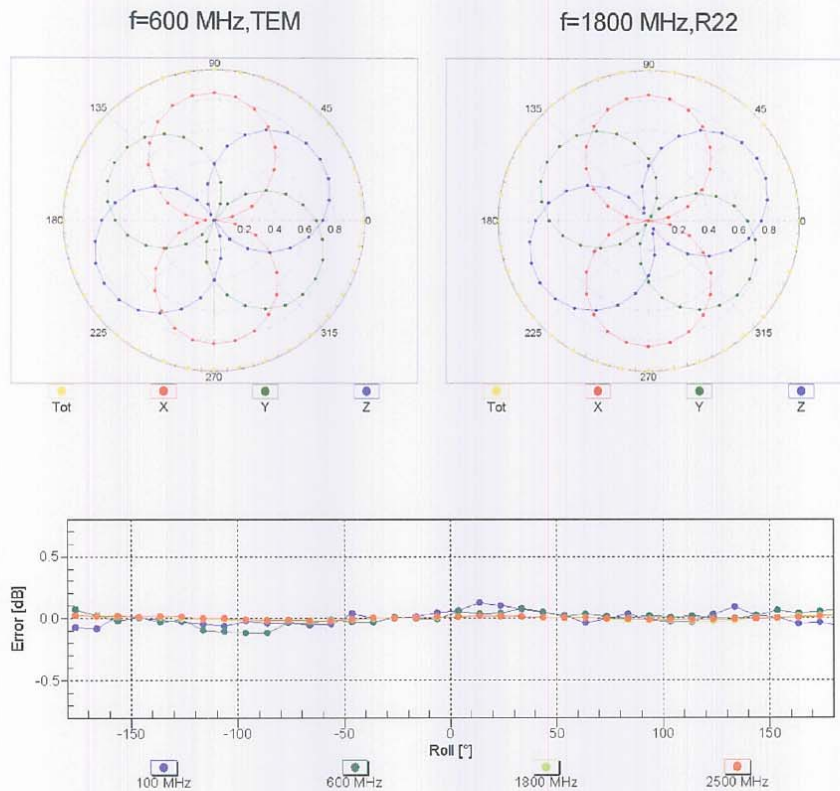

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ ($k=2$)


Certificate No: EX3-3716_Nov14

Page 8 of 11

EX3DV4- SN:3716

November 18, 2014

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell, $f_{\text{eval}} = 1900 \text{ MHz}$)

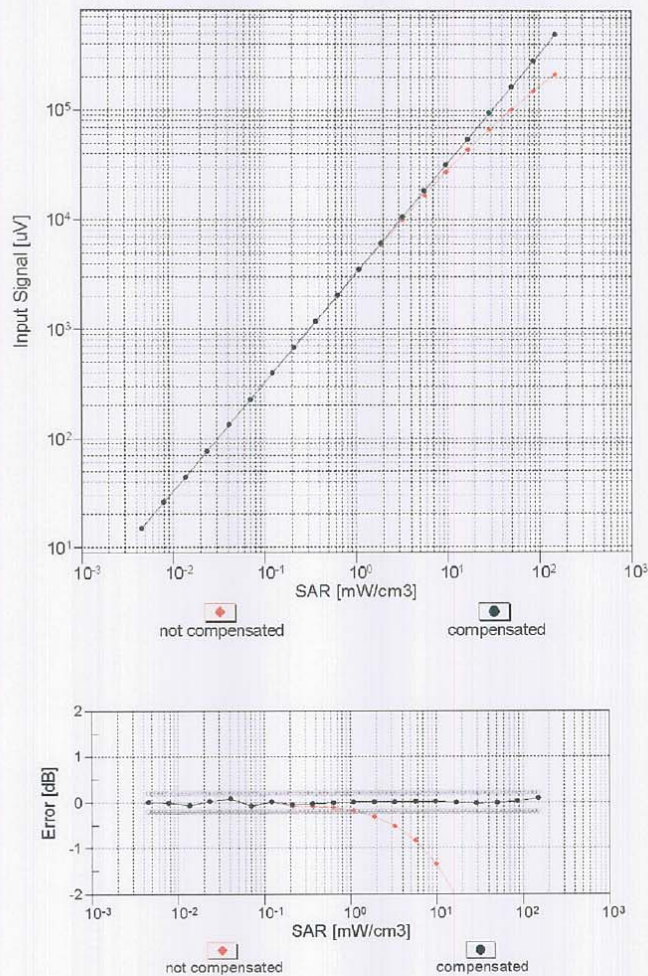

Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Certificate No: EX3-3716_Nov14

Page 9 of 11


EMC-003 (Rev.2)

HEAD OFFICE : 301-14 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-799-9500, FAX: 82-31-799-9599)
EMC Testing Div. : 307-51 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-765-8289, FAX: 82-31-766-2904)

EX3DV4- SN:3716


November 18, 2014

Conversion Factor Assessment

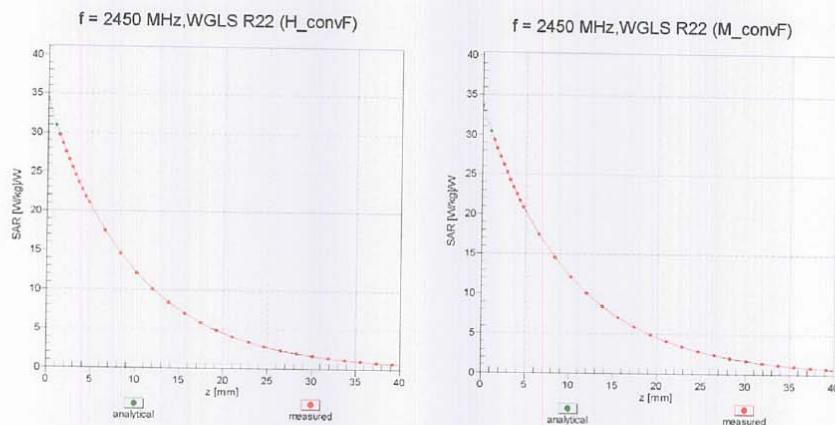

Deviation from Isotropy in Liquid

Error (ϕ , θ), f = 900 MHz

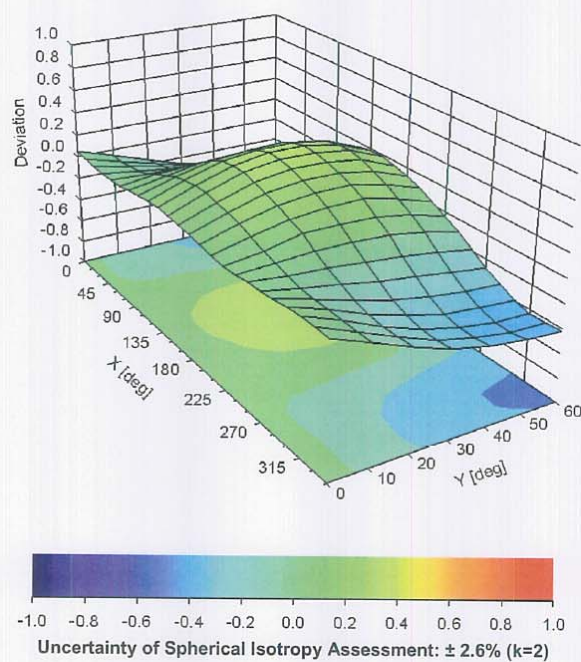

Certificate No: EX3-3716_Nov14

Page 10 of 11

EMC-003 (Rev.2)

HEAD OFFICE : 301-14 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-799-9500, FAX: 82-31-799-9599)

EMC Testing Div. : 307-51 Daessangnyeong-ri, Chowol-eup, Gwangju-si, Gyeonggi-do 464-862 Korea (TEL: 82-31-765-8289, FAX: 82-31-766-2904)

EX3DV4- SN:3716

November 18, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3716

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-76.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm