

DFS TEST REPORT

Application No.: SHCR2501000043HS
FCC ID: 2BFI4AL550
Applicant: Shanghai MediWorks Precision Instruments CO., Ltd.
Address of Applicant: No.7, Ming Pu Phase 2, No. 3279 San Lu Road, Min Hang District, 20110, Shanghai, China
Manufacturer: Shanghai MediWorks Precision Instruments CO., Ltd.
Address of Manufacturer: No.7, Ming Pu Phase 2, No. 3279 San Lu Road, Min Hang District, 20110, Shanghai, China
Factory: Shanghai MediWorks Precision Instruments CO., Ltd.
Address of Factory: No.7, Ming Pu Phase 2, No. 3279 San Lu Road, Min Hang District, 20110, Shanghai, China
Equipment Under Test (EUT):
EUT Name: Optical Biometer
Model No.: AL550, AL551, AL552
Trade Mark: 
Standard(s) : 47 CFR Part 15, Subpart E 15.407
KDB 905462 D02 UNII DFS Compliance Procedures New Rules v02
KDB 905462 D03 UNII Clients Without Radar Detection New Rules v01r02
KDB 905462 D04 Operational Modes for DFS Testing New Rules v01
Date of Receipt: 2025-01-07
Date of Test: 2025-01-13 to 2025-01-22
Date of Issue: 2025-01-22

Test Result:	Pass*
---------------------	--------------

* In the configuration tested, the EUT complied with the standards specified above.

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein.

Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Member of the SGS Group (SGS SA)



SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

SHEM-TRF-001 Rev. 02 Sep01, 2023

Report No.: SHCR250100004303

Page: 2 of 20

Revision Record			
Version	Description	Date	Remark
00	Original	2025-01-22	/

Authorized for issue by:			
Tested By		Bill Wu	
		Bill Wu / Project Engineer	
Approved By		Parlam Zhan	
		Parlam Zhan / Reviewer	

2 Test Summary

Item	Standard	Method	Requirement	Result
Channel Move Time	47 CFR Part 15, Subpart E 15.407	KDB 905462 D02 Section 7.8.3	KDB 905462 D02 Section 5.1	Pass
Channel Closing Transmission Time	47 CFR Part 15, Subpart E 15.407	KDB 905462 D02 Section 7.8.3	KDB 905462 D02 Section 5.1	Pass
Non-occupancy period	47 CFR Part 15, Subpart E 15.407	KDB 905462 D02 Section 7.8.3	KDB 905462 D02 Section 5.1	Pass

Note: There are series models mentioned in this report, and they are the similar in electrical and electronic characters. Only difference is AL551 and AL552 have fewer software functions compared to AL550, as shown in the table below, Consider the difference only the model AL550 was tested.

Model Performance Indicator		AL550	AL551	AL552
Axial length measurements		Applicable	Applicable	Applicable
Corneal thickness measurements		Applicable	Applicable	Not applicable
Anterior chamber depth measurements		Applicable	Applicable	Not applicable
Lens thickness measurements		Applicable	Applicable	Not applicable
Corneal topography	Area measurements	Applicable	Applicable	Not applicable
	Sample density measurement	Applicable	Applicable	Not applicable
	Performance measurements and reports	Applicable	Applicable	Not applicable
	Results shown in colors	Applicable	Applicable	Not applicable
Radius of curvature measurements		Applicable	Applicable	Applicable
Measurement of main meridian axial position		Applicable	Applicable	Applicable
Pupil diameter measurement range		Applicable	Applicable	Applicable
White to white measurement range		Applicable	Applicable	Applicable
Projection ring diameter		Applicable	Applicable	Not applicable

Software Features				
Settings	General	Applicable	Applicable	Applicable
	Date and time	Applicable	Applicable	Applicable
	Network	Applicable	Applicable	Applicable
	Report	Applicable	Applicable	Applicable
	Capture	Applicable	Applicable	Applicable



SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

SHEM-TRF-001 Rev. 02 Sep01, 2023

Report No.: SHCR250100004303

Page: 4 of 20

	Corneal topography	Applicable	Applicable	Not applicable
	DICOM	Applicable	Applicable	Applicable
	Refractive index	Applicable	Applicable	Applicable
	RGP management	Applicable	Applicable	Not applicable
	Accounts	Applicable	Applicable	Applicable
	Storage	Applicable	Applicable	Applicable
	About	Applicable	Applicable	Applicable
Patient information management	Add patients	Applicable	Applicable	Applicable
	View patients	Applicable	Applicable	Applicable
	Edit patients	Applicable	Applicable	Applicable
Medical case management	Create new medical cases	Applicable	Applicable	Applicable
	Delete medical cases	Applicable	Applicable	Applicable
	View medical cases	Applicable	Applicable	Applicable
Capture	Automatic image data capture	Applicable	Applicable	Applicable
	Manual image data capture	Applicable	Applicable	Applicable
Corneal topography and axial measurement	Overview	Applicable	Applicable	Applicable
	Topographic maps	Applicable	Applicable	Not applicable
	Four maps	Applicable	Applicable	Not applicable
	Shape factor	Applicable	Applicable	Not applicable
	Zernike	Applicable	Applicable	Not applicable
	RGP	Applicable	Applicable	Not applicable
	Pupil & Cornea	Applicable	Applicable	Applicable
	Axial measurement	Applicable	Applicable	Applicable
	IOL calculation	Applicable	Not applicable	Not applicable
	Comparison	Applicable	Applicable	Applicable
	Report	Applicable	Applicable	Applicable



SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

SHEN-TRF-001 Rev. 02 Sep01, 2023

Report No.: SHCR250100004303

Page: 5 of 20

3 Contents

	Page
1 COVER PAGE.....	1
2 TEST SUMMARY	3
3 CONTENTS.....	5
4 GENERAL INFORMATION.....	6
4.1 DETAILS OF E.U.T.	6
4.2 SUPPORT UNIT	7
4.3 TEST LOCATION	7
4.4 TEST FACILITY	7
4.5 DEVIATION FROM STANDARDS	7
4.6 ABNORMALITIES FROM STANDARD CONDITIONS.....	7
5 EQUIPMENT LIST	8
6 DYNAMIC FREQUENCY SELECTION	9
6.1 APPLICABILITY OF DFS REQUIREMENTS.....	9
6.2 DFS DETECTION THRESHOLDS	10
6.3 DFS RESPONSE REQUIREMENTS	10
6.4 CLIENT DEVICE REQUIREMENT	11
6.5 PARAMETERS OF RADAR TEST WAVEFORMS	12
6.5.1 Short Pulse Radar Test Waveforms.....	12
6.5.2 Long Pulse Radar Test Waveform	14
6.5.3 Frequency Hopping Radar Test Waveform	15
6.6 CALIBRATION OF RADAR WAVEFORM	16
6.6.1 Radar Waveform Calibration Procedure.....	16
6.6.2 Conducted Calibration Setup	16
6.6.3 Radar Waveform Calibration Result.....	17
6.7 CHANNEL MOVE TIME AND CHANNEL CLOSING TRANSMISSION TIME AND.....	18
6.7.1 Test Procedure.....	18
6.7.2 Test Setup.....	19
6.7.3 Channel Loading	19
6.7.4 Test Result.....	20



SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

SHEN-TRF-001 Rev. 02 Sep01, 2023

Report No.: SHCR250100004303

Page: 6 of 20

4 General Information

4.1 Details of E.U.T.

Power supply: AC 100-240V,50/60Hz

Test Voltage: AC 120V 60Hz

Operation Frequency:	Band	Mode	Frequency Range(MHz)	Number of channels
	Band 1	802.11a/n(HT20)/ac(HT20)	5180-5240	4
		802.11n(HT40)/ac(HT40)	5190-5230	2
		802.11ac(HT80)	5210	1
	Band 2A	802.11a/n(HT20)/ac(HT20)	5260-5320	4
		802.11n(HT40)/ac(HT40)	5270-5310	2
		802.11ac(HT80)	5290	1
	Band 2C	802.11a/n(HT20)/ac(HT20)	5500-5700	11
		802.11n(HT40)/ac(HT40)	5510-5670	5
		802.11ac(HT80)	5530	1
	Band 3	802.11a/n(HT20)/ac(HT20)	5745-5825	5
		802.11n(HT40)/ac(HT40)	5755-5795	2
		802.11ac(HT80)	5775	1
Modulation Type:	802.11a: OFDM (64QAM, 16QAM, QPSK, BPSK) 802.11n: OFDM (BPSK, QPSK, 16QAM, 64QAM) 802.11ac: OFDM (BPSK, QPSK, 16QAM, 64QAM, 256QAM)			
Channel Spacing:	802.11a/n(HT20)/ac(HT20): 20MHz 802.11n(HT40)/ac(HT40): 40MHz 802.11ac(HT80): 80MHz			
Antenna Gain:	Antenna 1: 4.03dBi Antenna 2: 4.03dBi (Provided by manufacturer) Directional gain: 7.04dBi			
Antenna Type:	Antenna 1: PIFA Antenna Antenna 2: PIFA Antenna			
DFS Function:	Slave without Radar detection			
TPC Function:	Not support			



SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

SHEN-TRF-001 Rev. 02 Sep01, 2023

Report No.: SHCR250100004303

Page: 7 of 20

4.2 Support Unit

Instrument	Manufacture	Model No	Serial No
Laptop PC	Lenovo	L460	N/A
Router	Tilgin Ab	HG2504	N/A

4.3 Test Location

All tests were performed at:

SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd. E&E Lab

588 West Jindu Road, Xinqiao, Songjiang, 201612 Shanghai, China

Tel: +86 21 6191 5666 Fax: +86 21 6191 5678

No tests were sub-contracted.

Note:

1. SGS is not responsible for wrong test results due to incorrect information (e.g. max. clock frequency, highest internal frequency, antenna gain, cable loss, etc) is provided by the applicant. (if applicable).
2. SGS is not responsible for the authenticity, integrity and the validity of the conclusion based on results of the data provided by applicant. (if applicable).
3. Sample source: sent by customer.

4.4 Test Facility

The test facility is recognized, certified, or accredited by the following organizations:

• **A2LA (Certificate No. 6332.01)**

SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd. is accredited by the American Association for Laboratory Accreditation(A2LA).

• **FCC (Designation Number: CN1301)**

SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd. has been recognized as an accredited testing laboratory.

• **ISED (CAB Identifier: CN0020)**

SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd. EMC Laboratory has been recognized by Innovation, Science and Economic Development Canada (ISED) as an accredited testing laboratory. Company Number: 8617A

• **VCCI (Member No.: 3061)**

The 3m Semi-anechoic chamber and Shielded Room of SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd. has been registered in accordance with the Regulations for Voluntary Control Measures with Registration No.: R-13868, C-14336, T-12221, G-10830 respectively.

4.5 Deviation from Standards

None

4.6 Abnormalities from Standard Conditions

None

5 Equipment List

Equipment	Manufacturer	Model No	Inventory No	Cal Date	Cal Due Date
RF Conducted Test					
Spectrum Analyzer	R&S	FSP-30	SHEN002-1	2024/12/18	2025-12-17
Spectrum Analyzer	Keysight	N9020B	SHEN241-1	2024/12/18	2025-12-17
Spectrum Analyzer	Agilent	N9020A	SHEN181-1	2024-07-31	2025-07-30
Signal Generator	R&S	SMR20	SHEN006-1	2024-07-31	2025-07-30
Signal Generator	Agilent	N5182A	SHEN182-1	2024-07-31	2025-07-30
Communication Tester	R&S	CMW270	SHEN183-1	2024-05-23	2025-05-22
Communication Tester	R&S	CMW500	SHEN268-1	2024-05-23	2025-05-22
Power Sensor	Keysight	U2021XA * 4	SHEN293-1	2024-07-31	2025-07-30
Splitter	Anritsu	MA1612A	SHEN185-1	/	/
Coupler	e-meca	803-S-1	SHEN186-1	/	/
High-low Temp Cabinet	Suzhou Zhihe	TL-40	SHEN087-1	2024-11-05	2026-11-04
AC Power Stabilizer	APC	KDF-31020T-V0-F0	SHEN216-1	2024/12/18	2025-12-17
DC Power Supply	HP	6010A	SHEN222-1	2024/12/18	2025-12-17
Conducted test Cable	/	RF01~RF04	/	2024/12/18	2025-12-17
Switcher	Tonscend	JS0806	SHEN293-1	2024-07-31	2025-07-30
Test software	Tonscend	JS Tonscend BT/WIFI System	Version: 2.6	/	/
Switcher+Power Sensor	TST	TSPS2023R	SHEN263-1	2024-07-31	2025-07-30
Test software	TST	TST PASS	Version: 2.0	/	/
RF Radiated Test					
EMI test Receiver	R&S	ESU40	SHEN051-1	2024/12/18	2025-12-17
Spectrum Analyzer	R&S	FSP-30	SHEN002-1	2024/12/18	2025-12-17
Communication Tester	R&S	CMW500	SHEN268-1	2024-05-23	2025-05-22
Loop Antenna (9kHz-30MHz)	Schwarzbeck	FMZB1519	SHEN135-1	2024/12/18	2025-12-17
Antenna (25MHz-2GHz)	Schwarzbeck	VULB9168	SHEN048-1	2023-09-03	2025-09-02
Antenna (25MHz-2GHz)	Schwarzbeck	VULB9168	SHEN202-1	2023-04-17	2025-04-16
Horn Antenna (1-18GHz)	Schwarzbeck	HF906	SHEN009-1	2024-08-05	2026-08-04
Horn Antenna (1-18GHz)	Schwarzbeck	BBHA9120D	SHEN050-1	2023-09-03	2025-09-02
Horn Antenna (14-40GHz)	Schwarzbeck	BBHA 9170	SHEN049-1	2023-09-03	2025-09-02
Pre-Amplifier	HP	8447D	SHEN236-1	2024/12/18	2025-12-17
High-amplifier (14-40GHz)	Schwarzbeck	10001	SHEN049-2	2024/12/18	2025-12-17
Band Filter	LORCH	9BRX-875/X150	SHEN156-1	/	/
Band Filter	LORCH	13BRX-1950/X500	SHEN083-2	/	/
Band Filter	LORCH	5BRX-2400/X200	SHEN155-1	/	/
Band Filter	LORCH	5BRX-5500/X1000	SHEN157-2	/	/
High pass Filter	Wainwright	WHK3.0/18G	SHEN157-1	/	/
High pass Filter	Wainwright	WHKS1700	SHEN157-3	/	/
Semi/Fully Anechoic	ST	11*6*6M	SHEN078-2	2023-05-06	2026-05-05
RE test Cable	/	PT18-NMNM-10M	SHEN217-2	2024/12/18	2025-12-17
Test software	ESE	E3	Version: 6.111221a	/	/

6 Dynamic Frequency Selection

6.1 Applicability of DFS requirements

Table 1: Applicability of DFS Requirements Prior to Use of a Channel

Requirement	Operational Mode		
	<input type="checkbox"/> Master	<input checked="" type="checkbox"/> Client Without Radar Detection	<input type="checkbox"/> Client with Radar Detection
Non-Occupancy Period	Yes	Not required	Yes
DFS Detection Threshold	Yes	Not required	Yes
Channel Availability Check Time	Yes	Not required	Not required
U-NII Detection Bandwidth	Yes	Not required	Yes

Table 2: Applicability of DFS requirements during normal operation

Requirement	Operational Mode	
	<input type="checkbox"/> Master Device or Client with Radar Detection	<input checked="" type="checkbox"/> Client Without Radar Detection
DFS Detection Threshold	Yes	Not required
Channel Closing Transmission Time	Yes	Yes
Channel Move Time	Yes	Yes
U-NII Detection Bandwidth	Yes	Not required

Additional requirements for devices with multiple bandwidth modes	<input type="checkbox"/> Master Device or Client with Radar Detection	<input checked="" type="checkbox"/> Client Without Radar Detection
U-NII Detection Bandwidth and Statistical Performance Check	All BW modes must be tested	Not required
Channel Move Time and Channel Closing Transmission Time	Test using widest BW mode available	Test using the widest BW mode available for the link
All other tests	Any single BW mode	Not required

Note: Frequencies selected for statistical performance check (Section 7.8.4) should include several frequencies within the radar detection bandwidth and frequencies near the edge of the radar detection bandwidth. For 802.11 devices, it is suggested to select frequencies in each of the bonded 20 MHz channels and the channel center frequency.

6.2 DFS Detection Thresholds

Table 3: DFS Detection Thresholds for Master Devices and Client Devices With Radar Detection

Maximum Transmit Power	Value (See Notes 1, 2, and 3)
EIRP \geq 200 milliwatt	-64 dBm
EIRP $<$ 200 milliwatt and power spectral density $<$ 10 dBm/MHz	-62 dBm
EIRP $<$ 200 milliwatt that do not meet the power spectral density requirement	-64 dBm
<p>Note 1: This is the level at the input of the receiver assuming a 0 dBi receive antenna.</p> <p>Note 2: Throughout these test procedures an additional 1 dB has been added to the amplitude of the test transmission waveforms to account for variations in measurement equipment. This will ensure that the test signal is at or above the detection threshold level to trigger a DFS response.</p> <p>Note3: EIRP is based on the highest antenna gain. For MIMO devices refer to KDB Publication 662911 D01.</p>	

6.3 DFS Response Requirements

Table 4: DFS Response Requirement Values

Parameter	Value
Non-occupancy period	Minimum 30 minutes
Channel Availability Check Time	60 seconds
Channel Move Time	10 seconds See Note 1.
Channel Closing Transmission Time	200 milliseconds + an aggregate of 60 milliseconds over remaining 10 second period. See Notes 1 and 2.
U-NII Detection Bandwidth	Minimum 100% of the U-NII 99% transmission power bandwidth. See Note 3.
<p>Note 1: <i>Channel Move Time</i> and the <i>Channel Closing Transmission Time</i> should be performed with Radar Type 0. The measurement timing begins at the end of the Radar Type 0 burst.</p> <p>Note 2: The <i>Channel Closing Transmission Time</i> is comprised of 200 milliseconds starting at the beginning of the <i>Channel Move Time</i> plus any additional intermittent control signals required facilitating a <i>Channel</i> move (an aggregate of 60 milliseconds) during the remainder of the 10 second period. The aggregate duration of control signals will not count quiet periods in between transmissions.</p> <p>Note 3: During the <i>U-NII Detection Bandwidth</i> detection test, radar type 0 should be used. For each frequency step the minimum percentage of detection is 90 percent. Measurements are performed with no data traffic.</p>	

6.4 Client Device Requirement

- a) A Client Device will not transmit before having received appropriate control signals from a Master Device.
- b) A Client Device will stop all its transmissions whenever instructed by a Master Device to which it is associated and will meet the Channel Move Time and Channel Closing Transmission Time requirements. The Client Device will not resume any transmissions until it has again received control signals from a Master Device.
- c) If a Client Device is performing In-Service Monitoring and detects a Radar Waveform above the DFS Detection Threshold, it will inform the Master Device. This is equivalent to the Master Device detecting the Radar Waveform and d) through f) of section 5.1.1 apply.
- d) Irrespective of Client Device or Master Device detection the Channel Move Time and Channel Closing Transmission Time requirements remain the same.
- e) The client test frequency must be monitored to ensure no transmission of any type has occurred for 30 minutes. Note: If the client moves with the master, the device is considered compliant if nothing appears in the client non-occupancy period test. For devices that shut down (rather than moving channels), no beacons should appear.

Remark: The device under test is moves frequency with the master

6.5 Parameters of radar test Waveforms

This section provides the parameters for required test waveforms, minimum percentage of successful detections, and the minimum number of trials that must be used for determining DFS conformance. Step intervals of 0.1 microsecond for Pulse Width, 1 microsecond for PRI, 1 MHz for chirp width and 1 for the number of pulses will be utilized for the random determination of specific test waveforms.

6.5.1 Short Pulse Radar Test Waveforms

Table 5 Short Pulse Radar Test Waveforms

Radar Type	Pulse Width (μsec)	PRI (μsec)	Number of Pulses	Minimum Percentage of Successful Detection	Minimum Number of Trials
0	1	1428	18	See Note 1	See Note 1
1	1	Test A	Roundup $\left\{ \left(\frac{1}{360} \right) \cdot \left(\frac{19 \cdot 10^6}{\text{PRI}_{\mu\text{SEC}}} \right) \right\}$	60%	30
		Test B			
2	1-5	150-230	23-29	60%	30
3	6-10	200-500	16-18	60%	30
4	11-20	200-500	12-16	60%	30
Aggregate (Radar Types 1-4)				80%	120
<p>Note 1: Short Pulse Radar Type 0 should be used for the detection bandwidth test, channel move time, and channel closing time tests.</p> <p>Test A: 15 unique PRI values randomly selected from the list of 23 PRI values in Table 5a</p> <p>Test B: 15 unique PRI values randomly selected within the range of 518-3066 μsec, with a minimum increment of 1 μsec, excluding PRI values selected in Test A</p>					

A minimum of 30 unique waveforms are required for each of the Short Pulse Radar Types 2 through 4. If more than 30 waveforms are used for Short Pulse Radar Types 2 through 4, then each additional waveform must also be unique and not repeated from the previous waveforms. If more than 30 waveforms are used for Short Pulse Radar Type 1, then each additional waveform is generated with Test B and must also be unique and not repeated from the previous waveforms in Tests A or B.

Test aggregate is average of the percentage of successful detections of short pulse radar types 1-4



SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

SHEM-TRF-001 Rev. 02 Sep01, 2023

Report No.: SHCR250100004303

Page: 13 of 20

Table 5a - Pulse Repetition Intervals Values for Test A

Pulse Repetition Frequency Number	Pulse Repetition Frequency (Pulses Per Second)	Pulse Repetition Interval (Microseconds)
1	1930.5	518
2	1858.7	538
3	1792.1	558
4	1730.1	578
5	1672.2	598
6	1618.1	618
7	1567.4	638
8	1519.8	658
9	1474.9	678
10	1432.7	698
11	1392.8	718
12	1355	738
13	1319.3	758
14	1285.3	778
15	1253.1	798
16	1222.5	818
17	1193.3	838
18	1165.6	858
19	1139	878
20	1113.6	898
21	1089.3	918
22	1066.1	938
23	326.2	3066

6.5.2 Long Pulse Radar Test Waveform

Table 6 – Long Pulse Radar Test Waveform

Radar Type	Pulse Width (μsec)	Chirp Width (MHz)	PRI (μsec)	Number of Pulses per Burst	Number of Bursts	Minimum Percentage of Successful Detection	Minimum Number of Trials
5	50-100	5-20	1000-2000	1-3	8-20	80%	30

The parameters for this waveform are randomly chosen. Thirty unique waveforms are required for the Long Pulse Radar Type waveforms. If more than 30 waveforms are used for the Long Pulse Radar Type waveforms, then each additional waveform must also be unique and not repeated from the previous waveforms.

Each waveform is defined as follows:

- 1) The transmission period for the Long Pulse Radar test signal is 12 seconds.
- 2) There are a total of 8 to 20 Bursts in the 12 second period, with the number of Bursts being randomly chosen. This number is Burst Count.
- 3) Each Burst consists of 1 to 3 pulses, with the number of pulses being randomly chosen. Each Burst within the 12 second sequence may have a different number of pulses.
- 4) The pulse width is between 50 and 100 microseconds, with the pulse width being randomly chosen. Each pulse within a Burst will have the same pulse width. Pulses in different Bursts may have different pulse widths.
- 5) Each pulse has a linear frequency modulated chirp between 5 and 20 MHz, with the chirp width being randomly chosen. Each pulse within a transmission period will have the same chirp width. The chirp is centered on the pulse. For example, with a radar frequency of 5300 MHz and a 20 MHz chirped signal, the chirp starts at 5290 MHz and ends at 5310 MHz.
- 6) If more than one pulse is present in a Burst, the time between the pulses will be between 1000 and 2000 microseconds, with the time being randomly chosen. If three pulses are present in a Burst, the random time interval between the first and second pulses is chosen independently of the random time interval between the second and third pulses.
- 7) The 12 second transmission period is divided into even intervals. The number of intervals is equal to Burst Count. Each interval is of length $(12,000,000 / \text{Burst Count})$ microseconds. Each interval contains one Burst. The start time for the Burst, relative to the beginning of the interval, is between 1 and $[(12,000,000 / \text{Burst Count}) - (\text{Total Burst Length}) + (\text{One Random PRI Interval})]$ microseconds, with the start time being randomly chosen. The step interval for the start time is 1 microsecond. The start time for each Burst is chosen randomly.

A representative example of a Long Pulse Radar Type waveform:

- 1) The total test waveform length is 12 seconds.
- 2) Eight (8) Bursts are randomly generated for the Burst Count.
- 3) Burst 1 has 2 randomly generated pulses.
- 4) The pulse width (for both pulses) is randomly selected to be 75 microseconds.
- 5) The PRI is randomly selected to be at 1213 microseconds.
- 6) Bursts 2 through 8 are generated using steps 3 – 5.
- 7) Each Burst is contained in even intervals of 1,500,000 microseconds. The starting location for Pulse 1, Burst 1 is randomly generated (1 to 1,500,000 minus the total Burst 1 length + 1 random PRI interval) at the 325,001 microsecond step. Bursts 2 through 8 randomly fall in successive 1,500,000 microsecond intervals (i.e. Burst 2 falls in the 1,500,001 – 3,000,000 microsecond range).



SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

SHEM-TRF-001 Rev. 02 Sep01, 2023

Report No.: SHCR250100004303

Page: 15 of 20

6.5.3 Frequency Hopping Radar Test Waveform

Table 7 – Frequency Hopping Radar Test Waveform

Type	Pulse Width (μsec)	PRI (μsec)	Pulses per Hop	Hopping Rate (kHz)	Hopping Sequence Length (msec)	Minimum Percentage of Successful Detection	Minimum Number of Trials
6	1	333	9	0.333	300	70%	30

For the Frequency Hopping Radar Type, the same Burst parameters are used for each waveform. The hopping sequence is different for each waveform and a 100-length segment is selected from the hopping sequence defined by the following algorithm:


The first frequency in a hopping sequence is selected randomly from the group of 475 integer frequencies from 5250 – 5724 MHz. Next, the frequency that was just chosen is removed from the group and a frequency is randomly selected from the remaining 474 frequencies in the group. This process continues until all 475 frequencies are chosen for the set. For selection of a random frequency, the frequencies remaining within the group are always treated as equally likely.

6.6 Calibration of Radar Waveform

6.6.1 Radar Waveform Calibration Procedure

- 1) A 50 ohm load is connected in place of the spectrum analyzer, and the spectrum analyzer is connected to place of the master
- 2) The interference Radar Detection Threshold Level is $-62\text{dBm} + (4.03)[\text{dBi}] + 1\text{db} = -56.97\text{dBm}$ that had been taken into account the output power range and antenna gain.
- 3) The following equipment setup was used to calibrate the conducted radar waveform. A vector signal generator was utilized to establish the test signal level for radar type 0. During this process there were no transmissions by either the master or client device. The spectrum analyzer was switched to the zero spans (time domain) at the frequency of the radar waveform generator. Peak detection was used. The spectrum analyzer resolution bandwidth (RBW) and video bandwidth (VBW) were set to 3 MHz.
- 4) The vector signal generator amplitude was set so that the power level measured at the spectrum analyzer was $-62\text{dBm} + (4.03)[\text{dBi}] + 1\text{db} = -56.97\text{dBm}$. Capture the spectrum analyzer plots on short pulse radar waveform

6.6.2 Conducted Calibration Setup






SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

SHEM-TRF-001 Rev. 02 Sep01, 2023

Report No.: SHCR250100004303

Page: 17 of 20

6.6.3 Radar Waveform Calibration Result

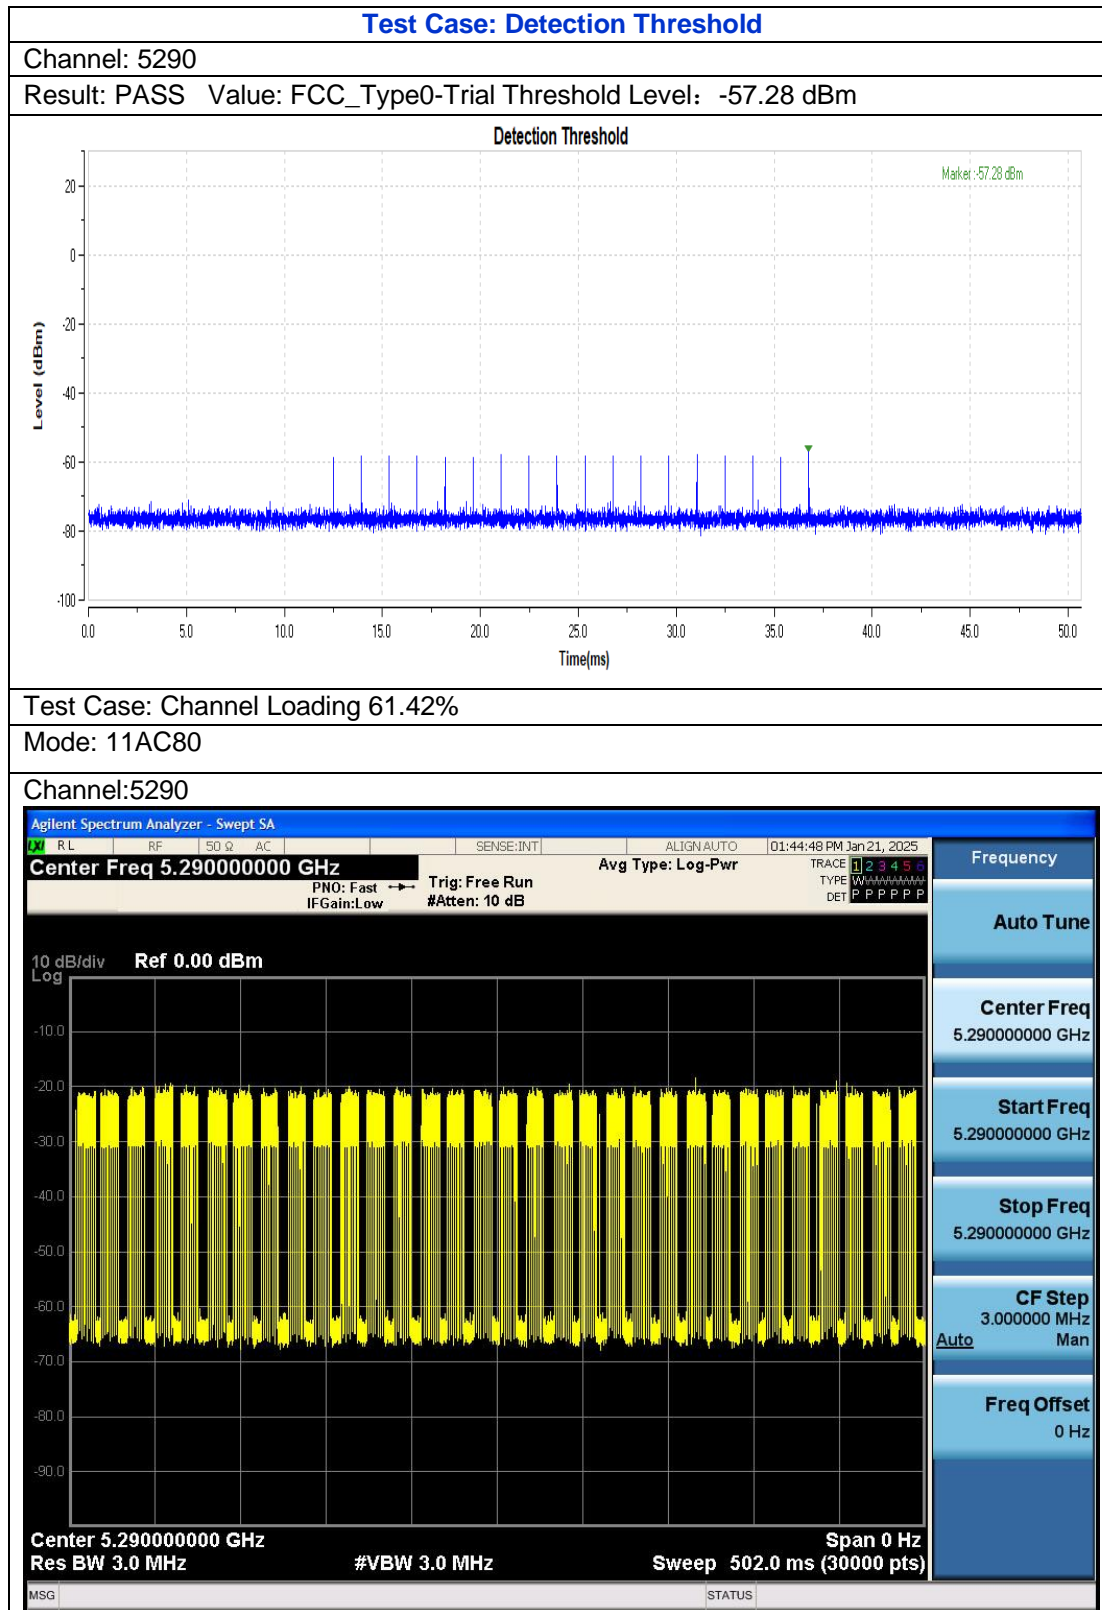


6.7 Channel Move Time and Channel Closing Transmission Time and Non-Occupancy Period

6.7.1 Test Procedure

- 1) The radar pulse generator is setup to provide a pulse at frequency that the master and client are operating. A type 0 radar pulse with a 1us pulse width and a 1428us PRI is used for the testing.
- 2) The vector signal generator is adjusted to provide the radar burst (18 pulses) at the level of approximately -61dBm at the antenna port of the master device.
- 3) A trigger is provided from the pulse generator to the DFS monitoring system in order to capture the traffic and the occurrence of the radar pulse.
- 4) EUT will associate with the master at channel. The file "iperf.exe" specified by the FCC is streamed from the PC 2 through the master and the client device to the PC 1 and played in full motion video using Media Player Classic Ver. 6.4.8.6 in order to properly load the network for the entire period of the test.
- 5) When radar burst with a level equal to the DFS Detection Threshold +1dB is generated on the operating channel of the U-NII device. At time T0 the radar waveform generator sends a burst of pulse of the radar waveform at Detection Threshold +1dB.
- 6) Observe the transmissions of the EUT at the end of the radar Burst on the Operating Channel. Measure and record the transmissions from the UUT during the observation time (Channel Move Time). One 15 seconds plot is reported for the Short Pulse Radar Type 0. The plot for the Short Pulse Radar Types start at the end of the radar burst. The Channel Move Time will be calculated based on the zoom in 600ms plot of the Short Pulse Radar Type.
- 7) Measurement of the aggregate duration of the Channel Closed Transmission Time method. With the spectrum analyzer set to zero span tuned to the center frequency of the EUT operating channel at the radar simulated frequency, peak detection, and max hold, the dwell time per bin is given by: $Dwell (0.3ms) = S (12000ms) / B (4000)$; where Dwell is the dwell time per spectrum analyzer sampling bin, S is sweep time and B is the number of spectrum analyzer sampling bins. An upper bound of the aggregate duration of the intermittent control signals of Channel Closing Transmission Time is calculated by: $C (ms) = N \times Dwell (0.3ms)$; where C is the Closing Time, N is the number of spectrum analyzer sampling bins (intermittent control signals) showing a U-NII transmission and Dwell is the dwell time per bin.
- 8) Measurement the EUT for more than 30 minutes following the channel move time to verify that no transmission or beacons occur on this channel.

6.7.2 Test Setup

Setup for Client with injection at the Master

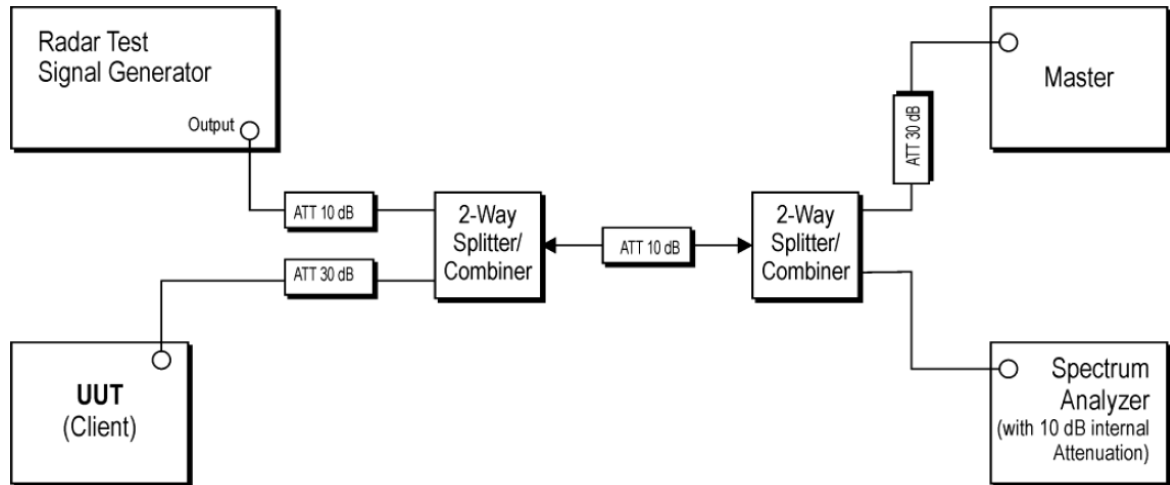

6.7.3 Channel Loading

System testing will be performed with channel-loading using means appropriate to the data types that are used by the unlicensed device. The following requirements apply:

<input type="checkbox"/>	a) The data file must be of a type that is typical for the device (i.e., MPEG-2, MPEG-4, WAV, MP3, MP4, AVI, etc.) and must generally be transmitting in a streaming mode.
<input type="checkbox"/>	b) Software to ping the client is permitted to simulate data transfer but must have random ping intervals.
<input checked="" type="checkbox"/>	c) Timing plots are required with calculations demonstrating a minimum channel loading of approximately 17% or greater. For example, channel loading can be estimated by setting the spectrum analyzer for zero span and approximate the Time On/ (Time On + Off Time). This can be done with any appropriate channel BW and modulation type.
<input type="checkbox"/>	d) Unicast or Multicast protocols are preferable but other protocols may be used. The appropriate protocol used must be described in the test procedures.





SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd.

SHEM-TRF-001 Rev. 02 Sep01, 2023

Report No.: SHCR250100004303

Page: 20 of 20

6.7.4 Test Result



- End of the Report -